


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX032421\  
 Data File : VX021422.D  
 Acq On : 24 Mar 2021 08:21  
 Operator : JC/MD  
 Sample : BFB  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X032421W.M  
 Title : SW846 8260  
 Last Update : Wed Mar 24 12:25:26 2021

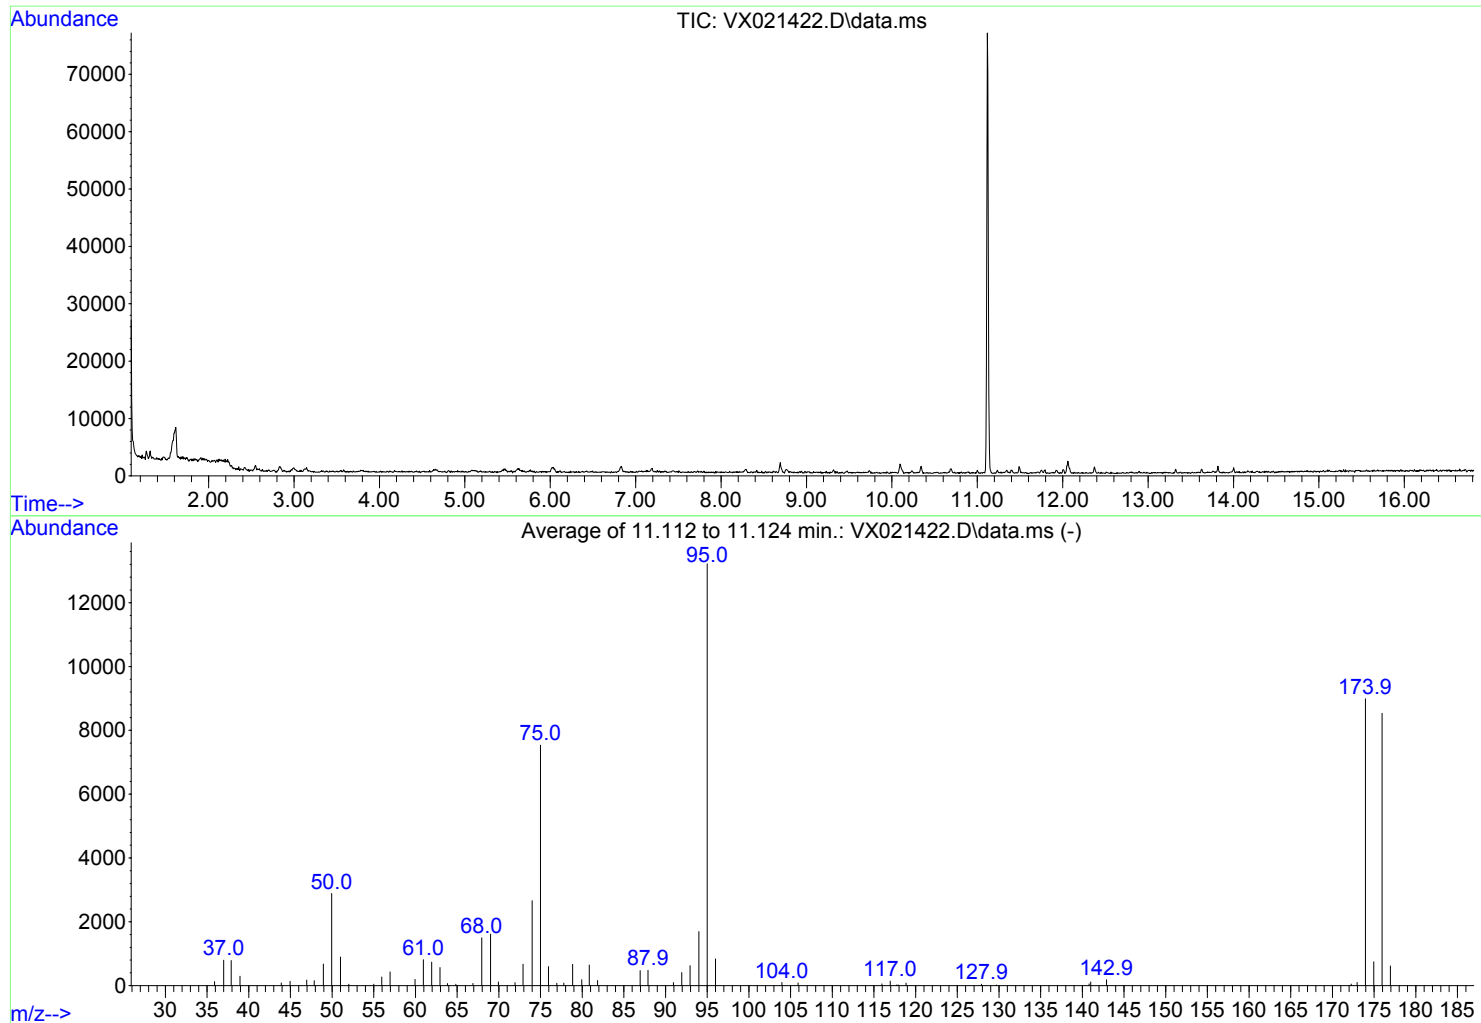

Spectrum Information: Average of 11.112 to 11.124 min.

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 21.9  | 2888  | PASS      |
| 75     | 95      | 30     | 60     | 57.0  | 7536  | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 13217 | PASS      |
| 96     | 95      | 5      | 9      | 6.3   | 838   | PASS      |
| 173    | 174     | 0.00   | 2      | 1.1   | 98    | PASS      |
| 174    | 95      | 50     | 100    | 68.0  | 8991  | PASS      |
| 175    | 174     | 5      | 9      | 8.3   | 746   | PASS      |
| 176    | 174     | 95     | 101    | 94.9  | 8535  | PASS      |
| 177    | 176     | 5      | 9      | 7.3   | 619   | PASS      |