

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
 Data File : VX021573.D
 Acq On : 29 Mar 2021 13:42
 Operator : JC/MD
 Sample : M1785-14 40X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-3RDL

Quant Time: Mar 30 03:27:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 24 12:25:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.629	168	62545	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.829	114	114308	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	121053	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.059	152	59501	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.029	65	53558	51.47	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 102.94%			
35) Dibromofluoromethane	5.464	113	41063	50.57	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 101.14%			
50) Toluene-d8	8.694	98	145889	50.42	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 100.84%			
62) 4-Bromofluorobenzene	11.118	95	64057	56.94	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 113.88%			
Target Compounds						Qvalue
3) Chloromethane	1.317	50	1291	1.67	ug/l	98
13) Acrolein	2.211	56	22	4.55	ug/l #	1
16) Acetone	2.423	43	321	0.82	ug/l	99
20) Methylene Chloride	2.835	84	207	0.27	ug/l #	70
29) Tetrahydrofuran	5.100	42	160	0.41	ug/l #	27
31) Cyclohexane	5.623	56	1684	1.47	ug/l #	4
36) 1,1-Dichloropropene	5.629	75	5637	5.03	ug/l #	50
38) Carbon Tetrachloride	5.623	117	6752	5.61	ug/l #	18
39) Methylcyclohexane	7.429	83	547	0.44	ug/l #	83
44) Trichloroethene	7.188	130	352	0.42	ug/l	76
51) 4-Methyl-2-Pentanone	8.694	43	824	0.64	ug/l #	1
55) 1,1,2-Trichloroethane	9.147	97	255	0.31	ug/l #	15
56) Ethyl methacrylate	9.147	69	20	2.09	ug/l #	1
67) Ethyl Benzene	10.235	91	5750	1.30	ug/l	100
68) m/p-Xylenes	10.341	106	7938	5.03	ug/l	89
69) o-Xylene	10.683	106	711	0.46	ug/l	81
73) Isopropylbenzene	11.000	105	20943	5.01	ug/l	99
74) N-amyl acetate	10.889	43	599	0.30	ug/l #	1
75) 1,1,2,2-Tetrachloroethane	11.259	83	394	0.27	ug/l #	26
76) 1,2,3-Trichloropropane	11.118	75	35307	25.49	ug/l #	38
78) n-propylbenzene	11.342	91	43954	8.90	ug/l	97
79) 2-Chlorotoluene	11.436	91	2002	0.67	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.489	105	8097	2.27	ug/l	97
81) trans-1,4-Dichloro-2-b...	11.118	75	35307	77.64	ug/l #	12
82) 4-Chlorotoluene	11.436	91	2002	0.56	ug/l #	45
83) tert-Butylbenzene	11.753	119	3160	0.91	ug/l	84
84) 1,2,4-Trimethylbenzene	11.789	105	177928	49.42	ug/l	98
85) sec-Butylbenzene	11.930	105	15344	3.83	ug/l	98
86) p-Isopropyltoluene	12.006	119	5815	1.59	ug/l	94
89) n-Butylbenzene	12.371	91	7801	2.33	ug/l #	71
90) Hexachloroethane	12.565	117	1033	1.57	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	12.995	75	67	2.14	ug/l #	1
95) Naphthalene	13.818	128	922	0.24	ug/l #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021573.D
Acq On : 29 Mar 2021 13:42
Operator : JC/MD
Sample : M1785-14 40X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL

Quant Time: Mar 30 03:27:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 24 12:25:26 2021
Response via : Initial Calibration




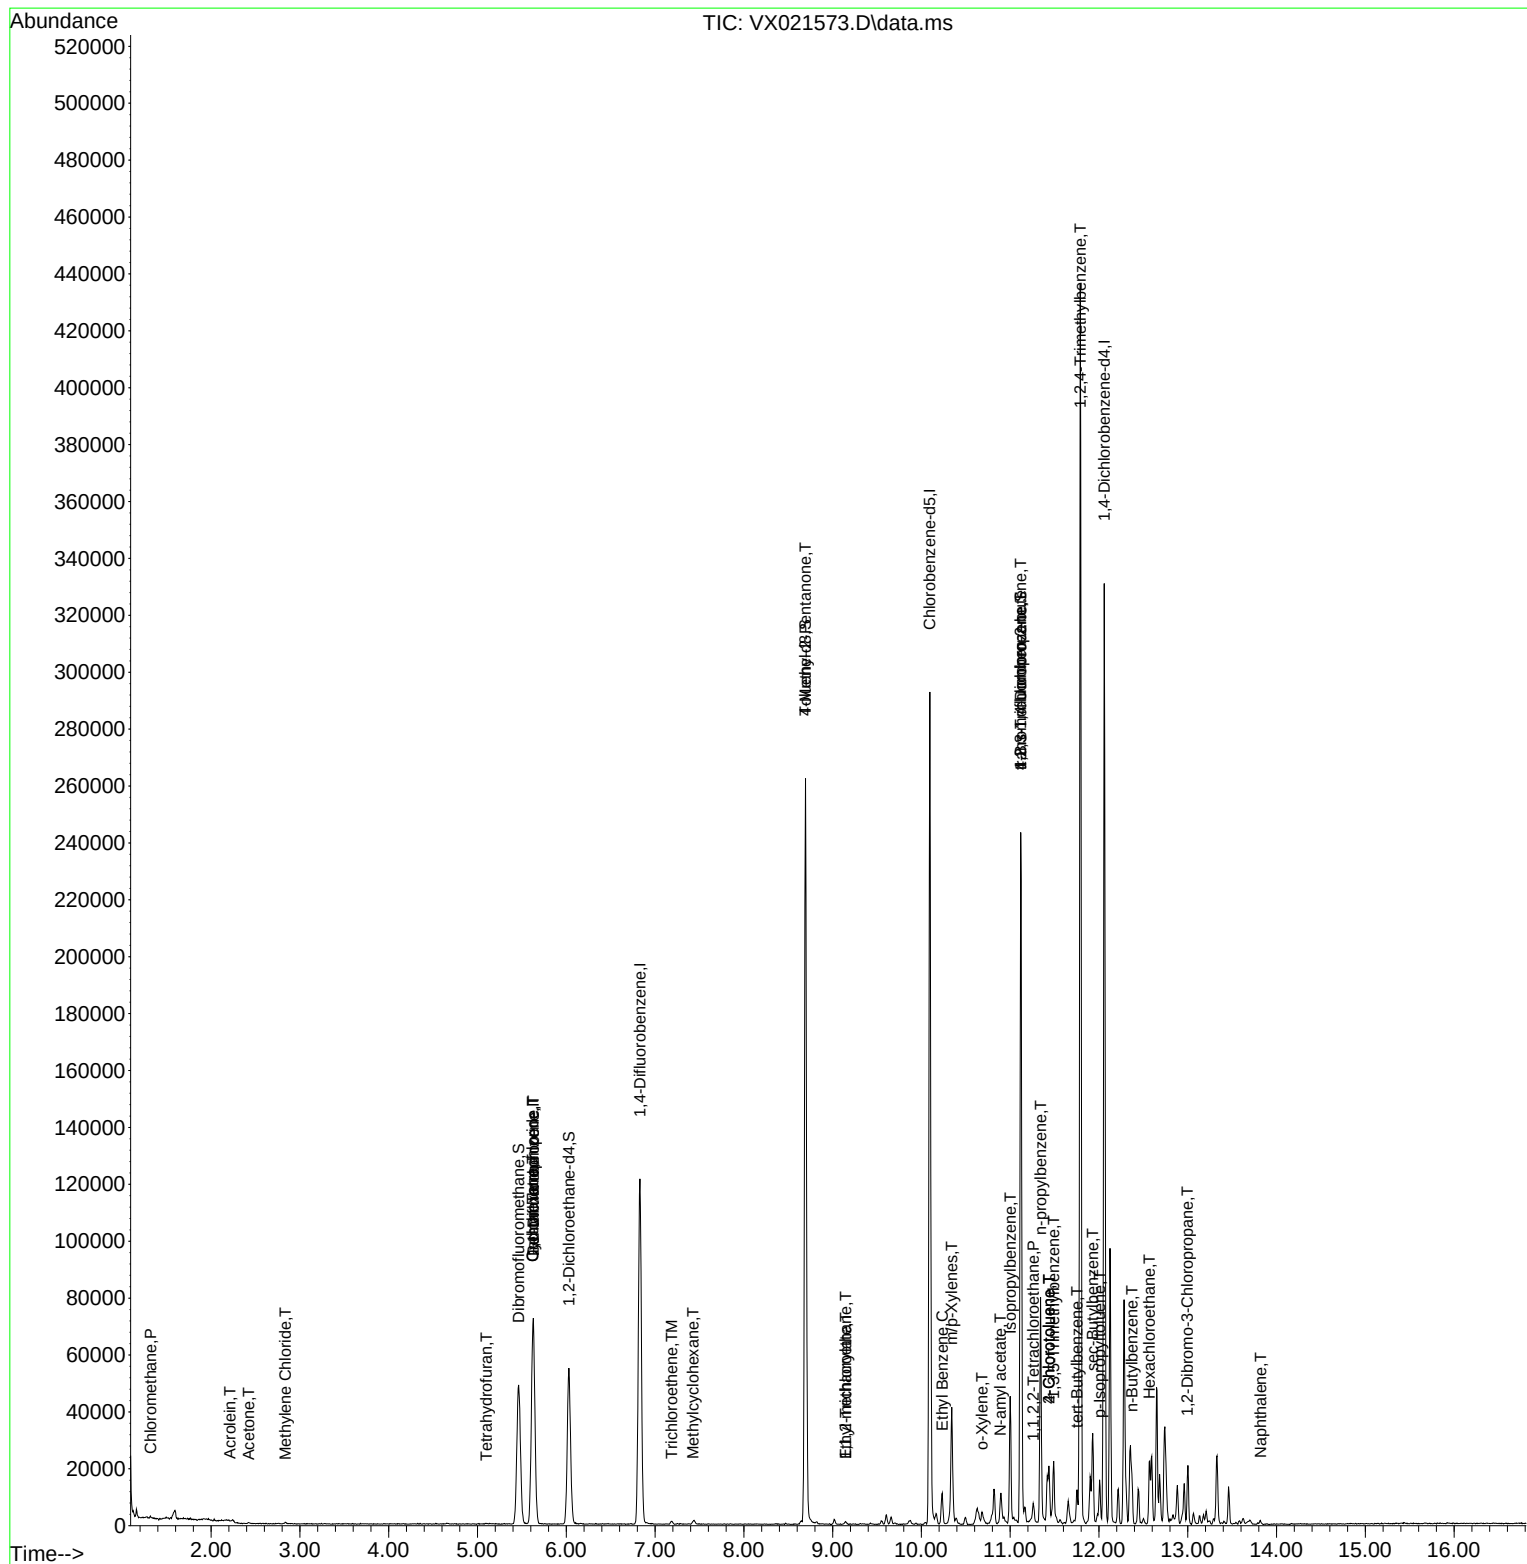


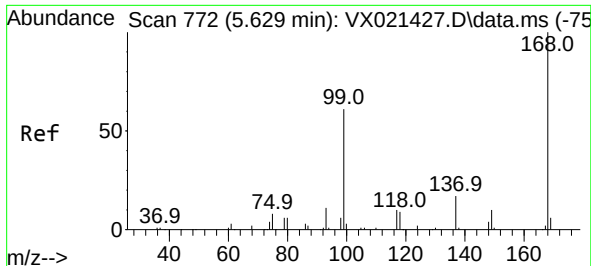

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.629 min Scan# 772
Delta R.T. 0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL


Tgt Ion:168 Resp: 62545
Ion Ratio Lower Upper
168 100
99 64.5 45.8 68.6

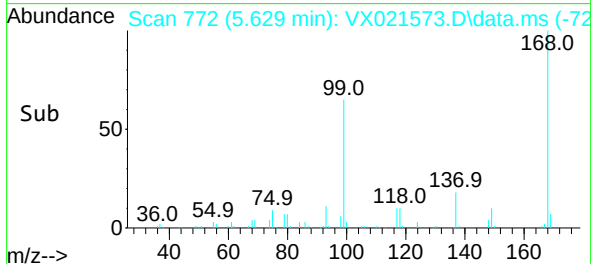

#3
Chloromethane
Concen: 1.67 ug/l
RT: 1.317 min Scan# 39
Delta R.T. 0.006 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion: 50 Resp: 1291
Ion Ratio Lower Upper
50 100
52 34.1 26.4 39.6


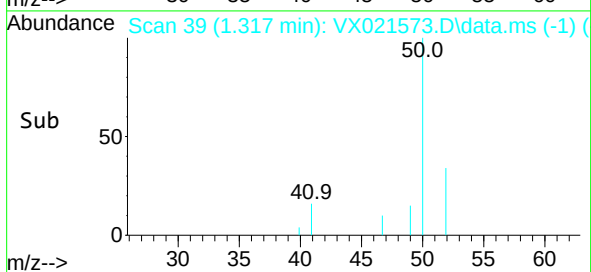

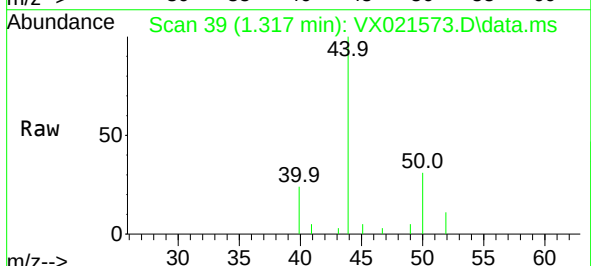




#13
Acrolein
Concen: 4.55 ug/l
RT: 2.211 min Scan# 191
Delta R.T. -0.065 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL


Tgt Ion: 56 Resp: 22
Ion Ratio Lower Upper
56 100
55 495.5 56.4 84.6#

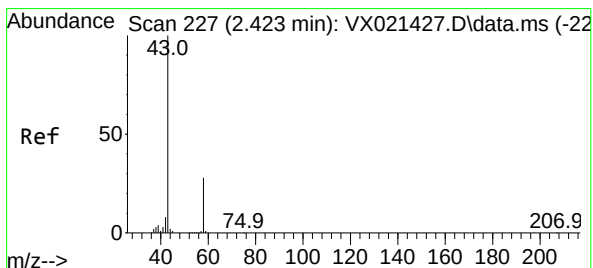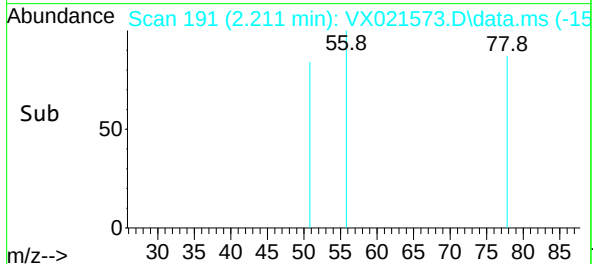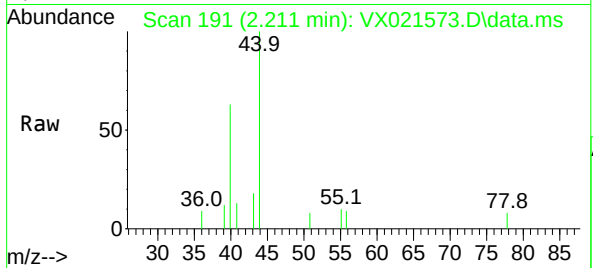

#16
Acetone
Concen: 0.82 ug/l
RT: 2.423 min Scan# 227
Delta R.T. -0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion: 43 Resp: 321
Ion Ratio Lower Upper
43 100
58 35.6 27.8 41.8

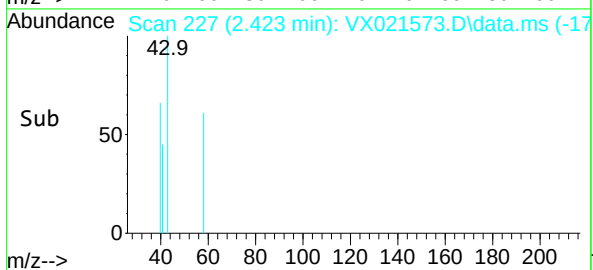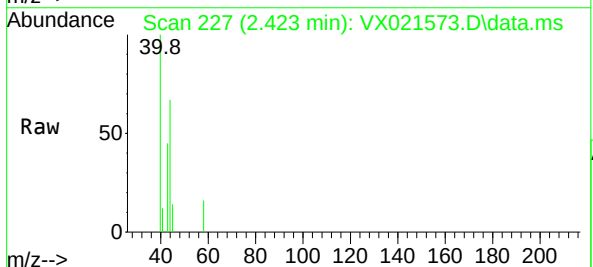



#20

Methylene Chloride

Concen: 0.27 ug/l

RT: 2.835 min Scan# 297

Delta R.T. 0.001 min

Lab File: VX021573.D

Acq: 29 Mar 2021 13:42

Tgt Ion: 84 Resp: 207





Ion Ratio Lower Upper

84 100

49 70.1 88.6 132.8#

51 53.5 27.0 40.6#

86 52.0 50.3 75.5

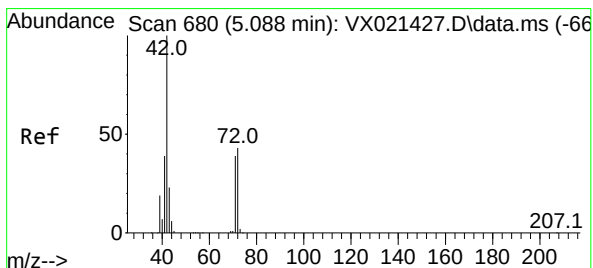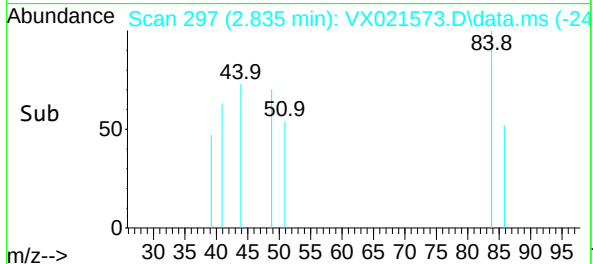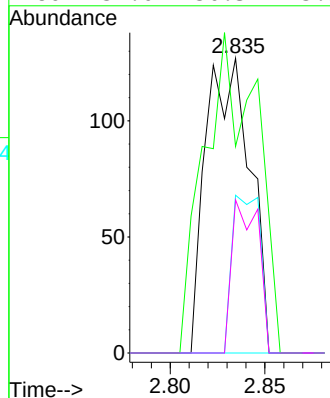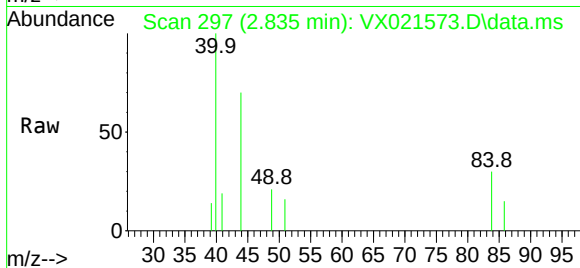

#29

Tetrahydrofuran

Concen: 0.41 ug/l

RT: 5.100 min Scan# 682

Delta R.T. 0.012 min

Lab File: VX021573.D

Acq: 29 Mar 2021 13:42




Tgt Ion: 42 Resp: 160


Ion Ratio Lower Upper

42 100

72 0.0 41.7 62.5#


71 0.0 38.4 57.6#

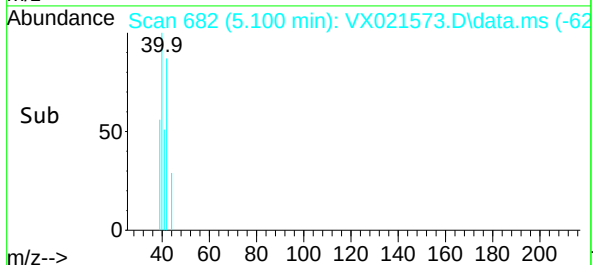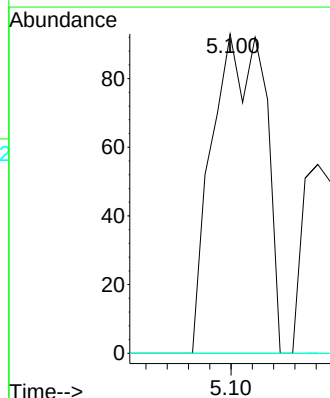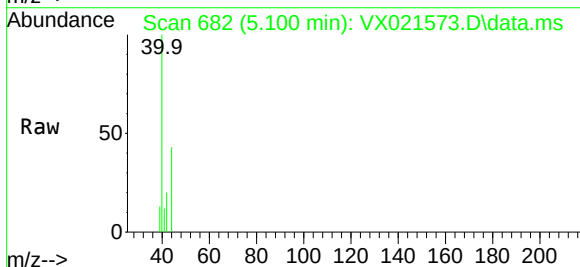






#31
Cyclohexane
Concen: 1.47 ug/l
RT: 5.623 min Scan# 771
Delta R.T. 0.076 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL



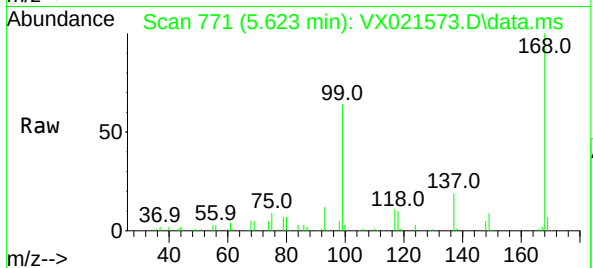



Tgt Ion: 56 Resp: 1684
Ion Ratio Lower Upper
56 100
69 185.2 25.3 37.9#
84 118.6 71.4 107.0#

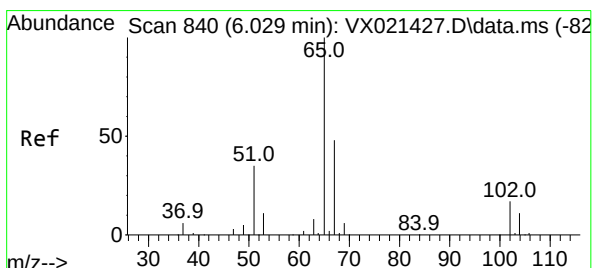

#33
1,2-Dichloroethane-d4
Concen: 51.47 ug/l
RT: 6.029 min Scan# 840
Delta R.T. 0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion: 65 Resp: 53558
Ion Ratio Lower Upper
65 100
67 49.3 0.0 105.4


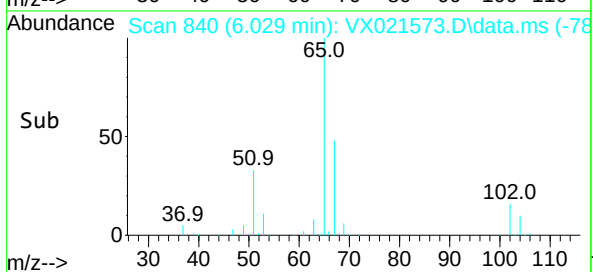




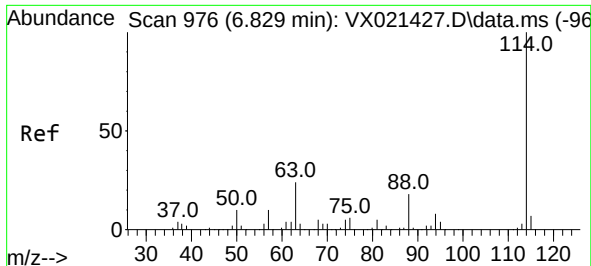

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.829 min Scan# 976
Delta R.T. 0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL


Tgt Ion:114 Resp: 114308
Ion Ratio Lower Upper
114 100
63 23.8 0.0 40.8
88 16.4 0.0 32.8

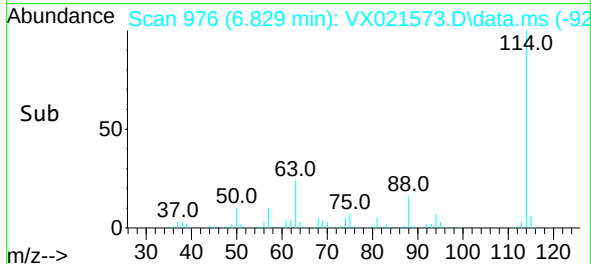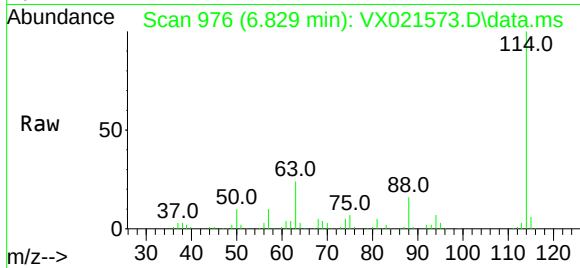

#35
Dibromofluoromethane
Concen: 50.57 ug/l
RT: 5.464 min Scan# 744
Delta R.T. 0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion:113 Resp: 41063
Ion Ratio Lower Upper
113 100
111 102.0 81.9 122.9
192 19.3 16.7 25.1

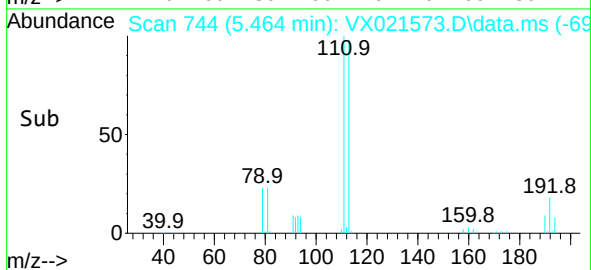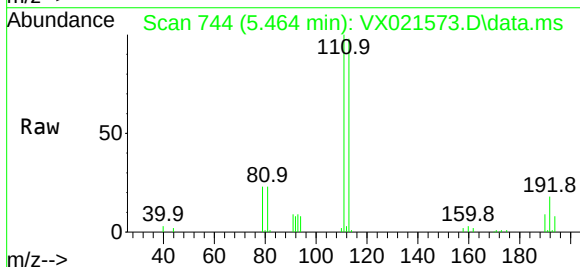



#36

1,1-Dichloropropene

Concen: 5.03 ug/l

RT: 5.629 min Scan# 772





Delta R.T. -0.135 min

Lab File: VX021573.D

Acq: 29 Mar 2021 13:42

Tgt Ion:	75	Resp:	5637
Ion	Ratio	Lower	Upper
75	100		
110	9.9	18.1	54.4#
77	0.0	25.3	37.9#

Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL

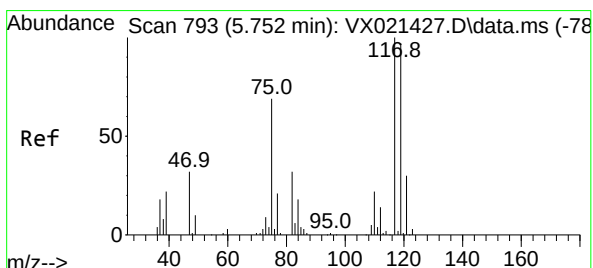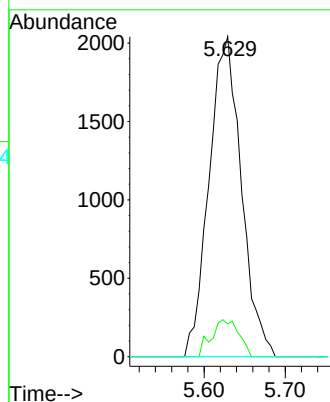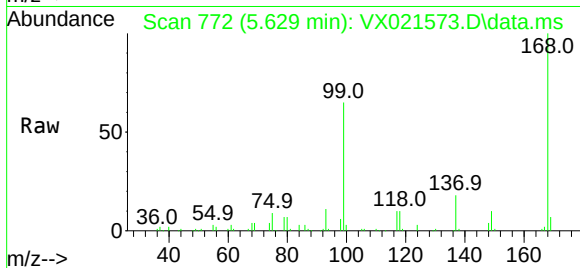

#38

Carbon Tetrachloride

Concen: 5.61 ug/l




RT: 5.623 min Scan# 771


Delta R.T. -0.129 min

Lab File: VX021573.D

Acq: 29 Mar 2021 13:42

Tgt Ion:	117	Resp:	6752
Ion	Ratio	Lower	Upper
117	100		
119	7.1	76.2	114.2#
121	0.0	24.8	37.2#

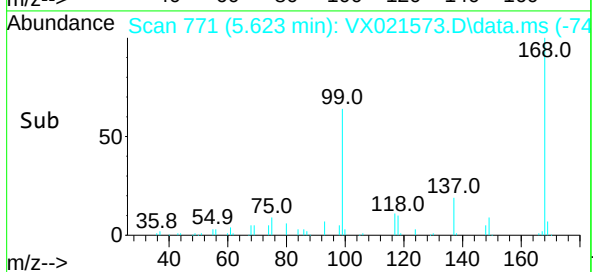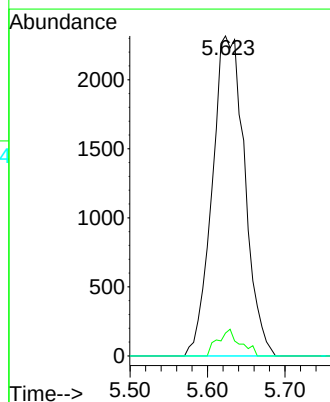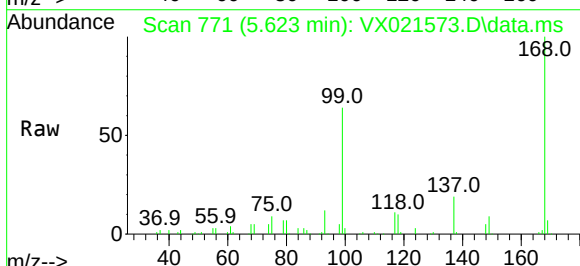



#39

Methylcyclohexane

Concen: 0.44 ug/l

RT: 7.429 min Scan# 1078

Delta R.T. -0.006 min

Lab File: VX021573.D

Acq: 29 Mar 2021 13:42





Instrument :

MSVOA_X

ClientSampleId :

MW-3RDL

Tgt Ion:	83	Resp:	547
Ion	Ratio	Lower	Upper
83	100		
55	80.8	58.9	88.3
98	27.5	38.1	57.1#

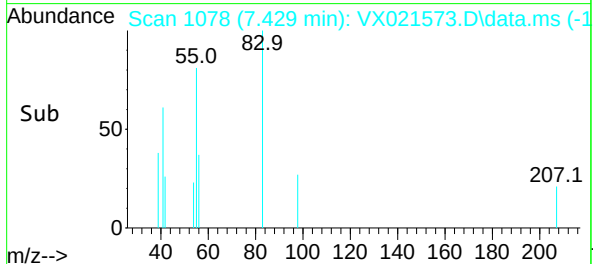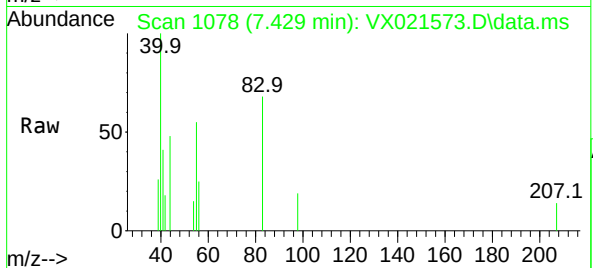

#44

Trichloroethene

Concen: 0.42 ug/l




RT: 7.188 min Scan# 1037


Delta R.T. 0.000 min

Lab File: VX021573.D

Acq: 29 Mar 2021 13:42

Tgt Ion:	130	Resp:	352
Ion	Ratio	Lower	Upper
130	100		
95	75.4	0.0	198.0

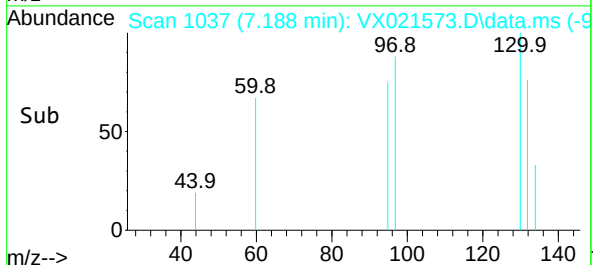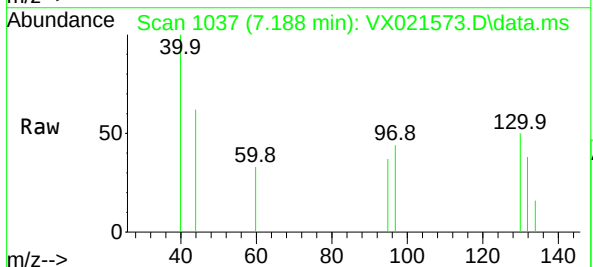



#50

Toluene-d8

Concen: 50.42 ug/l

RT: 8.694 min Scan# 1293

Delta R.T. 0.000 min

Lab File: VX021573.D





Acq: 29 Mar 2021 13:42

Tgt Ion: 98 Resp: 145889

Ion Ratio Lower Upper

98 100

100 65.0 51.9 77.9

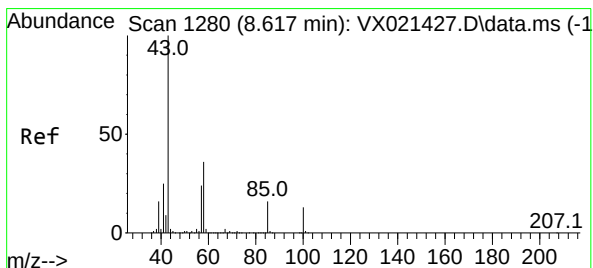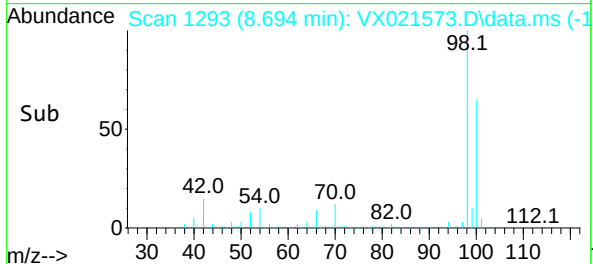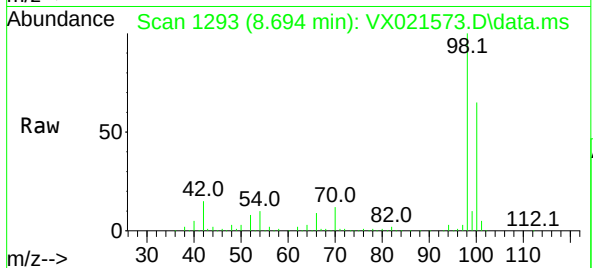

#51

4-Methyl-2-Pentanone

Concen: 0.64 ug/l

RT: 8.694 min Scan# 1293

Delta R.T. 0.077 min

Lab File: VX021573.D




Acq: 29 Mar 2021 13:42


Tgt Ion: 43 Resp: 824

Ion Ratio Lower Upper

43 100


58 173.7 35.4 53.0#

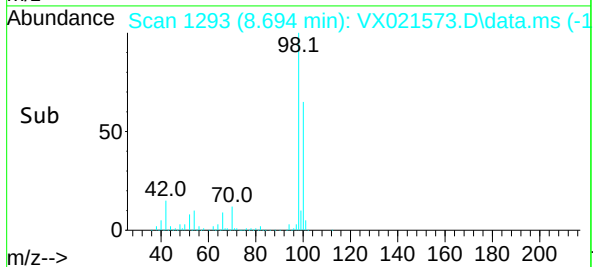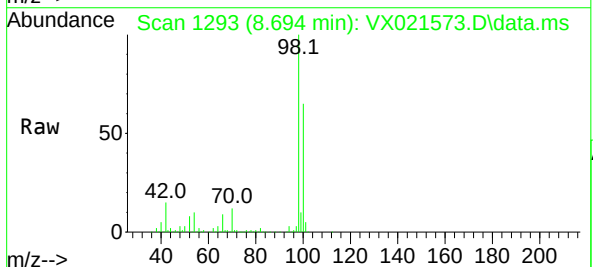



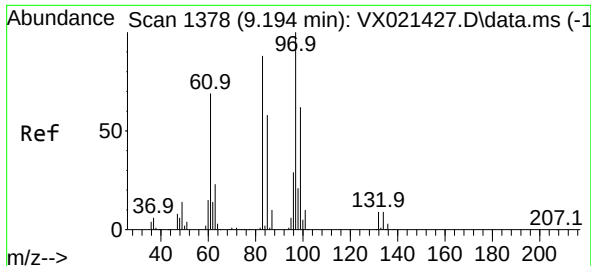


#55
1,1,2-Trichloroethane
Concen: 0.31 ug/l
RT: 9.147 min Scan# 1370
Delta R.T. -0.047 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Instrument :
MSVOA_X
ClientSampled :
MW-3RDL







Tgt Ion: 97	Resp: 255
Ion Ratio	Lower Upper
97	100
83	0.0 69.3 103.9#
85	0.0 44.3 66.5#
99	0.0 50.3 75.5#

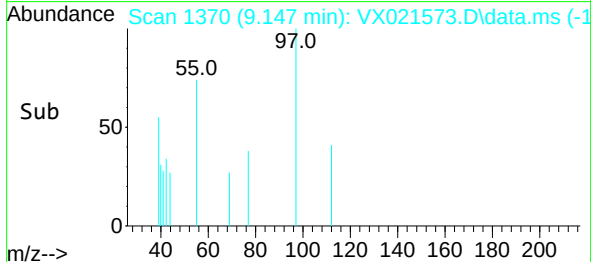

#56
Ethyl methacrylate
Concen: 2.09 ug/l
RT: 9.147 min Scan# 1370
Delta R.T. -0.012 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion: 69	Resp: 20
Ion Ratio	Lower Upper
69	100
41	1060.0 46.8 70.2#
39	1045.0 24.7 37.1#


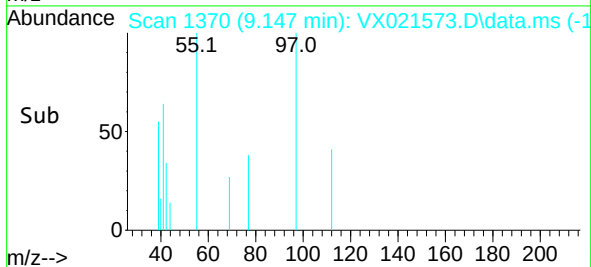

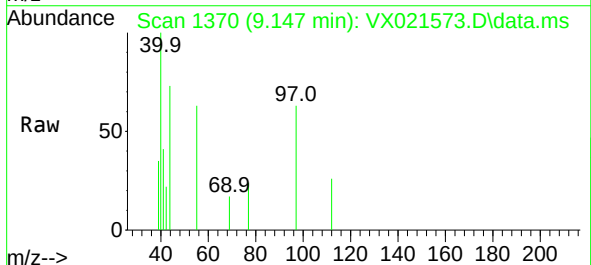


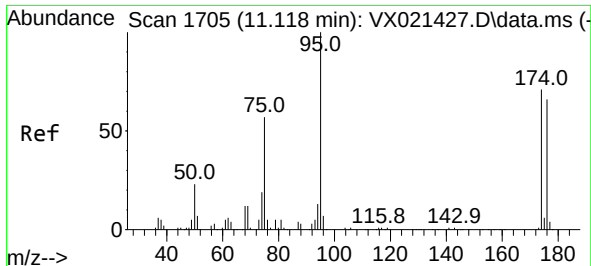

#62
4-Bromofluorobenzene
Concen: 56.94 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL


Tgt Ion: 95 Resp: 64057
Ion Ratio Lower Upper
95 100
174 72.0 0.0 154.6
176 72.1 0.0 155.8

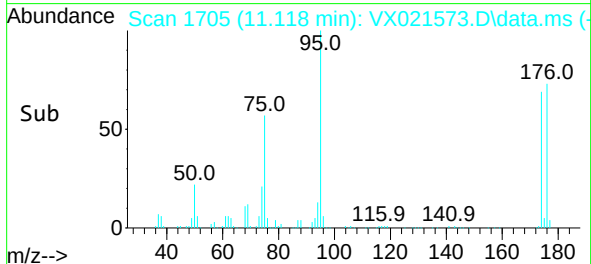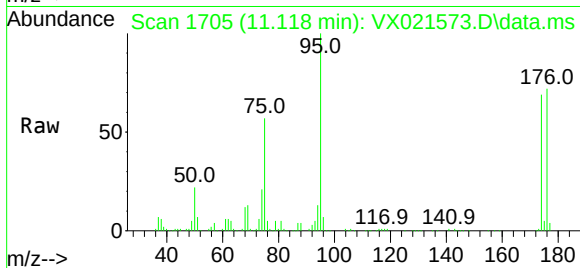

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. 0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion: 117 Resp: 121053
Ion Ratio Lower Upper
117 100
82 59.7 47.4 71.2
119 34.5 26.6 39.8


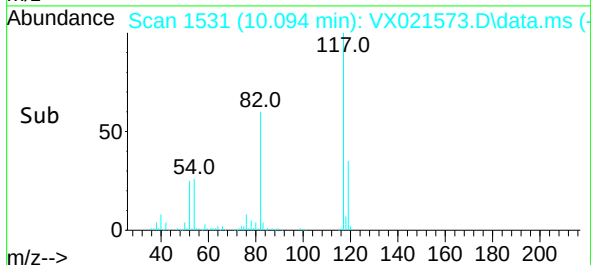

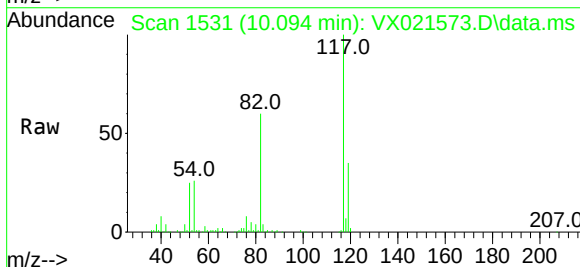




#67
Ethyl Benzene
Concen: 1.30 ug/l
RT: 10.235 min Scan# 1555
Delta R.T. 0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL


Tgt Ion: 91 Resp: 5750
Ion Ratio Lower Upper
91 100
106 31.0 24.6 37.0

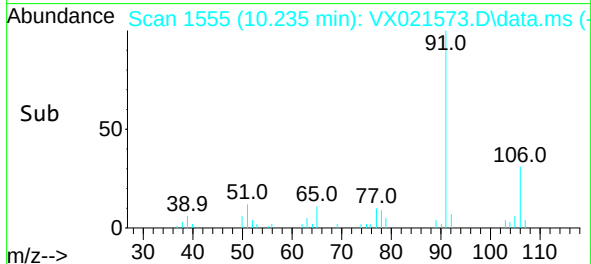

#68
m/p-Xylenes
Concen: 5.03 ug/l
RT: 10.341 min Scan# 1573
Delta R.T. 0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion: 106 Resp: 7938
Ion Ratio Lower Upper
106 100
91 219.8 162.8 244.2




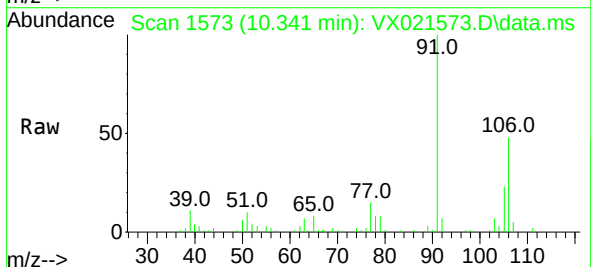


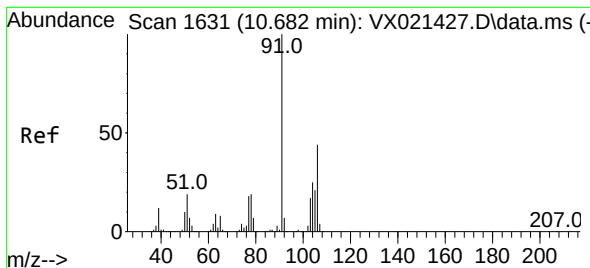

#69
o-Xylene
Concen: 0.46 ug/l
RT: 10.683 min Scan# 1631
Delta R.T. 0.001 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL


Tgt Ion:106 Resp: 711
Ion Ratio Lower Upper
106 100
91 246.4 108.1 324.2

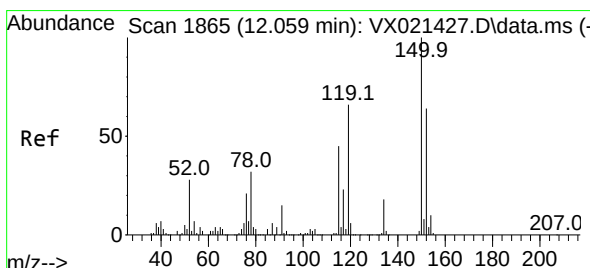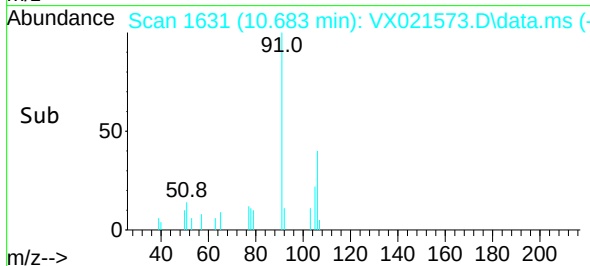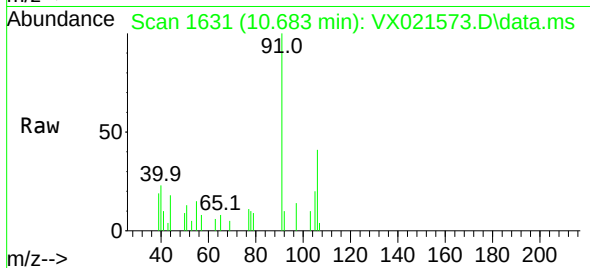

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.059 min Scan# 1865
Delta R.T. 0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion:152 Resp: 59501
Ion Ratio Lower Upper
152 100
115 63.3 41.1 123.3
150 158.9 0.0 349.0


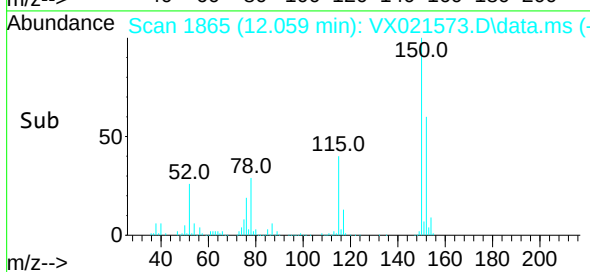

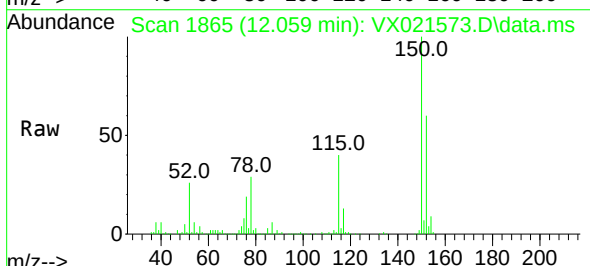




#73
Isopropylbenzene
Concen: 5.01 ug/l
RT: 11.000 min Scan# 1685
Delta R.T. 0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL


Tgt Ion:105 Resp: 20943
Ion Ratio Lower Upper
105 100
120 25.7 13.2 39.6

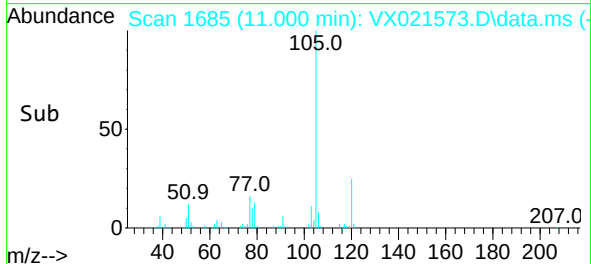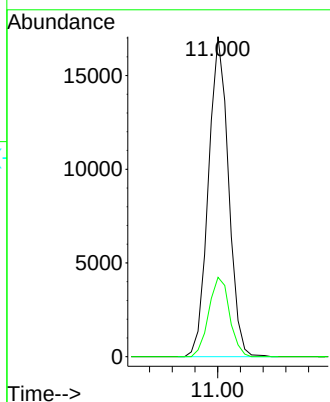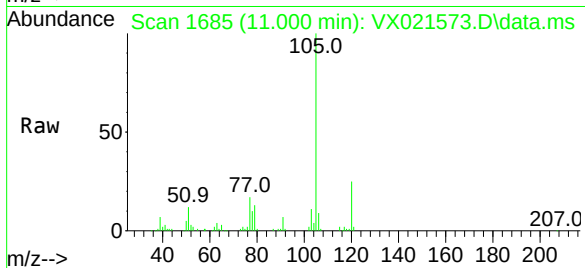

#74
N-ethyl acetate
Concen: 0.30 ug/l
RT: 10.889 min Scan# 1666
Delta R.T. 0.006 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion: 43 Resp: 599
Ion Ratio Lower Upper
43 100
70 95.7 39.0 58.6#
55 360.9 21.5 32.3#
61 0.0 22.1 33.1#


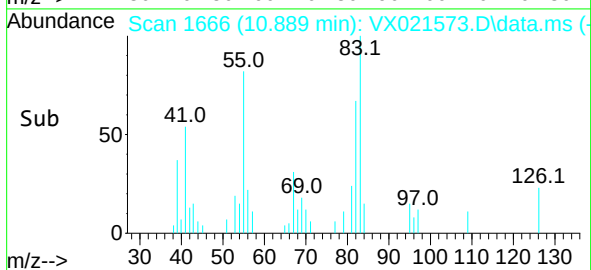
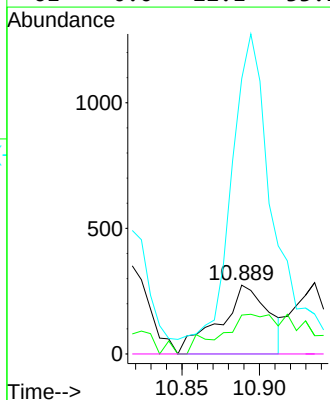
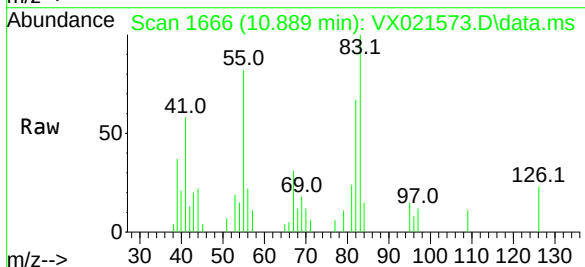


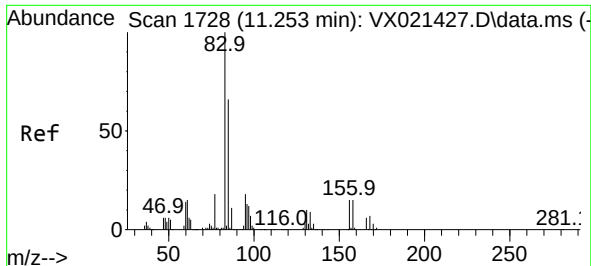

#75
1,1,2,2-Tetrachloroethane
Concen: 0.27 ug/l
RT: 11.259 min Scan# 1729
Delta R.T. 0.006 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL


Tgt Ion: 83 Resp: 394
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.2#
85 0.0 31.8 95.4#

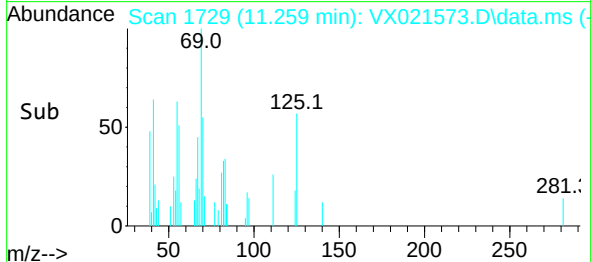

#76
1,2,3-Trichloropropane
Concen: 25.49 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.159 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion: 75 Resp: 35307
Ion Ratio Lower Upper
75 100
77 1.1 19.1 57.5#


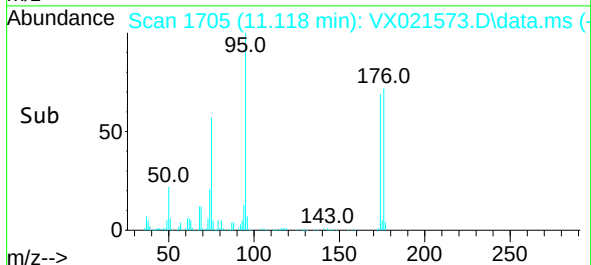

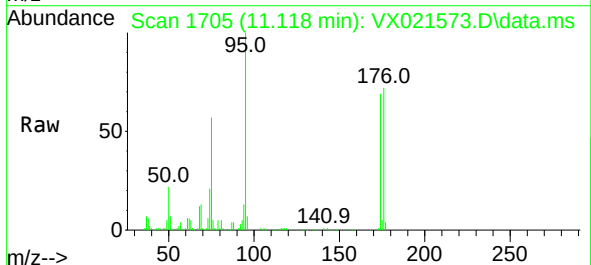


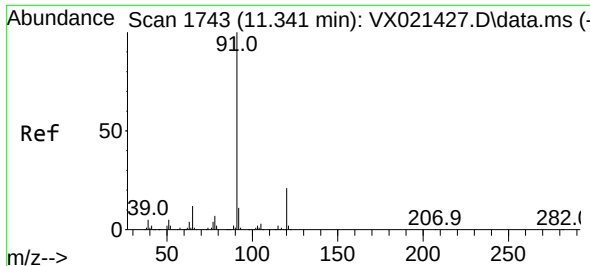

#78
n-propylbenzene
Concen: 8.90 ug/l
RT: 11.342 min Scan# 1743
Delta R.T. 0.001 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampled :
MW-3RDL


Tgt Ion: 91 Resp: 43954
Ion Ratio Lower Upper
91 100
120 21.4 11.5 34.5

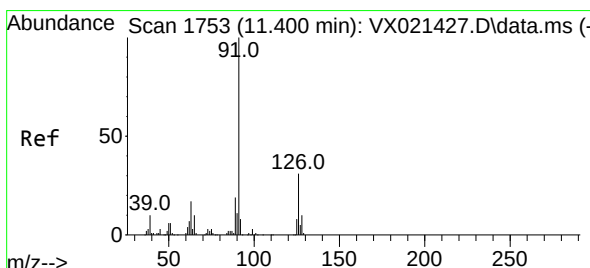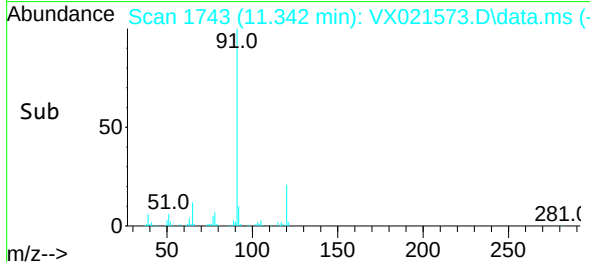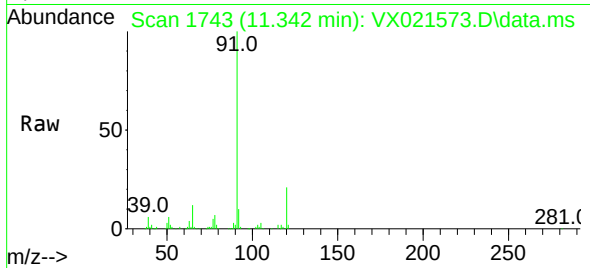

#79
2-Chlorotoluene
Concen: 0.67 ug/l
RT: 11.436 min Scan# 1759
Delta R.T. 0.036 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion: 91 Resp: 2002
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#


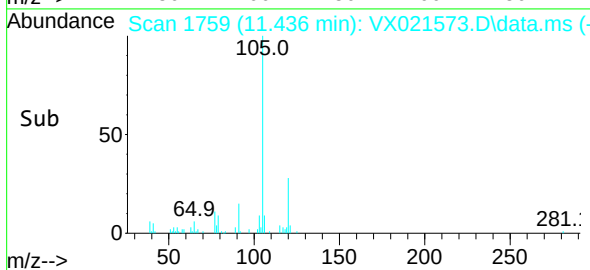

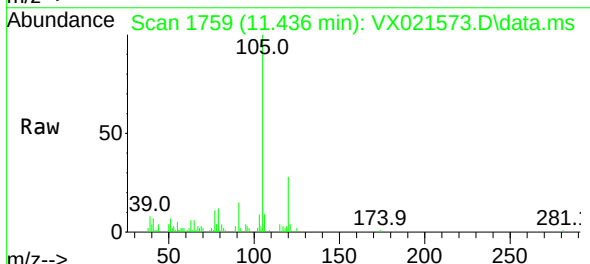




#80
1,3,5-Trimethylbenzene
Concen: 2.27 ug/l
RT: 11.489 min Scan# 1768
Delta R.T. 0.001 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL


Tgt Ion:105 Resp: 8097
Ion Ratio Lower Upper
105 100
120 49.7 23.8 71.5

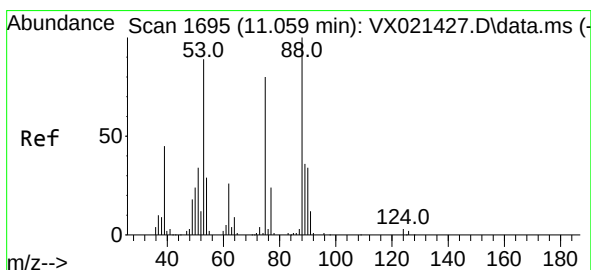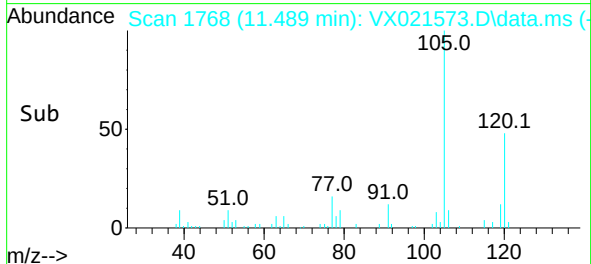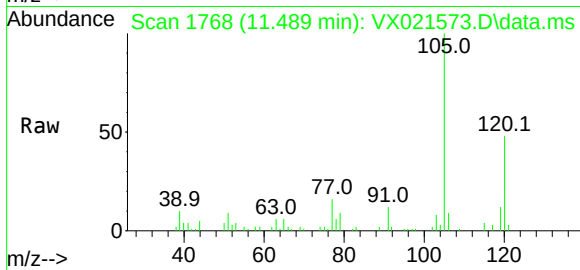

#81
trans-1,4-Dichloro-2-butene
Concen: 77.64 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. 0.059 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion: 75 Resp: 35307
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#


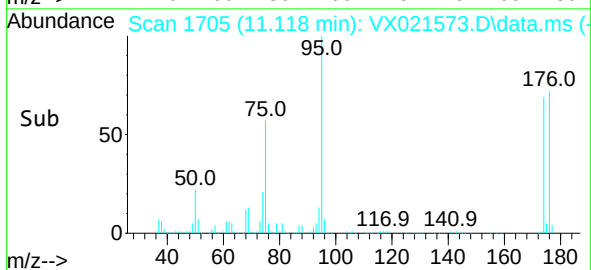

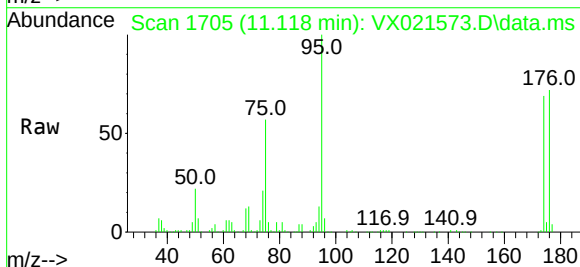




#82
4-Chlorotoluene
Concen: 0.56 ug/l
RT: 11.436 min Scan# 1759
Delta R.T. -0.058 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampled :
MW-3RDL


Tgt Ion: 91 Resp: 2002
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

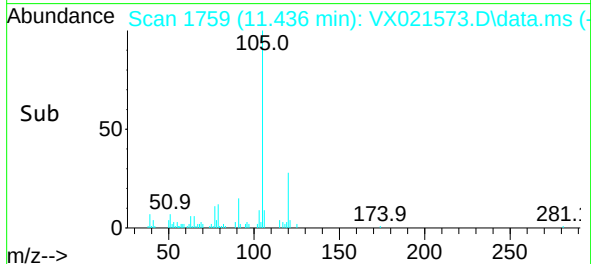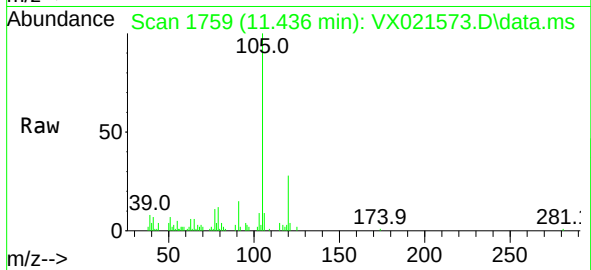

#83
tert-Butylbenzene
Concen: 0.91 ug/l
RT: 11.753 min Scan# 1813
Delta R.T. 0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion: 119 Resp: 3160
Ion Ratio Lower Upper
119 100
91 71.6 27.9 83.7
134 22.9 11.3 33.9


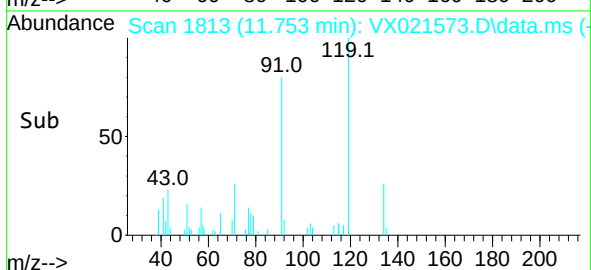

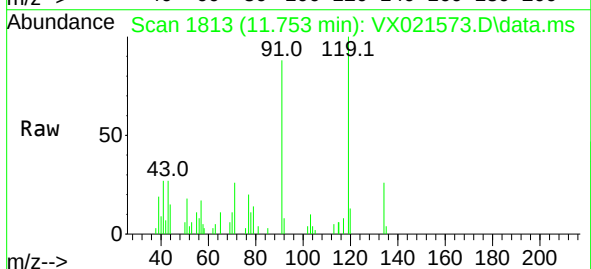




#84
1,2,4-Trimethylbenzene
Concen: 49.42 ug/l
RT: 11.789 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL


Tgt Ion:105 Resp: 177928
Ion Ratio Lower Upper
105 100
120 43.4 22.4 67.3

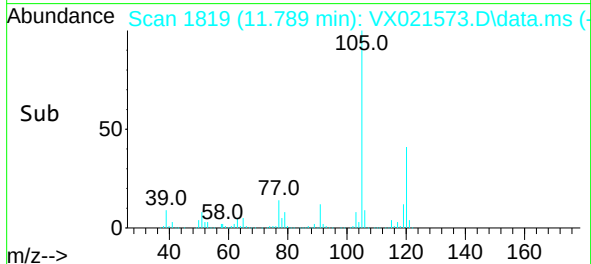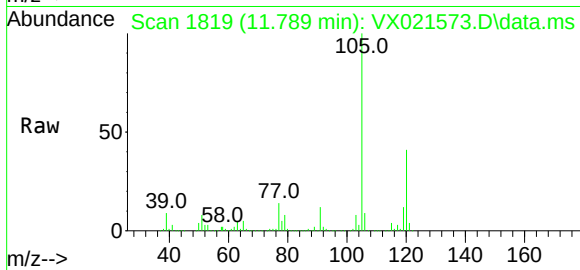

#85
sec-Butylbenzene
Concen: 3.83 ug/l
RT: 11.930 min Scan# 1843
Delta R.T. -0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion:105 Resp: 15344
Ion Ratio Lower Upper
105 100
134 18.8 10.0 29.8


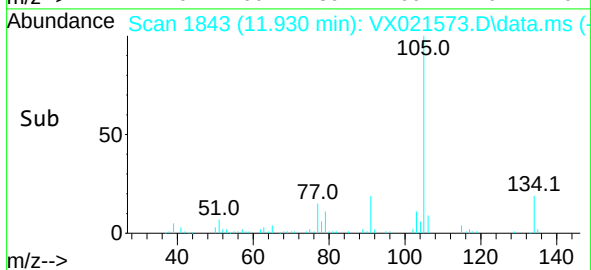

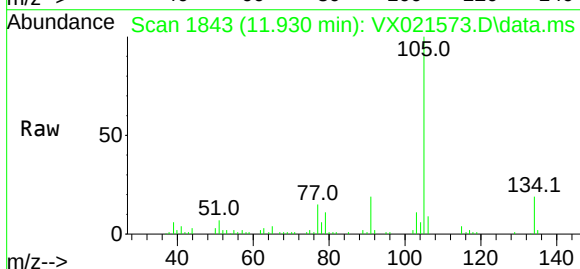


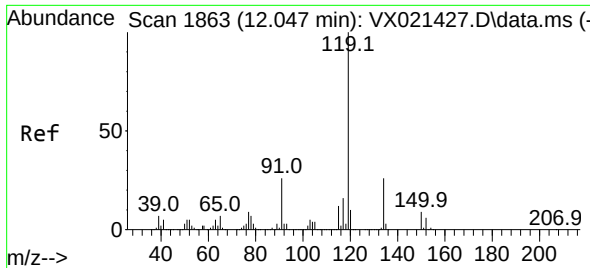

#86
p-Isopropyltoluene
Concen: 1.59 ug/l
RT: 12.006 min Scan# 1856
Delta R.T. -0.041 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42




Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL


Tgt Ion:119 Resp: 5815
Ion Ratio Lower Upper
119 100
134 26.5 12.9 38.7
91 29.0 11.7 35.0

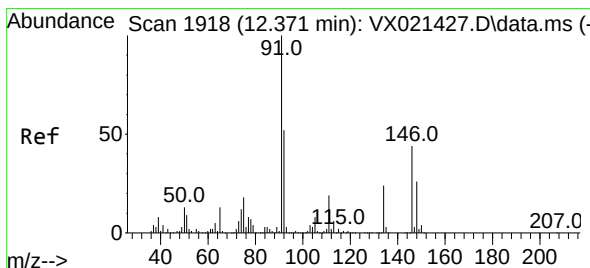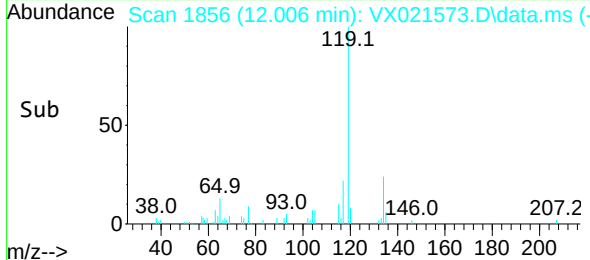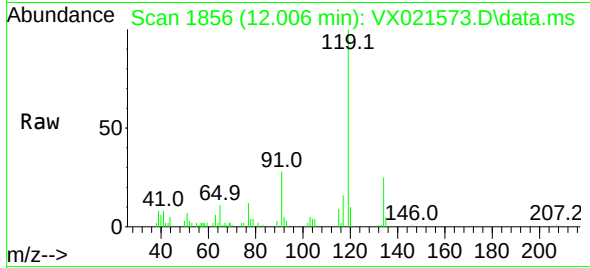

#89
n-Butylbenzene
Concen: 2.33 ug/l
RT: 12.371 min Scan# 1918
Delta R.T. 0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Tgt Ion: 91 Resp: 7801
Ion Ratio Lower Upper
91 100
92 42.4 27.4 82.0
134 53.7 13.2 39.5#

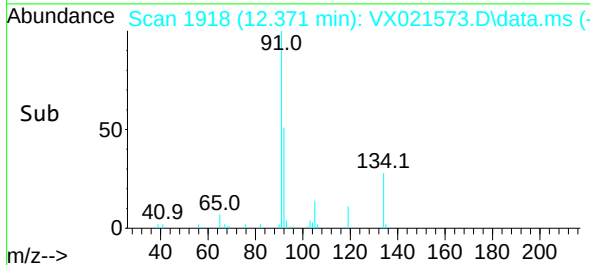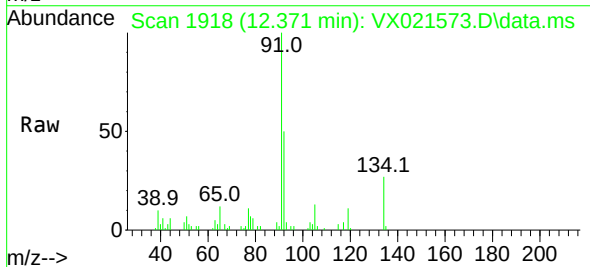



#90

Hexachloroethane

Concen: 1.57 ug/l

RT: 12.565 min Scan# 1951

Delta R.T. -0.012 min

Lab File: VX021573.D

Acq: 29 Mar 2021 13:42

Instrument :

MSVOA_X

ClientSampleId :





MW-3RDL

Tgt Ion:117 Resp: 1033

Ion Ratio Lower Upper

117 100

201 0.0 40.4 121.2#

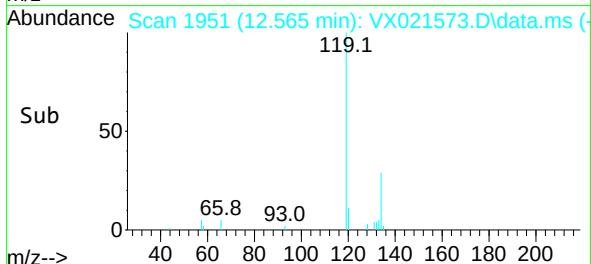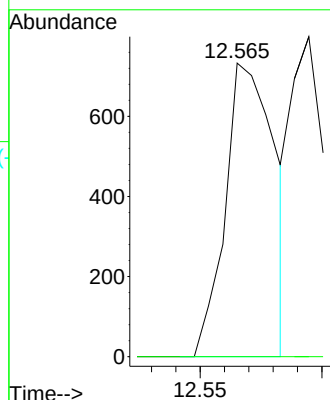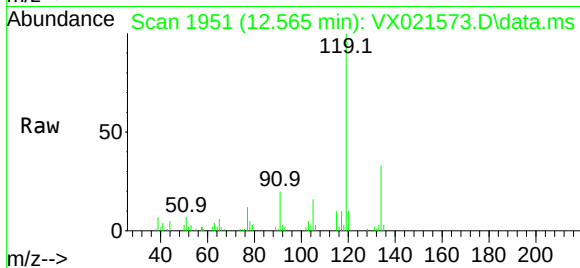

#92

1,2-Dibromo-3-Chloropropane

Concen: 2.14 ug/l

RT: 12.995 min Scan# 2024

Delta R.T. 0.012 min

Lab File: VX021573.D

Acq: 29 Mar 2021 13:42




Tgt Ion: 75 Resp: 67


Ion Ratio Lower Upper

75 100

155 0.0 45.3 135.9#


157 0.0 57.7 173.1#

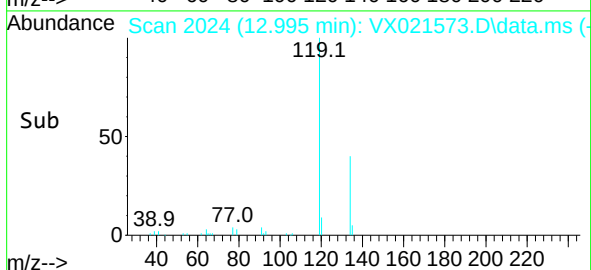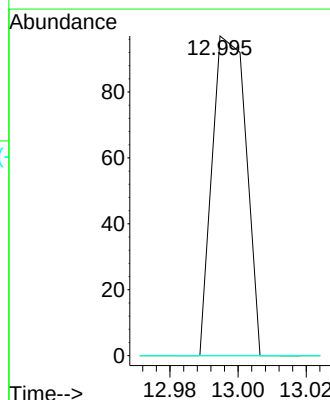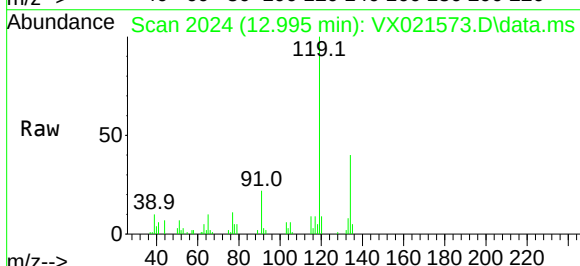

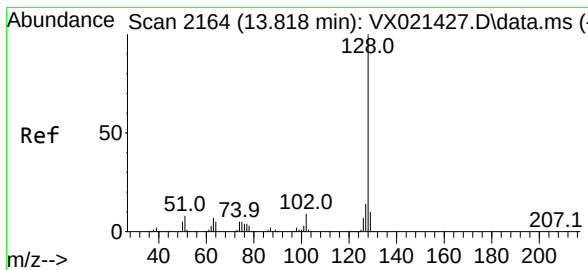

#95
Naphthalene
Concen: 0.24 ug/l
RT: 13.818 min Scan# 2164
Delta R.T. 0.000 min
Lab File: VX021573.D
Acq: 29 Mar 2021 13:42

Instrument :
MSVOA_X
ClientSampleId :
MW-3RDL

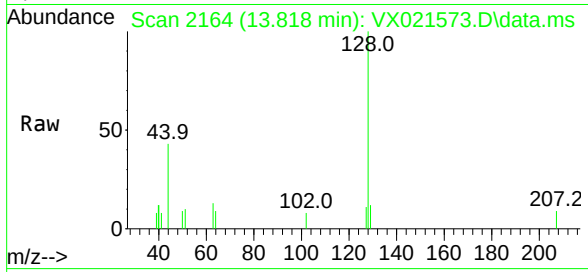

Tgt Ion:128 Resp: 922
Ion Ratio Lower Upper
128 100
127 9.8 10.3 15.5#
129 14.1 8.8 13.2#

