

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
 Data File : VX021574.D
 Acq On : 29 Mar 2021 14:05
 Operator : JC/MD
 Sample : M1785-15 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-4

Quant Time: Mar 30 03:27:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
 Quant Title : SW846 8260
 QLast Update : Wed Mar 24 12:25:26 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.623	168	62597	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.829	114	114338	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.094	117	118030	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.059	152	58057	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.029	65	53166	51.05	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 102.10%	
35) Dibromofluoromethane	5.464	113	40807	50.24	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.48%	
50) Toluene-d8	8.694	98	145276	50.20	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 100.40%	
62) 4-Bromofluorobenzene	11.118	95	63160	56.13	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 112.26%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.317	50	1379	1.78	ug/l	91
10) Methyl Iodide	2.499	142	18	6.67	ug/l #	42
11) Tert butyl alcohol	3.005	59	288	1.67	ug/l #	73
13) Acrolein	2.223	56	20	4.52	ug/l #	14
16) Acetone	2.423	43	481	1.22	ug/l	88
18) Methyl Acetate	2.752	43	269	0.24	ug/l #	47
20) Methylene Chloride	2.834	84	213	0.28	ug/l #	66
27) cis-1,2-Dichloroethene	4.552	96	459	0.57	ug/l	90
29) Tetrahydrofuran	5.117	42	163	0.42	ug/l #	27
31) Cyclohexane	5.629	56	1765	1.54	ug/l #	32
36) 1,1-Dichloropropene	5.623	75	5507	4.92	ug/l #	50
38) Carbon Tetrachloride	5.629	117	7042	5.85	ug/l #	15
44) Trichloroethene	7.194	130	227	0.27	ug/l	75
67) Ethyl Benzene	10.235	91	24267	5.61	ug/l	100
68) m/p-Xylenes	10.341	106	5299	3.44	ug/l	91
69) o-Xylene	10.682	106	797	0.53	ug/l	75
73) Isopropylbenzene	11.000	105	20719	5.08	ug/l	98
76) 1,2,3-Trichloropropane	11.118	75	35550	26.30	ug/l #	39
78) n-propylbenzene	11.341	91	41572	8.63	ug/l	98
79) 2-Chlorotoluene	11.418	91	1358	0.46	ug/l #	41
80) 1,3,5-Trimethylbenzene	11.488	105	6790	1.95	ug/l	99
81) trans-1,4-Dichloro-2-b...	11.118	75	35550	80.12	ug/l #	12
82) 4-Chlorotoluene	11.418	91	1358	0.39	ug/l #	45
83) tert-Butylbenzene	11.753	119	2725	0.80	ug/l	80
84) 1,2,4-Trimethylbenzene	11.788	105	274528	78.14	ug/l	97
85) sec-Butylbenzene	11.930	105	12010	3.07	ug/l	91
86) p-Isopropyltoluene	12.218	119	5504	1.54	ug/l	94
89) n-Butylbenzene	12.371	91	6586	2.02	ug/l #	71
90) Hexachloroethane	12.571	117	1471	2.29	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	13.000	75	115	2.27	ug/l #	1
95) Naphthalene	13.818	128	19299	5.10	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX032921\
Data File : VX021574.D
Acq On : 29 Mar 2021 14:05
Operator : JC/MD
Sample : M1785-15 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-4

Quant Time: Mar 30 03:27:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X032421W.M
Quant Title : SW846 8260
QLast Update : Wed Mar 24 12:25:26 2021
Response via : Initial Calibration



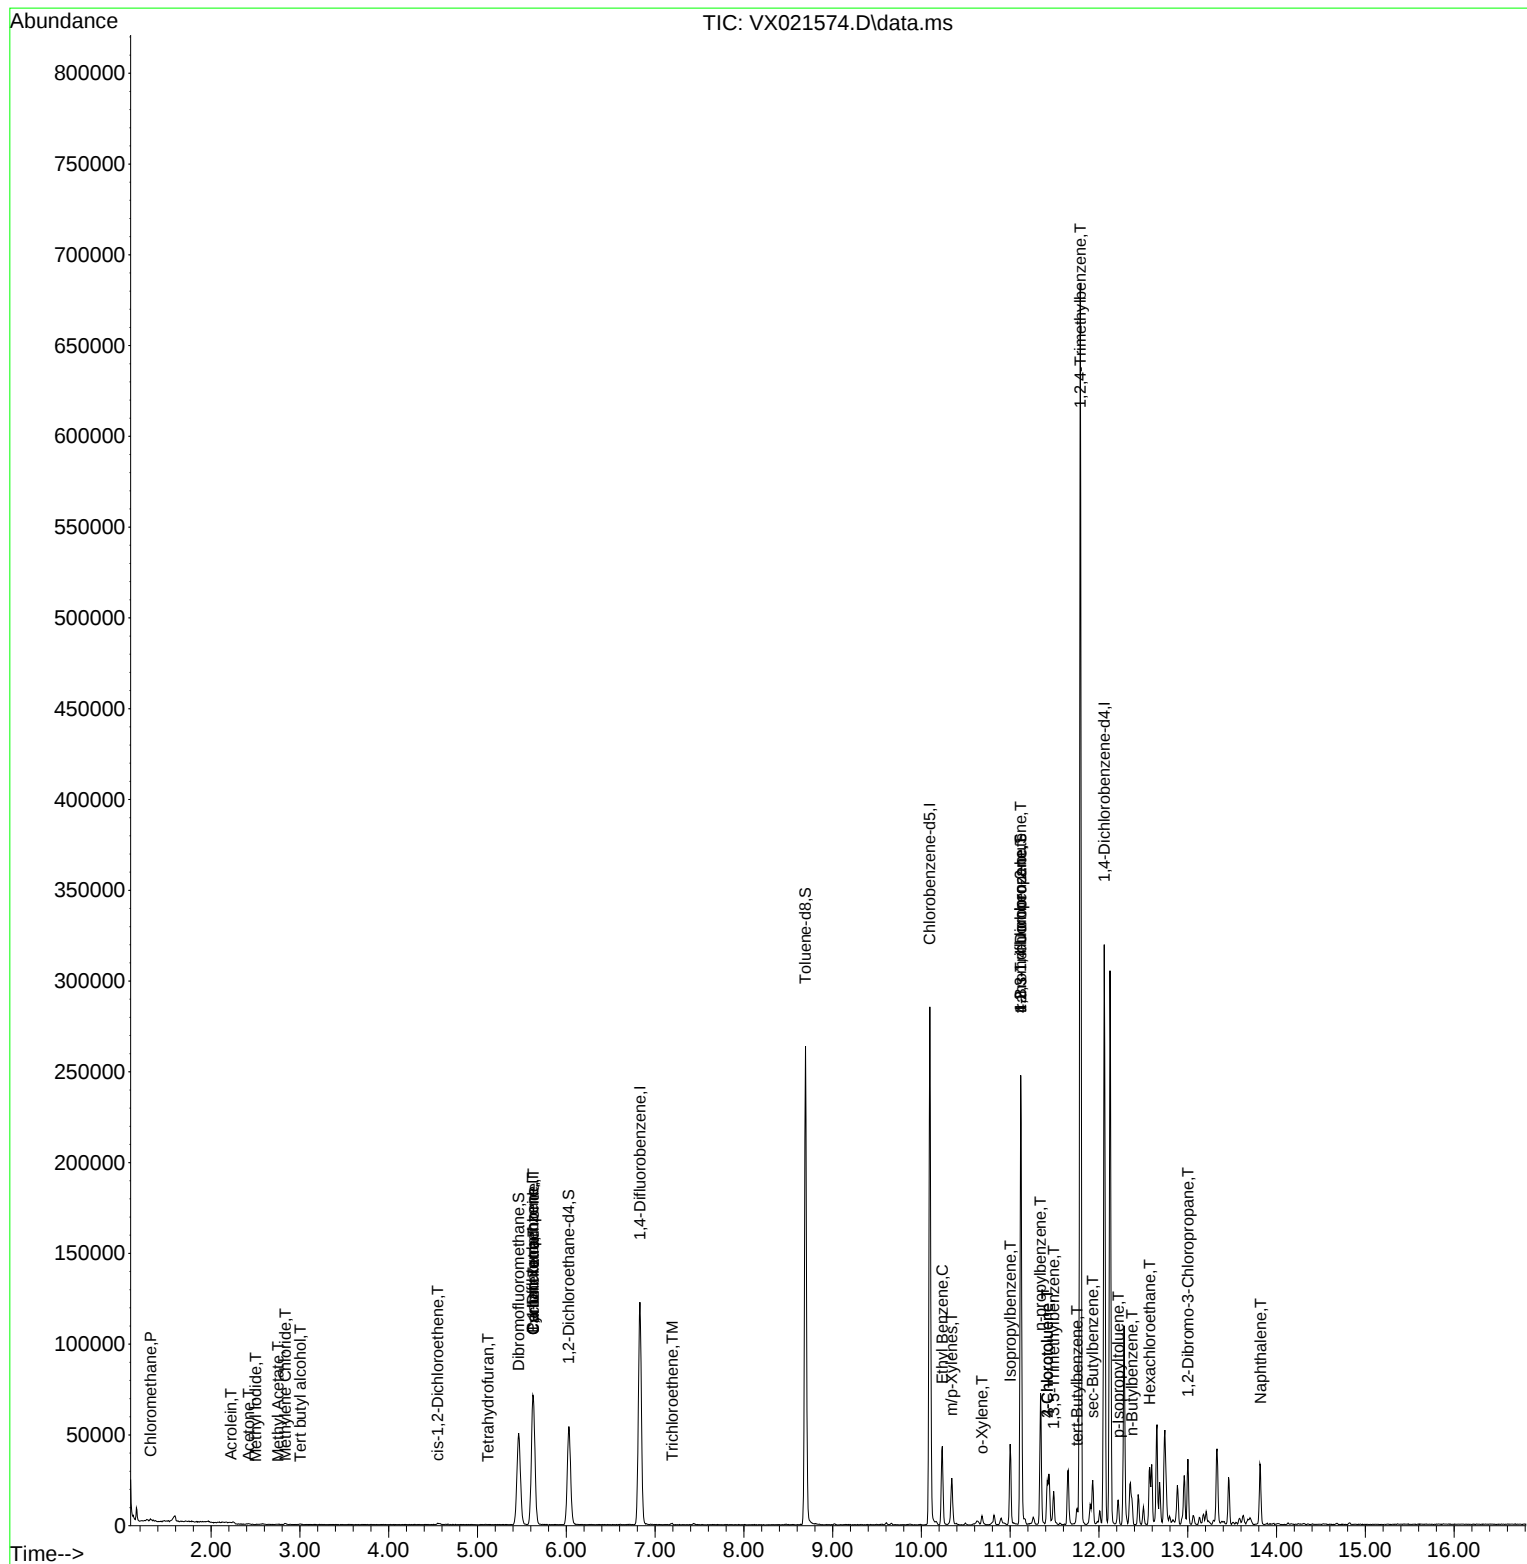




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.623 min Scan# 771
Delta R.T. -0.006 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampleId :
MW-4


Tgt Ion:168 Resp: 62597
Ion Ratio Lower Upper
168 100
99 63.5 45.8 68.6

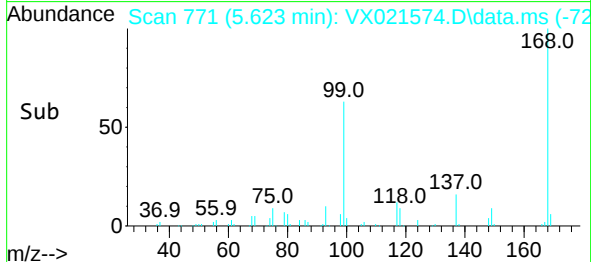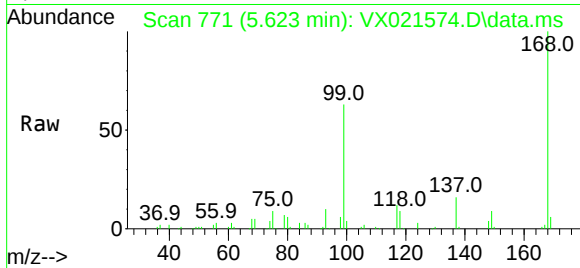

#3
Chloromethane
Concen: 1.78 ug/l
RT: 1.317 min Scan# 39
Delta R.T. 0.006 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion: 50 Resp: 1379
Ion Ratio Lower Upper
50 100
52 28.2 26.4 39.6


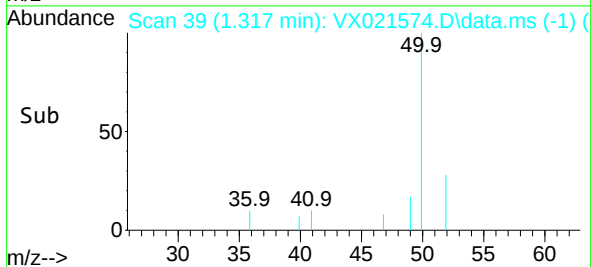

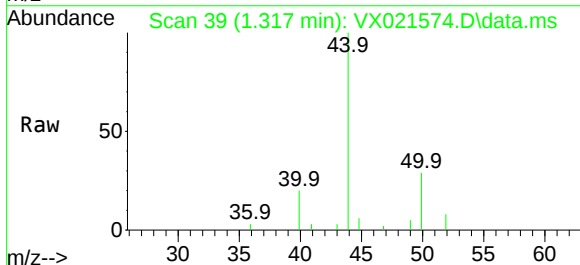


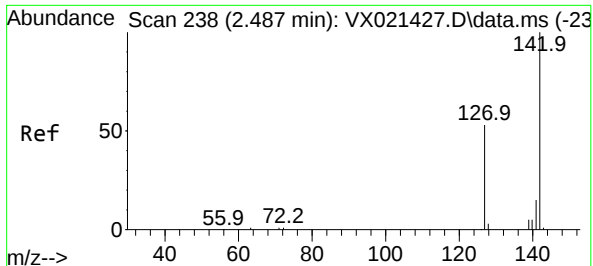

#10
Methyl Iodide
Concen: 6.67 ug/l
RT: 2.499 min Scan# 240
Delta R.T. 0.012 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampleId :
MW-4


Tgt Ion:142 Resp: 18
Ion Ratio Lower Upper
142 100
127 0.0 33.3 49.9#
141 0.0 11.4 17.0#

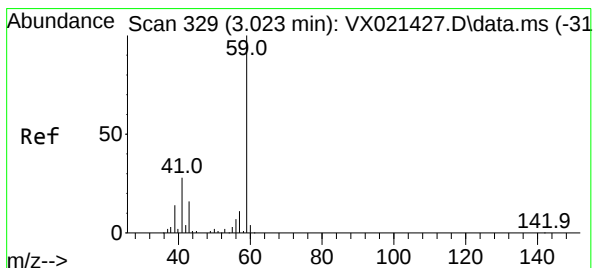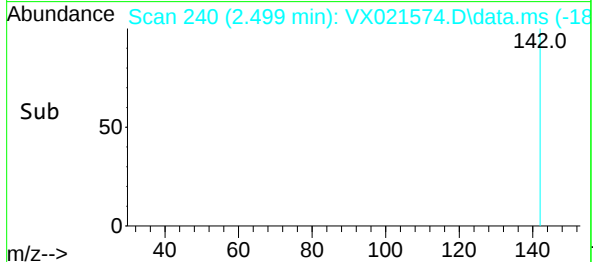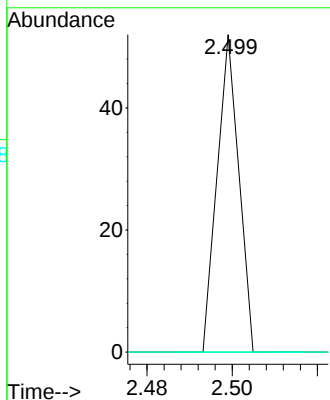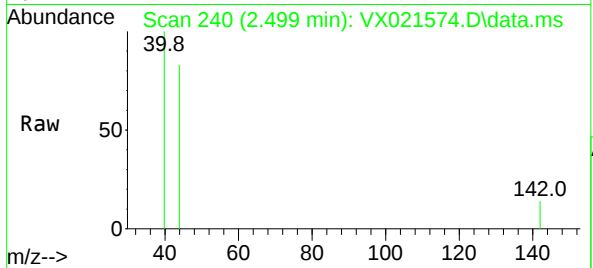

#11
Tert butyl alcohol
Concen: 1.67 ug/l
RT: 3.005 min Scan# 326
Delta R.T. -0.018 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion: 59 Resp: 288
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#


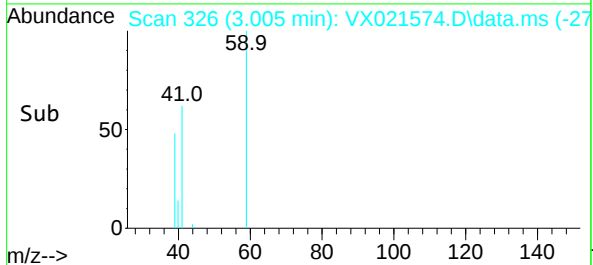
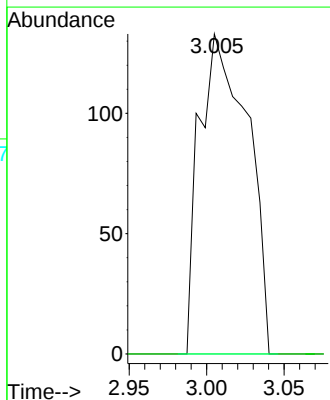
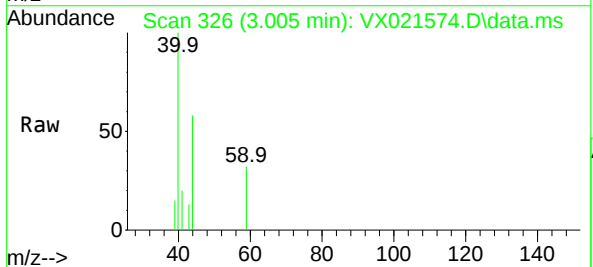


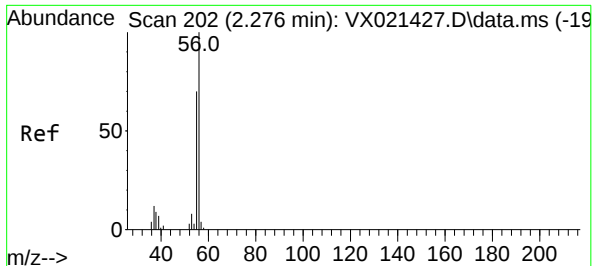

#13
Acrolein
Concen: 4.52 ug/l
RT: 2.223 min Scan# 193
Delta R.T. -0.053 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampleId :
MW-4


Tgt Ion: 56 Resp: 20
Ion Ratio Lower Upper
56 100
55 0.0 56.4 84.6#

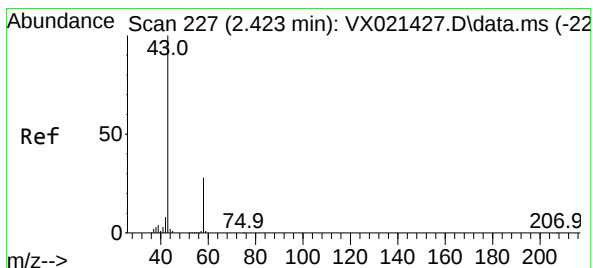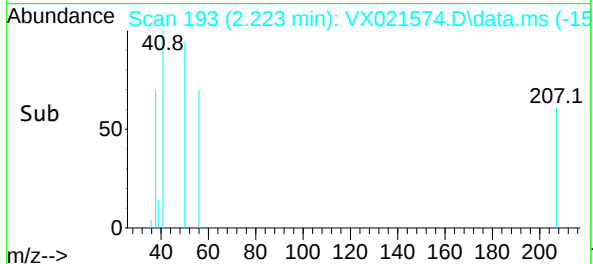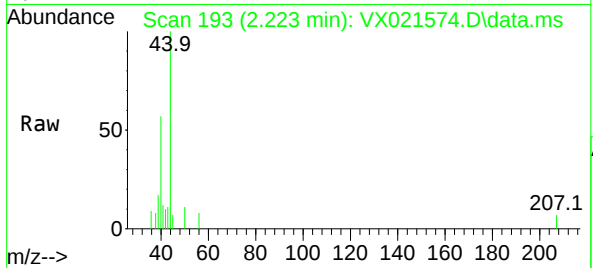

#16
Acetone
Concen: 1.22 ug/l
RT: 2.423 min Scan# 227
Delta R.T. -0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion: 43 Resp: 481
Ion Ratio Lower Upper
43 100
58 27.9 27.8 41.8


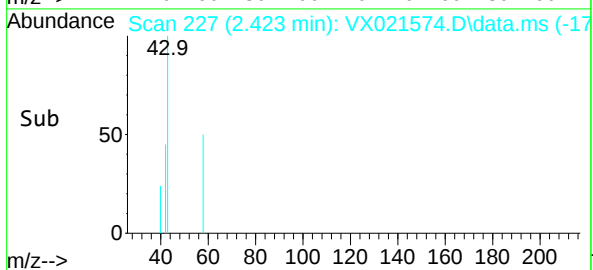

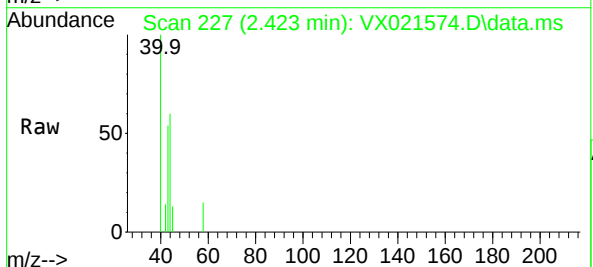


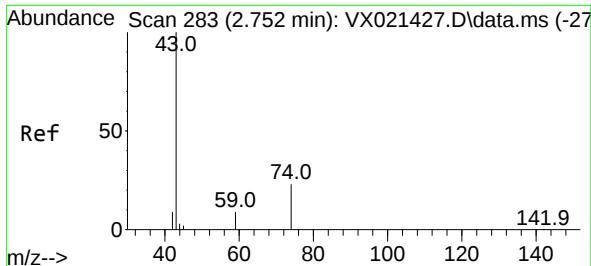

#18
Methyl Acetate
Concen: 0.24 ug/l
RT: 2.752 min Scan# 283
Delta R.T. -0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampled :
MW-4


Tgt Ion: 43 Resp: 269
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

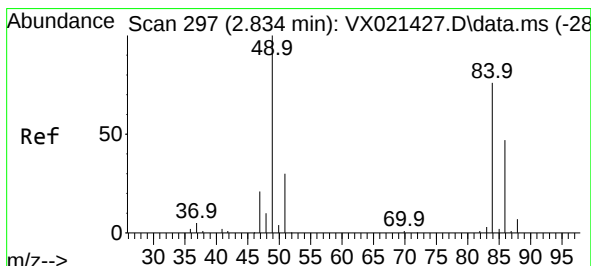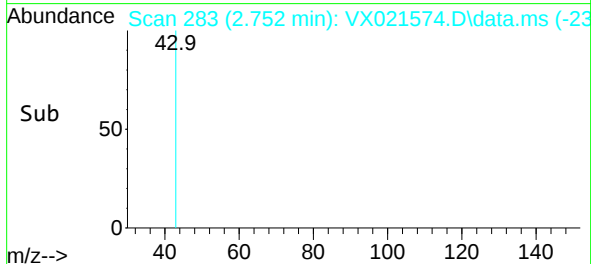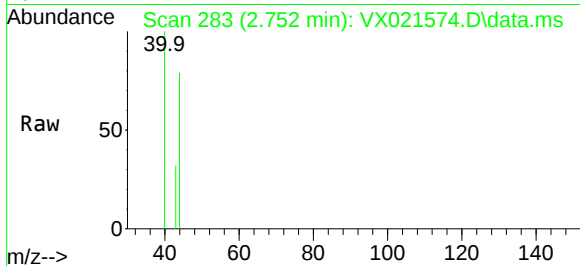

#20
Methylene Chloride
Concen: 0.28 ug/l
RT: 2.834 min Scan# 297
Delta R.T. 0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion: 84 Resp: 213
Ion Ratio Lower Upper
84 100
49 144.4 88.6 132.8#
51 91.7 27.0 40.6#
86 63.2 50.3 75.5

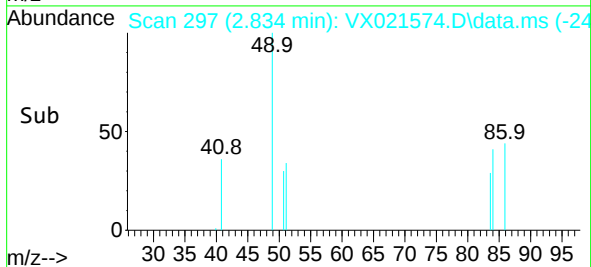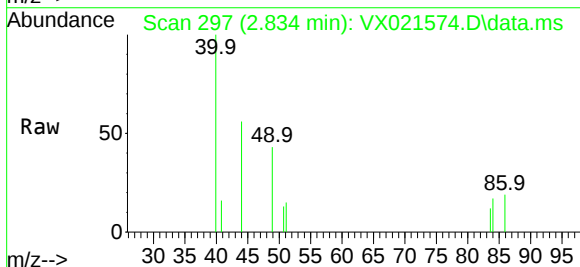



#27

cis-1,2-Dichloroethene

Concen: 0.57 ug/l

RT: 4.552 min Scan# 589

Delta R.T. -0.006 min

Lab File: VX021574.D

Acq: 29 Mar 2021 14:05

Tgt Ion: 96 Resp: 459





Ion	Ratio	Lower	Upper
96	100		
61	153.6	0.0	285.6
98	54.0	0.0	129.6

Instrument :

MSVOA_X

ClientSampled :

MW-4

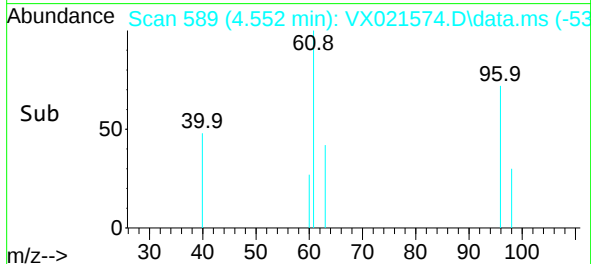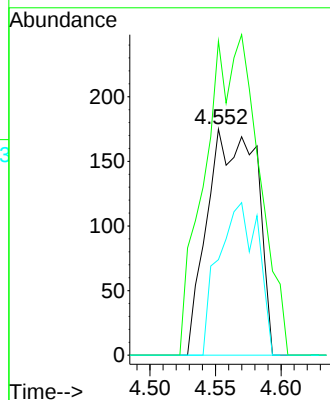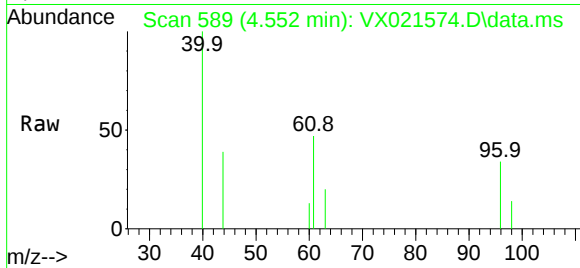

#29

Tetrahydrofuran

Concen: 0.42 ug/l

RT: 5.117 min Scan# 685




Delta R.T. 0.029 min


Lab File: VX021574.D

Acq: 29 Mar 2021 14:05

Tgt Ion: 42 Resp: 163


Ion	Ratio	Lower	Upper
42	100		
72	0.0	41.7	62.5#
71	0.0	38.4	57.6#

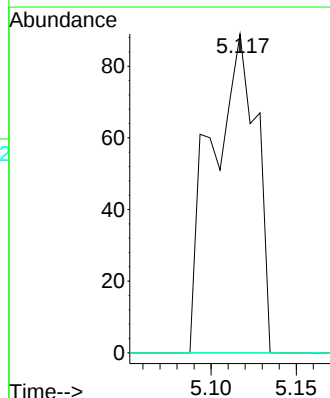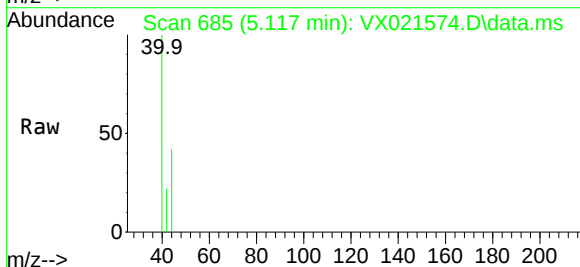



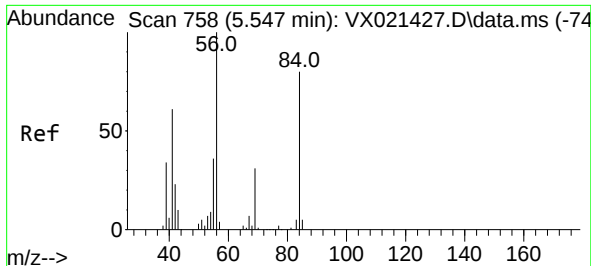


#31
Cyclohexane
Concen: 1.54 ug/l
RT: 5.629 min Scan# 772
Delta R.T. 0.082 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05


Instrument :
MSVOA_X
ClientSampleId :
MW-4

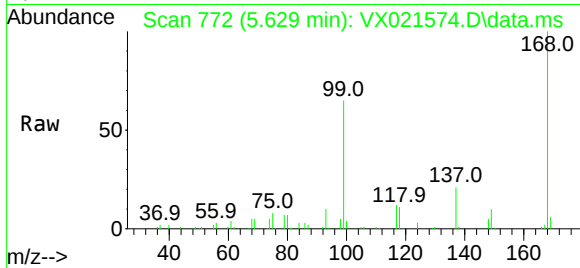



Tgt Ion: 56 Resp: 1765
Ion Ratio Lower Upper
56 100
69 168.3 25.3 37.9#
84 94.0 71.4 107.0

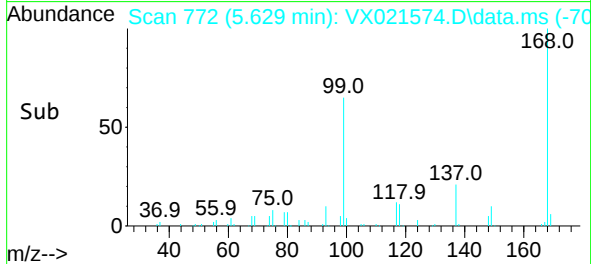


#33
1,2-Dichloroethane-d4
Concen: 51.05 ug/l
RT: 6.029 min Scan# 840
Delta R.T. -0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

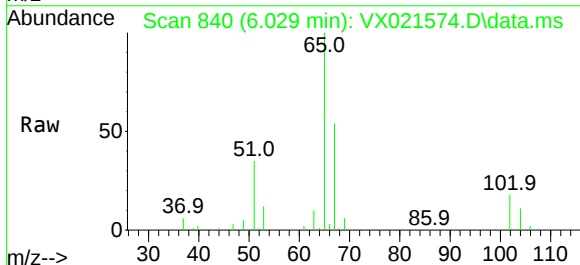

Tgt Ion: 65 Resp: 53166
Ion Ratio Lower Upper
65 100
67 49.9 0.0 105.4




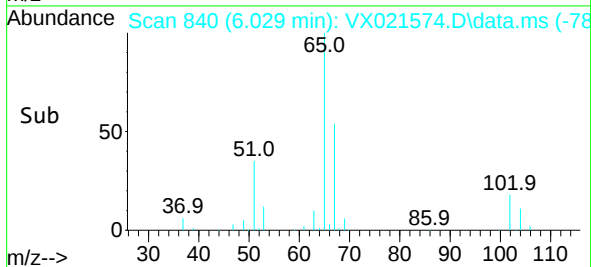


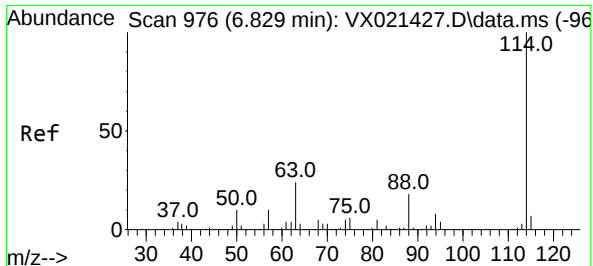

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.829 min Scan# 976
Delta R.T. -0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampleId :
MW-4


Tgt Ion:114 Resp: 114338
Ion Ratio Lower Upper
114 100
63 23.7 0.0 40.8
88 16.8 0.0 32.8

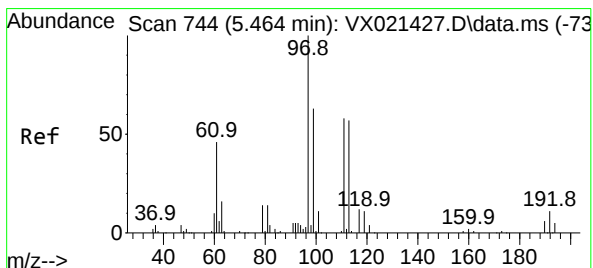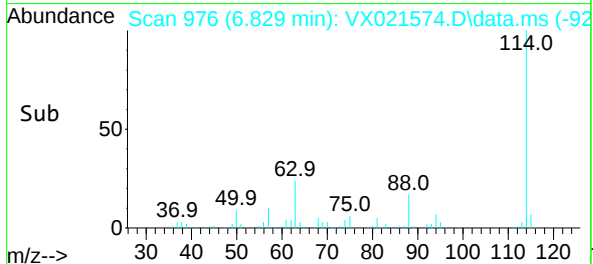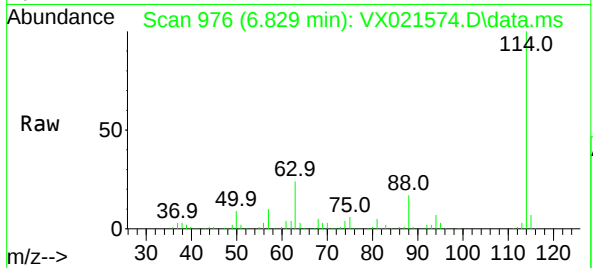

#35
Dibromofluoromethane
Concen: 50.24 ug/l
RT: 5.464 min Scan# 744
Delta R.T. 0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion:113 Resp: 40807
Ion Ratio Lower Upper
113 100
111 103.0 81.9 122.9
192 19.2 16.7 25.1

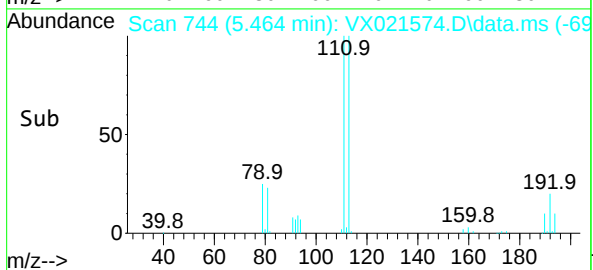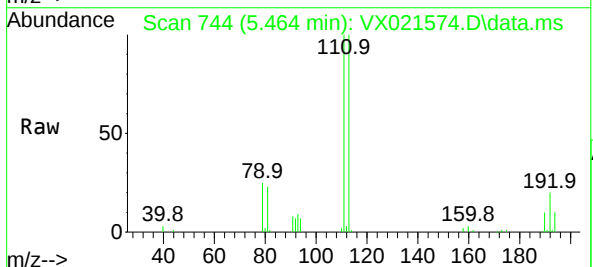




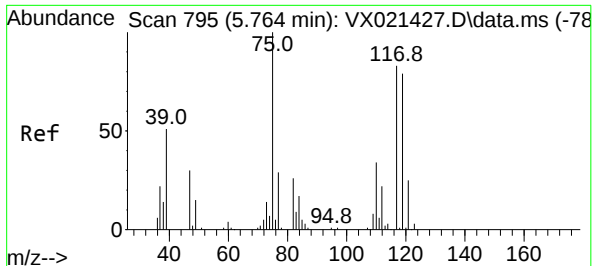


#36

1,1-Dichloropropene
Concen: 4.92 ug/l
RT: 5.623 min Scan# 771
Delta R.T. -0.141 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Instrument :
MSVOA_X
ClientSampleId :
MW-4




Tgt Ion: 75 Resp: 5507
Ion Ratio Lower Upper
75 100
110 10.1 18.1 54.4#
77 0.0 25.3 37.9#

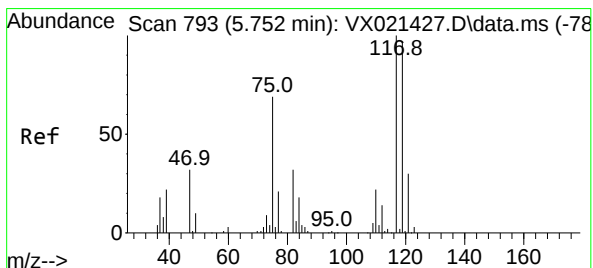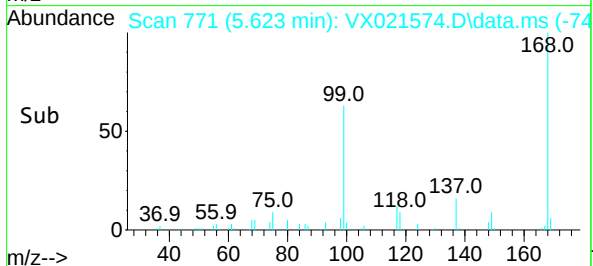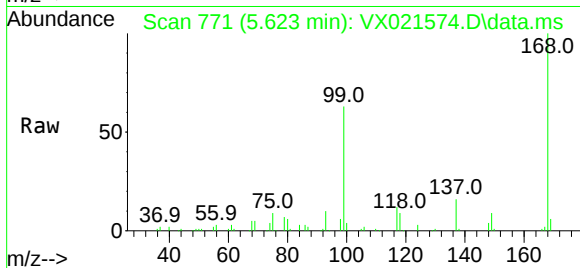


#38

Carbon Tetrachloride
Concen: 5.85 ug/l
RT: 5.629 min Scan# 772
Delta R.T. -0.123 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion: 117 Resp: 7042
Ion Ratio Lower Upper
117 100
119 4.0 76.2 114.2#
121 0.0 24.8 37.2#


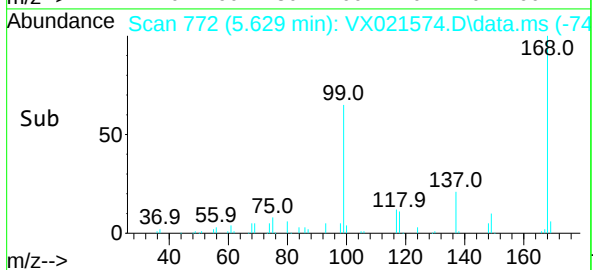

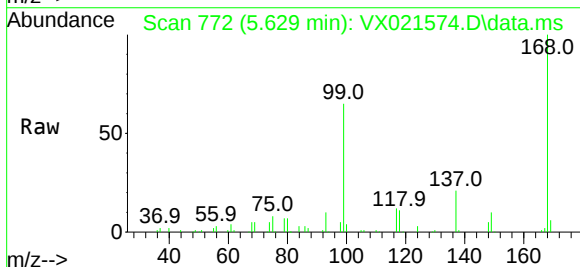


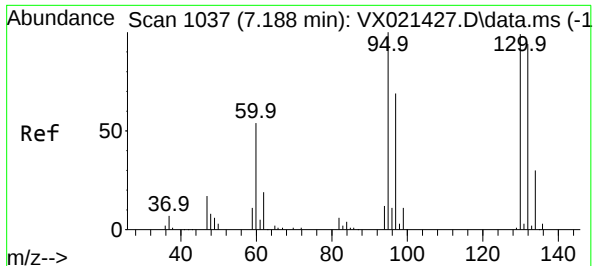

#44
Trichloroethene
Concen: 0.27 ug/l
RT: 7.194 min Scan# 1038
Delta R.T. 0.006 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampleId :
MW-4


Tgt Ion:130 Resp: 227
Ion Ratio Lower Upper
130 100
95 74.1 0.0 198.0

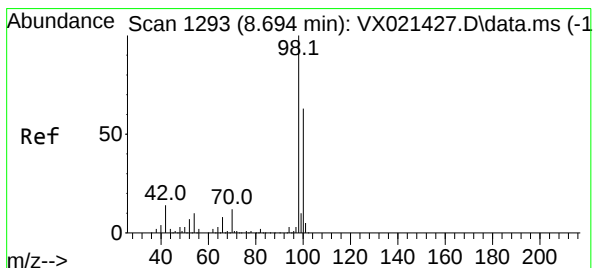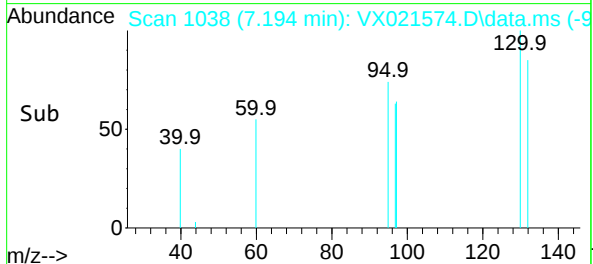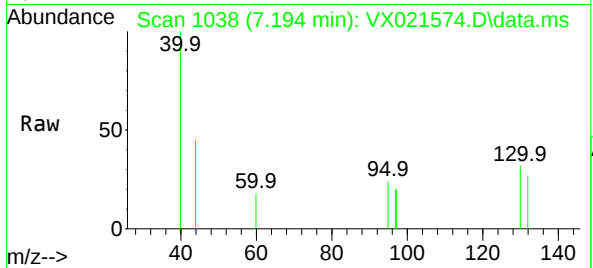

#50
Toluene-d8
Concen: 50.20 ug/l
RT: 8.694 min Scan# 1293
Delta R.T. -0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion: 98 Resp: 145276
Ion Ratio Lower Upper
98 100
100 64.8 51.9 77.9


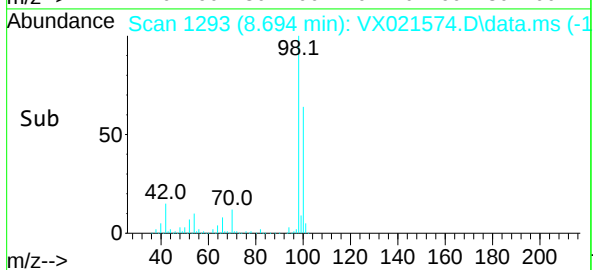

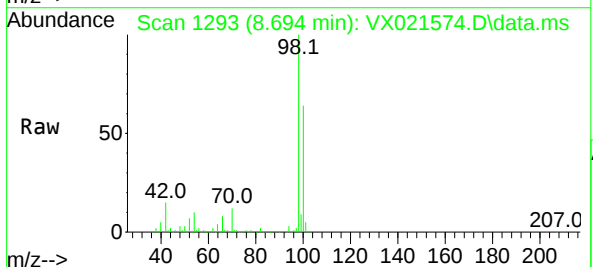


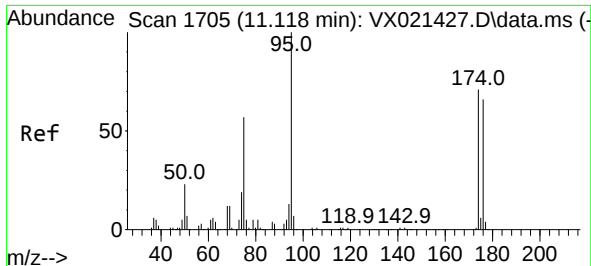

#62
4-Bromofluorobenzene
Concen: 56.13 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. -0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampleId :
MW-4


Tgt Ion:	95	Resp:	63160
Ion	Ratio	Lower	Upper
95	100		
174	74.5	0.0	154.6
176	71.3	0.0	155.8

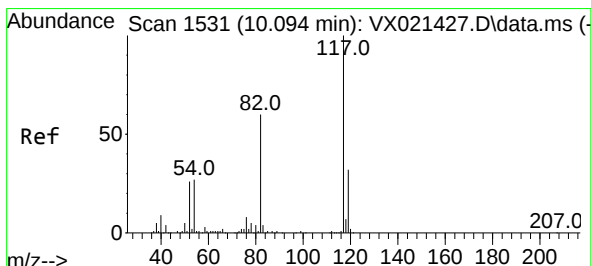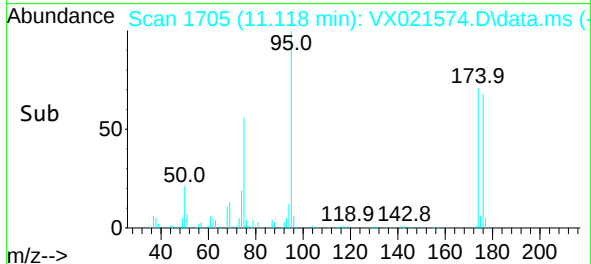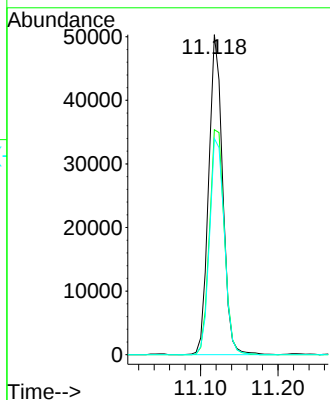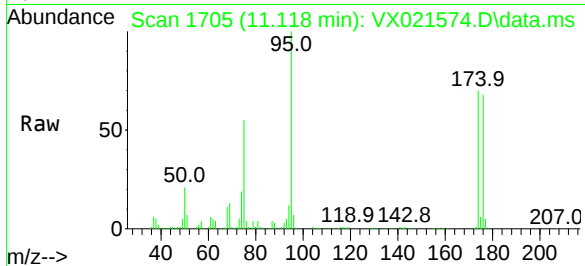

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.094 min Scan# 1531
Delta R.T. 0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion:	117	Resp:	118030
Ion	Ratio	Lower	Upper
117	100		
82	62.4	47.4	71.2
119	33.9	26.6	39.8

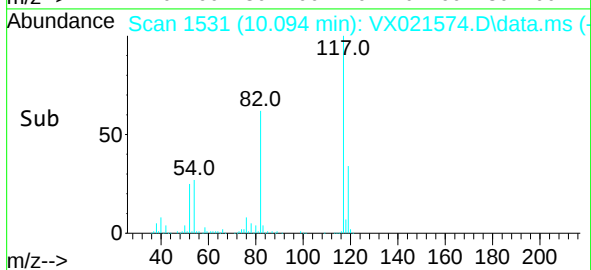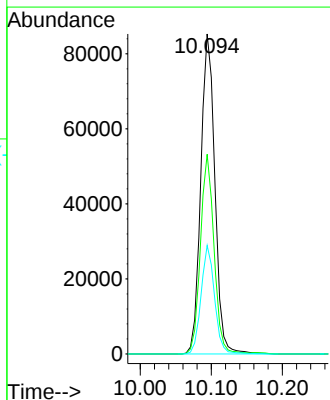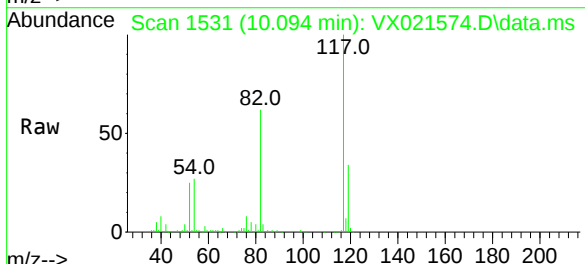



#67

Ethyl Benzene

Concen: 5.61 ug/l

RT: 10.235 min Scan# 1555

Delta R.T. 0.000 min

Lab File: VX021574.D

Acq: 29 Mar 2021 14:05

Tgt Ion: 91 Resp: 24267

Ion Ratio Lower Upper

91 100





106 30.6 24.6 37.0

Instrument :

MSVOA_X

ClientSampled :

MW-4

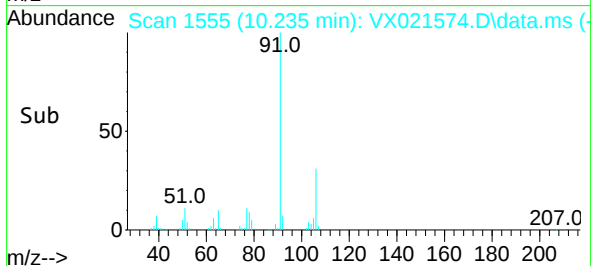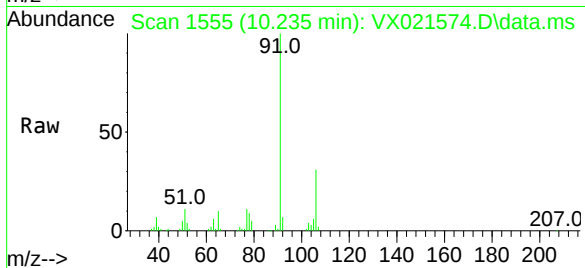

#68

m/p-Xylenes

Concen: 3.44 ug/l

RT: 10.341 min Scan# 1573

Delta R.T. 0.000 min

Lab File: VX021574.D




Acq: 29 Mar 2021 14:05


Tgt Ion:106 Resp: 5299

Ion Ratio Lower Upper

106 100

91 217.1 162.8 244.2


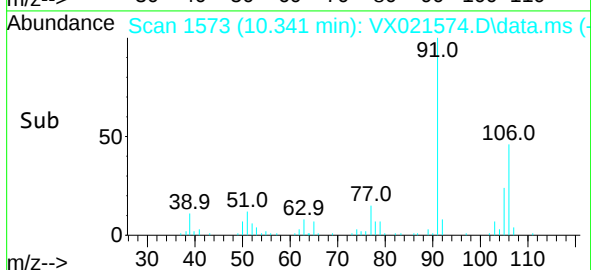

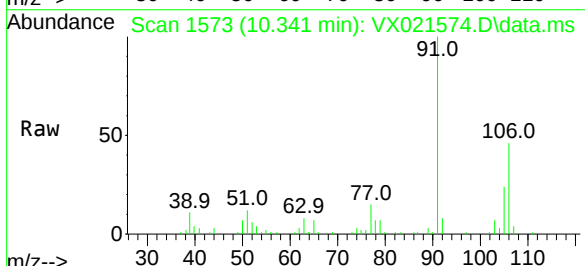


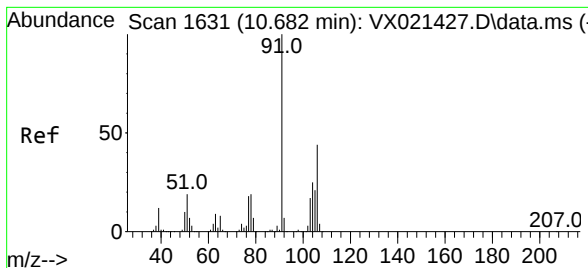

#69
o-Xylene
Concen: 0.53 ug/l
RT: 10.682 min Scan# 1631
Delta R.T. 0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampled :
MW-4


Tgt Ion:106 Resp: 797
Ion Ratio Lower Upper
106 100
91 256.2 108.1 324.2

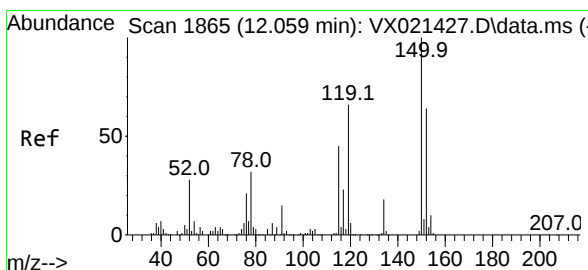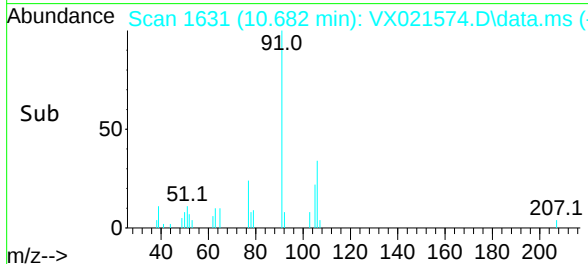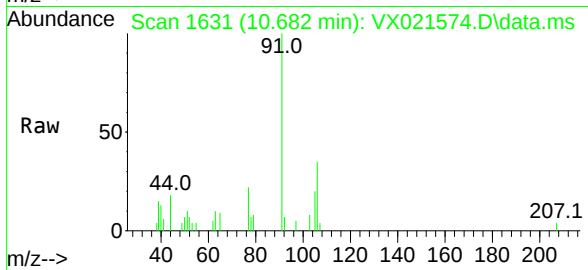

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.059 min Scan# 1865
Delta R.T. 0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion:152 Resp: 58057
Ion Ratio Lower Upper
152 100
115 62.0 41.1 123.3
150 160.0 0.0 349.0

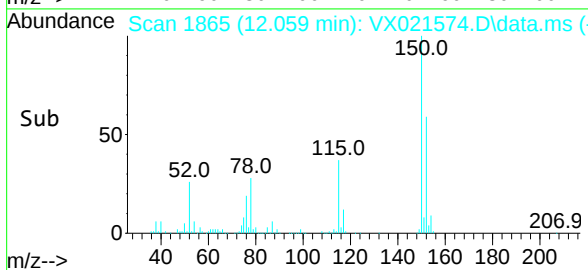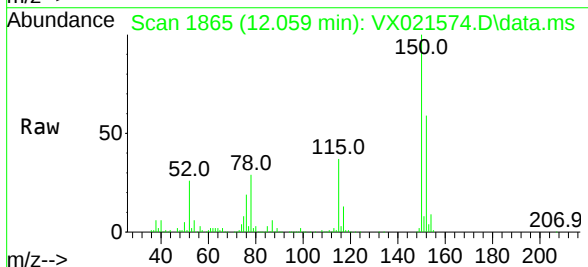



#73

Isopropylbenzene

Concen: 5.08 ug/l

RT: 11.000 min Scan# 1685

Delta R.T. 0.000 min

Lab File: VX021574.D





Acq: 29 Mar 2021 14:05

Tgt Ion:105 Resp: 20719

Ion Ratio Lower Upper

105 100

120 25.6 13.2 39.6

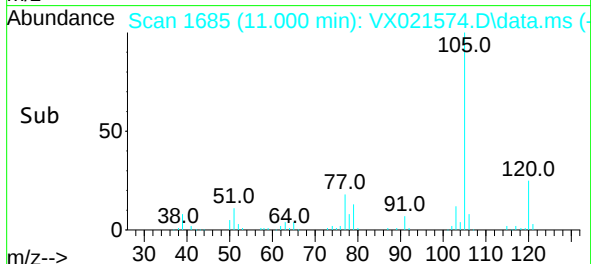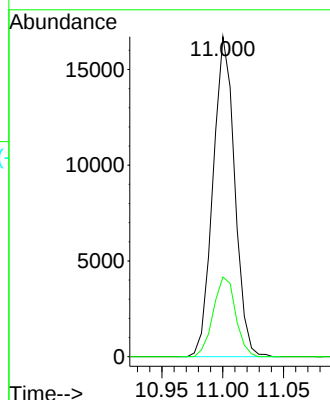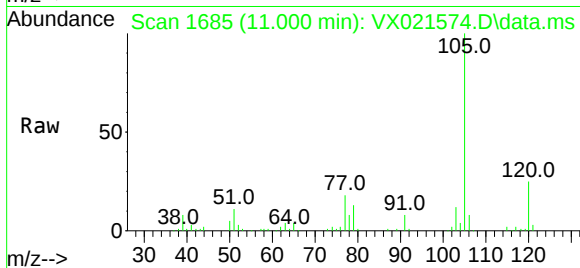

#76

1,2,3-Trichloropropane

Concen: 26.30 ug/l

RT: 11.118 min Scan# 1705

Delta R.T. -0.159 min

Lab File: VX021574.D




Acq: 29 Mar 2021 14:05


Tgt Ion: 75 Resp: 35550

Ion Ratio Lower Upper

75 100

77 1.2 19.1 57.5#


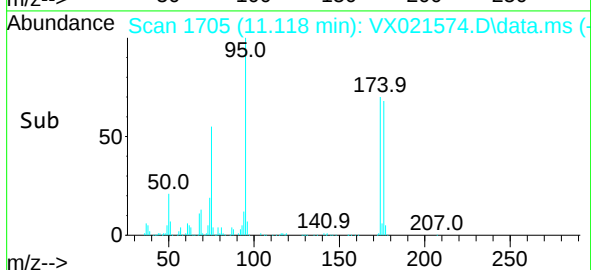
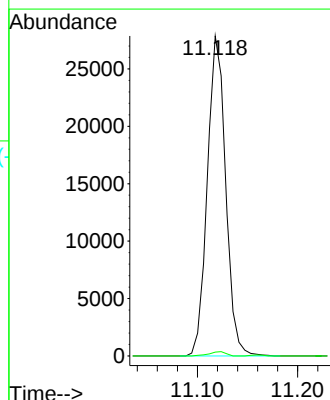
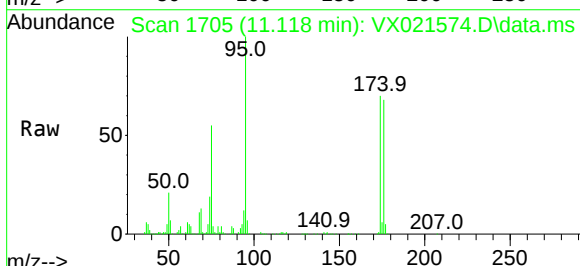


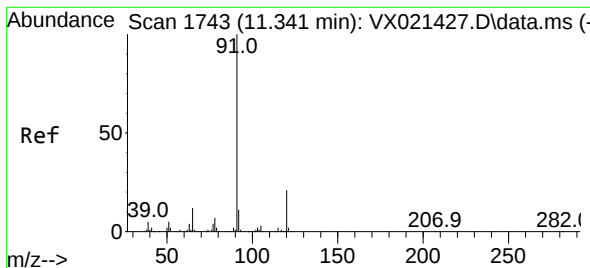

#78
n-propylbenzene
Concen: 8.63 ug/l
RT: 11.341 min Scan# 1743
Delta R.T. 0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampled :
MW-4


Tgt Ion: 91 Resp: 41572
Ion Ratio Lower Upper
91 100
120 22.3 11.5 34.5

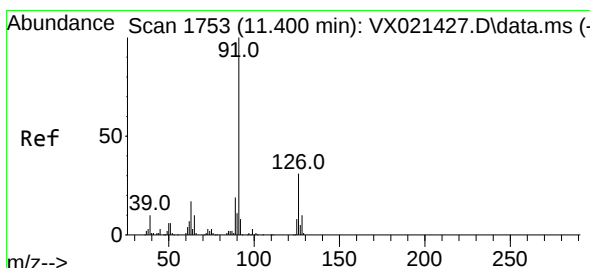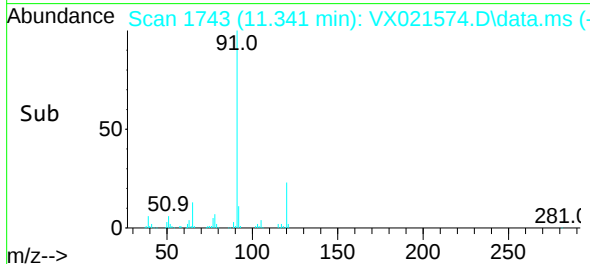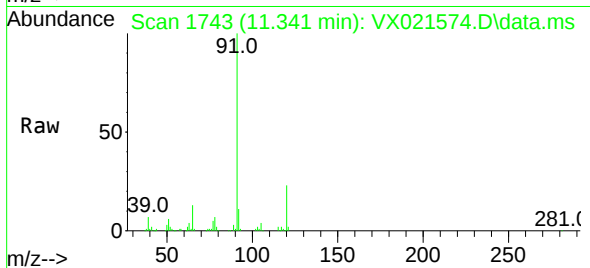

#79
2-Chlorotoluene
Concen: 0.46 ug/l
RT: 11.418 min Scan# 1756
Delta R.T. 0.018 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion: 91 Resp: 1358
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#


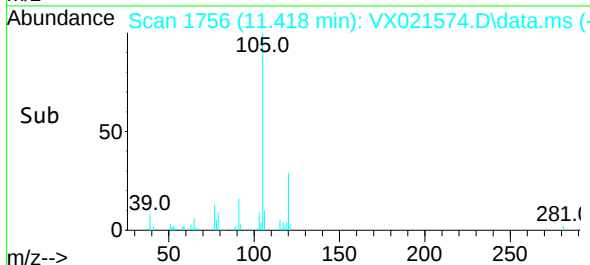

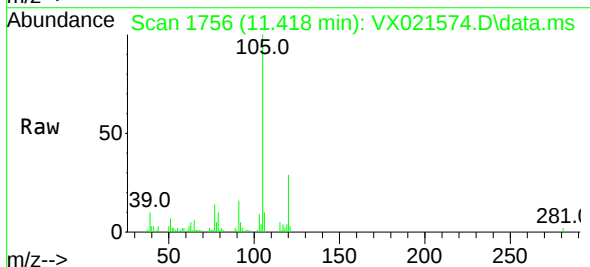


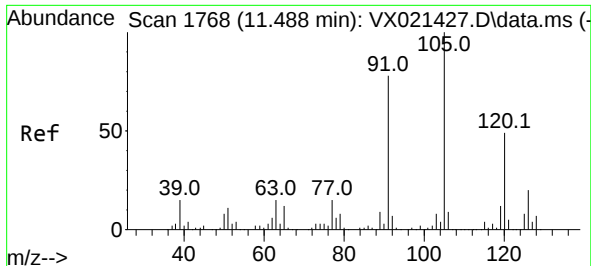

#80
1,3,5-Trimethylbenzene
Concen: 1.95 ug/l
RT: 11.488 min Scan# 1768
Delta R.T. 0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampled :
MW-4


Tgt Ion:105 Resp: 6790
Ion Ratio Lower Upper
105 100
120 47.1 23.8 71.5

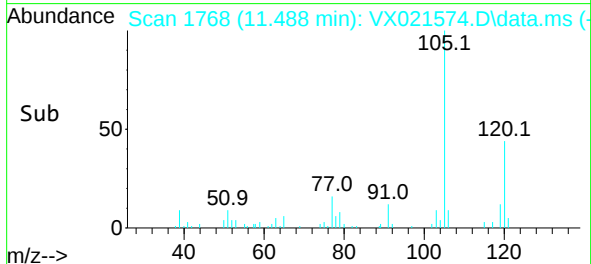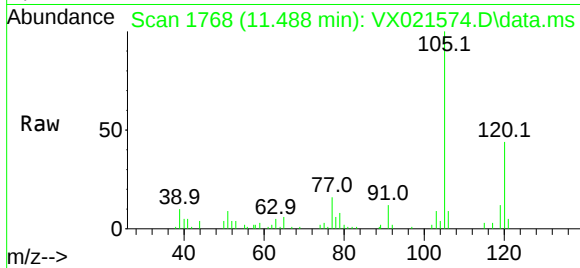

#81
trans-1,4-Dichloro-2-butene
Concen: 80.12 ug/l
RT: 11.118 min Scan# 1705
Delta R.T. 0.059 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion: 75 Resp: 35550
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#


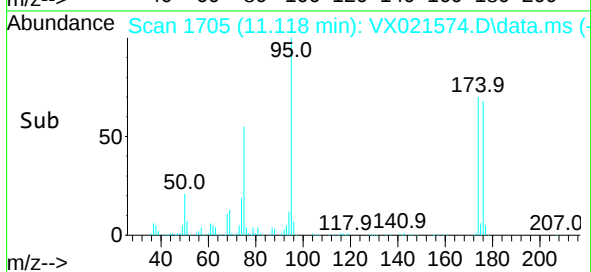

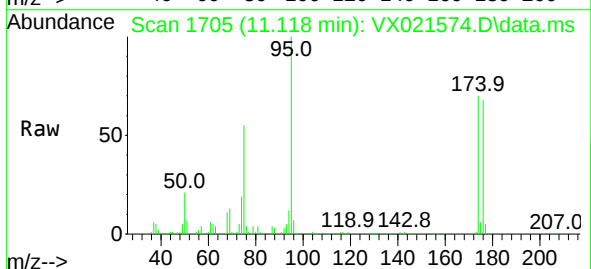




#82
4-Chlorotoluene
Concen: 0.39 ug/l
RT: 11.418 min Scan# 1756
Delta R.T. -0.076 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampled :
MW-4


Tgt Ion: 91 Resp: 1358
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

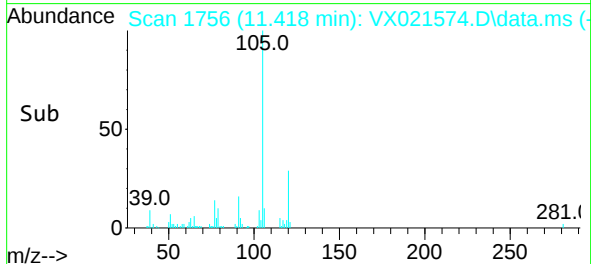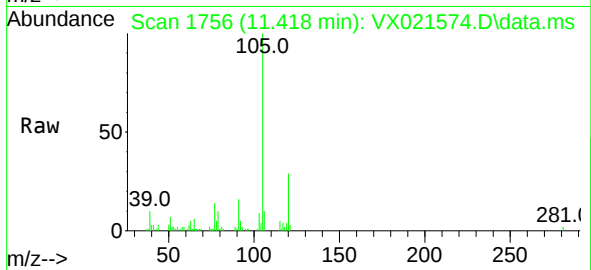

#83
tert-Butylbenzene
Concen: 0.80 ug/l
RT: 11.753 min Scan# 1813
Delta R.T. 0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion: 119 Resp: 2725
Ion Ratio Lower Upper
119 100
91 74.9 27.9 83.7
134 25.0 11.3 33.9

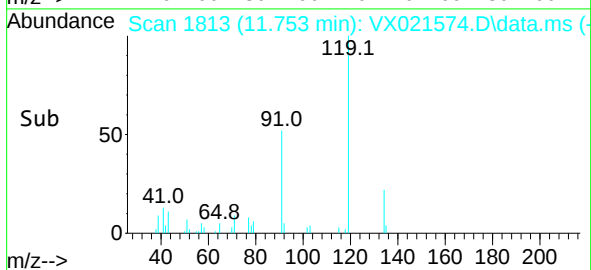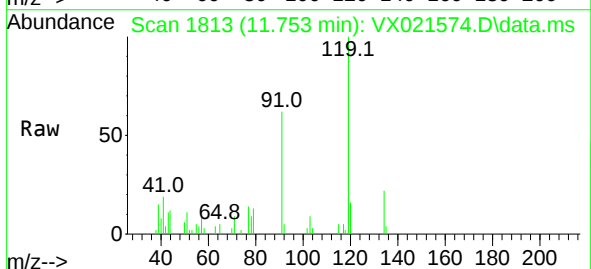



#84

1,2,4-Trimethylbenzene

Concen: 78.14 ug/l

RT: 11.788 min Scan# 1819

Delta R.T. -0.001 min

Lab File: VX021574.D





Acq: 29 Mar 2021 14:05

Tgt Ion:105 Resp: 274528

Ion Ratio Lower Upper

105 100

120 43.1 22.4 67.3

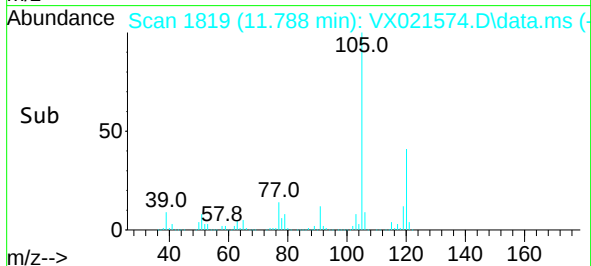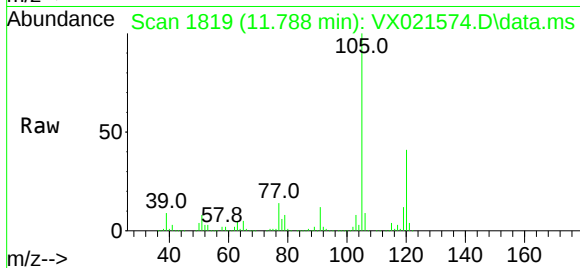

#85

sec-Butylbenzene

Concen: 3.07 ug/l

RT: 11.930 min Scan# 1843

Delta R.T. -0.000 min

Lab File: VX021574.D




Acq: 29 Mar 2021 14:05


Tgt Ion:105 Resp: 12010

Ion Ratio Lower Upper

105 100

134 15.9 10.0 29.8


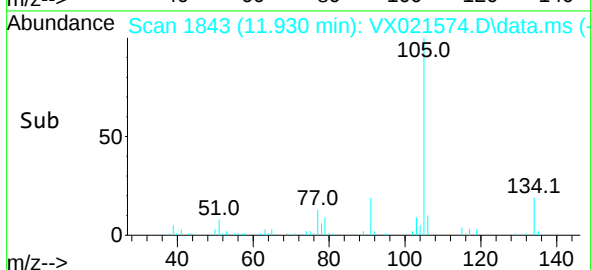

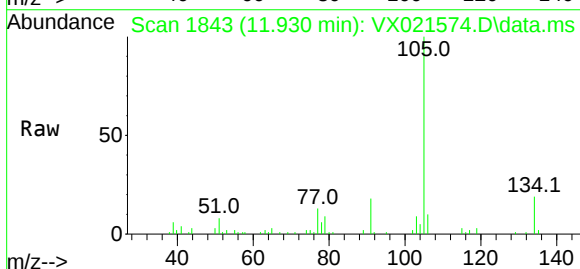


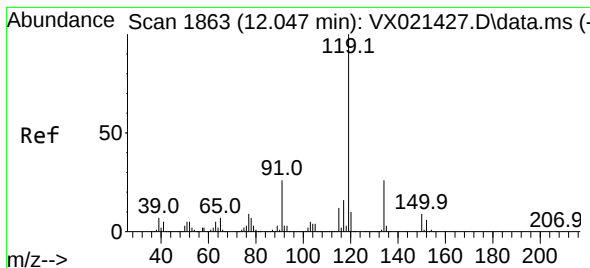

#86
p-Isopropyltoluene
Concen: 1.54 ug/l
RT: 12.218 min Scan# 1892
Delta R.T. 0.171 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampled :
MW-4


Tgt Ion:	119	Resp:	5504
Ion	Ratio	Lower	Upper
119	100		
134	28.2	12.9	38.7
91	26.5	11.7	35.0

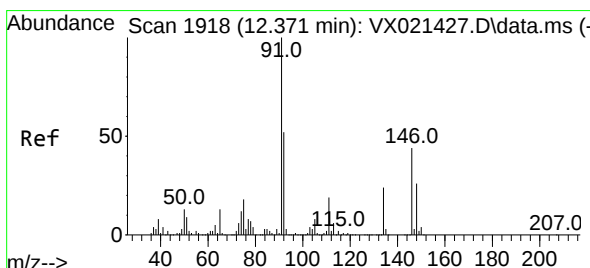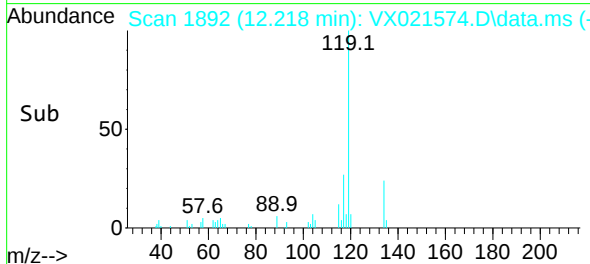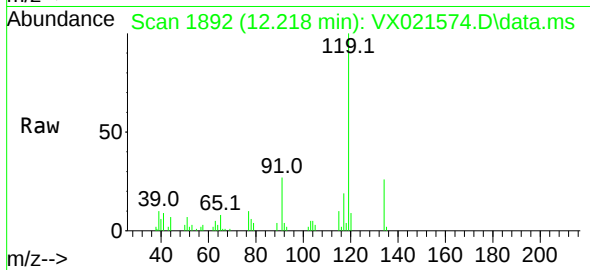

#89
n-Butylbenzene
Concen: 2.02 ug/l
RT: 12.371 min Scan# 1918
Delta R.T. -0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Tgt Ion:	91	Resp:	6586
Ion	Ratio	Lower	Upper
91	100		
92	43.3	27.4	82.0
134	55.0	13.2	39.5#


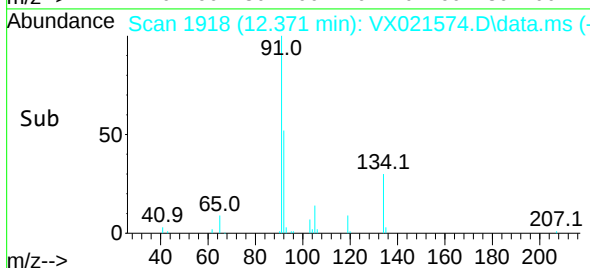

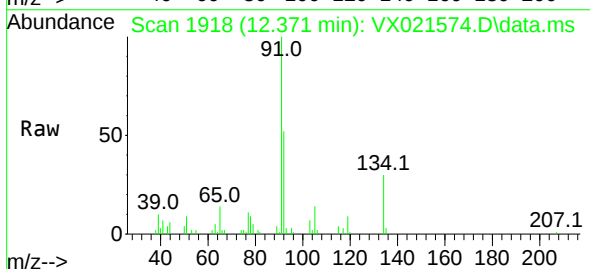




#90
Hexachloroethane
Concen: 2.29 ug/l
RT: 12.571 min Scan# 1952
Delta R.T. -0.006 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05




Instrument :
MSVOA_X
ClientSampled :
MW-4


Tgt Ion:117 Resp: 1471
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

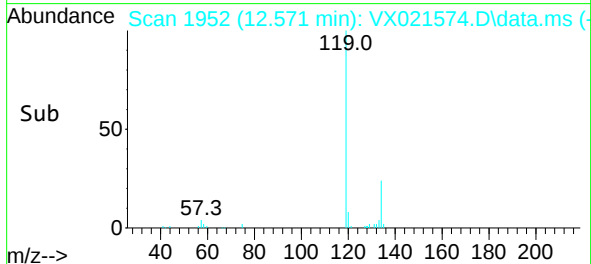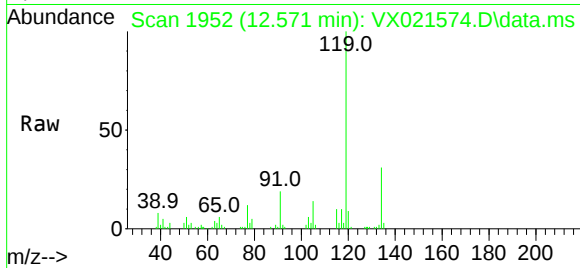

#92
1,2-Dibromo-3-Chloropropane
Concen: 2.27 ug/l
RT: 13.000 min Scan# 2025
Delta R.T. 0.017 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05


Tgt Ion: 75 Resp: 115
Ion Ratio Lower Upper
75 100
155 0.0 45.3 135.9#
157 0.0 57.7 173.1#

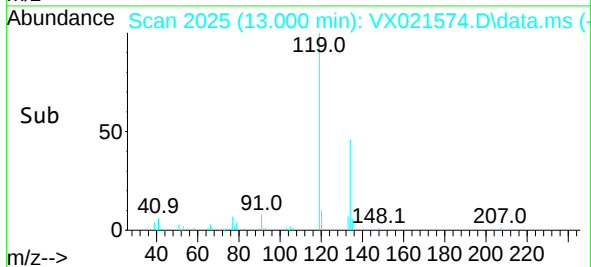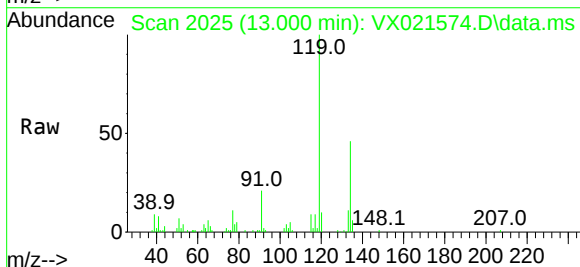

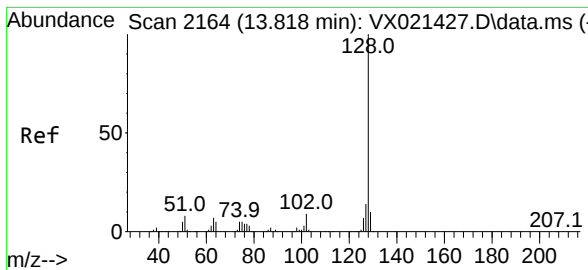

#95
Naphthalene
Concen: 5.10 ug/l
RT: 13.818 min Scan# 2164
Delta R.T. 0.000 min
Lab File: VX021574.D
Acq: 29 Mar 2021 14:05

Instrument :
MSVOA_X
ClientSampleId :
MW-4

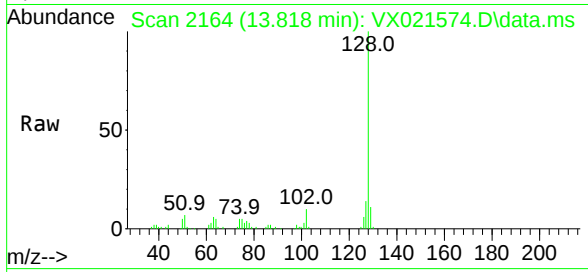

Tgt Ion:	128	Resp:	19299
Ion	Ratio	Lower	Upper
128	100		
127	13.7	10.3	15.5
129	11.1	8.8	13.2

