

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120822\
 Data File : BN023093.D
 Acq On : 08 Dec 2022 14:00
 Operator : CG/JU
 Sample : SSTDICC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Quant Time: Dec 09 07:27:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 09 07:25:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.020	152	9714	0.400	ng	0.00
7) Naphthalene-d8	10.839	136	29087	0.400	ng	# 0.00
13) Acenaphthene-d10	14.666	164	16291	0.400	ng	0.00
19) Phenanthrene-d10	17.414	188	36859	0.400	ng	0.00
29) Chrysene-d12	21.593	240	29376	0.400	ng	# 0.00
35) Perylene-d12	24.060	264	26107	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.550	112	1863	0.083	ng	0.00
5) Phenol-d6	7.168	99	2237	0.079	ng	0.00
8) Nitrobenzene-d5	9.174	82	1799	0.082	ng	-0.01
11) 2-Methylnaphthalene-d10	12.423	152	4254	0.077	ng	0.00
14) 2,4,6-Tribromophenol	16.148	330	489	0.071	ng	0.00
15) 2-Fluorobiphenyl	13.287	172	6390	0.088	ng	-0.01
27) Fluoranthene-d10	19.439	212	7606	0.075	ng	0.00
31) Terphenyl-d14	20.035	244	4494	0.081	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.398	88	955	0.079	ng	98
3) n-Nitrosodimethylamine	3.745	42	772	0.066	ng	96
6) bis(2-Chloroethyl)ether	7.435	93	2688	0.086	ng	98
9) Naphthalene	10.882	128	7179	0.083	ng	97
10) Hexachlorobutadiene	11.181	225	1383	0.085	ng	# 99
12) 2-Methylnaphthalene	12.113	142	983	0.074	ng	# 77
16) Acenaphthylene	14.388	152	5509	0.072	ng	100
17) Acenaphthene	14.730	154	4487	0.080	ng	99
18) Fluorene	15.703	166	4794	0.077	ng	99
21) 4-Bromophenyl-phenylether	16.595	248	1805	0.081	ng	99
22) Hexachlorobenzene	16.719	284	2356	0.082	ng	98
23) Atrazine	16.868	200	1151	0.071	ng	# 96
24) Pentachlorophenol	17.054	266	861	0.102	ng	98
25) Phenanthrene	17.451	178	10530	0.085	ng	99
26) Anthracene	17.538	178	7515	0.075	ng	100
28) Fluoranthene	19.468	202	10024	0.074	ng	100
30) Pyrene	19.831	202	10098	0.082	ng	100
32) Benzo(a)anthracene	21.584	228	8542	0.079	ng	99
33) Chrysene	21.638	228	10544	0.087	ng	99
34) Bis(2-ethylhexyl)phtha...	21.504	149	3706	0.079	ng	98
36) Indeno(1,2,3-cd)pyrene	26.630	276	9677	0.070	ng	# 82
37) Benzo(b)fluoranthene	23.306	252	8869	0.074	ng	# 85
38) Benzo(k)fluoranthene	23.355	252	8393	0.069	ng	# 87
39) Benzo(a)pyrene	23.949	252	7407	0.077	ng	# 77
40) Dibenzo(a,h)anthracene	26.656	278	7491	0.068	ng	94
41) Benzo(g,h,i)perylene	27.425	276	7959	0.071	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120822\
Data File : BN023093.D
Acq On : 08 Dec 2022 14:00
Operator : CG/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Quant Time: Dec 09 07:27:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 07:25:53 2022
Response via : Initial Calibration




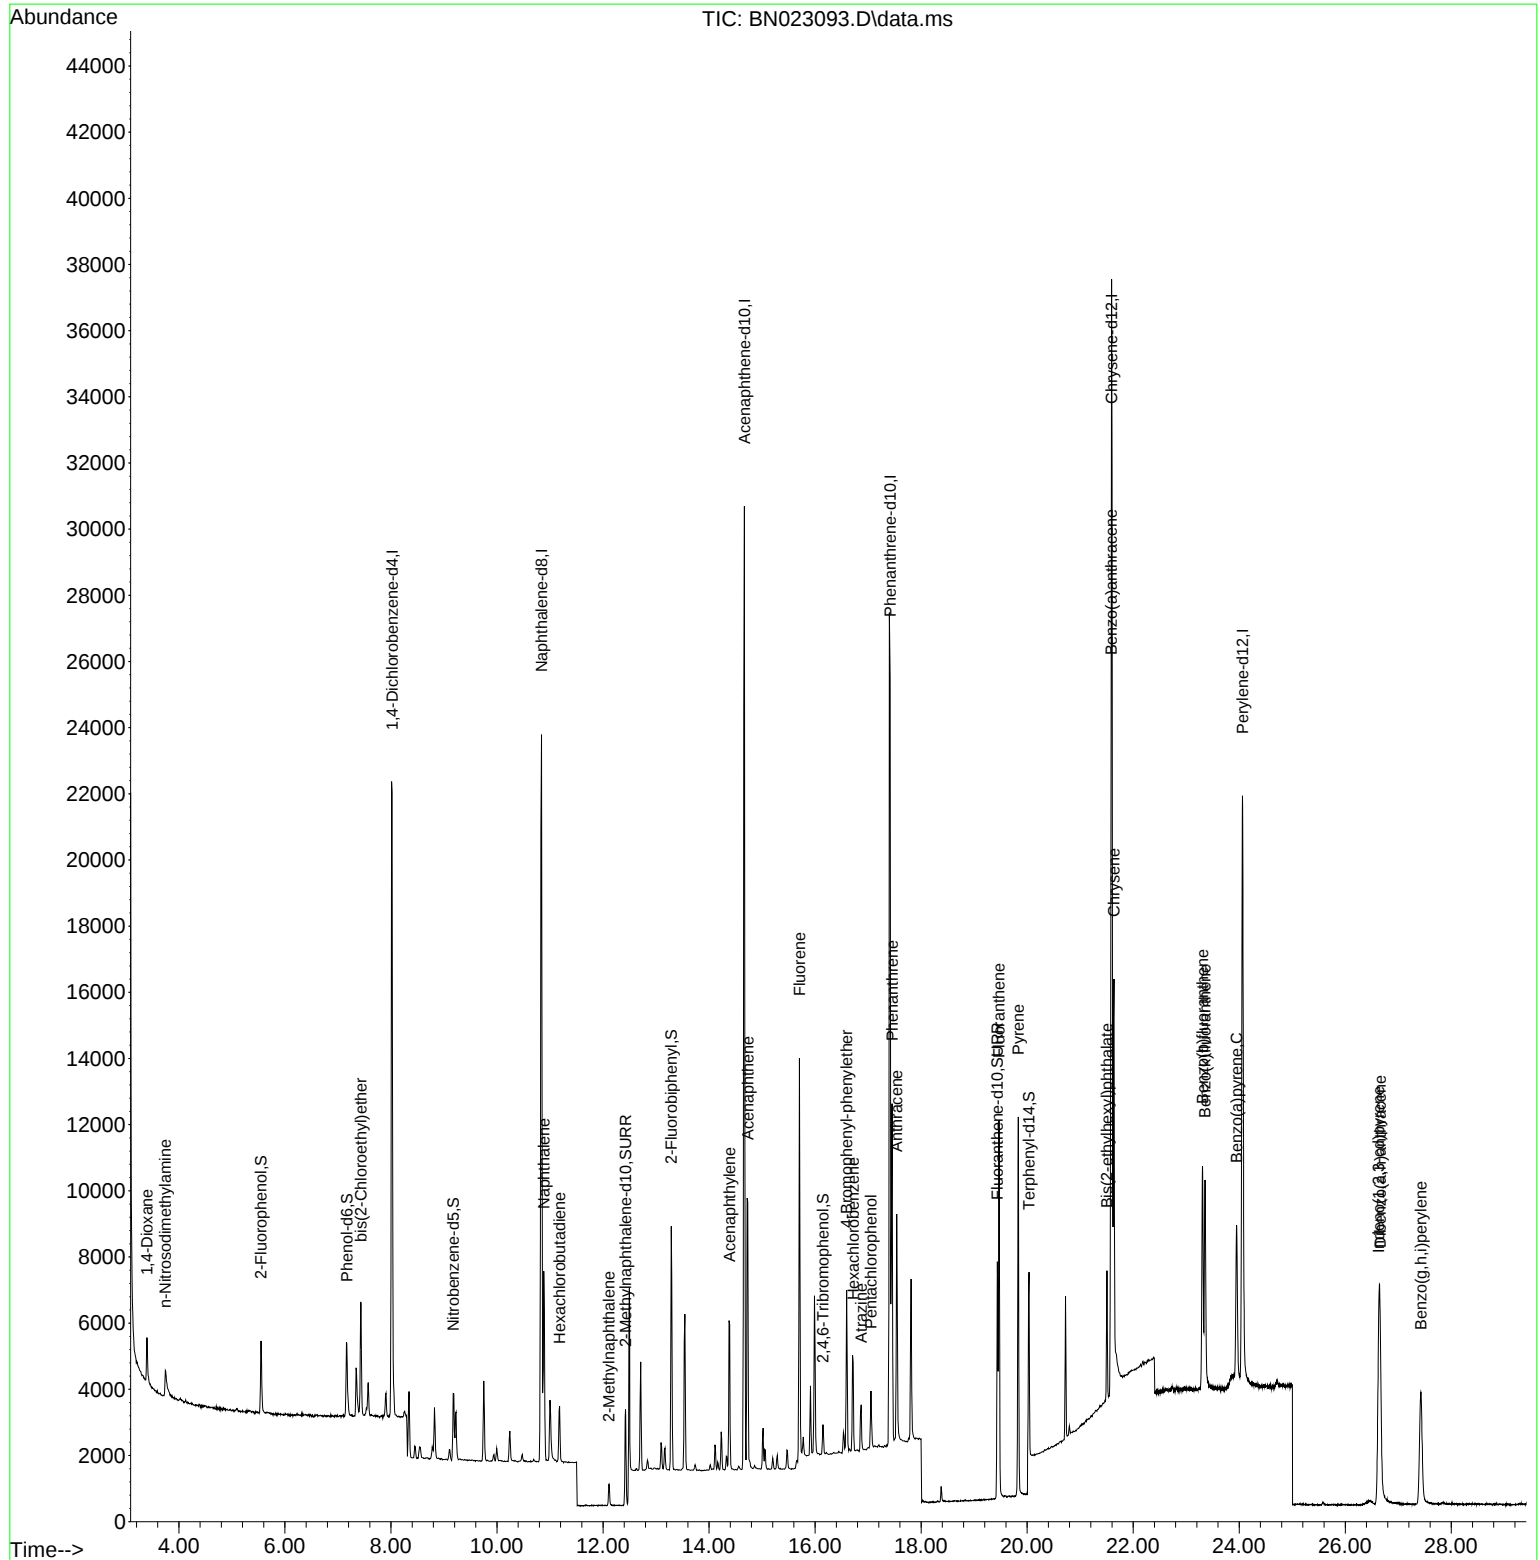




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 8.020 min Scan# 684
 Delta R.T. 0.000 min
 Lab File: BN023093.D
 Acq: 08 Dec 2022 14:00




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:152 Resp: 9714
 Ion Ratio Lower Upper
 152 100
 150 152.5 125.6 188.4
 115 57.6 49.0 73.4

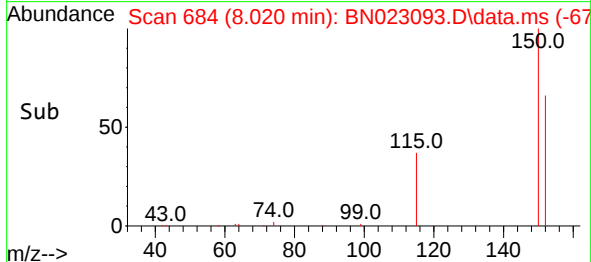

#2
 1,4-Dioxane
 Concen: 0.079 ng
 RT: 3.398 min Scan# 44
 Delta R.T. -0.000 min
 Lab File: BN023093.D
 Acq: 08 Dec 2022 14:00

Tgt Ion: 88 Resp: 955
 Ion Ratio Lower Upper
 88 100
 43 31.8 23.3 34.9
 58 72.9 58.0 87.0

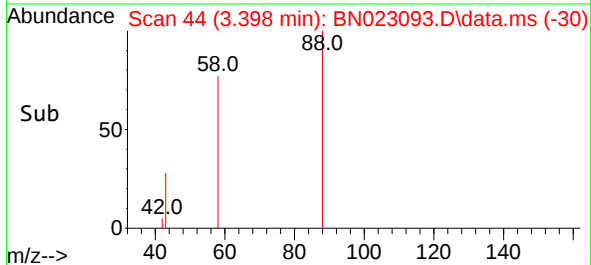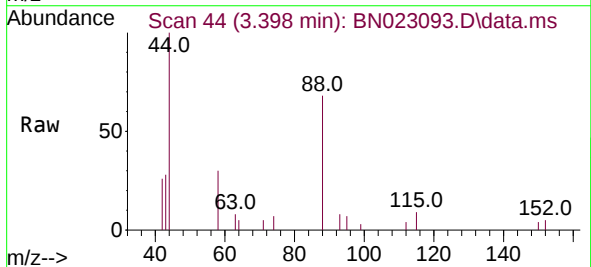




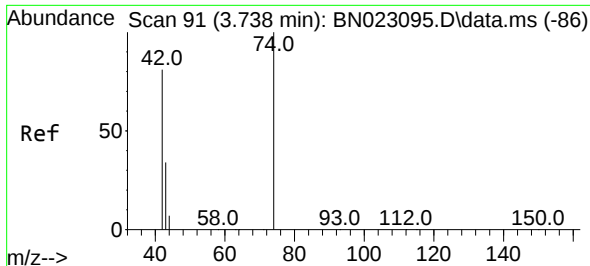


#3
 n-Nitrosodimethylamine
 Concen: 0.066 ng
 RT: 3.745 min Scan# 91
 Delta R.T. 0.007 min
 Lab File: BN023093.D
 Acq: 08 Dec 2022 14:00

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1

Tgt Ion: 42 Resp: 772




Ion	Ratio	Lower	Upper
42	100		
74	124.9	95.8	143.6
44	10.5	8.4	12.6

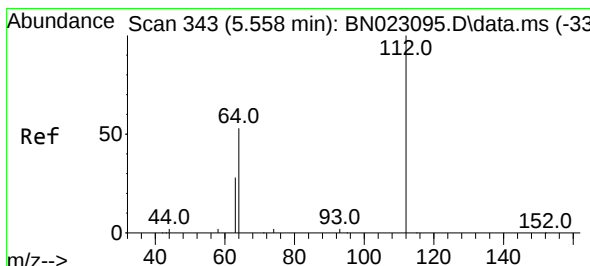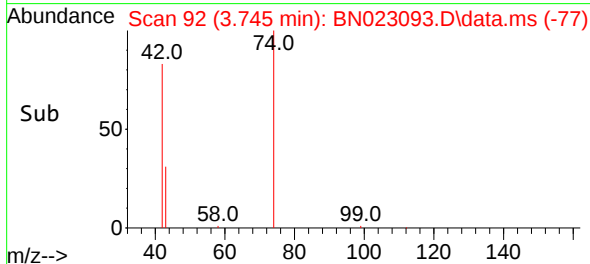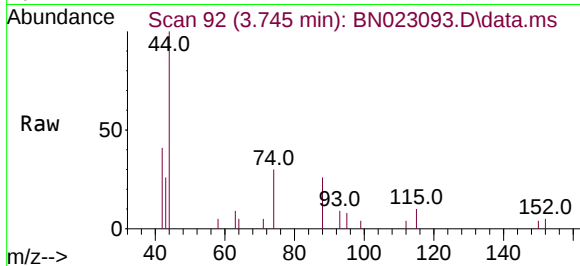


#4
 2-Fluorophenol
 Concen: 0.083 ng
 RT: 5.550 min Scan# 342
 Delta R.T. -0.007 min
 Lab File: BN023093.D
 Acq: 08 Dec 2022 14:00

Tgt Ion: 112 Resp: 1863

Ion	Ratio	Lower	Upper
112	100		
64	56.0	44.4	66.6
63	30.5	23.7	35.5


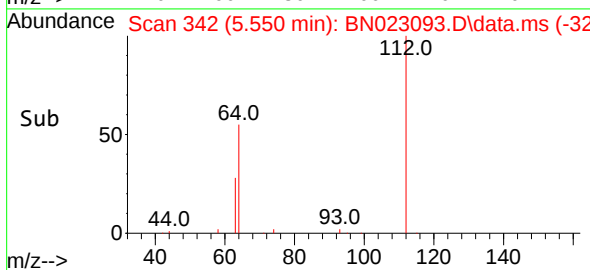

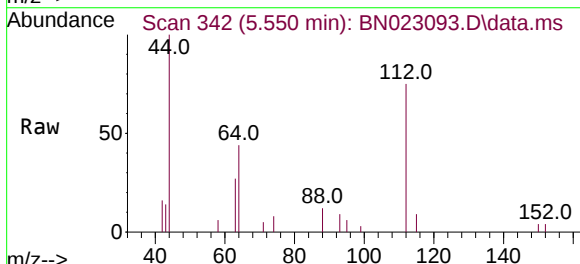




#5
Phenol-d6
Concen: 0.079 ng
RT: 7.168 min Scan# 566
Delta R.T. -0.000 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	99	Resp:	2237
Ion	Ratio	Lower	Upper
99	100		
42	20.8	16.3	24.5
71	32.1	26.5	39.7

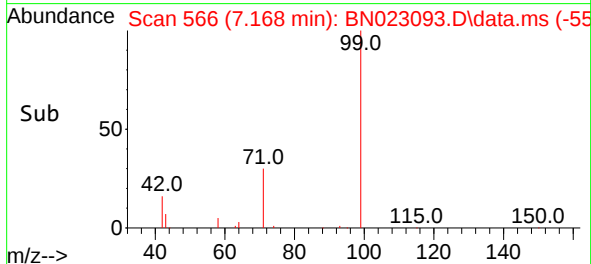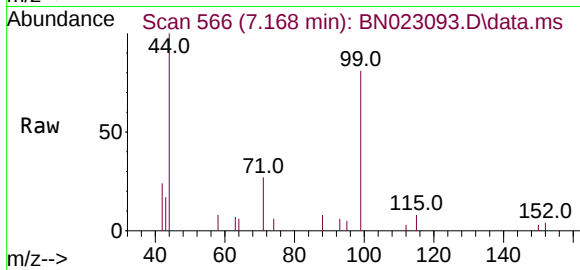

#6
bis(2-Chloroethyl)ether
Concen: 0.086 ng
RT: 7.435 min Scan# 603
Delta R.T. -0.000 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Tgt Ion:	93	Resp:	2688
Ion	Ratio	Lower	Upper
93	100		
63	70.5	58.1	87.1
95	31.3	25.2	37.8


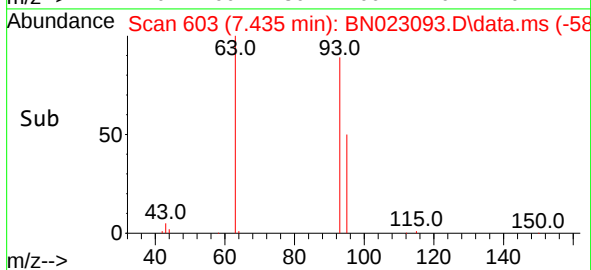

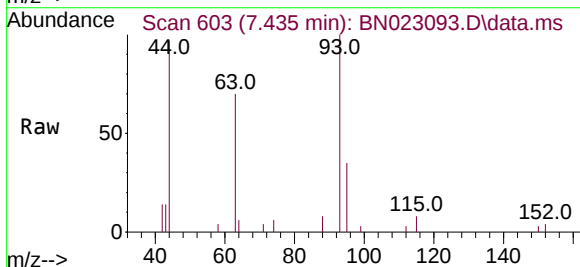




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.839 min Scan# 90
Delta R.T. -0.000 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	136	Resp:	29087
Ion Ratio	Lower	Upper	
136	100		
137	10.9	9.0	13.4
54	6.2	6.5	9.7#
68	5.5	5.4	8.2

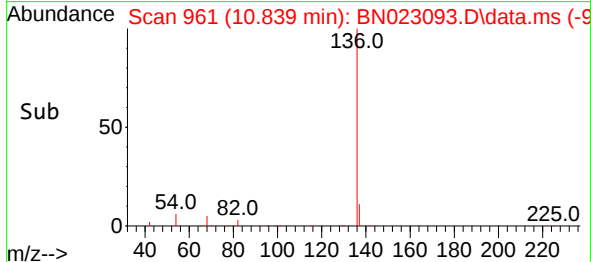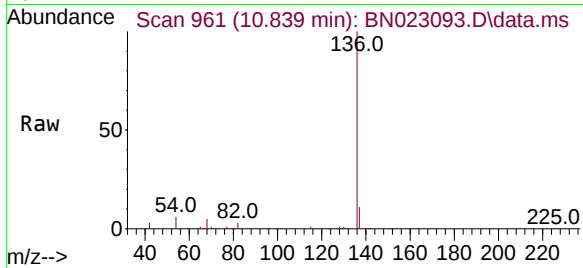

#8
Nitrobenzene-d5
Concen: 0.082 ng
RT: 9.174 min Scan# 805
Delta R.T. -0.011 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Tgt Ion:	82	Resp:	1799
Ion Ratio	Lower	Upper	
82	100		
128	39.9	31.4	47.2
54	58.9	41.0	61.4


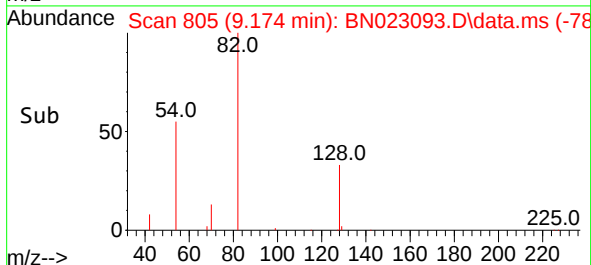
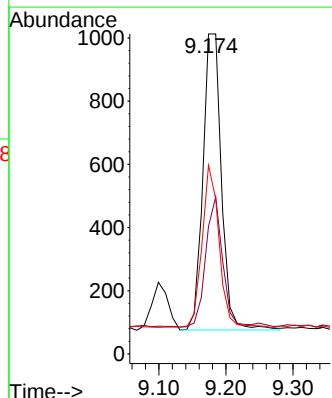
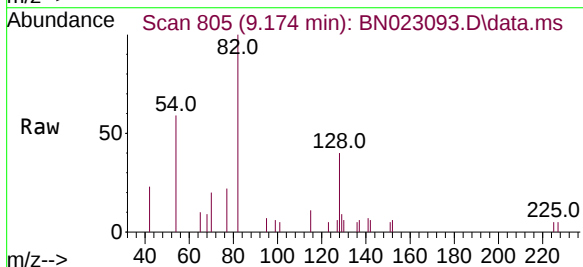




#9
Naphthalene
Concen: 0.083 ng
RT: 10.882 min Scan# 966
Delta R.T. -0.011 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	128	Resp:	7179
Ion	Ratio	Lower	Upper
128	100		
129	12.4	9.0	13.6
127	14.0	10.5	15.7

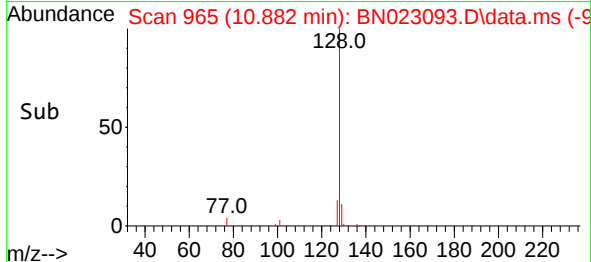

#10
Hexachlorobutadiene
Concen: 0.085 ng
RT: 11.181 min Scan# 993
Delta R.T. -0.000 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Tgt Ion:	225	Resp:	1383
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.5	51.1	76.7


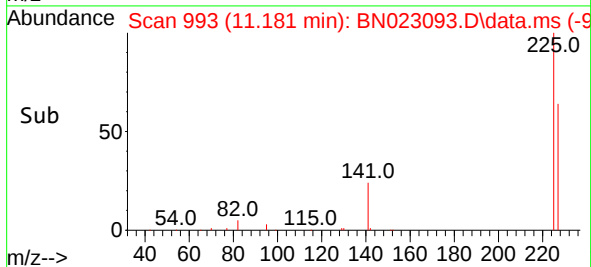

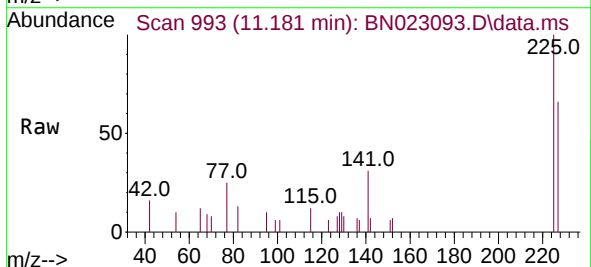




#11
2-Methylnaphthalene-d10
Concen: 0.077 ng
RT: 12.423 min Scan# 1184
Delta R.T. -0.004 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:152 Resp: 4254
Ion Ratio Lower Upper
152 100
151 18.7 15.1 22.7

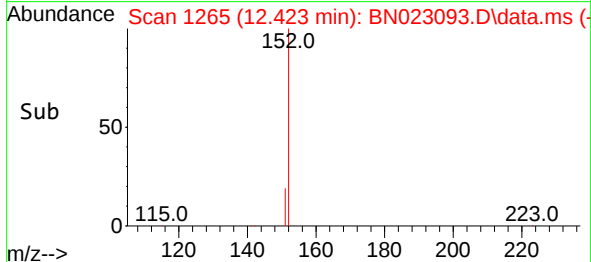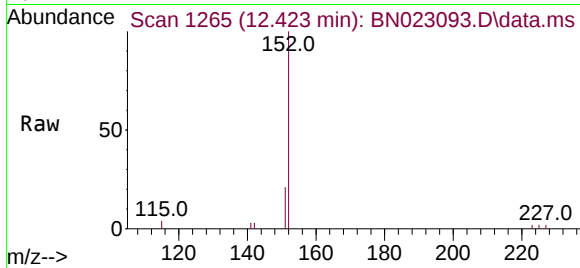

#12
2-Methylnaphthalene
Concen: 0.074 ng
RT: 12.113 min Scan# 1183
Delta R.T. -0.004 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Tgt Ion:142 Resp: 983
Ion Ratio Lower Upper
142 100
141 21.0 10.9 16.3#
115 18.0 5.7 8.5#


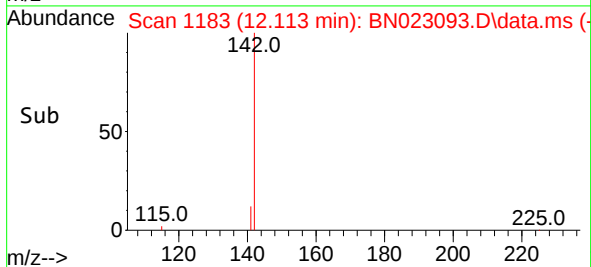

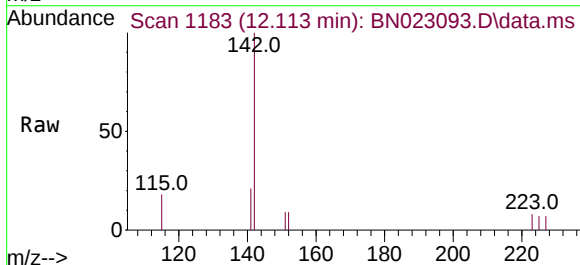




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.666 min Scan# 1489
Delta R.T. -0.000 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:164 Resp: 16291
Ion Ratio Lower Upper
164 100
162 102.7 83.4 125.0
160 49.6 41.8 62.8

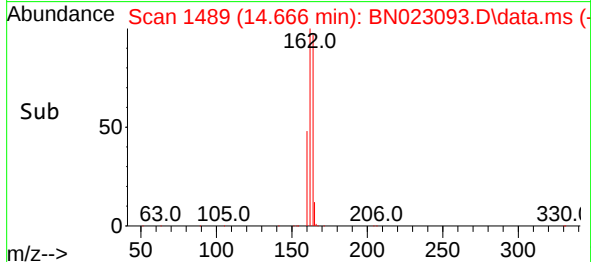

#14
2,4,6-Tribromophenol
Concen: 0.071 ng
RT: 16.148 min Scan# 1622
Delta R.T. -0.000 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Tgt Ion:330 Resp: 489
Ion Ratio Lower Upper
330 100
332 98.4 77.3 115.9
141 40.9 33.5 50.3


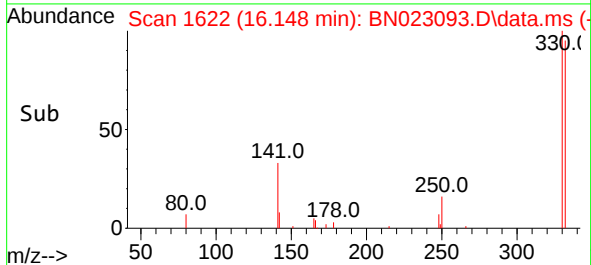

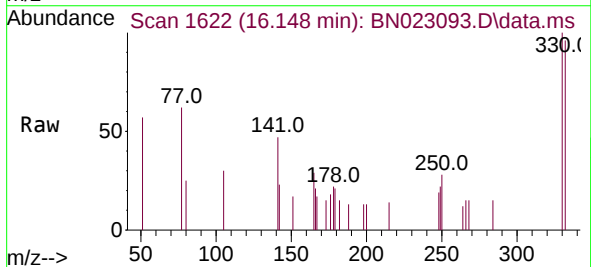




#15
2-Fluorobiphenyl
Concen: 0.088 ng
RT: 13.287 min Scan# 1360
Delta R.T. -0.011 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:172 Resp: 6390
Ion Ratio Lower Upper
172 100
171 35.9 27.4 41.0
170 25.1 17.9 26.9

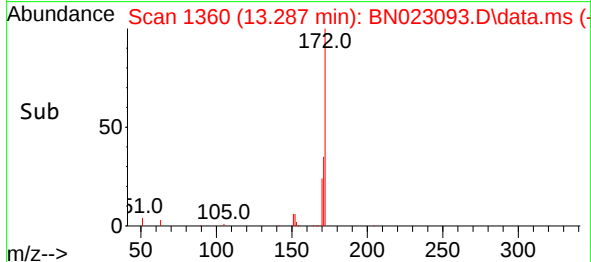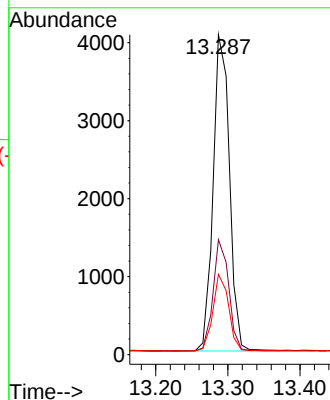

#16
Acenaphthylene
Concen: 0.072 ng
RT: 14.388 min Scan# 1463
Delta R.T. -0.000 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Tgt Ion:152 Resp: 5509
Ion Ratio Lower Upper
152 100
151 19.4 15.4 23.2
153 13.2 10.3 15.5


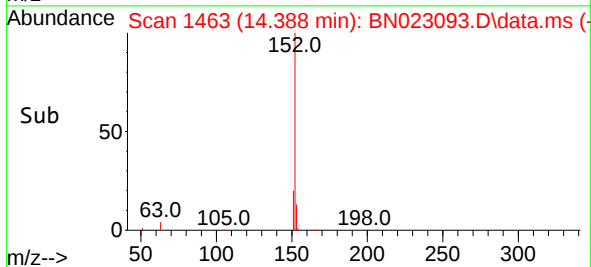
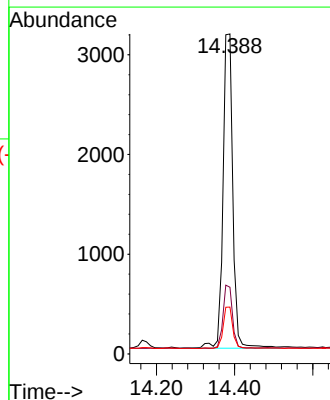
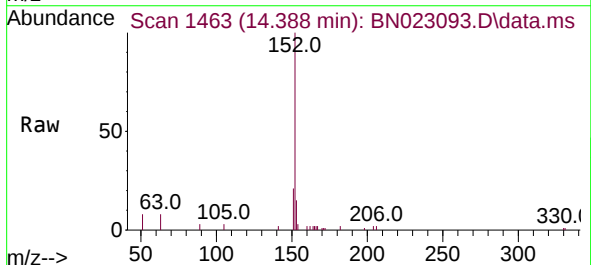




#17
Acenaphthene
Concen: 0.080 ng
RT: 14.730 min Scan# 1495
Delta R.T. -0.000 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:154 Resp: 4487
Ion Ratio Lower Upper
154 100
153 109.9 88.6 132.8
152 59.5 48.1 72.1

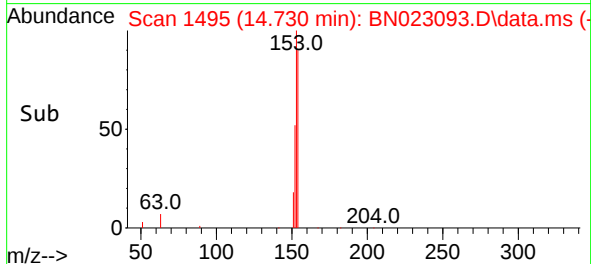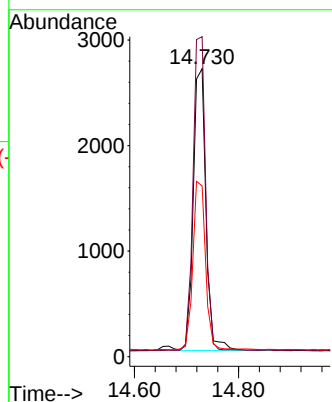

#18
Fluorene
Concen: 0.077 ng
RT: 15.703 min Scan# 1586
Delta R.T. -0.000 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Tgt Ion:166 Resp: 4794
Ion Ratio Lower Upper
166 100
165 100.7 79.8 119.6
167 13.7 10.6 16.0

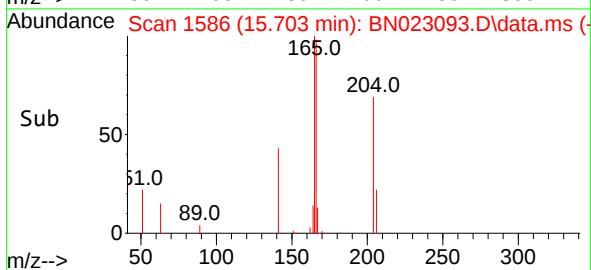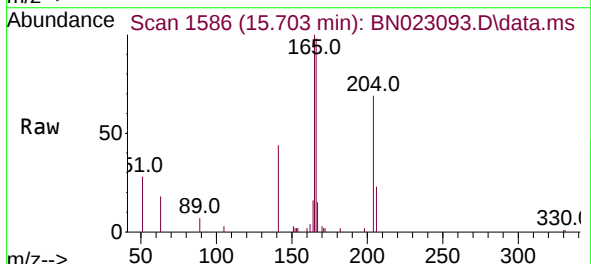



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.414 min Scan# 11

Delta R.T. -0.000 min

Lab File: BN023093.D

Acq: 08 Dec 2022 14:00

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:188 Resp: 36859

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 7.3 6.1 9.1

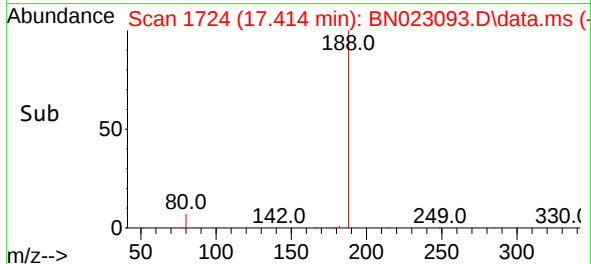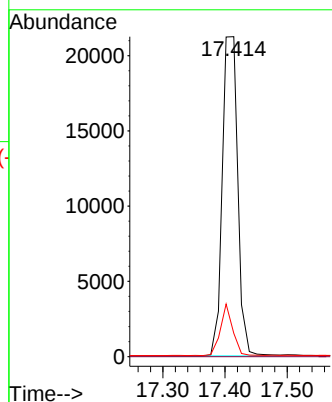

#21

4-Bromophenyl-phenylether

Concen: 0.081 ng

RT: 16.595 min Scan# 1658

Delta R.T. -0.000 min

Lab File: BN023093.D

Acq: 08 Dec 2022 14:00




Tgt Ion:248 Resp: 1805


Ion Ratio Lower Upper

248 100

250 92.9 74.3 111.5

141 83.1 65.0 97.6

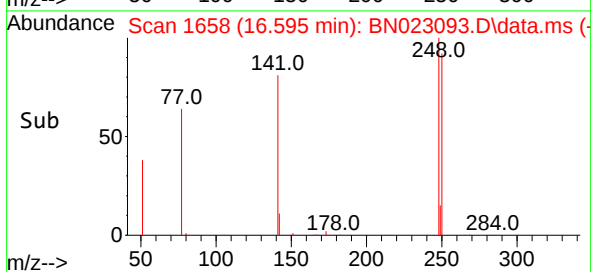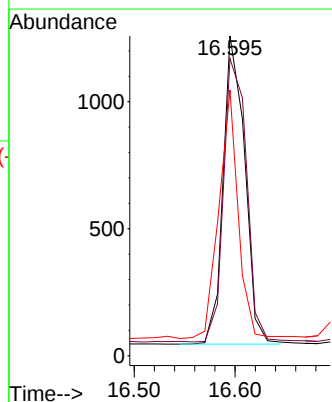



#22

Hexachlorobenzene

Concen: 0.082 ng

RT: 16.719 min Scan# 1668

Delta R.T. -0.000 min

Lab File: BN023093.D

Acq: 08 Dec 2022 14:00

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:284 Resp: 2356

Ion Ratio Lower Upper

284 100

142 39.7 31.0 46.4

249 31.7 24.4 36.6

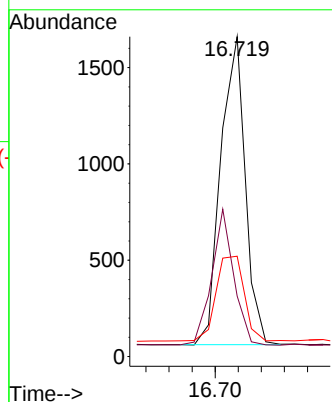

#23

Atrazine

Concen: 0.071 ng

RT: 16.868 min Scan# 1680

Delta R.T. -0.000 min

Lab File: BN023093.D

Acq: 08 Dec 2022 14:00




Tgt Ion:200 Resp: 1151


Ion Ratio Lower Upper

200 100

173 27.4 18.2 27.4#

215 48.4 38.0 57.0

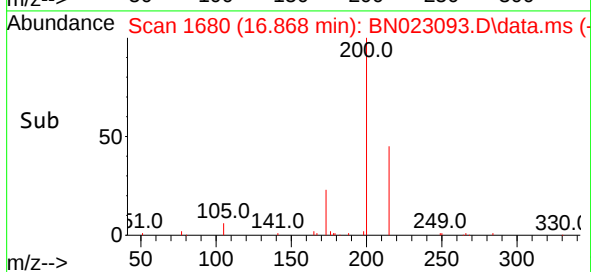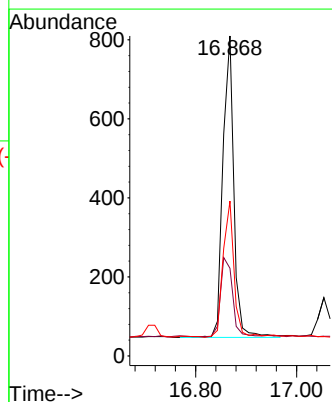



#24

Pentachlorophenol

Concen: 0.102 ng

RT: 17.054 min Scan# 1695

Delta R.T. -0.000 min

Lab File: BN023093.D

Acq: 08 Dec 2022 14:00

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:266 Resp: 861

Ion Ratio Lower Upper

266 100

264 60.6 50.1 75.1

268 63.9 49.7 74.5

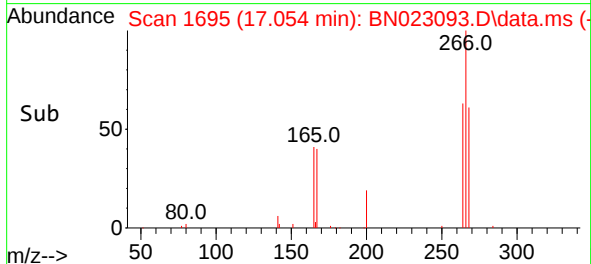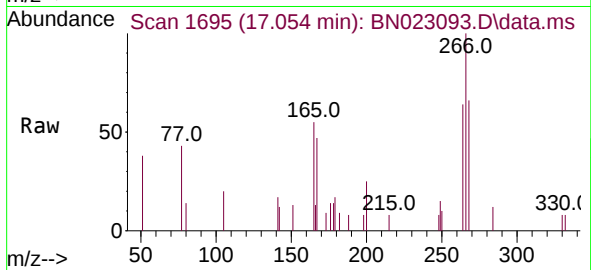

#25

Phenanthrene

Concen: 0.085 ng

RT: 17.451 min Scan# 1727

Delta R.T. -0.000 min

Lab File: BN023093.D

Acq: 08 Dec 2022 14:00




Tgt Ion:178 Resp: 10530


Ion Ratio Lower Upper

178 100

176 19.5 15.4 23.2

179 15.7 12.2 18.2




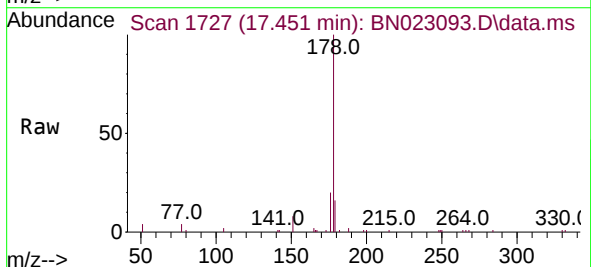


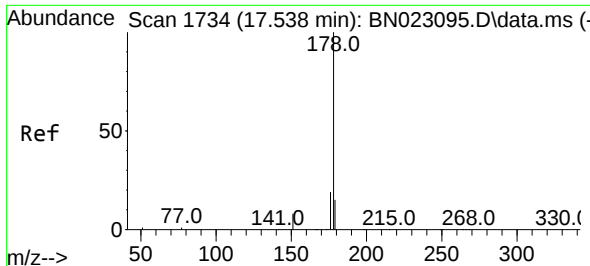

#26
 Anthracene
 Concen: 0.075 ng
 RT: 17.538 min Scan# 1734
 Delta R.T. -0.000 min
 Lab File: BN023093.D
 Acq: 08 Dec 2022 14:00




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:	178	Resp:	7515
Ion Ratio	Lower	Upper	
178	100		
176	18.7	15.1	22.7
179	15.2	12.2	18.4

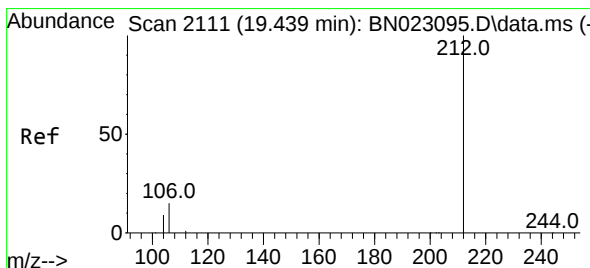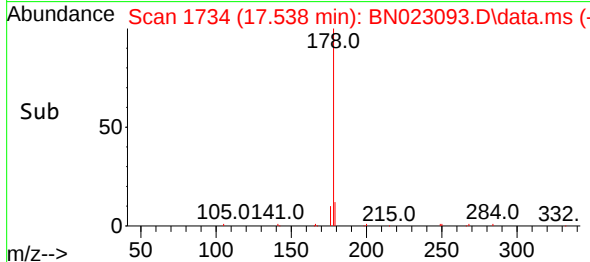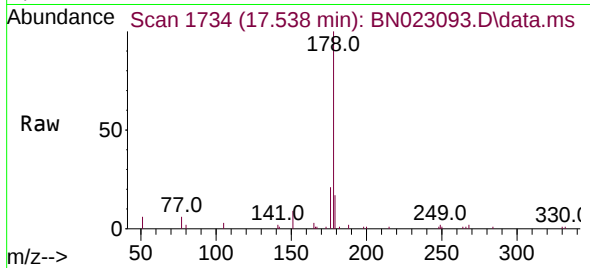

#27
 Fluoranthene-d10
 Concen: 0.075 ng
 RT: 19.439 min Scan# 2111
 Delta R.T. -0.000 min
 Lab File: BN023093.D
 Acq: 08 Dec 2022 14:00

Tgt Ion:	212	Resp:	7606
Ion Ratio	Lower	Upper	
212	100		
106	16.3	13.0	19.4
104	9.1	7.5	11.3


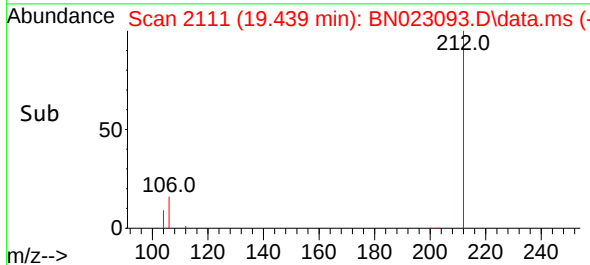

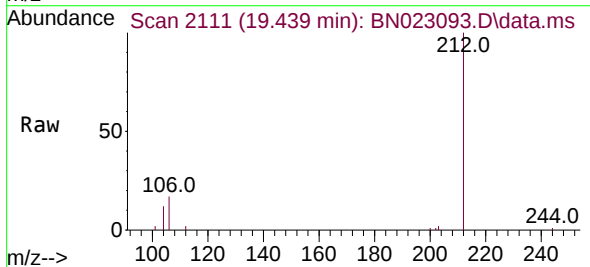


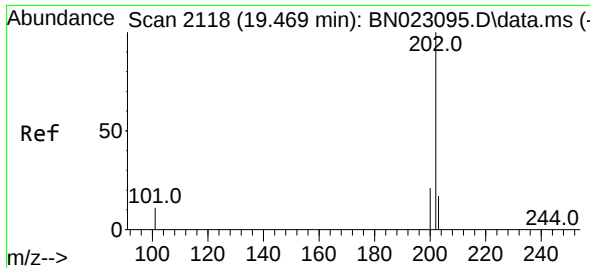

#28
Fluoranthene
Concen: 0.074 ng
RT: 19.468 min Scan# 2118
Delta R.T. -0.000 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:202 Resp: 10024
Ion Ratio Lower Upper
202 100
101 11.8 9.7 14.5
203 17.1 13.8 20.6

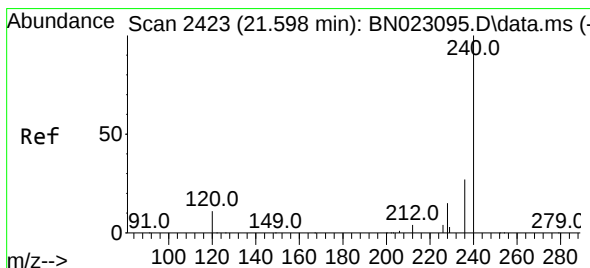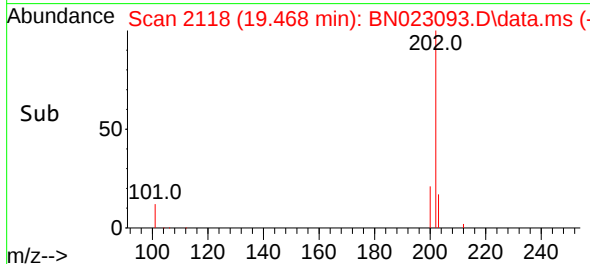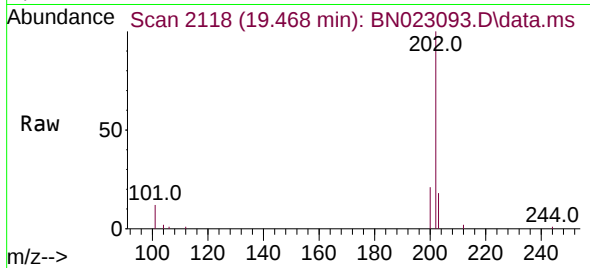

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.593 min Scan# 2423
Delta R.T. -0.005 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Tgt Ion:240 Resp: 29376
Ion Ratio Lower Upper
240 100
120 20.3 10.1 15.1#
236 28.6 22.2 33.4


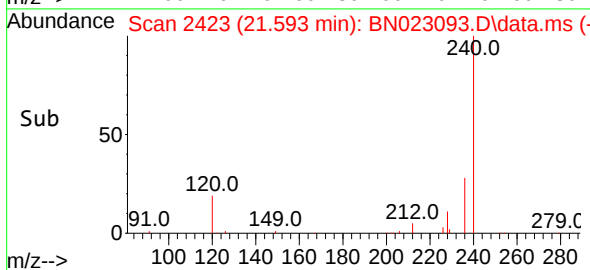

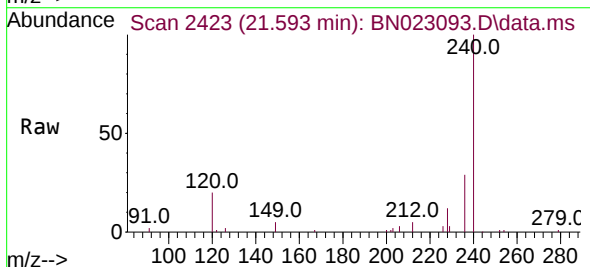




#30
Pyrene
Concen: 0.082 ng
RT: 19.831 min Scan# 2204
Delta R.T. -0.000 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:	202	Resp:	10098
Ion Ratio	Lower	Upper	
202	100		
200	20.9	16.9	25.3
203	18.0	14.2	21.4

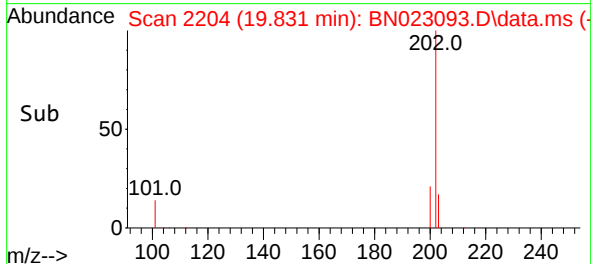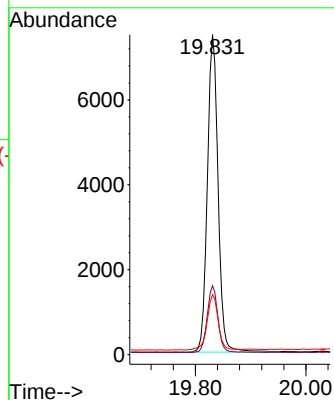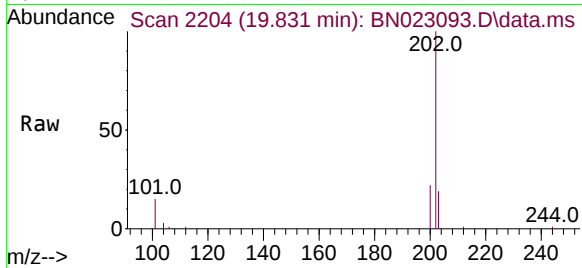

#31
Terphenyl-d14
Concen: 0.081 ng
RT: 20.035 min Scan# 2249
Delta R.T. 0.004 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Tgt Ion:	244	Resp:	4494
Ion Ratio	Lower	Upper	
244	100		
212	9.5	7.6	11.4
122	12.3	12.6	18.8

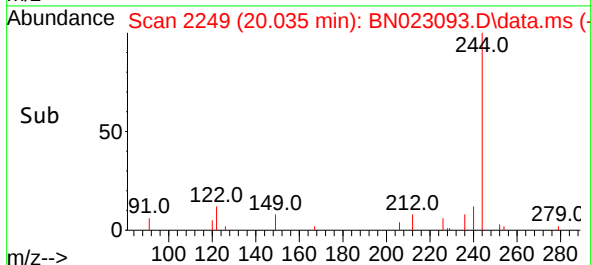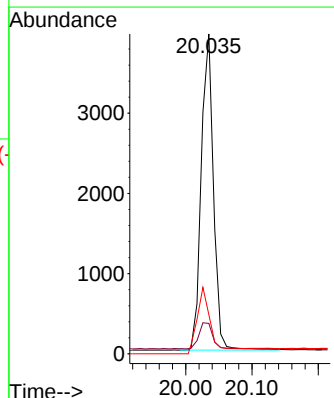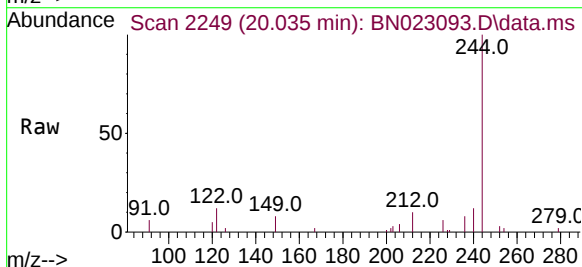

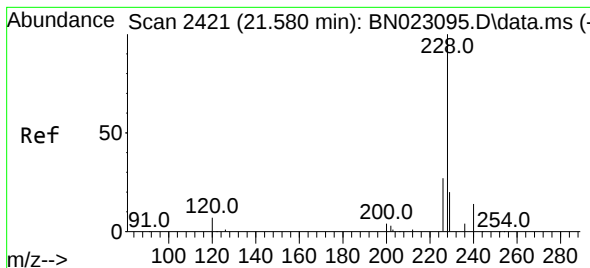

#32

Benzo(a)anthracene

Concen: 0.079 ng

RT: 21.584 min Scan# 2421

Delta R.T. 0.004 min

Lab File: BN023093.D

Acq: 08 Dec 2022 14:00

Instrument :

BNA_N

ClientSampleId :

SSTDICC0.1





Tgt Ion:228 Resp: 8542

Ion Ratio Lower Upper

228 100

226 27.1 22.0 33.0

229 20.5 15.8 23.8

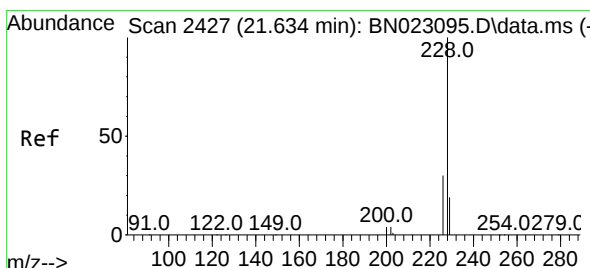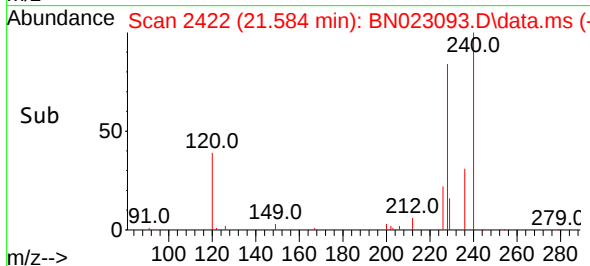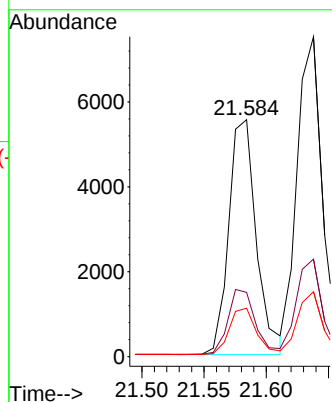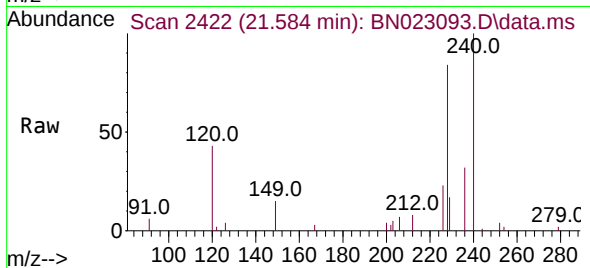

#33

Chrysene

Concen: 0.087 ng

RT: 21.638 min Scan# 2428

Delta R.T. 0.004 min

Lab File: BN023093.D

Acq: 08 Dec 2022 14:00




Tgt Ion:228 Resp: 10544


Ion Ratio Lower Upper

228 100

226 30.5 24.4 36.6

229 20.3 15.6 23.4


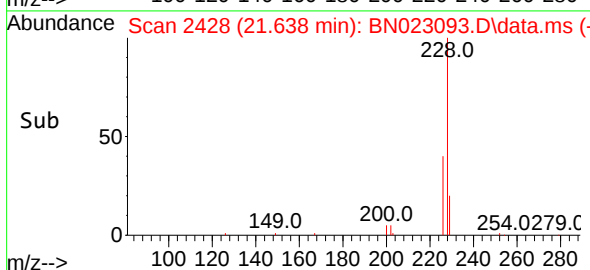

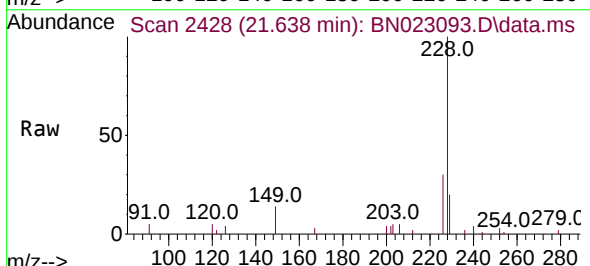


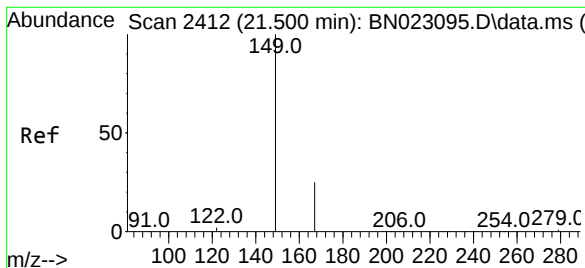

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.079 ng
 RT: 21.504 min Scan# 2413
 Delta R.T. 0.004 min
 Lab File: BN023093.D
 Acq: 08 Dec 2022 14:00




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:149 Resp: 3706
 Ion Ratio Lower Upper
 149 100
 167 24.0 20.2 30.2
 279 3.0 2.3 3.5

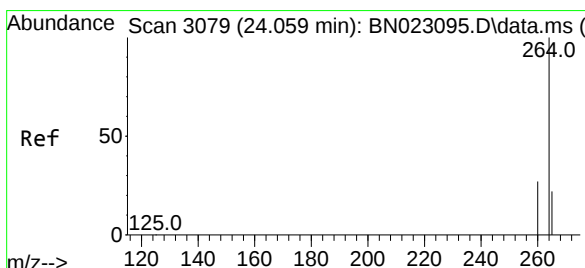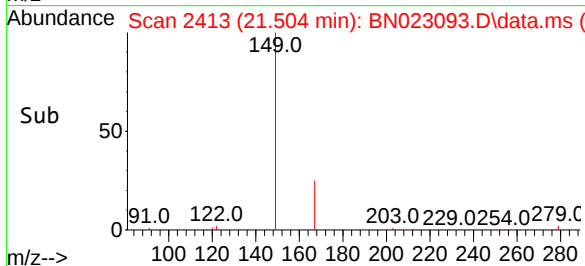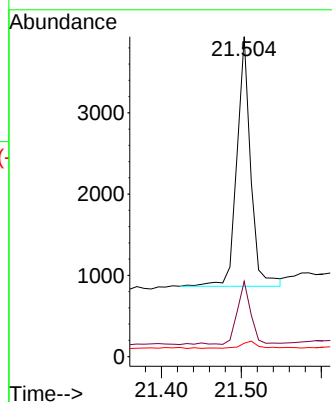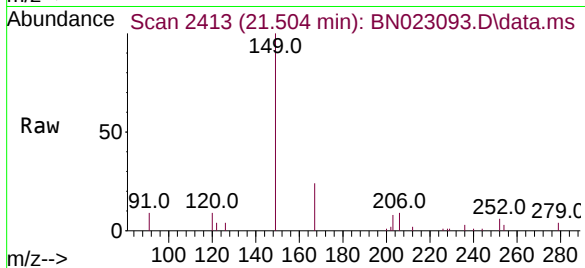

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 24.060 min Scan# 3079
 Delta R.T. 0.001 min
 Lab File: BN023093.D
 Acq: 08 Dec 2022 14:00

Tgt Ion:264 Resp: 26107
 Ion Ratio Lower Upper
 264 100
 260 26.2 21.7 32.5
 265 40.9 43.2 64.8#


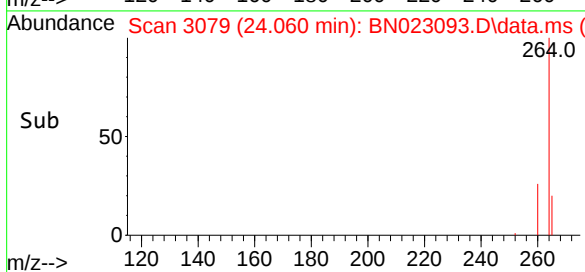
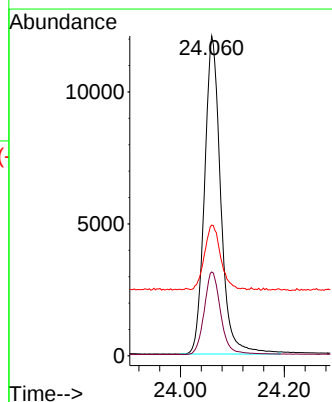
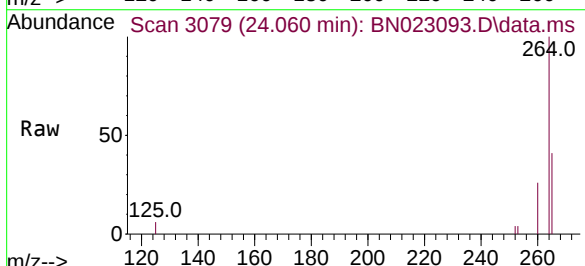




#36
Indeno(1,2,3-cd)pyrene
Concen: 0.070 ng
RT: 26.630 min Scan# 3959
Delta R.T. -0.002 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:276 Resp: 9677
Ion Ratio Lower Upper
276 100
138 13.9 25.0 37.6#
277 24.8 19.8 29.8

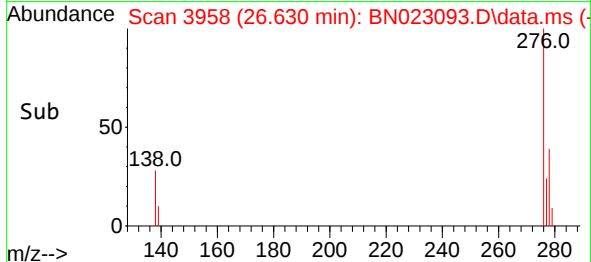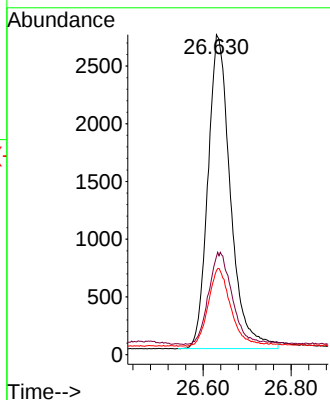

#37
Benzo(b)fluoranthene
Concen: 0.074 ng
RT: 23.306 min Scan# 2821
Delta R.T. 0.001 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Tgt Ion:252 Resp: 8869
Ion Ratio Lower Upper
252 100
253 28.8 19.0 28.4#
125 25.0 12.8 19.2#


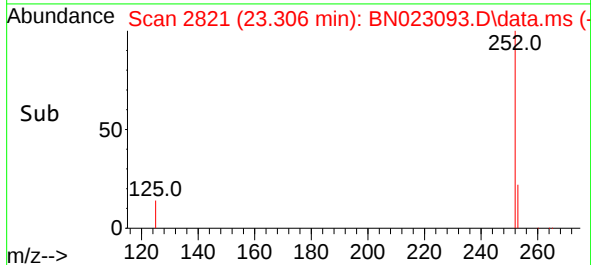
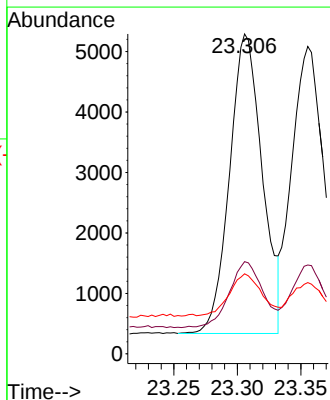
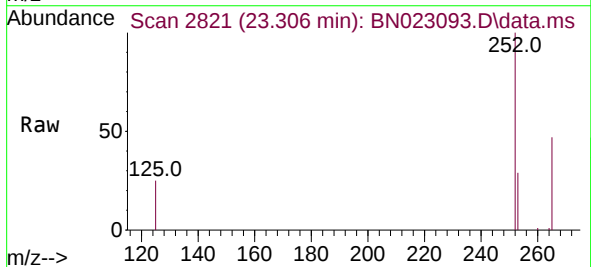




#38
Benzo(k)fluoranthene
Concen: 0.069 ng
RT: 23.355 min Scan# 2837
Delta R.T. 0.004 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:252 Resp: 8393
Ion Ratio Lower Upper
252 100
253 28.9 19.1 28.7#
125 23.2 12.5 18.7#

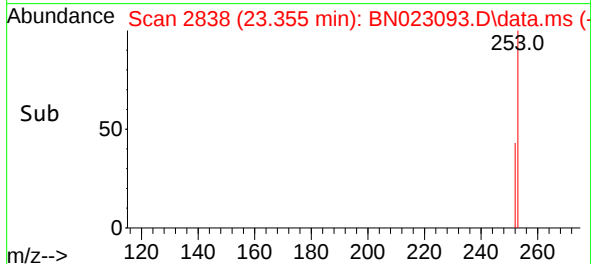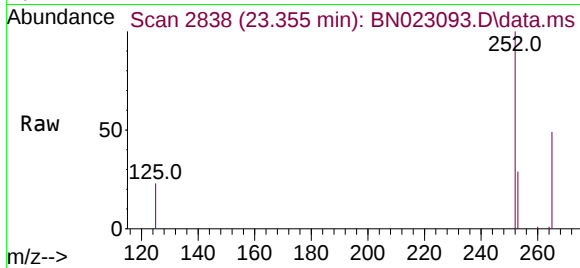

#39
Benzo(a)pyrene
Concen: 0.077 ng
RT: 23.949 min Scan# 3041
Delta R.T. 0.001 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Tgt Ion:252 Resp: 7407
Ion Ratio Lower Upper
252 100
253 33.2 20.6 30.8#
125 35.5 15.8 23.8#


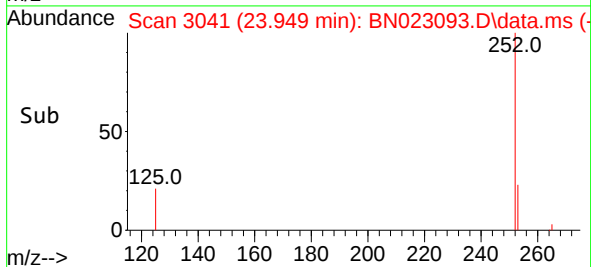

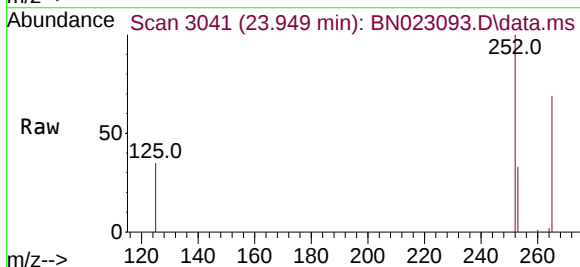




#40
Dibenzo(a,h)anthracene
Concen: 0.068 ng
RT: 26.656 min Scan# 3966
Delta R.T. 0.004 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Tgt Ion:278 Resp: 7491
Ion Ratio Lower Upper
278 100
139 24.3 17.5 26.3
279 28.7 20.5 30.7

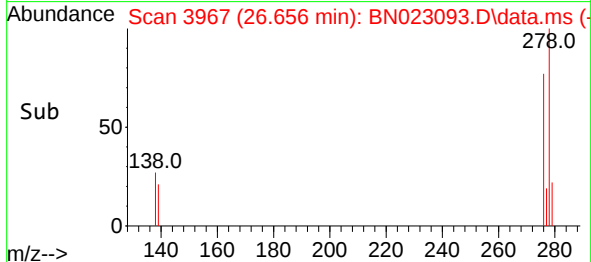

#41
Benzo(g,h,i)perylene
Concen: 0.071 ng
RT: 27.425 min Scan# 4230
Delta R.T. 0.001 min
Lab File: BN023093.D
Acq: 08 Dec 2022 14:00

Tgt Ion:276 Resp: 7959
Ion Ratio Lower Upper
276 100
277 26.5 19.9 29.9
138 29.9 22.2 33.2

