
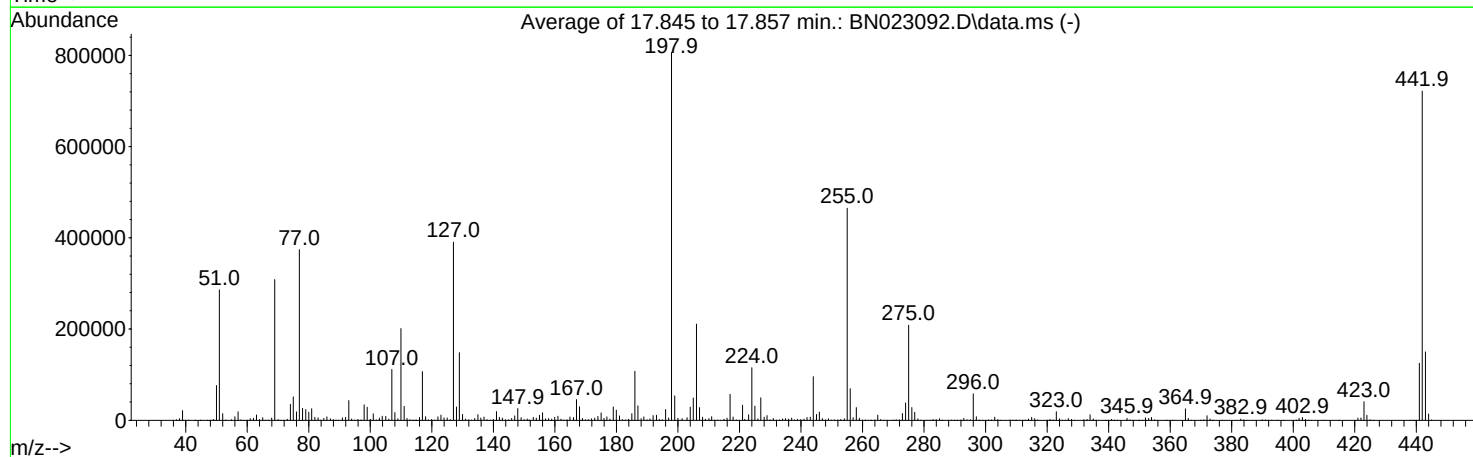


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120822\
 Data File : BN023092.D
 Acq On : 08 Dec 2022 12:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 09 07:44:40 2022

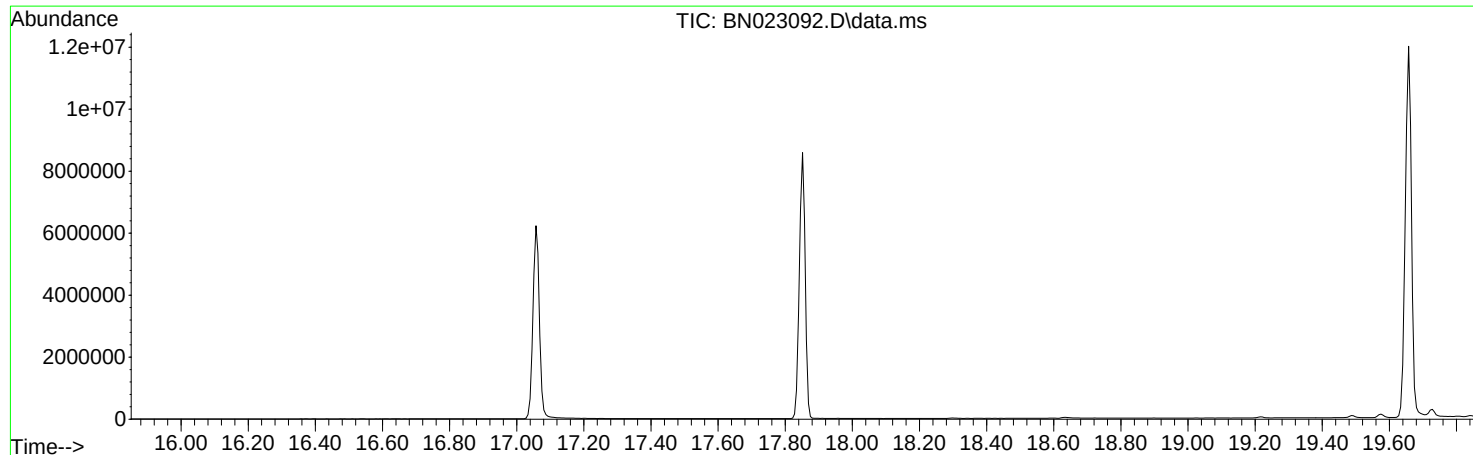




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.5	286051	PASS
68	69	0.00	2	1.6	5003	PASS
69	198	0.00	100	38.2	308437	PASS
70	69	0.00	2	0.5	1672	PASS
127	198	10	80	48.4	390485	PASS
197	198	0.00	2	0.6	5002	PASS
198	198	100	100	100.0	806400	PASS
199	198	5	9	6.6	53560	PASS
275	198	10	60	25.9	208533	PASS
365	198	1	100	3.1	25240	PASS
441	198	0.01	100	15.5	125061	PASS
442	442	50	100	100.0	721600	PASS
443	442	15	24	20.8	149963	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120822\
Data File : BN023092.D
Acq On : 08 Dec 2022 12:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 09 09:10:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 09:10:48 2022
Response via : Initial Calibration

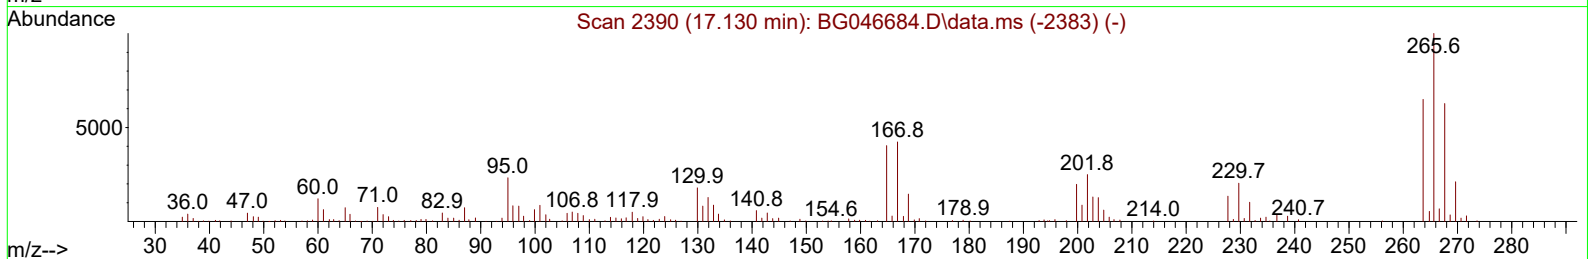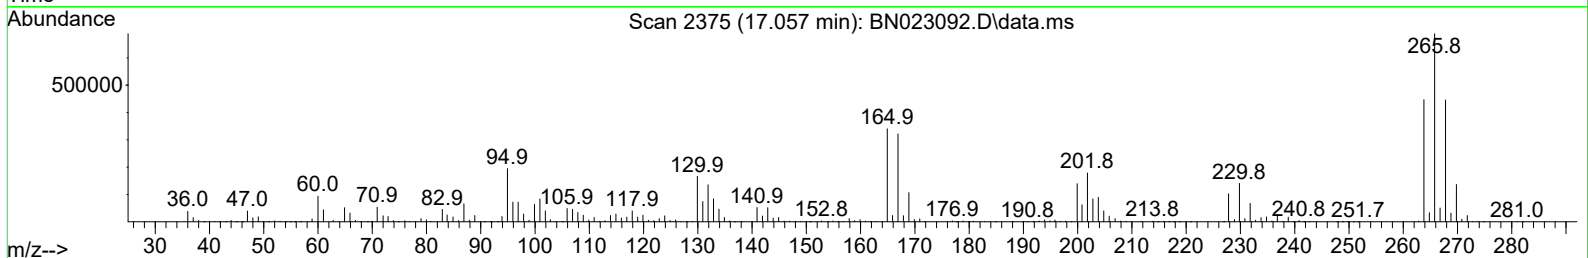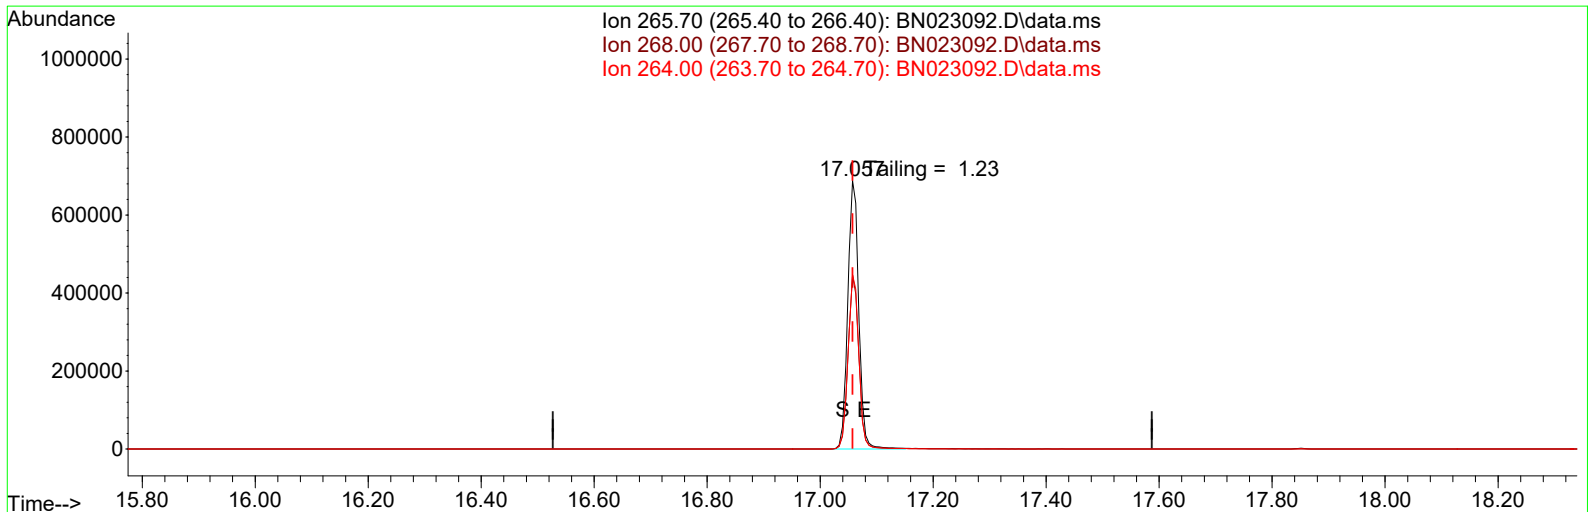

TIC: BN023092.D\data.ms

(70) Pentachlorophenol (C)

17.057min (0.000) 22077.14 ng




response 935928

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.79
264.00	61.60	64.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN120822\
 Data File : BN023092.D
 Acq On : 08 Dec 2022 12:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 09 09:10:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 09 09:10:48 2022
 Response via : Initial Calibration

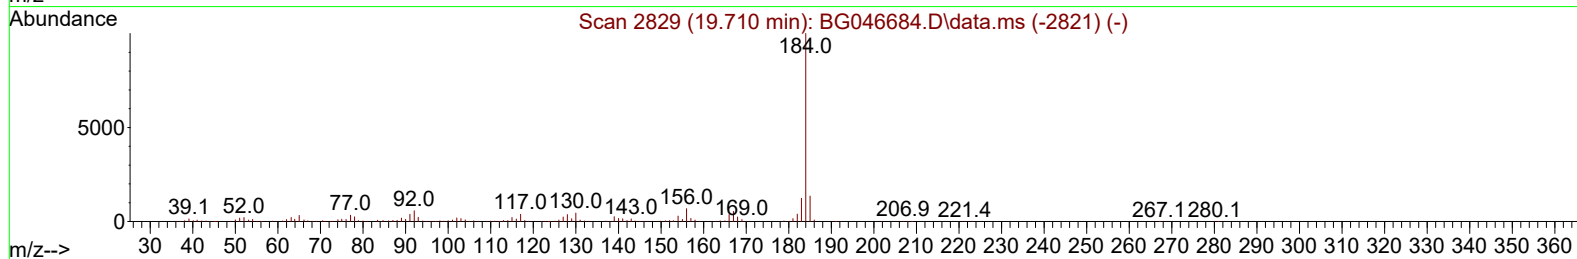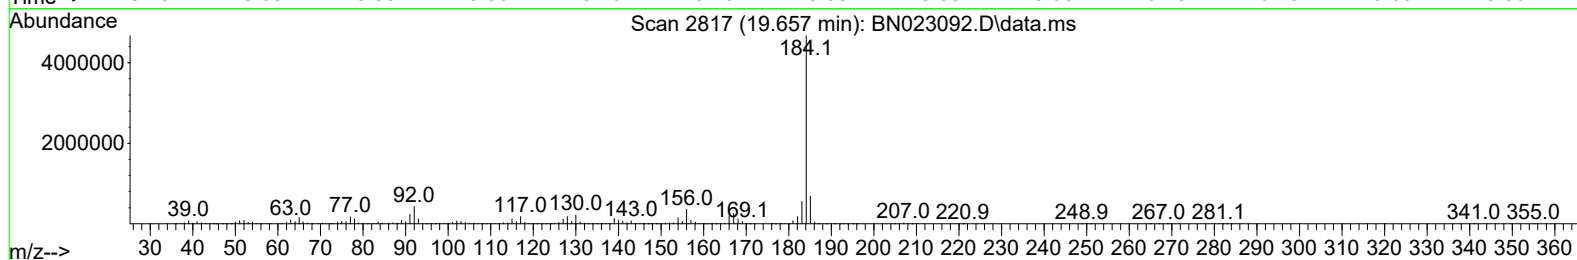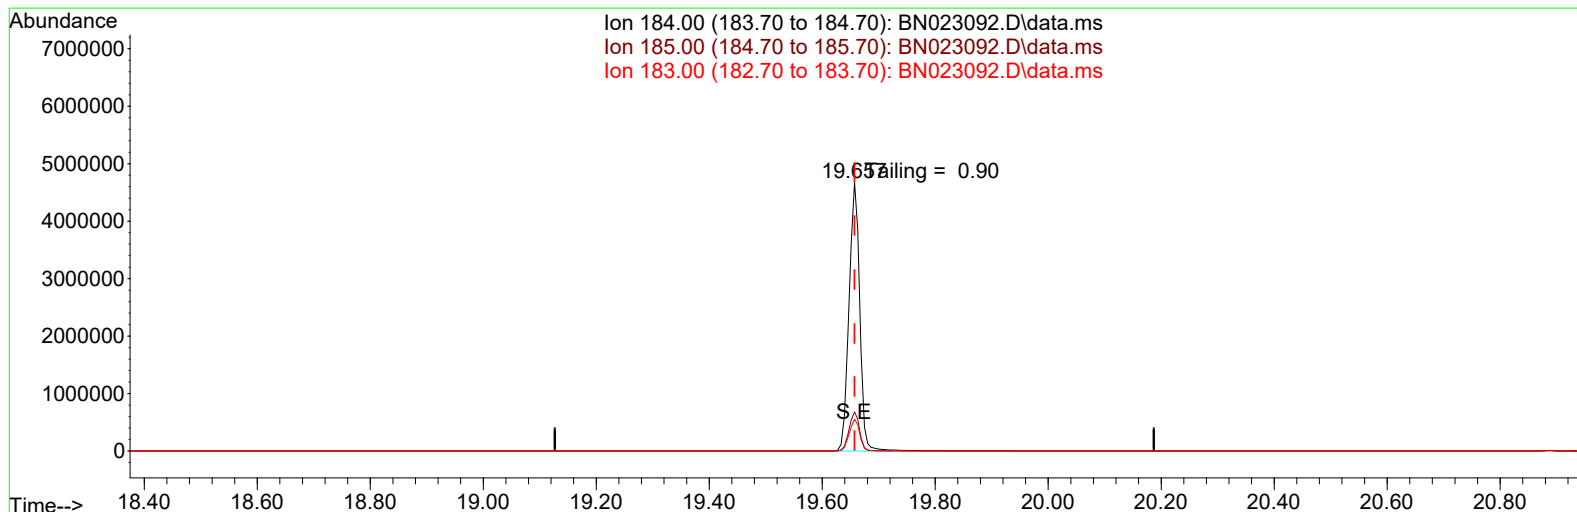

TIC: BN023092.D\data.ms

(77) Benzidine

19.657min (0.000) 3431862.86 ng

response 6135730

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.62
183.00	13.20	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/8/2022	BNA_N	<u>BN023092.D</u>
Compound Name	Response	Retention Time
DDT	2597977	20.886
DDD	21198	20.498
DDE	214	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
21412	2619389	0.82

Instrument :
BNA_N
ClientSampleId :
DFTPP