


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121922\
 Data File : BN023279.D
 Acq On : 19 Dec 2022 10:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 19 15:44:58 2022

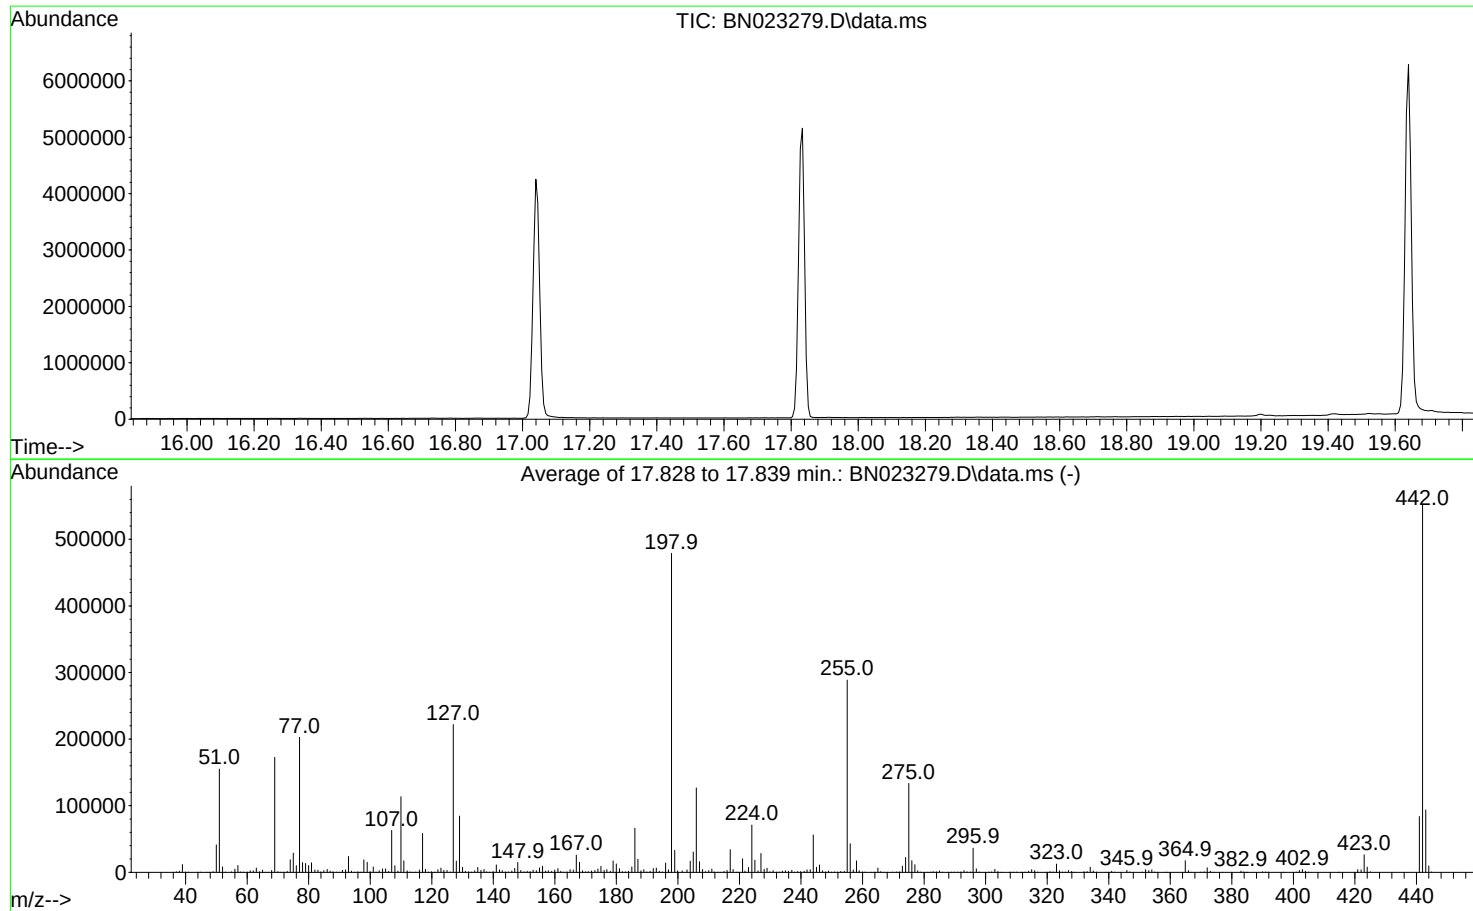




AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2498

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	155011	PASS
68	69	0.00	2	1.6	2838	PASS
69	198	0.00	100	36.0	172621	PASS
70	69	0.00	2	0.6	1058	PASS
127	198	10	80	46.3	221845	PASS
197	198	0.00	2	0.8	3681	PASS
198	198	100	100	100.0	478933	PASS
199	198	5	9	6.8	32725	PASS
275	198	10	60	27.9	133419	PASS
365	198	1	100	3.6	17402	PASS
441	198	0.01	100	17.5	83835	PASS
442	442	50	100	100.0	552363	PASS
443	442	15	24	16.9	93541	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121922\  
Data File : BN023279.D  
Acq On    : 19 Dec 2022  10:45  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 20 06:26:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 06:26:03 2022
Response via : Initial Calibration

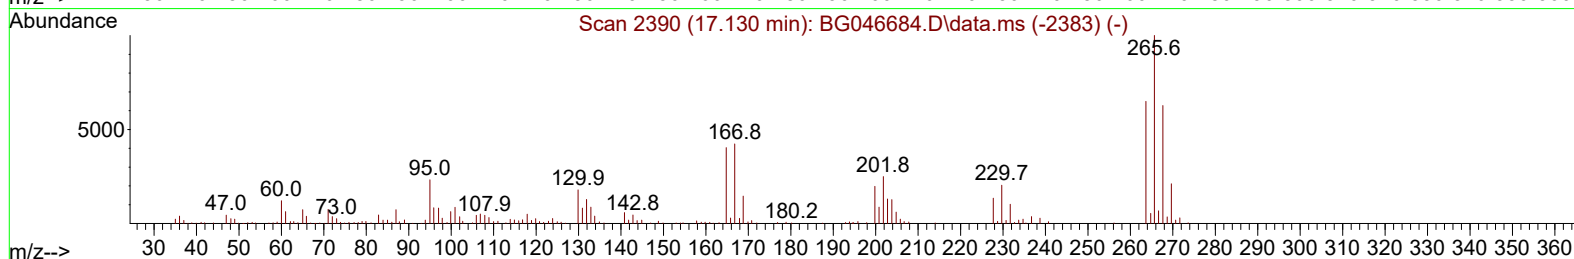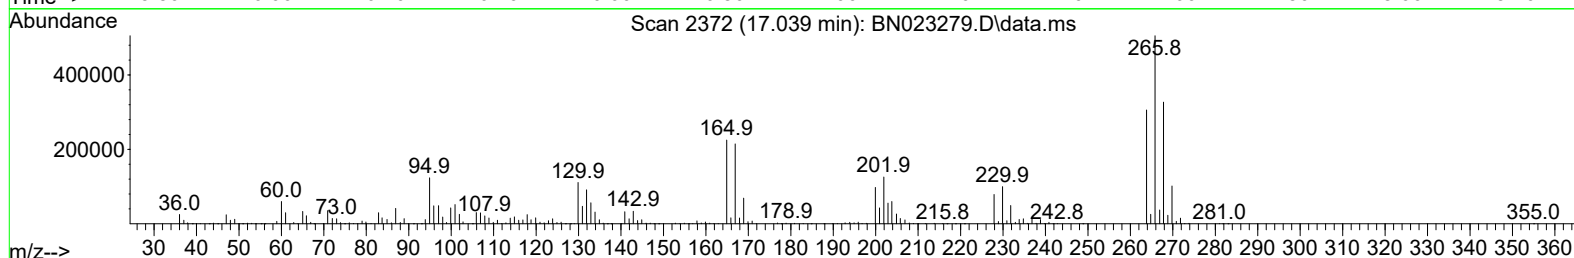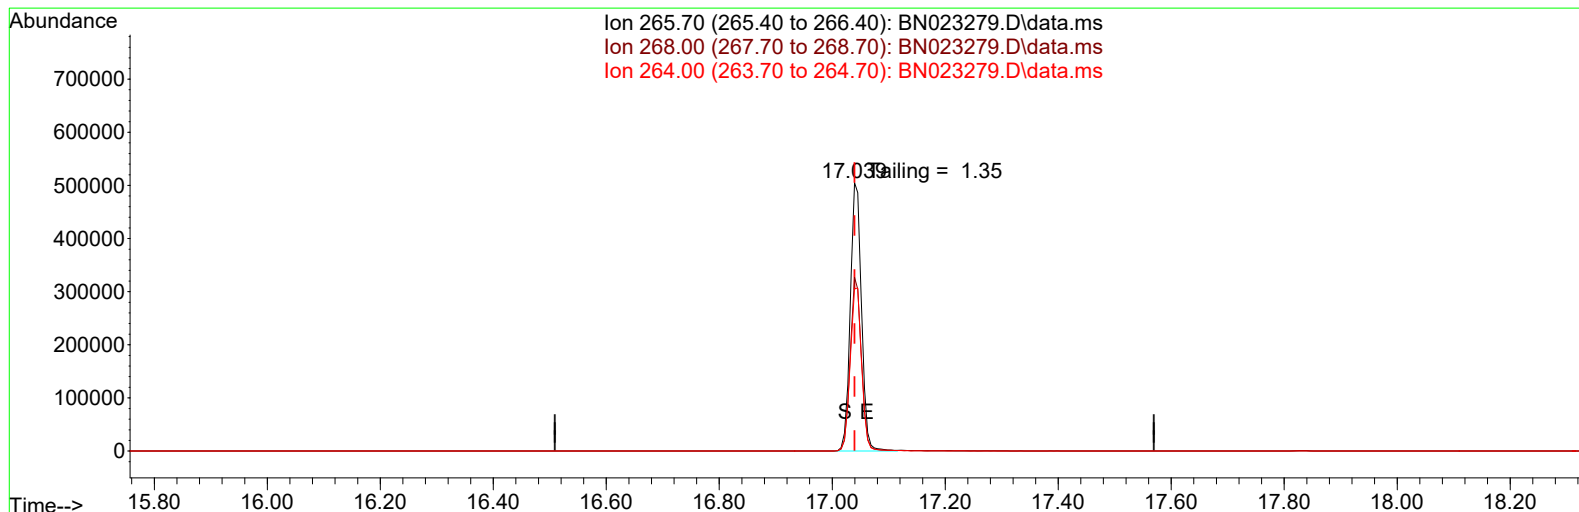

TIC: BN023279.D\data.ms

(70) Pentachlorophenol (C)

17.039min (0.000) 25233.58 ng

response **695470**

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------

268.00	62.20	64.68
--------	-------	-------




264.00	61.60	60.53
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121922\
Data File : BN023279.D
Acq On : 19 Dec 2022 10:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 20 06:26:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 06:26:03 2022
Response via : Initial Calibration

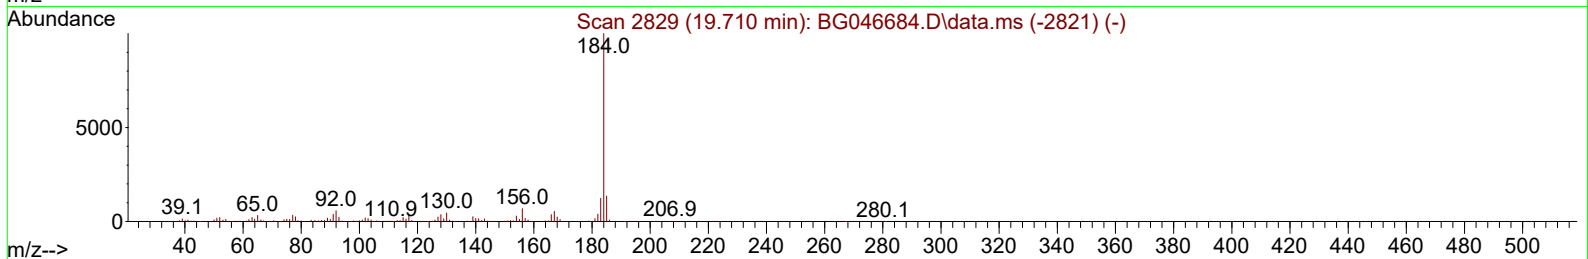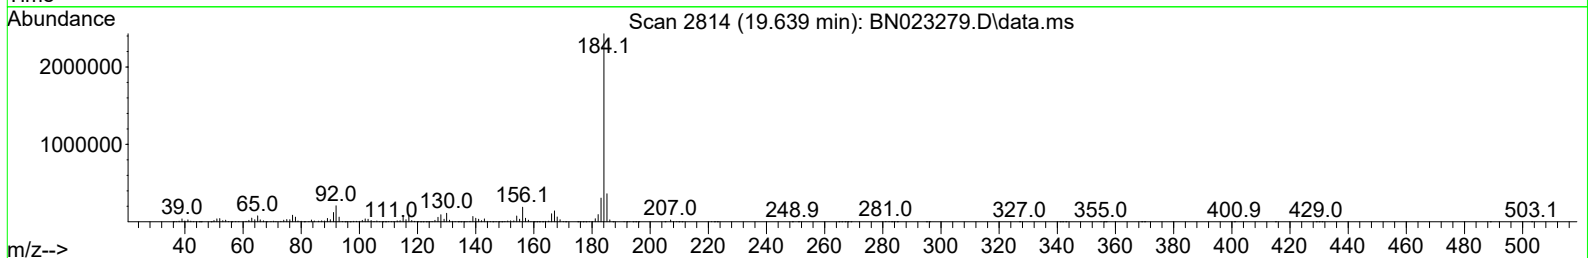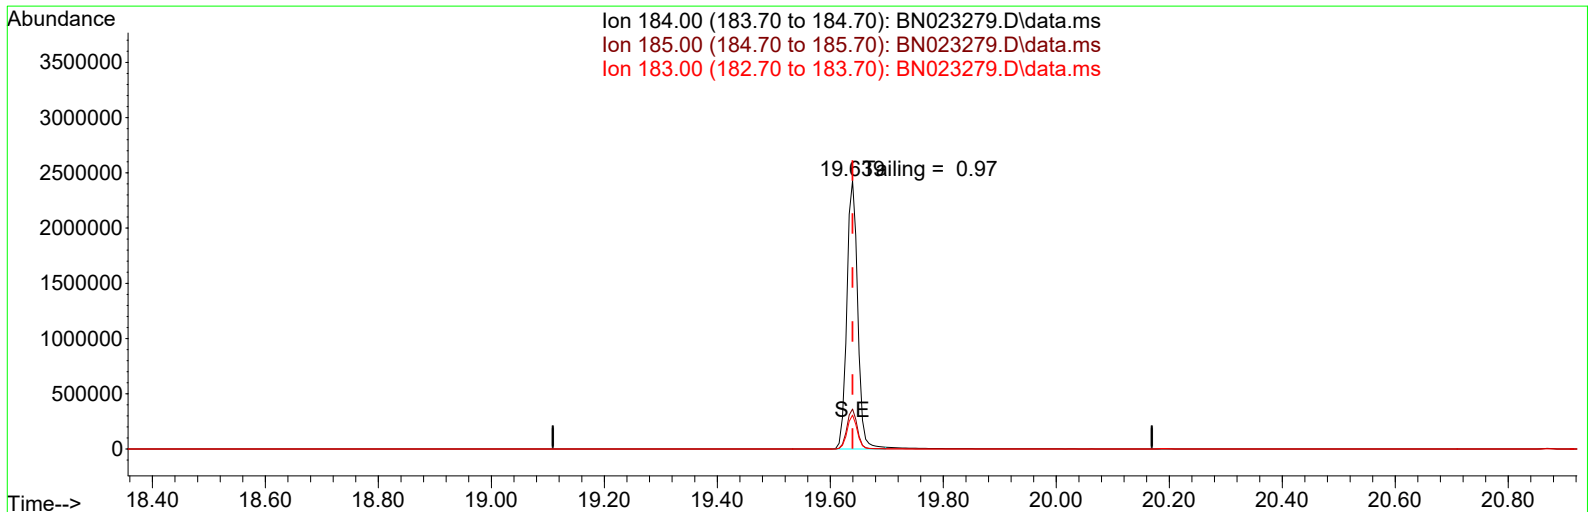

TIC: BN023279.D\data.ms

(77) Benzidine

19.639min (0.000) 579785.01 ng

response 3234848

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.91
183.00	13.20	12.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/19/2022	BNA_N	<u>BN023279.D</u>
Compound Name	Response	Retention Time
DDT	1544427	20.869
DDD	201124	20.427
DDE	7574	19.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
208698	1753125	11.90

Instrument :
BNA_N
ClientSampleId :
DFTPP