



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX121522\
Data File : VX033429.D
Acq On : 15 Dec 2022 09:39
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X120722W.M
Title : SW846 8260
Last Update : Wed Dec 07 12:43:54 2022

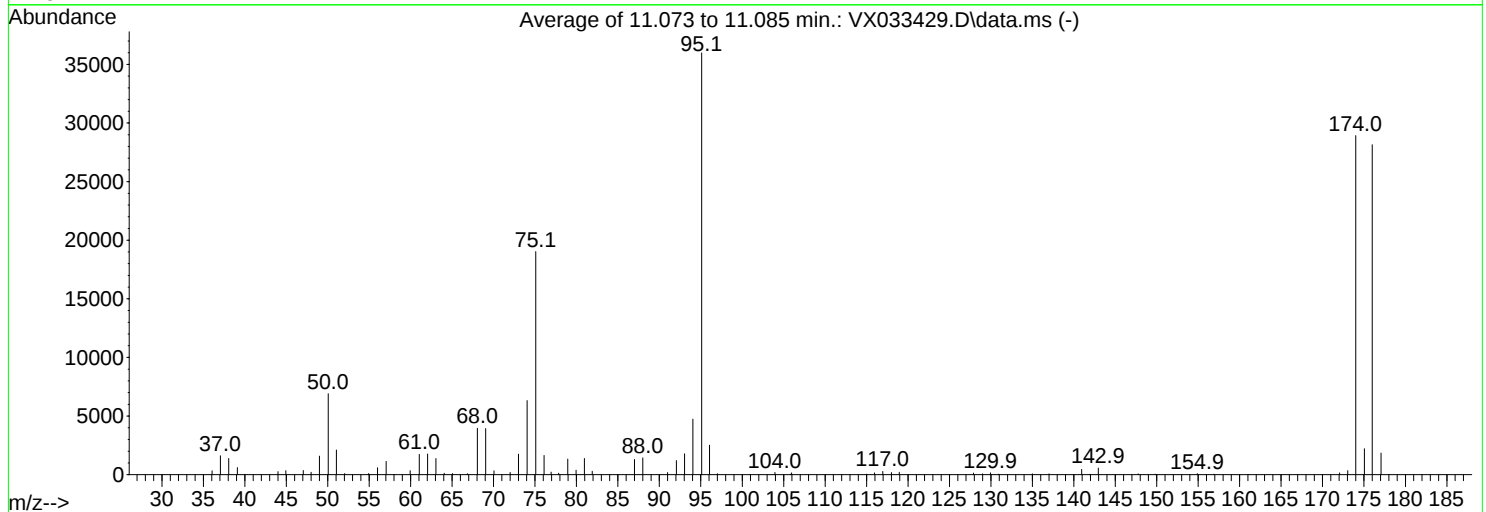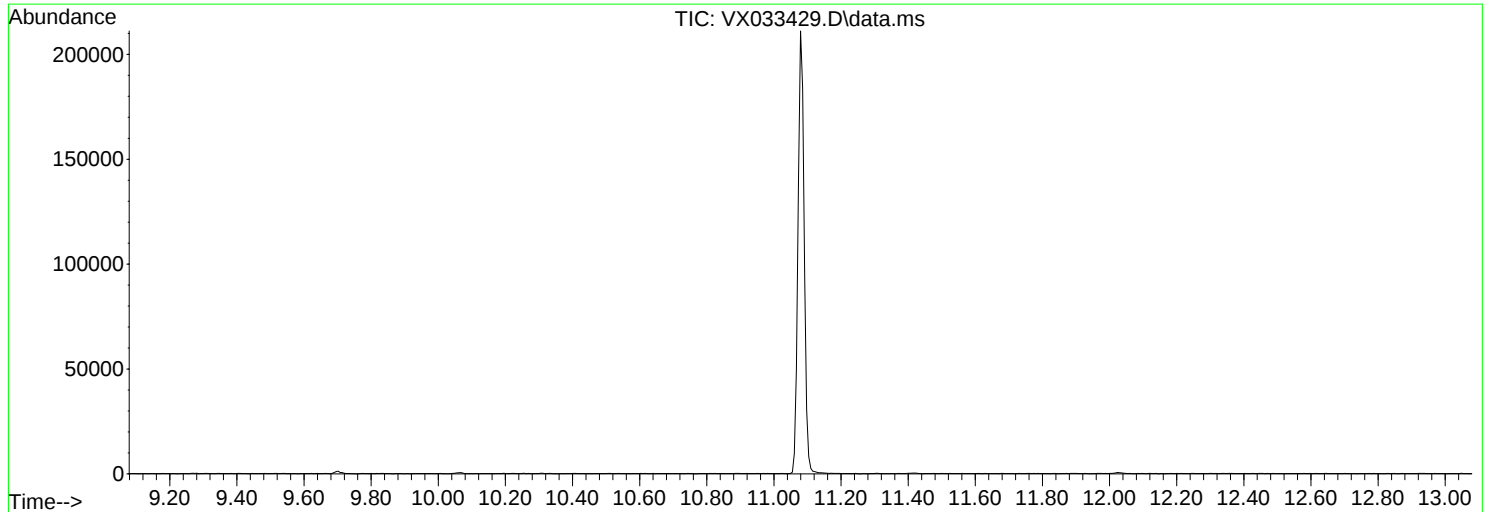

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	6908	PASS
75	95	30	60	52.9	19031	PASS
95	95	100	100	100.0	35987	PASS
96	95	5	9	7.0	2518	PASS
173	174	0.00	2	1.2	336	PASS
174	95	50	100	80.4	28931	PASS
175	174	5	9	7.6	2209	PASS
176	174	95	101	97.3	28149	PASS
177	176	5	9	6.6	1847	PASS