

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012023\
 Data File : PP054782.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Jan 2023 22:00
 Operator : YP\AJ
 Sample : 01232-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 B-P-19B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/23/2023
 Supervised By :Ankita Jodhani 01/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 05:51:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 18 04:34:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.332	3.580	39164744	31748120	21.330m	19.834
2) SA Decachlor...	10.092	8.598	27629542	27740185	20.584	19.371

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP012023\
Data File : PP054782.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Jan 2023 22:00
Operator : YP\AJ
Sample : 01232-07
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
B-P-19B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/23/2023
Supervised By :Ankita Jodhani 01/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 05:51:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP011723.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 18 04:34:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

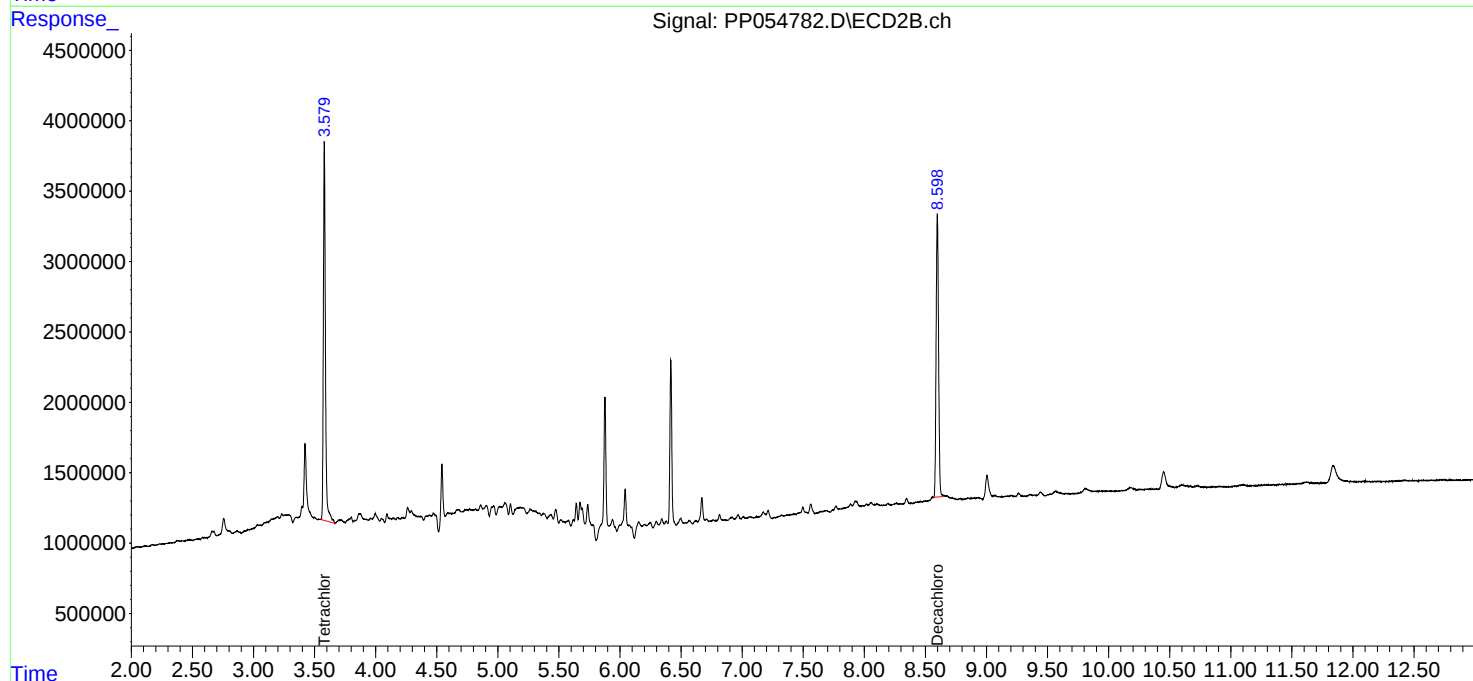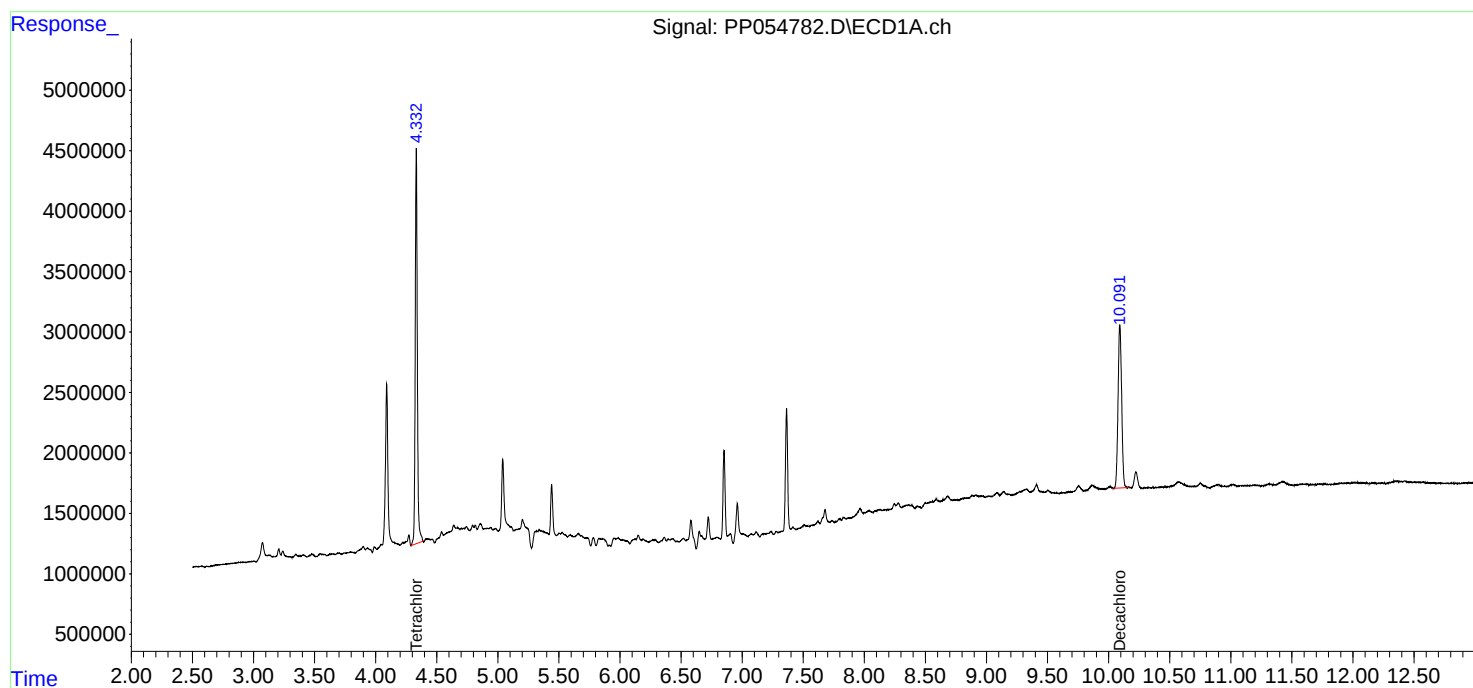

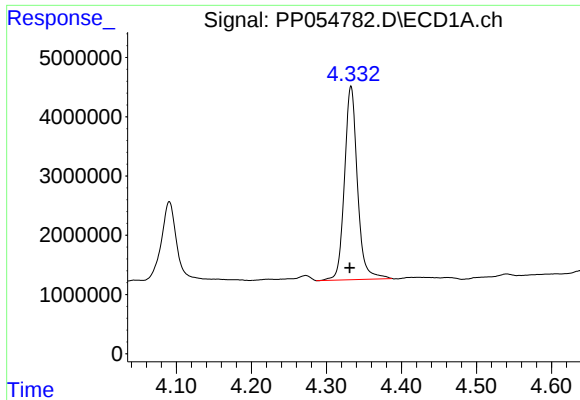


#1 Tetrachloro-m-xylene

R.T.: 4.332 min
Delta R.T.: 0.001 min
Response: 39164744
Conc: 21.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
B-P-19B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/23/2023
Supervised By :Ankita Jodhani 01/23/2023

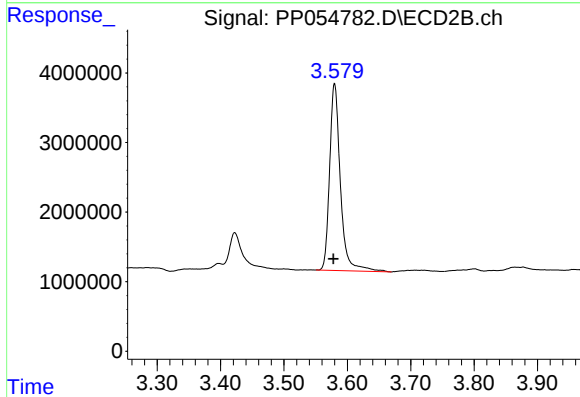


#1 Tetrachloro-m-xylene

R.T.: 3.580 min
Delta R.T.: 0.002 min
Response: 31748120
Conc: 19.83 ng/ml

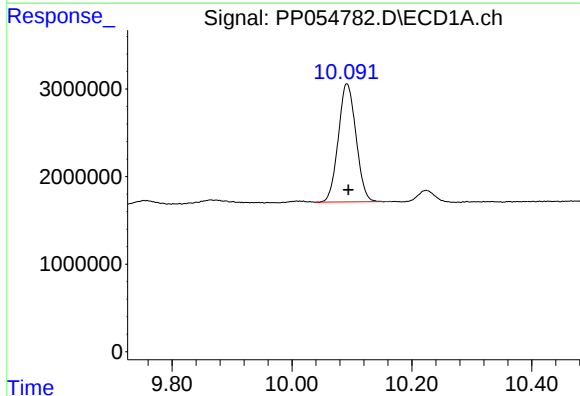

#2 Decachlorobiphenyl

R.T.: 10.092 min
Delta R.T.: -0.003 min
Response: 27629542
Conc: 20.58 ng/ml

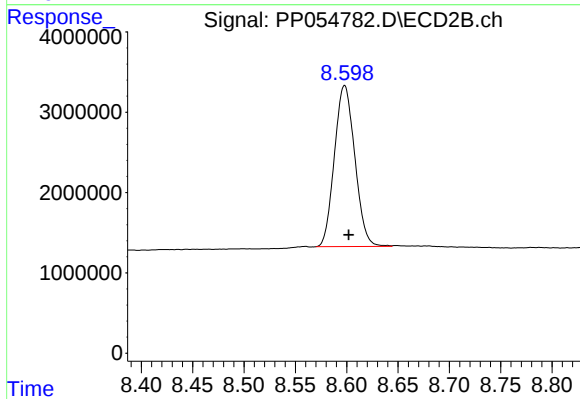

#2 Decachlorobiphenyl

R.T.: 8.598 min
Delta R.T.: -0.004 min
Response: 27740185
Conc: 19.37 ng/ml