
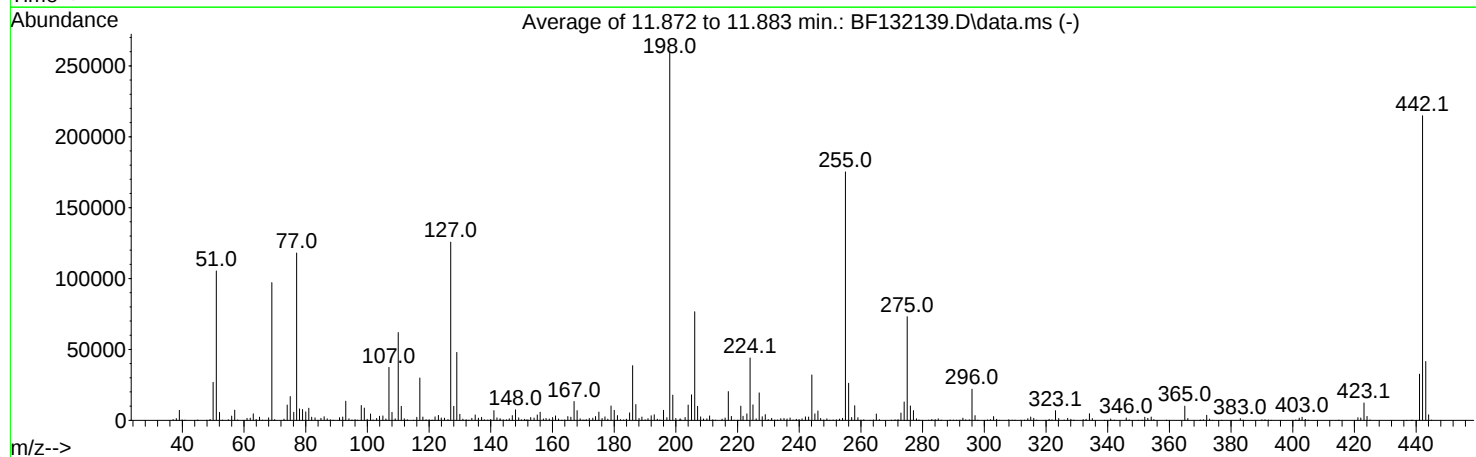


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF011923\  
 Data File : BF132139.D  
 Acq On : 19 Jan 2023 10:46  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF011923.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jan 20 00:50:42 2023

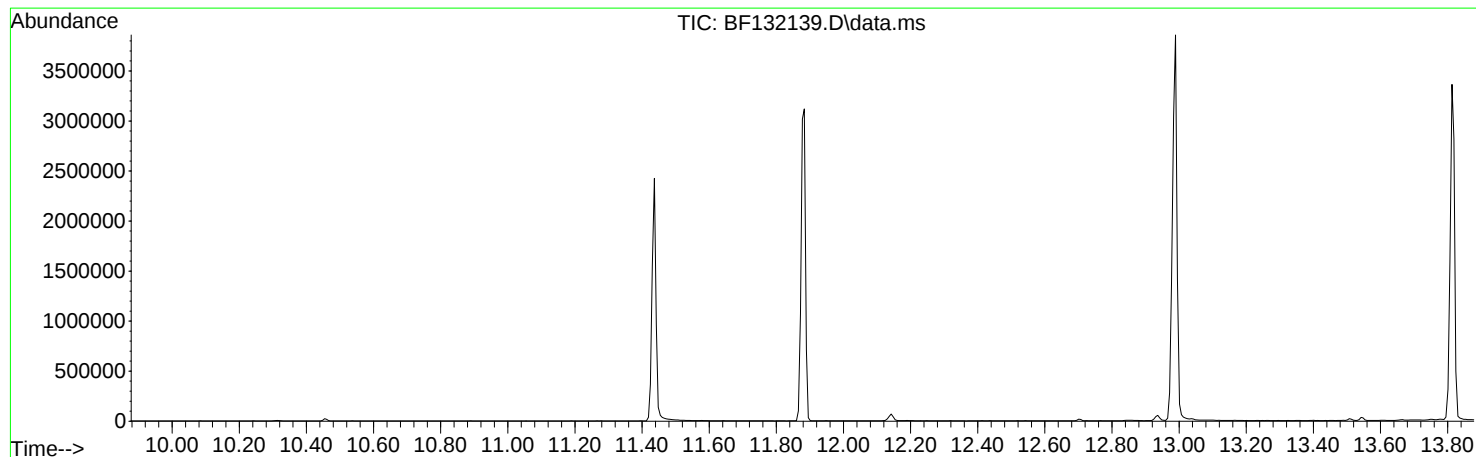




AutoFind: Scans 1536, 1537, 1538; Background Corrected with Scan 1531

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 40.6         | 105352     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1732       | PASS                |
| 69             | 198             | 0.00            | 100             | 37.4         | 97160      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 531        | PASS                |
| 127            | 198             | 10              | 80              | 48.4         | 125669     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.7          | 1878       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 259491     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 17763      | PASS                |
| 275            | 198             | 10              | 60              | 28.2         | 73136      | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 10047      | PASS                |
| 441            | 198             | 0.01            | 100             | 12.5         | 32537      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 214824     | PASS                |
| 443            | 442             | 15              | 24              | 19.3         | 41519      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF011923\  
 Data File : BF132139.D  
 Acq On : 19 Jan 2023 10:46  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Jan 20 05:07:54 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF011923.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jan 20 00:50:42 2023  
 Response via : Initial Calibration

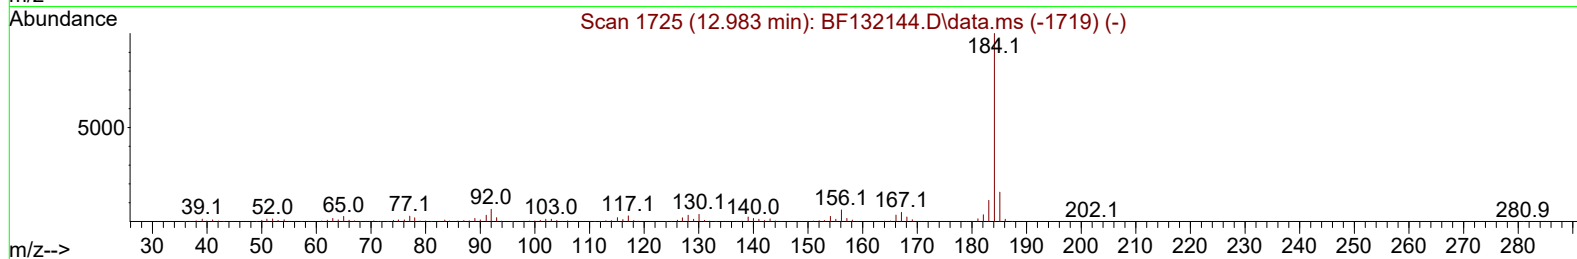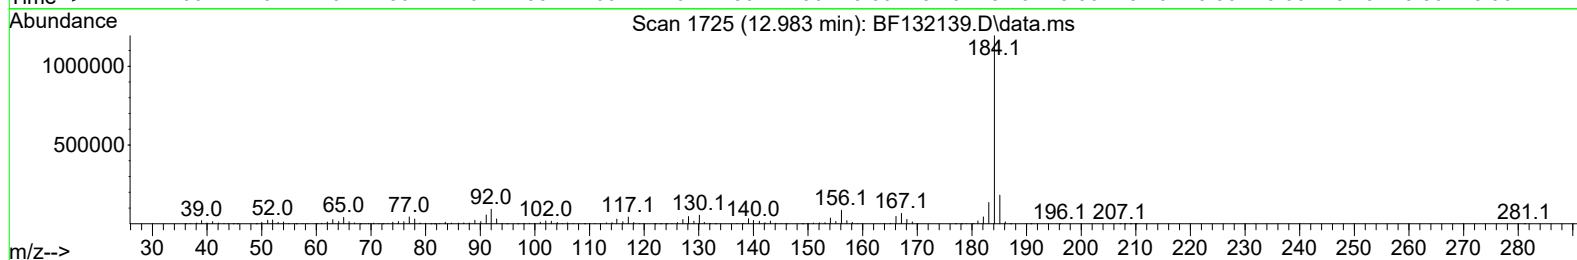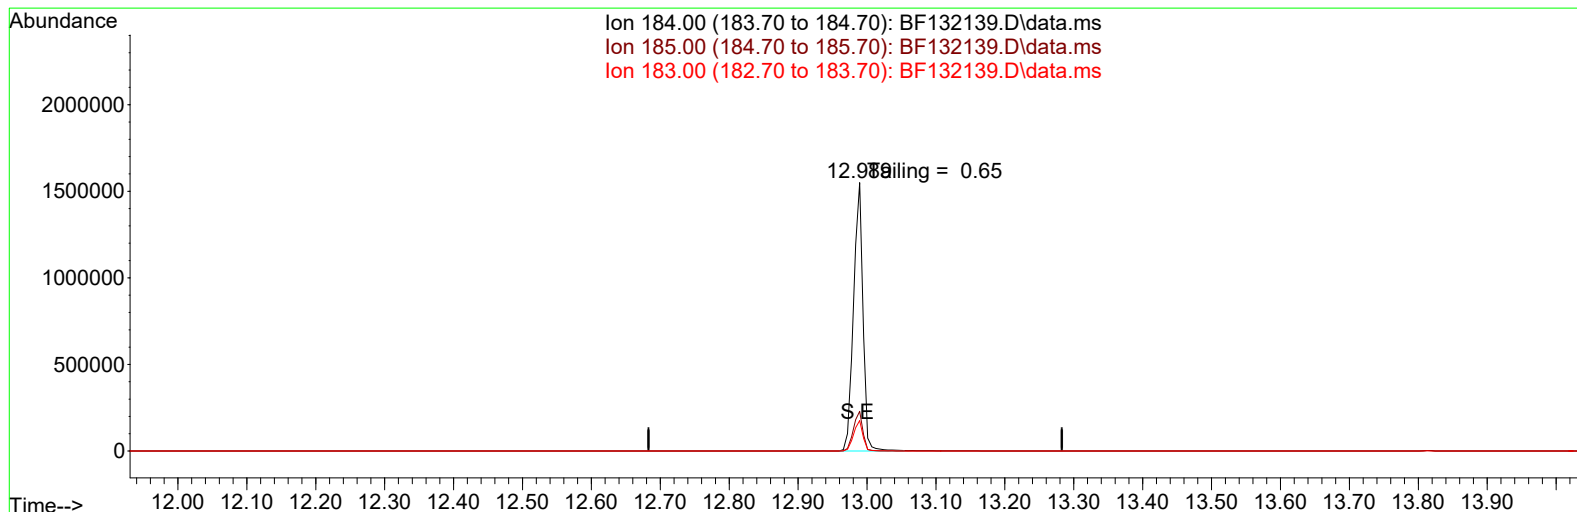

TIC: BF132139.D\data.ms

**(77) Benzidine**

12.983min (-12.983) 0.00 ng




response 0

| Ion    | Exp%   | Act%  |
|--------|--------|-------|
| 184.00 | 100.00 | 0.00  |
| 185.00 | 15.60  | 0.00# |
| 183.00 | 11.20  | 0.00# |
| 0.00   | 0.00   | 0.00  |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF011923\  
 Data File : BF132139.D  
 Acq On : 19 Jan 2023 10:46  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Jan 20 05:07:54 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF011923.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jan 20 00:50:42 2023  
 Response via : Initial Calibration

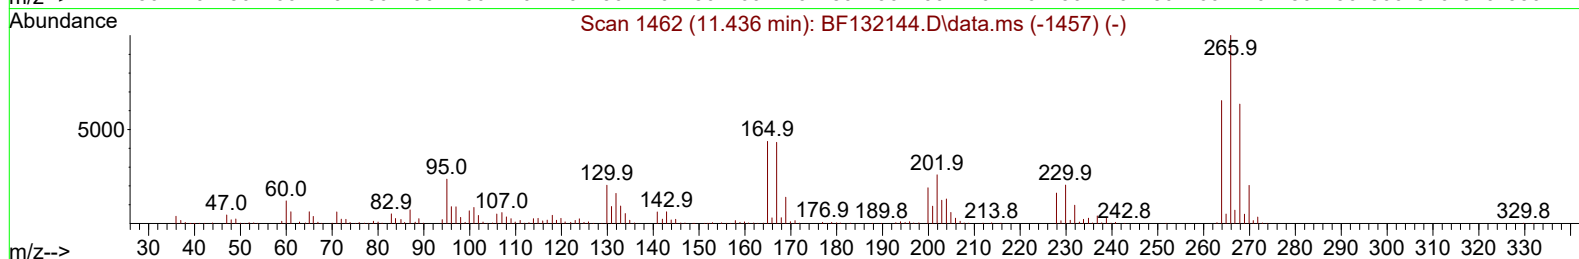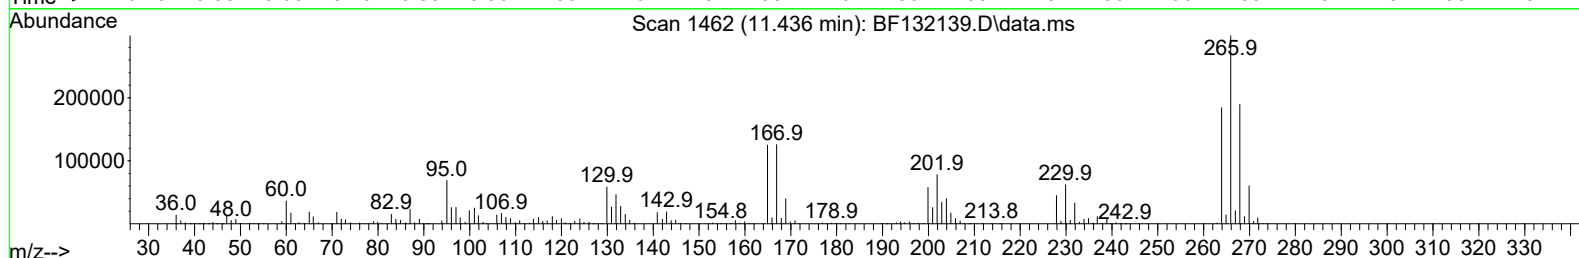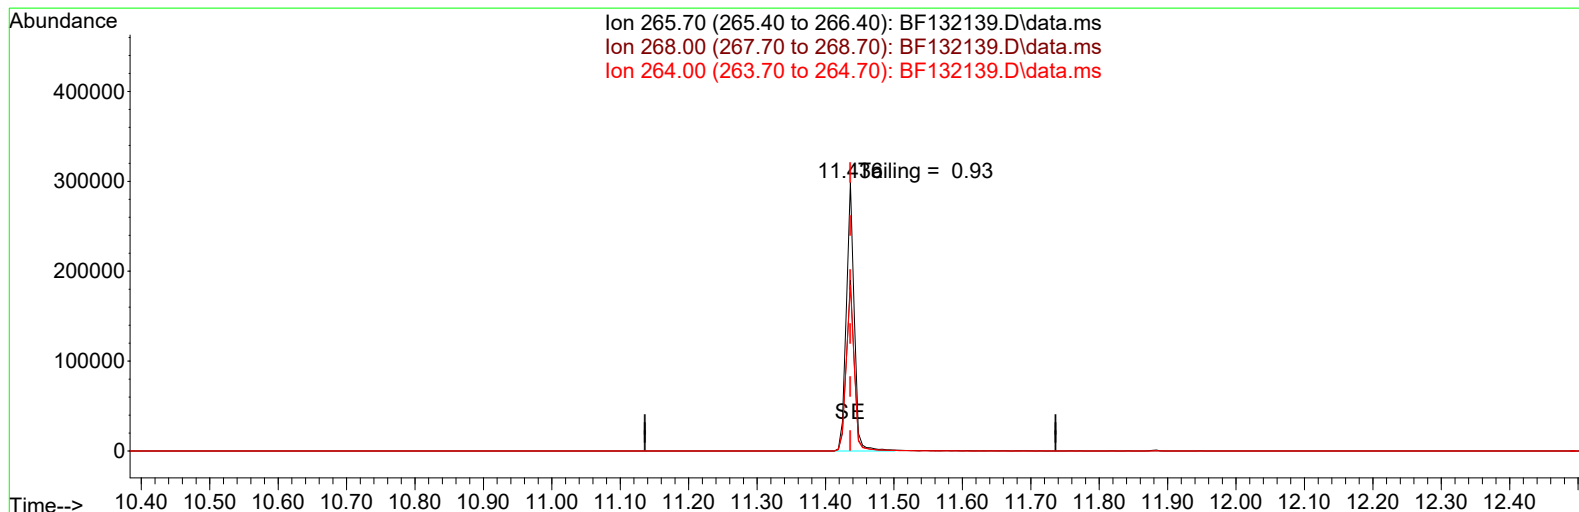

TIC: BF132139.D\data.ms

**(70) Pentachlorophenol (C)**

**11.436min (+ 0.000) 469730.41 ng**

**response 241341**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.50  | 63.47  |
| 264.00 | 65.40  | 61.76  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 1/19/2023     | BNA_F            | <u>BF132139.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 531182           | 13.813             |
| DDD           | 6943             | 13.542             |
| DDE           | 353              | 13.172             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 7296          | 538478           | 1.35               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP