
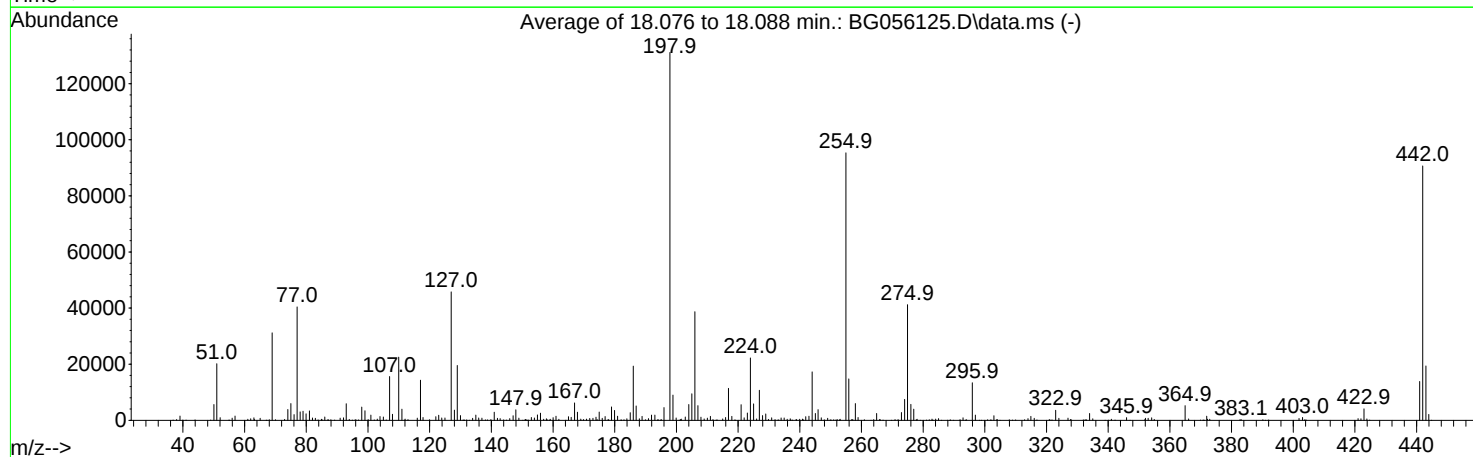


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122722\
 Data File : BG056125.D
 Acq On : 27 Dec 2022 14:13
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 28 05:20:14 2022

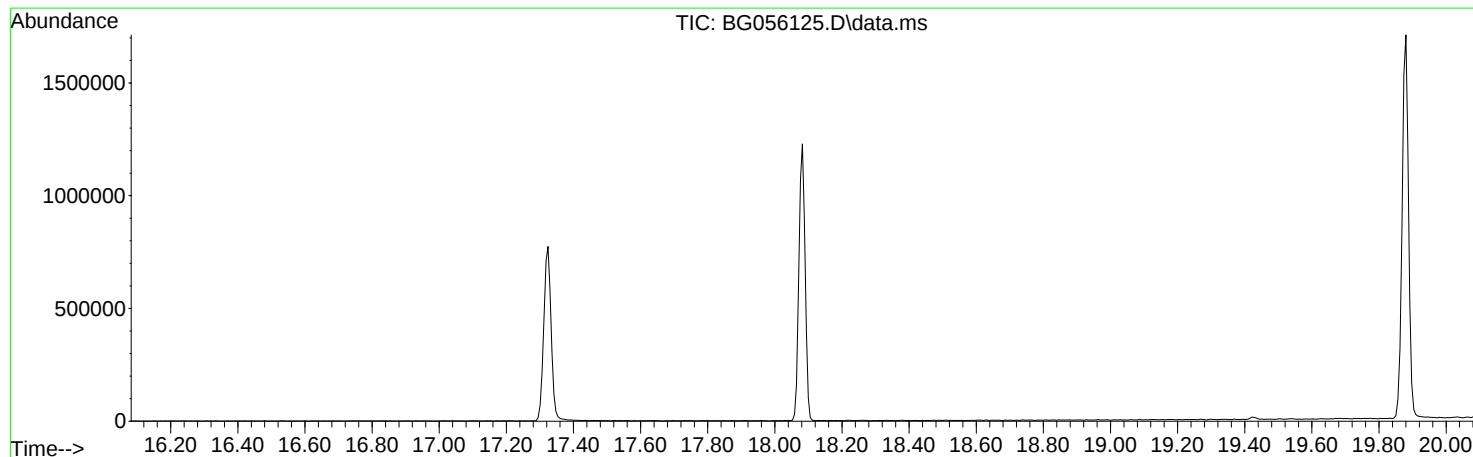




AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2510

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.4	20160	PASS
68	69	0.00	2	0.7	205	PASS
69	198	0.00	100	23.8	31181	PASS
70	69	0.00	2	0.6	187	PASS
127	198	10	80	34.9	45787	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	131133	PASS
199	198	5	9	6.8	8962	PASS
275	198	10	60	31.4	41187	PASS
365	198	1	100	4.0	5228	PASS
441	198	0.01	100	10.6	13843	PASS
442	442	50	100	100.0	90691	PASS
443	442	15	24	21.4	19397	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122722\
Data File : BG056125.D
Acq On : 27 Dec 2022 14:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 28 06:08:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

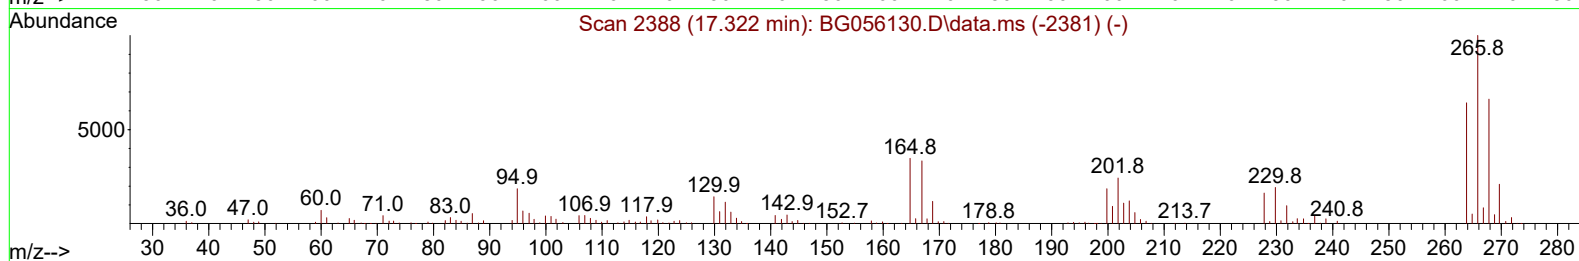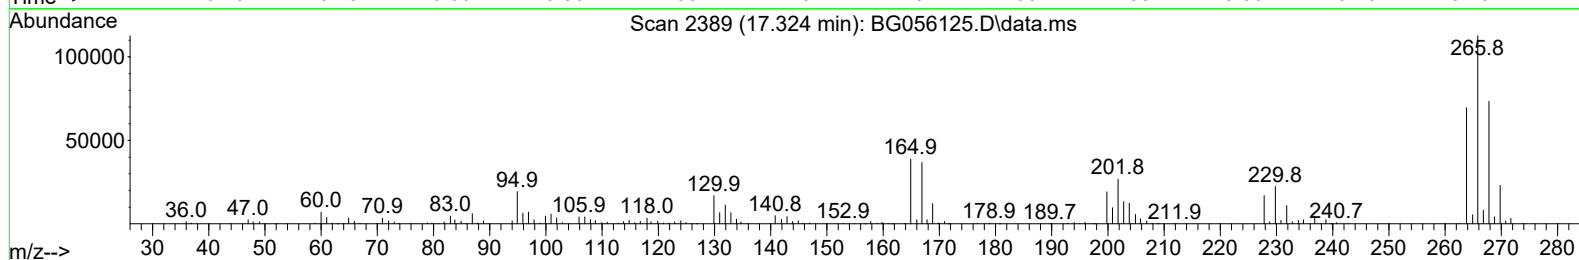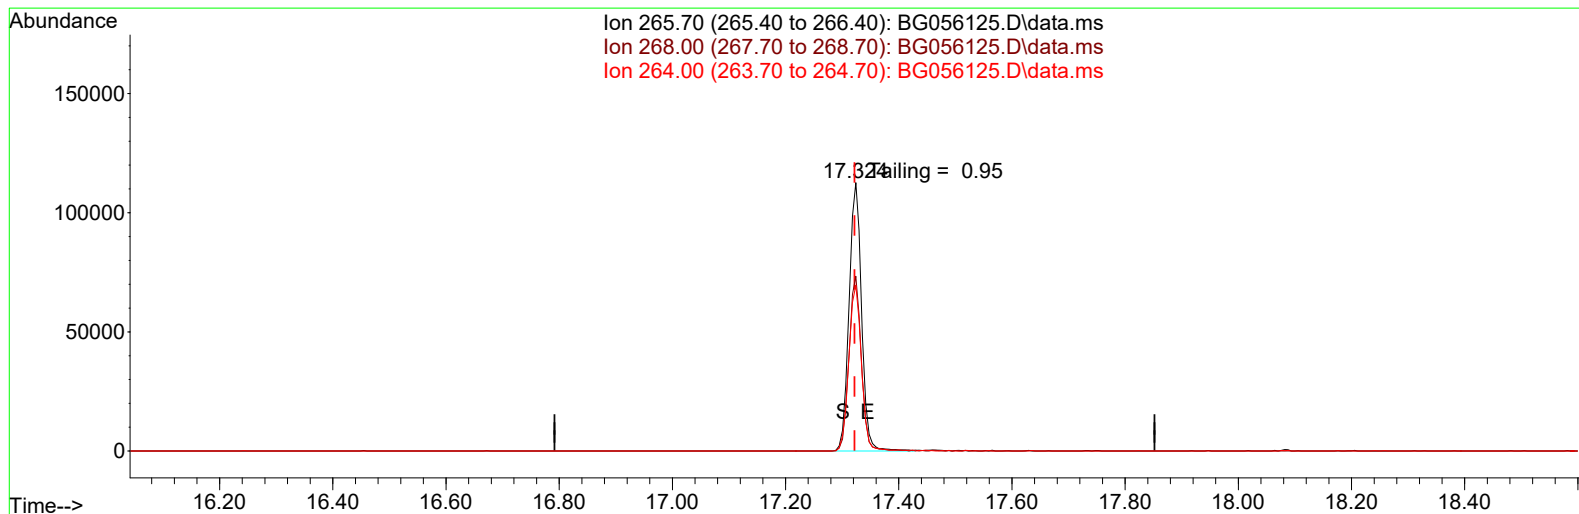

TIC: BG056125.D\data.ms

(70) Pentachlorophenol (C)

17.324min (+ 0.002) 311339.09 ng




response 173323

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	65.12
264.00	64.30	61.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG122722\
Data File : BG056125.D
Acq On : 27 Dec 2022 14:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Dec 28 06:08:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 28 05:20:14 2022
Response via : Initial Calibration

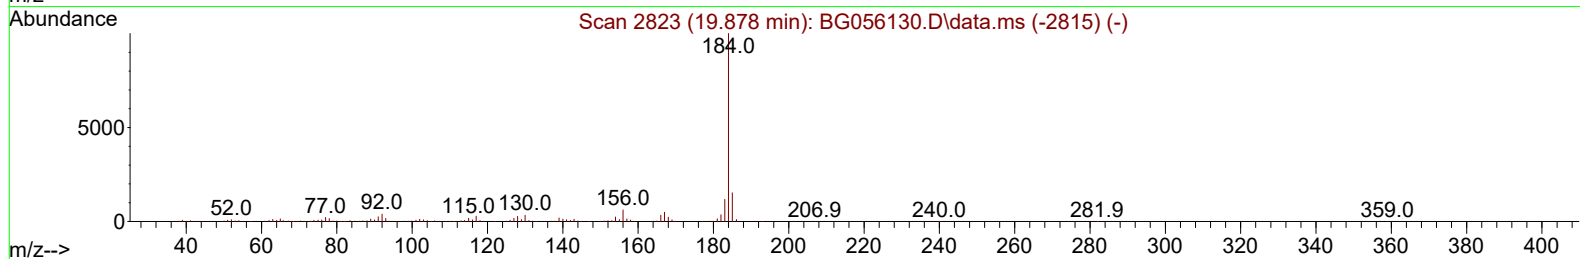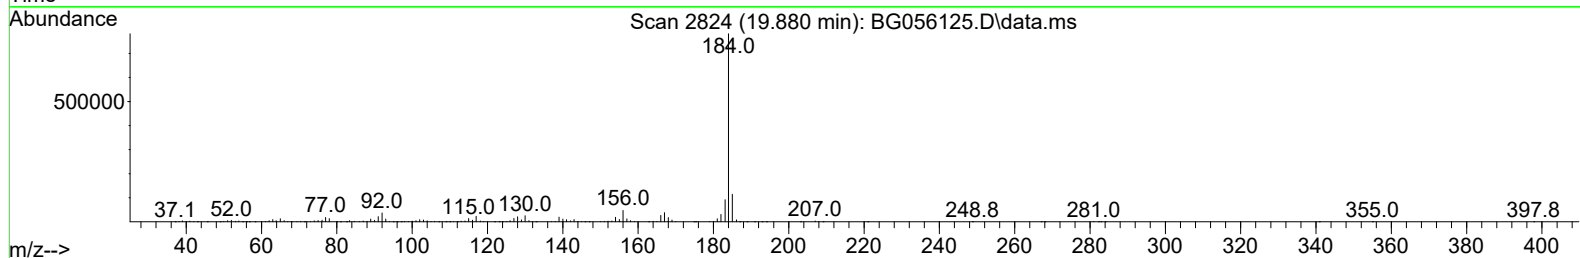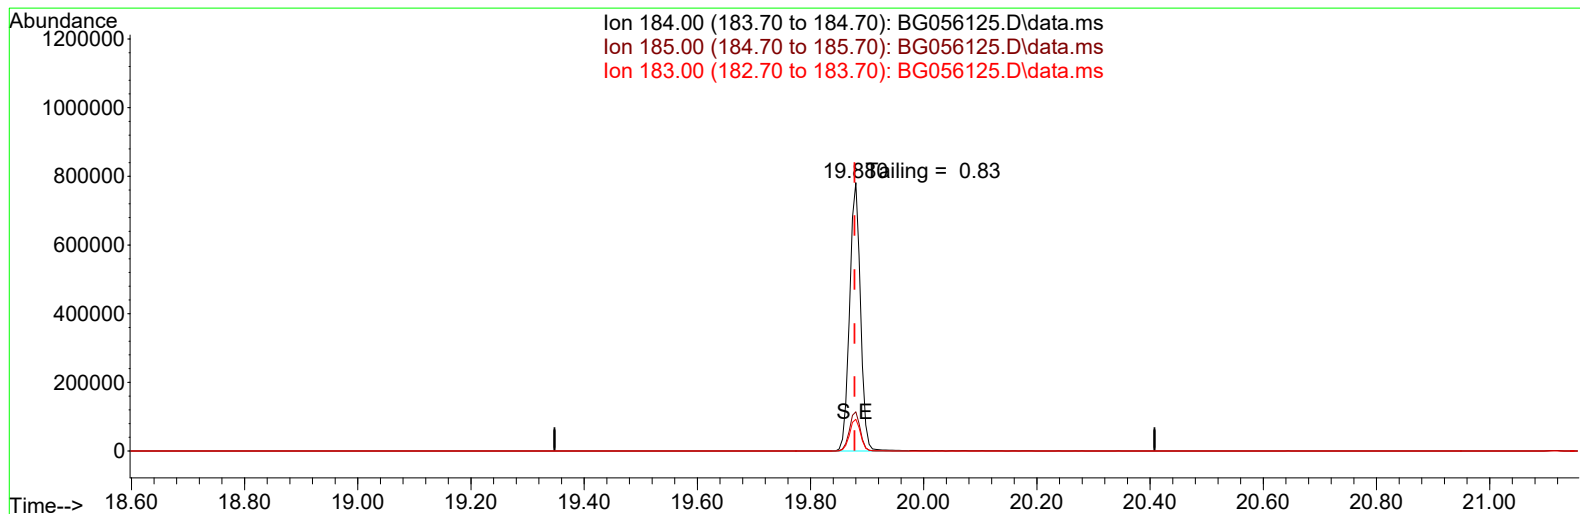

TIC: BG056125.D\data.ms

(77) Benzidine

19.880min (+ 0.002) 489409.95 ng

response 1046213

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.63
183.00	11.70	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/27/2022	BNA_G	BG056125.D
Compound Name	Response	Retention Time
DDT	475579	21.114
DDD	6426	20.714
DDE	0	20.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6426	482005	1.33

Instrument :
BNA_G
ClientSampleId :
DFTPP