
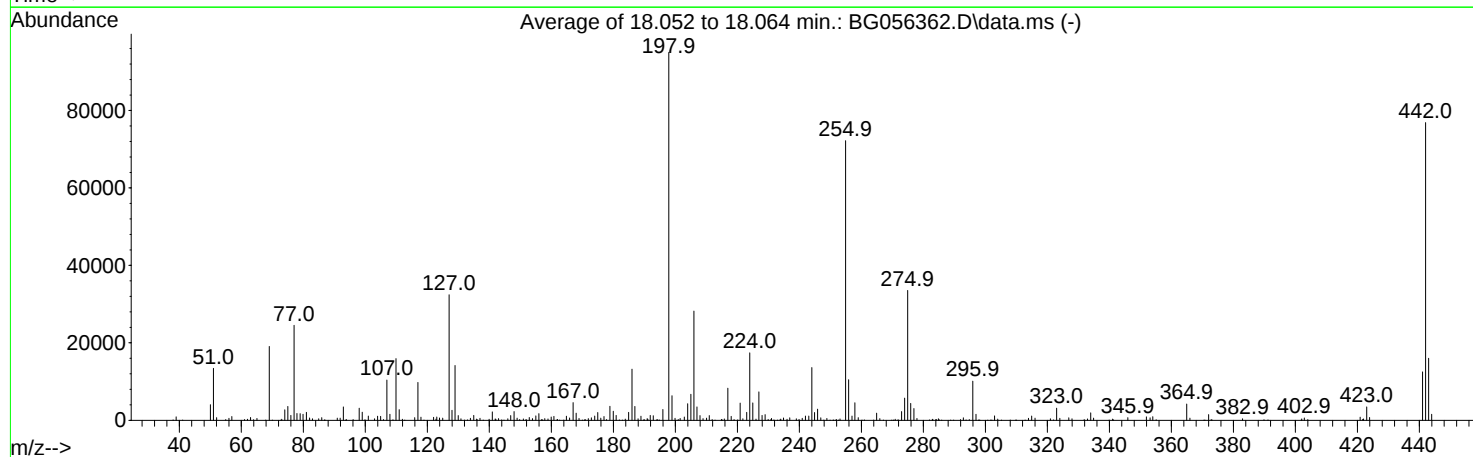


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012023\
Data File : BG056362.D
Acq On : 20 Jan 2023 11:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 19 00:31:30 2023

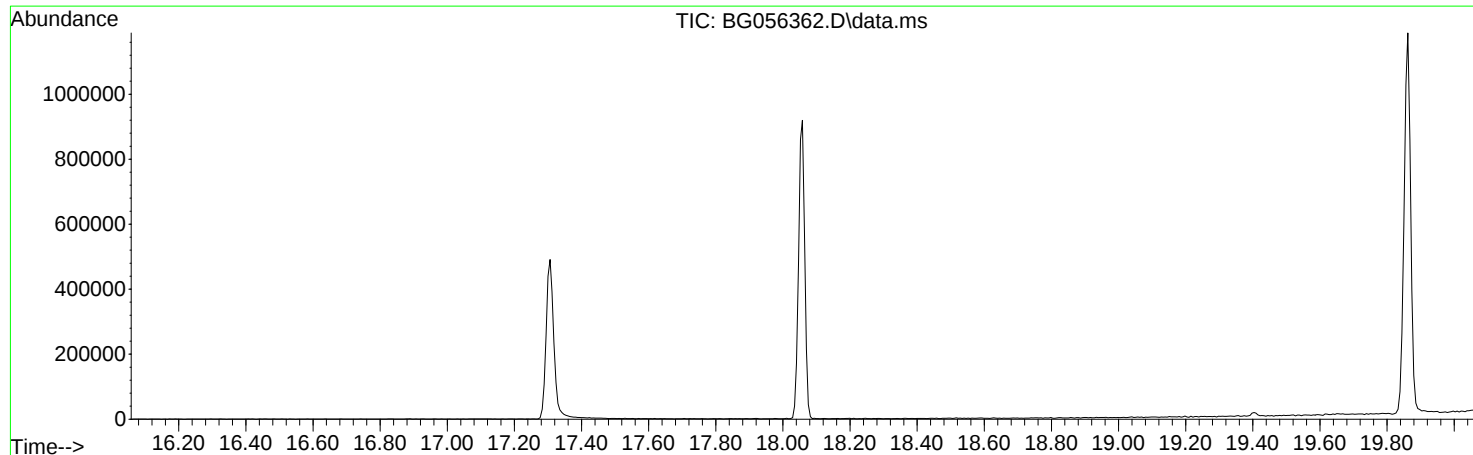




AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	14.1	13408	PASS
68	69	0.00	2	0.4	67	PASS
69	198	0.00	100	20.1	19060	PASS
70	69	0.00	2	0.3	53	PASS
127	198	10	80	34.1	32427	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	94995	PASS
199	198	5	9	6.7	6325	PASS
275	198	10	60	35.3	33512	PASS
365	198	1	100	4.4	4190	PASS
441	198	0.01	100	13.1	12489	PASS
442	442	50	100	100.0	76885	PASS
443	442	15	24	20.8	16001	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012023\
Data File : BG056362.D
Acq On : 20 Jan 2023 11:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 23 01:11:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:31:30 2023
Response via : Initial Calibration

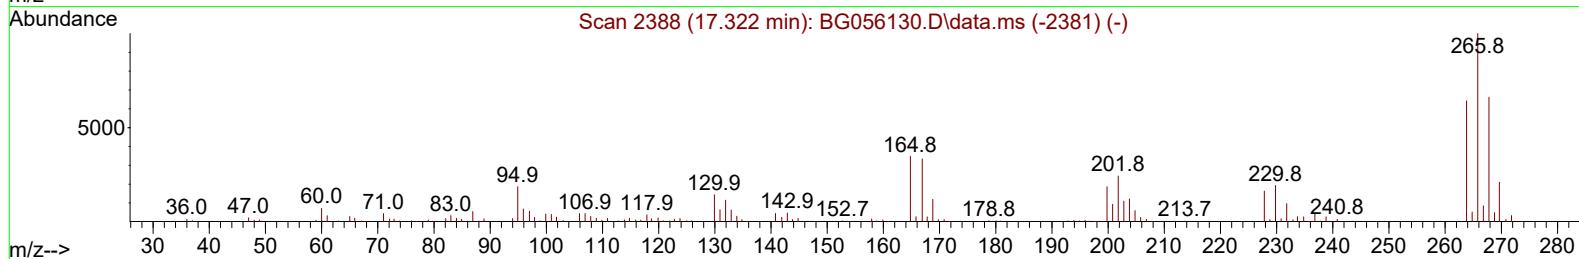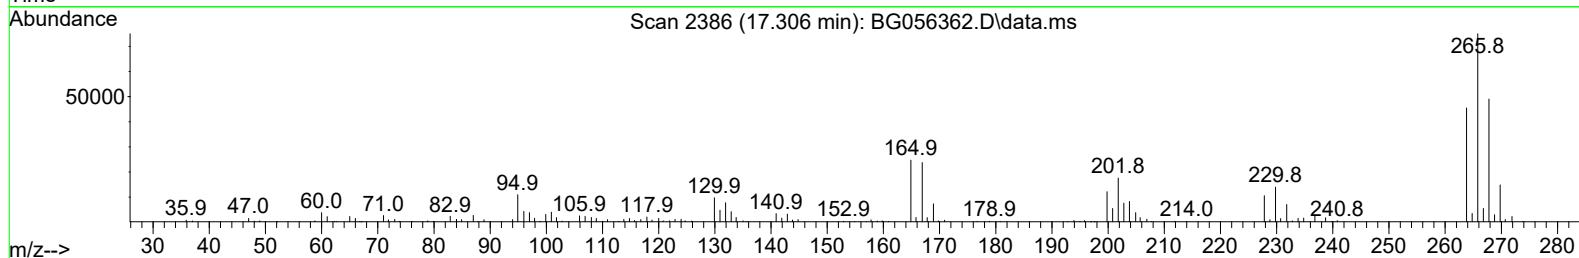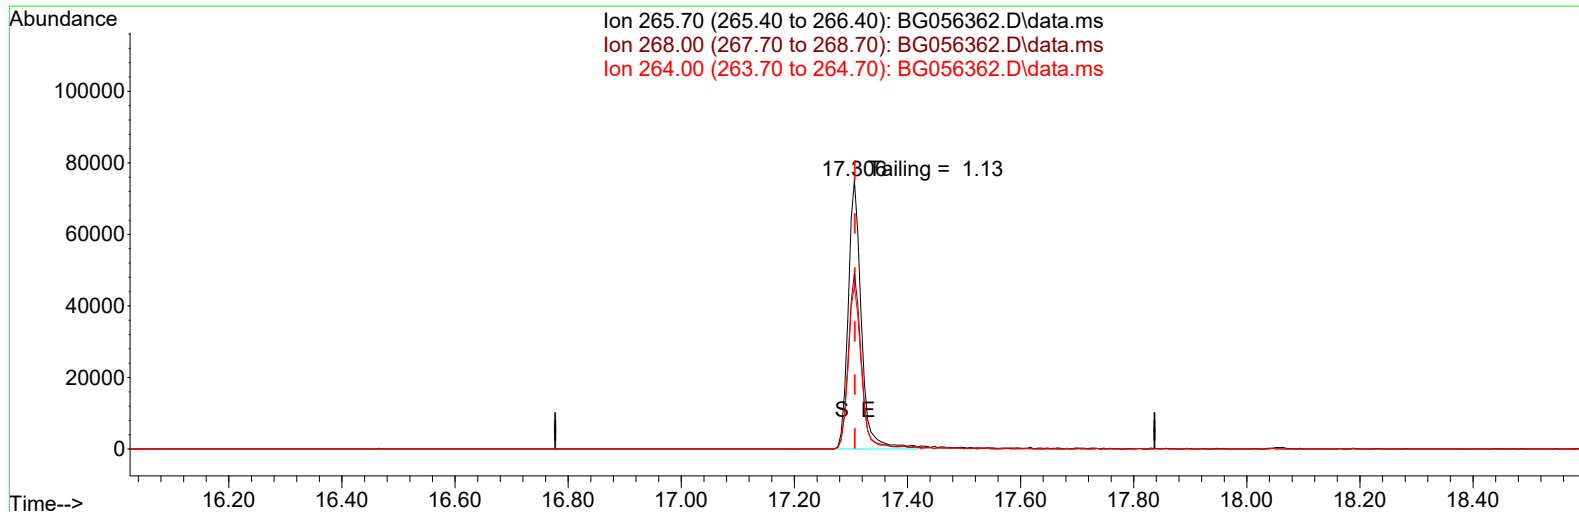

TIC: BG056362.D\data.ms

(70) Pentachlorophenol (C)

17.306min (-0.001) 24675.65 ng




response 121606

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	65.36
264.00	64.30	60.61
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012023\  
Data File : BG056362.D  
Acq On    : 20 Jan 2023  11:01  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 23 01:11:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:31:30 2023
Response via : Initial Calibration

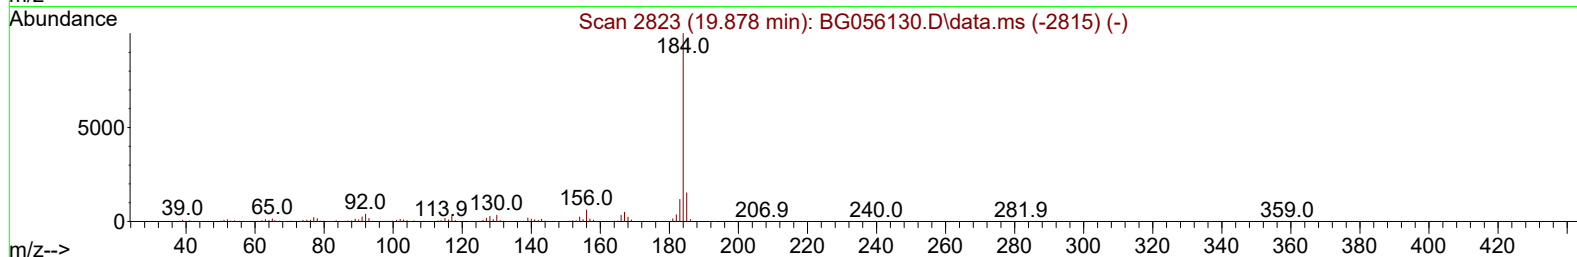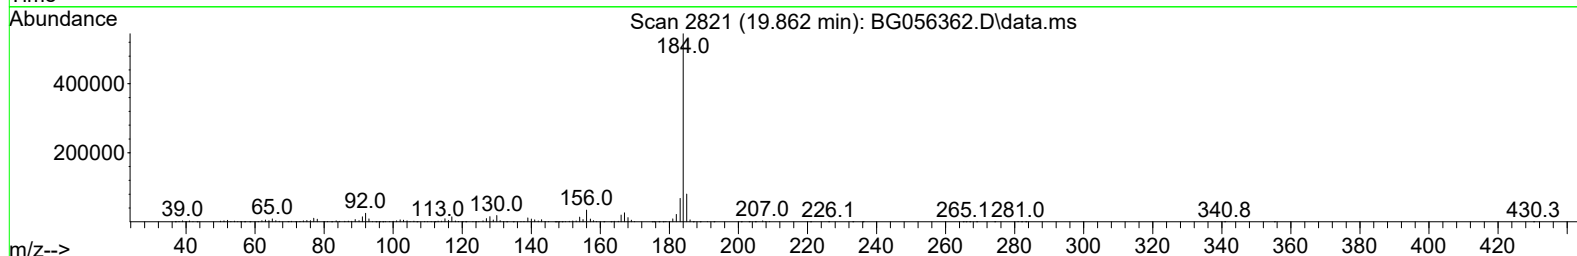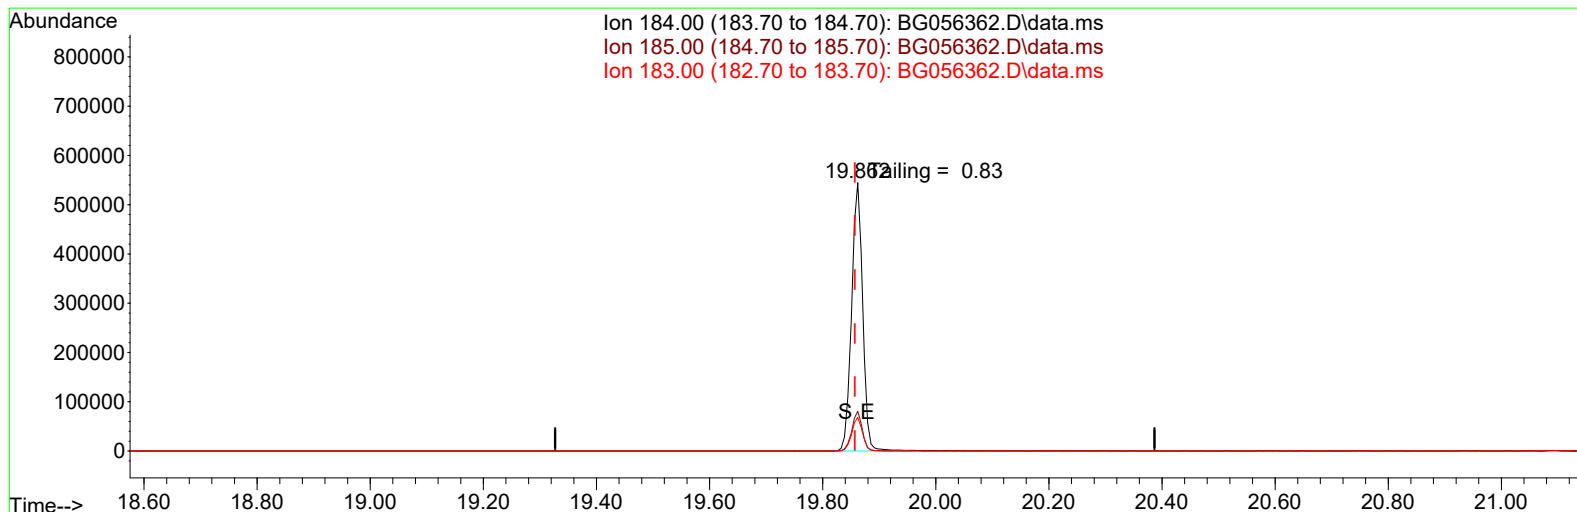

TIC: BG056362.D\data.ms

(77) Benzidine

19.862min (+ 0.005) 375019.64 ng

response **735969**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	15.20	14.79
--------	-------	-------

183.00	11.70	12.48
--------	-------	-------

0.00 0.00 0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/20/2023	BNA_G	<u>BG056362.D</u>
Compound Name	Response	Retention Time
DDT	336671	21.09
DDD	11056	20.638
DDE	1300	20.138
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12356	349027	3.54

Instrument :
BNA_G
ClientSampleId :
DFTPP