


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
Data File : BG056402.D
Acq On : 24 Jan 2023 14:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 25 04:54:56 2023

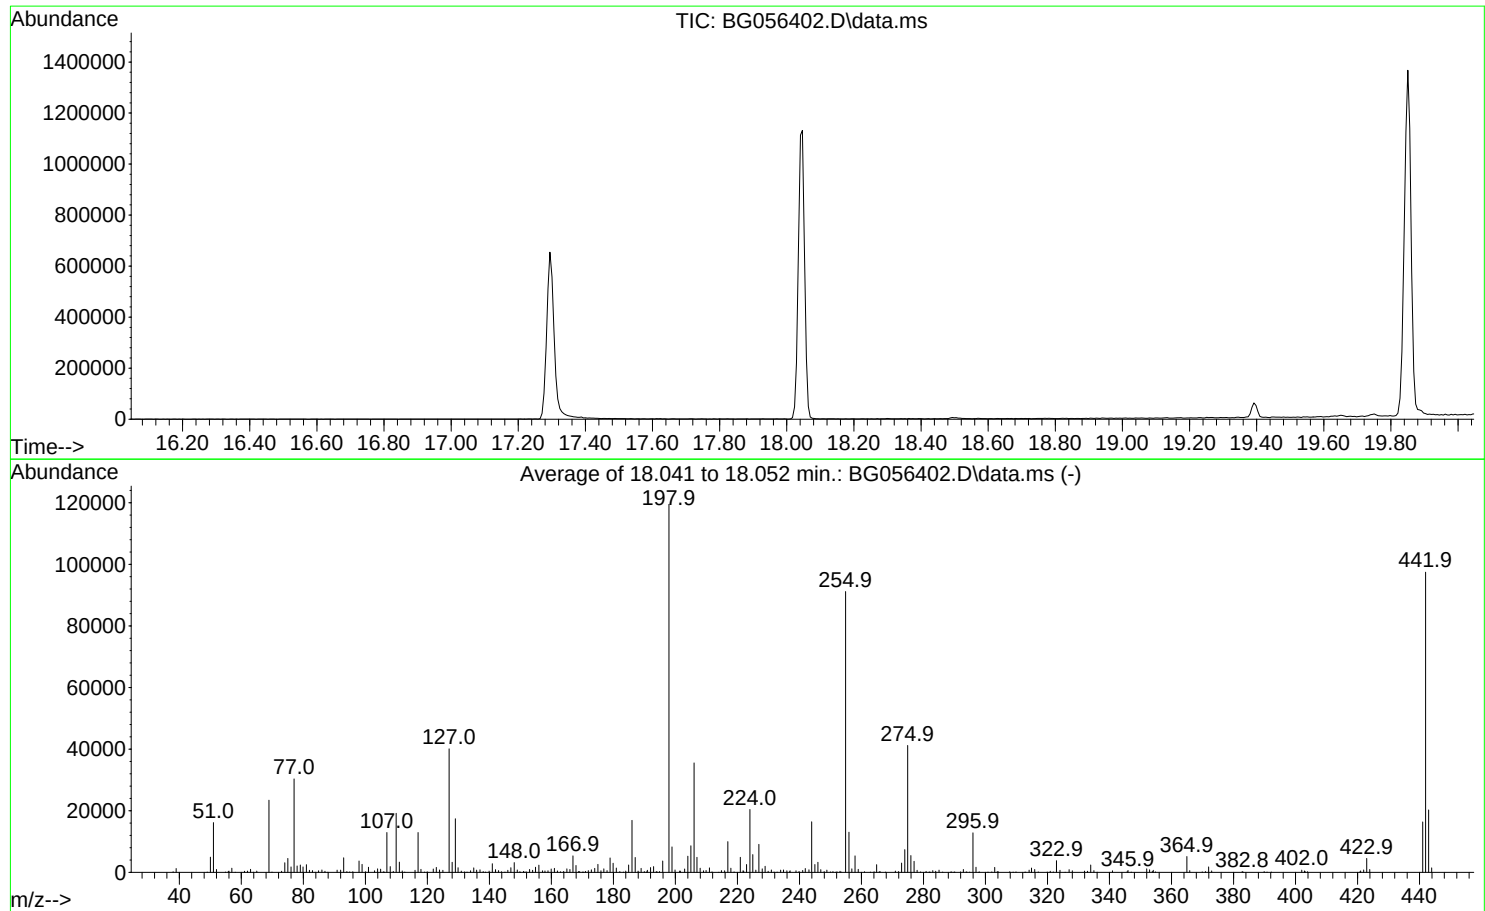




AutoFind: Scans 2511, 2512, 2513; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	13.5	16130	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	19.6	23416	PASS
70	69	0.00	2	0.3	70	PASS
127	198	10	80	33.6	40109	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	119448	PASS
199	198	5	9	6.9	8243	PASS
275	198	10	60	34.5	41197	PASS
365	198	1	100	4.3	5125	PASS
441	198	0.01	100	13.7	16337	PASS
442	442	50	100	100.0	97448	PASS
443	442	15	24	20.8	20221	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
Data File : BG056402.D
Acq On : 24 Jan 2023 14:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 25 08:31:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 04:54:56 2023
Response via : Initial Calibration

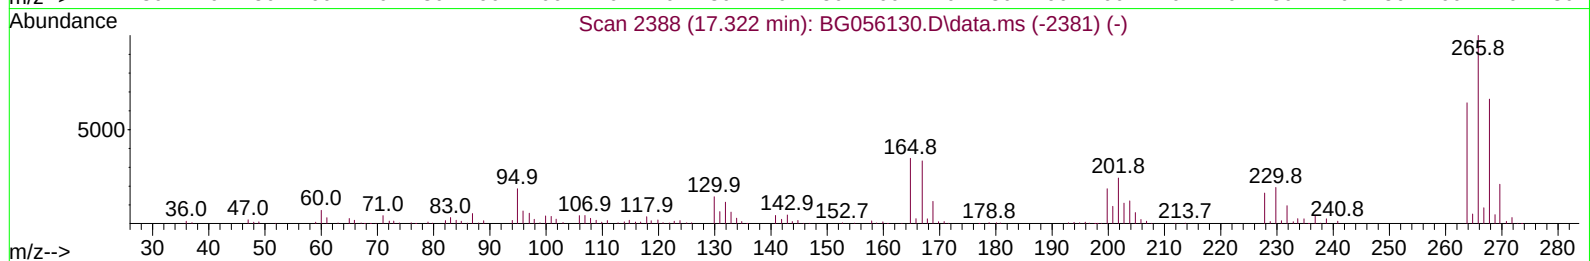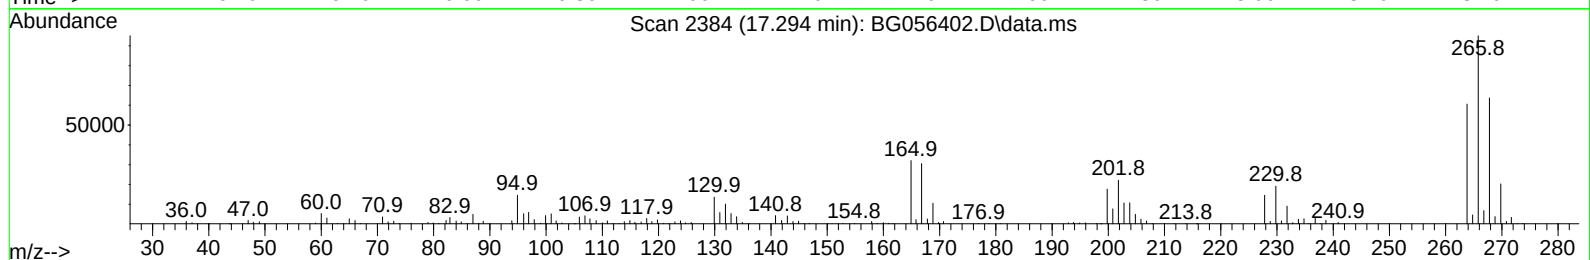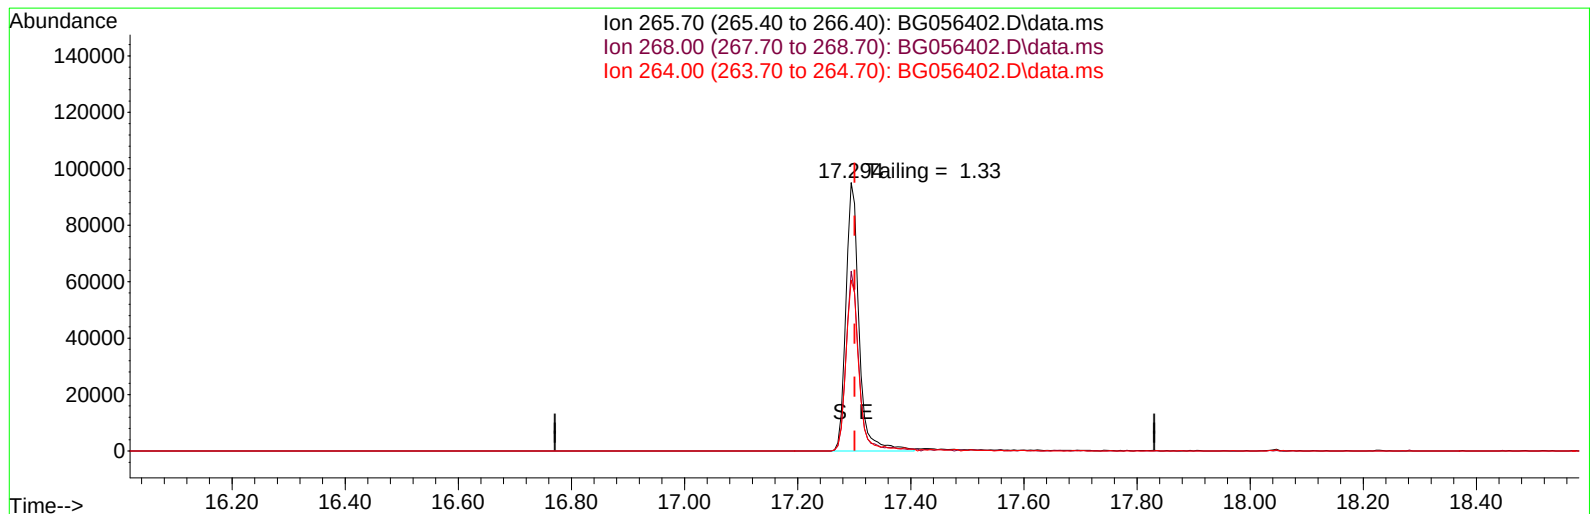

TIC: BG056402.D\data.ms

(70) Pentachlorophenol (C)

17.294min (-0.006) 23265.80 ng




response 153939

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	66.97
264.00	64.30	63.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012423\
Data File : BG056402.D
Acq On : 24 Jan 2023 14:15
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 25 08:31:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 04:54:56 2023
Response via : Initial Calibration

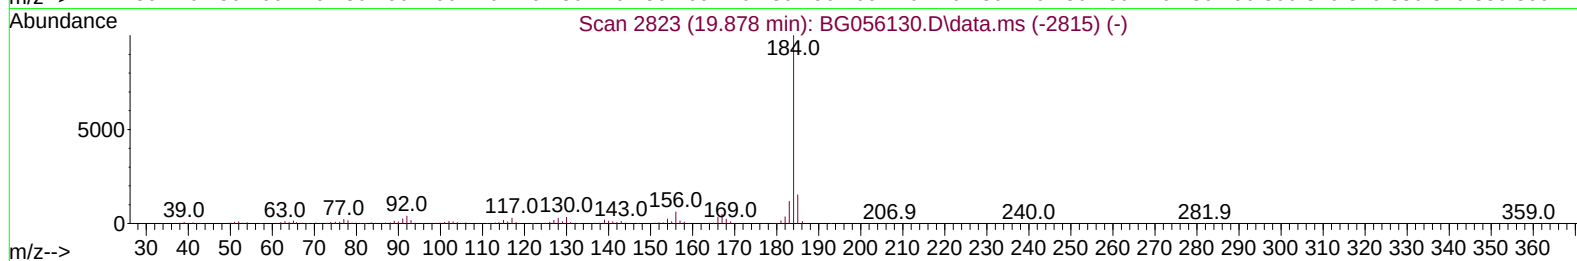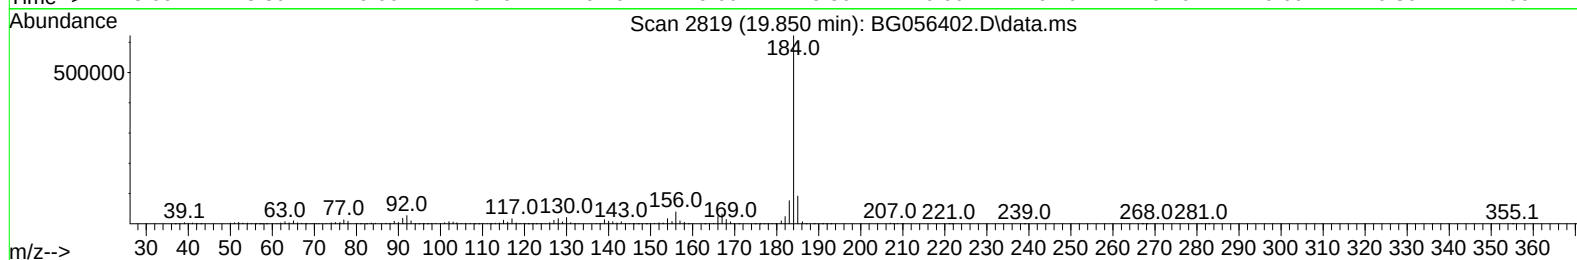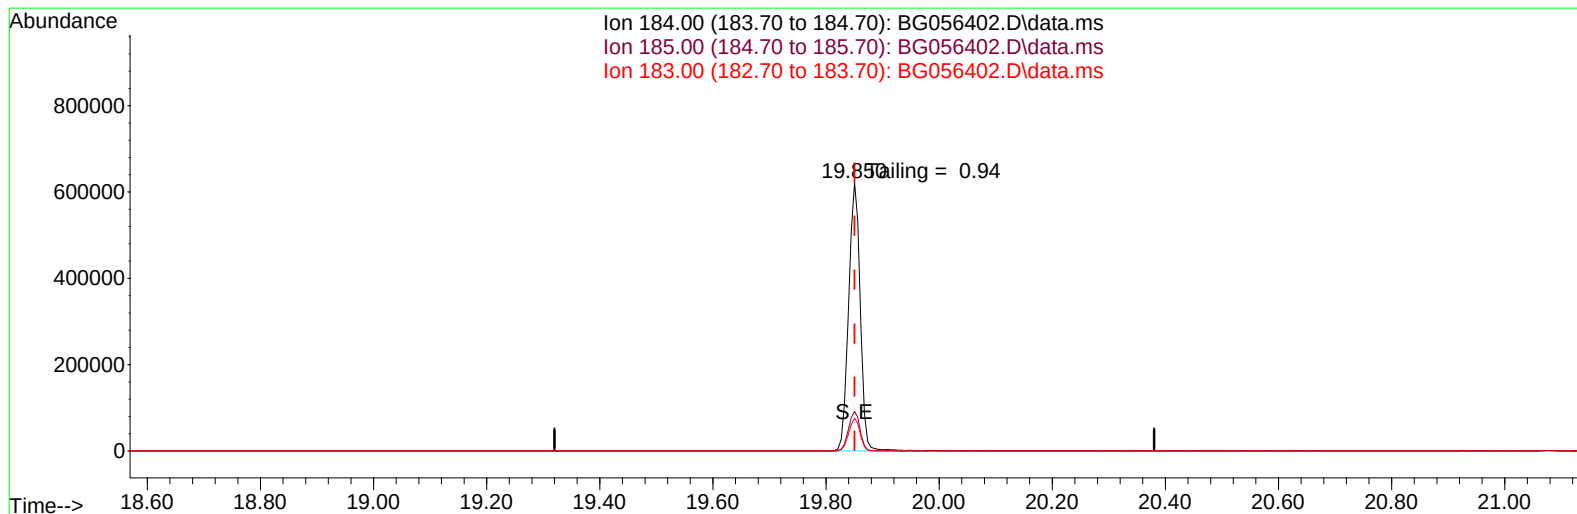

TIC: BG056402.D\data.ms

(77) Benzidine

19.850min (+ 0.000) 416502.24 ng

response 890358

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.76
183.00	11.70	12.24
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/24/2023	BNA_G	<u>BG056402.D</u>
Compound Name	Response	Retention Time
DDT	431605	21.078
DDD	22595	20.626
DDE	1699	20.126
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24294	455899	5.33

Instrument :
BNA_G
ClientSampleId :
DFTPP