

Prep Standard - Chemical Standard Summary**Order ID :** O1233**Test :** Diesel Range Organics**Prepbatch ID :** PB150379,**Sequence ID/Qc Batch ID:** FF012023,FF012323,**Standard ID :**

EP2279,EP2293,PP20614,PP21001,PP21133,PP21134,PP21215,PP21323,PP21324,PP21325,PP21326,PP21327,

Chemical ID :E2865,E3386,E3412,E3419,E3427,E3432,E3452,E3456,E3459,P10858,P11154,P11164,P11165,P11166,P11167,P11168,
P11169,P11473,P11474,P11749,P11750,P11751,

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2279	11/28/2022	04/13/2023	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 11/28/2022

FROM 4000.00000gram of E3412 = Final Quantity: 4000.000 gram

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2017	1:1 ACETONE/METHYLENE CHLORIDE	EP2293	01/17/2023	06/21/2023	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 01/17/2023

FROM 8000.00000ml of E3452 + 8000.00000ml of E3456 = Final Quantity: 16000.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3979	100/100 PPM DRO ICV (RESTEK)	PP20614	08/26/2022	01/27/2023	Yogesh Patel	None	None	Ankita Jodhani
								08/29/2022

FROM 1.00000ml of P11154 + 2.00000ml of P11749 + 7.00000ml of E3386 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3609	20 PPM DRO SPIKE SOLUTION (RESTEK)	PP21001	10/24/2022	01/27/2023	Yogesh Patel	None	None	Ankita Jodhani
								10/27/2022

FROM 1.00000ml of P10858 + 1.00000ml of P11749 + 48.00000ml of E3419 = Final Quantity: 50.000 ml

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
433	100/100 PPM DRO (Restek)	PP21133	11/14/2022	05/07/2023	Yogesh Patel	None	None	Ankita Jodhani 11/15/2022
<u>FROM</u>	1.00000ml of P11164 + 1.00000ml of P11750 + 1.00000ml of P11751 + 7.00000ml of E3427 = Final Quantity: 10.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3796	100/100 PPM DRO STD (CPI)	PP21134	11/14/2022	05/07/2023	Yogesh Patel	None	None	Ankita Jodhani 11/15/2022
<u>FROM</u>	1.00000ml of P11165 + 1.00000ml of P11473 + 1.00000ml of P11474 + 7.00000ml of E3427 = Final Quantity: 10.000 ml							

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
147	20 PPM DRO Surrogate Spike Solution	PP21215	12/02/2022	05/22/2023	Yogesh Patel	None	None	Ankita Jodhani 12/05/2022
<u>FROM</u> 1.00000ml of P11166 + 1.00000ml of P11167 + 1.00000ml of P11168 + 1.00000ml of P11169 + 196.00000ml of E3432 = Final Quantity: 200.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
435	50 PPM ICC DRO STD (Restek)	PP21323	12/30/2022	05/07/2023	Yogesh Patel	None	None	Ankita Jodhani 01/03/2023
<u>FROM</u>	0.50000ml of E3452 + 0.50000ml of PP21133 = Final Quantity: 1.000 ml							

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
437	20 PPM ICC DRO STD (Restek)	PP21324	12/30/2022	05/07/2023	Yogesh Patel	None	None	Ankita Jodhani
01/03/2023								

FROM 0.80000ml of E3452 + 0.20000ml of PP21133 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
438	10 PPM ICC DRO STD (Restek)	PP21325	12/30/2022	05/07/2023	Yogesh Patel	None	None	Ankita Jodhani
01/03/2023								

FROM 0.90000ml of E3452 + 0.10000ml of PP21133 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
439	5 PPM ICC DRO STD (Restek)	PP21326	12/30/2022	05/07/2023	Yogesh Patel	None	None	Ankita Jodhani
01/03/2023								

FROM 0.90000ml of E3452 + 0.10000ml of PP21323 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3608	50 PPM ICV DRO STD (RESTEK)	PP21327	12/30/2022	01/27/2023	Yogesh Patel	None	None	Ankita Jodhani
01/03/2023								

FROM 0.50000ml of E3452 + 0.50000ml of PP20614 = Final Quantity: 1.000 ml

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	12/31/2024	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	22G0762001	02/14/2023	08/15/2022 / Rajesh	08/05/2022 / Rajesh	E3386

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	139404	04/13/2023	10/18/2022 / Rajesh	10/13/2022 / Rajesh	E3412

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	22H1562002	03/17/2023	10/17/2022 / Rajesh	09/28/2022 / Rajesh	E3419

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	2212962012	05/07/2023	11/07/2022 / Rajesh	10/18/2022 / Rajesh	E3427

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	2212962012	05/22/2023	11/22/2022 / Rajesh	11/14/2022 / Rajesh	E3432

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	22K0762004	06/21/2023	12/29/2022 / Rajesh	12/21/2022 / Rajesh	E3452

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	22J0461011	07/17/2023	01/17/2023 / Rajesh	01/11/2023 / Rajesh	E3456

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	22J1962006	07/19/2023	01/19/2023 / Rajesh	12/19/2022 / Rajesh	E3459

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0174144	03/14/2023	09/14/2022 / yogesh	07/09/2021 / Abdul	P10858

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	02/09/2023	08/09/2022 / yogesh	10/29/2021 / Abdul	P11154

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	05/14/2023	11/14/2022 / yogesh	10/29/2021 / Abdul	P11164

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	05/14/2023	11/14/2022 / yogesh	10/29/2021 / Abdul	P11165

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	06/02/2023	12/02/2022 / yogesh	10/29/2021 / Abdul	P11166

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	06/02/2023	12/02/2022 / yogesh	10/29/2021 / Abdul	P11167

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	06/02/2023	12/02/2022 / yogesh	10/29/2021 / Abdul	P11168

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	06/02/2023	12/02/2022 / yogesh	10/29/2021 / Abdul	P11169

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110400-05-01 / TRPH Standard (C8-C40), 500 mg/L, 1 ml	472647	05/14/2023	11/14/2022 / yogesh	02/10/2022 / Yogesh	P11473

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110400-05-01 / TRPH Standard (C8-C40), 500 mg/L, 1 ml	472647	05/14/2023	11/14/2022 / yogesh	02/10/2022 / Yogesh	P11474

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0181886	01/27/2023	07/27/2022 / yogesh	05/27/2022 / Sohil	P11749

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0181886	05/14/2023	11/14/2022 / yogesh	05/27/2022 / Sohil	P11750

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0181886	05/14/2023	11/14/2022 / yogesh	05/27/2022 / Sohil	P11751



5580 Skylane Blvd
Santa Rosa, CA 95403
(707)525-5788
(800)878-7654 Toll Free
(707)545-7901 Fax

Manufacturer's Quality System
Audited & Registered
by TUV USA to ISO 9001:2015

Date Received: _____

Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.: Lot No.: Storage:

Z-110400 472647 $\leq -10^{\circ}\text{C}$
-05-01

Solvent:

Hexane

Exp. Date:

11/18/2023

Description:

TRPH Standard (C8-C40), 500 mg/L, 10 x 1 ml

-10PAK	Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
decane (C10)		124-18-5	99.5	415.7.1P	500.2 \pm 2.29
docosane (C22)		629-97-0	99	420.1.1P	502.4 \pm 5.5
dodecane (C12)		112-40-3	99.2	416.7.1P	500.7 \pm 2.29
dotriacontane (C32)		544-85-4	98	425.29.2P	499.8 \pm 5.47
eicosane (C20)		112-95-8	98.9	419.29.1P	505.1 \pm 2.31
hexacosane (C26)		630-01-3	99.3	422.7.2P	500 \pm 2.29
hexatriacontane (C36)		630-06-8	98	427.29.1P	500.3 \pm 5.48
n-hexadecane (C16)		544-76-3	99.45	368.271.1P	499.6 \pm 2.23
octacosane (C28)		630-02-4	98.7	423.400.1P	498.3 \pm 5.45
n-octadecane (C18)		593-45-3	99.5	418.29.1P	501.9 \pm 2.24
octane (C8)		111-65-9	99.5	385.9.1P	499.8 \pm 2.23
octatriacontane (C38)		7194-85-6	99	428.7.1P	499.8 \pm 2.29
tetracontane (C40)		4181-95-7	100	429.7.1P	504.1 \pm 5.52
n-tetradecane (C14)		629-59-4	99	417.29.4P	500.4 \pm 5.48
tetratriacontane (C34)		14167-59-0	98.1	426.7.2P	499.6 \pm 2.28
triacontane (C30)		638-68-6	99.5	424.7.1.1P	499.9 \pm 2.29
tetracosane (C24)		646-31-1	99	421.1.1P	500.1 \pm 5.47

P11469
J
P11488
Y.P.
02/12/22

Let the standard warm to room temperature and sonicate before opening.

*Not a certified value

Certified By: _____

Jarrett Howard
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.
Concentration (correct for purity) and uncertainty (95% confidence) values
listed are determined gravimetrically.



5580 Skylane Blvd
Santa Rosa, CA 95403
(707)525-5788
(800)878-7654 Toll Free
(707)545-7901 Fax

Manufacturer's Quality System
Audited & Registered
by TUV USA to ISO 9001:2015

Date Received: _____

Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.: Lot No.: Storage:

Z-110400 472647 $\leq -10^{\circ}\text{C}$
-05-01

Solvent:

Hexane

Exp. Date:

11/18/2023

Description:

TRPH Standard (C8-C40), 500 mg/L, 10 x 1 ml

-10PAK	Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
decane (C10)		124-18-5	99.5	415.7.1P	500.2 \pm 2.29
docosane (C22)		629-97-0	99	420.1.1P	502.4 \pm 5.5
dodecane (C12)		112-40-3	99.2	416.7.1P	500.7 \pm 2.29
dotriacontane (C32)		544-85-4	98	425.29.2P	499.8 \pm 5.47
eicosane (C20)		112-95-8	98.9	419.29.1P	505.1 \pm 2.31
hexacosane (C26)		630-01-3	99.3	422.7.2P	500 \pm 2.29
hexatriacontane (C36)		630-06-8	98	427.29.1P	500.3 \pm 5.48
n-hexadecane (C16)		544-76-3	99.45	368.271.1P	499.6 \pm 2.23
octacosane (C28)		630-02-4	98.7	423.400.1P	498.3 \pm 5.45
n-octadecane (C18)		593-45-3	99.5	418.29.1P	501.9 \pm 2.24
octane (C8)		111-65-9	99.5	385.9.1P	499.8 \pm 2.23
octatriacontane (C38)		7194-85-6	99	428.7.1P	499.8 \pm 2.29
tetracontane (C40)		4181-95-7	100	429.7.1P	504.1 \pm 5.52
n-tetradecane (C14)		629-59-4	99	417.29.4P	500.4 \pm 5.48
tetratriacontane (C34)		14167-59-0	98.1	426.7.2P	499.6 \pm 2.28
triacontane (C30)		638-68-6	99.5	424.7.1.1P	499.9 \pm 2.29
tetracosane (C24)		646-31-1	99	421.1.1P	500.1 \pm 5.47

P11469
J
P11488
Y.P.
02/12/22

Let the standard warm to room temperature and sonicate before opening.

*Not a certified value

Certified By: _____

Jarrett Howard
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.
Concentration (correct for purity) and uncertainty (95% confidence) values
listed are determined gravimetrically.

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1

Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 22G0762001
Manufactured Date: 2022-05-23
Expiration Date: 2023-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	6
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	≤ 10	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.1 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP 08 8/15/22

E 3386


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1




**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**



MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MÉXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT : SODIUM SULFATE CRYSTALS ANHYDROUS
QUALITY : ACS (CODE RMB3375) **FORMULA :** Na₂SO₄
SPECIFICATION NUMBER : 6399 **RELEASE DATE:** OCT/28/2021
LOT NUMBER : 139404

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.8 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.0
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.002 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.2 %
Retained on US Standard No. 60 sieve	Min. 94%	97.6 %
Through US Standard No. 60 sieve	Max. 5%	2.1 %
Through US Standard No. 100 sieve	Max. 10%	0.2 %
COMMENTS		
 QC: PhC Irma Belmares		

If you need further details, please call our factory or contact our local distributor.

E 3412

Recd. by RP on 10/13/22

RE-02-01, Ed. 3

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 22H1562002
Manufactured Date: 2022-07-28
Expiration Date: 2023-10-27
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	≤ 10	10
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.3 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 10/17/22

E 3419


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 2212962012
Manufactured Date: 2022-09-10
Expiration Date: 2023-12-10
Revision No.: 0


Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	2
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	≤ 10	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	< 0.1 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3427


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 2212962012
Manufactured Date: 2022-09-10
Expiration Date: 2023-12-10
Revision No.: 0


Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	2
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	≤ 10	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	< 0.1 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3432


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700
Page 1 of 1

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 22K0762004
Manufactured Date: 2022-10-10
Expiration Date: 2024-01-09
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	4
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	≤ 10	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.5 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3452


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Acetone
CMOS



Material No.: 9005-05
Batch No.: 22J0461011
Manufactured Date: 2022-09-29
Retest Date: 2027-09-28
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.2
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.2 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	4.9 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd. by R2 on 01/11/23

>>> Continued on page 2 >>>

E 3456

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Acetone
CMOS



Material No.: 9005-05
Batch No.: 22J0461011

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	1.8 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	4 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Acetone
CMOS




Material No.: 9005-05
Batch No.: 22J0461011

Test	Specification	Result
------	---------------	--------

For Microelectronic Use

Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC

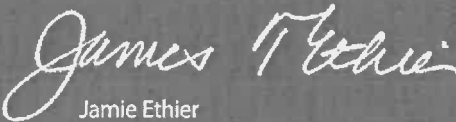
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 22J1962006
Manufactured Date: 2022-09-23
Expiration Date: 2023-12-23
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	6
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8\%$	100.0 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	≤ 10 ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02\%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3459


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Page 1 of 1



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266 **Lot No.:** A0174144

Description : Florida TRPH Standard
Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : August 31, 2028 **Storage:** 25°C nominal

Handling: Sonicate prior to use. **Ship:** Ambient

P 10853
↓
P 10862
07/12/2021

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	n-Octane (C8) CAS # 111-65-9 (Lot SHBM4827) Purity 99%	504.5 µg/mL	+/- 2.9966 µg/mL +/- 12.5340 µg/mL +/- 15.0241 µg/mL	Gravimetric Unstressed Stressed
2	n-Decane (C10) CAS # 124-18-5 (Lot SHBL4313) Purity 99%	500.5 µg/mL	+/- 2.9728 µg/mL +/- 12.4347 µg/mL +/- 14.9050 µg/mL	Gravimetric Unstressed Stressed
3	n-Dodecane (C12) CAS # 112-40-3 (Lot SHBK0925) Purity 99%	501.5 µg/mL	+/- 2.9788 µg/mL +/- 12.4595 µg/mL +/- 14.9348 µg/mL	Gravimetric Unstressed Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 (Lot STBJ7343) Purity 99%	502.5 µg/mL	+/- 2.9847 µg/mL +/- 12.4844 µg/mL +/- 14.9646 µg/mL	Gravimetric Unstressed Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 (Lot SHBM4146) Purity 98%	501.3 µg/mL	+/- 2.9774 µg/mL +/- 12.4538 µg/mL +/- 14.9280 µg/mL	Gravimetric Unstressed Stressed
6	n-Octadecane (C18) CAS # 593-45-3 (Lot VZKOJ) Purity 97%	500.5 µg/mL	+/- 2.9729 µg/mL +/- 12.4352 µg/mL +/- 14.9056 µg/mL	Gravimetric Unstressed Stressed
7	n-Eicosane (C20) CAS # 112-95-8 (Lot MKCF7888) Purity 99%	501.5 µg/mL	+/- 2.9788 µg/mL +/- 12.4595 µg/mL +/- 14.9348 µg/mL	Gravimetric Unstressed Stressed

8	n-Docosane (C22)		504.0	µg/mL	+/-	2.9936	µg/mL	Gravimetric
	CAS # 629-97-0	(Lot MKCL8918)			+/-	12.5216	µg/mL	Unstressed
	Purity 99%				+/-	15.0093	µg/mL	Stressed
9	n-Tetracosane (C24)		500.5	µg/mL	+/-	2.9728	µg/mL	Gravimetric
	CAS # 646-31-1	(Lot MKBZ5406V)			+/-	12.4347	µg/mL	Unstressed
	Purity 99%				+/-	14.9050	µg/mL	Stressed
10	n-Hexacosane (C26)		502.0	µg/mL	+/-	2.9817	µg/mL	Gravimetric
	CAS # 630-01-3	(Lot MKCD4540)			+/-	12.4719	µg/mL	Unstressed
	Purity 99%				+/-	14.9497	µg/mL	Stressed
11	n-Octacosane (C28)		501.5	µg/mL	+/-	2.9788	µg/mL	Gravimetric
	CAS # 630-02-4	(Lot BCCB6836)			+/-	12.4595	µg/mL	Unstressed
	Purity 99%				+/-	14.9348	µg/mL	Stressed
12	n-Triacontane (C30)		504.2	µg/mL	+/-	2.9949	µg/mL	Gravimetric
	CAS # 638-68-6	(Lot MKCJ4572)			+/-	12.5268	µg/mL	Unstressed
	Purity 98%				+/-	15.0155	µg/mL	Stressed
13	n-Dotriacontane (C32)		501.0	µg/mL	+/-	2.9758	µg/mL	Gravimetric
	CAS # 544-85-4	(Lot BCBW0661)			+/-	12.4471	µg/mL	Unstressed
	Purity 99%				+/-	14.9199	µg/mL	Stressed
14	n-Tetratriacontane (C34)		504.5	µg/mL	+/-	2.9966	µg/mL	Gravimetric
	CAS # 14167-59-0	(Lot OML4N)			+/-	12.5340	µg/mL	Unstressed
	Purity 99%				+/-	15.0241	µg/mL	Stressed
15	n-Hexatriacontane (C36)		502.0	µg/mL	+/-	2.9817	µg/mL	Gravimetric
	CAS # 630-06-8	(Lot MKCK2834)			+/-	12.4719	µg/mL	Unstressed
	Purity 99%				+/-	14.9497	µg/mL	Stressed
16	n-Octatriacontane (C38)		501.5	µg/mL	+/-	2.9788	µg/mL	Gravimetric
	CAS # 7194-85-6	(Lot 0000050904)			+/-	12.4595	µg/mL	Unstressed
	Purity 99%				+/-	14.9348	µg/mL	Stressed
17	n-Tetracontane (C40)		504.6	µg/mL	+/-	2.9969	µg/mL	Gravimetric
	CAS # 4181-95-7	(Lot 4LJYN)			+/-	12.5354	µg/mL	Unstressed
	Purity 98%				+/-	15.0257	µg/mL	Stressed
Solvent: Hexane								
	CAS # 110-54-3							
	Purity 99%							

P 10853
↓

P 10862

AR
07/12/2021

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:


330°C

Det. Type:

FID

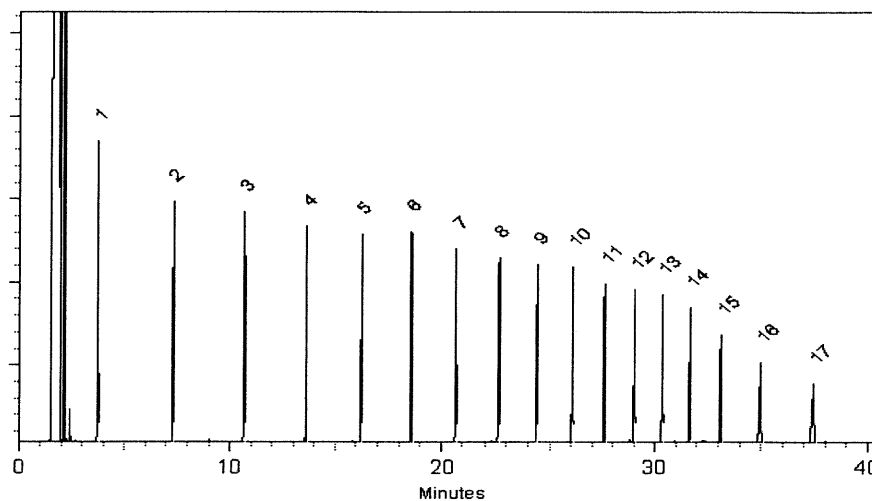

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dalton Stover - Operations Technician I

Date Mixed: 06-Jul-2021

Balance: 1128353505


Alexis Shelow - Operations Tech I

Date Passed: 08-Jul-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

Solvent(s):
Methylene chloride

Lot#
104929

72072
091120
n-Tetracosane-d50

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

091130
Ambient (20 °C)
1000
23060

Weight(s) shown below were combined and diluted to (mL):

200.0


5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Formulated By:	Benson Chan	091120	DATE
Reviewed By:	Pedro L. Rentas	091120	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LDSO
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	----------------------------------	--	----------------	------

1. n-Tetracosane-d50 2072 PR-26606 1000 98.7 0.2 99.0 0.20471 0.20481 1000.5 4.1 16416-32-3 N/A

Method GCMSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

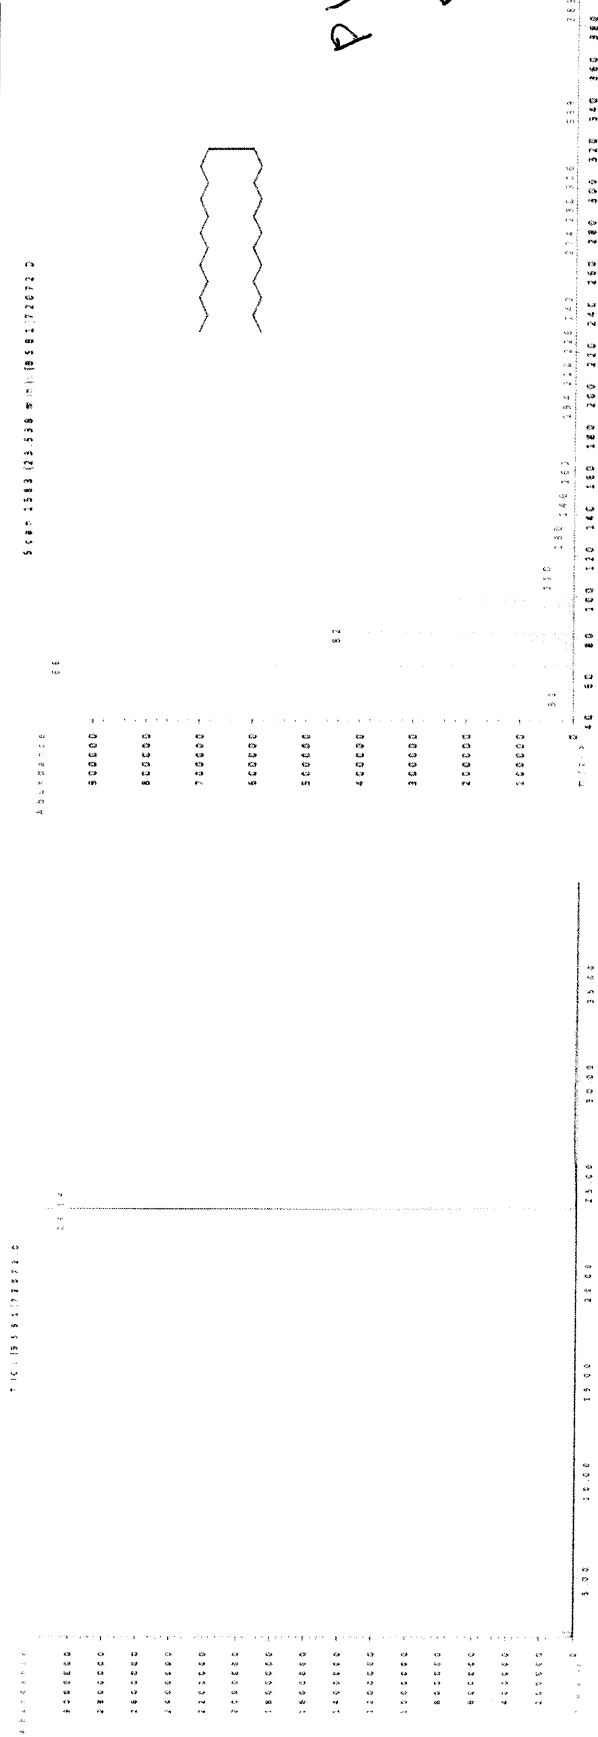

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"

Run Length: 35.00 min, 20999 points at 10 points/second.
Created: Thu, Sep 17, 2020 at 9:46:03 AM.
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".
Analyzed using Method "GC4-M1".

Comments

GC4-M1 Analysis by Candice Warren
Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness
Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,
Air (detector) = 360 mL
Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.
Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

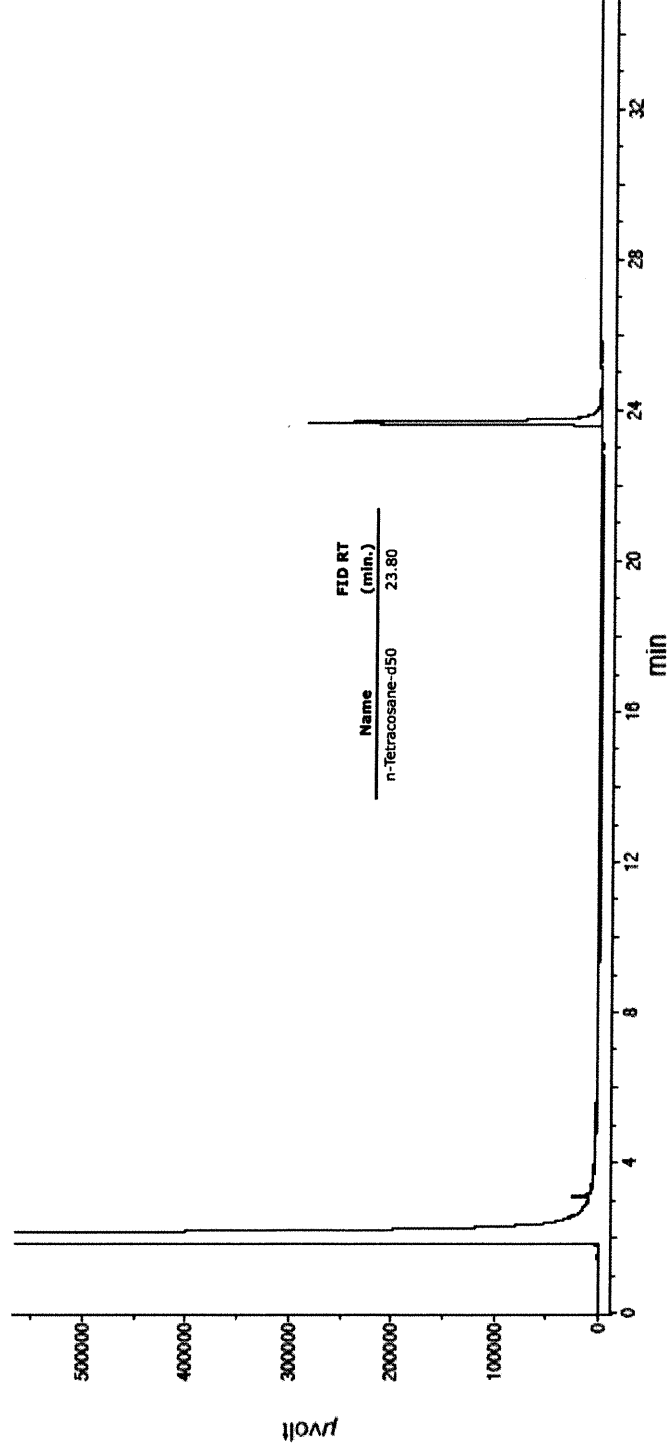

P11176
 11/02/21
 12

CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

Solvent(s):
Methylene chloride

Formulated By:	DATE
Benson Chan	091120
Reviewed By:	DATE
Pedro L. Rentas	091120


Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

Weight(s) shown below were combined and diluted to (mL):

5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)
1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20481	1000.5	4.1	16416-32-3 N/A

Method GCMSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

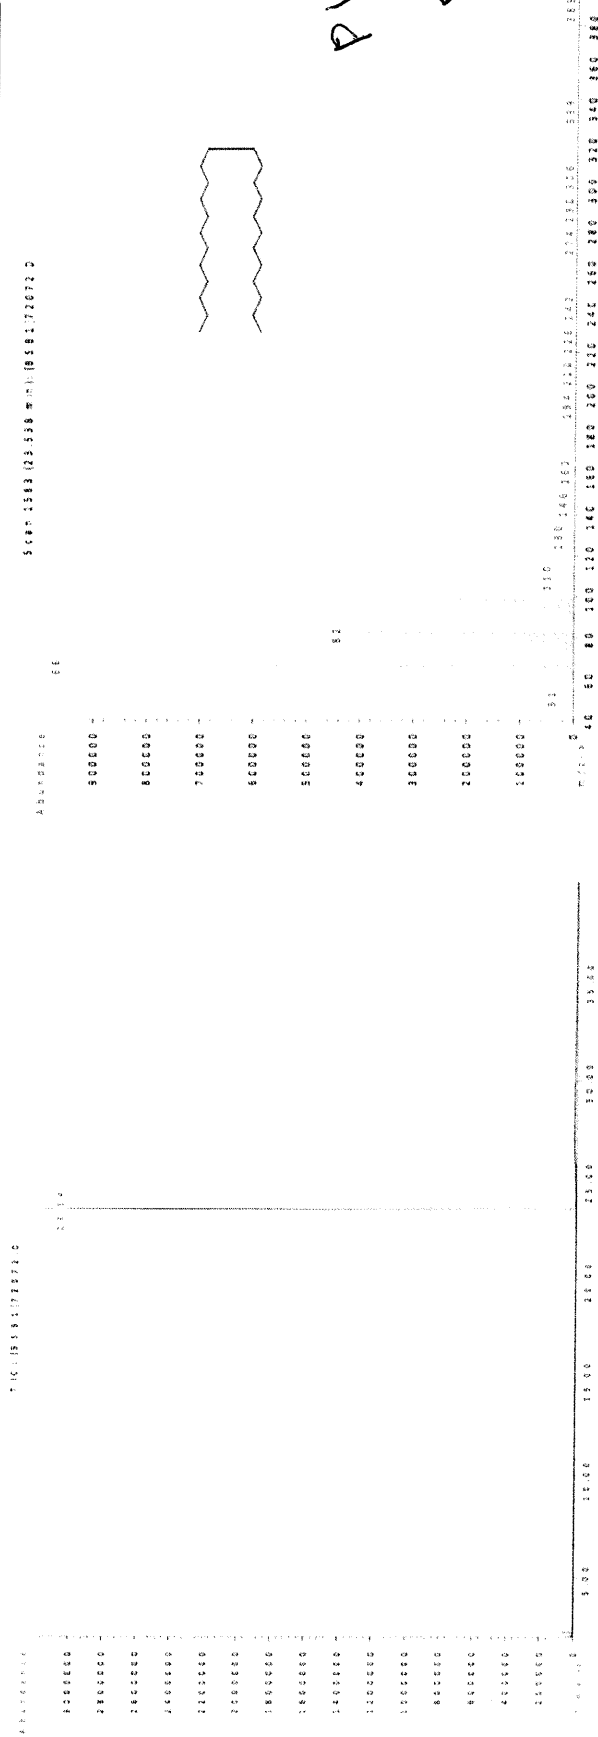

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"

Run Length: 35.00 min, 20999 points at 10 points/second.
Created: Thu, Sep 17, 2020 at 9:46:03 AM.
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".
Analyzed using Method "GC4-M1".

Comments

GC4-M1 Analysis by Candice Warren
Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness
Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,
Air (detector) = 360 mL
Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.
Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

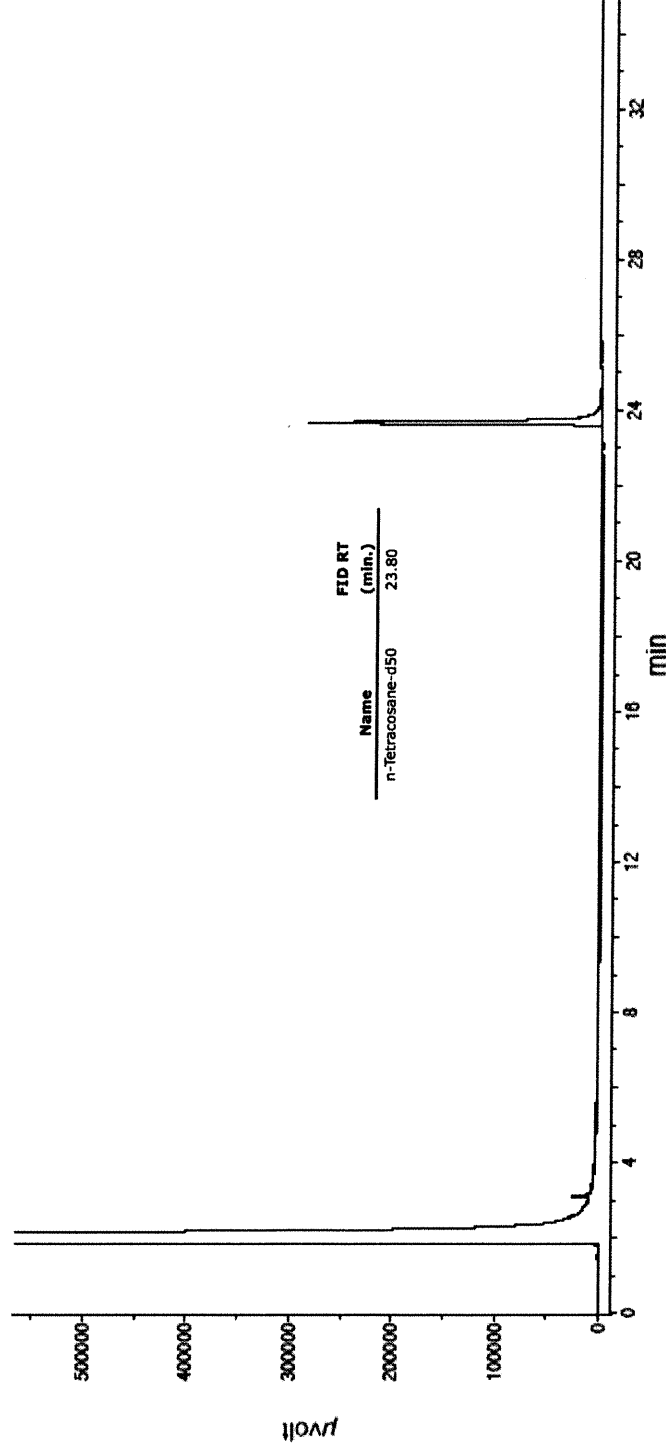

P11176
 11/02/21
 12

CERTIFIED WEIGHT REPORT

Part Number:
 Lot Number:
 Description:

72072
091120
n-Tetracosane-d50

Solvent(s):
Lot#
104929

Formulated By:	Benson Chan	091120	DATE
Reviewed By:	Pedro L. Rentas	091120	DATE

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:


091130
Ambient (20 °C)
1000
23060

Weight(s) shown below were combined and diluted to (mL):
200.0
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LDSO
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	----------------------------------	--	----------------	------

1. n-Tetracosane-d50 2072 PR-26606 1000 98.7 0.2 99.0 0.20471 0.20481 1000.5 4.1 16416-32-3 N/A

Method GCMSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

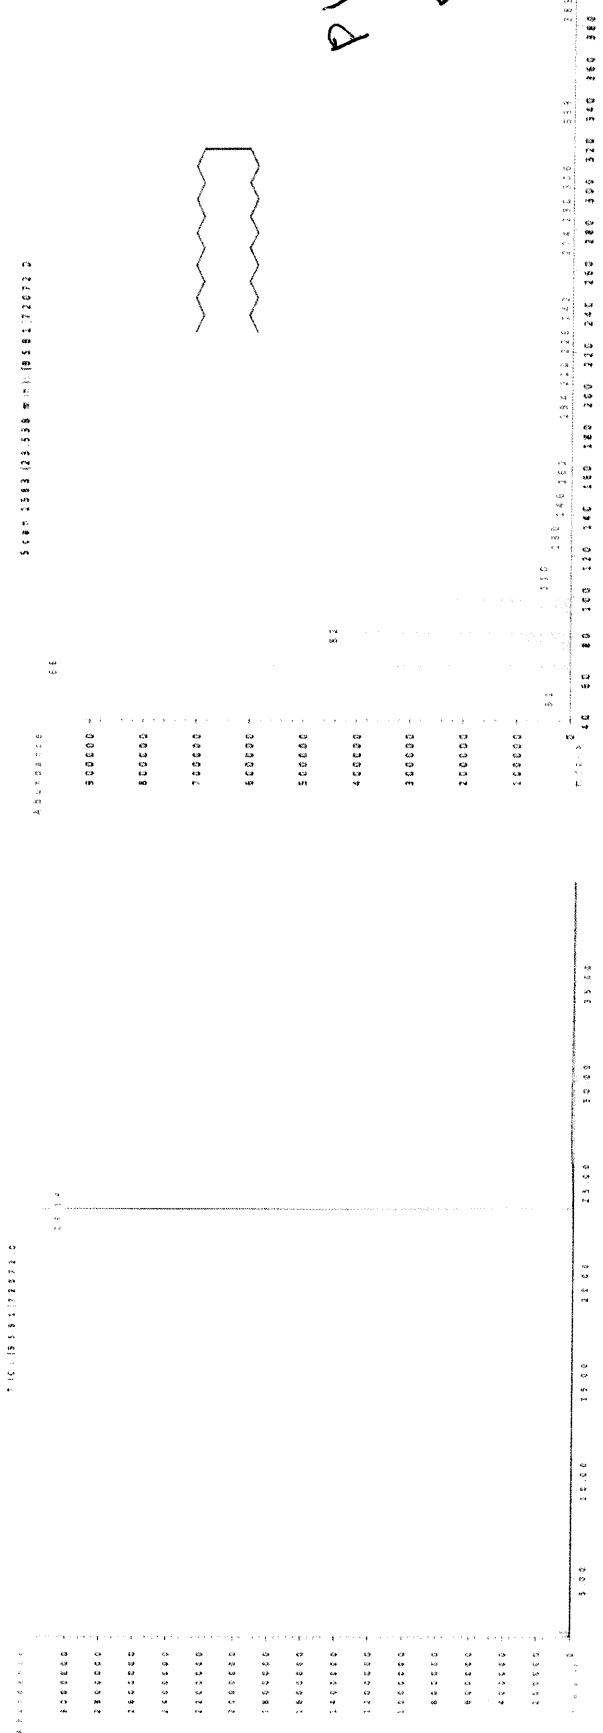

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
 Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
 Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
 All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
 Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"

Run Length: 35.00 min, 20999 points at 10 points/second.
Created: Thu, Sep 17, 2020 at 9:46:03 AM.
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".
Analyzed using Method "GC4-M1".

Comments

GC4-M1 Analysis by Candice Warren
Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness
Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,
Air (detector) = 360 mL
Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.
Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

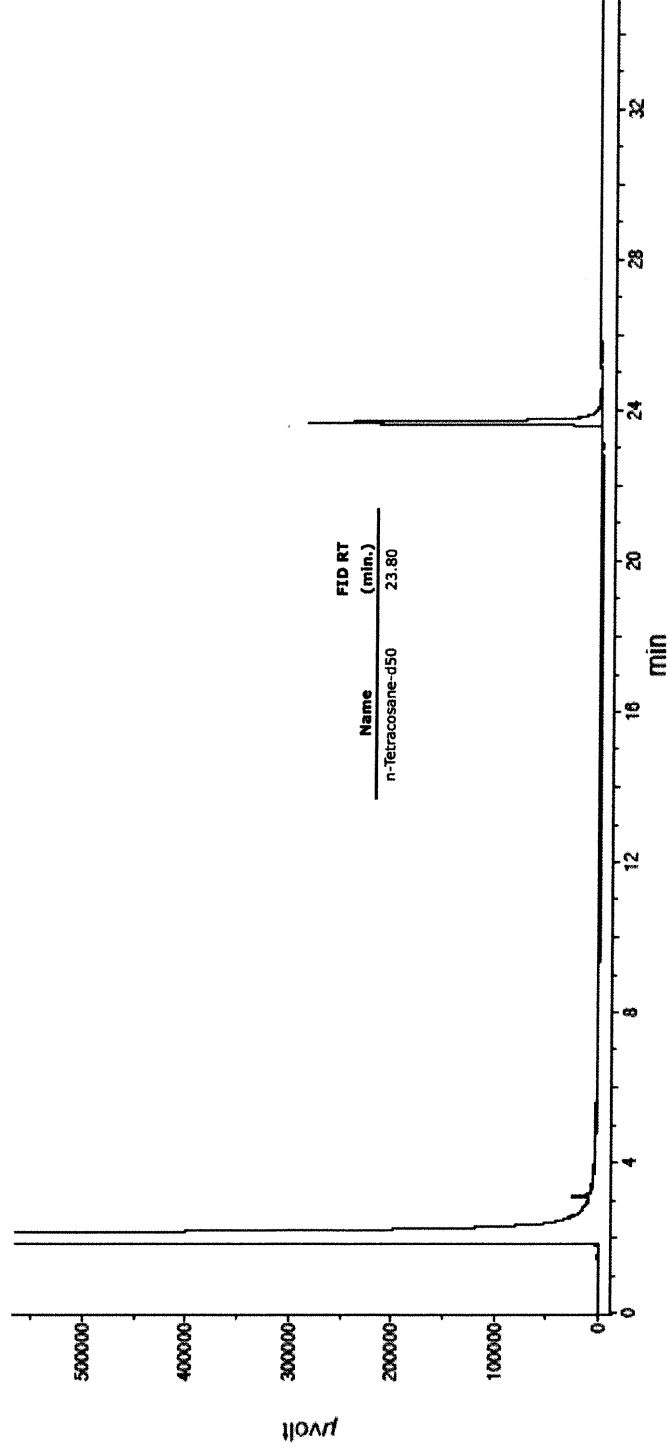

P1117b
 11/02/21
 12

CERTIFIED WEIGHT REPORT

Part Number:
 Lot Number:
 Description:

72072
091120
n-Tetracosane-d50

Solvent(s):
Lot#
104929

Formulated By:	Benson Chan	091120	DATE
Reviewed By:	Pedro L. Rentas	091120	DATE

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:


091130
Ambient (20 °C)
1000
23060

Weight(s) shown below were combined and diluted to (mL):
200.0
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LDSO
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	----------------------------------	--	----------------	------

1. n-Tetracosane-d50 2072 PR-26606 1000 98.7 0.2 99.0 0.20471 0.20481 1000.5 4.1 16416-32-3 N/A

Method GCMSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

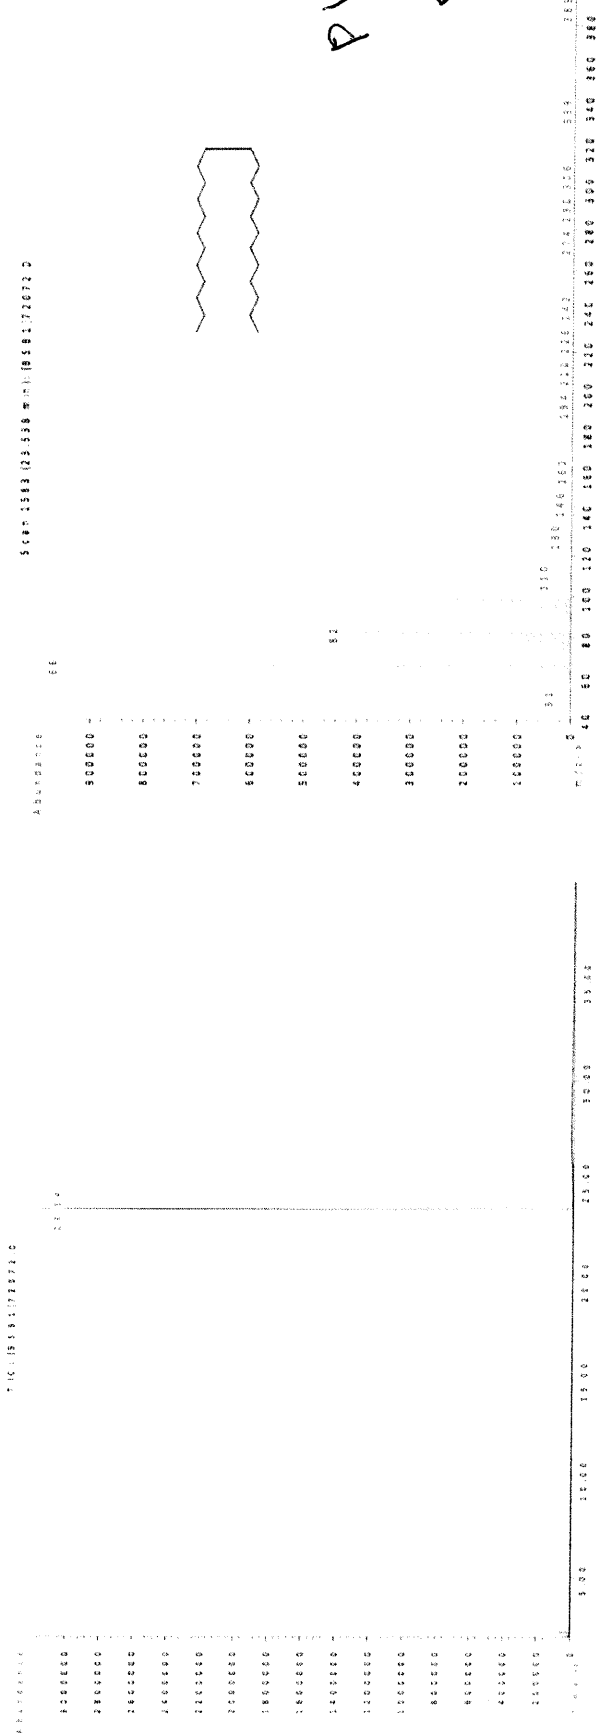

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
 Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
 Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
 All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
 Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"

Run Length: 35.00 min, 20999 points at 10 points/second.
Created: Thu, Sep 17, 2020 at 9:46:03 AM.
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".
Analyzed using Method "GC4-M1".

Comments

GC4-M1 Analysis by Candice Warren
Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness
Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,
Air (detector) = 360 mL
Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.
Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

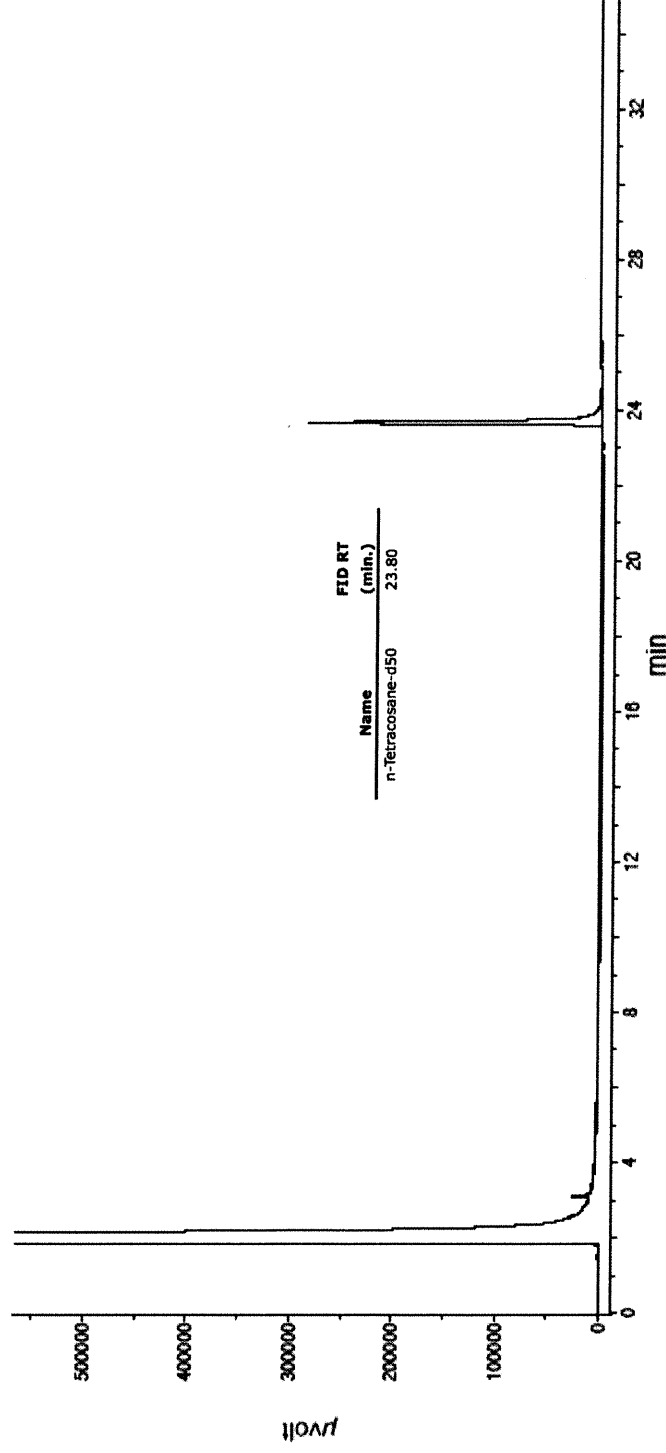

P1117b
 11/02/21
 12

CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

Solvent(s):
Methylene chloride

Lot#
104929

72072
091120
n-Tetracosane-d50

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

091130
Ambient (20 °C)
1000
23060

Weight(s) shown below were combined and diluted to (mL):

200.0


5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Formulated By:	Benson Chan	DATE	091120
Reviewed By:	Pedro L. Rentas	DATE	091120

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LDSO
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	----------------------------------	--	----------------	------

1. n-Tetracosane-d50 2072 PR-26606 1000 98.7 0.2 99.0 0.20471 0.20481 1000.5 4.1 16416-32-3 N/A N/A

Method GCMSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

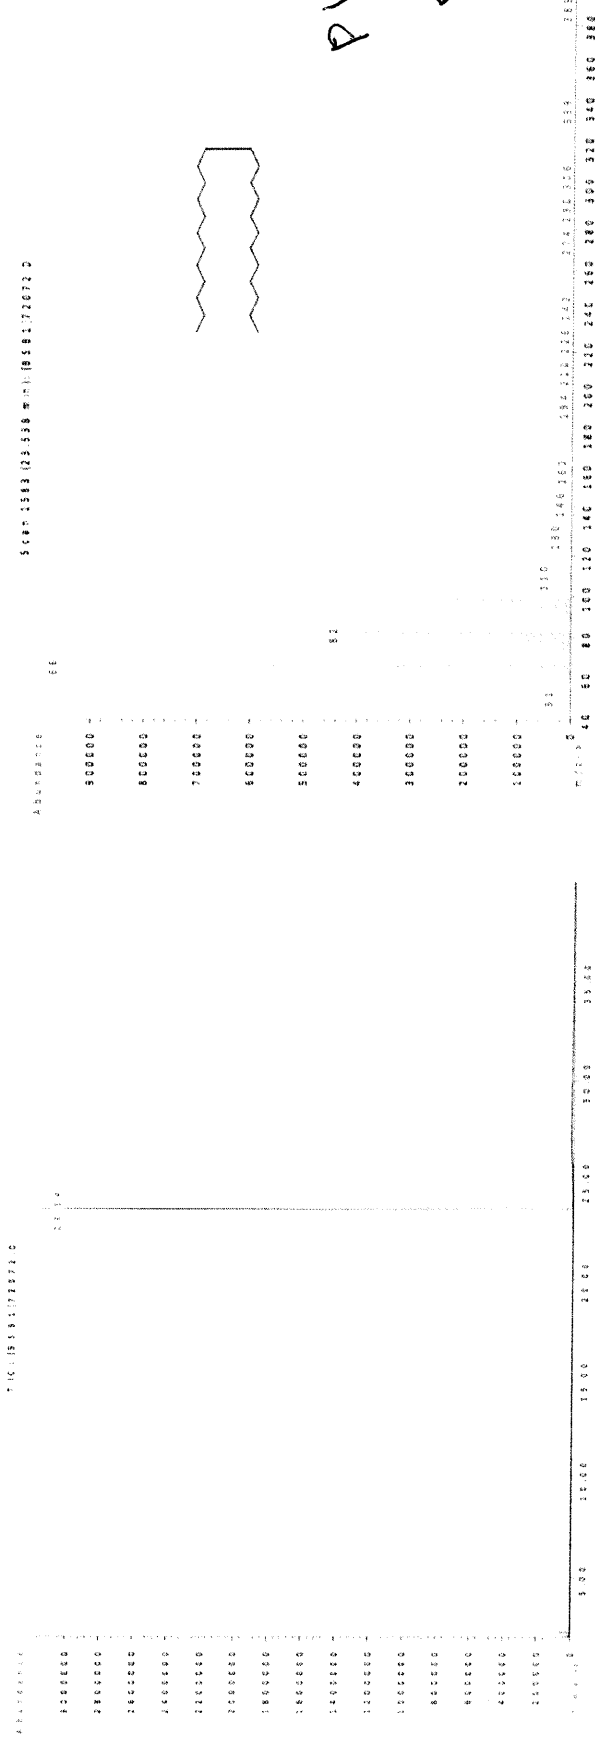

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"

Run Length: 35.00 min, 20999 points at 10 points/second.
Created: Thu, Sep 17, 2020 at 9:46:03 AM.
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".
Analyzed using Method "GC4-M1".

Comments

GC4-M1 Analysis by Candice Warren
Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness
Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,
Air (detector) = 360 mL
Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.
Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

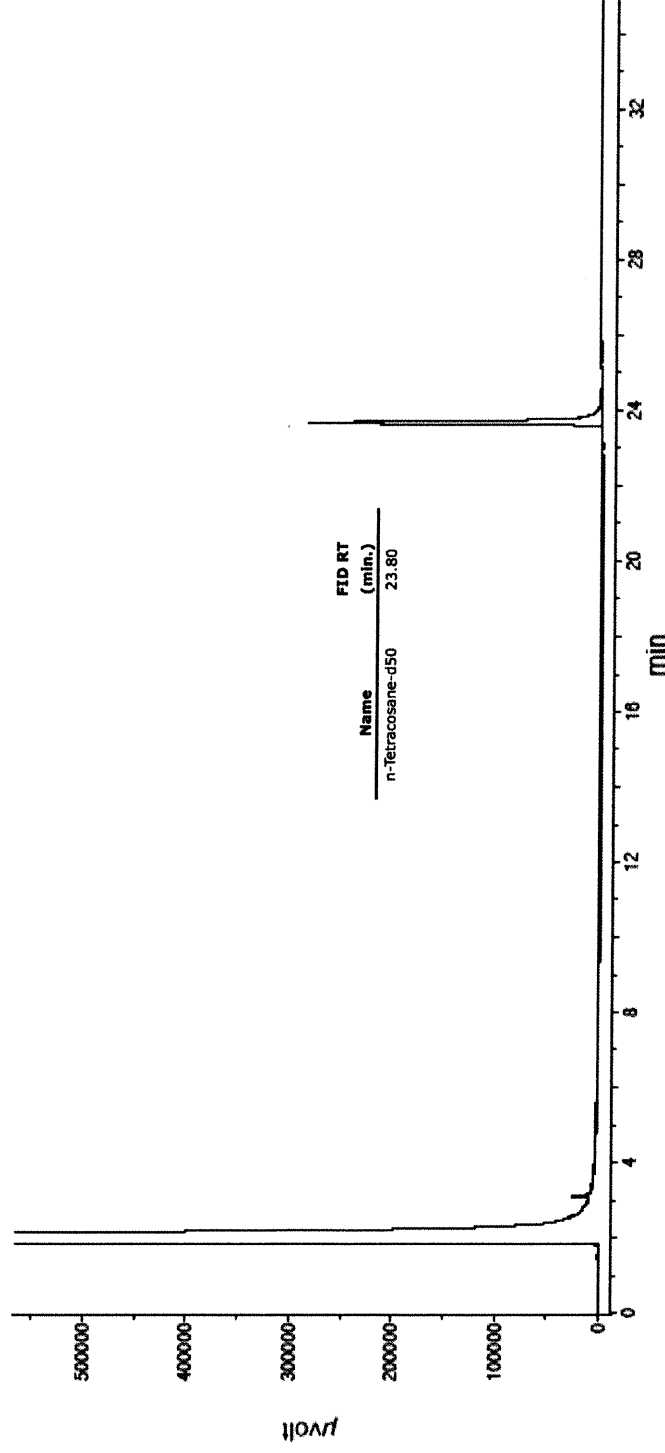

P11147
 P11176
 11/02/21

CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

Solvent(s):
Methylene chloride

72072	Lot#
091120	104929
n-Tetracosane-d50	

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:


091130
Ambient (20 °C)
1000
23060

Weight(s) shown below were combined and diluted to (mL):
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LDSO
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	----------------------------------	--	----------------	------

1. n-Tetracosane-d50 2072 PR-26606 1000 98.7 0.2 99.0 0.20471 0.20481 1000.5 4.1 16416-32-3 N/A

Method GCMSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

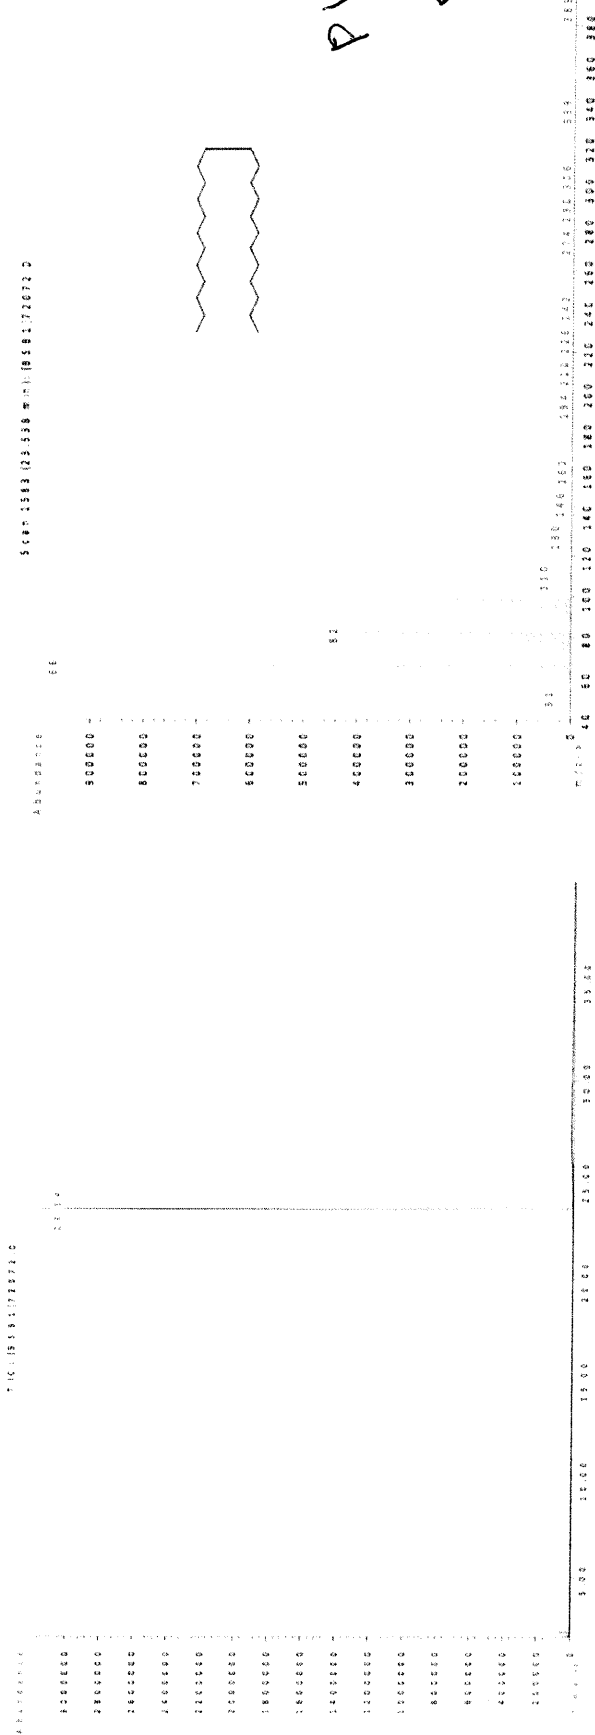

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"

Run Length: 35.00 min, 20999 points at 10 points/second.
Created: Thu, Sep 17, 2020 at 9:46:03 AM.
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".
Analyzed using Method "GC4-M1".

Comments

GC4-M1 Analysis by Candice Warren
Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness
Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,
Air (detector) = 360 mL
Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.
Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

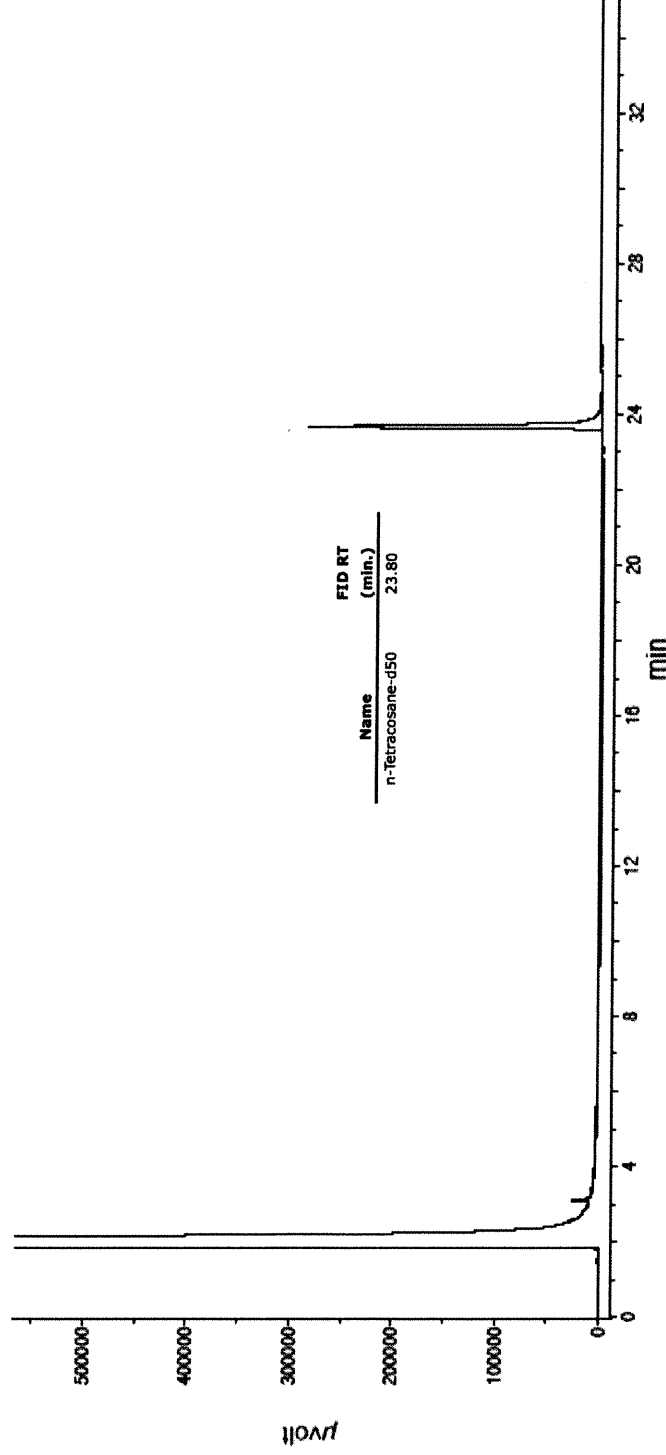

P11147
 P11176
 11/02/21

CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

Solvent(s):
Methylene chloride

Lot#
104929

72072
091120
n-Tetracosane-d50

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

091130
Ambient (20 °C)
1000
23060

Weight(s) shown below were combined and diluted to (mL):

200.0


5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Formulated By:	Benson Chan	091120	DATE
Reviewed By:	Pedro L. Rentas	091120	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LDSO
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	----------------------------------	--	----------------	------

1. n-Tetracosane-d50 2072 PR-26606 1000 98.7 0.2 99.0 0.20471 0.20481 1000.5 4.1 16416-32-3 N/A N/A

Method GCMSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

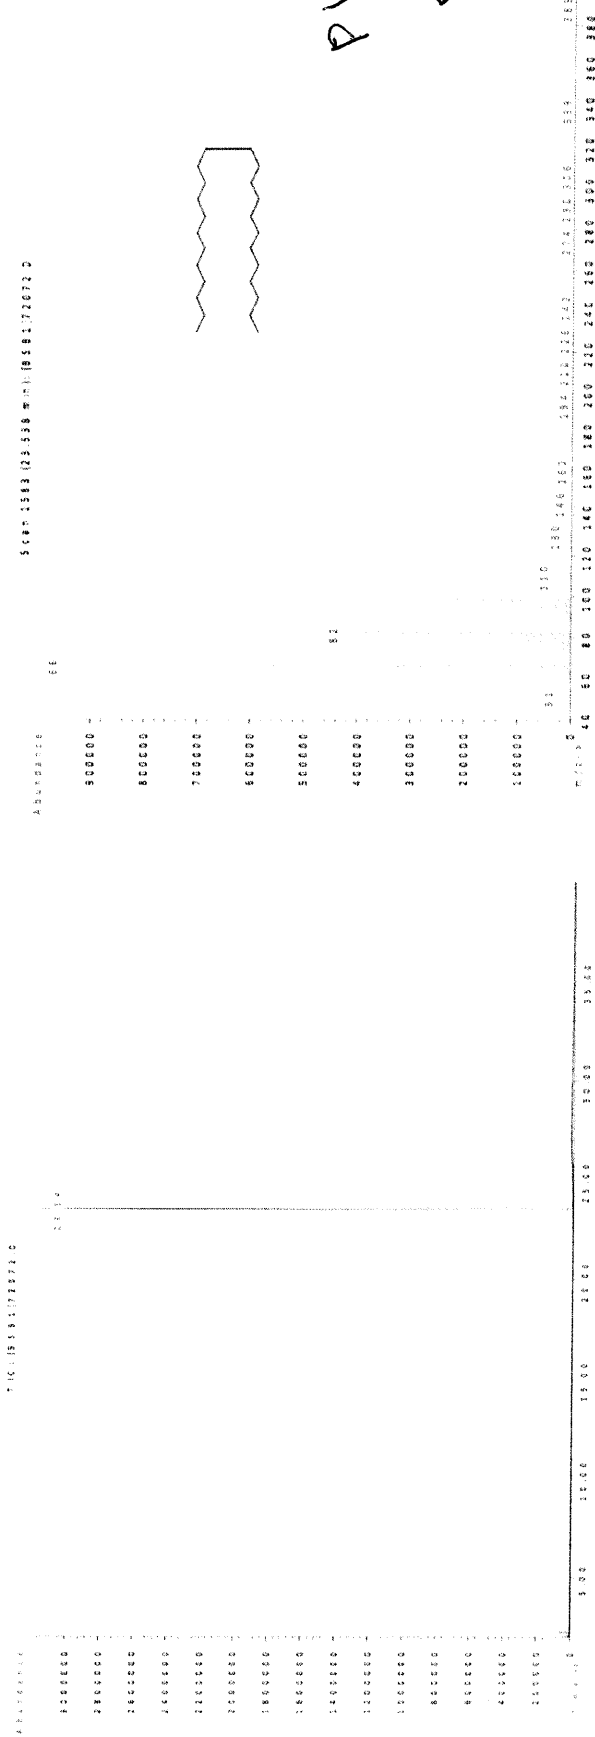

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"

Run Length: 35.00 min, 20999 points at 10 points/second.

Created: Thu, Sep 17, 2020 at 9:46:03 AM.

Sampled: Sequence "091420-GC4M2", Method "GC4-M1".

Analyzed using Method "GC4-M1".

Comments

GC4-M1 Analysis by Candice Warren

Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness


Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,

Air (detector) = 360 mL

Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.

Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.

Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

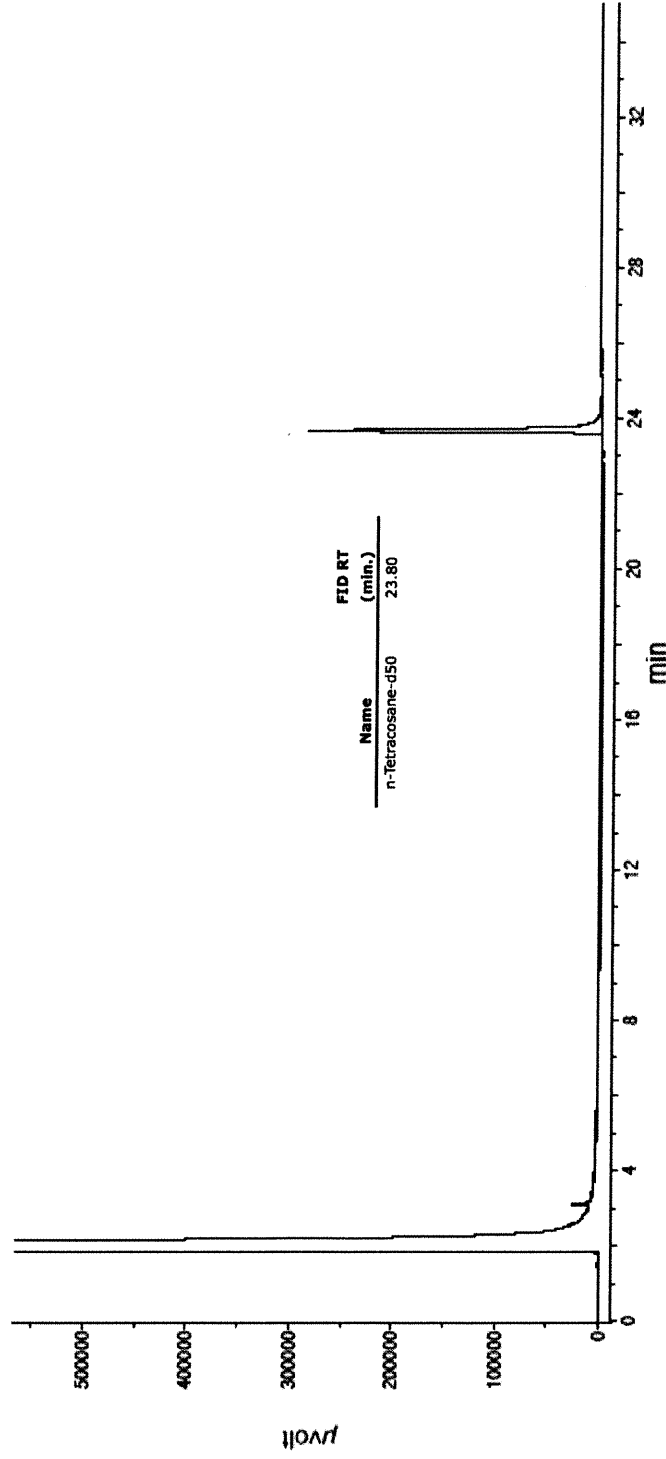

P1114P
 K1117b
 11/02/21



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis

P11749 to P11758

Received by SJ 5/27/2022



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266 **Lot No.:** A0181886
Description : Florida TRPH Standard
Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : March 31, 2029 **Storage:** 25°C nominal
Handling: Sonicate prior to use. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	n-Octane (C8) CAS # 111-65-9 (Lot SHBM4827) Purity 99%	501.6 µg/mL	+/- 2.9794 µg/mL Gravimetric +/- 12.4620 µg/mL Unstressed +/- 14.9378 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 (Lot SHBM1113) Purity 99%	501.8 µg/mL	+/- 2.9802 µg/mL Gravimetric +/- 12.4657 µg/mL Unstressed +/- 14.9423 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 (Lot SHBK0925) Purity 99%	500.9 µg/mL	+/- 2.9752 µg/mL Gravimetric +/- 12.4446 µg/mL Unstressed +/- 14.9169 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 (Lot STBK2282) Purity 99%	500.7 µg/mL	+/- 2.9740 µg/mL Gravimetric +/- 12.4396 µg/mL Unstressed +/- 14.9110 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 (Lot SHBM4146) Purity 98%	500.5 µg/mL	+/- 2.9727 µg/mL Gravimetric +/- 12.4343 µg/mL Unstressed +/- 14.9046 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 (Lot UE5NG) Purity 98%	500.5 µg/mL	+/- 2.9730 µg/mL Gravimetric +/- 12.4355 µg/mL Unstressed +/- 14.9061 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 (Lot MKCF7888) Purity 99%	500.6 µg/mL	+/- 2.9731 µg/mL Gravimetric +/- 12.4359 µg/mL Unstressed +/- 14.9065 µg/mL Stressed

8	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	501.5 µg/mL	+/- 2.9785 +/- 12.4583 +/- 14.9333	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCJ8741)	500.6 µg/mL	+/- 2.9731 +/- 12.4359 +/- 14.9065	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	500.5 µg/mL	+/- 2.9728 +/- 12.4347 +/- 14.9050	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	500.6 µg/mL	+/- 2.9734 +/- 12.4371 +/- 14.9080	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) CAS # 638-68-6 Purity 99%	(Lot MKCN9321)	501.7 µg/mL	+/- 2.9799 +/- 12.4645 +/- 14.9408	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	501.8 µg/mL	+/- 2.9805 +/- 12.4670 +/- 14.9437	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	501.3 µg/mL	+/- 2.9773 +/- 12.4533 +/- 14.9274	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot U25B014)	502.4 µg/mL	+/- 2.9841 +/- 12.4819 +/- 14.9616	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 97%	(Lot 0000127235)	501.7 µg/mL	+/- 2.9801 +/- 12.4653 +/- 14.9417	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) CAS # 4181-95-7 Purity 98%	(Lot PADGI)	500.2 µg/mL	+/- 2.9713 +/- 12.4282 +/- 14.8973	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
Solvent: Hexane CAS # 110-54-3 Purity 99%						

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)


Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

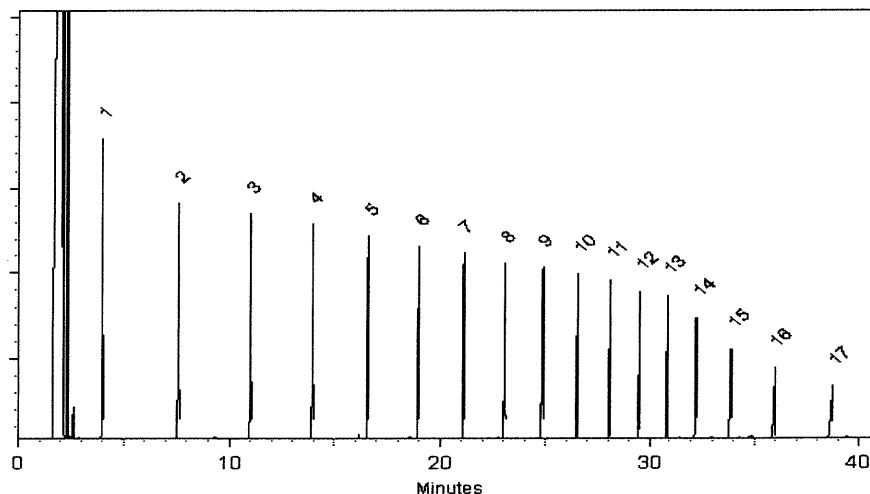

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Penelope S. Riglin
Penelope Riglin - Operations Tech I

Date Mixed: 16-Feb-2022 **Balance:** 1128360905

Clara Windle
Clara Windle - Operations Technician I

Date Passed: 21-Feb-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis

P11749 to P11758

Received by SJ 5/27/2022



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266 **Lot No.:** A0181886
Description : Florida TRPH Standard
Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : March 31, 2029 **Storage:** 25°C nominal
Handling: Sonicate prior to use. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	n-Octane (C8) CAS # 111-65-9 (Lot SHBM4827) Purity 99%	501.6 µg/mL	+/- 2.9794 µg/mL Gravimetric +/- 12.4620 µg/mL Unstressed +/- 14.9378 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 (Lot SHBM1113) Purity 99%	501.8 µg/mL	+/- 2.9802 µg/mL Gravimetric +/- 12.4657 µg/mL Unstressed +/- 14.9423 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 (Lot SHBK0925) Purity 99%	500.9 µg/mL	+/- 2.9752 µg/mL Gravimetric +/- 12.4446 µg/mL Unstressed +/- 14.9169 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 (Lot STBK2282) Purity 99%	500.7 µg/mL	+/- 2.9740 µg/mL Gravimetric +/- 12.4396 µg/mL Unstressed +/- 14.9110 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 (Lot SHBM4146) Purity 98%	500.5 µg/mL	+/- 2.9727 µg/mL Gravimetric +/- 12.4343 µg/mL Unstressed +/- 14.9046 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 (Lot UE5NG) Purity 98%	500.5 µg/mL	+/- 2.9730 µg/mL Gravimetric +/- 12.4355 µg/mL Unstressed +/- 14.9061 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 (Lot MKCF7888) Purity 99%	500.6 µg/mL	+/- 2.9731 µg/mL Gravimetric +/- 12.4359 µg/mL Unstressed +/- 14.9065 µg/mL Stressed

8	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	501.5 µg/mL	+/- 2.9785 +/- 12.4583 +/- 14.9333	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCJ8741)	500.6 µg/mL	+/- 2.9731 +/- 12.4359 +/- 14.9065	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	500.5 µg/mL	+/- 2.9728 +/- 12.4347 +/- 14.9050	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	500.6 µg/mL	+/- 2.9734 +/- 12.4371 +/- 14.9080	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) CAS # 638-68-6 Purity 99%	(Lot MKCN9321)	501.7 µg/mL	+/- 2.9799 +/- 12.4645 +/- 14.9408	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	501.8 µg/mL	+/- 2.9805 +/- 12.4670 +/- 14.9437	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	501.3 µg/mL	+/- 2.9773 +/- 12.4533 +/- 14.9274	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot U25B014)	502.4 µg/mL	+/- 2.9841 +/- 12.4819 +/- 14.9616	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 97%	(Lot 0000127235)	501.7 µg/mL	+/- 2.9801 +/- 12.4653 +/- 14.9417	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) CAS # 4181-95-7 Purity 98%	(Lot PADGI)	500.2 µg/mL	+/- 2.9713 +/- 12.4282 +/- 14.8973	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
Solvent:	Hexane CAS # 110-54-3 Purity 99%					

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)


Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

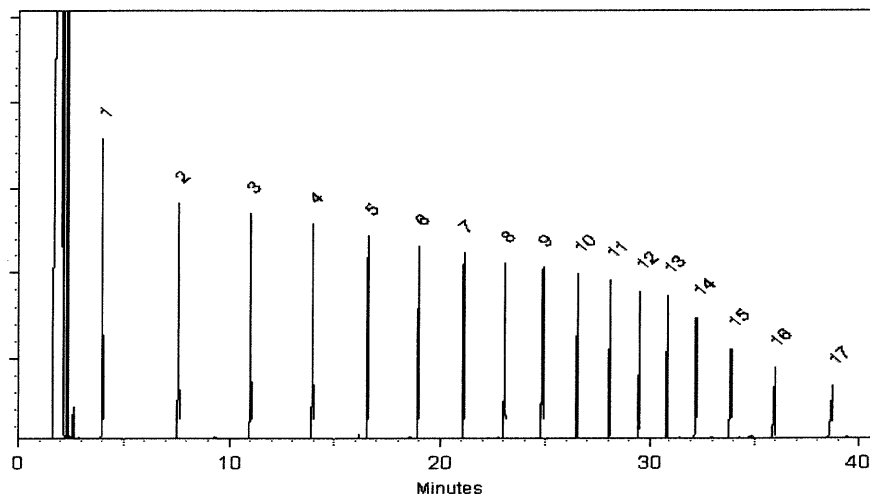

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Penelope S. Riglin
Penelope Riglin - Operations Tech I

Date Mixed: 16-Feb-2022 Balance: 1128360905

Clara Windle
Clara Windle - Operations Technician I

Date Passed: 21-Feb-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis

P11749 to P11758

Received by SJ 5/27/2022



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266 **Lot No.:** A0181886
Description : Florida TRPH Standard
Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : March 31, 2029 **Storage:** 25°C nominal
Handling: Sonicate prior to use. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	n-Octane (C8) CAS # 111-65-9 (Lot SHBM4827) Purity 99%	501.6 µg/mL	+/- 2.9794 µg/mL Gravimetric +/- 12.4620 µg/mL Unstressed +/- 14.9378 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 (Lot SHBM1113) Purity 99%	501.8 µg/mL	+/- 2.9802 µg/mL Gravimetric +/- 12.4657 µg/mL Unstressed +/- 14.9423 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 (Lot SHBK0925) Purity 99%	500.9 µg/mL	+/- 2.9752 µg/mL Gravimetric +/- 12.4446 µg/mL Unstressed +/- 14.9169 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 (Lot STBK2282) Purity 99%	500.7 µg/mL	+/- 2.9740 µg/mL Gravimetric +/- 12.4396 µg/mL Unstressed +/- 14.9110 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 (Lot SHBM4146) Purity 98%	500.5 µg/mL	+/- 2.9727 µg/mL Gravimetric +/- 12.4343 µg/mL Unstressed +/- 14.9046 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 (Lot UE5NG) Purity 98%	500.5 µg/mL	+/- 2.9730 µg/mL Gravimetric +/- 12.4355 µg/mL Unstressed +/- 14.9061 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 (Lot MKCF7888) Purity 99%	500.6 µg/mL	+/- 2.9731 µg/mL Gravimetric +/- 12.4359 µg/mL Unstressed +/- 14.9065 µg/mL Stressed

8	n-Docosane (C22)		501.5	µg/mL	+/-	2.9785	µg/mL	Gravimetric
	CAS # 629-97-0	(Lot MKCL8918)			+/-	12.4583	µg/mL	Unstressed
	Purity 99%				+/-	14.9333	µg/mL	Stressed
9	n-Tetracosane (C24)		500.6	µg/mL	+/-	2.9731	µg/mL	Gravimetric
	CAS # 646-31-1	(Lot MKCJ8741)			+/-	12.4359	µg/mL	Unstressed
	Purity 99%				+/-	14.9065	µg/mL	Stressed
10	n-Hexacosane (C26)		500.5	µg/mL	+/-	2.9728	µg/mL	Gravimetric
	CAS # 630-01-3	(Lot MKCD4540)			+/-	12.4347	µg/mL	Unstressed
	Purity 99%				+/-	14.9050	µg/mL	Stressed
11	n-Octacosane (C28)		500.6	µg/mL	+/-	2.9734	µg/mL	Gravimetric
	CAS # 630-02-4	(Lot BCCG0084)			+/-	12.4371	µg/mL	Unstressed
	Purity 99%				+/-	14.9080	µg/mL	Stressed
12	n-Triacontane (C30)		501.7	µg/mL	+/-	2.9799	µg/mL	Gravimetric
	CAS # 638-68-6	(Lot MKCN9321)			+/-	12.4645	µg/mL	Unstressed
	Purity 99%				+/-	14.9408	µg/mL	Stressed
13	n-Dotriacontane (C32)		501.8	µg/mL	+/-	2.9805	µg/mL	Gravimetric
	CAS # 544-85-4	(Lot BCBW0661)			+/-	12.4670	µg/mL	Unstressed
	Purity 99%				+/-	14.9437	µg/mL	Stressed
14	n-Tetratriacontane (C34)		501.3	µg/mL	+/-	2.9773	µg/mL	Gravimetric
	CAS # 14167-59-0	(Lot OML4N)			+/-	12.4533	µg/mL	Unstressed
	Purity 99%				+/-	14.9274	µg/mL	Stressed
15	n-Hexatriacontane (C36)		502.4	µg/mL	+/-	2.9841	µg/mL	Gravimetric
	CAS # 630-06-8	(Lot U25B014)			+/-	12.4819	µg/mL	Unstressed
	Purity 99%				+/-	14.9616	µg/mL	Stressed
16	n-Octatriacontane (C38)		501.7	µg/mL	+/-	2.9801	µg/mL	Gravimetric
	CAS # 7194-85-6	(Lot 0000127235)			+/-	12.4653	µg/mL	Unstressed
	Purity 97%				+/-	14.9417	µg/mL	Stressed
17	n-Tetracontane (C40)		500.2	µg/mL	+/-	2.9713	µg/mL	Gravimetric
	CAS # 4181-95-7	(Lot PADGI)			+/-	12.4282	µg/mL	Unstressed
	Purity 98%				+/-	14.8973	µg/mL	Stressed
Solvent:	Hexane							
	CAS # 110-54-3							
	Purity 99%							

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

330°C

Det. Type:

FID

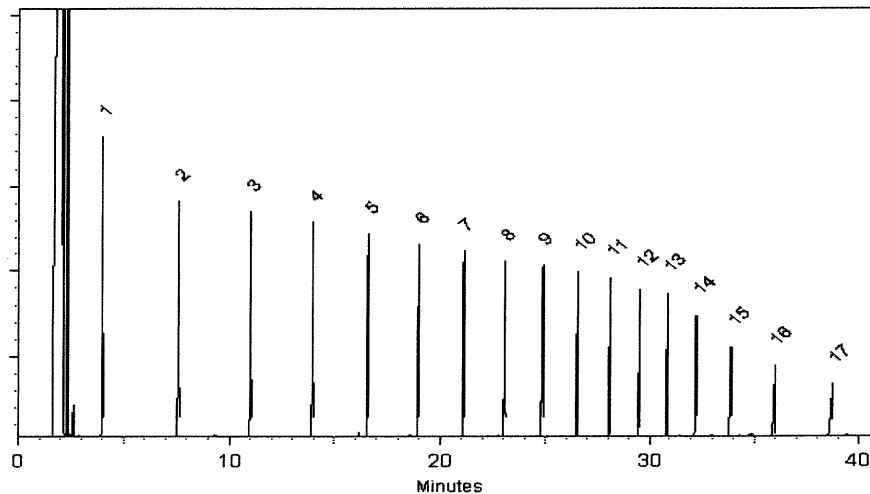

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Penelope Riglin - Operations Tech I

Date Mixed: 16-Feb-2022

Balance: 1128360905

Clara Windle - Operations Technician I

Date Passed: 21-Feb-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.