

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012023\
 Data File : PL080446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Jan 2023 01:19
 Operator : AR\AJ
 Sample : 01233-04
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 B-P36A

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/23/2023
 Supervised By : Ankita Jodhani 01/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 21 06:21:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 20 17:01:11 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.350	2.689	42299982	43650345	19.722m	19.873
28) SA Decachlor...	8.789	7.838	32194984	40145490	18.389	16.850

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012023\
Data File : PL080446.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Jan 2023 01:19
Operator : AR\AJ
Sample : 01233-04
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
B-P36A


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/23/2023
Supervised By : Ankita Jodhani 01/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 21 06:21:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Fri Jan 20 17:01:11 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

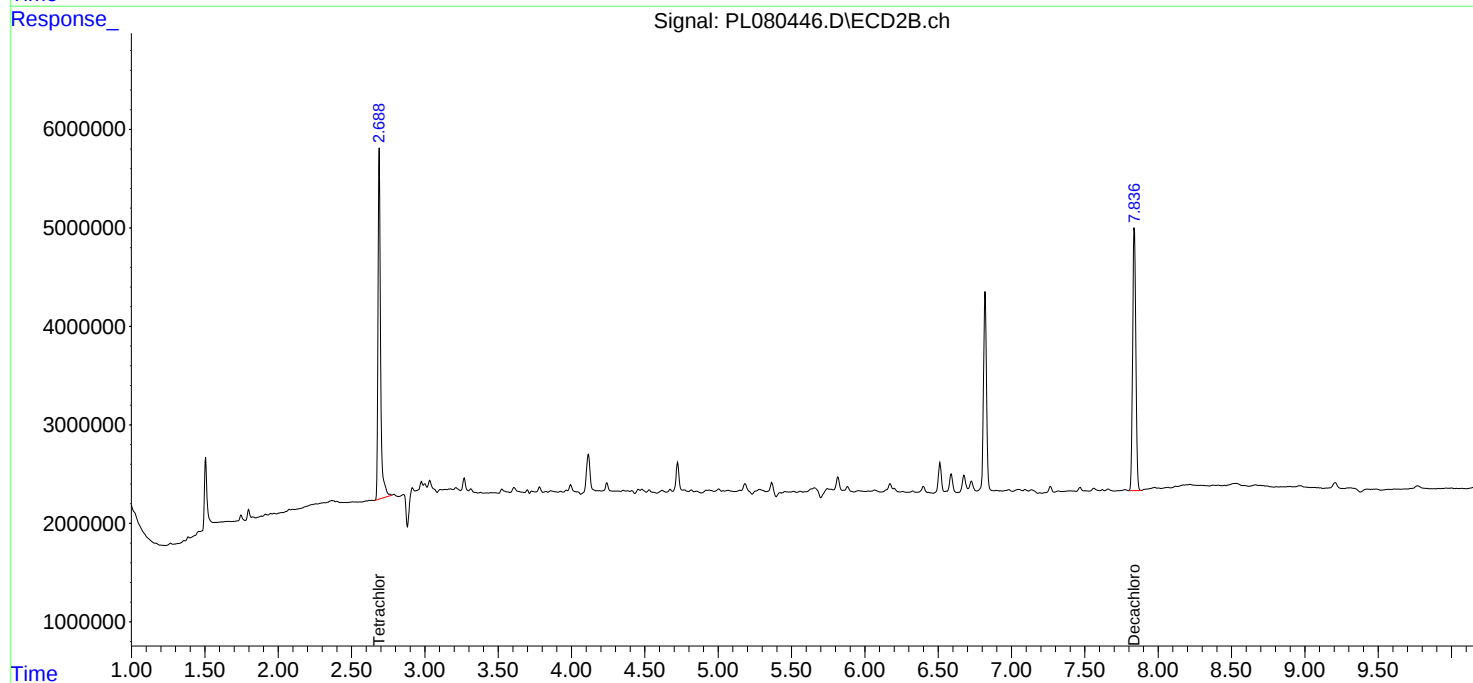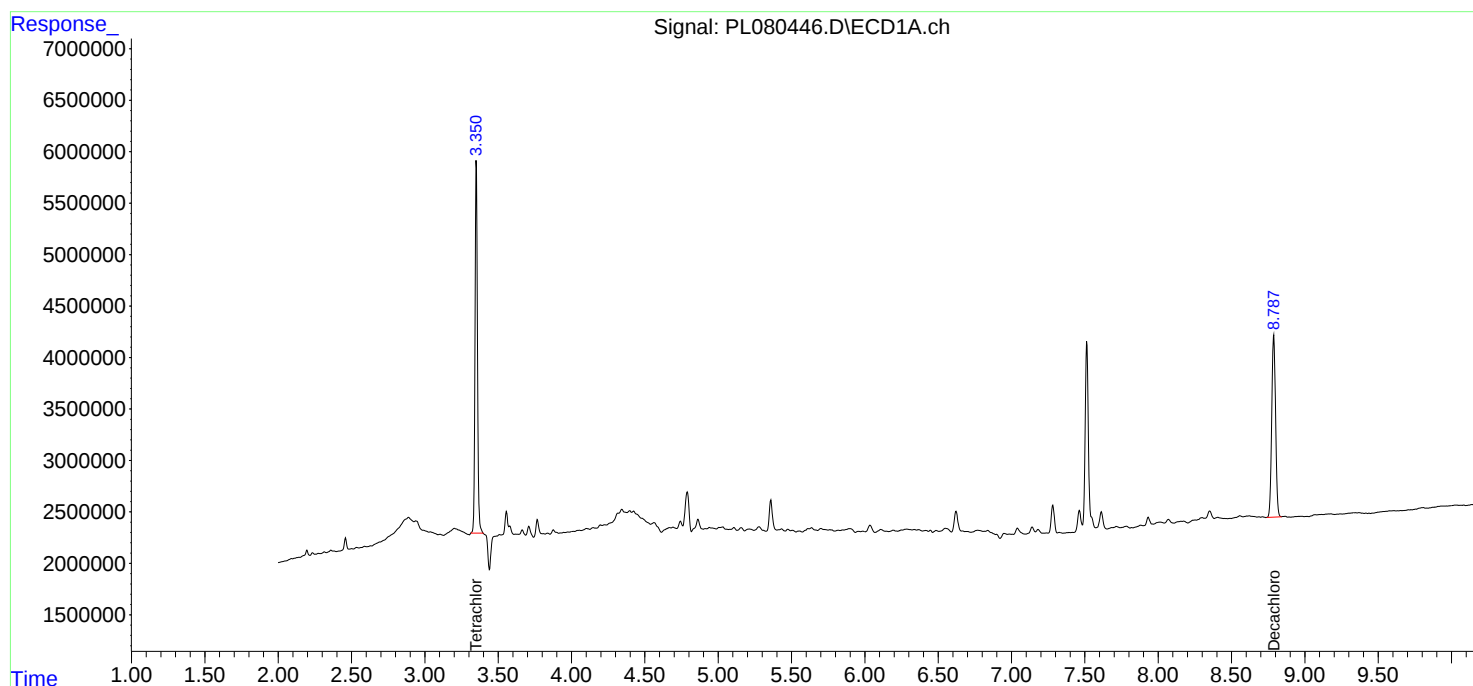

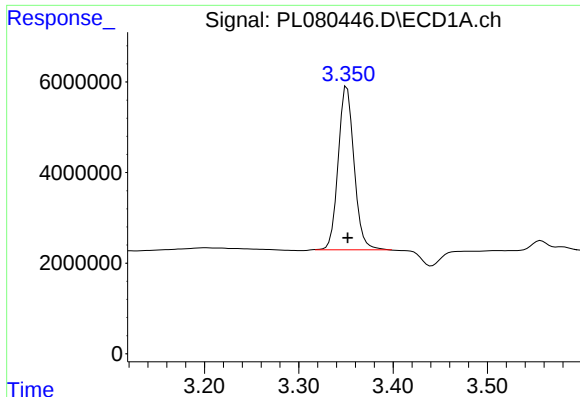


#1 Tetrachloro-m-xylene

R.T.: 3.350 min
Delta R.T.: -0.002 min
Response: 42299982
Conc: 19.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
B-P36A


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/23/2023
Supervised By :Ankita Jodhani 01/23/2023

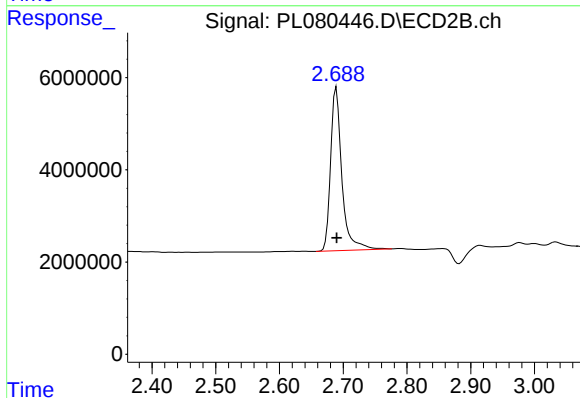


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 43650345
Conc: 19.87 ng/ml

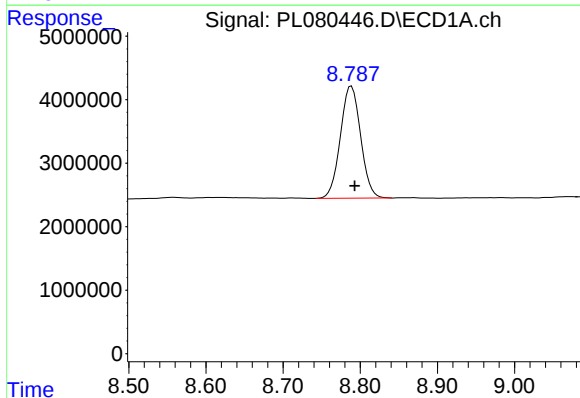

#28 Decachlorobiphenyl

R.T.: 8.789 min
Delta R.T.: -0.005 min
Response: 32194984
Conc: 18.39 ng/ml

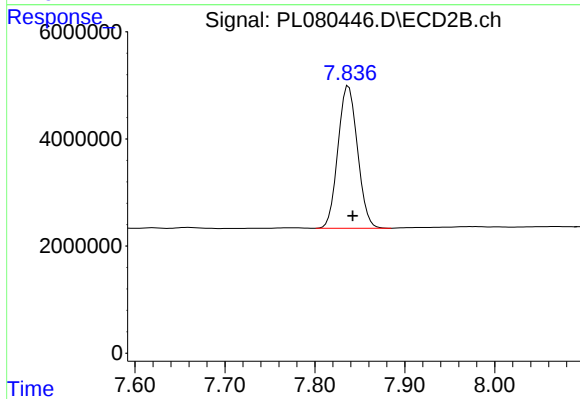

#28 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: -0.004 min
Response: 40145490
Conc: 16.85 ng/ml