



Prep Standard - Chemical Standard Summary

Order ID : O1233

Test : Pesticide-TCL

Prepbatch ID : PB150373,

Sequence ID/Qc Batch ID: pl012023,

Standard ID :

EP2279,EP2294,PP20663,PP20664,PP20666,PP20667,PP20668,PP20674,PP20675,PP20676,PP20677,PP20678,PP20679,PP20680,PP20681,PP20682,PP20683,PP20684,PP20685,PP20686,PP20687,PP20688,PP20689,PP20714,PP20715,PP20716,PP20717,PP20718,PP21237,PP21328,PP21357,

Chemical ID :

E2865,E3390,E3393,E3403,E3412,E3435,E3436,E3453,E3455,E3456,P10278,P10581,P10711,P10786,P10886,P11061,P11790,P11811,P8733,P8742,P9648,P9653,W2938,W2939,

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2279	11/28/2022	04/13/2023	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 11/28/2022

FROM 4000.00000gram of E3412 = Final Quantity: 4000.000 gram

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	EP2294	01/17/2023	07/16/2023	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 01/17/2023

FROM 8000.00000ml of E3455 + 8000.00000ml of E3456 = Final Quantity: 16000.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP20663	09/01/2022	03/01/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 1.00000ml of P10581 + 9.00000ml of E3390 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3629	20 PPM PEST stock Solution 1st source(RESTEK)	PP20664	09/01/2022	03/01/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 1.00000ml of P9653 + 9.00000ml of E3390 = Final Quantity: 10.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1273	20 PPM Mirex Stock (Primary Source)	PP20666	09/01/2022	03/01/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 1.00000ml of P8733 + 9.00000ml of E3390 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3663	20 PPM MIREX Stock STD (Secondary source)	PP20667	09/01/2022	03/01/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 1.00000ml of P9648 + 9.00000ml of E3390 = Final Quantity: 10.000 ml

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3630	100/100 PPB PEST Working std.1st Source(RESTEK)	PP20668	09/01/2022	03/01/2023	Abdul Mirza	None	None	Ankita Jodhani 09/09/2022
<u>FROM</u> 98.50000ml of E3390 + 0.50000ml of PP20663 + 0.50000ml of PP20664 + 0.50000ml of PP20666 = Final Quantity: 100.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
386	1000/100 PPB Chlordane STD (Restek)	PP20674	09/01/2022	03/01/2023	Abdul Mirza	None	None	Ankita Jodhani 09/09/2022
<u>FROM</u> 0.10000ml of P8742 + 99.40000ml of E3393 + 0.50000ml of PP20663 = Final Quantity: 100.000 ml								

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3746	1000/100 ppb Chlordane STD-RESTEK 2ND SOURCE	PP20675	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.10000ml of P10278 + 0.50000ml of P8742 + 99.40000ml of W2939 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3631	75 PPB ICAL PEST STD(RESTEK)	PP20676	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.25000ml of W2938 + 0.75000ml of PP20668 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3632	50 PPB ICAL PEST STD(RESTEK)	PP20677	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.50000ml of W2938 + 0.50000ml of PP20668 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3633	25 PPB ICAL PEST STD(RESTEK)	PP20678	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.75000ml of W2938 + 0.25000ml of PP20668 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3634	5 PPB ICAL PEST STD(RESTEK)	PP20679	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.90000ml of W2938 + 0.10000ml of PP20677 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
528	CHLOR 750 PPB STD	PP20680	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.25000ml of W2938 + 0.75000ml of PP20674 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
529	CHLOR 500 PPB STD	PP20681	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.50000ml of W2938 + 0.50000ml of PP20674 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
530	CHLOR 250 PPB STD	PP20682	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.75000ml of W2938 + 0.25000ml of PP20674 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3408	CHLOR 50 PPB STD	PP20683	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.90000ml of W2938 + 0.10000ml of PP20681 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
383	1000/100 PPB Toxaphene STD (Restek)	PP20684	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.10000ml of P10711 + 99.40000ml of W2938 + 0.50000ml of PP20663 = Final Quantity: 100.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3669	1000/100 PPB TOXAPHENE STD 2nd source (RESTEK)	PP20685	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.10000ml of P11811 + 99.40000ml of W2939 + 0.50000ml of PP20663 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
533	TOX 750 PPB STD	PP20686	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.25000ml of W2939 + 0.75000ml of PP20684 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
534	TOX 500 PPB STD	PP20687	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.50000ml of W2939 + 0.50000ml of PP20684 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
535	TOX 250 PPB STD	PP20688	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.75000ml of W2939 + 0.25000ml of PP20684 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2217	TOX 100 PPB STD	PP20689	09/01/2022	02/23/2023	Abdul Mirza	None	None	Ankita Jodhani
09/09/2022								

FROM 0.90000ml of W2939 + 0.10000ml of PP20684 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1472	20 PPM Pest Stock Solution 2nd Source	PP20714	09/07/2022	03/07/2023	Ankita Jodhani	None	None	Yogesh Patel
09/09/2022								

FROM 1.00000ml of P11061 + 9.00000ml of E3393 = Final Quantity: 10.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
80	100/100 PPB Pesticide Working Solution 2nd Source	PP20715	09/07/2022	03/01/2023	Ankita Jodhani	None	None	Yogesh Patel
09/09/2022								

FROM 98.50000ml of E3393 + 0.50000ml of PP20663 + 0.50000ml of PP20667 + 0.50000ml of PP20714 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3988	50 PPB PEST ICV STD(RESTEK)	PP20716	09/07/2022	03/01/2023	Ankita Jodhani	None	None	Yogesh Patel
09/09/2022								

FROM 0.50000ml of E3393 + 0.50000ml of PP20715 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
532	CHLOR 500 PPB ICV STD	PP20717	09/07/2022	02/23/2023	Ankita Jodhani	None	None	Yogesh Patel
09/09/2022								

FROM 0.50000ml of E3393 + 0.50000ml of PP20675 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3670	TOX 500 PPB ICV std (RESTEK)	PP20718	09/07/2022	02/23/2023	Ankita Jodhani	None	None	Yogesh Patel
09/09/2022								

FROM 0.50000ml of E3393 + 0.50000ml of PP20685 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
79	500 PPB Pesticide Spike Solution	PP21237	12/06/2022	03/01/2023	Abdul Mirza	None	None	Ankita Jodhani
12/07/2022								

FROM 95.00000ml of E3435 + 2.50000ml of PP20667 + 2.50000ml of PP20714 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
758	PEM Mix w/Surr	PP21328	01/04/2023	07/03/2023	Abdul Mirza	None	None	Ankita Jodhani
01/05/2023								

FROM 1.00000ml of P11790 + 99.00000ml of E3453 = Final Quantity: 100.000 ml

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP21357	01/10/2023	06/08/2023	Abdul Mirza	None	None	Ankita Jodhani 01/12/2023
<u>FROM</u>	1.00000ml of P10786 + 999.00000ml of E3436 = Final Quantity: 1000.000 ml							

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	12/31/2024	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	21L2662004	03/01/2023	09/01/2022 / Rajesh	08/24/2022 / Rajesh	E3390

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	21L2662004	03/07/2023	09/07/2022 / Rajesh	08/31/2022 / Rajesh	E3393

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
phenomenex	FS0006 / Cleanert SPE Silica, 1000 mg/6ml, 30PK	X0607-FS	03/23/2023	10/28/2022 / Sohil	09/23/2022 / Rajesh	E3403

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	139404	10/23/2023	10/18/2022 / Rajesh	10/13/2022 / Rajesh	E3412

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	22D1162003	06/05/2023	12/05/2022 / Rajesh	12/05/2022 / Rajesh	E3435

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	22E1562001	06/08/2023	12/08/2022 / Rajesh	12/05/2022 / Rajesh	E3436

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	22G0362002	07/03/2023	01/03/2023 / Rajesh	01/03/2023 / Rajesh	E3453

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	22G0362002	07/16/2023	01/16/2023 / Rajesh	01/11/2023 / Rajesh	E3455

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	22J0461011	07/17/2023	01/17/2023 / Rajesh	01/11/2023 / Rajesh	E3456

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32021 / Pesticide Mix, chlordane (technical), 1000ug/mL, hexane, 1mL,	A0162956	03/01/2023	09/01/2022 / Abdul	03/04/2021 / Abdul	P10278

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0171211	03/01/2023	09/01/2022 / Abdul	05/24/2021 / Abdul	P10581

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32005 / Toxaphene Standard	A0169056	03/01/2023	09/01/2022 / Abdul	06/17/2021 / dhaval	P10711

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0172332	07/10/2023	01/10/2023 / Abdul	06/17/2021 / dhaval	P10786

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
ULTRA Scientific	CLP-242 / Pesticide Resolution Check Mixture	0006617274	07/18/2023	01/18/2023 / Ankita	07/13/2021 / Ankita	P10886

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
ULTRA Scientific	CLP-242 / Pesticide Resolution Check Mixture	0006617274	07/18/2023	01/18/2023 / Ankita	07/13/2021 / Ankita	P10886

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32291 / Pesticide Mix, CLP method, organochlorine Std AB#1, 200ug/mL, hexane/toluene, 1mL/ampul	A0168439	03/07/2023	09/07/2022 / Ankita	09/29/2021 / Abdul	P11061

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32074 / Pesticide Performance Evaluation Mix w/Surrogate	A0183168	07/04/2023	01/04/2023 / Abdul	05/27/2022 / Sohil	P11790

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32005 / Toxaphene Standard	A0177326	03/01/2023	09/01/2022 / Abdul	06/17/2022 / Ankita	P11811

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	79136 / Mirex, 1000 ug/ml	030818	03/01/2023	09/01/2022 / Abdul	07/30/2019 / Ankita	P8733

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32021 / Pesticide Mix, chlordane (technical), 1000ug/mL, hexane, 1mL,	A0144623	03/01/2023	09/01/2022 / Abdul	07/30/2019 / somina	P8742

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	79136 / Mirex, 1000 ug/ml	061820	03/01/2023	09/01/2022 / Abdul	06/19/2020 / Sohil	P9648

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32291 / Pesticide Mix, CLP method, organochlorine Std AB#1, 200ug/mL, hexane/toluene, 1mL/ampul	A0154466	03/01/2023	09/01/2022 / Abdul	06/22/2020 / Sohil	P9653

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	2280762004	02/23/2023	07/25/2022 / JIGNESH	07/25/2022 / JIGNESH	W2938



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	2280762004	02/23/2023	07/25/2022 / JIGNESH	07/25/2022 / JIGNESH	W2939



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

DD
06/17/2021

Catalog No.: 32000 Lot No.: A0172332
Description: Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul
Container Size: 2 mL Pkg Amt: > 1 mL
Expiration Date: August 31, 2027 Storage: 10°C or colder
Handling: Contains PCBs - sonicate prior to use. Ship: Ambient

P10783
To - (10)
P10792

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene CAS # 877-09-8 (Lot 0052481) Purity 98%	200.7 µg/mL	+/- 1.1840 µg/mL Gravimetric +/- 6.3622 µg/mL Unstressed +/- 8.3106 µg/mL Stressed
2	Decachlorobiphenyl (BZ# 209) CAS # 2051-24-3 (Lot 30679) Purity 99%	200.2 µg/mL	+/- 1.1810 µg/mL Gravimetric +/- 6.3463 µg/mL Unstressed +/- 8.2897 µg/mL Stressed
Solvent:	Acetone CAS # 67-64-1 Purity 99%		

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

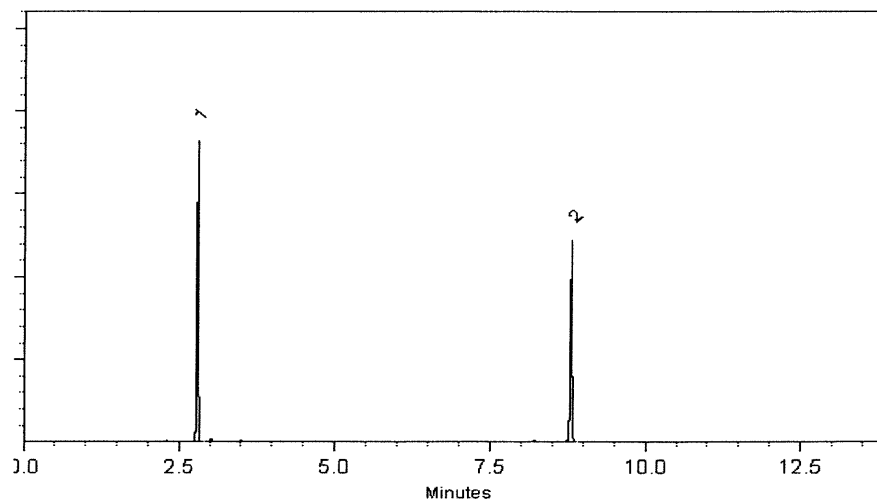

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 12-May-2021

Balance: B707717271

Alexis Shelow
Alexis Shelow - Operations Tech I

Date Passed: 14-May-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32005 Lot No.: A0169056
Description : Toxaphene Standard
Toxaphene Standard 1000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : May 31, 2025 Storage: 10°C or colder
Ship: Ambient

DD
06/17/2021
P10708
To - (S)
P10712

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Toxaphene	1,000.0 µg/mL	+/- 5.9397 µg/mL Gravimetric
	CAS # 8001-35-2 (Lot 1051817)		+/- 31.7072 µg/mL Unstressed
	Purity ----%		+/- 41.4130 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

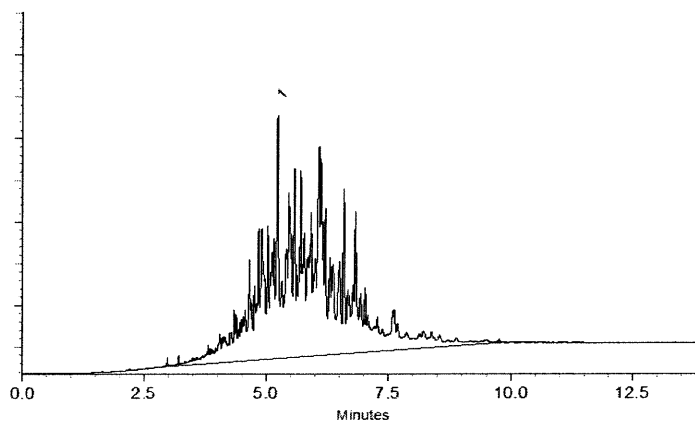

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 14-Feb-2021

Balance: B707717271

Justine Alibertson
Justine Alibertson - Operations Tech-ARM QC

Date Passed: 18-Feb-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1

Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent



Material No.: 9262-03

Batch No.: 21L2662004

Manufactured Date: 2021-11-24

Expiration Date: 2023-02-23

Revision No.: 0


Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	2
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	< 1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD
Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 8/24/22

E33901


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent



Material No.: 9262-03
Batch No.: 21L2662004
Manufactured Date: 2021-11-24
Expiration Date: 2023-02-23
Revision No.: 0


Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	2
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	< 1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD
Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 8/31/22

E3393


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Cleanert Florisil

1g/6ml 30/pkg

LOT#:X0607-FS

MFG#:E01389



CAT# FS0006



Made in China

 Agela Technologies

E3403






**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**



MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MÉXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT : SODIUM SULFATE CRYSTALS ANHYDROUS
QUALITY : ACS (CODE RMB3375) **FORMULA :** Na₂SO₄
SPECIFICATION NUMBER : 6399 **RELEASE DATE:** OCT/28/2021
LOT NUMBER : 139404

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.8 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.0
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.002 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.2 %
Retained on US Standard No. 60 sieve	Min. 94%	97.6 %
Through US Standard No. 60 sieve	Max. 5%	2.1 %
Through US Standard No. 100 sieve	Max. 10%	0.2 %
COMMENTS		
 QC: PhC Irma Belmares		

If you need further details, please call our factory or contact our local distributor.

E 3412

Recd. by RP on 10/13/22

RE-02-01, Ed. 3

Material No.: 9254-03
Batch No.: 22D1162003
Manufactured Date: 2022-03-20
Expiration Date: 2025-03-19
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.4 %	99.8 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	< 1.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	≤ 0.3	0.2
Titration Base (µeq/g)	≤ 0.6	< 0.1
Water (H ₂ O)	≤ 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	< 1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Rec'd by RP on 12/5/22

E 3435


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Page 1 of 1

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03
Batch No.: 22E1562001
Manufactured Date: 2022-05-03
Expiration Date: 2025-05-02
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.4 %	99.8 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	< 1.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H ₂ O)	≤ 0.5 %	0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 12/5/22

E3436

Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent



Material No.: 9262-03
Batch No.: 22G0362002
Manufactured Date: 2022-06-17
Expiration Date: 2023-09-16
Revision No.: 0

Certificate of Analysis


Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	2
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	2
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.5 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	97 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 01/03/23

E 3453

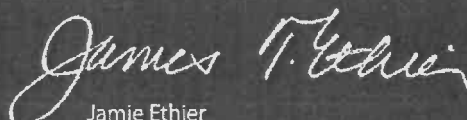
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent



Material No.: 9262-03
Batch No.: 22G0362002
Manufactured Date: 2022-06-17
Expiration Date: 2023-09-16
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	2
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	2
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.5 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	97 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RL on 11/11/23

E 3455


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Acetone
CMOS



Material No.: 9005-05
Batch No.: 22J0461011
Manufactured Date: 2022-09-29
Retest Date: 2027-09-28
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.8 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.2
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.2 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities – Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities – Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Calcium (Ca)	≤ 25.0 ppb	4.9 ppb
Trace Impurities – Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities – Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

Recd. by R2 on 01/11/23

>>> Continued on page 2 >>>

E 3456

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Acetone
CMOS



Material No.: 9005-05
Batch No.: 22J0461011

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	1.8 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	4 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	2 par/ml

>>> Continued on page 3 >>>

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Acetone
CMOS



Material No.: 9005-05
Batch No.: 22J0461011

Test	Specification	Result
------	---------------	--------

For Microelectronic Use

Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32021 Lot No.: A0162956
Description : Chlordane Standard
Chlordane Standard 1000µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : October 31, 2026 Storage: 10°C or colder

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)			
1	Chlordane	1,007.0 µg/mL	+/-	5.9813	µg/mL	Gravimetric
	CAS # 57-74-9 (Lot 142990)		+/-	31.9292	µg/mL	Unstressed
	Purity ----%		+/-	41.7029	µg/mL	Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 10275
P 10276
P 10277
P 10278
P 10279

AR
03.05.2021

Tech Tips:

CAS #57-74-9 nomenclature is based on EPA method 8081B.

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


helium-constant pressure 20 psi.

200°C to 300°C
@ 25°C/min. (hold 10 min.)

250°C

300°C

ECD

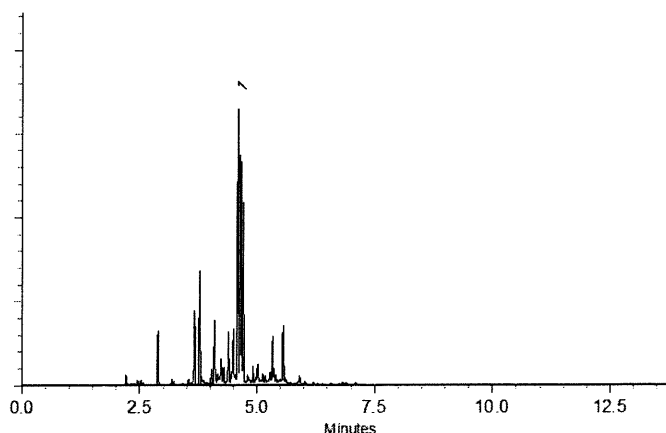

Lane Kibe
Lane Kibe - Mix Technician

Date Mixed: 27-Jul-2020

Balance: 1127510105


Justine Albertson - Operations Tech-ARM QC

Date Passed: 29-Jul-2020

**Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397**

1505.20.E0



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 Lot No.: A0171211
Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : July 31, 2027 Storage: 10°C or colder
Handling: Contains PCBs - sonicate prior to use. Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene CAS # 877-09-8 (Lot 0052481) Purity 98%	199.9 µg/mL	+/- 1.1875 µg/mL Gravimetric +/- 6.3389 µg/mL Unstressed +/- 8.2793 µg/mL Stressed
2	Decachlorobiphenyl (BZ# 209) CAS # 2051-24-3 (Lot ER071509-01) Purity 99%	200.0 µg/mL	+/- 1.1879 µg/mL Gravimetric +/- 6.3414 µg/mL Unstressed +/- 8.2826 µg/mL Stressed

Solvent: Acetone
CAS # 67-64-1
Purity 99%

P 10573
↓
P 10582
|

AR
05/25/2021

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

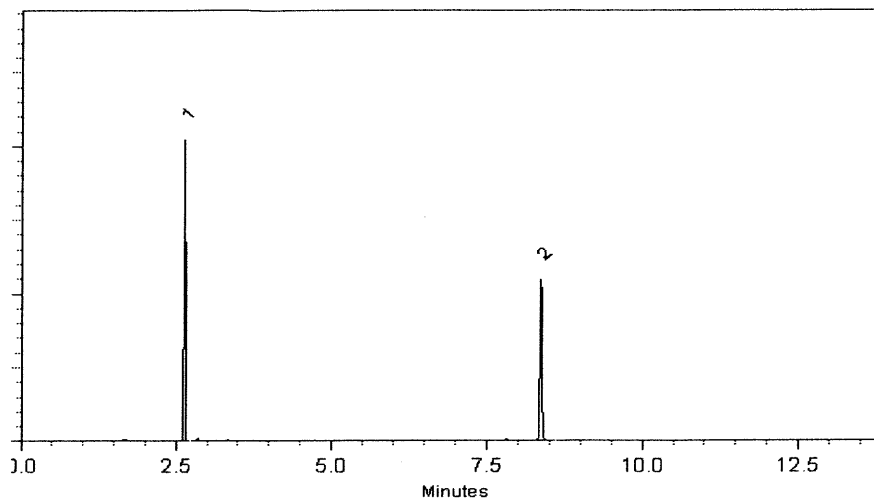

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Jeremy Johnson - Mfg. Supervisor

Date Mixed: 12-Apr-2021

Balance: 1128342314

Marlina Cowan - Operations Tech I

Date Passed: 19-Apr-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



Certificate of Analysis

Product Name: Pesticides Resolution Check Standard

Product Number: CLP-242-1

Lot Issue Date: 08-Jul-2021

Lot Number: 0006617274

Expiration Date: 31-Aug-2023

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration \pm Uncertainty
trans-chlordane	005103-74-2	RM02726	10.0 \pm 0.1 ng/mL
4,4'-DDE	000072-55-9	RM02892	20.1 \pm 0.1 ng/mL
decachlorobiphenyl (BZ # 209)	002051-24-3	RM01256	20.1 \pm 0.1 ng/mL
dieldrin	000060-57-1	RM16038	20.0 \pm 0.1 ng/mL
endosulfan I	000959-98-8	RM15536	10.0 \pm 0.1 ng/mL
endosulfan sulfate	001031-07-8	RM15389	20.0 \pm 0.1 ng/mL
endrin ketone	053494-70-5	NT00720	20.0 \pm 0.1 ng/mL
methoxychlor	000072-43-5	RM14186	100.1 \pm 0.5 ng/mL
2,4,5,6-tetrachloro-m-xylene	000877-09-8	RM13844	20.1 \pm 0.1 ng/mL

Matrix: hexane

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

P 10883

↓

P 10902

AJ
07/13/21



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 1 of 2

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937

Certificate of Analysis

Product Number: CLP-242-1

Lot Number: 0006617274

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.


Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:



Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32291 **Lot No.:** A0168439

Description : Organochlorine Pesticide Mix AB #1

Organochlorine Pesticide Mix AB #1 200µg/mL, Hexane/Toluene(50:50), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2025 **Storage:** 10°C or colder

Ship: Ambient

P11061
↓
P11065
AR
9/30/2024

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	alpha-BHC CAS # 319-84-6 (Lot 0012018BHC) Purity 99%	200.5 µg/mL	+/- 1.4217 µg/mL +/- 9.1674 µg/mL +/- 13.2104 µg/mL	Gravimetric Unstressed Stressed
2	gamma-BHC (Lindane) CAS # 58-89-9 (Lot 10972000) Purity 97%	200.8 µg/mL	+/- 1.4238 µg/mL +/- 9.1807 µg/mL +/- 13.2295 µg/mL	Gravimetric Unstressed Stressed
3	beta-BHC CAS # 319-85-7 (Lot SL210106) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL +/- 9.1446 µg/mL +/- 13.1774 µg/mL	Gravimetric Unstressed Stressed
4	delta-BHC CAS # 319-86-8 (Lot ER02101401) Purity 98%	199.9 µg/mL	+/- 1.4176 µg/mL +/- 9.1409 µg/mL +/- 13.1722 µg/mL	Gravimetric Unstressed Stressed
5	Heptachlor CAS # 76-44-8 (Lot 0006540595) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL +/- 9.1446 µg/mL +/- 13.1774 µg/mL	Gravimetric Unstressed Stressed
6	Aldrin CAS # 309-00-2 (Lot 11129800) Purity 97%	199.8 µg/mL	+/- 1.4169 µg/mL +/- 9.1363 µg/mL +/- 13.1656 µg/mL	Gravimetric Unstressed Stressed
7	Heptachlor epoxide (isomer B) CAS # 1024-57-3 (Lot 10039000) Purity 99%	200.5 µg/mL	+/- 1.4217 µg/mL +/- 9.1674 µg/mL +/- 13.2104 µg/mL	Gravimetric Unstressed Stressed

8	trans-Chlordane CAS # 5103-74-2 Purity 99%	(Lot 32095)	200.5 µg/mL	+/- +/- +/-	1.4217 9.1674 13.2104	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	cis-Chlordane CAS # 5103-71-9 Purity 99%	(Lot 31707)	200.0 µg/mL	+/- +/- +/-	1.4182 9.1446 13.1774	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	Endosulfan I CAS # 959-98-8 Purity 99%	(Lot BCBS8631)	200.5 µg/mL	+/- +/- +/-	1.4217 9.1674 13.2104	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	4,4'-DDE CAS # 72-55-9 Purity 99%	(Lot GHYQG)	200.0 µg/mL	+/- +/- +/-	1.4182 9.1446 13.1774	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	Dieldrin CAS # 60-57-1 Purity 98%	(Lot 10714300)	200.4 µg/mL	+/- +/- +/-	1.4211 9.1633 13.2045	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	Endrin CAS # 72-20-8 Purity 98%	(Lot 11129700)	199.9 µg/mL	+/- +/- +/-	1.4176 9.1409 13.1722	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	4,4'-DDD CAS # 72-54-8 Purity 99%	(Lot HAN02)	200.5 µg/mL	+/- +/- +/-	1.4217 9.1674 13.2104	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	Endosulfan II CAS # 33213-65-9 Purity 99%	(Lot 11129400)	201.0 µg/mL	+/- +/- +/-	1.4253 9.1903 13.2433	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	4,4'-DDT CAS # 50-29-3 Purity 99%	(Lot S37912V)	200.0 µg/mL	+/- +/- +/-	1.4182 9.1446 13.1774	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	Endrin aldehyde CAS # 7421-93-4 Purity 98%	(Lot 30455)	200.9 µg/mL	+/- +/- +/-	1.4245 9.1857 13.2367	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
18	Endosulfan sulfate CAS # 1031-07-8 Purity 99%	(Lot BCCB0424)	200.0 µg/mL	+/- +/- +/-	1.4182 9.1446 13.1774	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
19	Methoxychlor CAS # 72-43-5 Purity 97%	(Lot 10720900)	199.8 µg/mL	+/- +/- +/-	1.4169 9.1363 13.1656	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
20	Endrin ketone CAS # 53494-70-5 Purity 97%	(Lot 11129600)	199.8 µg/mL	+/- +/- +/-	1.4169 9.1363 13.1656	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
Solvent: Hexane/Toluene (50:50) CAS # 110-54-3/108-88-3 Purity 99%							

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
150°C to 300°C
@ 4°C/min. (hold 5 min.)

Inj. Temp:
200°C

Det. Temp:
300°C

Det. Type:
ECD

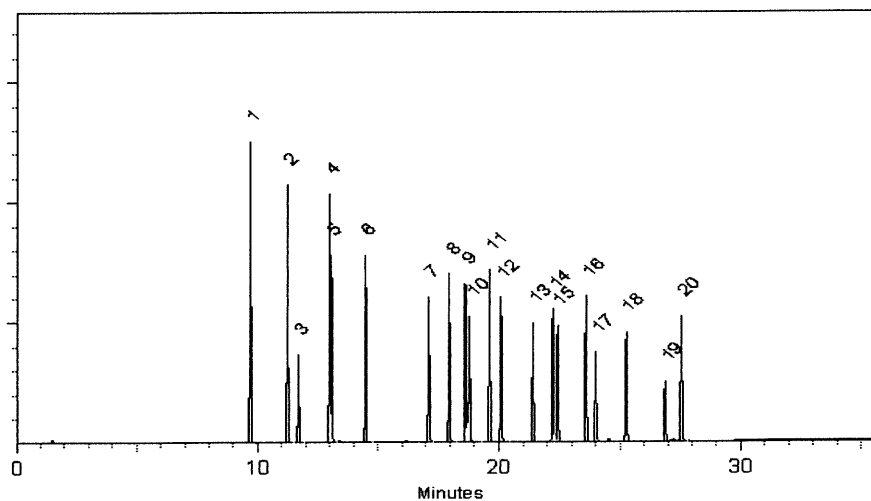

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Matt Fragassi - Mix Technician

Date Mixed: 25-Jan-2021

Balance: 1128342314


Marlene Cowan - Operations Tech I

Date Passed: 29-Jan-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11061
↓
P11065
AR
9/30/2021

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis

P11789 to P11793

Received by SJ 5/27/2022



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32074 **Lot No.:** A0183168

Description : Pesticide Performance Eval Mix w/Surrogate

Performance Evaluation Std. 3/90 SOW w/surrogates 1-25µg/mL,
Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : March 31, 2026 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	2,4,5,6-Tetrachloro-m-xylene CAS # 877-09-8 (Lot 0052481) Purity 98%	2.0 µg/mL	+/- 0.1220 +/- 0.1523 +/- 0.1799	µg/mL Gravimetric Unstressed Stressed
2	alpha-BHC CAS # 319-84-6 (Lot 12469000) Purity 99%	1.0 µg/mL	+/- 0.0610 +/- 0.0762 +/- 0.0900	µg/mL Gravimetric Unstressed Stressed
3	gamma-BHC (Lindane) CAS # 58-89-9 (Lot 12642100) Purity 99%	1.0 µg/mL	+/- 0.0610 +/- 0.0762 +/- 0.0900	µg/mL Gravimetric Unstressed Stressed
4	beta-BHC CAS # 319-85-7 (Lot BCCCC6425) Purity 99%	1.0 µg/mL	+/- 0.0610 +/- 0.0762 +/- 0.0900	µg/mL Gravimetric Unstressed Stressed
5	Endrin CAS # 72-20-8 (Lot 13000500) Purity 99%	5.1 µg/mL	+/- 0.3045 +/- 0.3805 +/- 0.4496	µg/mL Gravimetric Unstressed Stressed
6	4,4'-DDT CAS # 50-29-3 (Lot 210916JLM) Purity 99%	10.1 µg/mL	+/- 0.6090 +/- 0.7609 +/- 0.8992	µg/mL Gravimetric Unstressed Stressed
7	Methoxychlor CAS # 72-43-5 (Lot 12555700) Purity 98%	25.2 µg/mL	+/- 1.5221 +/- 1.9018 +/- 2.2475	µg/mL Gravimetric Unstressed Stressed

8	Decachlorobiphenyl (BZ# 209)	2.0 µg/mL	+/- 0.1221	µg/mL	Gravimetric
	CAS # 2051-24-3 (Lot 30679)		+/- 0.1524	µg/mL	Unstressed
	Purity 99%		+/- 0.1800	µg/mL	Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:
30m x .25mm x .2µm
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
150°C to 300°C
@ 4°C/min. (hold 5 min.)

Inj. Temp:
200°C

Det. Temp:
300°C


Det. Type:
ECD

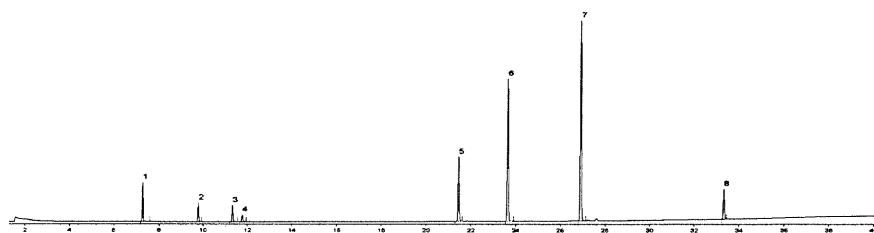

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Brittany Federinko - Operations Tech I

Date Mixed: 22-Mar-2022 **Balance:** 1128360905


John Lidgett - AD Chemist

Date Passed: 24-Mar-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

P11794 to P11798

Received by SJ 5/27/2022



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32074 **Lot No.:** A0183168

Description : Pesticide Performance Eval Mix w/Surrogate

Performance Evaluation Std. 3/90 SOW w/surrogates 1-25µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : March 31, 2026 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)			
1	2,4,5,6-Tetrachloro-m-xylene	2.0 µg/mL	+/-	0.1220	µg/mL	Gravimetric
	CAS # 877-09-8 (Lot 0052481)		+/-	0.1523	µg/mL	Unstressed
	Purity 98%		+/-	0.1799	µg/mL	Stressed
2	alpha-BHC	1.0 µg/mL	+/-	0.0610	µg/mL	Gravimetric
	CAS # 319-84-6 (Lot 12469000)		+/-	0.0762	µg/mL	Unstressed
	Purity 99%		+/-	0.0900	µg/mL	Stressed
3	gamma-BHC (Lindane)	1.0 µg/mL	+/-	0.0610	µg/mL	Gravimetric
	CAS # 58-89-9 (Lot 12642100)		+/-	0.0762	µg/mL	Unstressed
	Purity 99%		+/-	0.0900	µg/mL	Stressed
4	beta-BHC	1.0 µg/mL	+/-	0.0610	µg/mL	Gravimetric
	CAS # 319-85-7 (Lot BCCC6425)		+/-	0.0762	µg/mL	Unstressed
	Purity 99%		+/-	0.0900	µg/mL	Stressed
5	Endrin	5.1 µg/mL	+/-	0.3045	µg/mL	Gravimetric
	CAS # 72-20-8 (Lot 13000500)		+/-	0.3805	µg/mL	Unstressed
	Purity 99%		+/-	0.4496	µg/mL	Stressed
6	4,4'-DDT	10.1 µg/mL	+/-	0.6090	µg/mL	Gravimetric
	CAS # 50-29-3 (Lot 210916JLM)		+/-	0.7609	µg/mL	Unstressed
	Purity 99%		+/-	0.8992	µg/mL	Stressed
7	Methoxychlor	25.2 µg/mL	+/-	1.5221	µg/mL	Gravimetric
	CAS # 72-43-5 (Lot 12555700)		+/-	1.9018	µg/mL	Unstressed
	Purity 98%		+/-	2.2475	µg/mL	Stressed

8	Decachlorobiphenyl (BZ# 209)	2.0 µg/mL	+/- 0.1221	µg/mL	Gravimetric
	CAS # 2051-24-3 (Lot 30679)		+/- 0.1524	µg/mL	Unstressed
	Purity 99%		+/- 0.1800	µg/mL	Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:
 30m x .25mm x .2um
 Rtx-CLP II (cat.# 11323)


Carrier Gas:
 helium-constant pressure 20 psi.

Temp. Program:
 150°C to 300°C
 @ 4°C/min. (hold 5 min.)

Inj. Temp:
 200°C

Det. Temp:
 300°C

Det. Type:
 ECD

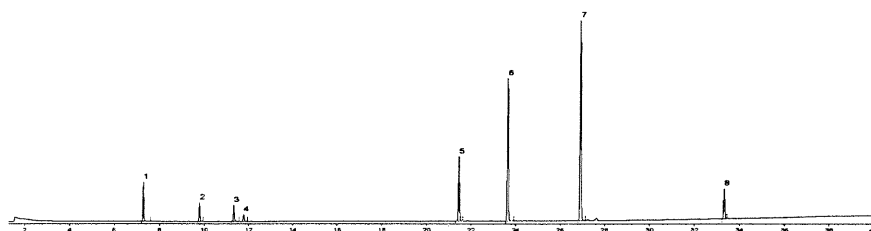

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brittany Federinko
 Brittany Federinko - Operations Tech I

Date Mixed: 22-Mar-2022 **Balance:** 1128360905

John Lidgett
 John Lidgett - AD Chemist

Date Passed: 24-Mar-2022

Manufactured under Restek's ISO 9001:2015
 Registered Quality System
 Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32005 Lot No.: A0177326
Description: Toxaphene Standard
Toxaphene Standard 1000 µg/mL, Hexane, 1mL/ampul
Container Size: 2 mL Pkg Amt: > 1 mL
Expiration Date: January 31, 2026 Storage: 10°C or colder
Ship: Ambient

P11811
✓
P11819
AJ
06/17/22

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Toxaphene	1,004.7 µg/mL	+/- 5.9674 µg/mL Gravimetric
	CAS # 8001-35-2 (Lot 1051817)		+/- 31.8552 µg/mL Unstressed
	Purity ----%		+/- 41.6063 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

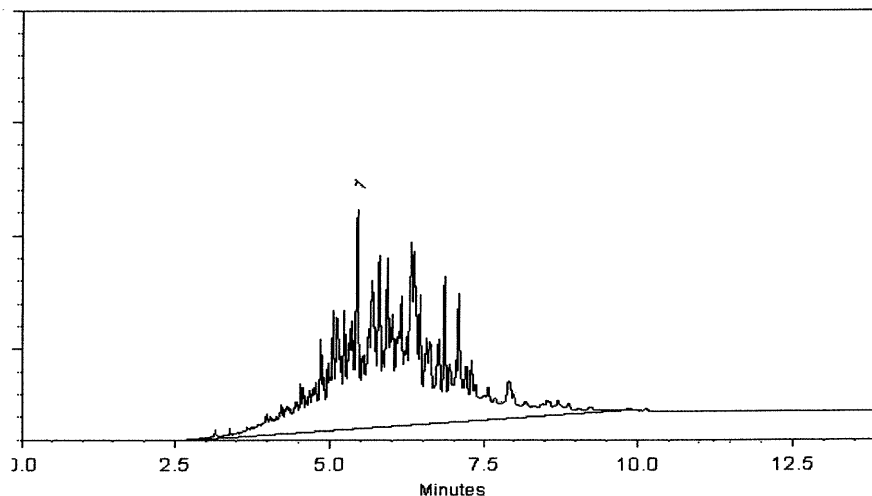

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler

Sam Moodler - Operations Tech I

Date Mixed: 11-Oct-2021

Balance: B442140311

Marlina Cowan

Marlina Cowan - Operations Tech I

Date Passed: 14-Oct-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED WEIGHT REPORT

Part Number: 79136
Lot Number: 030818
Description: Mirex

Expiration Date: 030823
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 2506734D
Weight(s) shown below were combined and diluted to (mL): 100.0

5E-05 Balance Uncertainty
0.057 Flask Uncertainty

Solvent(s): Acetone
Lot# 81025


<i>Gabriel Holland</i>	030818
Formulated By: Gabriel Holland	DATE
<i>Pedro L. Rentas</i>	030818
Reviewed By: Pedro L. Rentas	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty	
									(+/-) (µg/mL)	OSHA PEL (TWA)

1. Mirex 437 7018700 1000 99.5 0.5 0.10051 0.10065 1001.4 10.2 2385-85-5 N/A orl-rat 306mg/kg

Method GC7MSD-1.M: Column: SPB-608 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (4min.), Temp 2 = 290°C (13.5 min.), Rate = 8°C/min., Injector B= 200°C, Detector B = 290°C. Split Ratio = 100:1, Scan Rate = 2. Analysis performed by Candice Warren.

TIC: 79136.D

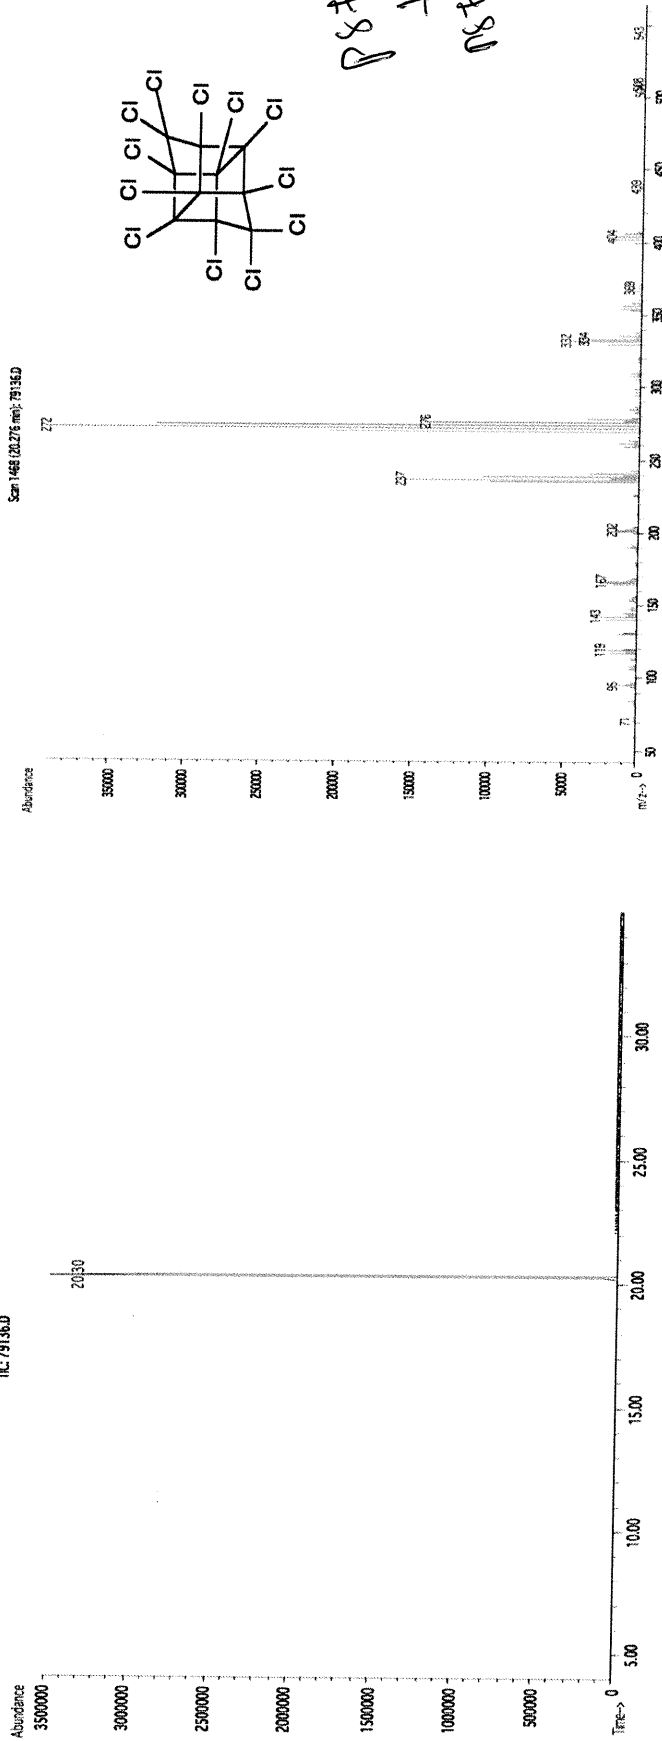


• The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
• Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
• Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
• All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
• Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

**Run 25, "P79136 L030818 [1000µg/mL in Acetone]"**

Run Length: 35.00 min, 21000 points at 10 points/second.
Created: Fri, Mar 9, 2018 at 3:46:52 AM.
Sampled: Sequence "030818-GC3M1", Method "GC3-M1".
Analyzed using Method "GC3-M1".

Comments

GC3-M1 Analysis by Candice Warren
Column ID SPB-608 30 meter X 0.53mm X5µm film thickness
Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
Rate = 8°C/min, Total run time = 35 min
Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
Standard injection = 1.5µL, Range=3

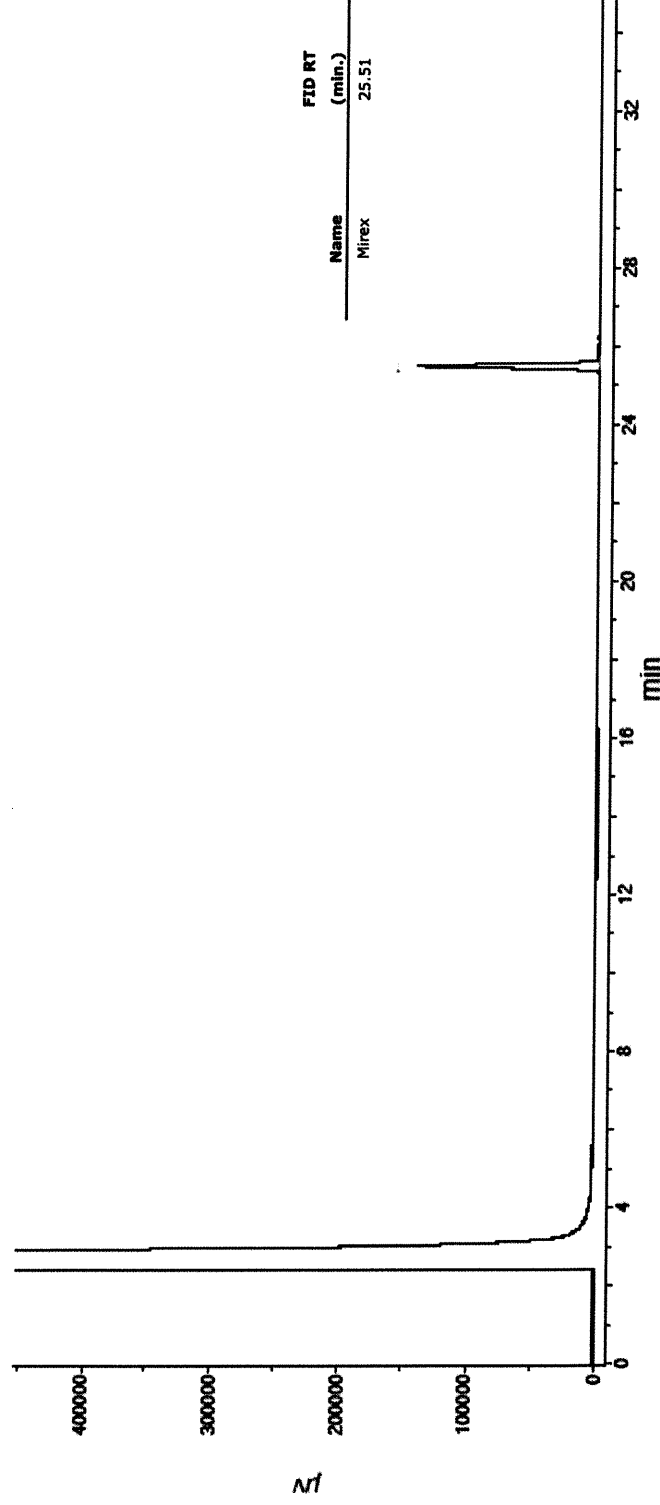



CERTIFIED REFERENCE MATERIAL

110 Benner Circle


Bellefonte, PA 16823-8812

Tel: (800)356-1688

Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32021

Lot No.: A0144623

Description :

Chlordane Standard

Chlordane Standard 1000µg/mL, Hexane, 1mL/ampul

Container Size :

2 mL

Pkg Amt: > 1 mL

Expiration Date :

April 30, 2025

Storage: 10°C or colder

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	Gravimetric
1	Chlordane	1,010.0 µg/mL	+/- 5.9272 µg/mL	Unstressed
	CAS # 57-74-9		+/- 32.0109 µg/mL	Stressed
	Purity ----%		+/- 41.8169 µg/mL	
	(Lot 142990)			
Solvent:	Hexane			
	CAS # 110-54-3			
	Purity 99%			

88742



88744

SM

7/30/19

Tech Tips:

CAS #57-74-9 nomenclature is based on EPA method 8081B.

Column:

30m x .25mm x 2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

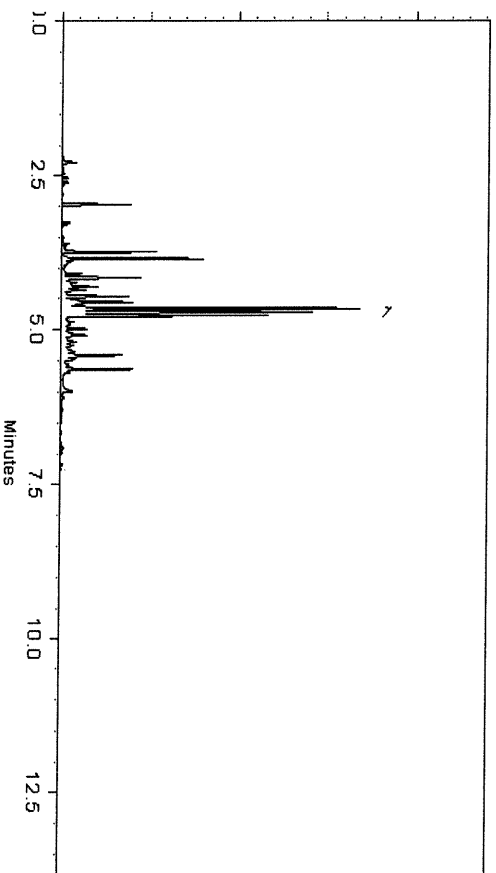

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Maggie Wang

Maggie Wang - Operations Technician I


Date Mixed: 04-Jan-2019

Balance: B251644995

Jennifer J Pollino
Jennifer Pollino - Operations Tech-ARM QC

Date Passed: 09-Jan-2019

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



Certified Reference Material CRM



P9644, P9645, P9646, P9647, P9648

Received by: SI 6/19/2020

CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

79136
061820
Mirex

Solvent(s):
Acetone

Lot#
81025

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

061825
Refrigerate (4 °C)
1000
23060

5E-05 Balance Uncertainty
0.001 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL):

50.0

Formulated By:

Benson Chan

061820

Reviewed By:

Pedro L. Rentas

061820

Expanded Uncertainty
(+/-) (µg/mL)
Actual Conc (µg/mL)
Actual Weight (g)
Target Weight (g)
Purity
Uncertainty
(%)
Nominal Conc (µg/mL)
Lot Number
RM#

10.3
1000.0
0.05030
0.05030
0.5
99.4
1000
9492400
437

Compound
Mirex
Method GC7MSD-1.M: Column: SPB-608 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (4min.), Temp 2 = 290°C (13.5 min.), Rate = 8°C/min., Injector B= 200°C, Detector B = 290°C. Split Ratio = 100:1, Scan Rate = 2. Analysis performed by Candice Warren.

orl-rat 306mg/kg

N/A

2385-85-5


OSHA PEL (TWA)

CAS#

LD50

TC: 79136.D

Scan 1468 (20.276 min): 79136.D

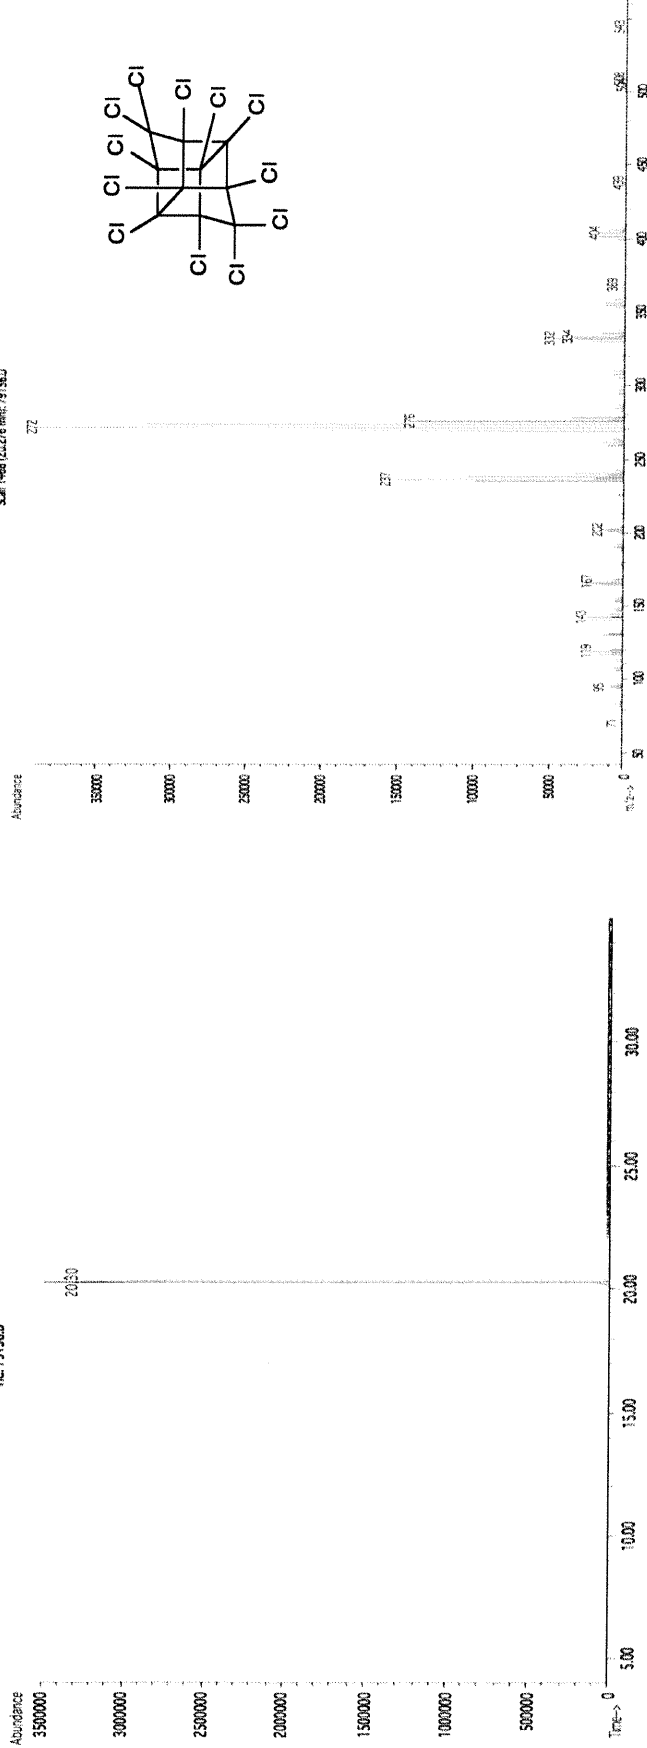

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32291 **Lot No.:** A0154466

Description : Organochlorine Pesticide Mix AB #1

Organochlorine Pesticide Mix AB #1 200µg/mL, Hexane/Toluene(50:50), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : October 31, 2023 **Storage:** 10°C or colder

P9649 P9654
P9650 P9655
P9651 P9656
P9652 P9657
P9653 P9658

SJ 6/22/2020

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	alpha-BHC CAS # 319-84-6 (Lot 0012018BHC) Purity 99%	201.6 µg/mL	+/- 1.1974 µg/mL Gravimetric +/- 9.1846 µg/mL Unstressed +/- 13.2599 µg/mL Stressed
2	gamma-BHC (Lindane) CAS # 58-89-9 (Lot 8521900) Purity 99%	201.6 µg/mL	+/- 1.1974 µg/mL Gravimetric +/- 9.1846 µg/mL Unstressed +/- 13.2599 µg/mL Stressed
3	beta-BHC CAS # 319-85-7 (Lot BCBS8692V) Purity 99%	200.0 µg/mL	+/- 1.1879 µg/mL Gravimetric +/- 9.1117 µg/mL Unstressed +/- 13.1547 µg/mL Stressed
4	delta-BHC CAS # 319-86-8 (Lot ER02101401) Purity 99%	200.0 µg/mL	+/- 1.1879 µg/mL Gravimetric +/- 9.1117 µg/mL Unstressed +/- 13.1547 µg/mL Stressed
5	Heptachlor CAS # 76-44-8 (Lot 0006467453) Purity 98%	200.3 µg/mL	+/- 1.1898 µg/mL Gravimetric +/- 9.1259 µg/mL Unstressed +/- 13.1752 µg/mL Stressed
6	Aldrin CAS # 309-00-2 (Lot 8737100) Purity 96%	200.1 µg/mL	+/- 1.1883 µg/mL Gravimetric +/- 9.1146 µg/mL Unstressed +/- 13.1589 µg/mL Stressed
7	Heptachlor epoxide (isomer B) CAS # 1024-57-3 (Lot 8666700) Purity 99%	200.0 µg/mL	+/- 1.1879 µg/mL Gravimetric +/- 9.1117 µg/mL Unstressed +/- 13.1547 µg/mL Stressed

8	trans-Chlordane			201.2	µg/mL	+/-	1.1951	µg/mL	Gravimetric
	CAS #	5103-74-2	(Lot ER06190604)			+/-	9.1664	µg/mL	Unstressed
	Purity	99%				+/-	13.2336	µg/mL	Stressed
9	cis-Chlordane			201.2	µg/mL	+/-	1.1951	µg/mL	Gravimetric
	CAS #	5103-71-9	(Lot 24407)			+/-	9.1664	µg/mL	Unstressed
	Purity	99%				+/-	13.2336	µg/mL	Stressed
10	Endosulfan I			202.0	µg/mL	+/-	1.1998	µg/mL	Gravimetric
	CAS #	959-98-8	(Lot BCBS8631)			+/-	9.2028	µg/mL	Unstressed
	Purity	99%				+/-	13.2862	µg/mL	Stressed
11	4,4'-DDE			200.8	µg/mL	+/-	1.1927	µg/mL	Gravimetric
	CAS #	72-55-9	(Lot GHYQG)			+/-	9.1481	µg/mL	Unstressed
	Purity	99%				+/-	13.2073	µg/mL	Stressed
12	Dieldrin			200.4	µg/mL	+/-	1.1903	µg/mL	Gravimetric
	CAS #	60-57-1	(Lot 8815700)			+/-	9.1299	µg/mL	Unstressed
	Purity	99%				+/-	13.1810	µg/mL	Stressed
13	Endrin			200.8	µg/mL	+/-	1.1927	µg/mL	Gravimetric
	CAS #	72-20-8	(Lot 8532900)			+/-	9.1481	µg/mL	Unstressed
	Purity	99%				+/-	13.2073	µg/mL	Stressed
14	4,4'-DDD			201.2	µg/mL	+/-	1.1951	µg/mL	Gravimetric
	CAS #	72-54-8	(Lot HAN02)			+/-	9.1664	µg/mL	Unstressed
	Purity	99%				+/-	13.2336	µg/mL	Stressed
15	Endosulfan II			200.0	µg/mL	+/-	1.1879	µg/mL	Gravimetric
	CAS #	33213-65-9	(Lot 8679900)			+/-	9.1117	µg/mL	Unstressed
	Purity	99%				+/-	13.1547	µg/mL	Stressed
16	4,4'-DDT			201.2	µg/mL	+/-	1.1951	µg/mL	Gravimetric
	CAS #	50-29-3	(Lot S37912V)			+/-	9.1664	µg/mL	Unstressed
	Purity	99%				+/-	13.2336	µg/mL	Stressed
17	Endrin aldehyde			200.8	µg/mL	+/-	1.1927	µg/mL	Gravimetric
	CAS #	7421-93-4	(Lot 30720)			+/-	9.1481	µg/mL	Unstressed
	Purity	99%				+/-	13.2073	µg/mL	Stressed
18	Endosulfan sulfate			202.0	µg/mL	+/-	1.1998	µg/mL	Gravimetric
	CAS #	1031-07-8	(Lot BCCB0424)			+/-	9.2028	µg/mL	Unstressed
	Purity	99%				+/-	13.2862	µg/mL	Stressed
19	Methoxychlor			200.4	µg/mL	+/-	1.1903	µg/mL	Gravimetric
	CAS #	72-43-5	(Lot 9013400)			+/-	9.1299	µg/mL	Unstressed
	Purity	99%				+/-	13.1810	µg/mL	Stressed
20	Endrin ketone			200.4	µg/mL	+/-	1.1903	µg/mL	Gravimetric
	CAS #	53494-70-5	(Lot 8618200)			+/-	9.1299	µg/mL	Unstressed
	Purity	99%				+/-	13.1810	µg/mL	Stressed
Solvent: Hexane/Toluene (50:50)									
	CAS #	110-54-3/108-88-3							
	Purity	99%							

Column:

3 x .25mm x .2um
CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

150°C to 300°C
@ 4°C/min. (hold 5 min.)

Inj. Temp:


200°C

Det. Temp:


300°C

Det. Type:

ECD

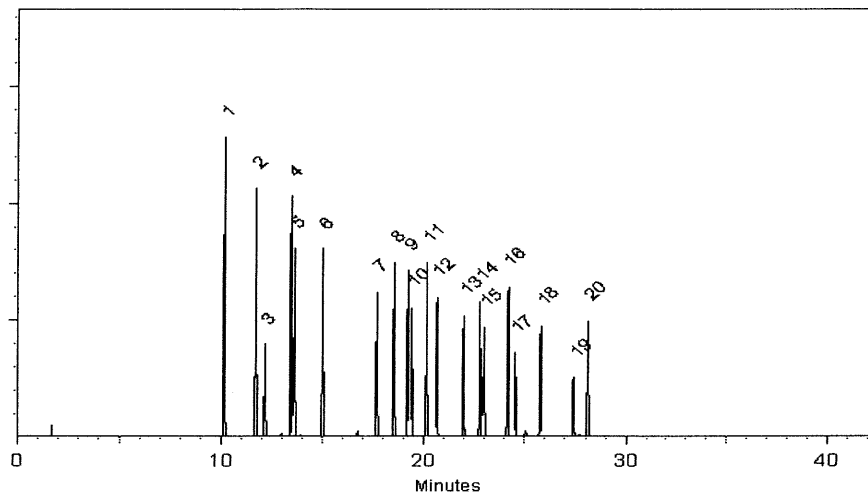

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Walker Workman - Operations Technician I

Date Mixed: 29-Oct-2019

Balance: 1128353505

Date Passed: 05-Nov-2019

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent



Material No.: 9262-03

Batch No.: 22B0762004

Manufactured Date: 2021-11-24

Expiration Date: 2023-02-23

Revision No.: 0

Certificate of Analysis

W2938
onatel
07/25/2022
JP

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	< 1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	< 0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD
Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent



Material No.: 9262-03

Batch No.: 22B0762004

Manufactured Date: 2021-11-24

Expiration Date: 2023-02-23

Revision No.: 0

Certificate of Analysis

W2938
onatel
07/25/2022
JP

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	< 1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	< 0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD
Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700