


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012423\
 Data File : BP013561.D
 Acq On : 24 Jan 2023 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 25 03:43:27 2023

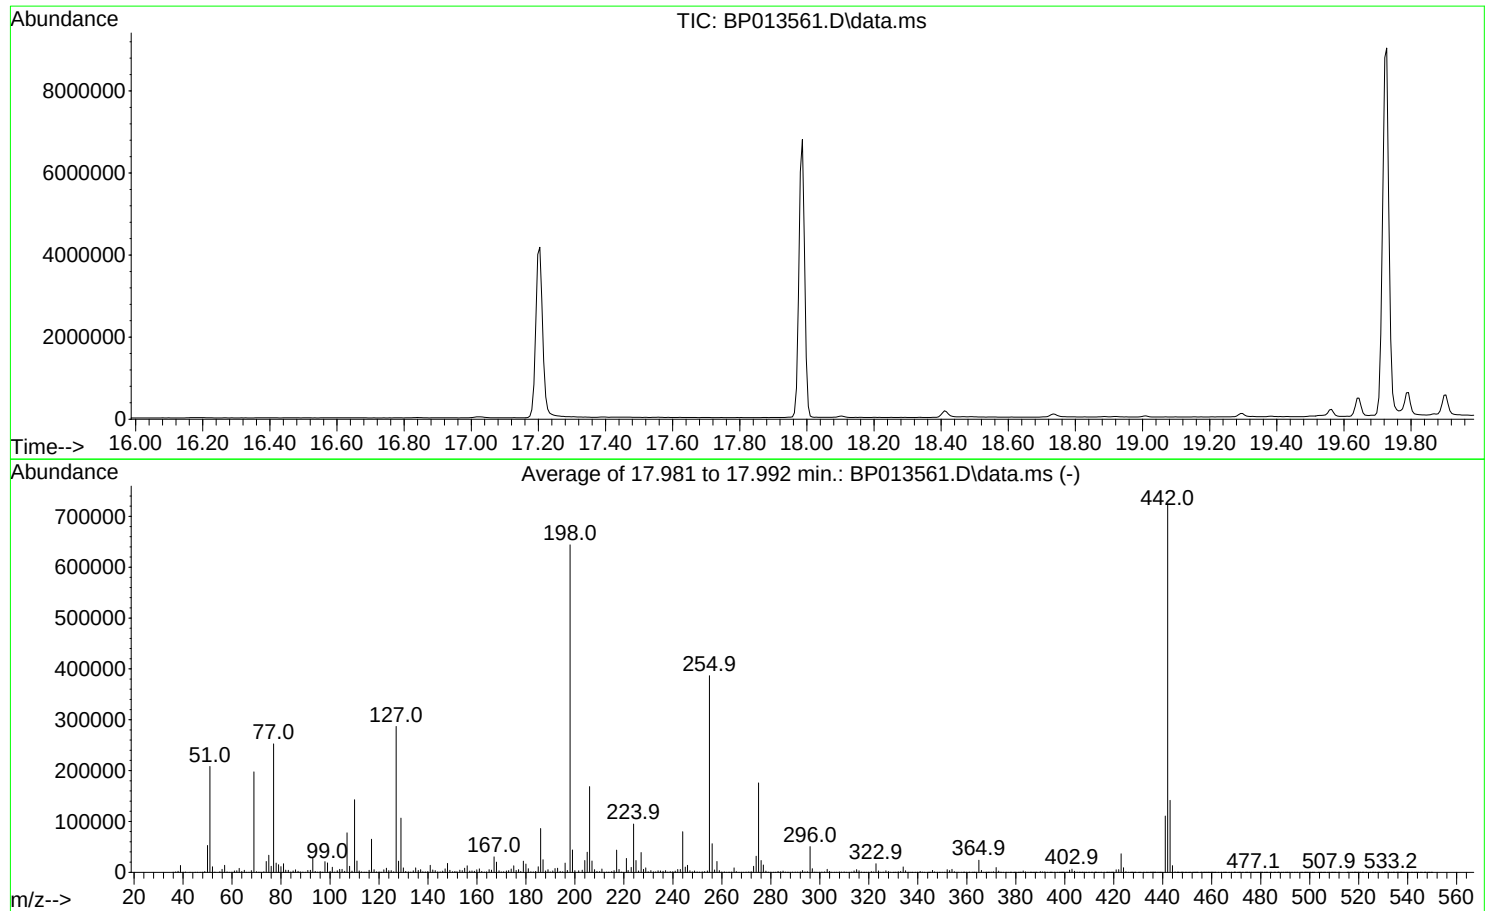




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	208032	PASS
68	69	0.00	2	1.6	3176	PASS
69	198	0.00	100	30.6	197329	PASS
70	69	0.00	2	0.5	1025	PASS
127	198	10	80	44.6	286997	PASS
197	198	0.00	2	0.5	3516	PASS
198	198	100	100	100.0	643968	PASS
199	198	5	9	6.8	43992	PASS
275	198	10	60	27.3	175787	PASS
365	198	1	100	3.7	23755	PASS
441	198	0.01	100	17.2	110696	PASS
442	442	100	100	100.0	723465	PASS
443	442	15	24	19.5	141424	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012423\
 Data File : BP013561.D
 Acq On : 24 Jan 2023 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 25 05:54:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 25 03:43:27 2023
 Response via : Initial Calibration

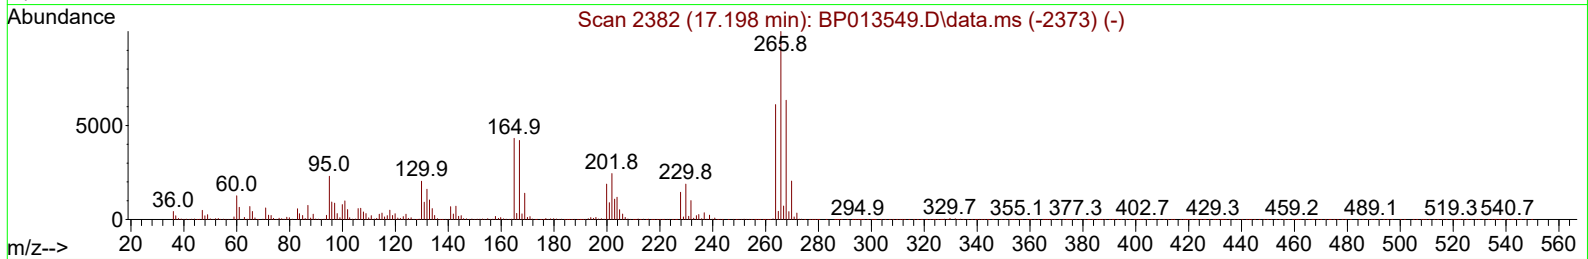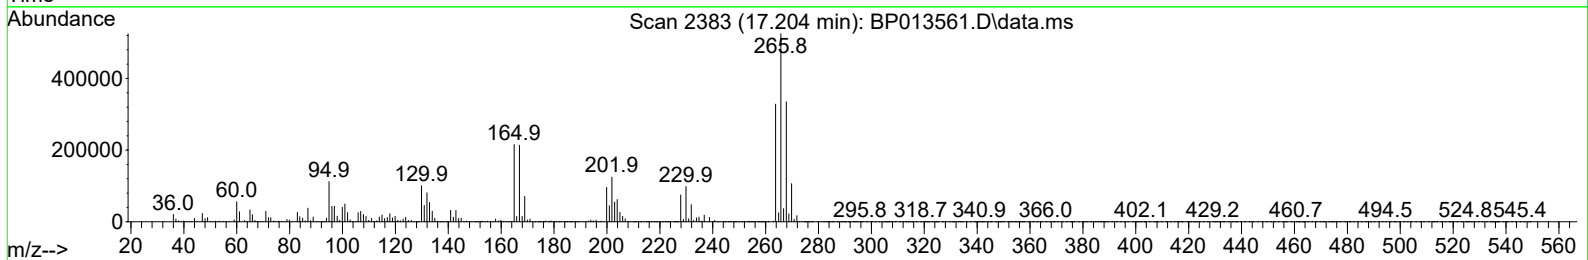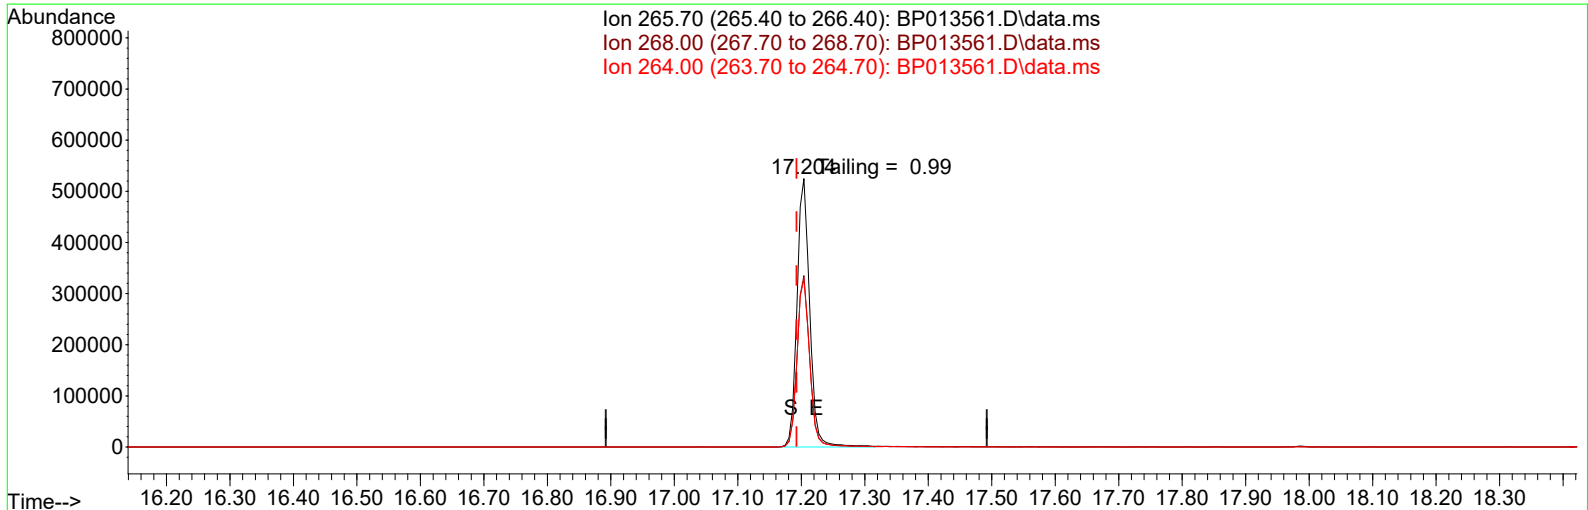

TIC: BP013561.D\data.ms

(70) Pentachlorophenol (C)

17.204min (+ 0.012) 507480.60 ng




response 738098

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	63.85
264.00	61.10	62.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012423\
 Data File : BP013561.D
 Acq On : 24 Jan 2023 09:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 25 05:54:27 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 25 03:43:27 2023
 Response via : Initial Calibration

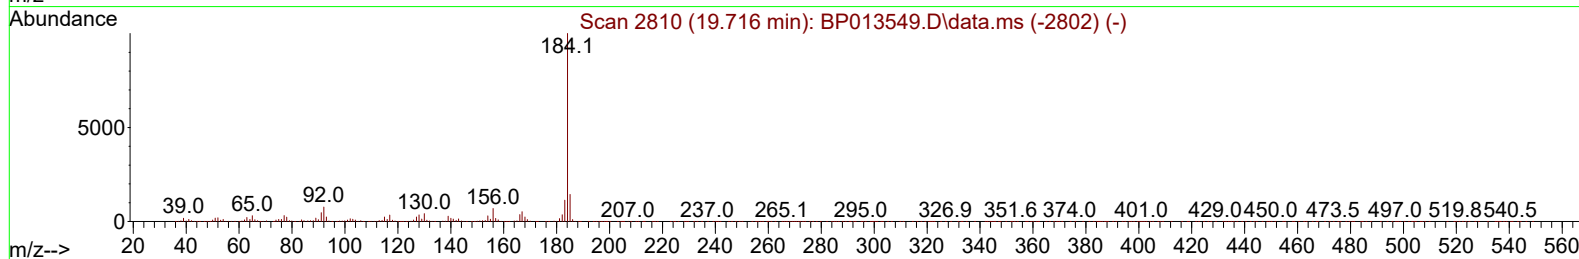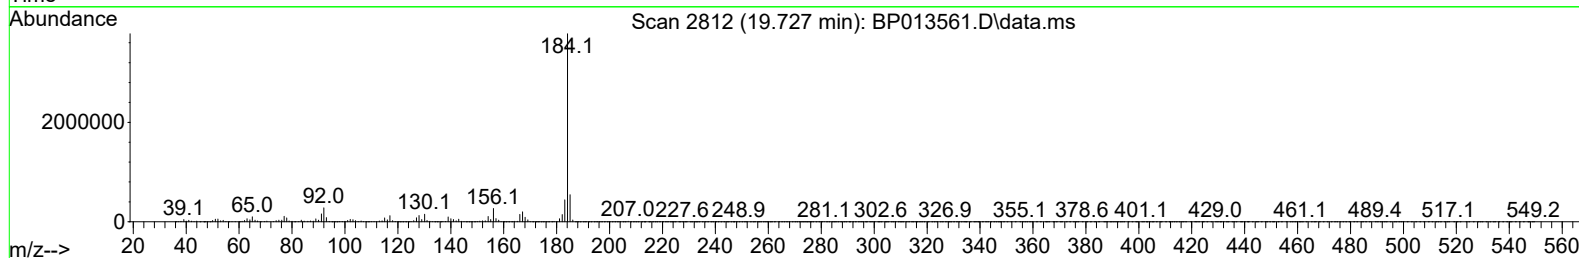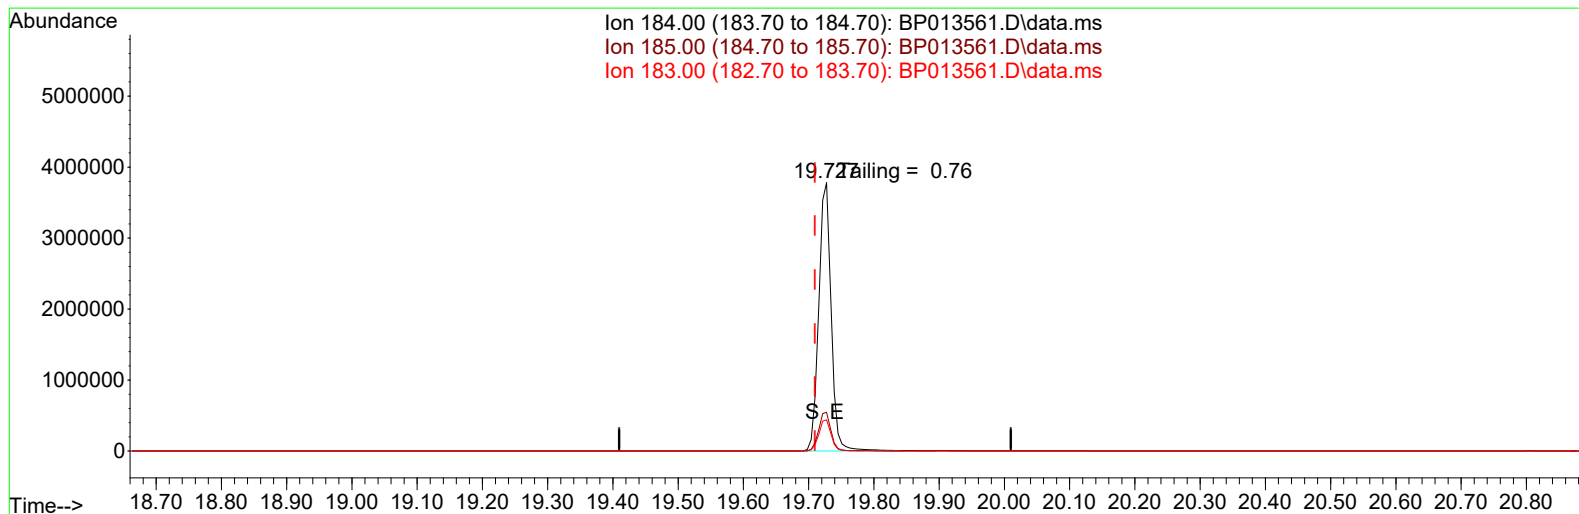

TIC: BP013561.D\data.ms

(77) Benzidine

19.727min (+ 0.017) 12021.93 ng

response 5000716

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.42
183.00	11.30	11.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/24/2023	BNA_P	<u>BP013561.D</u>
Compound Name	Response	Retention Time
DDT	2051182	20.922
DDD	26353	20.545
DDE	1510	19.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27863	2079045	1.34

Instrument :
BNA_P
ClientSampleId :
DFTPP