


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012423\
Data File : BP013570.D
Acq On : 24 Jan 2023 14:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 25 03:43:27 2023

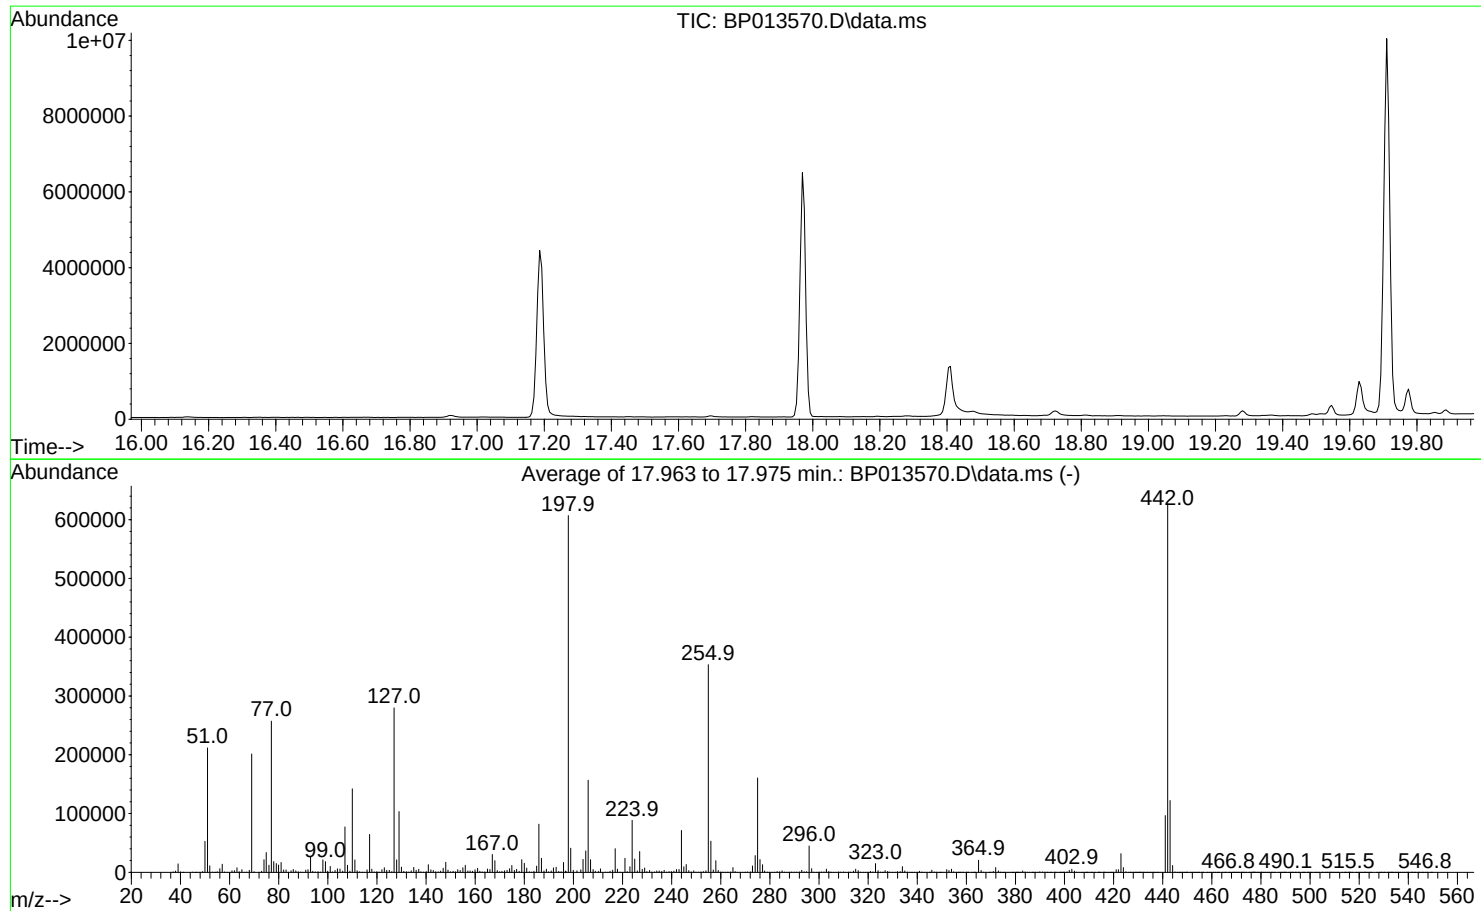




AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2502

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	211597	PASS
68	69	0.00	2	1.7	3424	PASS
69	198	0.00	100	33.2	201447	PASS
70	69	0.00	2	0.5	1018	PASS
127	198	10	80	46.1	279631	PASS
197	198	0.00	2	0.4	2190	PASS
198	198	100	100	100.0	607125	PASS
199	198	5	9	6.8	41023	PASS
275	198	10	60	26.4	160504	PASS
365	198	1	100	3.4	20609	PASS
441	198	0.01	100	15.9	96521	PASS
442	442	100	100	100.0	625920	PASS
443	442	15	24	19.5	122139	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012423\
 Data File : BP013570.D
 Acq On : 24 Jan 2023 14:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jan 25 05:55:48 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 25 03:43:27 2023
 Response via : Initial Calibration

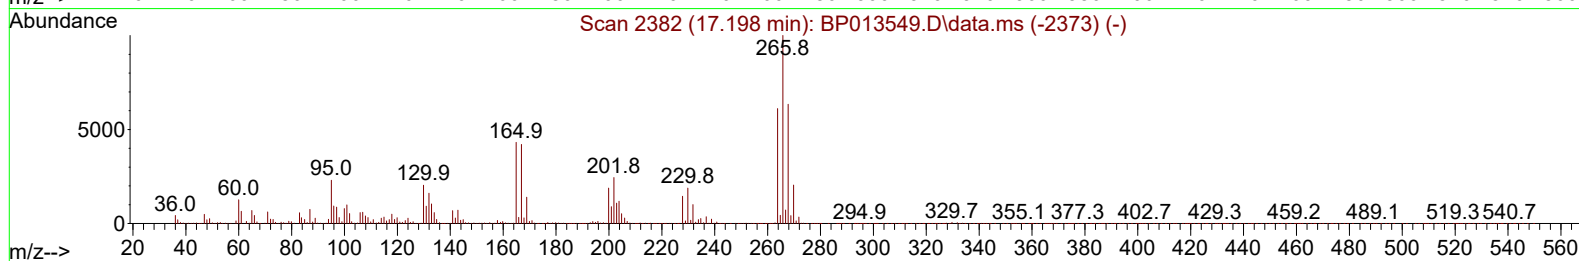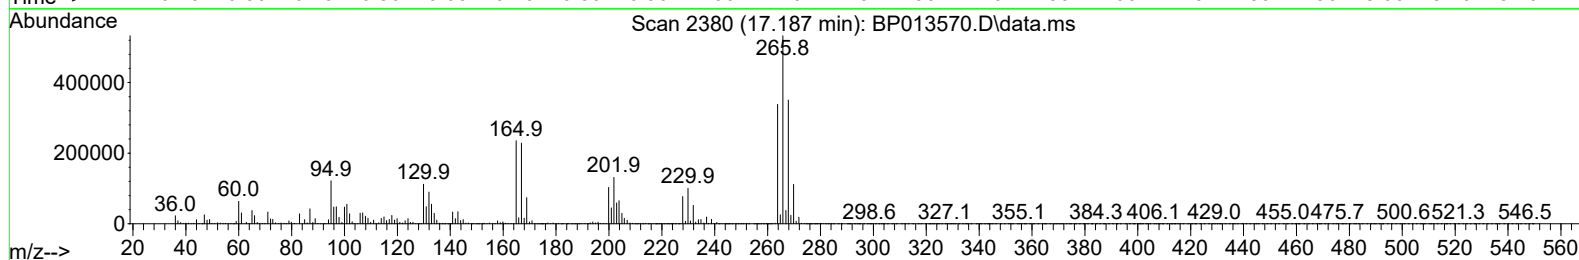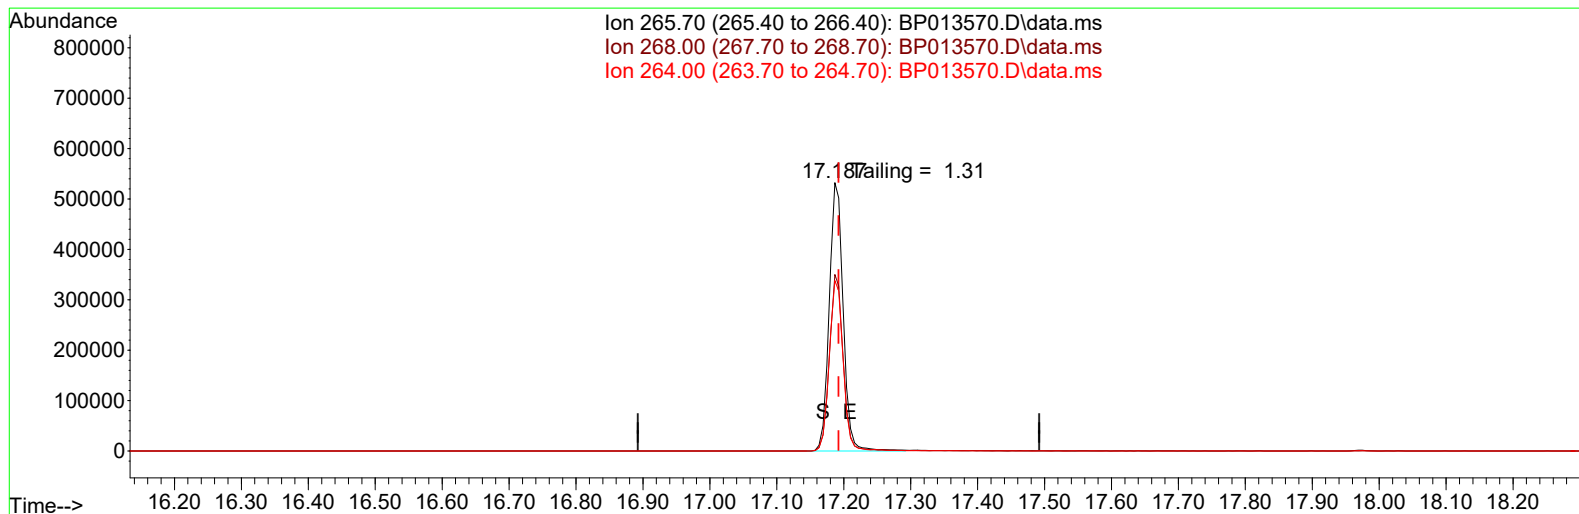

TIC: BP013570.D\data.ms

(70) Pentachlorophenol (C)

17.187min (-0.006) 3605533.60 ng




response 771186

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	65.77
264.00	61.10	63.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012423\
Data File : BP013570.D
Acq On : 24 Jan 2023 14:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 25 05:55:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 25 03:43:27 2023
Response via : Initial Calibration

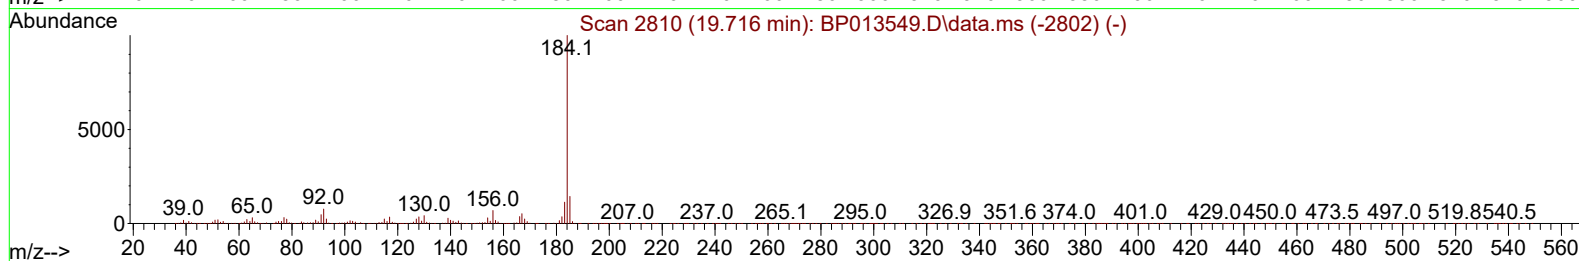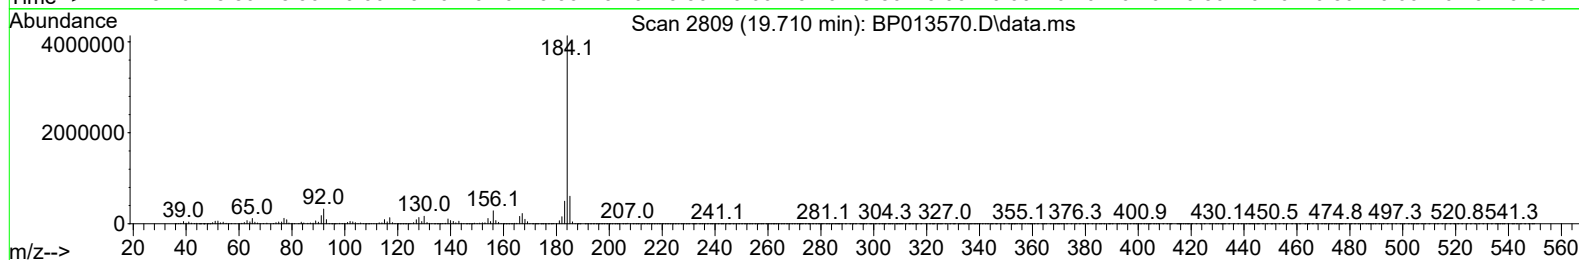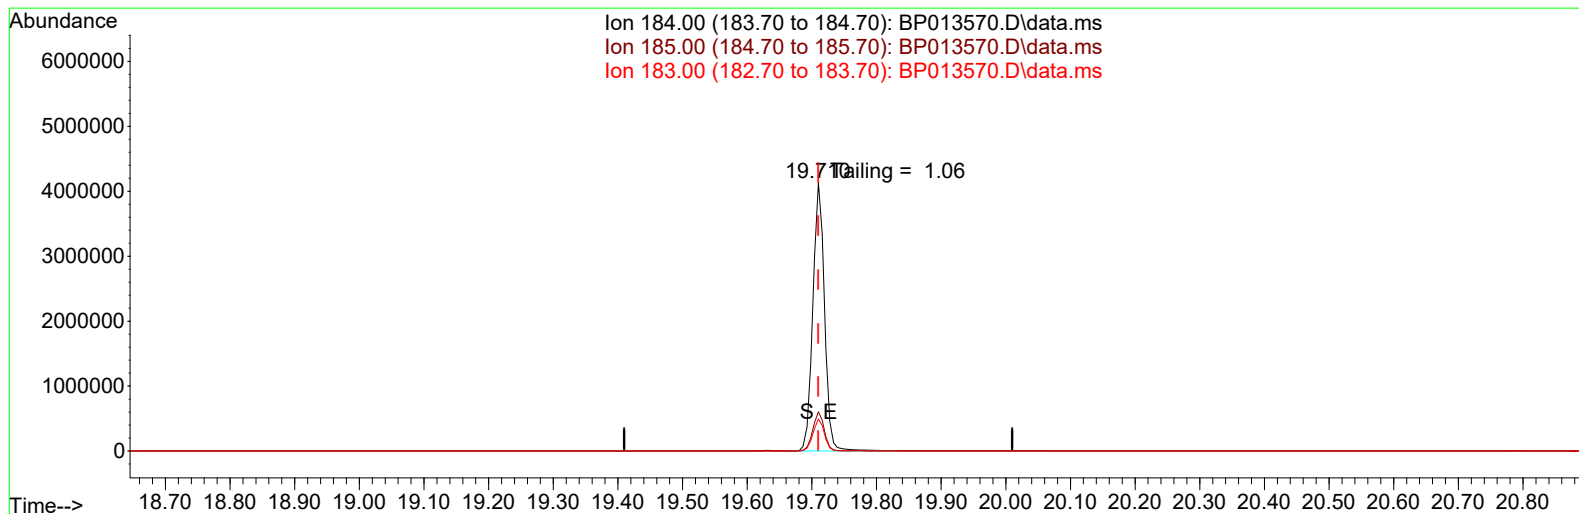

TIC: BP013570.D\data.ms

(77) Benzidine

19.710min (-0.000) 7395893.28 ng

response 5208315

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.60
183.00	11.30	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/24/2023	BNA_P	<u>BP013570.D</u>
Compound Name	Response	Retention Time
DDT	2182546	20.91
DDD	31504	20.533
DDE	1321	19.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
32825	2215371	1.48

Instrument :
BNA_P
ClientSampleId :
DFTPP