
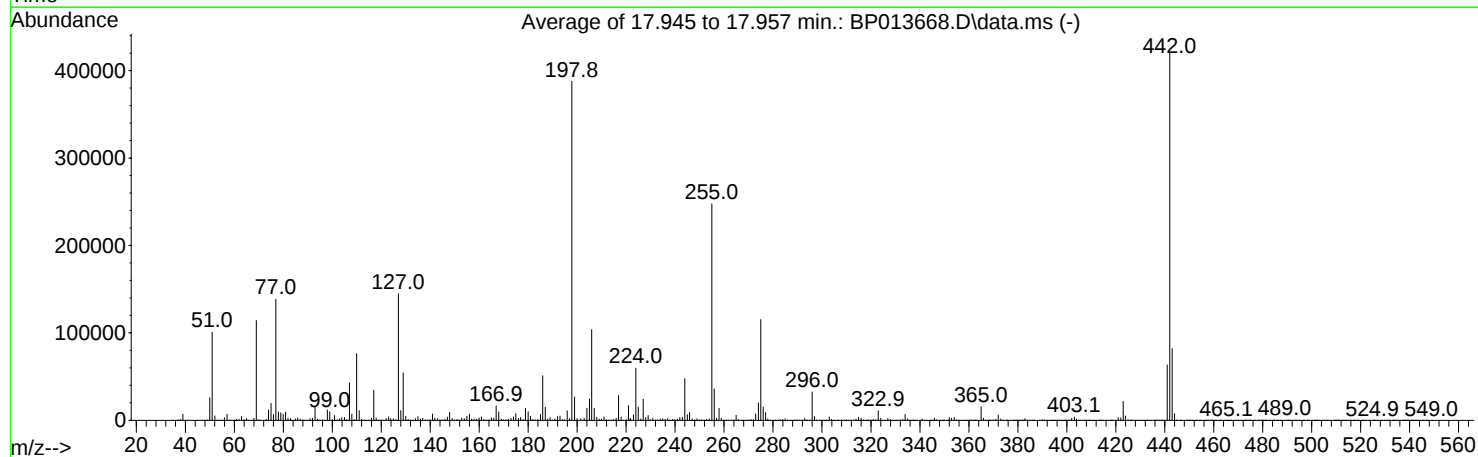


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP013123\  
Data File : BP013668.D  
Acq On : 31 Jan 2023 10:47  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP013123.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Feb 01 03:43:48 2023

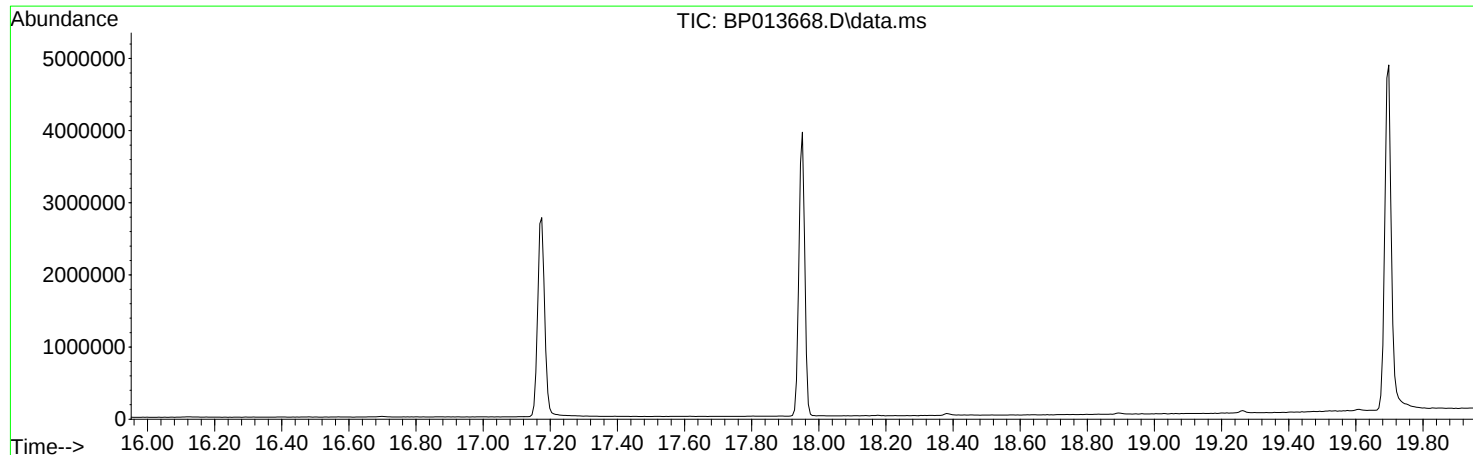




AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2500

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 26.0         | 100852     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 2052       | PASS                |
| 69             | 198             | 0.00            | 100             | 29.4         | 114090     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.6          | 711        | PASS                |
| 127            | 198             | 10              | 80              | 37.3         | 144733     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 1900       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 387796     | PASS                |
| 199            | 198             | 5               | 9               | 6.8          | 26563      | PASS                |
| 275            | 198             | 10              | 60              | 29.7         | 115181     | PASS                |
| 365            | 198             | 1               | 100             | 4.0          | 15400      | PASS                |
| 441            | 198             | 0.01            | 100             | 16.4         | 63451      | PASS                |
| 442            | 442             | 100             | 100             | 100.0        | 420821     | PASS                |
| 443            | 442             | 15              | 24              | 19.5         | 81981      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP013123\  
Data File : BP013668.D  
Acq On : 31 Jan 2023 10:47  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Feb 01 08:00:16 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP013123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Feb 01 03:43:48 2023  
Response via : Initial Calibration

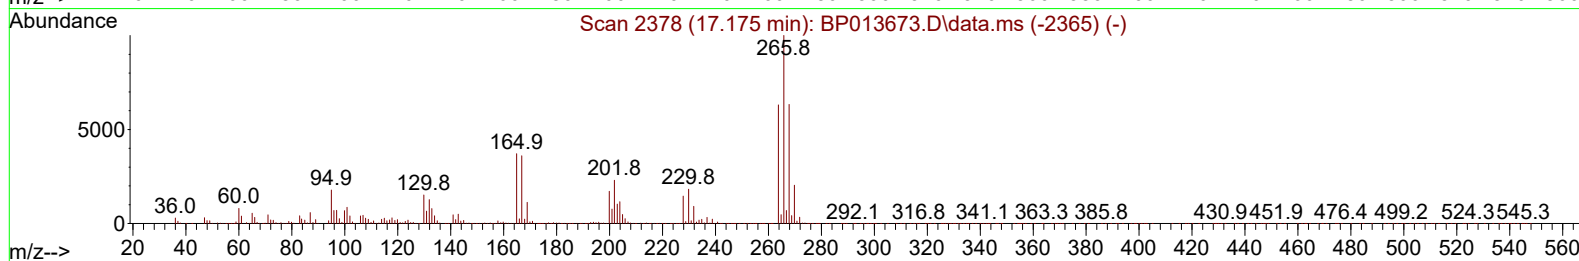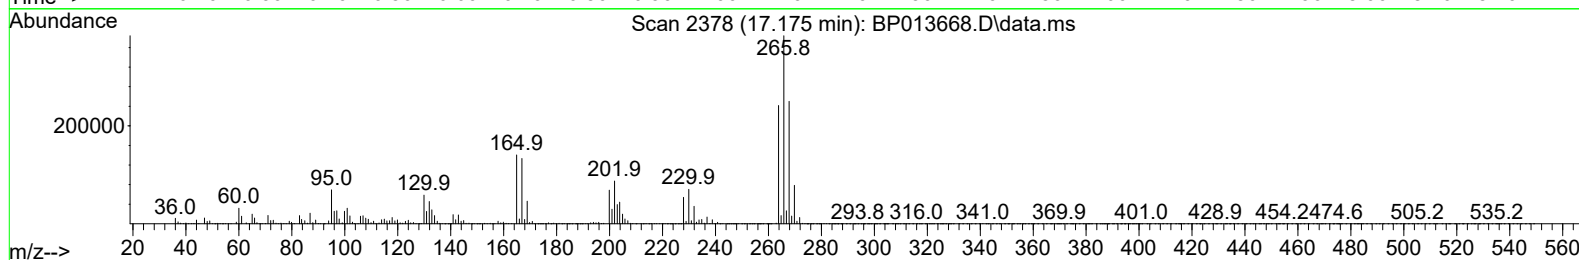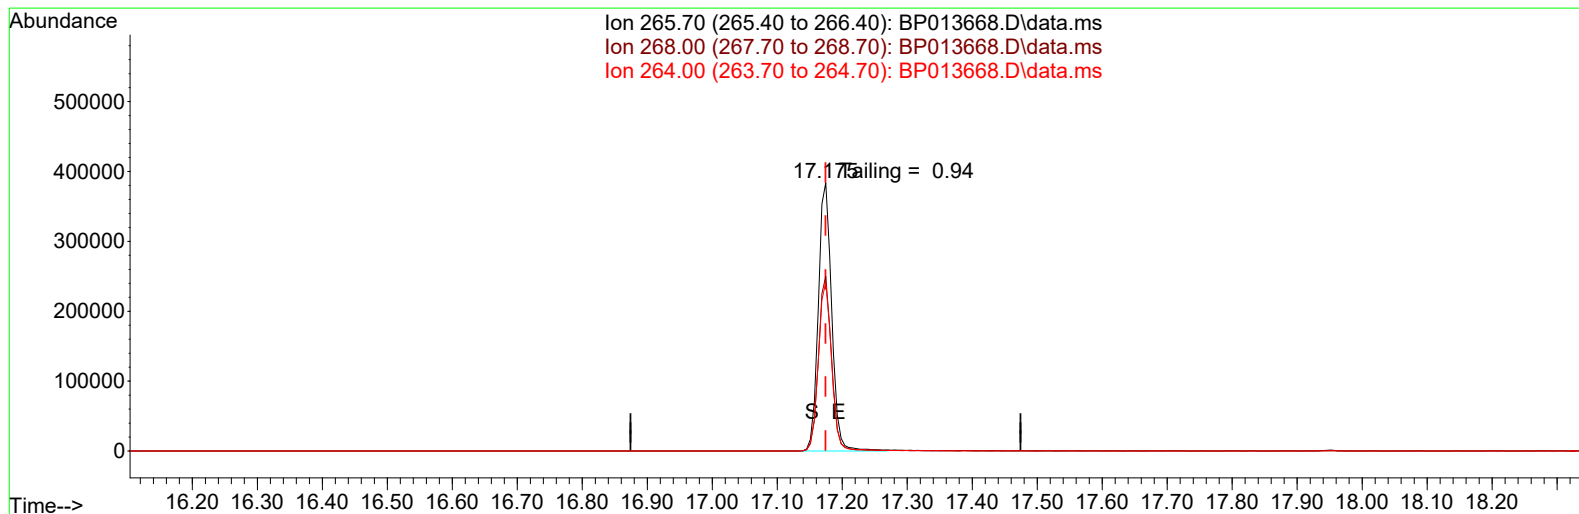

TIC: BP013668.D\data.ms

**(70) Pentachlorophenol (C)**

17.175min (+ 0.000) 2464284.36 ng




response 553780

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.40  | 65.07  |
| 264.00 | 63.10  | 62.91  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP013123\  
Data File : BP013668.D  
Acq On : 31 Jan 2023 10:47  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP

Quant Time: Feb 01 08:00:16 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP013123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Feb 01 03:43:48 2023  
Response via : Initial Calibration

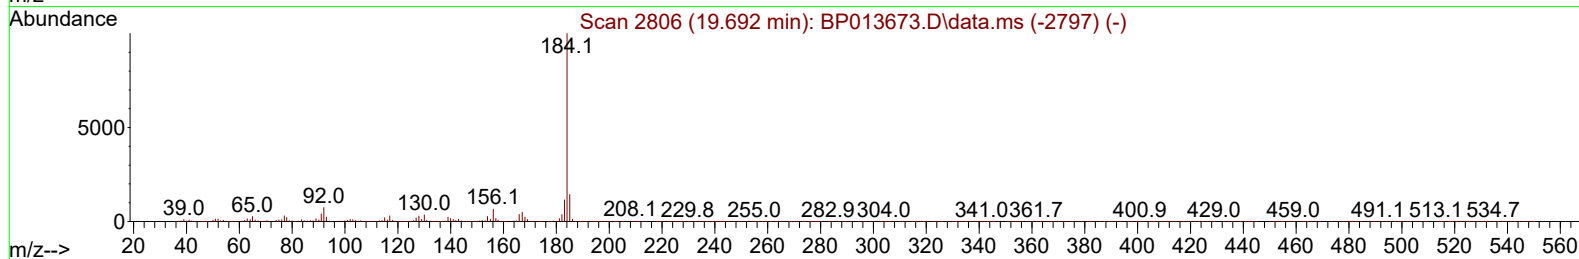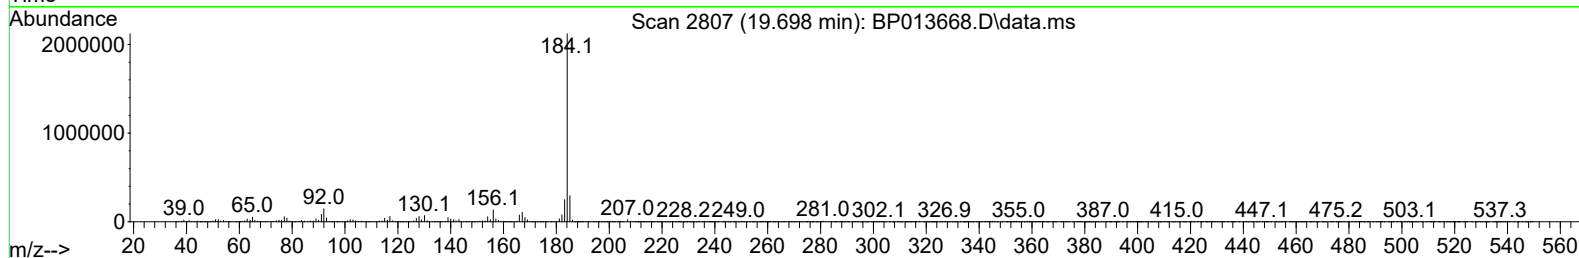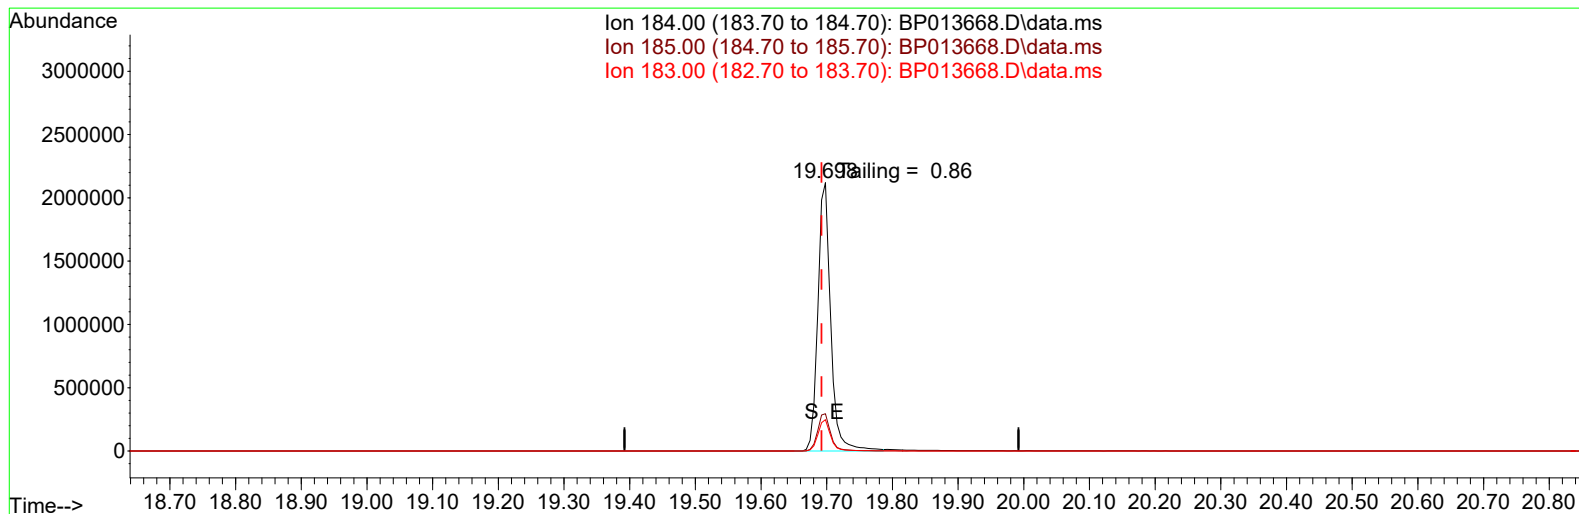

TIC: BP013668.D\data.ms

(77) Benzidine

19.698min (+ 0.006) 2755273.69 ng

response 2916120

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.30  | 13.90  |
| 183.00 | 11.50  | 11.72  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 1/31/2023     | BNA_P            | <u>BP013668.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1142397          | 20.892             |
| DDD           | 9738             | 20.516             |
| DDE           | 557              | 19.969             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 10295         | 1152692          | 0.89               |
|               |                  |                    |

Instrument :  
BNA\_P  
ClientSampleId :  
DFTPP