
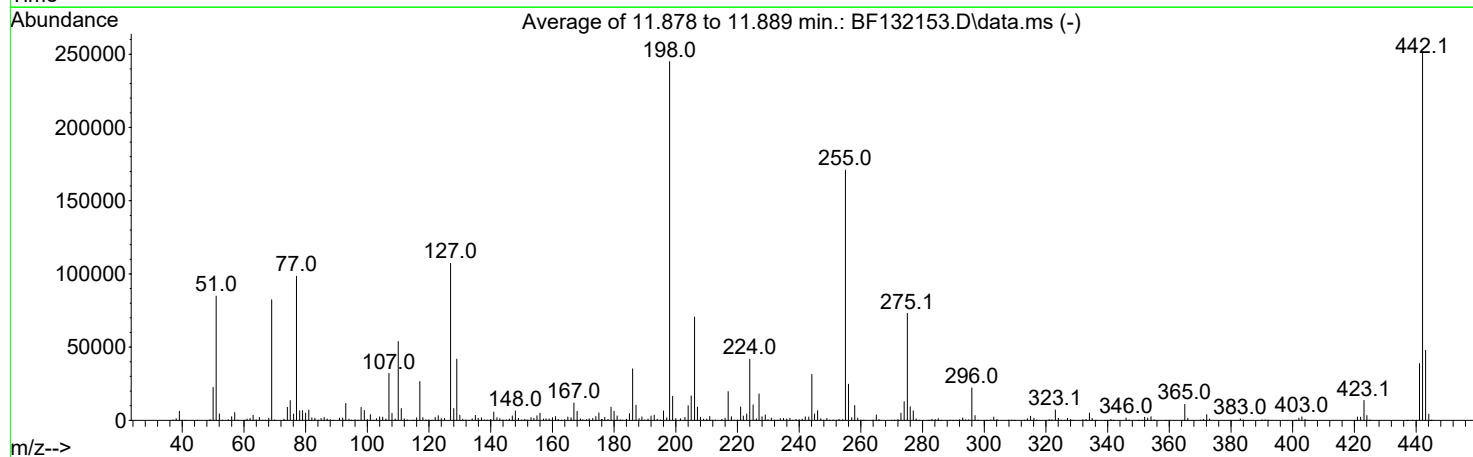


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012023\
Data File : BF132153.D
Acq On : 20 Jan 2023 09:28
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 20 00:50:42 2023

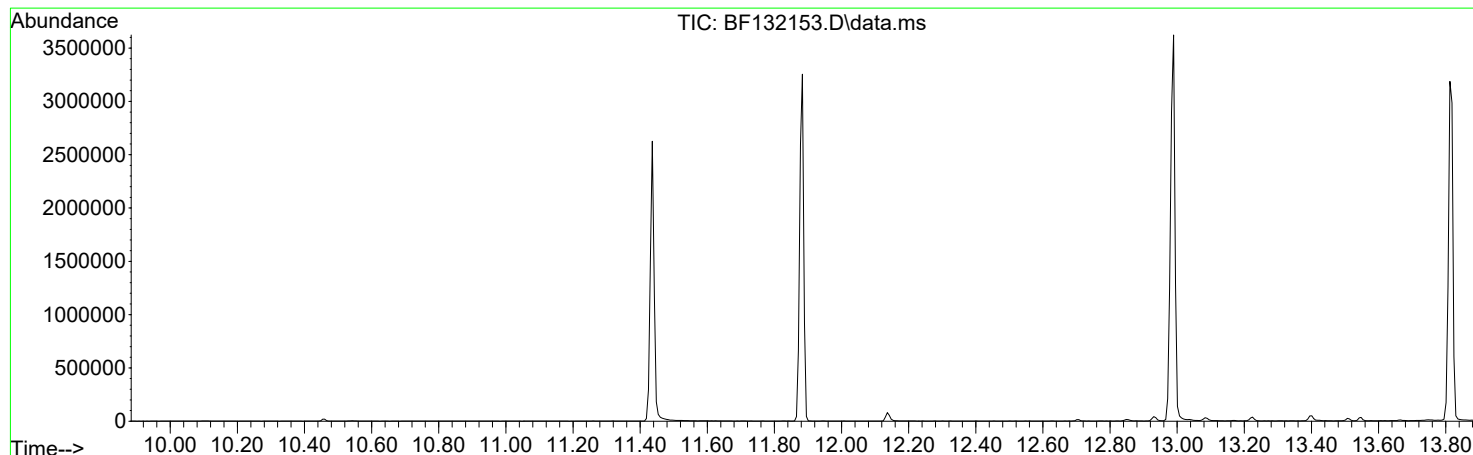

AutoFind: Scans 1537, 1538, 1539; Background Corrected with Scan 1532

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	34.7	84945	PASS
68	69	0.00	2	1.8	1506	PASS
69	198	0.00	100	33.6	82360	PASS
70	69	0.00	2	0.4	361	PASS
127	198	10	80	43.8	107208	PASS
197	198	0.00	2	0.7	1770	PASS
198	198	100	100	100.0	244979	PASS
199	198	5	9	6.7	16375	PASS
275	198	10	60	29.8	73059	PASS
365	198	1	100	4.5	10967	PASS
441	198	0.01	100	15.9	38843	PASS
442	442	50	100	100.0	251179	PASS
443	442	15	24	19.1	47917	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/20/2023	BNA_F	<u>BF132153.D</u>
Compound Name	Response	Retention Time
DDT	532910	13.819
DDD	8362	13.548
DDE	646	13.172
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9008	541918	1.66

Instrument :
BNA_F
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012023\  
Data File : BF132153.D  
Acq On    : 20 Jan 2023  09:28  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 21 05:30:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 20 00:50:42 2023
Response via : Initial Calibration

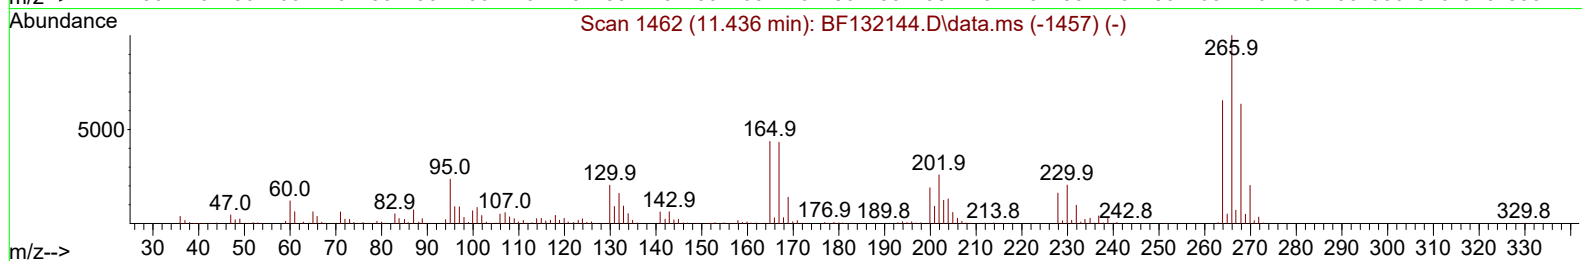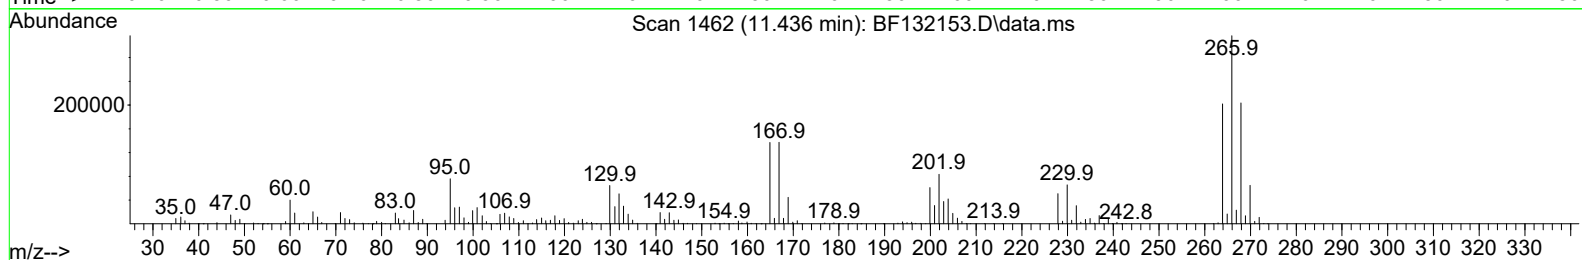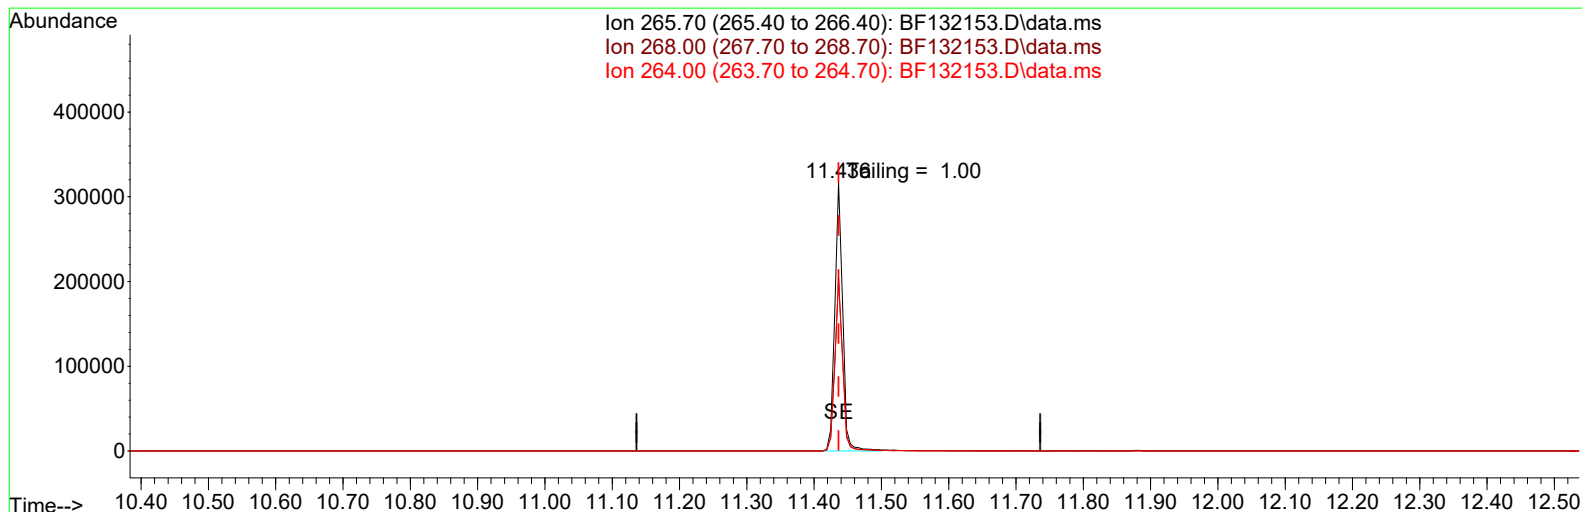

TIC: BF132153.D\data.ms

(70) Pentachlorophenol (C)

11.436min (+ 0.000) 81291.37 ng




response 258825

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	64.30
264.00	65.40	63.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012023\
 Data File : BF132153.D
 Acq On : 20 Jan 2023 09:28
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jan 21 05:30:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jan 20 00:50:42 2023
 Response via : Initial Calibration

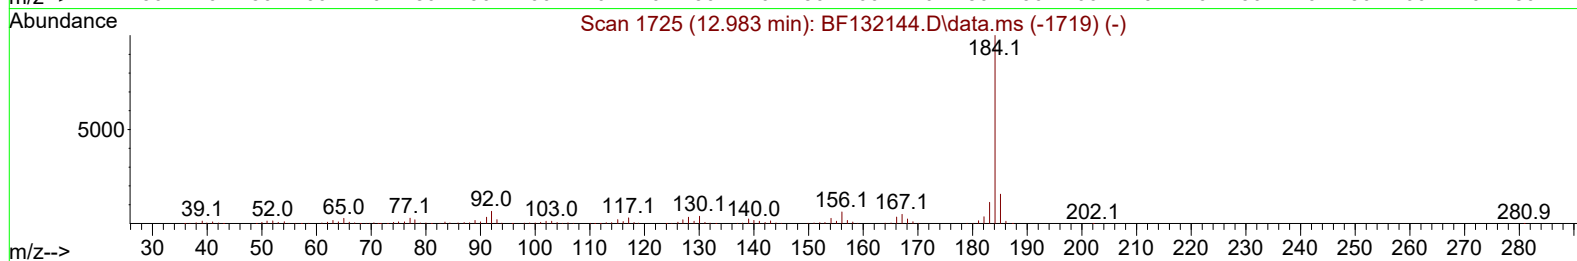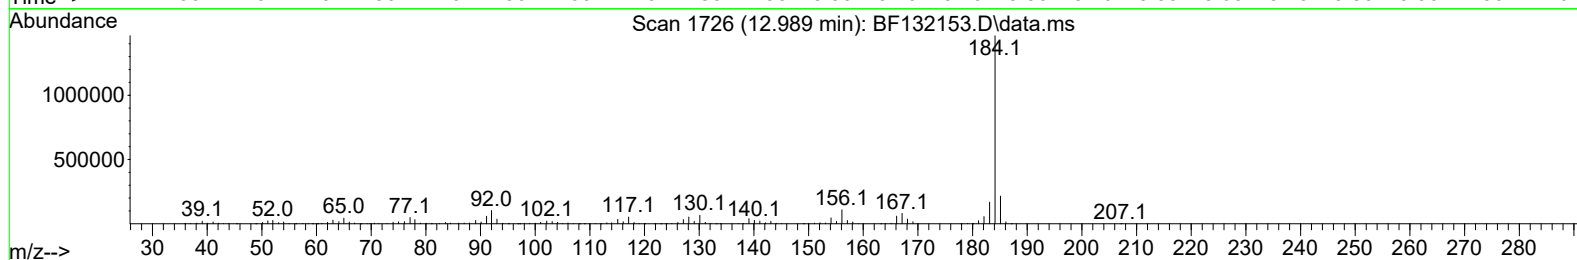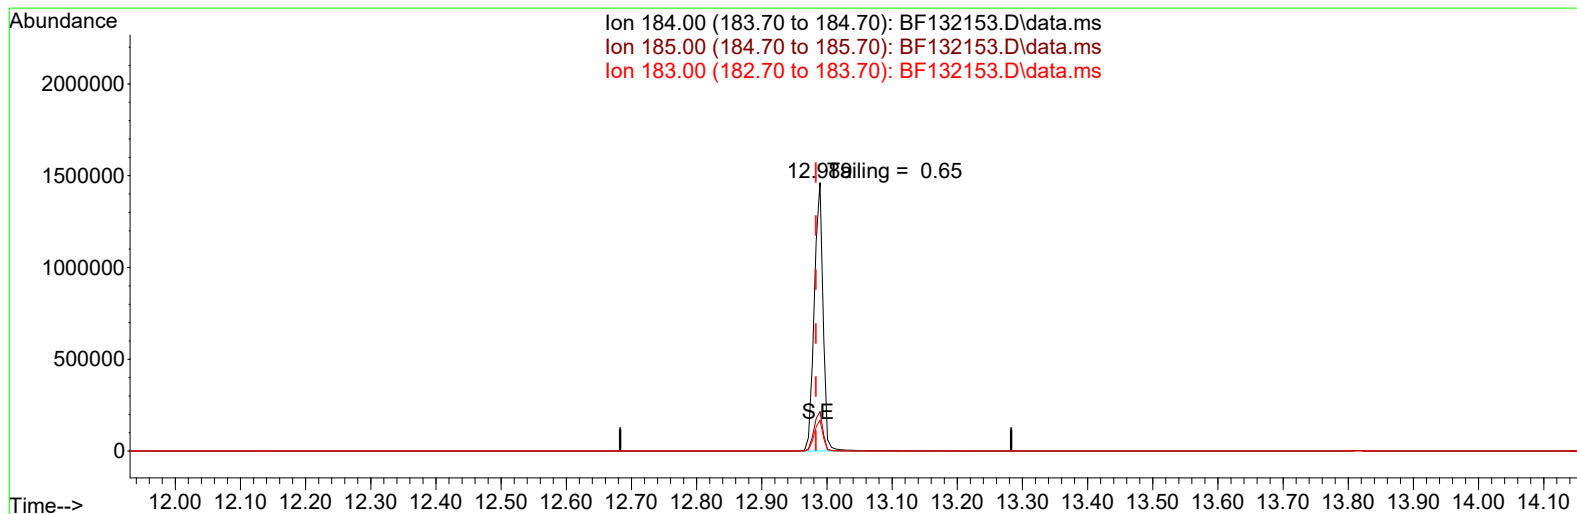

TIC: BF132153.D\data.ms

(77) Benzidine

12.989min (+ 0.006) 13201.89 ng

response 1380589

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.60	14.72
183.00	11.20	11.51
0.00	0.00	0.00