


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012023\
 Data File : BF132163.D
 Acq On : 20 Jan 2023 16:08
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 20 00:50:42 2023

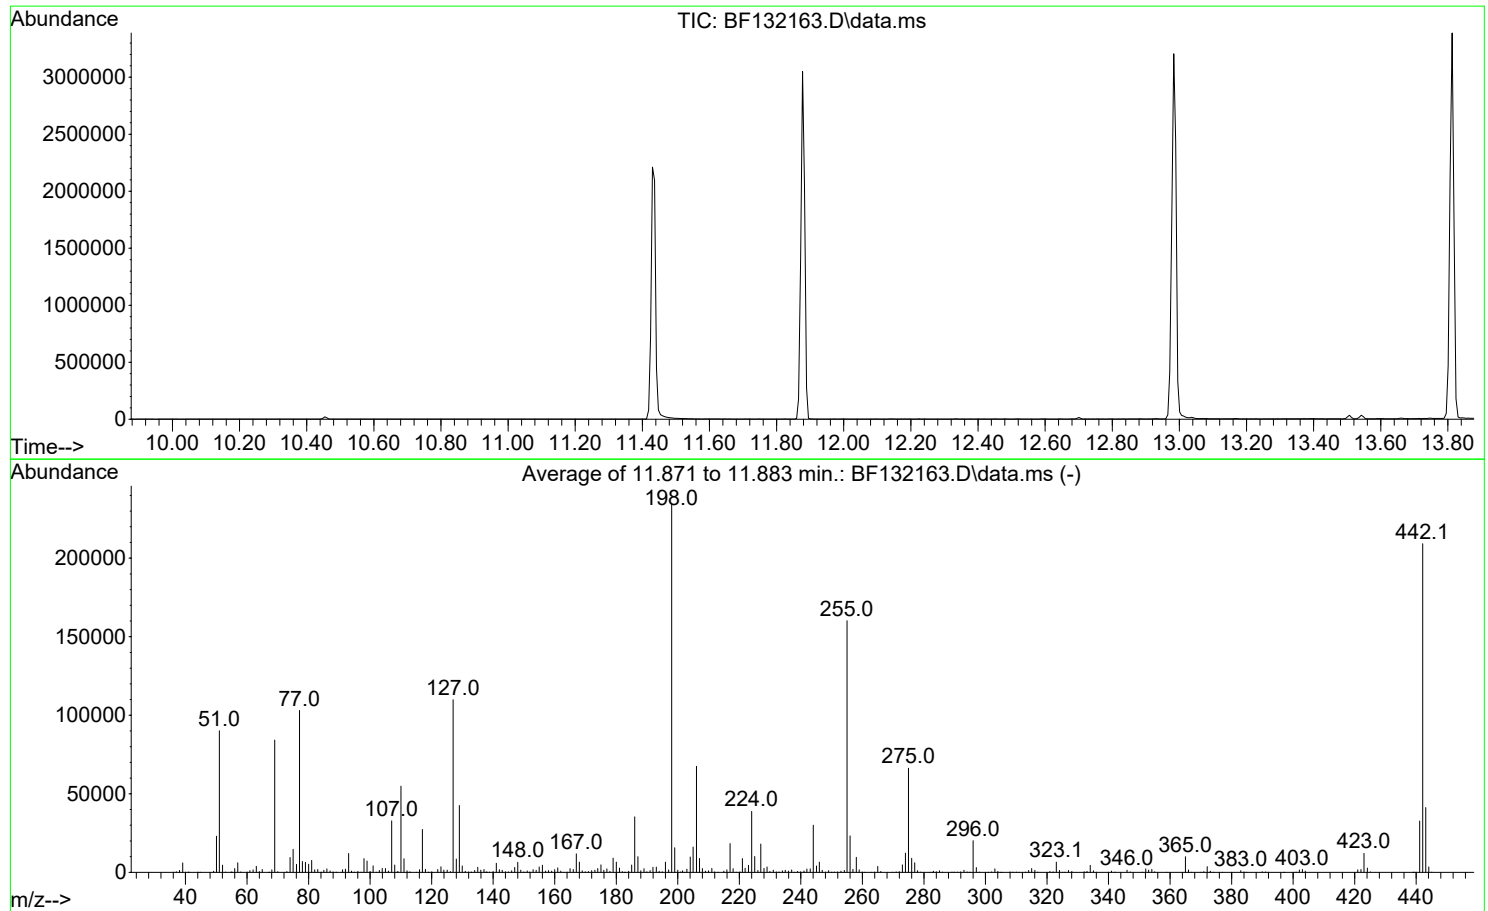

AutoFind: Scans 1536, 1537, 1538; Background Corrected with Scan 1531

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	90128	PASS
68	69	0.00	2	1.9	1614	PASS
69	198	0.00	100	36.0	84219	PASS
70	69	0.00	2	0.5	412	PASS
127	198	10	80	46.9	109877	PASS
197	198	0.00	2	0.7	1548	PASS
198	198	100	100	100.0	234176	PASS
199	198	5	9	6.7	15675	PASS
275	198	10	60	28.3	66331	PASS
365	198	1	100	4.3	9988	PASS
441	198	0.01	100	13.9	32650	PASS
442	442	50	100	100.0	209173	PASS
443	442	15	24	19.7	41258	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/20/2023	BNA_F	<u>BF132163.D</u>
Compound Name	Response	Retention Time
DDT	531722	13.813
DDD	9556	13.507
DDE	599	13.166
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10155	541877	1.87

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF012023\
Data File : BF132163.D
Acq On : 20 Jan 2023 16:08
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jan 21 05:32:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF011923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 20 00:50:42 2023
Response via : Initial Calibration

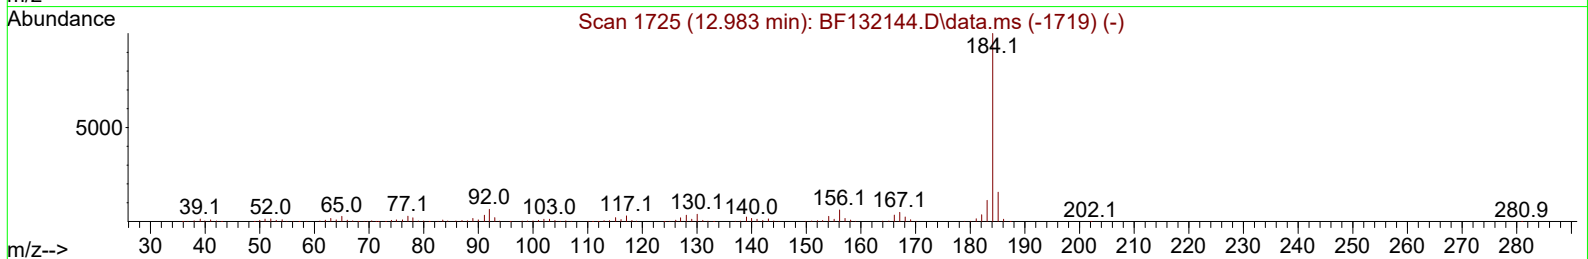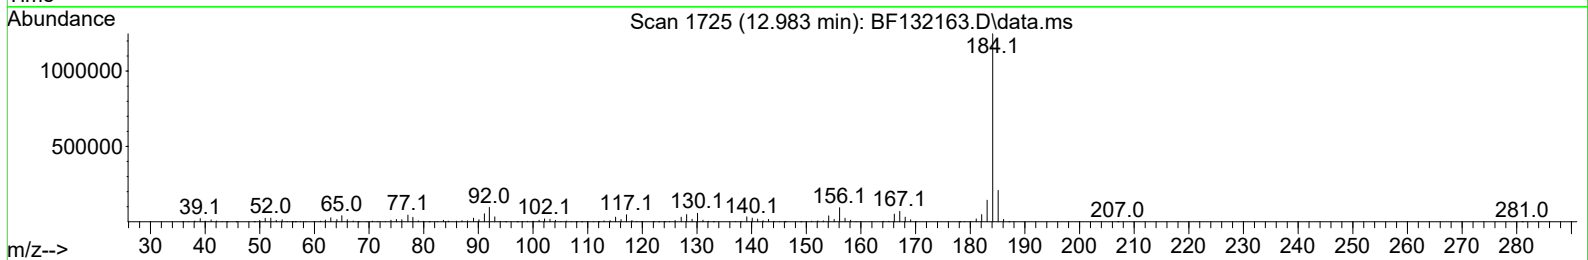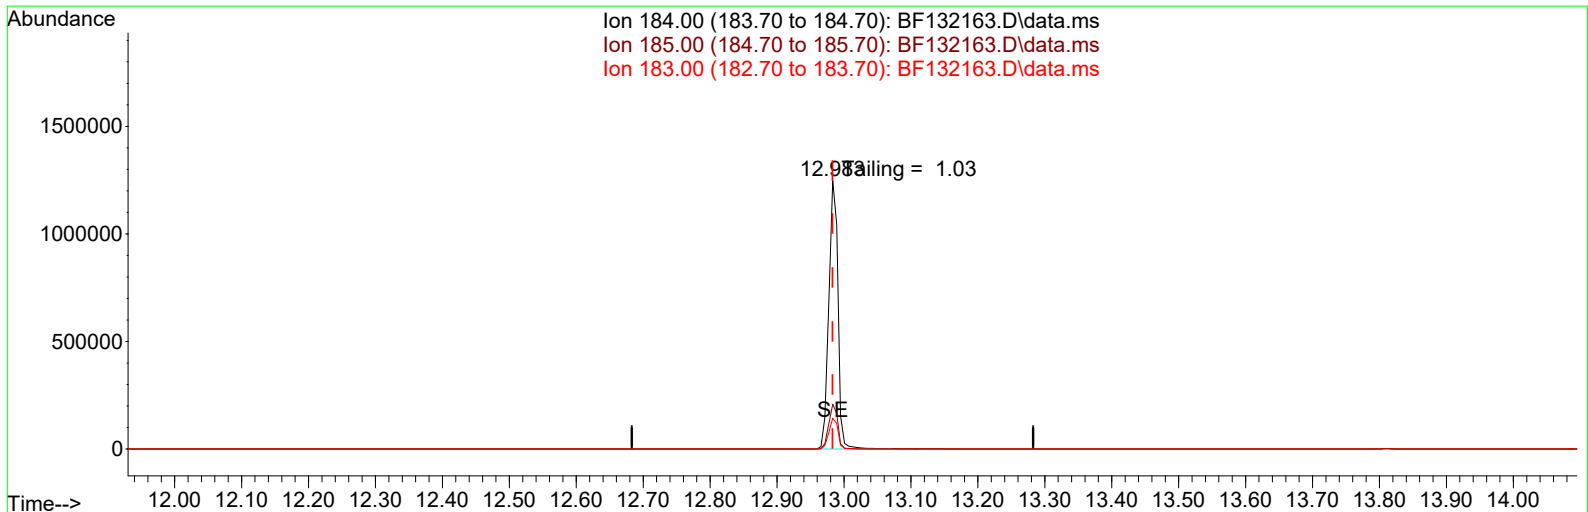

TIC: BF132163.D\data.ms

(77) Benzidine

12.983min (+ 0.000) 697715.54 ng

response 1194065

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.60	16.72
183.00	11.20	11.48
0.00	0.00	0.00