
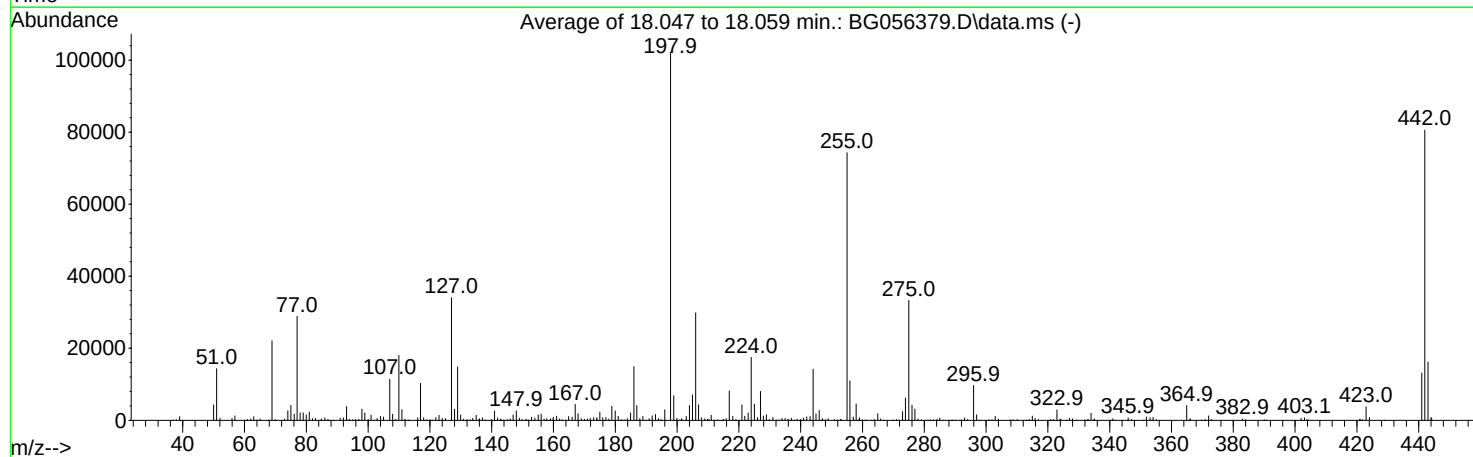


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012323\
Data File : BG056379.D
Acq On : 23 Jan 2023 10:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 19 00:31:30 2023

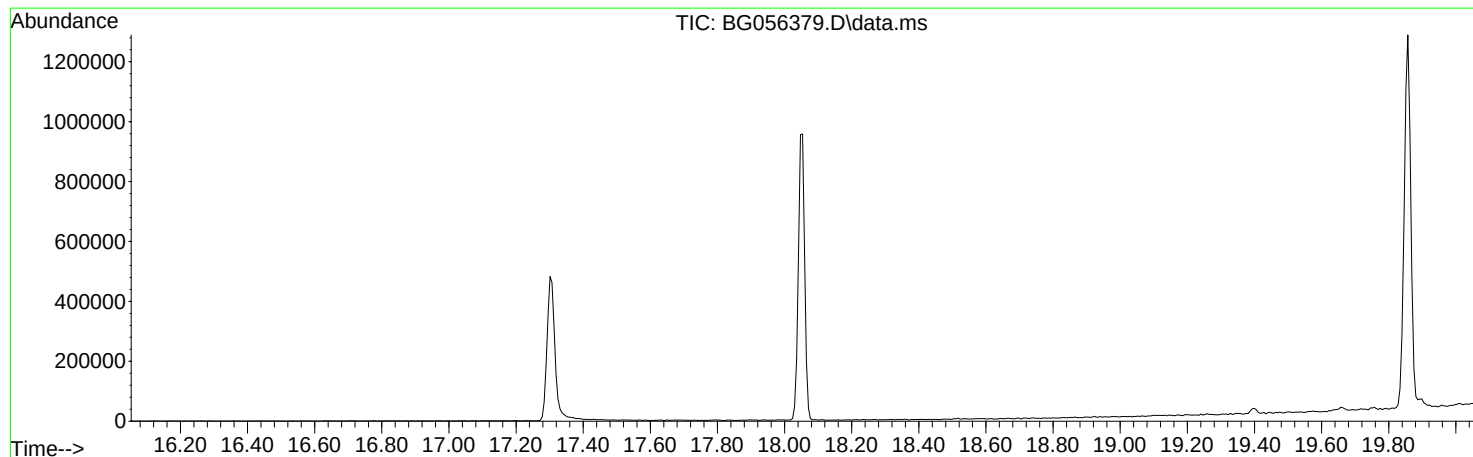




AutoFind: Scans 2512, 2513, 2514; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	14.0	14345	PASS
68	69	0.00	2	0.4	97	PASS
69	198	0.00	100	21.6	22095	PASS
70	69	0.00	2	0.8	183	PASS
127	198	10	80	33.3	34013	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	102163	PASS
199	198	5	9	6.7	6806	PASS
275	198	10	60	32.6	33299	PASS
365	198	1	100	4.0	4075	PASS
441	198	0.01	100	12.8	13078	PASS
442	442	50	100	100.0	80573	PASS
443	442	15	24	20.1	16215	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012323\
Data File : BG056379.D
Acq On : 23 Jan 2023 10:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 24 04:48:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:31:30 2023
Response via : Initial Calibration

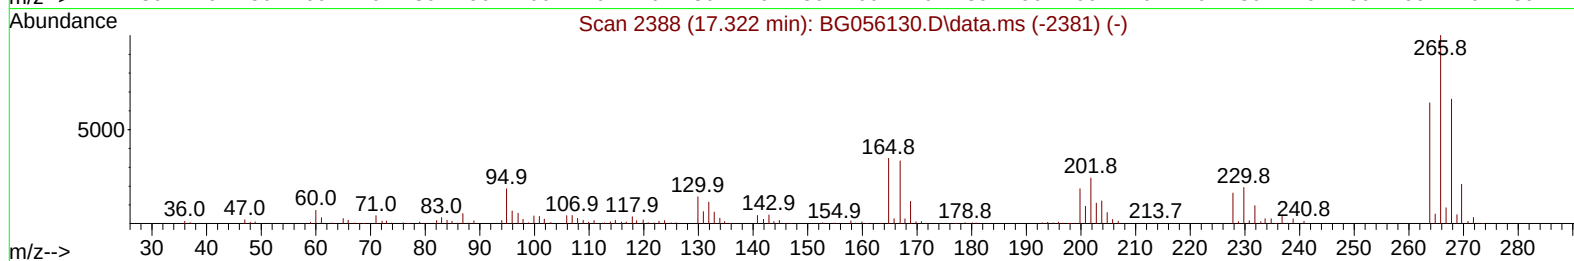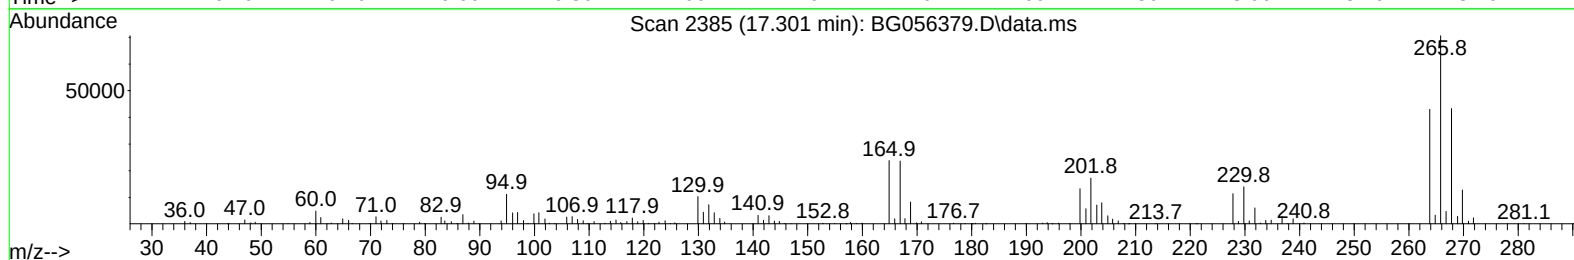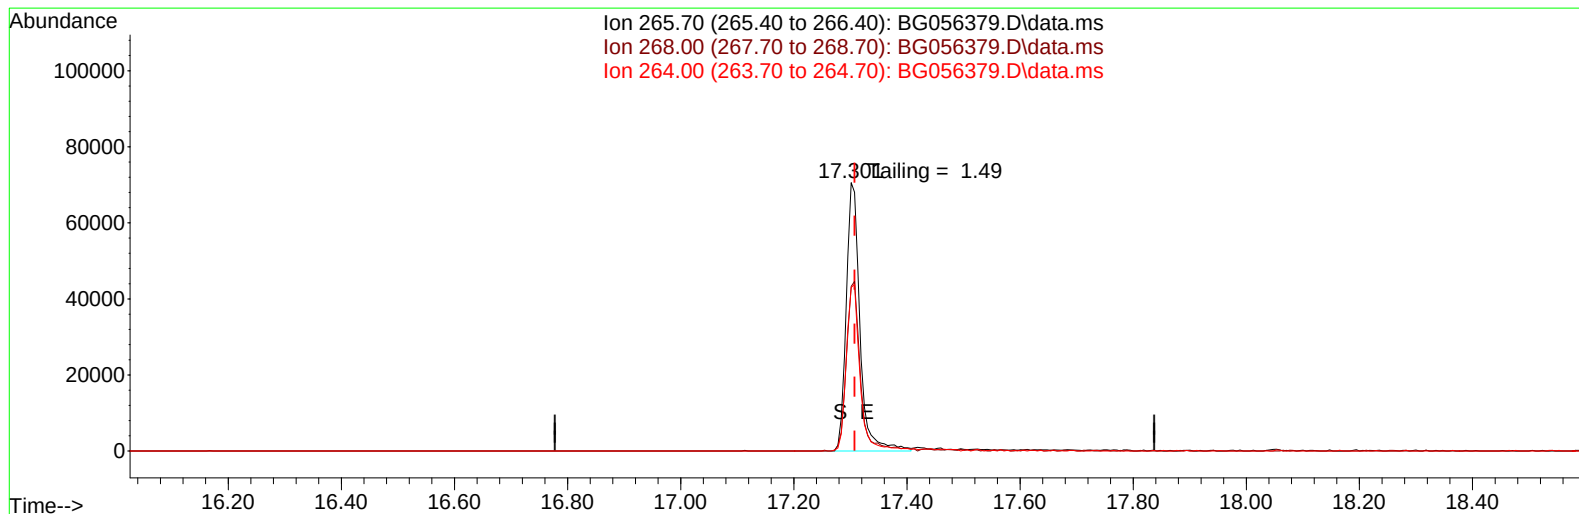

TIC: BG056379.D\data.ms

(70) Pentachlorophenol (C)

17.301min (-0.006) 207454.78 ng




response 119277

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	61.37
264.00	64.30	60.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG012323\
Data File : BG056379.D
Acq On : 23 Jan 2023 10:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 24 04:48:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 00:31:30 2023
Response via : Initial Calibration

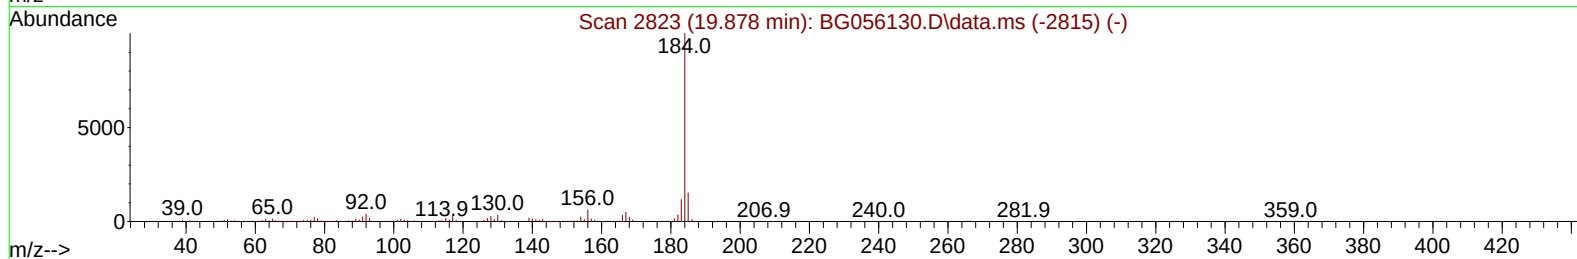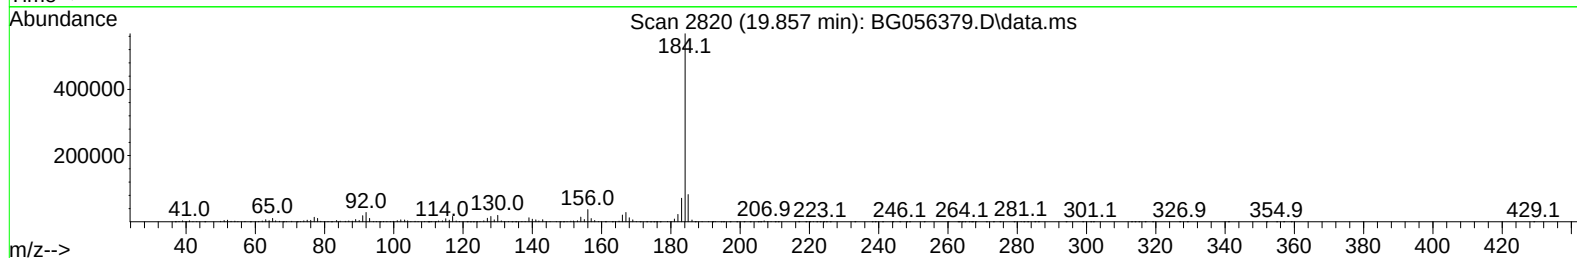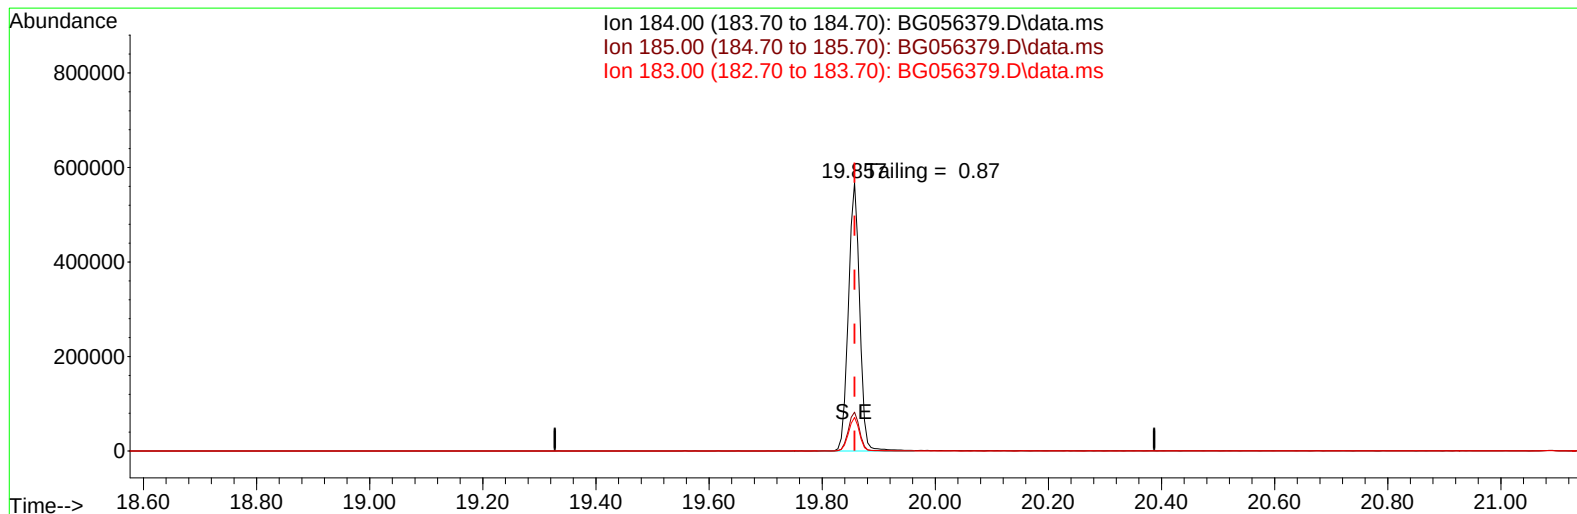

TIC: BG056379.D\data.ms

(77) Benzidine

19.857min (+ 0.000) 38441.69 ng

response 788090

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.48
183.00	11.70	12.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/23/2023	BNA_G	<u>BG056379.D</u>
Compound Name	Response	Retention Time
DDT	355347	21.085
DDD	9088	20.639
DDE	1108	20.133
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10196	365543	2.79

Instrument :
BNA_G
ClientSampleId :
DFTPP