


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
 Data File : BP013544.D
 Acq On : 23 Jan 2023 10:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 24 04:44:15 2023

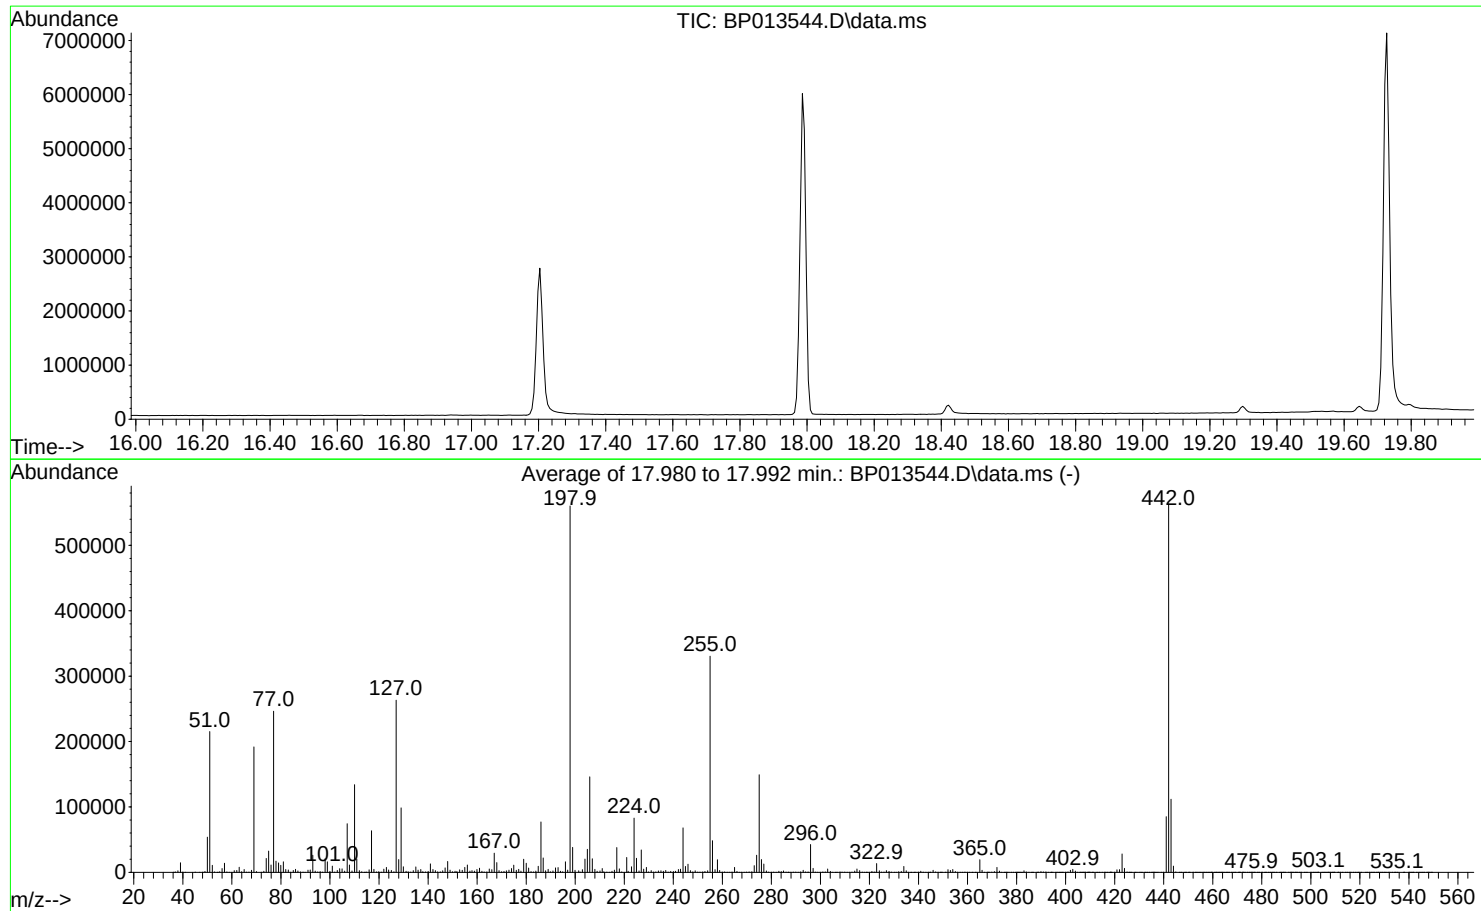




AutoFind: Scans 2515, 2516, 2517; Background Corrected with Scan 2505

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	215161	PASS
68	69	0.00	2	1.7	3171	PASS
69	198	0.00	100	34.2	191778	PASS
70	69	0.00	2	0.6	1101	PASS
127	198	10	80	47.0	263314	PASS
197	198	0.00	2	0.6	3272	PASS
198	198	100	100	100.0	560212	PASS
199	198	5	9	6.8	37959	PASS
275	198	10	60	26.6	149212	PASS
365	198	1	100	3.4	19282	PASS
441	198	0.01	100	15.2	85136	PASS
442	442	100	100	100.0	562603	PASS
443	442	15	24	19.9	111780	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
Data File : BP013544.D
Acq On : 23 Jan 2023 10:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 24 06:33:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 04:44:15 2023
Response via : Initial Calibration

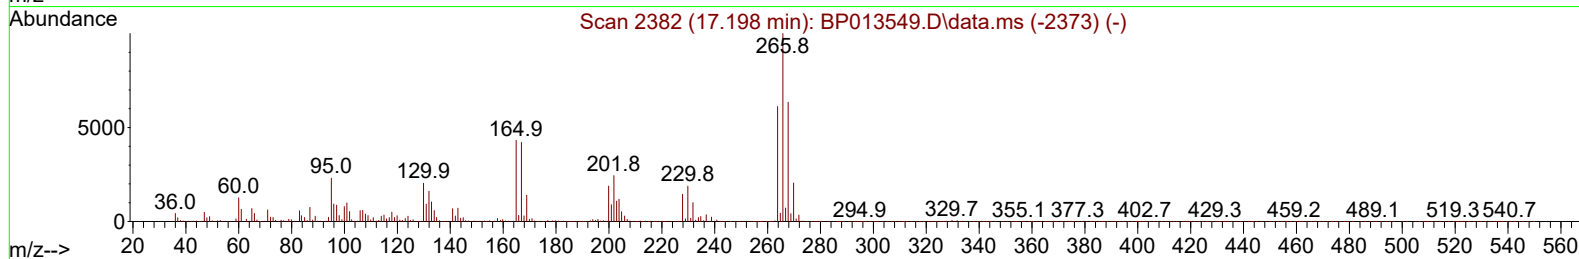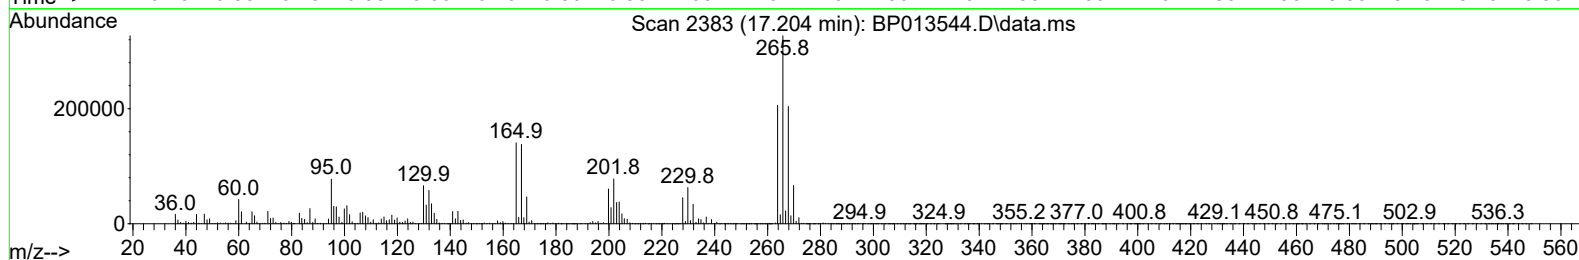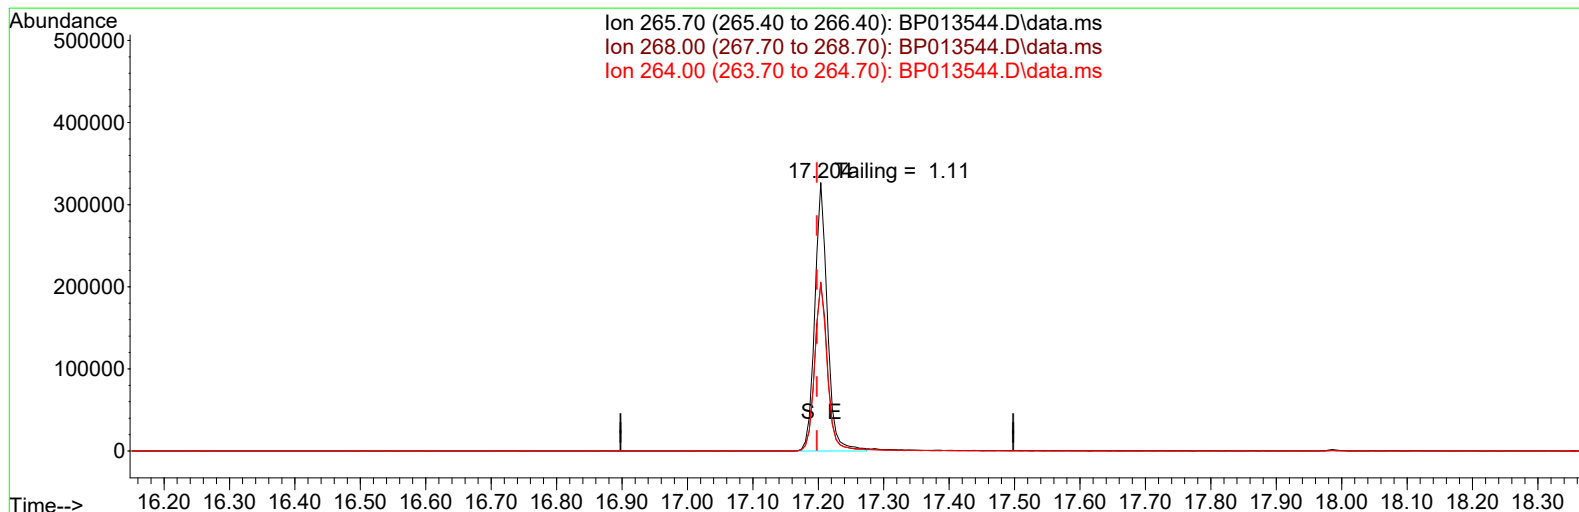

TIC: BP013544.D\data.ms

(70) Pentachlorophenol (C)

17.204min (+ 0.006) 143380.43 ng




response 446504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.40	62.40
264.00	61.10	62.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP012323\
Data File : BP013544.D
Acq On : 23 Jan 2023 10:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jan 24 06:33:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP012323.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 24 04:44:15 2023
Response via : Initial Calibration

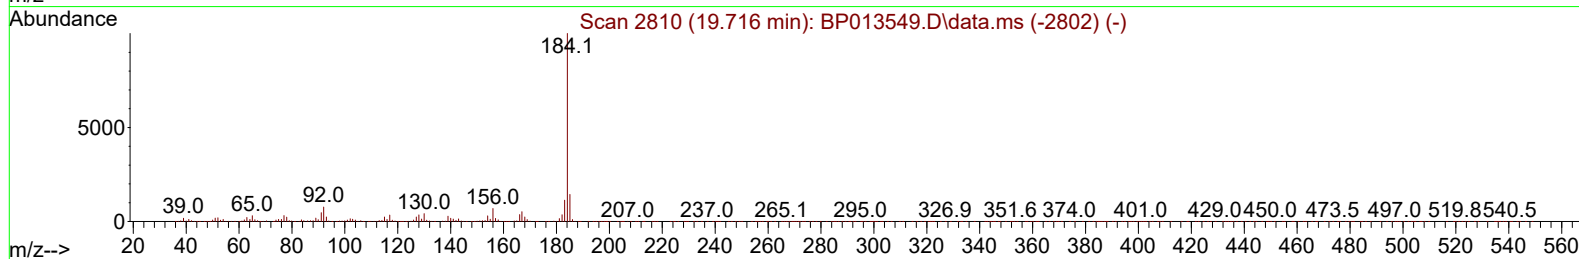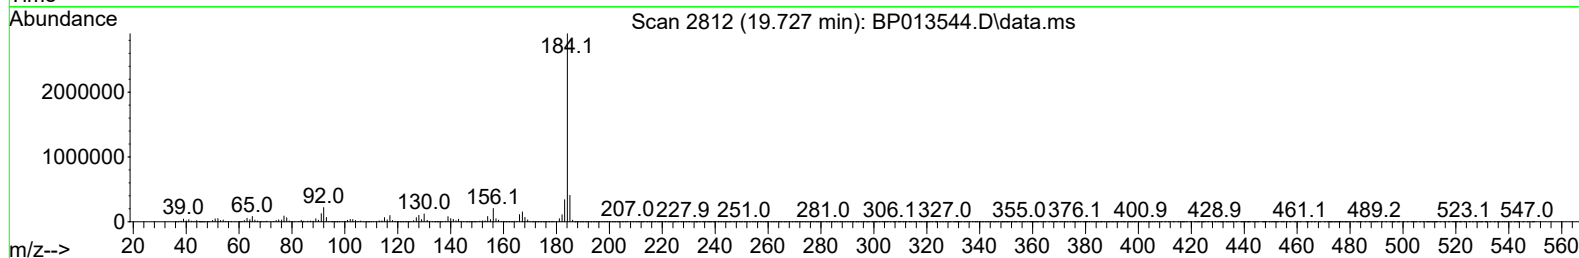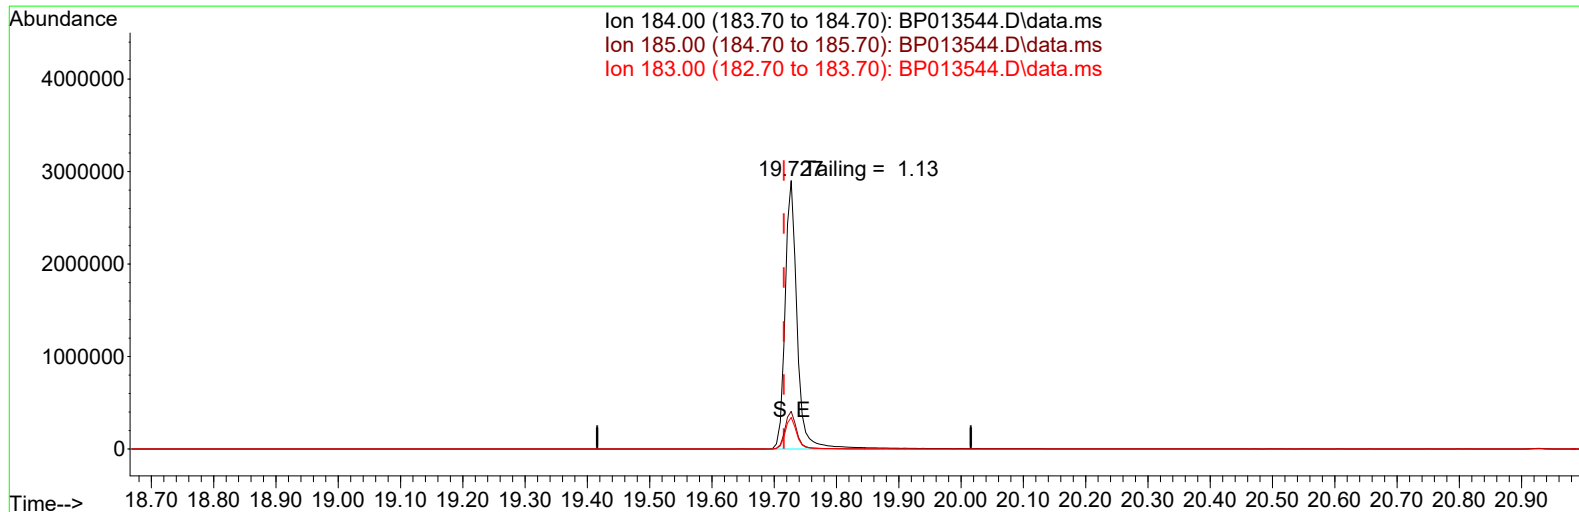

TIC: BP013544.D\data.ms

(77) Benzidine

19.727min (+ 0.011) 235734.26 ng

response 3930835

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.04
183.00	11.30	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/23/2023	BNA_P	<u>BP013544.D</u>
Compound Name	Response	Retention Time
DDT	1143440	20.927
DDD	15344	20.551
DDE	848	19.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16192	1159632	1.40

Instrument :
BNA_P
ClientSampleId :
DFTPP