

Prep Standard - Chemical Standard Summary**Order ID :** O2213**Test :** Herbicide**Prepbatch ID :** PB151928,**Sequence ID/Qc Batch ID:** ps041223,**Standard ID :**

EP2318,EP2320,PP21339,PP21341,PP21342,PP21343,PP21344,PP21345,PP21346,PP21349,PP21350,PP21769,PP21867,

Chemical ID :

E2865,E3370,E3412,E3453,E3477,E3486,E3487,M4587,M5211,P10284,P10293,P10320,P10339,P11986,P11987,P12055,P12056,P12057,P12058,P12059,P12060,P12061,P12062,P12063,P12064,P8999,

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2017	1:1 ACETONE/METHYLENE CHLORIDE	EP2318	03/30/2023	09/22/2023	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 03/30/2023

FROM 8000.00000ml of E3486 + 8000.00000ml of E3487 = Final Quantity: 16000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
601	Acidified Sodium Sulphate 2	EP2320	03/30/2023	07/13/2023	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	RUPESHKUMAR SHAH 03/30/2023

FROM 100.00000ml of E3370 + 150.00000ml of M5211 + 3000.00000ml of E3412 = Final Quantity: 3000.000 gram

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

[illegible]

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
36	2000 PPB Herb Working Solution	PP21341	01/09/2023	07/03/2023	Abdul Mirza	None	None	Ankita Jodhani 01/09/2023
<u>FROM</u>	1.00000ml of P10339 + 1.00000ml of P8999 + 98.00000ml of E3453 = Final Quantity: 100.000 ml							

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
191	1500 PPB ICC Herb Std	PP21342	01/09/2023	07/03/2023	Abdul Mirza	None	None	Ankita Jodhani
01/09/2023								

FROM 0.25000ml of E3453 + 0.75000ml of PP21341 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
194	1000 PPB ICC Herb STD	PP21343	01/09/2023	07/03/2023	Abdul Mirza	None	None	Ankita Jodhani
01/09/2023								

FROM 0.50000ml of E3453 + 0.50000ml of PP21341 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
195	750 PPB ICC Herb STD	PP21344	01/09/2023	07/03/2023	Abdul Mirza	None	None	Ankita Jodhani
01/09/2023								

FROM 0.25000ml of E3453 + 0.75000ml of PP21343 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
196	500 PPB ICC Herb STD	PP21345	01/09/2023	07/03/2023	Abdul Mirza	None	None	Ankita Jodhani
01/09/2023								

FROM 0.50000ml of E3453 + 0.50000ml of PP21343 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
197	200 PPB ICC Herb STD	PP21346	01/09/2023	07/03/2023	Abdul Mirza	None	None	Ankita Jodhani
01/09/2023								

FROM 0.80000ml of E3453 + 0.20000ml of PP21343 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3909	1000 PPB HERB MIX ICV STD(RESTEK+ABSOLUTE)	PP21349	01/09/2023	07/03/2023	Abdul Mirza	None	None	Ankita Jodhani
01/09/2023								

FROM 0.50000ml of E3453 + 0.50000ml of PP21339 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3910	750 PPB ICV HERB STD(RESTEK+ABSOLUTE)	PP21350	01/09/2023	07/03/2023	Abdul Mirza	None	None	Ankita Jodhani
01/09/2023								

FROM 0.25000ml of E3453 + 0.75000ml of PP21349 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1848	5000/500000 PPB Herbicide Spike (Free Acid)	PP21769	03/06/2023	08/28/2023	Abdul Mirza	None	None	Ankita Jodhani
03/07/2023								

FROM 1.25000ml of P11986 + 1.25000ml of P11987 + 47.50000ml of E3477 = Final Quantity: 50.000 ml

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
60	5000 PPB Herbicide Surg Spike (Free Acid)	PP21867	03/28/2023	09/27/2023	Abdul Mirza	None	None	Ankita Jodhani 03/28/2023
<u>FROM</u> 1.25000ml of P12055 + 1.25000ml of P12056 + 1.25000ml of P12057 + 1.25000ml of P12058 + 1.25000ml of P12059 + 1.25000ml of P12060 + 1.25000ml of P12061 + 1.25000ml of P12062 + 1.25000ml of P12063 + 1.25000ml of P12064 + 487.50000ml of E3487 = Final Quantity: 500.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	12/31/2024	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9244-03 / Ether, Anhydrous, Purified (cs/4x4L)	0000288039	07/13/2023	08/01/2022 / Rajesh	07/13/2022 / Rajesh	E3370

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	139404	10/23/2023	10/18/2022 / Rajesh	10/13/2022 / Rajesh	E3412

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	22G0362002	07/03/2023	01/03/2023 / Rajesh	01/03/2023 / Rajesh	E3453

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	22L2862006	09/27/2023	02/28/2023 / Rajesh	02/23/2023 / Rajesh	E3477

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	23A0362012	09/22/2023	03/22/2023 / Rajesh	02/28/2023 / Rajesh	E3486

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	22L2862006	09/27/2023	03/27/2023 / Rajesh	03/22/2023 / Rajesh	E3487

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9530-33 / Hydrochloric Acid, Instra-Analyzed (cs/6x2.5L)	0000251602	01/17/2025	08/18/2020 / Dodley	02/20/2020 / Dodley	M4587

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	22D0862014	01/20/2025	08/22/2022 /	04/26/2022 / mohan	M5211

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32062 / Herbicide Mix, 500/8000, Standard #4 [methyl ester] 200ug/mL, hexane, 1mL/ampul	A0154920	07/09/2023	01/09/2023 / Abdul	03/05/2021 / dhaval	P10284

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32059 / Herbicide Mix#3 (Methyl Ester), 20000 ug/ml	A0167291	07/09/2023	01/09/2023 / Abdul	03/05/2021 / dhaval	P10293

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	70934 / Dalapan methyl ester	062819	07/09/2023	01/09/2023 / Abdul	03/05/2021 / dhaval	P10320

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32055 / Herbicide Mix, 500/8000, Standard #1 [methyl ester] 200ug/mL, hexane, 1mL/ampul	A0165730	07/09/2023	01/09/2023 / Abdul	03/05/2021 / dhaval	P10339

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006686742	09/06/2023	03/06/2023 / Abdul	08/01/2022 / Yogesh	P11986

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006686742	09/06/2023	03/06/2023 / Abdul	08/01/2022 / Yogesh	P11986

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006686742	09/06/2023	03/06/2023 / Abdul	08/01/2022 / Yogesh	P11987

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006686742	09/06/2023	03/06/2023 / Abdul	08/01/2022 / Yogesh	P11987

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0184439	09/28/2023	03/28/2023 / Abdul	08/09/2022 / Ankita	P12055

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0184439	09/28/2023	03/28/2023 / Abdul	08/09/2022 / Ankita	P12056

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0184439	09/28/2023	03/28/2023 / Abdul	08/09/2022 / Ankita	P12057

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0184439	09/28/2023	03/28/2023 / Abdul	08/09/2022 / Ankita	P12058

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0184439	09/28/2023	03/28/2023 / Abdul	08/09/2022 / Ankita	P12059

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0184439	09/28/2023	03/28/2023 / Abdul	08/09/2022 / Ankita	P12060

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0184439	09/28/2023	03/28/2023 / Abdul	08/09/2022 / Ankita	P12061

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0184439	09/28/2023	03/28/2023 / Abdul	08/09/2022 / Ankita	P12062

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0184439	09/28/2023	03/28/2023 / Abdul	08/09/2022 / Ankita	P12063

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0184439	09/28/2023	03/28/2023 / Abdul	08/09/2022 / Ankita	P12064

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32050 / Herbicide, 8000 series, 515 Surrogate [ester] 2,4-dichlorophenyl acetic acid methyl ester, 1mL, 200ug/mL, Hexane	A0152705	07/09/2023	01/09/2023 / Abdul	10/11/2019 / Stephen	P8999



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32055 Lot No.: A0165730
Description : Herbicide Mix #1/ME (Methyl Ester)
Herbicide Mix #1/ME (Methyl Ester) 200 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : October 31, 2027 Storage: 10°C or colder
Handling: This product is photosensitive. Ship: Ambient

2D
P10336
To - (5)
P10340
03/05/2021

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	Dicamba methyl ester CAS # 6597-78-0 (Lot 6580100) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL +/- 6.7507 µg/mL +/- 6.7507 µg/mL	Gravimetric Unstressed Stressed
2	Dichlorprop methyl ester CAS # 57153-17-0 (Lot 8578700) Purity 98%	201.9 µg/mL	+/- 1.4315 µg/mL +/- 6.8141 µg/mL +/- 6.8141 µg/mL	Gravimetric Unstressed Stressed
3	2,4-D methyl ester CAS # 1928-38-7 (Lot 5209600) Purity 99%	202.0 µg/mL	+/- 1.4323 µg/mL +/- 6.8182 µg/mL +/- 6.8182 µg/mL	Gravimetric Unstressed Stressed
4	2,4,5-TP (silvex) methyl ester CAS # 4841-20-7 (Lot 504400) Purity 99%	202.0 µg/mL	+/- 1.4323 µg/mL +/- 6.8182 µg/mL +/- 6.8182 µg/mL	Gravimetric Unstressed Stressed
5	2,4,5-T methyl ester CAS # 1928-37-6 (Lot 6875800) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL +/- 6.7507 µg/mL +/- 6.7507 µg/mL	Gravimetric Unstressed Stressed
6	Dinoseb methyl ether CAS # 6099-79-2 (Lot 4362100) Purity 99%	202.0 µg/mL	+/- 1.4323 µg/mL +/- 6.8182 µg/mL +/- 6.8182 µg/mL	Gravimetric Unstressed Stressed
7	2,4-DB methyl ester CAS # 18625-12-2 (Lot 6847200) Purity 99%	202.0 µg/mL	+/- 1.4323 µg/mL +/- 6.8182 µg/mL +/- 6.8182 µg/mL	Gravimetric Unstressed Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)


Carrier Gas:
hydrogen, constant pressure, 10 psi

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

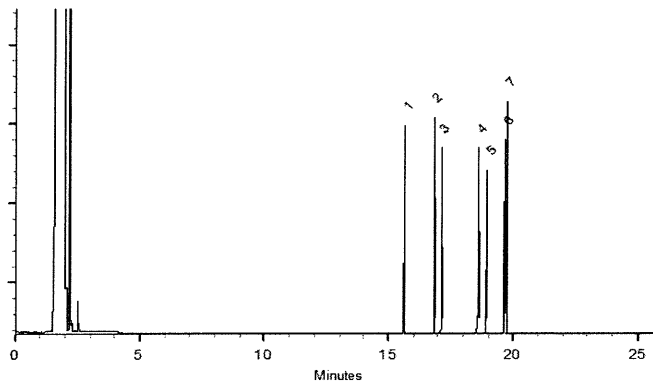

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Tom Suckar - Mix Technician

Date Mixed: 27-Oct-2020

Balance: B707717271


Justine Albertson - Operations Tech-ARM QC

Date Passed: 29-Oct-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32059 Lot No.: A0167291
Description : Herbicide Mix #3/ME (Methyl Ester)
Herbicide Mix #3/ME (Methyl Ester) 20,000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : December 31, 2027 Storage: 10°C or colder
Handling: This product is photosensitive. Ship: Ambient

DP
03/05/2021

P10290
To - (5)
P10294

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	MCPP (Mecoprop) methyl ester CAS # 23844-56-6 (Lot 11046600) Purity 99%	20,044.0 µg/mL	+/- 185.4909 µg/mL Gravimetric +/- 686.9695 µg/mL Unstressed +/- 686.9695 µg/mL Stressed
2	MCPA methyl ester CAS # 2436-73-9 (Lot SL201209) Purity 99%	20,012.0 µg/mL	+/- 185.1948 µg/mL Gravimetric +/- 685.8728 µg/mL Unstressed +/- 685.8728 µg/mL Stressed
Solvent:	Hexane CAS # 110-54-3 Purity 99%		

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

330°C

Det. Type:

FID

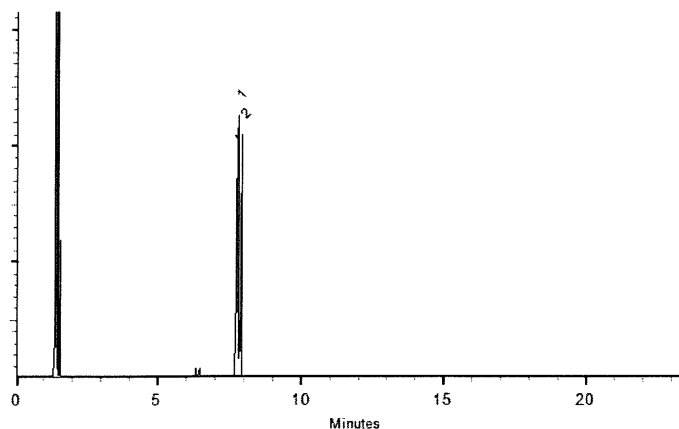

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Bookhamer - Operations Technician I

Date Mixed: 16-Dec-2020

Balance: B442140311

Justine Albertson - Operations Tech-ARM QC

Date Passed: 18-Dec-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

DD
02/05/2021

P10280
TO
P10284 - (S)

Catalog No. : 32062 **Lot No.:** A0154920

Description : Herbicide Mix #4/ME (Methyl Ester)
Herbicide Mix #4/ME (Methyl Ester) 200µg/mL,
Hexane/Methyl-tert-butyl-ether, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2026 **Storage:** 10°C or colder

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	3,5-Dichlorobenzoic acid methyl ester CAS # 2905-67-1 (Lot 3903900) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL +/- 6.7507 µg/mL +/- 6.7507 µg/mL	Gravimetric Unstressed Stressed
2	4-Nitroanisole CAS # 100-17-4 (Lot 24765/7) Purity 99%	202.0 µg/mL	+/- 1.4323 µg/mL +/- 6.8182 µg/mL +/- 6.8182 µg/mL	Gravimetric Unstressed Stressed
3	Pentachloroanisole CAS # 1825-21-4 (Lot 7921100) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL +/- 6.7507 µg/mL +/- 6.7507 µg/mL	Gravimetric Unstressed Stressed
4	Chloramben methyl ester CAS # 7286-84-2 (Lot 6487100) Purity 98%	199.9 µg/mL	+/- 1.4176 µg/mL +/- 6.7480 µg/mL +/- 6.7480 µg/mL	Gravimetric Unstressed Stressed
5	Bentazon methyl ester CAS # 61592-45-8 (Lot 817100) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL +/- 6.7507 µg/mL +/- 6.7507 µg/mL	Gravimetric Unstressed Stressed
6	Picloram methyl ester CAS # 14143-55-6 (Lot 853300) Purity 98%	199.9 µg/mL	+/- 1.4176 µg/mL +/- 6.7480 µg/mL +/- 6.7480 µg/mL	Gravimetric Unstressed Stressed
7	DCPA methyl ester (Chlorthal-dimethyl) CAS # 1861-32-1 (Lot 8816400) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL +/- 6.7507 µg/mL +/- 6.7507 µg/mL	Gravimetric Unstressed Stressed

8	Acifluorfen methyl ester	200.0 µg/mL	+/- 1.4182	µg/mL	Gravimetric
	CAS # 50594-67-7 (Lot 6282300)		+/- 6.7507	µg/mL	Unstressed
	Purity 99%		+/- 6.7507	µg/mL	Stressed

Solvent: Hexane/Methyl-tert-butyl-ether
CAS # 110-54-3/1634-04-4
Purity 99%

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)


Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

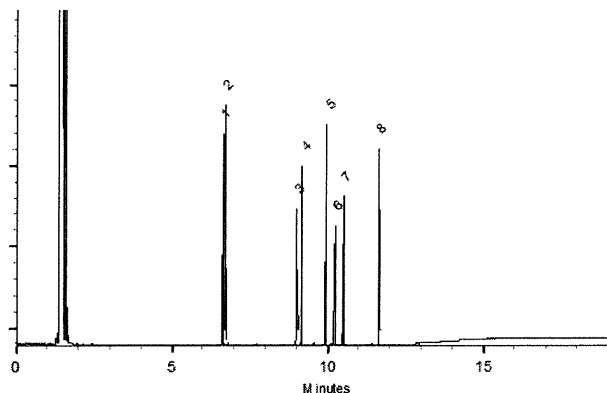

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Jessica McClenahan - Operations Technician I

Date Mixed: 11-Nov-2019 **Balance:** 1128360905


Justine Albertson - Operations Tech-ARM QC

Date Passed: 18-Nov-2019

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



Certified Reference Material CRM



CERTIFIED WEIGHT REPORT

Part Number: 70934
Lot Number: 062121
Description: Dalapon methyl ester

Solvent(s): Methanol
Lot# DY186-US

Expiration Date: 062126
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 6UTB

5E-05 Balance Uncertainty
0.0003 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 10.0


Formulated By:	Prashant Chauhan	062121	DATE
Reviewed By:	Pedro L. Rentas	062121	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information		
										(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LD50

1. Dalapon methyl ester 934 8116100 1000 97.6 0.5 0.01027 0.01035 1008.1 14.2 17640-02-7 N/A orl-rat 970mg/kg

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 200°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Melissa Stonier.

TIC: [BSB9]70934.D

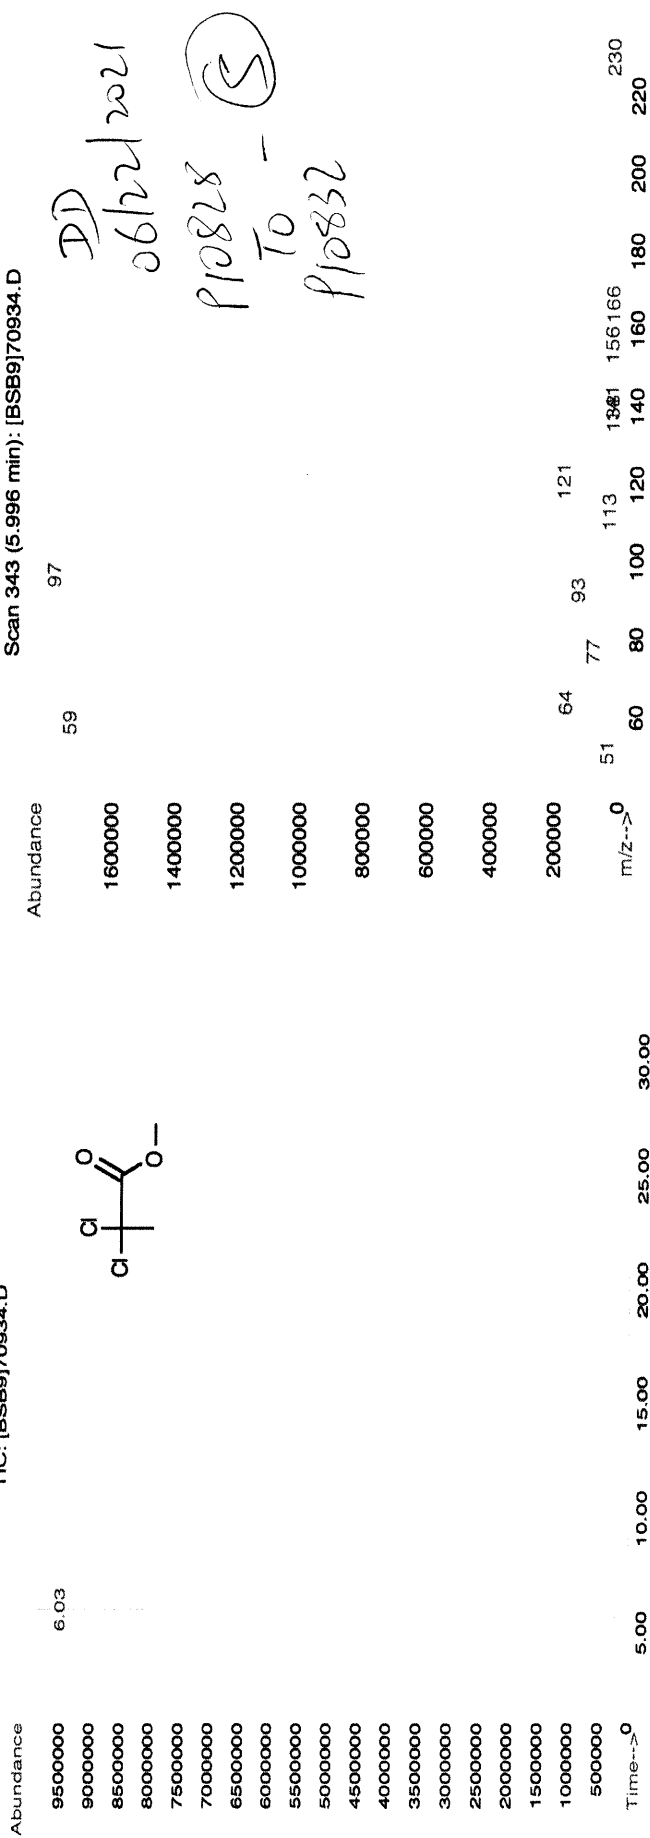

* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1

Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Ether, Anhydrous
BAKER ANALYZED® A.C.S. Reagent
Contains BHT as a Preservative
Suitable for Fat Extraction



Material No.: 9244-03
Batch No.: 0000288039
Manufactured Date: 2021/07/22
Expiration Date: 2023/07/22
Revision No: 1

Certificate of Analysis

Meets ACS Reagent Chemical Requirements,

Test	Specification	Result
Assay ((C ₂ H ₅) ₂ O) (by GC, corrected for water)	>= 99.0 %	100.0
Alcohol (C ₂ H ₅ OH)	Passes Test	PT
Carbonyl Compounds (as HCHO) (by polarography)	<= 0.001 %	< 0.001
Color (APHA)	<= 10	< 5
Peroxide (as H ₂ O ₂)	<= 1 ppm	< 1
Preservative (BHT)	>= 7 ppm	9
Residue after Evaporation	<= 0.0010 %	< 0.0010
Titration Acid (μeq/g)	<= 0.2	< 0.2
Water (by KF, coulometric)	<= 0.01 %	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US

Recd. by RP on 7/13/22

E 3370


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700




**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**



MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MÉXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT : SODIUM SULFATE CRYSTALS ANHYDROUS
QUALITY : ACS (CODE RMB3375) **FORMULA :** Na₂SO₄
SPECIFICATION NUMBER : 6399 **RELEASE DATE:** OCT/28/2021
LOT NUMBER : 139404

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.8 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.0
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.002 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.2 %
Retained on US Standard No. 60 sieve	Min. 94%	97.6 %
Through US Standard No. 60 sieve	Max. 5%	2.1 %
Through US Standard No. 100 sieve	Max. 10%	0.2 %
COMMENTS		
 QC: PhC Irma Belmares		

If you need further details, please call our factory or contact our local distributor.

E 3412

Recd. by RP on 10/13/22

RE-02-01, Ed. 3

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent



Material No.: 9262-03
Batch No.: 22G0362002
Manufactured Date: 2022-06-17
Expiration Date: 2023-09-16
Revision No.: 0

Certificate of Analysis


Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	2
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	2
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.5 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	97 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 01/03/23

E 3453

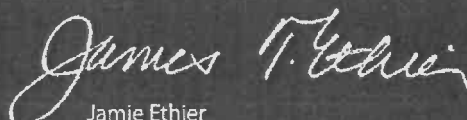
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Acetone

BAKER RESI-ANALYZED® Reagent

For Organic Residue Analysis



Material No.: 9254-03

Batch No.: 22L2862006

Manufactured Date: 2022-12-19

Expiration Date: 2025-12-18

Revision No.: 0

Certificate of Analysis


Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H ₂ O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	4

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 2/23/23

E 3477

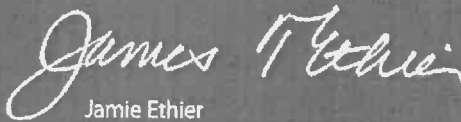
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Page 1 of 1

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 23A0362012
Manufactured Date: 2022-11-23
Expiration Date: 2024-02-22
Revision No.: 0


Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	2
Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	≤ 10	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	< 0.1 ppm
Titration Acid ($\mu\text{eq/g}$)	≤ 0.3	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3486


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03
Batch No.: 22L2862006
Manufactured Date: 2022-12-19
Expiration Date: 2025-12-18
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H ₂ O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	4

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP ON 3/22/23

E 3487


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

M4587

Hydrochloric Acid, 36.5–38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis

Recieve Date: 2/20/20



Material No.: 9530-33
Batch No.: 0000251602
Manufactured Date: 2020/01/17
Retest Date: 2025/01/15
Revision No: 1

Certificate of Analysis

Test	Specification	Result
ACS – Assay (as HCl) (by acid–base titrn)	36.5 – 38.0 %	37.7
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	< 1
ACS – Specific Gravity at 60°/60°F	1.185 – 1.192	1.191
ACS – Bromide (Br)	<= 0.005 %	< 0.005
ACS – Extractable Organic Substances	<= 5 ppm	< 1
ACS – Free Chlorine (as Cl ₂)	<= 0.5 ppm	< 0.5
Phosphate (PO ₄)	<= 0.05 ppm	< 0.03
Sulfate (SO ₄)	<= 0.5 ppm	< 0.3
Sulfite (SO ₃)	<= 0.8 ppm	0.3
Ammonium (NH ₄)	<= 3 ppm	< 1
Trace Impurities – Arsenic (As)	<= 0.010 ppm	< 0.003
Trace Impurities – Aluminum (Al)	<= 10.0 ppb	< 0.2
Arsenic and Antimony (as As)	<= 5 ppb	< 3
Trace Impurities – Barium (Ba)	<= 1.0 ppb	< 0.2
Trace Impurities – Beryllium (Be)	<= 1.0 ppb	< 0.2
Trace Impurities – Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities – Boron (B)	<= 20.0 ppb	< 5.0
Trace Impurities – Cadmium (Cd)	<= 1.0 ppb	< 0.3
Trace Impurities – Calcium (Ca)	<= 50.0 ppb	14.2
Trace Impurities – Chromium (Cr)	<= 1.0 ppb	< 0.4
Trace Impurities – Cobalt (Co)	<= 1.0 ppb	< 0.3
Trace Impurities – Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities – Gallium (Ga)	<= 1.0 ppb	< 0.2


For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Material No.: 9530-33
Batch No.: 0000251602

Test	Specification	Result
Trace Impurities – Germanium (Ge)	<= 3.0 ppb	< 2.0
Trace Impurities – Gold (Au)	<= 4.0 ppb	0.2
Heavy Metals (as Pb)	<= 100 ppb	< 50
Trace Impurities – Iron (Fe)	<= 15.0 ppb	1.8
Trace Impurities – Lead (Pb)	<= 1.0 ppb	< 0.5
Trace Impurities – Lithium (Li)	<= 1.0 ppb	< 0.2
Trace Impurities – Magnesium (Mg)	<= 10.0 ppb	0.4
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	< 0.1
Trace Impurities – Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities – Nickel (Ni)	<= 4.0 ppb	< 0.3
Trace Impurities – Niobium (Nb)	<= 1.0 ppb	< 0.2
Trace Impurities – Potassium (K)	<= 9.0 ppb	< 2.0
Trace Impurities – Selenium (Se), For Information Only	ppb	1.0
Trace Impurities – Silicon (Si)	<= 100.0 ppb	< 10.0
Trace Impurities – Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities – Sodium (Na)	<= 100.0 ppb	< 5.0
Trace Impurities – Strontium (Sr)	<= 1.0 ppb	< 0.2
Trace Impurities – Tantalum (Ta)	<= 1.0 ppb	< 0.9
Trace Impurities – Thallium (Tl)	<= 5.0 ppb	< 2.0
Trace Impurities – Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities – Titanium (Ti)	<= 1.0 ppb	0.2
Trace Impurities – Vanadium (V)	<= 1.0 ppb	< 0.2
Trace Impurities – Zinc (Zn)	<= 5.0 ppb	0.6
Trace Impurities – Zirconium (Zr)	<= 1.0 ppb	< 0.1

For Laboratory, Research or Manufacturing Use
Product Information (not specifications):
Appearance (clear, fuming liquid)
Meets ACS Specifications

Country of Origin: US
Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Sulfuric Acid

BAKER INSTRA-ANALYZED® Reagent

For Trace Metal Analysis

Low Selenium

avantor™



Material No.: 9673-33

Batch No.: 22D0862014

Manufactured Date: 2022-02-23

Retest Date: 2027-02-22

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
ACS – Assay (H ₂ SO ₄)	95.0 – 98.0 %	96.5 %
Appearance	Passes Test	Passes Test
ACS – Color (APHA)	≤ 10	5
ACS – Residue after Ignition	≤ 3 ppm	< 1 ppm
ACS – Substances Reducing Permanganate (as SO ₂)	≤ 2 ppm	< 2 ppm
Ammonium (NH ₄)	≤ 1 ppm	< 1 ppm
Chloride (Cl)	≤ 0.1 ppm	< 0.1 ppm
Nitrate (NO ₃)	≤ 0.2 ppm	< 0.1 ppm
Phosphate (PO ₄)	≤ 0.5 ppm	< 0.1 ppm
Trace Impurities – Aluminum (Al)	≤ 30.0 ppb	1.7 ppb
Arsenic and Antimony (as As)	≤ 4.0 ppb	< 2.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 2.0 ppb	< 0.3 ppb
Trace Impurities – Chromium (Cr)	≤ 6.0 ppb	< 0.4 ppb
Trace Impurities – Cobalt (Co)	≤ 0.5 ppb	< 0.3 ppb
Trace Impurities – Copper (Cu)	≤ 1.0 ppb	< 0.1 ppb
Trace Impurities – Gold (Au)	≤ 10.0 ppb	< 0.2 ppb
Heavy Metals (as Pb)	≤ 500.0 ppb	< 100.0 ppb
Trace Impurities – Iron (Fe)	≤ 50.0 ppb	2.0 ppb
Trace Impurities – Lead (Pb)	≤ 0.5 ppb	< 0.5 ppb
Trace Impurities – Magnesium (Mg)	≤ 7.0 ppb	0.6 ppb
Trace Impurities – Manganese (Mn)	≤ 1.0 ppb	< 0.4 ppb
Trace Impurities – Mercury (Hg)	≤ 0.5 ppb	< 0.1 ppb
Trace Impurities – Nickel (Ni)	≤ 2.0 ppb	< 0.3 ppb
Trace Impurities – Potassium (K)	≤ 500.0 ppb	< 2.0 ppb
Trace Impurities – Selenium (Se)	≤ 50.0 ppb	12.1 ppb
Trace Impurities – Silicon (Si)	≤ 100.0 ppb	4.4 ppb
Trace Impurities – Silver (Ag)	≤ 1.0 ppb	< 0.3 ppb

>>> Continued on page 2 >>>

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium



Material No.: 9673-33
Batch No.: 22D0862014

Test	Specification	Result
Trace Impurities – Sodium (Na)	≤ 500.0 ppb	6.2 ppb
Trace Impurities – Strontium (Sr)	≤ 5.0 ppb	< 0.2 ppb
Trace Impurities – Tin (Sn)	≤ 5.0 ppb	< 0.8 ppb
Trace Impurities – Zinc (Zn)	≤ 5.0 ppb	0.6 ppb

For Laboratory, Research, or Manufacturing Use

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

A handwritten signature in cursive script that reads 'Jamie Ethier'.
Jamie Ethier
Vice President Global Quality



Trusted Answers

Agilent

ISO 17034

Reference Material Certificate
Product Information Sheet

Product Name: Chlorinated Herbicides Standard

Product Number: HBM-8151A-1

Storage Conditions: Store at Room Temperature (15° to 30°C).

Lot Number: 000686742

Lot Issue Date: 13-Jun-2022

Expiration Date: 31-Jul-2024

Component Name	CERTIFIED VALUES			CAS#	Analyte Lot
	Concentration	Expanded	Uncertainty		
acifluorfen	100.1 ±	0.5 µg/mL		050594-66-6	NT02057
bentazon	100.1 ±	0.5 µg/mL		025057-89-0	RM19026
chloramben	100.2 ±	0.5 µg/mL		000133-90-4	RM03672
2,4-D	100.3 ±	0.5 µg/mL		000094-75-7	RM17172
daleapon	100.3 ±	0.5 µg/mL		000075-99-0	RM19654
2,4-DB	100.2 ±	0.5 µg/mL		000094-82-6	RM02866
tetrachloroterephthalic acid	100.2 ±	0.5 µg/mL		002136-79-0	RM13887
dicamba	100.3 ±	0.5 µg/mL		001918-00-9	RM15881
3,5-dichlorobenzoic acid	100.2 ±	0.5 µg/mL		000051-36-5	RM02768
dichlorprop	100.2 ±	0.5 µg/mL		000120-36-5	RM19240
diuron	100.3 ±	0.5 µg/mL		000088-85-7	RM19863
MCPA	10030 ±	50 µg/mL		000094-74-6	RM12220
MCPP (mecoprop)	10026 ±	50 µg/mL		000093-65-2	RM09273
4-nitrophenol	100.3 ±	0.5 µg/mL		000100-02-7	RM03752
pentachlorophenol	100.2 ±	0.5 µg/mL		000087-86-5	RM02474
picloram	100.2 ±	0.5 µg/mL		001918-02-1	RM19110
silvex	100.2 ±	0.5 µg/mL		000093-72-1	RM19595
2,4,5-T	100.3 ±	0.5 µg/mL		000093-76-5	NT01808

Matrix: methanol (methyl alcohol)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.


Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.


Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:



Monica Bourgeois
QMS Representative



Trusted Answers

Agilent

ISO 17034

Reference Material Certificate
Product Information Sheet

Product Name: Chlorinated Herbicides Standard

Product Number: HBM-8151A-1

Storage Conditions: Store at Room Temperature (15° to 30°C).

Lot Number: 0006686742

Lot Issue Date: 13-Jun-2022

Expiration Date: 31-Jul-2024

Component Name	CERTIFIED VALUES			CAS#	Analyte Lot
	Concentration	Expanded Uncertainty			
acifluorfen	100.1 ± 0.5 µg/mL	050594-66-6	NT02057		
bentazon	100.1 ± 0.5 µg/mL	025057-89-0	RM19026		
chloramben	100.2 ± 0.5 µg/mL	000133-90-4	RM03672		
2,4-D	100.3 ± 0.5 µg/mL	000094-75-7	RM17172		
delepon	100.3 ± 0.5 µg/mL	000075-99-0	RM19654		
2,4-DB	100.2 ± 0.5 µg/mL	000094-82-6	RM02866		
tetrachloroterephthalic acid	100.2 ± 0.5 µg/mL	002136-79-0	RM13887		
dicamba	100.3 ± 0.5 µg/mL	001918-00-9	RM15881		
3,5-dichlorobenzoic acid	100.2 ± 0.5 µg/mL	000051-36-5	RM02768		
dichlorprop	100.2 ± 0.5 µg/mL	000120-36-5	RM19240		
diuron	100.3 ± 0.5 µg/mL	000088-85-7	RM19863		
MCPA	10030 ± 50 µg/mL	000094-74-6	RM12220		
MCPP (mecoprop)	10026 ± 50 µg/mL	000093-65-2	RM09273		
4-nitrophenol	100.3 ± 0.5 µg/mL	000100-02-7	RM03752		
pentachlorophenol	100.2 ± 0.5 µg/mL	000087-86-5	RM02474		
picloram	100.2 ± 0.5 µg/mL	001918-02-1	RM19110		
silvex	100.2 ± 0.5 µg/mL	000093-72-1	RM19595		
2,4,5-T	100.3 ± 0.5 µg/mL	000093-76-5	NT01808		

Matrix: methanol (methyl alcohol)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.


Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:



Monica Bourgeois
QMS Representative



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32049 **Lot No.:** A0184439
Description : 2,4-Dichlorophenylacetic Acid Standard
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : January 31, 2025 **Storage:** 10°C or colder
Handling: This product is photosensitive. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.3 µg/mL	+/- 1.1813 µg/mL Gravimetric +/- 10.6525 µg/mL Unstressed +/- 10.6704 µg/mL Stressed

Solvent: Methanol
CAS # 67-56-1
Purity 99%

P12047

↓

P12076

AJ

08/09/22

Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

Column:
150mm x 4.6mm
Allure C18 Cat. (#9164565)


Flow Rate:
1.0 ml/min.

Mobile Phase A:
0.14% H₃PO₄ in water

Mobile Phase B:
acetonitrile

Mobile Phase Composition:
90%B Isocratic

Det. Type:
Wavelength: 220 & 254 nm

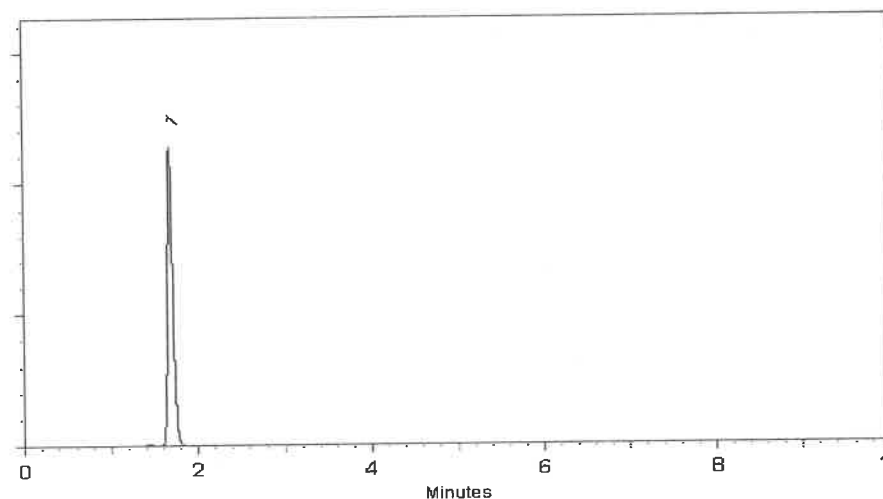


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Whitney Bennett - Operation Tech I

Date Mixed: 24-Apr-2022

Balance: 1128342314


Date Passed: 26-Apr-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32049 **Lot No.:** A0184439
Description : 2,4-Dichlorophenylacetic Acid Standard
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : January 31, 2025 **Storage:** 10°C or colder
Handling: This product is photosensitive. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.3 µg/mL	+/- 1.1813 µg/mL Gravimetric +/- 10.6525 µg/mL Unstressed +/- 10.6704 µg/mL Stressed

Solvent: Methanol
CAS # 67-56-1
Purity 99%

P12047

↓

P12076

AJ
08/09/22

Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

Column:
150mm x 4.6mm
Allure C18 Cat. (#9164565)


Flow Rate:
1.0 ml/min.

Mobile Phase A:
0.14% H₃PO₄ in water

Mobile Phase B:
acetonitrile

Mobile Phase Composition:
90%B Isocratic

Det. Type:
Wavelength: 220 & 254 nm

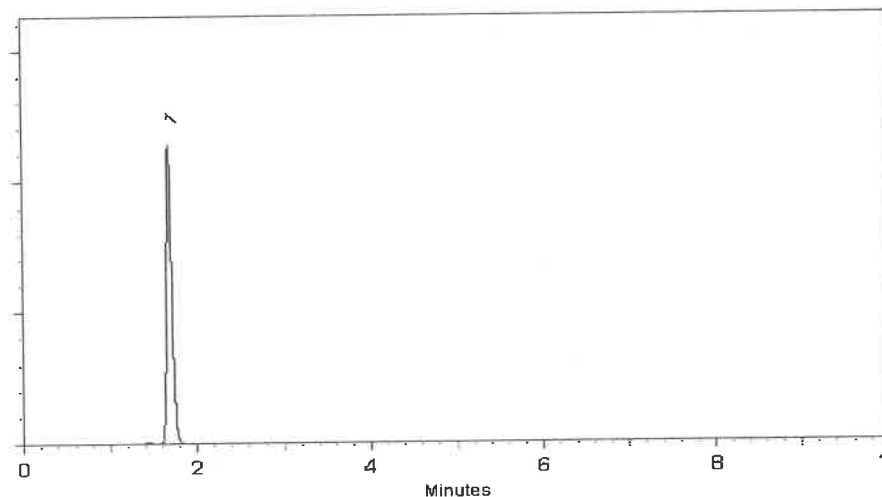


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Whitney Bennett - Operation Tech I

Date Mixed: 24-Apr-2022

Balance: 1128342314


Date Passed: 26-Apr-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32049 **Lot No.:** A0184439
Description : 2,4-Dichlorophenylacetic Acid Standard
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : January 31, 2025 **Storage:** 10°C or colder
Handling: This product is photosensitive. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.3 µg/mL	+/- 1.1813 µg/mL Gravimetric +/- 10.6525 µg/mL Unstressed +/- 10.6704 µg/mL Stressed

Solvent: Methanol
CAS # 67-56-1
Purity 99%

P12047

↓

P12076

AJ
08/09/22

Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

Column:
150mm x 4.6mm
Allure C18 Cat. (#9164565)


Flow Rate:
1.0 ml/min.

Mobile Phase A:
0.14% H₃PO₄ in water

Mobile Phase B:
acetonitrile

Mobile Phase Composition:
90%B Isocratic

Det. Type:
Wavelength: 220 & 254 nm

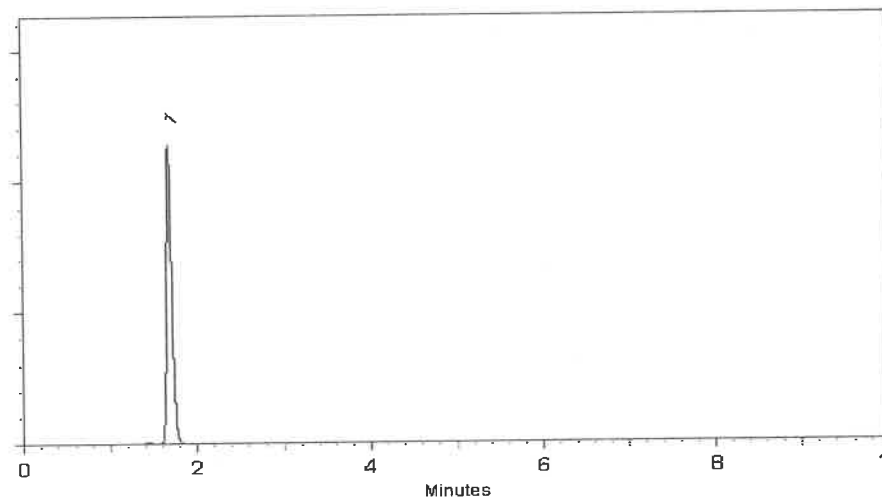


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Whitney Bennett - Operation Tech I

Date Mixed: 24-Apr-2022

Balance: 1128342314


Date Passed: 26-Apr-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32049 **Lot No.:** A0184439

Description : 2,4-Dichlorophenylacetic Acid Standard
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2025 **Storage:** 10°C or colder

Handling: This product is photosensitive. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.3 µg/mL	+/- 1.1813 µg/mL Gravimetric +/- 10.6525 µg/mL Unstressed +/- 10.6704 µg/mL Stressed

Solvent: Methanol
CAS # 67-56-1
Purity 99%

P12047

↓

P12076

AJ

08/09/22

Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

Column:
150mm x 4.6mm
Allure C18 Cat. (#9164565)


Flow Rate:
1.0 ml/min.

Mobile Phase A:
0.14% H₃PO₄ in water

Mobile Phase B:
acetonitrile

Mobile Phase Composition:
90%B Isocratic

Det. Type:
Wavelength: 220 & 254 nm

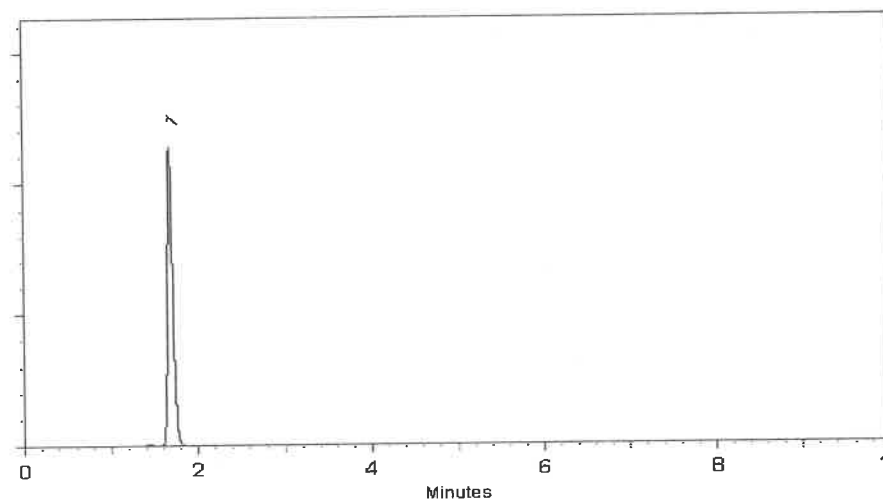

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Whitney Bennett - Operation Tech I

Date Mixed: 24-Apr-2022

Balance: 1128342314


Date Passed: 26-Apr-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32049 **Lot No.:** A0184439

Description : 2,4-Dichlorophenylacetic Acid Standard
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2025 **Storage:** 10°C or colder

Handling: This product is photosensitive. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.3 µg/mL	+/- 1.1813 µg/mL Gravimetric +/- 10.6525 µg/mL Unstressed +/- 10.6704 µg/mL Stressed

Solvent: Methanol
CAS # 67-56-1
Purity 99%

P12047

↓

P12076

AJ

08/09/22

Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

Column:
150mm x 4.6mm
Allure C18 Cat. (#9164565)


Flow Rate:
1.0 ml/min.

Mobile Phase A:
0.14% H₃PO₄ in water

Mobile Phase B:
acetonitrile

Mobile Phase Composition:
90%B Isocratic

Det. Type:
Wavelength: 220 & 254 nm

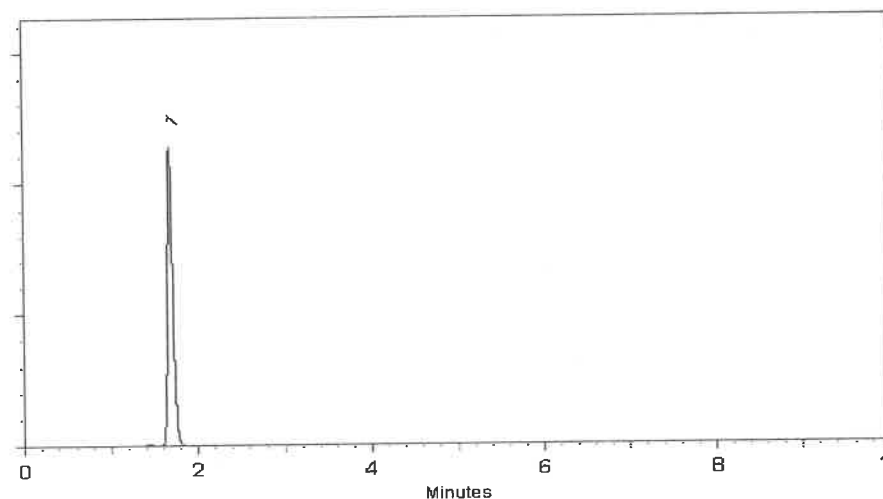


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Whitney Bennett - Operation Tech I

Date Mixed: 24-Apr-2022

Balance: 1128342314


Date Passed: 26-Apr-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32049 **Lot No.:** A0184439
Description : 2,4-Dichlorophenylacetic Acid Standard
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : January 31, 2025 **Storage:** 10°C or colder
Handling: This product is photosensitive. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.3 µg/mL	+/- 1.1813 µg/mL Gravimetric +/- 10.6525 µg/mL Unstressed +/- 10.6704 µg/mL Stressed

Solvent: Methanol
CAS # 67-56-1
Purity 99%

P12047

↓

P12076

AJ

08/09/22

Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

Column:
150mm x 4.6mm
Allure C18 Cat.(#9164565)


Flow Rate:
1.0 ml/min.

Mobile Phase A:
0.14% H₃PO₄ in water

Mobile Phase B:
acetonitrile

Mobile Phase Composition:
90%B Isocratic

Det. Type:
Wavelength: 220 & 254 nm

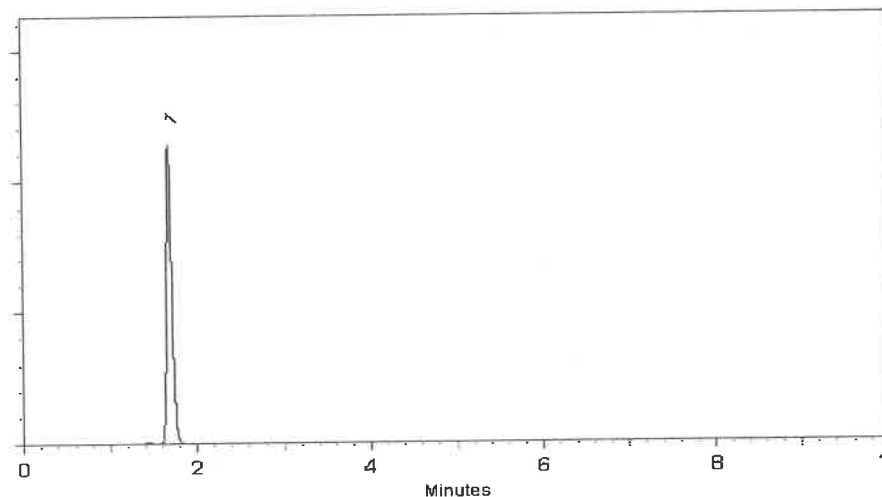


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Whitney Bennett - Operation Tech I

Date Mixed: 24-Apr-2022

Balance: 1128342314


Date Passed: 26-Apr-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32049 **Lot No.:** A0184439
Description : 2,4-Dichlorophenylacetic Acid Standard
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : January 31, 2025 **Storage:** 10°C or colder
Handling: This product is photosensitive. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.: K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.3 µg/mL	+/- 1.1813 µg/mL Gravimetric +/- 10.6525 µg/mL Unstressed +/- 10.6704 µg/mL Stressed

Solvent: Methanol
CAS # 67-56-1
Purity 99%

P12047

↓

P12076

AJ

08/09/22

Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

Column:
150mm x 4.6mm
Allure C18 Cat.(#9164565)


Flow Rate:
1.0 ml/min.

Mobile Phase A:
0.14% H₃PO₄ in water

Mobile Phase B:
acetonitrile

Mobile Phase Composition:
90%B Isocratic

Det. Type:
Wavelength: 220 & 254 nm

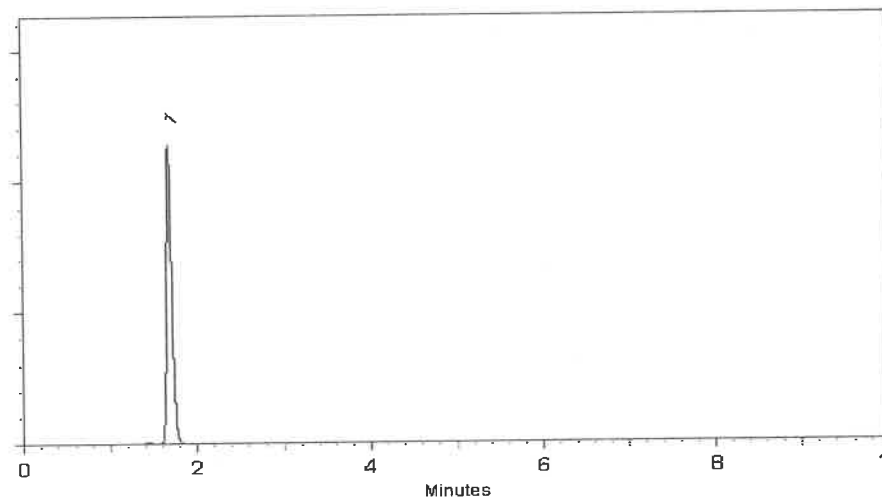


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Whitney Bennett - Operation Tech I

Date Mixed: 24-Apr-2022

Balance: 1128342314


Date Passed: 26-Apr-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32049 **Lot No.:** A0184439
Description : 2,4-Dichlorophenylacetic Acid Standard
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : January 31, 2025 **Storage:** 10°C or colder
Handling: This product is photosensitive. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.3 µg/mL	+/- 1.1813 µg/mL Gravimetric +/- 10.6525 µg/mL Unstressed +/- 10.6704 µg/mL Stressed

Solvent: Methanol
CAS # 67-56-1
Purity 99%

P12047

↓

P12076

AJ

08/09/22

Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

Column:
150mm x 4.6mm
Allure C18 Cat. (#9164565)


Flow Rate:
1.0 ml/min.

Mobile Phase A:
0.14% H₃PO₄ in water

Mobile Phase B:
acetonitrile

Mobile Phase Composition:
90%B Isocratic

Det. Type:
Wavelength: 220 & 254 nm

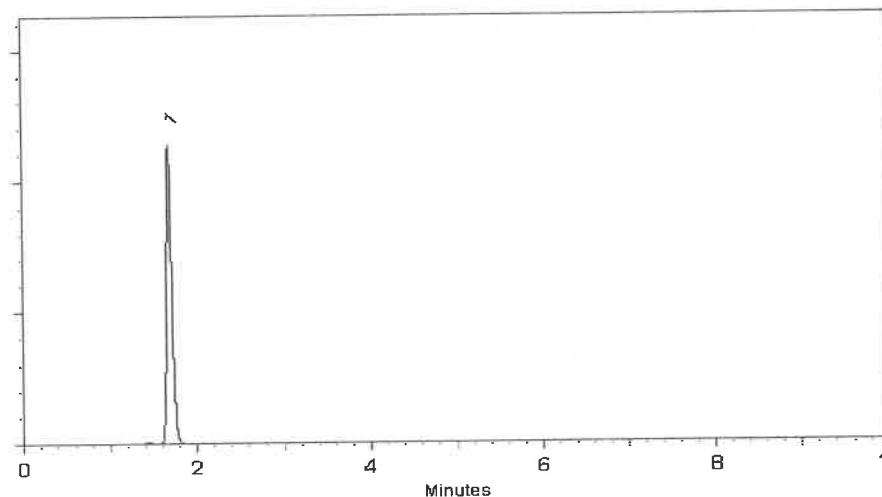


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Whitney Bennett - Operation Tech I

Date Mixed: 24-Apr-2022

Balance: 1128342314


Date Passed: 26-Apr-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32049 **Lot No.:** A0184439

Description : 2,4-Dichlorophenylacetic Acid Standard
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2025 **Storage:** 10°C or colder

Handling: This product is photosensitive. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.3 µg/mL	+/- 1.1813 µg/mL Gravimetric +/- 10.6525 µg/mL Unstressed +/- 10.6704 µg/mL Stressed

Solvent: Methanol
CAS # 67-56-1
Purity 99%

P12047

↓

P12076

AJ

08/09/22

Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

Column:
150mm x 4.6mm
Allure C18 Cat. (#9164565)


Flow Rate:
1.0 ml/min.

Mobile Phase A:
0.14% H₃PO₄ in water

Mobile Phase B:
acetonitrile

Mobile Phase Composition:
90%B Isocratic

Det. Type:
Wavelength: 220 & 254 nm

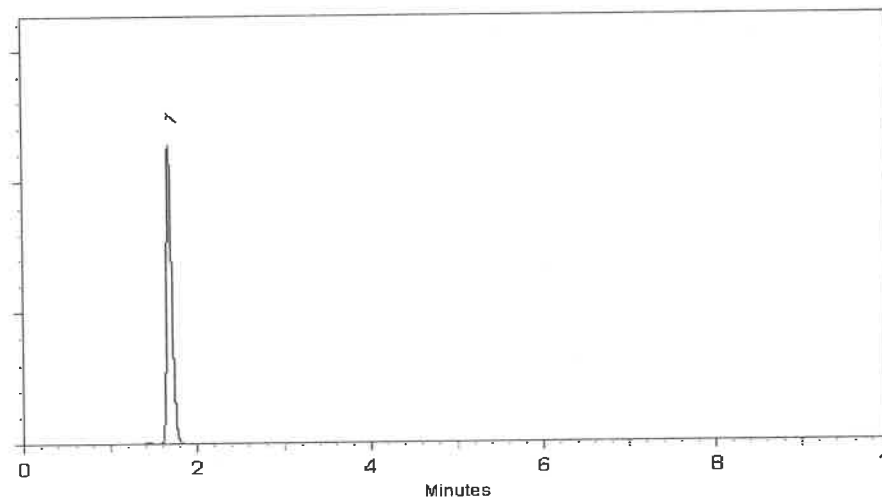


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Whitney Bennett - Operation Tech I

Date Mixed: 24-Apr-2022

Balance: 1128342314


Date Passed: 26-Apr-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32049 **Lot No.:** A0184439
Description : 2,4-Dichlorophenylacetic Acid Standard
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : January 31, 2025 **Storage:** 10°C or colder
Handling: This product is photosensitive. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.3 µg/mL	+/- 1.1813 µg/mL Gravimetric +/- 10.6525 µg/mL Unstressed +/- 10.6704 µg/mL Stressed

Solvent: Methanol
CAS # 67-56-1
Purity 99%

P12047

↓

P12076

AJ
08/09/22

Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

Column:
150mm x 4.6mm
Allure C18 Cat. (#9164565)


Flow Rate:
1.0 ml/min.

Mobile Phase A:
0.14% H₃PO₄ in water

Mobile Phase B:
acetonitrile

Mobile Phase Composition:
90%B Isocratic

Det. Type:
Wavelength: 220 & 254 nm

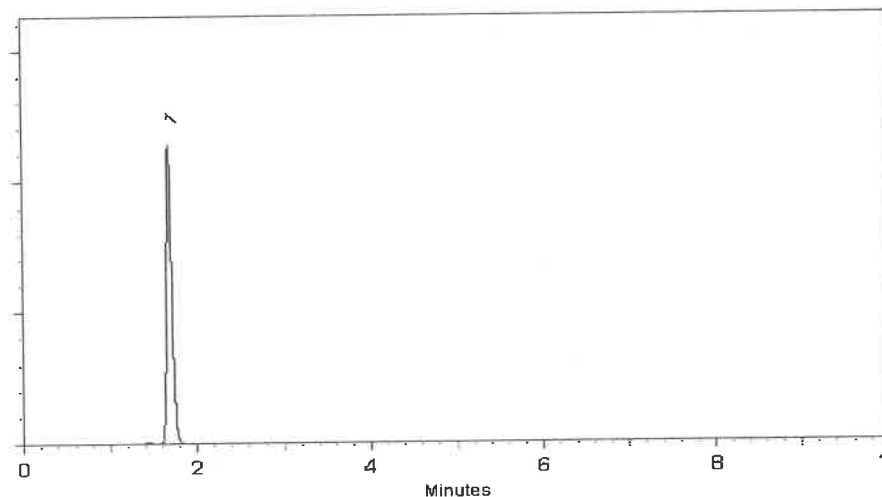


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Whitney Bennett - Operation Tech I

Date Mixed: 24-Apr-2022

Balance: 1128342314


Date Passed: 26-Apr-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32050 Lot No.: A0152705
Description : 2,4-Dichlorophenylacetic Acid Methyl Ester Standard
515 Surrogate (ester) 2, 4-dichlorophenyl Acetic Acid Methyl Ester
200µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : June 30, 2026 Storage: 10°C or colder
Handling: This product is photosensitive.

Received by
SG on 10/11/19
P8999
-
P9008

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)			
1	2,4-Dichlorophenyl acetic acid methyl ester	200.0 µg/mL	+/- 1.4182	µg/mL	Gravimetric	
	CAS # 55954-23-9 (Lot CSC42194-01)		+/- 6.7507	µg/mL	Unstressed	
	Purity 99%		+/- 6.7507	µg/mL	Stressed	

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

330°C

Det. Type:

FID

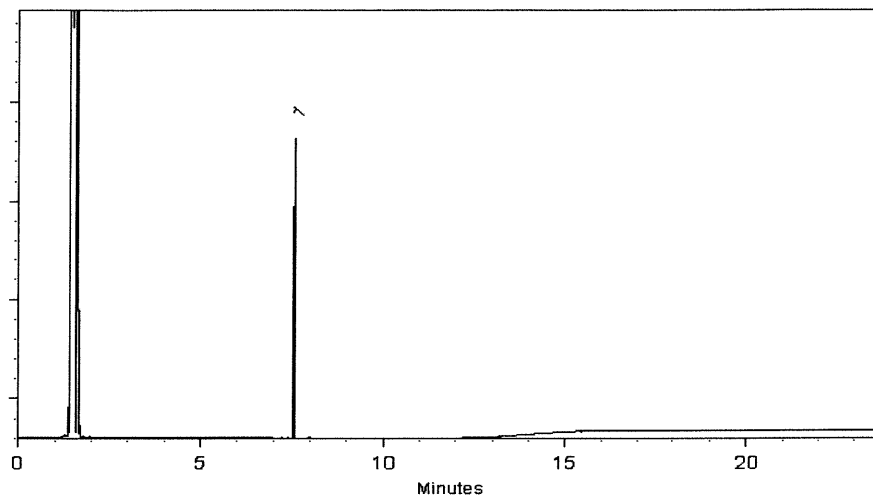

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Cydnei L. Crust
Cydnei L. Crust - Mix Technician

Date Mixed: 09-Sep-2019

Balance: B707717271

Fang-Yun Lo
Fang-Yun Lo - GC Analyst

Date Passed: 11-Sep-2019

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397