



## Prep Standard - Chemical Standard Summary

**Order ID :** O2213

**Test :** TPH GC

**Prepbatch ID :** PB151919,

**Sequence ID/Qc Batch ID:** FG040823,

**Standard ID :**

EP2321,PP21568,PP21569,PP21661,PP21703,PP21824,PP21825,PP21826,PP21827,PP21828,

**Chemical ID :**

E3412,E3459,E3464,E3470,E3483,E3486,P11170,P11171,P11172,P11173,P11174,P11175,P11176,P11475,P11476,P11754,P11755,P11756,P11757,P11758,P11852,

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	<a href="#">EP2321</a>	03/31/2023	09/30/2023	RUPESHKUMAR SHAH	None	None	Rajesh Parikh
								03/31/2023

**FROM** 1.00000gram of E3412 = Final Quantity: 4000.000 gram

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
433	100/100 PPM DRO (Restek)	<a href="#">PP21568</a>	01/27/2023	07/19/2023	Yogesh Patel	None	None	Ankita Jodhani
								01/30/2023

**FROM** 1.25000ml of P11170 + 1.25000ml of P11171 + 1.25000ml of P11754 + 1.25000ml of P11755 + 1.25000ml of P11756 + 1.25000ml of P11757 + 17.50000ml of E3459 = Final Quantity: 25.000 ml

**284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900**

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3796	100/100 PPM DRO STD (CPI)	<a href="#">PP21569</a>	01/27/2023	07/19/2023	Yogesh Patel	None	None	Ankita Jodhani 01/30/2023
<u>FROM</u>	1.00000ml of P11172 + 1.00000ml of P11475 + 1.00000ml of P11476 + 7.00000ml of E3459 = Final Quantity: 10.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
147	20 PPM DRO Surrogate Spike Solution	<a href="#">PP21661</a>	02/16/2023	08/02/2023	Abdul Mirza	None	None	Sohil Jodhani 02/16/2023
<b><u>FROM</u></b> 1.00000ml of P11173 + 1.00000ml of P11174 + 1.00000ml of P11175 + 1.00000ml of P11176 + 196.00000ml of E3464 = Final Quantity: 200.000 ml								

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3609	20 PPM DRO SPIKE SOLUTION (RESTEK)	<a href="#">PP21703</a>	02/23/2023	08/22/2023	Yogesh Patel	None	None	Ankita Jodhani
02/24/2023								

**FROM** 1.00000ml of P11758 + 1.00000ml of P11852 + 48.00000ml of E3470 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
435	50 PPM ICC DRO STD (Restek)	<a href="#">PP21824</a>	03/15/2023	07/19/2023	Yogesh Patel	None	None	Ankita Jodhani
03/16/2023								

**FROM** 0.50000ml of E3483 + 0.50000ml of PP21568 = Final Quantity: 1.000 ml

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
437	20 PPM ICC DRO STD (Restek)	<a href="#">PP21825</a>	03/15/2023	07/19/2023	Yogesh Patel	None	None	Ankita Jodhani
03/16/2023								

**FROM** 0.80000ml of E3483 + 0.20000ml of PP21568 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
438	10 PPM ICC DRO STD (Restek)	<a href="#">PP21826</a>	03/15/2023	07/19/2023	Yogesh Patel	None	None	Ankita Jodhani
03/16/2023								

**FROM** 0.90000ml of E3483 + 0.10000ml of PP21568 = Final Quantity: 1.000 ml

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
439	5 PPM ICC DRO STD (Restek)	<a href="#">PP21827</a>	03/15/2023	07/19/2023	Yogesh Patel	None	None	Ankita Jodhani
03/16/2023								

**FROM** 0.90000ml of E3483 + 0.10000ml of PP21824 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3797	50 PPM DRO ICV STD (CPI)	<a href="#">PP21828</a>	03/15/2023	07/19/2023	Yogesh Patel	None	None	Ankita Jodhani
03/16/2023								

**FROM** 0.50000ml of E3483 + 0.50000ml of PP21569 = Final Quantity: 1.000 ml

**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	139404	10/23/2023	10/18/2022 / Rajesh	10/13/2022 / Rajesh	E3412

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	22J1962006	07/19/2023	01/19/2023 / Rajesh	12/19/2022 / Rajesh	E3459

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	22L0562002	08/02/2023	02/02/2023 / Rajesh	01/24/2023 / Rajesh	E3464

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	22L0562002	08/22/2023	02/22/2023 / Rajesh	01/24/2023 / Rajesh	E3470

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	23A0362012	11/08/2023	03/08/2023 / Rajesh	02/28/2023 / Rajesh	E3483

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	23A0362012	09/22/2023	03/22/2023 / Rajesh	02/28/2023 / Rajesh	E3486

**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	07/27/2023	01/27/2023 / yogesh	10/29/2021 / Abdul	P11170

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	07/27/2023	01/27/2023 / yogesh	10/29/2021 / Abdul	P11171

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	07/27/2023	01/27/2023 / yogesh	10/29/2021 / Abdul	P11172

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	08/16/2023	02/16/2023 / Abdul	10/29/2021 / Abdul	P11173

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	08/16/2023	02/16/2023 / Abdul	10/29/2021 / Abdul	P11174

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	08/16/2023	02/16/2023 / Abdul	10/29/2021 / Abdul	P11175



**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	08/16/2023	02/16/2023 / Abdul	10/29/2021 / Abdul	P11176

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110400-05-01 / TRPH Standard (C8-C40), 500 mg/L, 1 ml	472647	07/27/2023	01/27/2023 / yogesh	02/10/2022 / Yogesh	P11475

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110400-05-01 / TRPH Standard (C8-C40), 500 mg/L, 1 ml	472647	07/27/2023	01/27/2023 / yogesh	02/10/2022 / Yogesh	P11476

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0181886	07/27/2023	01/27/2023 / yogesh	05/27/2022 / Sohil	P11754

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0181886	07/27/2023	01/27/2023 / yogesh	05/27/2022 / Sohil	P11755

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0181886	07/27/2023	01/27/2023 / yogesh	05/27/2022 / Sohil	P11756



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0181886	07/27/2023	01/27/2023 / yogesh	05/27/2022 / Sohil	P11757

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0181886	08/23/2023	02/23/2023 / yogesh	05/27/2022 / Sohil	P11758

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0184585	08/23/2023	02/23/2023 / yogesh	06/17/2022 / Yogesh	P11852



5580 Skylane Blvd  
Santa Rosa, CA 95403  
(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.: Lot No.: Storage:

Z-110400 472647  $\leq -10^{\circ}\text{C}$   
-05-01

Solvent:

Hexane

Exp. Date:

11/18/2023

Description:

TRPH Standard (C8-C40), 500 mg/L, 10 x 1 ml

-10PAK	Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
decane (C10)		124-18-5	99.5	415.7.1P	500.2 $\pm$ 2.29
docosane (C22)		629-97-0	99	420.1.1P	502.4 $\pm$ 5.5
dodecane (C12)		112-40-3	99.2	416.7.1P	500.7 $\pm$ 2.29
dotriacontane (C32)		544-85-4	98	425.29.2P	499.8 $\pm$ 5.47
eicosane (C20)		112-95-8	98.9	419.29.1P	505.1 $\pm$ 2.31
hexacosane (C26)		630-01-3	99.3	422.7.2P	500 $\pm$ 2.29
hexatriacontane (C36)		630-06-8	98	427.29.1P	500.3 $\pm$ 5.48
n-hexadecane (C16)		544-76-3	99.45	368.271.1P	499.6 $\pm$ 2.23
octacosane (C28)		630-02-4	98.7	423.400.1P	498.3 $\pm$ 5.45
n-octadecane (C18)		593-45-3	99.5	418.29.1P	501.9 $\pm$ 2.24
octane (C8)		111-65-9	99.5	385.9.1P	499.8 $\pm$ 2.23
octatriacontane (C38)		7194-85-6	99	428.7.1P	499.8 $\pm$ 2.29
tetracontane (C40)		4181-95-7	100	429.7.1P	504.1 $\pm$ 5.52
n-tetradecane (C14)		629-59-4	99	417.29.4P	500.4 $\pm$ 5.48
tetratriacontane (C34)		14167-59-0	98.1	426.7.2P	499.6 $\pm$ 2.28
triacontane (C30)		638-68-6	99.5	424.7.1.1P	499.9 $\pm$ 2.29
tetracosane (C24)		646-31-1	99	421.1.1P	500.1 $\pm$ 5.47

P11469  
J  
P11488  
Y.P.  
02/12/22

Let the standard warm to room temperature and sonicate before opening.

\*Not a certified value

Certified By: \_\_\_\_\_

Jarrett Howard  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.





5580 Skylane Blvd  
Santa Rosa, CA 95403  
(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.: Lot No.: Storage:

Z-110400 472647  $\leq -10^{\circ}\text{C}$   
-05-01

Solvent:

Hexane

Exp. Date:

11/18/2023

Description:

TRPH Standard (C8-C40), 500 mg/L, 10 x 1 ml

-10PAK	Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
decane (C10)		124-18-5	99.5	415.7.1P	500.2 $\pm$ 2.29
docosane (C22)		629-97-0	99	420.1.1P	502.4 $\pm$ 5.5
dodecane (C12)		112-40-3	99.2	416.7.1P	500.7 $\pm$ 2.29
dotriacontane (C32)		544-85-4	98	425.29.2P	499.8 $\pm$ 5.47
eicosane (C20)		112-95-8	98.9	419.29.1P	505.1 $\pm$ 2.31
hexacosane (C26)		630-01-3	99.3	422.7.2P	500 $\pm$ 2.29
hexatriacontane (C36)		630-06-8	98	427.29.1P	500.3 $\pm$ 5.48
n-hexadecane (C16)		544-76-3	99.45	368.271.1P	499.6 $\pm$ 2.23
octacosane (C28)		630-02-4	98.7	423.400.1P	498.3 $\pm$ 5.45
n-octadecane (C18)		593-45-3	99.5	418.29.1P	501.9 $\pm$ 2.24
octane (C8)		111-65-9	99.5	385.9.1P	499.8 $\pm$ 2.23
octatriacontane (C38)		7194-85-6	99	428.7.1P	499.8 $\pm$ 2.29
tetracontane (C40)		4181-95-7	100	429.7.1P	504.1 $\pm$ 5.52
n-tetradecane (C14)		629-59-4	99	417.29.4P	500.4 $\pm$ 5.48
tetratriacontane (C34)		14167-59-0	98.1	426.7.2P	499.6 $\pm$ 2.28
triacontane (C30)		638-68-6	99.5	424.7.1.1P	499.9 $\pm$ 2.29
tetracosane (C24)		646-31-1	99	421.1.1P	500.1 $\pm$ 5.47

P11469  
J  
P11488  
Y.P.  
02/12/22

Let the standard warm to room temperature and sonicate before opening.

\*Not a certified value

Certified By: \_\_\_\_\_

Jarrett Howard  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.






**PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.**



MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MÉXICO  
CP 64070  
TEL +52 81 13 52 57 57  
www.pqm.com.mx

# CERTIFICATE OF ANALYSIS

**PRODUCT :** SODIUM SULFATE CRYSTALS ANHYDROUS  
**QUALITY :** ACS (CODE RMB3375) **FORMULA :** Na<sub>2</sub>SO<sub>4</sub>  
**SPECIFICATION NUMBER :** 6399 **RELEASE DATE:** OCT/28/2021  
**LOT NUMBER :** 139404

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na <sub>2</sub> SO <sub>4</sub> )	Min. 99.0%	99.8 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.0
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO <sub>4</sub> )	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.002 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.2 %
Retained on US Standard No. 60 sieve	Min. 94%	97.6 %
Through US Standard No. 60 sieve	Max. 5%	2.1 %
Through US Standard No. 100 sieve	Max. 10%	0.2 %
COMMENTS		
 QC: PhC Irma Belmares		

If you need further details, please call our factory or contact our local distributor.

E 3412

Recd. by RP on 10/13/22

RE-02-01, Ed. 3

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 22J1962006  
Manufactured Date: 2022-09-23  
Expiration Date: 2023-12-23  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	6
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8\%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0$ ppm	0.1 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10$ ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02\%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3459

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC  
100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700  
Page 1 of 1



Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 22L0562002  
Manufactured Date: 2022-10-20  
Expiration Date: 2024-01-19  
Revision No.: 0


## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	2
Assay (CH <sub>2</sub> Cl <sub>2</sub> ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0$ ppm	< 0.1 ppm
Titration Acid ( $\mu$ eq/g)	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10$ ppm	5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3464

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Page 1 of 1

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 22L0562002  
Manufactured Date: 2022-10-20  
Expiration Date: 2024-01-19  
Revision No.: 0


## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	2
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	< 0.1 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3470

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 23A0362012  
Manufactured Date: 2022-11-23  
Expiration Date: 2024-02-22  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	2
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	< 0.1 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3483

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 23A0362012  
Manufactured Date: 2022-11-23  
Expiration Date: 2024-02-22  
Revision No.: 0


## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	2
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	< 0.1 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3486

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

**CERTIFIED WEIGHT REPORT**

**Part Number:**  
Lot Number:  
Description:

**Solvent(s):**  
Methylene chloride  
**Lot#**  
104929

**72072**  
**091120**  
n-Tetracosane-d50

**Expiration Date:**  
**Recommended Storage:**  
**Nominal Concentration (µg/mL):**  
**NIST Test ID#:**


091130  
Ambient (20 °C)  
1000  
23060

**Weight(s) shown below were combined and diluted to (mL):**  
5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LDSO
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	----------------------------------	--	----------------	------

1. n-Tetracosane-d50 2072 PR-26606 1000 98.7 0.2 99.0 0.20471 0.20481 1000.5 4.1 16416-32-3 N/A N/A

**Method GCMSD-3.M:** Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

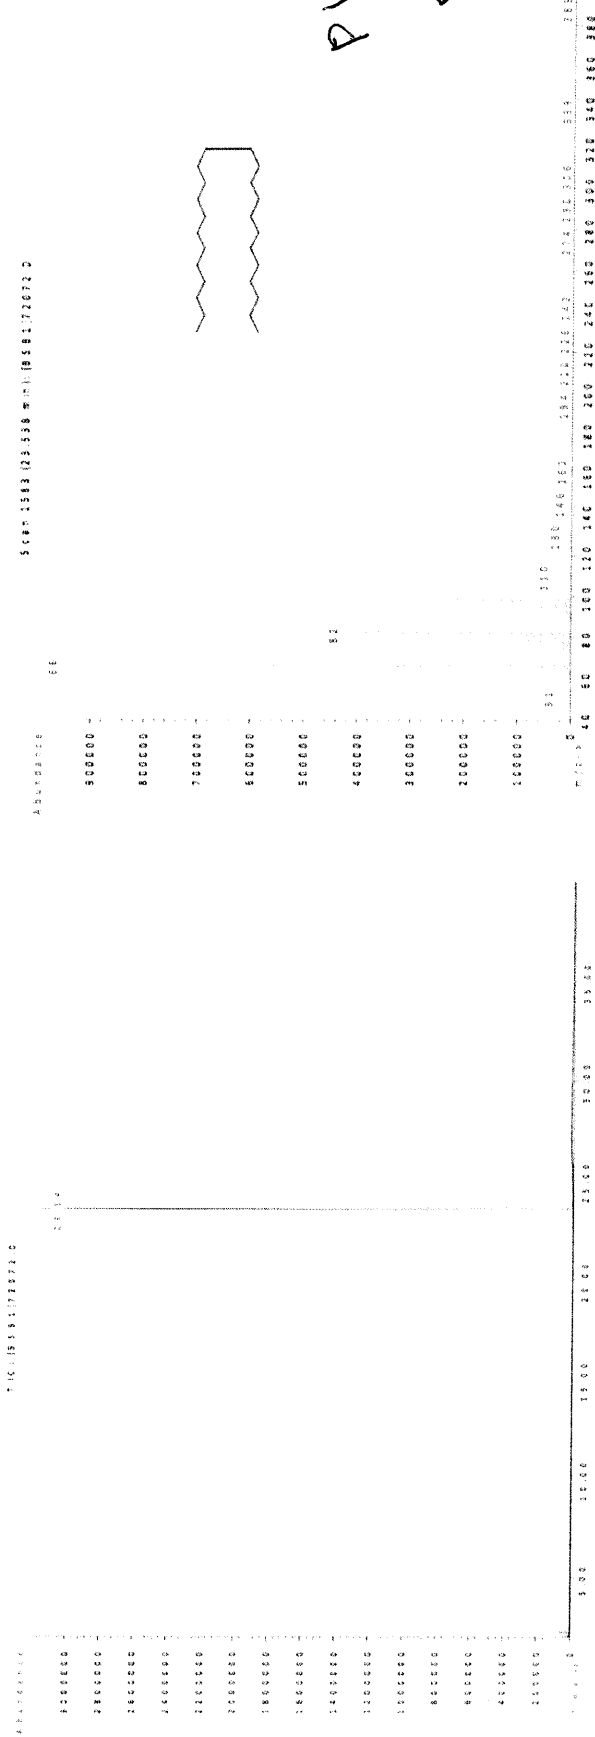

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
Standards are certified (±) 0.5% of the stated value, unless otherwise stated.  
All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




**Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"**


Run Length: 35.00 min, 20999 points at 10 points/second.  
Created: Thu, Sep 17, 2020 at 9:46:03 AM.  
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".  
Analyzed using Method "GC4-M1".

**Comments**

GC4-M1 Analysis by Candice Warren  
Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness  
Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,  
Air (detector) = 360 mL  
Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.  
Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.  
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

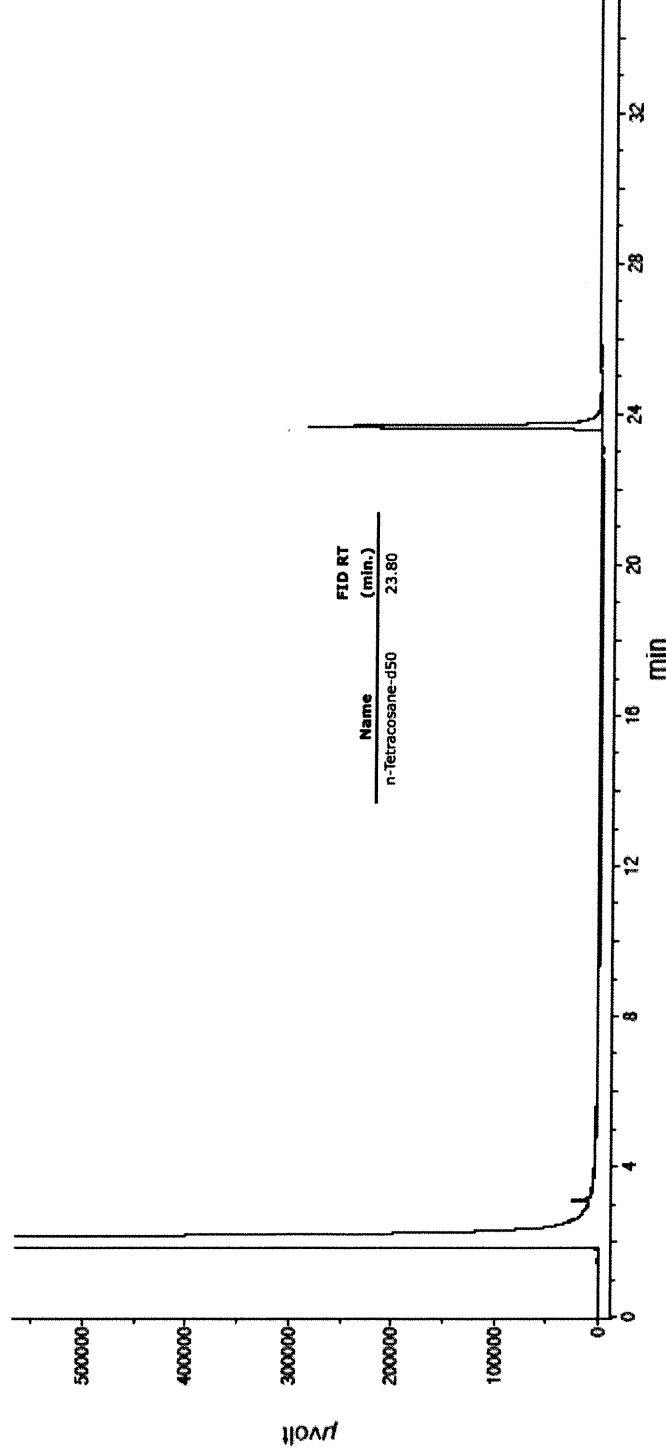

P11176  
 11/02/21  
 12



**CERTIFIED WEIGHT REPORT**

**Part Number:**  
Lot Number:  
Description:

**Solvent(s):**  
Methylene chloride

<b>Formulated By:</b>	<b>DATE</b>
Benson Chan	091120
<b>Reviewed By:</b>	<b>DATE</b>
Pedro L. Rentas	091120

**Expiration Date:**  
**Recommended Storage:**  
**Nominal Concentration (µg/mL):**  
**NIST Test ID#:**


**Weight(s) shown below were combined and diluted to (mL):**

5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LDSO
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	----------------------------------	--	----------------	------

1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20481	1000.5	4.1	16416-32-3	N/A	N/A
----------------------	------	----------	------	------	-----	------	---------	---------	--------	-----	------------	-----	-----

**Method GCMSD-3.M:** Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

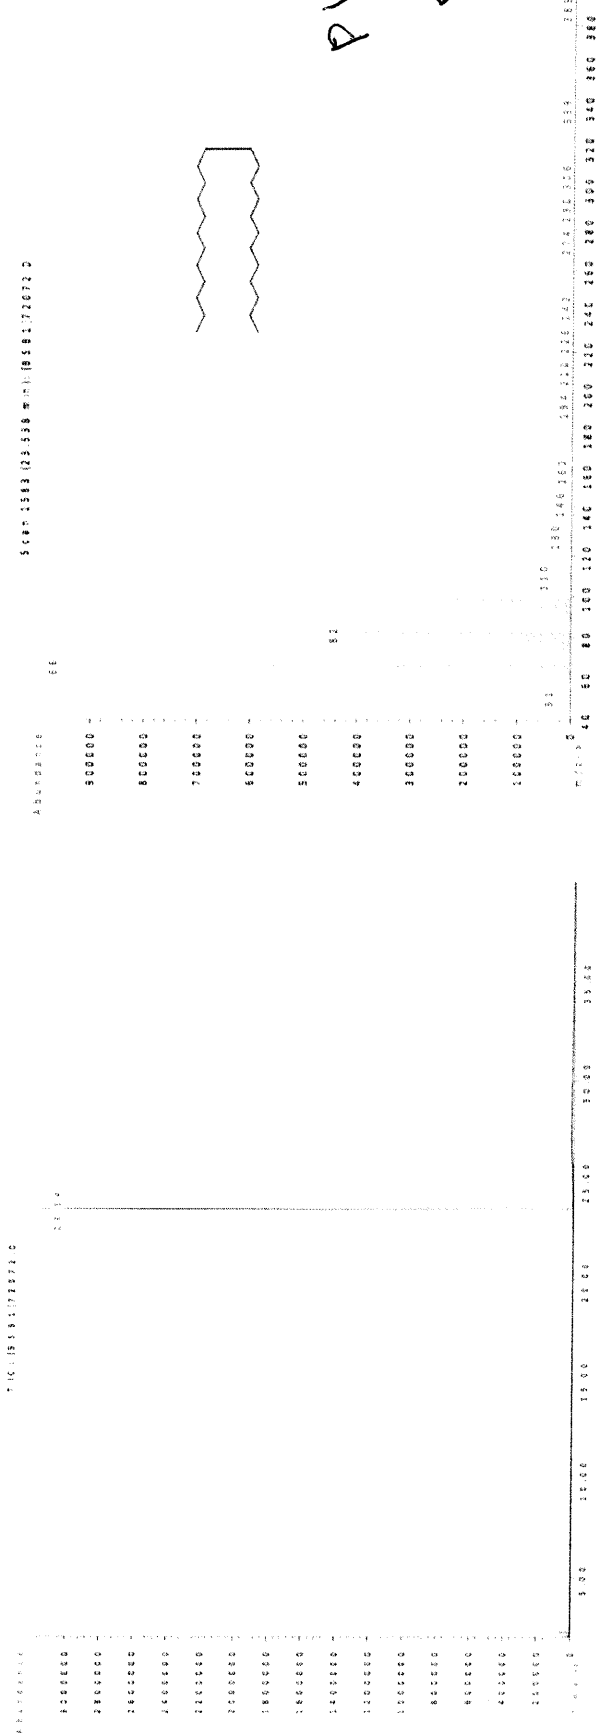

• The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
• Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
• Standards are certified (±) 0.5% of the stated value, unless otherwise stated.  
• All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
• Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



**Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"**

Run Length: 35.00 min, 20999 points at 10 points/second.

Created: Thu, Sep 17, 2020 at 9:46:03 AM.

Sampled: Sequence "091420-GC4M2", Method "GC4-M1".

Analyzed using Method "GC4-M1".

**Comments**

GC4-M1 Analysis by Candice Warren

Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness


Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,

Air (detector) = 360 mL

Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.

Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.

Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

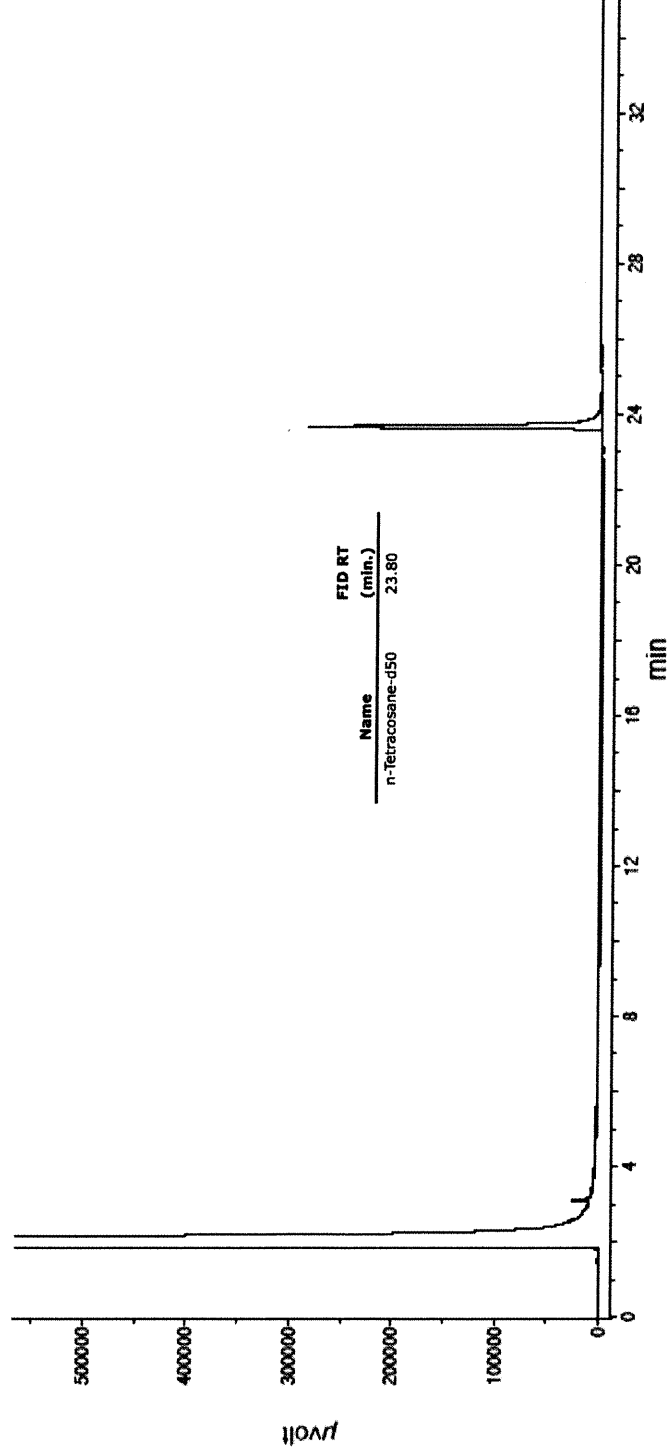

P11147  
 P11176  
 11/02/21



**CERTIFIED WEIGHT REPORT**

**Part Number:**  
Lot Number:  
Description:

**Solvent(s):**  
Methylene chloride

<b>Formulated By:</b>	<b>DATE</b>
Benson Chan	091120
<b>Reviewed By:</b>	<b>DATE</b>
Pedro L. Rentas	091120


**Expiration Date:**  
**Recommended Storage:**  
**Nominal Concentration (µg/mL):**  
**NIST Test ID#:**

**Weight(s)** shown below were combined and diluted to (mL):

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LDSO
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	----------------------------------	--	----------------	------

1. n-Tetracosane-d50 2072 PR-26606 1000 98.7 0.2 99.0 0.20471 0.20481 1000.5 4.1 16416-32-3 N/A

**Method GCMSD-3.M:** Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

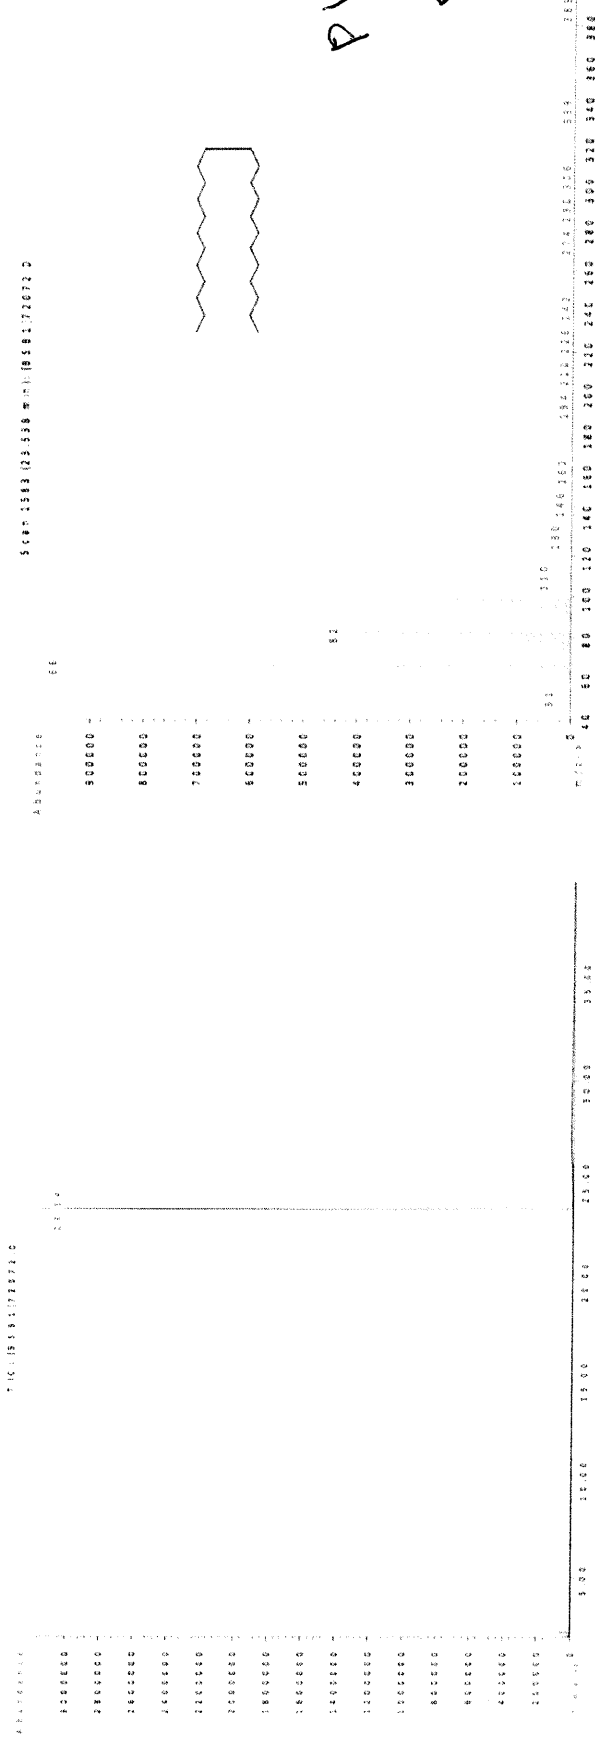

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
Standards are certified (±) 0.5% of the stated value, unless otherwise stated.  
All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




# **Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"**

Run Length: 35.00 min, 20999 points at 10 points/second.  
Created: Thu, Sep 17, 2020 at 9:46:03 AM.  
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".  
Analyzed using Method "GC4-M1".

## **Comments**

GC4-M1 Analysis by Candice Warren  
Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness  
Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,  
Air (detector) = 360 mL  
Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.  
Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.  
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

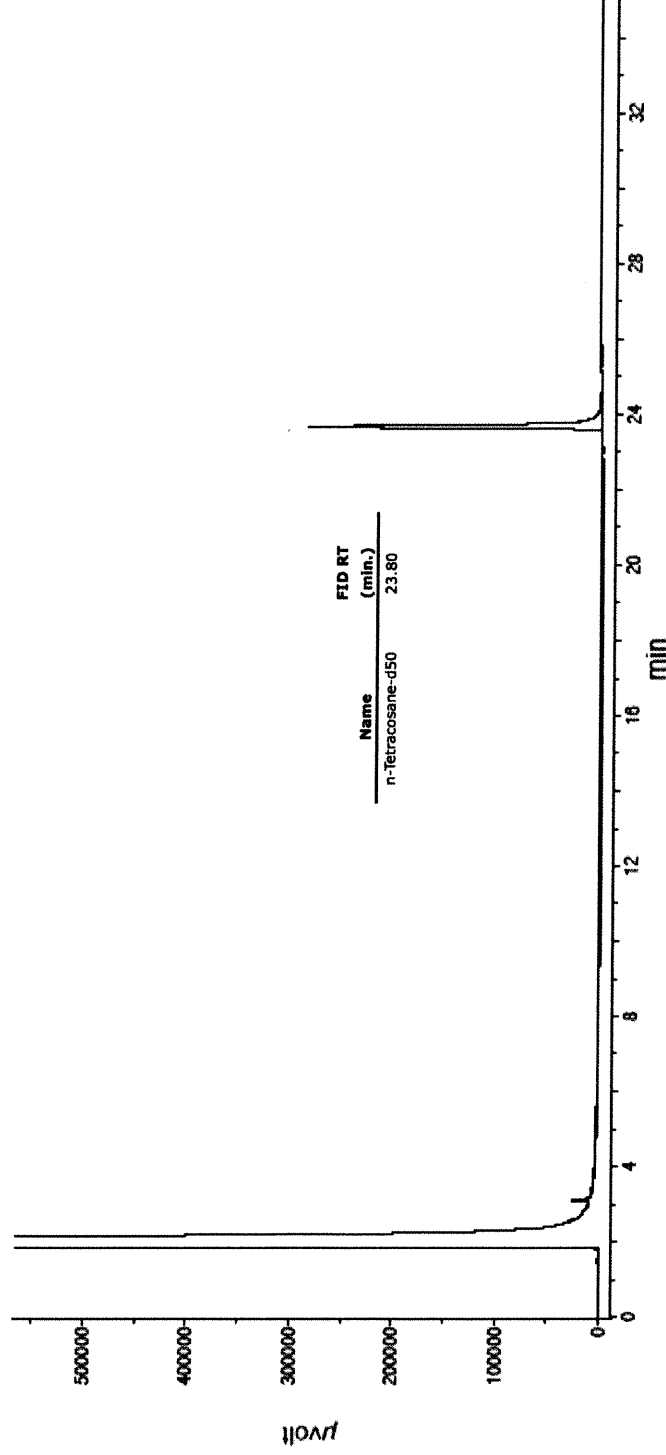

P11176  
 11/02/21  
 12

**CERTIFIED WEIGHT REPORT**

**Part Number:**  
Lot Number:  
Description:

**Solvent(s):**  
Methylene chloride

<b>72072</b>	<b>Lot#</b>
091120	104929
n-Tetracosane-d50	

**Expiration Date:**  
**Recommended Storage:**  
**Nominal Concentration (µg/mL):**  
**NIST Test ID#:**


091130  
Ambient (20 °C)  
1000  
23060

**Weight(s) shown below were combined and diluted to (mL):**  
5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LDSO
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	----------------------------------	--	----------------	------

1. n-Tetracosane-d50 2072 PR-26606 1000 98.7 0.2 99.0 0.20471 0.20481 1000.5 4.1 16416-32-3 N/A

**Method GCMSD-3.M:** Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

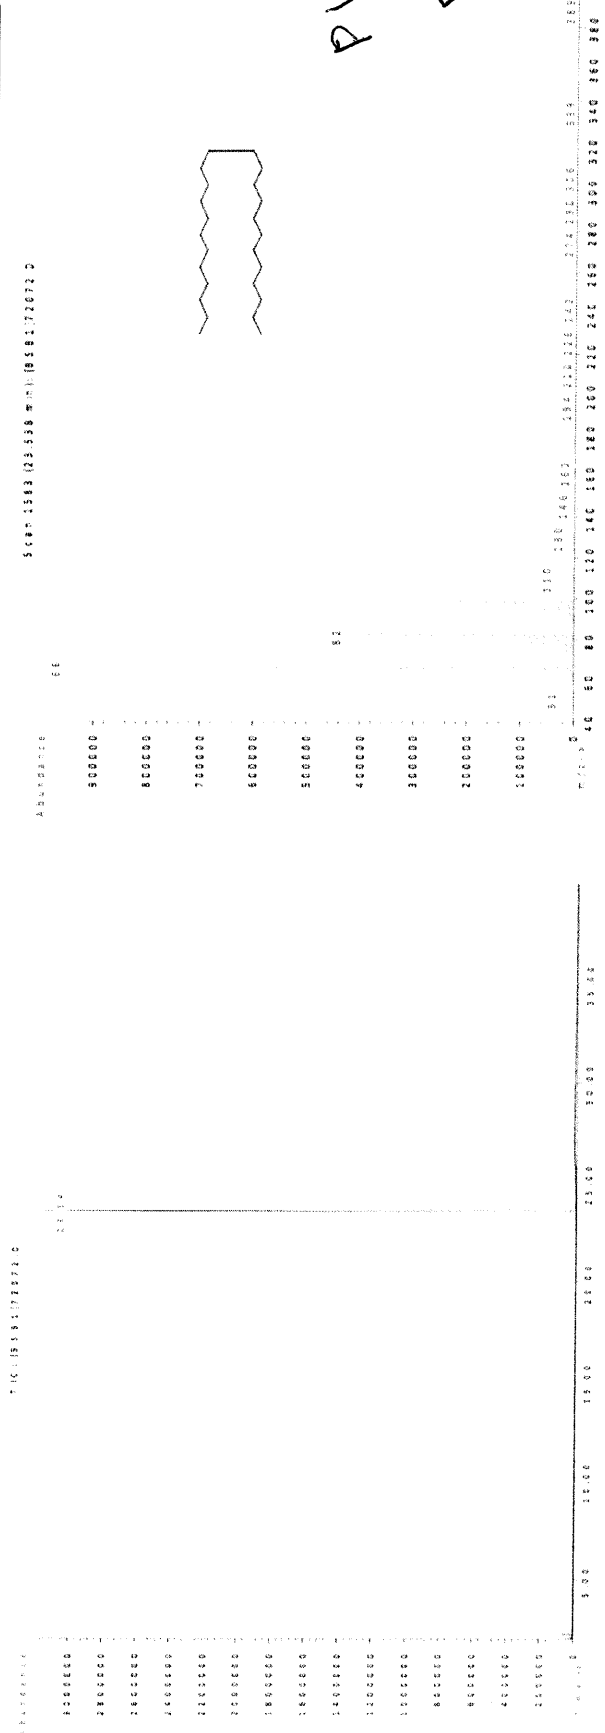

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
Standards are certified (±) 0.5% of the stated value, unless otherwise stated.  
All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

11/10/21  
AR  
P 111147  
P 111176




# **Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"**

Run Length: 35.00 min, 20999 points at 10 points/second.  
Created: Thu, Sep 17, 2020 at 9:46:03 AM.  
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".  
Analyzed using Method "GC4-M1".

## **Comments**

GC4-M1 Analysis by Candice Warren  
Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness  
Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,  
Air (detector) = 360 mL  
Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.  
Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.  
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

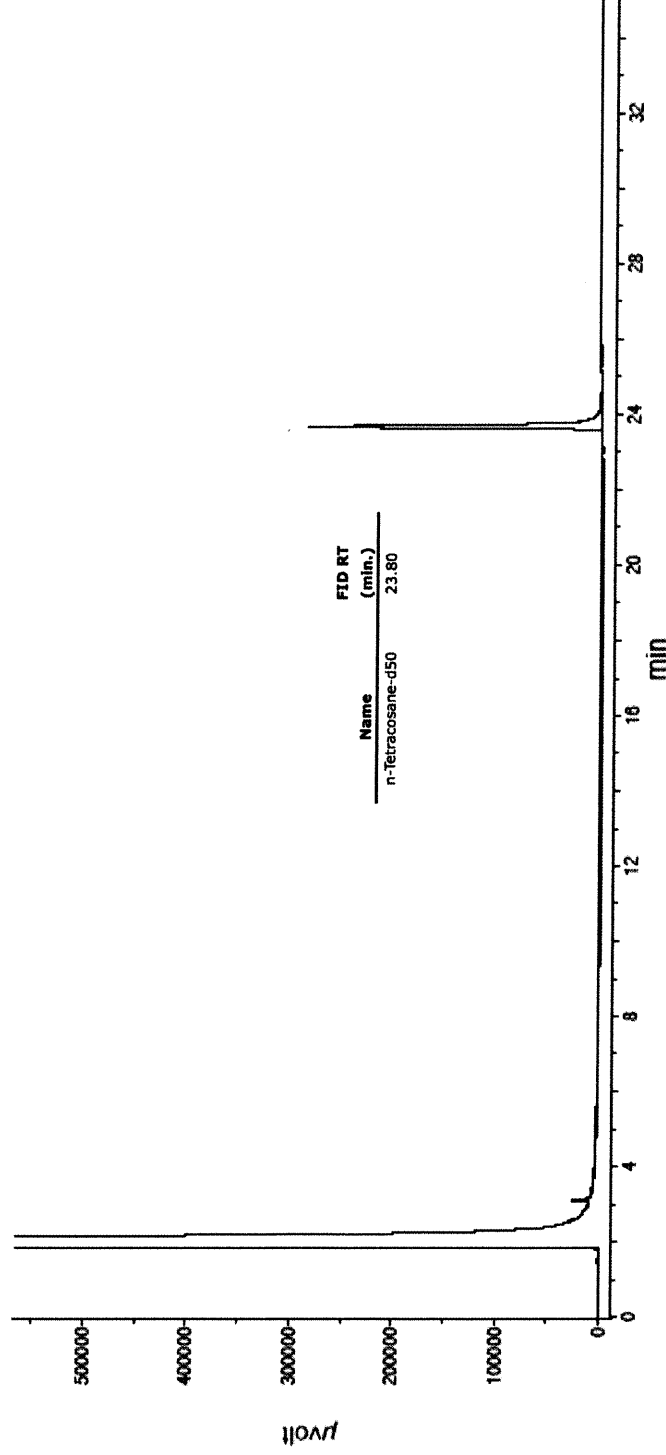

P11176  
 11/02/21  
 12

**CERTIFIED WEIGHT REPORT**

**Part Number:**  
 Lot Number:  
 Description:

**72072**  
**091120**  
**n-Tetracosane-d50**

**Solvent(s):**  
**Lot#**

**Methylene chloride**  
**104929**

**Expiration Date:**  
**Recommended Storage:**  
**Nominal Concentration (µg/mL):**  
**NIST Test ID#:**

**091130**  
**Ambient (20 °C)**  
**1000**  
**23060**

**Weight(s) shown below were combined and diluted to (mL):**

**200.0**  
**0.058**

**5E-05**  
**Balance Uncertainty**  
**0.058**  
**Flask Uncertainty**

**Formulated By:**  
**Reviewed By:**  
**DATE**

**Benson Chan**  
**Pedro L. Rentas**  
**091120**  
**091120**


**SDS Information**

**Expanded**  
**Uncertainty**  
**(+/-) (µg/mL)**  
**CAS#**  
**OSHA PEL (TWA)**  
**LDSO**

**4.1**  
**16416-32-3**  
**N/A**

**1. n-Tetracosane-d50**  
**2072**  
**PR-26606**  
**1000**  
**98.7**  
**0.2**  
**99.0**  
**0.20471**  
**0.20481**  
**1000.5**  
**4.1**  
**16416-32-3**  
**N/A**  
**N/A**

**Method GCMSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.**

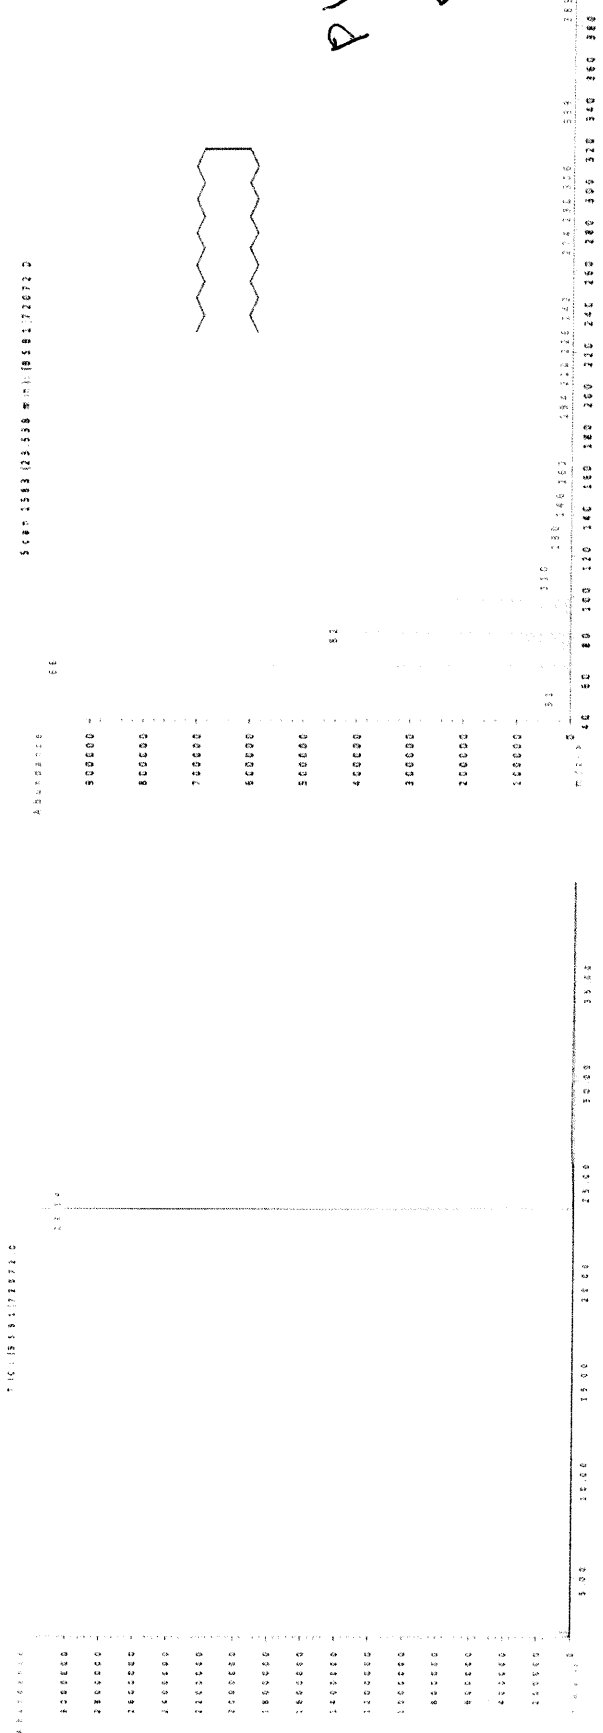

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
 Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
 Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.  
 All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
 Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




# **Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"**

Run Length: 35.00 min, 20999 points at 10 points/second.  
Created: Thu, Sep 17, 2020 at 9:46:03 AM.  
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".  
Analyzed using Method "GC4-M1".

## **Comments**

GC4-M1 Analysis by Candice Warren  
Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness  
Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,  
Air (detector) = 360 mL  
Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.  
Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.  
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

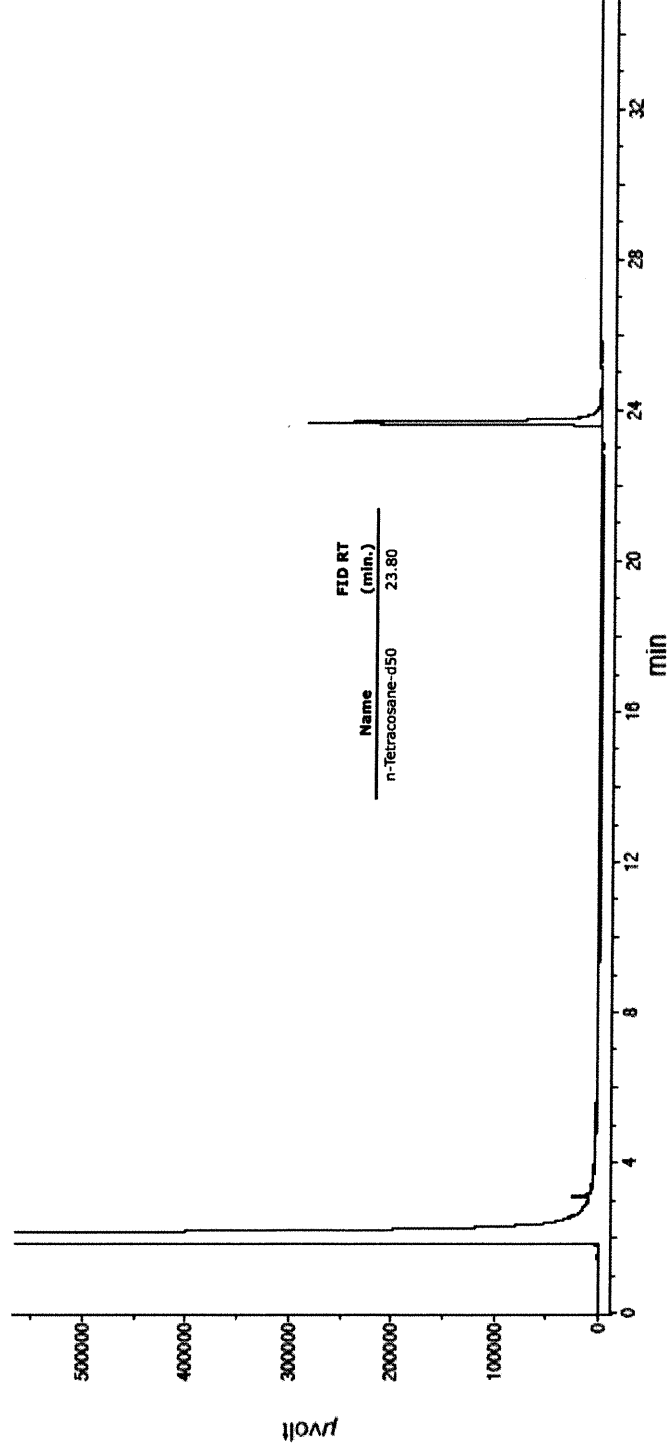

P1117b  
 P1117b  
 11/02/21

**CERTIFIED WEIGHT REPORT**

**Part Number:**  
Lot Number:  
Description:

**Solvent(s):**  
Methylene chloride  
**Lot#**  
104929

**72072**  
**091120**  
n-Tetracosane-d50

**Expiration Date:**  
**Recommended Storage:**  
**Nominal Concentration (µg/mL):**  
**NIST Test ID#:**


**091130**  
Ambient (20 °C)  
1000  
23060

**Weight(s) shown below were combined and diluted to (mL):**  
5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LDSO
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	----------------------------------	--	----------------	------

1. n-Tetracosane-d50 2072 PR-26606 1000 98.7 0.2 99.0 0.20471 0.20481 1000.5 4.1 16416-32-3 N/A N/A

**Method GCMSD-3.M:** Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

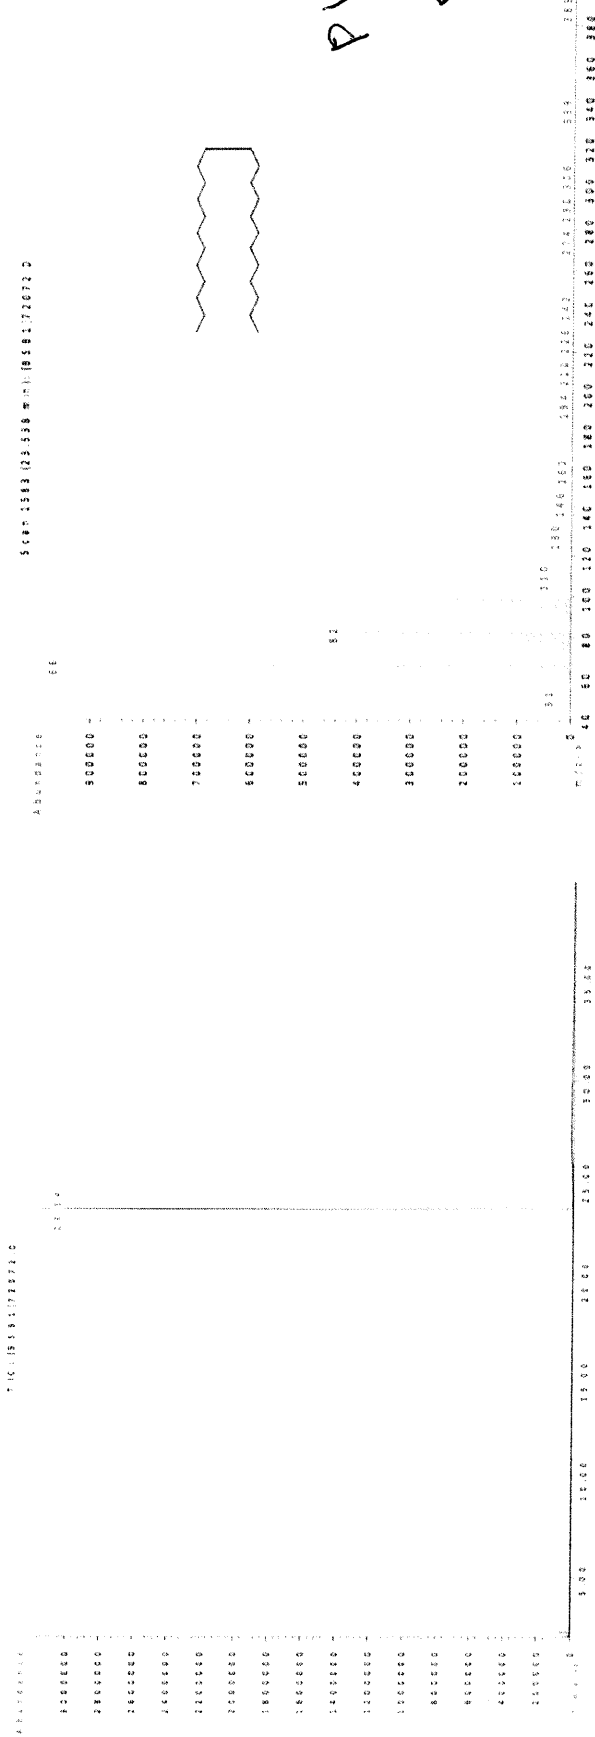

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
Standards are certified (±) 0.5% of the stated value, unless otherwise stated.  
All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




# **Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"**

Run Length: 35.00 min, 20999 points at 10 points/second.  
Created: Thu, Sep 17, 2020 at 9:46:03 AM.  
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".  
Analyzed using Method "GC4-M1".

## **Comments**

GC4-M1 Analysis by Candice Warren  
Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness  
Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,  
Air (detector) = 360 mL  
Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.  
Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.  
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

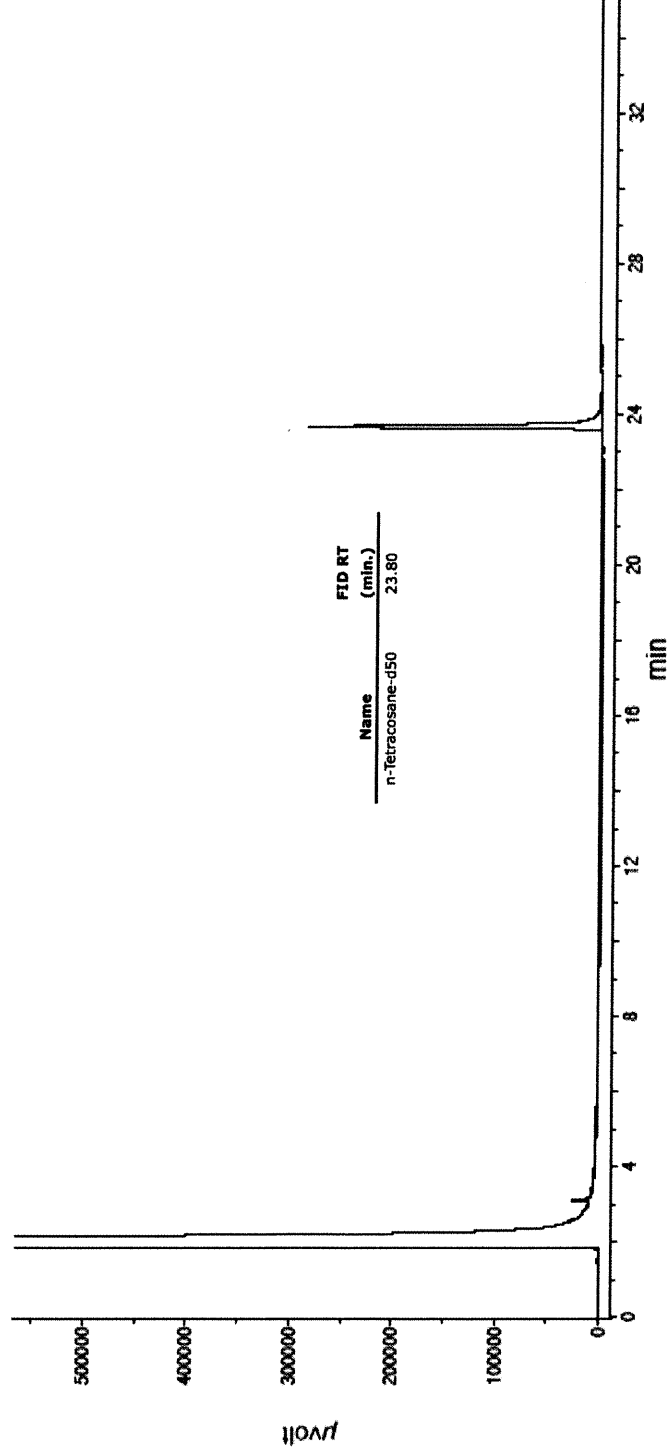

P11176  
 11/02/21  
 12



**CERTIFIED WEIGHT REPORT**

**Part Number:**  
 Lot Number:  
 Description:

**72072**  
**091120**  
 n-Tetracosane-d50

**Solvent(s):**  
 Methylene chloride

**Lot#**  
 104929

**Expiration Date:**  
**Recommended Storage:**  
**Nominal Concentration (µg/mL):**  
**NIST Test ID#:**

091130  
 Ambient (20 °C)  
 1000  
 23060

5E-05 Balance Uncertainty  
 0.058 Flask Uncertainty


**Weight(s) shown below were combined and diluted to (mL):** 200.0

Formulated By:	Benson Chan	091120	DATE
Reviewed By:	Pedro L. Rentas	091120	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	(Solvent Safety Info. On Attached pg.)	OSHA PEL (TWA)	LDSO
----------	-----	------------	----------------------	------------	------------------------	------------	------------------	------------------	---------------------	----------------------------------	--	----------------	------

1. n-Tetracosane-d50 2072 PR-26606 1000 98.7 0.2 99.0 0.20471 0.20481 1000.5 4.1 16416-32-3 N/A

**Method GCMSD-3.M:** Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

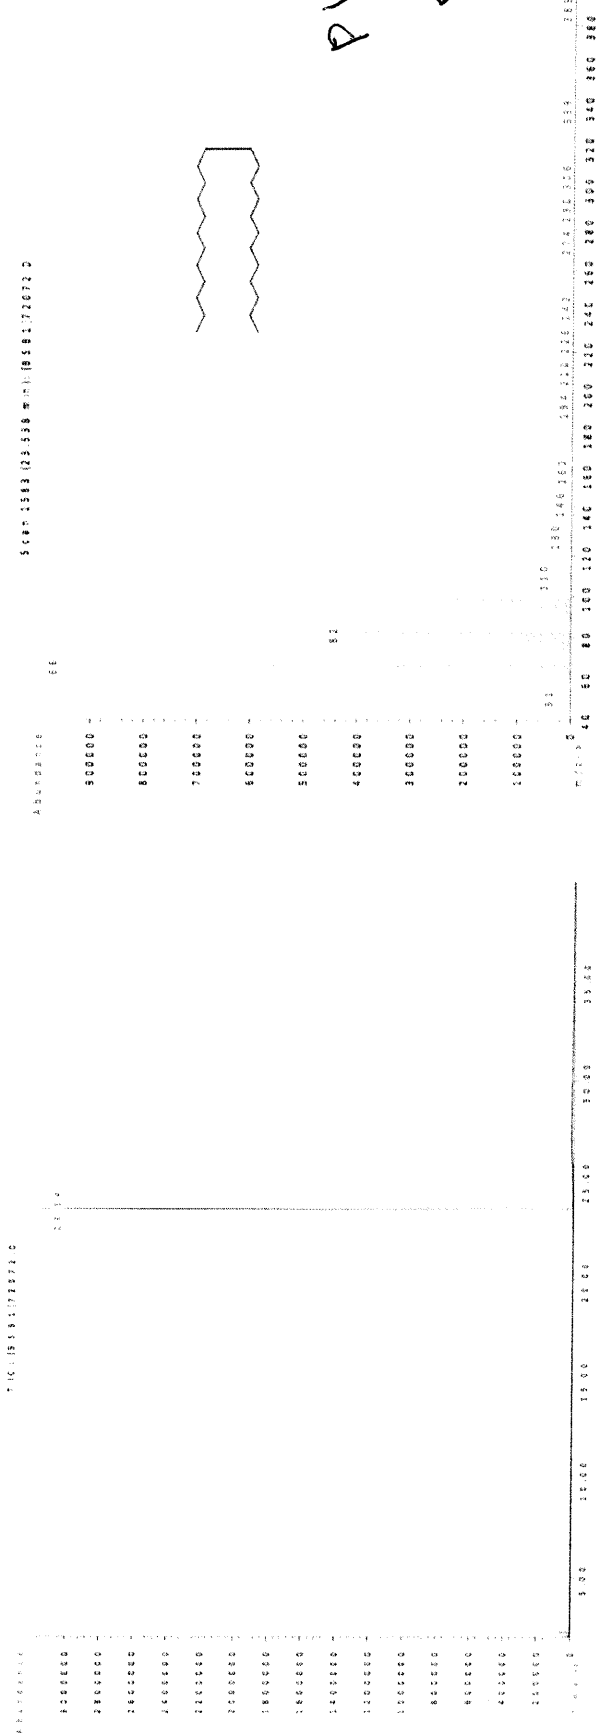

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
 Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
 Standards are certified (±) 0.5% of the stated value, unless otherwise stated.  
 All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
 Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Handwritten notes: *11/10/21*, *AR*, *11/10/21*, *11/10/21*




# **Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"**

Run Length: 35.00 min, 20999 points at 10 points/second.  
Created: Thu, Sep 17, 2020 at 9:46:03 AM.  
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".  
Analyzed using Method "GC4-M1".

## **Comments**

GC4-M1 Analysis by Candice Warren  
Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness  
Flow rates: Total Flow = 300 ml/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,  
Air (detector) = 360 mL  
Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.  
Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.  
Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

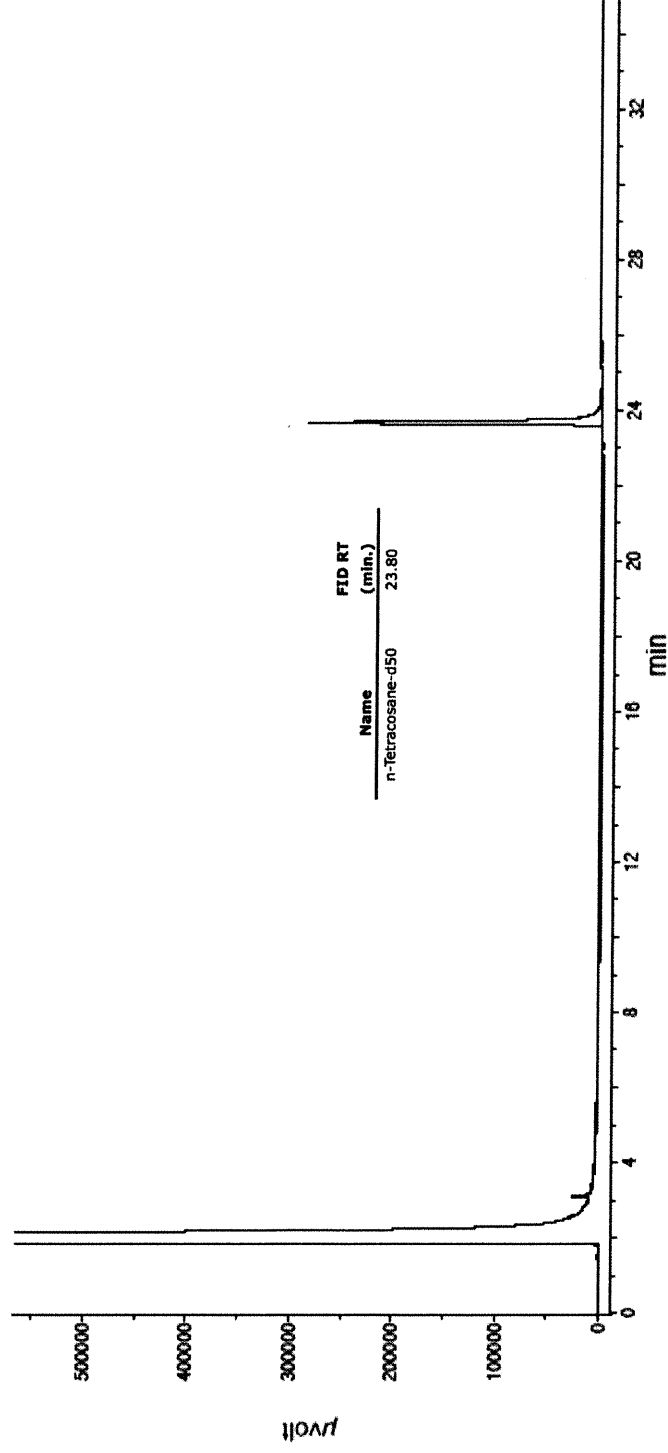

P11176  
 11/02/21  
 12



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis

P11749 to P11758

Received by SJ 5/27/2022



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31266 **Lot No.:** A0181886  
**Description :** Florida TRPH Standard  
Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** March 31, 2029 **Storage:** 25°C nominal  
**Handling:** Sonicate prior to use. **Ship:** Ambient

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	n-Octane (C8) CAS # 111-65-9 (Lot SHBM4827) Purity 99%	501.6 µg/mL	+/- 2.9794 µg/mL Gravimetric +/- 12.4620 µg/mL Unstressed +/- 14.9378 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 (Lot SHBM1113) Purity 99%	501.8 µg/mL	+/- 2.9802 µg/mL Gravimetric +/- 12.4657 µg/mL Unstressed +/- 14.9423 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 (Lot SHBK0925) Purity 99%	500.9 µg/mL	+/- 2.9752 µg/mL Gravimetric +/- 12.4446 µg/mL Unstressed +/- 14.9169 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 (Lot STBK2282) Purity 99%	500.7 µg/mL	+/- 2.9740 µg/mL Gravimetric +/- 12.4396 µg/mL Unstressed +/- 14.9110 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 (Lot SHBM4146) Purity 98%	500.5 µg/mL	+/- 2.9727 µg/mL Gravimetric +/- 12.4343 µg/mL Unstressed +/- 14.9046 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 (Lot UE5NG) Purity 98%	500.5 µg/mL	+/- 2.9730 µg/mL Gravimetric +/- 12.4355 µg/mL Unstressed +/- 14.9061 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 (Lot MKCF7888) Purity 99%	500.6 µg/mL	+/- 2.9731 µg/mL Gravimetric +/- 12.4359 µg/mL Unstressed +/- 14.9065 µg/mL Stressed

8	n-Docosane (C22) <b>CAS #</b> 629-97-0 <b>Purity</b> 99%	(Lot MKCL8918)	501.5 µg/mL	+/- 2.9785 +/- 12.4583 +/- 14.9333	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) <b>CAS #</b> 646-31-1 <b>Purity</b> 99%	(Lot MKCJ8741)	500.6 µg/mL	+/- 2.9731 +/- 12.4359 +/- 14.9065	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) <b>CAS #</b> 630-01-3 <b>Purity</b> 99%	(Lot MKCD4540)	500.5 µg/mL	+/- 2.9728 +/- 12.4347 +/- 14.9050	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) <b>CAS #</b> 630-02-4 <b>Purity</b> 99%	(Lot BCCG0084)	500.6 µg/mL	+/- 2.9734 +/- 12.4371 +/- 14.9080	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) <b>CAS #</b> 638-68-6 <b>Purity</b> 99%	(Lot MKCN9321)	501.7 µg/mL	+/- 2.9799 +/- 12.4645 +/- 14.9408	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) <b>CAS #</b> 544-85-4 <b>Purity</b> 99%	(Lot BCBW0661)	501.8 µg/mL	+/- 2.9805 +/- 12.4670 +/- 14.9437	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) <b>CAS #</b> 14167-59-0 <b>Purity</b> 99%	(Lot OML4N)	501.3 µg/mL	+/- 2.9773 +/- 12.4533 +/- 14.9274	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) <b>CAS #</b> 630-06-8 <b>Purity</b> 99%	(Lot U25B014)	502.4 µg/mL	+/- 2.9841 +/- 12.4819 +/- 14.9616	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) <b>CAS #</b> 7194-85-6 <b>Purity</b> 97%	(Lot 0000127235)	501.7 µg/mL	+/- 2.9801 +/- 12.4653 +/- 14.9417	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) <b>CAS #</b> 4181-95-7 <b>Purity</b> 98%	(Lot PADGI)	500.2 µg/mL	+/- 2.9713 +/- 12.4282 +/- 14.8973	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
<b>Solvent:</b>	Hexane <b>CAS #</b> 110-54-3 <b>Purity</b> 99%					

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)


**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

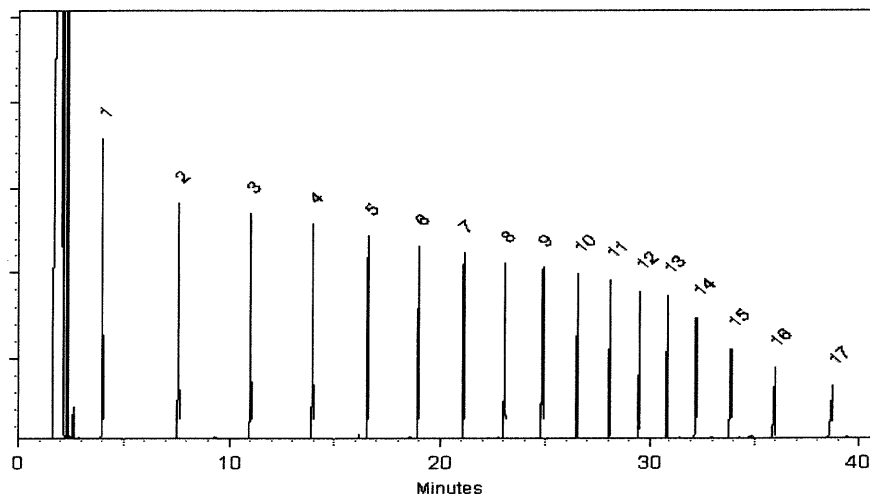

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope S. Riglin*  
Penelope Riglin - Operations Tech I

Date Mixed: 16-Feb-2022      Balance: 1128360905

*Clara Windle*  
Clara Windle - Operations Technician I

Date Passed: 21-Feb-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis

P11749 to P11758

Received by SJ 5/27/2022



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31266 **Lot No.:** A0181886  
**Description :** Florida TRPH Standard  
Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** March 31, 2029 **Storage:** 25°C nominal  
**Handling:** Sonicate prior to use. **Ship:** Ambient

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	n-Octane (C8) CAS # 111-65-9 (Lot SHBM4827) Purity 99%	501.6 µg/mL	+/- 2.9794 µg/mL Gravimetric +/- 12.4620 µg/mL Unstressed +/- 14.9378 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 (Lot SHBM1113) Purity 99%	501.8 µg/mL	+/- 2.9802 µg/mL Gravimetric +/- 12.4657 µg/mL Unstressed +/- 14.9423 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 (Lot SHBK0925) Purity 99%	500.9 µg/mL	+/- 2.9752 µg/mL Gravimetric +/- 12.4446 µg/mL Unstressed +/- 14.9169 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 (Lot STBK2282) Purity 99%	500.7 µg/mL	+/- 2.9740 µg/mL Gravimetric +/- 12.4396 µg/mL Unstressed +/- 14.9110 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 (Lot SHBM4146) Purity 98%	500.5 µg/mL	+/- 2.9727 µg/mL Gravimetric +/- 12.4343 µg/mL Unstressed +/- 14.9046 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 (Lot UE5NG) Purity 98%	500.5 µg/mL	+/- 2.9730 µg/mL Gravimetric +/- 12.4355 µg/mL Unstressed +/- 14.9061 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 (Lot MKCF7888) Purity 99%	500.6 µg/mL	+/- 2.9731 µg/mL Gravimetric +/- 12.4359 µg/mL Unstressed +/- 14.9065 µg/mL Stressed

8	n-Docosane (C22) <b>CAS #</b> 629-97-0 <b>Purity</b> 99%	(Lot MKCL8918)	501.5 µg/mL	+/- 2.9785 +/- 12.4583 +/- 14.9333	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) <b>CAS #</b> 646-31-1 <b>Purity</b> 99%	(Lot MKCJ8741)	500.6 µg/mL	+/- 2.9731 +/- 12.4359 +/- 14.9065	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) <b>CAS #</b> 630-01-3 <b>Purity</b> 99%	(Lot MKCD4540)	500.5 µg/mL	+/- 2.9728 +/- 12.4347 +/- 14.9050	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) <b>CAS #</b> 630-02-4 <b>Purity</b> 99%	(Lot BCCG0084)	500.6 µg/mL	+/- 2.9734 +/- 12.4371 +/- 14.9080	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) <b>CAS #</b> 638-68-6 <b>Purity</b> 99%	(Lot MKCN9321)	501.7 µg/mL	+/- 2.9799 +/- 12.4645 +/- 14.9408	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) <b>CAS #</b> 544-85-4 <b>Purity</b> 99%	(Lot BCBW0661)	501.8 µg/mL	+/- 2.9805 +/- 12.4670 +/- 14.9437	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) <b>CAS #</b> 14167-59-0 <b>Purity</b> 99%	(Lot OML4N)	501.3 µg/mL	+/- 2.9773 +/- 12.4533 +/- 14.9274	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) <b>CAS #</b> 630-06-8 <b>Purity</b> 99%	(Lot U25B014)	502.4 µg/mL	+/- 2.9841 +/- 12.4819 +/- 14.9616	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) <b>CAS #</b> 7194-85-6 <b>Purity</b> 97%	(Lot 0000127235)	501.7 µg/mL	+/- 2.9801 +/- 12.4653 +/- 14.9417	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) <b>CAS #</b> 4181-95-7 <b>Purity</b> 98%	(Lot PADGI)	500.2 µg/mL	+/- 2.9713 +/- 12.4282 +/- 14.8973	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
<b>Solvent:</b>	Hexane <b>CAS #</b> 110-54-3 <b>Purity</b> 99%					



**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)


**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

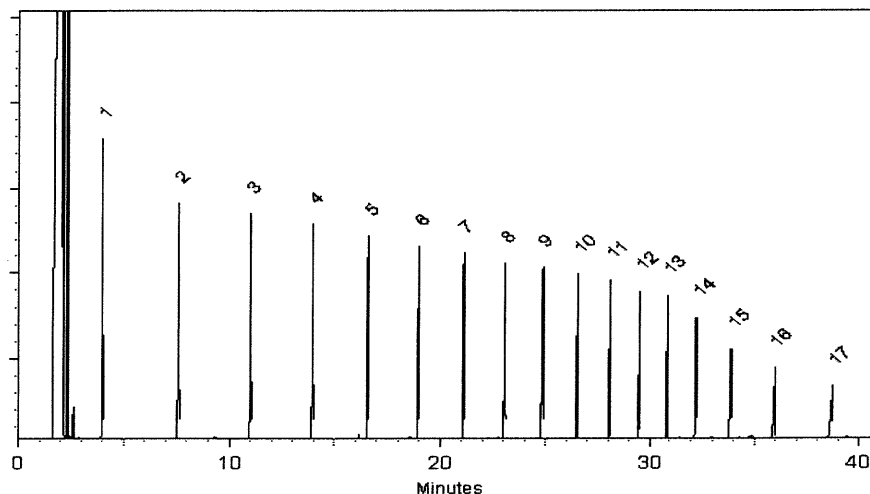

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope S. Riglin*  
Penelope Riglin - Operations Tech I

Date Mixed: 16-Feb-2022      Balance: 1128360905

*Clara Windle*  
Clara Windle - Operations Technician I

Date Passed: 21-Feb-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis

P11749 to P11758

Received by SJ 5/27/2022



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31266 **Lot No.:** A0181886  
**Description :** Florida TRPH Standard  
Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** March 31, 2029 **Storage:** 25°C nominal  
**Handling:** Sonicate prior to use. **Ship:** Ambient

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	n-Octane (C8) CAS # 111-65-9 (Lot SHBM4827) Purity 99%	501.6 µg/mL	+/- 2.9794 µg/mL Gravimetric +/- 12.4620 µg/mL Unstressed +/- 14.9378 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 (Lot SHBM1113) Purity 99%	501.8 µg/mL	+/- 2.9802 µg/mL Gravimetric +/- 12.4657 µg/mL Unstressed +/- 14.9423 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 (Lot SHBK0925) Purity 99%	500.9 µg/mL	+/- 2.9752 µg/mL Gravimetric +/- 12.4446 µg/mL Unstressed +/- 14.9169 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 (Lot STBK2282) Purity 99%	500.7 µg/mL	+/- 2.9740 µg/mL Gravimetric +/- 12.4396 µg/mL Unstressed +/- 14.9110 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 (Lot SHBM4146) Purity 98%	500.5 µg/mL	+/- 2.9727 µg/mL Gravimetric +/- 12.4343 µg/mL Unstressed +/- 14.9046 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 (Lot UE5NG) Purity 98%	500.5 µg/mL	+/- 2.9730 µg/mL Gravimetric +/- 12.4355 µg/mL Unstressed +/- 14.9061 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 (Lot MKCF7888) Purity 99%	500.6 µg/mL	+/- 2.9731 µg/mL Gravimetric +/- 12.4359 µg/mL Unstressed +/- 14.9065 µg/mL Stressed

8	n-Docosane (C22) <b>CAS #</b> 629-97-0 <b>Purity</b> 99%	(Lot MKCL8918)	501.5 µg/mL	+/- 2.9785 +/- 12.4583 +/- 14.9333	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) <b>CAS #</b> 646-31-1 <b>Purity</b> 99%	(Lot MKCJ8741)	500.6 µg/mL	+/- 2.9731 +/- 12.4359 +/- 14.9065	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) <b>CAS #</b> 630-01-3 <b>Purity</b> 99%	(Lot MKCD4540)	500.5 µg/mL	+/- 2.9728 +/- 12.4347 +/- 14.9050	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) <b>CAS #</b> 630-02-4 <b>Purity</b> 99%	(Lot BCCG0084)	500.6 µg/mL	+/- 2.9734 +/- 12.4371 +/- 14.9080	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) <b>CAS #</b> 638-68-6 <b>Purity</b> 99%	(Lot MKCN9321)	501.7 µg/mL	+/- 2.9799 +/- 12.4645 +/- 14.9408	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) <b>CAS #</b> 544-85-4 <b>Purity</b> 99%	(Lot BCBW0661)	501.8 µg/mL	+/- 2.9805 +/- 12.4670 +/- 14.9437	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) <b>CAS #</b> 14167-59-0 <b>Purity</b> 99%	(Lot OML4N)	501.3 µg/mL	+/- 2.9773 +/- 12.4533 +/- 14.9274	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) <b>CAS #</b> 630-06-8 <b>Purity</b> 99%	(Lot U25B014)	502.4 µg/mL	+/- 2.9841 +/- 12.4819 +/- 14.9616	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) <b>CAS #</b> 7194-85-6 <b>Purity</b> 97%	(Lot 0000127235)	501.7 µg/mL	+/- 2.9801 +/- 12.4653 +/- 14.9417	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) <b>CAS #</b> 4181-95-7 <b>Purity</b> 98%	(Lot PADGI)	500.2 µg/mL	+/- 2.9713 +/- 12.4282 +/- 14.8973	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
<b>Solvent:</b>	Hexane <b>CAS #</b> 110-54-3 <b>Purity</b> 99%					

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)


**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

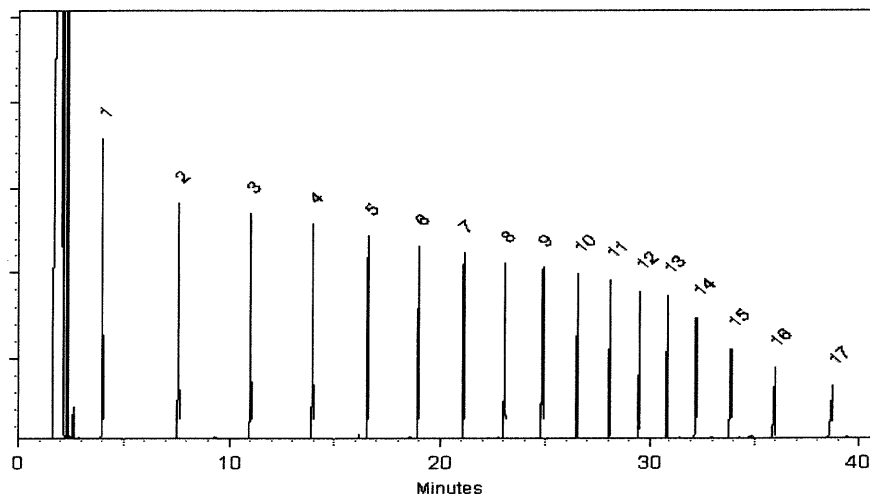

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope S. Riglin*  
Penelope Riglin - Operations Tech I

**Date Mixed:** 16-Feb-2022      **Balance:** 1128360905

*Clara Windle*  
Clara Windle - Operations Technician I

**Date Passed:** 21-Feb-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis

P11749 to P11758

Received by SJ 5/27/2022



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31266 **Lot No.:** A0181886

**Description :** Florida TRPH Standard  
Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** March 31, 2029 **Storage:** 25°C nominal

**Handling:** Sonicate prior to use. **Ship:** Ambient

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	n-Octane (C8) CAS # 111-65-9 (Lot SHBM4827) Purity 99%	501.6 µg/mL	+/- 2.9794 µg/mL Gravimetric +/- 12.4620 µg/mL Unstressed +/- 14.9378 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 (Lot SHBM1113) Purity 99%	501.8 µg/mL	+/- 2.9802 µg/mL Gravimetric +/- 12.4657 µg/mL Unstressed +/- 14.9423 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 (Lot SHBK0925) Purity 99%	500.9 µg/mL	+/- 2.9752 µg/mL Gravimetric +/- 12.4446 µg/mL Unstressed +/- 14.9169 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 (Lot STBK2282) Purity 99%	500.7 µg/mL	+/- 2.9740 µg/mL Gravimetric +/- 12.4396 µg/mL Unstressed +/- 14.9110 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 (Lot SHBM4146) Purity 98%	500.5 µg/mL	+/- 2.9727 µg/mL Gravimetric +/- 12.4343 µg/mL Unstressed +/- 14.9046 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 (Lot UE5NG) Purity 98%	500.5 µg/mL	+/- 2.9730 µg/mL Gravimetric +/- 12.4355 µg/mL Unstressed +/- 14.9061 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 (Lot MKCF7888) Purity 99%	500.6 µg/mL	+/- 2.9731 µg/mL Gravimetric +/- 12.4359 µg/mL Unstressed +/- 14.9065 µg/mL Stressed

8	n-Docosane (C22) <b>CAS #</b> 629-97-0 <b>Purity</b> 99%	(Lot MKCL8918)	501.5 µg/mL	+/- 2.9785 +/- 12.4583 +/- 14.9333	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) <b>CAS #</b> 646-31-1 <b>Purity</b> 99%	(Lot MKCJ8741)	500.6 µg/mL	+/- 2.9731 +/- 12.4359 +/- 14.9065	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) <b>CAS #</b> 630-01-3 <b>Purity</b> 99%	(Lot MKCD4540)	500.5 µg/mL	+/- 2.9728 +/- 12.4347 +/- 14.9050	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) <b>CAS #</b> 630-02-4 <b>Purity</b> 99%	(Lot BCCG0084)	500.6 µg/mL	+/- 2.9734 +/- 12.4371 +/- 14.9080	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) <b>CAS #</b> 638-68-6 <b>Purity</b> 99%	(Lot MKCN9321)	501.7 µg/mL	+/- 2.9799 +/- 12.4645 +/- 14.9408	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) <b>CAS #</b> 544-85-4 <b>Purity</b> 99%	(Lot BCBW0661)	501.8 µg/mL	+/- 2.9805 +/- 12.4670 +/- 14.9437	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) <b>CAS #</b> 14167-59-0 <b>Purity</b> 99%	(Lot OML4N)	501.3 µg/mL	+/- 2.9773 +/- 12.4533 +/- 14.9274	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) <b>CAS #</b> 630-06-8 <b>Purity</b> 99%	(Lot U25B014)	502.4 µg/mL	+/- 2.9841 +/- 12.4819 +/- 14.9616	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) <b>CAS #</b> 7194-85-6 <b>Purity</b> 97%	(Lot 0000127235)	501.7 µg/mL	+/- 2.9801 +/- 12.4653 +/- 14.9417	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) <b>CAS #</b> 4181-95-7 <b>Purity</b> 98%	(Lot PADGI)	500.2 µg/mL	+/- 2.9713 +/- 12.4282 +/- 14.8973	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
<b>Solvent:</b> Hexane <b>CAS #</b> 110-54-3 <b>Purity</b> 99%						



**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

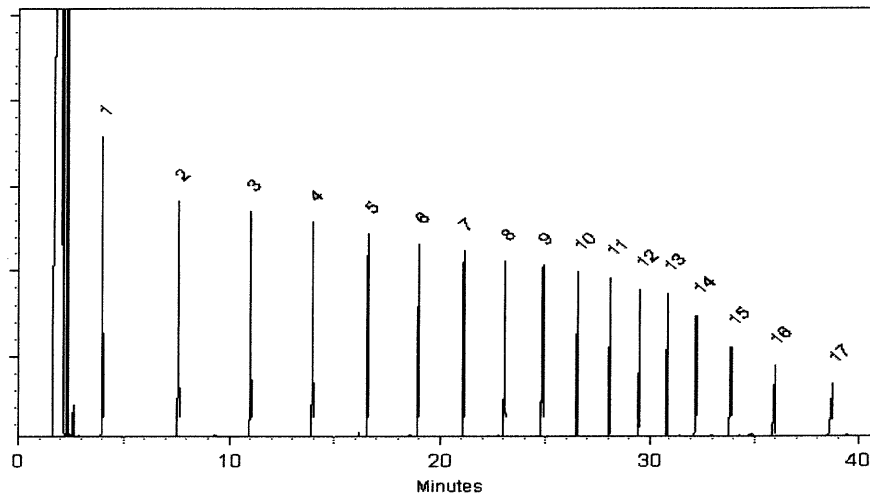

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope S. Riglin*

Penelope Riglin - Operations Tech I

Date Mixed: 16-Feb-2022

Balance: 1128360905

*Clara Windle*

Clara Windle - Operations Technician I

Date Passed: 21-Feb-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis

P11749 to P11758

Received by SJ 5/27/2022



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31266 **Lot No.:** A0181886

**Description :** Florida TRPH Standard  
Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** March 31, 2029 **Storage:** 25°C nominal

**Handling:** Sonicate prior to use. **Ship:** Ambient

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	n-Octane (C8) CAS # 111-65-9 (Lot SHBM4827) Purity 99%	501.6 µg/mL	+/- 2.9794 µg/mL Gravimetric +/- 12.4620 µg/mL Unstressed +/- 14.9378 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 (Lot SHBM1113) Purity 99%	501.8 µg/mL	+/- 2.9802 µg/mL Gravimetric +/- 12.4657 µg/mL Unstressed +/- 14.9423 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 (Lot SHBK0925) Purity 99%	500.9 µg/mL	+/- 2.9752 µg/mL Gravimetric +/- 12.4446 µg/mL Unstressed +/- 14.9169 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 (Lot STBK2282) Purity 99%	500.7 µg/mL	+/- 2.9740 µg/mL Gravimetric +/- 12.4396 µg/mL Unstressed +/- 14.9110 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 (Lot SHBM4146) Purity 98%	500.5 µg/mL	+/- 2.9727 µg/mL Gravimetric +/- 12.4343 µg/mL Unstressed +/- 14.9046 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 (Lot UE5NG) Purity 98%	500.5 µg/mL	+/- 2.9730 µg/mL Gravimetric +/- 12.4355 µg/mL Unstressed +/- 14.9061 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 (Lot MKCF7888) Purity 99%	500.6 µg/mL	+/- 2.9731 µg/mL Gravimetric +/- 12.4359 µg/mL Unstressed +/- 14.9065 µg/mL Stressed

8	n-Docosane (C22) <b>CAS #</b> 629-97-0 <b>Purity</b> 99%	(Lot MKCL8918)	501.5 µg/mL	+/- 2.9785 +/- 12.4583 +/- 14.9333	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) <b>CAS #</b> 646-31-1 <b>Purity</b> 99%	(Lot MKCJ8741)	500.6 µg/mL	+/- 2.9731 +/- 12.4359 +/- 14.9065	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) <b>CAS #</b> 630-01-3 <b>Purity</b> 99%	(Lot MKCD4540)	500.5 µg/mL	+/- 2.9728 +/- 12.4347 +/- 14.9050	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) <b>CAS #</b> 630-02-4 <b>Purity</b> 99%	(Lot BCCG0084)	500.6 µg/mL	+/- 2.9734 +/- 12.4371 +/- 14.9080	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) <b>CAS #</b> 638-68-6 <b>Purity</b> 99%	(Lot MKCN9321)	501.7 µg/mL	+/- 2.9799 +/- 12.4645 +/- 14.9408	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) <b>CAS #</b> 544-85-4 <b>Purity</b> 99%	(Lot BCBW0661)	501.8 µg/mL	+/- 2.9805 +/- 12.4670 +/- 14.9437	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) <b>CAS #</b> 14167-59-0 <b>Purity</b> 99%	(Lot OML4N)	501.3 µg/mL	+/- 2.9773 +/- 12.4533 +/- 14.9274	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) <b>CAS #</b> 630-06-8 <b>Purity</b> 99%	(Lot U25B014)	502.4 µg/mL	+/- 2.9841 +/- 12.4819 +/- 14.9616	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) <b>CAS #</b> 7194-85-6 <b>Purity</b> 97%	(Lot 0000127235)	501.7 µg/mL	+/- 2.9801 +/- 12.4653 +/- 14.9417	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) <b>CAS #</b> 4181-95-7 <b>Purity</b> 98%	(Lot PADGI)	500.2 µg/mL	+/- 2.9713 +/- 12.4282 +/- 14.8973	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
<b>Solvent:</b>	Hexane <b>CAS #</b> 110-54-3 <b>Purity</b> 99%					

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

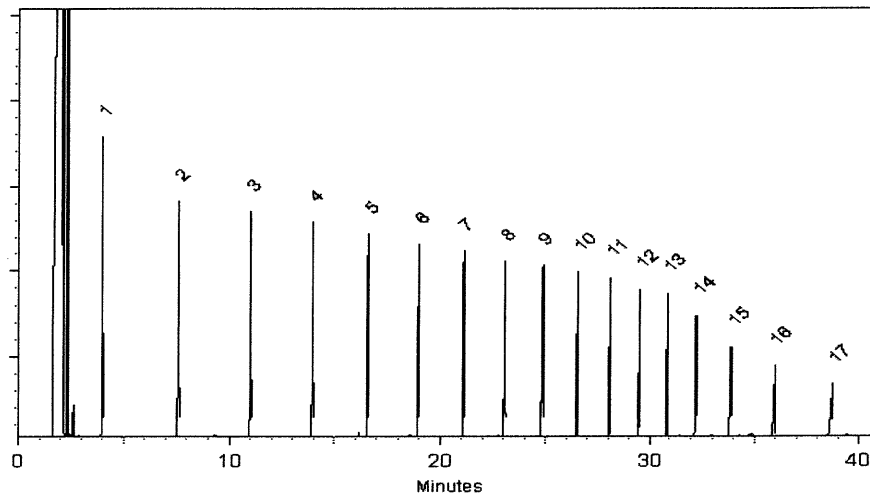

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope S. Riglin*

Penelope Riglin - Operations Tech I

Date Mixed: 16-Feb-2022

Balance: 1128360905

*Clara Windle*

Clara Windle - Operations Technician I

Date Passed: 21-Feb-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31266 Lot No.: A0184585

Description : Florida TRPH Standard

Container Size : 2 mL Pkg Amt: > 1 mL

Expiration Date : May 31, 2029 Storage: 25°C nominal

Handling: Sonicate prior to use. Ship: Ambient

P11852  
↓  
y.p  
06/17  
P1866

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.I.; K=2)
1	n-Octane (C8) CAS # 111-65-9 Purity 99%	500.3 µg/mL (Lot SHBN3807)	+/- 2.9718 µg/mL Gravimetric +/- 12.4305 µg/mL Unstressed +/- 14.9001 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99%	501.7 µg/mL (Lot SHBN8619)	+/- 2.9797 µg/mL Gravimetric +/- 12.4637 µg/mL Unstressed +/- 14.9398 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 Purity 99%	504.7 µg/mL (Lot SHBN7174)	+/- 2.9976 µg/mL Gravimetric +/- 12.5382 µg/mL Unstressed +/- 15.0291 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 Purity 99%	503.7 µg/mL (Lot STBJ3715)	+/- 2.9916 µg/mL Gravimetric +/- 12.5133 µg/mL Unstressed +/- 14.9993 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 Purity 98%	502.7 µg/mL (Lot SHBM4146)	+/- 2.9861 µg/mL Gravimetric +/- 12.4903 µg/mL Unstressed +/- 14.9717 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 Purity 98%	502.7 µg/mL (Lot UESNG)	+/- 2.9861 µg/mL Gravimetric +/- 12.4903 µg/mL Unstressed +/- 14.9717 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 Purity 97%	500.5 µg/mL (Lot MKCN8767)	+/- 2.9729 µg/mL Gravimetric +/- 12.4352 µg/mL Unstressed +/- 14.9056 µg/mL Stressed

8	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	501.3 µg/mL	+/- 2.9778 +/- 12.4554 +/- 14.9298	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	502.3 µg/mL	+/- 2.9837 +/- 12.4802 +/- 14.9596	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	501.0 µg/mL	+/- 2.9758 +/- 12.4471 +/- 14.9199	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	502.3 µg/mL	+/- 2.9837 +/- 12.4802 +/- 14.9596	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) CAS # 638-68-6 Purity 98%	(Lot MKCJ4572)	500.8 µg/mL	+/- 2.9745 +/- 12.4416 +/- 14.9134	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	501.0 µg/mL	+/- 2.9758 +/- 12.4471 +/- 14.9199	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	503.0 µg/mL	+/- 2.9877 +/- 12.4968 +/- 14.9795	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot U25B014)	503.0 µg/mL	+/- 2.9877 +/- 12.4968 +/- 14.9795	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 97%	(Lot 0000127235)	501.5 µg/mL	+/- 2.9787 +/- 12.4593 +/- 14.9345	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) CAS # 4181-95-7 Purity 98%	(Lot PADGI)	504.7 µg/mL	+/- 2.9978 +/- 12.5390 +/- 15.0301	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
<b>Solvent:</b> Hexane						
CAS # 110-54-3						
Purity 99%						



**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**


330°C

**Det. Type:**

FID

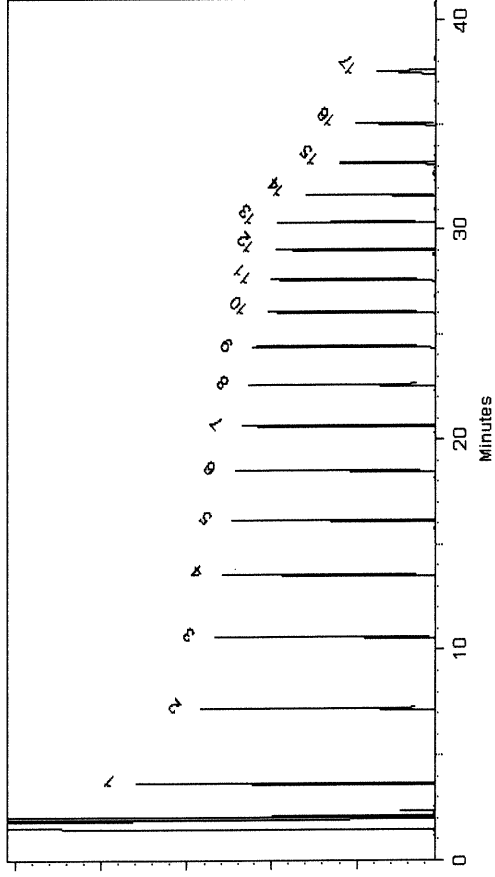

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Lane Kibe - Mix Technician

Date Mixed: 27-Apr-2022 Balance: 1128360905

  
Peng-Yen Lu - QC Analyst

Date Passed: 29-Apr-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.