



Prep Standard - Chemical Standard Summary

Order ID : O2213

Test : VOCGC Group 1

Prepbatch ID : PB151926,

Sequence ID/Qc Batch ID: PR040623,

Standard ID :

PP21522,PP21523,PP21524,PP21525,PP21869,PP21870,PP21871,PP21872,PP21873,PP21874,PP21886,PP21889,P
P21890,PP21891,PP21892,

Chemical ID :

DAILY,E3484,M4459,P10221,P10333,P12211,V13216,W2606,

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2263	EDB-DBCP 2 PPM Stock Solution	PP21522	01/25/2023	07/25/2023	Ankita Jodhani	None	None	Sohil Jodhani 01/25/2023
<u>FROM</u>	0.01000ml of P10221 + 0.01000ml of P10333 + 9.98000ml of V13216 = Final Quantity: 10.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2264	EDB-DBCP 2 PPM Stock Solution 2nd Source	PP21523	01/25/2023	07/25/2023	Ankita Jodhani	None	None	Sohil Jodhani 01/25/2023
<u>FROM</u> 0.10000ml of P12211 + 9.90000ml of V13216 = Final Quantity: 10.000 ml								

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2517	EDB-DBCP 100 PPB Working Solution	PP21524	01/25/2023	07/25/2023	Ankita Jodhani	None	None	Sohil Jodhani
01/25/2023								

FROM 9.50000ml of V13216 + 0.50000ml of PP21522 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2518	EDB-DBCP 100 PPB Working Sol. 2nd Source	PP21525	01/25/2023	07/25/2023	Ankita Jodhani	None	None	Sohil Jodhani
01/25/2023								

FROM 9.50000ml of V13216 + 0.50000ml of PP21523 = Final Quantity: 10.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2269	M8011-504.1 0.5 PPB STD	PP21869	03/28/2023	04/28/2023	Ankita Jodhani	None	None	Sohil Jodhani
03/28/2023								

FROM 35.00000ml of W2606 + 0.17500ml of PP21524 = Final Quantity: 35.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2270	M8011-504.1 0.25 PPB STD	PP21870	03/28/2023	04/28/2023	Ankita Jodhani	None	None	Sohil Jodhani
03/28/2023								

FROM 35.00000ml of W2606 + 0.08750ml of PP21524 = Final Quantity: 35.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2271	M8011-504.1 0.1 PPB STD	PP21871	03/28/2023	04/28/2023	Ankita Jodhani	None	None	Sohil Jodhani
03/28/2023								

FROM 35.00000ml of W2606 + 0.03500ml of PP21524 = Final Quantity: 35.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2272	M8011-504.1 0.05 PPB STD	PP21872	03/28/2023	04/28/2023	Ankita Jodhani	None	None	Sohil Jodhani
03/28/2023								

FROM 35.00000ml of W2606 + 0.01750ml of PP21524 = Final Quantity: 35.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2273	M8011-504.1 0.025 PPB STD	PP21873	03/28/2023	04/28/2023	Ankita Jodhani	None	None	Sohil Jodhani
03/28/2023								

FROM 35.00000ml of W2606 + 0.00880ml of PP21524 = Final Quantity: 35.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2274	M8011-504.1 0.1 PPB ICV STD	PP21874	03/28/2023	04/28/2023	Ankita Jodhani	None	None	Sohil Jodhani
03/28/2023								

FROM 35.00000ml of W2606 + 0.03500ml of PP21525 = Final Quantity: 35.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2519	M8011-504.1 0.1 PPB CCC	PP21886	04/06/2023	04/07/2023	Ankita Jodhani	None	None	Sohil Jodhani
04/07/2023								

FROM 35.00000ml of W2606 + 0.03500ml of PP21524 = Final Quantity: 35.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2275	M8011-504.1 0.25 PPB LCS STD	PP21889	04/06/2023	04/07/2023	Ankita Jodhani	None	None	Sohil Jodhani
04/07/2023								

FROM 35.00000ml of W2606 + 0.08750ml of PP21525 = Final Quantity: 35.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2275	M8011-504.1 0.25 PPB LCS STD	PP21890	04/06/2023	04/07/2023	Ankita Jodhani	None	None	Sohil Jodhani
04/07/2023								

FROM 35.00000ml of W2606 + 0.08750ml of PP21525 = Final Quantity: 35.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3653	M8011-504.1 LOD 0.025 PPB	PP21891	04/06/2023	04/07/2023	Ankita Jodhani	None	None	Sohil Jodhani
04/07/2023								

FROM 35.00000ml of W2606 + 0.00880ml of PP21524 = Final Quantity: 35.000 ml

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3759	M8011-504.1 LOQ 0.025 PPB	PP21892	04/06/2023	04/07/2023	Ankita Jodhani	None	None	Sohil Jodhani 04/07/2023
<u>FROM</u> 35.00000ml of W2606 + 0.00880ml of PP21524 = Final Quantity: 35.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	23A2662017	09/22/2023	03/22/2023 / Rajesh	03/15/2023 / Rajesh	E3484

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3624-05 / Sodium Chloride, Crystal (cs/4x2.5kg)	0000237721	04/13/2026	10/03/2022 / Ankita	10/30/2019 / AMANDEEP	M4459

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30270 / 1,2-Dibromo-3-Chloropropene Standard, 2,000 ug/ml	A0164625	07/25/2023	01/25/2023 / Ankita	01/19/2021 / Abdul	P10221

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30272 / 1,2-Dibromoethane Standard, 2000 ug/ml	A0154067	07/25/2023	01/25/2023 / Ankita	03/04/2021 / Abdul	P10333

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30239 / 504.1 Calibration Mix (3 components)	A0170154	07/25/2023	01/25/2023 / Ankita	11/28/2022 / Ankita	P12211

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA9077-02 / Methanol, Purge/Trap (cs=6x1L)	22C2362001	02/14/2025	01/25/2023 / Ankita	09/13/2022 / SAM	V13216



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	10/24/2024	10/24/2019 / apatel	10/24/2019 / apatel	W2606

Sodium Chloride, Crystal
BAKER ANALYZED® A.C.S. Reagent



From M4452 to M4459

Received on : 10/30/2019

Received by : AK

Material No.: 3624-05

Batch No.: 0000237721

Manufactured Date: 2019/04/15

Retest Date: 2026/04/13

Revision No: 1

Certificate of Analysis

Meets ACS Reagent Chemical Requirements,


Test	Specification	Result
Assay (NaCl) (by Ag titrn)	$\geq 99.0 \%$	100.3
pH of 5% Solution at 25°C	5.0 - 9.0	6.0
ACS - Insoluble Matter	$\leq 0.005 \%$	< 0.001
Iodide (I)	$\leq 0.002 \%$	< 0.002
Bromide (Br)	$\leq 0.01 \%$	< 0.01
Chlorate and Nitrate (as NO_3)	$\leq 0.003 \%$	< 0.001
ACS - Phosphate (PO_4)	$\leq 5 \text{ ppm}$	< 5
Sulfate (SO_4)	$\leq 0.004 \%$	< 0.004
Barium (Ba)	Passes Test	PT
ACS - Heavy Metals (as Pb)	$\leq 5 \text{ ppm}$	< 5
Iron (Fe)	$\leq 2 \text{ ppm}$	< 2
Calcium (Ca)	$\leq 0.002 \%$	< 0.001
Magnesium (Mg)	$\leq 0.001 \%$	< 0.001
Potassium (K)	$\leq 0.005 \%$	0.002

For Laboratory, Research or Manufacturing Use

Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US

Packaging Site: Paris Mfg Ctr & DC

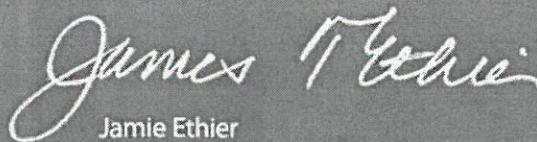
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Material No.: 9262-03
Batch No.: 23A2662017
Manufactured Date: 2023-01-10
Expiration Date: 2024-04-10
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	< 1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	< 1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	97 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 3/15/23

E 3484


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis



Material No.: 9077-02
Batch No.: 22C2362001
Manufactured Date: 2022-02-15
Expiration Date: 2025-02-14
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (CH ₃ OH) (by GC, corrected for water)	≥ 99.9 %	100.0 %
Residue after Evaporation	≤ 1.0 ppm	< 0.1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.3
Titration Base (μeq/g)	≤ 0.10	0.03
Water (by KF, coulometric)	≤ 0.08 %	< 0.01 %
Volatile Organic Trace Analysis – Below EPA 8260B CRQL	Conforms	Conforms

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700
Page 1 of 1



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30270 Lot No.: A0164625
Description : 1,2-Dibromo-3-chloropropane Standard
1,2-Dibromo-3-Chloropropane 2000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : September 30, 2025 Storage: 0°C or colder
Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	1,2-Dibromo-3-chloropropane CAS # 96-12-8 (Lot FBL01) Purity 97%	2,006.0 µg/mL	+/- 18.6543 µg/mL Gravimetric +/- 113.4106 µg/mL Unstressed +/- 116.0210 µg/mL Stressed

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

P10221
AR
01/19/2021

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:


200°C

Det. Temp:

250°C

Det. Type:

FID

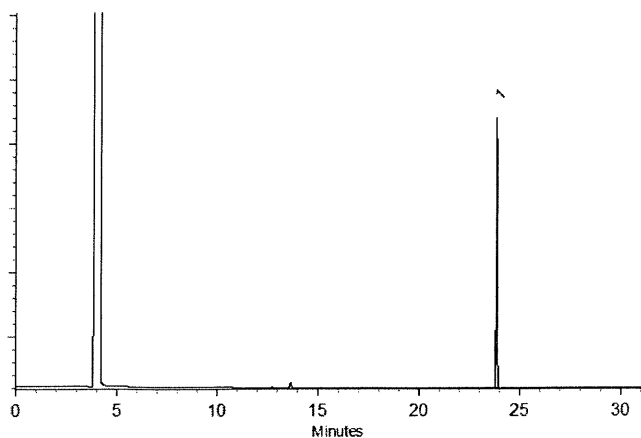

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Katelyn McGinnis - Operations Tech I

Date Mixed: 22-Sep-2020

Balance: 1127510105


Justine Albertson - Operations Tech-ARM QC

Date Passed: 24-Sep-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30272 Lot No.: A0151983
Description : 1,2-Dibromoethane Standard
1,2-Dibromoethane 2000µg/mL, P&T Methanol, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : August 31, 2024 Storage: 0°C or colder

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	1,2-Dibromoethane (EDB)	2,004.0 µg/mL	+/- 11.9032 µg/mL Gravimetric
	CAS # 106-93-4 (Lot BCBH3877V)		+/- 112.3887 µg/mL Unstressed
	Purity 99%		+/- 115.0172 µg/mL Stressed

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

P10332

P10335

AR
03/05/21

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:


200°C

Det. Temp:

250°C

Det. Type:

FID

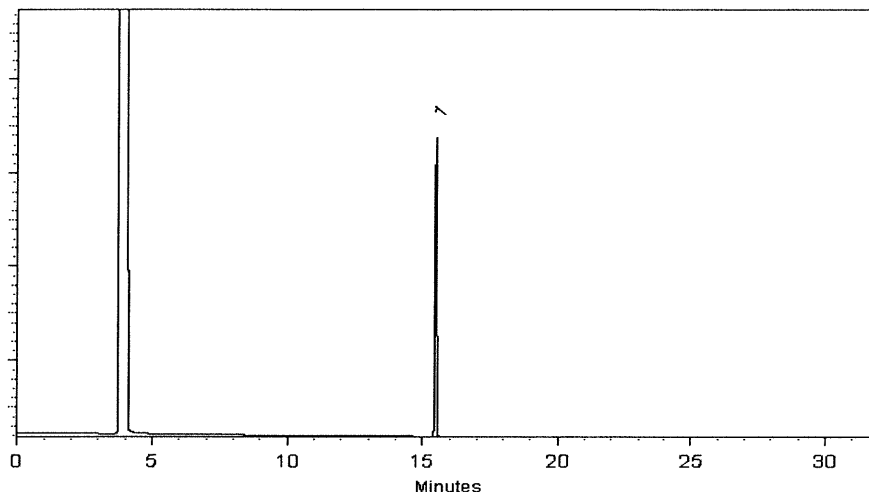

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Matt Fragassi - Mix Technician

Date Mixed: 18-Aug-2019

Balance: 1128342314


Tyler Brown - Operations Tech-ARM QC

Date Passed: 20-Aug-2019

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30239 **Lot No.:** A0170154

Description : 504.1 Calibration Mix

504.1 Calibration Std 200µg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : March 31, 2026 **Storage:** 0°C or colder

Ship: Ambient

P12211
↓
P12215
AJ
11/28/22

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	1,2-Dibromoethane (EDB) CAS # 106-93-4 Purity 99% (Lot BCBP2268V)	200.5 µg/mL	+/- 1.4217 µg/mL Gravimetric +/- 11.2713 µg/mL Unstressed +/- 11.5336 µg/mL Stressed
2	1,2,3-Trichloropropane CAS # 96-18-4 Purity 99% (Lot BCBH8722V)	200.0 µg/mL	+/- 1.4182 µg/mL Gravimetric +/- 11.2431 µg/mL Unstressed +/- 11.5049 µg/mL Stressed
3	1,2-Dibromo-3-chloropropane CAS # 96-12-8 Purity 97% (Lot FBL01)	199.8 µg/mL	+/- 1.4169 µg/mL Gravimetric +/- 11.2330 µg/mL Unstressed +/- 11.4945 µg/mL Stressed

Solvent: P&T Methanol
CAS # 67-56-1
Purity 99%

Column:

105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)

Carrier Gas:

hydrogen-constant pressure 11.0 psi.

Temp. Program:

40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:


200°C

Det. Temp:

250°C

Det. Type:

FID

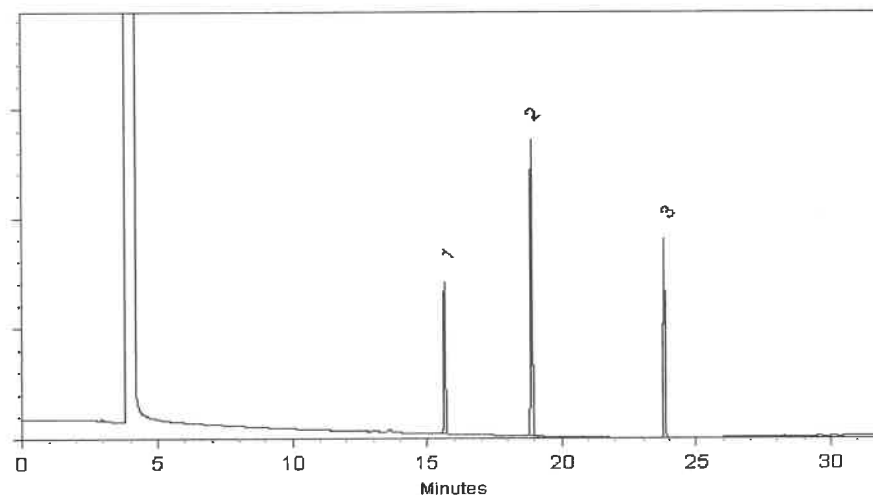

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Erik Strommer - Operations Tech I

Date Mixed: 15-Mar-2021

Balance: B251644995


Alexis Shelow - Operations Tech I

Date Passed: 16-Mar-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397