

Prep Standard - Chemical Standard Summary**Order ID :** O3572**Test :** Pesticide-TCL**Prepbatch ID :** PB154697,**Sequence ID/Qc Batch ID:** PD080923,**Standard ID :**

EP2368,EP2372,PP21731,PP21733,PP21773,PP22265,PP22271,PP22272,PP22273,PP22274,PP22275,PP22276,PP22277,PP22278,PP22279,PP22283,PP22284,PP22285,PP22286,PP22287,PP22288,PP22289,PP22290,PP22291,PP22292,PP22293,PP22294,PP22295,PP22296,PP22297,PP22298,PP22299,PP22339,PP22388,PP22450,PP22451,

Chemical ID :

E2865,E3412,E3465,E3469,E3477,E3520,E3531,E3533,E3544,E3546,E3550,P10345,P10887,P11062,P11063,P11142,P11143,P11388,P11389,P11741,P11791,P11813,P11892,P12404,P12596,P12606,P9049,

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	EP2368	07/31/2023	01/21/2024	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 07/31/2023

FROM 8000.00000ml of E3546 + 8000.00000ml of E3550 = Final Quantity: 8000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2372	08/02/2023	10/23/2023	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	RUPESHKUMAR SHAH 08/02/2023

FROM 4000.00000gram of E3412 = Final Quantity: 4000.000 gram

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1472	20 PPM Pest Stock Solution 2nd Source	PP21731	02/24/2023	08/20/2023	Abdul Mirza	None	None	Ankita Jodhani
03/01/2023								

FROM 1.00000ml of P11062 + 9.00000ml of E3469 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3663	20 PPM MIREX Stock STD (Secondary source)	PP21733	02/24/2023	08/20/2023	Abdul Mirza	None	None	Ankita Jodhani
03/01/2023								

FROM 0.20000ml of P11142 + 9.80000ml of E3469 = Final Quantity: 10.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2156	100 PPB Pest Spike for LOD-LOQ (Restek)	PP21773	03/08/2023	08/20/2023	Abdul Mirza	None	None	Ankita Jodhani
03/09/2023								

FROM 99.00000ml of E3477 + 0.50000ml of PP21731 + 0.50000ml of PP21733 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
758	PEM Mix w/Surr	PP22265	07/03/2023	12/17/2023	Abdul Mirza	None	None	Yogesh Patel
07/05/2023								

FROM 1.00000ml of P11791 + 99.00000ml of E3520 = Final Quantity: 100.000 ml

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3629	20 PPM PEST stock Solution 1st source(RESTEK)	PP22271	07/03/2023	01/03/2024	Abdul Mirza	None	None	Yogesh Patel 07/05/2023
<u>FROM</u> 1.00000ml of P11063 + 9.00000ml of E3533 = Final Quantity: 10.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1472	20 PPM Pest Stock Solution 2nd Source	PP22272	07/03/2023	01/03/2024	Abdul Mirza	None	None	Yogesh Patel 07/05/2023
<u>FROM</u>	1.00000ml of P10345 + 9.00000ml of E3533 = Final Quantity: 10.000 ml							

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1273	20 PPM Mirex Stock (Primary Source)	PP22273	07/03/2023	01/03/2024	Abdul Mirza	None	None	Yogesh Patel 07/05/2023
<u>FROM</u> 0.20000ml of P9049 + 9.80000ml of E3533 = Final Quantity: 10.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3663	20 PPM MIREX Stock STD (Secondary source)	PP22274	07/03/2023	01/03/2024	Abdul Mirza	None	None	Yogesh Patel 07/05/2023
<u>FROM</u>	0.20000ml of P11143 + 9.80000ml of E3533 = Final Quantity: 10.000 ml							

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP22275	07/03/2023	01/03/2024	Abdul Mirza	None	None	Yogesh Patel
07/05/2023								

FROM 1.00000ml of P11741 + 9.00000ml of E3533 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3630	100/100 PPB PEST Working std.1st Source(RESTEK)	PP22276	07/03/2023	01/03/2024	Abdul Mirza	None	None	Yogesh Patel
07/05/2023								

FROM 98.50000ml of E3533 + 0.50000ml of PP22271 + 0.50000ml of PP22273 + 0.50000ml of PP22275 = Final Quantity: 100.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
80	100/100 PPB Pesticide Working Solution 2nd Source	PP22277	07/03/2023	01/03/2024	Abdul Mirza	None	None	Yogesh Patel
								07/05/2023

FROM 98.50000ml of E3533 + 0.50000ml of PP22272 + 0.50000ml of PP22274 + 0.50000ml of PP22275 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3631	75 PPB ICAL PEST STD(RESTEK)	PP22278	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed
								07/07/2023

FROM 0.25000ml of E3533 + 0.75000ml of PP22276 = Final Quantity: 1.000 ml

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3632	50 PPB ICAL PEST STD(RESTEK)	PP22279	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023
<u>FROM</u> 0.50000ml of E3533 + 0.50000ml of PP22276 = Final Quantity: 1.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3633	25 PPB ICAL PEST STD(RESTEK)	PP22283	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023
<u>FROM</u>	0.75000ml of E3533 + 0.25000ml of PP22276 = Final Quantity: 1.000 ml							

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3634	5 PPB ICAL PEST STD(RESTEK)	PP22284	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023
<u>FROM</u>	0.90000ml of E3533 + 0.10000ml of PP22279 = Final Quantity: 1.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3988	50 PPB PEST ICV STD(RESTEK)	PP22285	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023
<u>FROM</u>	0.50000ml of E3533 + 0.50000ml of PP22277 = Final Quantity: 1.000 ml							

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
386	1000/100 PPB Chlordane STD (Restek)	PP22286	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023

FROM 0.10000ml of P12596 + 99.40000ml of E3533 + 0.50000ml of PP22275 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
528	CHLOR 750 PPB STD	PP22287	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023

FROM 0.25000ml of E3533 + 0.75000ml of PP22286 = Final Quantity: 1.000 ml

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
529	CHLOR 500 PPB STD	PP22288	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023
<u>FROM</u>	0.50000ml of E3533 + 0.50000ml of PP22286 = Final Quantity: 1.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
530	CHLOR 250 PPB STD	PP22289	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023
<u>FROM</u> 0.75000ml of E3533 + 0.25000ml of PP22286 = Final Quantity: 1.000 ml								

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3408	CHLOR 50 PPB STD	PP22290	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023

FROM 0.90000ml of E3533 + 0.10000ml of PP22288 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3746	1000/100 ppb Chlordane STD-RESTEK 2ND SOURCE	PP22291	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023

FROM 0.10000ml of P12606 + 99.40000ml of E3533 + 0.50000ml of PP22275 = Final Quantity: 100.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
532	CHLOR 500 PPB ICV STD	PP22292	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023

FROM 0.50000ml of E3533 + 0.50000ml of PP22291 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
383	1000/100 PPB Toxaphene STD (Restek)	PP22293	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023

FROM 0.10000ml of P11388 + 99.40000ml of E3533 + 0.50000ml of PP22275 = Final Quantity: 100.000 ml

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
533	TOX 750 PPB STD	PP22294	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023
<u>FROM</u>	0.25000ml of E3533 + 0.75000ml of PP22293 = Final Quantity: 1.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
534	TOX 500 PPB STD	PP22295	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023
<u>FROM</u> 0.50000ml of E3533 + 0.50000ml of PP22293 = Final Quantity: 1.000 ml								

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
535	TOX 250 PPB STD	PP22296	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023
<u>FROM</u>	0.75000ml of E3533 + 0.25000ml of PP22293 = Final Quantity: 1.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2217	TOX 100 PPB STD	PP22297	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023
<u>FROM</u> 0.90000ml of E3533 + 0.10000ml of PP22293 = Final Quantity: 1.000 ml								

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3669	1000/100 PPB TOXAPHENE STD 2nd source (RESTEK)	PP22298	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023

FROM 0.10000ml of P11813 + 99.40000ml of E3533 + 0.50000ml of PP22275 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3670	TOX 500 PPB ICV std (RESTEK)	PP22299	07/03/2023	01/03/2024	Ankita Jodhani	None	None	mohammad ahmed 07/07/2023

FROM 0.50000ml of E3533 + 0.50000ml of PP22298 = Final Quantity: 1.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
79	500 PPB Pesticide Spike Solution	PP22339	07/10/2023	11/30/2023	Abdul Mirza	None	None	Ankita Jodhani
07/10/2023								

FROM 95.00000ml of E3465 + 2.50000ml of PP22272 + 2.50000ml of PP22274 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP22388	07/20/2023	01/17/2024	Ankita Jodhani	None	None	Sohil Jodhani
07/25/2023								

FROM 1.00000ml of P12404 + 999.00000ml of E3544 = Final Quantity: 1000.000 ml

CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1501	1000 ppb CHLORDANE SPIKE (RESTEK)	PP22450	08/02/2023	01/21/2024	Abdul Mirza	None	None	Ankita Jodhani
08/03/2023								

FROM 0.10000ml of P11892 + 99.90000ml of E3546 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3878	1000 PPB TOXAPHENE SPIKE (RESTEK)	PP22451	08/02/2023	01/21/2024	Abdul Mirza	None	None	Ankita Jodhani
08/03/2023								

FROM 0.10000ml of P11389 + 99.90000ml of E3546 = Final Quantity: 100.000 ml

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	12/31/2024	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	139404	10/23/2023	10/18/2022 / Rajesh	10/13/2022 / Rajesh	E3412

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	9005-05 / Acetone Ultra (cs/4x4L)	22J2461015	03/12/2024	02/21/2023 / Rajesh	02/15/2023 / Rajesh	E3465

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	22G0362001	08/20/2023	02/20/2023 / Rajesh	02/16/2023 / Rajesh	E3469

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	22L2862006	09/27/2023	02/28/2023 / Rajesh	02/23/2023 / Rajesh	E3477

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	23C2462011	01/19/2024	06/17/2023 / Rajesh	06/15/2023 / Rajesh	E3520

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
phenomenex	FS0006 / Cleanert SPE Silica, 1000 mg/6ml, 30PK	YO307-2	12/24/2023	08/07/2023 / Rajesh	06/21/2023 / Rajesh	E3531

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	23C2462011	01/03/2024	07/03/2023 / Rajesh	06/29/2023 / Rajesh	E3533

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	22L2862006	01/17/2024	07/17/2023 / Rajesh	07/12/2023 / Rajesh	E3544

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	22L2862006	03/12/2024	07/21/2023 / Rajesh	07/20/2023 / Rajesh	E3546

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	23C2462011	01/27/2024	07/27/2023 / Rajesh	07/27/2023 / Rajesh	E3550

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32291 / Pesticide Mix, CLP method, organochlorine Std AB#1, 200ug/mL, hexane/toluene, 1mL/ampul	A0162166	01/03/2024	07/03/2023 / Abdul	03/05/2021 / Abdul	P10345

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
ULTRA Scientific	CLP-242 / Pesticide Resolution Check Mixture	0006617274	08/31/2023	07/03/2023 / Ankita	07/13/2021 / Ankita	P10887

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
ULTRA Scientific	CLP-242 / Pesticide Resolution Check Mixture	0006617274	08/31/2023	07/03/2023 / Ankita	07/13/2021 / Ankita	P10887

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32291 / Pesticide Mix, CLP method, organochlorine Std AB#1, 200ug/mL, hexane/toluene, 1mL/ampul	A0168439	08/24/2023	02/24/2023 / Abdul	09/29/2021 / Abdul	P11062

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32291 / Pesticide Mix, CLP method, organochlorine Std AB#1, 200ug/mL, hexane/toluene, 1mL/ampul	A0168439	01/03/2024	07/03/2023 / Abdul	09/29/2021 / Abdul	P11063

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	79136 / Mirex, 1000 ug/ml	102821	08/24/2023	02/24/2023 / Abdul	10/29/2021 / Abdul	P11142

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	79136 / Mirex, 1000 ug/ml	102821	01/03/2024	07/03/2023 / Abdul	10/29/2021 / Abdul	P11143

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32005 / Toxaphene Standard	A0176614	01/05/2024	07/03/2023 / Ankita	02/09/2022 / Ankita	P11388

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32005 / Toxaphene Standard	A0176614	02/02/2024	08/02/2023 / Abdul	02/09/2022 / Ankita	P11389

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0179404	01/03/2024	07/03/2023 / Abdul	05/27/2022 / Sohil	P11741

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32074 / Pesticide Performance Evaluation Mix w/Surrogate	A0183168	01/03/2024	07/03/2023 / Abdul	05/27/2022 / Sohil	P11791

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32005 / Toxaphene Standard	A0177326	01/05/2024	07/03/2023 / Ankita	06/17/2022 / Ankita	P11813

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32021 / Chlordane Std.	A0181737	02/02/2024	08/02/2023 / Abdul	06/17/2022 / Abdul	P11892

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A192797	01/20/2024	07/20/2023 / Ankita	03/16/2023 / Abdul	P12404

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32021 / Chlordane Std.	A0193299	01/03/2024	07/03/2023 / Abdul	07/03/2023 / Abdul	P12596

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32021 / Chlordane Std.	A0197993	01/03/2024	07/03/2023 / Abdul	07/03/2023 / Abdul	P12606

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	79136 / Mirex, 1000 ug/ml	112018	01/03/2024	07/03/2023 / Abdul	11/01/2019 / Stephen	P9049

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1

Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700




**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**



MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MÉXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT : SODIUM SULFATE CRYSTALS ANHYDROUS
QUALITY : ACS (CODE RMB3375) **FORMULA :** Na₂SO₄
SPECIFICATION NUMBER : 6399 **RELEASE DATE:** OCT/28/2021
LOT NUMBER : 139404

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.8 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.0
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.002 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.2 %
Retained on US Standard No. 60 sieve	Min. 94%	97.6 %
Through US Standard No. 60 sieve	Max. 5%	2.1 %
Through US Standard No. 100 sieve	Max. 10%	0.2 %
COMMENTS		
 QC: PhC Irma Belmares		

If you need further details, please call our factory or contact our local distributor.

E 3412

Recd. by RP on 10/13/22

RE-02-01, Ed. 3

Acetone
CMOS



Material No.: 9005-05
Batch No.: 22J2461015
Manufactured Date: 2022-10-20
Retest Date: 2027-10-19
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Color (APHA)	≤ 10	< 5
Residue after Evaporation	≤ 5 ppm	< 1 ppm
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.5	0.1
Water (H ₂ O)	≤ 0.5 %	0.2 %
Solubility in H ₂ O	Passes Test	Passes Test
Chloride (Cl)	≤ 0.2 ppm	< 0.2 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.05 ppm
Trace Impurities - Aluminum (Al)	≤ 50.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 5.0 ppb
Trace Impurities - Barium (Ba)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities - Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities - Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities - Cadmium (Cd)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Calcium (Ca)	≤ 25.0 ppb	3.4 ppb
Trace Impurities - Chromium (Cr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Germanium (Ge)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities - Gold (Au)	≤ 20 ppb	< 5 ppb
Trace Impurities - Iron (Fe)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities - Lead (Pb)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities - Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities - Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb

>>> Continued on page 2 >>>

E 3465
Recd. by RP on 2/15/23

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Acetone
CMOS



Material No.: 9005-05
Batch No.: 22J2461015

Test	Specification	Result
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Nickel (Ni)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 10.0 ppb	< 10.0 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Strontium (Sr)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 50.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	1.8 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater (Rion KS42AF)	≤ 100 par/ml	15 par/ml
Particle Count – 1.0 µm and greater (Rion KS42AF)	≤ 8 par/ml	4 par/ml

>>> Continued on page 3 >>>

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700
Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700



Material No.: 9262-03
Batch No.: 22G0362002
Manufactured Date: 2022-06-17
Expiration Date: 2023-09-16
Revision No.: 0

Certificate of Analysis


Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	2
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	2
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.5 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	97 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Rec'd by R? on 2/16/23

E 3469


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700
Page 1 of 1

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03
Batch No.: 22L2862006
Manufactured Date: 2022-12-19
Expiration Date: 2025-12-18
Revision No.: 0

Certificate of Analysis


Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H ₂ O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	4

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 2/23/23

E 3477

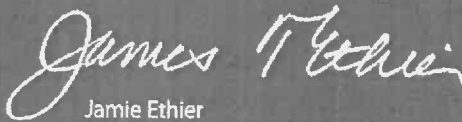
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700
Page 1 of 1

Material No.: 9262-03
Batch No.: 23C2462011
Manufactured Date: 2023-03-10
Expiration Date: 2024-06-08
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	< 1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	97 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 6/15/23

E 3520


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Cleanert Florisil

1g/6ml 30/pkg

固相萃取产品

LOT#: Y0307-2

MFG#: F00549



CAT# FS0006

Agela Technologies

Made in China

E3531



Material No.: 9262-03
Batch No.: 23C2462011
Manufactured Date: 2023-03-10
Expiration Date: 2024-06-08
Revision No.: 0

Certificate of Analysis


Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	< 1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	97 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by R² on 6/29/23

E 3533

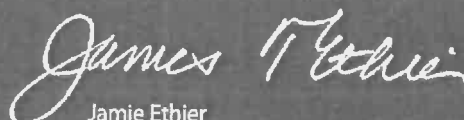
Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Page 1 of 1

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03
Batch No.: 22L2862006
Manufactured Date: 2022-12-19
Expiration Date: 2025-12-18
Revision No.: 0

Certificate of Analysis


Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H ₂ O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	4

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 7/12/23

E3544


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700
Page 1 of 1

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03
Batch No.: 22L2862006
Manufactured Date: 2022-12-19
Expiration Date: 2025-12-18
Revision No.: 0

Certificate of Analysis


Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H ₂ O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	4

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 4/20/23

E3546


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Hexanes (95% n-hexane)
BAKER RESI-ANALYZED® Reagent



Material No.: 9262-03
Batch No.: 23C2462011
Manufactured Date: 2023-03-10
Expiration Date: 2024-06-08
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	< 1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	97 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by R1 on 7/27/23

E3550

James Ethier

Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32021 **Lot No.:** A0181737

Description : Chlordane Standard

Chlordane Standard 1000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : May 31, 2028 **Storage:** 10°C or colder

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Chlordane CAS # 57-74-9 (Lot 978545) Purity ----%	1,006.0 µg/mL	+/- 5.9753 µg/mL Gravimetric +/- 31.8975 µg/mL Unstressed +/- 41.6615 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Tech Tips:

CAS #57-74-9 nomenclature is based on EPA method 8081B.

P 11892
↓
P 11896
5

06/17/2022

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

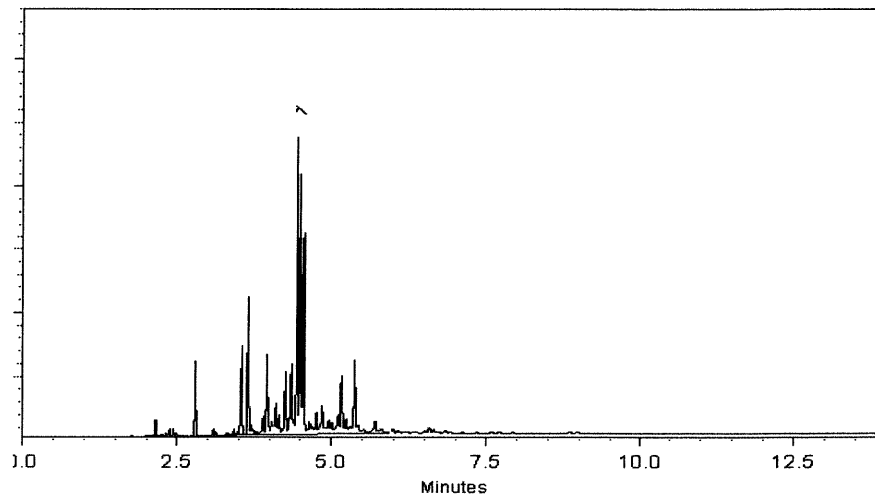

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Josh McCloskey - Operations Technician I

Date Mixed: 11-Feb-2022


Balance: B442140311


Marlene Cowan - Operations Tech I

Date Passed: 24-Feb-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 11892 / (5)
P 11896 /


06/17/2022



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32291 **Lot No.:** A0162166

Description : Organochlorine Pesticide Mix AB #1

Organochlorine Pesticide Mix AB #1 200µg/mL, Hexane/Toluene(50:50), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : June 30, 2024 **Storage:** 10°C or colder

Handwritten notes:
P10336
P10340
P10341
P10345
AR
03/8/21

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	alpha-BHC CAS # 319-84-6 (Lot 0012018BHC) Purity 99%	202.0 µg/mL	+/- 1.4323 µg/mL Gravimetric +/- 9.2360 µg/mL Unstressed +/- 13.3092 µg/mL Stressed
2	gamma-BHC (Lindane) CAS # 58-89-9 (Lot 9823200) Purity 99%	201.5 µg/mL	+/- 1.4288 µg/mL Gravimetric +/- 9.2131 µg/mL Unstressed +/- 13.2763 µg/mL Stressed
3	beta-BHC CAS # 319-85-7 (Lot G138918) Purity 99%	201.0 µg/mL	+/- 1.4253 µg/mL Gravimetric +/- 9.1903 µg/mL Unstressed +/- 13.2433 µg/mL Stressed
4	delta-BHC CAS # 319-86-8 (Lot ER02101401) Purity 99%	201.5 µg/mL	+/- 1.4288 µg/mL Gravimetric +/- 9.2131 µg/mL Unstressed +/- 13.2763 µg/mL Stressed
5	Heptachlor CAS # 76-44-8 (Lot 0006530009) Purity 99%	201.0 µg/mL	+/- 1.4253 µg/mL Gravimetric +/- 9.1903 µg/mL Unstressed +/- 13.2433 µg/mL Stressed
6	Aldrin CAS # 309-00-2 (Lot 9298200) Purity 97%	200.3 µg/mL	+/- 1.4203 µg/mL Gravimetric +/- 9.1585 µg/mL Unstressed +/- 13.1975 µg/mL Stressed
7	Heptachlor epoxide (isomer B) CAS # 1024-57-3 (Lot 10039000) Purity 99%	201.5 µg/mL	+/- 1.4288 µg/mL Gravimetric +/- 9.2131 µg/mL Unstressed +/- 13.2763 µg/mL Stressed

8	trans-Chlordane			201.0	µg/mL	+/-	1.4253	µg/mL	Gravimetric
	CAS #	5103-74-2	(Lot ER061906-04)			+/-	9.1903	µg/mL	Unstressed
	Purity	99%				+/-	13.2433	µg/mL	Stressed
9	cis-Chlordane			201.0	µg/mL	+/-	1.4253	µg/mL	Gravimetric
	CAS #	5103-71-9	(Lot 31707)			+/-	9.1903	µg/mL	Unstressed
	Purity	99%				+/-	13.2433	µg/mL	Stressed
10	Endosulfan I			200.0	µg/mL	+/-	1.4182	µg/mL	Gravimetric
	CAS #	959-98-8	(Lot BCBS8631)			+/-	9.1446	µg/mL	Unstressed
	Purity	99%				+/-	13.1774	µg/mL	Stressed
11	4,4'-DDE			200.0	µg/mL	+/-	1.4182	µg/mL	Gravimetric
	CAS #	72-55-9	(Lot GHYQG)			+/-	9.1446	µg/mL	Unstressed
	Purity	99%				+/-	13.1774	µg/mL	Stressed
12	Dieldrin			201.4	µg/mL	+/-	1.4280	µg/mL	Gravimetric
	CAS #	60-57-1	(Lot 9448800)			+/-	9.2081	µg/mL	Unstressed
	Purity	98%				+/-	13.2690	µg/mL	Stressed
13	Endrin			201.9	µg/mL	+/-	1.4315	µg/mL	Gravimetric
	CAS #	72-20-8	(Lot 9863200)			+/-	9.2305	µg/mL	Unstressed
	Purity	98%				+/-	13.3013	µg/mL	Stressed
14	4,4'-DDD			201.5	µg/mL	+/-	1.4288	µg/mL	Gravimetric
	CAS #	72-54-8	(Lot HAN02)			+/-	9.2131	µg/mL	Unstressed
	Purity	99%				+/-	13.2763	µg/mL	Stressed
15	Endosulfan II			201.0	µg/mL	+/-	1.4253	µg/mL	Gravimetric
	CAS #	33213-65-9	(Lot 8999300)			+/-	9.1903	µg/mL	Unstressed
	Purity	99%				+/-	13.2433	µg/mL	Stressed
16	4,4'-DDT			200.0	µg/mL	+/-	1.4182	µg/mL	Gravimetric
	CAS #	50-29-3	(Lot S37912V)			+/-	9.1446	µg/mL	Unstressed
	Purity	99%				+/-	13.1774	µg/mL	Stressed
17	Endrin aldehyde			200.5	µg/mL	+/-	1.4217	µg/mL	Gravimetric
	CAS #	7421-93-4	(Lot 30606)			+/-	9.1674	µg/mL	Unstressed
	Purity	99%				+/-	13.2104	µg/mL	Stressed
18	Endosulfan sulfate			202.0	µg/mL	+/-	1.4323	µg/mL	Gravimetric
	CAS #	1031-07-8	(Lot BCCB0424)			+/-	9.2360	µg/mL	Unstressed
	Purity	99%				+/-	13.3092	µg/mL	Stressed
19	Methoxychlor			201.5	µg/mL	+/-	1.4288	µg/mL	Gravimetric
	CAS #	72-43-5	(Lot 9863300)			+/-	9.2131	µg/mL	Unstressed
	Purity	99%				+/-	13.2763	µg/mL	Stressed
20	Endrin ketone			200.5	µg/mL	+/-	1.4217	µg/mL	Gravimetric
	CAS #	53494-70-5	(Lot 9985500)			+/-	9.1674	µg/mL	Unstressed
	Purity	99%				+/-	13.2104	µg/mL	Stressed
Solvent:	Hexane/Toluene (50:50)								
	CAS #	110-54-3/108-88-3							
	Purity	99%							

Column:

1 x .25mm x .2um
CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

150°C to 300°C
@ 4°C/min. (hold 5 min.)

Inj. Temp:


200°C

Det. Temp:

300°C

Det. Type:

ECD

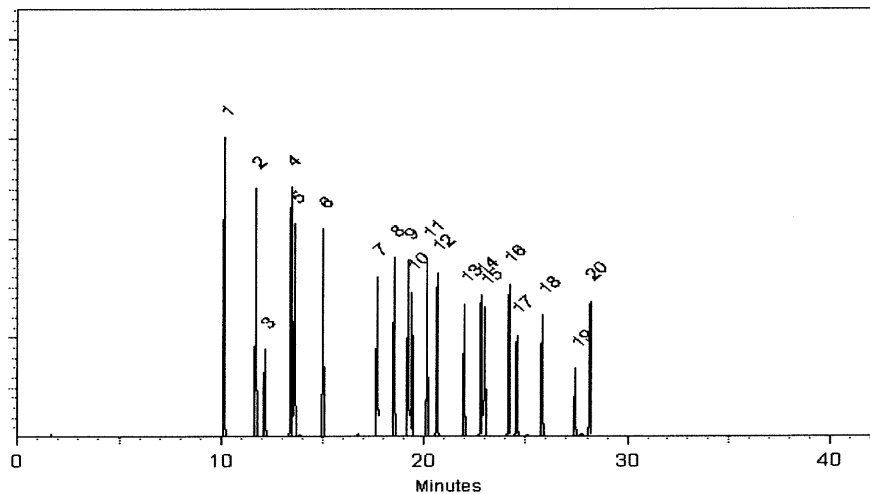

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Cory Meyer
Cory Meyer - Operations Tech I

Date Mixed: 29-Jun-2020

Balance: 1128353505

Jennifer Pollino
Jennifer Pollino - Operations Tech-ARM QC

Date Passed: 06-Jul-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



Certificate of Analysis

Product Name: Pesticides Resolution Check Standard

Product Number: CLP-242-1

Lot Issue Date: 08-Jul-2021

Lot Number: 0006617274

Expiration Date: 31-Aug-2023

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration \pm Uncertainty
trans-chlordane	005103-74-2	RM02726	10.0 \pm 0.1 ng/mL
4,4'-DDE	000072-55-9	RM02892	20.1 \pm 0.1 ng/mL
decachlorobiphenyl (BZ # 209)	002051-24-3	RM01256	20.1 \pm 0.1 ng/mL
dieldrin	000060-57-1	RM16038	20.0 \pm 0.1 ng/mL
endosulfan I	000959-98-8	RM15536	10.0 \pm 0.1 ng/mL
endosulfan sulfate	001031-07-8	RM15389	20.0 \pm 0.1 ng/mL
endrin ketone	053494-70-5	NT00720	20.0 \pm 0.1 ng/mL
methoxychlor	000072-43-5	RM14186	100.1 \pm 0.5 ng/mL
2,4,5,6-tetrachloro-m-xylene	000877-09-8	RM13844	20.1 \pm 0.1 ng/mL

Matrix: hexane

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

P 10883

↓

P 10902

AJ
07/13/21



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 1 of 2

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937

Certificate of Analysis

Product Number: CLP-242-1

Lot Number: 0006617274

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.


Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:



Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32291 **Lot No.:** A0168439

Description : Organochlorine Pesticide Mix AB #1

Organochlorine Pesticide Mix AB #1 200µg/mL, Hexane/Toluene(50:50), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2025 **Storage:** 10°C or colder

Ship: Ambient

P11061
↓
P11065
AR
9/30/2024

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	alpha-BHC CAS # 319-84-6 (Lot 0012018BHC) Purity 99%	200.5 µg/mL	+/- 1.4217 µg/mL Gravimetric +/- 9.1674 µg/mL Unstressed +/- 13.2104 µg/mL Stressed
2	gamma-BHC (Lindane) CAS # 58-89-9 (Lot 10972000) Purity 97%	200.8 µg/mL	+/- 1.4238 µg/mL Gravimetric +/- 9.1807 µg/mL Unstressed +/- 13.2295 µg/mL Stressed
3	beta-BHC CAS # 319-85-7 (Lot SL210106) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL Gravimetric +/- 9.1446 µg/mL Unstressed +/- 13.1774 µg/mL Stressed
4	delta-BHC CAS # 319-86-8 (Lot ER02101401) Purity 98%	199.9 µg/mL	+/- 1.4176 µg/mL Gravimetric +/- 9.1409 µg/mL Unstressed +/- 13.1722 µg/mL Stressed
5	Heptachlor CAS # 76-44-8 (Lot 0006540595) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL Gravimetric +/- 9.1446 µg/mL Unstressed +/- 13.1774 µg/mL Stressed
6	Aldrin CAS # 309-00-2 (Lot 11129800) Purity 97%	199.8 µg/mL	+/- 1.4169 µg/mL Gravimetric +/- 9.1363 µg/mL Unstressed +/- 13.1656 µg/mL Stressed
7	Heptachlor epoxide (isomer B) CAS # 1024-57-3 (Lot 10039000) Purity 99%	200.5 µg/mL	+/- 1.4217 µg/mL Gravimetric +/- 9.1674 µg/mL Unstressed +/- 13.2104 µg/mL Stressed

8	trans-Chlordane CAS # 5103-74-2 Purity 99%	(Lot 32095)	200.5 µg/mL	+/- +/- +/-	1.4217 9.1674 13.2104	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	cis-Chlordane CAS # 5103-71-9 Purity 99%	(Lot 31707)	200.0 µg/mL	+/- +/- +/-	1.4182 9.1446 13.1774	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	Endosulfan I CAS # 959-98-8 Purity 99%	(Lot BCBS8631)	200.5 µg/mL	+/- +/- +/-	1.4217 9.1674 13.2104	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	4,4'-DDE CAS # 72-55-9 Purity 99%	(Lot GHYQG)	200.0 µg/mL	+/- +/- +/-	1.4182 9.1446 13.1774	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	Dieldrin CAS # 60-57-1 Purity 98%	(Lot 10714300)	200.4 µg/mL	+/- +/- +/-	1.4211 9.1633 13.2045	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	Endrin CAS # 72-20-8 Purity 98%	(Lot 11129700)	199.9 µg/mL	+/- +/- +/-	1.4176 9.1409 13.1722	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	4,4'-DDD CAS # 72-54-8 Purity 99%	(Lot HAN02)	200.5 µg/mL	+/- +/- +/-	1.4217 9.1674 13.2104	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	Endosulfan II CAS # 33213-65-9 Purity 99%	(Lot 11129400)	201.0 µg/mL	+/- +/- +/-	1.4253 9.1903 13.2433	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	4,4'-DDT CAS # 50-29-3 Purity 99%	(Lot S37912V)	200.0 µg/mL	+/- +/- +/-	1.4182 9.1446 13.1774	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	Endrin aldehyde CAS # 7421-93-4 Purity 98%	(Lot 30455)	200.9 µg/mL	+/- +/- +/-	1.4245 9.1857 13.2367	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
18	Endosulfan sulfate CAS # 1031-07-8 Purity 99%	(Lot BCCB0424)	200.0 µg/mL	+/- +/- +/-	1.4182 9.1446 13.1774	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
19	Methoxychlor CAS # 72-43-5 Purity 97%	(Lot 10720900)	199.8 µg/mL	+/- +/- +/-	1.4169 9.1363 13.1656	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
20	Endrin ketone CAS # 53494-70-5 Purity 97%	(Lot 11129600)	199.8 µg/mL	+/- +/- +/-	1.4169 9.1363 13.1656	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
Solvent: Hexane/Toluene (50:50) CAS # 110-54-3/108-88-3 Purity 99%							

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
150°C to 300°C
@ 4°C/min. (hold 5 min.)

Inj. Temp:
200°C

Det. Temp:
300°C

Det. Type:
ECD

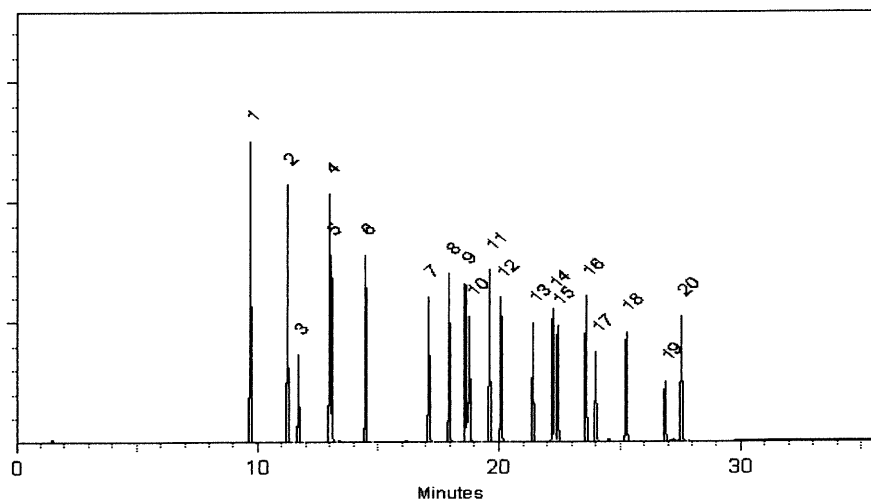

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Matt Fragassi - Mix Technician

Date Mixed: 25-Jan-2021

Balance: 1128342314


Marlene Cowan - Operations Tech I

Date Passed: 29-Jan-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11061
↓
P11065
AR
9/30/2021

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32291 **Lot No.:** A0168439

Description : Organochlorine Pesticide Mix AB #1

Organochlorine Pesticide Mix AB #1 200µg/mL, Hexane/Toluene(50:50), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2025 **Storage:** 10°C or colder

Ship: Ambient

P11061
↓
P11065
AR
9/30/2024

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	alpha-BHC CAS # 319-84-6 (Lot 0012018BHC) Purity 99%	200.5 µg/mL	+/- 1.4217 µg/mL Gravimetric +/- 9.1674 µg/mL Unstressed +/- 13.2104 µg/mL Stressed
2	gamma-BHC (Lindane) CAS # 58-89-9 (Lot 10972000) Purity 97%	200.8 µg/mL	+/- 1.4238 µg/mL Gravimetric +/- 9.1807 µg/mL Unstressed +/- 13.2295 µg/mL Stressed
3	beta-BHC CAS # 319-85-7 (Lot SL210106) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL Gravimetric +/- 9.1446 µg/mL Unstressed +/- 13.1774 µg/mL Stressed
4	delta-BHC CAS # 319-86-8 (Lot ER02101401) Purity 98%	199.9 µg/mL	+/- 1.4176 µg/mL Gravimetric +/- 9.1409 µg/mL Unstressed +/- 13.1722 µg/mL Stressed
5	Heptachlor CAS # 76-44-8 (Lot 0006540595) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL Gravimetric +/- 9.1446 µg/mL Unstressed +/- 13.1774 µg/mL Stressed
6	Aldrin CAS # 309-00-2 (Lot 11129800) Purity 97%	199.8 µg/mL	+/- 1.4169 µg/mL Gravimetric +/- 9.1363 µg/mL Unstressed +/- 13.1656 µg/mL Stressed
7	Heptachlor epoxide (isomer B) CAS # 1024-57-3 (Lot 10039000) Purity 99%	200.5 µg/mL	+/- 1.4217 µg/mL Gravimetric +/- 9.1674 µg/mL Unstressed +/- 13.2104 µg/mL Stressed

8	trans-Chlordane CAS # 5103-74-2 Purity 99%	(Lot 32095)	200.5 µg/mL	+/- +/- +/-	1.4217 9.1674 13.2104	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	cis-Chlordane CAS # 5103-71-9 Purity 99%	(Lot 31707)	200.0 µg/mL	+/- +/- +/-	1.4182 9.1446 13.1774	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	Endosulfan I CAS # 959-98-8 Purity 99%	(Lot BCBS8631)	200.5 µg/mL	+/- +/- +/-	1.4217 9.1674 13.2104	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	4,4'-DDE CAS # 72-55-9 Purity 99%	(Lot GHYQG)	200.0 µg/mL	+/- +/- +/-	1.4182 9.1446 13.1774	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	Dieldrin CAS # 60-57-1 Purity 98%	(Lot 10714300)	200.4 µg/mL	+/- +/- +/-	1.4211 9.1633 13.2045	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	Endrin CAS # 72-20-8 Purity 98%	(Lot 11129700)	199.9 µg/mL	+/- +/- +/-	1.4176 9.1409 13.1722	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	4,4'-DDD CAS # 72-54-8 Purity 99%	(Lot HAN02)	200.5 µg/mL	+/- +/- +/-	1.4217 9.1674 13.2104	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	Endosulfan II CAS # 33213-65-9 Purity 99%	(Lot 11129400)	201.0 µg/mL	+/- +/- +/-	1.4253 9.1903 13.2433	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	4,4'-DDT CAS # 50-29-3 Purity 99%	(Lot S37912V)	200.0 µg/mL	+/- +/- +/-	1.4182 9.1446 13.1774	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	Endrin aldehyde CAS # 7421-93-4 Purity 98%	(Lot 30455)	200.9 µg/mL	+/- +/- +/-	1.4245 9.1857 13.2367	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
18	Endosulfan sulfate CAS # 1031-07-8 Purity 99%	(Lot BCCB0424)	200.0 µg/mL	+/- +/- +/-	1.4182 9.1446 13.1774	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
19	Methoxychlor CAS # 72-43-5 Purity 97%	(Lot 10720900)	199.8 µg/mL	+/- +/- +/-	1.4169 9.1363 13.1656	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
20	Endrin ketone CAS # 53494-70-5 Purity 97%	(Lot 11129600)	199.8 µg/mL	+/- +/- +/-	1.4169 9.1363 13.1656	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
Solvent: Hexane/Toluene (50:50) CAS # 110-54-3/108-88-3 Purity 99%							

Column:
30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
150°C to 300°C
@ 4°C/min. (hold 5 min.)

Inj. Temp:
200°C

Det. Temp:
300°C

Det. Type:
ECD

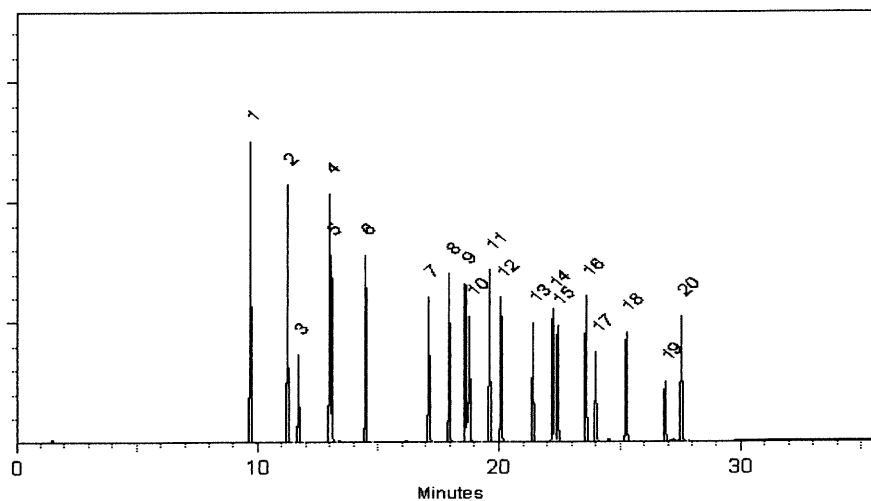

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Matt Fragassi - Mix Technician

Date Mixed: 25-Jan-2021

Balance: 1128342314


Marlene Cowan - Operations Tech I

Date Passed: 29-Jan-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P11061
↓
P11065
AR
9/30/2021

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:


- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



Certified Reference Material CRM



CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

79136
102821
Mirex

Solvent(s):
Lot#
Acetone **81025**

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

102826
Refrigerate (4 °C)
1000
6UTB

5E-05 **Balance Uncertainty**
0.006 **Flask Uncertainty**


Weight(s) shown below were combined and diluted to (mL):

50.0

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded SDS Information		
									Uncertainty (+/-) (µg/mL)	(Solvent Safety Info. On Attached pg.)	(SHA PEL (TWA) LD50)

1. Mirex	437	9492400	1000	99.4	0.5	0.05034	0.05039	1000.9	10.3	2385-85-5	N/A	orl-rat 306mg/kg
----------	-----	---------	------	------	-----	---------	---------	--------	------	-----------	-----	------------------


Method GC7MSD-1.M: Column: SPB-608 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (4min.), Temp 2 = 290°C (13.5 min.), Rate = 8°C/min., Injector B = 200°C, Detector B = 290°C. Split Ratio = 100:1, Scan Rate = 2. Analysis performed by Candice Warren.

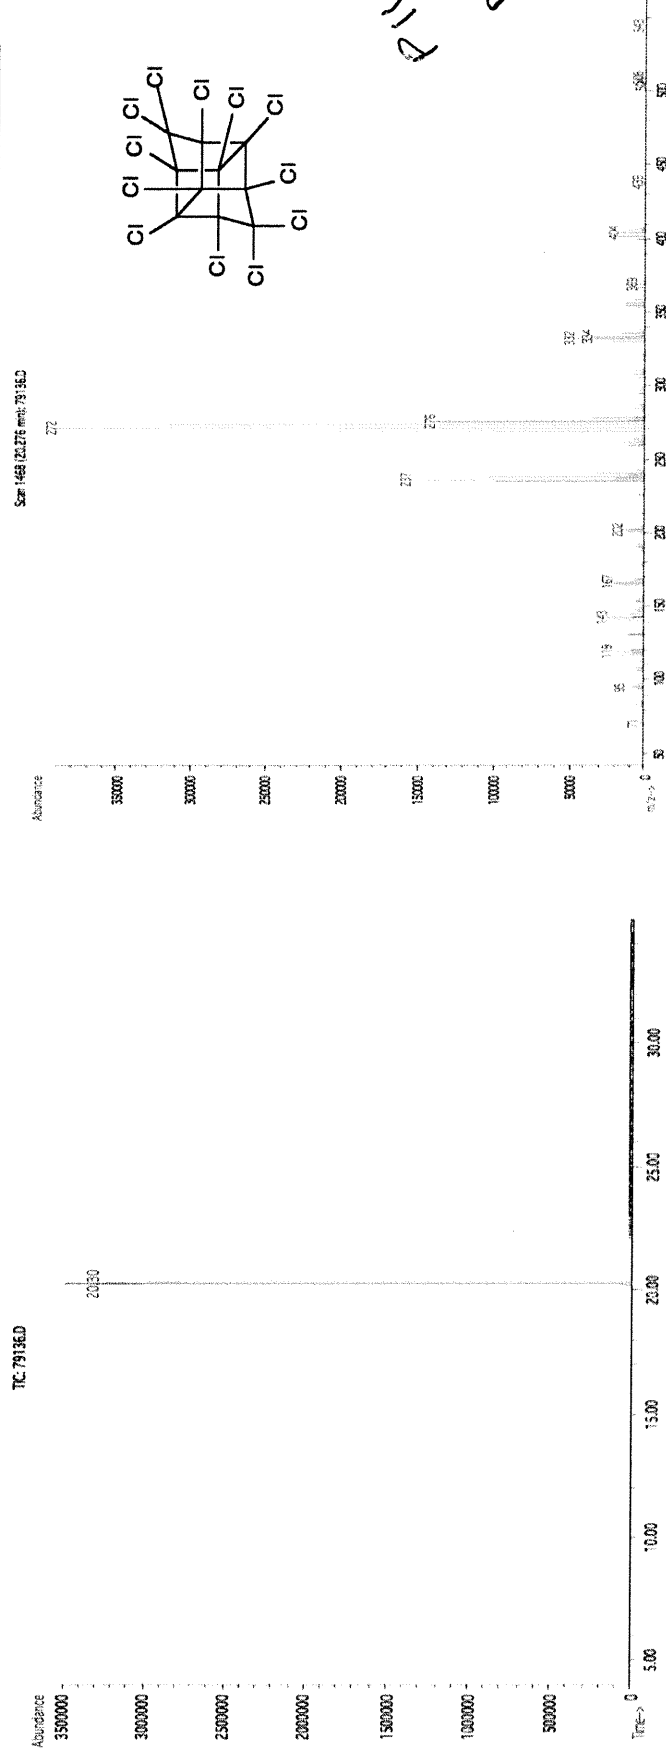

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Certified Reference Material CRM



CERTIFIED WEIGHT REPORT

Part Number:
Lot Number:
Description:

79136
102821
Mirex

Solvent(s):
Lot#
Acetone **81025**

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test ID#:

102826
Refrigerate (4 °C)
1000
6UTB

5E-05 **Balance Uncertainty**
0.006 **Flask Uncertainty**

Weight(s) shown below were combined and diluted to (mL):


50.0

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded SDS Information		
									Uncertainty (+/-) (µg/mL)	(Solvent Safety Info. On Attached pg.)	(SHA PEL (TWA) LD50)



1. Mirex	437	9492400	1000	99.4	0.5	0.05034	0.05039	1000.9	10.3	2385-85-5	N/A	orl-rat 306mg/kg
----------	-----	---------	------	------	-----	---------	---------	--------	------	-----------	-----	------------------

Method GC7MSD-1.M: Column: SPB-608 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (4min.), Temp 2 = 290°C (13.5 min.), Rate = 8°C/min., Injector B = 200°C, Detector B = 290°C. Split Ratio = 100:1, Scan Rate = 2. Analysis performed by Candice Warren.

TC: 79136.D

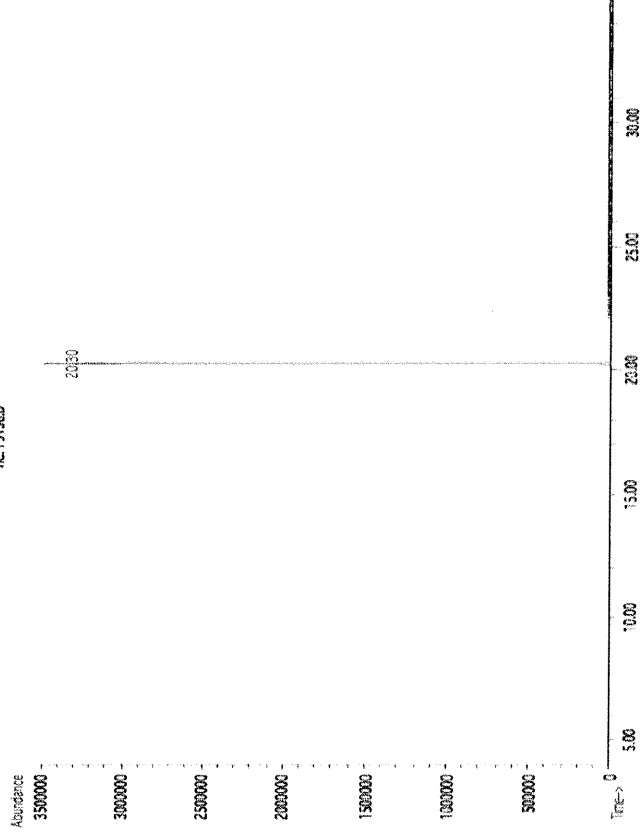

Scan 1468 (20.26 min): 79136.D

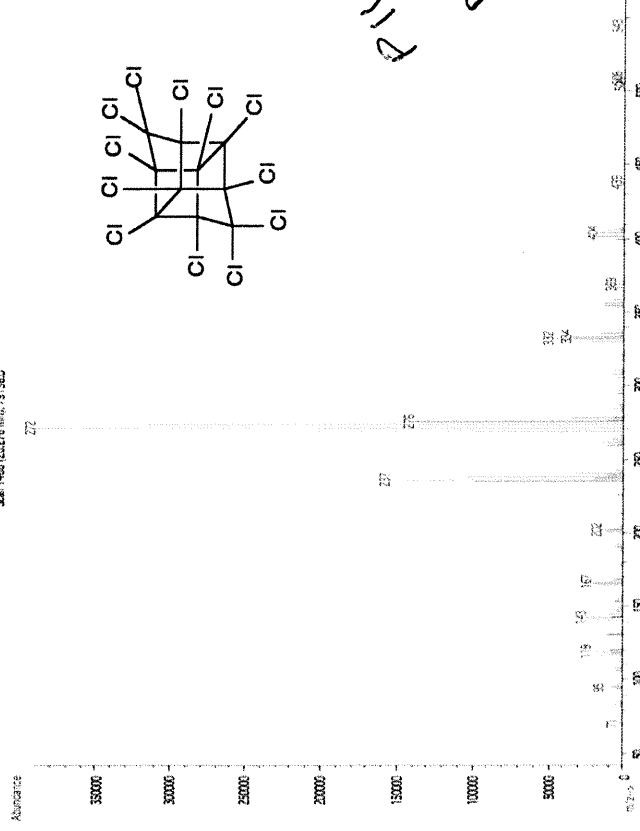

Handwritten: P1142
P1146
11/02/21

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).




CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32005 **Lot No.:** A0176614

Description: Toxaphene Standard

Toxaphene Standard 1000 µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: December 31, 2025 **Storage:** 10°C or colder

Ship: Ambient

P11384 AJ
P11393 02/09/22

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Toxaphene CAS # 8001-35-2 Purity ---%	(Lot 1051817) 1,005.3 µg/mL	+/- 5.9714 µg/mL +/- 31.8763 µg/mL +/- 41.6339 µg/mL
			Gravimetric Unstressed Stressed

Solvent: Hexane

CAS # 110-54-3
Purity 99%

Column:

30m x .25mm x .2um
Rtx-CLP II (Cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

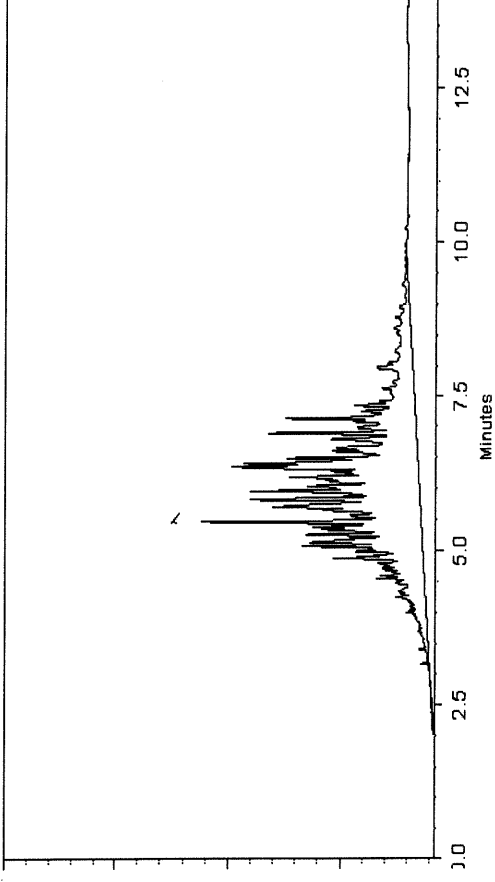

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Buddy Meyer
Buddy Meyer - Sales Technician

Date Mixed: 21-Sep-2021 Balance: 1128360905

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 22-Sep-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397




CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32005 **Lot No.:** A0176614

Description: Toxaphene Standard

Toxaphene Standard 1000 µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL **Pkg Amt:** > 1 mL

Expiration Date: December 31, 2025 **Storage:** 10°C or colder

Ship: Ambient

P11384 AJ
P11393 02/09/22

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Toxaphene CAS # 8001-35-2 Purity ---%	1,005.3 µg/mL (Lot 1051817)	+/- 5.9714 µg/mL +/- 31.8763 µg/mL +/- 41.6339 µg/mL

Solvent:

Hexane
CAS # 110-54-3
Purity 99%

Gravimetric
Unstressed
Stressed

Column:

30m x .25mm x .2um
Rtx-CLP II (Cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

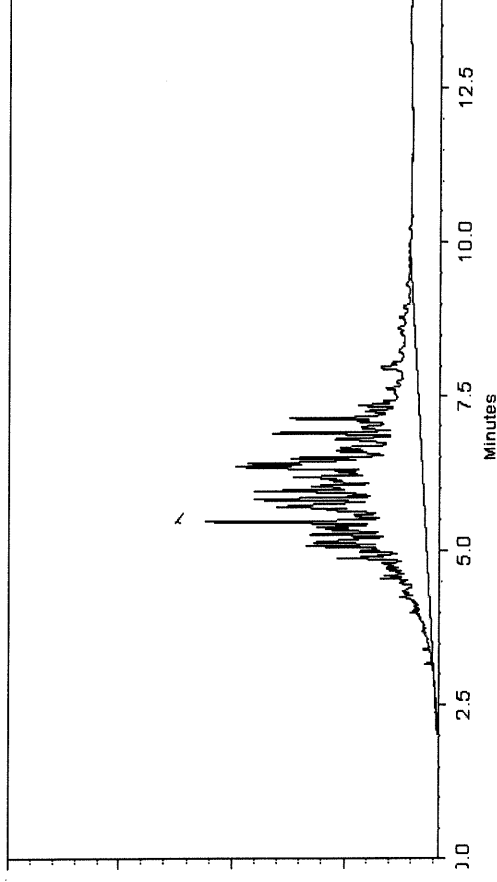

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Buddy Meyer
Buddy Meyer - Sales Technician

Date Mixed: 21-Sep-2021 Balance: 1128360905

Marlene Cowan
Marlene Cowan - Operations Tech I

Date Passed: 22-Sep-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis

P11739 to P11748

Received by SJ 5/27/2022



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0179404

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : March 31, 2028 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene CAS # 877-09-8 (Lot 0052481) Purity 98%	200.7 µg/mL	+/- 1.1840 µg/mL Gravimetric +/- 6.3622 µg/mL Unstressed +/- 8.3106 µg/mL Stressed
2	Decachlorobiphenyl (BZ# 209) CAS # 2051-24-3 (Lot 30679) Purity 99%	200.8 µg/mL	+/- 1.1845 µg/mL Gravimetric +/- 6.3653 µg/mL Unstressed +/- 8.3146 µg/mL Stressed

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

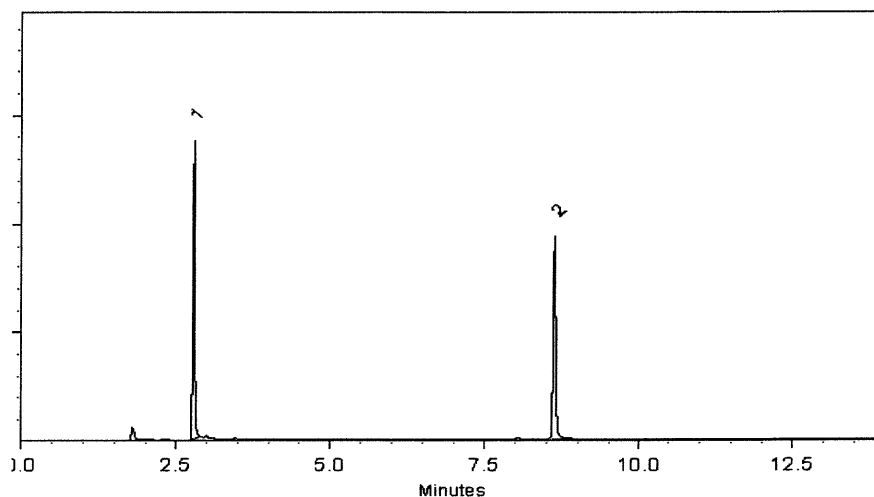


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Matt Fragassi - Mix Technician

Date Mixed: 09-Dec-2021

Balance: 1127510105


Clara Windle - Operations Technician I

Date Passed: 14-Dec-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis

P11789 to P11793

Received by SJ 5/27/2022



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32074 **Lot No.:** A0183168

Description : Pesticide Performance Eval Mix w/Surrogate

Performance Evaluation Std. 3/90 SOW w/surrogates 1-25µg/mL,
Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : March 31, 2026 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	2,4,5,6-Tetrachloro-m-xylene CAS # 877-09-8 (Lot 0052481) Purity 98%	2.0 µg/mL	+/- 0.1220 +/- 0.1523 +/- 0.1799	µg/mL Gravimetric Unstressed Stressed
2	alpha-BHC CAS # 319-84-6 (Lot 12469000) Purity 99%	1.0 µg/mL	+/- 0.0610 +/- 0.0762 +/- 0.0900	µg/mL Gravimetric Unstressed Stressed
3	gamma-BHC (Lindane) CAS # 58-89-9 (Lot 12642100) Purity 99%	1.0 µg/mL	+/- 0.0610 +/- 0.0762 +/- 0.0900	µg/mL Gravimetric Unstressed Stressed
4	beta-BHC CAS # 319-85-7 (Lot BCCCC6425) Purity 99%	1.0 µg/mL	+/- 0.0610 +/- 0.0762 +/- 0.0900	µg/mL Gravimetric Unstressed Stressed
5	Endrin CAS # 72-20-8 (Lot 13000500) Purity 99%	5.1 µg/mL	+/- 0.3045 +/- 0.3805 +/- 0.4496	µg/mL Gravimetric Unstressed Stressed
6	4,4'-DDT CAS # 50-29-3 (Lot 210916JLM) Purity 99%	10.1 µg/mL	+/- 0.6090 +/- 0.7609 +/- 0.8992	µg/mL Gravimetric Unstressed Stressed
7	Methoxychlor CAS # 72-43-5 (Lot 12555700) Purity 98%	25.2 µg/mL	+/- 1.5221 +/- 1.9018 +/- 2.2475	µg/mL Gravimetric Unstressed Stressed

8	Decachlorobiphenyl (BZ# 209)	2.0 µg/mL	+/- 0.1221	µg/mL	Gravimetric
	CAS # 2051-24-3 (Lot 30679)		+/- 0.1524	µg/mL	Unstressed
	Purity 99%		+/- 0.1800	µg/mL	Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:
30m x .25mm x .2µm
Rtx-CLP II (cat.# 11323)


Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
150°C to 300°C
@ 4°C/min. (hold 5 min.)

Inj. Temp:
200°C

Det. Temp:
300°C


Det. Type:
ECD

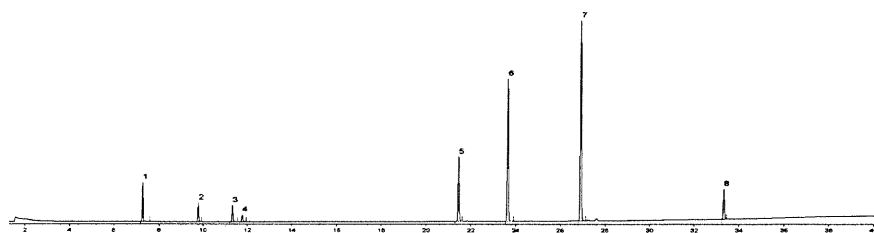

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Brittany Federinko - Operations Tech I

Date Mixed: 22-Mar-2022 **Balance:** 1128360905


John Lidgett - AD Chemist

Date Passed: 24-Mar-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

P11794 to P11798

Received by SJ 5/27/2022



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32074 **Lot No.:** A0183168

Description : Pesticide Performance Eval Mix w/Surrogate

Performance Evaluation Std. 3/90 SOW w/surrogates 1-25µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : March 31, 2026 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene CAS # 877-09-8 (Lot 0052481) Purity 98%	2.0 µg/mL	+/- 0.1220 µg/mL Gravimetric +/- 0.1523 µg/mL Unstressed +/- 0.1799 µg/mL Stressed
2	alpha-BHC CAS # 319-84-6 (Lot 12469000) Purity 99%	1.0 µg/mL	+/- 0.0610 µg/mL Gravimetric +/- 0.0762 µg/mL Unstressed +/- 0.0900 µg/mL Stressed
3	gamma-BHC (Lindane) CAS # 58-89-9 (Lot 12642100) Purity 99%	1.0 µg/mL	+/- 0.0610 µg/mL Gravimetric +/- 0.0762 µg/mL Unstressed +/- 0.0900 µg/mL Stressed
4	beta-BHC CAS # 319-85-7 (Lot BCCC6425) Purity 99%	1.0 µg/mL	+/- 0.0610 µg/mL Gravimetric +/- 0.0762 µg/mL Unstressed +/- 0.0900 µg/mL Stressed
5	Endrin CAS # 72-20-8 (Lot 13000500) Purity 99%	5.1 µg/mL	+/- 0.3045 µg/mL Gravimetric +/- 0.3805 µg/mL Unstressed +/- 0.4496 µg/mL Stressed
6	4,4'-DDT CAS # 50-29-3 (Lot 210916JLM) Purity 99%	10.1 µg/mL	+/- 0.6090 µg/mL Gravimetric +/- 0.7609 µg/mL Unstressed +/- 0.8992 µg/mL Stressed
7	Methoxychlor CAS # 72-43-5 (Lot 12555700) Purity 98%	25.2 µg/mL	+/- 1.5221 µg/mL Gravimetric +/- 1.9018 µg/mL Unstressed +/- 2.2475 µg/mL Stressed

8	Decachlorobiphenyl (BZ# 209)	2.0 µg/mL	+/- 0.1221	µg/mL	Gravimetric
	CAS # 2051-24-3 (Lot 30679)		+/- 0.1524	µg/mL	Unstressed
	Purity 99%		+/- 0.1800	µg/mL	Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:
 30m x .25mm x .2um
 Rtx-CLP II (cat.# 11323)


Carrier Gas:
 helium-constant pressure 20 psi.

Temp. Program:
 150°C to 300°C
 @ 4°C/min. (hold 5 min.)

Inj. Temp:
 200°C

Det. Temp:
 300°C

Det. Type:
 ECD

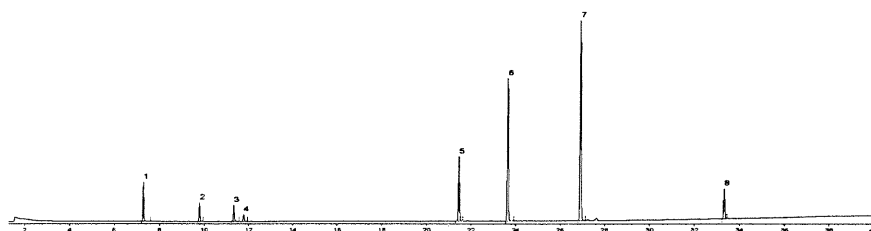

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brittany Federinko
 Brittany Federinko - Operations Tech I

Date Mixed: 22-Mar-2022 **Balance:** 1128360905

John Lidgett
 John Lidgett - AD Chemist

Date Passed: 24-Mar-2022

Manufactured under Restek's ISO 9001:2015
 Registered Quality System
 Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32005 Lot No.: A0177326
Description : Toxaphene Standard
Toxaphene Standard 1000 µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : January 31, 2026 Storage: 10°C or colder
Ship: Ambient

P11811
✓
P11819
AJ
06/17/22

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Toxaphene	1,004.7 µg/mL	+/- 5.9674 µg/mL Gravimetric
	CAS # 8001-35-2 (Lot 1051817)		+/- 31.8552 µg/mL Unstressed
	Purity ----%		+/- 41.6063 µg/mL Stressed

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

300°C

Det. Type:

ECD

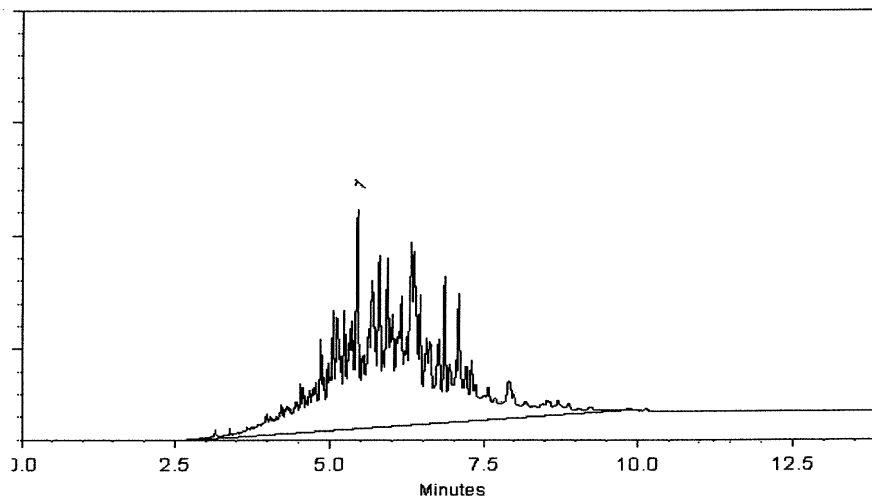

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler

Sam Moodler - Operations Tech I

Date Mixed: 11-Oct-2021

Balance: B442140311

Marlina Cowan

Marlina Cowan - Operations Tech I

Date Passed: 14-Oct-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32000 **Lot No.:** A0192797
Description: Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul
Container Size: 2 mL **Pkg Amt:** > 1 mL
Expiration Date: March 31, 2029 **Storage:** 10°C or colder
Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	201.1 µg/mL	+/- 11.1565
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	201.2 µg/mL	+/- 11.1620

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

P12401
↓
P12405 (5)

RAUF
03.21.2023

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1µl

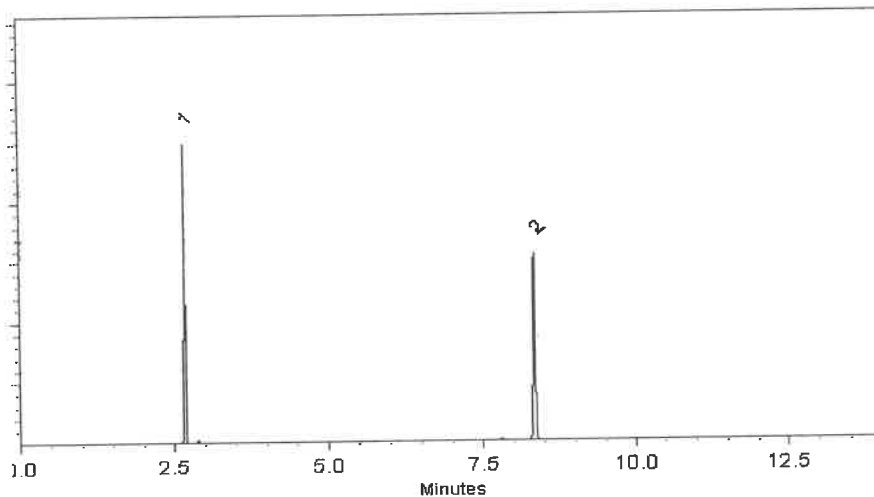

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Jess Hoy - Operations Tech I


Date Mixed: 19-Dec-2022

Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 21-Dec-2022

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P12401
↓
P12405

03.21.2023



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis *chromatographic plus*



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32021 Lot No.: A0197993
Description: Chlordane Standard
Chlordane Standard 1000µg/mL, Hexane, 1mL/ampul
Container Size: 2 mL Pkg Amt: > 1 mL
Expiration Date: August 31, 2029 Storage: 10°C or colder
Ship: Ambient

Handwritten: P 12606, P 12610, 5 Five, 7/3/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	Chlordane 10% trans-Chlordane; 9% cis-Chlordane; 81% other isomers	57-74-9	978545	----	1,005.0 µg/mL	+/- 55.7700

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Tech Tips:

CAS #57-74-9 nomenclature is based on EPA method 8081B.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. { hold 10 min.}

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

0.2µl

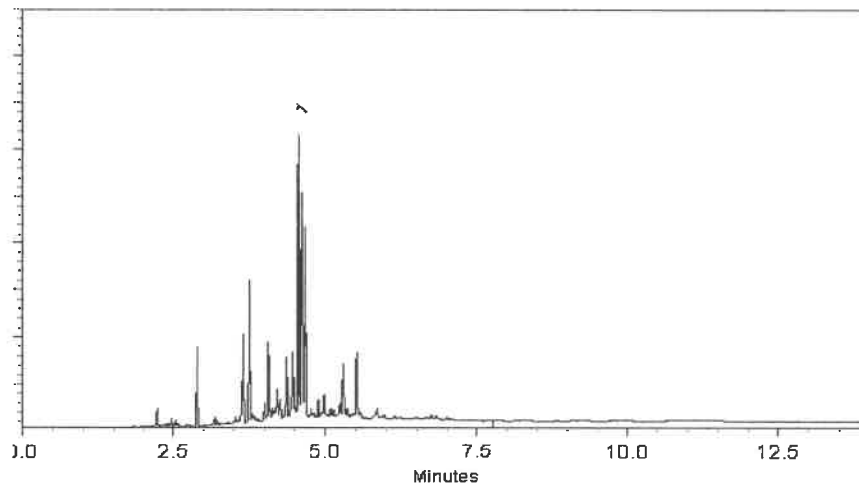

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Morgan Craighead - Mix Technician


Date Mixed: 11-May-2023

Balance Serial # 1128360905

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 16-May-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED WEIGHT REPORT


Part Number: 72072
Lot Number: 112018
Description: n-Tetracosane-d50
Expiration Date: 112028
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 2684186
Weight(s) shown below were combined and diluted to (mL): 200.0

Solvent(s): Methylene chloride
Lot#: 102669
Received by
SG on 11/11/19
p9044-p9053
5E-05 Balance Uncertainty
0.058 Flask Uncertainty


Formulated By:	Prashant Chauhan	112018	DATE
Reviewed By:	Pedro Rentas	112018	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)
1. n-Tetracosane-d50	2072	PR-17753/09216TC1	1000	98	0.2	0.20411	0.20415	1000.2	4.2	18416-32-3 N/A
Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.										

TC 720720

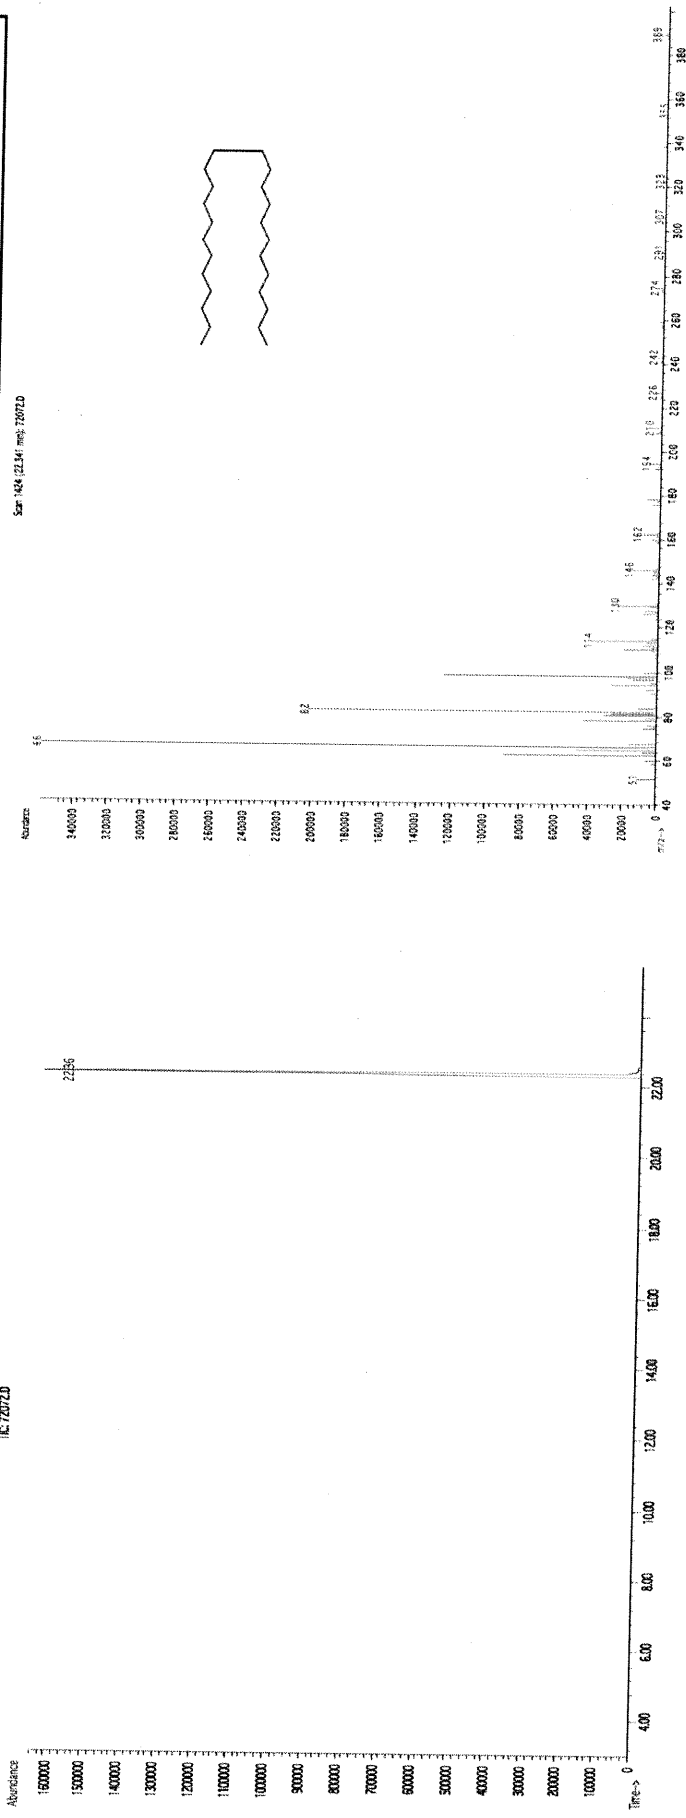

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
• Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
• All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
• Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Run 40, "P72072 L112018 [1000µg/mL in MeCl2]"

Run Length: 35.00 min, 20999 points at 10 points/second.

Created: Thu, Nov 22, 2018 at 7:23:18 AM.

Sampled: Sequence "112018-GC4M1", Method "GC4-M1".

Analyzed using Method "GC4-M1".

Comments

GC4-M1 Analysis by Melissa Stonier

Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness

Flow rates: Total Flow = 300 mL/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL, Air (detector) = 360 mL

Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.

Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.

Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

