



## Prep Standard - Chemical Standard Summary

**Order ID :** O3572

**Test :** TPH GC

**Prepbatch ID :** PB154660,

**Sequence ID/Qc Batch ID:** FE083123,

**Standard ID :**

EP2372,PP22108,PP22137,PP22320,PP22321,PP22322,PP22323,PP22324,PP22325,PP22326,

**Chemical ID :**

E3412,E3515,E3518,E3532,E3548,P11476,P11477,P11576,P11577,P11855,P11856,P11857,P11858,P11968,P11969,P11971,

**284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900**

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	<a href="#">EP2372</a>	08/02/2023	10/23/2023	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	RUPESHKUMAR SHAH 08/02/2023
<b><u>FROM</u></b>	4000.00000gram of E3412 = Final Quantity: 4000.000 gram							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
147	20 PPM DRO Surrogate Spike Solution	<a href="#">PP22108</a>	06/08/2023	12/01/2023	Abdul Mirza	None	None	Ankita Jodhani 06/12/2023
<u>FROM</u>	1.00000ml of P11576 + 1.00000ml of P11577 + 1.00000ml of P11968 + 1.00000ml of P11969 + 196.00000ml of E3515 = Final Quantity: 200.000 ml							

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3609	20 PPM DRO SPIKE SOLUTION (RESTEK)	<a href="#">PP22137</a>	06/19/2023	12/13/2023	Yogesh Patel	None	None	Ankita Jodhani
06/20/2023								

**FROM** 1.00000ml of P11855 + 1.00000ml of P11856 + 48.00000ml of E3518 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
433	100/100 PPM DRO (Restek)	<a href="#">PP22320</a>	07/06/2023	12/08/2023	Yogesh Patel	None	None	Ankita Jodhani
07/06/2023								

**FROM** 1.00000ml of P11857 + 1.00000ml of P11858 + 1.00000ml of P11969 + 7.00000ml of E3532 = Final Quantity: 10.000 ml

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3796	100/100 PPM DRO STD (CPI)	<a href="#">PP22321</a>	07/06/2023	12/08/2023	Yogesh Patel	None	None	Ankita Jodhani
07/06/2023								

**FROM** 1.00000ml of P11476 + 1.00000ml of P11477 + 1.00000ml of P11971 + 7.00000ml of E3532 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
435	50 PPM ICC DRO STD (Restek)	<a href="#">PP22322</a>	07/06/2023	12/08/2023	Yogesh Patel	None	None	Ankita Jodhani
07/06/2023								

**FROM** 0.50000ml of E3532 + 0.50000ml of PP22320 = Final Quantity: 1.000 ml

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
437	20 PPM ICC DRO STD (Restek)	<a href="#">PP22323</a>	07/06/2023	12/08/2023	Yogesh Patel	None	None	Ankita Jodhani
07/06/2023								

**FROM** 0.80000ml of E3532 + 0.20000ml of PP22320 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
438	10 PPM ICC DRO STD (Restek)	<a href="#">PP22324</a>	07/06/2023	12/08/2023	Yogesh Patel	None	None	Ankita Jodhani
07/06/2023								

**FROM** 0.90000ml of E3532 + 0.10000ml of PP22320 = Final Quantity: 1.000 ml

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
439	5 PPM ICC DRO STD (Restek)	<a href="#">PP22325</a>	07/06/2023	12/08/2023	Yogesh Patel	None	None	Ankita Jodhani
07/06/2023								

**FROM** 0.90000ml of E3532 + 0.10000ml of PP22322 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3797	50 PPM DRO ICV STD (CPI)	<a href="#">PP22326</a>	07/06/2023	12/08/2023	Yogesh Patel	None	None	Ankita Jodhani
07/06/2023								

**FROM** 0.50000ml of E3532 + 0.50000ml of PP22321 = Final Quantity: 1.000 ml

**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	139404	10/23/2023	10/18/2022 / Rajesh	10/13/2022 / Rajesh	E3412

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	23C1362018	12/01/2023	06/01/2023 / Rajesh	05/17/2023 / Rajesh	E3515

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	23E0962014	12/13/2023	06/13/2023 / Rajesh	06/07/2023 / Rajesh	E3518

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	23E0962014	12/26/2023	06/27/2023 / Rajesh	06/26/2023 / Rajesh	E3532

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	23F1262016	01/22/2024	07/22/2023 / Rajesh	07/12/2023 / Rajesh	E3548

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110400-05-01 / TRPH Standard (C8-C40), 500 mg/L, 1 ml	472647	07/27/2023	01/27/2023 / yogesh	02/10/2022 / Yogesh	P11476

**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110400-05-01 / TRPH Standard (C8-C40), 500 mg/L, 1 ml	472647	01/06/2024	07/06/2023 / yogesh	02/10/2022 / Yogesh	P11477

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	12/08/2023	06/08/2023 / Abdul	03/14/2022 / yogesh	P11576

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	12/08/2023	06/08/2023 / Abdul	03/14/2022 / yogesh	P11577

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0184585	12/19/2023	06/19/2023 / yogesh	06/17/2022 / Yogesh	P11855

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0184585	12/19/2023	06/19/2023 / yogesh	06/17/2022 / Yogesh	P11856

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0184585	01/06/2024	07/06/2023 / yogesh	06/17/2022 / Yogesh	P11857



**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0184585	01/06/2024	07/06/2023 / yogesh	06/17/2022 / Yogesh	P11858

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	12/08/2023	06/08/2023 / Abdul	07/25/2022 / Yogesh	P11968

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	12/08/2023	06/08/2023 / Abdul	07/25/2022 / Yogesh	P11969

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	091120	01/06/2024	07/06/2023 / yogesh	07/25/2022 / Yogesh	P11971



## CERTIFIED WEIGHT REPORT

Part Number: **72072**  
Lot Number: **091120**  
Description: **n-Tetracosane-d50**

Solvent(s):  
Methylene chloride Lot# 104929

		091120
Formulated By:	Benson Chan	DATE
		091120
Reviewed By:	Pedro L. Rentas	DATE

Expiration Date: 091130  
Recommended Storage: Ambient (20 °C)  
Nominal Concentration (µg/mL): 1000  
NIST Test ID#: 23060




5E-05 Balance Uncertainty

0.058 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 200.0



Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
											CAS#	OSHA PEL (TWA)	LD50
1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20481	1000.5	4.1	16416-32-3	N/A	N/A

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

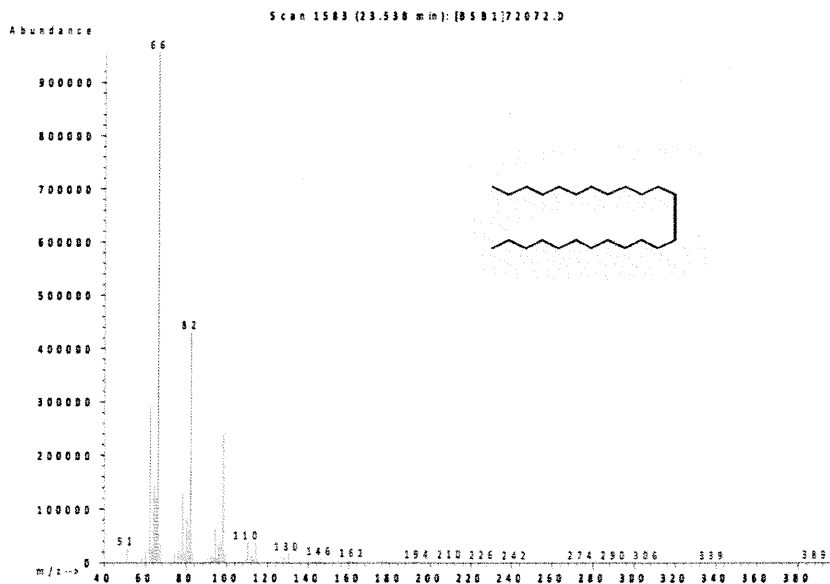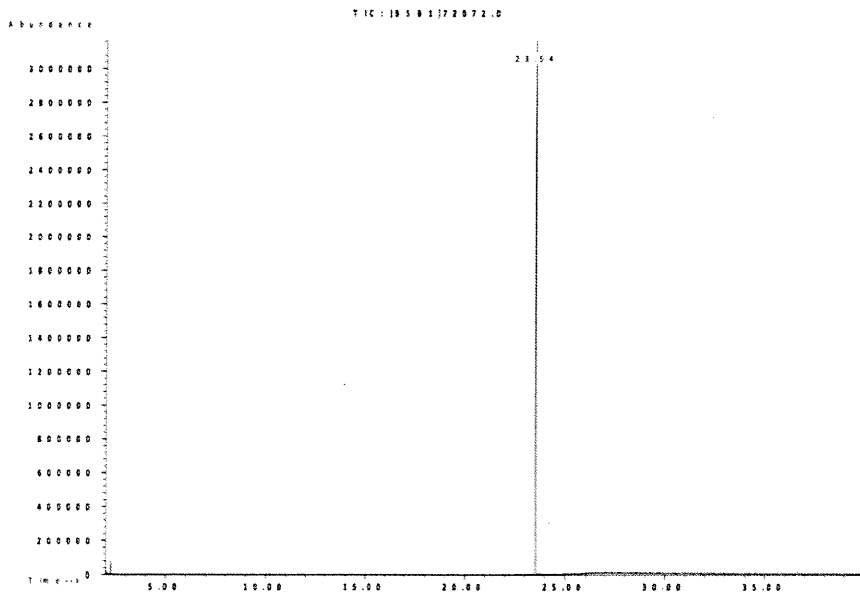

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

P11568  
↓  
P11577  
Y.P  
02/14/22

**Run 75, "P72072 L091120 (1000µg/mL in MeCl2)"**

Run Length: 35.00 min, 20999 points at 10 points/second.  
Created: Thu, Sep 17, 2020 at 9:46:03 AM.  
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".  
Analyzed using Method "GC4-M1".

**Comments**

GC4-M1 Analysis by Candice Warren


Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness

Flow rates: Total Flow = 300 mL/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,  
Air (detector) = 360 mL

Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.

Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDaq Channel 1.

Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

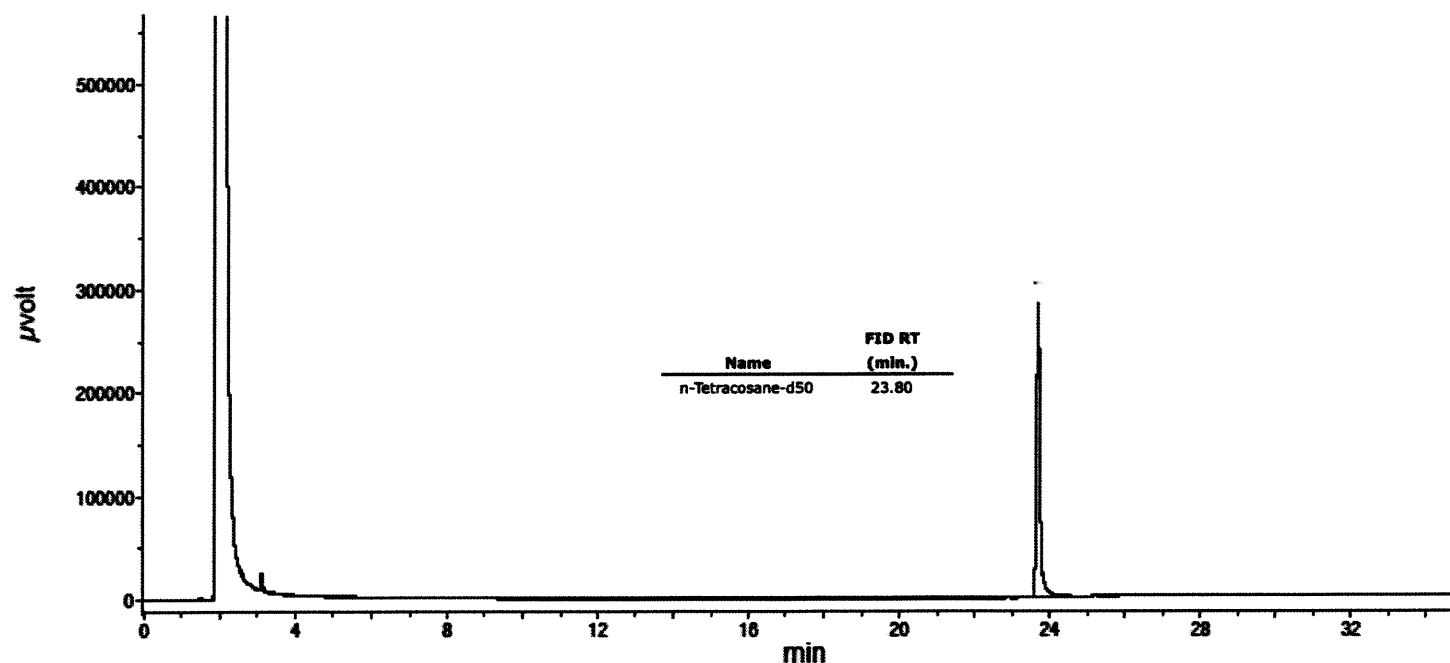

## Safety Data Sheet (SDS)

GHS/OSHA Compliant

## Section I Product and Company Identification

## IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHYLENE CHLORIDE

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rosotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 May 1, 2019

## Section II - Hazards Identification

## GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H302	Harmful if swallowed.	H315,H320	Causes skin and eye irritation.
H351	Suspected of causing cancer.	H335	May cause respiratory irritation.
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: WARNING

## Section III - Composition

Components:	CAS#:	OSHA PEL (TWA)	LD50 orl-rat	% (optional)
Dichloromethane	75-09-2	50 ppm	> 2,000 mg/kg	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.  
INTENDED USE: REFERENCE MATERIAL

## Section IV. FIRST AID MEASURES

General advice Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.

If inhaled If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.

In case of skin contact Wash with soap and water. Consult a physician.

In case of eye contact Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.

If swallowed Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

## Section V. FIREFIGHTING MEASURES

Suitable extinguishing media Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.

Protective equipment for fire Wear self contained breathing apparatus for fire fighting if necessary.

## Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.

Environmental precautions Prevent further leakage or spillage if safe to do so. Do not let product enter drains.

Clean up Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

## Section VII. HANDLING AND STORAGE

Precautions for safe handling Avoid contact with skin and eyes. Avoid inhalation of vapour or mist.

Storage Conditions Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge. Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

## Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methylene chloride 75-09-2 TWA 50 ppm

Potential for skin absorption, ingestion and inhalation.

Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection. Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

## Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS

Boiling Point	40°C	Specific Gravity (H2O = 1)	1.325
---------------	------	----------------------------	-------

Vapor Pressure (mm Hg)	353	Melting Point	-97°C
Vapor Density (AIR = 1)	2.93	Evaporation rate (Butyl Acetate = 1)	0.71
Solubility in Water	Slightly soluble		

Appearance and Odor CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
Possibility of hazardous reactions No data available  
Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
Materials to avoid Alkali metals, Aluminum, Oxidizing agents, Bases, Amines, Magnesium, Acids, Vinyl compounds  
Hazardous decomposition products - No data available

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - Rat - > 2,000 mg/kg  
LC50 Inhalation - Rat - 52,000 mg/m<sup>3</sup>  
LD50 Dermal - Rat - > 2,000 mg/kg  
Toxic if absorbed through skin. Causes skin irritation.  
Eye damage/eye irritation  
Toxic if inhaled. Causes respiratory tract irritation.  
Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 1000 lbs.**

LC50 193.00 mg/l - 96 h  
EC50 1,682.00 mg/l - 48 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**



DOT (US) IATA  
UN number: 1593 Class: 6.1 Packing group: III UN number: 1593 Class: 6.1 Packing group: III  
Proper shipping name: Dichloromethane Proper shipping name: Dichloromethane  
Reportable Quantity (RQ): 1000 lbs

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by skin absorption, Irritant  
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.



## CERTIFIED WEIGHT REPORT

Part Number: **72072**  
 Lot Number: **091120**  
 Description: **n-Tetracosane-d50**

Solvent(s):  
 Methylene chloride Lot# 104929

		091120
Formulated By:	Benson Chan	DATE
		091120
Reviewed By:	Pedro L. Rentas	DATE

Expiration Date: 091130  
 Recommended Storage: Ambient (20 °C)  
 Nominal Concentration (µg/mL): 1000  
 NIST Test ID#: 23060



5E-05 Balance Uncertainty

0.058 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 200.0



Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
											CAS#	OSHA PEL (TWA)	LD50
1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20481	1000.5	4.1	16416-32-3	N/A	N/A

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

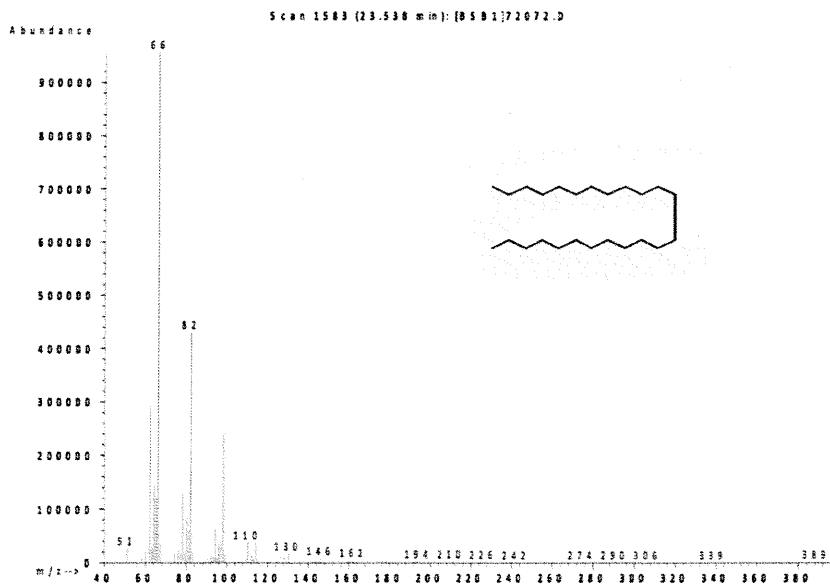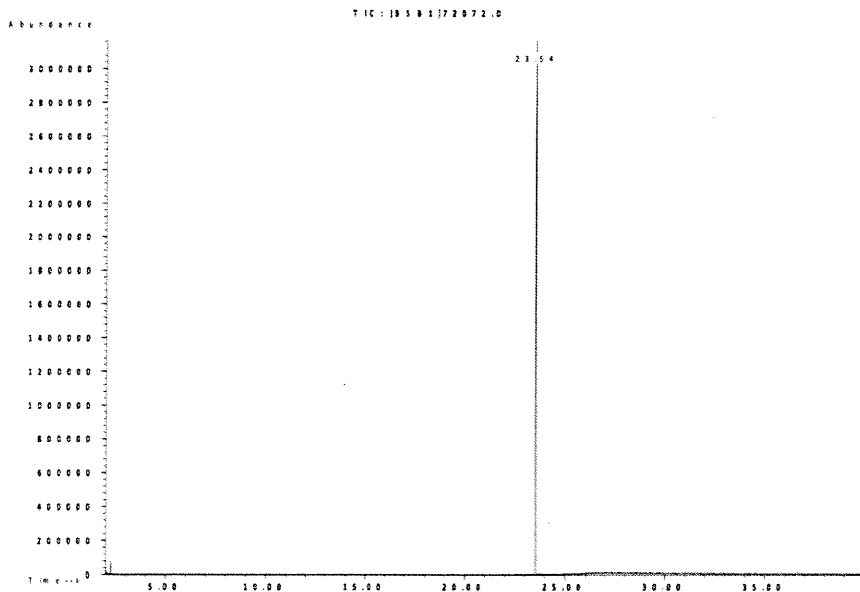

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

P11568  
 ↓  
 P11577  
 Y.P  
 02/14/22

**Run 75, "P72072 L091120 (1000µg/mL in MeCl2)"**

Run Length: 35.00 min, 20999 points at 10 points/second.  
Created: Thu, Sep 17, 2020 at 9:46:03 AM.  
Sampled: Sequence "091420-GC4M2", Method "GC4-M1".  
Analyzed using Method "GC4-M1".

**Comments**

GC4-M1 Analysis by Candice Warren


Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness

Flow rates: Total Flow = 300 mL/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,  
Air (detector) = 360 mL

Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.

Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDaq Channel 1.

Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

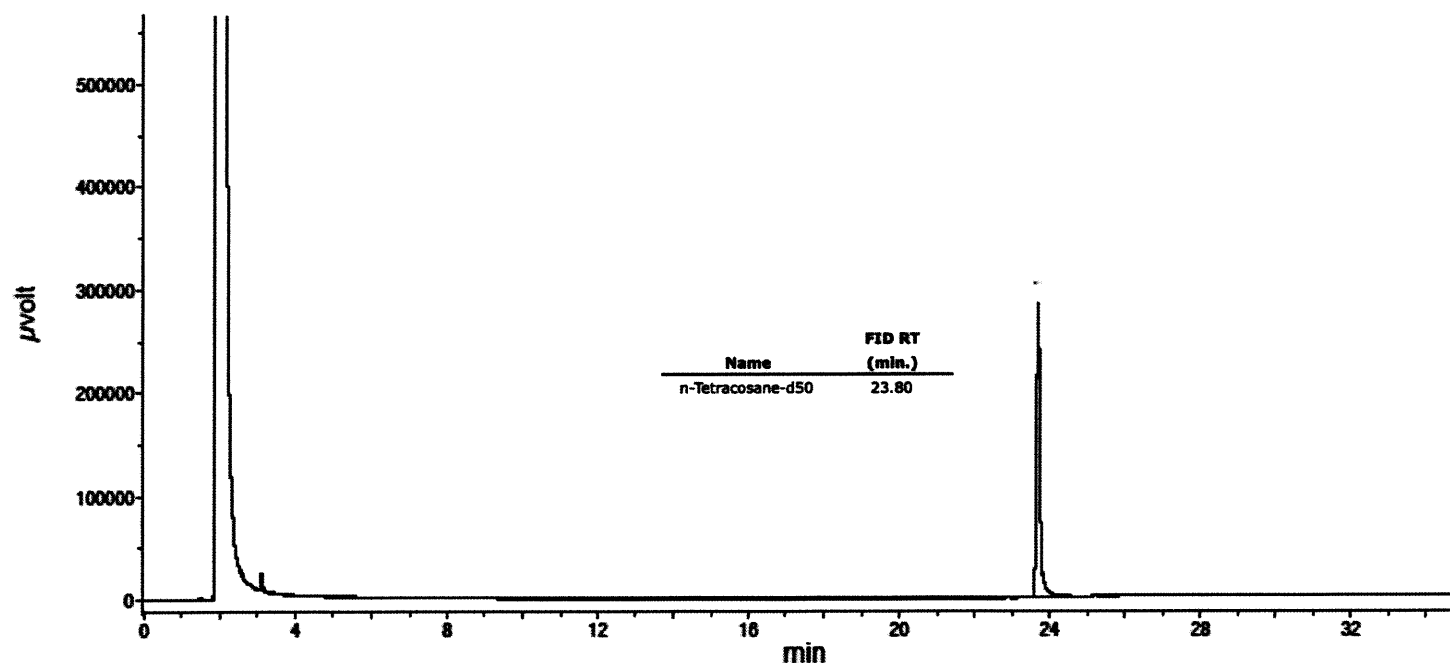

## Safety Data Sheet (SDS)

GHS/OSHA Compliant

## Section I Product and Company Identification

## IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHYLENE CHLORIDE

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rosotto Dr. Hamden CT, 06514	Emergency Telephone International	1-352-323-3500
		Date Prepared/Revised	May 1, 2019

## Section II - Hazards Identification

## GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H302	Harmful if swallowed.	H315,H320	Causes skin and eye irritation.
H351	Suspected of causing cancer.	H335	May cause respiratory irritation.
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: WARNING

## Section III - Composition

Components:	CAS#:	OSHA PEL (TWA)	LD50 orl-rat	% (optional)
Dichloromethane	75-09-2	50 ppm	> 2,000 mg/kg	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.  
INTENDED USE: REFERENCE MATERIAL

## Section IV. FIRST AID MEASURES

**General advice** Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.

**If inhaled** If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.

**In case of skin contact** Wash with soap and water. Consult a physician.

**In case of eye contact** Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.

**If swallowed** Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

## Section V. FIREFIGHTING MEASURES

**Suitable extinguishing media** Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.

**Protective equipment for fire** Wear self contained breathing apparatus for fire fighting if necessary.

## Section VI. ACCIDENTAL RELEASE MEASURES

**Personal precautions** Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.

**Environmental precautions** Prevent further leakage or spillage if safe to do so. Do not let product enter drains.

**Clean up** Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

## Section VII. HANDLING AND STORAGE

**Precautions for safe handling** Avoid contact with skin and eyes. Avoid inhalation of vapour or mist.

**Storage Conditions** Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge. Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

## Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methylene chloride 75-09-2 TWA 50 ppm

Potential for skin absorption, ingestion and inhalation.

Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection. Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

## Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS

Boiling Point	40°C	Specific Gravity (H2O = 1)	1.325
---------------	------	----------------------------	-------

**Absolute Standards Inc.**PO Box 5585  
Hamden, CT 06518-0585Phone: 203-281-2917  
FAX: 203-281-2922

Vapor Pressure (mm Hg)	353	Melting Point	-97°C
Vapor Density (AIR = 1)	2.93	Evaporation rate (Butyl Acetate = 1)	0.71
Solubility in Water	Slightly soluble		

Appearance and Odor CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.

**Section X. STABILITY AND REACTIVITY**

Chemical stability Stable under recommended storage conditions.  
Possibility of hazardous reactions No data available  
Conditions to avoid Heat, flames, sparks, extreme temperature and sunlight.  
Materials to avoid Alkali metals, Aluminum, Oxidizing agents, Bases, Amines, Magnesium, Acids, Vinyl compounds  
Hazardous decomposition products - No data available

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - Rat - > 2,000 mg/kg  
LC50 Inhalation - Rat - 52,000 mg/m<sup>3</sup>  
LD50 Dermal - Rat - > 2,000 mg/kg  
Toxic if absorbed through skin. Causes skin irritation.  
Eye damage/eye irritation  
Toxic if inhaled. Causes respiratory tract irritation.  
Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 1000 lbs.**

LC50 193.00 mg/l - 96 h  
EC50 1,682.00 mg/l - 48 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**


DOT (US) IATA  
UN number: 1593 Class: 6.1 Packing group: III UN number: 1593 Class: 6.1 Packing group: III  
Proper shipping name: Dichloromethane Proper shipping name: Dichloromethane  
Reportable Quantity (RQ): 1000 lbs

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by skin absorption, Irritant  
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.

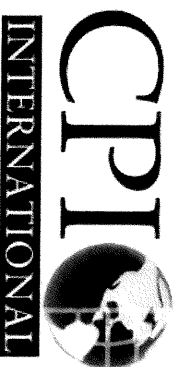

5580 Skylane Blvd  
Santa Rosa, CA 95403  
(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0 Page 1 of 1

Catalog No.: Lot No.: Storage:

Z-110400 472647  $\leq -10^{\circ}\text{C}$   
-05-01

Solvent:

Hexane

Exp. Date:

11/18/2023

Description:

TRPH Standard (C8-C40), 500 mg/L, 10 x 1 ml

-10PAK	Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
decane (C10)		124-18-5	99.5	415.7.1P	500.2 $\pm$ 2.29
docosane (C22)		629-97-0	99	420.1.1P	502.4 $\pm$ 5.5
dodecane (C12)		112-40-3	99.2	416.7.1P	500.7 $\pm$ 2.29
dotriacontane (C32)		544-85-4	98	425.29.2P	499.8 $\pm$ 5.47
eicosane (C20)		112-95-8	98.9	419.29.1P	505.1 $\pm$ 2.31
hexacosane (C26)		630-01-3	99.3	422.7.2P	500 $\pm$ 2.29
hexatriacontane (C36)		630-06-8	98	427.29.1P	500.3 $\pm$ 5.48
n-hexadecane (C16)		544-76-3	99.45	368.271.1P	499.6 $\pm$ 2.23
octacosane (C28)		630-02-4	98.7	423.400.1P	498.3 $\pm$ 5.45
n-octadecane (C18)		593-45-3	99.5	418.29.1P	501.9 $\pm$ 2.24
octane (C8)		111-65-9	99.5	385.9.1P	499.8 $\pm$ 2.23
octatriacontane (C38)		7194-85-6	99	428.7.1P	499.8 $\pm$ 2.29
tetracontane (C40)		4181-95-7	100	429.7.1P	504.1 $\pm$ 5.52
n-tetradecane (C14)		629-59-4	99	417.29.4P	500.4 $\pm$ 5.48
tetratriacontane (C34)		14167-59-0	98.1	426.7.2P	499.6 $\pm$ 2.28
triacontane (C30)		638-68-6	99.5	424.7.1.1P	499.9 $\pm$ 2.29
tetracosane (C24)		646-31-1	99	421.1.1P	500.1 $\pm$ 5.47

P11469  
J  
P11488  
Y.P.  
02/12/22

Let the standard warm to room temperature and sonicate before opening.

\*Not a certified value

Certified By: \_\_\_\_\_

Jarrett Howard  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.





5580 Skyline Blvd  
Santa Rosa, CA 95403  
(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Rev 0

Page 1 of 1

Catalog No.: Lot No.: Storage:

Z-110400 472647  $\leq -10^{\circ}\text{C}$   
-05-01

Solvent:

Hexane

Exp. Date:

11/18/2023

Description:

TRPH Standard (C8-C40), 500 mg/L, 10 x 1 ml

-10PAK	Compound	CAS No.	Purity (%)	Compound Lot No.	Concentration, mg/L
decane (C10)		124-18-5	99.5	415.7.1P	500.2 $\pm$ 2.29
docosane (C22)		629-97-0	99	420.1.1P	502.4 $\pm$ 5.5
dodecane (C12)		112-40-3	99.2	416.7.1P	500.7 $\pm$ 2.29
dotriacontane (C32)		544-85-4	98	425.29.2P	499.8 $\pm$ 5.47
eicosane (C20)		112-95-8	98.9	419.29.1P	505.1 $\pm$ 2.31
hexacosane (C26)		630-01-3	99.3	422.7.2P	500 $\pm$ 2.29
hexatriacontane (C36)		630-06-8	98	427.29.1P	500.3 $\pm$ 5.48
n-hexadecane (C16)		544-76-3	99.45	368.271.1P	499.6 $\pm$ 2.23
octacosane (C28)		630-02-4	98.7	423.400.1P	498.3 $\pm$ 5.45
n-octadecane (C18)		593-45-3	99.5	418.29.1P	501.9 $\pm$ 2.24
octane (C8)		111-65-9	99.5	385.9.1P	499.8 $\pm$ 2.23
octatriacontane (C38)		7194-85-6	99	428.7.1P	499.8 $\pm$ 2.29
tetracontane (C40)		4181-95-7	100	429.7.1P	504.1 $\pm$ 5.52
n-tetradecane (C14)		629-59-4	99	417.29.4P	500.4 $\pm$ 5.48
tetratriacontane (C34)		14167-59-0	98.1	426.7.2P	499.6 $\pm$ 2.28
triacontane (C30)		638-68-6	99.5	424.7.1.1P	499.9 $\pm$ 2.29
tetracosane (C24)		646-31-1	99	421.1.1P	500.1 $\pm$ 5.47

P11469  
J  
P11488  
Y.P.  
02/12/22

Let the standard warm to room temperature and sonicate before opening.

\*Not a certified value

Certified By: \_\_\_\_\_

Jarrett Howard  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.






**PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.**



MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MÉXICO  
CP 64070  
TEL +52 81 13 52 57 57  
www.pqm.com.mx

# CERTIFICATE OF ANALYSIS

**PRODUCT :** SODIUM SULFATE CRYSTALS ANHYDROUS  
**QUALITY :** ACS (CODE RMB3375) **FORMULA :** Na<sub>2</sub>SO<sub>4</sub>  
**SPECIFICATION NUMBER :** 6399 **RELEASE DATE:** OCT/28/2021  
**LOT NUMBER :** 139404

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na <sub>2</sub> SO <sub>4</sub> )	Min. 99.0%	99.8 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.0
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO <sub>4</sub> )	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.002 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.2 %
Retained on US Standard No. 60 sieve	Min. 94%	97.6 %
Through US Standard No. 60 sieve	Max. 5%	2.1 %
Through US Standard No. 100 sieve	Max. 10%	0.2 %
COMMENTS		
 QC: PhC Irma Belmares		

If you need further details, please call our factory or contact our local distributor.

E 3412

Recd. by RP on 10/13/22

RE-02-01, Ed. 3

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 23C1362018  
Manufactured Date: 2023-01-26  
Expiration Date: 2024-04-26  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	5
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.9 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

E3515

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 23E0962014  
Manufactured Date: 2023-04-24  
Expiration Date: 2024-07-23  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	6
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	< 0.1 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

E3518

Ken Koehnlein  
Sr. Manager, Quality Assurance

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 23E0962014  
Manufactured Date: 2023-04-24  
Expiration Date: 2024-07-23  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	6
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	< 0.1 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

E 3532

Ken Koehnlein  
Sr. Manager, Quality Assurance

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 23F1262016  
Manufactured Date: 2023-05-17  
Expiration Date: 2024-08-15  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	4
Assay (CH <sub>2</sub> Cl <sub>2</sub> ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0$ ppm	< 1.0 ppm
Titration Acid ( $\mu$ eq/g)	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10$ ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC  
Manufacturer source batch: MG23E17953

E 3548

Ken Koehnlein  
Sr. Manager, Quality Assurance

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31266 Lot No.: A0184585

Description : Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL Pkg Amt: > 1 mL

Expiration Date : May 31, 2029 Storage: 25°C nominal

Handling: Sonicate prior to use. Ship: Ambient

P11852  
↓  
y.p  
06/17  
P1866

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.I.; K=2)
1	n-Octane (C8) CAS # 111-65-9 Purity 99%	500.3 µg/mL (Lot SHBN3807)	+/- 2.9718 µg/mL Gravimetric +/- 12.4305 µg/mL Unstressed +/- 14.9001 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99%	501.7 µg/mL (Lot SHBN8619)	+/- 2.9797 µg/mL Gravimetric +/- 12.4637 µg/mL Unstressed +/- 14.9398 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 Purity 99%	504.7 µg/mL (Lot SHBN7174)	+/- 2.9976 µg/mL Gravimetric +/- 12.5382 µg/mL Unstressed +/- 15.0291 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 Purity 99%	503.7 µg/mL (Lot STBJ3715)	+/- 2.9916 µg/mL Gravimetric +/- 12.5133 µg/mL Unstressed +/- 14.9993 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 Purity 98%	502.7 µg/mL (Lot SHBM4146)	+/- 2.9861 µg/mL Gravimetric +/- 12.4903 µg/mL Unstressed +/- 14.9717 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 Purity 98%	502.7 µg/mL (Lot UESNG)	+/- 2.9861 µg/mL Gravimetric +/- 12.4903 µg/mL Unstressed +/- 14.9717 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 Purity 97%	500.5 µg/mL (Lot MKCN8767)	+/- 2.9729 µg/mL Gravimetric +/- 12.4352 µg/mL Unstressed +/- 14.9056 µg/mL Stressed

8	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	501.3 µg/mL	+/- 2.9778 +/- 12.4554 +/- 14.9298	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	502.3 µg/mL	+/- 2.9837 +/- 12.4802 +/- 14.9596	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	501.0 µg/mL	+/- 2.9758 +/- 12.4471 +/- 14.9199	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	502.3 µg/mL	+/- 2.9837 +/- 12.4802 +/- 14.9596	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) CAS # 638-68-6 Purity 98%	(Lot MKCJ4572)	500.8 µg/mL	+/- 2.9745 +/- 12.4416 +/- 14.9134	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	501.0 µg/mL	+/- 2.9758 +/- 12.4471 +/- 14.9199	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetatriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	503.0 µg/mL	+/- 2.9877 +/- 12.4968 +/- 14.9795	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot U25B014)	503.0 µg/mL	+/- 2.9877 +/- 12.4968 +/- 14.9795	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 97%	(Lot 0000127235)	501.5 µg/mL	+/- 2.9787 +/- 12.4593 +/- 14.9345	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) CAS # 4181-95-7 Purity 98%	(Lot PADGI)	504.7 µg/mL	+/- 2.9978 +/- 12.5390 +/- 15.0301	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
<b>Solvent:</b> Hexane						
CAS # 110-54-3						
Purity 99%						

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**


330°C

**Det. Type:**

FID

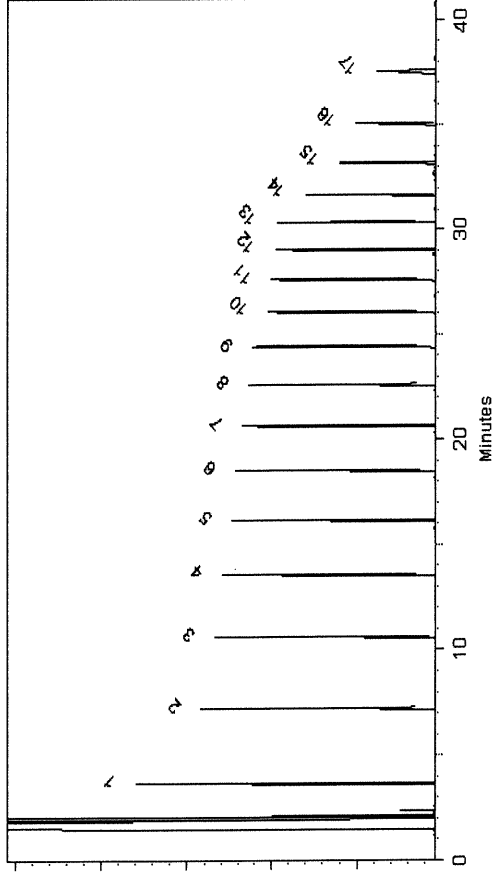

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Lane Kibe - Mix Technician

Date Mixed: 27-Apr-2022 Balance: 1128360905

  
Pong Yuen Lu - QC Analyst

Date Passed: 29-Apr-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31266 Lot No.: A0184585

Description : Florida TRPH Standard

Container Size : 2 mL Pkg Amt: > 1 mL

Expiration Date : May 31, 2029 Storage: 25°C nominal

Handling: Sonicate prior to use. Ship: Ambient

P11852  
↓  
y.p  
06/17  
P1866

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.I.; K=2)
1	n-Octane (C8) CAS # 111-65-9 Purity 99%	500.3 µg/mL (Lot SHBN3807)	+/- 2.9718 µg/mL Gravimetric +/- 12.4305 µg/mL Unstressed +/- 14.9001 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99%	501.7 µg/mL (Lot SHBN8619)	+/- 2.9797 µg/mL Gravimetric +/- 12.4637 µg/mL Unstressed +/- 14.9398 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 Purity 99%	504.7 µg/mL (Lot SHBN7174)	+/- 2.9976 µg/mL Gravimetric +/- 12.5382 µg/mL Unstressed +/- 15.0291 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 Purity 99%	503.7 µg/mL (Lot STBJ3715)	+/- 2.9916 µg/mL Gravimetric +/- 12.5133 µg/mL Unstressed +/- 14.9993 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 Purity 98%	502.7 µg/mL (Lot SHBM4146)	+/- 2.9861 µg/mL Gravimetric +/- 12.4903 µg/mL Unstressed +/- 14.9717 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 Purity 98%	502.7 µg/mL (Lot UESNG)	+/- 2.9861 µg/mL Gravimetric +/- 12.4903 µg/mL Unstressed +/- 14.9717 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 Purity 97%	500.5 µg/mL (Lot MKCN8767)	+/- 2.9729 µg/mL Gravimetric +/- 12.4352 µg/mL Unstressed +/- 14.9056 µg/mL Stressed

8	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	501.3 µg/mL	+/- 2.9778 +/- 12.4554 +/- 14.9298	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	502.3 µg/mL	+/- 2.9837 +/- 12.4802 +/- 14.9596	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	501.0 µg/mL	+/- 2.9758 +/- 12.4471 +/- 14.9199	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	502.3 µg/mL	+/- 2.9837 +/- 12.4802 +/- 14.9596	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) CAS # 638-68-6 Purity 98%	(Lot MKCJ4572)	500.8 µg/mL	+/- 2.9745 +/- 12.4416 +/- 14.9134	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	501.0 µg/mL	+/- 2.9758 +/- 12.4471 +/- 14.9199	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	503.0 µg/mL	+/- 2.9877 +/- 12.4968 +/- 14.9795	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot U25B014)	503.0 µg/mL	+/- 2.9877 +/- 12.4968 +/- 14.9795	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 97%	(Lot 0000127235)	501.5 µg/mL	+/- 2.9787 +/- 12.4593 +/- 14.9345	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) CAS # 4181-95-7 Purity 98%	(Lot PADGI)	504.7 µg/mL	+/- 2.9978 +/- 12.5390 +/- 15.0301	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
<b>Solvent:</b> Hexane						
CAS # 110-54-3						
Purity 99%						

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**


330°C

**Det. Type:**

FID

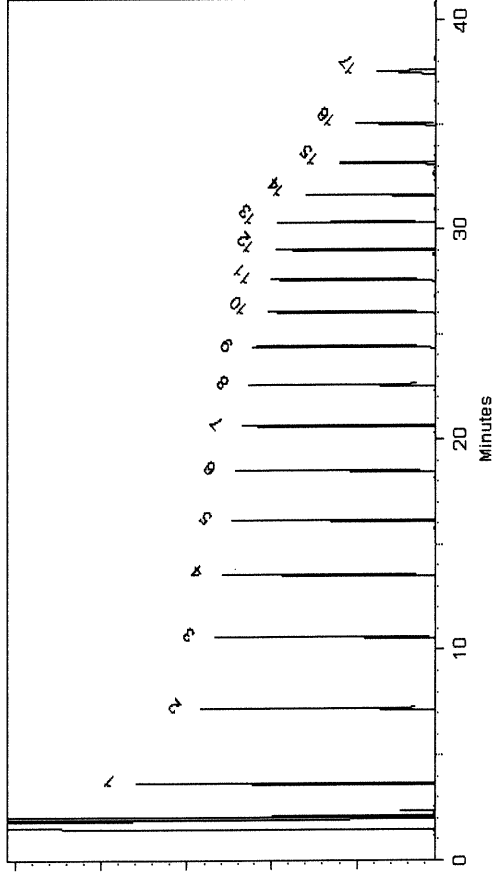

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Lane Kibe - Mix Technician

Date Mixed: 27-Apr-2022 Balance: 1128360905

  
Peng-Yuan Lu - QC Analyst

Date Passed: 29-Apr-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31266 Lot No.: A0184585

Description : Florida TRPH Standard

Container Size : 2 mL Pkg Amt: > 1 mL

Expiration Date : May 31, 2029 Storage: 25°C nominal

Handling: Sonicate prior to use. Ship: Ambient

P11852  
↓  
y.p  
06/17  
P1866

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.I.; K=2)
1	n-Octane (C8) CAS # 111-65-9 Purity 99%	500.3 µg/mL (Lot SHBN3807)	+/- 2.9718 µg/mL Gravimetric +/- 12.4305 µg/mL Unstressed +/- 14.9001 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99%	501.7 µg/mL (Lot SHBN8619)	+/- 2.9797 µg/mL Gravimetric +/- 12.4637 µg/mL Unstressed +/- 14.9398 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 Purity 99%	504.7 µg/mL (Lot SHBN7174)	+/- 2.9976 µg/mL Gravimetric +/- 12.5382 µg/mL Unstressed +/- 15.0291 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 Purity 99%	503.7 µg/mL (Lot STBJ3715)	+/- 2.9916 µg/mL Gravimetric +/- 12.5133 µg/mL Unstressed +/- 14.9993 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 Purity 98%	502.7 µg/mL (Lot SHBM4146)	+/- 2.9861 µg/mL Gravimetric +/- 12.4903 µg/mL Unstressed +/- 14.9717 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 Purity 98%	502.7 µg/mL (Lot UESNG)	+/- 2.9861 µg/mL Gravimetric +/- 12.4903 µg/mL Unstressed +/- 14.9717 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 Purity 97%	500.5 µg/mL (Lot MKCN8767)	+/- 2.9729 µg/mL Gravimetric +/- 12.4352 µg/mL Unstressed +/- 14.9056 µg/mL Stressed

8	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	501.3 µg/mL	+/- 2.9778 +/- 12.4554 +/- 14.9298	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	502.3 µg/mL	+/- 2.9837 +/- 12.4802 +/- 14.9596	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	501.0 µg/mL	+/- 2.9758 +/- 12.4471 +/- 14.9199	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	502.3 µg/mL	+/- 2.9837 +/- 12.4802 +/- 14.9596	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) CAS # 638-68-6 Purity 98%	(Lot MKCJ4572)	500.8 µg/mL	+/- 2.9745 +/- 12.4416 +/- 14.9134	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	501.0 µg/mL	+/- 2.9758 +/- 12.4471 +/- 14.9199	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	503.0 µg/mL	+/- 2.9877 +/- 12.4968 +/- 14.9795	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot U25B014)	503.0 µg/mL	+/- 2.9877 +/- 12.4968 +/- 14.9795	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 97%	(Lot 0000127235)	501.5 µg/mL	+/- 2.9787 +/- 12.4593 +/- 14.9345	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) CAS # 4181-95-7 Purity 98%	(Lot PADGI)	504.7 µg/mL	+/- 2.9978 +/- 12.5390 +/- 15.0301	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
<b>Solvent:</b> Hexane						
CAS # 110-54-3						
Purity 99%						

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**


330°C

**Det. Type:**

FID

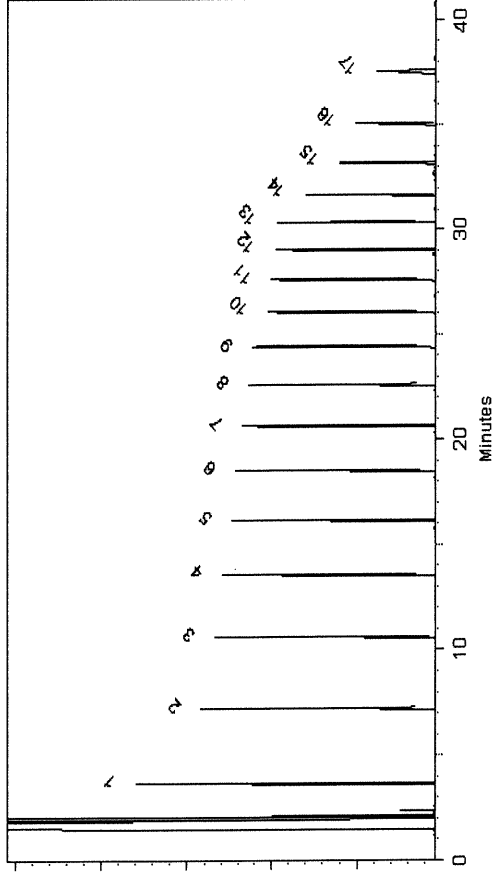

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Lane Kibe - Mix Technician

Date Mixed: 27-Apr-2022 Balance: 1128360905

  
Pong Yuen Lu - QC Analyst

Date Passed: 29-Apr-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.




110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31266 Lot No.: A0184585

Description : Florida TRPH Standard

Container Size : 2 mL Pkg Amt: > 1 mL

Expiration Date : May 31, 2029 Storage: 25°C nominal

Handling: Sonicate prior to use. Ship: Ambient

P11852  
↓  
y.p  
06/17  
P1866

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.I.; K=2)
1	n-Octane (C8) CAS # 111-65-9 Purity 99%	500.3 µg/mL (Lot SHBN3807)	+/- 2.9718 µg/mL Gravimetric +/- 12.4305 µg/mL Unstressed +/- 14.9001 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99%	501.7 µg/mL (Lot SHBN8619)	+/- 2.9797 µg/mL Gravimetric +/- 12.4637 µg/mL Unstressed +/- 14.9398 µg/mL Stressed
3	n-Dodecane (C12) CAS # 112-40-3 Purity 99%	504.7 µg/mL (Lot SHBN7174)	+/- 2.9976 µg/mL Gravimetric +/- 12.5382 µg/mL Unstressed +/- 15.0291 µg/mL Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 Purity 99%	503.7 µg/mL (Lot STBJ3715)	+/- 2.9916 µg/mL Gravimetric +/- 12.5133 µg/mL Unstressed +/- 14.9993 µg/mL Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 Purity 98%	502.7 µg/mL (Lot SHBM4146)	+/- 2.9861 µg/mL Gravimetric +/- 12.4903 µg/mL Unstressed +/- 14.9717 µg/mL Stressed
6	n-Octadecane (C18) CAS # 593-45-3 Purity 98%	502.7 µg/mL (Lot UESNG)	+/- 2.9861 µg/mL Gravimetric +/- 12.4903 µg/mL Unstressed +/- 14.9717 µg/mL Stressed
7	n-Eicosane (C20) CAS # 112-95-8 Purity 97%	500.5 µg/mL (Lot MKCN8767)	+/- 2.9729 µg/mL Gravimetric +/- 12.4352 µg/mL Unstressed +/- 14.9056 µg/mL Stressed

8	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	501.3 µg/mL	+/- 2.9778 +/- 12.4554 +/- 14.9298	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	502.3 µg/mL	+/- 2.9837 +/- 12.4802 +/- 14.9596	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	501.0 µg/mL	+/- 2.9758 +/- 12.4471 +/- 14.9199	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	502.3 µg/mL	+/- 2.9837 +/- 12.4802 +/- 14.9596	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) CAS # 638-68-6 Purity 98%	(Lot MKCJ4572)	500.8 µg/mL	+/- 2.9745 +/- 12.4416 +/- 14.9134	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	501.0 µg/mL	+/- 2.9758 +/- 12.4471 +/- 14.9199	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	503.0 µg/mL	+/- 2.9877 +/- 12.4968 +/- 14.9795	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot U25B014)	503.0 µg/mL	+/- 2.9877 +/- 12.4968 +/- 14.9795	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 97%	(Lot 0000127235)	501.5 µg/mL	+/- 2.9787 +/- 12.4593 +/- 14.9345	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) CAS # 4181-95-7 Purity 98%	(Lot PADGI)	504.7 µg/mL	+/- 2.9978 +/- 12.5390 +/- 15.0301	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
<b>Solvent:</b> Hexane						
CAS # 110-54-3						
Purity 99%						

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**


330°C

**Det. Type:**

FID

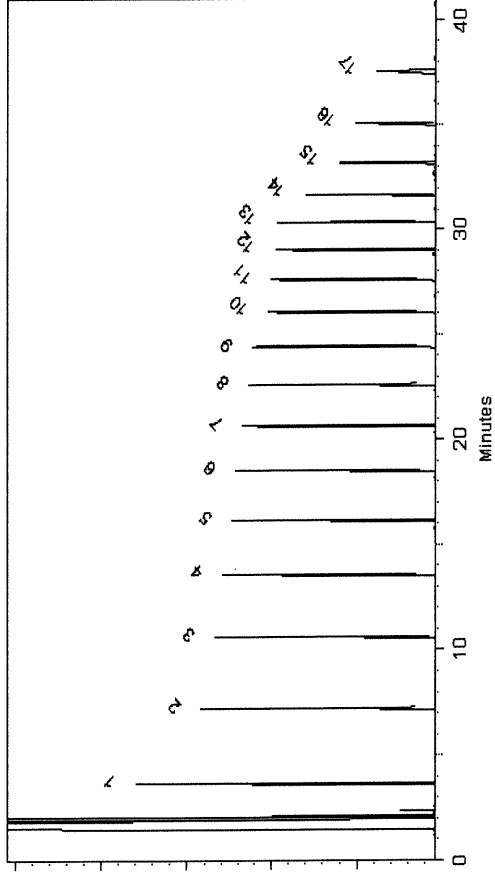

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Lane Kibe - Mix Technician

Date Mixed: 27-Apr-2022 Balance: 1128360905

  
Pong Yuen Lu - QC Analyst

Date Passed: 29-Apr-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



**CERTIFIED WEIGHT REPORT**

Part Number: **72072**  
Lot Number: **091120**  
Description: **n-Tetracosane-d50**

Solvent(s):  
Methylene chloride Lot# 104929

		091120
Formulated By:	Benson Chan	DATE
		091120
Reviewed By:	Pedro L. Rentas	DATE

P11968  
J  
P11977  
} 7.4  
0.718




Expiration Date: 091130  
Recommended Storage: Ambient (20 °C)  
Nominal Concentration (µg/mL): 1000  
NIST Test ID#: 23060

5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 200.0

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
											CAS#	OSHA PEL (TWA)	LD50
1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20481	1000.5	4.1	16416-32-3	N/A	N/A

**Method GC8MSD-3.M:** Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

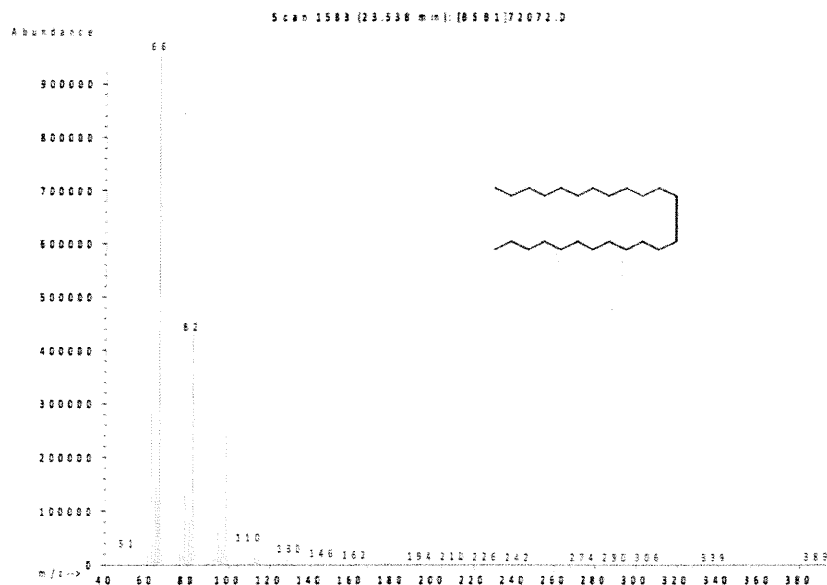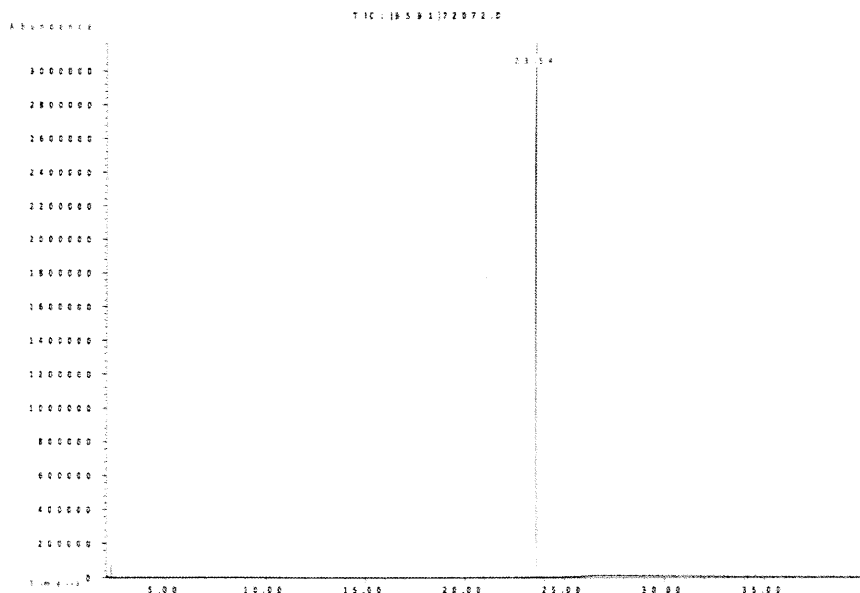

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

**Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"**

Run Length: 35.00 min, 20999 points at 10 points/second.

Created: Thu, Sep 17, 2020 at 9:46:03 AM.

Sampled: Sequence "091420-GC4M2", Method "GC4-M1".

Analyzed using Method "GC4-M1".

**Comments**

GC4-M1 Analysis by Candice Warren

Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness


Flow rates: Total Flow = 300 mL/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,

Air (detector) = 360 mL

Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.

Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDaq Channel 1.

Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

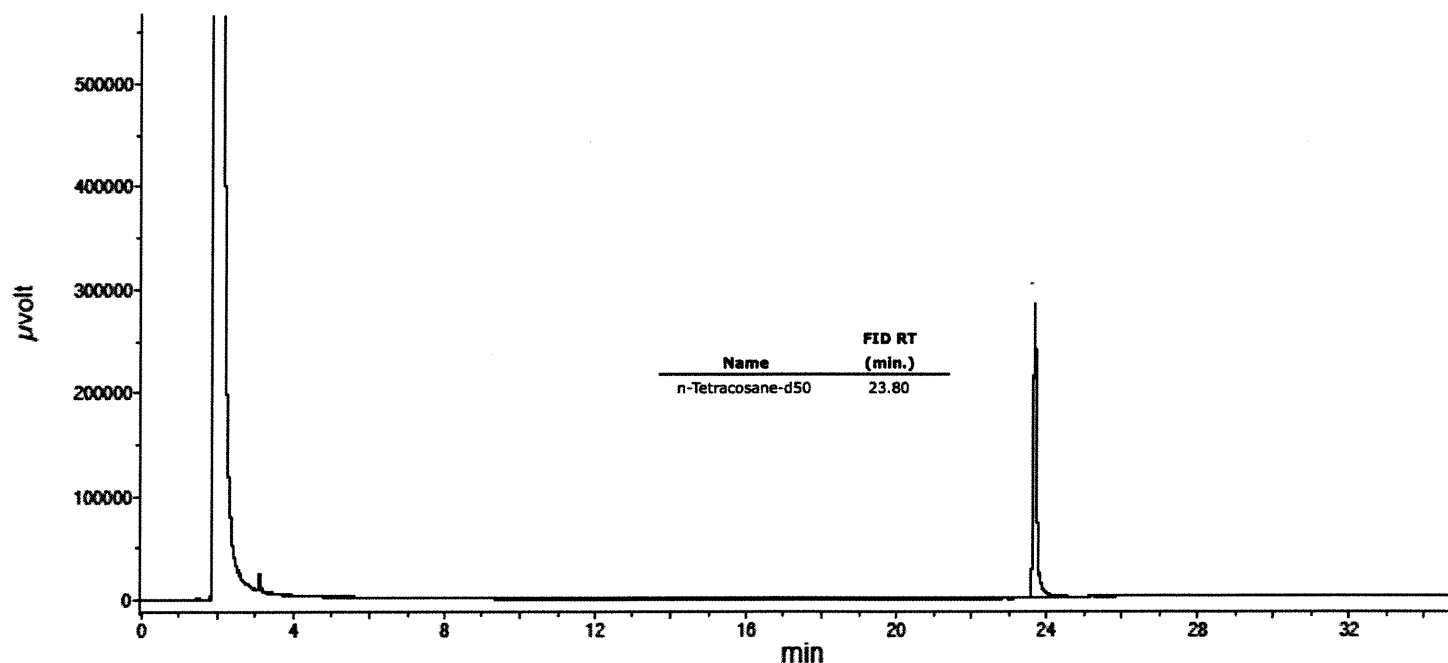



**CERTIFIED WEIGHT REPORT**

Part Number: **72072**  
Lot Number: **091120**  
Description: **n-Tetracosane-d50**

Solvent(s):  
Methylene chloride  
Lot#  
104929

		091120
Formulated By:	Benson Chan	DATE
		091120
Reviewed By:	Pedro L. Rentas	DATE




P11968  
J  
P11977  
} 7.4  
0.718

Expiration Date: 091130  
Recommended Storage: Ambient (20 °C)  
Nominal Concentration (µg/mL): 1000  
NIST Test ID#: 23060  
5E-05 Balance Uncertainty

Weight(s) shown below were combined and diluted to (mL): 200.0 0.058 Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
											CAS#	OSHA PEL (TWA)	LD50
1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20481	1000.5	4.1	16416-32-3	N/A	N/A

**Method GC8MSD-3.M:** Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

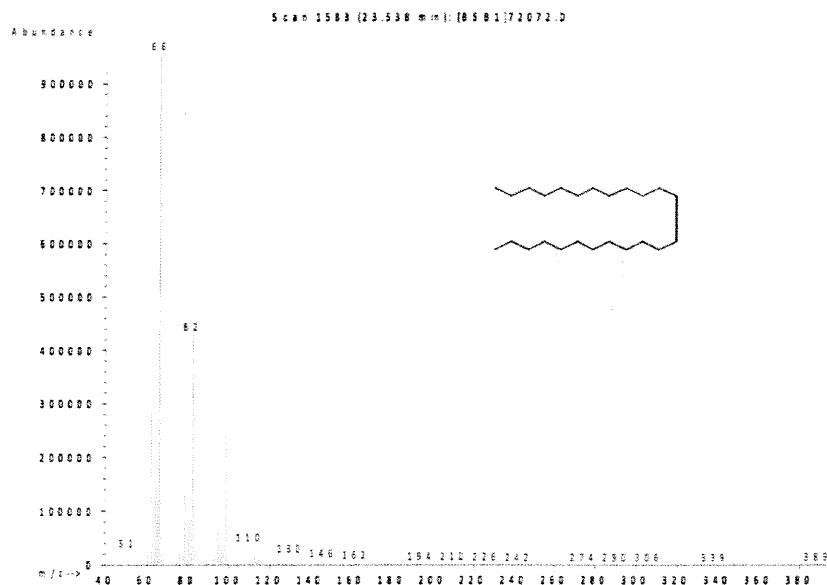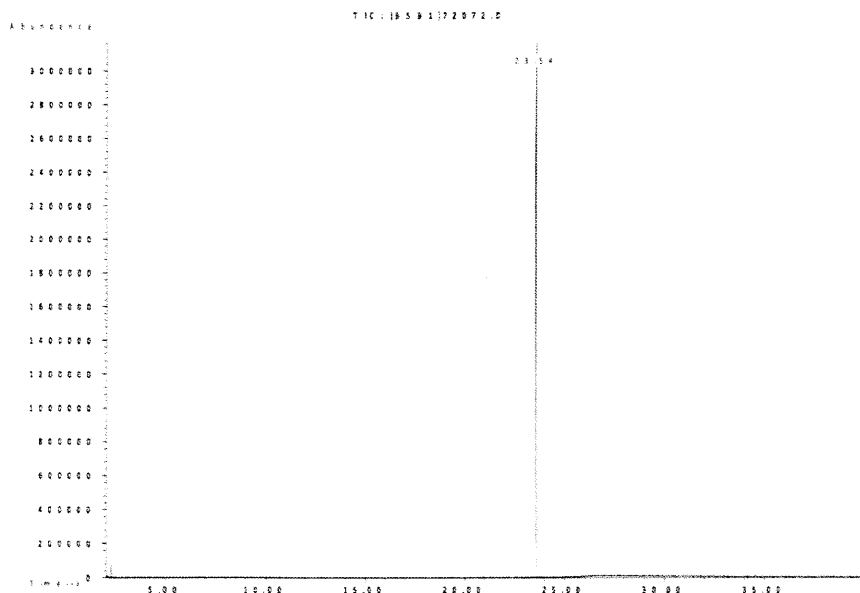

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

**Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"**

Run Length: 35.00 min, 20999 points at 10 points/second.

Created: Thu, Sep 17, 2020 at 9:46:03 AM.

Sampled: Sequence "091420-GC4M2", Method "GC4-M1".

Analyzed using Method "GC4-M1".

**Comments**

GC4-M1 Analysis by Candice Warren

Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness


Flow rates: Total Flow = 300 mL/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,

Air (detector) = 360 mL

Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.

Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDaq Channel 1.

Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

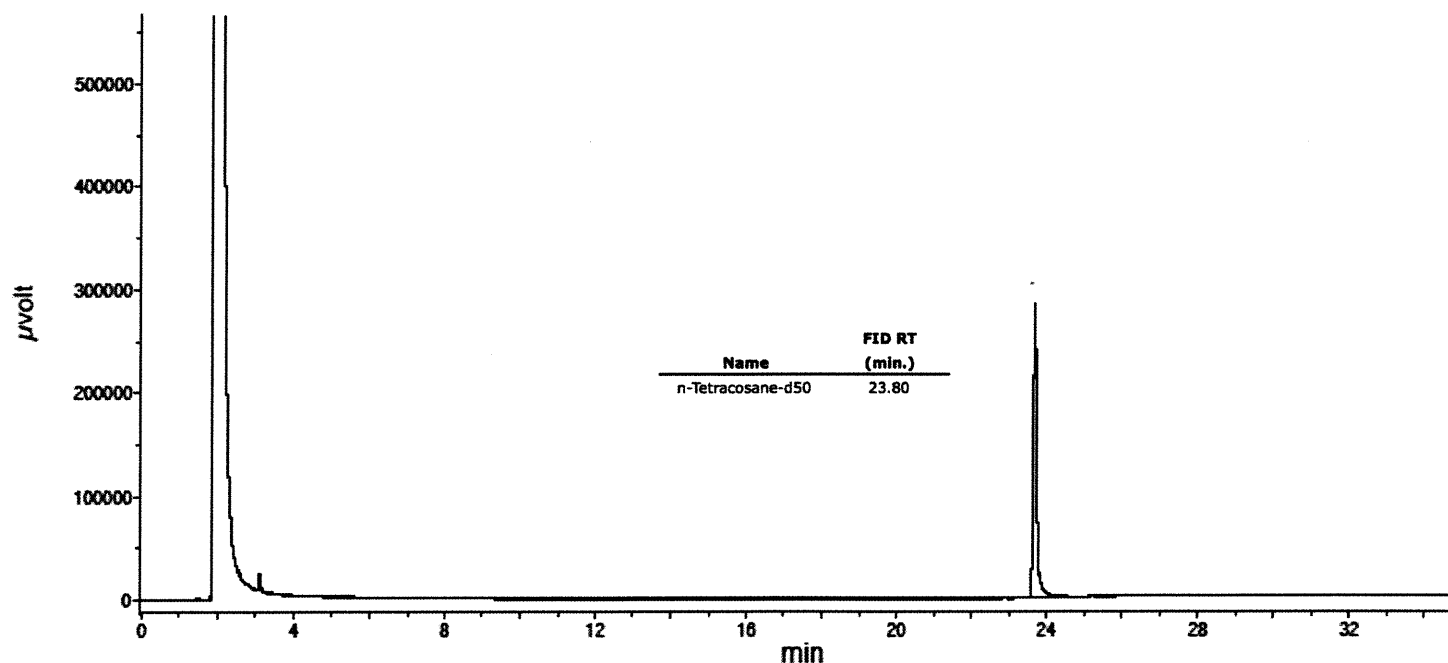



**CERTIFIED WEIGHT REPORT**

**Part Number:** 72072  
**Lot Number:** 091120  
**Description:** n-Tetracosane-d50

**Solvent(s):**  
Methylene chloride  
**Lot#**  
104929

		091120
<b>Formulated By:</b>	Benson Chan	<b>DATE</b>
		091120
<b>Reviewed By:</b>	Pedro L. Rentas	<b>DATE</b>




P11968  
J  
P11977  
} 7.4  
0.718

**Expiration Date:** 091130  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** 1000  
**NIST Test ID#:** 23060  
**5E-05 Balance Uncertainty**

**Weight(s) shown below were combined and diluted to (mL):** 200.0  
**0.058 Flask Uncertainty**

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
											CAS#	OSHA PEL (TWA)	LD50
1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20481	1000.5	4.1	16416-32-3	N/A	N/A

**Method GC8MSD-3.M:** Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

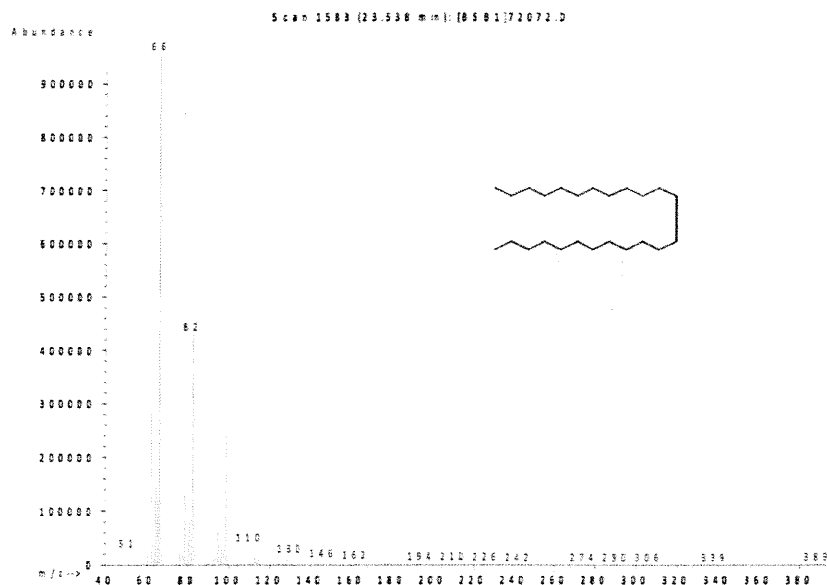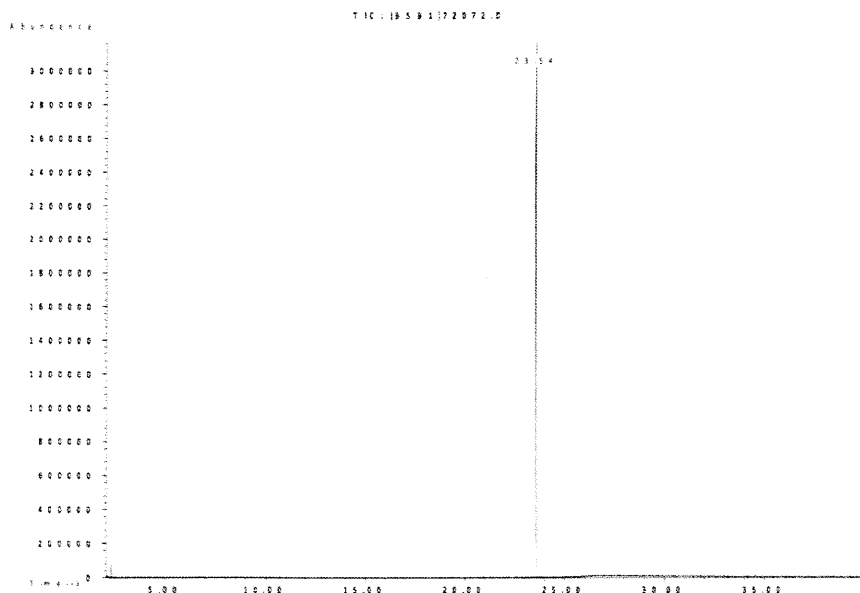

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

**Run 75, "P72072 L091120 [1000µg/mL in MeCl2]"**

Run Length: 35.00 min, 20999 points at 10 points/second.

Created: Thu, Sep 17, 2020 at 9:46:03 AM.

Sampled: Sequence "091420-GC4M2", Method "GC4-M1".

Analyzed using Method "GC4-M1".

**Comments**

GC4-M1 Analysis by Candice Warren

Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness

Flow rates: Total Flow = 300 mL/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL,

Air (detector) = 360 mL

Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.

Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDaq Channel 1.

Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

