
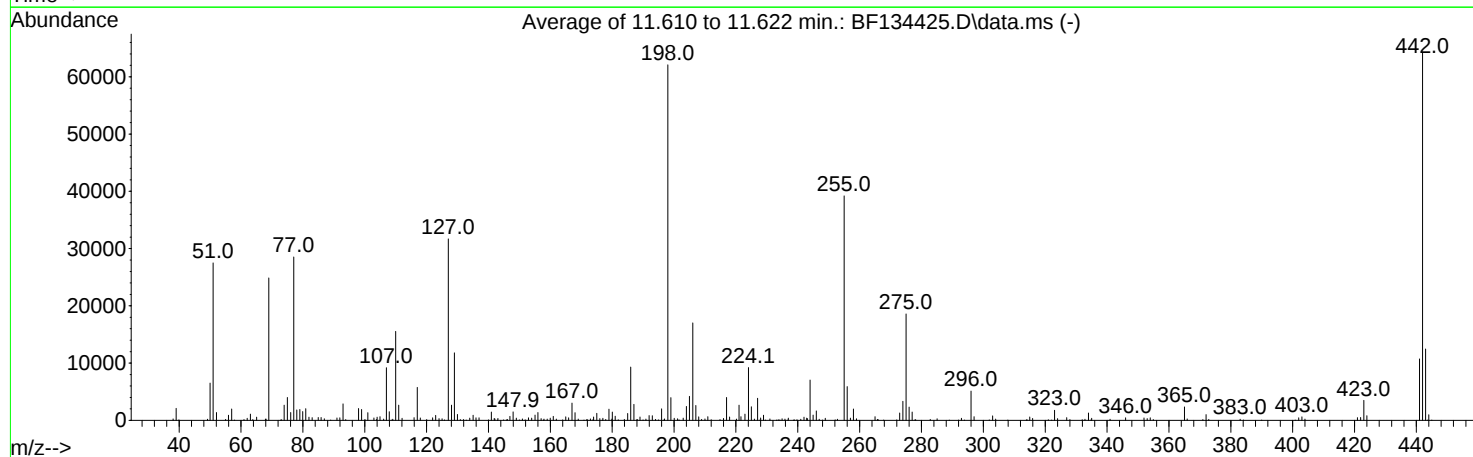


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072423\
Data File : BF134425.D
Acq On : 24 Jul 2023 12:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 25 01:46:04 2023

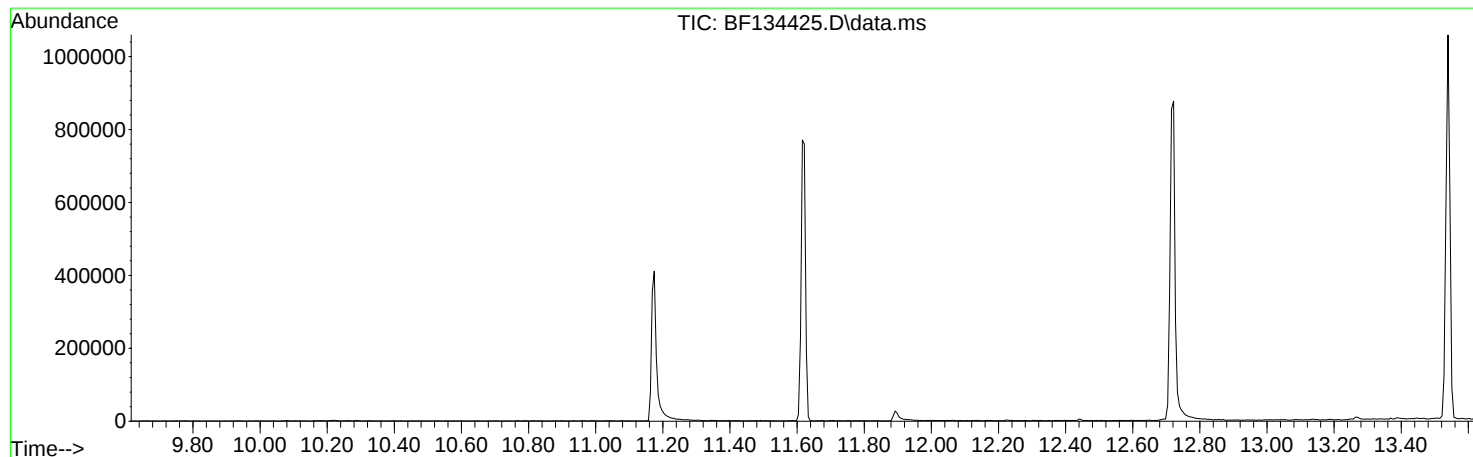

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	27503	PASS
68	69	0.00	2	0.9	228	PASS
69	198	0.00	100	40.1	24871	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.0	31683	PASS
197	198	0.00	2	0.4	245	PASS
198	198	100	100	100.0	62093	PASS
199	198	5	9	6.4	3981	PASS
275	198	10	60	29.9	18581	PASS
365	198	1	100	3.8	2356	PASS
441	198	0.01	100	17.3	10730	PASS
442	442	50	100	100.0	64243	PASS
443	442	15	24	19.4	12462	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/24/2023	BNA_F	<u>BF134425.D</u>
Compound Name	Response	Retention Time
DDT	169209	13.539
DDD	2179	13.269
DDE	0	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2179	171388	1.27

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072423\
Data File : BF134425.D
Acq On : 24 Jul 2023 12:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 25 04:25:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

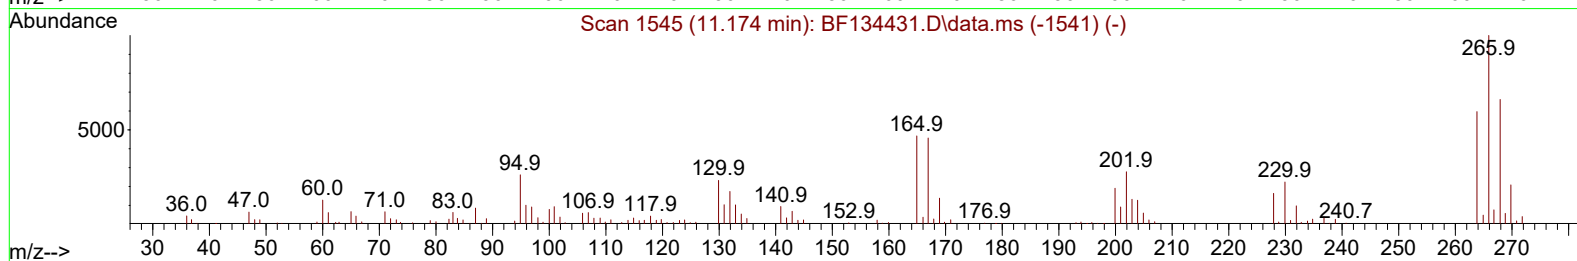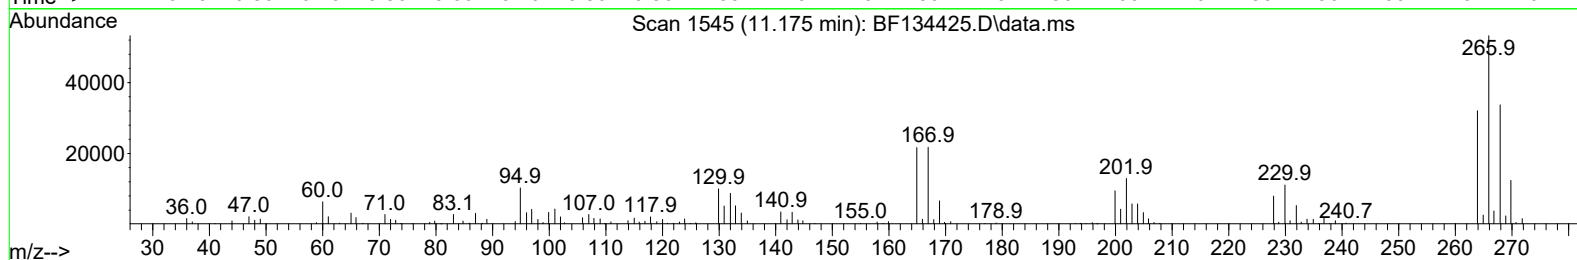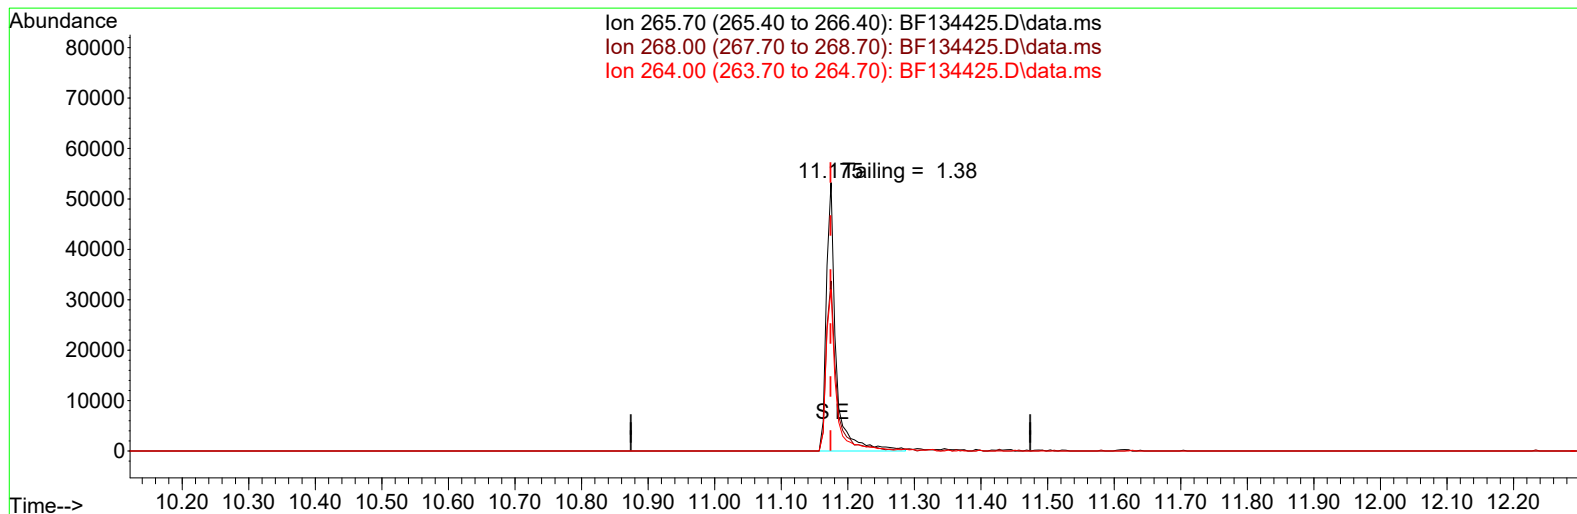

TIC: BF134425.D\data.ms

(70) Pentachlorophenol (C)

11.175min (+ 0.001) 37497.50 ng




response 54169

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	63.30
264.00	59.70	60.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072423\
Data File : BF134425.D
Acq On : 24 Jul 2023 12:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 25 04:25:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

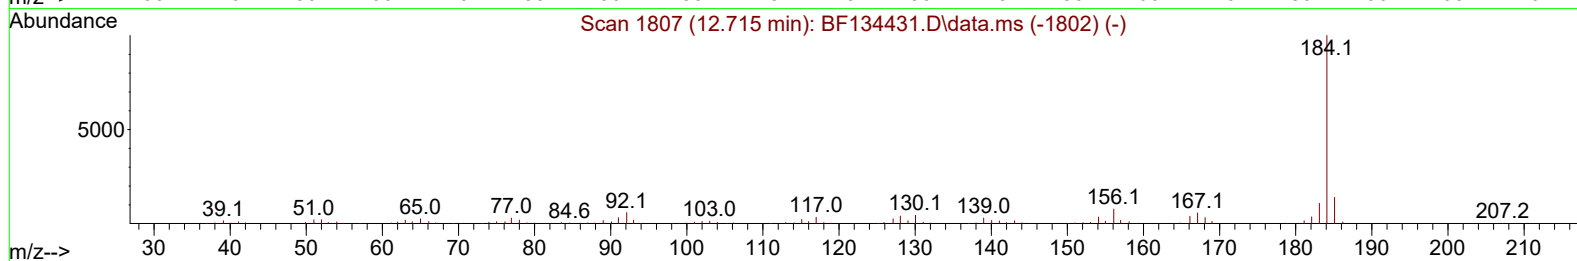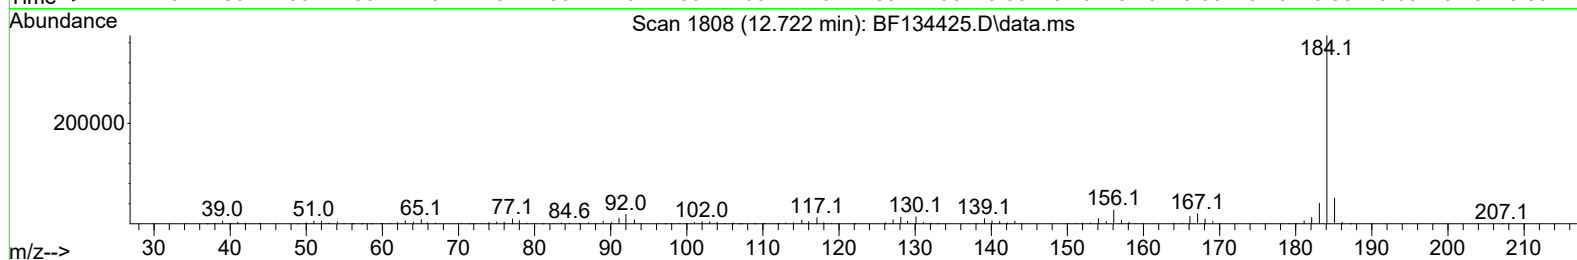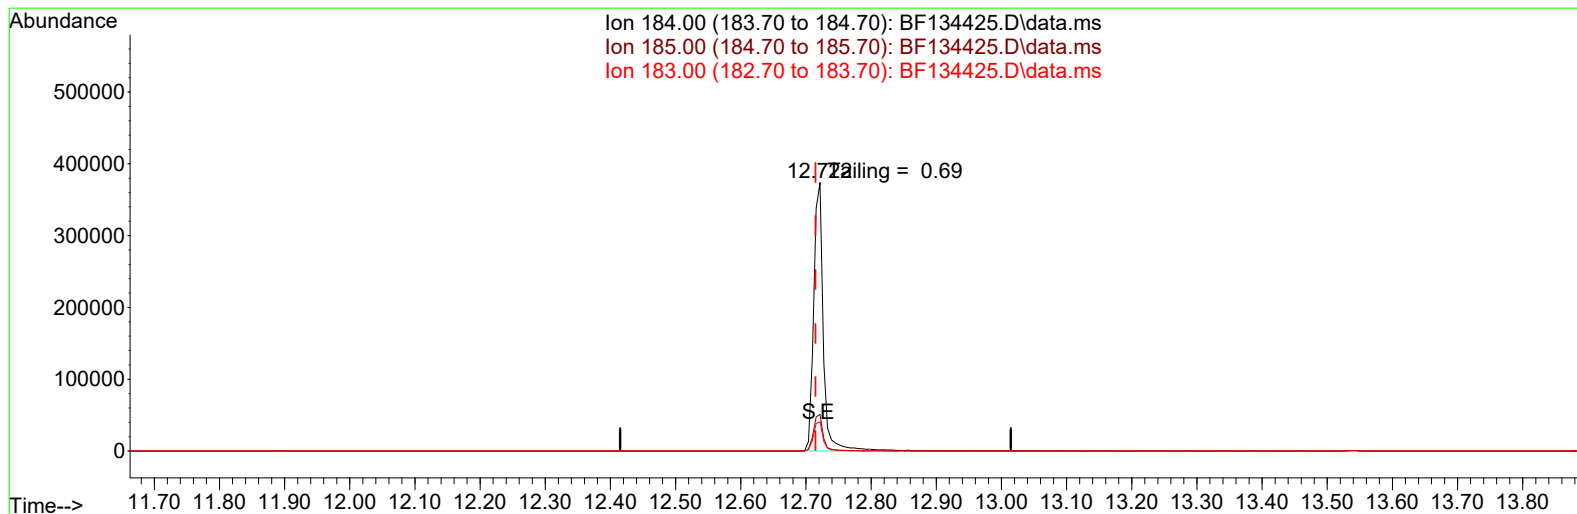

TIC: BF134425.D\data.ms

(77) Benzidine

12.722min (+ 0.007) 340931.88 ng

response 385818

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.66
183.00	10.80	10.94
0.00	0.00	0.00