
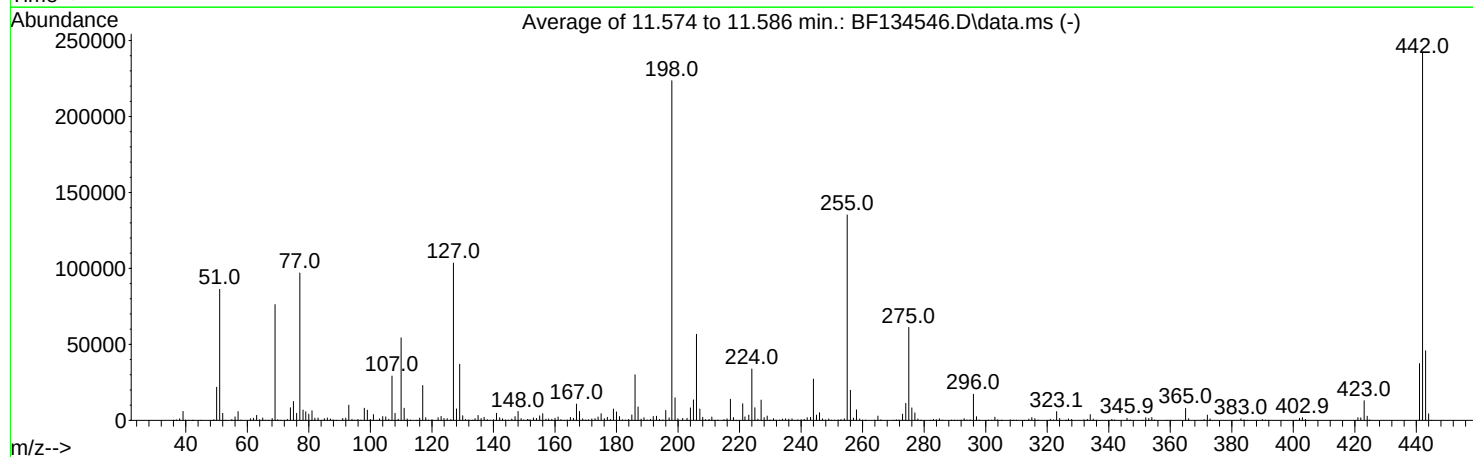


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080123\
 Data File : BF134546.D
 Acq On : 01 Aug 2023 13:54
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 02 02:20:34 2023

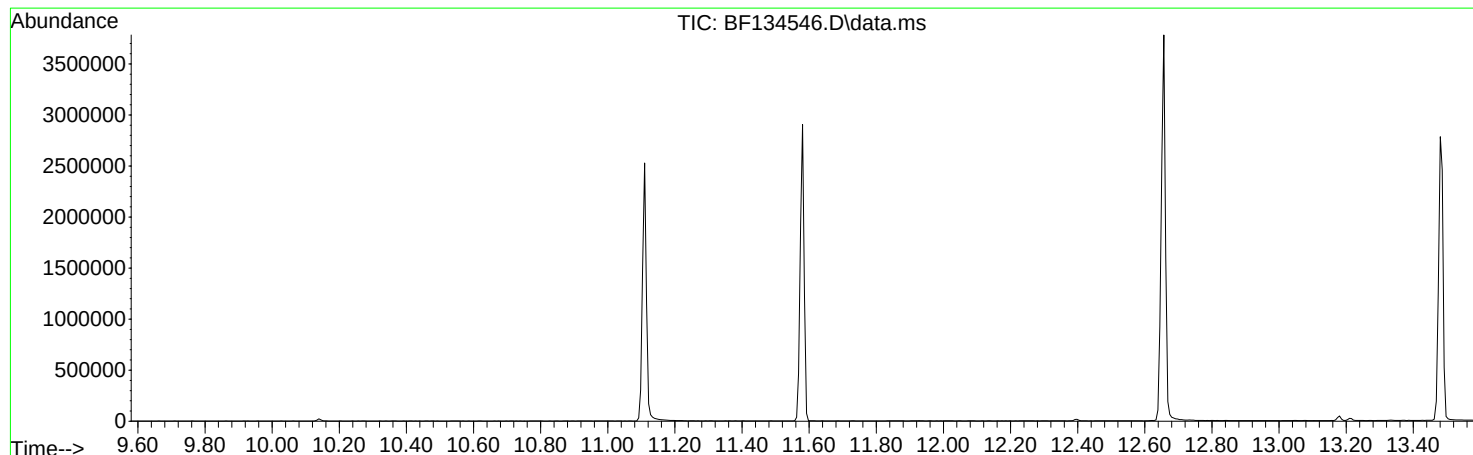




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	86294	PASS
68	69	0.00	2	1.7	1319	PASS
69	198	0.00	100	34.1	76248	PASS
70	69	0.00	2	0.5	416	PASS
127	198	10	80	46.3	103560	PASS
197	198	0.00	2	0.8	1718	PASS
198	198	100	100	100.0	223547	PASS
199	198	5	9	6.6	14851	PASS
275	198	10	60	27.4	61155	PASS
365	198	1	100	3.5	7916	PASS
441	198	0.01	100	16.7	37376	PASS
442	442	50	100	100.0	242109	PASS
443	442	15	24	18.9	45819	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080123\
Data File : BF134546.D
Acq On : 01 Aug 2023 13:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 04:17:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

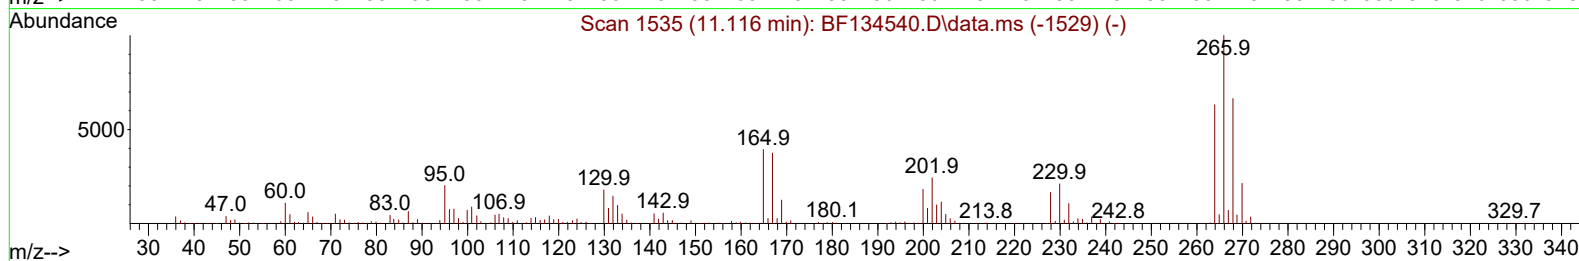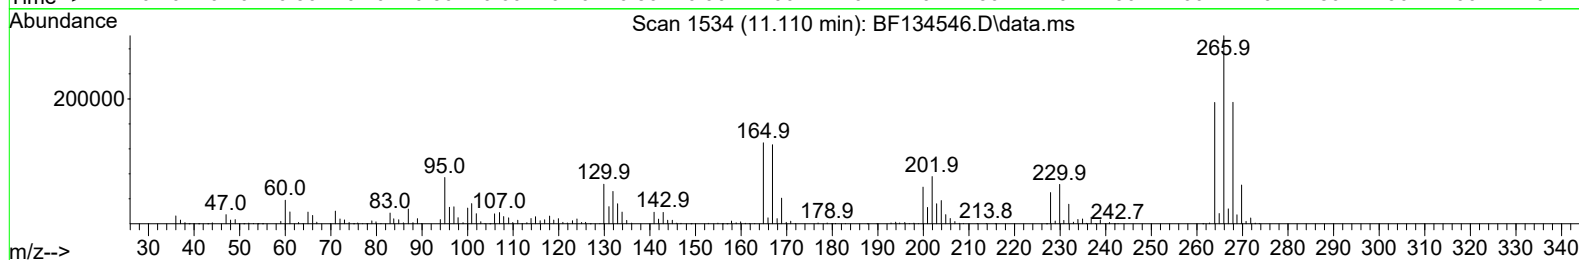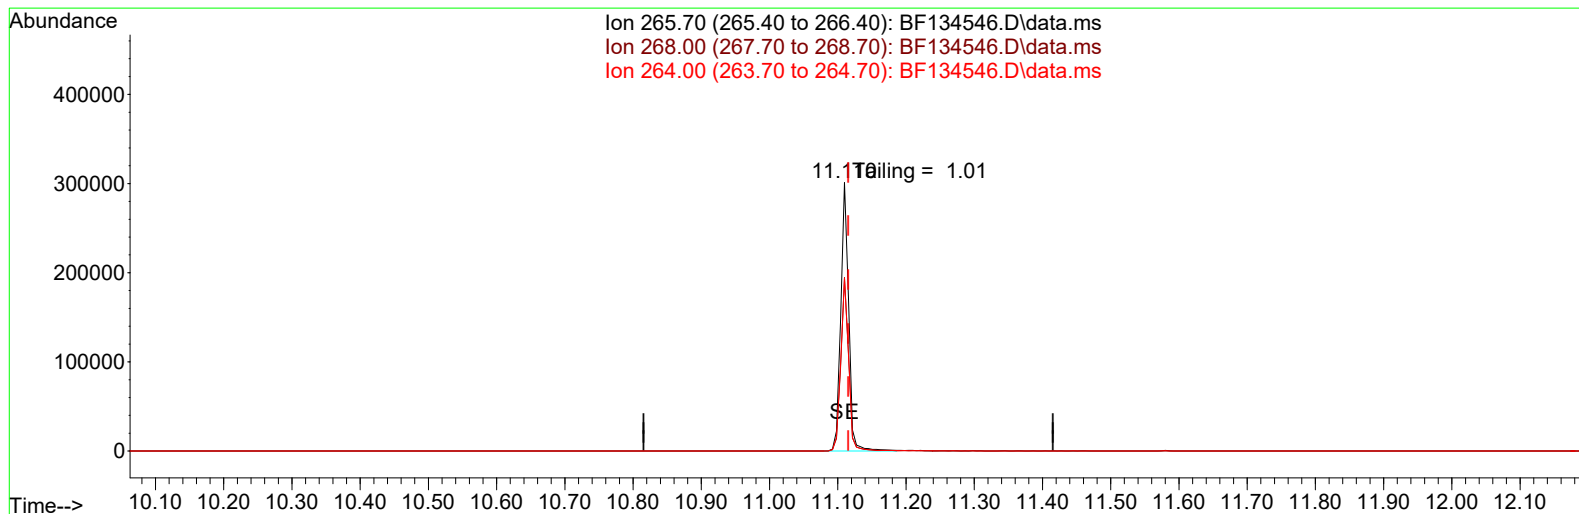

TIC: BF134546.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.006) 576934.29 ng




response 243630

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	64.58
264.00	59.70	64.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080123\
Data File : BF134546.D
Acq On : 01 Aug 2023 13:54
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 04:17:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

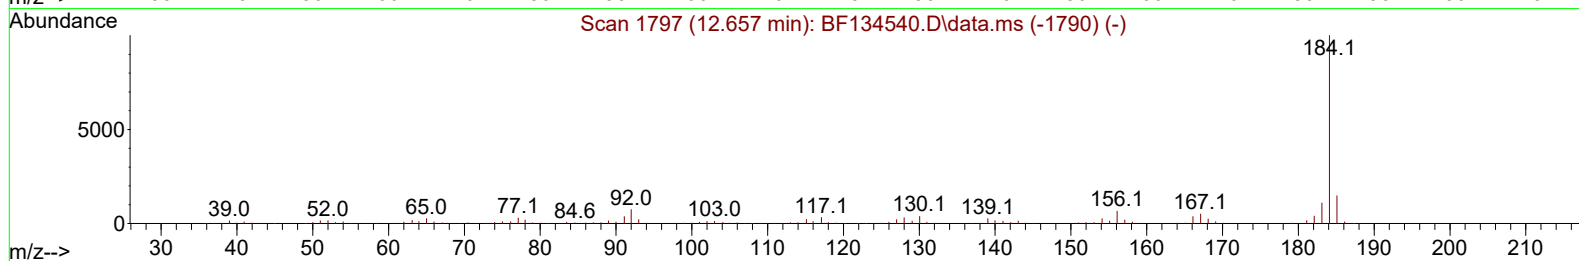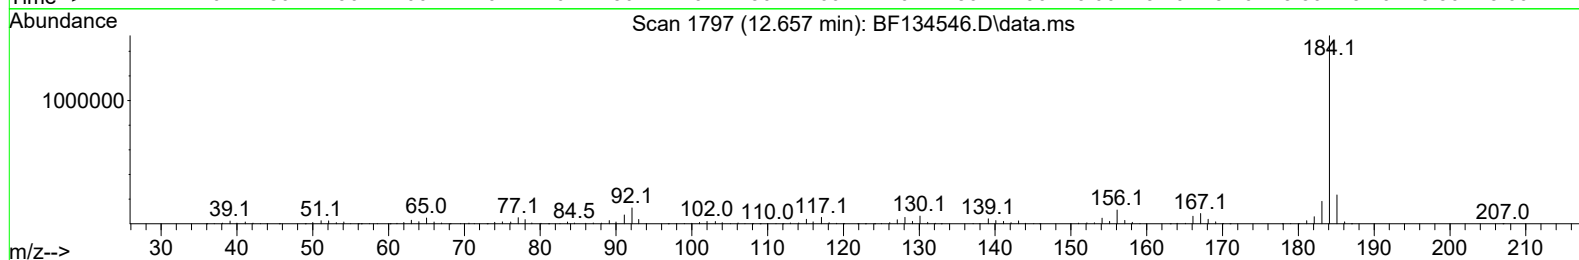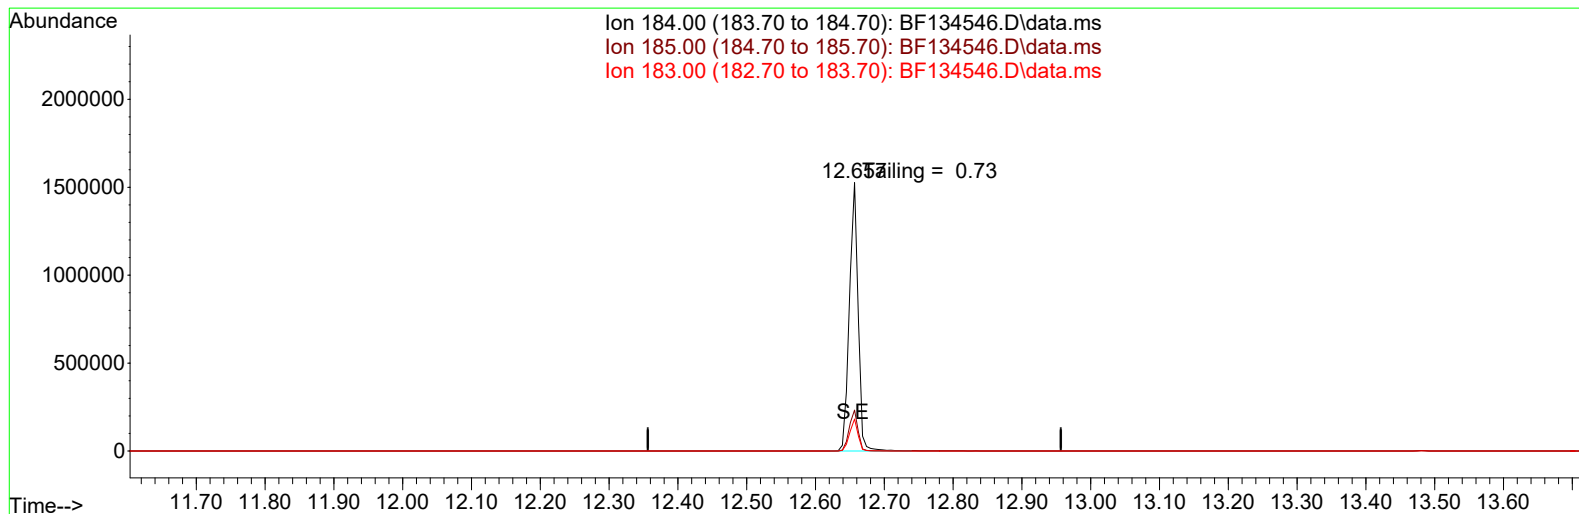

TIC: BF134546.D\data.ms

(77) Benzidine

12.657min (-12.657) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	14.00	0.00#
183.00	10.80	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/1/2023	BNA_F	<u>BF134546.D</u>
Compound Name	Response	Retention Time
DDT	482479	13.48
DDD	10648	13.18
DDE	80	12.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10728	493207	2.18

Instrument :
BNA_F
ClientSampleId :
DFTPP