
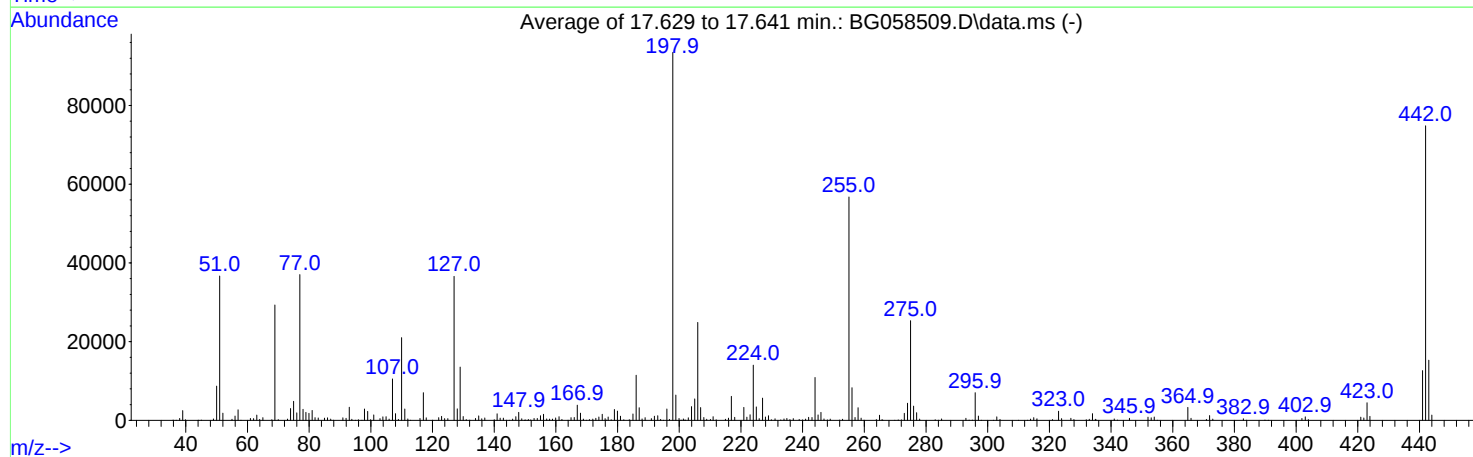


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058509.D
Acq On : 28 Jul 2023 8:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

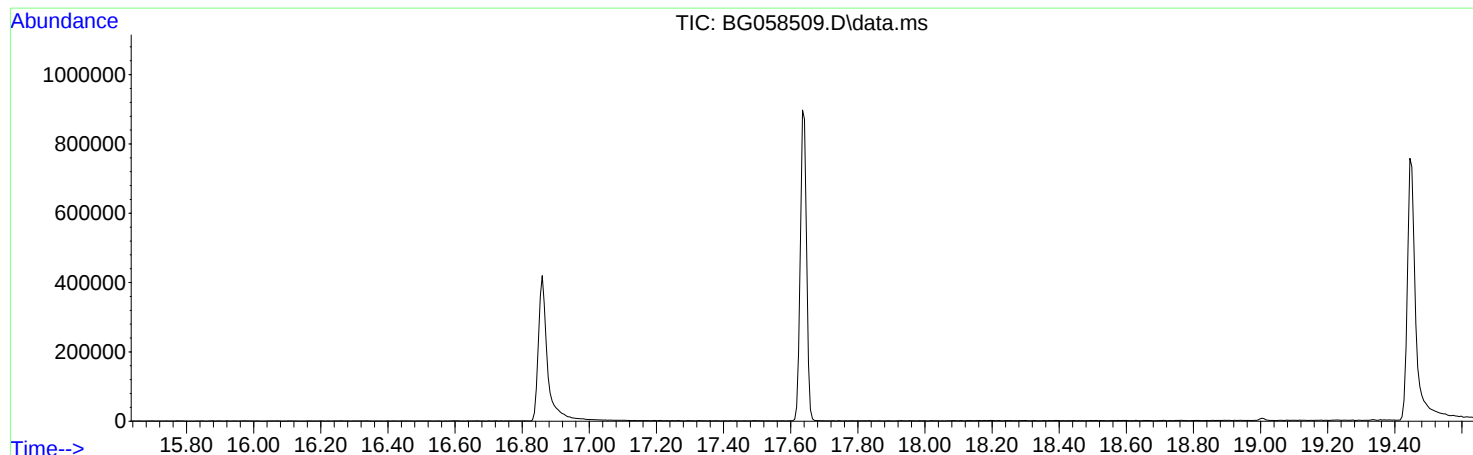




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	36656	PASS
68	69	0.00	2	0.5	145	PASS
69	198	0.00	100	31.4	29331	PASS
70	69	0.00	2	0.7	212	PASS
127	198	10	80	39.1	36589	PASS
197	198	0.00	2	0.2	230	PASS
198	198	100	100	100.0	93461	PASS
199	198	5	9	6.9	6446	PASS
275	198	10	60	27.1	25331	PASS
365	198	1	100	3.5	3287	PASS
441	198	0.01	100	13.5	12629	PASS
442	442	50	100	100.0	74859	PASS
443	442	15	24	20.4	15277	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058509.D
Acq On : 28 Jul 2023 8:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 28 15:27:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 14:44:42 2023
Response via : Initial Calibration

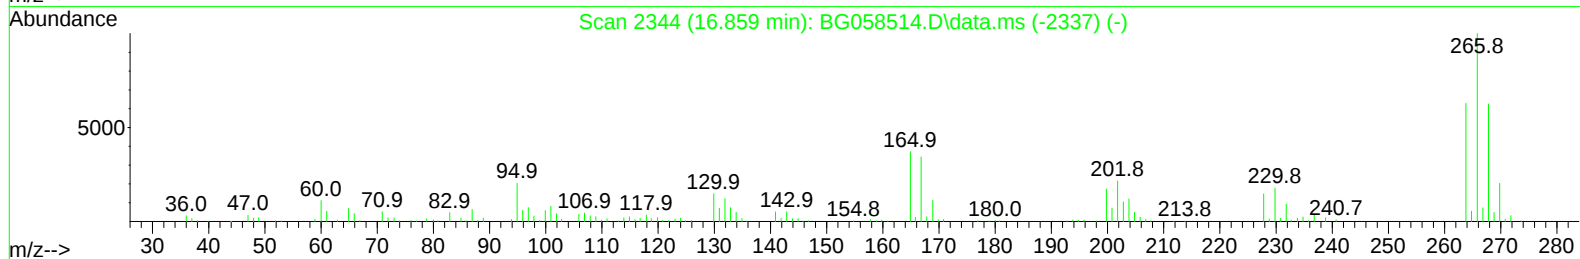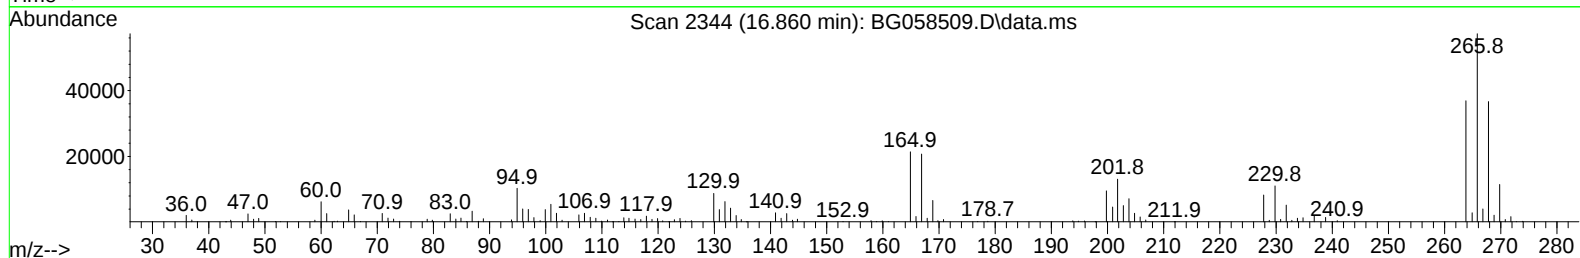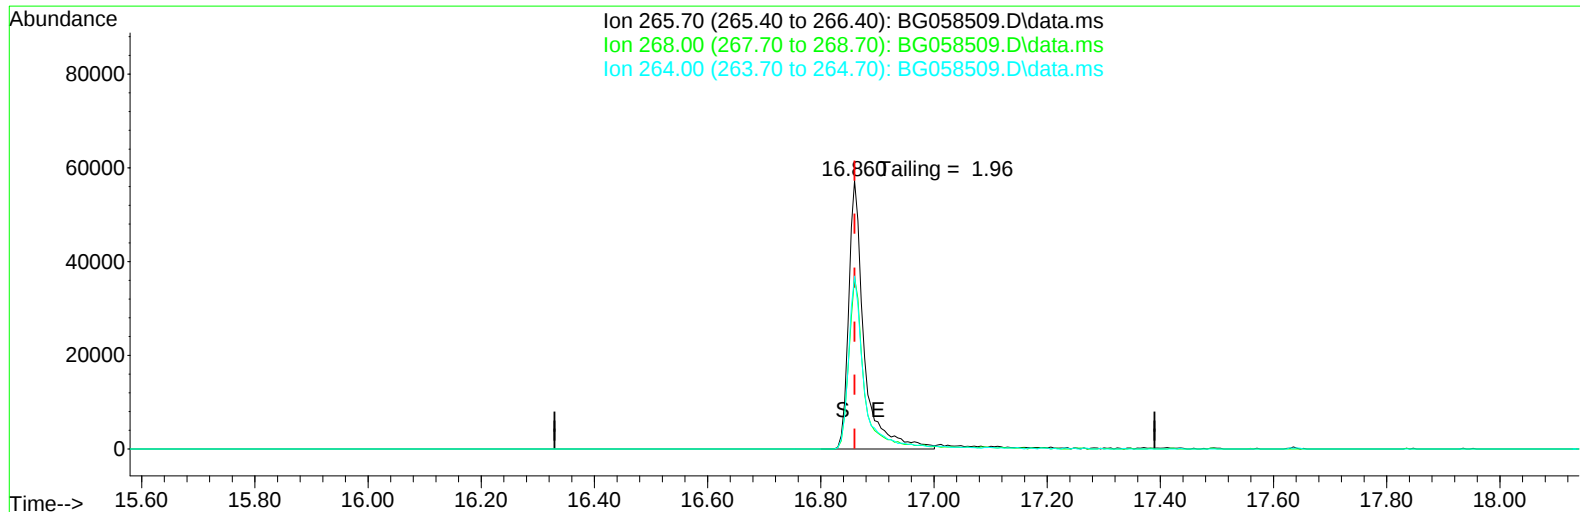

TIC: BG058509.D\data.ms

(70) Pentachlorophenol (C)

16.860min (+ 0.000) 26830.98 ng




response 109111

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	63.99
264.00	63.60	64.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG072823\
Data File : BG058509.D
Acq On : 28 Jul 2023 8:40
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jul 28 15:27:08 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 14:44:42 2023
Response via : Initial Calibration

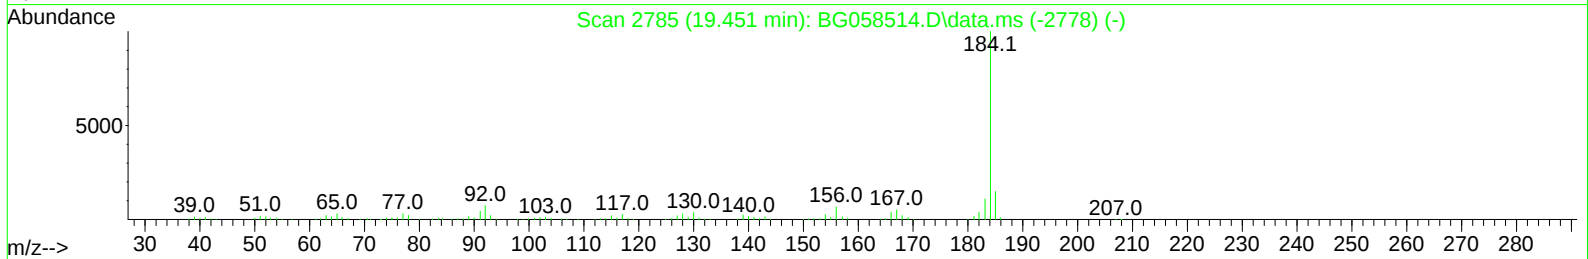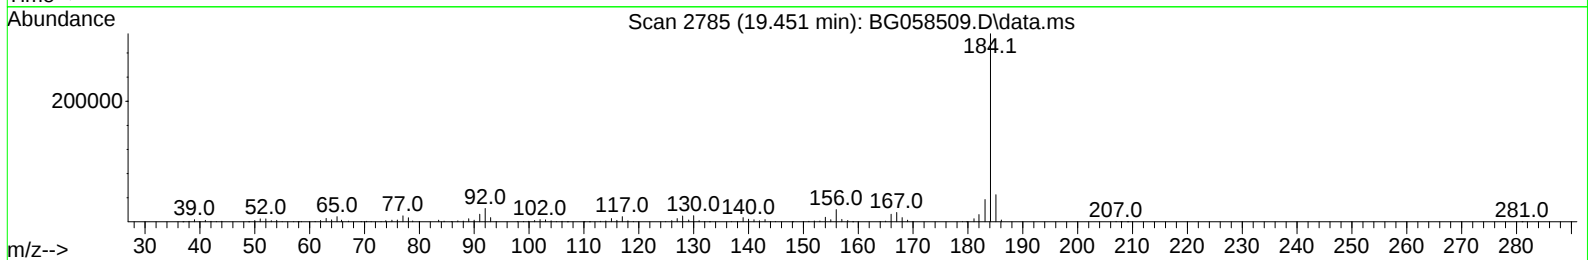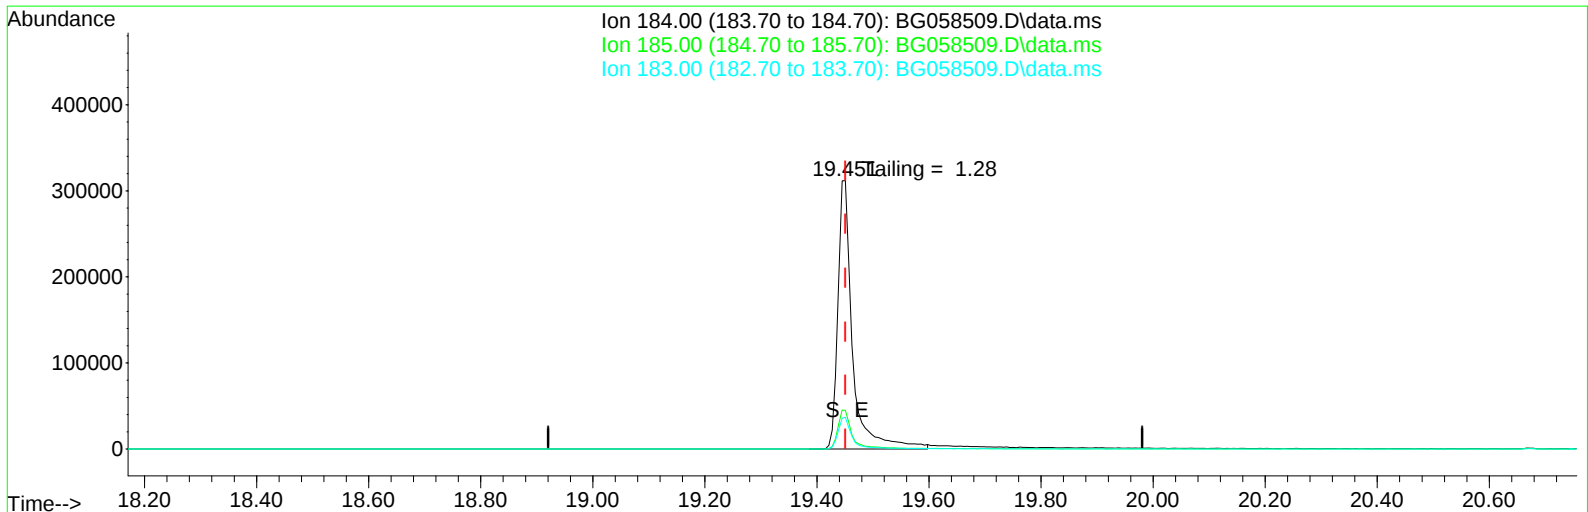

TIC: BG058509.D\data.ms

(77) Benzidine

19.451min (+ 0.000) 689236.40 ng

response 595742

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.46
183.00	11.20	11.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/28/2023	BNA_G	<u>BG058509.D</u>
Compound Name	Response	Retention Time
DDT	278134	20.673
DDD	36075	20.238
DDE	422	19.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
36497	314631	11.60

Instrument :
BNA_G
ClientSampleId :
DFTPP