
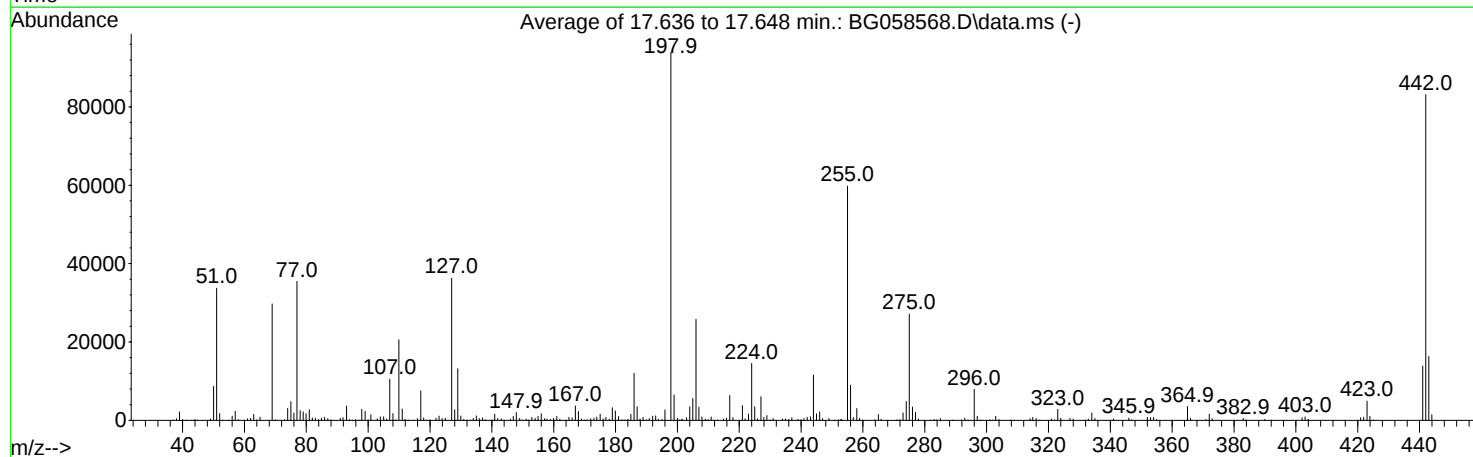


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080223\
Data File : BG058568.D
Acq On : 2 Aug 2023 7:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 28 22:29:07 2023

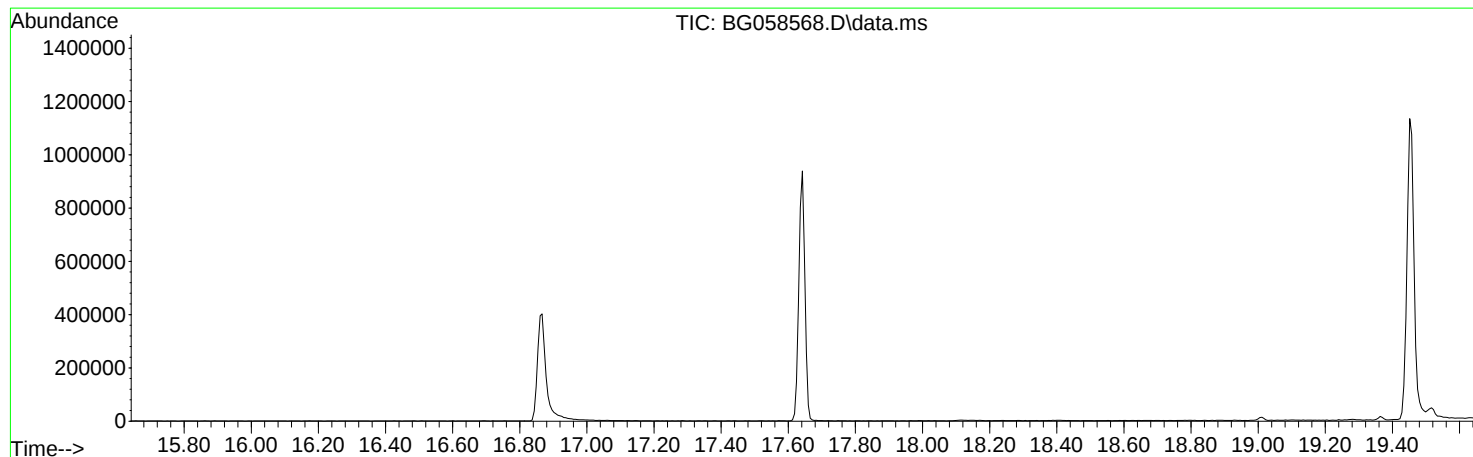




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	33704	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.6	29699	PASS
70	69	0.00	2	0.5	163	PASS
127	198	10	80	38.6	36264	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	93907	PASS
199	198	5	9	6.9	6476	PASS
275	198	10	60	28.9	27157	PASS
365	198	1	100	3.7	3477	PASS
441	198	0.01	100	14.8	13869	PASS
442	442	50	100	100.0	83157	PASS
443	442	15	24	19.6	16271	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080223\
Data File : BG058568.D
Acq On : 2 Aug 2023 7:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 02 13:12:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

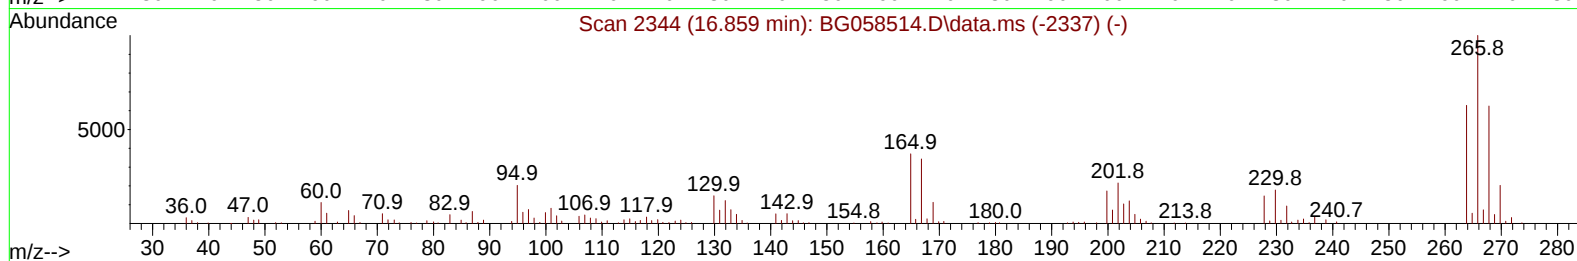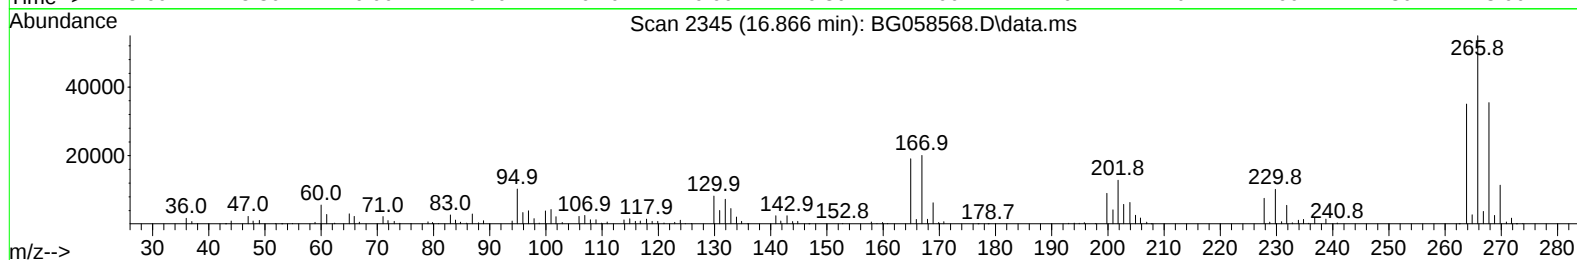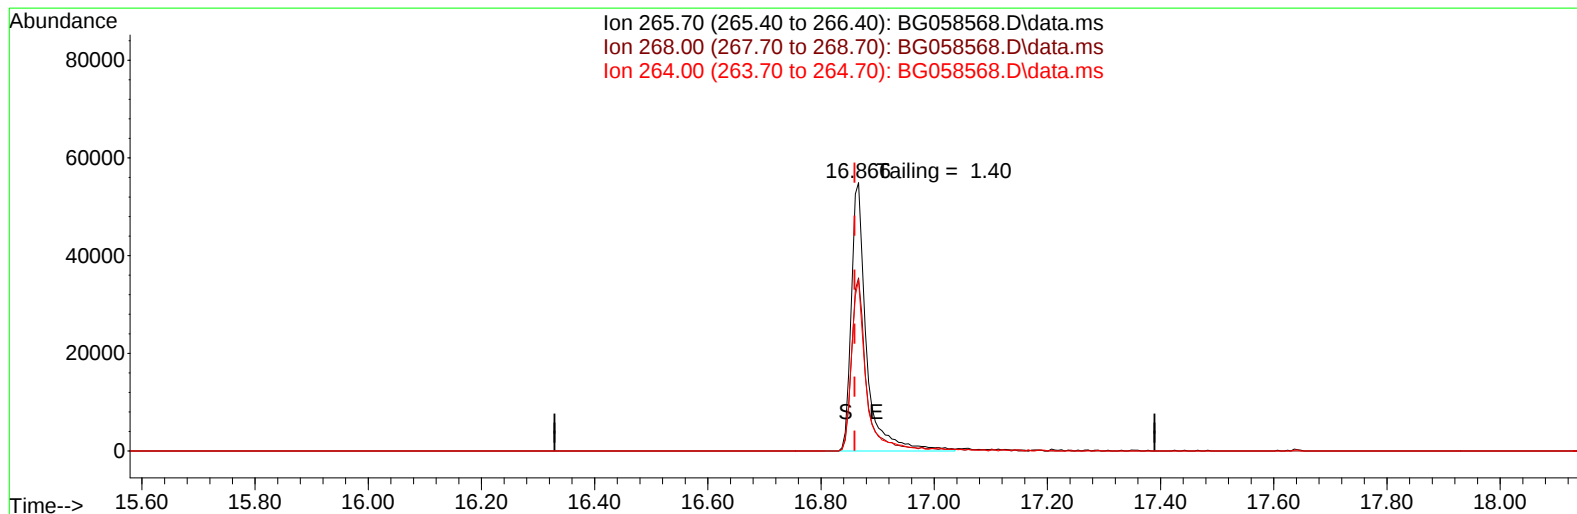

TIC: BG058568.D\data.ms

(70) Pentachlorophenol (C)

16.866min (+ 0.007) 24371.16 ng




response 103007

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	64.55
264.00	62.80	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG080223\
Data File : BG058568.D
Acq On : 2 Aug 2023 7:54
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Aug 02 13:12:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 22:29:07 2023
Response via : Initial Calibration

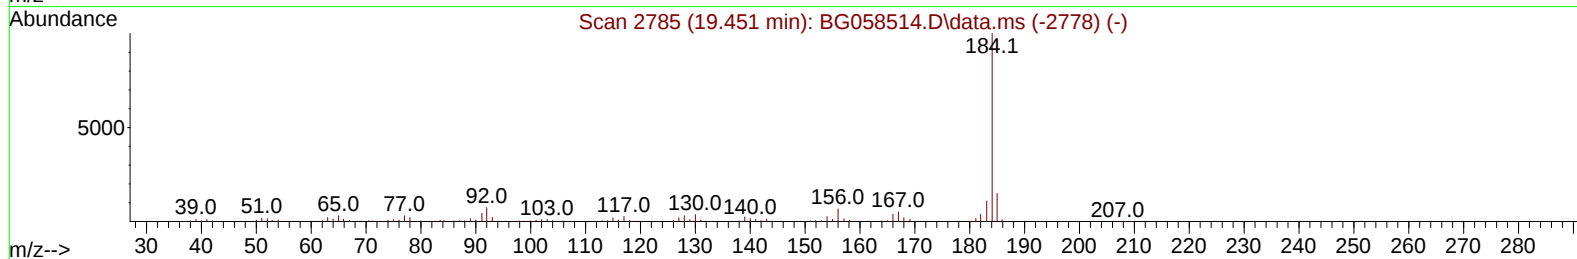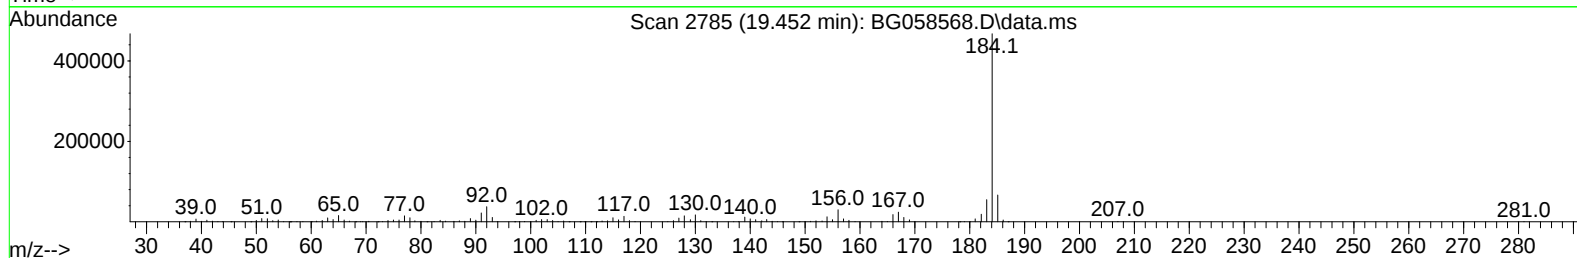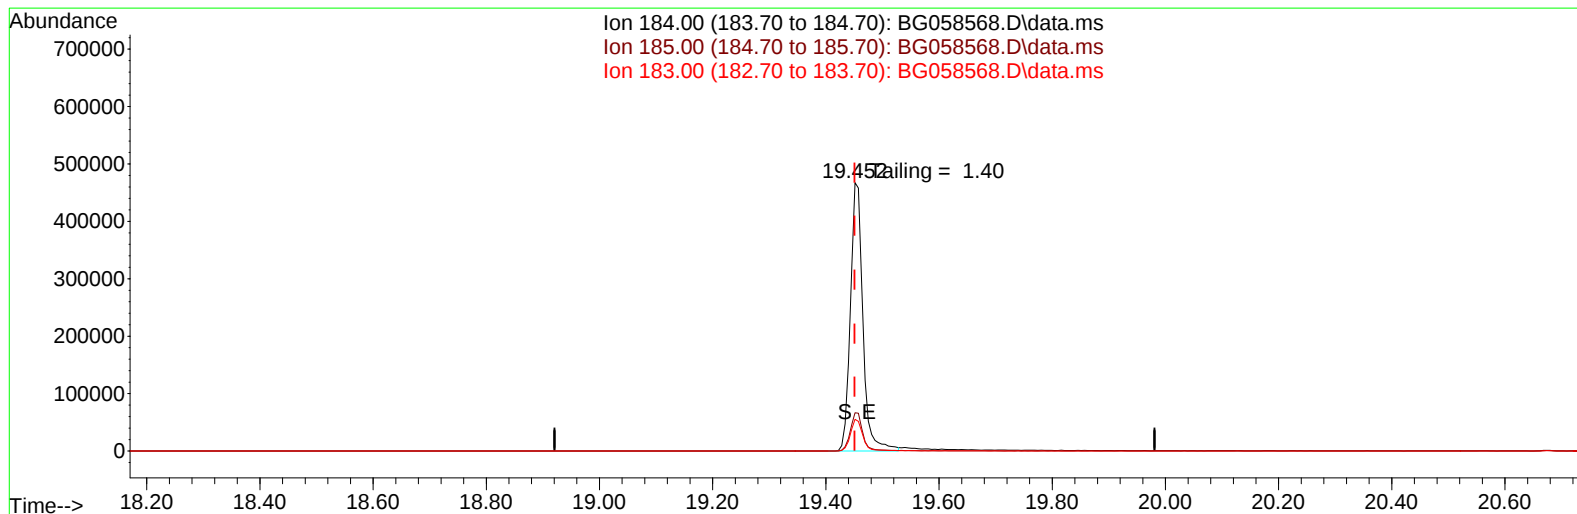

TIC: BG058568.D\data.ms

(77) Benzidine

19.452min (+ 0.001) 0.00 ng

response 736507

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.27
183.00	10.90	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2023	BNA_G	<u>BG058568.D</u>
Compound Name	Response	Retention Time
DDT	358023	20.674
DDD	5744	20.286
DDE	67	19.74
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5811	363834	1.60

Instrument :
BNA_G
ClientSampleId :
DFTPP