


Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM072823\  
Data File : BM041157.D  
Acq On : 28 Jul 2023 09:37  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Sat Jul 29 00:19:24 2023

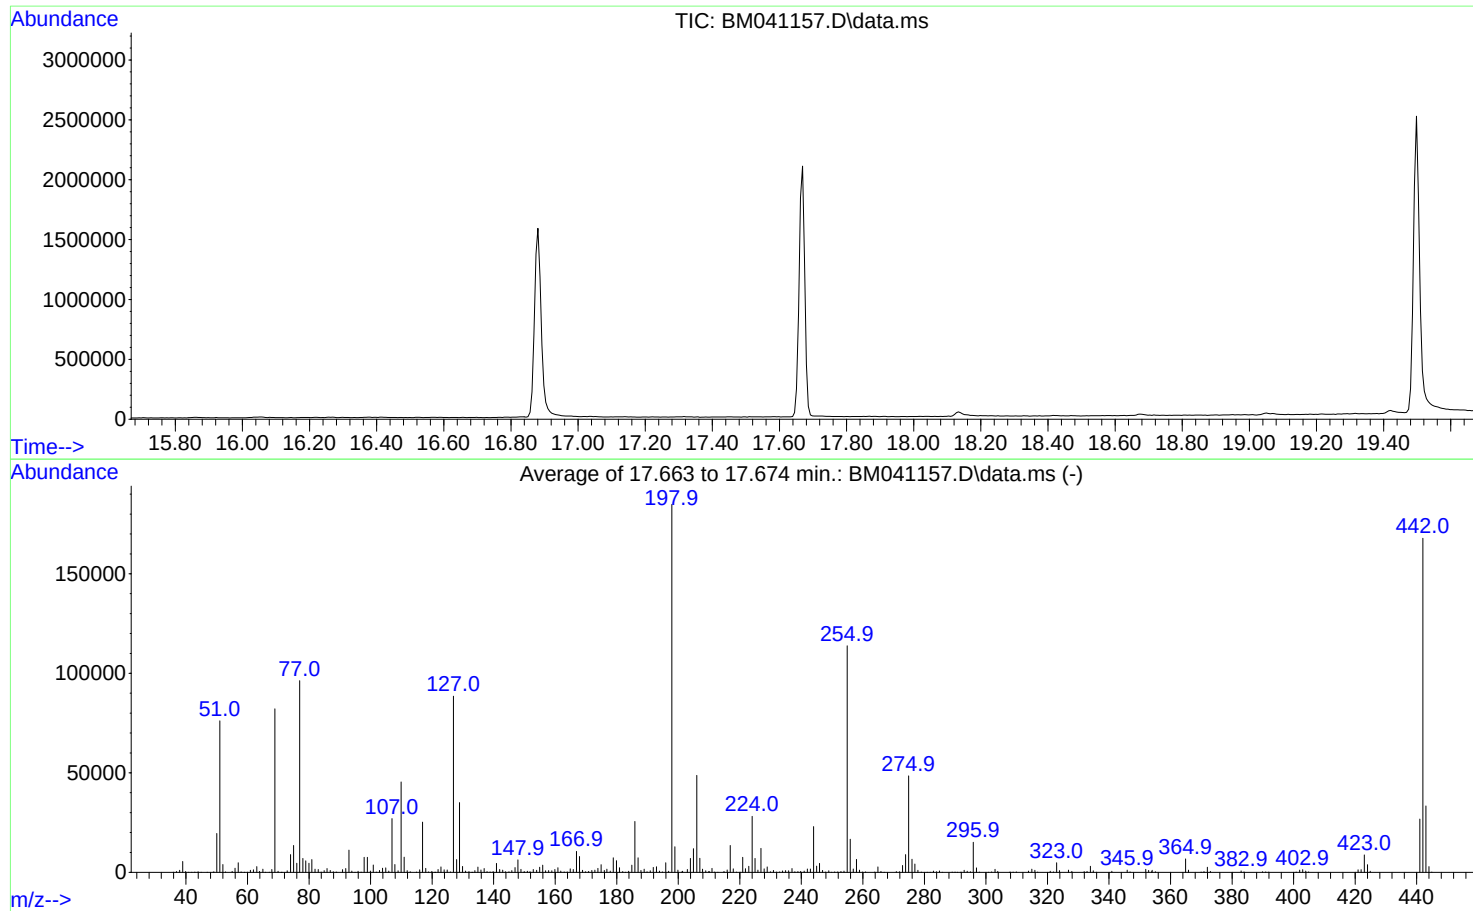




AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2454

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 41.2         | 76123      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.8          | 1464       | PASS                |
| 69             | 198             | 0.00            | 100             | 44.5         | 82170      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.7          | 539        | PASS                |
| 127            | 198             | 10              | 80              | 47.9         | 88523      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 581        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 184811     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 12841      | PASS                |
| 275            | 198             | 10              | 60              | 26.2         | 48491      | PASS                |
| 365            | 198             | 1               | 100             | 3.6          | 6722       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.5         | 26797      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 167851     | PASS                |
| 443            | 442             | 15              | 24              | 19.9         | 33379      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM072823\  
Data File : BM041157.D  
Acq On : 28 Jul 2023 09:37  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Jul 29 04:31:06 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jul 29 00:19:24 2023  
Response via : Initial Calibration

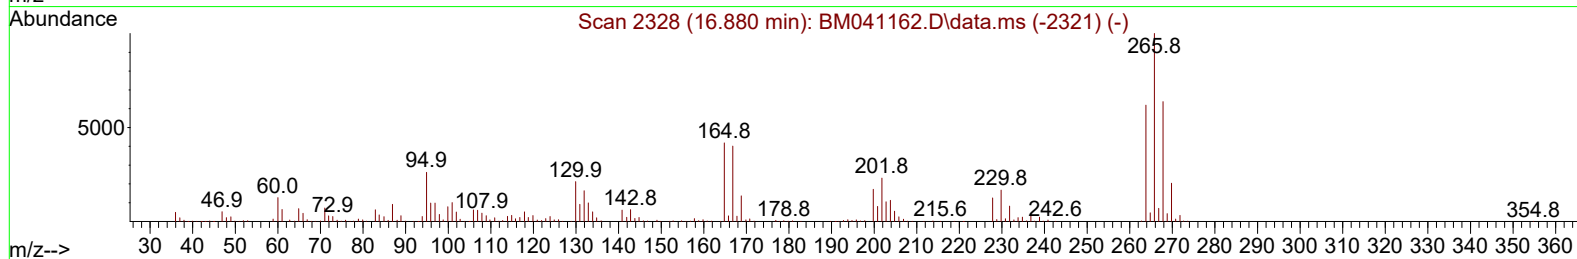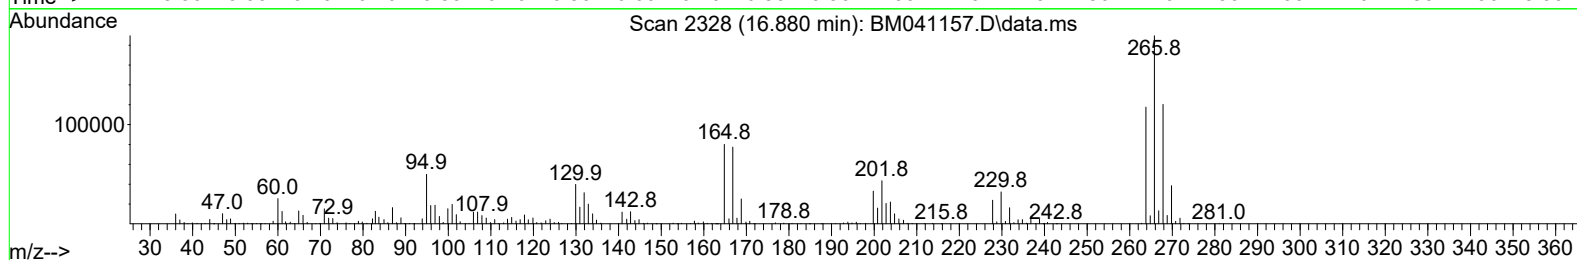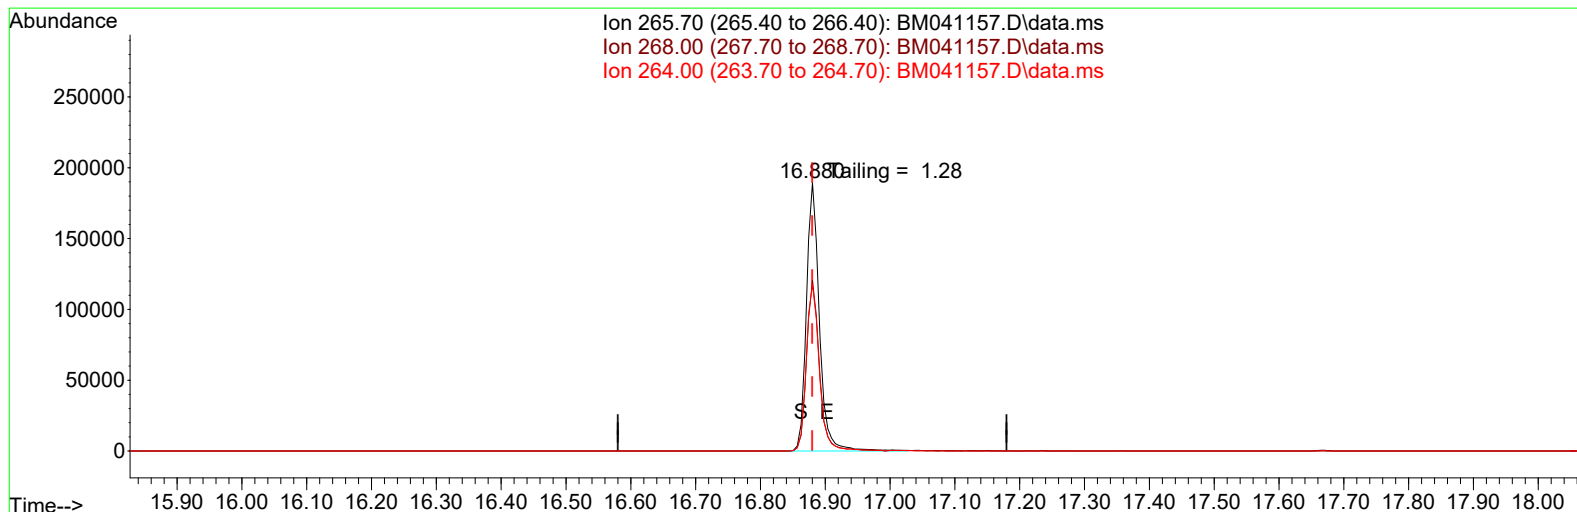

TIC: BM041157.D\data.ms

**(70) Pentachlorophenol (C)**

16.880min (+ 0.000) 0.00 ng




response 264374

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.80  | 63.49  |
| 264.00 | 61.80  | 62.04  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM072823\  
Data File : BM041157.D  
Acq On : 28 Jul 2023 09:37  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP

Quant Time: Jul 29 04:31:06 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM072823.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jul 29 00:19:24 2023  
Response via : Initial Calibration

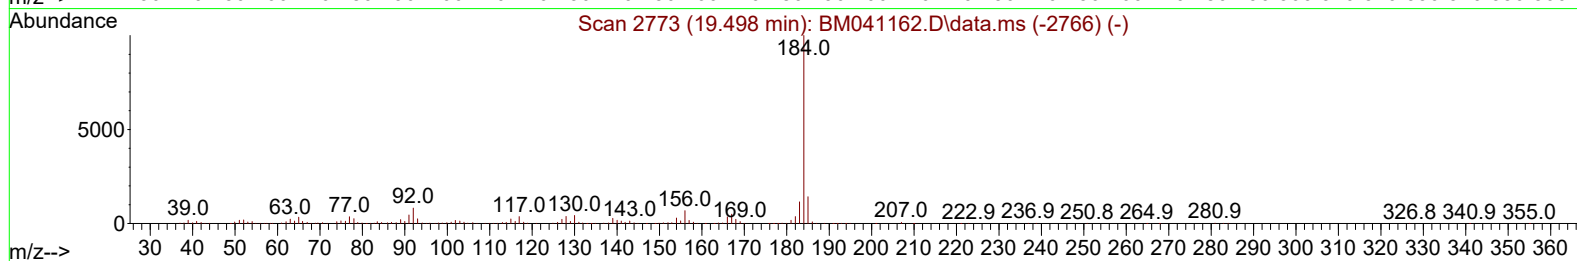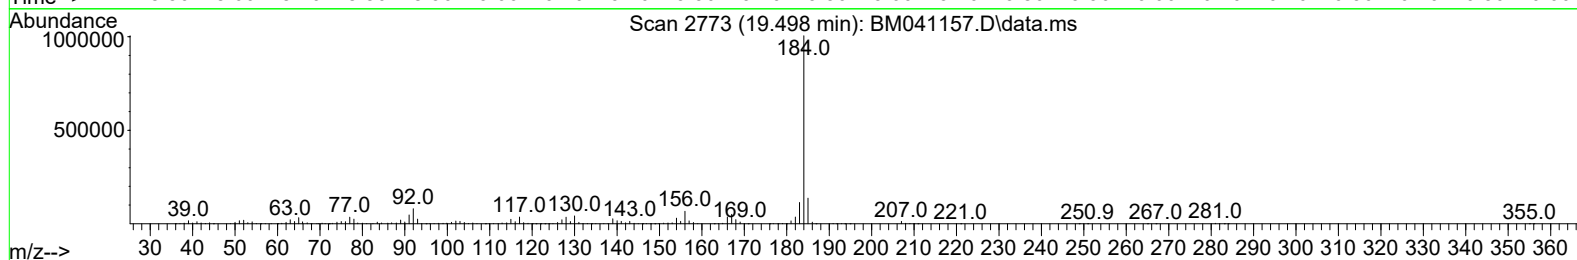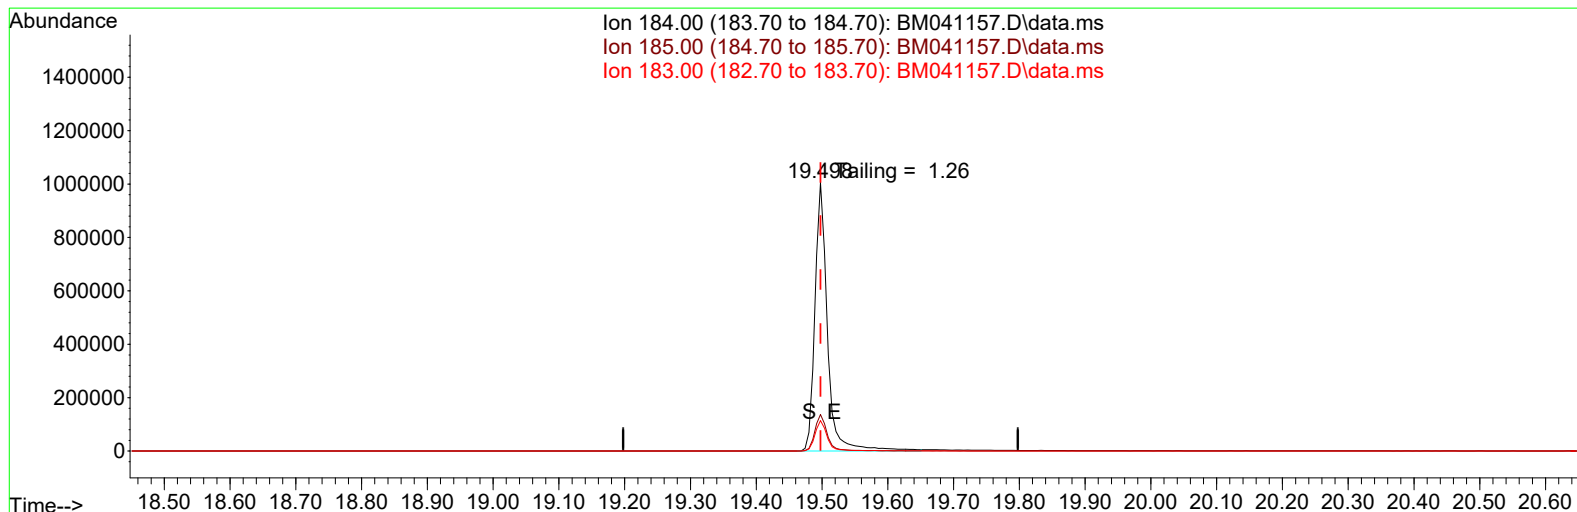

TIC: BM041157.D\data.ms

(77) Benzidine

19.498min (-0.000) 0.00 ng

response 1327248

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 13.60  |
| 183.00 | 11.50  | 11.35  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 7/28/2023     | BNA_M            | <u>BM041157.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 634693           | 20.721             |
| DDD           | 5028             | 20.333             |
| DDE           | 0                | 19.892             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 5028          | 639721           | 0.79               |
|               |                  |                    |

Instrument :  
BNA\_M  
ClientSampleId :  
DFTPP