


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072823\
Data File : BM041168.D
Acq On : 28 Jul 2023 16:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jul 29 00:19:24 2023

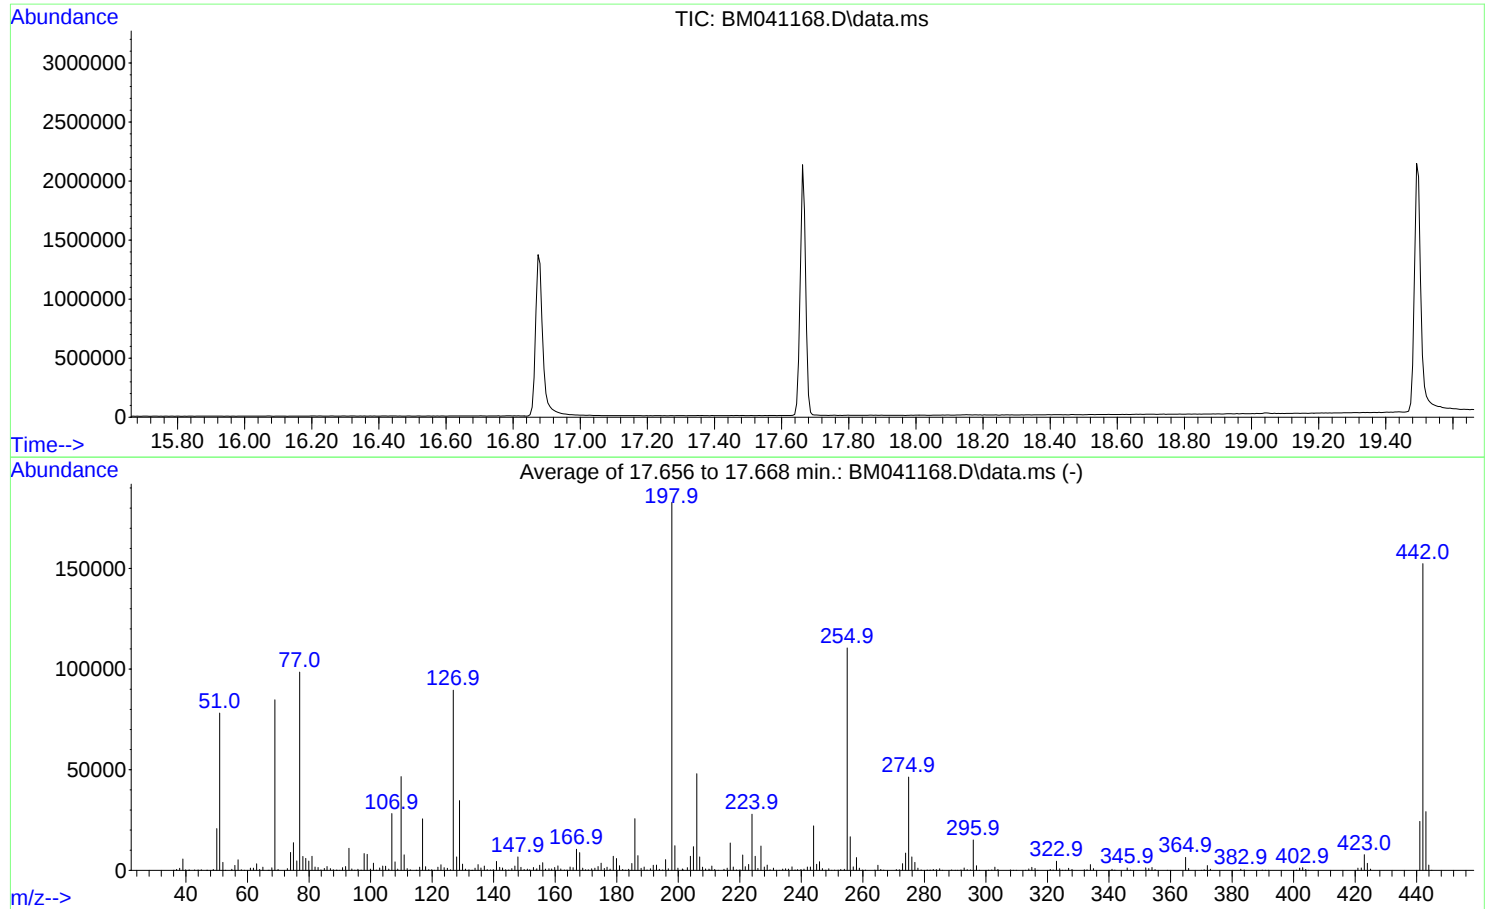




AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2454

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	78187	PASS
68	69	0.00	2	1.5	1241	PASS
69	198	0.00	100	46.4	84789	PASS
70	69	0.00	2	0.6	514	PASS
127	198	10	80	49.0	89536	PASS
197	198	0.00	2	0.4	815	PASS
198	198	100	100	100.0	182784	PASS
199	198	5	9	6.7	12214	PASS
275	198	10	60	25.3	46328	PASS
365	198	1	100	3.5	6473	PASS
441	198	0.01	100	13.3	24323	PASS
442	442	50	100	100.0	152400	PASS
443	442	15	24	19.1	29177	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072823\
Data File : BM041168.D
Acq On : 28 Jul 2023 16:33
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jul 29 04:32:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jul 29 00:19:24 2023
Response via : Initial Calibration

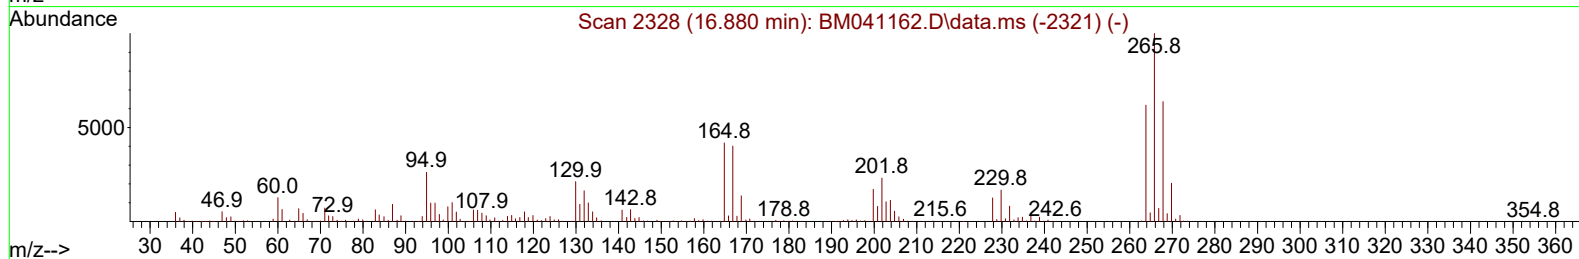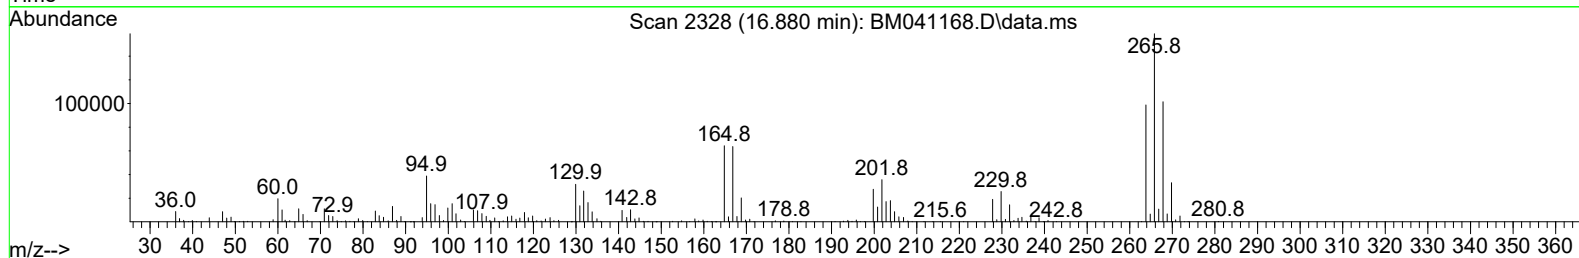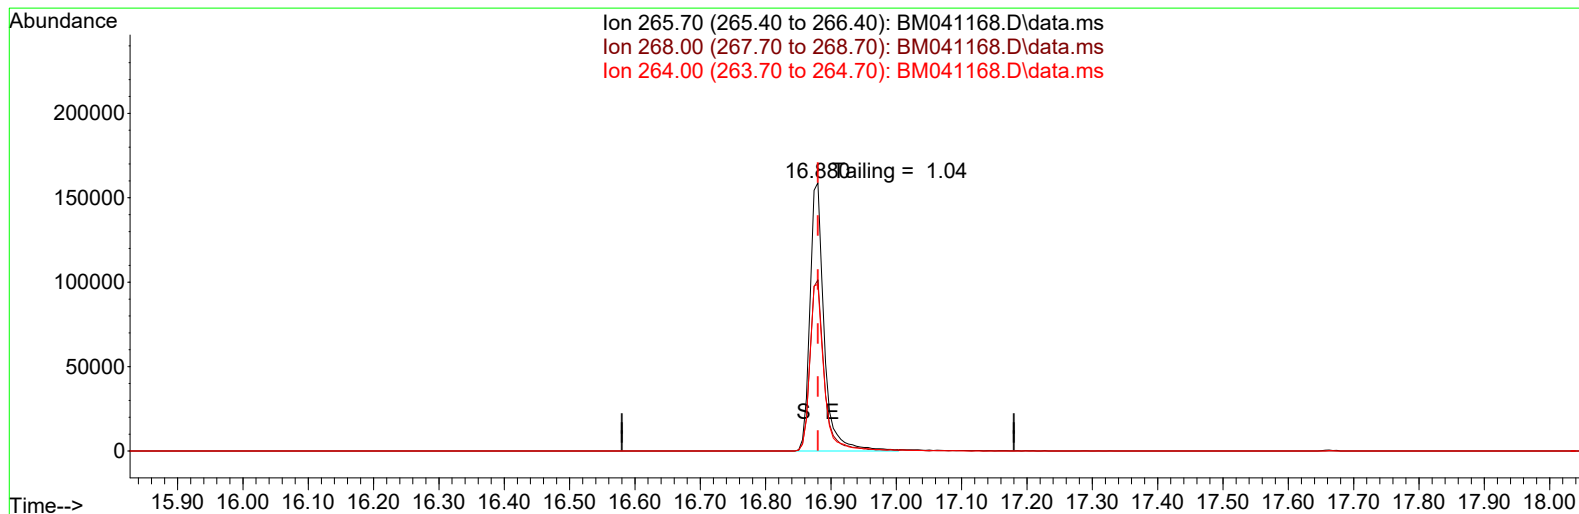

TIC: BM041168.D\data.ms

(70) Pentachlorophenol (C)

16.880min (-0.000) 0.00 ng




response 242566

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.83
264.00	61.80	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM072823\
 Data File : BM041168.D
 Acq On : 28 Jul 2023 16:33
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jul 29 04:32:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM072823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jul 29 00:19:24 2023
 Response via : Initial Calibration

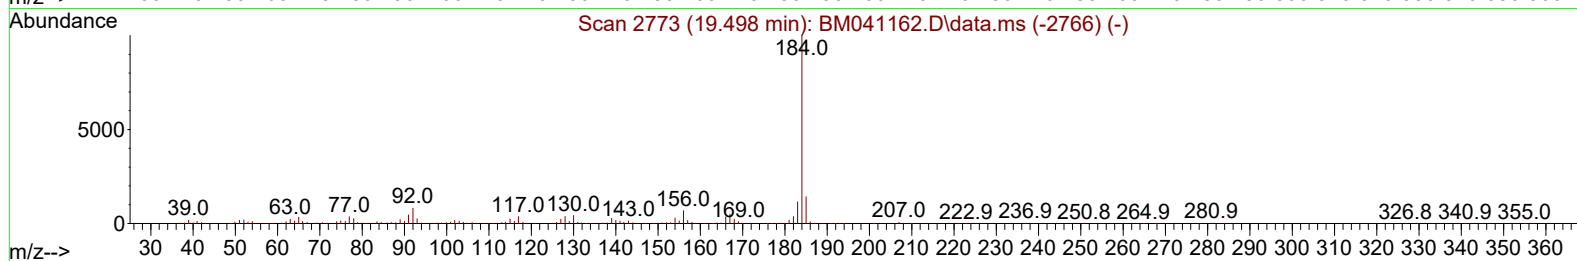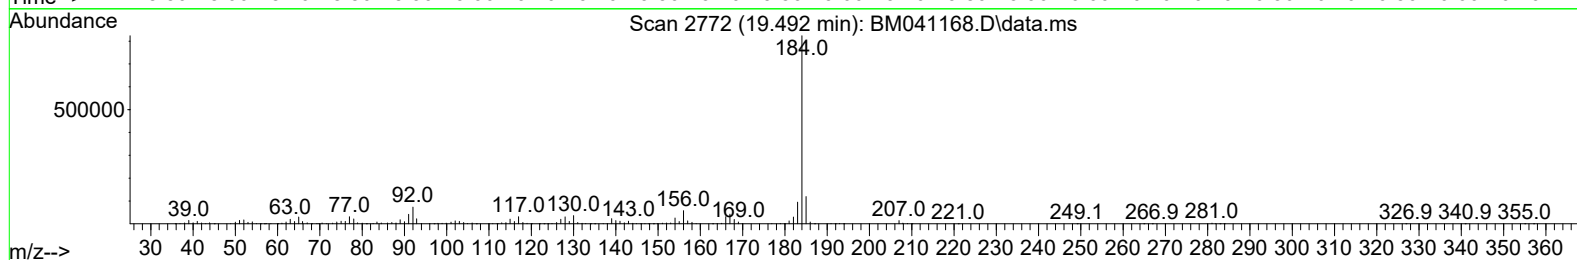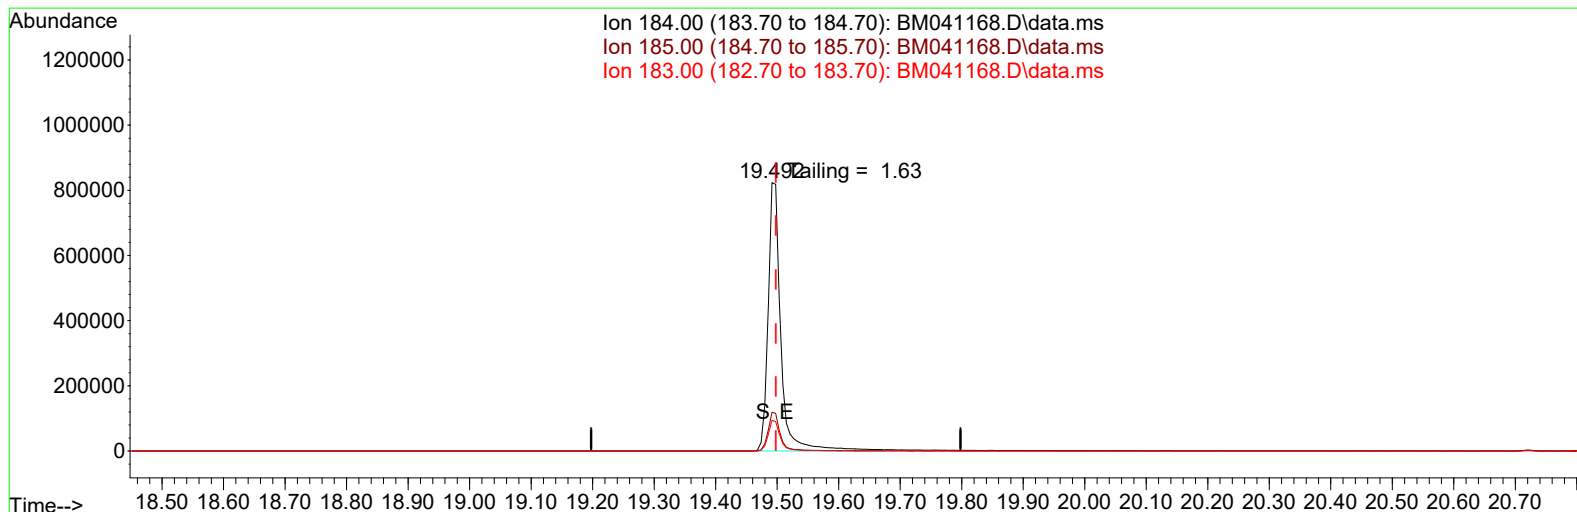

TIC: BM041168.D\data.ms

(77) Benzidine

19.492min (-0.006) 1371060.88 ng

response 1214682

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.46
183.00	11.50	11.47
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/28/2023	BNA_M	<u>BM041168.D</u>
Compound Name	Response	Retention Time
DDT	699038	20.721
DDD	6846	20.327
DDE	0	19.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6846	705884	0.97

Instrument :
BNA_M
ClientSampleId :
DFTPP