
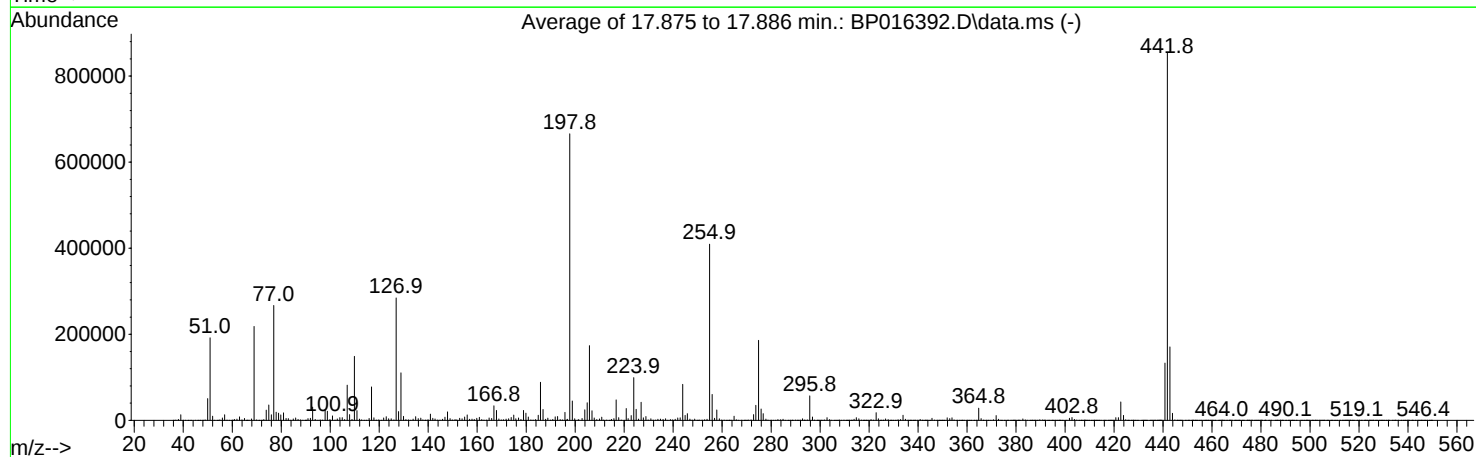


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072723\
 Data File : BP016392.D
 Acq On : 27 Jul 2023 09:55
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 28 01:48:25 2023

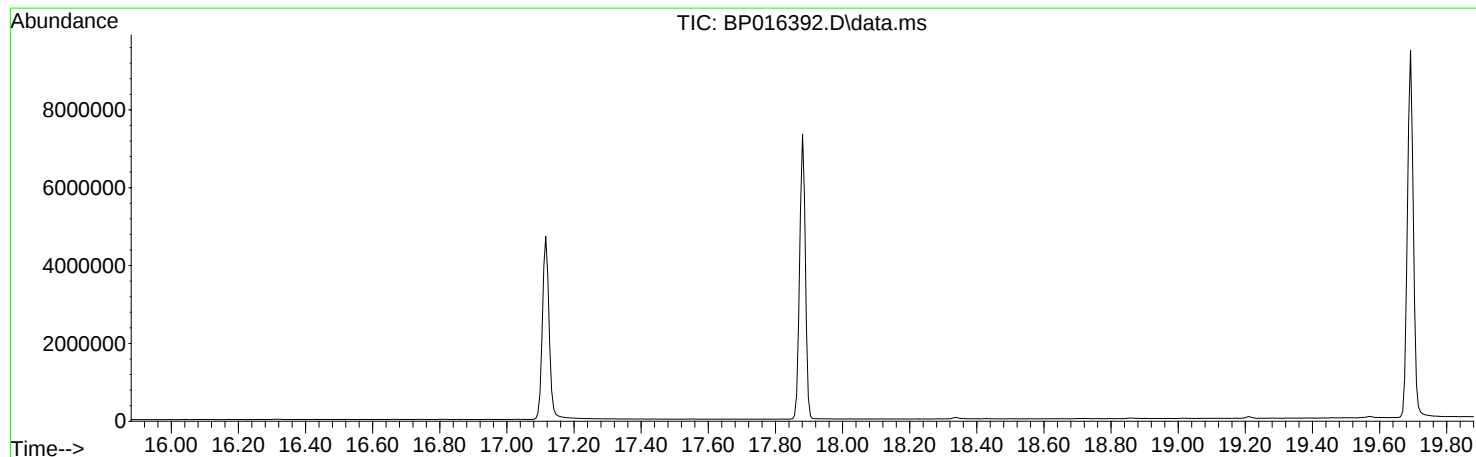




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	191899	PASS
68	69	0.00	2	1.6	3500	PASS
69	198	0.00	100	32.8	218170	PASS
70	69	0.00	2	0.5	1122	PASS
127	198	10	80	42.7	284544	PASS
197	198	0.00	2	0.4	2682	PASS
198	198	100	100	100.0	665877	PASS
199	198	5	9	6.8	45040	PASS
275	198	10	60	27.9	185892	PASS
365	198	1	100	4.2	28203	PASS
441	198	0.01	100	20.0	133110	PASS
442	442	100	100	100.0	854821	PASS
443	442	15	24	20.0	170739	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072723\
Data File : BP016392.D
Acq On : 27 Jul 2023 09:55
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 28 04:44:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 28 01:48:25 2023
Response via : Initial Calibration

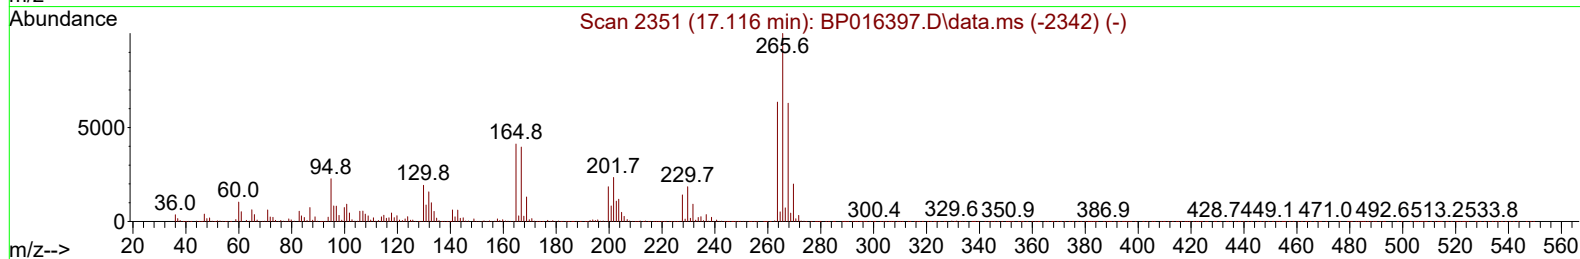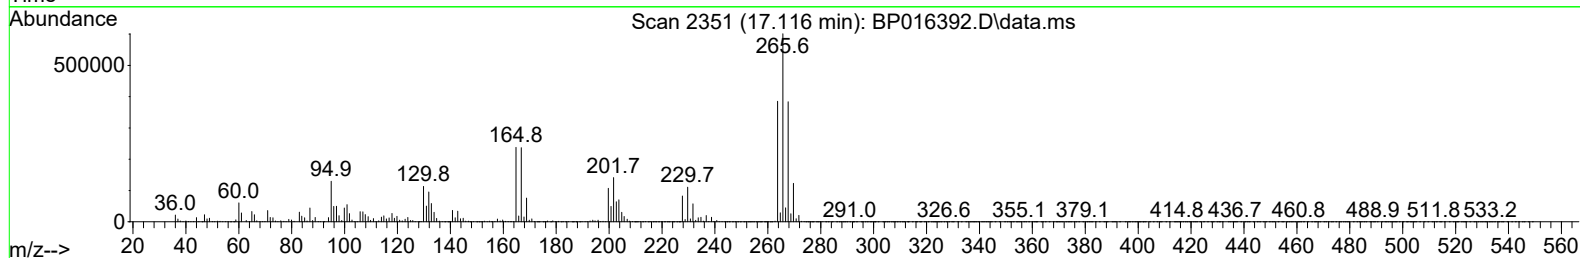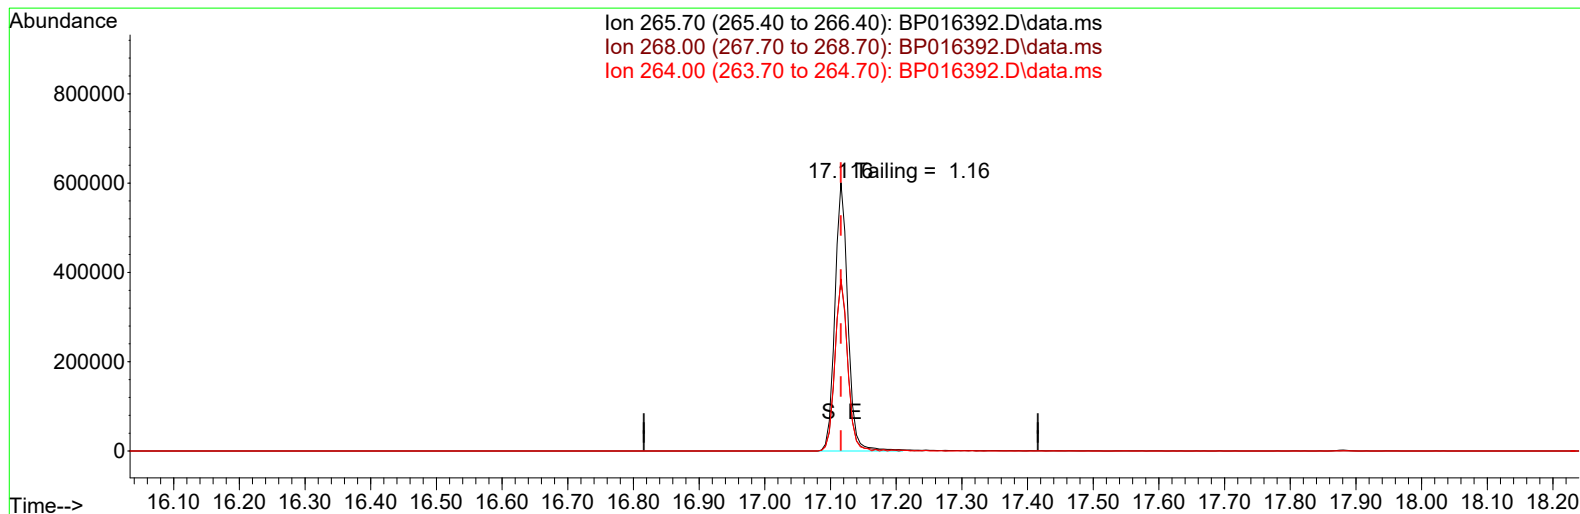

TIC: BP016392.D\data.ms

(70) Pentachlorophenol (C)

17.116min (-0.000) 104614.76 ng




response 830934

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.40	68.10
264.00	68.60	68.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072723\
 Data File : BP016392.D
 Acq On : 27 Jul 2023 09:55
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 28 04:44:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 28 01:48:25 2023
 Response via : Initial Calibration

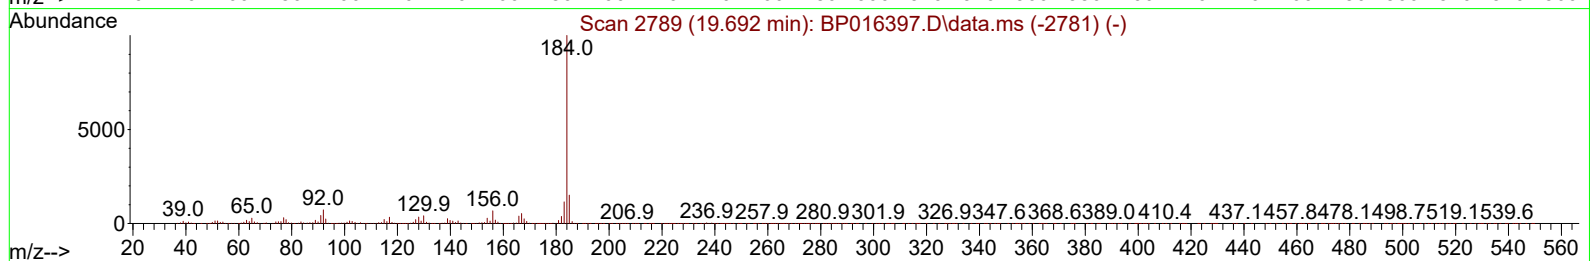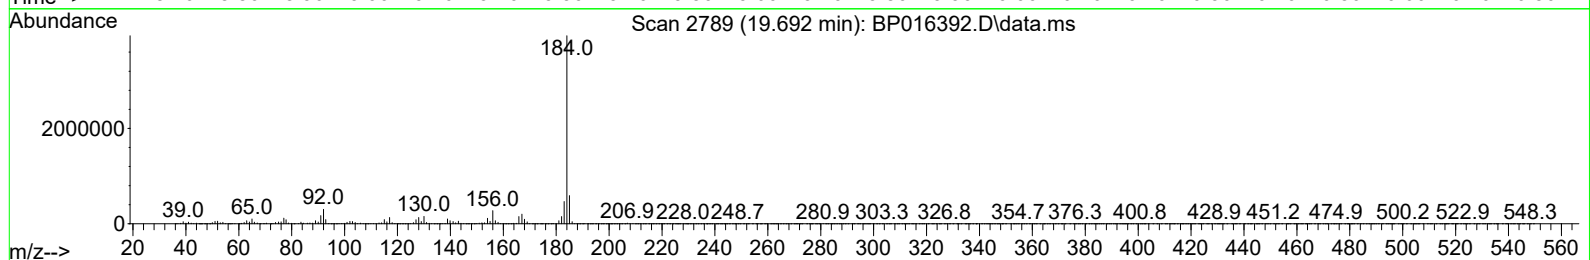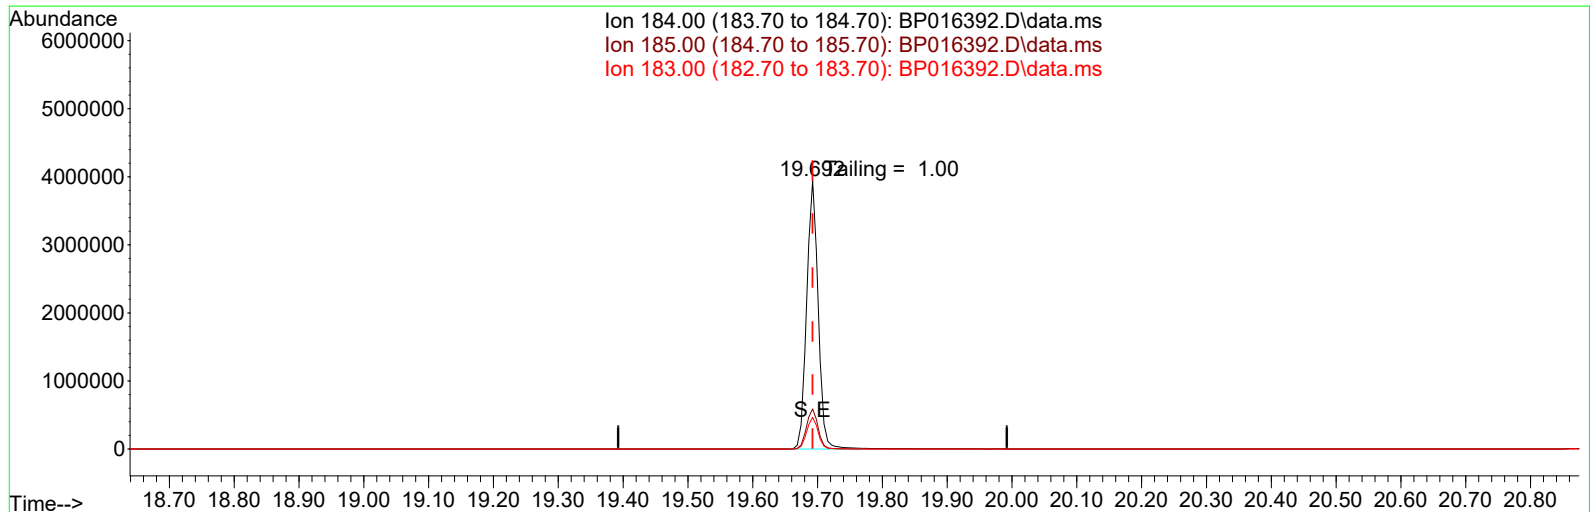

TIC: BP016392.D\data.ms

(77) Benzidine

19.692min (-0.000) 180967.88 ng

response 4885195

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.00	14.97
183.00	11.50	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/27/2023	BNA_P	<u>BP016392.D</u>
Compound Name	Response	Retention Time
DDT	2215988	20.869
DDD	25289	20.486
DDE	486	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
25775	2241763	1.15

Instrument :
BNA_P
ClientSampleId :
DFTPP