
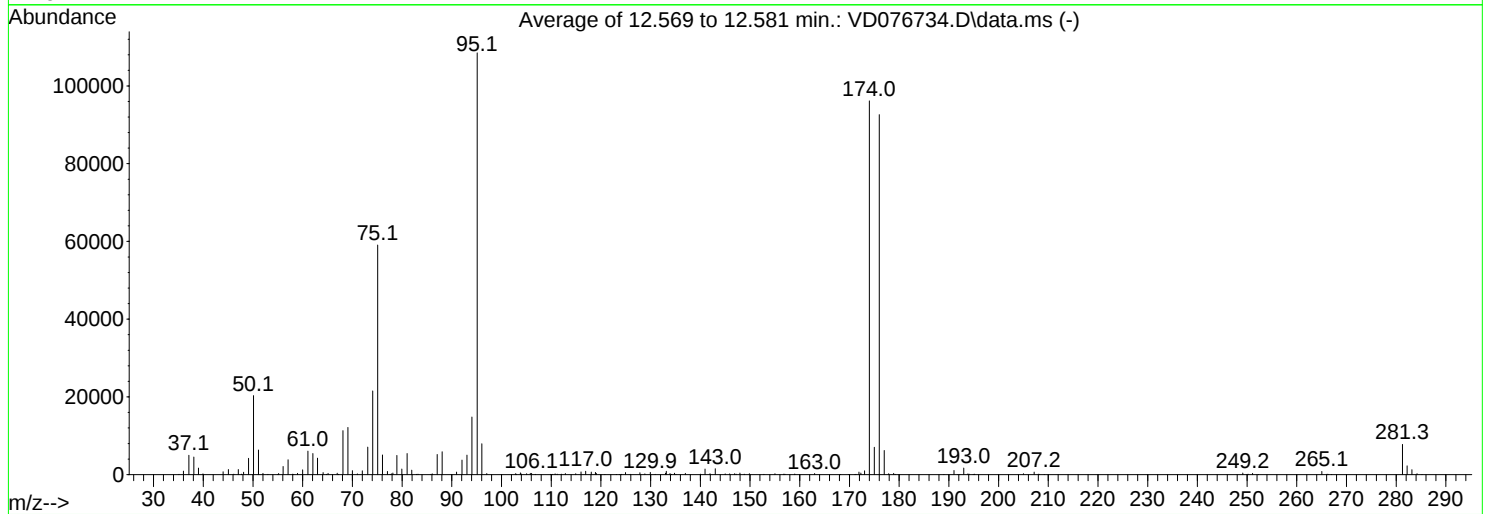


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD071423\
Data File : VD076734.D
Acq On : 14 Jul 2023 10:44
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D071423S.M
Title : SW846 8260
Last Update : Mon Jul 17 08:07:52 2023

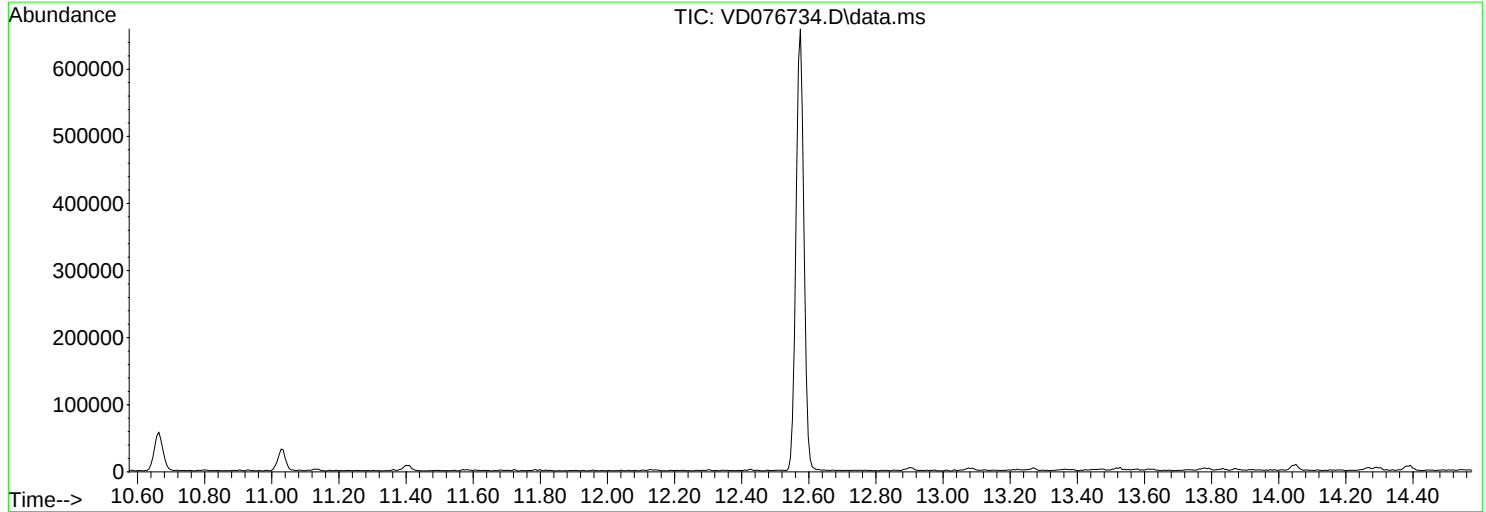

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	20332	PASS
75	95	30	60	54.4	59080	PASS
95	95	100	100	100.0	108512	PASS
96	95	5	9	7.3	7929	PASS
173	174	0.00	2	1.0	1000	PASS
174	95	50	100	88.6	96152	PASS
175	174	5	9	7.3	7052	PASS
176	174	95	101	96.3	92608	PASS
177	176	5	9	6.7	6208	PASS