



## Prep Standard - Chemical Standard Summary

**Order ID :** O4699

**Test :** EPH

**Prepbatch ID :** PB156102,

**Sequence ID/Qc Batch ID:** FC100523AL,

**Standard ID :**

EP2385,EP2394,PP21954,PP21955,PP21956,PP21957,PP21958,PP21959,PP21960,PP22391,PP22542,PP22543,

**Chemical ID :**

E3412,E3480,E3495,E3566,E3567,E3572,E3576,M5653,P11134,P11263,P11735,P11829,P12171,P12377,P12378,P12379,P12380,P12480,P12524,P12579,P12580,P12581,P12582,P12675,P12676,P12677,P12678,W2606,

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3319	6N HCL	<a href="#">EP2385</a>	09/05/2023	02/17/2024	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 09/05/2023

**FROM** 219.00000ml of M5653 + 781.00000ml of W2606 = Final Quantity: 1000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	<a href="#">EP2394</a>	10/03/2023	10/23/2023	RUPESHKUMAR SHAH	Extraction_SCALE_2 (EX-SC-2)	None	Rajesh Parikh 10/03/2023

**FROM** 1.00000gram of E3412 = Final Quantity: 4000.000 gram

**284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900**

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
781	100 PPM Aliphatic HC Working STD (Restek)	<a href="#">PP21954</a>	04/20/2023	10/19/2023	Yogesh Patel	None	None	Ankita Jodhani 04/24/2023
<b><u>FROM</u></b> 0.25000ml of P11735 + 0.25000ml of P12171 + 1.25000ml of P11829 + 23.25000ml of E3495 = Final Quantity: 25.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2900	100 PPM Aliphatic HC STD (Absolute)	<a href="#">PP21955</a>	04/20/2023	10/19/2023	Yogesh Patel	None	None	Ankita Jodhani 04/24/2023
<b><u>FROM</u></b> 0.25000ml of P11735 + 0.25000ml of P12171 + 2.50000ml of P11134 + 22.00000ml of E3495 = Final Quantity: 25.000 ml								

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
783	50 PPM Aliphatic HC STD	<a href="#">PP21956</a>	04/20/2023	10/19/2023	Yogesh Patel	None	None	Ankita Jodhani
04/24/2023								

**FROM** 0.50000ml of E3495 + 0.50000ml of PP21954 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
784	20 PPM Aliphatic HC STD	<a href="#">PP21957</a>	04/20/2023	10/19/2023	Yogesh Patel	None	None	Ankita Jodhani
04/24/2023								

**FROM** 0.80000ml of E3495 + 0.20000ml of PP21954 = Final Quantity: 1.000 ml

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
785	10 PPM Aliphatic HC STD	<a href="#">PP21958</a>	04/20/2023	10/19/2023	Yogesh Patel	None	None	Ankita Jodhani
04/24/2023								

**FROM** 0.90000ml of E3495 + 0.10000ml of PP21954 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
786	5 PPM Aliphatic HC STD	<a href="#">PP21959</a>	04/20/2023	10/19/2023	Yogesh Patel	None	None	Ankita Jodhani
04/24/2023								

**FROM** 0.90000ml of E3495 + 0.10000ml of PP21956 = Final Quantity: 1.000 ml

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2901	20 PPM Aliphatic HC STD ICV (Absolute)	<a href="#">PP21960</a>	04/20/2023	10/19/2023	Yogesh Patel	None	None	Ankita Jodhani
04/24/2023								

**FROM** 0.80000ml of E3495 + 0.20000ml of PP21955 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2589	20 PPM NJ EPH SPIKE for LOD-LOQ	<a href="#">PP22391</a>	07/24/2023	01/24/2024	Yogesh Patel	None	None	Ankita Jodhani
07/25/2023								

**FROM** 1.00000ml of P12480 + 1.00000ml of P12524 + 8.00000ml of P11263 = Final Quantity: 10.000 ml

**284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900**

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1331	100 PPM NJEPH Fractionating Surrogate	<a href="#">PP22542</a>	09/12/2023	03/09/2024	Yogesh Patel	None	None	Ankita Jodhani 09/13/2023
<p><b><u>FROM</u></b> 1.25000ml of P12675 + 1.25000ml of P12676 + 1.25000ml of P12677 + 1.25000ml of P12678 + 195.00000ml of E3567 = Final Quantity: 200.000 ml</p>								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1339	100 PPM NJEPH Surrogate Spike	<a href="#">PP22543</a>	09/13/2023	03/12/2024	Yogesh Patel	None	None	Ankita Jodhani 09/15/2023
<b><u>FROM</u></b> 1.25000ml of P12377 + 1.25000ml of P12378 + 1.25000ml of P12379 + 1.25000ml of P12380 + 1.25000ml of P12579 + 1.25000ml of P12580 + 1.25000ml of P12581 + 1.25000ml of P12582 + 490.00000ml of E3566 = Final Quantity: 500.000 ml								

**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	139404	04/10/2024	10/18/2022 / Rajesh	10/13/2022 / Rajesh	E3412

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
phenomenex	SI500025-30 / Cleanert SPE Silica, 5000 mg/25 ml	YO119-QJ	12/10/2023	05/11/2023 / Rajesh	02/24/2023 / Rajesh	E3480

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	23A2662017	12/09/2023	04/19/2023 / rajesh	04/13/2023 / Rajesh	E3495

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	22L2862006	03/12/2024	09/12/2023 / Rajesh	09/08/2023 / Rajesh	E3566

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	23C2462011	04/16/2024	09/09/2023 / Rajesh	09/08/2023 / Rajesh	E3567

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	23H2962015	03/25/2024	09/25/2023 / Rajesh	09/25/2023 / Rajesh	E3572



**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	23G1262009	03/28/2024	09/28/2023 / Rajesh	09/28/2023 / Rajesh	E3576

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9530-33 / Hydrochloric Acid, Instra-Analyzed (cs/6x2.5L)	22E1662006	02/17/2024	08/29/2023 / bin	04/11/2022 / Al-Terek	M5653

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	95899 / NJ EPH Aliphatic n-Hydrocarbons-Revised, 1000 PPM	09282109	10/20/2023	04/20/2023 / yogesh	10/29/2021 / Abdul	P11134

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	HP782 / Pentane, 1L	21080835	11/13/2024	12/16/2021 / Ankita	12/16/2021 / Ankita	P11263

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0183688	10/20/2023	04/20/2023 / yogesh	05/27/2022 / Sohil	P11735

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30540 / Custom NJEPH Aliphatics Calibration Standard	A0184811	10/20/2023	04/20/2023 / yogesh	06/17/2022 / Ankita	P11829

**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0183404	10/20/2023	04/20/2023 / yogesh	11/10/2022 / Yogesh	P12171

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0190428	03/13/2024	09/13/2023 / yogesh	03/16/2023 / Yogesh	P12377

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0190428	03/13/2024	09/13/2023 / yogesh	03/16/2023 / Yogesh	P12378

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0190428	03/13/2024	09/13/2023 / yogesh	03/16/2023 / Yogesh	P12379

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31098 / 1-Chlorooctadecane Standard	A0190428	03/13/2024	09/13/2023 / yogesh	03/16/2023 / Yogesh	P12380

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30542 / Custom NJEPH Aliphatics Matrix Spike Mix	A0195645	01/24/2024	07/24/2023 / yogesh	05/23/2023 / Yogesh	P12480

**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	30543 / Custom NJEPH Aromatics Matrix Spike Mix	A0195695	01/24/2024	07/24/2023 / yogesh	06/30/2023 / Yogesh	P12524

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0197729	03/13/2024	09/13/2023 / yogesh	06/30/2023 / Yogesh	P12579

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0197729	03/13/2024	09/13/2023 / yogesh	06/30/2023 / Yogesh	P12580

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0197729	03/13/2024	09/13/2023 / yogesh	06/30/2023 / Yogesh	P12581

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31097 / o-Terphenyl Standard	A0197729	03/13/2024	09/13/2023 / yogesh	06/30/2023 / Yogesh	P12582

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0196246	03/12/2024	09/12/2023 / yogesh	07/19/2023 / yogesh	P12675

**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0196246	03/12/2024	09/12/2023 / yogesh	07/19/2023 / yogesh	P12676

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0196246	03/12/2024	09/12/2023 / yogesh	07/19/2023 / yogesh	P12677

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31480 / MA Fractionation Surrogate Spike Mix	A0196246	03/12/2024	09/12/2023 / yogesh	07/19/2023 / yogesh	P12678

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	10/24/2024	10/24/2019 / apatel	10/24/2019 / apatel	W2606




**PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.**



MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MÉXICO  
CP 64070  
TEL +52 81 13 52 57 57  
www.pqm.com.mx

## CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na <sub>2</sub> SO <sub>4</sub>
SPECIFICATION NUMBER :	6399	RELEASE DATE:	OCT/28/2021
LOT NUMBER :	139404		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na <sub>2</sub> SO <sub>4</sub> )	Min. 99.0%	99.8 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.0
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO <sub>4</sub> )	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.002 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.2 %
Retained on US Standard No. 60 sieve	Min. 94%	97.6 %
Through US Standard No. 60 sieve	Max. 5%	2.1 %
Through US Standard No. 100 sieve	Max. 10%	0.2 %
COMMENTS		
 QC: PhC Irma Belmares		

If you need further details, please call our factory or contact our local distributor.

E 3412

Recd. by RP on 10/13/22

RE-02-01, Ed. 3

**Cleanert EPH**

5g/25ml 15/pkg

固相萃取产品

LOT#:Y0119-QJ

MFG#:F00137

Made in China



**CAT# SI500025-30**

Agela Technologies

E 3480



Material No.: 9262-03  
Batch No.: 23A2662017  
Manufactured Date: 2023-01-10  
Expiration Date: 2024-04-10  
Revision No.: 0

## Certificate of Analysis


Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	< 1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	< 1
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	≥ 99.5 %	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	97 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 4/13/23

E34951

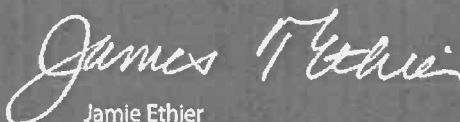  
Jamie Ethier  
Vice President Global Quality

Acetone

BAKER RESI-ANALYZED® Reagent

For Organic Residue Analysis



Material No.: 9254-03

Batch No.: 22L2862006

Manufactured Date: 2022-12-19

Expiration Date: 2025-12-18

Revision No.: 0

## Certificate of Analysis


Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	≤ 0.3	0.1
Titration Base (µeq/g)	≤ 0.6	< 0.1
Water (H <sub>2</sub> O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	4

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 9/8/23

E 3566

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1



Hexanes (95% n-hexane)  
BAKER RESI-ANALYZED® Reagent



Material No.: 9262-03  
Batch No.: 23C2462011  
Manufactured Date: 2023-03-10  
Expiration Date: 2024-06-08  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	$\leq 5$	< 1
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	97 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0$ ppm	0.3 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 9/8/23

E 3567

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 23H2962015  
Manufactured Date: 2023-08-08  
Expiration Date: 2024-11-06  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	7
Assay (CH <sub>2</sub> Cl <sub>2</sub> ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0$ ppm	0.1 ppm
Titration Acid ( $\mu$ eq/g)	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10$ ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC  
Manufacturer source batch: MG23H08469

E 3572

Ken Koehnlein  
Sr. Manager, Quality Assurance

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1

Material No.: 9262-03  
Batch No.: 23G1262009  
Manufactured Date: 2023-06-01  
Expiration Date: 2024-08-30  
Revision No.: 0

## Certificate of Analysis


Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	3
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	≥ 99.5 %	99.6 %
Assay (as n-Hexane) (by GC, corrected for water)	≥ 95 %	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	≤ 0.05 %	0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 9/28/23

E 3576



Ken Koehnlein  
Sr. Manager, Quality Assurance

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Hydrochloric Acid, 36.5–38.0%  
BAKER INSTRA–ANALYZED® Reagent  
For Trace Metal Analysis



M5651 M5652 M5653  
M5654 M5655 M5656

Material No.: 9530–33  
Batch No.: 22E1662006  
Manufactured Date: 2022–04–11  
Retest Date: 2027–04–10  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
ACS – Assay (as HCl) (by acid–base titrn)	36.5 – 38.0 %	37.6 %
ACS – Color (APHA)	≤ 10	5
ACS – Residue after Ignition	≤ 3 ppm	< 1 ppm
ACS – Specific Gravity at 60°/60°F	1.185 – 1.192	1.190
ACS – Bromide (Br)	≤ 0.005 %	< 0.005 %
ACS – Extractable Organic Substances	≤ 5 ppm	< 1 ppm
ACS – Free Chlorine (as Cl <sub>2</sub> )	≤ 0.5 ppm	< 0.5 ppm
Phosphate (PO <sub>4</sub> )	≤ 0.05 ppm	< 0.03 ppm
Sulfate (SO <sub>4</sub> )	≤ 0.5 ppm	< 0.3 ppm
Sulfite (SO <sub>3</sub> )	≤ 0.8 ppm	0.3 ppm
Ammonium (NH <sub>4</sub> )	≤ 3 ppm	< 1 ppm
Trace Impurities – Arsenic (As)	≤ 0.010 ppm	< 0.003 ppm
Trace Impurities – Aluminum (Al)	≤ 10.0 ppb	< 0.2 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 3.0 ppb
Trace Impurities – Barium (Ba)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Beryllium (Be)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Bismuth (Bi)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Boron (B)	≤ 20.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 1.0 ppb	< 0.3 ppb
Trace Impurities – Calcium (Ca)	≤ 50.0 ppb	37.0 ppb
Trace Impurities – Chromium (Cr)	≤ 1.0 ppb	< 0.4 ppb
Trace Impurities – Cobalt (Co)	≤ 1.0 ppb	< 0.3 ppb
Trace Impurities – Copper (Cu)	≤ 1.0 ppb	< 0.1 ppb
Trace Impurities – Gallium (Ga)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Germanium (Ge)	≤ 3.0 ppb	< 2.0 ppb
Trace Impurities – Gold (Au)	≤ 4.0 ppb	0.2 ppb
Heavy Metals (as Pb)	≤ 100 ppb	< 50 ppb
Trace Impurities – Iron (Fe)	≤ 15 ppb	1 ppb

>>> Continued on page 2 >>>

Hydrochloric Acid, 36.5–38.0%  
BAKER INSTRA–ANALYZED® Reagent  
For Trace Metal Analysis



Material No.: 9530–33  
Batch No.: 22E1662006

Test	Specification	Result
Trace Impurities – Lead (Pb)	≤ 1.0 ppb	< 0.5 ppb
Trace Impurities – Lithium (Li)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Magnesium (Mg)	≤ 10.0 ppb	1.0 ppb
Trace Impurities – Manganese (Mn)	≤ 1.0 ppb	< 0.4 ppb
Trace Impurities – Mercury (Hg)	≤ 0.5 ppb	0.1 ppb
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 3.0 ppb
Trace Impurities – Nickel (Ni)	≤ 4.0 ppb	< 0.3 ppb
Trace Impurities – Niobium (Nb)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Potassium (K)	≤ 9.0 ppb	< 2.0 ppb
Trace Impurities – Selenium (Se), For Information Only		1.0 ppb
Trace Impurities – Silicon (Si)	≤ 100.0 ppb	< 0.4 ppb
Trace Impurities – Silver (Ag)	≤ 1.0 ppb	< 0.3 ppb
Trace Impurities – Sodium (Na)	≤ 100.0 ppb	1.9 ppb
Trace Impurities – Strontium (Sr)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Tantalum (Ta)	≤ 1.0 ppb	< 0.9 ppb
Trace Impurities – Thallium (Tl)	≤ 5.0 ppb	< 2.0 ppb
Trace Impurities – Tin (Sn)	≤ 5.0 ppb	< 0.8 ppb
Trace Impurities – Titanium (Ti)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Vanadium (V)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Zinc (Zn)	≤ 5.0 ppb	< 0.3 ppb
Trace Impurities – Zirconium (Zr)	≤ 1.0 ppb	< 0.1 ppb

>>> Continued on page 3 >>>

Hydrochloric Acid, 36.5–38.0%  
BAKER INSTRA–ANALYZED® Reagent  
For Trace Metal Analysis



Material No.: 9530–33  
Batch No.: 22E1662006

Test	Specification	Result
------	---------------	--------

For Laboratory, Research, or Manufacturing Use  
Product Information (not specifications):  
Appearance (clear, fuming liquid)  
Meets ACS Specifications  
Storage Condition: Store below 25 °C.

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700



**Certified Reference Material CRM**



**CERTIFIED WEIGHT REPORT**

Part Number: **95899**

Lot Number: **092821**

Description: **NJ EPH Aliphatic n-Hydrocarbons - Revised**

20 components

Expiration Date: **092831**

Recommended Storage: **Ambient (20 °C)**

Nominal Concentration (µg/mL): **1000**

NIST Test ID#: **8LUTB**

SE-05 Balance Uncertainty  
0.005 Peak Uncertainty

Weight(s) shown below were combined and diluted to (mL): **25.0**  
**CAUTION: Sonicate Before Use**

Solvent(s): **Cyclohexane**  
Lot# **28930**

Formulated By: <i>[Signature]</i>	Benson Chan	092821
Reviewed By: <i>[Signature]</i>	Pedro L. Renterias	092821
		DATE

Compound	(R#)	Lot Number	DIL Factor	Initial Vol (mL)	Initial Conc (µg/mL)	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty	Uncertainty Pipette	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	SDS Information		LD50
															(Solvent Safety Info. On Attached pg.)		
1. 2-Methylnaphthalene	(0214)	MKB3783V	NA	NA	NA	1000	97	0.2	NA	0.02577	0.02581	1001.6	5.7	91-57-6	N/A	or:at 1650mg/kg	
2. Naphthalene	(0222)	MKB28680V	NA	NA	NA	1000	100	0.2	NA	0.02500	0.02506	1002.6	5.7	91-20-3	10 ppm (50mg/mL)	or:at 490mg/kg	
3. n-Nonane	95708	081621	1.00	25.00	1000.8	1000	NA	0.013	NA	NA	NA	1000.9	4.2	111-84-2	200 ppm (1050mg/mL)	or:at 216mg/kg	
4. n-Decane	95708	081621	1.00	25.00	1000.9	1000	NA	0.013	NA	NA	NA	1001.1	4.2	124-18-5	N/A	N/A	
5. n-Dodecane	95708	081621	1.00	25.00	1001.2	1000	NA	0.013	NA	NA	NA	1001.3	4.2	112-40-3	N/A	N/A	
6. n-Tetradecane	95708	081621	1.00	25.00	1002.0	1000	NA	0.013	NA	NA	NA	1002.2	4.2	629-59-4	N/A	N/A	
7. n-Hexadecane	95708	081621	1.00	25.00	1001.9	1000	NA	0.013	NA	NA	NA	1002.0	4.2	544-76-3	N/A	N/A	
8. n-Octadecane	95708	081621	1.00	25.00	1011.8	1000	NA	0.013	NA	NA	NA	1012.0	4.2	583-45-3	N/A	N/A	
9. n-Eicosane	95708	081621	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	1000.7	4.2	112-95-8	N/A	N/A	
10. n-Heneicosane	95708	081621	1.00	25.00	1001.2	1000	NA	0.013	NA	NA	NA	1001.4	4.2	629-94-7	N/A	N/A	
11. n-Docosane	95708	081621	1.00	25.00	1001.6	1000	NA	0.013	NA	NA	NA	1001.7	4.2	629-97-0	N/A	N/A	
12. n-Tetracosane	95708	081621	1.00	25.00	1001.3	1000	NA	0.013	NA	NA	NA	1001.4	4.2	646-31-1	N/A	N/A	
13. n-Hexacosane	95708	081621	1.00	25.00	1000.4	1000	NA	0.013	NA	NA	NA	1000.5	4.2	630-01-3	N/A	N/A	
14. n-Octacosane	95708	081621	1.00	25.00	1001.7	1000	NA	0.013	NA	NA	NA	1001.2	4.2	638-68-6	N/A	N/A	
15. n-Triacontane	95708	081621	1.00	25.00	1001.0	1000	NA	0.013	NA	NA	NA	1000.9	4.2	544-85-4	N/A	N/A	
16. n-Dotriacontane	95708	081621	1.00	25.00	1000.7	1000	NA	0.013	NA	NA	NA	1000.9	4.2	14167-59-0	N/A	N/A	
17. n-Tetracontane	95708	081621	1.00	25.00	1000.8	1000	NA	0.013	NA	NA	NA	1000.9	4.2	630-06-8	N/A	N/A	
18. n-Hexatriacontane	95708	081621	1.00	25.00	1000.9	1000	NA	0.013	NA	NA	NA	1001.1	4.2	7194-95-6	N/A	N/A	
19. n-Octatriacontane	95708	081621	1.00	25.00	1000.8	1000	NA	0.013	NA	NA	NA	1000.6	4.3	4181-95-7	N/A	N/A	
20. n-Tetracontane	95708	081621	1.00	25.00	1000.5	1000	NA	0.013	NA	NA	NA	1000.6	4.3			N/A	


\* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
\* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
\* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.  
\* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
\* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

P 111132  
P 111136  
11/11/21



Method GC8HOT.M: Column: SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 320°C (20 min.), Rate = 30°C/min., Injector B = 250°C, Detector B = 300°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by Melissa Stonier.

TIC: 95899.D

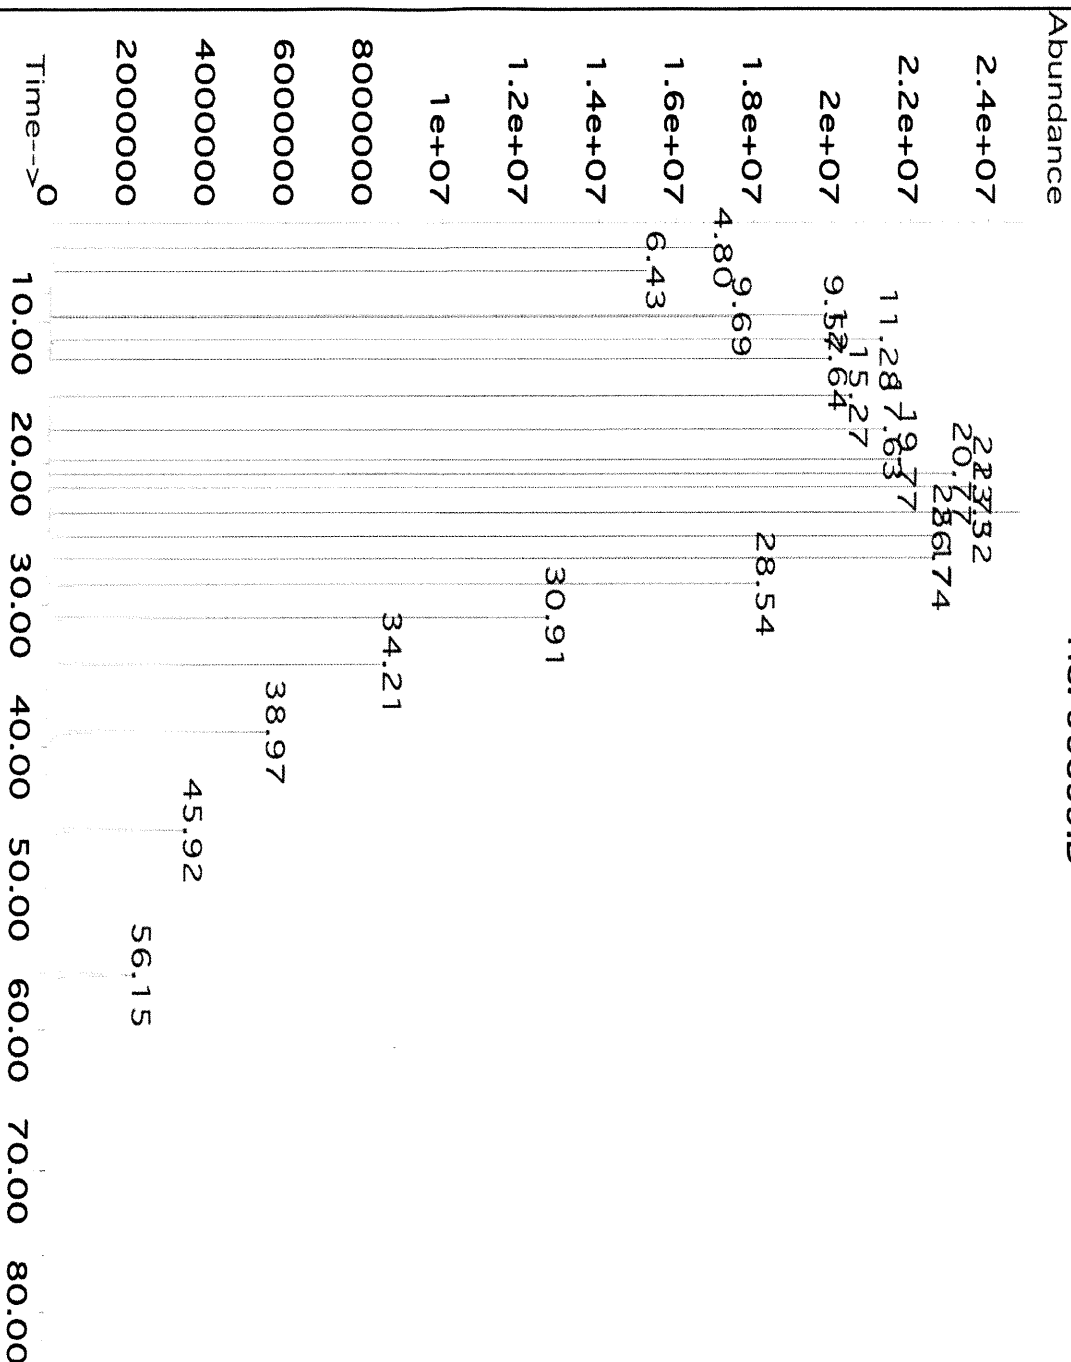





# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis

P11719 to P11738

Received by SJ : 5/27/2022



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31097 **Lot No.:** A0183688  
**Description :** o-Terphenyl Standard  
o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** November 30, 2025 **Storage:** 10°C or colder  
**Handling:** Sonicate prior to use. **Ship:** Ambient

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	o-Terphenyl CAS # 84-15-1 Purity 99% (Lot MKCH4487)	10,006.9 µg/mL	+/- 58.1808 µg/mL Gravimetric +/- 450.7156 µg/mL Unstressed +/- 500.1247 µg/mL Stressed

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**


330°C

**Det. Type:**

FID

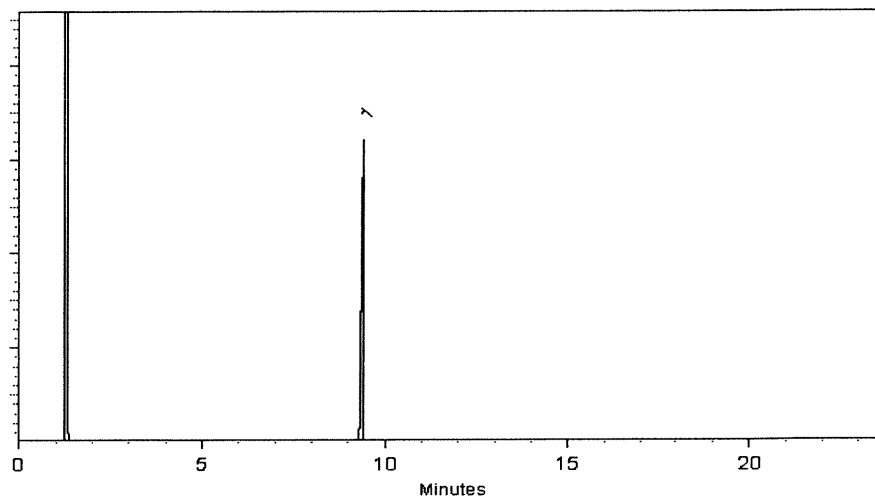


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
**Nick Yaw - Operations Tech I**

**Date Mixed:** 05-Apr-2022

**Balance:** 1128360905

  
**Clara Windle - Operations Technician I**

**Date Passed:** 07-Apr-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.




1110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No.: 30540 Lot No.: A0184811

Description: NJEPH Aliphatics Calibration Standard

Aliphatics Calibration Standard 2000µg/mL, Hexane/Carbon Disulfide (80:20), 1mL/ampul

Container Size: 2 mL Pkg Amt: > 1 mL

Expiration Date: June 30, 2029 Storage: 25°C nominal

Handling: Sonicate prior to use. Ship: Ambient

p11827  
AJ  
06/14/22  
p11831

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	n-Nonane (C9) CAS # 111-84-2 Purity 99%	2,015.3 µg/mL (Lot SHBN5361)	+/- 11.8271 µg/mL Gravimetric +/- 50.0358 µg/mL Unstressed +/- 59.9888 µg/mL Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99%	2,010.7 µg/mL (Lot SHBN8619)	+/- 11.7997 µg/mL Gravimetric +/- 49.9200 µg/mL Unstressed +/- 59.8498 µg/mL Stressed
3	Naphthalene CAS # 91-20-3 Purity 99%	2,013.3 µg/mL (Lot MKCH0219)	+/- 11.8154 µg/mL Gravimetric +/- 49.9862 µg/mL Unstressed +/- 59.9292 µg/mL Stressed
4	n-Dodecane (C12) CAS # 112-40-3 Purity 99%	2,007.3 µg/mL (Lot SHBK0925)	+/- 11.7802 µg/mL Gravimetric +/- 49.8372 µg/mL Unstressed +/- 59.7506 µg/mL Stressed
5	2-Methylnaphthalene CAS # 91-57-6 Purity 96%	2,010.2 µg/mL (Lot STBK0259)	+/- 11.7972 µg/mL Gravimetric +/- 49.9094 µg/mL Unstressed +/- 59.8371 µg/mL Stressed
6	n-Tetradecane (C14) CAS # 629-59-4 Purity 99%	2,010.0 µg/mL (Lot STBK2282)	+/- 11.7958 µg/mL Gravimetric +/- 49.9034 µg/mL Unstressed +/- 59.8300 µg/mL Stressed
7	n-Hexadecane (C16) CAS # 544-76-3 Purity 98%	2,012.9 µg/mL (Lot SHBM4146)	+/- 11.8129 µg/mL Gravimetric +/- 49.9759 µg/mL Unstressed +/- 59.9169 µg/mL Stressed

8	n-Octadecane (C18) CAS # 593-45-3 Purity 98%	(Lot UE5NG)	2,019.5 µg/mL	+/- 11.8513 +/- 50.1381 +/- 60.1114	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Eicosane (C20) CAS # 112-95-8 Purity 99%	(Lot MKCF7888)	2,008.7 µg/mL	+/- 11.7880 +/- 49.8703 +/- 59.7903	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Heneicosane (C21) CAS # 629-94-7 Purity 99%	(Lot MKCL3226)	2,015.3 µg/mL	+/- 11.8271 +/- 50.0358 +/- 59.9888	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Docosane (C22) CAS # 629-97-0 Purity 99%	(Lot MKCL8918)	2,012.7 µg/mL	+/- 11.8115 +/- 49.9696 +/- 59.9094	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Tetracosane (C24) CAS # 646-31-1 Purity 99%	(Lot MKCN2863)	2,018.0 µg/mL	+/- 11.8428 +/- 50.1020 +/- 60.0681	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Hexacosane (C26) CAS # 630-01-3 Purity 99%	(Lot MKCD4540)	2,009.3 µg/mL	+/- 11.7919 +/- 49.8869 +/- 59.8102	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Octacosane (C28) CAS # 630-02-4 Purity 99%	(Lot BCCG0084)	2,020.0 µg/mL	+/- 11.8545 +/- 50.1517 +/- 60.1277	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Triacontane (C30) CAS # 638-68-6 Purity 99%	(Lot MKCN9321)	2,018.7 µg/mL	+/- 11.8467 +/- 50.1186 +/- 60.0880	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Dotriacontane (C32) CAS # 544-85-4 Purity 99%	(Lot BCBW0661)	2,017.3 µg/mL	+/- 11.8388 +/- 50.0855 +/- 60.0483	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetatriacontane (C34) CAS # 14167-59-0 Purity 99%	(Lot OML4N)	2,014.0 µg/mL	+/- 11.8193 +/- 50.0027 +/- 59.9491	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
18	n-Hexatriacontane (C36) CAS # 630-06-8 Purity 99%	(Lot U25B014)	2,019.3 µg/mL	+/- 11.8506 +/- 50.1351 +/- 60.1078	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
19	n-Octatriacontane (C38) CAS # 7194-85-6 Purity 97%	(Lot 0000127235)	2,017.0 µg/mL	+/- 11.8366 +/- 50.0761 +/- 60.0370	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
20	n-Tetracontane (C40) CAS # 4181-95-7 Purity 98%	(Lot PADGI)	2,014.2 µg/mL	+/- 11.8206 +/- 50.0084 +/- 59.9558	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed

**Solvent:** Hexane/Carbon disulfide (80:20)

CAS # 110-54-3/75-15-0  
Purity 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

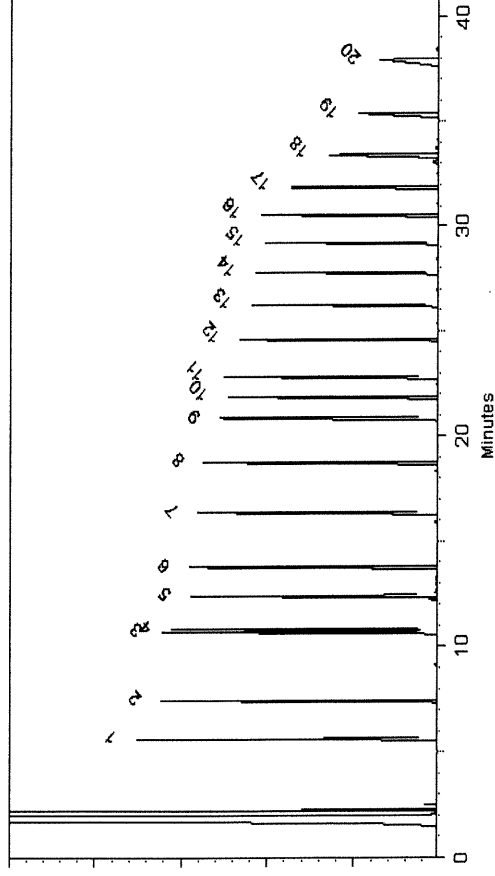

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Brittany Federinko - Operations Tech I

**Date Mixed:** 03-May-2022 **Balance:** 11.28360905

Christie Mills - Operations Technician II

**Date Passed:** 06-May-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No.: 31098 Lot No.: A0190428

Description: 1-Chlorooctadecane Standard  
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride,  
1mL/ampul

Container Size: 2 mL Pkg Amt: > 1 mL

Expiration Date: November 30, 2029 Storage: 10°C or colder  
Ship: Ambient

P12371 } 7.0  
          } 03/16/23  
P12385 }

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L., $k=2$ )
1	1-Chlorooctadecane CAS # 3386-33-2 Purity 99%	10,066.3 µg/mL (Lot 13661500)	+/- 58.5260 µg/mL +/- 564.4046 µg/mL +/- 577.6110 µg/mL

Solvent: Methylene chloride  
CAS # 75-09-2  
Purity 99%

Gravimetric  
Unstressed  
Stressed



**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

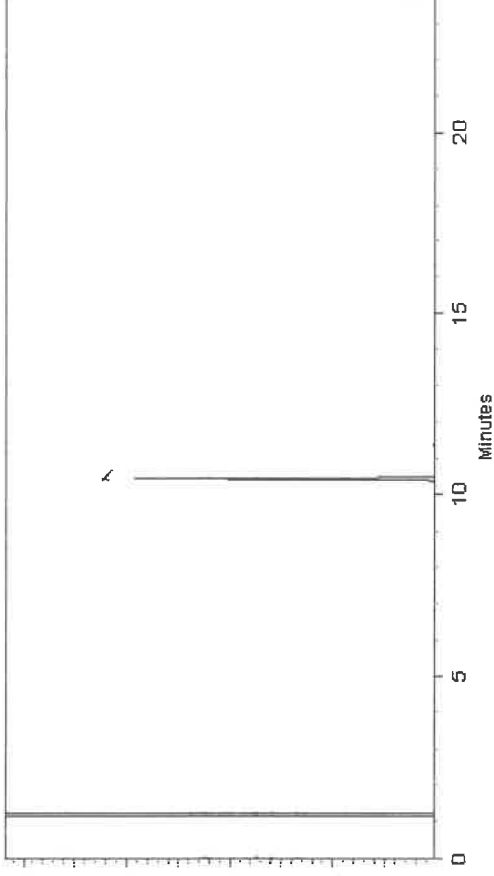

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Malina Homan - Operations Technician I

Date Mixed: 10-Oct-2022 Balance: B442140311

Christie Mills - Operations Tech II - ARM QC

Date Passed: 13-Oct-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.






110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No.: 31098 Lot No.: A0190428

Description: 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride,  
1mL/ampul

Container Size: 2 mL Pkg Amt: > 1 mL

Expiration Date: November 30, 2029 Storage: 10°C or colder

Ship: Ambient

P12371 } 7.0  
          } 03/16/23  
P12385 }

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L., $k=2$ )
1	1-Chlorooctadecane CAS # 3386-33-2 Purity 99%	10,066.3 µg/mL (Lot 13661500)	+/- 58.5260 µg/mL +/- 564.4046 µg/mL +/- 577.6110 µg/mL

Solvent: Methylene chloride  
CAS # 75-09-2  
Purity 99%

Gravimetric  
Unstressed  
Stressed

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

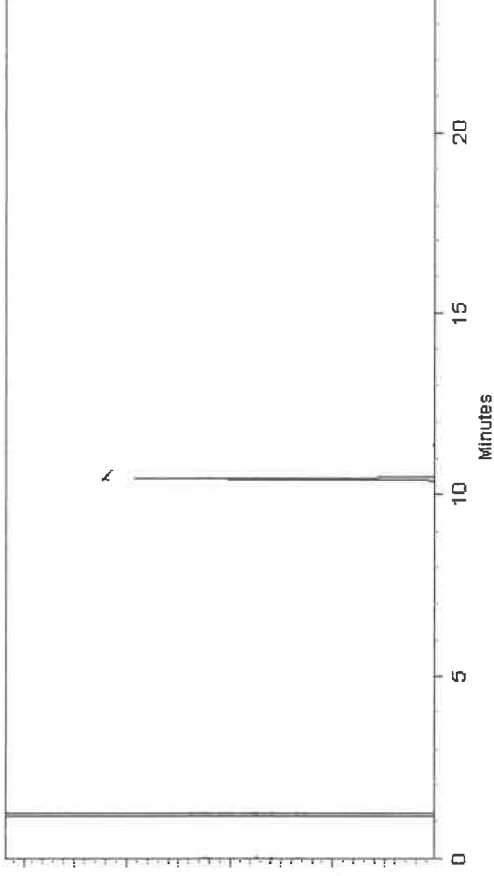

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Malina Homan - Operations Technician I

Date Mixed: 10-Oct-2022 Balance: B442140311

Christie Mills - Operations Tech II - ARM QC

Date Passed: 13-Oct-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.






110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No.: 31098 Lot No.: A0190428

Description: 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride,  
1mL/ampul

Container Size: 2 mL Pkg Amt: > 1 mL

Expiration Date: November 30, 2029 Storage: 10°C or colder

Ship: Ambient

P12371 } 7.0  
          } 03/16/23  
P12385 }

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L., $k=2$ )
1	1-Chlorooctadecane CAS # 3386-33-2 Purity 99%	10,066.3 µg/mL (Lot 13661500)	+/- 58.5260 µg/mL +/- 564.4046 µg/mL +/- 577.6110 µg/mL

Solvent: Methylene chloride  
CAS # 75-09-2  
Purity 99%

Gravimetric  
Unstressed  
Stressed



**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

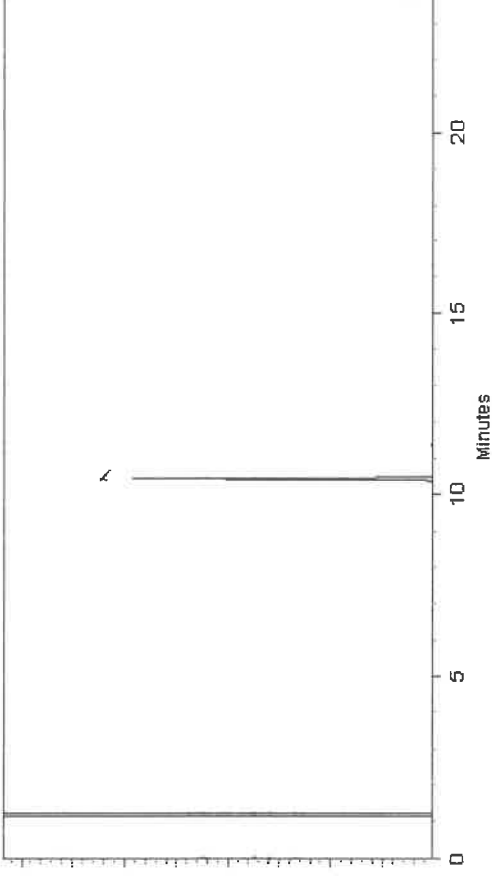

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Malina Homan - Operations Technician I

Date Mixed: 10-Oct-2022 Balance: B442140311

Christie Mills - Operations Tech II - ARM QC

Date Passed: 13-Oct-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

[www.restek.com](http://www.restek.com)

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No.: 31098 Lot No.: A0190428

Description: 1-Chlorooctadecane Standard  
1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride,  
1mL/ampul

Container Size: 2 mL Pkg Amt: > 1 mL

Expiration Date: November 30, 2029 Storage: 10°C or colder  
Ship: Ambient

P12371 } 7.0  
↓ } 03/16/23  
P12385 }

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L., $k=2$ )
1	1-Chlorooctadecane CAS # 3386-33-2 Purity 99%	10,066.3 µg/mL (Lot 13661500)	+/- 58.5260 µg/mL +/- 564.4046 µg/mL +/- 577.6110 µg/mL

Solvent: Methylene chloride  
CAS # 75-09-2  
Purity 99%

Gravimetric  
Unstressed  
Stressed

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

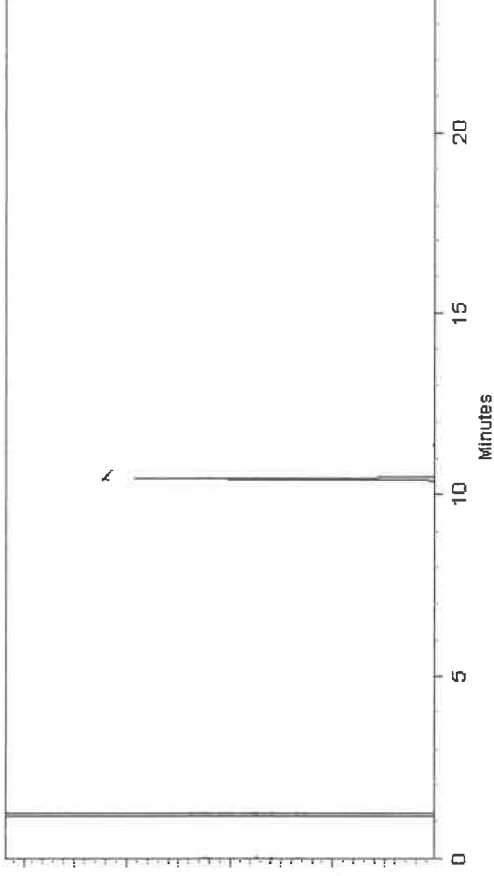

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Malina Homan - Operations Technician I

Date Mixed: 10-Oct-2022 Balance: B442140311

Christie Mills - Operations Tech II - ARM QC

Date Passed: 13-Oct-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.






## CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No.: 30542

Lot No.: A0195645

Description: NIEPH Aliphatics Matrix Spike Mix

NIEPH Aliphatics Matrix Spike Mix 200 µg/mL, n-Pentane, 5mL/ampul

Container Size: 5 mL

Pkg Amt: > 5 mL

Expiration Date: April 30, 2030

Storage: 10°C or colder

Handling: Sonicate prior to use.

Ship: Ambient

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Nonane (C <sub>9</sub> )	111-84-2	SHBN5361	99%	202.0 µg/mL	+/- 5.2184
2	n-Decane (C <sub>10</sub> )	124-18-5	SHBN8619	99%	201.3 µg/mL	+/- 5.2012
3	n-Dodecane (C <sub>12</sub> )	112-40-3	SHBP7054	99%	202.0 µg/mL	+/- 5.2184
4	n-Tetradecane (C <sub>14</sub> )	629-59-4	STBK5437	99%	201.7 µg/mL	+/- 5.2098
5	n-Hexadecane (C <sub>16</sub> )	544-76-3	SHBQ0897	99%	201.3 µg/mL	+/- 5.2012
6	n-Octadecane (C <sub>18</sub> )	593-45-3	UESNG	98%	201.6 µg/mL	+/- 5.2068
7	n-Eicosane (C <sub>20</sub> )	112-95-8	MKCN8767	97%	200.8 µg/mL	+/- 5.1871
8	n-Heneicosane (C <sub>21</sub> )	629-94-7	MKCL3226	99%	201.0 µg/mL	+/- 5.1926
9	n-Docosane (C <sub>22</sub> )	629-97-0	MKCL8918	99%	200.7 µg/mL	+/- 5.1839
10	n-Tetracosane (C <sub>24</sub> )	646-31-1	MKCQ8345	99%	201.3 µg/mL	+/- 5.2012
11	n-Hexacosane (C <sub>26</sub> )	630-01-3	MKCD4540	99%	201.0 µg/mL	+/- 5.1926
12	n-Octacosane (C <sub>28</sub> )	630-02-4	BCBS1577V	99%	201.7 µg/mL	+/- 5.2098
13	n-Triacontane (C <sub>30</sub> )	638-68-6	MKCQ9436	97%	200.8 µg/mL	+/- 5.1871
14	n-Dotriacontane (C <sub>32</sub> )	544-85-4	BCBW0661	99%	200.3 µg/mL	+/- 5.1753
15	n-Tetracontane (C <sub>34</sub> )	14167-59-0	D3MZN	99%	200.3 µg/mL	+/- 5.1753
16	n-Hexatriacontane (C <sub>36</sub> )	630-06-8	Z27H018	99%	200.3 µg/mL	+/- 5.1753
17	n-Octatriacontane (C <sub>38</sub> )	7194-85-6	0000145137	96%	201.6 µg/mL	+/- 5.2081




18	n-Tetracontane (C40)	4181-95-7	BSBME	99%	201.3	µg/mL	+/- 5.2012
----	----------------------	-----------	-------	-----	-------	-------	------------

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** n-Pentane  
**CAS #** 109-66-0  
**Purity** 99%

## Quality Confirmation Test

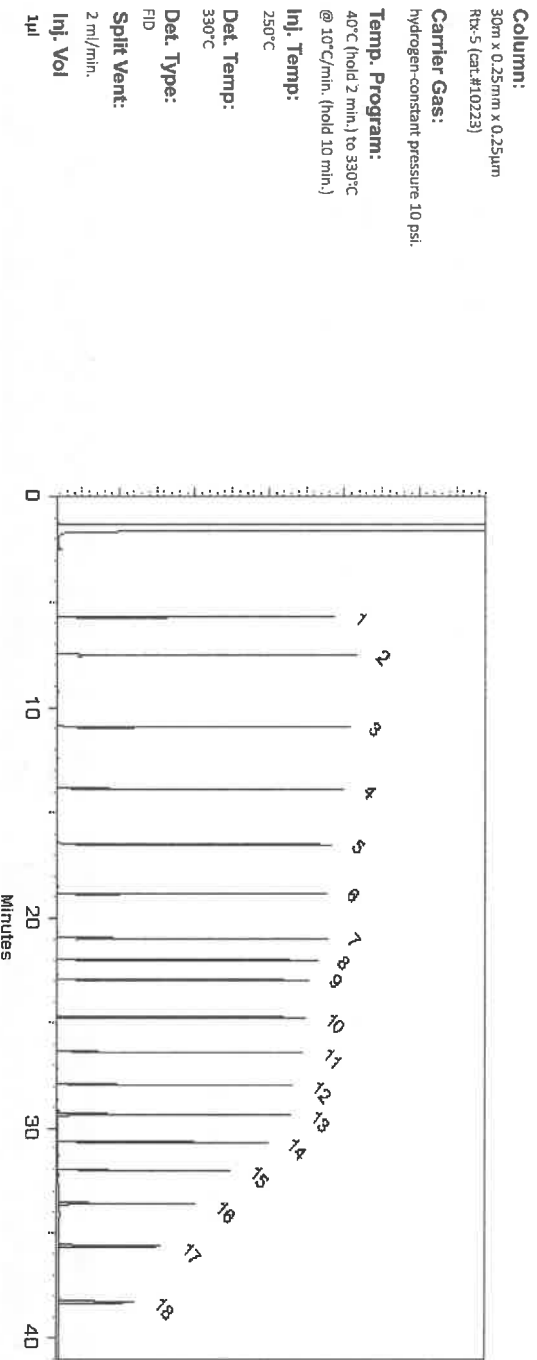

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*[Signature]*  
Morgan Craighhead - Mtx Technician

**Date Mixed:** 08-Mar-2023

**Balance Serial #** B442140311

*[Signature]*  
Fang-Yun Wenner - Operations Lead Tech - ARN QC

**Date Passed:** 10-Mar-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FIM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2 mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.






110 Benner Circle  
Belleville, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*

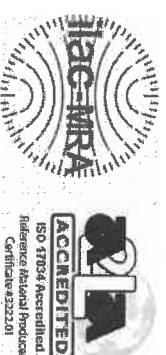

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 30543

Lot No.: A0195695

Description : NJEPH Aromatics Matrix Spike Mix

NJEPH Aromatics Matrix Spike Mix 200µg/mL, Acetone/Toluene (50:50), 5mL/ampul

Container Size : 5 mL

Pkg Amt: > 5 mL

Expiration Date : February 28, 2029

Storage: 10°C or colder

Handling: Sonication required. Mix is

photosensitive.

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	1,2,3-Trimethylbenzene	526-73-8	8776.10-36	98%	200.7 µg/mL	+/- 9.0431
2	Naphthalene	91-20-3	MKCH0219	99%	200.8 µg/mL	+/- 9.0474
3	2-Methylnaphthalene	91-57-6	STBK0259	96%	200.1 µg/mL	+/- 9.0143
4	Acenaphthylene	208-96-8	L10L	95%	199.9 µg/mL	+/- 9.0060
5	Acenaphthene	83-32-9	MKCR7169	99%	200.0 µg/mL	+/- 9.0114
6	Fluorene	86-73-7	10236068	99%	201.2 µg/mL	+/- 9.0655
7	Phenanthrene	85-01-8	MKCQ2033	99%	200.4 µg/mL	+/- 9.0294
8	Anthracene	120-12-7	MKCP3968	99%	200.0 µg/mL	+/- 9.0114
9	Fluoranthene	206-44-0	MKCF7378	99%	200.0 µg/mL	+/- 9.0114
10	Pyrene	129-00-0	BCCG7845	99%	200.4 µg/mL	+/- 9.0294
11	Benz(a)anthracene	56-55-3	RP230103RSRA	97%	200.1 µg/mL	+/- 9.0173
12	Chrysene	218-01-9	468677R16R	99%	200.8 µg/mL	+/- 9.0474
13	Benzo(b)fluoranthene	205-99-2	012013B	99%	200.7 µg/mL	+/- 9.0420
14	Benzo(k)fluoranthene	207-08-9	012022K	99%	200.8 µg/mL	+/- 9.0474
15	Benzo(a)pyrene	50-32-8	J6LUE-00	99%	200.8 µg/mL	+/- 9.0474
16	Indeno(1,2,3-cd)pyrene	193-39-5	12-JKL-118-9	99%	201.6 µg/mL	+/- 9.0835

P12516 } 7.8.  
P12535 } 06/30/23


17	Dibenz(a,h)anthracene	53-70-3	ER032211-01	99%	201.2	µg/mL	+/- 9.0655
18	Benzo(g,h,i)perylene	191-24-2	PMEVE	98%	200.1	µg/mL	+/- 9.0149

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Acetone/Toluene (50:50)  
**CAS #** 67-64-1/108-88-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)  
**Carrier Gas:**  
hydrogen-constant pressure 10 psi.  
**Temp. Program:**  
100°C (hold 1 min.) to 330°C  
@ 4°C/min. (hold 5 min.)  
**Inj. Temp:**  
250°C  
**Det. Temp:**  
330°C  
**Det. Type:**  
FID  
**Split Vent:**  
20 ml/min.  
**Inj. Vol**  
1µl

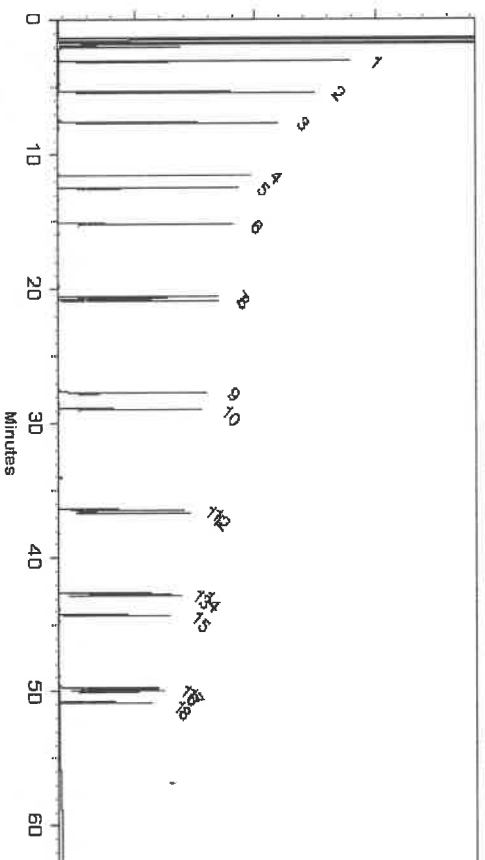

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Morgan Craighead - Mix Technician

Date Mixed: 09-Mar-2023

Balance Serial # 1128360905

Marina Cowan - Operations Tech II ARM QC

Date Passed: 15-Mar-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FIM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





## CERTIFIED REFERENCE MATERIAL



ISO 17025 Accredited  
Reference Material Producer  
Certificate # 2322301



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## Certificate of Analysis

*chromatographic plus*



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate # 1322202

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31097

Lot No.: A0197729

Description : o-Terphenyl Standard

o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : December 31, 2026

Storage: 10°C or colder

Handling: Sonicate prior to use.

Ship: Ambient

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.I., K=2)
1	o-Terphenyl	84-15-1	MKCH4487	99%	10,007.5 µg/mL	+/- 450.7438

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride

CAS # 75-09-2

Purity 99%

11574  
2  
9.18  
0125955  
06130



## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
10 ml/min.

**Inj. Vol**  
1µl

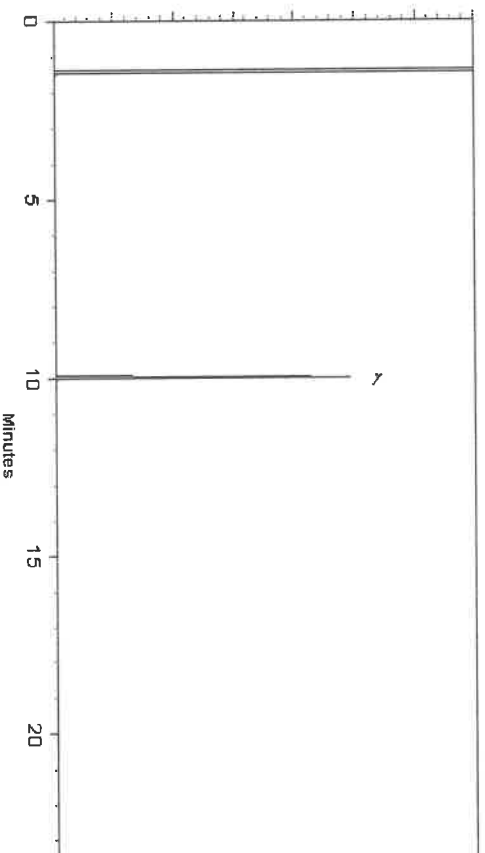

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*[Signature]*  
**Alicia Leathers - Operation Technician I**  
*[Signature]*  
**Jennifer Pollino - Operations Tech III - RRM QC**

**Date Mixed:** 03-May-2023  
**Balance Serial #** 1128360905  
**Date Passed:** 08-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FIM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





## Safety Data Sheet

Revision Date: 05/04/23

[www.restek.com](http://www.restek.com)

2 Letter ISO country code/language code: US/EN

### 1. IDENTIFICATION

Catalog Number / Product Name:	31097 / o-Terphenyl Standard
Company:	Restek Corporation
Address:	110 Benner Circle Bellefonte, Pa. 16823
Phone#:	814-353-1300
Fax#:	814-353-1309
Emergency#:	800-424-9300 (CHEMTREC) 703-527-3887 (Outside the US)
Email:	<a href="http://www.restek.com">www.restek.com</a>
Revision Number:	15
Intended use:	For Laboratory use only. This chemical/product is not and cannot be distributed in commerce (as defined in TSCA section 3(5)) or processed (as defined in TSCA section 3(13)) for consumer paint or coating removal.

### 2. HAZARD(S) IDENTIFICATION

#### Emergency Overview:

GHS Hazard  
Symbols:



GHS  
Classification: Carcinogenicity Category 2

GHS Signal  
Word: Warning

GHS Hazard:  
Suspected of causing cancer.

GHS  
Precautions:

Safety  
Precautions: Obtain special instructions before use.  
Do not handle until all safety precautions have been read and understood.  
Wear protective gloves/protective clothing/eye protection/face protection.

First Aid  
Measures: If exposed or concerned: Get medical advice/attention.

Storage: Store locked up.

Disposal: Dispose of contents/container according to section 13 of the SDS.

Single  
Exposure  
Target Organs: No data available

Repeated  
Exposure  
Target Organs: No data available

### 3. COMPOSITION / INFORMATION ON INGREDIENT

Chemical Name	CAS #	INEC #	% Composition
Methylene chloride (dichloromethane)	75-09-2	200-838-9	99
o-terphenyl	84-15-1	201-517-6	1

#### 4. FIRST-AID MEASURES

<b>Inhalation:</b>	Remove to fresh air. If breathing is difficult, have a trained individual administer oxygen. If not breathing, give artificial respiration and have a trained individual administer oxygen. Get medical attention immediately.
<b>Eyes:</b>	Immediately flush eyes with plenty of water for at least 20 minutes retracting eyelids often. Tilt the head to prevent chemical from transferring to the uncontaminated eye. Get immediate medical attention and monitor the eye daily as advised by your physician. Serious harm (damage) may result if treatment is delayed. Continue to flush eyes while awaiting medical attention
<b>Skin Contact:</b>	Wash with soap and water. Remove contaminated clothing, launder immediately, and discard contaminated leather goods. Get medical attention immediately.
<b>Ingestion:</b>	Do not induce vomiting and seek medical attention immediately. Drink two glasses of water or milk to dilute. Provide medical care provider with this SDS. Never give anything by mouth to an unconscious person

#### 5. FIRE-FIGHTING MEASURES

<b>Extinguishing Media:</b>	Use alcohol resistant foam, carbon dioxide, or dry chemical when fighting fires. Water or foam may cause frothing if liquid is burning but it still may be a useful extinguishing agent if carefully applied to the surface of the fire. Do Not direct a stream of water into the hot burning liquid. Use methods suitable to fight surrounding fire.
<b>Fire and/or Explosion Hazards:</b>	Material may be ignited only if preheated to temperatures above the high flash point, for example in a fire.
<b>Fire Fighting Methods and Protection:</b>	Do not enter fire area without proper protection including self- contained breathing apparatus and full protective equipment.
<b>Hazardous Combustion Products:</b>	Carbon dioxide, Carbon monoxide

#### 6. ACCIDENTAL RELEASE MEASURES

<b>Personal Precautions and Equipment:</b>	Exposure to the spilled material may be severely irritating or toxic. Follow personal protective equipment recommendations found in Section 8 of this SDS. Personal protective equipment needs must be evaluated based on information provided on this sheet and the special circumstances created by the spill including: the material spilled, the quantity of the spill, the area in which the spill occurred, and the expertise of employees in the area responding to the spill. Never exceed any occupational exposure limits.
<b>Methods for Clean-up:</b>	Prevent the spread of any spill to minimize harm to human health and the environment if safe to do so. Wear complete and proper personal protective equipment following the recommendation of Section 8 at a minimum. Dike with suitable absorbent material like granulated clay. Gather and store in a sealed container pending a waste disposal evaluation.

#### 7. HANDLING AND STORAGE

<b>Handling Technical Measures and Precautions:</b>	Toxic or severely irritating material. Avoid contacting and avoid breathing the material. Use only in a well ventilated area. As with all chemicals, good industrial hygiene practices should be followed when handling this material.
<b>Storage Technical Measures and Conditions:</b>	Store in a cool dry place. Isolate from incompatible materials. Keep container closed when not in use

#### 8. EXPOSURE CONTROLS / PERSONAL PROTECTION

<b>United States:</b>					
<b>Chemical Name</b>	<b>CAS No.</b>	<b>IDLH</b>	<b>ACGIH STEL</b>	<b>ACGIH TLV-TWA</b>	<b>OSHA Exposure Limit</b>
Methylene chloride (dichloromethane)	75-09-2	2300 ppm IDLH	None Known	50 ppm TWA	25 ppm TWA; 125 ppm STEL (15 min. TWA)

o-terphenyl	84-15-1	500 mg/m3 IDLH	None Known	Not established	No data available
-------------	---------	-------------------	------------	-----------------	-------------------

**Personal Protection:**  
**Engineering Measures:**

Local exhaust ventilation or other engineering controls are normally required when handling or using this product to avoid overexposure.

**Respiratory Protection:** Respiratory protection may be required to avoid overexposure when handling this product. General or local exhaust ventilation is the preferred means of protection. Use a respirator if general room ventilation is not available or sufficient to eliminate symptoms.

**Eye Protection:**

Wear chemically resistant safety glasses with side shields when handling this product. Wear additional eye protection such as chemical splash goggles and/or face shield when the possibility exists for eye contact with splashing or spraying liquid, or airborne material. Do not wear contact lenses. Have an eye wash station available.

**Skin Protection:**

Avoid skin contact by wearing chemically resistant gloves, an apron and other protective equipment depending upon conditions of use. Inspect gloves for chemical break-through and replace at regular intervals. Clean protective equipment regularly. Wash hands and other exposed areas with mild soap and water before eating, drinking, and when leaving work.

**Medical Conditions Aggravated By Exposure:** Eye disease Skin disease including eczema and sensitization Respiratory disease including asthma and bronchitis

**9. PHYSICAL AND CHEMICAL PROPERTIES**

<b>Appearance, color:</b>	Colorless
<b>Odor:</b>	Strong
<b>Physical State:</b>	No data available
<b>pH:</b>	Not applicable
<b>Vapor Pressure:</b>	No data available
<b>Boiling Point (°C):</b>	2.93 (air = 1)
<b>Melting Point (°C):</b>	40 °C at 1013 hPa (ECHA_API)
<b>Flash Point (°F):</b>	-96.7 °C.
<b>Flammability:</b>	230
<b>Upper Flammable/Explosive Limit, % in air:</b>	Combustible at elevated temperatures
<b>Lower Flammable/Explosive Limit, % in air:</b>	No data available
<b>Autoignition Temperature (°C):</b>	No data available
<b>Decomposition Temperature (°C):</b>	556 deg C
<b>Specific Gravity:</b>	No data available
<b>Evaporation Rate:</b>	1.3254 - 1.3258 g/cm3 at 20 °C
<b>Odor Threshold:</b>	No data available
<b>Solubility:</b>	ND
<b>Partition Coefficient: n-octanol in water:</b>	Moderate; 50-99%
<b>VOC % by weight:</b>	No data available
<b>Molecular Weight:</b>	99
	No data available

**10. STABILITY AND REACTIVITY**

**Stability:** Stable under normal conditions.

**Conditions to Avoid:** Temperatures above the high flash point of this combustible material in combination with sparks, open flames, or other sources of ignition. Contamination High temperatures

**Materials to Avoid / Chemical Incompatibility:** Strong oxidizing agents Cautics (bases)

**Hazardous Decomposition Products:** Carbon dioxide Carbon monoxide

**11. TOXICOLOGICAL INFORMATION**

**Routes of Entry:** Inhalation Absorption Ingestion Skin contact Eye contact

**Target Organs Potentially Affected By Exposure:** Skin, Cardiovascular System, Eyes, Liver, Respiratory Tract

**Chemical Interactions That Change Toxicity:** None Known

**Immediate (Acute) Health Effects by Route of Exposure:**

**Inhalation Irritation:** Can cause moderate respiratory irritation, dizziness, weakness, fatigue, nausea and headache.

**Inhalation Toxicity:** Harmful! Can cause systemic damage (see "Target Organs")Inhalation may cause severe central nervous system depression (including unconsciousness).

**Skin Contact:** Contact causes severe skin irritation and possible burns.

**Skin Absorption:** Harmful if absorbed through the skin. May cause severe irritation and systemic damage.

**Eye Contact:** Contact with the eyes may cause moderate to severe eye injury. Eye contact may result in tearing and reddening, but not likely to permanently injure eye tissue. Temporary vision impairment (cloudy or blurred vision) is possible.

**Ingestion Irritation:** Irritating to mouth, throat, and stomach. Can cause abdominal discomfort, nausea, vomiting and diarrhea.

**Ingestion Toxicity:** Harmful if swallowed. May cause systemic poisoning.

**Long-Term (Chronic) Health Effects:**

**Carcinogenicity:** Contains a probable or known human carcinogen.

**Reproductive and Developmental Toxicity:** No data available to indicate product or any components present at greater than 0.1% may cause birth defects.

**Inhalation:** Upon prolonged and/or repeated exposure, can cause moderate respiratory irritation, dizziness, weakness, fatigue, nausea and headache.Harmful! Can cause systemic damage upon prolonged and/or repeated exposure (see "Target Organs")

**Skin Absorption:** Upon prolonged or repeated exposure, harmful if absorbed through the skin. May cause severe irritation and systemic damage

**Component Toxicological Data:**

**NIOSH:** **CAS No.** **LD50/LC50**

**Chemical Name** Oral LD50 Rat 1900 mg/kg

**o-Terphenyl** Dermal LD50 Rat >2000 mg/kg; Inhalation LC50

**Dichloromethane** Rat 53 mg/L 6 h; Oral LD50 Rat 1600 mg/kg

**Component Carcinogenic Data:**

**OSHA:** **CAS No.**

**Chemical Name**

**Methylene chloride** 75-09-2

25 ppm TWA (8 hr.); 125 ppm STEL (15 min.); 12.5 ppm Action Level (see 29 CFR 1910.1051); effective date for respiratory protection for certain employers to achieve the 8-hour TWA PEL is August 31, 1998; the start up date to install engineering controls is December 10, 1998.; {OSHA - 29 CFR 1910 Specifically Regulate

**ACGIH:** **CAS No.**

**Chemical Name** A3 - Confirmed Animal Carcinogen with

**Dichloromethane** 75-09-2 Unknown Relevance to Humans

**NIOSH:** **CAS No.**

**Chemical Name** potential occupational carcinogen

**Methylene chloride** 75-09-2

**NTP:** **CAS No.**

**Chemical Name**

**No data available**

**IARC:** **CAS No.** **Group No.**

**Chemical Name** 75-09-2 Group 2A

**Monograph 110 [2017];**

**Monograph 71 [1999]**

**12. ECOLOGICAL INFORMATION**

**Overview:** Moderate ecological hazard. This product may be dangerous

**Mobility:**  
**Persistence:**  
**Bioaccumulation:**  
**Degradability:**  
**Ecological Toxicity Data:**

to plants and/or wildlife. Keep out of waterways.

No data

No data

No data

No data

No data available

### 13. DISPOSAL CONSIDERATIONS

**Waste Description of Spent Product:**

Spent or discarded material is a hazardous waste. Mixing spent or discarded material with other materials may render the mixture hazardous. Perform a hazardous waste determination on mixtures.

**Disposal Methods:**

Incinerate spent or discarded material a permitted hazardous waste facility.

**Waste Disposal of Packaging:**

Comply with all Local, State, Federal, and Provincial Environmental Regulations.

### 14. TRANSPORTATION INFORMATION

**United States:**

**DOT Proper Shipping Name:**

Toxic, liquids, organic, n.o.s. (Dichloromethane, o-Terphenyl)

**UN Number:**

UN2810

**Hazard Class:**

6.1

**Packing Group:**

III

**International:**

**IATA Proper Shipping Name:**

Toxic, liquids, organic, n.o.s. (Dichloromethane, o-Terphenyl)

UN2810

6.1

III

**UN Number:**

6.1

**Hazard Class:**

III

**Packing Group:**

**Marine Pollutant:** No

Chemical Name	CAS#	Marine Pollutant	Severe Marine Pollutant
No data available			

### 15. REGULATORY INFORMATION

**United States:**

This chemical/product is not and cannot be distributed in commerce (as defined in TSCA section 3(5)) or processed (as defined in TSCA section 3(13)) for consumer paint or coating removal.

Chemical Name	CAS#	CERCLA	SARA 313	SARA EHS 313	TSCA
Methylene chloride (dichloromethane)	75-09-2	X	X	-	X
o-terphenyl	84-15-1	-	-	-	X

The following chemicals are listed on CA Prop 65:

Chemical Name	CAS #	Regulation
Dichloromethane	75-09-2	Prop 65 Cancer
Dichloromethane (Methylene chloride)		

**State Right To Know Listing:**

Chemical Name	CAS#	New Jersey	Massachusetts	Pennsylvania	California
Methylene chloride (dichloromethane)	75-09-2	X	X	X	X
o-terphenyl	84-15-1	-	X	-	-



## 16. OTHER INFORMATION

---

**Prior Version Date:** 04/27/23

**Other Information:** Any changes to the SDS compared to previous versions are marked by a vertical line in front of the concerned paragraph.

**References:**

No data available

**Disclaimer:**

Restek Corporation provides the descriptions, data and information contained herein in good faith but makes no representation as to its comprehensiveness or accuracy. It is provided for your guidance only. Because many factors may affect processing or application/use, Restek Corporation recommends you perform an assessment to determine the suitability of a product for your particular purpose prior to use. No warranties of any kind, either expressed or implied, including fitness for a particular purpose, are made regarding products described, data or information set forth. In no case shall the descriptions, information, or data provided be considered a part of our terms and conditions of sale. Further, the descriptions, data and information furnished hereunder are given gratis. No obligation or liability for the description, data and information given are assumed. All such being given and accepted at your risk.



## CERTIFIED REFERENCE MATERIAL



ISO 17025 Accredited  
Reference Material Producer  
Certificate # 2322301



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate # 1322202

110 Benner Circle

Belleville, PA 16823-8812

Tel: 1-814-353-1300

Fax: 1-814-353-1309

www.restek.com

# Certificate of Analysis

*chromatographic plus*

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31097

Lot No.: A0197729

Description : o-Terphenyl Standard

o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : December 31, 2026

Storage: 10°C or colder

Handling:

Sonicate prior to use.

Ship: Ambient

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	MKCH4487	99%	10,007.5 µg/mL	+/- 450.7438

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride

CAS # 75-09-2

Purity 99%

11574  
2  
912595  
4.1.P.  
06130

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
10 ml/min.

**Inj. Vol**  
1µl

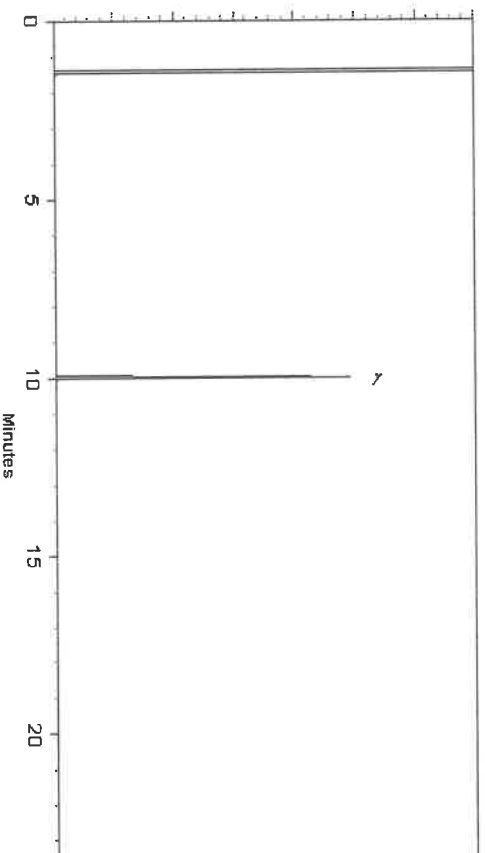

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*[Signature]*  
Alicia Leathers - Operation Technician I  
*[Signature]*  
Jennifer Pollino - Operations Tech III - ARM GC

Date Mixed: 03-May-2023      Balance Serial # 1128360905  
Date Passed: 08-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FIM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





## Safety Data Sheet

Revision Date: 05/04/23

[www.restek.com](http://www.restek.com)

2 Letter ISO country code/language code: US/EN

### 1. IDENTIFICATION

Catalog Number / Product Name:  
Company:  
Address:  
Phone#:  
Fax#:  
Emergency#:  
Email:  
Revision Number:  
Intended use:

31097 / o-Terphenyl Standard  
Restek Corporation  
110 Benner Circle  
Bellefonte, Pa. 16823  
814-353-1300  
814-353-1309  
800-424-9300 (CHEMTREC)  
703-527-3887 (Outside the US)  
[www.restek.com](http://www.restek.com)  
15

For Laboratory use only. This chemical/product is not and cannot be distributed in commerce (as defined in TSCA section 3(5)) or processed (as defined in TSCA section 3(13)) for consumer paint or coating removal.

### 2. HAZARD(S) IDENTIFICATION

#### Emergency Overview:

GHS Hazard  
Symbols:



GHS  
Classification: Carcinogenicity Category 2

GHS Signal  
Word: Warning

GHS Hazard:  
GHS  
Precautions: Suspected of causing cancer.

Safety  
Precautions: Obtain special instructions before use.  
Do not handle until all safety precautions have been read and understood.  
Wear protective gloves/protective clothing/eye protection/face protection.

First Aid  
Measures: If exposed or concerned: Get medical advice/attention.

Storage: Store locked up.

Disposal: Dispose of contents/container according to section 13 of the SDS.

Single  
Exposure  
Target Organs: No data available

Repeated  
Exposure  
Target Organs: No data available

### 3. COMPOSITION / INFORMATION ON INGREDIENT

Chemical Name	CAS #	INEC #	% Composition
Methylene chloride (dichloromethane)	75-09-2	200-838-9	99
o-terphenyl	84-15-1	201-517-6	1

#### 4. FIRST-AID MEASURES

<b>Inhalation:</b>	Remove to fresh air. If breathing is difficult, have a trained individual administer oxygen. If not breathing, give artificial respiration and have a trained individual administer oxygen. Get medical attention immediately.
<b>Eyes:</b>	Immediately flush eyes with plenty of water for at least 20 minutes retracting eyelids often. Tilt the head to prevent chemical from transferring to the uncontaminated eye. Get immediate medical attention and monitor the eye daily as advised by your physician. Serious harm (damage) may result if treatment is delayed. Continue to flush eyes while awaiting medical attention
<b>Skin Contact:</b>	Wash with soap and water. Remove contaminated clothing, launder immediately, and discard contaminated leather goods. Get medical attention immediately.
<b>Ingestion:</b>	Do not induce vomiting and seek medical attention immediately. Drink two glasses of water or milk to dilute. Provide medical care provider with this SDS. Never give anything by mouth to an unconscious person

#### 5. FIRE-FIGHTING MEASURES

<b>Extinguishing Media:</b>	Use alcohol resistant foam, carbon dioxide, or dry chemical when fighting fires. Water or foam may cause frothing if liquid is burning but it still may be a useful extinguishing agent if carefully applied to the surface of the fire. Do Not direct a stream of water into the hot burning liquid. Use methods suitable to fight surrounding fire.
<b>Fire and/or Explosion Hazards:</b>	Material may be ignited only if preheated to temperatures above the high flash point, for example in a fire.
<b>Fire Fighting Methods and Protection:</b>	Do not enter fire area without proper protection including self- contained breathing apparatus and full protective equipment.
<b>Hazardous Combustion Products:</b>	Carbon dioxide, Carbon monoxide

#### 6. ACCIDENTAL RELEASE MEASURES

<b>Personal Precautions and Equipment:</b>	Exposure to the spilled material may be severely irritating or toxic. Follow personal protective equipment recommendations found in Section 8 of this SDS. Personal protective equipment needs must be evaluated based on information provided on this sheet and the special circumstances created by the spill including: the material spilled, the quantity of the spill, the area in which the spill occurred, and the expertise of employees in the area responding to the spill. Never exceed any occupational exposure limits.
<b>Methods for Clean-up:</b>	Prevent the spread of any spill to minimize harm to human health and the environment if safe to do so. Wear complete and proper personal protective equipment following the recommendation of Section 8 at a minimum. Dike with suitable absorbent material like granulated clay. Gather and store in a sealed container pending a waste disposal evaluation.

#### 7. HANDLING AND STORAGE

<b>Handling Technical Measures and Precautions:</b>	Toxic or severely irritating material. Avoid contacting and avoid breathing the material. Use only in a well ventilated area. As with all chemicals, good industrial hygiene practices should be followed when handling this material.
<b>Storage Technical Measures and Conditions:</b>	Store in a cool dry place. Isolate from incompatible materials. Keep container closed when not in use

#### 8. EXPOSURE CONTROLS / PERSONAL PROTECTION

<b>United States:</b>					
<b>Chemical Name</b>	<b>CAS No.</b>	<b>IDLH</b>	<b>ACGIH STEL</b>	<b>ACGIH TLV-TWA</b>	<b>OSHA Exposure Limit</b>
Methylene chloride (dichloromethane)	75-09-2	2300 ppm IDLH	None Known	50 ppm TWA	25 ppm TWA; 125 ppm STEL (15 min. TWA)

o-terphenyl	84-15-1	500 mg/m3 IDLH	None Known	Not established	No data available
-------------	---------	-------------------	------------	-----------------	-------------------

**Personal Protection:**

Local exhaust ventilation or other engineering controls are normally required when handling or using this product to avoid overexposure.

**Engineering Measures:**

**Respiratory Protection:**

Respiratory protection may be required to avoid overexposure when handling this product. General or local exhaust ventilation is the preferred means of protection. Use a respirator if general room ventilation is not available or sufficient to eliminate symptoms.

**Eye Protection:**

Wear chemically resistant safety glasses with side shields when handling this product. Wear additional eye protection such as chemical splash goggles and/or face shield when the possibility exists for eye contact with splashing or spraying liquid, or airborne material. Do not wear contact lenses. Have an eye wash station available.

**Skin Protection:**

Avoid skin contact by wearing chemically resistant gloves, an apron and other protective equipment depending upon conditions of use. Inspect gloves for chemical break-through and replace at regular intervals. Clean protective equipment regularly. Wash hands and other exposed areas with mild soap and water before eating, drinking, and when leaving work.

**Medical Conditions Aggravated By Exposure:**

Eye disease Skin disease including eczema and sensitization Respiratory disease including asthma and bronchitis

**9. PHYSICAL AND CHEMICAL PROPERTIES**

<b>Appearance, color:</b>	Colorless
<b>Odor:</b>	Strong
<b>Physical State:</b>	No data available
<b>pH:</b>	Not applicable
<b>Vapor Pressure:</b>	No data available
<b>Boiling Point (°C):</b>	2.93 (air = 1)
<b>Melting Point (°C):</b>	40 °C at 1013 hPa (ECHA_API)
<b>Flash Point (°F):</b>	-96.7 °C.
<b>Flammability:</b>	230
<b>Upper Flammable/Explosive Limit, % in air:</b>	Combustible at elevated temperatures
<b>Lower Flammable/Explosive Limit, % in air:</b>	No data available
<b>Autoignition Temperature (°C):</b>	No data available
<b>Decomposition Temperature (°C):</b>	556 deg C
<b>Specific Gravity:</b>	No data available
<b>Evaporation Rate:</b>	1.3254 - 1.3258 g/cm3 at 20 °C
<b>Odor Threshold:</b>	No data available
<b>Solubility:</b>	ND
<b>Partition Coefficient: n-octanol in water:</b>	Moderate; 50-99%
<b>VOC % by weight:</b>	No data available
<b>Molecular Weight:</b>	99
	No data available

**10. STABILITY AND REACTIVITY**

<b>Stability:</b>	Stable under normal conditions.
<b>Conditions to Avoid:</b>	Temperatures above the high flash point of this combustible material in combination with sparks, open flames, or other sources of ignition. Contamination High temperatures

**Materials to Avoid / Chemical Incompatibility:**

Strong oxidizing agents Cautics (bases)  
Carbon dioxide Carbon monoxide

**Hazardous Decomposition Products:**

**11. TOXICOLOGICAL INFORMATION**

<b>Routes of Entry:</b>	Inhalation Absorption Ingestion Skin contact Eye contact
<b>Target Organs Potentially Affected By Exposure:</b>	Skin, Cardiovascular System, Eyes, Liver, Respiratory Tract
<b>Chemical Interactions That Change Toxicity:</b>	None Known

**Immediate (Acute) Health Effects by Route of Exposure:**

**Inhalation Irritation:** Can cause moderate respiratory irritation, dizziness, weakness, fatigue, nausea and headache.



**Inhalation Toxicity:** Harmful! Can cause systemic damage (see "Target Organs")Inhalation may cause severe central nervous system depression (including unconsciousness).

**Skin Contact:** Contact causes severe skin irritation and possible burns.

**Skin Absorption:** Harmful if absorbed through the skin. May cause severe irritation and systemic damage.

**Eye Contact:** Contact with the eyes may cause moderate to severe eye injury. Eye contact may result in tearing and reddening, but not likely to permanently injure eye tissue. Temporary vision impairment (cloudy or blurred vision) is possible.

**Ingestion Irritation:** Irritating to mouth, throat, and stomach. Can cause abdominal discomfort, nausea, vomiting and diarrhea.

**Ingestion Toxicity:** Harmful if swallowed. May cause systemic poisoning.

**Long-Term (Chronic) Health Effects:**

**Carcinogenicity:** Contains a probable or known human carcinogen.

**Reproductive and Developmental Toxicity:** No data available to indicate product or any components present at greater than 0.1% may cause birth defects.

**Inhalation:** Upon prolonged and/or repeated exposure, can cause moderate respiratory irritation, dizziness, weakness, fatigue, nausea and headache.Harmful! Can cause systemic damage upon prolonged and/or repeated exposure (see "Target Organs")

**Skin Absorption:** Upon prolonged or repeated exposure, harmful if absorbed through the skin. May cause severe irritation and systemic damage

**Component Toxicological Data:**

**NIOSH:** **CAS No.** **LD50/LC50**

**Chemical Name** Oral LD50 Rat 1900 mg/kg

**o-Terphenyl** Dermal LD50 Rat >2000 mg/kg; Inhalation LC50

**Dichloromethane** Rat 53 mg/L 6 h; Oral LD50 Rat 1600 mg/kg

**Component Carcinogenic Data:**

**OSHA:** **CAS No.**

**Chemical Name**

**Methylene chloride** 75-09-2

25 ppm TWA (8 hr.); 125 ppm STEL (15 min.); 12.5 ppm Action Level (see 29 CFR 1910.1051); effective date for respiratory protection for certain employers to achieve the 8-hour TWA PEL is August 31, 1998; the start up date to install engineering controls is December 10, 1998.; {OSHA - 29 CFR 1910 Specifically Regulate

**ACGIH:** **CAS No.**

**Chemical Name** A3 - Confirmed Animal Carcinogen with

**Dichloromethane** 75-09-2 Unknown Relevance to Humans

**NIOSH:** **CAS No.**

**Chemical Name** potential occupational carcinogen

**Methylene chloride** 75-09-2

**NTP:** **CAS No.**

**Chemical Name**

**No data available**

**IARC:** **CAS No.** **Group No.**

**Chemical Name** 75-09-2 Group 2A

**Monograph 110 [2017];**

**Monograph 71 [1999]**

**12. ECOLOGICAL INFORMATION**

**Overview:** Moderate ecological hazard. This product may be dangerous

**Mobility:**  
**Persistence:**  
**Bioaccumulation:**  
**Degradability:**  
**Ecological Toxicity Data:**

to plants and/or wildlife. Keep out of waterways.  
No data  
No data  
No data  
No data  
No data available

### 13. DISPOSAL CONSIDERATIONS

**Waste Description of Spent Product:**

**Disposal Methods:**

**Waste Disposal of Packaging:**

Spent or discarded material is a hazardous waste. Mixing spent or discarded material with other materials may render the mixture hazardous. Perform a hazardous waste determination on mixtures.  
Incinerate spent or discarded material a permitted hazardous waste facility.  
Comply with all Local, State, Federal, and Provincial Environmental Regulations.

### 14. TRANSPORTATION INFORMATION

**United States:**

**DOT Proper Shipping Name:**

Toxic, liquids, organic, n.o.s. (Dichloromethane, o-Terphenyl)

**UN Number:**

UN2810

**Hazard Class:**

6.1

**Packing Group:**

III

**International:**

**IATA Proper Shipping Name:**

Toxic, liquids, organic, n.o.s. (Dichloromethane, o-Terphenyl)

UN2810

6.1

III

**Hazard Class:**

6.1

**Packing Group:**

III

**Marine Pollutant:** No

Chemical Name	CAS#	Marine Pollutant	Severe Marine Pollutant
No data available			

### 15. REGULATORY INFORMATION

**United States:**

This chemical/product is not and cannot be distributed in commerce (as defined in TSCA section 3(5)) or processed (as defined in TSCA section 3(13)) for consumer paint or coating removal.

Chemical Name	CAS#	CERCLA	SARA 313	SARA EHS 313	TSCA
Methylene chloride (dichloromethane)	75-09-2	X	X	-	X
o-terphenyl	84-15-1	-	-	-	X

The following chemicals are listed on CA Prop 65:

Chemical Name	CAS #	Regulation
Dichloromethane	75-09-2	
Dichloromethane (Methylene chloride)	75-09-2	Prop 65 Cancer

**State Right To Know Listing:**

Chemical Name	CAS#	New Jersey	Massachusetts	Pennsylvania	California
Methylene chloride (dichloromethane)	75-09-2	X	X	X	X
o-terphenyl	84-15-1	-	X	-	-

## 16. OTHER INFORMATION

---

**Prior Version Date:** 04/27/23

**Other Information:** Any changes to the SDS compared to previous versions are marked by a vertical line in front of the concerned paragraph.

**References:**

No data available

**Disclaimer:**

Restek Corporation provides the descriptions, data and information contained herein in good faith but makes no representation as to its comprehensiveness or accuracy. It is provided for your guidance only. Because many factors may affect processing or application/use, Restek Corporation recommends you perform an assessment to determine the suitability of a product for your particular purpose prior to use. No warranties of any kind, either expressed or implied, including fitness for a particular purpose, are made regarding products described, data or information set forth. In no case shall the descriptions, information, or data provided be considered a part of our terms and conditions of sale. Further, the descriptions, data and information furnished hereunder are given gratis. No obligation or liability for the description, data and information given are assumed. All such being given and accepted at your risk.



## CERTIFIED REFERENCE MATERIAL



ISO 17025 Accredited  
Reference Material Producer  
Certificate # 2322301



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

## Certificate of Analysis

*chromatographic plus*

www.restek.com



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate # 1322202

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31097

Lot No.: A0197729

Description : o-Terphenyl Standard

o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : December 31, 2026

Storage: 10°C or colder

Handling: Sonicate prior to use.

Ship: Ambient

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.L.; K=2)
1	o-Terphenyl	84-15-1	MKCH4487	99%	10,007.5 µg/mL	+/- 450.7438

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride

CAS # 75-09-2

Purity 99%

11574  
2  
912595  
4.1.P.  
06130

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
10 ml/min.

**Inj. Vol**  
1µl

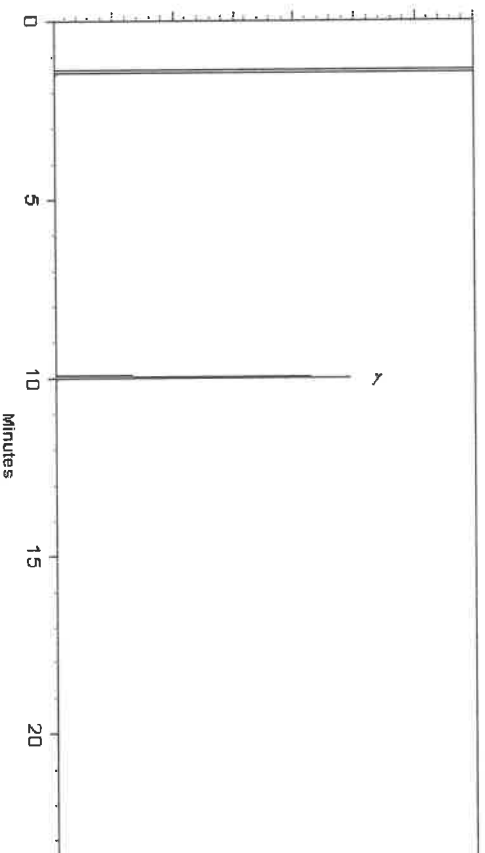

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Alicia Leathers*  
**Alicia Leathers - Operation Technician I**  
*Jennifer Polino*  
**Jennifer Polino - Operations Tech III - RRM GC**

**Date Mixed:** 03-May-2023  
**Balance Serial #** 1128360905  
**Date Passed:** 08-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FIM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





## Safety Data Sheet

Revision Date: 05/04/23

[www.restek.com](http://www.restek.com)

2 Letter ISO country code/language code: US/EN

### 1. IDENTIFICATION

Catalog Number / Product Name:  
Company:  
Address:  
Phone#:  
Fax#:  
Emergency#:  
Email:  
Revision Number:  
Intended use:

31097 / o-Terphenyl Standard  
Restek Corporation  
110 Benner Circle  
Bellefonte, Pa. 16823  
814-353-1300  
814-353-1309  
800-424-9300 (CHEMTREC)  
703-527-3887 (Outside the US)  
[www.restek.com](http://www.restek.com)  
15

For Laboratory use only. This chemical/product is not and cannot be distributed in commerce (as defined in TSCA section 3(5)) or processed (as defined in TSCA section 3(13)) for consumer paint or coating removal.

### 2. HAZARD(S) IDENTIFICATION

#### Emergency Overview:

GHS Hazard  
Symbols:



GHS  
Classification: Carcinogenicity Category 2

GHS Signal  
Word: Warning

GHS Hazard:  
Suspected of causing cancer.

GHS  
Precautions:

Safety  
Precautions: Obtain special instructions before use.  
Do not handle until all safety precautions have been read and understood.  
Wear protective gloves/protective clothing/eye protection/face protection.

First Aid  
Measures: If exposed or concerned: Get medical advice/attention.

Storage: Store locked up.

Disposal: Dispose of contents/container according to section 13 of the SDS.

Single  
Exposure  
Target Organs: No data available

Repeated  
Exposure  
Target Organs: No data available

### 3. COMPOSITION / INFORMATION ON INGREDIENT



Chemical Name	CAS #	INEC #	% Composition
Methylene chloride (dichloromethane)	75-09-2	200-838-9	99
o-terphenyl	84-15-1	201-517-6	1

#### 4. FIRST-AID MEASURES

<b>Inhalation:</b>	Remove to fresh air. If breathing is difficult, have a trained individual administer oxygen. If not breathing, give artificial respiration and have a trained individual administer oxygen. Get medical attention immediately.
<b>Eyes:</b>	Immediately flush eyes with plenty of water for at least 20 minutes retracting eyelids often. Tilt the head to prevent chemical from transferring to the uncontaminated eye. Get immediate medical attention and monitor the eye daily as advised by your physician. Serious harm (damage) may result if treatment is delayed. Continue to flush eyes while awaiting medical attention
<b>Skin Contact:</b>	Wash with soap and water. Remove contaminated clothing, launder immediately, and discard contaminated leather goods. Get medical attention immediately.
<b>Ingestion:</b>	Do not induce vomiting and seek medical attention immediately. Drink two glasses of water or milk to dilute. Provide medical care provider with this SDS. Never give anything by mouth to an unconscious person

#### 5. FIRE-FIGHTING MEASURES

<b>Extinguishing Media:</b>	Use alcohol resistant foam, carbon dioxide, or dry chemical when fighting fires. Water or foam may cause frothing if liquid is burning but it still may be a useful extinguishing agent if carefully applied to the surface of the fire. Do Not direct a stream of water into the hot burning liquid. Use methods suitable to fight surrounding fire.
<b>Fire and/or Explosion Hazards:</b>	Material may be ignited only if preheated to temperatures above the high flash point, for example in a fire.
<b>Fire Fighting Methods and Protection:</b>	Do not enter fire area without proper protection including self- contained breathing apparatus and full protective equipment.
<b>Hazardous Combustion Products:</b>	Carbon dioxide, Carbon monoxide

#### 6. ACCIDENTAL RELEASE MEASURES

<b>Personal Precautions and Equipment:</b>	Exposure to the spilled material may be severely irritating or toxic. Follow personal protective equipment recommendations found in Section 8 of this SDS. Personal protective equipment needs must be evaluated based on information provided on this sheet and the special circumstances created by the spill including: the material spilled, the quantity of the spill, the area in which the spill occurred, and the expertise of employees in the area responding to the spill. Never exceed any occupational exposure limits.
<b>Methods for Clean-up:</b>	Prevent the spread of any spill to minimize harm to human health and the environment if safe to do so. Wear complete and proper personal protective equipment following the recommendation of Section 8 at a minimum. Dike with suitable absorbent material like granulated clay. Gather and store in a sealed container pending a waste disposal evaluation.

#### 7. HANDLING AND STORAGE

<b>Handling Technical Measures and Precautions:</b>	Toxic or severely irritating material. Avoid contacting and avoid breathing the material. Use only in a well ventilated area. As with all chemicals, good industrial hygiene practices should be followed when handling this material.
<b>Storage Technical Measures and Conditions:</b>	Store in a cool dry place. Isolate from incompatible materials. Keep container closed when not in use

#### 8. EXPOSURE CONTROLS / PERSONAL PROTECTION

<b>United States:</b>					
<b>Chemical Name</b>	<b>CAS No.</b>	<b>IDLH</b>	<b>ACGIH STEL</b>	<b>ACGIH TLV-TWA</b>	<b>OSHA Exposure Limit</b>
Methylene chloride (dichloromethane)	75-09-2	2300 ppm IDLH	None Known	50 ppm TWA	25 ppm TWA; 125 ppm STEL (15 min. TWA)

o-terphenyl	84-15-1	500 mg/m3 IDLH	None Known	Not established	No data available
-------------	---------	-------------------	------------	-----------------	-------------------

**Personal Protection:**

Local exhaust ventilation or other engineering controls are normally required when handling or using this product to avoid overexposure.

**Engineering Measures:**

**Respiratory Protection:**

Respiratory protection may be required to avoid overexposure when handling this product. General or local exhaust ventilation is the preferred means of protection. Use a respirator if general room ventilation is not available or sufficient to eliminate symptoms.

**Eye Protection:**

Wear chemically resistant safety glasses with side shields when handling this product. Wear additional eye protection such as chemical splash goggles and/or face shield when the possibility exists for eye contact with splashing or spraying liquid, or airborne material. Do not wear contact lenses. Have an eye wash station available.

**Skin Protection:**

Avoid skin contact by wearing chemically resistant gloves, an apron and other protective equipment depending upon conditions of use. Inspect gloves for chemical break-through and replace at regular intervals. Clean protective equipment regularly. Wash hands and other exposed areas with mild soap and water before eating, drinking, and when leaving work.

**Medical Conditions Aggravated By Exposure:**

Eye disease Skin disease including eczema and sensitization Respiratory disease including asthma and bronchitis

**9. PHYSICAL AND CHEMICAL PROPERTIES**

<b>Appearance, color:</b>	Colorless
<b>Odor:</b>	Strong
<b>Physical State:</b>	No data available
<b>pH:</b>	Not applicable
<b>Vapor Pressure:</b>	No data available
<b>Boiling Point (°C):</b>	2.93 (air = 1)
<b>Melting Point (°C):</b>	40 °C at 1013 hPa (ECHA_API)
<b>Flash Point (°F):</b>	-96.7 °C.
<b>Flammability:</b>	230
<b>Upper Flammable/Explosive Limit, % in air:</b>	Combustible at elevated temperatures
<b>Lower Flammable/Explosive Limit, % in air:</b>	No data available
<b>Autoignition Temperature (°C):</b>	No data available
<b>Decomposition Temperature (°C):</b>	556 deg C
<b>Specific Gravity:</b>	No data available
<b>Evaporation Rate:</b>	1.3254 - 1.3258 g/cm3 at 20 °C
<b>Odor Threshold:</b>	No data available
<b>Solubility:</b>	ND
<b>Partition Coefficient: n-octanol in water:</b>	Moderate; 50-99%
<b>VOC % by weight:</b>	No data available
<b>Molecular Weight:</b>	99
	No data available

**10. STABILITY AND REACTIVITY**

<b>Stability:</b>	Stable under normal conditions.
<b>Conditions to Avoid:</b>	Temperatures above the high flash point of this combustible material in combination with sparks, open flames, or other sources of ignition. Contamination High temperatures

**Materials to Avoid / Chemical Incompatibility:**

Strong oxidizing agents Cautics (bases)

**Hazardous Decomposition Products:**

Carbon dioxide Carbon monoxide

**11. TOXICOLOGICAL INFORMATION**

<b>Routes of Entry:</b>	Inhalation Absorption Ingestion Skin contact Eye contact
<b>Target Organs Potentially Affected By Exposure:</b>	Skin, Cardiovascular System, Eyes, Liver, Respiratory Tract
<b>Chemical Interactions That Change Toxicity:</b>	None Known

**Immediate (Acute) Health Effects by Route of Exposure:**

**Inhalation Irritation:** Can cause moderate respiratory irritation, dizziness, weakness, fatigue, nausea and headache.

**Inhalation Toxicity:** Harmful! Can cause systemic damage (see "Target Organs")Inhalation may cause severe central nervous system depression (including unconsciousness).

**Skin Contact:** Contact causes severe skin irritation and possible burns.

**Skin Absorption:** Harmful if absorbed through the skin. May cause severe irritation and systemic damage.

**Eye Contact:** Contact with the eyes may cause moderate to severe eye injury. Eye contact may result in tearing and reddening, but not likely to permanently injure eye tissue. Temporary vision impairment (cloudy or blurred vision) is possible.

**Ingestion Irritation:** Irritating to mouth, throat, and stomach. Can cause abdominal discomfort, nausea, vomiting and diarrhea.

**Ingestion Toxicity:** Harmful if swallowed. May cause systemic poisoning.

**Long-Term (Chronic) Health Effects:**

**Carcinogenicity:** Contains a probable or known human carcinogen.

**Reproductive and Developmental Toxicity:** No data available to indicate product or any components present at greater than 0.1% may cause birth defects.

**Inhalation:** Upon prolonged and/or repeated exposure, can cause moderate respiratory irritation, dizziness, weakness, fatigue, nausea and headache.Harmful! Can cause systemic damage upon prolonged and/or repeated exposure (See "Target Organs")

**Skin Absorption:** Upon prolonged or repeated exposure, harmful if absorbed through the skin. May cause severe irritation and systemic damage

**Component Toxicological Data:**

**NIOSH:** **CAS No.** **LD50/LC50**

**Chemical Name** Oral LD50 Rat 1900 mg/kg

**o-Terphenyl** Dermal LD50 Rat >2000 mg/kg; Inhalation LC50

**Dichloromethane** Rat 53 mg/L 6 h; Oral LD50 Rat 1600 mg/kg

**Component Carcinogenic Data:**

**OSHA:** **CAS No.**

**Chemical Name**

**Methylene chloride** 75-09-2

25 ppm TWA (8 hr.); 125 ppm STEL (15 min.); 12.5 ppm Action Level (see 29 CFR 1910.1051); effective date for respiratory protection for certain employers to achieve the 8-hour TWA PEL is August 31, 1998; the start up date to install engineering controls is December 10, 1998.; {OSHA - 29 CFR 1910 Specifically Regulate

**ACGIH:** **CAS No.**

**Chemical Name** A3 - Confirmed Animal Carcinogen with

**Dichloromethane** 75-09-2 Unknown Relevance to Humans

**NIOSH:** **CAS No.**

**Chemical Name** potential occupational carcinogen

**Methylene chloride** 75-09-2

**NTP:** **CAS No.**

**Chemical Name**

**No data available**

**IARC:** **CAS No.** **Group No.**

**Chemical Name** 75-09-2 Group 2A

**Monograph 110 [2017];**

**Monograph 71 [1999]**

**12. ECOLOGICAL INFORMATION**

**Overview:** Moderate ecological hazard. This product may be dangerous

**Mobility:**  
**Persistence:**  
**Bioaccumulation:**  
**Degradability:**  
**Ecological Toxicity Data:**

to plants and/or wildlife. Keep out of waterways.

No data

No data

No data

No data

No data available

### 13. DISPOSAL CONSIDERATIONS

**Waste Description of Spent Product:**

**Disposal Methods:**

**Waste Disposal of Packaging:**

Spent or discarded material is a hazardous waste. Mixing spent or discarded material with other materials may render the mixture hazardous. Perform a hazardous waste determination on mixtures. Incinerate spent or discarded material a permitted hazardous waste facility. Comply with all Local, State, Federal, and Provincial Environmental Regulations.

### 14. TRANSPORTATION INFORMATION

**United States:**

**DOT Proper Shipping Name:**

Toxic, liquids, organic, n.o.s. (Dichloromethane, o-Terphenyl)

**UN Number:**

UN2810

**Hazard Class:**

6.1

**Packing Group:**

III

**International:**

**IATA Proper Shipping Name:**

Toxic, liquids, organic, n.o.s. (Dichloromethane, o-Terphenyl)

UN2810

6.1

III

**Hazard Class:**

6.1

**Packing Group:**

III

**Marine Pollutant:** No

Chemical Name	CAS#	Marine Pollutant	Severe Marine Pollutant
No data available			

### 15. REGULATORY INFORMATION

**United States:**

This chemical/product is not and cannot be distributed in commerce (as defined in TSCA section 3(5)) or processed (as defined in TSCA section 3(13)) for consumer paint or coating removal.

Chemical Name	CAS#	CERCLA	SARA 313	SARA EHS 313	TSCA
Methylene chloride (dichloromethane)	75-09-2	X	X	-	X
o-terphenyl	84-15-1	-	-	-	X

The following chemicals are listed on CA Prop 65:

Chemical Name	CAS #	Regulation
Dichloromethane	75-09-2	Prop 65 Cancer
Dichloromethane (Methylene chloride)		

**State Right To Know Listing:**

Chemical Name	CAS#	New Jersey	Massachusetts	Pennsylvania	California
Methylene chloride (dichloromethane)	75-09-2	X	X	X	X
o-terphenyl	84-15-1	-	X	-	-

## 16. OTHER INFORMATION

---

**Prior Version Date:** 04/27/23

**Other Information:** Any changes to the SDS compared to previous versions are marked by a vertical line in front of the concerned paragraph.

**References:**

No data available

**Disclaimer:**

Restek Corporation provides the descriptions, data and information contained herein in good faith but makes no representation as to its comprehensiveness or accuracy. It is provided for your guidance only. Because many factors may affect processing or application/use, Restek Corporation recommends you perform an assessment to determine the suitability of a product for your particular purpose prior to use. No warranties of any kind, either expressed or implied, including fitness for a particular purpose, are made regarding products described, data or information set forth. In no case shall the descriptions, information, or data provided be considered a part of our terms and conditions of sale. Further, the descriptions, data and information furnished hereunder are given gratis. No obligation or liability for the description, data and information given are assumed. All such being given and accepted at your risk.



## CERTIFIED REFERENCE MATERIAL



ISO 17025 Accredited  
Reference Material Producer  
Certificate # 2322301



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate # 1322202

110 Benner Circle

Belleville, PA 16823-8812

Tel: 1-814-353-1300

Fax: 1-814-353-1309

www.restek.com

# Certificate of Analysis

## chromatographic plus

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31097

Lot No.: A0197729

Description : o-Terphenyl Standard

o-Terphenyl Standard 10,000 µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : December 31, 2026

Storage: 10°C or colder

Handling:

Sonicate prior to use.

Ship: Ambient

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty* (95% C.I., K=2)
1	o-Terphenyl	84-15-1	MKCH4487	99%	10,007.5 µg/mL	+/- 450.7438

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Methylene chloride

CAS # 75-09-2

Purity 99%

11574  
2  
9.18  
012595  
06130

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
10 ml/min.

**Inj. Vol**  
1µl

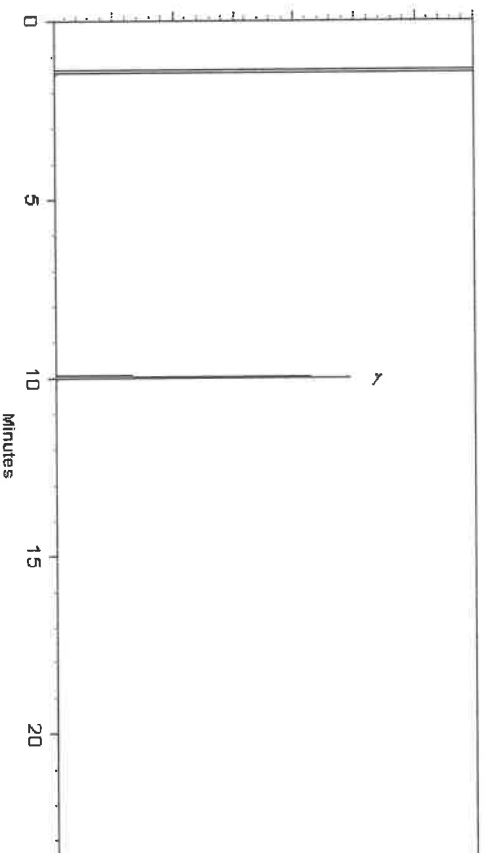

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Alicia Leathers*  
**Alicia Leathers - Operation Technician I**  
*Jennifer Polino*  
**Jennifer Polino - Operations Tech III - RRM GC**

**Date Mixed:** 03-May-2023  
**Balance Serial #** 1128360905  
**Date Passed:** 08-May-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FIM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







## Safety Data Sheet

Revision Date: 05/04/23

[www.restek.com](http://www.restek.com)

2 Letter ISO country code/language code: US/EN

### 1. IDENTIFICATION

Catalog Number / Product Name:	31097 / o-Terphenyl Standard
Company:	Restek Corporation
Address:	110 Benner Circle Bellefonte, Pa. 16823
Phone#:	814-353-1300
Fax#:	814-353-1309
Emergency#:	800-424-9300 (CHEMTREC) 703-527-3887 (Outside the US)
Email:	<a href="http://www.restek.com">www.restek.com</a>
Revision Number:	15
Intended use:	For Laboratory use only. This chemical/product is not and cannot be distributed in commerce (as defined in TSCA section 3(5)) or processed (as defined in TSCA section 3(13)) for consumer paint or coating removal.

### 2. HAZARD(S) IDENTIFICATION

#### Emergency Overview:

GHS Hazard  
Symbols:



GHS  
Classification: Carcinogenicity Category 2

GHS Signal  
Word: Warning

GHS Hazard: Suspected of causing cancer.

GHS  
Precautions:

Safety  
Precautions: Obtain special instructions before use.  
Do not handle until all safety precautions have been read and understood.  
Wear protective gloves/protective clothing/eye protection/face protection.

First Aid  
Measures: If exposed or concerned: Get medical advice/attention.

Storage: Store locked up.

Disposal: Dispose of contents/container according to section 13 of the SDS.

Single  
Exposure  
Target Organs: No data available

Repeated  
Exposure  
Target Organs: No data available

### 3. COMPOSITION / INFORMATION ON INGREDIENT

Chemical Name	CAS #	INEC #	% Composition
Methylene chloride (dichloromethane)	75-09-2	200-838-9	99
o-terphenyl	84-15-1	201-517-6	1

#### 4. FIRST-AID MEASURES

<b>Inhalation:</b>	Remove to fresh air. If breathing is difficult, have a trained individual administer oxygen. If not breathing, give artificial respiration and have a trained individual administer oxygen. Get medical attention immediately.
<b>Eyes:</b>	Immediately flush eyes with plenty of water for at least 20 minutes retracting eyelids often. Tilt the head to prevent chemical from transferring to the uncontaminated eye. Get immediate medical attention and monitor the eye daily as advised by your physician. Serious harm (damage) may result if treatment is delayed. Continue to flush eyes while awaiting medical attention
<b>Skin Contact:</b>	Wash with soap and water. Remove contaminated clothing, launder immediately, and discard contaminated leather goods. Get medical attention immediately.
<b>Ingestion:</b>	Do not induce vomiting and seek medical attention immediately. Drink two glasses of water or milk to dilute. Provide medical care provider with this SDS. Never give anything by mouth to an unconscious person

#### 5. FIRE-FIGHTING MEASURES

<b>Extinguishing Media:</b>	Use alcohol resistant foam, carbon dioxide, or dry chemical when fighting fires. Water or foam may cause frothing if liquid is burning but it still may be a useful extinguishing agent if carefully applied to the surface of the fire. Do Not direct a stream of water into the hot burning liquid. Use methods suitable to fight surrounding fire.
<b>Fire and/or Explosion Hazards:</b>	Material may be ignited only if preheated to temperatures above the high flash point, for example in a fire.
<b>Fire Fighting Methods and Protection:</b>	Do not enter fire area without proper protection including self- contained breathing apparatus and full protective equipment.
<b>Hazardous Combustion Products:</b>	Carbon dioxide, Carbon monoxide

#### 6. ACCIDENTAL RELEASE MEASURES

<b>Personal Precautions and Equipment:</b>	Exposure to the spilled material may be severely irritating or toxic. Follow personal protective equipment recommendations found in Section 8 of this SDS. Personal protective equipment needs must be evaluated based on information provided on this sheet and the special circumstances created by the spill including: the material spilled, the quantity of the spill, the area in which the spill occurred, and the expertise of employees in the area responding to the spill. Never exceed any occupational exposure limits.
<b>Methods for Clean-up:</b>	Prevent the spread of any spill to minimize harm to human health and the environment if safe to do so. Wear complete and proper personal protective equipment following the recommendation of Section 8 at a minimum. Dike with suitable absorbent material like granulated clay. Gather and store in a sealed container pending a waste disposal evaluation.

#### 7. HANDLING AND STORAGE

<b>Handling Technical Measures and Precautions:</b>	Toxic or severely irritating material. Avoid contacting and avoid breathing the material. Use only in a well ventilated area. As with all chemicals, good industrial hygiene practices should be followed when handling this material.
<b>Storage Technical Measures and Conditions:</b>	Store in a cool dry place. Isolate from incompatible materials. Keep container closed when not in use

#### 8. EXPOSURE CONTROLS / PERSONAL PROTECTION

<b>United States:</b>					
<b>Chemical Name</b>	<b>CAS No.</b>	<b>IDLH</b>	<b>ACGIH STEL</b>	<b>ACGIH TLV-TWA</b>	<b>OSHA Exposure Limit</b>
Methylene chloride (dichloromethane)	75-09-2	2300 ppm IDLH	None Known	50 ppm TWA	25 ppm TWA; 125 ppm STEL (15 min. TWA)

o-terphenyl	84-15-1	500 mg/m3 IDLH	None Known	Not established	No data available
-------------	---------	-------------------	------------	-----------------	-------------------

**Personal Protection:**

Local exhaust ventilation or other engineering controls are normally required when handling or using this product to avoid overexposure.

**Engineering Measures:**

**Respiratory Protection:**

Respiratory protection may be required to avoid overexposure when handling this product. General or local exhaust ventilation is the preferred means of protection. Use a respirator if general room ventilation is not available or sufficient to eliminate symptoms.

**Eye Protection:**

Wear chemically resistant safety glasses with side shields when handling this product. Wear additional eye protection such as chemical splash goggles and/or face shield when the possibility exists for eye contact with splashing or spraying liquid, or airborne material. Do not wear contact lenses. Have an eye wash station available.

**Skin Protection:**

Avoid skin contact by wearing chemically resistant gloves, an apron and other protective equipment depending upon conditions of use. Inspect gloves for chemical break-through and replace at regular intervals. Clean protective equipment regularly. Wash hands and other exposed areas with mild soap and water before eating, drinking, and when leaving work.

**Medical Conditions Aggravated By Exposure:**

Eye disease Skin disease including eczema and sensitization Respiratory disease including asthma and bronchitis

**9. PHYSICAL AND CHEMICAL PROPERTIES**

<b>Appearance, color:</b>	Colorless
<b>Odor:</b>	Strong
<b>Physical State:</b>	No data available
<b>pH:</b>	Not applicable
<b>Vapor Pressure:</b>	No data available
<b>Boiling Point (°C):</b>	2.93 (air = 1)
<b>Melting Point (°C):</b>	40 °C at 1013 hPa (ECHA_API)
<b>Flash Point (°F):</b>	-96.7 °C.
<b>Flammability:</b>	230
<b>Upper Flammable/Explosive Limit, % in air:</b>	Combustible at elevated temperatures
<b>Lower Flammable/Explosive Limit, % in air:</b>	No data available
<b>Autoignition Temperature (°C):</b>	No data available
<b>Decomposition Temperature (°C):</b>	556 deg C
<b>Specific Gravity:</b>	No data available
<b>Evaporation Rate:</b>	1.3254 - 1.3258 g/cm3 at 20 °C
<b>Odor Threshold:</b>	No data available
<b>Solubility:</b>	ND
<b>Partition Coefficient: n-octanol in water:</b>	Moderate; 50-99%
<b>VOC % by weight:</b>	No data available
<b>Molecular Weight:</b>	99
	No data available

**10. STABILITY AND REACTIVITY**

<b>Stability:</b>	Stable under normal conditions.
<b>Conditions to Avoid:</b>	Temperatures above the high flash point of this combustible material in combination with sparks, open flames, or other sources of ignition. Contamination High temperatures

**Materials to Avoid / Chemical Incompatibility:**

Strong oxidizing agents Cautics (bases)

**Hazardous Decomposition Products:**

Carbon dioxide Carbon monoxide

**11. TOXICOLOGICAL INFORMATION**

<b>Routes of Entry:</b>	Inhalation Absorption Ingestion Skin contact Eye contact
<b>Target Organs Potentially Affected By Exposure:</b>	Skin, Cardiovascular System, Eyes, Liver, Respiratory Tract
<b>Chemical Interactions That Change Toxicity:</b>	None Known

**Immediate (Acute) Health Effects by Route of Exposure:**

**Inhalation Irritation:** Can cause moderate respiratory irritation, dizziness, weakness, fatigue, nausea and headache.

**Inhalation Toxicity:** Harmful! Can cause systemic damage (see "Target Organs")Inhalation may cause severe central nervous system depression (including unconsciousness).

**Skin Contact:** Contact causes severe skin irritation and possible burns.

**Skin Absorption:** Harmful if absorbed through the skin. May cause severe irritation and systemic damage.

**Eye Contact:** Contact with the eyes may cause moderate to severe eye injury. Eye contact may result in tearing and reddening, but not likely to permanently injure eye tissue. Temporary vision impairment (cloudy or blurred vision) is possible.

**Ingestion Irritation:** Irritating to mouth, throat, and stomach. Can cause abdominal discomfort, nausea, vomiting and diarrhea.

**Ingestion Toxicity:** Harmful if swallowed. May cause systemic poisoning.

**Long-Term (Chronic) Health Effects:**

**Carcinogenicity:** Contains a probable or known human carcinogen.

**Reproductive and Developmental Toxicity:** No data available to indicate product or any components present at greater than 0.1% may cause birth defects.

**Inhalation:** Upon prolonged and/or repeated exposure, can cause moderate respiratory irritation, dizziness, weakness, fatigue, nausea and headache.Harmful! Can cause systemic damage upon prolonged and/or repeated exposure (see "Target Organs")

**Skin Absorption:** Upon prolonged or repeated exposure, harmful if absorbed through the skin. May cause severe irritation and systemic damage

**Component Toxicological Data:**

**NIOSH:** **CAS No.** **LD50/LC50**

**Chemical Name** Oral LD50 Rat 1900 mg/kg

**o-Terphenyl** Dermal LD50 Rat >2000 mg/kg; Inhalation LC50

**Dichloromethane** Rat 53 mg/L 6 h; Oral LD50 Rat 1600 mg/kg

**Component Carcinogenic Data:**

**OSHA:** **CAS No.**

**Chemical Name**

**Methylene chloride** 75-09-2

25 ppm TWA (8 hr.); 125 ppm STEL (15 min.); 12.5 ppm Action Level (see 29 CFR 1910.1051); effective date for respiratory protection for certain employers to achieve the 8-hour TWA PEL is August 31, 1998; the start up date to install engineering controls is December 10, 1998.; {OSHA - 29 CFR 1910 Specifically Regulate

**ACGIH:** **CAS No.**

**Chemical Name** A3 - Confirmed Animal Carcinogen with

**Dichloromethane** 75-09-2 Unknown Relevance to Humans

**NIOSH:** **CAS No.**

**Chemical Name** potential occupational carcinogen

**Methylene chloride** 75-09-2

**NTP:** **CAS No.**

**Chemical Name**

**No data available**

**IARC:** **CAS No.** **Group No.**

**Chemical Name** 75-09-2 Group 2A

**Monograph 110 [2017];**

**Monograph 71 [1999]**

**12. ECOLOGICAL INFORMATION**

**Overview:** Moderate ecological hazard. This product may be dangerous

**Mobility:**  
**Persistence:**  
**Bioaccumulation:**  
**Degradability:**  
**Ecological Toxicity Data:**

to plants and/or wildlife. Keep out of waterways.  
No data  
No data  
No data  
No data  
No data available

### 13. DISPOSAL CONSIDERATIONS

**Waste Description of Spent Product:**

**Disposal Methods:**

**Waste Disposal of Packaging:**

Spent or discarded material is a hazardous waste. Mixing spent or discarded material with other materials may render the mixture hazardous. Perform a hazardous waste determination on mixtures.  
Incinerate spent or discarded material a permitted hazardous waste facility.  
Comply with all Local, State, Federal, and Provincial Environmental Regulations.

### 14. TRANSPORTATION INFORMATION

**United States:**

**DOT Proper Shipping Name:**

Toxic, liquids, organic, n.o.s. (Dichloromethane, o-Terphenyl)

**UN Number:**

UN2810

**Hazard Class:**

6.1

**Packing Group:**

III

**International:**

**IATA Proper Shipping Name:**

Toxic, liquids, organic, n.o.s. (Dichloromethane, o-Terphenyl)

UN2810

**UN Number:**

6.1

**Hazard Class:**

III

**Packing Group:**

**Marine Pollutant:** No

Chemical Name	CAS#	Marine Pollutant	Severe Marine Pollutant
No data available			

### 15. REGULATORY INFORMATION

**United States:**

This chemical/product is not and cannot be distributed in commerce (as defined in TSCA section 3(5)) or processed (as defined in TSCA section 3(13)) for consumer paint or coating removal.

Chemical Name	CAS#	CERCLA	SARA 313	SARA EHS 313	TSCA
Methylene chloride (dichloromethane)	75-09-2	X	X	-	X
o-terphenyl	84-15-1	-	-	-	X

The following chemicals are listed on CA Prop 65:

Chemical Name	CAS #	Regulation
Dichloromethane	75-09-2	
Dichloromethane (Methylene chloride)	75-09-2	Prop 65 Cancer

**State Right To Know Listing:**

Chemical Name	CAS#	New Jersey	Massachusetts	Pennsylvania	California
Methylene chloride (dichloromethane)	75-09-2	X	X	X	X
o-terphenyl	84-15-1	-	X	-	-

## 16. OTHER INFORMATION

---

**Prior Version Date:** 04/27/23

**Other Information:** Any changes to the SDS compared to previous versions are marked by a vertical line in front of the concerned paragraph.

**References:**

No data available

**Disclaimer:**

Restek Corporation provides the descriptions, data and information contained herein in good faith but makes no representation as to its comprehensiveness or accuracy. It is provided for your guidance only. Because many factors may affect processing or application/use, Restek Corporation recommends you perform an assessment to determine the suitability of a product for your particular purpose prior to use. No warranties of any kind, either expressed or implied, including fitness for a particular purpose, are made regarding products described, data or information set forth. In no case shall the descriptions, information, or data provided be considered a part of our terms and conditions of sale. Further, the descriptions, data and information furnished hereunder are given gratis. No obligation or liability for the description, data and information given are assumed. All such being given and accepted at your risk.



## CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Belleville, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31480

Lot No.: A0196246

Description : MA Fractionation Surrogate Spike Mix

MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : February 28, 2029

Storage: 10°C or colder

Handling: Sonication required. Mix is

photosensitive.

P12665  
↓  
P12684 } 7-P  
07/19/23

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L., K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,025.1 µg/mL	+/- 181.3135
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,021.1 µg/mL	+/- 181.1342

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%



## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

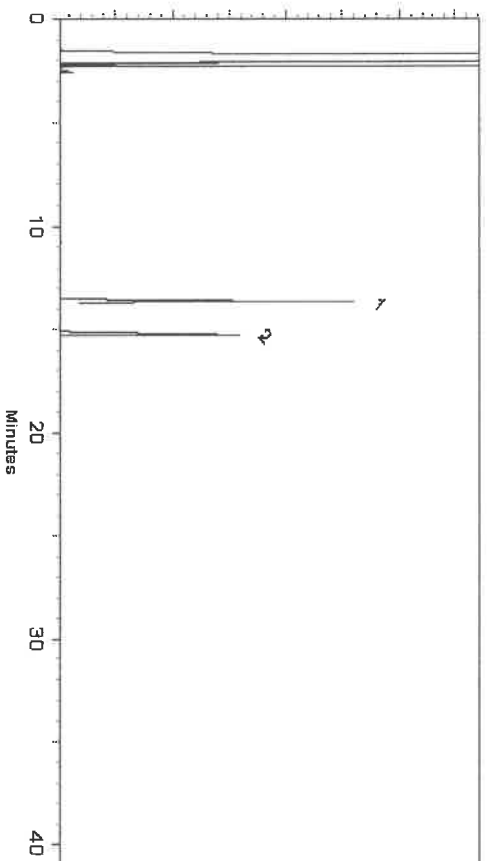

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

**Stacey Wanner - Operations Technician I**  
  


**Date Mixed:** 24-Mar-2023

**Balance Serial #** 1128360905

**Date Passed:** 28-Mar-2023

**Jennifer Polino - Operations Tech III - ARM QC**

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





## CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Belleville, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31480

Lot No.: A0196246

Description : MA Fractionation Surrogate Spike Mix

MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : February 28, 2029

Storage: 10°C or colder

Handling: Sonication required. Mix is

photosensitive.

P12665  
↓  
P12684 } 7-P  
07/19/23

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L., K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,025.1 µg/mL	+/- 181.3135
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,021.1 µg/mL	+/- 181.1342

\* Expanded Uncertainty displayed in same units as Grav. Conc.


Solvent: Hexane

CAS # 110-54-3

Purity 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)  
**Carrier Gas:**  
hydrogen-constant pressure 10 psi.  
**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)  
**Inj. Temp:**  
250°C  
**Det. Temp:**  
330°C  
**Det. Type:**  
FID  
**Split Vent:**  
2 ml/min.  
**Inj. Vol**  
1µl

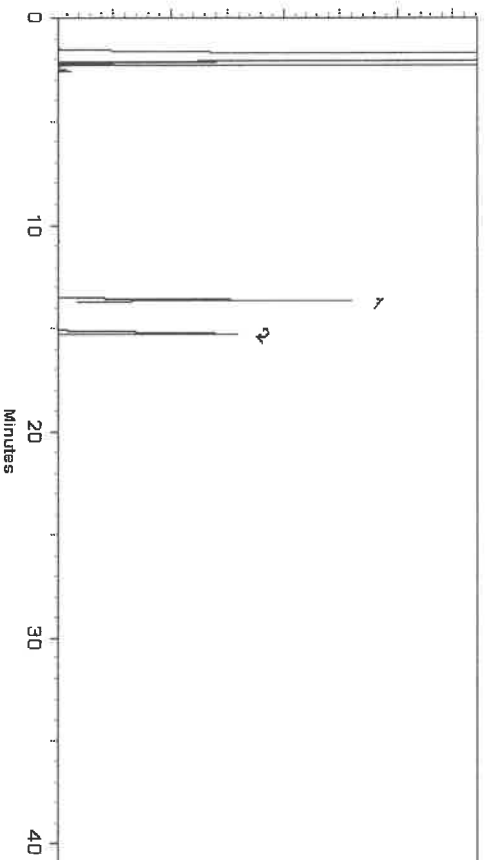

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

**Stacey Wanner - Operations Technician I**  
  


**Date Mixed:** 24-Mar-2023  
**Balance Serial #** 1128360905  
**Date Passed:** 28-Mar-2023

**Jennifer Polino - Operations Tech III - ARM QC**

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





## CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Belleville, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31480

Lot No.: A0196246

Description : MA Fractionation Surrogate Spike Mix

MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : February 28, 2029

Storage: 10°C or colder

Handling: Sonication required. Mix is

photosensitive.

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L., K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,025.1 µg/mL	+/- 181.3135
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,021.1 µg/mL	+/- 181.1342

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

P12665  
↓  
P12684 } 7-P  
07/19/23



## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

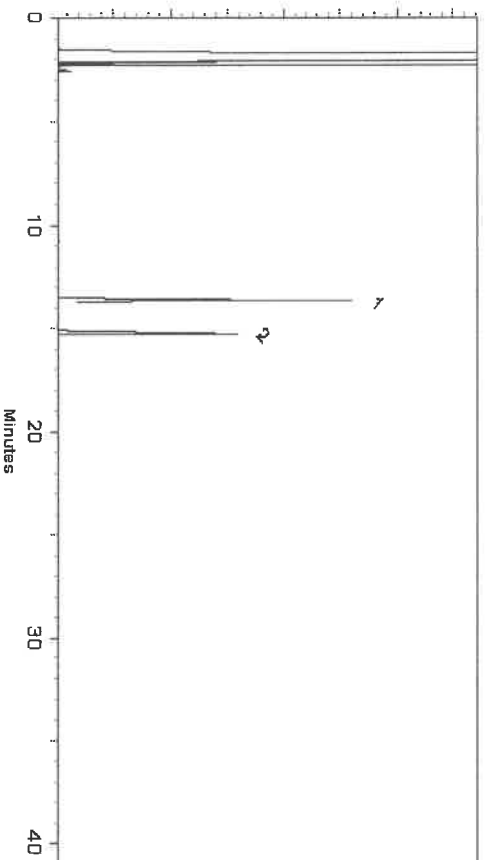

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

**Stacey Wanner - Operations Technician I**  
  


Date Mixed: 24-Mar-2023

Balance Serial # 1128360905

**Jennifer Polino - Operations Tech III - ARM QC**

Date Passed: 28-Mar-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





## CERTIFIED REFERENCE MATERIAL

110 Benner Circle

Belleville, PA 16823-8812

Tel: 1-814-353-1300

Fax: 1-814-353-1309

[www.restek.com](http://www.restek.com)

## Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31480

Lot No.: A0196246

Description : MA Fractionation Surrogate Spike Mix

MA Fractionation Surrogate Spike Mix 4000µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : February 28, 2029

Storage: 10°C or colder

Handling: Sonication required. Mix is

photosensitive.

P12665  
↓  
P12684 } 7-P  
07/19/23

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L., K=2)
1	2-Fluorobiphenyl	321-60-8	00021384	99%	4,025.1 µg/mL	+/- 181.3135
2	2-Bromonaphthalene	580-13-2	STBC5362V	99%	4,021.1 µg/mL	+/- 181.1342

\* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

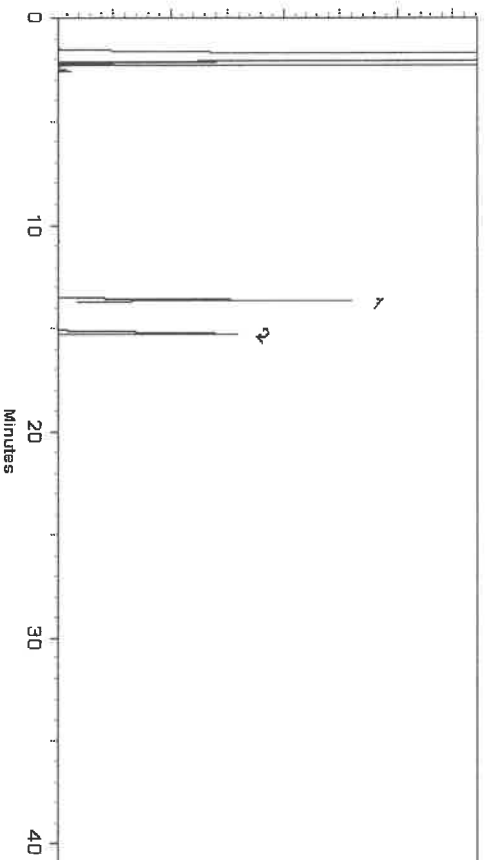

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

**Stacey Wanner - Operations Technician I**  
  


Date Mixed: 24-Mar-2023

Balance Serial # 1128360905

**Jennifer Polino - Operations Tech III - ARM QC**

Date Passed: 28-Mar-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

*k* is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





## CERTIFIED REFERENCE MATERIAL

110 Benner Circle

Bellefonte, PA 16823-8812

Tel: (800)356-1688

Fax: (814)353-1309

[www.restek.com](http://www.restek.com)

## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31098

Lot No.: A0183404

Description : 1-Chlorooctadecane Standard

1-Chlorooctadecane Standard 10,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : April 30, 2029

Storage: 10°C or colder

Ship: Ambient

42166  
✓ Y.P.  
P2166 11/14/22

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	µg/mL	Gravimetric
1	1-Chlorooctadecane CAS # 3386-33-2 Purity 99%	(Lot 12882200)  10,051.0 µg/mL	+/- 58.4374 +/- 563.5496 +/- 576.7359	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%



**Column:**

30m x 0.25mm x 0.25µm  
Rx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

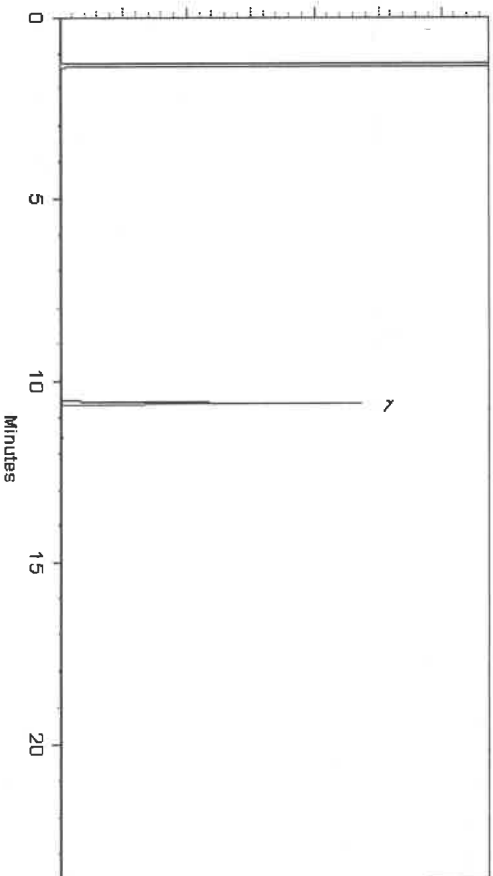

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Brittany Federin*  
**Brittany Federin** - Operations Tech I

**Date Mixed:** 28-Mar-2022

**Balance:** 1128353505

*Maureen Cowan*  
**Maureen Cowan** - Operations Tech I

**Date Passed:** 31-Mar-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

