



2-Nitrophenol

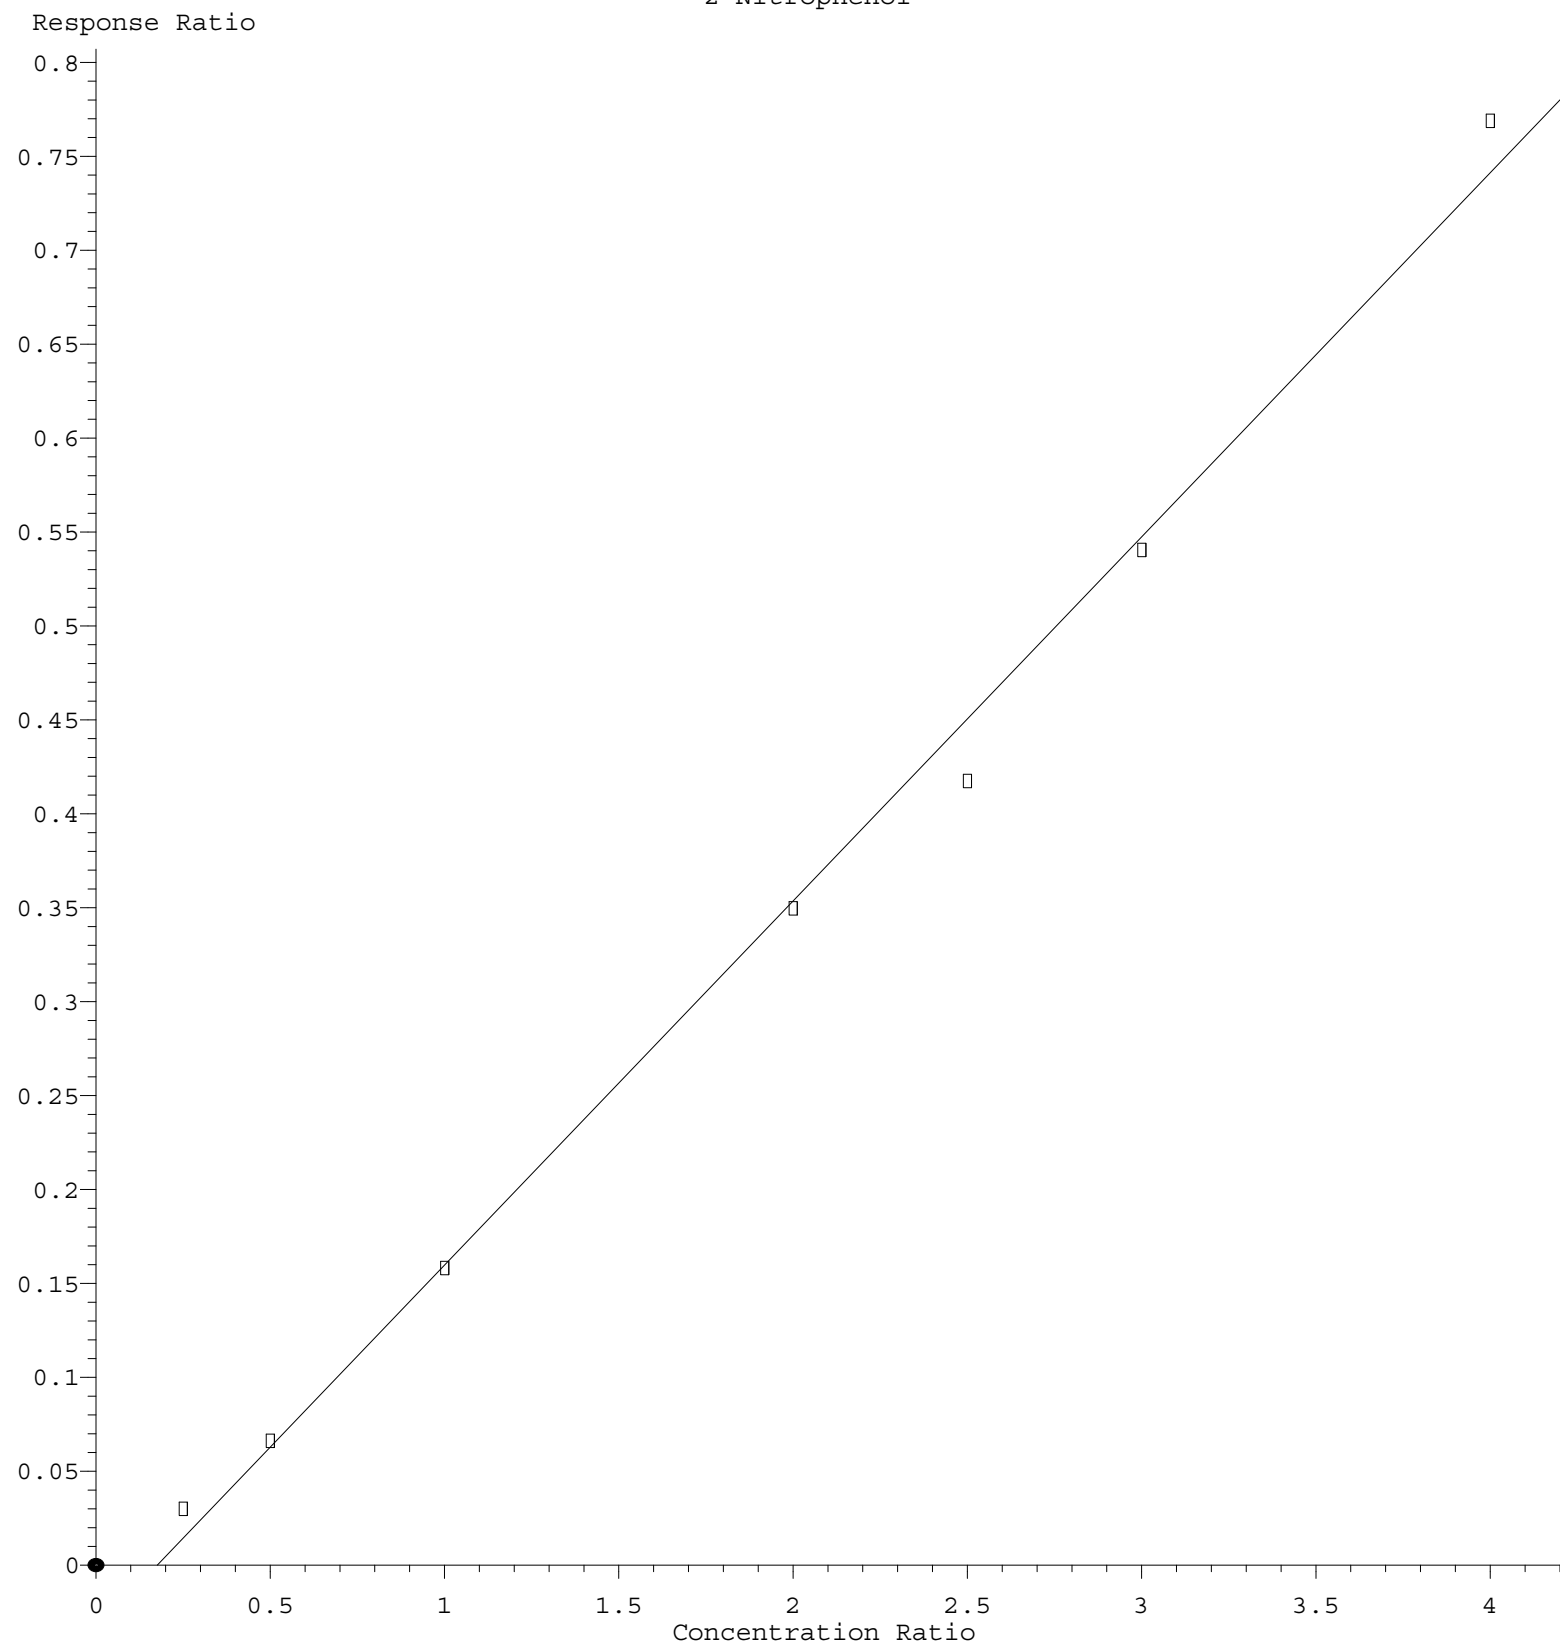

Response = 1.939e-001 * Amt - 3.410e-002
 Coef of Det (r^2) = 0.994980 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM103023.M
 Calibration Table Last Updated: Tue Oct 31 02:55:18 2023

Dibenzo (a,h) anthracene

Response Ratio

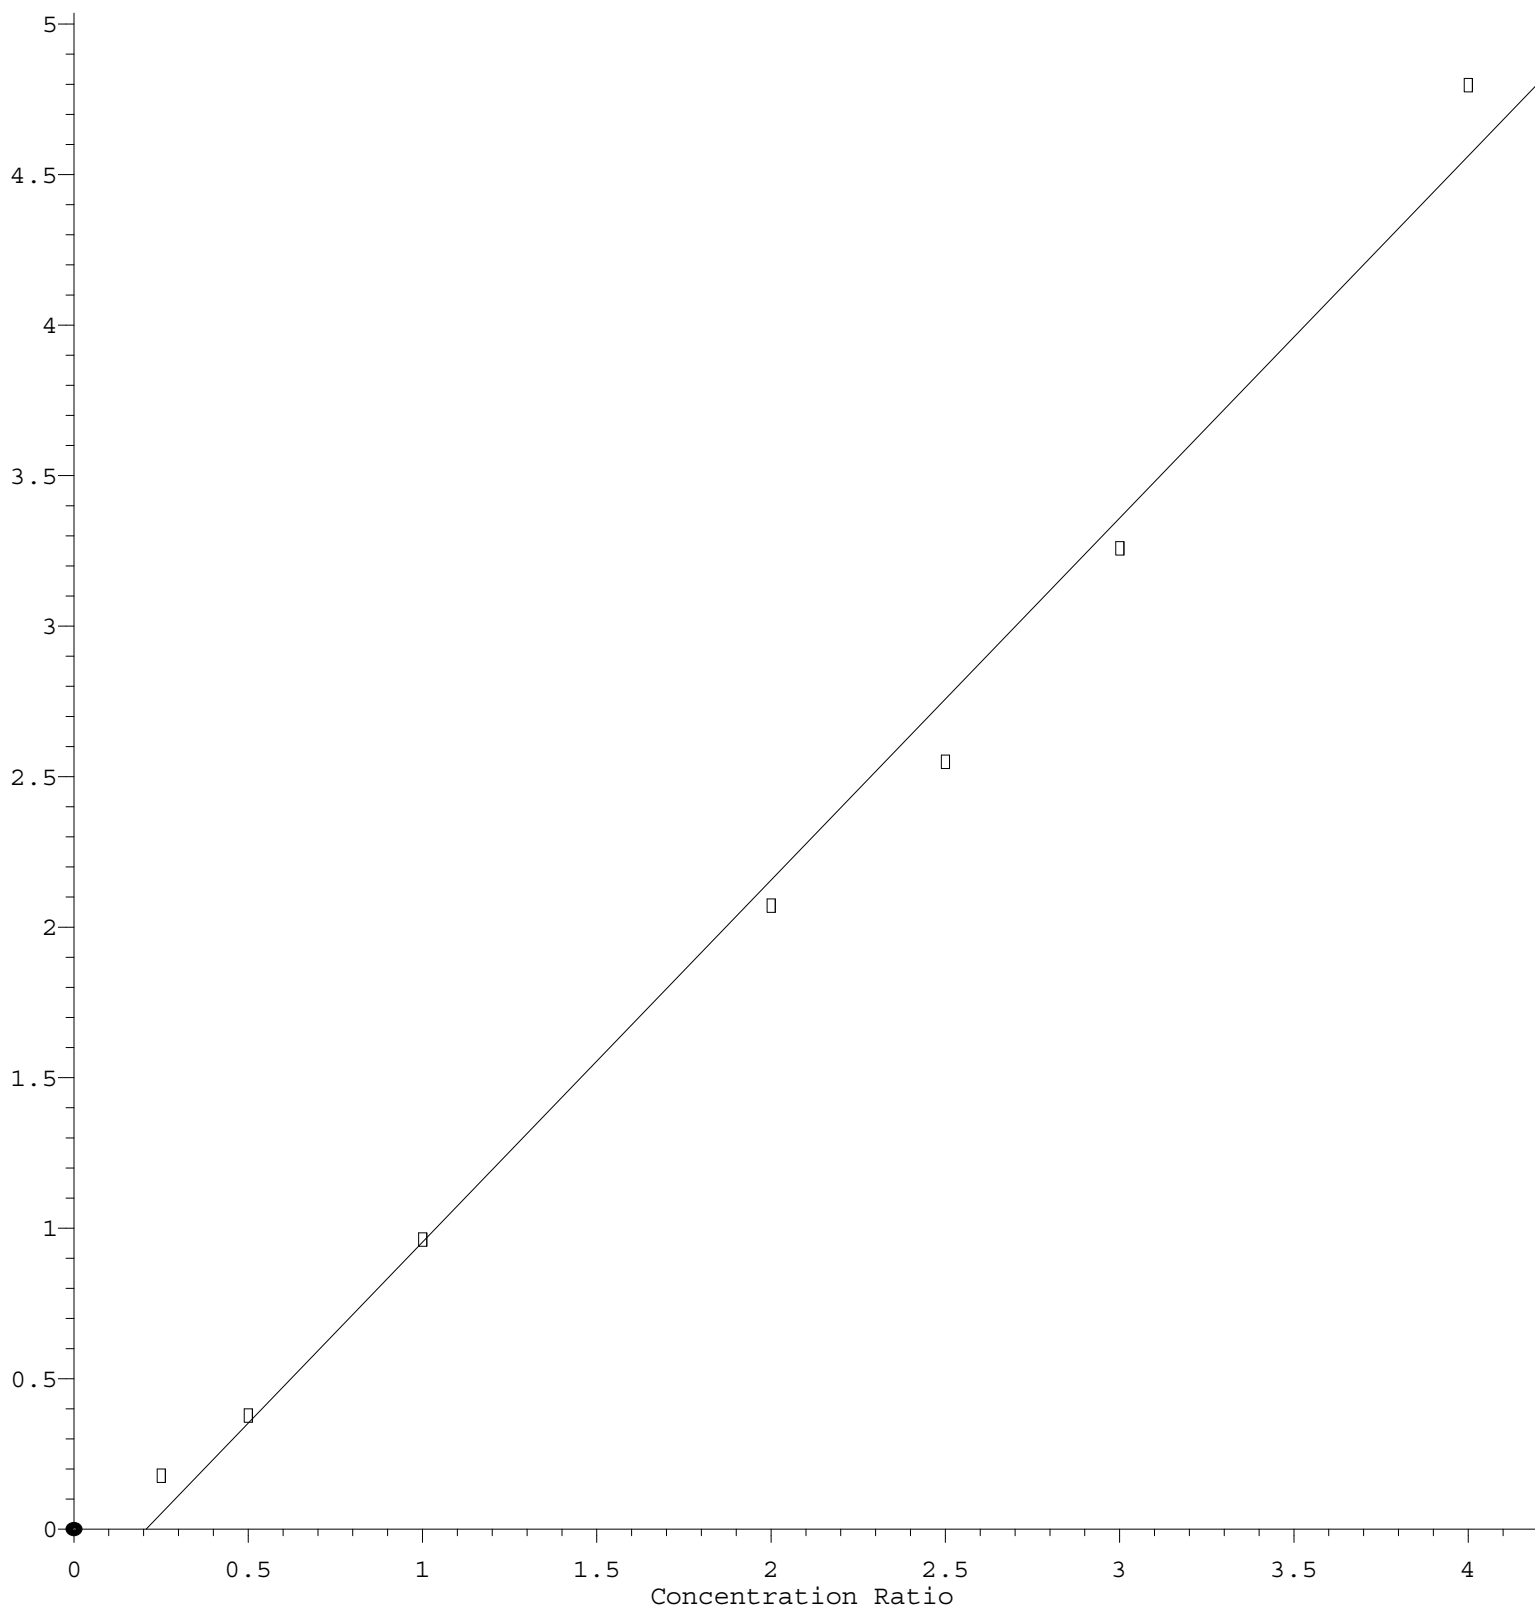


$$\text{Response} = 1.203\text{e}+000 * \text{Amt} - 2.488\text{e}-001$$

Coef of Det (r^2) = 0.992070 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM103023.M

Calibration Table Last Updated: Tue Oct 31 02:55:18 2023


4,6-Dinitro-2-methylphenol

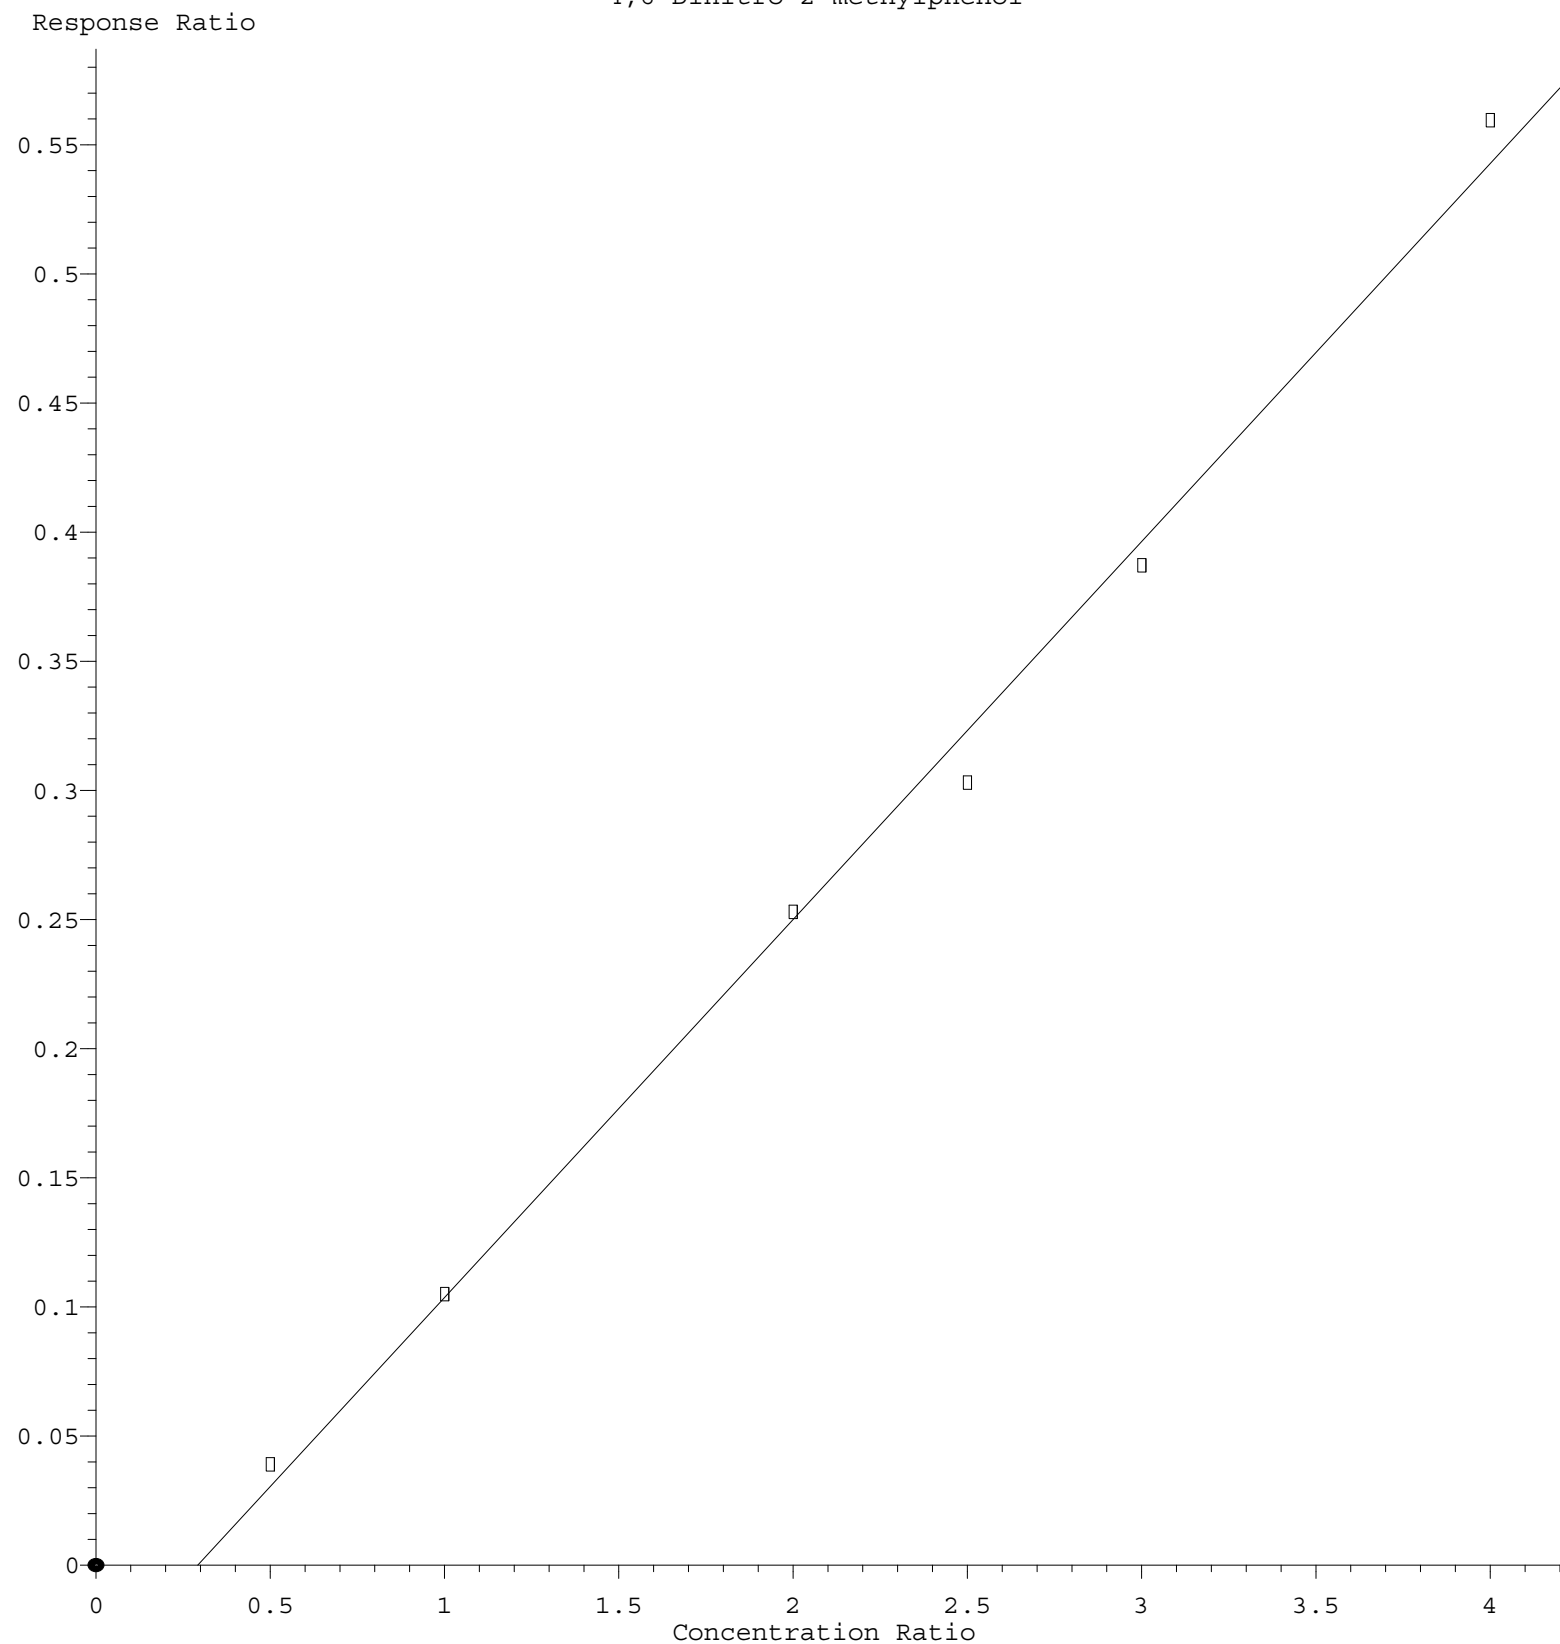

Response = $1.464 \times 10^{-1} \times \text{Amt} - 4.270 \times 10^{-2}$
 Coef of Det (r^2) = 0.995211 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM103023.M
 Calibration Table Last Updated: Tue Oct 31 02:55:18 2023

4-Nitroaniline

Response Ratio

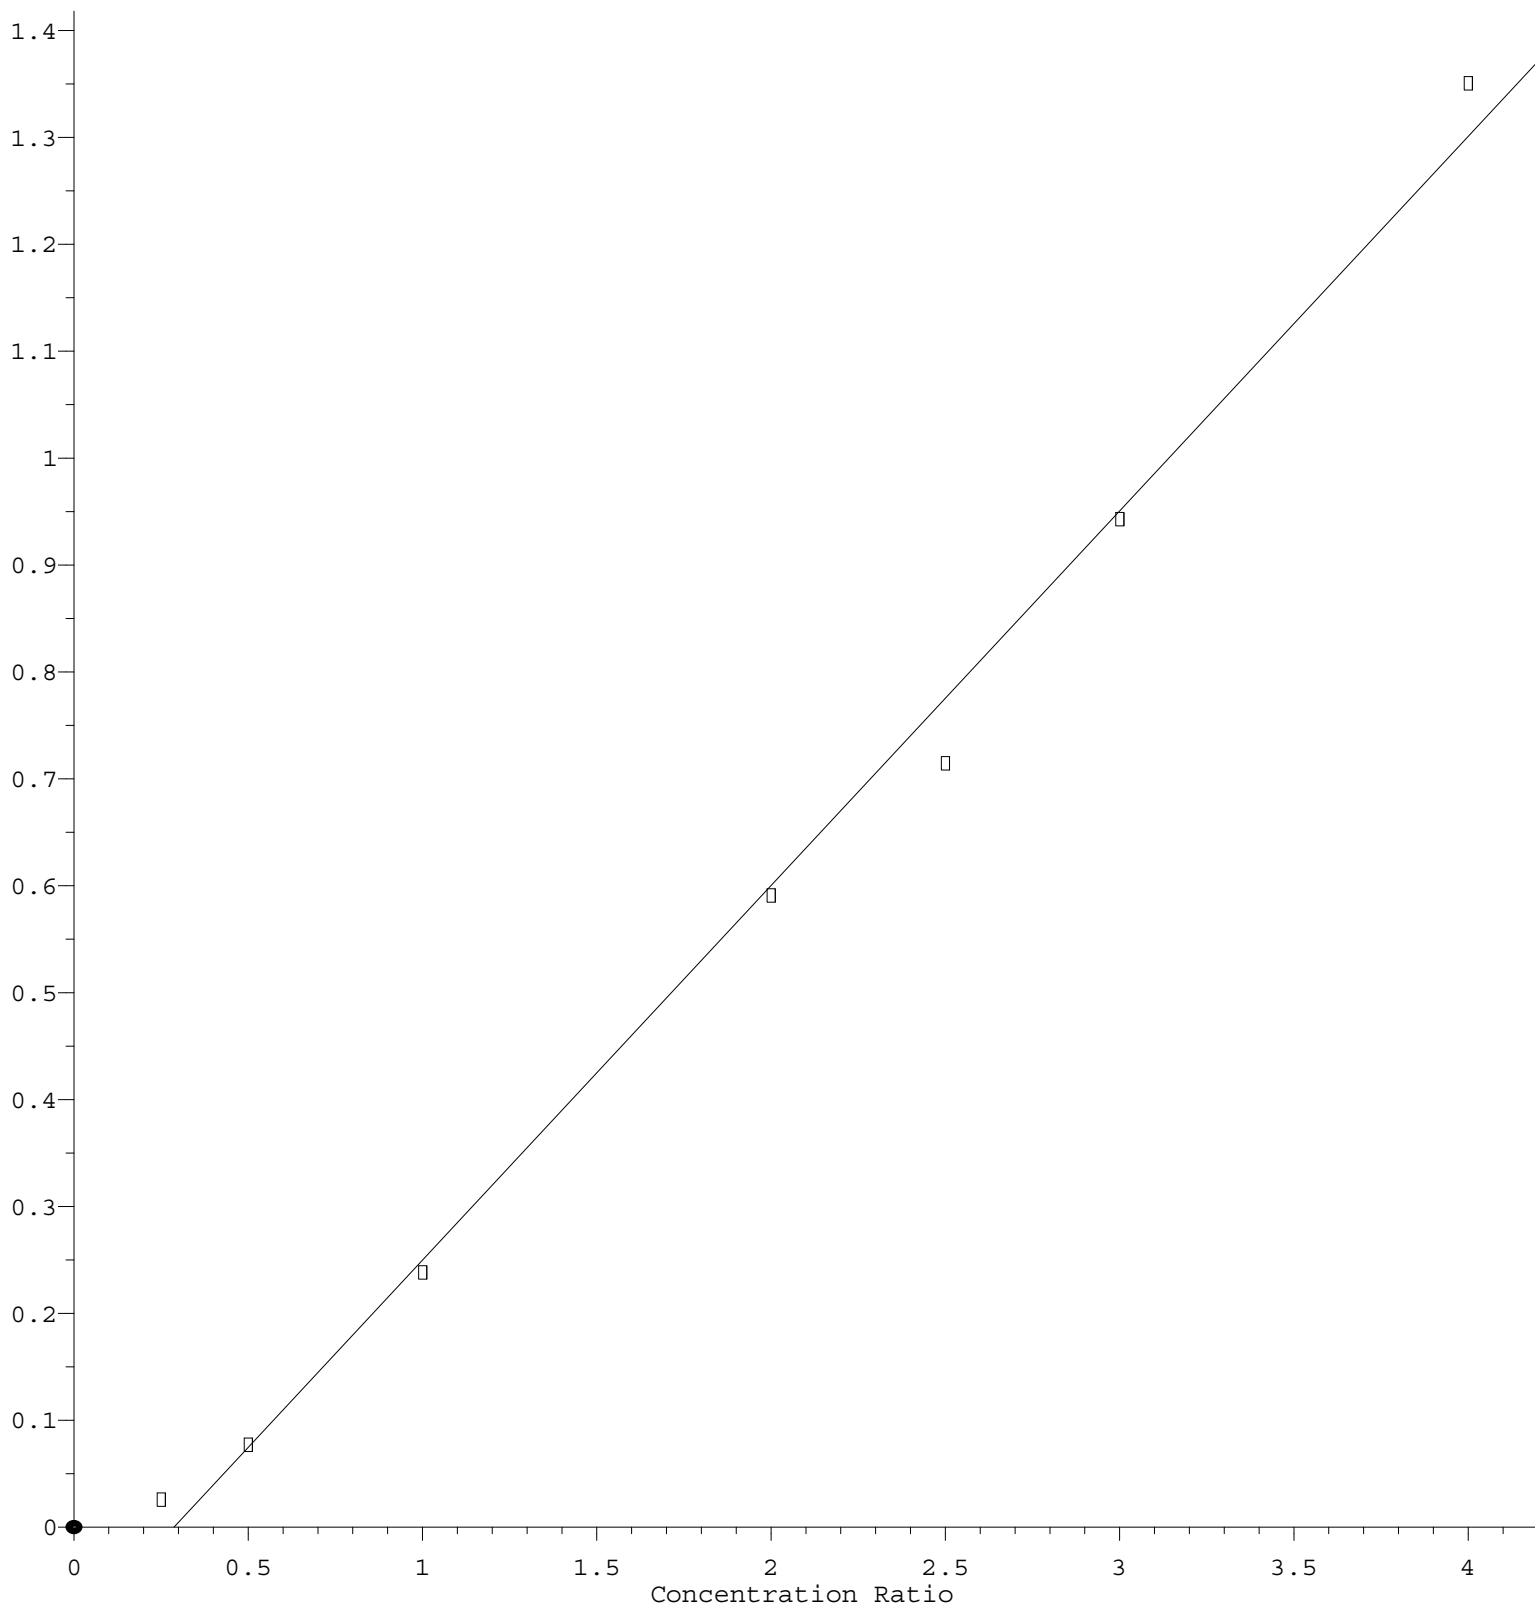

$$\text{Response} = 3.505\text{e-}001 * \text{Amt} - 1.006\text{e-}001$$


Coef of Det (r^2) = 0.994394 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM103023.M

Calibration Table Last Updated: Tue Oct 31 02:55:18 2023

2,4-Dinitrotoluene

Response Ratio

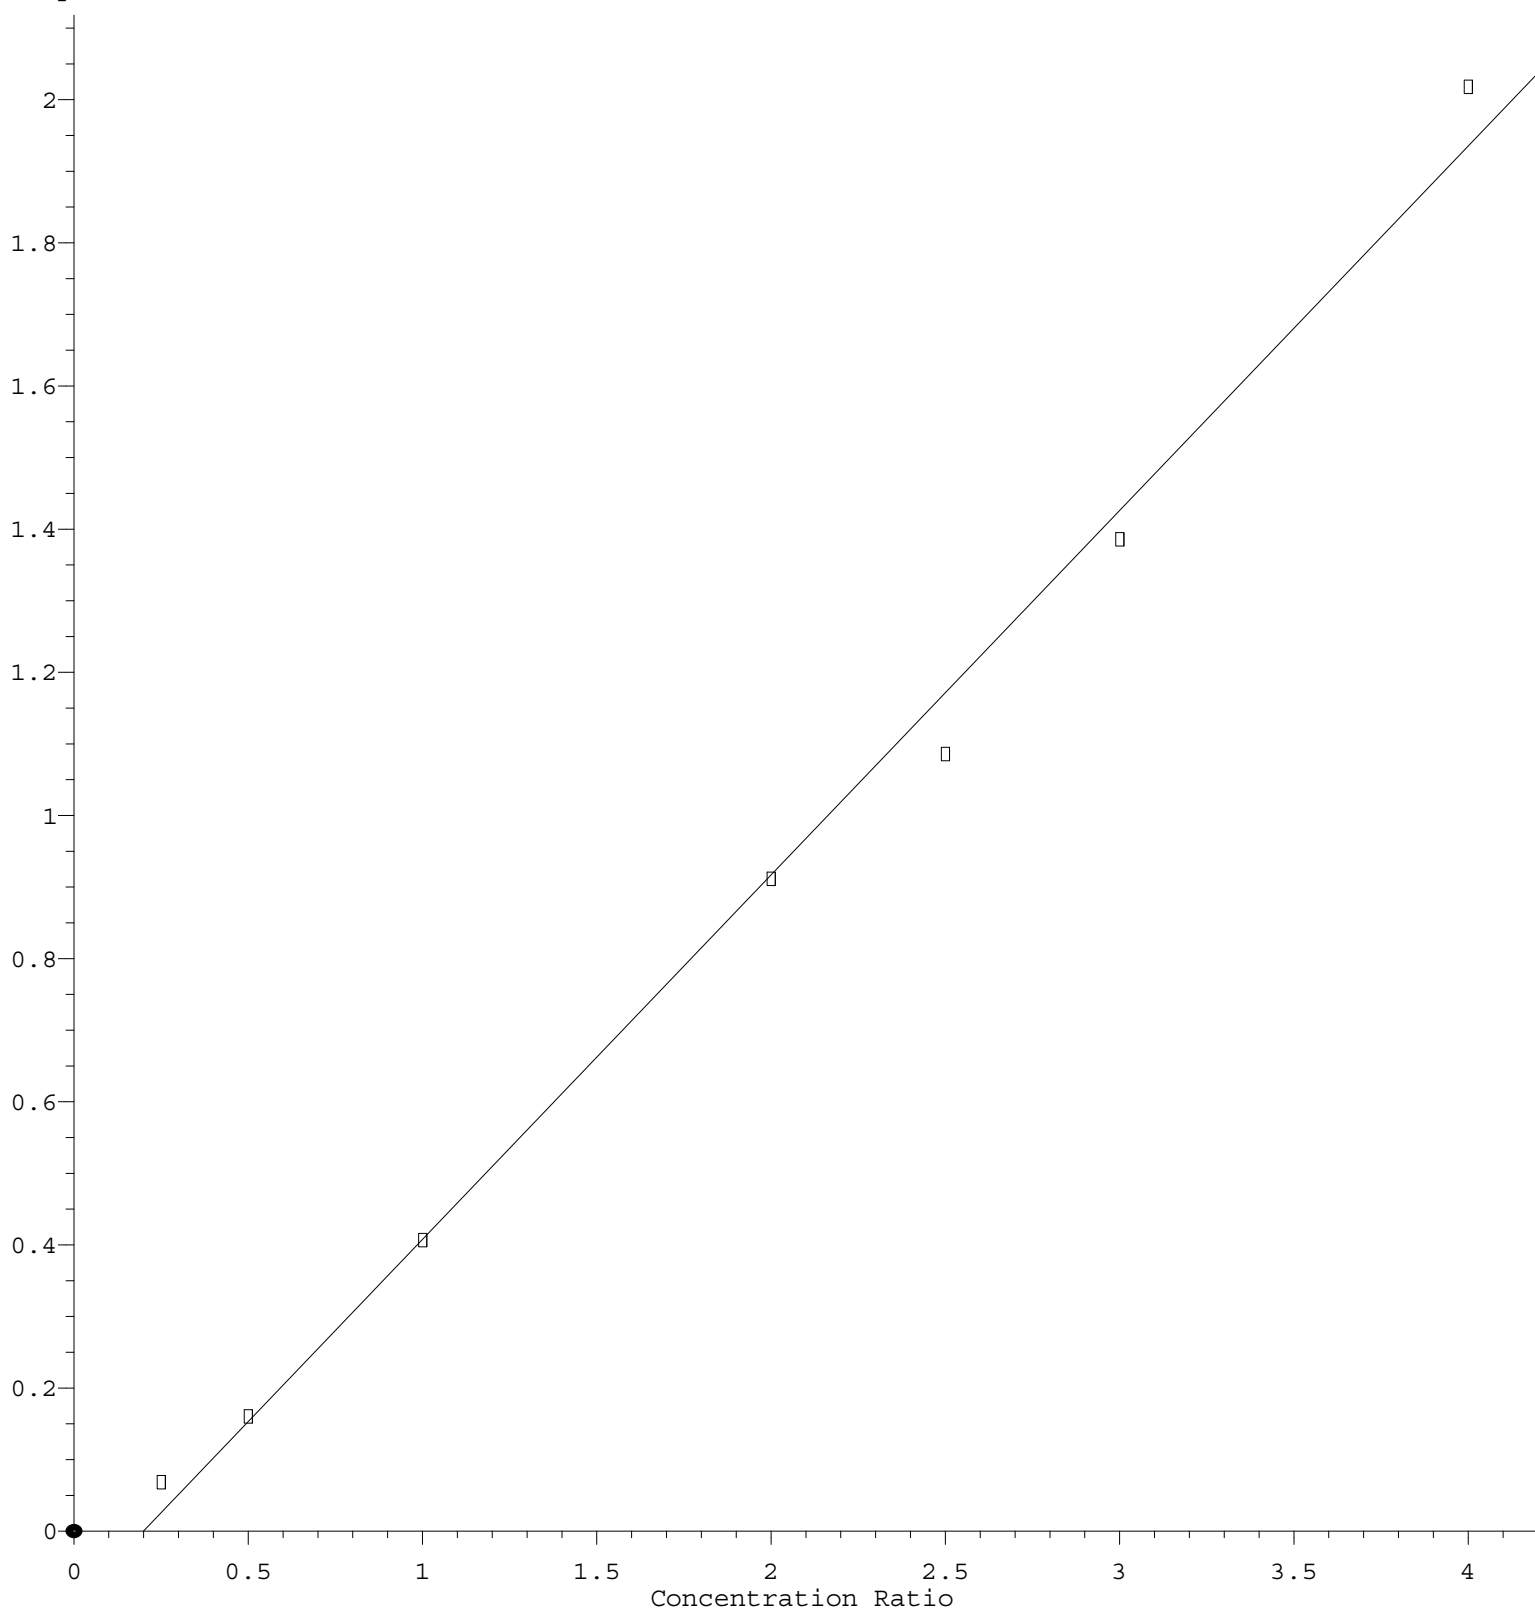

$$\text{Response} = 5.090\text{e-}001 * \text{Amt} - 1.011\text{e-}001$$


Coef of Det (r^2) = 0.994084 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM103023.M

Calibration Table Last Updated: Tue Oct 31 02:55:18 2023

4-Nitrophenol

Response Ratio

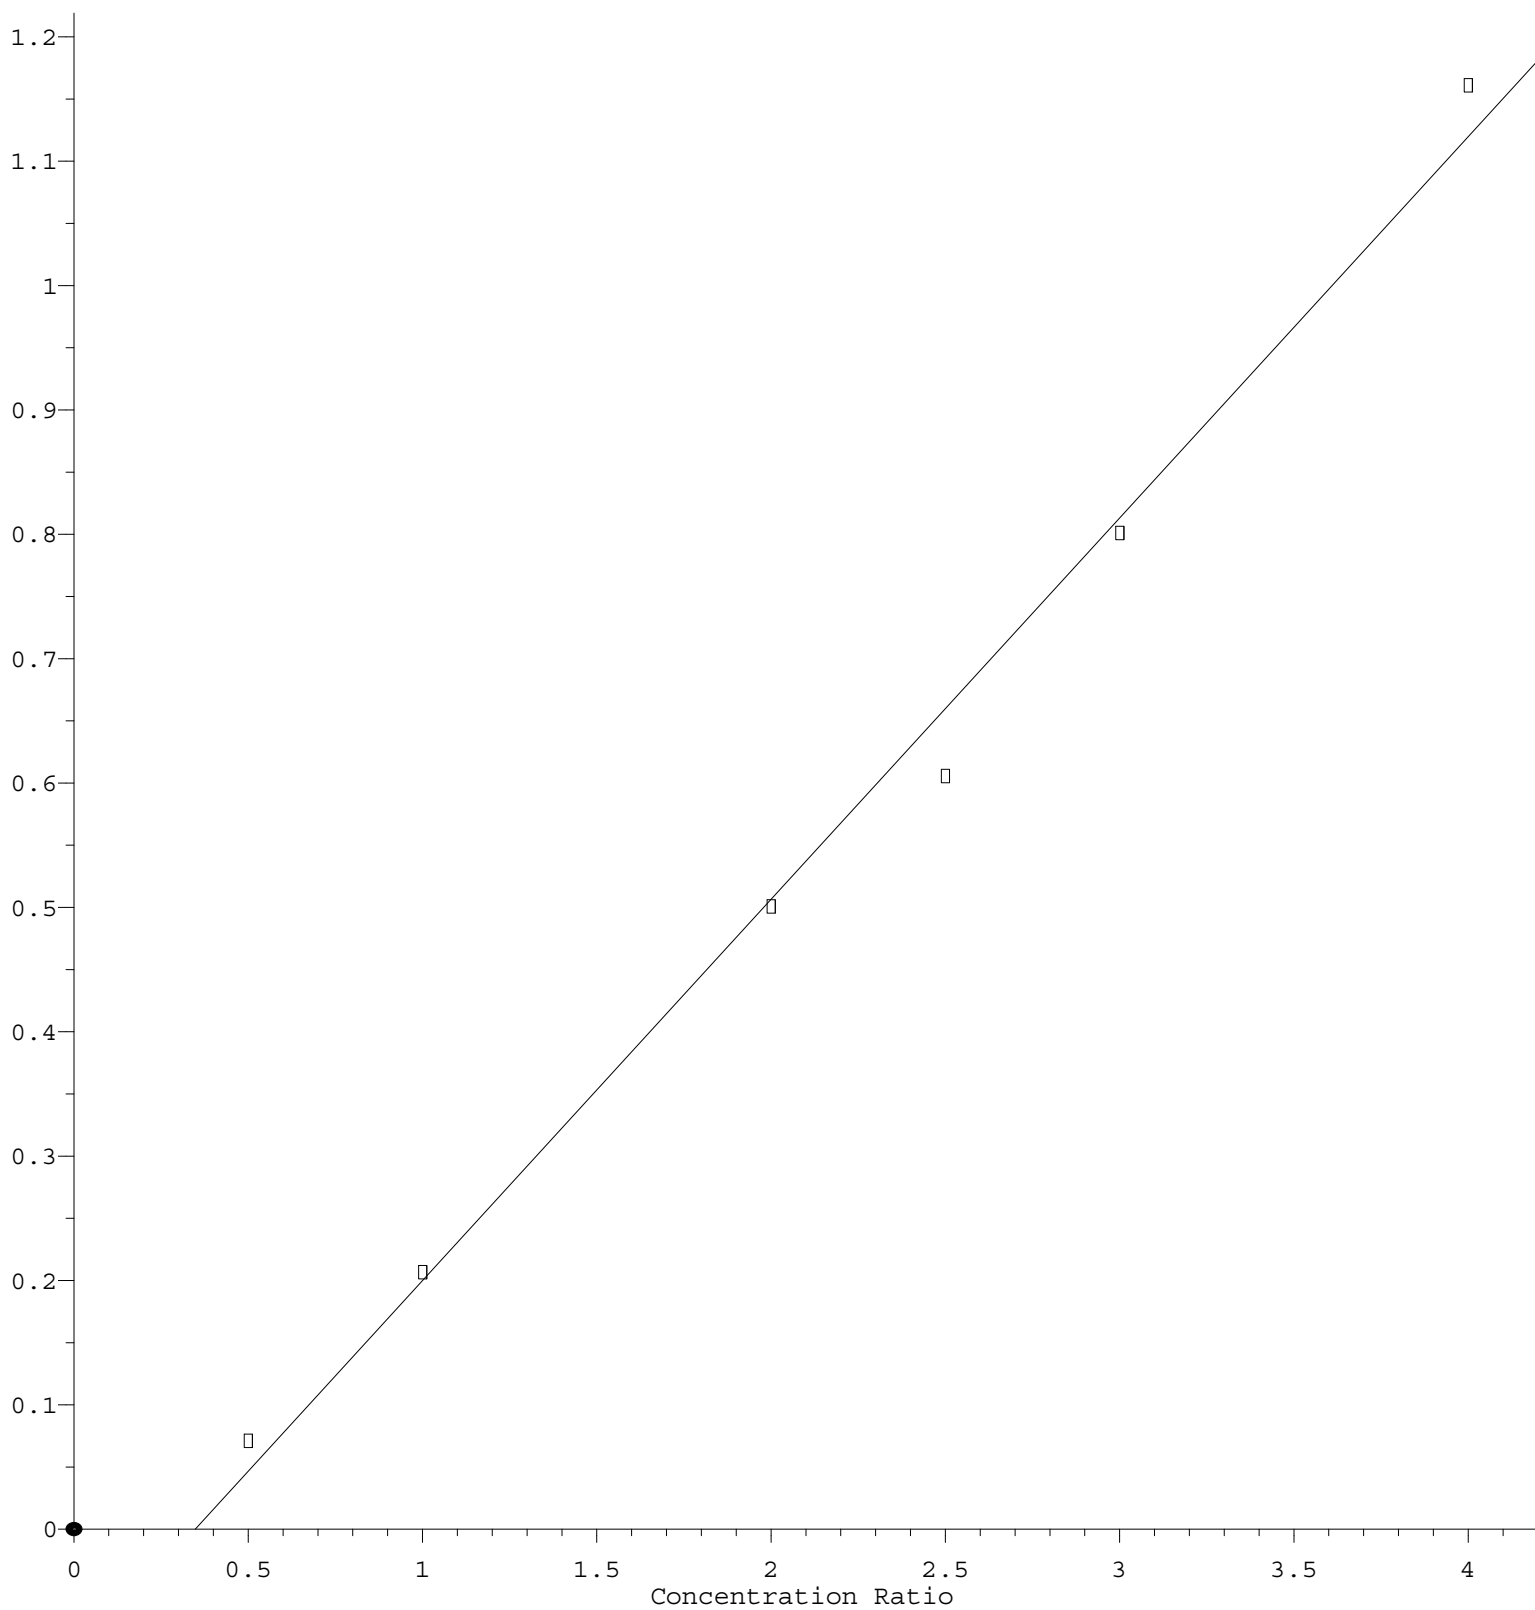

$$\text{Response} = 3.066\text{e-}001 * \text{Amt} - 1.066\text{e-}001$$


Coef of Det (r^2) = 0.993073 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM103023.M

Calibration Table Last Updated: Tue Oct 31 02:55:18 2023

2,4-Dinitrophenol

Response Ratio

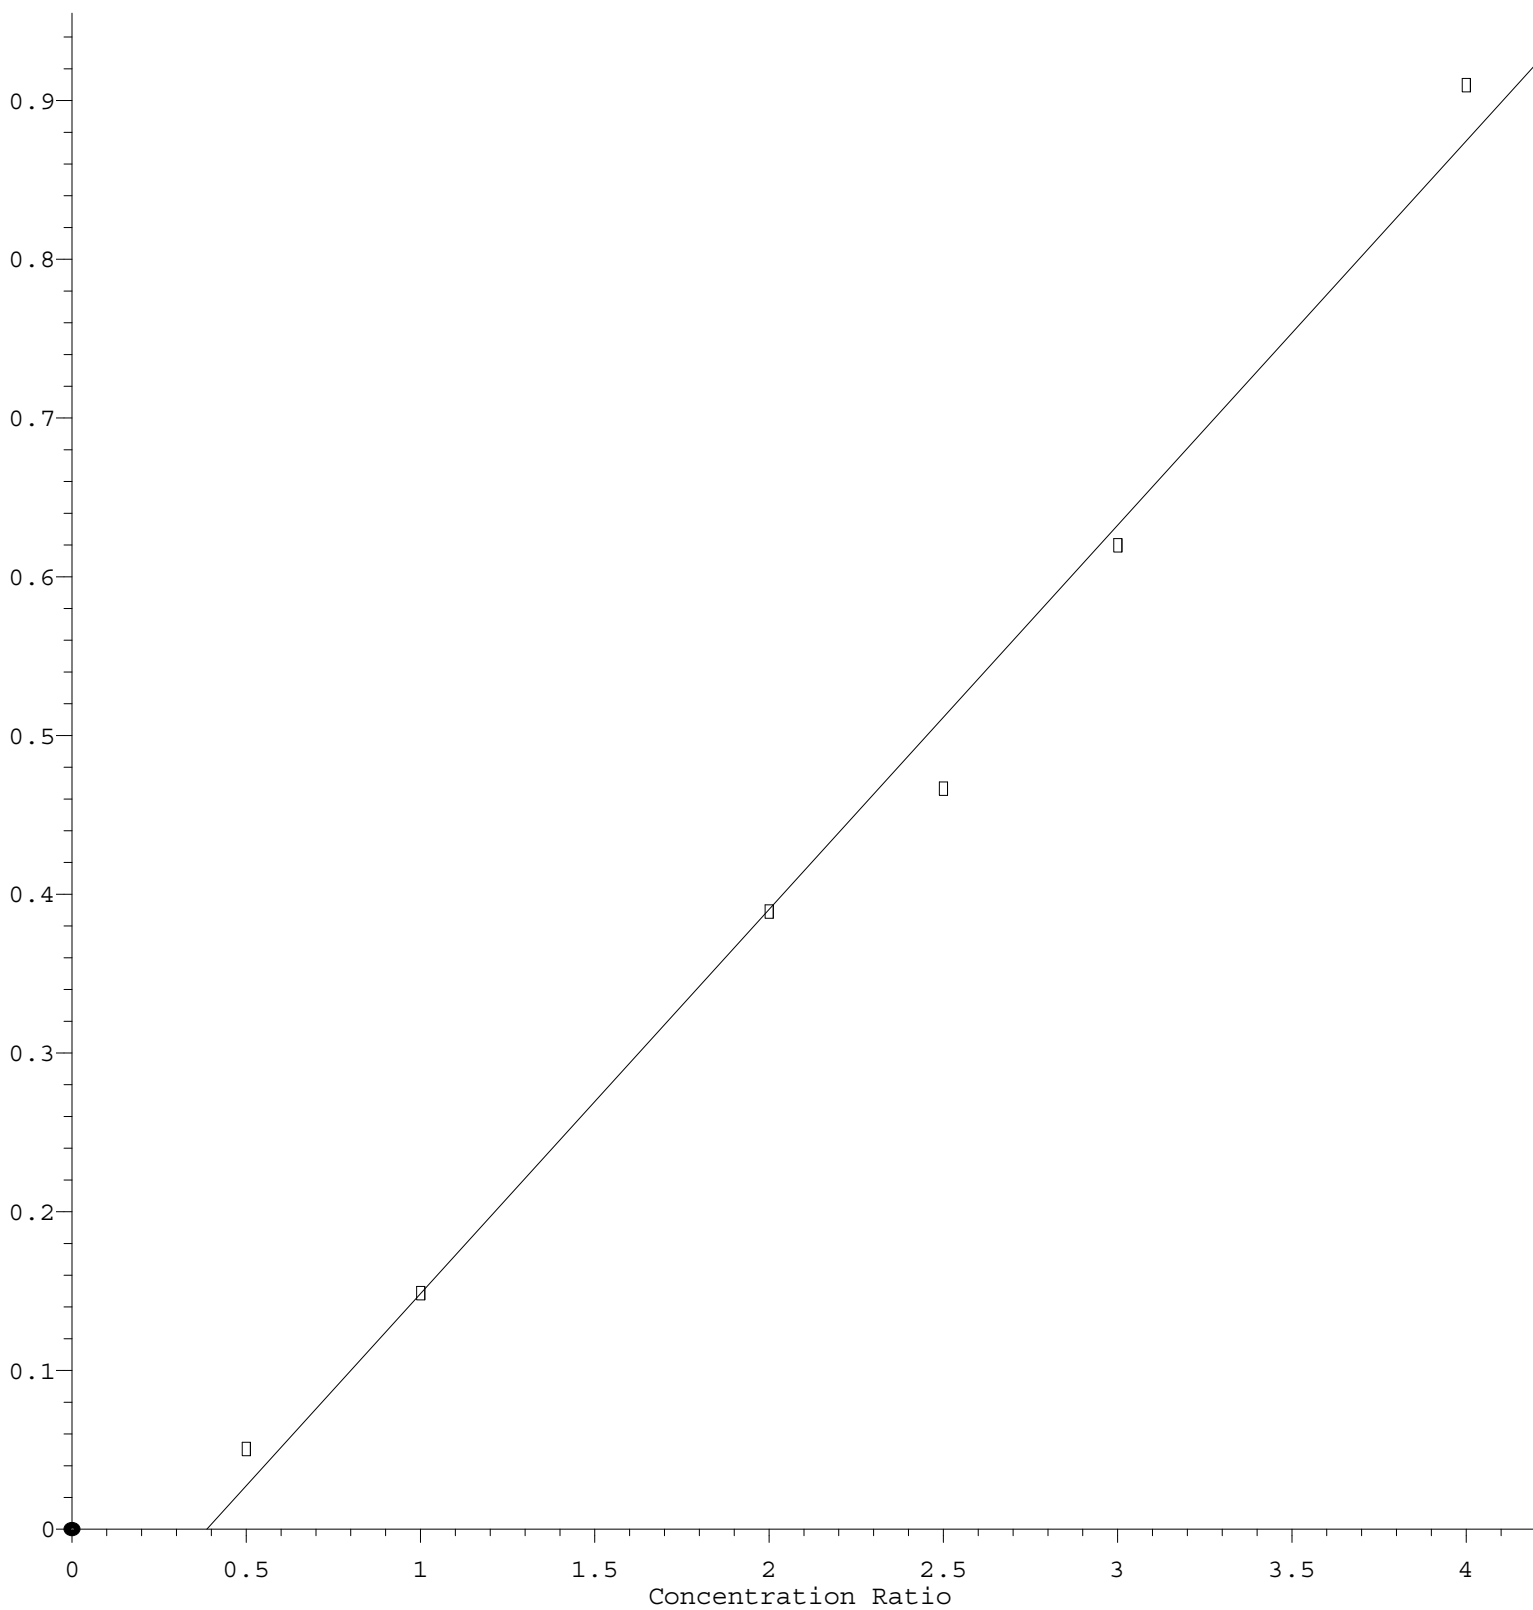

$$\text{Response} = 2.420\text{e-}001 * \text{Amt} - 9.376\text{e-}002$$


Coef of Det (r^2) = 0.991969 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM103023.M

Calibration Table Last Updated: Tue Oct 31 02:55:18 2023

3-Nitroaniline

Response Ratio

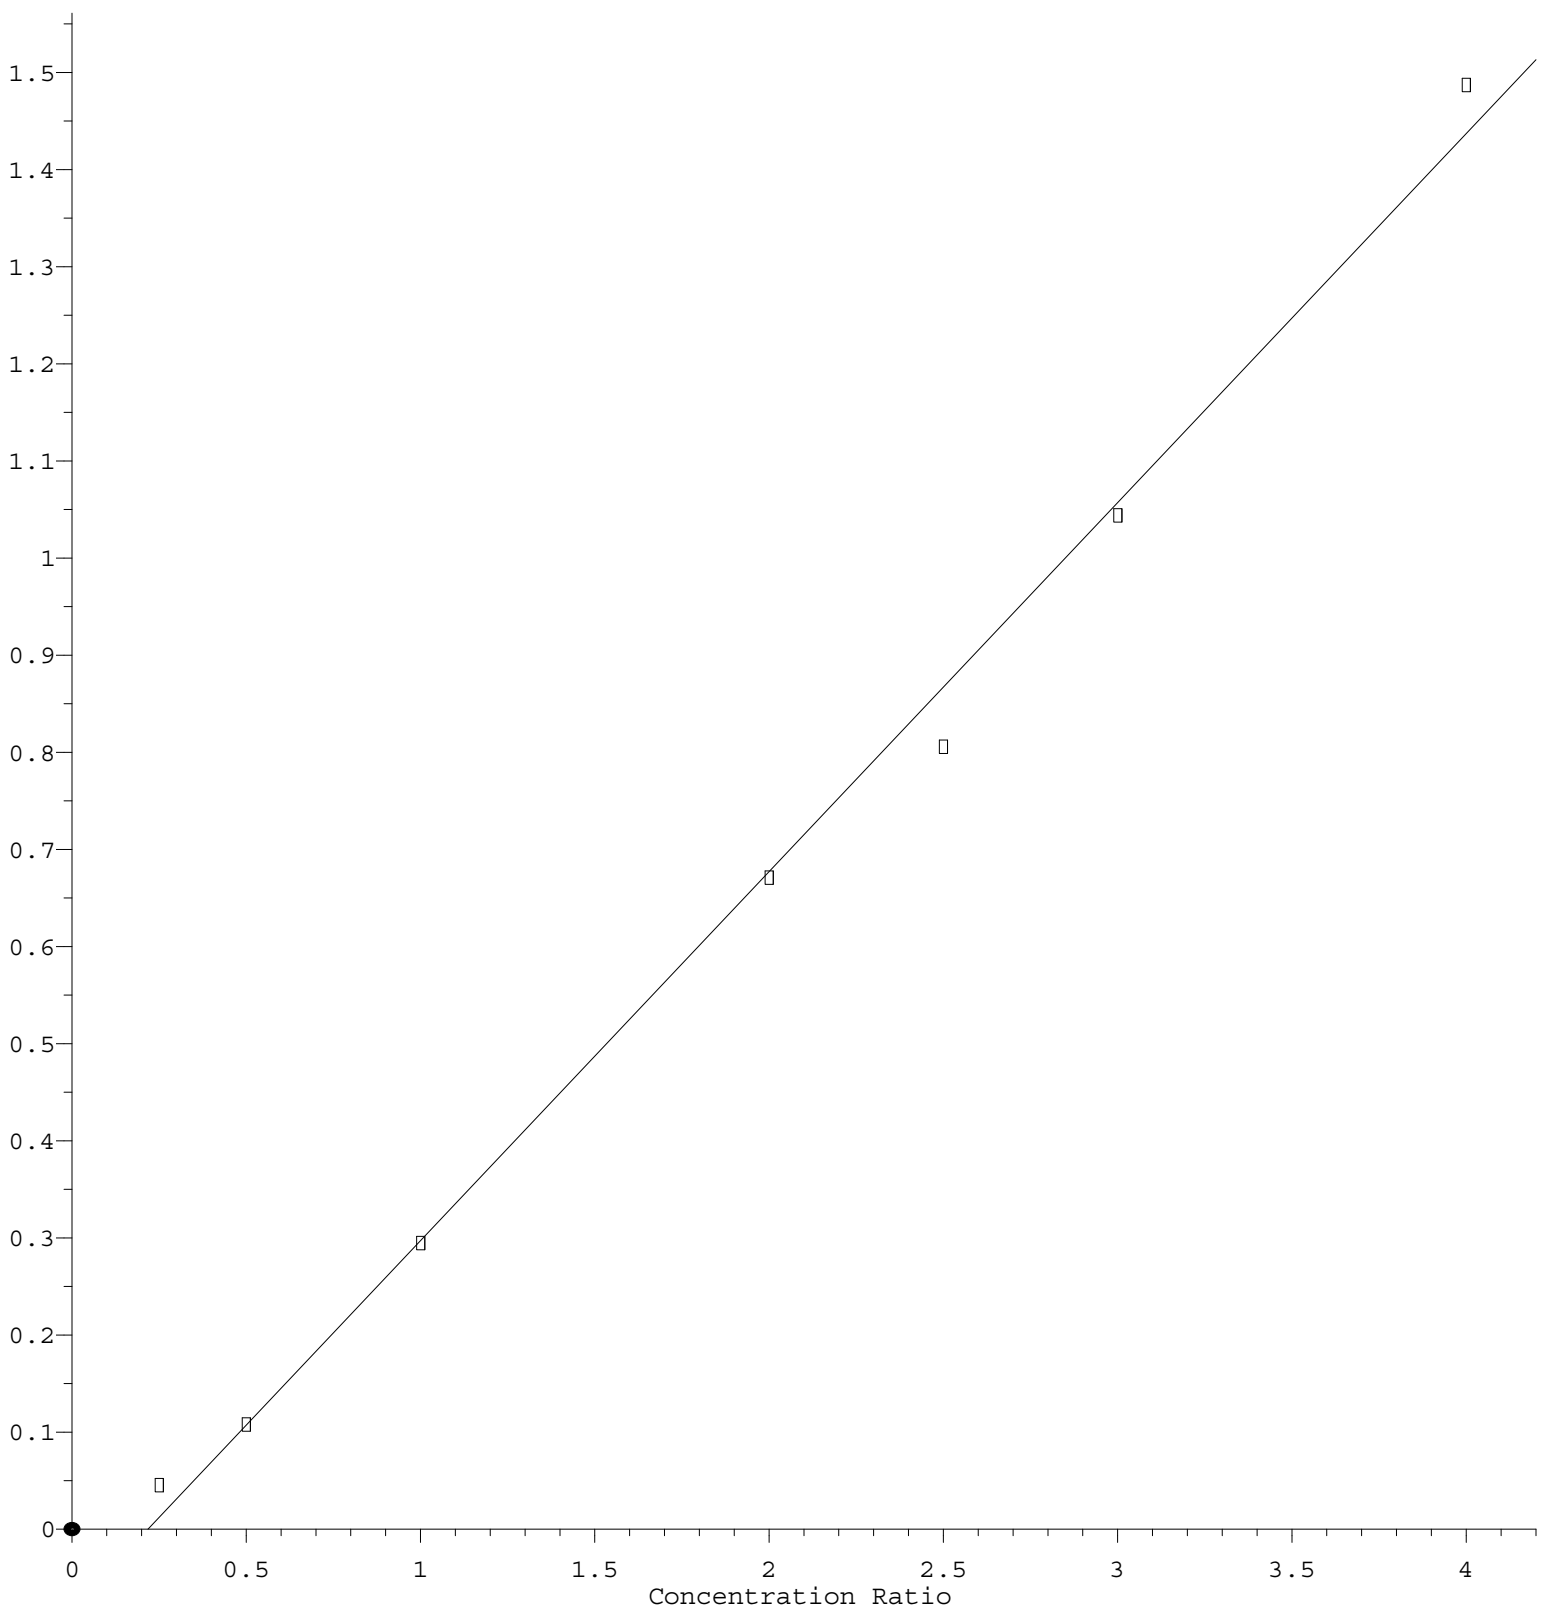

$$\text{Response} = 3.799\text{e-}001 * \text{Amt} - 8.267\text{e-}002$$


Coef of Det (r^2) = 0.995441 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM103023.M

Calibration Table Last Updated: Tue Oct 31 02:55:18 2023

2-Nitroaniline

Response Ratio

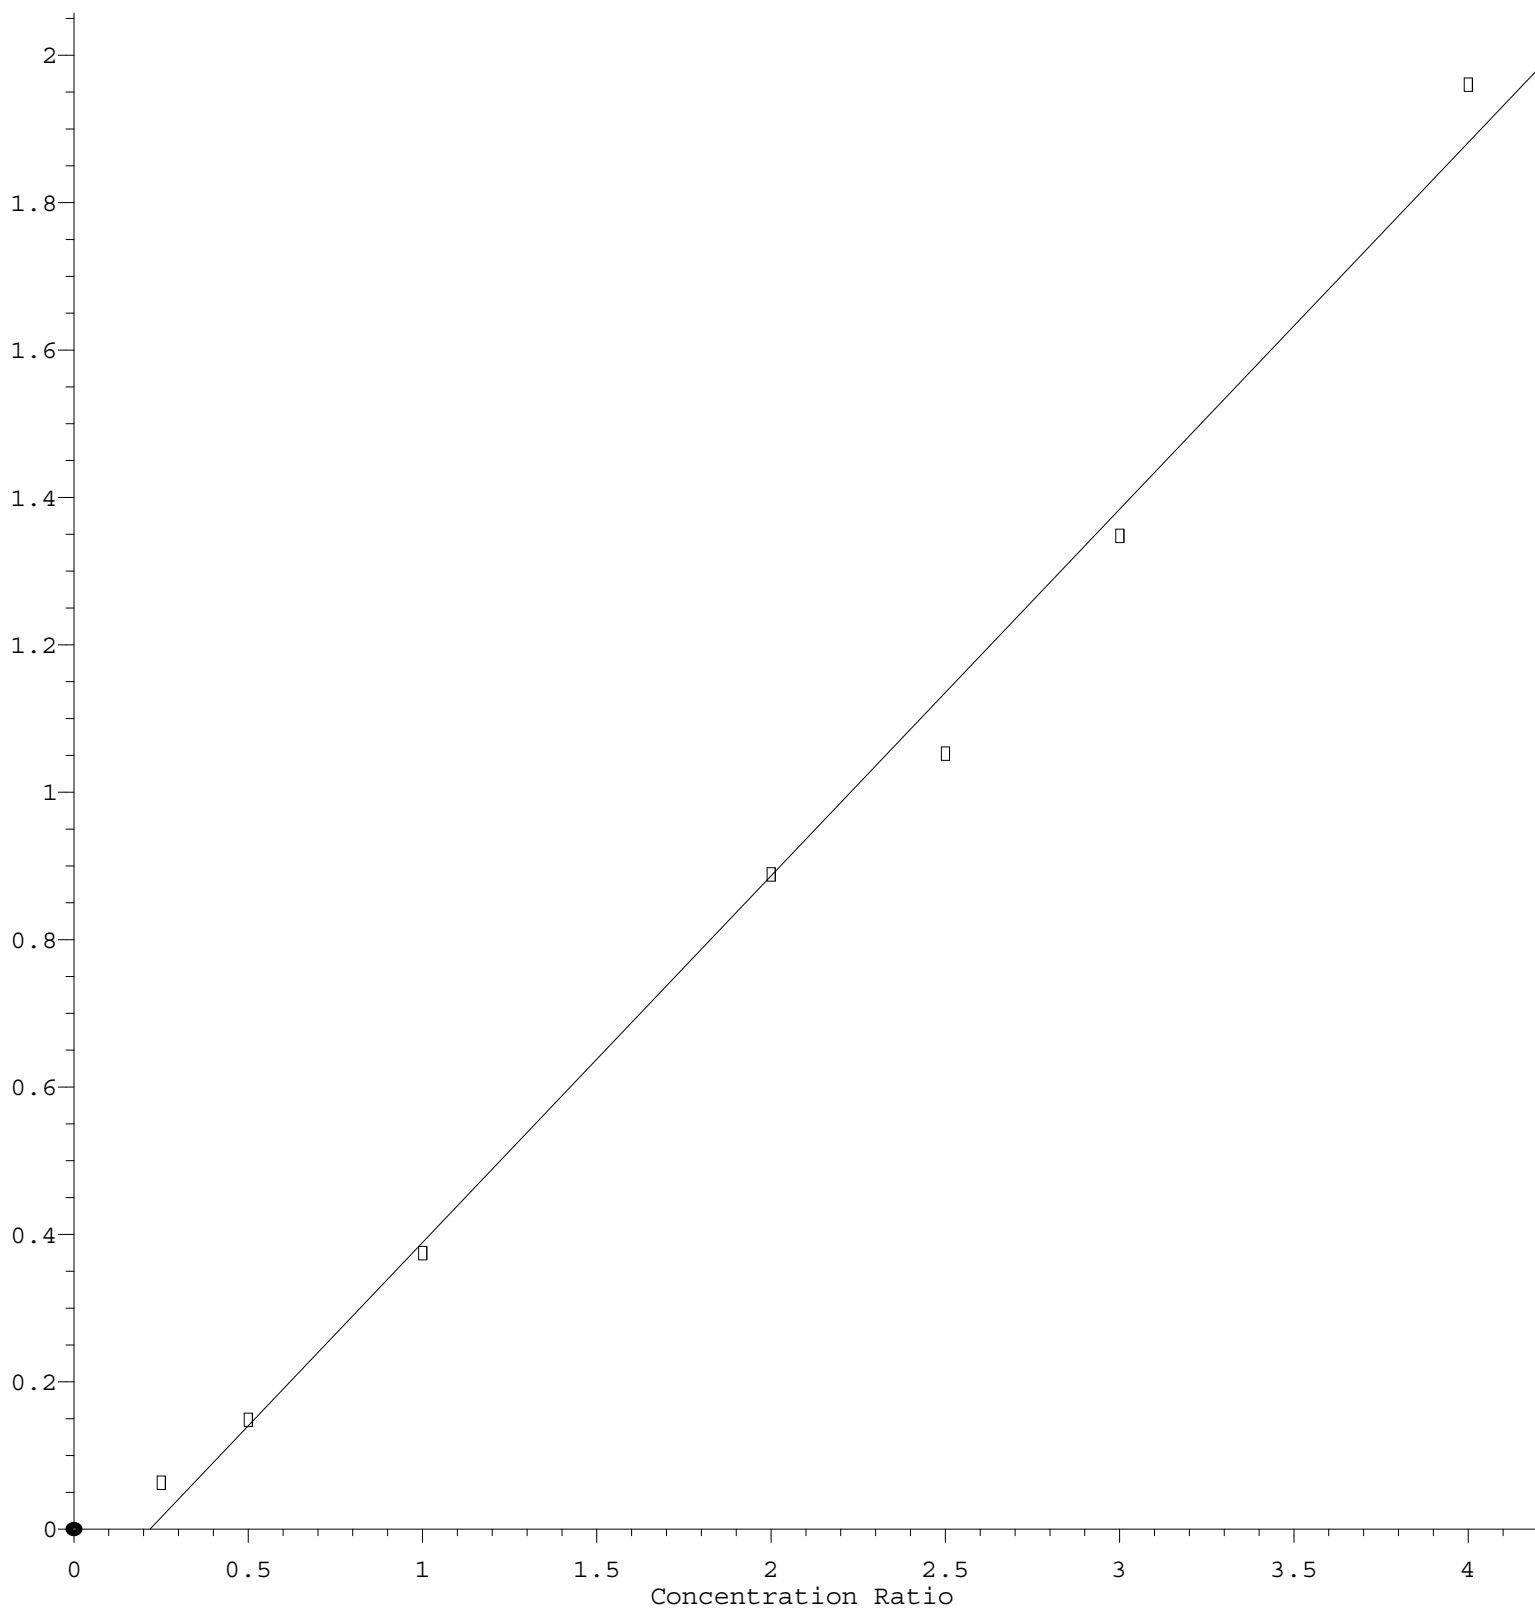

$$\text{Response} = 4.975\text{e-}001 * \text{Amt} - 1.082\text{e-}001$$


Coef of Det (r^2) = 0.994104 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM103023.M

Calibration Table Last Updated: Tue Oct 31 02:55:18 2023

Hexachlorocyclopentadiene

Response Ratio

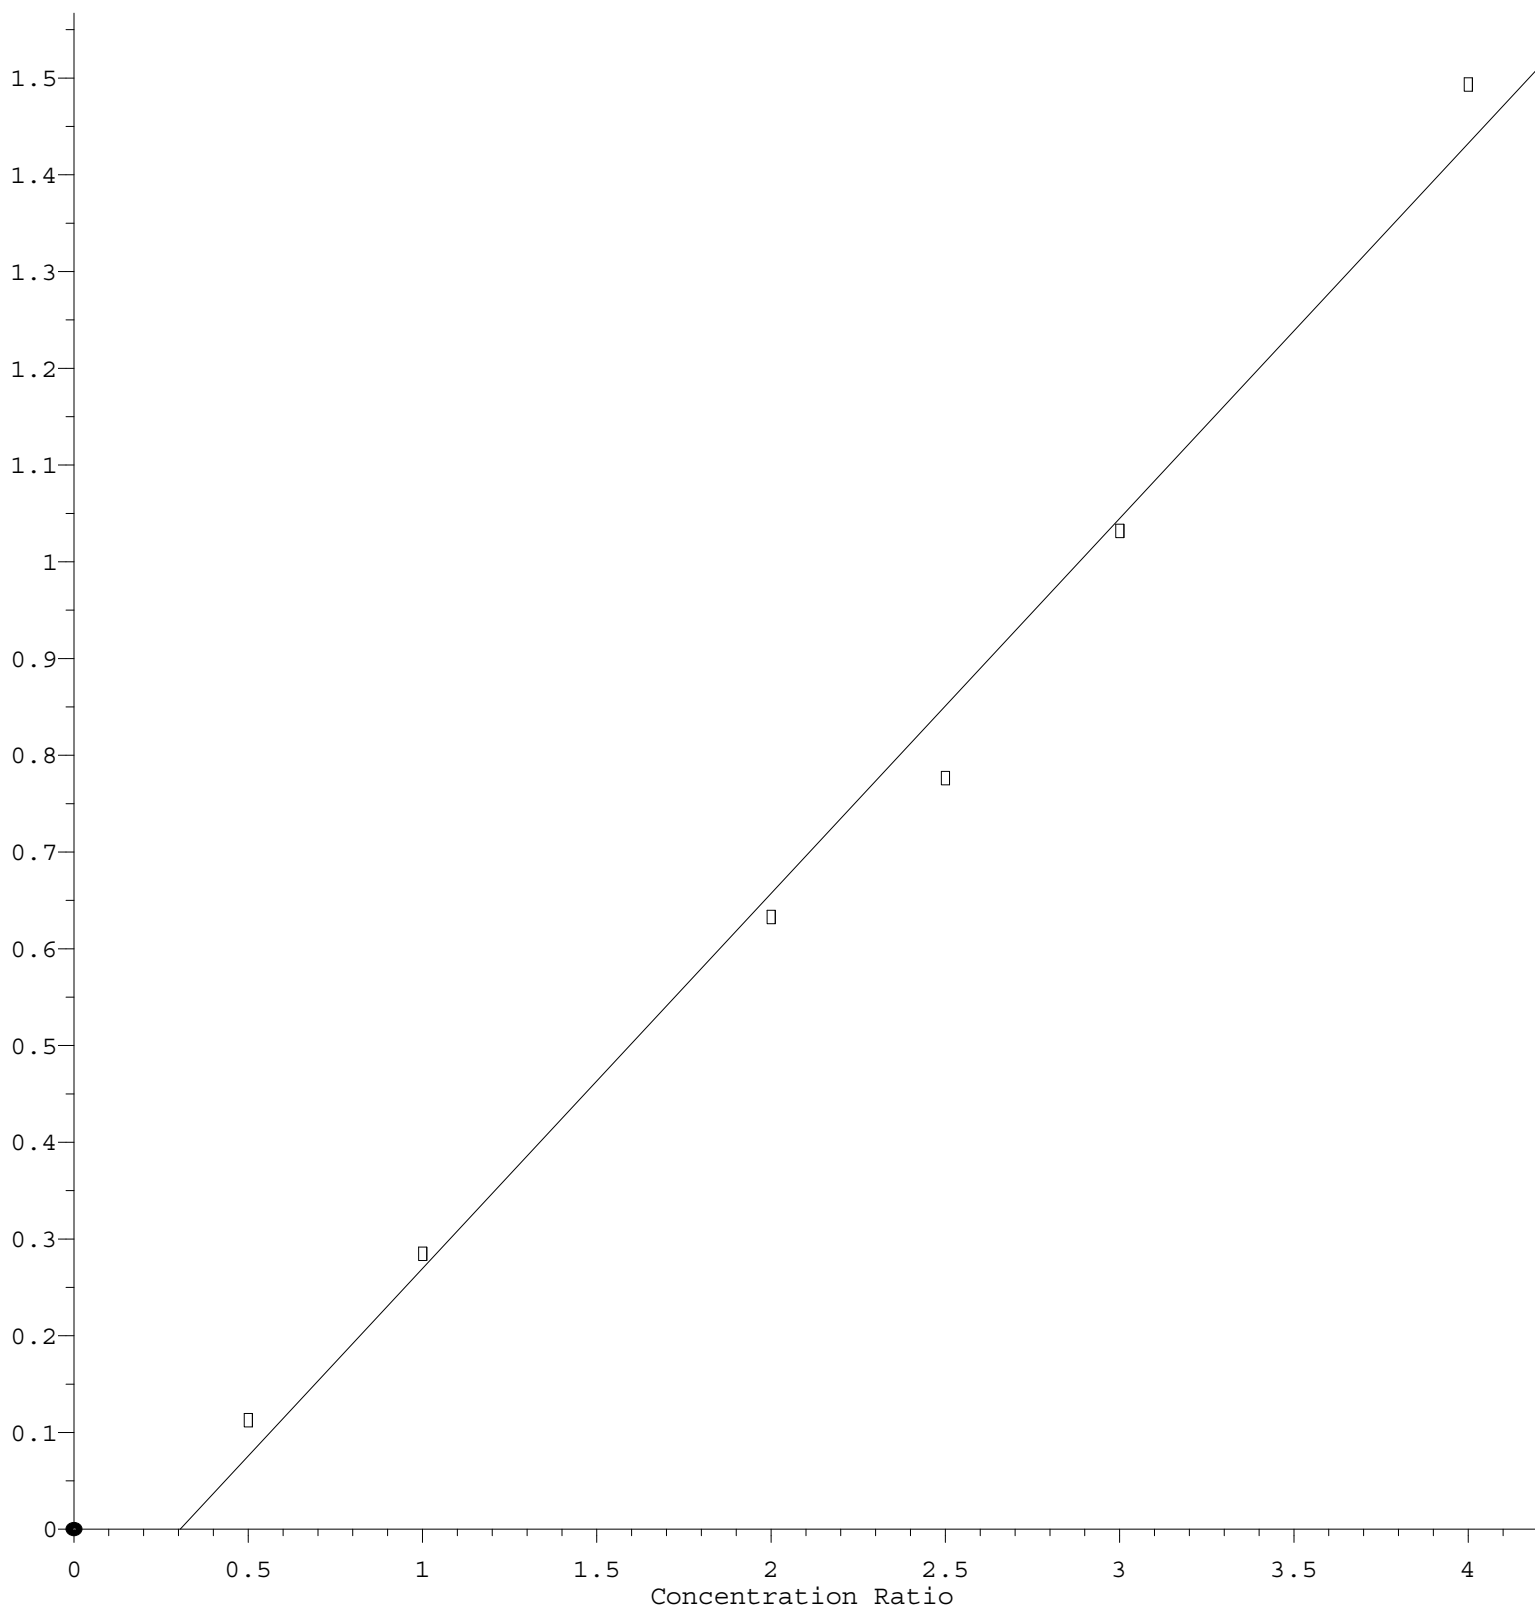


$$\text{Response} = 3.877\text{e-}001 * \text{Amt} - 1.182\text{e-}001$$

Coef of Det (r^2) = 0.990807 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM103023.M

Calibration Table Last Updated: Tue Oct 31 02:55:18 2023

Benzoic acid

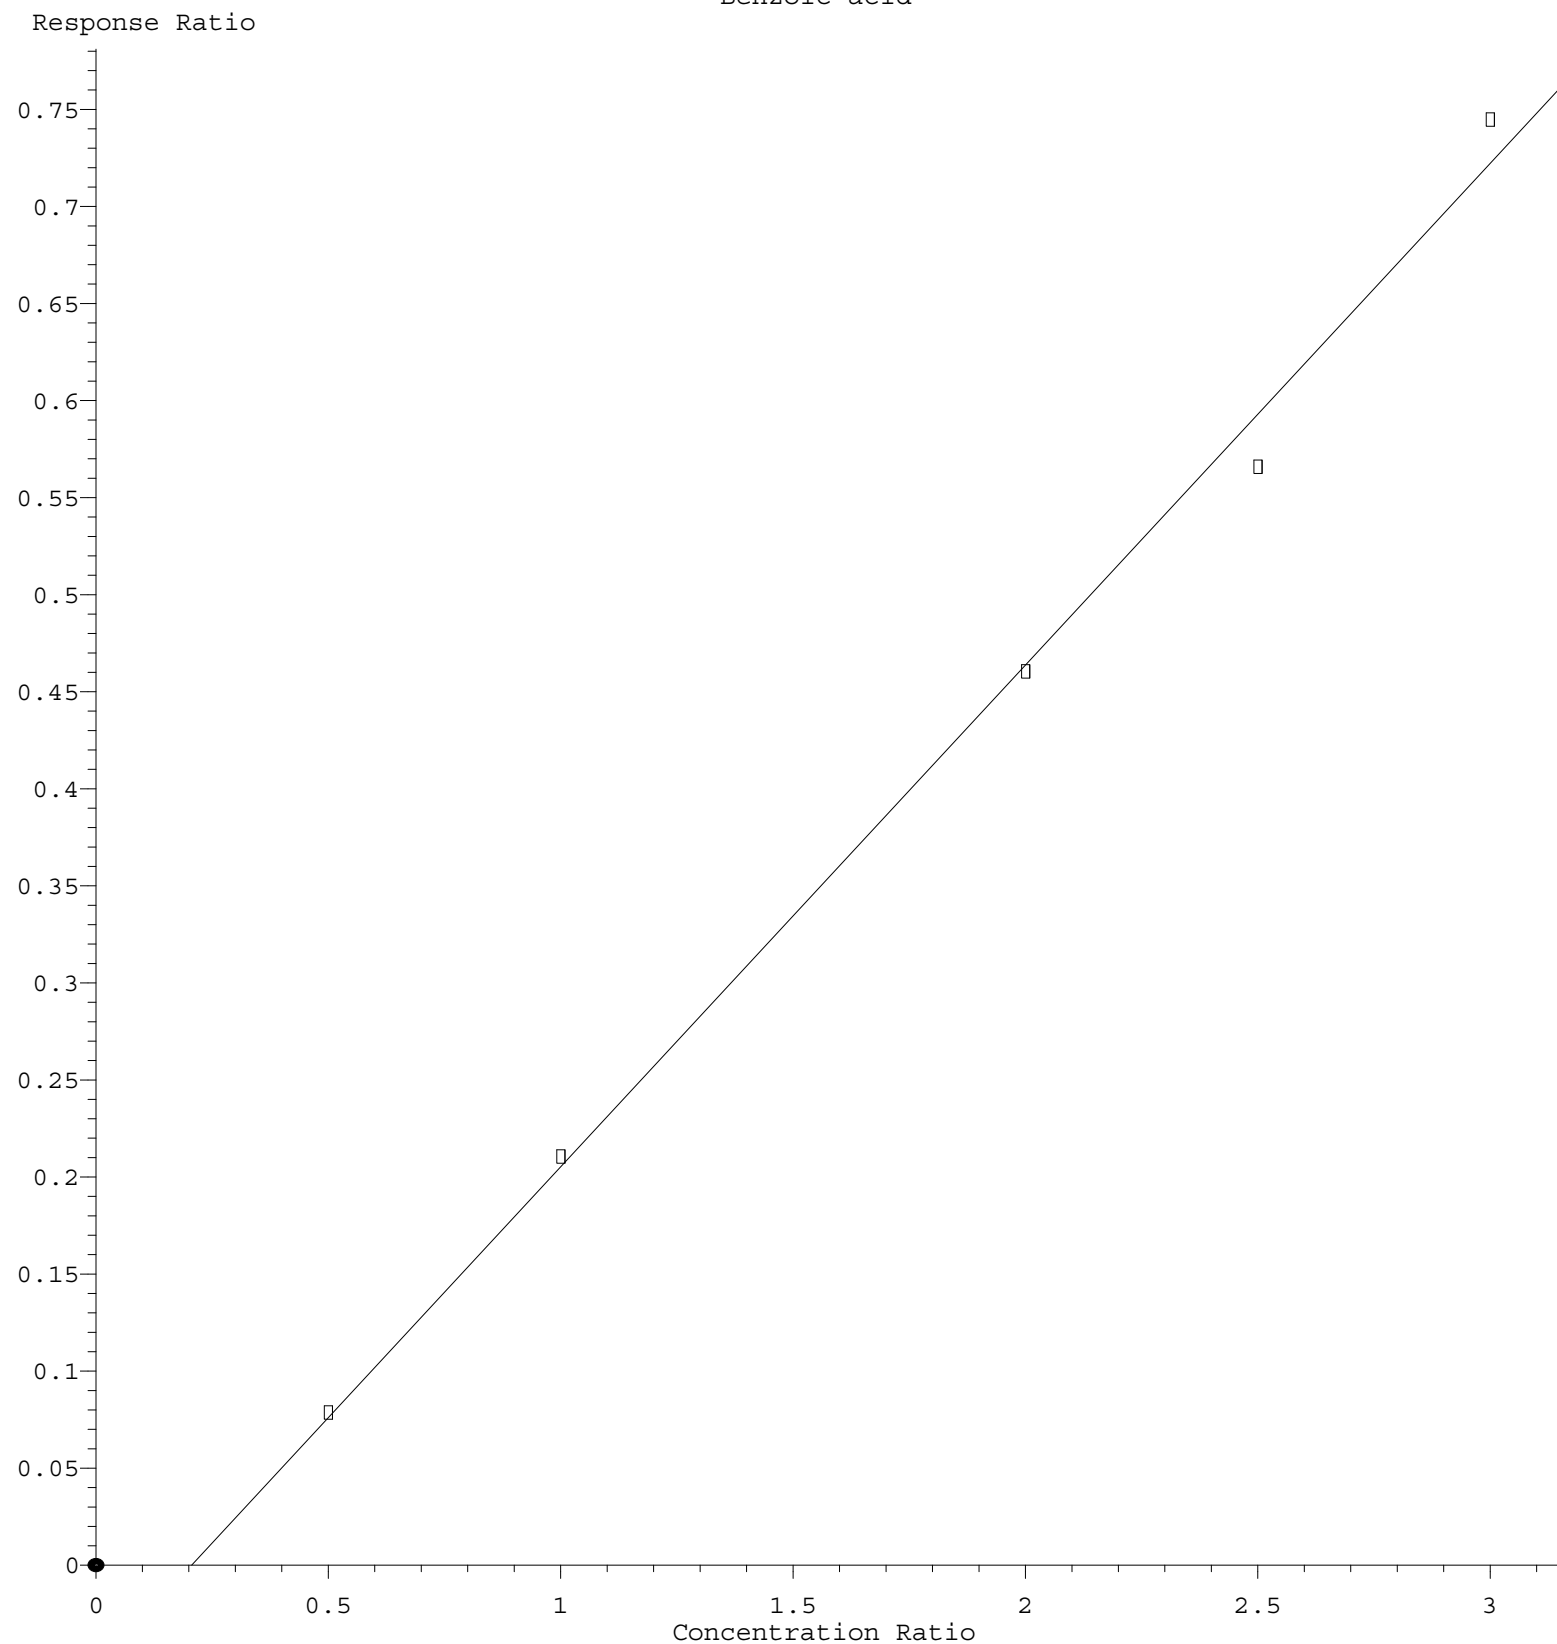

$\text{Response} = 2.584\text{e-}001 * \text{Amt} - 5.312\text{e-}002$
 Coef of Det (r^2) = 0.995538 Curve Fit: Linear
 Method Name: Z:\svoasrv\HPCHEM1\BNA M\Methods\8270-BM103023.M
 Calibration Table Last Updated: Tue Oct 31 02:55:18 2023