


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103023\
Data File : BF136022.D
Acq On : 30 Oct 2023 11:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 31 01:13:02 2023

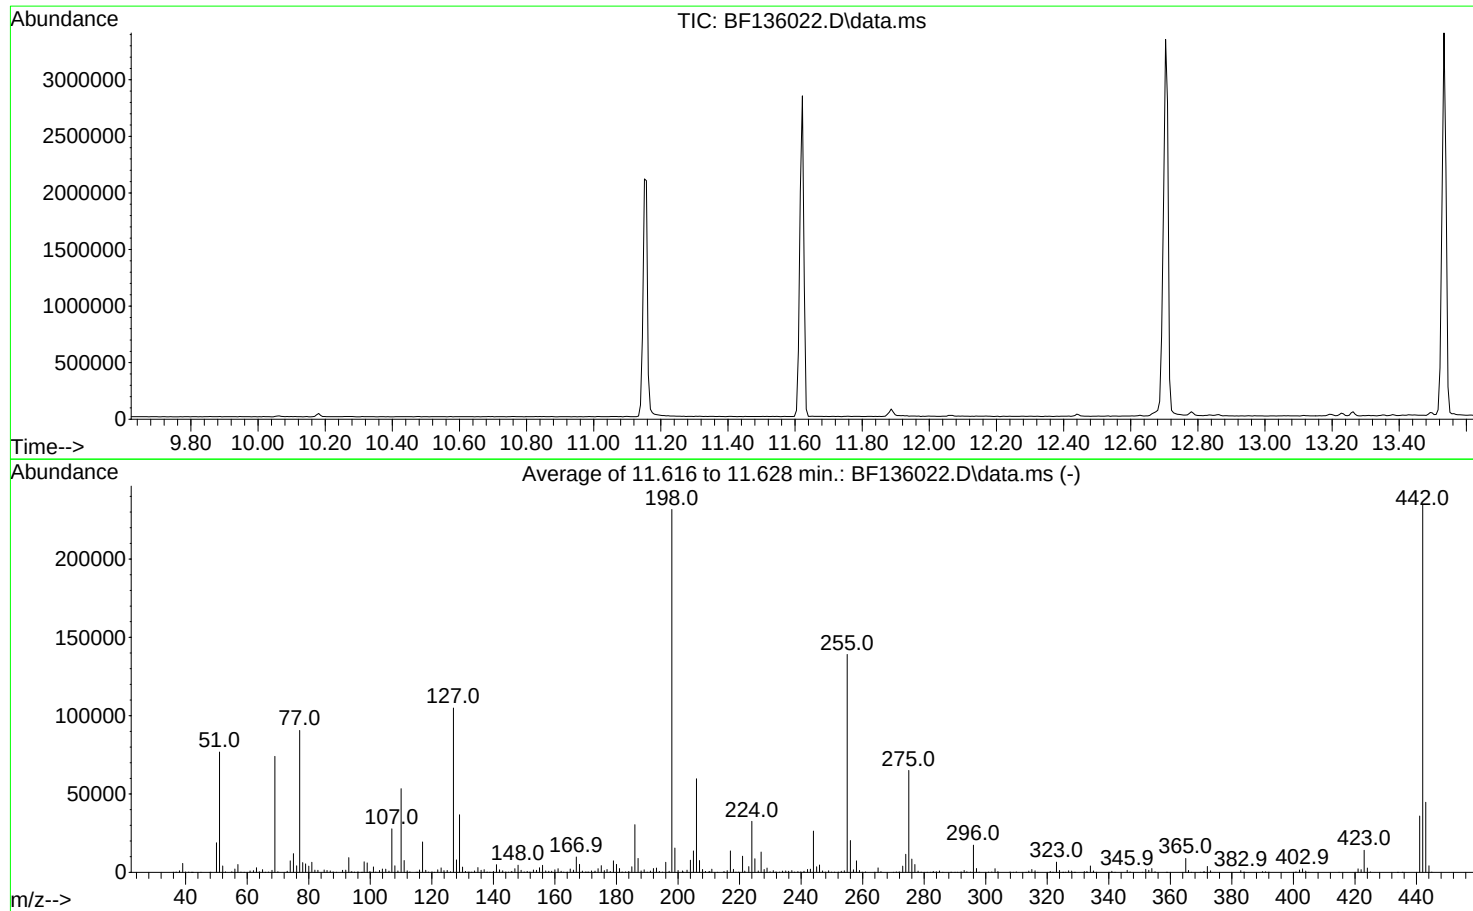




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	76773	PASS
68	69	0.00	2	1.8	1316	PASS
69	198	0.00	100	32.0	74048	PASS
70	69	0.00	2	0.6	435	PASS
127	198	10	80	45.3	104917	PASS
197	198	0.00	2	0.3	757	PASS
198	198	100	100	100.0	231611	PASS
199	198	5	9	6.7	15492	PASS
275	198	10	60	28.1	65048	PASS
365	198	1	100	3.8	8891	PASS
441	198	0.01	100	15.5	35931	PASS
442	442	50	100	100.0	234816	PASS
443	442	15	24	19.0	44715	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103023\
Data File : BF136022.D
Acq On : 30 Oct 2023 11:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 31 01:19:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

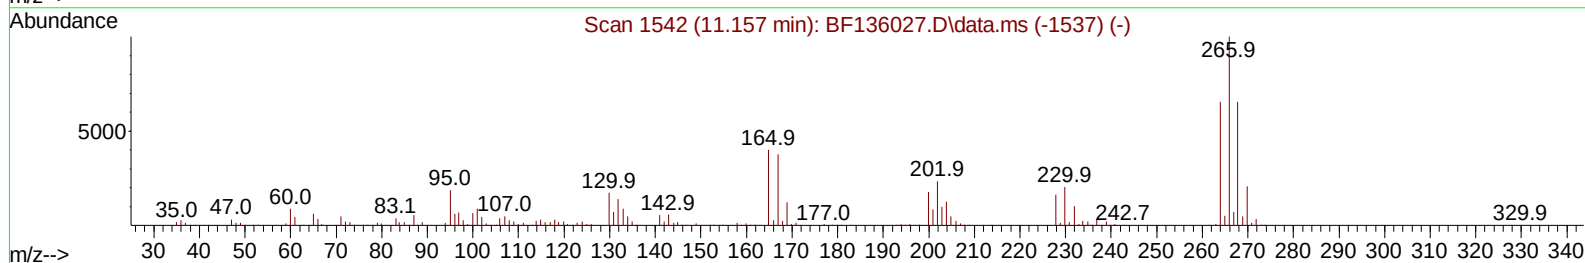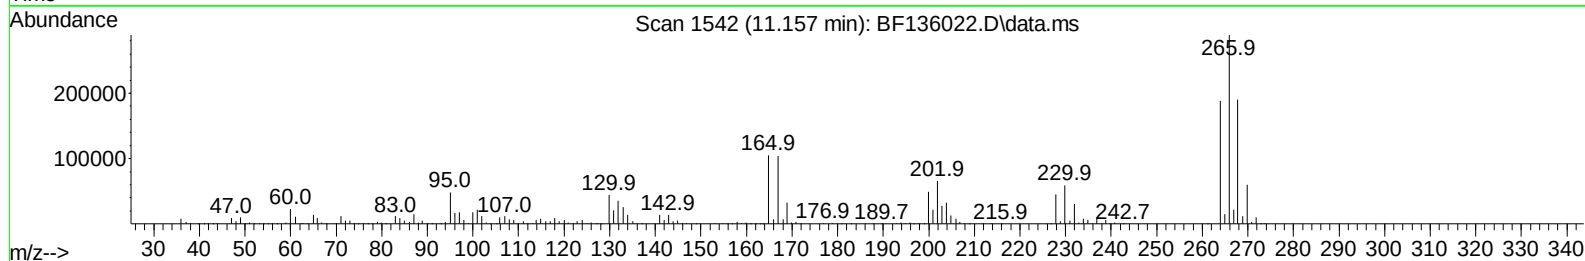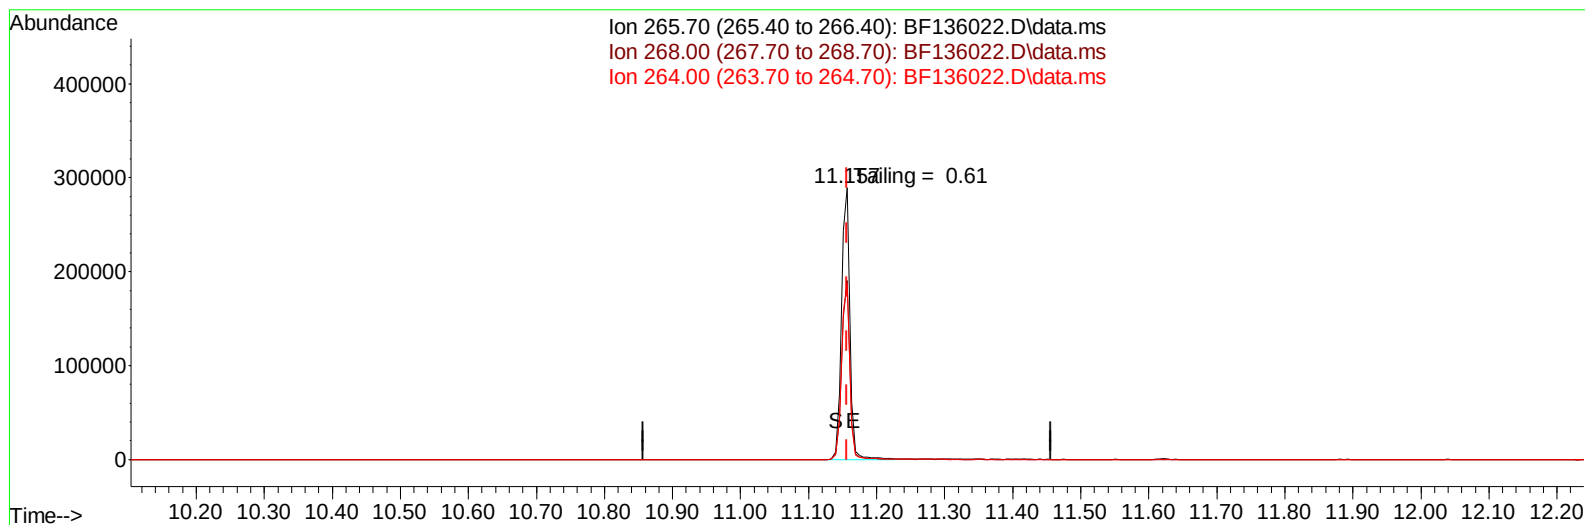

TIC: BF136022.D\data.ms

(70) Pentachlorophenol (C)

11.157min (+ 0.000) 31322.27 ng




response 247319

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	65.83
264.00	65.30	65.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF103023\
Data File : BF136022.D
Acq On : 30 Oct 2023 11:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 31 01:19:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 31 01:13:02 2023
Response via : Initial Calibration

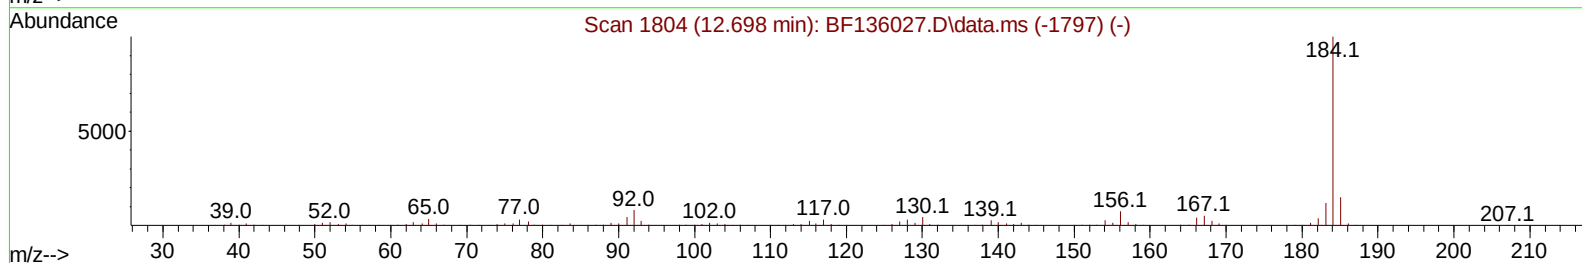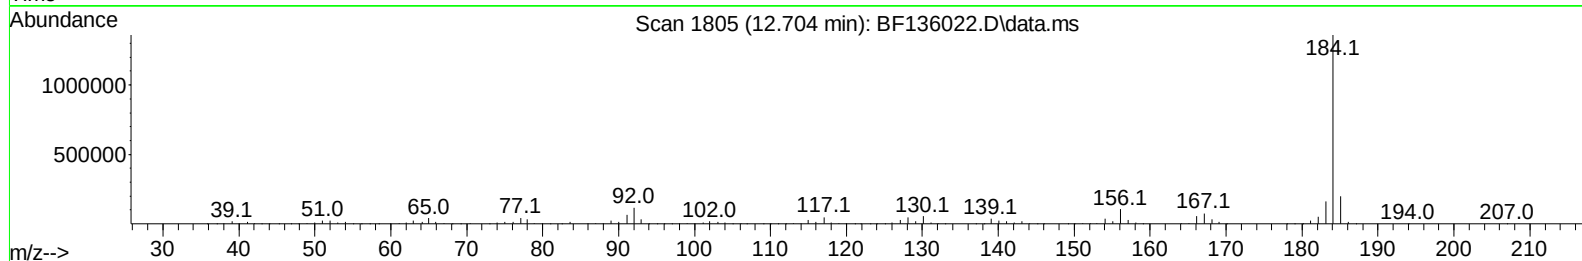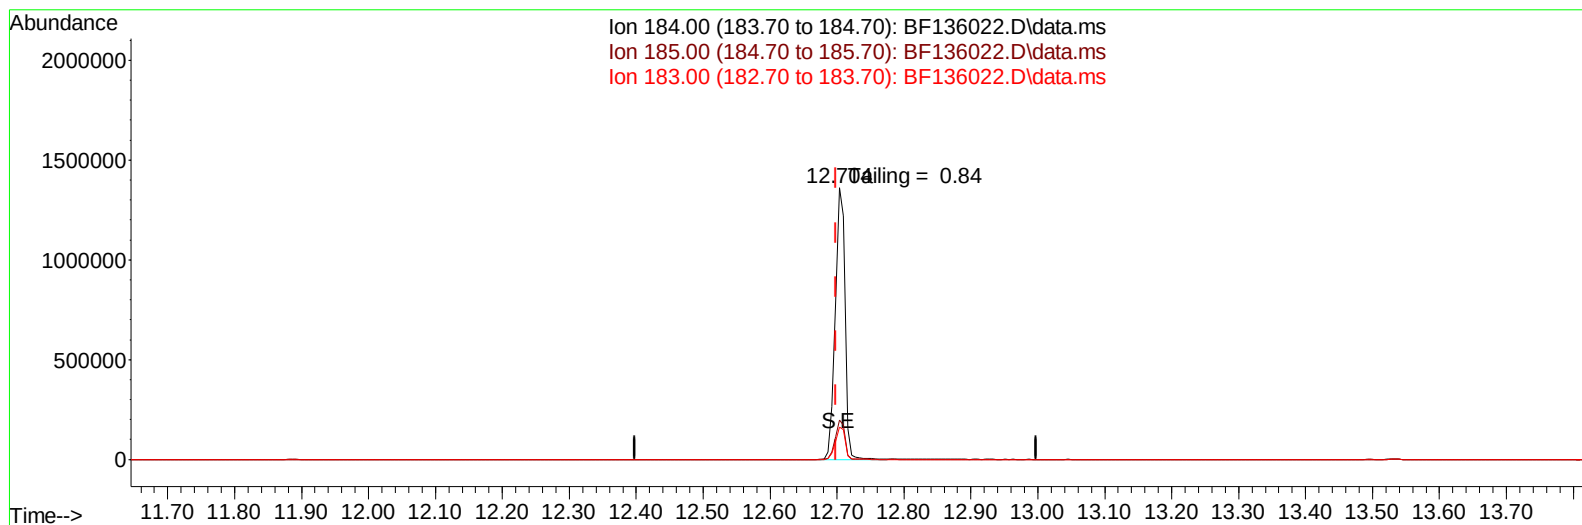

TIC: BF136022.D\data.ms

(77) Benzidine

12.704min (+ 0.006) 70133.47 ng

response 1380629

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.44
183.00	11.90	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/30/2023	BNA_F	<u>BF136022.D</u>
Compound Name	Response	Retention Time
DDT	571640	13.533
DDD	9565	13.263
DDE	214	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9779	581419	1.68

Instrument :
BNA_F
ClientSampleId :
DFTPP