


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103023\
Data File : BM042487.D
Acq On : 30 Oct 2023 09:52
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Oct 31 02:55:18 2023

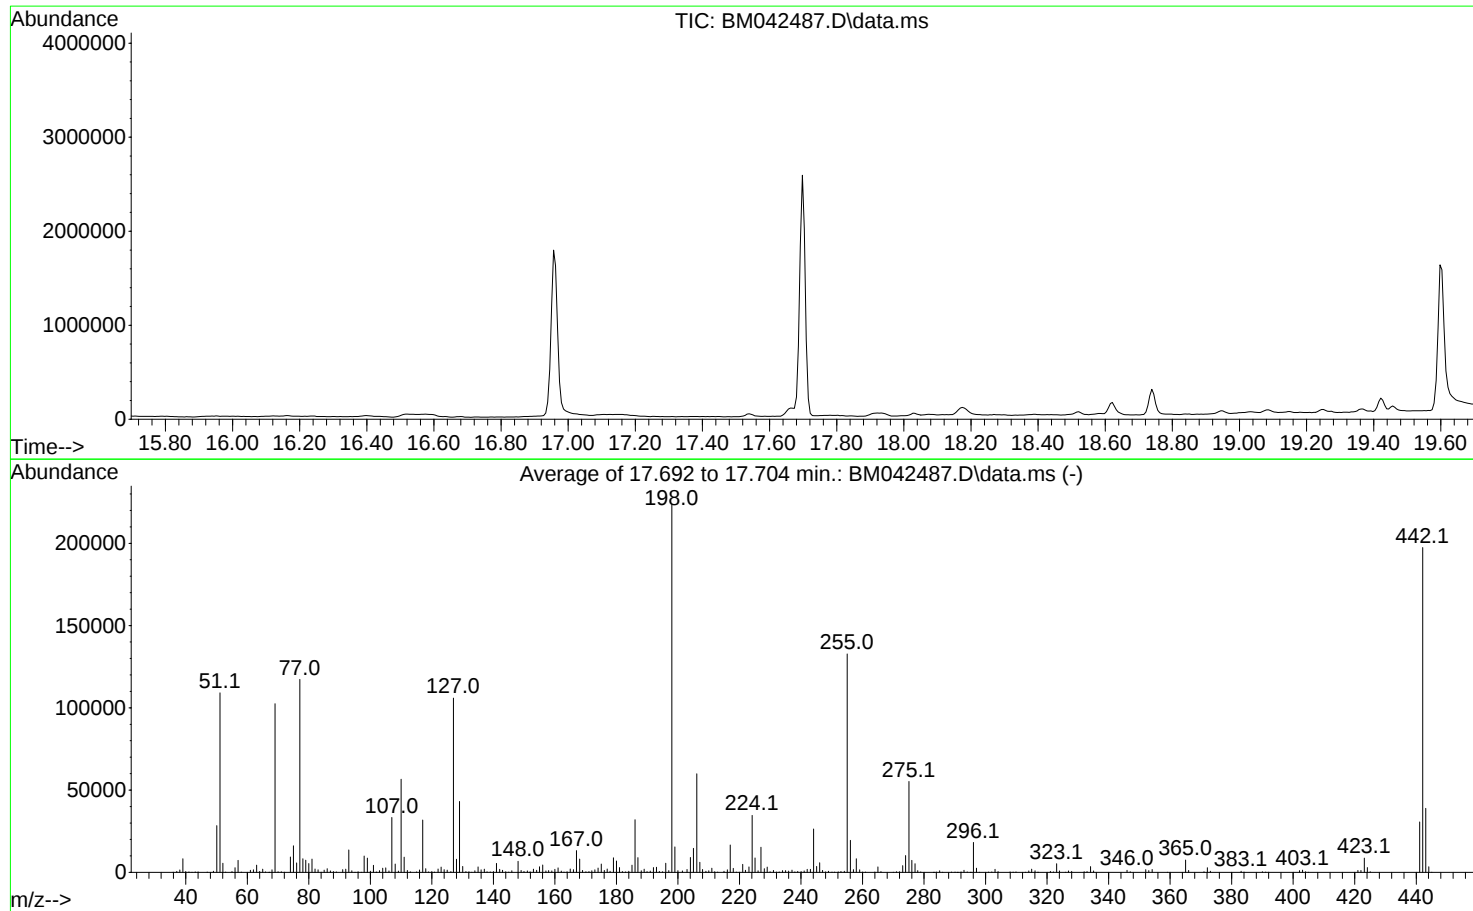




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	109094	PASS
68	69	0.00	2	1.5	1548	PASS
69	198	0.00	100	45.8	102490	PASS
70	69	0.00	2	0.4	384	PASS
127	198	10	80	47.4	105891	PASS
197	198	0.00	2	0.5	1098	PASS
198	198	100	100	100.0	223595	PASS
199	198	5	9	6.9	15426	PASS
275	198	10	60	24.7	55259	PASS
365	198	1	100	3.4	7521	PASS
441	198	0.01	100	13.7	30664	PASS
442	442	50	100	100.0	197456	PASS
443	442	15	24	19.7	38947	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM103023\
Data File : BM042487.D
Acq On : 30 Oct 2023 09:52
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 30 16:45:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM103023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 30 16:44:27 2023
Response via : Initial Calibration

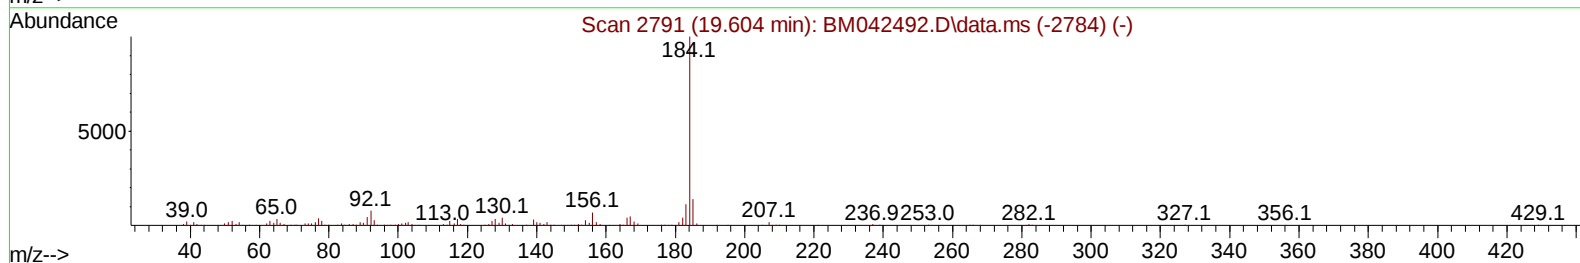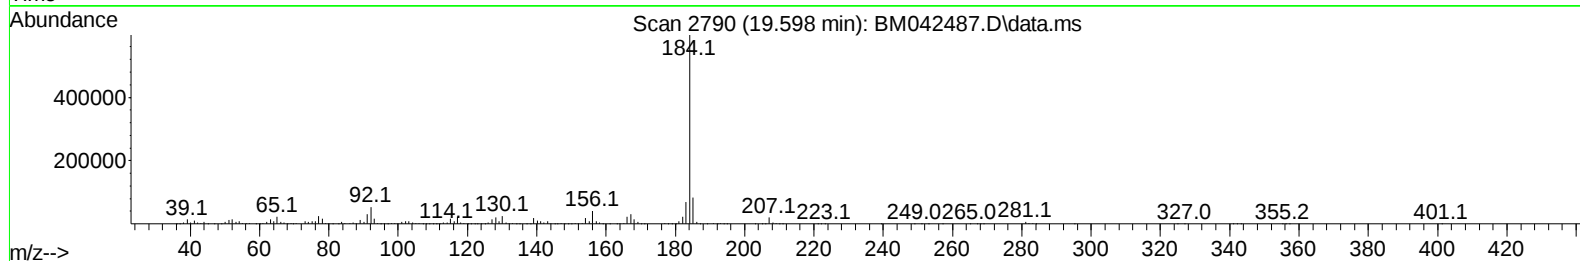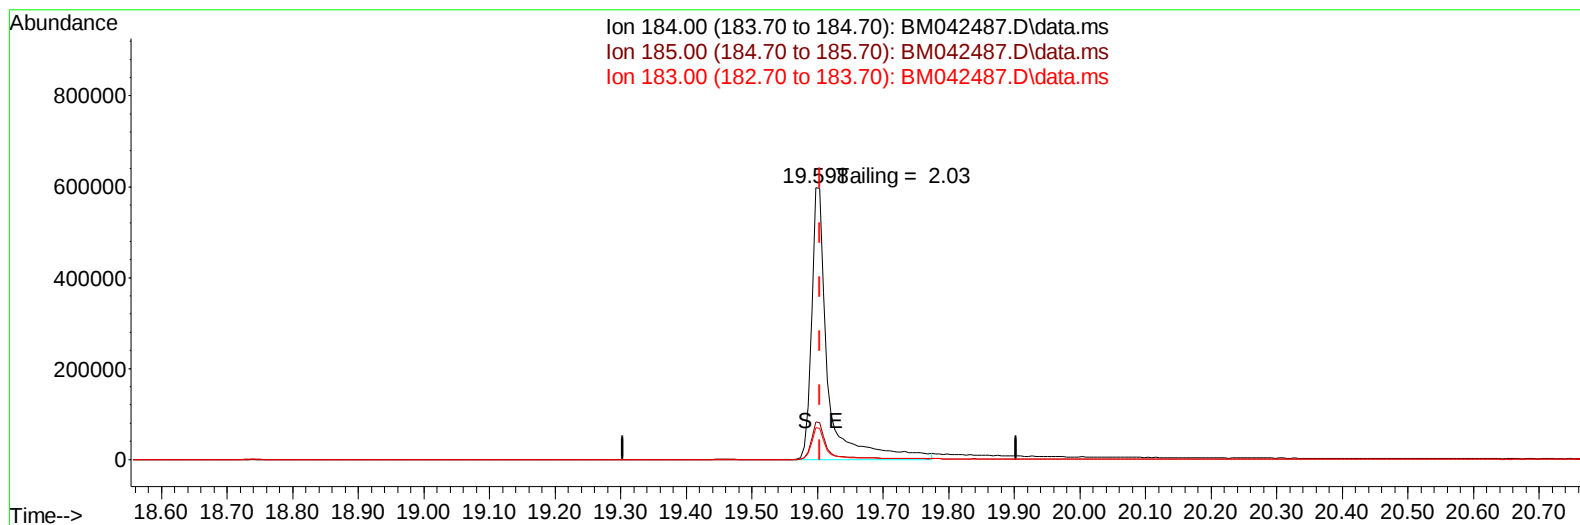

TIC: BM042487.D\data.ms

(77) Benzidine

19.598min (-0.006) 107031.09 ng

response 1037677

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.89
183.00	11.20	11.58
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/30/2023	BNA_M	<u>BM042487.D</u>
Compound Name	Response	Retention Time
DDT	764265	20.786
DDD	12766	20.35
DDE	557	19.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13323	777588	1.71

Instrument :
BNA_M
ClientSampleId :
DFTPP