

**Prep Standard - Chemical Standard Summary****Order ID :** P1187**Test :** Herbicide**Prepbatch ID :** PB158539,**Sequence ID/Qc Batch ID:** PS012224,**Standard ID :**

EP2423,EP2436,PP22990,PP22991,PP23008,PP23009,PP23010,PP23011,PP23012,PP23013,PP23014,PP23015,PP23016,

**Chemical ID :**

E2865,E3370,E3551,E3665,E3666,E3672,E3674,M5037,M5641,P11178,P12418,P12419,P12628,P12644,P12645,P12646,P12647,P12706,P8805,P8827,P8900,P9003,

# CHEMTECH

284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900

## Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2017	1:1 ACETONE/METHYLENE CHLORIDE	<a href="#">EP2423</a>	12/18/2023	06/14/2024	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 12/18/2023

**FROM** 8000.00000ml of E3665 + 8000.00000ml of E3666 = Final Quantity: 16000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
601	Acidified Sodium Sulphate 2	<a href="#">EP2436</a>	01/16/2024	07/03/2024	Rajesh Parikh	Extraction_SC ALE_2 (EX-SC-2)	None	RUPESHKUMAR SHAH 01/16/2024

**FROM** 100.00000ml of E3370 + 150.00000ml of M5037 + 3000.00000ml of E3551 = Final Quantity: 3000.000 gram

**284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900**

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1848	5000/500000 PPB Herbicide Spike (Free Acid)	<a href="#">PP22990</a>	01/03/2024	07/03/2024	Abdul Mirza	None	None	Ankita Jodhani 01/08/2024

<b>FROM</b>	1.25000ml of P12418 + 1.25000ml of P12419 + 47.50000ml of E3674 = Final Quantity: 50.000 ml
-------------	---

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
60	5000 PPB Herbicide Surg Spike (Free Acid)	<a href="#">PP22991</a>	01/04/2024	06/21/2024	Abdul Mirza	None	None	Ankita Jodhani 01/08/2024

<b>FROM</b>	1.25000ml of P12644 + 1.25000ml of P12645 + 1.25000ml of P12646 + 1.25000ml of P12647 + 195.00000ml of E3674 = Final Quantity: 200.000 ml
-------------	--

**284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900**

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1321	2/200 PPM Herb Mega Mix	<a href="#">PP23008</a>	01/09/2024	06/23/2024	Abdul Mirza	None	None	Ankita Jodhani 01/10/2024
<u>FROM</u>	0.20000ml of P8827 + 1.00000ml of P12628 + 1.00000ml of P8805 + 1.00000ml of P8900 + 1.00000ml of P9003 + 95.80000ml of E3672 = Final Quantity: 100.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1452	1500 PPB HERB MIX STD	<a href="#">PP23009</a>	01/09/2024	06/23/2024	Abdul Mirza	None	None	Ankita Jodhani 01/10/2024
<u>FROM</u>	0.25000ml of E3672 + 0.75000ml of PP23008 = Final Quantity: 1.000 ml							

**284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900**

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1453	1000 PPB Herb MIX STD	<a href="#">PP23010</a>	01/09/2024	06/23/2024	Abdul Mirza	None	None	Ankita Jodhani 01/10/2024
<u>FROM</u>	0.50000ml of E3672 + 0.50000ml of PP23008 = Final Quantity: 1.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1454	750 PPB Herb MIX STD	<a href="#">PP23011</a>	01/09/2024	06/23/2024	Abdul Mirza	None	None	Ankita Jodhani
01/10/2024								
<u>FROM</u>	0.25000ml of E3672 + 0.75000ml of PP23010 = Final Quantity: 1.000 ml							

**284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900**

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1455	500 PPB Herb MIX STD	<a href="#">PP23012</a>	01/09/2024	06/23/2024	Abdul Mirza	None	None	Ankita Jodhani 01/10/2024
<b><u>FROM</u></b> 0.50000ml of E3672 + 0.50000ml of PP23010 = Final Quantity: 1.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1456	200 PPB Herb MIX STD	<a href="#">PP23013</a>	01/09/2024	06/23/2024	Abdul Mirza	None	None	Ankita Jodhani 01/10/2024
<b><u>FROM</u></b> 0.80000ml of E3672 + 0.20000ml of PP23010 = Final Quantity: 1.000 ml								

**284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900**

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1851	2/200 PPM Herb Mega Mix 2nd Source	<a href="#">PP23014</a>	01/09/2024	06/23/2024	Abdul Mirza	None	None	Ankita Jodhani 01/10/2024
<b><u>FROM</u></b> 0.50000ml of P11178 + 1.00000ml of P12706 + 48.50000ml of E3672 = Final Quantity: 50.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1854	1000 PPB HERB MIX ICV STD	<a href="#">PP23015</a>	01/09/2024	06/23/2024	Abdul Mirza	None	None	Ankita Jodhani 01/10/2024
<u>FROM</u>	0.50000ml of E3672 + 0.50000ml of PP23014 = Final Quantity: 1.000 ml							

**284, Sheffield Street, Mountainside NJ 07092 (908) 789 - 8900**

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1691	750 PPB ICV HERB STD	<a href="#">PP23016</a>	01/09/2024	06/23/2024	Abdul Mirza	None	None	Ankita Jodhani
01/10/2024								

<u>FROM</u>	0.25000ml of E3672 + 0.75000ml of PP23015 = Final Quantity: 1.000 ml
-------------	--



**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	0000243821	12/31/2024	04/30/2020 / RAJESH	04/28/2020 / RAJESH	E2865

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9244-03 / Ether, Anhydrous, Purified (cs/4x4L)	0000288039	07/17/2024	08/01/2022 / Rajesh	07/13/2022 / Rajesh	E3370

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	07/03/2024	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	23J1162022	12/05/2024	12/09/2023 / Rajesh	11/29/2023 / Rajesh	E3665

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	23H1462005	06/14/2024	12/14/2023 / Rajesh	12/14/2023 / Rajesh	E3666

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	23G1262009	06/23/2024	12/23/2023 / Rajesh	12/21/2023 / Rajesh	E3672

**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	23H1462005	07/03/2024	01/03/2024 / Rajesh	01/03/2024 / Rajesh	E3674

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	0000250349	12/15/2024	01/06/2022 / mohan	09/18/2021 / mohan	M5037

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	WW-LFS-1 / Laboratory Fortified Stock Solution 1, 125 ml	T2-MEB723367	04/17/2024	04/18/2023 / bin	04/16/2023 / bin	M5641

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32050 / Herbicide, 8000 series, 515 Surrogate [ester] 2,4-dichlorophenyl acetic acid methyl ester, 1mL, 200ug/mL, Hexane	A0172864	07/09/2024	01/09/2024 / Abdul	11/01/2021 / Abdul	P11178

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006686742	07/03/2024	01/03/2024 / Abdul	02/16/2023 / Abdul	P12418

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006686742	07/03/2024	01/03/2024 / Abdul	02/16/2023 / Abdul	P12418

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006686742	07/03/2024	01/03/2024 / Abdul	02/16/2023 / Abdul	P12419

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006686742	07/03/2024	01/03/2024 / Abdul	02/16/2023 / Abdul	P12419

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32055 / Herbicide Mix, 500/8000, Standard #1 [methyl ester] 200ug/mL, hexane, 1mL/ampul	A192429	07/09/2024	01/09/2024 / Abdul	07/03/2023 / Abdul	P12628

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0190000	06/21/2024	12/21/2023 / Abdul	07/03/2023 / Abdul	P12644

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0190000	06/21/2024	12/21/2023 / Abdul	07/03/2023 / Abdul	P12645

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0190000	06/21/2024	12/21/2023 / Abdul	07/03/2023 / Abdul	P12646

**CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32049 / Herbicide, 8000 series, 515 Surrogate [free acid] 2,4-dichlorophenyl acetic acid, 1mL, 200ug/mL, MeOH	A0190000	06/21/2024	12/21/2023 / Abdul	07/03/2023 / Abdul	P12647

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151M / Chlorinated Herbicide Mixtures, Methyl Esters	0006752480	07/09/2024	01/09/2024 / Abdul	08/09/2023 / Abdul	P12706

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151M / Chlorinated Herbicide Mixtures, Methyl Esters	0006752480	07/09/2024	01/09/2024 / Abdul	08/09/2023 / Abdul	P12706

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32062 / Herbicide Mix, 500/8000, Standard #4 [methyl ester] 200ug/mL, hexane, 1mL/ampul	A0131940	07/09/2024	01/09/2024 / Abdul	08/16/2019 / Stephen	P8805

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32254 / Dalapon Methyl Ester, 1000 ug/ml	A0148063	07/09/2024	01/09/2024 / Abdul	08/16/2019 / Stephen	P8827

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32059 / Herbicide Mix#3 (Methyl Ester), 20000 ug/ml	A0152499	07/09/2024	01/09/2024 / Abdul	08/16/2019 / Stephen	P8900



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

### CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32050 / Herbicide, 8000 series, 515 Surrogate [ester] 2,4-dichlorophenyl acetic acid methyl ester, 1mL, 200ug/mL, Hexane	A0152705	07/09/2024	01/09/2024 / Abdul	10/11/2019 / Stephen	P9003

Sand  
Purified  
Washed and Ignited



Material No.: 3382-05  
Batch No.: 0000243821  
Manufactured Date: 2018/04/09  
Retest Date: 2025/04/07  
Revision No: 1

## Certificate of Analysis

Test	Specification	Result
Substances Soluble in HCl	$\leq 0.16\%$	0.01

For Laboratory, Research or Manufacturing Use  
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US  
Packaging Site: Paris Mfg Ctr & DC

E 2865

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC  
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Ether, Anhydrous  
BAKER ANALYZED® A.C.S. Reagent  
Contains BHT as a Preservative  
Suitable for Fat Extraction



Material No.: 9244-03  
Batch No.: 0000288039  
Manufactured Date: 2021/07/22  
Expiration Date: 2023/07/22  
Revision No: 1

## Certificate of Analysis

Meets ACS Reagent Chemical Requirements,

Test	Specification	Result
Assay ((C <sub>2</sub> H <sub>5</sub> ) <sub>2</sub> O) (by GC, corrected for water)	>= 99.0 %	100.0
Alcohol (C <sub>2</sub> H <sub>5</sub> OH)	Passes Test	PT
Carbonyl Compounds (as HCHO) (by polarography)	<= 0.001 %	< 0.001
Color (APHA)	<= 10	< 5
Peroxide (as H <sub>2</sub> O <sub>2</sub> )	<= 1 ppm	< 1
Preservative (BHT)	>= 7 ppm	9
Residue after Evaporation	<= 0.0010 %	< 0.0010
Titration Acid (μeq/g)	<= 0.2	< 0.2
Water (by KF, coulometric)	<= 0.01 %	0.01

For Laboratory, Research or Manufacturing Use  
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US

Recd. by RP on 7/13/22

E 3370

  
Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



**PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MEXICO  
CP 64070  
TEL +52 81 13 52 57 57  
www.pqm.com.mx

## CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na <sub>2</sub> SO <sub>4</sub>
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na <sub>2</sub> SO <sub>4</sub> )	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO <sub>4</sub> )	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

### COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3



Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 23J1162022  
Manufactured Date: 2023-09-06  
Expiration Date: 2024-12-05  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	2
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	2
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	10
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.3 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC  
Manufacturer source batch: MG23I06692

E3665

Ken Koehnlein  
Sr. Manager, Quality Assurance

Hexanes (95% n-hexane)  
BAKER RESI-ANALYZED® Reagent



Material No.: 9262-03  
Batch No.: 23G1262009  
Manufactured Date: 2023-06-01  
Expiration Date: 2024-08-30  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	$\leq 5$	3
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.6 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0$ ppm	0.3 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 12/14/23

E 3666

Ken Koehnlein  
Sr. Manager, Quality Assurance

Acetone  
BAKER RESI-ANALYZED® Reagent  
For Organic Residue Analysis

 **avantortm**



Material No.: 9254-03  
Batch No.: 23H1462005  
Manufactured Date: 2023-07-26  
Expiration Date: 2026-07-25  
Revision No.: 0

## Certificate of Analysis


Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H <sub>2</sub> O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 1/3/24

E 3674



Ken Koehnlein  
Sr. Manager, Quality Assurance

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Sulfuric Acid

BAKER INSTRA-ANALYZED® Reagent

For Trace Metal Analysis

Low Selenium

avantorsm



Material No.: 9673-33

Batch No.: 0000250349

Manufactured Date: 2019/12/17

Retest Date: 2024/12/15

Revision No: 1

MS037-38-39-40  
no

## Certificate of Analysis

Test	Specification	Result
ACS - Assay (H <sub>2</sub> SO <sub>4</sub> )	95.0 - 98.0 %	96.5
Appearance	Passes Test	PT
ACS - Color (APHA)	<= 10	5
ACS - Residue after Ignition	<= 3 ppm	1
ACS - Substances Reducing Permanganate (as SO <sub>2</sub> )	<= 2 ppm	< 2
Ammonium (NH <sub>4</sub> )	<= 1 ppm	< 1
Chloride (Cl)	<= 0.1 ppm	< 0.1
Nitrate (NO <sub>3</sub> )	<= 0.2 ppm	< 0.1
Phosphate (PO <sub>4</sub> )	<= 0.5 ppm	< 0.1
Trace Impurities - Aluminum (Al)	<= 30.0 ppb	0.2
Arsenic and Antimony (as As)	<= 4 ppb	< 2
Trace Impurities - Barium (Ba)	<= 10.0 ppb	< 1.0
Trace Impurities - Beryllium (Be)	<= 10.0 ppb	< 1.0
Trace Impurities - Bismuth (Bi)	<= 10.0 ppb	< 1.0
Trace Impurities - Boron (B)	<= 10.0 ppb	< 5.0
Trace Impurities - Cadmium (Cd)	<= 2.0 ppb	< 0.3
Trace Impurities - Calcium (Ca)	<= 50.0 ppb	2.9
Trace Impurities - Chromium (Cr)	<= 6.0 ppb	< 0.4
Trace Impurities - Cobalt (Co)	<= 0.5 ppb	< 0.3
Trace Impurities - Copper (Cu)	<= 1.0 ppb	< 0.1
Trace Impurities - Gallium (Ga)	<= 10.0 ppb	< 1.0
Trace Impurities - Germanium (Ge)	<= 10.0 ppb	< 10.0
Trace Impurities - Gold (Au)	<= 10.0 ppb	< 0.2
Heavy Metals (as Pb)	<= 500 ppb	< 100

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC


100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

Material No.: 9673-33  
Batch No.: 0000250349

Test	Specification	Result
Trace Impurities - Iron (Fe)	<= 50.0 ppb	4.1
Trace Impurities - Lead (Pb)	<= 0.5 ppb	< 0.5
Trace Impurities - Lithium (Li)	<= 10.0 ppb	< 1.0
Trace Impurities - Magnesium (Mg)	<= 7.0 ppb	0.4
Trace Impurities - Manganese (Mn)	<= 1.0 ppb	< 0.4
Trace Impurities - Mercury (Hg)	<= 0.5 ppb	< 0.1
Trace Impurities - Molybdenum (Mo)	<= 10.0 ppb	< 5.0
Trace Impurities - Nickel (Ni)	<= 2.0 ppb	< 0.3
Trace Impurities - Niobium (Nb)	<= 10.0 ppb	< 1.0
Trace Impurities - Potassium (K)	<= 500.0 ppb	< 2.0
Trace Impurities - Selenium (Se)	<= 50.0 ppb	22.9
Trace Impurities - Silicon (Si)	<= 100.0 ppb	< 10.0
Trace Impurities - Silver (Ag)	<= 1.0 ppb	< 0.3
Trace Impurities - Sodium (Na)	<= 500.0 ppb	2.7
Trace Impurities - Strontium (Sr)	<= 5.0 ppb	< 0.2
Trace Impurities - Tantalum (Ta)	<= 10.0 ppb	< 5.0
Trace Impurities - Thallium (Tl)	<= 20.0 ppb	< 5.0
Trace Impurities - Tin (Sn)	<= 5.0 ppb	< 0.8
Trace Impurities - Titanium (Ti)	<= 10.0 ppb	< 1.0
Trace Impurities - Vanadium (V)	<= 10.0 ppb	< 1.0
Trace Impurities - Zinc (Zn)	<= 5.0 ppb	0.3
Trace Impurities - Zirconium (Zr)	<= 10.0 ppb	< 1.0

For Laboratory, Research or Manufacturing Use

Country of Origin: US  
Packaging Site: Phillipsburg Mfg Ctr & DC

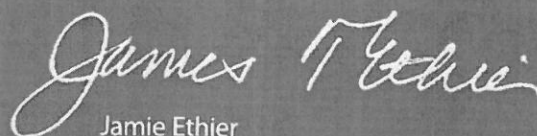

Jamie Ethier  
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC  
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

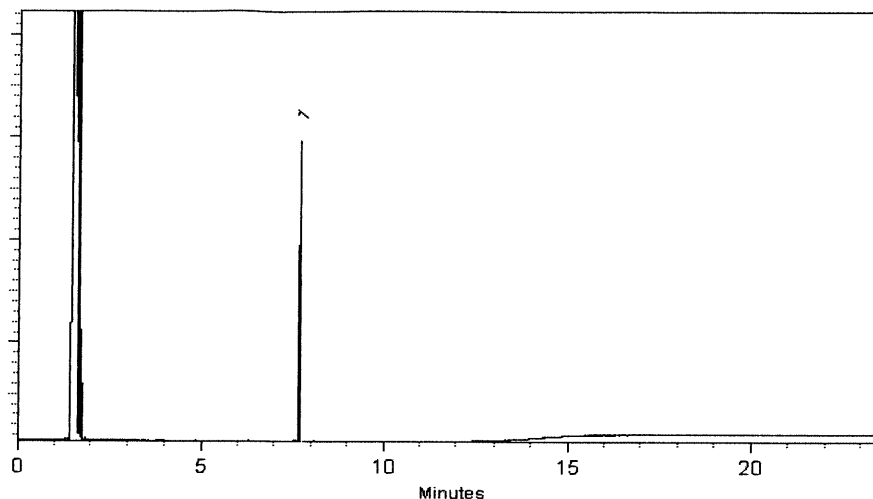


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Katelyn McGinnis - Operations Tech I

Date Mixed: 28-May-2021

Balance: B345965662

  
Marlene Cowan - Operations Tech I

Date Passed: 02-Jun-2021

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

1911177  
70  
P 111 86  
AR  
11/02/21



CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32050 **Lot No.:** A0172864

**Description :** 2,4-Dichlorophenylacetic Acid Methyl Ester Standard

515 Surrogate (ester) 2, 4-dichlorophenyl Acetic Acid Methyl Ester  
200µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** February 29, 2028 **Storage:** 10°C or colder

**Handling:** This product is photosensitive. **Ship:** Ambient

## CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-Dichlorophenyl acetic acid methyl ester	202.0 µg/mL	+/- 1.4323 µg/mL Gravimetric
	CAS # 55954-23-9 (Lot CSC42194-01)		+/- 6.8182 µg/mL Unstressed
	Purity 99%		+/- 6.8182 µg/mL Stressed

**Solvent:** Hexane  
CAS # 110-54-3  
Purity 99%

P11177  
↓  
P11186  
—  
AR  
01/02/21

**Reference Material Certificate**  
**Product Information Sheet**

**Product Name:** Chlorinated Herbicides Standard  
**Product Number:** HBM-8151A-1  
**Storage Conditions:** Store at Room Temperature (15° to 30°C).

**Lot Number:** 0006686742  
**Lot Issue Date:** 13-Jun-2022  
**Expiration Date:** 31-Jul-2024

Component Name	CERTIFIED VALUES			CAS#	Analyte Lot
	Concentration	Expanded Uncertainty			
acifluorfen	100.1	± 0.5 µg/mL		050594-66-6	NT02057
bentazon	100.1	± 0.5 µg/mL		025057-89-0	RM19026
chloramben	100.2	± 0.5 µg/mL		000133-90-4	RM03672
2,4-D	100.3	± 0.5 µg/mL		000094-75-7	RM17172
dalapon	100.3	± 0.5 µg/mL		000075-99-0	RM19654
2,4-DB	100.2	± 0.5 µg/mL		000094-82-6	RM02866
tetrachloroterephthalic acid	100.2	± 0.5 µg/mL		002136-79-0	RM13887
dicamba	100.3	± 0.5 µg/mL		001918-00-9	RM15881
3,5-dichlorobenzoic acid	100.2	± 0.5 µg/mL		000051-36-5	RM02768
dichlorprop	100.2	± 0.5 µg/mL		000120-36-5	RM19240
dinoseb	100.3	± 0.5 µg/mL		000088-85-7	RM19863
MCPA	10030	± 50 µg/mL		000094-74-6	RM12220
MCPP (mecoprop)	10026	± 50 µg/mL		000093-65-2	RM09273
4-nitrophenol	100.3	± 0.5 µg/mL		000100-02-7	RM03752
pentachlorophenol	100.2	± 0.5 µg/mL		000087-86-5	RM02474
picloram	100.2	± 0.5 µg/mL		001918-02-1	RM19110
silvex	100.2	± 0.5 µg/mL		000093-72-1	RM19595
2,4,5-T	100.3	± 0.5 µg/mL		000093-76-5	NT01808

**Matrix:** methanol (methyl alcohol)

**Description:**

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

*Handwritten:* P 12406, P 12420, 15, RAUF, 02/20/23



**Homogeneity:**

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

**Instructions for Use:**

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

**Safety:**

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this analytical reference material.

**Intended Use:**

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

**Expiration of Certification:**


The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.


**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

**Sample lot approver:**

  
Monica Bourgeois  
QMS Representative

  
P. 12406  
↓  
P. 12420  
(15)

  
02-20-2023



RM was produced in accordance with the TUV/SUD registered ISO 9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1

ISO 17034 Cert  
No. AR-1936

ISO 17025

**Reference Material Certificate**  
**Product Information Sheet**

**Product Name:** Chlorinated Herbicides Standard  
**Product Number:** HBM-8151A-1  
**Storage Conditions:** Store at Room Temperature (15° to 30°C).

**Lot Number:** 0006686742  
**Lot Issue Date:** 13-Jun-2022  
**Expiration Date:** 31-Jul-2024

Component Name	CERTIFIED VALUES			CAS#	Analyte Lot
	Concentration	Expanded Uncertainty			
acifluorfen	100.1	± 0.5 µg/mL		050594-66-6	NT02057
bentazon	100.1	± 0.5 µg/mL		025057-89-0	RM19026
chloramben	100.2	± 0.5 µg/mL		000133-90-4	RM03672
2,4-D	100.3	± 0.5 µg/mL		000094-75-7	RM17172
dalapon	100.3	± 0.5 µg/mL		000075-99-0	RM19654
2,4-DB	100.2	± 0.5 µg/mL		000094-82-6	RM02866
tetrachloroterephthalic acid	100.2	± 0.5 µg/mL		002136-79-0	RM13887
dicamba	100.3	± 0.5 µg/mL		001918-00-9	RM15881
3,5-dichlorobenzoic acid	100.2	± 0.5 µg/mL		000051-36-5	RM02768
dichlorprop	100.2	± 0.5 µg/mL		000120-36-5	RM19240
dinoseb	100.3	± 0.5 µg/mL		000088-85-7	RM19863
MCPA	10030	± 50 µg/mL		000094-74-6	RM12220
MCPP (mecoprop)	10026	± 50 µg/mL		000093-65-2	RM09273
4-nitrophenol	100.3	± 0.5 µg/mL		000100-02-7	RM03752
pentachlorophenol	100.2	± 0.5 µg/mL		000087-86-5	RM02474
picloram	100.2	± 0.5 µg/mL		001918-02-1	RM19110
silvex	100.2	± 0.5 µg/mL		000093-72-1	RM19595
2,4,5-T	100.3	± 0.5 µg/mL		000093-76-5	NT01808

**Matrix:** methanol (methyl alcohol)

**Description:**

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1089.

*Handwritten:* P 12406, P 12420, 15, RAUF, 02/20/23

**Homogeneity:**

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

**Instructions for Use:**

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

**Safety:**

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this analytical reference material.

**Intended Use:**

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

**Expiration of Certification:**


The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.


**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

**Sample lot approver:**

  
Monica Bourgeois  
QMS Representative

  
P. 12406  
↓  
P. 12420  
(15)

  
02-20-2023



RM was produced in accordance with the TUV/SUD registered ISO 9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1

ISO 17034 Cert  
No. AR-1936

ISO 17025



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis chromatographic plus



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32055 **Lot No.:** A0192429

**Description :** Herbicide Mix #1/ME (Methyl Ester)  
Herbicide Mix #1/ME (Methyl Ester) 200 µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2029 **Storage:** 10°C or colder

**Handling:** This product is photosensitive. **Ship:** Ambient

P12626 / 5  
P12630  
7/5/2023

#### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dicamba methyl ester	6597-78-0	11705400	99%	201.6 µg/mL	+/- 3.4204
2	Dichlorprop methyl ester	57153-17-0	11672100	99%	201.4 µg/mL	+/- 3.4170
3	2,4-D methyl ester	1928-38-7	10048000	99%	201.2 µg/mL	+/- 3.4136
4	2,4,5-TP (silvex) methyl ester	4841-20-7	6364900	99%	201.2 µg/mL	+/- 3.4136
5	2,4,5-T methyl ester	1928-37-6	6875800	98%	200.7 µg/mL	+/- 3.4052
6	Dinoseb methyl ether	6099-79-2	12914300	99%	200.8 µg/mL	+/- 3.4068
7	2,4-DB methyl ester	18625-12-2	12542000	99%	201.0 µg/mL	+/- 3.4102

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

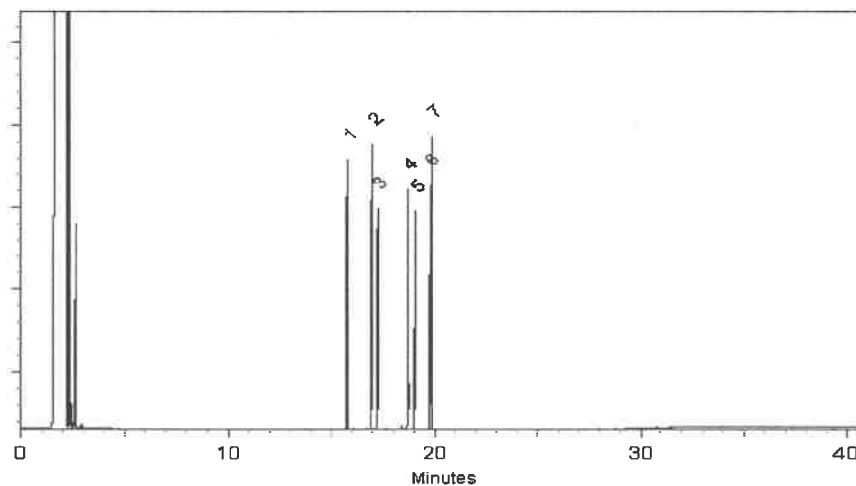

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Penelope Riglin - Operations Tech I

Date Mixed: 09-Dec-2022

Balance Serial # 1128360905

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 12-Dec-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397




110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 32049 Lot No.: A0190000  
Description : 2,4-Dichlorophenylacetic Acid Standard  
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul  
Container Size : 2 mL Pkg Amt: > 1 mL  
Expiration Date : June 30, 2025 Storage: 10°C or colder  
Handling: This product is photosensitive. Ship: Ambient

P 12631  
↓  
P 12650  
(20)

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.8 µg/mL	+/- 1.1843 µg/mL Gravimetric +/- 10.6791 µg/mL Unstressed +/- 10.6970 µg/mL Stressed

Solvent: Methanol  
CAS # 67-56-1  
Purity 99%

#### Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

**Column:**  
150mm x 4.6mm  
Allure C18 Cat. (#9164565)


**Flow Rate:**  
1.0 ml/min.

**Mobile Phase A:**  
0.14% H<sub>3</sub>PO<sub>4</sub> in water

**Mobile Phase B:**  
acetonitrile

**Mobile Phase Composition:**  
90%B Isocratic

**Det. Type:**  
Wavelength: 220 & 254 nm

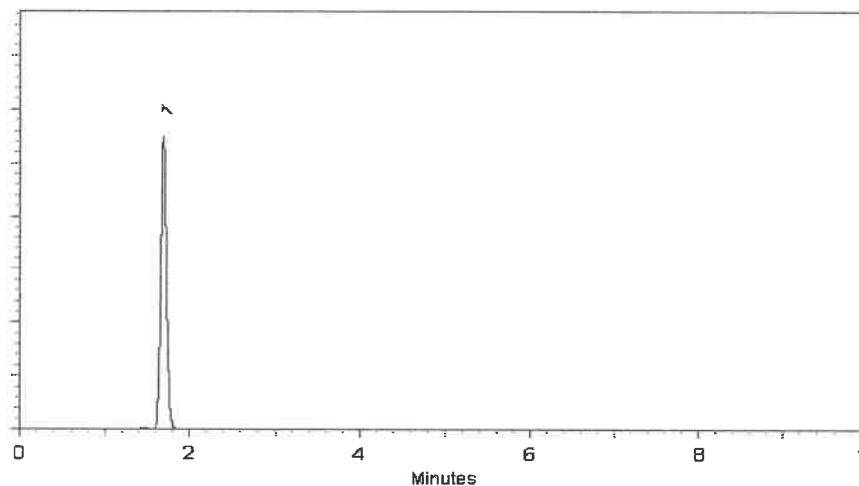

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Bryan Snyder - Operations Tech I

**Date Mixed:** 27-Sep-2022      **Balance:** 1128353505

  
Marlina Cowan - Operations Tech II ARM QC

**Date Passed:** 29-Sep-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397




110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 32049 Lot No.: A0190000  
Description : 2,4-Dichlorophenylacetic Acid Standard  
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul  
Container Size : 2 mL Pkg Amt: > 1 mL  
Expiration Date : June 30, 2025 Storage: 10°C or colder  
Handling: This product is photosensitive. Ship: Ambient

P 12631  
↓  
P 12650  
(20)

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.8 µg/mL	+/- 1.1843 µg/mL Gravimetric +/- 10.6791 µg/mL Unstressed +/- 10.6970 µg/mL Stressed

Solvent: Methanol  
CAS # 67-56-1  
Purity 99%

#### Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.



**Column:**  
150mm x 4.6mm  
Allure C18 Cat. (#9164565)


**Flow Rate:**  
1.0 ml/min.

**Mobile Phase A:**  
0.14% H<sub>3</sub>PO<sub>4</sub> in water

**Mobile Phase B:**  
acetonitrile

**Mobile Phase Composition:**  
90%B Isocratic

**Det. Type:**  
Wavelength: 220 & 254 nm

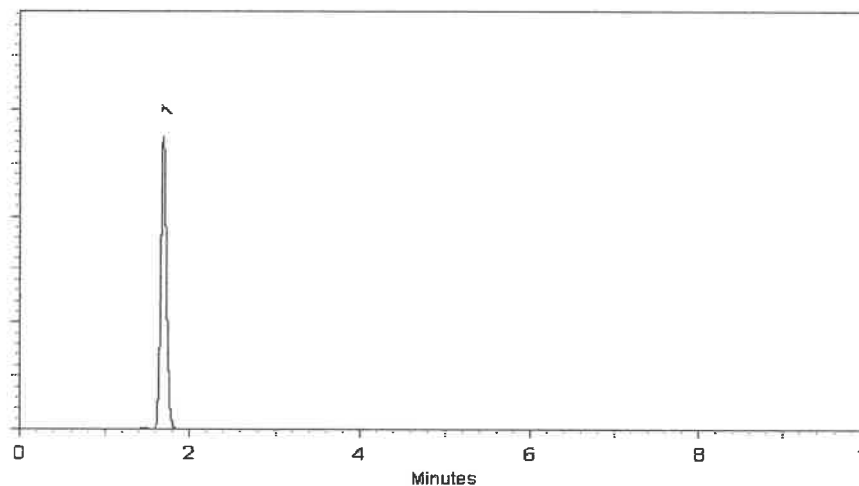

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Bryan Snyder - Operations Tech I

**Date Mixed:** 27-Sep-2022      **Balance:** 1128353505

  
Marlina Cowan - Operations Tech II ARM QC

**Date Passed:** 29-Sep-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 32049 Lot No.: A0190000  
Description : 2,4-Dichlorophenylacetic Acid Standard  
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul  
Container Size : 2 mL Pkg Amt: > 1 mL  
Expiration Date : June 30, 2025 Storage: 10°C or colder  
Handling: This product is photosensitive. Ship: Ambient

P 12631  
↓  
P 12650  
(20)

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.8 µg/mL	+/- 1.1843 µg/mL Gravimetric +/- 10.6791 µg/mL Unstressed +/- 10.6970 µg/mL Stressed

Solvent: Methanol  
CAS # 67-56-1  
Purity 99%

#### Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

**Column:**  
150mm x 4.6mm  
Allure C18 Cat. (#9164565)


**Flow Rate:**  
1.0 ml/min.

**Mobile Phase A:**  
0.14% H<sub>3</sub>PO<sub>4</sub> in water

**Mobile Phase B:**  
acetonitrile

**Mobile Phase Composition:**  
90%B Isocratic

**Det. Type:**  
Wavelength: 220 & 254 nm

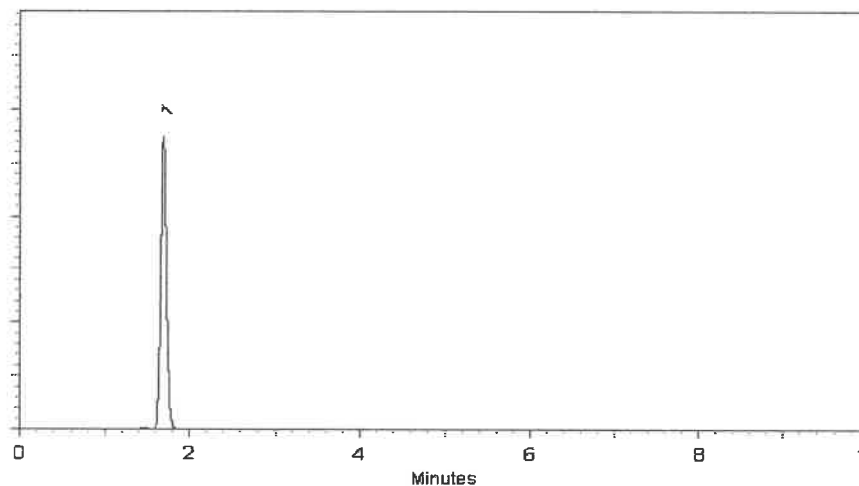

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Bryan Snyder - Operations Tech I

**Date Mixed:** 27-Sep-2022      **Balance:** 1128353505

  
Marlina Cowan - Operations Tech II ARM QC

**Date Passed:** 29-Sep-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 32049 Lot No.: A0190000  
Description : 2,4-Dichlorophenylacetic Acid Standard  
2, 4-Dichlorophenyl Acetic Acid 200µg/mL, Methanol, 1mL/ampul  
Container Size : 2 mL Pkg Amt: > 1 mL  
Expiration Date : June 30, 2025 Storage: 10°C or colder  
Handling: This product is photosensitive. Ship: Ambient

P 12631  
↓  
P 12650  
20

#### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-dichlorophenylacetic acid CAS # 19719-28-9 (Lot S30618V) Purity 99%	200.8 µg/mL	+/- 1.1843 µg/mL Gravimetric +/- 10.6791 µg/mL Unstressed +/- 10.6970 µg/mL Stressed

Solvent: Methanol  
CAS # 67-56-1  
Purity 99%

#### Specific Reference Material Notes:

Failure to derivatize this standard will lead to incorrect quantitative results.

**Column:**  
150mm x 4.6mm  
Allure C18 Cat. (#9164565)


**Flow Rate:**  
1.0 ml/min.

**Mobile Phase A:**  
0.14% H<sub>3</sub>PO<sub>4</sub> in water

**Mobile Phase B:**  
acetonitrile

**Mobile Phase Composition:**  
90%B Isocratic

**Det. Type:**  
Wavelength: 220 & 254 nm

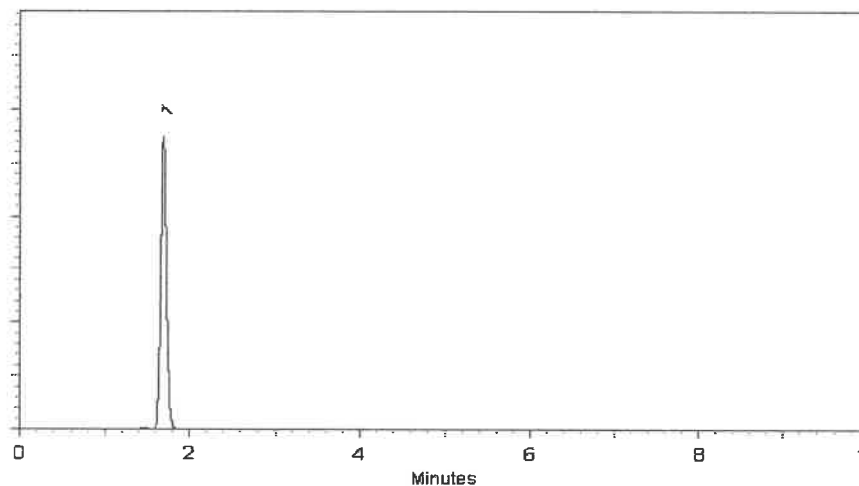

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Bryan Snyder - Operations Tech I

**Date Mixed:** 27-Sep-2022      **Balance:** 1128353505

  
Marlina Cowan - Operations Tech II ARM QC

**Date Passed:** 29-Sep-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

P12706  
↓  
P12715  
/ (10)  
/ 1  
/ 8/15/23

**ISO 17034**

**Reference Material Certificate**  
**Product Information Sheet**

**Product Name:** Chlorinated Methylated Herbicides Standard

**Lot Number:** 0006752480

**Product Number:** HBM-8151M-1

**Lot Issue Date:** 18-Jul-2023

**Storage Conditions:** Store at Room Temperature (15° to 30°C).

**Expiration Date:** 31-Aug-2025

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
acifluorfen methyl ester	100.3 ±	0.5 µg/mL	050594-67-7	RM03058
bentazon methyl derivative	100.2 ±	0.5 µg/mL	061592-45-8	RM13829
chloramben methyl ester	100.4 ±	0.5 µg/mL	007286-84-2	RM03055
2,4-D methyl ester	100.2 ±	0.5 µg/mL	001928-38-7	RM03040
dalapon methyl ester	100.4 ±	0.5 µg/mL	017640-02-7	RM14219
2,4-DB methyl ester	100.2 ±	0.5 µg/mL	018625-12-2	RM03029
DCPA	100.2 ±	0.5 µg/mL	001861-32-1	RM13426
dicamba methyl ester	100.4 ±	0.5 µg/mL	006597-78-0	RM03039
methyl-3,5-dichlorobenzoate	100.1 ±	0.5 µg/mL	002905-67-1	RM03048
dichlorprop methyl ester	100.4 ±	0.5 µg/mL	057153-17-0	NT02086
dinoseb methyl ether	100.5 ±	0.5 µg/mL	006099-79-2	RM03051
MCPA methyl ester	10031 ±	50 µg/mL	002436-73-9	RM12863
MCPP methyl ester	10031 ±	50 µg/mL	023844-56-6	RM20060
4-nitroanisole	100.3 ±	0.5 µg/mL	000100-17-4	RM02806
pentachloroanisole	100.4 ±	0.5 µg/mL	001825-21-4	RM02457
picloram methyl ester	100.2 ±	0.5 µg/mL	014143-55-6	RM03044
silvex methyl ester	100.2 ±	0.5 µg/mL	004841-20-7	RM03799
2,4,5-T methyl ester	100.4 ±	0.5 µg/mL	001928-37-6	RM03033

**Matrix:** methanol (methyl alcohol)

**Description:**

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

**Instructions for Use:**

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

**Safety:**

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this analytical reference material.

**Intended Use:**

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

**Expiration of Certification:**

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

  
Monica Bourgeois  
QMS Representative

P12706 / (10)  
↓  
P12715  
✓ RAUF  
8.15.23



ISO 17034  
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.2

ISO 17025  
Cert No. AT-1937



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Received by  
SG on 8/16/19  
P8807  
P8806

Catalog No.: 32062 Lot No.: A0131940  
Description: Herbicide Mix #4/ME (Methyl Ester)  
Standard #4 (methyl ester) 200µg/mL, Hexane/MTBE(90:10), 1mL/ampul  
Container Size: 2 mL Pkg Amt: > 1 mL  
Expiration Date: October 31, 2024 Storage: 10°C or colder

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)			
1	3,5-Dichlorobenzoic acid methyl ester CAS # 2905-67-1 (Lot 3903900) Purity 99%	202.0 µg/mL	+/- 1.4323	µg/mL	Gravimetric	
			+/- 6.8182	µg/mL	Unstressed	
			+/- 6.8182	µg/mL	Stressed	
2	4-Nitroanisole CAS # 100-17-4 (Lot 24765/7) Purity 99%	200.0 µg/mL	+/- 1.4182	µg/mL	Gravimetric	
			+/- 6.7507	µg/mL	Unstressed	
			+/- 6.7507	µg/mL	Stressed	
3	Pentachloroanisole CAS # 1825-21-4 (Lot 6390100) Purity 99%	201.0 µg/mL	+/- 1.4253	µg/mL	Gravimetric	
			+/- 6.7844	µg/mL	Unstressed	
			+/- 6.7844	µg/mL	Stressed	
4	Chloramben methyl ester CAS # 7286-84-2 (Lot 6487100) Purity 98%	200.9 µg/mL	+/- 1.4245	µg/mL	Gravimetric	
			+/- 6.7810	µg/mL	Unstressed	
			+/- 6.7810	µg/mL	Stressed	
5	Bentazon methyl ester CAS # 61592-45-8 (Lot 817100) Purity 99%	202.0 µg/mL	+/- 1.4323	µg/mL	Gravimetric	
			+/- 6.8182	µg/mL	Unstressed	
			+/- 6.8182	µg/mL	Stressed	
6	Picloram methyl ester CAS # 14143-55-6 (Lot 459-31B) Purity 98%	200.9 µg/mL	+/- 1.4245	µg/mL	Gravimetric	
			+/- 6.7810	µg/mL	Unstressed	
			+/- 6.7810	µg/mL	Stressed	
7	DCPA methyl ester (Chlorthal-dimethyl) CAS # 1861-32-1 (Lot 84-92B) Purity 99%	201.0 µg/mL	+/- 1.4253	µg/mL	Gravimetric	
			+/- 6.7844	µg/mL	Unstressed	
			+/- 6.7844	µg/mL	Stressed	



8	Acifluorfen methyl ester		200.0 µg/mL	+/- 1.4182	µg/mL	Gravimetric
	CAS # 50594-67-7	(Lot 6282300)		+/- 6.7507	µg/mL	Unstressed
	Purity 99%			+/- 6.7507	µg/mL	Stressed

**Solvent:** Hexane/Methyl-tert-butyl-ether  
**CAS #** 110-54-3/1634-04-4  
**Purity** 99%

**Column:**  
 30m x 0.25mm x 0.25µm  
 Rtx-5 (cat.#10223)


**Carrier Gas:**  
 hydrogen-constant pressure 10 psi.

**Temp. Program:**  
 75°C (hold 1 min.) to 330°C  
 @ 20°C/min. (hold 10 min.)

**Inj. Temp:**  
 250°C

**Det. Temp:**  
 330°C

**Det. Type:**  
 FID

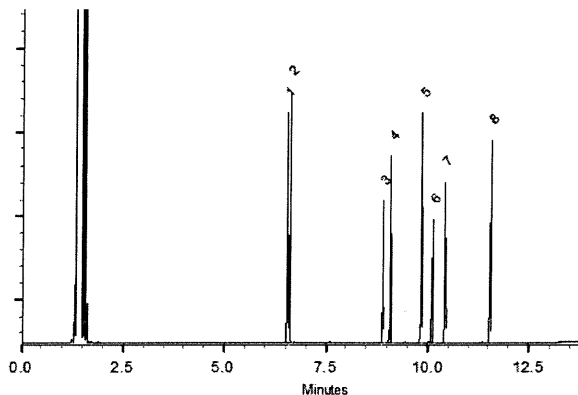

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Cheryl Graham*  
 Cheryl Graham - Mix Technician

**Date Mixed:** 29-Oct-2017

**Balance:** B442140311

*Justine Albertson*  
 Justine Albertson - Operations Tech-ARM QC

**Date Passed:** 30-Oct-2017

Manufactured under Restek's ISO 9001:2008  
 Registered Quality System  
 Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32254 **Lot No.:** A0148063  
**Description :** Dalapon methyl ester Standard  
Dalapon methyl ester 1000µg/mL, Methanol, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2026 **Storage:** 10°C or colder  
**Handling:** This product is photosensitive.

Received by  
SG on 8/16/19  
P8828  
P8826

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Dalapon methyl ester CAS # 17640-02-7 Purity 98% (Lot 1764600)	999.6 µg/mL	+/- 10.0697 µg/mL Gravimetric +/- 34.4896 µg/mL Unstressed +/- 34.4896 µg/mL Stressed

**Solvent:** Methanol  
CAS # 67-56-1  
Purity 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

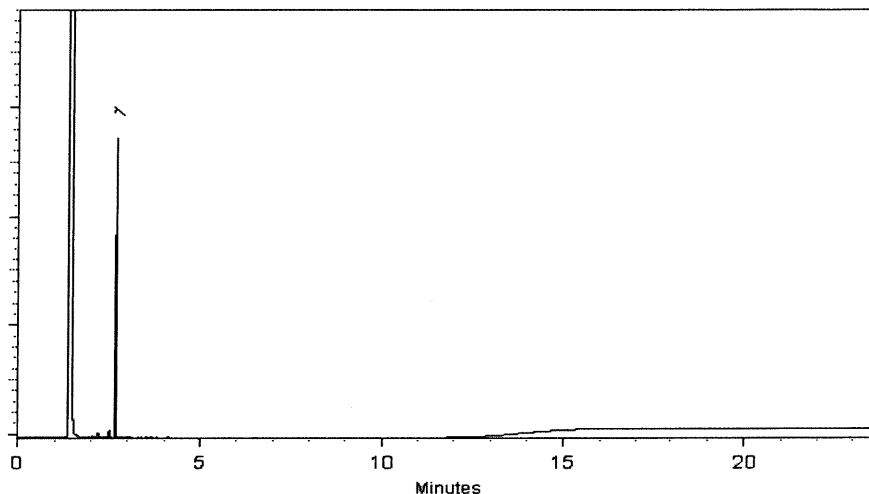

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Bookhamer - Operations Technician I

Date Mixed: 11-Apr-2019

Balance: 1127510105

  
Feng-Yin Lo - QC Analyst

Date Passed: 15-Apr-2019

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Received by  
SG on 9/10/19  
P8892  
P8896

**Catalog No. :** 32059 **Lot No.:** A0152499

**Description :** Herbicide Mix #3/ME (Methyl Ester)  
Herbicide Mix #3/ME (Methyl Ester) 20,000 µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** September 30, 2026 **Storage:** 10°C or colder

**Handling:** This product is photosensitive.

### CERTIFIED VALUES

Elution Order	Compound		Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)							
1	MCPP (Mecoprop) methyl ester		20,004.0    μg/mL	+/-	185.1208	μg/mL	Gravimetric				
	CAS #	23844-56-6                      (Lot 8685200)						+/-	685.5986	μg/mL	Unstressed
	Purity	99%						+/-	685.5986	μg/mL	Stressed
2	MCPA methyl ester		20,012.0    μg/mL	+/-	185.1948	μg/mL	Gravimetric				
	CAS #	2436-73-9                      (Lot 7964600)						+/-	685.8728	μg/mL	Unstressed
	Purity	99%						+/-	685.8728	μg/mL	Stressed
Solvent:	Hexane										
	CAS #	110-54-3									
	Purity	99%									

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

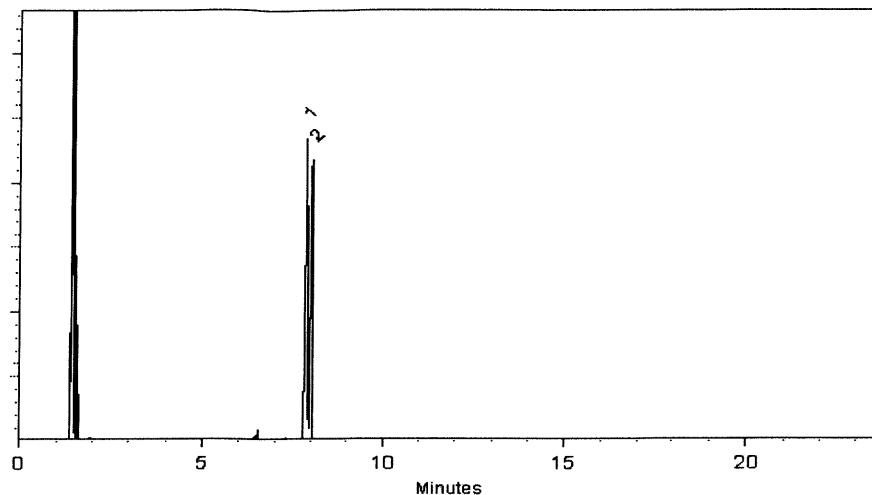

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Bookhamer - Operations Technician I

Date Mixed: 03-Sep-2019

Balance: 1128360905

Jennifer Pollino - Operations Tech-ARM QC

Date Passed: 05-Sep-2019

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 32050 Lot No.: A0152705  
Description : 2,4-Dichlorophenylacetic Acid Methyl Ester Standard  
515 Surrogate (ester) 2, 4-dichlorophenyl Acetic Acid Methyl Ester  
200µg/mL, Hexane, 1mL/ampul  
Container Size : 2 mL Pkg Amt: > 1 mL  
Expiration Date : June 30, 2026 Storage: 10°C or colder  
Handling: This product is photosensitive.

Received by  
SG on 10/11/19  
P8999  
-  
P9008

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-Dichlorophenyl acetic acid methyl ester CAS # 55954-23-9 (Lot CSC42194-01) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL Gravimetric +/- 6.7507 µg/mL Unstressed +/- 6.7507 µg/mL Stressed

Solvent: Hexane  
CAS # 110-54-3  
Purity 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

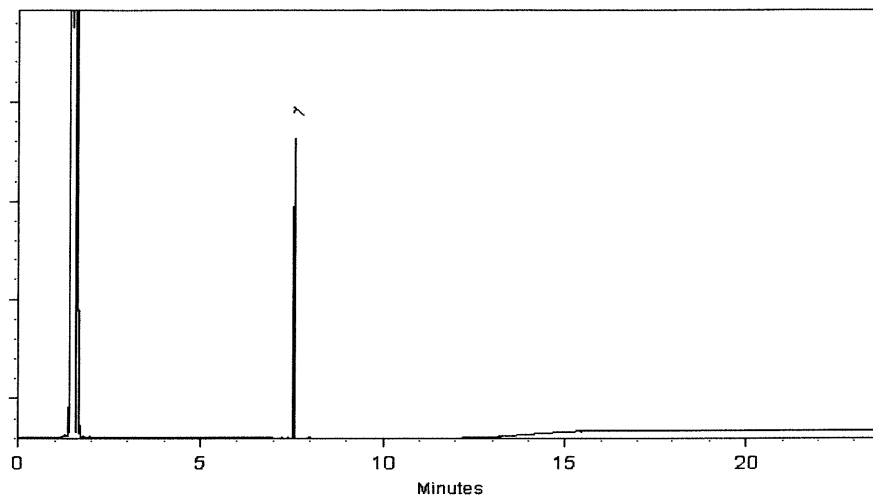

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Cydnei L. Crust*  
Cydnei L. Crust - Mix Technician

**Date Mixed:** 09-Sep-2019

**Balance:** B707717271

*Fang-Yun Lo*  
Fang-Yun Lo - GC Analyst

**Date Passed:** 11-Sep-2019

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

# Certificate of Analysis

300 Technology Drive  
Christiansburg, VA 24073 USA  
inorganicventures.com

P: 800-669-6799/540-585-3030  
F: 540-585-3012  
info@inorganicventures.com

## 1.0 ACCREDITATION / REGISTRATION

**INORGANIC VENTURES** is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



## 2.0 PRODUCT DESCRIPTION

Product Code:	Multi Analyte Custom Grade Solution
Catalog Number:	WW-LFS-1
Lot Number:	T2-MEB723367
Matrix:	5% (v/v) HNO <sub>3</sub>



Value / Analyte(s):	1 000 µg/mL ea: Potassium,	
	600 µg/mL ea: Phosphorus,	
	300 µg/mL ea: Sodium,	Iron,
	200 µg/mL ea: Magnesium, Cerium, Thallium,	Aluminum, Selenium,
	100 µg/mL ea: Lead,	Calcium,
	80 µg/mL ea: Arsenic,	
	70 µg/mL ea: Mercury,	
	50 µg/mL ea: Nickel,	
	40 µg/mL ea: Chromium,	
	30 µg/mL ea: Copper, Vanadium,	Boron,
	20 µg/mL ea: Zinc, Barium, Cadmium, Manganese,	Strontium, Beryllium, Cobalt, Lithium,
	7.5 µg/mL ea: Silver	

### 3.0 CERTIFIED VALUES AND UNCERTAINTIES

<b>ANALYTE</b>	<b>CERTIFIED VALUE</b>	<b>ANALYTE</b>	<b>CERTIFIED VALUE</b>
Aluminum, Al	200.0 ± 0.7 µg/mL	Arsenic, As	80.0 ± 0.7 µg/mL
Barium, Ba	20.00 ± 0.09 µg/mL	Beryllium, Be	20.00 ± 0.13 µg/mL
Boron, B	30.00 ± 0.18 µg/mL	Cadmium, Cd	20.00 ± 0.09 µg/mL
Calcium, Ca	100.0 ± 0.4 µg/mL	Cerium, Ce	200.0 ± 0.8 µg/mL
Chromium, Cr	40.00 ± 0.30 µg/mL	Cobalt, Co	20.00 ± 0.10 µg/mL
Copper, Cu	30.00 ± 0.13 µg/mL	Iron, Fe	300.0 ± 1.3 µg/mL
Lead, Pb	100.0 ± 0.4 µg/mL	Lithium, Li	20.00 ± 0.08 µg/mL
Magnesium, Mg	200.0 ± 0.8 µg/mL	Manganese, Mn	20.00 ± 0.08 µg/mL
Mercury, Hg	70.0 ± 0.3 µg/mL	Nickel, Ni	50.00 ± 0.22 µg/mL
Phosphorus, P	600.0 ± 2.7 µg/mL	Potassium, K	1 000 ± 4 µg/mL
Selenium, Se	200.0 ± 1.3 µg/mL	Silver, Ag	7.50 ± 0.03 µg/mL
Sodium, Na	300.0 ± 1.4 µg/mL	Strontium, Sr	20.01 ± 0.08 µg/mL
Thallium, Tl	200.0 ± 1.4 µg/mL	Vanadium, V	30.00 ± 0.13 µg/mL
Zinc, Zn	20.00 ± 0.09 µg/mL		

**Density:** 1.034 g/mL (measured at 20 ± 4 °C)

**Assay Information:**

<b>ANALYTE</b>	<b>METHOD</b>	<b>NIST SRM#</b>	<b>SRM LOT#</b>
Ag	ICP Assay	3151	160729
Ag	Volhard	999c	999c
Ag	Calculated		See Sec. 4.2
Al	ICP Assay	3101a	140903
Al	EDTA	928	928
As	ICP Assay	3103a	100818
B	ICP Assay	3107	190605
Ba	ICP Assay	3104a	140909
Ba	Gravimetric		See Sec. 4.2
Be	ICP Assay	3105a	090514
Ca	ICP Assay	3109a	130213
Ca	EDTA	928	928
Cd	ICP Assay	3108	130116
Cd	EDTA	928	928
Ce	ICP Assay	3110	090504
Ce	EDTA	928	928
Co	ICP Assay	3113	190630
Co	EDTA	928	928
Cr	ICP Assay	3112a	170630
Cu	ICP Assay	3114	121207
Cu	EDTA	928	928
Fe	ICP Assay	3126a	140812
Fe	EDTA	928	928
Hg	ICP Assay	3133	160921
Hg	EDTA	928	928
K	ICP Assay	3141a	140813
K	Gravimetric		See Sec. 4.2
Li	ICP Assay	3129a	100714
Li	Gravimetric		See Sec. 4.2
Mg	ICP Assay	3131a	140110
Mg	EDTA	928	928
Mn	ICP Assay	3132	050429
Mn	EDTA	928	928
Na	ICP Assay	Traceable to 3152A	S2-NA700842
Na	Gravimetric		See Sec. 4.2
Ni	ICP Assay	3136	120619
Ni	EDTA	928	928
P	ICP Assay	3139a	060717
P	Acidimetric	84L	84L
Pb	ICP Assay	3128	101026
Pb	EDTA	928	928
Se	ICP Assay	3149	100901
Sr	EDTA	928	928
Sr	ICP Assay	Traceable to 3153a	K2-SR650985
Tl	ICP Assay	3158	151215
V	IC Assay	3165	160906
V	EDTA	928	928
Zn	ICP Assay	3168a	120629
Zn	EDTA	928	928

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of  $k = 2$ .

#### Characterization of CRM/RM by Two or More Methods

Certified Value,  $X_{\text{CRM/RM}}$ , where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum(w_i)(X_i)$$

$X_i$  = mean of Assay Method  $i$  with standard uncertainty  $u_{\text{char } i}$

$w_i$  = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum(1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

$k$  = coverage factor = 2

$u_{\text{char}} = [\sum(w_i)^2(u_{\text{char } i}^2)]^{1/2}$  where  $u_{\text{char } i}$  are the errors from each characterization method

$u_{\text{bb}}$  = bottle to bottle homogeneity standard uncertainty

$u_{\text{Its}}$  = long term stability standard uncertainty (storage)

$u_{\text{ts}}$  = transport stability standard uncertainty

#### Characterization of CRM/RM by One Method

Certified Value,  $X_{\text{CRM/RM}}$ , where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a)(u_{\text{char } a})$$

$X_a$  = mean of Assay Method A with

$u_{\text{char } a}$  = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

$k$  = coverage factor = 2

$u_{\text{char } a}$  = the errors from characterization

$u_{\text{bb}}$  = bottle to bottle homogeneity standard uncertainty

$u_{\text{Its}}$  = long term stability standard uncertainty (storage)

$u_{\text{ts}}$  = transport stability standard uncertainty

## 4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

### 4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

### 4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

### 4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

## 5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

## 6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

## 7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

### 7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit [www.inorganicventures.com/TCT](http://www.inorganicventures.com/TCT)

**Low Silver Note:** This solution contains "LOW" levels of Silver. Please store this entire bottle inside a sealed glass jar.

## 8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

## 9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

## 10.0 QUALITY STANDARD DOCUMENTATION

### 10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

### 10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

### 10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

## 11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

### 11.1 Certification Issue Date

August 30, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

### 11.2 Lot Expiration Date

- **August 30, 2026**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

### 11.3 Period of Validity


- Sealed TCT Bag Open Date: \_\_\_\_\_

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

## 12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

### Certificate Approved By:

Thomas Kozikowski  
Manager, Quality Control



### Certifying Officer:

Paul Gaines  
Chairman / Senior Technical Director

