


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022924\
Data File : BF137438.D
Acq On : 29 Feb 2024 12:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 01 12:53:33 2024

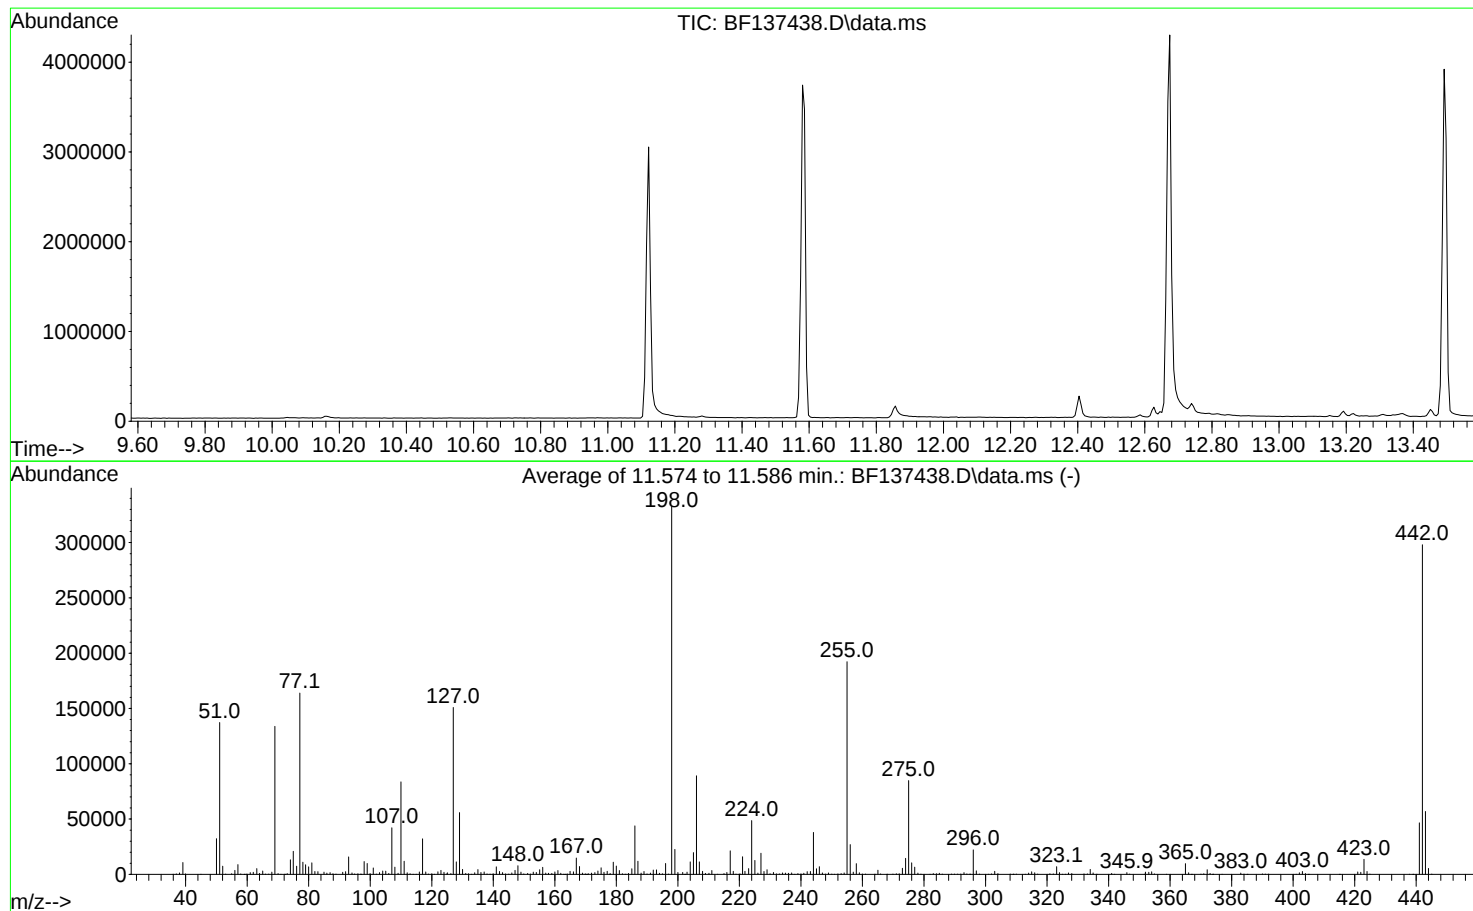




AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	137316	PASS
68	69	0.00	2	1.5	2001	PASS
69	198	0.00	100	40.2	133872	PASS
70	69	0.00	2	0.5	695	PASS
127	198	10	80	45.4	150923	PASS
197	198	0.00	2	0.1	294	PASS
198	198	100	100	100.0	332629	PASS
199	198	5	9	6.8	22609	PASS
275	198	10	60	25.5	84720	PASS
365	198	1	100	2.9	9638	PASS
441	198	0.01	100	14.0	46649	PASS
442	442	50	100	100.0	298093	PASS
443	442	15	24	19.1	56885	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022924\
Data File : BF137438.D
Acq On : 29 Feb 2024 12:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 01 03:46:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 03:39:04 2024
Response via : Initial Calibration

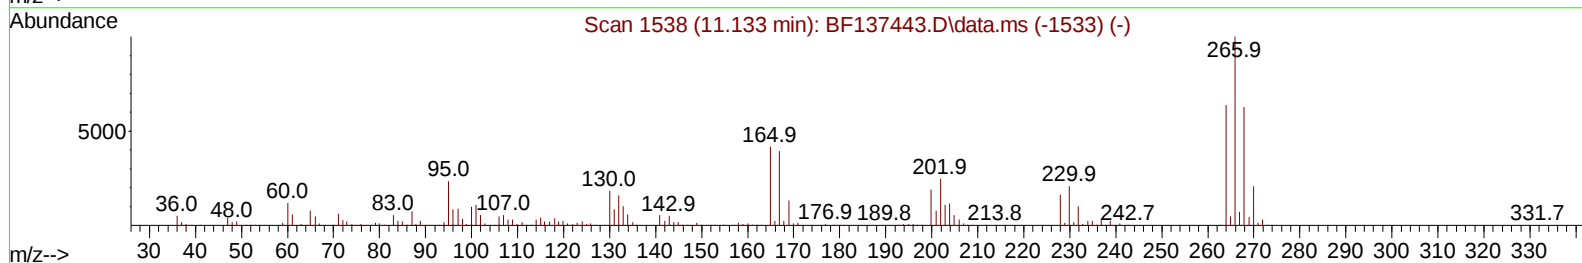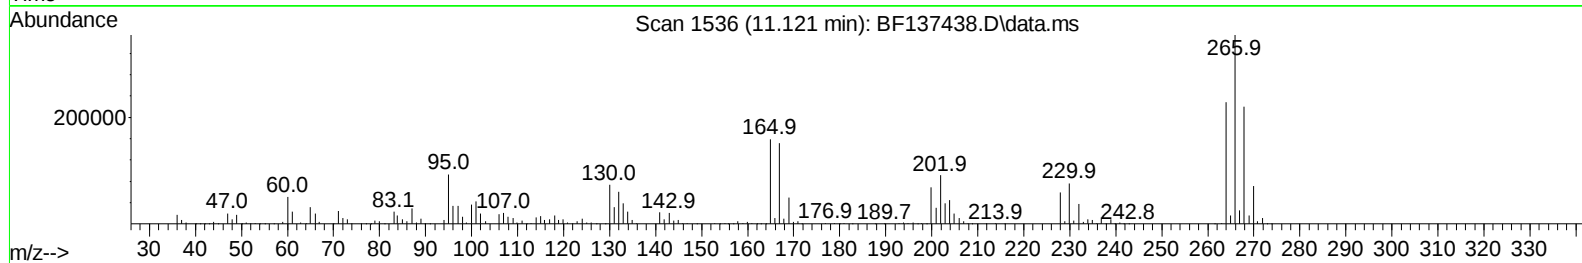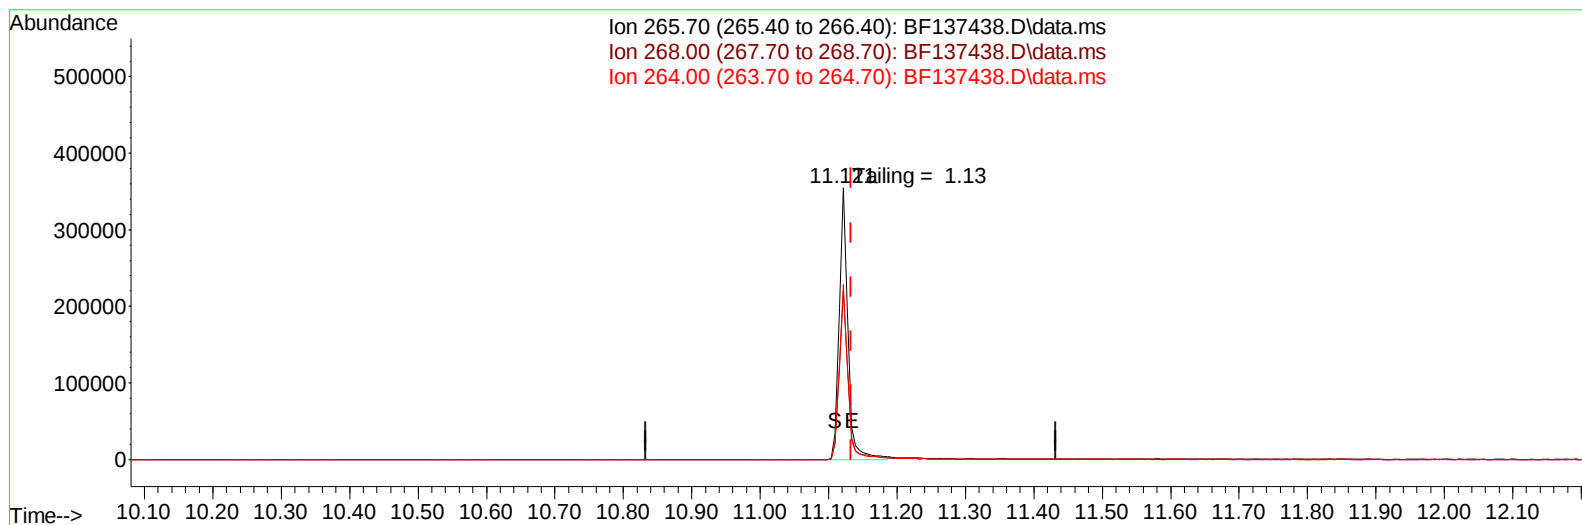

TIC: BF137438.D\data.ms

(70) Pentachlorophenol (C)

11.121min (-0.012) 648810.93 ng




response 319291

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.70	62.17
264.00	63.60	64.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF022924\
Data File : BF137438.D
Acq On : 29 Feb 2024 12:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 01 03:46:48 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF022924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 03:39:04 2024
Response via : Initial Calibration

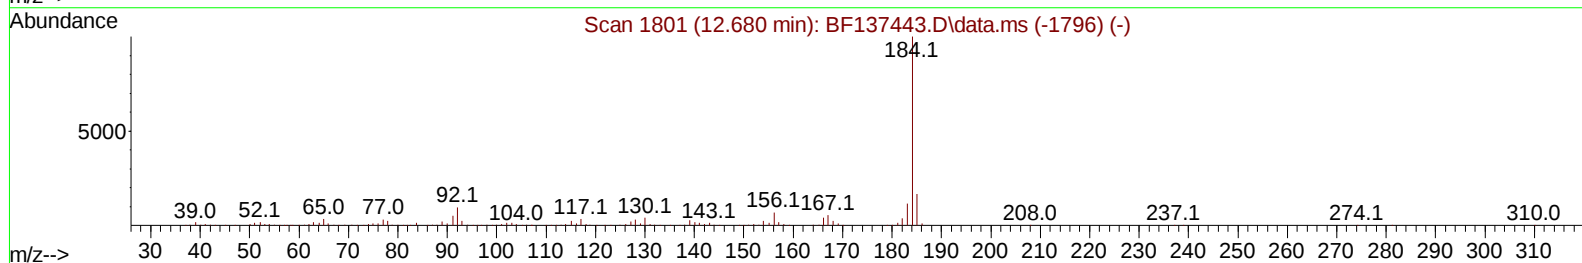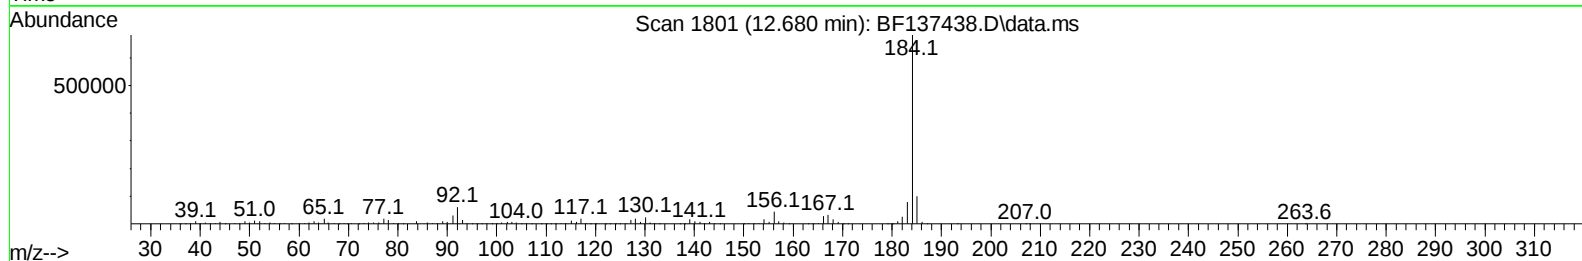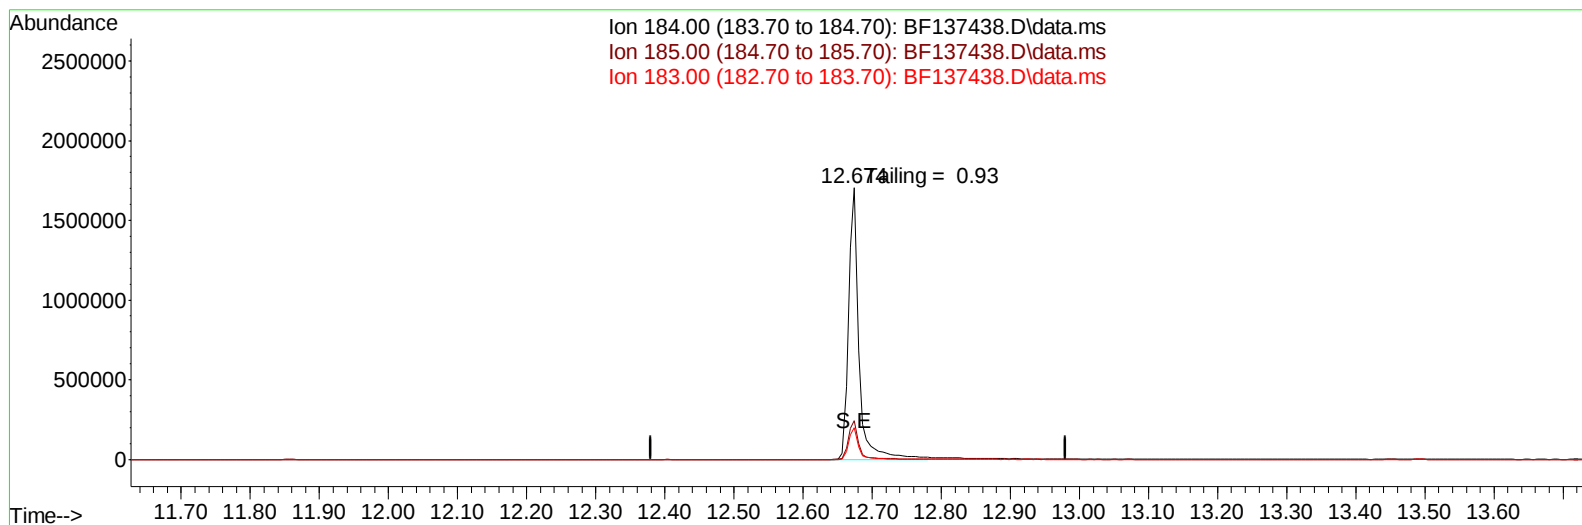

TIC: BF137438.D\data.ms

(77) Benzidine

12.680min (-12.680) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	16.50	0.00#
183.00	11.60	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/29/2024	BNA_F	<u>BF137438.D</u>
Compound Name	Response	Retention Time
DDT	638313	13.492
DDD	13327	13.192
DDE	1300	12.857
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14627	652940	2.24

Instrument :
BNA_F
ClientSampleId :
DFTPP