


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031324\
Data File : BG060620.D
Acq On : 13 Mar 2024 10:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 00:45:22 2024

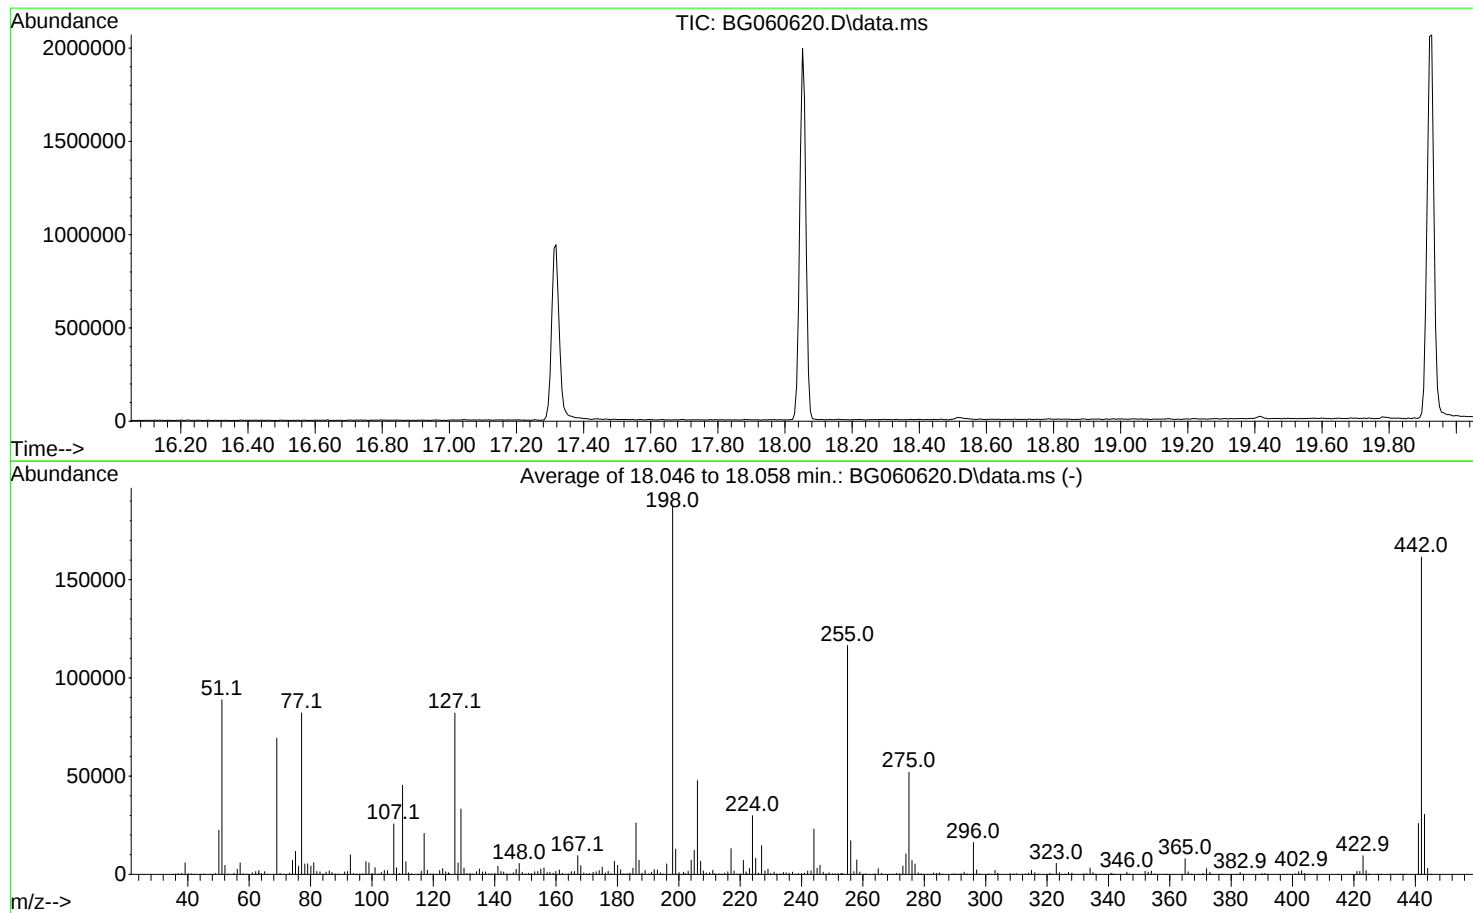




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	88843	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.0	69307	PASS
70	69	0.00	2	0.5	354	PASS
127	198	10	80	43.8	82093	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	187264	PASS
199	198	5	9	6.9	12835	PASS
275	198	10	60	27.8	51968	PASS
365	198	1	100	4.3	7959	PASS
441	198	0.01	100	13.8	25915	PASS
442	442	50	100	100.0	161400	PASS
443	442	15	24	18.9	30555	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031324\
Data File : BG060620.D
Acq On : 13 Mar 2024 10:02
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 14 00:52:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 00:45:22 2024
Response via : Initial Calibration

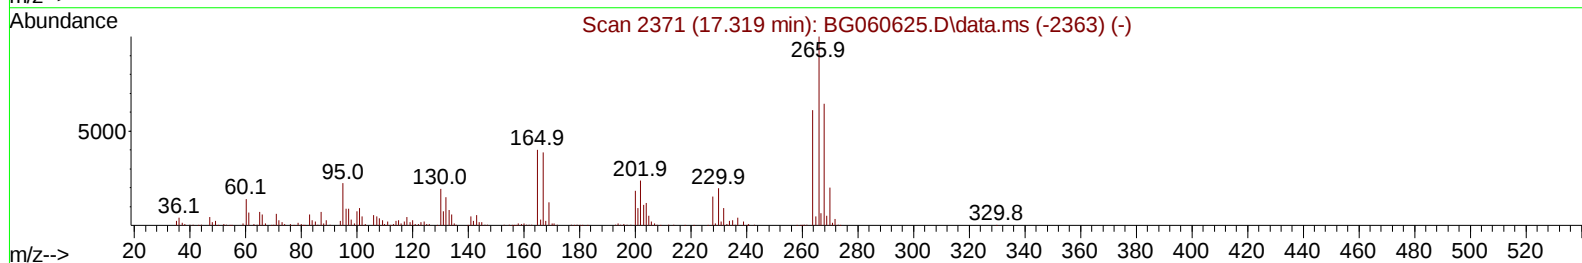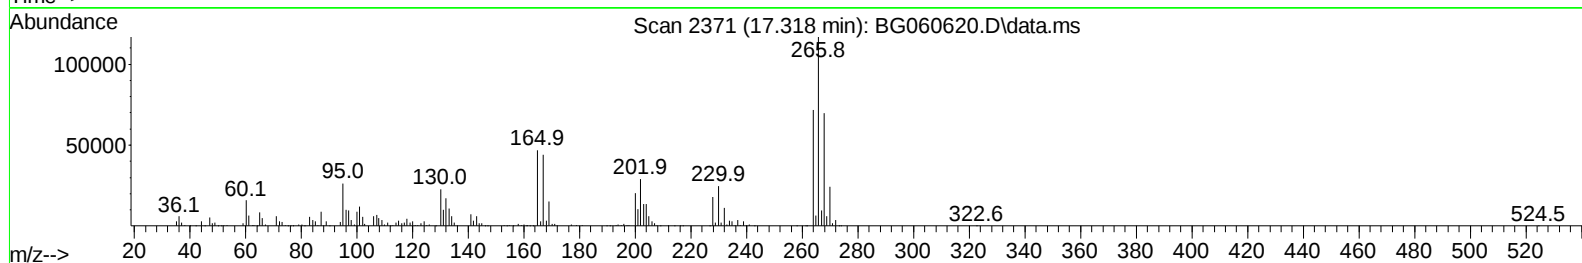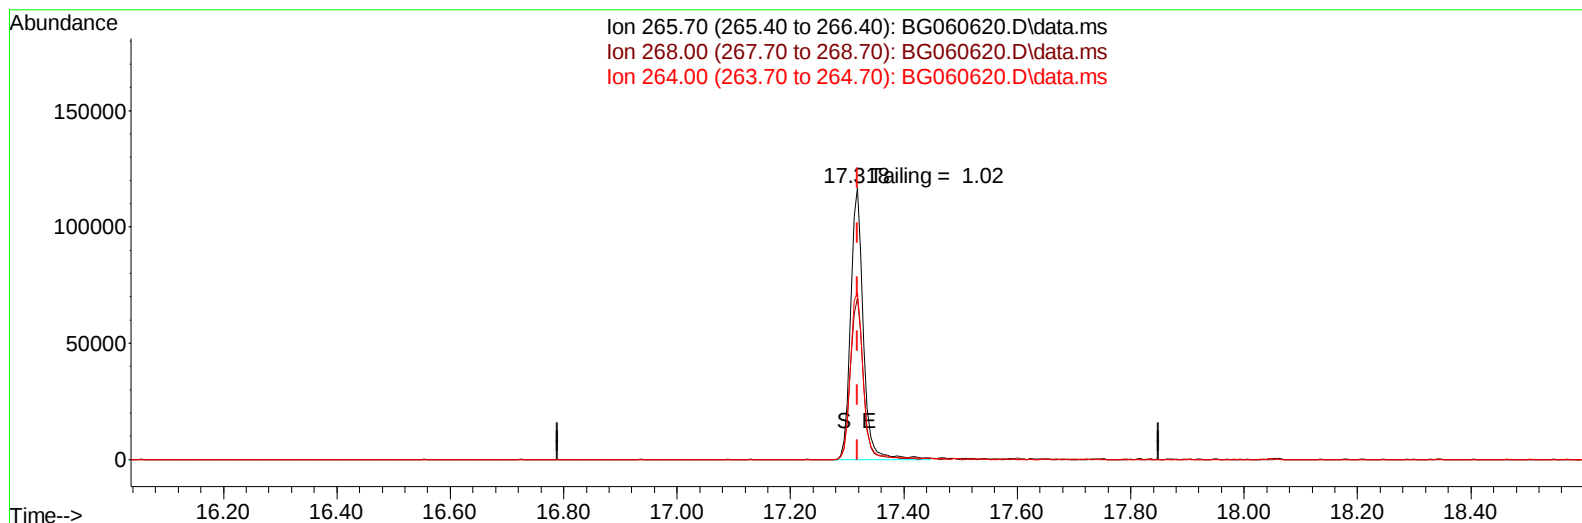

TIC: BG060620.D\data.ms

(70) Pentachlorophenol (C)

17.318min (-0.001) 405314.76 ng

response 179139

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	59.60
264.00	61.10	61.40
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/13/2024	BNA_G	<u>BG060620.D</u>
Compound Name	Response	Retention Time
DDT	448327	21.137
DDD	10923	20.678
DDE	0	20.117
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10923	459250	2.38

Instrument :
BNA_G
ClientSampleId :
DFTPP