
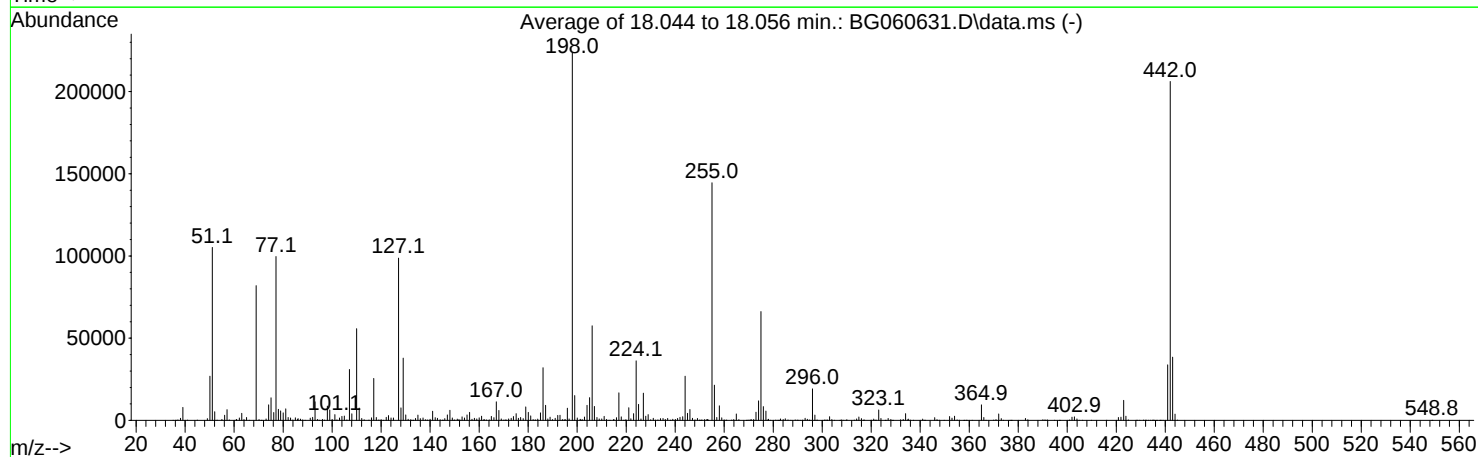


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031424\
Data File : BG060631.D
Acq On : 14 Mar 2024 9:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 00:45:22 2024

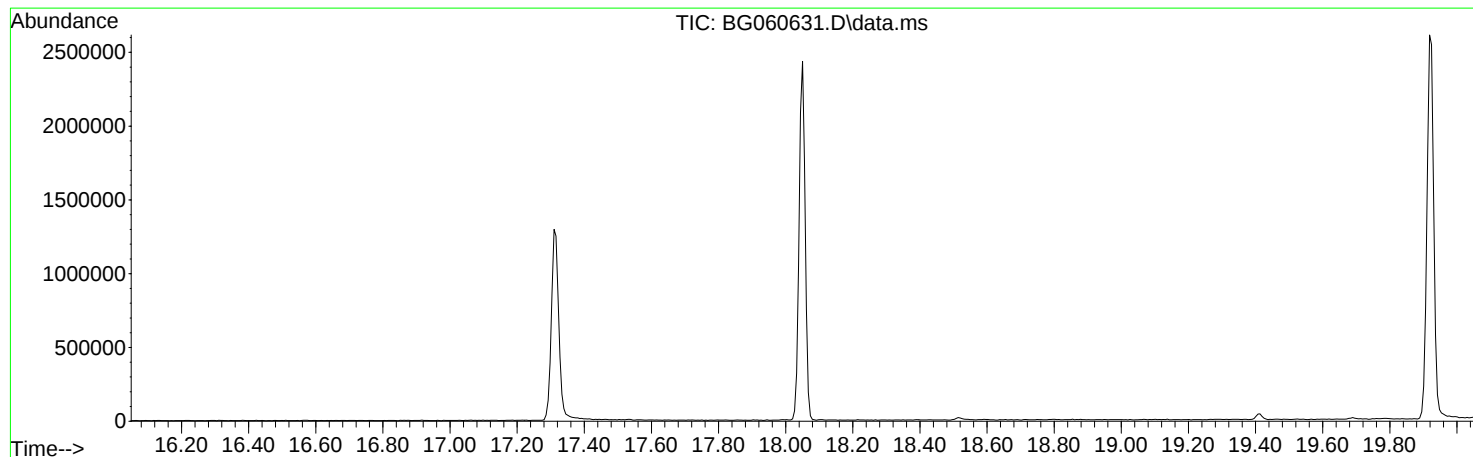




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	105189	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.6	81973	PASS
70	69	0.00	2	0.6	482	PASS
127	198	10	80	44.1	98709	PASS
197	198	0.00	2	0.4	876	PASS
198	198	100	100	100.0	223765	PASS
199	198	5	9	6.7	15103	PASS
275	198	10	60	29.6	66189	PASS
365	198	1	100	4.2	9493	PASS
441	198	0.01	100	15.1	33749	PASS
442	442	50	100	100.0	206165	PASS
443	442	15	24	18.6	38427	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031424\
Data File : BG060631.D
Acq On : 14 Mar 2024 9:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 14 12:23:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 00:45:22 2024
Response via : Initial Calibration

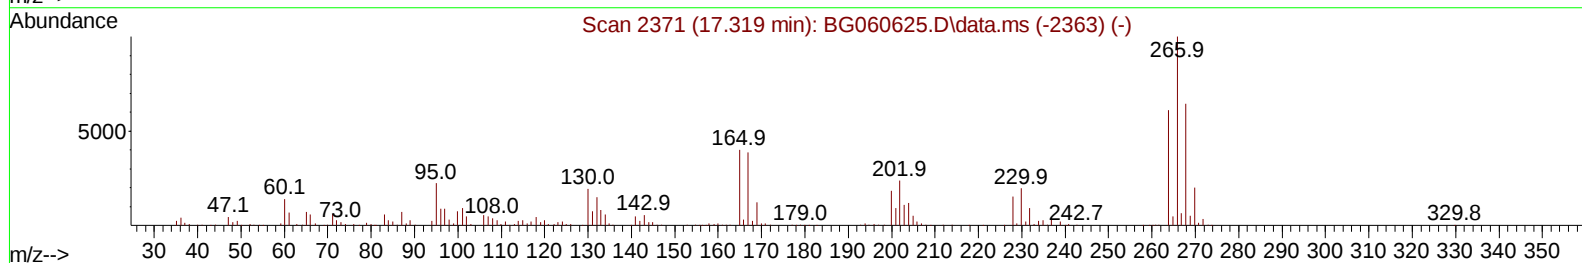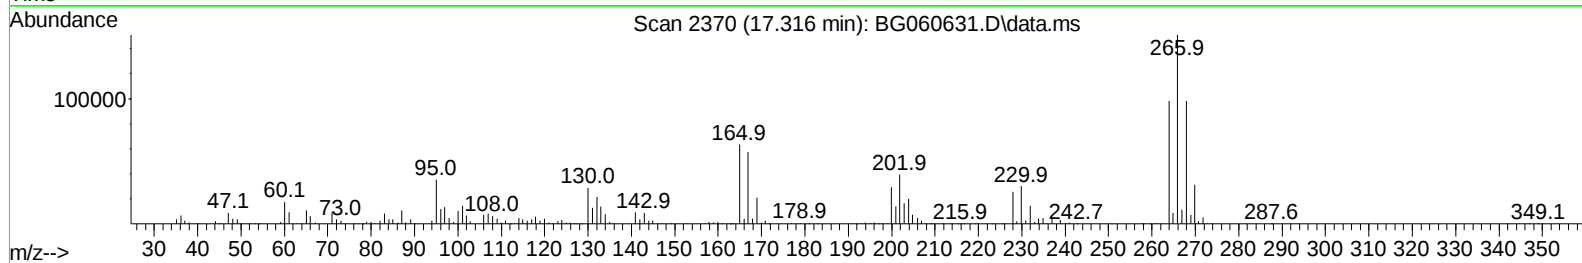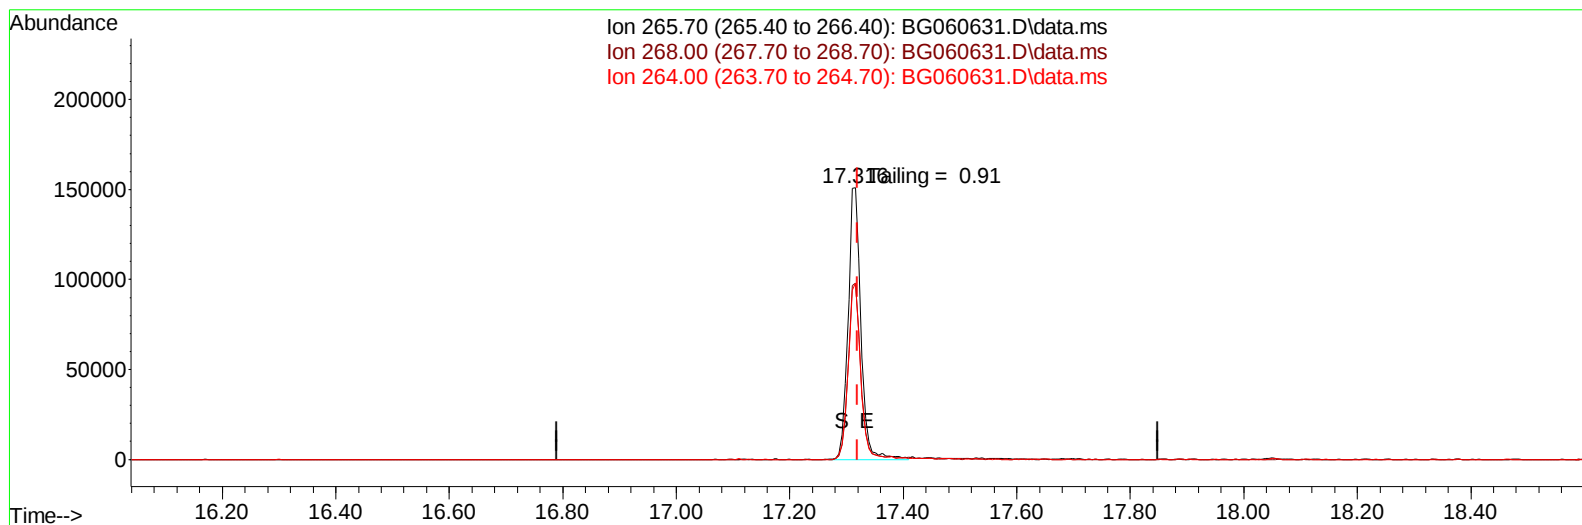

TIC: BG060631.D\data.ms

(70) Pentachlorophenol (C)

17.316min (-0.003) 241234.25 ng




response 238440

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	65.08
264.00	61.10	65.07
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031424\
Data File : BG060631.D
Acq On : 14 Mar 2024 9:44
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 14 12:23:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 00:45:22 2024
Response via : Initial Calibration

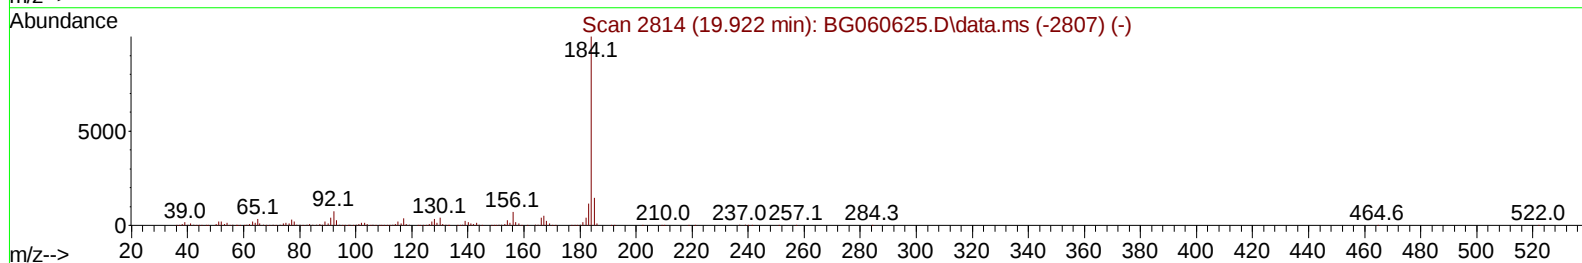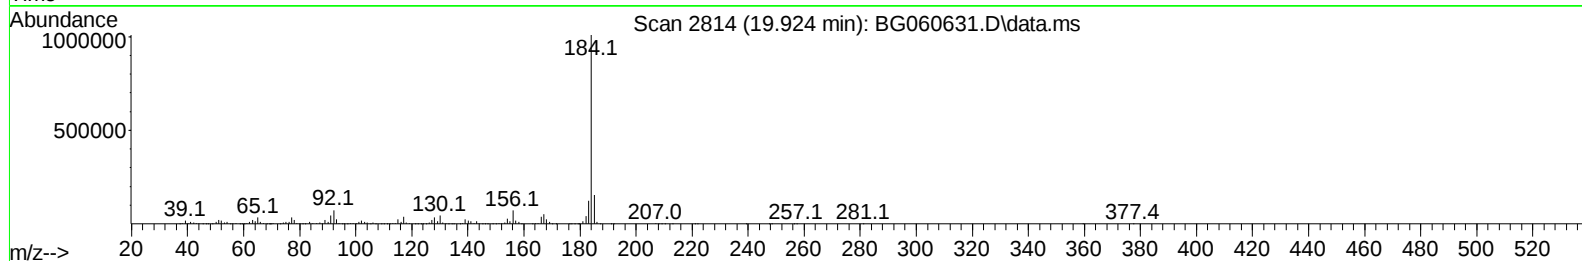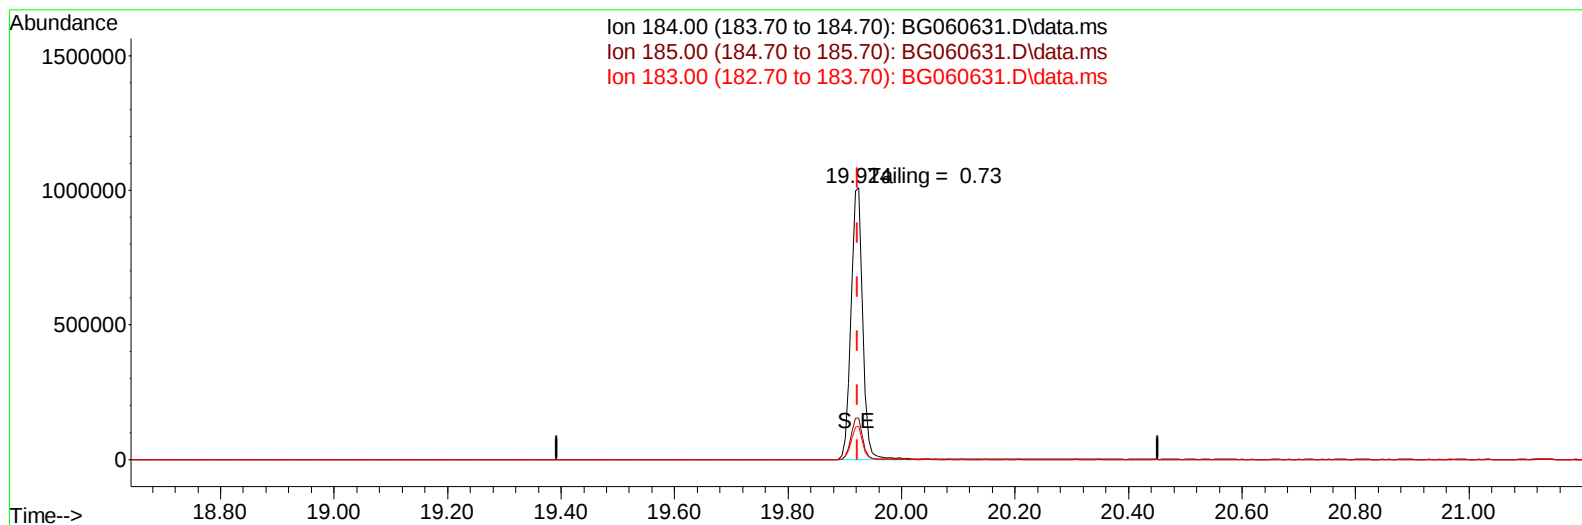

TIC: BG060631.D\data.ms

(77) Benzydine

19.924min (+ 0.002) 5207.67 ng

response 1443715

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	15.11
183.00	11.50	12.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/14/2024	BNA_G	<u>BG060631.D</u>
Compound Name	Response	Retention Time
DDT	585704	21.135
DDD	13691	20.676
DDE	721	20.165
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14412	600116	2.40

Instrument :
BNA_G
ClientSampleId :
DFTPP