


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031424\
Data File : BG060648.D
Acq On : 14 Mar 2024 21:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 00:45:22 2024

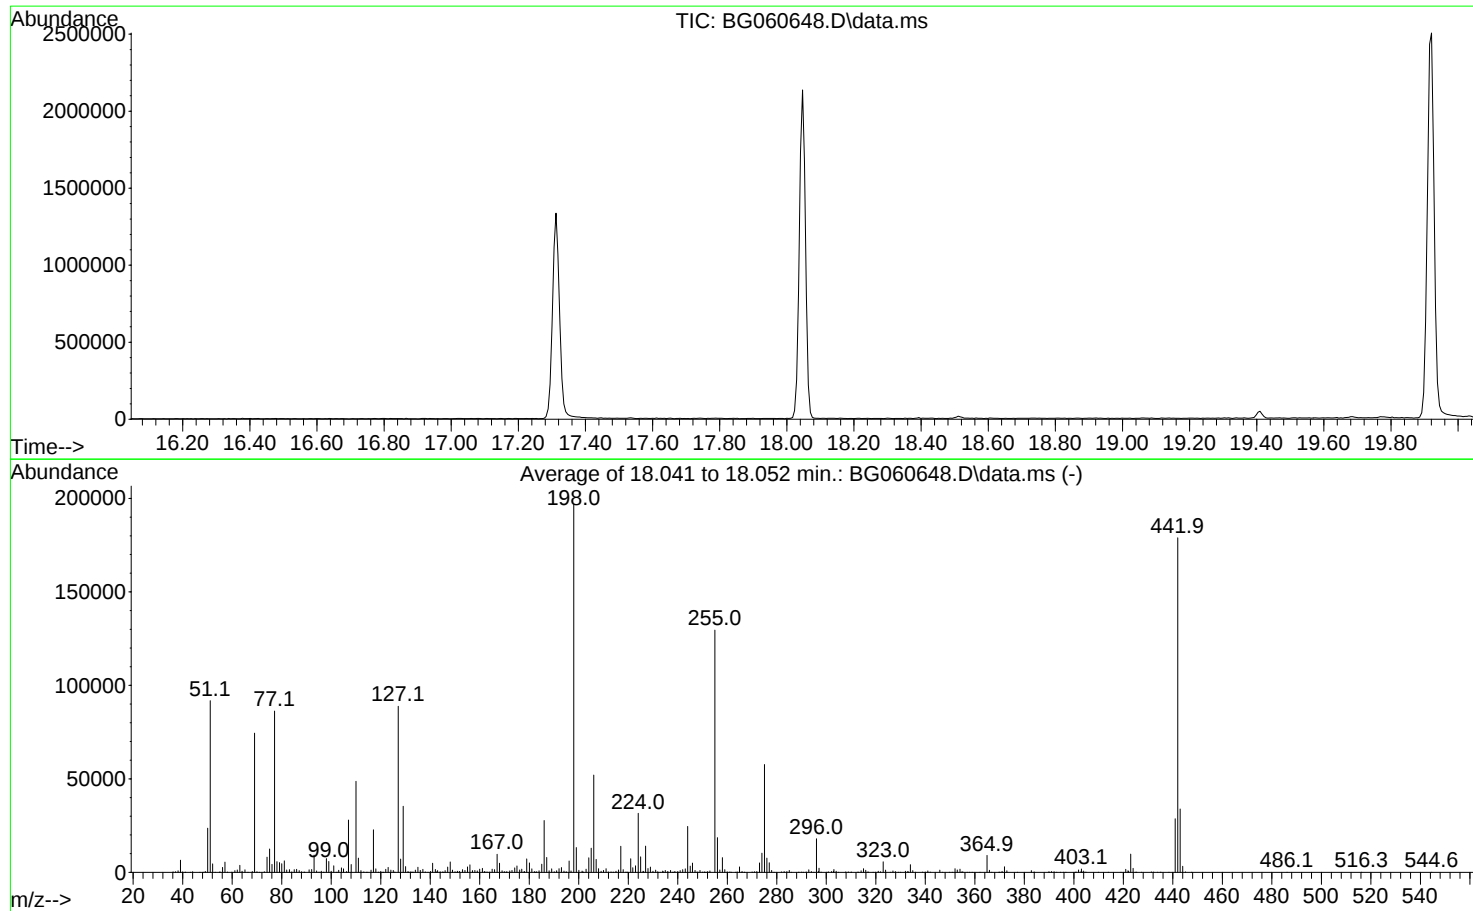




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2487

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	46.7	91803	PASS
68	69	0.00	2	0.6	465	PASS
69	198	0.00	100	37.9	74475	PASS
70	69	0.00	2	0.5	340	PASS
127	198	10	80	45.2	88861	PASS
197	198	0.00	2	0.4	763	PASS
198	198	100	100	100.0	196736	PASS
199	198	5	9	6.8	13290	PASS
275	198	10	60	29.3	57675	PASS
365	198	1	100	4.6	9038	PASS
441	198	0.01	100	14.6	28659	PASS
442	442	50	100	100.0	178965	PASS
443	442	15	24	18.9	33907	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031424\
Data File : BG060648.D
Acq On : 14 Mar 2024 21:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 15 02:26:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 00:45:22 2024
Response via : Initial Calibration

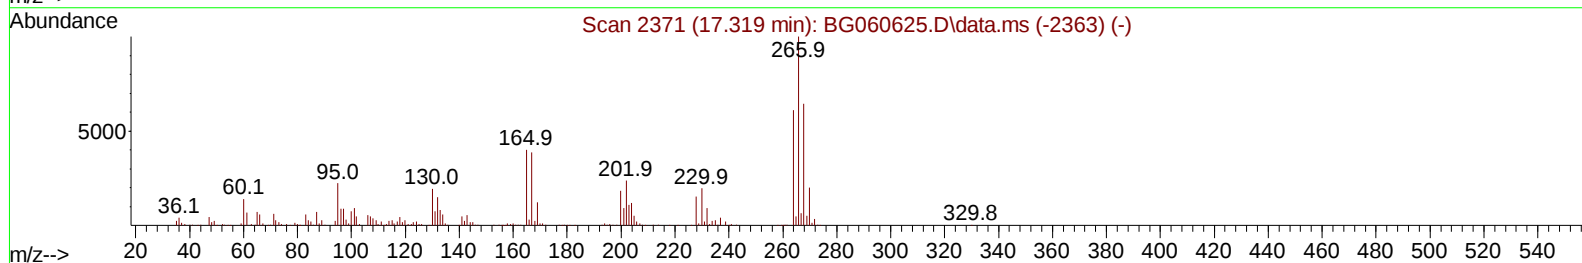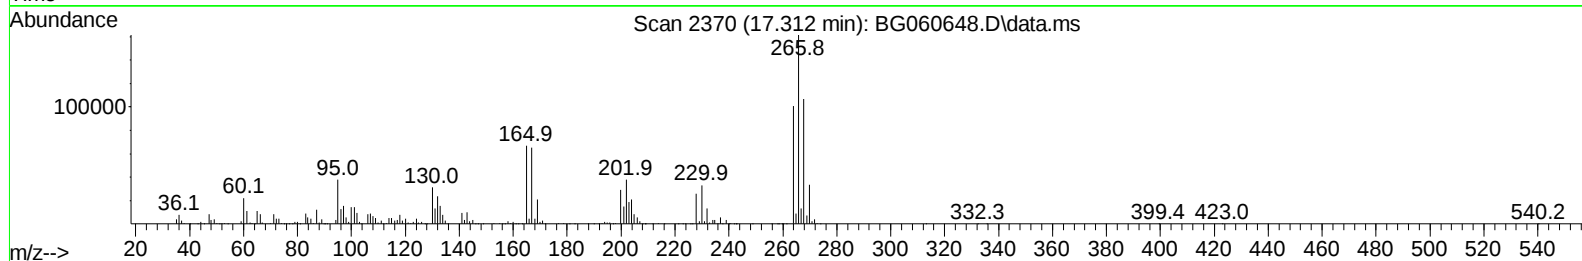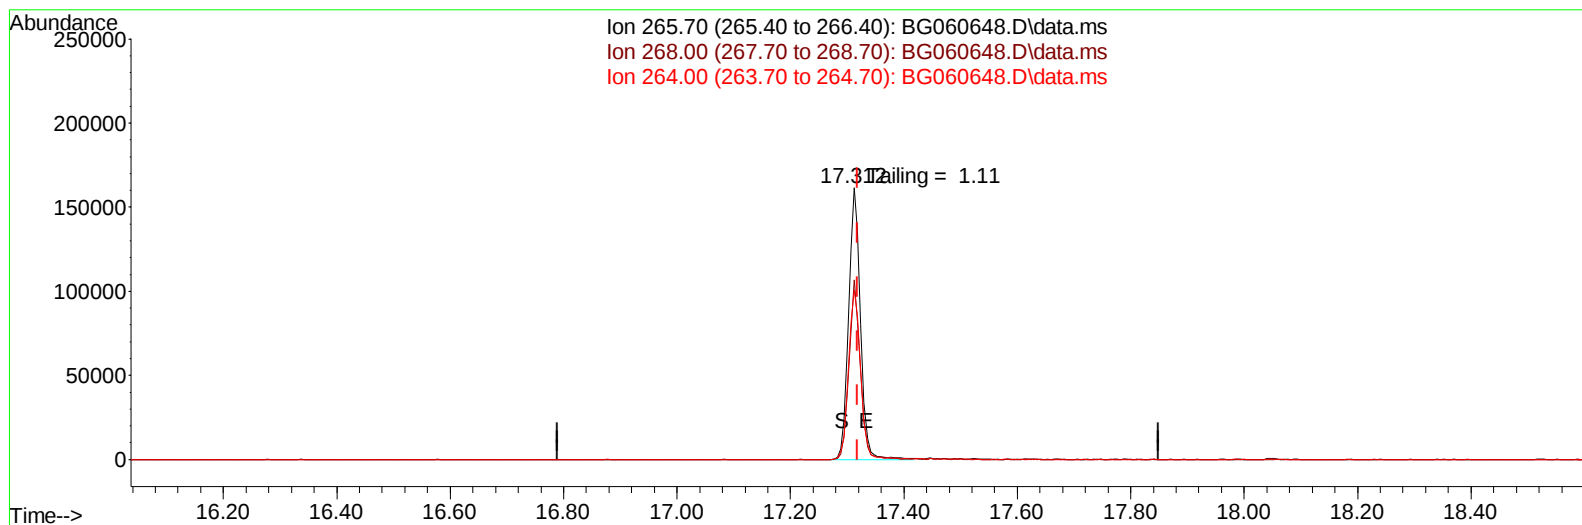

TIC: BG060648.D\data.ms

(70) Pentachlorophenol (C)

17.312min (-0.007) 359159.45 ng




response 233780

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	66.07
264.00	61.10	62.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG031424\
Data File : BG060648.D
Acq On : 14 Mar 2024 21:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 15 02:26:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 00:45:22 2024
Response via : Initial Calibration

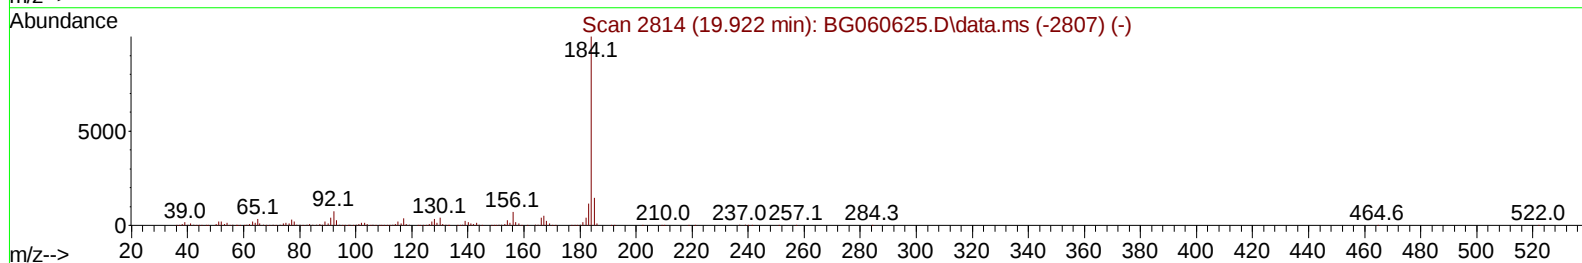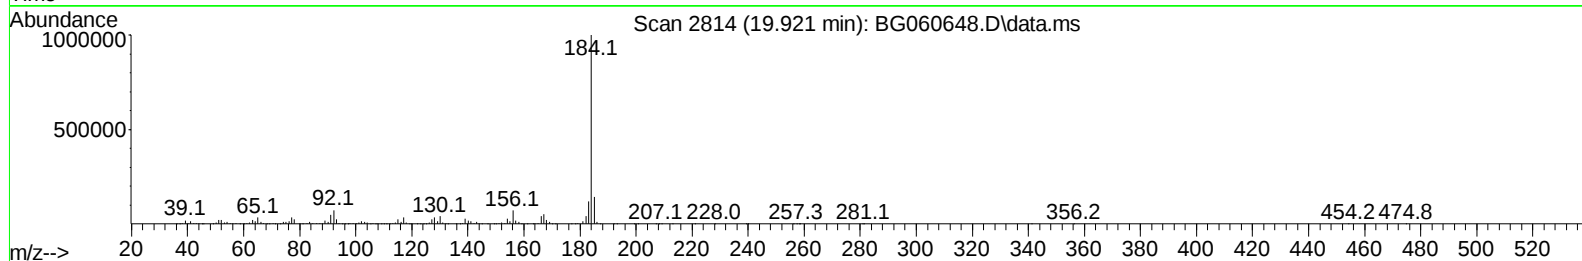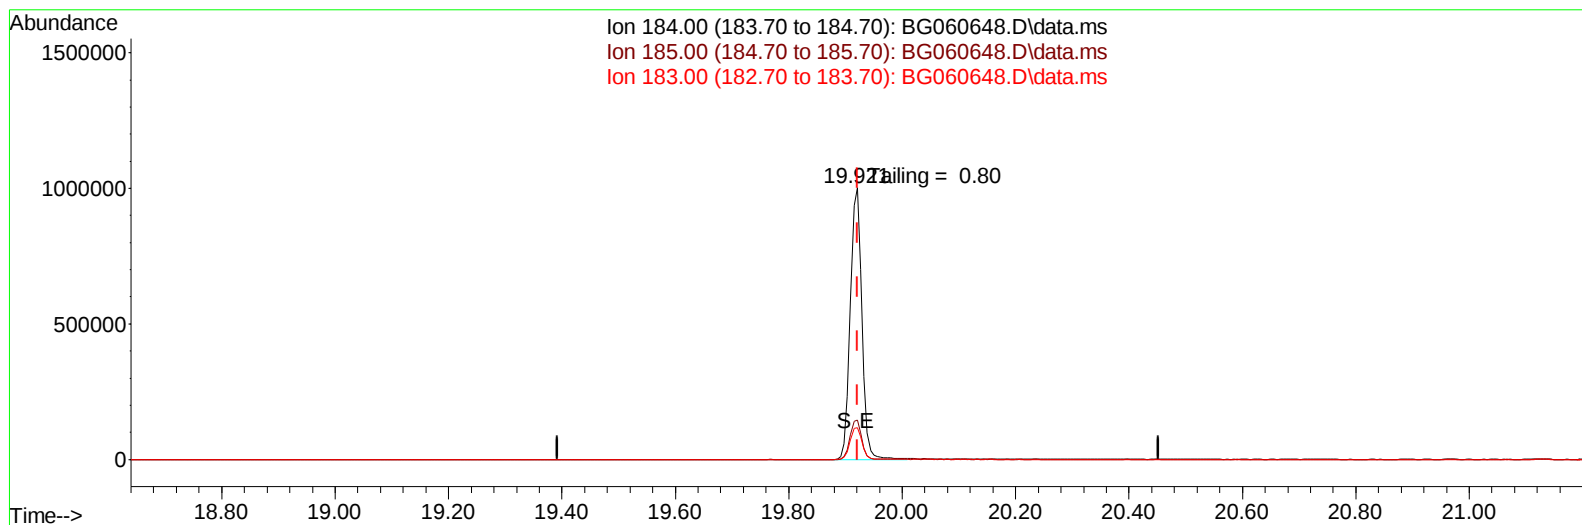

TIC: BG060648.D\data.ms

(77) Benzidine

19.921min (-0.001) 735570.01 ng

response 1421367

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.43
183.00	11.50	11.76
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/14/2024	BNA_G	<u>BG060648.D</u>
Compound Name	Response	Retention Time
DDT	602623	21.131
DDD	12421	20.673
DDE	1154	20.162
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13575	616198	2.20

Instrument :
BNA_G
ClientSampleId :
DFTPP