

Prep Standard - Chemical Standard Summary

Order ID : P2403
Test : Diesel Range Organics
Prepbatch ID : PB160781,
Sequence ID/Qc Batch ID: FG050924,

Standard ID :
EP2479,EP2480,PP23069,PP23111,PP23139,PP23140,PP23142,PP23366,PP23367,PP23368,PP23369,PP23370,PP23371,PP23372,PP23373,PP23374,

Chemical ID :
E2865,E3551,E3678,E3706,E3734,E3736,P11120,P12303,P12305,P12306,P12307,P13105,P13112,P9825,V11253,V14137,W2606,



| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|---|----------------------|------------------------|------------------|------------------------|--------------------|------------------------|------------------|-----------------------------------|
| 3923 | Baked Sodium Sulfate | EP2479 | 05/02/2024 | 07/03/2024 | Rajesh Parikh | Extraction_SC ALE_2 | None | RUPESHKUMAR SHAH 05/02/2024 |
| <u>FROM</u> 4000.00000gram of E3551 = Final Quantity: 4000.000 gram <div></div> | | | | | | | | |

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|---|--------------------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|-----------------------------------|
| 2017 | 1:1 ACETONE/METHYLENE CHLORIDE | EP2480 | 05/02/2024 | 10/30/2024 | Rajesh Parikh | None | None | RUPESHKUMAR SHAH 05/02/2024 |
| <u>FROM</u> 8000.00000ml of E3734 + 8000.00000ml of E3736 = Final Quantity: 16000.000 ml | | | | | | | | |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 231 | 10 PPM GRO STD 1ST SOURCE | PP23139 | 03/11/2024 | 08/12/2024 | Yogesh Patel | None | None | Ankita Jodhani |
| | | | | | | | | 03/18/2024 |

FROM 0.11100ml of P11120 + 9.89000ml of V14137 = Final Quantity: 10.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 233 | 10 PPM GRO STD 2nd SOURCE | PP23140 | 03/11/2024 | 08/12/2024 | Yogesh Patel | None | None | Ankita Jodhani |
| | | | | | | | | 03/18/2024 |

FROM 0.11100ml of P9825 + 9.89000ml of V14137 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3619 | 25 PPM AAA-TFT Surg | PP23142 | 03/11/2024 | 08/12/2024 | Yogesh Patel | None | None | Ankita Jodhani |
| | | | | | | | | 03/18/2024 |

FROM 0.10000ml of V11253 + 9.90000ml of V14137 = Final Quantity: 10.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 238 | 5 PPB ICC GRO STD | PP23366 | 05/08/2024 | 08/12/2024 | Yogesh Patel | None | None | Ankita Jodhani |
| | | | | | | | | 05/09/2024 |

FROM 5.00000ml of W2606 + 0.00100ml of PP23142 + 0.00250ml of PP23139 = Final Quantity: 5.004 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 237 | 10 PPB ICC GRO STD | PP23367 | 05/08/2024 | 08/12/2024 | Yogesh Patel | None | None | Ankita Jodhani |
| | | | | | | | | 05/09/2024 |

FROM 5.00000ml of W2606 + 0.00200ml of PP23142 + 0.00500ml of PP23139 = Final Quantity: 5.007 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 239 | 20 PPB ICC GRO STD | PP23368 | 05/08/2024 | 08/12/2024 | Yogesh Patel | None | None | Ankita Jodhani |
| | | | | | | | | 05/09/2024 |

FROM 5.00000ml of W2606 + 0.00400ml of PP23142 + 0.01000ml of PP23139 = Final Quantity: 5.014 ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922



| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|------------------------------|
| 240 | 20 PPB ICV GRO STD | PP23371 | 05/08/2024 | 08/12/2024 | Yogesh Patel | None | None | Ankita Jodhani 05/09/2024 |

| FROM | |
|--|----------------------------|
| 5.00000ml of W2606 + 0.00400ml of PP23142 + 0.01000ml of PP23140 | = Final Quantity: 5.014 ml |

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|------------------------------|
| 241 | 20 PPB CCC GRO STD | PP23372 | 05/08/2024 | 08/12/2024 | Yogesh Patel | None | None | Ankita Jodhani 05/13/2024 |

| FROM | |
|---|--|
| 5.00000ml of W2606 + 0.00400ml of PP23142 + 0.01000ml of PP23139 = Final Quantity: 5.014 ml | |



| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|--|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|------------------------------|
| 241 | 20 PPB CCC GRO STD | PP23373 | 05/08/2024 | 08/12/2024 | Yogesh Patel | None | None | Ankita Jodhani 05/13/2024 |
| <u>FROM</u> 5.00000ml of W2606 + 0.00400ml of PP23142 + 0.01000ml of PP23139 = Final Quantity: 5.014 ml | | | | | | | | |

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|--|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|------------------------------|
| 241 | 20 PPB CCC GRO STD | PP23374 | 05/08/2024 | 08/12/2024 | Yogesh Patel | None | None | Ankita Jodhani 05/13/2024 |
| <u>FROM</u> 5.00000ml of W2606 + 0.00400ml of PP23142 + 0.01000ml of PP23139 = Final Quantity: 5.014 ml | | | | | | | | |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-3382-05 / Sand, Purified (cs/4x2.5kg) | 0000243821 | 12/31/2024 | 04/30/2020 / RAJESH | 04/28/2020 / RAJESH | E2865 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-----------------------------|--|--------|-----------------|-------------------------|-----------------------------|----------------|
| PCI Scientific Supply, Inc. | PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1 | 313201 | 07/03/2024 | 01/03/2024 / Rajesh | 07/20/2023 / Rajesh | E3551 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L) | 23K0962009 | 07/16/2024 | 01/16/2024 / Rajesh | 01/11/2024 / Rajesh | E3678 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L) | 24A1562007 | 08/19/2024 | 02/19/2024 / RUPESH | 01/31/2024 / RUPESH | E3706 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 23H1462005 | 10/30/2024 | 04/30/2024 / Rajesh | 04/19/2024 / Rajesh | E3734 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L) | 24C0162011 | 11/01/2024 | 05/01/2024 / Rajesh | 04/26/2024 / Rajesh | E3736 |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-----------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30065 / GRO Mix (EPA) | A0161776 | 09/11/2024 | 03/15/2024 / yogesh | 02/10/2021 / Sohil | P11120 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|---------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 72072 / n-Tetracosane-d50, 1000 ug/ml | 101122 | 08/05/2024 | 02/05/2024 / Ankita | 02/22/2023 / Yogesh | P12303 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|---------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 72072 / n-Tetracosane-d50, 1000 ug/ml | 101122 | 08/05/2024 | 02/05/2024 / Ankita | 02/22/2023 / Yogesh | P12305 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|---------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 72072 / n-Tetracosane-d50, 1000 ug/ml | 101122 | 08/05/2024 | 02/05/2024 / Ankita | 02/22/2023 / Yogesh | P12306 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|---------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 72072 / n-Tetracosane-d50, 1000 ug/ml | 101122 | 08/05/2024 | 02/05/2024 / Sohil | 02/22/2023 / Yogesh | P12307 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31266 / Florida TRPH Standard | A0204859 | 08/21/2024 | 02/21/2024 / yogesh | 01/12/2024 / Yogesh | P13105 |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 31266 / Florida TRPH Standard | A0204859 | 08/21/2024 | 02/21/2024 / yogesh | 01/12/2024 / Yogesh | P13112 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-----------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30065 / GRO Mix (EPA) | A0155991 | 09/11/2024 | 03/15/2024 / yogesh | 09/11/2020 / DHAVAL | P9825 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--|----------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 30068 / VOA Mix, a, a, a-trifluorotoluene 2500uq/ml, P&T methanol, 1ml | A0158026 | 09/15/2024 | 03/15/2024 / yogesh | 09/11/2020 / DHAVAL | V11253 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA9077-02 / Methanol, Purge/Trap (cs=6x1L) | 22L0562016 | 08/12/2024 | 02/12/2024 / SAM | 02/06/2024 / SAM | V14137 |

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---------------------|---------------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | DIW / DI Water | Daily Lab-Certified | 10/24/2024 | 10/24/2019 / apatel | 10/24/2019 / apatel | W2606 |



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 30065 **Lot No.:** A0161776

Description : Gasoline Range Organics Mix (EPA)

Gasoline Range Organics Mix (EPA) 500 - 1500µg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2027 **Storage:** 0°C or colder

CERTIFIED VALUES

| Elution Order | Compound | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2) |
|---------------|--|-----------------------------|--|
| 1 | 2-Methylpentane CAS # 107-83-5 (Lot MKCB1674V) Purity 99% | 1,507.0 µg/mL | +/- 8.9511 µg/mL Gravimetric +/- 84.5158 µg/mL Unstressed +/- 86.4925 µg/mL Stressed |
| 2 | 2,2,4-Trimethylpentane (isooctane) CAS # 540-84-1 (Lot SHBF8066V) Purity 99% | 1,511.0 µg/mL | +/- 8.9749 µg/mL Gravimetric +/- 84.7402 µg/mL Unstressed +/- 86.7221 µg/mL Stressed |
| 3 | n-Heptane (C7) CAS # 142-82-5 (Lot SHBK8626) Purity 98% | 498.8 µg/mL | +/- 2.9628 µg/mL Gravimetric +/- 27.9749 µg/mL Unstressed +/- 28.6292 µg/mL Stressed |
| 4 | Benzene CAS # 71-43-2 (Lot SHBK5679) Purity 99% | 500.0 µg/mL | +/- 2.9698 µg/mL Gravimetric +/- 28.0411 µg/mL Unstressed +/- 28.6969 µg/mL Stressed |
| 5 | Toluene CAS # 108-88-3 (Lot MKCH9232) Purity 99% | 1,510.0 µg/mL | +/- 8.9689 µg/mL Gravimetric +/- 84.6841 µg/mL Unstressed +/- 86.6647 µg/mL Stressed |
| 6 | Ethylbenzene CAS # 100-41-4 (Lot SHBL0706) Purity 99% | 504.0 µg/mL | +/- 2.9936 µg/mL Gravimetric +/- 28.2654 µg/mL Unstressed +/- 28.9265 µg/mL Stressed |
| 7 | m-Xylene CAS # 108-38-3 (Lot SHBL0265) Purity 99% | 1,005.0 µg/mL | +/- 5.9694 µg/mL Gravimetric +/- 56.3626 µg/mL Unstressed +/- 57.6808 µg/mL Stressed |

| | | | | | | | | | | |
|----------|------------------------|---------|-----------------|---------|-------|-----|---------|-------|-------------|------------|
| 8 | o-Xylene | | | 1,007.0 | µg/mL | +/- | 5.9813 | µg/mL | Gravimetric | |
| | CAS # | 95-47-6 | (Lot SHBK7739) | | | +/- | 56.4747 | | µg/mL | Unstressed |
| | Purity | 99% | | | | +/- | 57.7956 | | µg/mL | Stressed |
| | | | | | | | | | | |
| 9 | 1,2,4-Trimethylbenzene | | | 1,008.0 | µg/mL | +/- | 5.9872 | µg/mL | Gravimetric | |
| | CAS # | 95-63-6 | (Lot WXBC4246V) | | | +/- | 56.5308 | | µg/mL | Unstressed |
| | Purity | 99% | | | | +/- | 57.8530 | | µg/mL | Stressed |
| | | | | | | | | | | |
| Solvent: | P&T Methanol | | | | | | | | | |
| | CAS # | 67-56-1 | | | | | | | | |
| | Purity | 99% | | | | | | | | |

Column:
105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)


Carrier Gas:
hydrogen-constant pressure 11.0 psi.

Temp. Program:
40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:
200°C

Det. Temp:
250°C

Det. Type:
FID

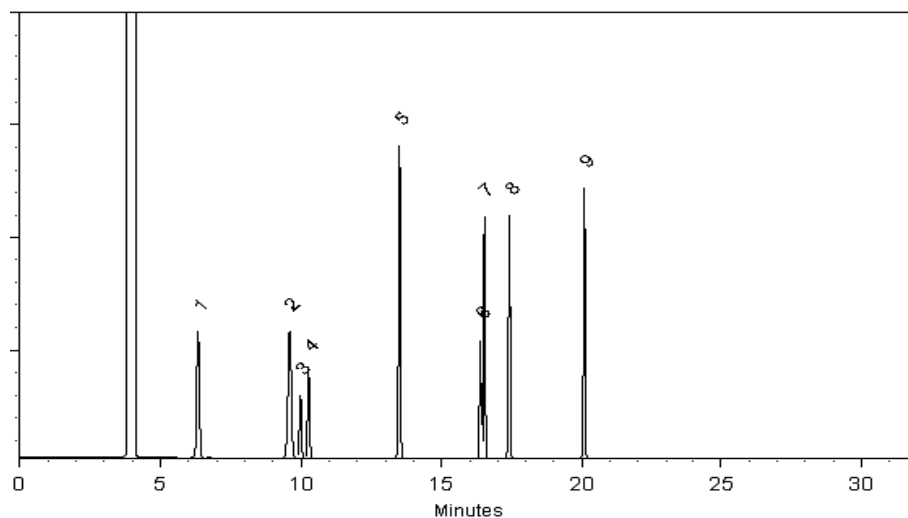

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Cydnei L. Crust
Cydnei L. Crust - Mix Technician

Date Mixed: 15-Jun-2020

Balance: B251644995

Fang-Yun Lo
Fang-Yun Lo - QC Analyst

Date Passed: 17-Jun-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

| Label Conditions | Standard Conditions | Non-Standard Conditions |
|---|---------------------|-------------------------|
| 25°C Nominal (Room Temperature) | < 60°C | ≥ 60°C up to 7 days |
| 10°C or colder (Refrigerate) | < 40°C | ≥ 40°C up to 7 days |
| 0°C or colder (Freezer) -20°C or colder (Deep Freezer) | < 25°C | ≥ 25°C up to 7 days |

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

Sand
Purified
Washed and Ignited



Material No.: 3382-05
Batch No.: 0000243821
Manufactured Date: 2018/04/09
Retest Date: 2025/04/07
Revision No: 1

Certificate of Analysis

| Test | Specification | Result |
|---------------------------|---------------|--------|
| Substances Soluble in HCl | $\leq 0.16\%$ | 0.01 |

For Laboratory, Research or Manufacturing Use
Meets Reagent Specifications for testing USP/NF monographs

Country of Origin: US
Packaging Site: Paris Mfg Ctr & DC

E 2865


Jamie Ethier
Vice President Global Quality

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone: 610.386.1700



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MEXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

| | | | |
|------------------------|-----------------------------------|---------------|---------------------------------|
| PRODUCT : | SODIUM SULFATE CRYSTALS ANHYDROUS | | |
| QUALITY : | ACS (CODE RMB3375) | FORMULA : | Na ₂ SO ₄ |
| SPECIFICATION NUMBER : | 6399 | RELEASE DATE: | ABR/21/2023 |
| LOT NUMBER : | 313201 | | |

| TEST | SPECIFICATIONS | LOT VALUES |
|--|----------------|-------------|
| Assay (Na ₂ SO ₄) | Min. 99.0% | 99.7 % |
| pH of a 5% solution at 25°C | 5.2 - 9.2 | 6.1 |
| Insoluble matter | Max. 0.01% | 0.005 % |
| Loss on ignition | Max. 0.5% | 0.1 % |
| Chloride (Cl) | Max. 0.001% | <0.001 % |
| Nitrogen compounds (as N) | Max. 5 ppm | <5 ppm |
| Phosphate (PO ₄) | Max. 0.001% | <0.001 % |
| Heavy metals (as Pb) | Max. 5 ppm | <5 ppm |
| Iron (Fe) | Max. 0.001% | <0.001 % |
| Calcium (Ca) | Max. 0.01% | 0.002 % |
| Magnesium (Mg) | Max. 0.005% | 0.001 % |
| Potassium (K) | Max. 0.008% | 0.003 % |
| Extraction-concentration suitability | Passes test | Passes test |
| Appearance | Passes test | Passes test |
| Identification | Passes test | Passes test |
| Solubility and foreign matter | Passes test | Passes test |
| Retained on US Standard No. 10 sieve | Max. 1% | 0.1 % |
| Retained on US Standard No. 60 sieve | Min. 94% | 97.3 % |
| Through US Standard No. 60 sieve | Max. 5% | 2.5 % |
| Through US Standard No. 100 sieve | Max. 10% | 0.1 % |

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 23K0962009
Manufactured Date: 2023-10-05
Expiration Date: 2025-01-03
Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|--|----------------|----------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | ≤ 5 | < 1 |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL) | ≤ 10 | 3 |
| Assay (CH ₂ Cl ₂) (by GC, exclusive of preservative, corrected for water) | $\geq 99.8 \%$ | 100.0 % |
| Color (APHA) | ≤ 10 | 10 |
| Residue after Evaporation | ≤ 1.0 ppm | 0.2 ppm |
| Titration Acid (μ eq/g) | ≤ 0.3 | < 0.1 |
| Chloride (Cl) | ≤ 10 ppm | < 5 ppm |
| Water (by KF, coulometric) | $\leq 0.02 \%$ | < 0.01 % |

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC
Manufacturer source batch: MG23J05873

E 3678

Ken Koehnlein
Sr. Manager, Quality Assurance

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 24A1562007
Manufactured Date: 2023-12-14
Expiration Date: 2025-03-14
Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|--|------------------------|----------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | ≤ 5 | < 1 |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL) | ≤ 10 | < 1 |
| Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water) | $\geq 99.8 \%$ | 100.0 % |
| Color (APHA) | ≤ 10 | 5 |
| Residue after Evaporation | $\leq 1.0 \text{ ppm}$ | 0.1 ppm |
| Titration Acid ($\mu\text{eq/g}$) | ≤ 0.3 | < 0.1 |
| Chloride (Cl) | $\leq 10 \text{ ppm}$ | < 5 ppm |
| Water (by KF, coulometric) | $\leq 0.02 \%$ | < 0.01 % |

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC
Manufacturer source batch: MG23L14152

E 3706

REC.
AS 2/19/24

Ken Koehnlein
Sr. Manager, Quality Assurance

Acetone
BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03
Batch No.: 23H1462005
Manufactured Date: 2023-07-26
Expiration Date: 2026-07-25
Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|---|---------------|-------------|
| Assay ((CH ₃) ₂ CO) (by GC, corrected for water) | ≥ 99.4 % | 99.7 % |
| Color (APHA) | ≤ 10 | 5 |
| Residue after Evaporation | ≤ 1.0 ppm | 0.3 ppm |
| Substances Reducing Permanganate | Passes Test | Passes Test |
| Titration Acid (μeq/g) | ≤ 0.3 | 0.1 |
| Titration Base (μeq/g) | ≤ 0.6 | < 0.1 |
| Water (H ₂ O) | ≤ 0.5 % | 0.3 % |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | ≤ 5 | < 1 |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL) | ≤ 10 | 1 |

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 4/19/24

E 3734

Ken Koehnlein
Sr. Manager, Quality Assurance

Methylene Chloride
ULTRA RESI-ANALYZED
For Organic Residue Analysis
(dichloromethane)



Material No.: 9266-A4
Batch No.: 24C0162011
Manufactured Date: 2024-01-04
Expiration Date: 2025-04-04
Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|--|----------------|----------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | ≤ 5 | < 1 |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL) | ≤ 10 | 2 |
| Assay (CH_2Cl_2) (by GC, exclusive of preservative, corrected for water) | $\geq 99.8\%$ | 100.0 % |
| Color (APHA) | ≤ 10 | 10 |
| Residue after Evaporation | ≤ 1.0 ppm | 0.2 ppm |
| Titration Acid ($\mu\text{eq/g}$) | ≤ 0.3 | < 0.1 |
| Chloride (Cl) | ≤ 10 ppm | < 5 ppm |
| Water (by KF, coulometric) | $\leq 0.02\%$ | < 0.01 % |

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC
Manufacturer source batch: MG24A04224

E 3736

Ken Koehnlein
Sr. Manager, Quality Assurance

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC
100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700
Page 1 of 1

Methanol
ULTRA RESI-ANALYZED
For Purge and Trap Analysis



Material No.: 9077-02
Batch No.: 22L0562016
Manufactured Date: 2022-10-26
Expiration Date: 2025-10-25
Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|---|---------------|----------|
| Assay (CH ₃ OH) (by GC, corrected for water) | ≥ 99.9 % | 100.0 % |
| Residue after Evaporation | ≤ 1.0 ppm | 0.2 ppm |
| Titration Acid (μeq/g) | ≤ 0.3 | 0.2 |
| Titration Base (μeq/g) | ≤ 0.10 | 0.03 |
| Water (by KF, coulometric) | ≤ 0.08 % | < 0.01 % |
| Volatile Organic Trace Analysis - Below EPA 8260B CRQL | Conforms | Conforms |

For Laboratory, Research, or Manufacturing Use
Performance Tested for Use in EPA Methods
500 Series for Drinking Water
600 Series for Wastewater
846 for Solid Waste

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Ethier
Vice President Global Quality



CERTIFIED WEIGHT REPORT

Part Number: **72072**
Lot Number: **101122**
Description: **n-Tetracosane-d50**

Solvent(s):
Methylene chloride
Lot#: 105345



| | | |
|-------------------------|------------------|--------|
| <i>Prashant Chauhan</i> | | 101122 |
| Formulated By: | Prashant Chauhan | DATE |
| <i>Pedro L. Rentas</i> | | 101122 |
| Reviewed By: | Pedro L. Rentas | DATE |

Expiration Date: 101132
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 6UTB
Weight(s) shown below were combined and diluted to (mL): 200.0

P12291
2
P12310
Y.P.
02/22/23

| Compound | RM# | Lot Number | Nominal Conc (µg/mL) | Purity (%) | Uncertainty Purity | Assay (%) | Target Weight(g) | Actual Weight(g) | Actual Conc (µg/mL) | Expanded Uncertainty (+/-) (µg/mL) | SDS Information (Solvent Safety Info. On Attached pg.) | | |
|----------------------|------|------------|----------------------|------------|--------------------|-----------|------------------|------------------|---------------------|------------------------------------|--|----------------|------|
| | | | | | | | | | | | CAS# | OSHA PEL (TWA) | LD50 |
| 1. n-Tetracosane-d50 | 2072 | PR-26606 | 1000 | 98.7 | 0.2 | 99.0 | 0.20471 | 0.20482 | 1000.6 | 4.1 | 16416-32-3 | N/A | N/A |

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

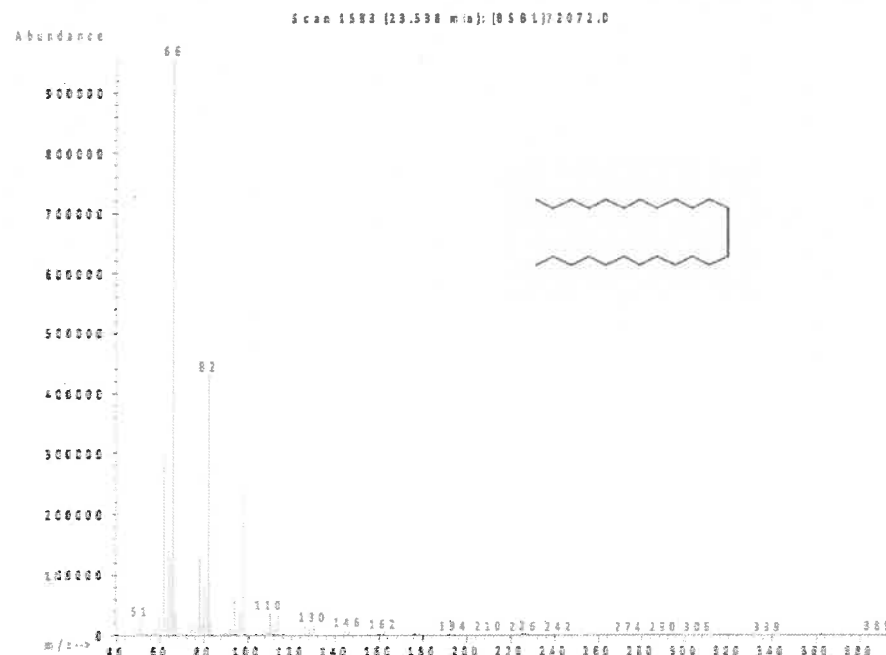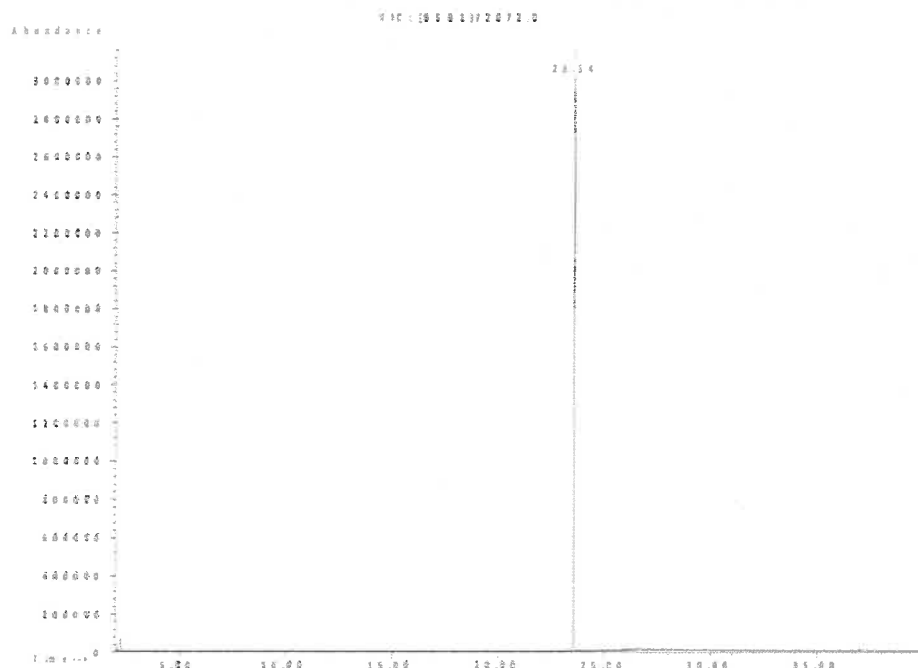

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHYLENE CHLORIDE

| | | | |
|---------------------|------------------------------------|--|-----------------------------------|
| Manufacturer's Name | ABSOLUTE STANDARDS INC | Emergency Telephone USA & CANADA | 1-800-535-5053 |
| Address | 44 Rosotto Dr. Hamden CT, 06514 | Emergency Telephone International Date Prepared/Revised | 1-352-323-3500 January 1, 2022 |

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

| | | | |
|----------|--------------------------------------|--------------|---|
| H302 | Harmful if swallowed. | H315,H320 | Causes skin and eye irritation. |
| H351 | Suspected of causing cancer. | H335 | May cause respiratory irritation. |
| P271 | Use in ventilated area | P280 | Use gloves, eye protection/face shield |
| P302,332 | If on skin, wash with soap and water | P305,351,338 | If in eyes, remove contacts, rinse with water |



Signal Word: WARNING



Section III - Composition

| | | | | |
|-----------------|---------|----------------|---------------|--------------|
| Components: | CAS#: | OSHA PEL (TWA) | LD50 orl-rat | % (optional) |
| Dichloromethane | 75-09-2 | 50 ppm | > 2,000 mg/kg | > 97 |

See Certified Weight Report For Other Analytes Present At Trace Quantities.
INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

| | |
|-------------------------|---|
| General advice | Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area. |
| If inhaled | If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician. |
| In case of skin contact | Wash with soap and water. Consult a physician. |
| In case of eye contact | Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician. |
| If swallowed | Do NOT induce vomiting. Rinse mouth with water. Consult a physician. |

Section V. FIREFIGHTING MEASURES

| | |
|-------------------------------|--|
| Suitable extinguishing media | Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide. |
| Protective equipment for fire | Wear self contained breathing apparatus for fire fighting if necessary. |

Section VI. ACCIDENTAL RELEASE MEASURES

| | |
|---------------------------|---|
| Personal precautions | Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations. |
| Environmental precautions | Prevent further leakage or spillage if safe to do so. Do not let product enter drains. |
| Clean up | Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13). |

Section VII. HANDLING AND STORAGE

| | |
|-------------------------------|--|
| Precautions for safe handling | Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. |
| Storage Conditions | Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge. Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage. |

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

| | |
|--|--|
| Methylene chloride 75-09-2 TWA 50 ppm | |
| Potential for skin absorption, ingestion and inhalation. | |
| Personal protective equipment | Respiratory protection |
| Personal contact with skin, eyes and clothing. | Wash hands thoroughly after handling the product |
| | Handle with gloves. Gloves must be inspected prior to use. |
| | Eye protection. |

Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS

| | | | |
|---------------|------|----------------------------|-------|
| Boiling Point | 40°C | Specific Gravity (H2O = 1) | 1.325 |
|---------------|------|----------------------------|-------|

| | | | |
|-------------------------|------------------|---|-------|
| Vapor Pressure (mm Hg) | 353 | Melting Point | -97°C |
| Vapor Density (AIR = 1) | 2.93 | Evaporation rate (Butyl Acetate = 1) | 0.71 |
| Solubility in Water | Slightly soluble | | |

Appearance and Odor CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.

Section X. STABILITY AND REACTIVITY

| | |
|------------------------------------|---|
| Chemical stability | Stable under recommended storage conditions. |
| Possibility of hazardous reactions | No data available |
| Conditions to avoid | Heat, flames, sparks, extreme temperature and sunlight. |
| Materials to avoid | Alkali metals, Aluminum, Oxidizing agents, Bases, Amines, Magnesium, Acids, Vinyl compounds |
| Hazardous decomposition products | - No data available |

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - Rat - > 2,000 mg/kg
LC50 Inhalation - Rat - 52,000 mg/m3
LD50 Dermal - Rat - > 2,000 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 1000 lbs.

LC50 193.00 mg/l - 96 h
EC50 1,682.00 mg/l - 48 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US) IATA
UN number: 1593 Class: 6.1 Packing group: III UN number: 1593 Class: 6.1 Packing group: III
Proper shipping name: Dichloromethane Proper shipping name: Dichloromethane
Reportable Quantity (RQ): 1000 lbs

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC. DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.

ABSOLUTE STANDARDS, INC.

ISO - 17034



Certificate of Analysis



Certified Reference Material (CRM)

Conformance: The "Certificate of Analysis" is applicable for CRM's, fulfilling the requirements in the current version of: ISO 17034.

Health & Safety: See the attached SDS & Certified Weight Report before use.

Intended Use: This Certified Reference Material (CRM) is intended primarily for use in the characterization of unknowns and the establishment of analyzer or instrument response factors by qualified personnel. Typical instrumental organic assays include: GC & LC, and inorganic assays include: ICP & AA. This product is for laboratory use only.

Characterization Values: In production, gravimetric/volumetric readings are certified to be within $\pm 0.5\%$ of the stated value & are valid between 18 °C & 30 °C. The measured characterization of uncertainty can be found on the Certified Weight Report. All product weighings are performed on an analytical balance that is calibrated to NIST Traceable standard weights & certified by the manufacturer. The volumetric glassware used is Class "A" type & conforms to ASTM E-288 unless otherwise stated. The solvents & compounds used are of the highest practical purity & typically meet or exceed ACS Reagent Grade & ACS Standards Grade specifications. The expanded uncertainty field on Certified Wt. Report represents CRM uncertainty as described in ISO 17034.

Homogeneity: Uncertainties that are due to the analytical procedure(s) are within $\pm 0.5\%$ unless specifically stated on the Certified Wt. Report.

Verification: Uncertainties that are due to the analytical procedure(s) are within $\pm 0.5\%$ unless specifically stated on the Certified Wt. Report.

Stability: Uncertainties for short-term stability are determined in accordance with ISO 17034. Long-term stability is determined in accordance with ISO 17034. The shelf life is limited by the stated expiration for each product. Expiration dates and additional technical information can be found on the Certified Weight Report and on the product label.

Uncertainty: UCRM is the expanded uncertainty which utilizes a $K = 2$ (coverage factor of 2), in accordance with ISO 17034 as listed above (Characterization, Homogeneity, Verification, and Stability).

Purity & Identity: Organic solutions are typically formulated from neat materials whose purity & identity have been characterized by GC-MSD & LC-PDA techniques with comparison to a NIST Traceable library of mass spectra when available. Additional characterization techniques may include but are not limited to: refractive index measurements of liquids, melting point measurements of solids, & GC-FID, ECD, PID, ELCD, LC-PDA measurements for purity. Inorganic solutions & neat are typically formulated from materials whose purity & identity have been characterized by ICPMS with comparison to a NIST SRM® when available. Additional characterization techniques may include but are not limited to: titrimetry, and densitometry.

Storage: Sealed ampules and other containers should be stored in the dark and at temperatures indicated on the Certified Weight Report or product label. Certification by Absolute Standards, Inc. is typically valid for 3 years from the date of manufacture. Each product will show its own expiration date as the limit of certification. Certified values are not applicable to opened ampules or for any materials stored in re-sealable containers. Please see the "Certified Weight Report" for specific values and any exceptions.

Usage: Ampules & bottles should be brought to room temperature (18 to 30 °C) before opening. Sonication may be required for high concentration solutions or solutions that may precipitate during storage. After opening, care should be exercised to avoid concentration changes owing to evaporation of the solvent or essential components. We recommend that a suitable re-sealable container be available before opening an ampule to decant the standard for short-term storage and use.

Minimum Sample Size: 0.5 uL for analytical applications.

Legal Notice: Warranty of products are as described when shipped. No warranty as to fitness for any particular application is expressed or implied. Errant shipments and/or quality claims must be made within 10 days of receipt. Liability is limited solely to the replacement of the product or refund of purchase price.

Certifying Officer: Stephen J. Arpie, M.S., Director General



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514

Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: StephenArpie@AbsoluteStandards.com

Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019

Page 1 of 2





CERTIFIED WEIGHT REPORT

Part Number: **72072**
Lot Number: **101122**
Description: **n-Tetracosane-d50**

Solvent(s):
Methylene chloride
Lot#: 105345

| | | |
|-------------------------|------------------|--------|
| <i>Prashant Chauhan</i> | | 101122 |
| Formulated By: | Prashant Chauhan | DATE |
| <i>Pedro L. Rentas</i> | | 101122 |
| Reviewed By: | Pedro L. Rentas | DATE |

Expiration Date: 101132
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 6UTB



Weight(s) shown below were combined and diluted to (mL): 200.0

5E-05 Balance Uncertainty
0.058 Flask Uncertainty

P12291
2
P12310
Y.P.
02/22/23

| Compound | RM# | Lot Number | Nominal Conc (µg/mL) | Purity (%) | Uncertainty Purity | Assay (%) | Target Weight(g) | Actual Weight(g) | Actual Conc (µg/mL) | Expanded Uncertainty (+/-) (µg/mL) | SDS Information (Solvent Safety Info. On Attached pg.) | | |
|----------------------|------|------------|----------------------|------------|--------------------|-----------|------------------|------------------|---------------------|------------------------------------|--|----------------|------|
| | | | | | | | | | | | CAS# | OSHA PEL (TWA) | LD50 |
| 1. n-Tetracosane-d50 | 2072 | PR-26606 | 1000 | 98.7 | 0.2 | 99.0 | 0.20471 | 0.20482 | 1000.6 | 4.1 | 16416-32-3 | N/A | N/A |

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

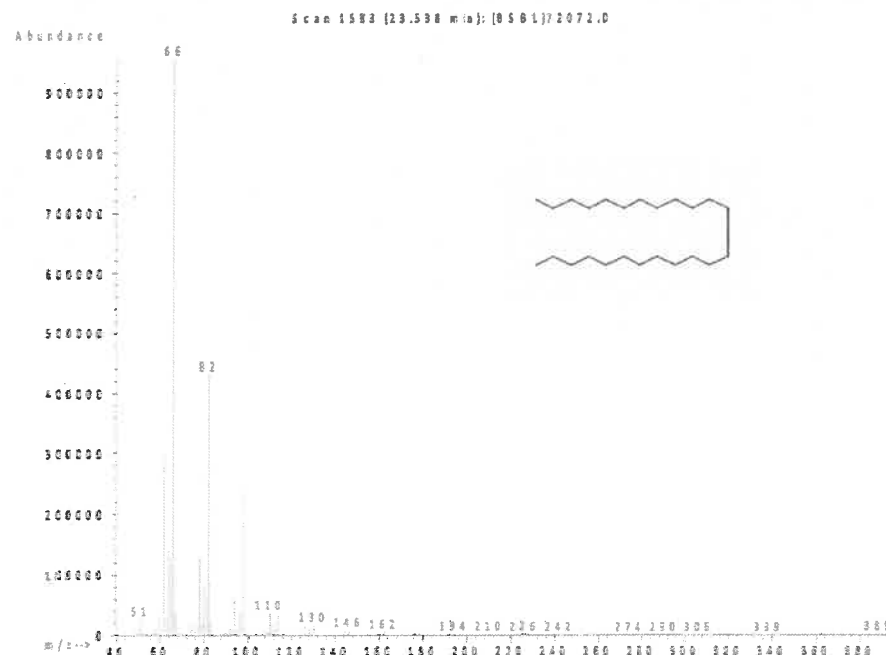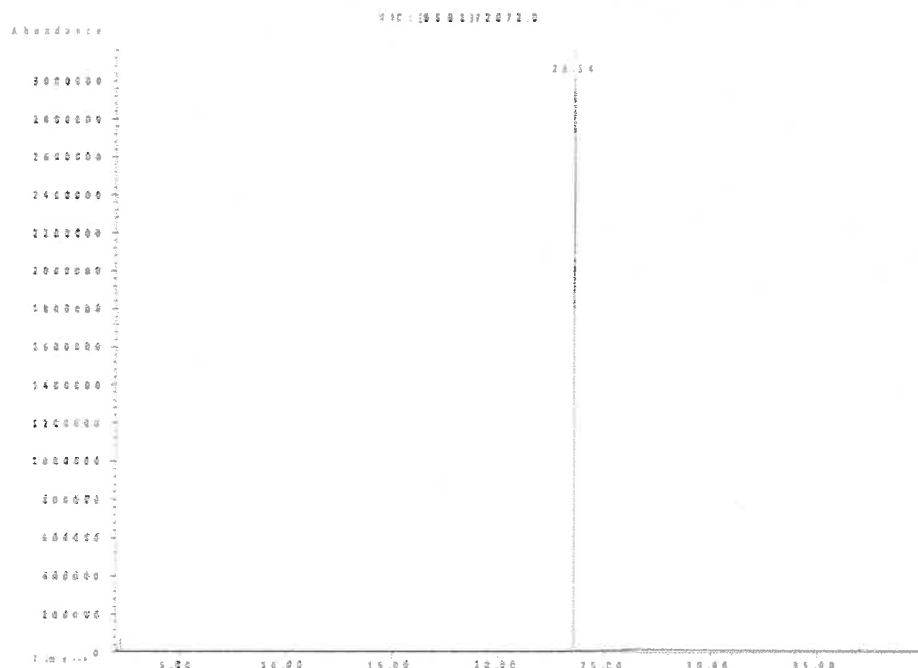

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHYLENE CHLORIDE

| | | | |
|---------------------|------------------------------------|--|-----------------------------------|
| Manufacturer's Name | ABSOLUTE STANDARDS INC | Emergency Telephone USA & CANADA | 1-800-535-5053 |
| Address | 44 Rosotto Dr. Hamden CT, 06514 | Emergency Telephone International Date Prepared/Revised | 1-352-323-3500 January 1, 2022 |

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

| | | | |
|----------|--------------------------------------|--------------|---|
| H302 | Harmful if swallowed. | H315,H320 | Causes skin and eye irritation. |
| H351 | Suspected of causing cancer. | H335 | May cause respiratory irritation. |
| P271 | Use in ventilated area | P280 | Use gloves, eye protection/face shield |
| P302,332 | If on skin, wash with soap and water | P305,351,338 | If in eyes, remove contacts, rinse with water |



Signal Word: WARNING

Section III - Composition

| | | | | |
|-----------------|---------|----------------|---------------|--------------|
| Components: | CAS#: | OSHA PEL (TWA) | LD50 orl-rat | % (optional) |
| Dichloromethane | 75-09-2 | 50 ppm | > 2,000 mg/kg | > 97 |

See Certified Weight Report For Other Analytes Present At Trace Quantities.
INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice
Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.

If inhaled
If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.

In case of skin contact
Wash with soap and water. Consult a physician.

In case of eye contact
Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.

If swallowed
Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Suitable extinguishing media
Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.

Protective equipment for fire
Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions
Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.

Environmental precautions
Prevent further leakage or spillage if safe to do so. Do not let product enter drains.

Clean up
Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling
Avoid contact with skin and eyes. Avoid inhalation of vapour or mist.

Storage Conditions
Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge. Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methylene chloride 75-09-2 TWA 50 ppm

Potential for skin absorption, ingestion and inhalation.

Personal protective equipment
Respiratory protection
Handle with gloves. Gloves must be inspected prior to use. Eye protection.

Personal contact with skin, eyes and clothing.
Wash hands thoroughly after handling the product.

Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS

| | | | |
|---------------|------|----------------------------|-------|
| Boiling Point | 40°C | Specific Gravity (H2O = 1) | 1.325 |
|---------------|------|----------------------------|-------|

| | | | |
|-------------------------|------------------|---|-------|
| Vapor Pressure (mm Hg) | 353 | Melting Point | -97°C |
| Vapor Density (AIR = 1) | 2.93 | Evaporation rate (Butyl Acetate = 1) | 0.71 |
| Solubility in Water | Slightly soluble | | |

Appearance and Odor CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.

Section X. STABILITY AND REACTIVITY

| | |
|------------------------------------|---|
| Chemical stability | Stable under recommended storage conditions. |
| Possibility of hazardous reactions | No data available |
| Conditions to avoid | Heat, flames, sparks, extreme temperature and sunlight. |
| Materials to avoid | Alkali metals, Aluminum, Oxidizing agents, Bases, Amines, Magnesium, Acids, Vinyl compounds |
| Hazardous decomposition products | - No data available |

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - Rat - > 2,000 mg/kg
LC50 Inhalation - Rat - 52,000 mg/m3
LD50 Dermal - Rat - > 2,000 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 1000 lbs.

LC50 193.00 mg/l - 96 h
EC50 1,682.00 mg/l - 48 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US) IATA
UN number: 1593 Class: 6.1 Packing group: III UN number: 1593 Class: 6.1 Packing group: III
Proper shipping name: Dichloromethane Proper shipping name: Dichloromethane
Reportable Quantity (RQ): 1000 lbs

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC. DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.

ABSOLUTE STANDARDS, INC.

ISO - 17034



Certificate of Analysis



Certified Reference Material (CRM)

Conformance: The "Certificate of Analysis" is applicable for CRM's, fulfilling the requirements in the current version of: ISO 17034.

Health & Safety: See the attached SDS & Certified Weight Report before use.

Intended Use: This Certified Reference Material (CRM) is intended primarily for use in the characterization of unknowns and the establishment of analyzer or instrument response factors by qualified personnel. Typical instrumental organic assays include: GC & LC, and inorganic assays include: ICP & AA. This product is for laboratory use only.

Characterization Values: In production, gravimetric/volumetric readings are certified to be within $\pm 0.5\%$ of the stated value & are valid between 18 °C & 30 °C. The measured characterization of uncertainty can be found on the Certified Weight Report. All product weighings are performed on an analytical balance that is calibrated to NIST Traceable standard weights & certified by the manufacturer. The volumetric glassware used is Class "A" type & conforms to ASTM E-288 unless otherwise stated. The solvents & compounds used are of the highest practical purity & typically meet or exceed ACS Reagent Grade & ACS Standards Grade specifications. The expanded uncertainty field on Certified Wt. Report represents CRM uncertainty as described in ISO 17034.

Homogeneity: Uncertainties that are due to the analytical procedure(s) are within $\pm 0.5\%$ unless specifically stated on the Certified Wt. Report.

Verification: Uncertainties that are due to the analytical procedure(s) are within $\pm 0.5\%$ unless specifically stated on the Certified Wt. Report.

Stability: Uncertainties for short-term stability are determined in accordance with ISO 17034. Long-term stability is determined in accordance with ISO 17034. The shelf life is limited by the stated expiration for each product. Expiration dates and additional technical information can be found on the Certified Weight Report and on the product label.

Uncertainty: UCRM is the expanded uncertainty which utilizes a $K = 2$ (coverage factor of 2), in accordance with ISO 17034 as listed above (Characterization, Homogeneity, Verification, and Stability).

Purity & Identity: Organic solutions are typically formulated from neat materials whose purity & identity have been characterized by GC-MSD & LC-PDA techniques with comparison to a NIST Traceable library of mass spectra when available. Additional characterization techniques may include but are not limited to: refractive index measurements of liquids, melting point measurements of solids, & GC-FID, ECD, PID, ELCD, LC-PDA measurements for purity. Inorganic solutions & neat are typically formulated from materials whose purity & identity have been characterized by ICPMS with comparison to a NIST SRM® when available. Additional characterization techniques may include but are not limited to: titrimetry, and densitometry.

Storage: Sealed ampules and other containers should be stored in the dark and at temperatures indicated on the Certified Weight Report or product label. Certification by Absolute Standards, Inc. is typically valid for 3 years from the date of manufacture. Each product will show its own expiration date as the limit of certification. Certified values are not applicable to opened ampules or for any materials stored in re-sealable containers. Please see the "Certified Weight Report" for specific values and any exceptions.

Usage: Ampules & bottles should be brought to room temperature (18 to 30 °C) before opening. Sonication may be required for high concentration solutions or solutions that may precipitate during storage. After opening, care should be exercised to avoid concentration changes owing to evaporation of the solvent or essential components. We recommend that a suitable re-sealable container be available before opening an ampule to decant the standard for short-term storage and use.

Minimum Sample Size: 0.5 uL for analytical applications.

Legal Notice: Warranty of products are as described when shipped. No warranty as to fitness for any particular application is expressed or implied. Errant shipments and/or quality claims must be made within 10 days of receipt. Liability is limited solely to the replacement of the product or refund of purchase price.

Certifying Officer: Stephen J. Arpie, M.S., Director General

Page 1 of 2



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514
Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: Stephen.Arpie@AbsoluteStandards.com
Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019



ABSOLUTE STANDARDS, INC.

ISO - 17034



Understanding the Certified Weight Report



Each Certified Reference Material (CRM) is supported by a Certified Weight Report. Assigned values for concentrations and associated uncertainties are based upon NIST traceable masses & volumes used in production.

Absolute Standards, Inc.
800-368-1131
www.absolutestandards.com



Certified Reference Material CRM



ISO 17034 Accredited
Scope: <http://AbsoluteStandards.com>

Part #
Lot #
Shelf Life

CERTIFIED WEIGHT REPORT


| Part Number: | 10000R | Solvent(s): | Methylene chloride | Lot# | 78782 |
|--|---|-------------|--------------------|---------|---------|
| Lot Number: | 070716 | | | | |
| Description: | CLP Priority Pollutant Internal Standards GC/MS Calibration - 8 components | | | | |
| Expiration Date: | 070721 | | | | |
| Recommended Storage Conditions: | Room Temp (20 °C) | | | | |
| Net Weight (g): | 4000 | | | | |
| NIST Test ID#: | 822-578572-11 | | | | |
| Weights shown below were combined and diluted to (mL): | | | | | |
| | Normal | Purity | Uncertainty | Actual | Target |
| Conc'd | Conc'd | Conc'd | Conc'd | Conc'd | Conc'd |
| 1,4-Dichlorobenzene-d4 | 118 | 99.9 | 0.2 | 2.04083 | 2.04083 |
| 2-Naphthalene-d8 | 223 | 99.9 | 0.2 | 2.02032 | 2.02032 |
| 3-Acetylphenanthrene-d10 | 4000 | 99.9 | 0.2 | 2.02032 | 2.02032 |
| 4-Phenanthrene-d10 | 249 | 99.9 | 0.2 | 2.04083 | 2.04083 |
| Chrysene-d12 | 92 | 99.9 | 0.2 | 2.04083 | 2.04083 |
| Pyrene-d12 | 247 | 99.9 | 0.2 | 2.04083 | 2.04083 |

Target
Compounds

Method of
Analysis

Run 35, *P10000R L070716 (4000g/mL in MeCl2)
Column: 100% DB-5, 0.25mm ID, 30m
Carrier Gas: Helium (molar ratio) = 25 mL
Injection Volume: 1 µL
Injection Temperature: 250°C
Oven Temperature: 50°C (1 min) to 300°C (10 min) to 320°C (1 min)
Total Run Time = 40 minutes. Injection = 0.5 µL, Range = 4

GC/MS Analysis by Mottet-Snyder
Column: 100% DB-5, 0.25mm ID, 30m
Carrier Gas: Helium (molar ratio) = 25 mL
Injection Volume: 1 µL
Injection Temperature: 250°C
Oven Temperature: 50°C (1 min) to 300°C (10 min) to 320°C (1 min)
Total Run Time = 40 minutes. Injection = 0.5 µL, Range = 4

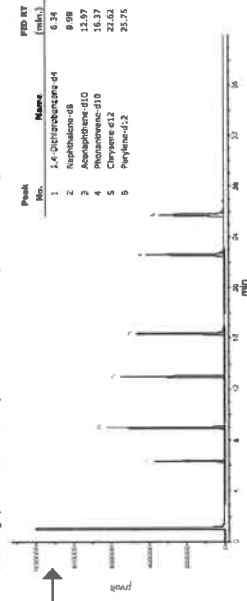

Qualitative
Quantitative

Formulator
Reviewer

Formulated By: *Pedro L. Rios*
Reviewed By: *Pedro L. Rios*
DATE: 070716
DATE: 070716

Actual
Concentration
Uncertainty
Values
Health &
Safety

| Conc'd | Actual | Uncertainty | Expanded | MSDS Information | (Solvent Safety Info. On Attached pg.) | LOD |
|--------------------------|--------|-------------|------------|------------------|--|------|
| 1,4-Dichlorobenzene-d4 | 4004.7 | 16.4 | 3895-42-1 | N/A | 10 ppm (100mg/L) | 1000 |
| 2-Naphthalene-d8 | 4001.9 | 16.2 | 1144-85-2 | 10 ppm (100mg/L) | 1000 | 1000 |
| 3-Acetylphenanthrene-d10 | 4004.2 | 16.2 | 16087-26-2 | N/A | 1000 | 1000 |
| 4-Phenanthrene-d10 | 4000.8 | 16.4 | 1517-82-2 | N/A | 1000 | 1000 |
| Chrysene-d12 | 4001.3 | 16.4 | 1714-83-6 | N/A | 1000 | 1000 |
| Pyrene-d12 | 4001.7 | 16.4 | 180-46-3 | N/A | 1000 | 1000 |

Absolute Standards, Inc. certifies that the above listed and independently analyzed (via analytical data for these products) are supported by a Certified Weight Report. They are supported for sale as these products are supported by a Certified Weight Report. They are supported for sale as these products are supported by a Certified Weight Report. They are supported for sale as these products are supported by a Certified Weight Report.

Absolute Standards, Inc.
Superior, IN

P10000R L070716
P10000R L070716

3rd Party
Comparison

| Analysis | Sup/Ass | Dev (%) |
|--------------------------|---------|---------|
| 1,4-Dichlorobenzene-d4 | 2.55 | 2.43 |
| 2-Naphthalene-d8 | 2.74 | 2.74 |
| 3-Acetylphenanthrene-d10 | 0.03 | 0.03 |
| 4-Phenanthrene-d10 | 1.92 | 1.92 |
| Chrysene-d12 | -1.72 | -1.72 |
| Pyrene-d12 | -0.56 | -0.56 |

Part # 10000R Lot # 041219

1 of 2

Printed: 5/8/2019, 12:55:50 PM

For More Information, Contact:

StephenArpie@AbsoluteStandards.com

Page 2 of 2



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514

Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: StephenArpie@AbsoluteStandards.com
Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019





CERTIFIED WEIGHT REPORT

Part Number: **72072**
Lot Number: **101122**
Description: **n-Tetracosane-d50**

Solvent(s):
Methylene chloride
Lot#: 105345

| | | |
|-------------------------|------------------|--------|
| <i>Prashant Chauhan</i> | | 101122 |
| Formulated By: | Prashant Chauhan | DATE |
| <i>Pedro L. Rentas</i> | | 101122 |
| Reviewed By: | Pedro L. Rentas | DATE |

Expiration Date: 101132
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 6UTB



Weight(s) shown below were combined and diluted to (mL): 200.0

5E-05 Balance Uncertainty
0.058 Flask Uncertainty

P12291
↓
P12310 } *Y.P.*
02/22/23

| Compound | RM# | Lot Number | Nominal Conc (µg/mL) | Purity (%) | Uncertainty Purity | Assay (%) | Target Weight(g) | Actual Weight(g) | Actual Conc (µg/mL) | Expanded Uncertainty (+/-) (µg/mL) | SDS Information (Solvent Safety Info. On Attached pg.) | | |
|----------------------|------|------------|----------------------|------------|--------------------|-----------|------------------|------------------|---------------------|------------------------------------|--|----------------|------|
| | | | | | | | | | | | CAS# | OSHA PEL (TWA) | LD50 |
| 1. n-Tetracosane-d50 | 2072 | PR-26606 | 1000 | 98.7 | 0.2 | 99.0 | 0.20471 | 0.20482 | 1000.6 | 4.1 | 16416-32-3 | N/A | N/A |

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

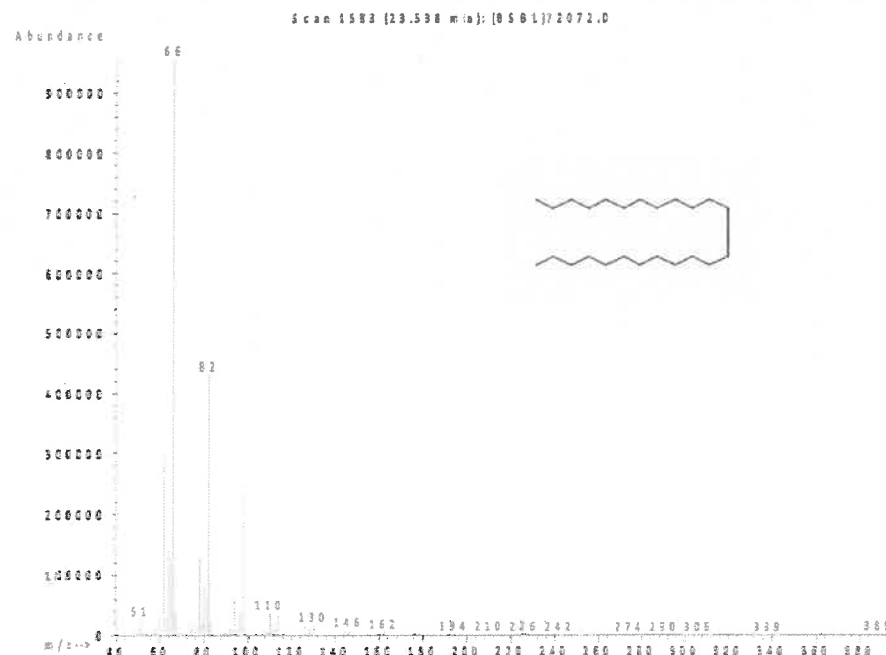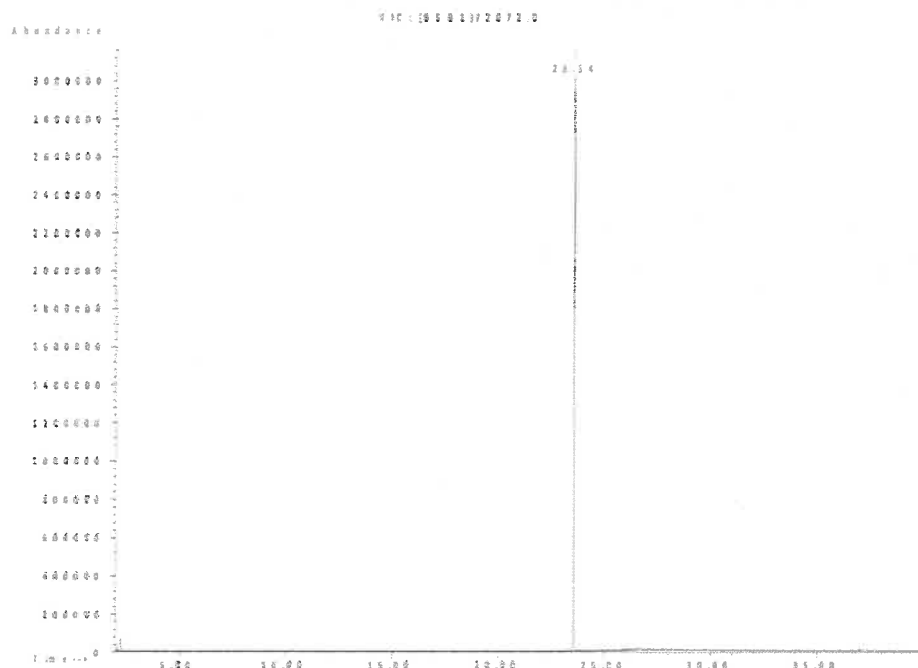

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHYLENE CHLORIDE

| | | | |
|---------------------|------------------------------------|--|-----------------------------------|
| Manufacturer's Name | ABSOLUTE STANDARDS INC | Emergency Telephone USA & CANADA | 1-800-535-5053 |
| Address | 44 Rosotto Dr. Hamden CT, 06514 | Emergency Telephone International Date Prepared/Revised | 1-352-323-3500 January 1, 2022 |

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

| | | | |
|----------|--------------------------------------|--------------|---|
| H302 | Harmful if swallowed. | H315,H320 | Causes skin and eye irritation. |
| H351 | Suspected of causing cancer. | H335 | May cause respiratory irritation. |
| P271 | Use in ventilated area | P280 | Use gloves, eye protection/face shield |
| P302,332 | If on skin, wash with soap and water | P305,351,338 | If in eyes, remove contacts, rinse with water |



Signal Word: WARNING

Section III - Composition

| | | | | |
|-----------------|---------|----------------|---------------|--------------|
| Components: | CAS#: | OSHA PEL (TWA) | LD50 orl-rat | % (optional) |
| Dichloromethane | 75-09-2 | 50 ppm | > 2,000 mg/kg | > 97 |

See Certified Weight Report For Other Analytes Present At Trace Quantities.
INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

General advice
If inhaled Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.
If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.
In case of skin contact
Wash with soap and water. Consult a physician.
In case of eye contact
Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.
If swallowed
Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

Section V. FIREFIGHTING MEASURES

Suitable extinguishing media
Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.
Protective equipment for fire
Wear self contained breathing apparatus for fire fighting if necessary.

Section VI. ACCIDENTAL RELEASE MEASURES

Personal precautions
Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.
Environmental precautions
Prevent further leakage or spillage if safe to do so. Do not let product enter drains.
Clean up
Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

Section VII. HANDLING AND STORAGE

Precautions for safe handling
Avoid contact with skin and eyes. Avoid inhalation of vapour or mist.
Storage Conditions
Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge.
Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methylene chloride 75-09-2 TWA 50 ppm
Potential for skin absorption, ingestion and inhalation.
Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection.
Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS

| | | | |
|---------------|------|----------------------------|-------|
| Boiling Point | 40°C | Specific Gravity (H2O = 1) | 1.325 |
|---------------|------|----------------------------|-------|

| | | | |
|-------------------------|------------------|---|-------|
| Vapor Pressure (mm Hg) | 353 | Melting Point | -97°C |
| Vapor Density (AIR = 1) | 2.93 | Evaporation rate (Butyl Acetate = 1) | 0.71 |
| Solubility in Water | Slightly soluble | | |

Appearance and Odor CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.

Section X. STABILITY AND REACTIVITY

| | |
|------------------------------------|---|
| Chemical stability | Stable under recommended storage conditions. |
| Possibility of hazardous reactions | No data available |
| Conditions to avoid | Heat, flames, sparks, extreme temperature and sunlight. |
| Materials to avoid | Alkali metals, Aluminum, Oxidizing agents, Bases, Amines, Magnesium, Acids, Vinyl compounds |
| Hazardous decomposition products | - No data available |

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - Rat - > 2,000 mg/kg
LC50 Inhalation - Rat - 52,000 mg/m3
LD50 Dermal - Rat - > 2,000 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 1000 lbs.

LC50 193.00 mg/l - 96 h
EC50 1,682.00 mg/l - 48 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US) IATA
UN number: 1593 Class: 6.1 Packing group: III UN number: 1593 Class: 6.1 Packing group: III
Proper shipping name: Dichloromethane Proper shipping name: Dichloromethane
Reportable Quantity (RQ): 1000 lbs

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC. DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.

ABSOLUTE STANDARDS, INC.

ISO - 17034



Certificate of Analysis



Certified Reference Material (CRM)

Conformance: The "Certificate of Analysis" is applicable for CRM's, fulfilling the requirements in the current version of: ISO 17034.

Health & Safety: See the attached SDS & Certified Weight Report before use.

Intended Use: This Certified Reference Material (CRM) is intended primarily for use in the characterization of unknowns and the establishment of analyzer or instrument response factors by qualified personnel. Typical instrumental organic assays include: GC & LC, and inorganic assays include: ICP & AA. This product is for laboratory use only.

Characterization Values: In production, gravimetric/volumetric readings are certified to be within $\pm 0.5\%$ of the stated value & are valid between 18 °C & 30 °C. The measured characterization of uncertainty can be found on the Certified Weight Report. All product weighings are performed on an analytical balance that is calibrated to NIST Traceable standard weights & certified by the manufacturer. The volumetric glassware used is Class "A" type & conforms to ASTM E-288 unless otherwise stated. The solvents & compounds used are of the highest practical purity & typically meet or exceed ACS Reagent Grade & ACS Standards Grade specifications. The expanded uncertainty field on Certified Wt. Report represents CRM uncertainty as described in ISO 17034.

Homogeneity: Uncertainties that are due to the analytical procedure(s) are within $\pm 0.5\%$ unless specifically stated on the Certified Wt. Report.

Verification: Uncertainties that are due to the analytical procedure(s) are within $\pm 0.5\%$ unless specifically stated on the Certified Wt. Report.

Stability: Uncertainties for short-term stability are determined in accordance with ISO 17034. Long-term stability is determined in accordance with ISO 17034. The shelf life is limited by the stated expiration for each product. Expiration dates and additional technical information can be found on the Certified Weight Report and on the product label.

Uncertainty: UCRM is the expanded uncertainty which utilizes a $K = 2$ (coverage factor of 2), in accordance with ISO 17034 as listed above (Characterization, Homogeneity, Verification, and Stability).

Purity & Identity: Organic solutions are typically formulated from neat materials whose purity & identity have been characterized by GC-MSD & LC-PDA techniques with comparison to a NIST Traceable library of mass spectra when available. Additional characterization techniques may include but are not limited to: refractive index measurements of liquids, melting point measurements of solids, & GC-FID, ECD, PID, ELCD, LC-PDA measurements for purity. Inorganic solutions & neat are typically formulated from materials whose purity & identity have been characterized by ICPMS with comparison to a NIST SRM® when available. Additional characterization techniques may include but are not limited to: titrimetry, and densitometry.

Storage: Sealed ampules and other containers should be stored in the dark and at temperatures indicated on the Certified Weight Report or product label. Certification by Absolute Standards, Inc. is typically valid for 3 years from the date of manufacture. Each product will show its own expiration date as the limit of certification. Certified values are not applicable to opened ampules or for any materials stored in re-sealable containers. Please see the "Certified Weight Report" for specific values and any exceptions.

Usage: Ampules & bottles should be brought to room temperature (18 to 30 °C) before opening. Sonication may be required for high concentration solutions or solutions that may precipitate during storage. After opening, care should be exercised to avoid concentration changes owing to evaporation of the solvent or essential components. We recommend that a suitable re-sealable container be available before opening an ampule to decant the standard for short-term storage and use.

Minimum Sample Size: 0.5 uL for analytical applications.

Legal Notice: Warranty of products are as described when shipped. No warranty as to fitness for any particular application is expressed or implied. Errant shipments and/or quality claims must be made within 10 days of receipt. Liability is limited solely to the replacement of the product or refund of purchase price.

Certifying Officer: Stephen J. Arpie, M.S., Director General



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514

Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: StephenArpie@AbsoluteStandards.com

Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019

Page 1 of 2



ABSOLUTE STANDARDS, INC.

ISO - 17034



Understanding the Certified Weight Report



Each Certified Reference Material (CRM) is supported by a Certified Weight Report. Assigned values for concentrations and associated uncertainties are based upon NIST traceable masses & volumes used in production.

Absolute Standards, Inc.
800-368-1131
www.absolutestandards.com

Certified Reference Material CRM
Scope: <http://AbsoluteStandards.com>

Part #
Lot #
Shelf Life

CERTIFIED WEIGHT REPORT

| Part Number: | Lot Number: | Description: | Expiration Date: | Recommended Storage Conditions: | NIST Test ID#: | Weight(s) shown below were combined and diluted to (mL): |
|---|-------------|----------------------------------|------------------|---------------------------------|----------------|--|
| 10000R 070716 CLP Priority Pollutant Internal Standards GC/MS Calibration - 8 components | 070716 | GC/MS Calibration - 8 components | 070721 | Room Temp (20 °C) 4000 | 822-578752-11 | 500.0 |
| 1. 1,4-Dichlorobenzene-d4 | 118 | PR-144807287CB1 | 4000 | 98 | 0.2 | 2.04083 |
| 2. Naphthalene-d8 | 223 | PR-23250031618PM1 | 4000 | 99 | 0.2 | 2.00032 |
| 3. Acenaphthene-d10 | 2 | PR-29444 | 4000 | 99 | 0.2 | 2.00032 |
| 4. Phenanthrene-d10 | 249 | PR-2905007171PM1 | 4000 | 98 | 0.2 | 2.04093 |
| 5. Chrysene-d12 | 92 | 1-12650 | 4000 | 98 | 0.2 | 2.04093 |
| 6. Pyrene-d12 | 247 | PR-24119 | 4000 | 98 | 0.2 | 2.04093 |


Target Compounds

Method of Analysis

Run 35, "P10000R L070716 (4000)@mL in MeC12"

Run Length: 40.00 min, 23000 points at 10 points/second.
Created: Sat, Jul 8, 2017 at 11:54:32 AM
Analyzed using Method "GC25-M2".

Comments:
GC25-M2 Analyzed by Melissa Stryker
Column ID: SPB-5, 0.25mm ID, 0.1mm film thickness, 100m
Carrier Gas: Helium, 1.0 mL/min, 30.0 psi
Hydrogen (make-up): 25 mL
Hydrogen (detector): 30 mL, Air (detector): 300 mL/min, Temp: 1 = 50°C (1 min)
Temp: 2 = 150°C (1 min), Temp: 3 = 250°C (1 min), Total Run Time = 40.00 minutes, Injector Temp = 250°C
FID Temp = 300°C, FID Split = 0.00, FID Split Ratio = 1.00, FID Split Volume = 0.00 mL
Gas Chromatograph = HP 5890, Auto Sampler = HP 7693, Standard Injection = 0.5 µL, Range = 4

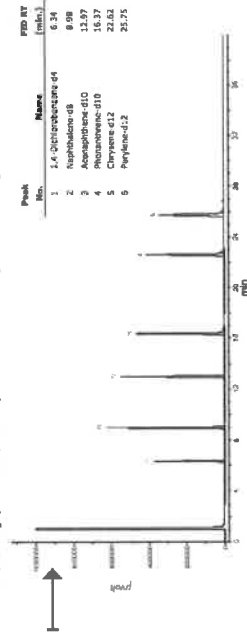

Qualitative Quantitative

Formulator Reviewer

Formulated By: *Pedro L. Ruelas*
Reviewed By: *Pedro L. Ruelas*
DATE: 07/07/16
DATE: 07/07/16

Actual Concentration
Uncertainty Values
Health & Safety

| Compound | Actual Conc (µg/mL) | Expanded Uncertainty (k=2) | MSDS Information (Solvent Safety Info. On Attached pg.) |
|---------------------------|---------------------|----------------------------|---|
| 1. 1,4-Dichlorobenzene-d4 | 4004.7 | 16.4 | 3806-62-1 N/A |
| 2. Naphthalene-d8 | 4001.9 | 16.2 | 114-66-2 10 ppm (20mg/200mL) - avoid skin contact |
| 3. Acenaphthene-d10 | 4004.2 | 16.2 | 16087-26-2 N/A |
| 4. Phenanthrene-d10 | 4000.8 | 16.4 | 1517-82-2 N/A |
| 5. Chrysene-d12 | 4001.3 | 16.4 | 1714-83-6 N/A |
| 6. Pyrene-d12 | 4001.7 | 16.4 | 1830-46-3 N/A |

Absolute Standards, Inc. certifies that the above listed and individually referenced (by analytical data) for these products. They are prepared for sale as these purity reviewed and certified by Absolute Standards, Inc. and are traceable to NIST and meet all specifications under the terms of agreement for Reciprocal Data Review (RDR).

Absolute Standards, Inc.
Superior, IN
P#10000R L070716
P#17004 L045560

3rd Party Comparison

| Analysis | Sup/Assay | Dev (%) |
|------------------------|-----------------------|---------|
| 1,4-Dichlorobenzene-d4 | (Sup/Assay) X 100-100 | 2.55 |
| Naphthalene-d8 | | 2.43 |
| Acenaphthene-d10 | | 2.74 |
| Phenanthrene-d10 | | 0.03 |
| Chrysene-d12 | | 1.92 |
| Pyrene-d12 | | -1.72 |
| Total | | -0.56 |

Part # 10000R Lot # 041219

1 of 2

Printed: 5/8/2019, 12:55:50 PM

For More Information, Contact:

StephenArpie@AbsoluteStandards.com

Page 2 of 2



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514

Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: StephenArpie@AbsoluteStandards.com
Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019





CERTIFIED WEIGHT REPORT

Part Number: **72072**
Lot Number: **101122**
Description: **n-Tetracosane-d50**

Solvent(s):
Methylene chloride

Lot#
105345

| | | |
|-------------------------|------------------|--------|
| <i>Prashant Chauhan</i> | | 101122 |
| Formulated By: | Prashant Chauhan | DATE |
| <i>Pedro L. Rentas</i> | | 101122 |
| Reviewed By: | Pedro L. Rentas | DATE |

Expiration Date: 101132
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 6UTB



Weight(s) shown below were combined and diluted to (mL): 200.0

5E-05 Balance Uncertainty
0.058 Flask Uncertainty

P12291
↓
P12310 } *Y.P.*
02/22/23

| Compound | RM# | Lot Number | Nominal Conc (µg/mL) | Purity (%) | Uncertainty Purity | Assay (%) | Target Weight(g) | Actual Weight(g) | Actual Conc (µg/mL) | Expanded Uncertainty (+/-) (µg/mL) | SDS Information (Solvent Safety Info. On Attached pg.) | | |
|----------------------|------|------------|----------------------|------------|--------------------|-----------|------------------|------------------|---------------------|------------------------------------|--|----------------|------|
| | | | | | | | | | | | CAS# | OSHA PEL (TWA) | LD50 |
| 1. n-Tetracosane-d50 | 2072 | PR-26606 | 1000 | 98.7 | 0.2 | 99.0 | 0.20471 | 0.20482 | 1000.6 | 4.1 | 16416-32-3 | N/A | N/A |

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

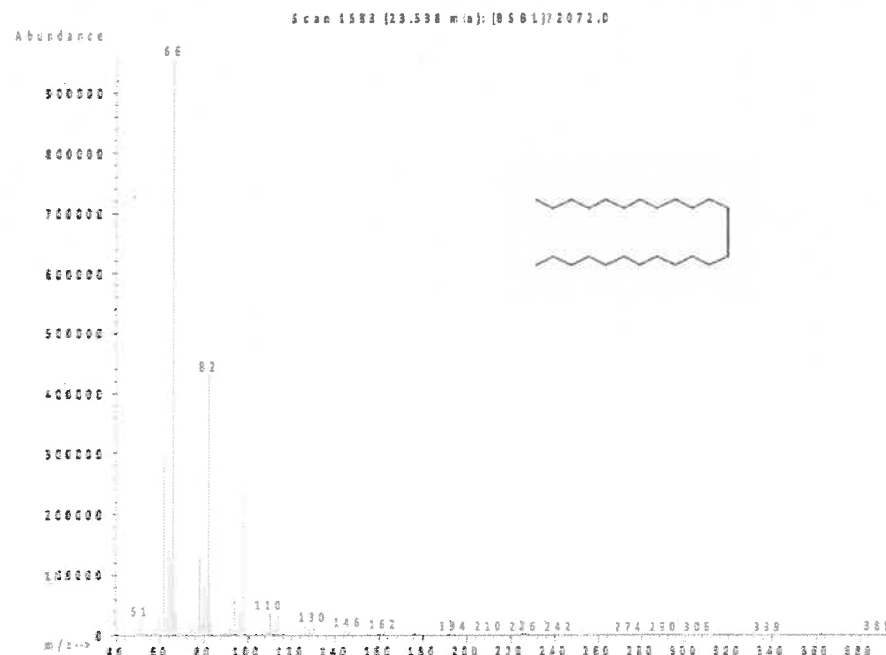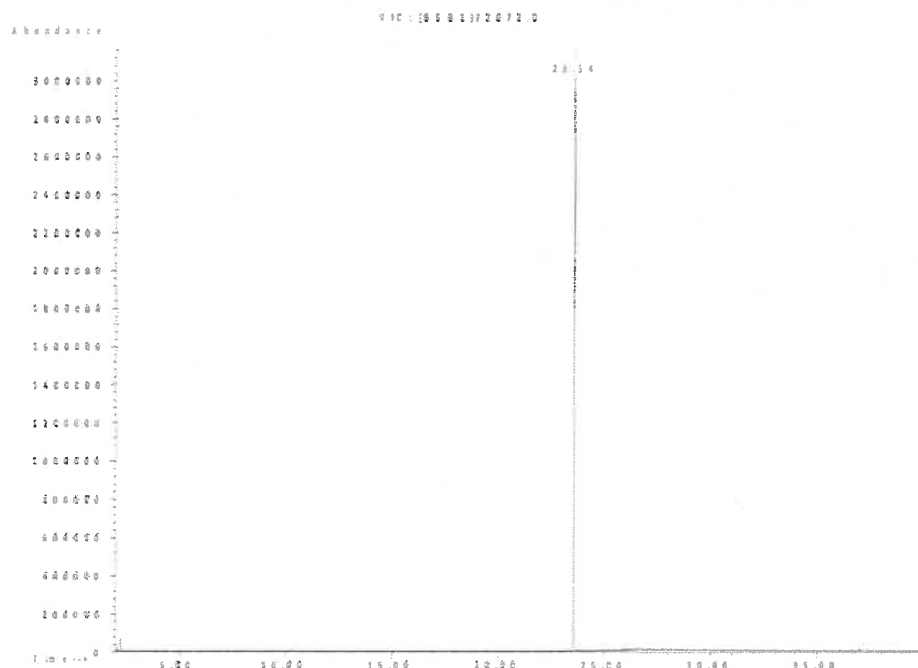

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Safety Data Sheet (SDS)

GHS/OSHA Compliant

Section I Product and Company Identification

IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHYLENE CHLORIDE

| | | | |
|---------------------|------------------------------------|--|-----------------------------------|
| Manufacturer's Name | ABSOLUTE STANDARDS INC | Emergency Telephone USA & CANADA | 1-800-535-5053 |
| Address | 44 Rosotto Dr. Hamden CT, 06514 | Emergency Telephone International Date Prepared/Revised | 1-352-323-3500 January 1, 2022 |

Section II - Hazards Identification

GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

| | | | |
|----------|--------------------------------------|--------------|---|
| H302 | Harmful if swallowed. | H315,H320 | Causes skin and eye irritation. |
| H351 | Suspected of causing cancer. | H335 | May cause respiratory irritation. |
| P271 | Use in ventilated area | P280 | Use gloves, eye protection/face shield |
| P302,332 | If on skin, wash with soap and water | P305,351,338 | If in eyes, remove contacts, rinse with water |



Signal Word: WARNING

Section III - Composition

| | | | | |
|-----------------|---------|----------------|---------------|--------------|
| Components: | CAS#: | OSHA PEL (TWA) | LD50 orl-rat | % (optional) |
| Dichloromethane | 75-09-2 | 50 ppm | > 2,000 mg/kg | > 97 |

See Certified Weight Report For Other Analytes Present At Trace Quantities.
INTENDED USE: REFERENCE MATERIAL

Section IV. FIRST AID MEASURES

| | |
|-------------------------|---|
| General advice | Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area. |
| If inhaled | If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician. |
| In case of skin contact | Wash with soap and water. Consult a physician. |
| In case of eye contact | Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician. |
| If swallowed | Do NOT induce vomiting. Rinse mouth with water. Consult a physician. |

Section V. FIREFIGHTING MEASURES

| | |
|-------------------------------|--|
| Suitable extinguishing media | Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide. |
| Protective equipment for fire | Wear self contained breathing apparatus for fire fighting if necessary. |

Section VI. ACCIDENTAL RELEASE MEASURES

| | |
|---------------------------|---|
| Personal precautions | Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations. |
| Environmental precautions | Prevent further leakage or spillage if safe to do so. Do not let product enter drains. |
| Clean up | Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13). |

Section VII. HANDLING AND STORAGE

| | |
|-------------------------------|---|
| Precautions for safe handling | Avoid contact with skin and eyes. Avoid inhalation of vapour or mist. |
| Storage Conditions | Use ventilation Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge. Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage. |

Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

| | |
|--|--|
| Methylene chloride 75-09-2 TWA 50 ppm | |
| Potential for skin absorption, ingestion and inhalation. | |
| Personal protective equipment | Respiratory protection |
| Personal contact with skin, eyes and clothing. | Wash hands thoroughly after handling the product |
| | Handle with gloves. Gloves must be inspected prior to use. |
| | Eye protection. |

Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS

| | | | |
|---------------|------|----------------------------|-------|
| Boiling Point | 40°C | Specific Gravity (H2O = 1) | 1.325 |
|---------------|------|----------------------------|-------|

| | | | |
|-------------------------|------------------|---|-------|
| Vapor Pressure (mm Hg) | 353 | Melting Point | -97°C |
| Vapor Density (AIR = 1) | 2.93 | Evaporation rate (Butyl Acetate = 1) | 0.71 |
| Solubility in Water | Slightly soluble | | |

Appearance and Odor CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.

Section X. STABILITY AND REACTIVITY

| | |
|------------------------------------|---|
| Chemical stability | Stable under recommended storage conditions. |
| Possibility of hazardous reactions | No data available |
| Conditions to avoid | Heat, flames, sparks, extreme temperature and sunlight. |
| Materials to avoid | Alkali metals, Aluminum, Oxidizing agents, Bases, Amines, Magnesium, Acids, Vinyl compounds |
| Hazardous decomposition products | - No data available |

Section XI. TOXICOLOGICAL INFORMATION

LD50 Oral - Rat - > 2,000 mg/kg
LC50 Inhalation - Rat - 52,000 mg/m3
LD50 Dermal - Rat - > 2,000 mg/kg
Toxic if absorbed through skin. Causes skin irritation.
Eye damage/eye irritation
Toxic if inhaled. Causes respiratory tract irritation.
Toxic if swallowed.

Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 1000 lbs.

LC50 193.00 mg/l - 96 h
EC50 1,682.00 mg/l - 48 h

Section XIII. DISPOSAL CONSIDERATIONS

Dispose with normal Laboratory Solvent Waste.

Section XIV. TRANSPORT INFORMATION

DOT (US) IATA
UN number: 1593 Class: 6.1 Packing group: III UN number: 1593 Class: 6.1 Packing group: III
Proper shipping name: Dichloromethane Proper shipping name: Dichloromethane
Reportable Quantity (RQ): 1000 lbs

Section XV. REGULATORY INFORMATION

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

Section XVI. Misc. INFORMATION

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC. DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.

ABSOLUTE STANDARDS, INC.

ISO - 17034



Certificate of Analysis



Certified Reference Material (CRM)

Conformance: The "Certificate of Analysis" is applicable for CRM's, fulfilling the requirements in the current version of: ISO 17034.

Health & Safety: See the attached SDS & Certified Weight Report before use.

Intended Use: This Certified Reference Material (CRM) is intended primarily for use in the characterization of unknowns and the establishment of analyzer or instrument response factors by qualified personnel. Typical instrumental organic assays include: GC & LC, and inorganic assays include: ICP & AA. This product is for laboratory use only.

Characterization Values: In production, gravimetric/volumetric readings are certified to be within $\pm 0.5\%$ of the stated value & are valid between 18 °C & 30 °C. The measured characterization of uncertainty can be found on the Certified Weight Report. All product weighings are performed on an analytical balance that is calibrated to NIST Traceable standard weights & certified by the manufacturer. The volumetric glassware used is Class "A" type & conforms to ASTM E-288 unless otherwise stated. The solvents & compounds used are of the highest practical purity & typically meet or exceed ACS Reagent Grade & ACS Standards Grade specifications. The expanded uncertainty field on Certified Wt. Report represents CRM uncertainty as described in ISO 17034.

Homogeneity: Uncertainties that are due to the analytical procedure(s) are within $\pm 0.5\%$ unless specifically stated on the Certified Wt. Report.

Verification: Uncertainties that are due to the analytical procedure(s) are within $\pm 0.5\%$ unless specifically stated on the Certified Wt. Report.

Stability: Uncertainties for short-term stability are determined in accordance with ISO 17034. Long-term stability is determined in accordance with ISO 17034. The shelf life is limited by the stated expiration for each product. Expiration dates and additional technical information can be found on the Certified Weight Report and on the product label.

Uncertainty: UCRM is the expanded uncertainty which utilizes a $K = 2$ (coverage factor of 2), in accordance with ISO 17034 as listed above (Characterization, Homogeneity, Verification, and Stability).

Purity & Identity: Organic solutions are typically formulated from neat materials whose purity & identity have been characterized by GC-MSD & LC-PDA techniques with comparison to a NIST Traceable library of mass spectra when available. Additional characterization techniques may include but are not limited to: refractive index measurements of liquids, melting point measurements of solids, & GC-FID, ECD, PID, ELCD, LC-PDA measurements for purity. Inorganic solutions & neat are typically formulated from materials whose purity & identity have been characterized by ICPMS with comparison to a NIST SRM® when available. Additional characterization techniques may include but are not limited to: titrimetry, and densitometry.

Storage: Sealed ampules and other containers should be stored in the dark and at temperatures indicated on the Certified Weight Report or product label. Certification by Absolute Standards, Inc. is typically valid for 3 years from the date of manufacture. Each product will show its own expiration date as the limit of certification. Certified values are not applicable to opened ampules or for any materials stored in re-sealable containers. Please see the "Certified Weight Report" for specific values and any exceptions.

Usage: Ampules & bottles should be brought to room temperature (18 to 30 °C) before opening. Sonication may be required for high concentration solutions or solutions that may precipitate during storage. After opening, care should be exercised to avoid concentration changes owing to evaporation of the solvent or essential components. We recommend that a suitable re-sealable container be available before opening an ampule to decant the standard for short-term storage and use.

Minimum Sample Size: 0.5 uL for analytical applications.

Legal Notice: Warranty of products are as described when shipped. No warranty as to fitness for any particular application is expressed or implied. Errant shipments and/or quality claims must be made within 10 days of receipt. Liability is limited solely to the replacement of the product or refund of purchase price.

Certifying Officer: Stephen J. Arpie, M.S., Director General



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514

Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: StephenArpie@AbsoluteStandards.com

Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019

Page 1 of 2



ABSOLUTE STANDARDS, INC.

ISO - 17034



Understanding the Certified Weight Report



Each Certified Reference Material (CRM) is supported by a Certified Weight Report. Assigned values for concentrations and associated uncertainties are based upon NIST traceable masses & volumes used in production.

Absolute Standards, Inc.
800-368-1131
www.absolutestandards.com



Certified Reference Material CRM



ISO 17034 Accredited
Scope: <http://AbsoluteStandards.com>

Part #
Lot #
Shelf Life

CERTIFIED WEIGHT REPORT

Part Number: 10008R
Lot Number: 070716
Description: CUP Priority Pollutant Internal Standards
GC/MS Calibration - 8 components
Expiration Date: 07/07/16
Recommended Storage Temperature (°C): 4000
NIST Test ID#: 822-57872-11
Weights shown below were combined and diluted to (mL):

| Compound | Stock | Lot Number | Normal Conc. (µg/mL) | Purity (%) | Target Weight (µg) | Actual Weight (µg) | Expanded Uncertainty (µg) | Actual Conc. (µg/mL) | Expanded Uncertainty (µg/mL) | Lot # |
|---------------------------|-------|-------------------|----------------------|------------|--------------------|--------------------|---------------------------|----------------------|------------------------------|------------|
| 1. 1,4-Dichlorobenzene-d4 | 118 | PR-144807287CB1 | 4000 | 99 | 0.2 | 2.04083 | 2.04395 | 4004.7 | 16.4 | 8965-82-1 |
| 2. Naphthalene-d8 | 223 | PR-23250031618PM1 | 4000 | 99 | 0.2 | 2.02032 | 2.02094 | 4001.9 | 16.2 | 1144-85-2 |
| 3. Acenaphthene-d10 | 2 | PR-25444 | 4000 | 99 | 0.2 | 2.02032 | 2.02245 | 4004.2 | 16.2 | 16087-26-2 |
| 4. Phenanthrene-d10 | 249 | PR-23050007171PM1 | 4000 | 99 | 0.2 | 2.04093 | 2.04198 | 4000.8 | 16.4 | 1517-82-2 |
| 5. Chrysene-d12 | 92 | 1-12650 | 4000 | 99 | 0.2 | 2.04093 | 2.04199 | 4001.3 | 16.4 | 1714-83-6 |
| 6. Pyrene-d12 | 247 | PR-24119 | 4000 | 99 | 0.2 | 2.04093 | 2.04199 | 4001.7 | 16.4 | 1891-06-3 |


Target Compounds

Method of Analysis

Run 35, *P10008R L070716 (4000µg/mL in MeCN)*

Run Length: 40.00 min, 23000 points at 10 points/second.
Created: Sat, Jul 9, 2016 at 11:54:32 AM
Analyzed using Method: GC25-M27

Comments:
GC25-M27 Analyzed by Melissa Stryker
Column ID: SPB-5, 0.25mm ID, 0.1mm film thickness, 100m
Carrier Gas: Helium, 1.0 mL/min, 30.0 psi
Hydrogen (make-up): 25 mL
Injection Volume: 1 µL
Injection Temperature: 250°C
Oven Temperature: 50°C to 300°C at 10°C/min, 1 min at 300°C
Total Run Time: 40.00 minutes, Injection = 0.5 µL, Range = 4

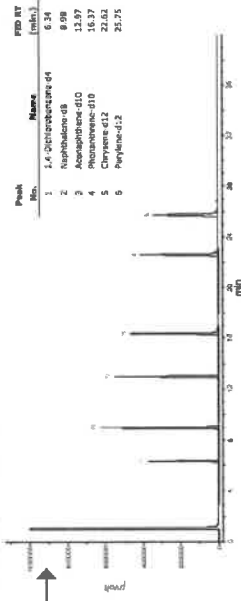

Qualitative Quantitative

Formulator Reviewer

Formulated By: *Paula Simon*
Reviewed By: *Paula Simon*
DATE: 07/07/16
DATE: 07/07/16

Actual Concentration
Uncertainty Values
Health & Safety

3rd Party Comparison

Absolute Standards, Inc.
Superior, IN
P#10008R L#070716
P#17004 L#A55600

| Analysis | Sup/Ass Dev (%) |
|------------------------|-----------------|
| 1,4-Dichlorobenzene-d4 | 2.55 |
| Naphthalene-d8 | 2.43 |
| Acenaphthene-d10 | 2.74 |
| Phenanthrene-d10 | 0.03 |
| Chrysene-d12 | 1.92 |
| Pyrene-d12 | -1.72 |
| Total | -0.56 |

For More Information, Contact:

StephenArpie@AbsoluteStandards.com

Page 2 of 2



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514
Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: StephenArpie@AbsoluteStandards.com
Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019





110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266 **Lot No.:** A0204859

Description : Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2030 **Storage:** 25°C nominal

Handling: Sonicate prior to use. **Ship:** Ambient

P13103 } Y.P.
↓
P13112 } 01/12/2024

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|--|
| 1 | n-Octane (C8) | 111-65-9 | SHBP9758 | 99% | 504.4 µg/mL | +/- 13.0305 |
| 2 | n-Decane (C10) | 124-18-5 | SHBQ1342 | 99% | 503.6 µg/mL | +/- 13.0098 |
| 3 | n-Dodecane (C12) | 112-40-3 | SHBP7054 | 99% | 503.6 µg/mL | +/- 13.0098 |
| 4 | n-Tetradecane (C14) | 629-59-4 | STBK5437 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 5 | n-Hexadecane (C16) | 544-76-3 | SHBP8192 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 6 | n-Octadecane (C18) | 593-45-3 | UE5NG | 98% | 504.1 µg/mL | +/- 13.0230 |
| 7 | n-Eicosane (C20) | 112-95-8 | MKCN8767 | 97% | 504.0 µg/mL | +/- 13.0204 |
| 8 | n-Docosane (C22) | 629-97-0 | MKCQ3882 | 99% | 503.6 µg/mL | +/- 13.0098 |
| 9 | n-Tetracosane (C24) | 646-31-1 | MKCQ8345 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 10 | n-Hexacosane (C26) | 630-01-3 | MKCQ4814 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 11 | n-Octacosane (C28) | 630-02-4 | BCCG0084 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 12 | n-Triacontane (C30) | 638-68-6 | MKCQ9436 | 97% | 504.0 µg/mL | +/- 13.0204 |
| 13 | n-Dotriacontane (C32) | 544-85-4 | BCBW0661 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 14 | n-Tetratriacontane (C34) | 14167-59-0 | OML4N | 99% | 504.4 µg/mL | +/- 13.0305 |
| 15 | n-Hexatriacontane (C36) | 630-06-8 | Z27H018 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 16 | n-Octatriacontane (C38) | 7194-85-6 | 0000145137 | 96% | 503.8 µg/mL | +/- 13.0152 |
| 17 | n-Tetracontane (C40) | 4181-95-7 | OKEGA | 99% | 503.6 µg/mL | +/- 13.0098 |

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

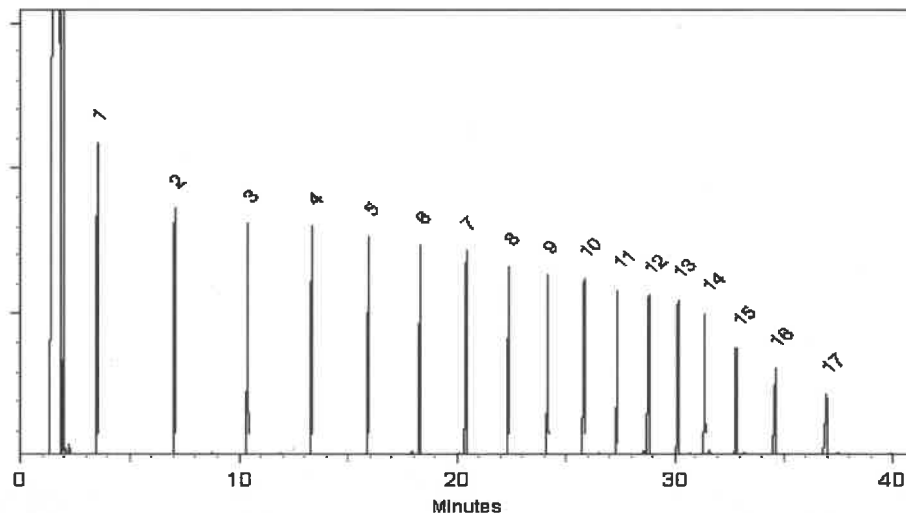

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 29-Nov-2023

Balance Serial # B442140311


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Dec-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31266 **Lot No.:** A0204859

Description : Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : December 31, 2030 **Storage:** 25°C nominal

Handling: Sonicate prior to use. **Ship:** Ambient

P13103 } Y.P.
↓
P13112 } 01/12/2024

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------------------|------------|------------|--------|-----------------------------|--|
| 1 | n-Octane (C8) | 111-65-9 | SHBP9758 | 99% | 504.4 µg/mL | +/- 13.0305 |
| 2 | n-Decane (C10) | 124-18-5 | SHBQ1342 | 99% | 503.6 µg/mL | +/- 13.0098 |
| 3 | n-Dodecane (C12) | 112-40-3 | SHBP7054 | 99% | 503.6 µg/mL | +/- 13.0098 |
| 4 | n-Tetradecane (C14) | 629-59-4 | STBK5437 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 5 | n-Hexadecane (C16) | 544-76-3 | SHBP8192 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 6 | n-Octadecane (C18) | 593-45-3 | UE5NG | 98% | 504.1 µg/mL | +/- 13.0230 |
| 7 | n-Eicosane (C20) | 112-95-8 | MKCN8767 | 97% | 504.0 µg/mL | +/- 13.0204 |
| 8 | n-Docosane (C22) | 629-97-0 | MKQC3882 | 99% | 503.6 µg/mL | +/- 13.0098 |
| 9 | n-Tetracosane (C24) | 646-31-1 | MKQC8345 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 10 | n-Hexacosane (C26) | 630-01-3 | MKQC4814 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 11 | n-Octacosane (C28) | 630-02-4 | BCCG0084 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 12 | n-Triacontane (C30) | 638-68-6 | MKQC9436 | 97% | 504.0 µg/mL | +/- 13.0204 |
| 13 | n-Dotriacontane (C32) | 544-85-4 | BCBW0661 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 14 | n-Tetratriacontane (C34) | 14167-59-0 | OML4N | 99% | 504.4 µg/mL | +/- 13.0305 |
| 15 | n-Hexatriacontane (C36) | 630-06-8 | Z27H018 | 99% | 504.0 µg/mL | +/- 13.0201 |
| 16 | n-Octatriacontane (C38) | 7194-85-6 | 0000145137 | 96% | 503.8 µg/mL | +/- 13.0152 |
| 17 | n-Tetracontane (C40) | 4181-95-7 | OKEGA | 99% | 503.6 µg/mL | +/- 13.0098 |

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:
30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:
hydrogen-constant pressure 10 psi.

Temp. Program:
40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
330°C

Det. Type:
FID

Split Vent:
2 ml/min.

Inj. Vol
1µl

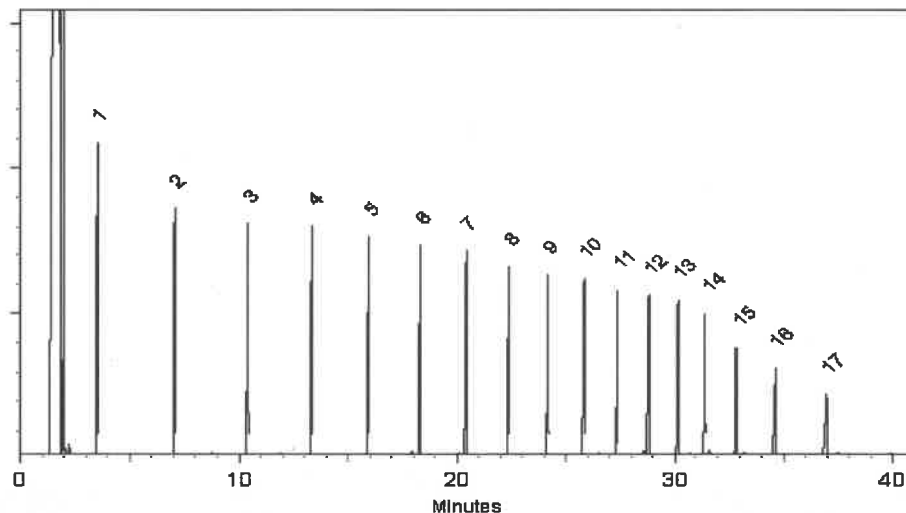

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 29-Nov-2023

Balance Serial # B442140311


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Dec-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

1st source

DP

P9817

To

10

P9826

Catalog No. : 30065 **Lot No.:** A0155991

Description : Gasoline Range Organics Mix (EPA)
Gasoline Range Organics Mix (EPA) 500 - 1500µg/mL, P&T Methanol, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2027 **Storage:** 0°C or colder

CERTIFIED VALUES

| Elution Order | Compound | Grav. Conc. (weight/volume) | Expanded Uncertainty (95% C.L.; K=2) |
|---------------|--|-----------------------------|--|
| 1 | 2-Methylpentane CAS # 107-83-5 (Lot MKCB1674V) Purity 98% | 1,505.3 µg/mL | +/- 8.9409 µg/mL Gravimetric +/- 84.4194 µg/mL Unstressed +/- 86.3938 µg/mL Stressed |
| 2 | 2,2,4-Trimethylpentane (isooctane) CAS # 540-84-1 (Lot SHBD2922V) Purity 99% | 1,504.0 µg/mL | +/- 8.9333 µg/mL Gravimetric +/- 84.3476 µg/mL Unstressed +/- 86.3203 µg/mL Stressed |
| 3 | n-Heptane (C7) CAS # 142-82-5 (Lot SHBK8626) Purity 98% | 500.8 µg/mL | +/- 2.9745 µg/mL Gravimetric +/- 28.0848 µg/mL Unstressed +/- 28.7417 µg/mL Stressed |
| 4 | Benzene CAS # 71-43-2 (Lot SHBK5679) Purity 99% | 501.0 µg/mL | +/- 2.9758 µg/mL Gravimetric +/- 28.0972 µg/mL Unstressed +/- 28.7543 µg/mL Stressed |
| 5 | Toluene CAS # 108-88-3 (Lot MKCH9232) Purity 99% | 1,505.0 µg/mL | +/- 8.9392 µg/mL Gravimetric +/- 84.4037 µg/mL Unstressed +/- 86.3777 µg/mL Stressed |
| 6 | Ethylbenzene CAS # 100-41-4 (Lot SHBJ4278) Purity 99% | 502.0 µg/mL | +/- 2.9817 µg/mL Gravimetric +/- 28.1533 µg/mL Unstressed +/- 28.8117 µg/mL Stressed |
| 7 | m-Xylene CAS # 108-38-3 (Lot SHBJ8743) Purity 99% | 1,004.0 µg/mL | +/- 5.9635 µg/mL Gravimetric +/- 56.3065 µg/mL Unstressed +/- 57.6234 µg/mL Stressed |

| | | | | | | |
|------------------------------|------------------------|-----------------|---------------|-------------|-------|-------------|
| 8 | o-Xylene | | 1,008.0 µg/mL | +/- 5.9872 | µg/mL | Gravimetric |
| | CAS # 95-47-6 | (Lot SHBK7739) | | +/- 56.5308 | µg/mL | Unstressed |
| | Purity 99% | | | +/- 57.8530 | µg/mL | Stressed |
| 9 | 1,2,4-Trimethylbenzene | | 1,004.5 µg/mL | +/- 5.9664 | µg/mL | Gravimetric |
| | CAS # 95-63-6 | (Lot MKBJ6229V) | | +/- 56.3345 | µg/mL | Unstressed |
| | Purity 98% | | | +/- 57.6521 | µg/mL | Stressed |
| Solvent: P&T Methanol | | | | | | |
| | CAS # 67-56-1 | | | | | |
| | Purity 99% | | | | | |

Column:
105m x 0.53mm x 3.0µm
Rtx-502.2 (cat.#10910)


Carrier Gas:
hydrogen-constant pressure 11.0 psi.

Temp. Program:
40°C (hold 2 min.) to 240°C
@ 8°C/min. (hold 5 min.)

Inj. Temp:
200°C

Det. Temp:
250°C

Det. Type:
FID

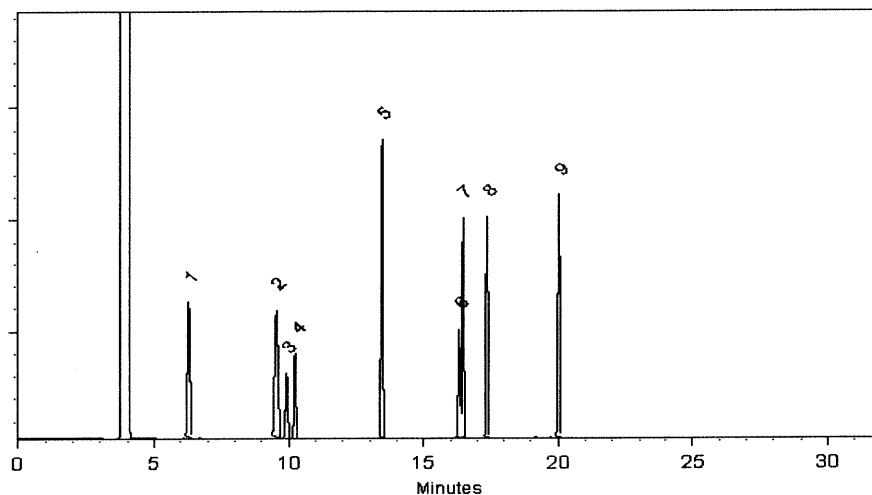

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Miranda Kline
Miranda Kline - Operations Technician I

Date Mixed: 19-Dec-2019

Balance: 1127510105

Feng-Yun Lo
Feng-Yun Lo - QC Analyst

Date Passed: 23-Dec-2019

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397