

### Prep Standard - Chemical Standard Summary

**Order ID :** P2834  
**Test :** Metals CLP Full  
  
**Prepbatch ID :** PB161712,  
**Sequence ID/Qc Batch ID:** LB131456,

**Standard ID :**  
MP80924,MP80925,MP80926,MP80927,MP80928,MP80931,MP80932,MP80933,MP80934,MP80935,MP80942,MP80944,  
MP81026,MP81115,MP81116,MP81119,MP81187,MP81208,MP81209,

**Chemical ID :**  
M4877,M4883,M4885,M4888,M4889,M4960,M4961,M5130,M5192,M5200,M5223,M5224,M5227,M5272,M5288,M5289,M5  
294,M5296,M5298,M5387,M5389,M5395,M5429,M5468,M5473,M5494,M5497,M5498,M5513,M5632,M5658,M5697,M5698  
,M5747,M5754,M5768,M5769,M5798,M5799,M5800,M5801,M5815,M5817,M5818,M5819,M5875,M5895,M5915,M5935,M5  
940,M5947,W2606,

## Metals STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>                   | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 902              | ICP AES CAL BLK ( SO/ICB/CCB) | <a href="#">MP80924</a> | 05/30/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | None             | Mohan Bera           |
|                  |                               |                         |                  |                        |                    |                |                  | 06/11/2024           |

**FROM** 125.00000ml of M5895 + 2350.00000ml of W2606 + 25.00000ml of M5915 = Final Quantity: 2500.000 ml

| <u>Recipe ID</u> | <u>NAME</u>         | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 1004             | ICPAES ISM01.2 (S5) | <a href="#">MP80925</a> | 05/30/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | METALS_PIPE      | Mohan Bera           |
|                  |                     |                         |                  |                        |                    |                | TTE_3 (A)        | 06/11/2024           |

**FROM** 0.25000ml of M5798 + 0.50000ml of M5429 + 0.50000ml of M5473 + 0.50000ml of M5815 + 0.50000ml of M5817 +  
12.50000ml of M5200 + 12.50000ml of M5288 + 12.50000ml of M5698 + 12.50000ml of M5819 + 13.75000ml of M5697 +  
14.50000ml of M5289 + 14.50000ml of M5298 + 14.50000ml of M5658 + 2.00000ml of M5513 + 22.50000ml of M5498 +  
22.50000ml of M5769 + 5.00000ml of M5272 + 5.00000ml of M5296 + 5.00000ml of M5395 + 5.00000ml of M5818 +  
5.00000ml of M5875 + 318.50000ml of MP80924 = Final Quantity: 500.000 ml

## Metals STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>        | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u>         | <u>Supervised By</u>     |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|--------------------------|--------------------------|
| 1005             | ICPAES ISM01.2(S4) | <a href="#">MP80926</a> | 05/30/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | METALS_PIPE<br>TTE_3 (A) | Mohan Bera<br>06/11/2024 |

**FROM** 50.00000ml of MP80924 + 50.00000ml of MP80925 = Final Quantity: 100.000 ml

| <u>Recipe ID</u> | <u>NAME</u>        | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u>         | <u>Supervised By</u>     |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|--------------------------|--------------------------|
| 1007             | ICPAES ISM01.2(S3) | <a href="#">MP80927</a> | 05/30/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | METALS_PIPE<br>TTE_3 (A) | Mohan Bera<br>06/11/2024 |

**FROM** 25.00000ml of MP80925 + 75.00000ml of MP80924 = Final Quantity: 100.000 ml

## Metals STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>        | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u>         | <u>Supervised By</u>     |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|--------------------------|--------------------------|
| 1008             | ICPAES ISM01.2(S2) | <a href="#">MP80928</a> | 05/30/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | METALS_PIPE<br>TTE_3 (A) | Mohan Bera<br>06/11/2024 |

**FROM** 12.50000ml of MP80925 + 87.50000ml of MP80924 = Final Quantity: 100.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u>         | <u>Supervised By</u>     |
|------------------|-------------|-------------------------|------------------|------------------------|--------------------|----------------|--------------------------|--------------------------|
| 2054             | ICV-ICPAES  | <a href="#">MP80931</a> | 05/30/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | METALS_PIPE<br>TTE_3 (A) | Mohan Bera<br>06/11/2024 |

**FROM** 10.00000ml of M5294 + 90.00000ml of MP80924 = Final Quantity: 100.000 ml



## Metals STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>       | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u>         | <u>Supervised By</u>     |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|--------------------------|--------------------------|
| 904              | ICP AES ICSA SOLN | <a href="#">MP80932</a> | 05/30/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | METALS_PIPE<br>TTE_3 (A) | Mohan Bera<br>06/11/2024 |

**FROM** 10.00000ml of M5130 + 90.00000ml of MP80924 = Final Quantity: 100.000 ml

| <u>Recipe ID</u> | <u>NAME</u>        | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u>         | <u>Supervised By</u>     |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|--------------------------|--------------------------|
| 905              | ICP AES ICSAB SOLN | <a href="#">MP80933</a> | 05/30/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | METALS_PIPE<br>TTE_3 (A) | Mohan Bera<br>06/11/2024 |

**FROM** 10.00000ml of M5130 + 10.00000ml of M5223 + 80.00000ml of MP80924 = Final Quantity: 100.000 ml



## Metals STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>  | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u>         | <u>Supervised By</u>     |
|------------------|--|-------------------------|------------------|------------------------|--------------------|----------------|--------------------------|--------------------------|
| 1119             | ICPAES ISM01.2(CCV)  | <a href="#">MP80934</a> | 05/30/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | METALS_PIPE<br>TTE_3 (A) | Mohan Bera<br>06/11/2024 |
| <u>FROM</u>      | 12.25000ml of M5289 + 12.50000ml of M5200 + 12.50000ml of M5298 + 7.50000ml of M5498 + 7.50000ml of M5769 + 125.00000ml of MP80925 + 322.75000ml of MP80924 = Final Quantity: 500.000 ml |                         |                  |                        |                    |                |                          |                          |

| <u>Recipe ID</u>  | <u>NAME</u>           | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u>         | <u>Supervised By</u>     |
|---|-----------------------|-------------------------|------------------|------------------------|--------------------|----------------|--------------------------|--------------------------|
| 2480  | ICP AES STD 6 ISM01.3 | <a href="#">MP80935</a> | 05/30/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | METALS_PIPE<br>TTE_3 (A) | Mohan Bera<br>06/11/2024 |
| <p><b><u>FROM</u></b> 8.00000ml of M5200 + 8.00000ml of M5289 + 8.00000ml of M5298 + 8.00000ml of M5498 + 8.00000ml of M5769 + 60.00000ml of MP80924 = Final Quantity: 100.000 ml</p> |                       |                         |                  |                        |                    |                |                          |                          |



| <u>Recipe ID</u>  | <u>NAME</u>          | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u>     |
|---|----------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|--------------------------|
| 919   | ICP AES INTERNAL STD | <a href="#">MP80942</a> | 05/30/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | None             | Mohan Bera<br>06/11/2024 |
| <b><u>FROM</u></b> 1.00000ml of M4961 + 10.00000ml of M4960 + 1969.00000ml of W2606 + 20.00000ml of M5915 = Final Quantity: 2000.000 ml |                      |                         |                  |                        |                    |                |                  |                          |

| <u>Recipe ID</u>   | <u>NAME</u>        | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u>     |
|--|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|--------------------------|
| 903  | ICP AES RINSE SOLN | <a href="#">MP80944</a> | 05/30/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | None             | Mohan Bera<br>06/11/2024 |
| <b><u>FROM</u></b> 200.00000ml of M5915 + 9800.00000ml of W2606 = Final Quantity: 10000.000 ml |                    |                         |                  |                        |                    |                |                  |                          |

## Metals STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u>        | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u>         | <u>Supervised By</u>     |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|--------------------------|--------------------------|
| 921              | ICPAES SPIKE SOL#6 | <a href="#">MP81026</a> | 06/10/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | METALS_PIPE<br>TTE_3 (A) | Mohan Bera<br>06/13/2024 |

**FROM** 0.12500ml of M4883 + 1.25000ml of M5192 + 25.00000ml of M5754 + 23.62500ml of MP80924 = Final Quantity: 50.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u>     |
|------------------|-------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|--------------------------|
| 3811             | SE-10PPM    | <a href="#">MP81115</a> | 06/17/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | None             | Mohan Bera<br>06/21/2024 |

**FROM** 0.10000ml of M4883 + 9.90000ml of MP80924 = Final Quantity: 10.000 ml

## Metals STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------|
| 3816             | TL-10PPM    | <a href="#">MP81116</a> | 06/17/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | None             | Mohan Bera           |
|                  |             |                         |                  |                        |                    |                |                  | 06/21/2024           |

**FROM** 0.10000ml of M4889 + 9.90000ml of MP80924 = Final Quantity: 10.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u>          | <u>PipetteID</u>          | <u>Supervised By</u> |
|------------------|-------------|-------------------------|------------------|------------------------|--------------------|-------------------------|---------------------------|----------------------|
| 169              | 1:1HNO3     | <a href="#">MP81119</a> | 06/21/2024       | 10/24/2024             | AI-Terek Isaac     | METALS_SCALE_2 (M SC-2) | METALS_PIPE_TTE_1 (ICP A) | Sarabjit Jaswal      |
|                  |             |                         |                  |                        |                    |                         |                           | 06/21/2024           |

**FROM** 1250.00000ml of M5935 + 1250.00000ml of W2606 = Final Quantity: 2500.000 ml



## Metals STANDARD PREPARATION LOG

[illegible]

| <u>Recipe ID</u>   | <u>NAME</u>   | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u>         | <u>Supervised By</u>     |
|--------------------|---|-------------------------|------------------|------------------------|--------------------|----------------|--------------------------|--------------------------|
| 994                | ICPAES ISM01.2 S1 (CONC.)   | <a href="#">MP81208</a> | 06/25/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | METALS_PIPE<br>TTE_3 (A) | Mohan Bera<br>06/27/2024 |
| <b><u>FROM</u></b> | 0.02000ml of M5815 + 0.03000ml of M5429 + 0.10000ml of M4877 + 0.10000ml of M5798 + 0.14000ml of M5799 +<br>0.20000ml of M4885 + 0.20000ml of M5192 + 0.20000ml of M5298 + 0.20000ml of M5473 + 0.20000ml of M5658 +<br>0.20000ml of M5747 + 0.20000ml of M5801 + 0.20000ml of M5817 + 0.30000ml of M5698 + 0.40000ml of M5289 +<br>0.50000ml of M4889 + 0.50000ml of M5697 + 0.70000ml of M4883 + 0.80000ml of M5494 + 1.00000ml of M5227 +<br>1.00000ml of M5800 + 1.20000ml of M5224 + 1.20000ml of M5819 + 10.00000ml of M5200 + 10.00000ml of M5288 +<br>10.00000ml of M5468 + 10.00000ml of M5497 + 10.00000ml of M5818 + 2.00000ml of M4888 + 4.00000ml of M5387 +<br>34.41000ml of MP80924 = Final Quantity: 100.000 ml |                         |                  |                        |                    |                |                          |                          |



| <u>Recipe ID</u> | <u>NAME</u>   | <u>NO.</u>              | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipettelD</u> | <u>Supervised By</u>     |
|------------------|---|-------------------------|------------------|------------------------|--------------------|----------------|------------------|--------------------------|
| 1003             | ICPAES ISM01.2 S1   | <a href="#">MP81209</a> | 06/25/2024       | 06/30/2024             | Sarabjit Jaswal    | None           | None             | Mohan Bera<br>06/27/2024 |
| <u>FROM</u>      | 0.50000ml of MP81208 + 99.50000ml of MP80924 = Final Quantity: 100.000 ml |                         |                  |                        |                    |                |                  |                          |

## CHEMICAL RECEIPT LOG BOOK

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57048 / Cd, 1000 PPM, 125 ml | 072821 | 07/28/2024      | 08/06/2021 / jaswal     | 08/05/2021 / jaswal         | M4877          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57034 / Se, 1000 PPM, 125 ml | 070221 | 07/02/2024      | 08/06/2021 / jaswal     | 08/05/2021 / jaswal         | M4883          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57047 / Ag, 1000 PPM, 125 ml | 072921 | 07/29/2024      | 08/06/2021 / jaswal     | 08/05/2021 / jaswal         | M4885          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57022 / Ti, 1000 PPM, 125 ml | 070721 | 07/07/2024      | 08/06/2021 / jaswal     | 08/05/2021 / jaswal         | M4888          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57081 / TI, 1000 PPM, 125 ml | 073021 | 07/30/2024      | 08/06/2021 / jaswal     | 08/05/2021 / jaswal         | M4889          |

| Supplier           | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Inorganic Ventures | CGIN10-5 / INDIUM 1 x 500 ml | 100721 | 10/07/2024      | 10/09/2021 / jaswal     | 10/08/2021 / jaswal         | M4960          |



## CHEMICAL RECEIPT LOG BOOK

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58139 / Y, 10000 PPM, 500 ml | 052521 | 06/25/2024      | 10/09/2021 / jaswal     | 01/25/2019 / jaswal         | M4961          |

| Supplier | ItemCode / ItemName              | Lot #     | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|----------------------------------|-----------|-----------------|-------------------------|-----------------------------|----------------|
| EPA      | PART A / ICSA ( ICP ) STOCK SOLN | ICSA-1211 | 11/19/2024      | 05/20/2024 / jaswal     | 04/20/2021 / bin            | M5130          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57042 / Mo, 1000 PPM, 125 ml | 051722 | 05/17/2025      | 07/01/2022 / bin        | 06/17/2022 / jaswal         | M5192          |

| Supplier                 | ItemCode / ItemName           | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58111 / Na, 10000 PPM, 500 ml | 092121 | 09/21/2024      | 06/23/2022 / bin        | 10/05/2021 / bin            | M5200          |

| Supplier | ItemCode / ItemName               | Lot #     | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|-----------------------------------|-----------|-----------------|-------------------------|-----------------------------|----------------|
| EPA      | PART B / ICSAB ( ICP ) STOCK SOLN | ICSB-0710 | 11/19/2024      | 05/20/2024 / jaswal     | 04/20/2021 / bin            | M5223          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57051 / Sb, 1000 PPM, 125 ml | 101521 | 10/15/2024      | 06/29/2022 / bin        | 10/18/2021 / bin            | M5224          |

## CHEMICAL RECEIPT LOG BOOK

| Supplier                 | ItemCode / ItemName         | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-----------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57023 / V, 1000 PPM, 125 ml | 100121 | 10/01/2024      | 07/01/2022 / bin        | 10/18/2021 / bin            | M5227          |

| Supplier                 | ItemCode / ItemName | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|---------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | / Antimony (Sb)     | 051822 | 05/18/2025      | 05/10/2023 / bin        | 08/24/2022 / jaswal         | M5272          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58119 / K, 10000 PPM, 500 ml | 071122 | 07/11/2025      | 09/01/2022 / jaswal     | 07/21/2022 / jaswal         | M5288          |

| Supplier                 | ItemCode / ItemName             | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|---------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58113 / Aluminum (Al) 10,000PPM | 070622 | 07/06/2025      | 09/02/2022 / jaswal     | 07/12/2022 / jaswal         | M5289          |

| Supplier | ItemCode / ItemName                  | Lot #    | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------|--------------------------------------|----------|-----------------|-------------------------|-----------------------------|----------------|
| EPA      | ICV-1 / ICV ( ICP/ICPMS ) STOCK SOLN | ICV-1014 | 01/01/2025      | 12/13/2023 / bin        | 02/20/2020 / bin            | M5294          |

| Supplier           | ItemCode / ItemName      | Lot #        | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------|--------------------------|--------------|-----------------|-------------------------|-----------------------------|----------------|
| Inorganic Ventures | Z9651Q / CHEM-CLP-4/.25L | S2-MEB711673 | 11/02/2026      | 09/19/2022 / jaswal     | 08/20/2022 / jaswal         | M5296          |

## CHEMICAL RECEIPT LOG BOOK

| Supplier                 | ItemCode / ItemName           | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58126 / Fe, 10000 PPM, 500 ml | 020422 | 02/04/2025      | 05/02/2023 / jaswal     | 06/15/2022 / jaswal         | M5298          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57056 / Ba, 1000 PPM, 125 ml | 072122 | 07/21/2025      | 11/01/2022 / jaswal     | 09/18/2022 / jaswal         | M5387          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57056 / Ba, 1000 PPM, 125 ml | 072122 | 07/21/2025      | 04/29/2024 / kareem     | 09/18/2022 / bin            | M5389          |

| Supplier           | ItemCode / ItemName                     | Lot #        | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------|---|--------------|-----------------|-------------------------|-----------------------------|----------------|
| Inorganic Ventures | CLPP-CAL-3 / CLP CAL SOLUTION #3, 125mL | T2-MEB714159 | 01/13/2027      | 01/30/2024 / bin        | 09/19/2022 / bin            | M5395          |

| Supplier                 | ItemCode / ItemName           | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57103 / Li, 10000 PPM, 125 ml | 070622 | 07/06/2025      | 01/30/2023 / bin        | 01/26/2023 / bin            | M5429          |

| Supplier                 | ItemCode / ItemName           | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58112 / Mg, 10000 PPM, 500 ml | 120922 | 12/09/2025      | 03/14/2023 / jaswal     | 03/14/2023 / jaswal         | M5468          |

## CHEMICAL RECEIPT LOG BOOK

| Supplier                 | ItemCode / ItemName           | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57138 / Sr, 10000 PPM, 125 ml | 082922 | 08/29/2025      | 03/16/2023 / jaswal     | 03/16/2023 / jaswal         | M5473          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57028 / Ni, 1000 PPM, 125 ml | 011223 | 01/12/2026      | 01/20/2023 / bin        | 01/19/2023 / bin            | M5494          |

| Supplier                 | ItemCode / ItemName           | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58120 / Ca, 10000 PPM, 500 ml | 031523 | 03/15/2026      | 03/18/2023 / bin        | 03/17/2023 / bin            | M5497          |

| Supplier                 | ItemCode / ItemName           | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58120 / Ca, 10000 PPM, 500 ml | 031523 | 03/15/2026      | 08/15/2023 / jaswal     | 03/17/2023 / bin            | M5498          |

| Supplier                 | ItemCode / ItemName           | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57182 / Pb, 10000 PPM, 125 ml | 061522 | 06/15/2025      | 03/19/2023 / bin        | 03/17/2023 / bin            | M5513          |

| Supplier                    | ItemCode / ItemName                 | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-----------------------------|-------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| PCI Scientific Supply, Inc. | 1403 / Hydrogen Peroxide, 30% 1 gal | 820803 | 08/31/2024      | 01/03/2024 / jaswal     | 08/03/2022 / Al-Terek       | M5632          |

## CHEMICAL RECEIPT LOG BOOK

| Supplier                 | ItemCode / ItemName                    | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|--|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58024 / Chromium, Cr, 500 ml, 1000 PPM | 060523 | 06/05/2026      | 08/28/2023 / jaswal     | 08/25/2023 / jaswal         | M5658          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58029 / Cu, 1000 PPM, 500 ml | 102523 | 10/25/2026      | 04/03/2024 / jaswal     | 10/27/2023 / jaswal         | M5697          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58025 / Mn, 1000 PPM, 500 ml | 102623 | 10/26/2026      | 04/18/2024 / jaswal     | 10/27/2023 / jaswal         | M5698          |

| Supplier                 | ItemCode / ItemName | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|---------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | / Lead (Pb) 1000PPM | 100923 | 10/09/2026      | 05/20/2024 / Jaswal     | 12/20/2023 / jaswal         | M5747          |

| Supplier                 | ItemCode / ItemName                                  | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|--|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 52166 / ICP-AES Spike sample water matrix (18 comp.) | 112823 | 11/28/2026      | 05/01/2024 / jaswal     | 12/15/2023 / jaswal         | M5754          |

| Supplier                 | ItemCode / ItemName           | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58112 / Mg, 10000 PPM, 500 ml | 091823 | 09/18/2026      | 01/08/2024 / bin        | 01/03/2024 / bin            | M5768          |

## CHEMICAL RECEIPT LOG BOOK

| Supplier                 | ItemCode / ItemName           | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|-------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58112 / Mg, 10000 PPM, 500 ml | 091823 | 09/18/2026      | 05/24/2024 / Jaswal     | 01/03/2024 / bin            | M5769          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57004 / Be, 1000 PPM, 125 ml | 102523 | 10/25/2026      | 02/09/2024 / bin        | 02/09/2024 / bin            | M5798          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57050 / Sn, 1000 PPM, 125 ml | 071123 | 07/11/2026      | 02/09/2024 / bin        | 02/09/2024 / bin            | M5799          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57027 / CO, 1000 PPM, 125 ml | 091923 | 09/19/2026      | 02/09/2024 / bin        | 02/09/2024 / bin            | M5800          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57033 / As, 1000 PPM, 125 ml | 111323 | 11/13/2026      | 02/09/2024 / bin        | 02/09/2024 / bin            | M5801          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57115 / P, 10000 PPM, 125 ml | 041723 | 04/17/2026      | 05/21/2024 / Jaswal     | 02/09/2024 / jaswal         | M5815          |

## CHEMICAL RECEIPT LOG BOOK

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57116 / S, 10000 PPM, 125 ml | 071123 | 07/11/2026      | 03/01/2024 / jaswal     | 02/09/2024 / jaswal         | M5817          |

| Supplier                 | ItemCode / ItemName          | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 57014 / Si, 1000 PPM, 125 ml | 122023 | 12/20/2026      | 03/06/2024 / jaswal     | 02/09/2024 / jaswal         | M5818          |

| Supplier                 | ItemCode / ItemName                | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|------------------------------------|--------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | 58030 / Zinc, Zn, 500 ml, 1000 PPM | 111623 | 11/16/2026      | 03/20/2024 / jaswal     | 02/09/2024 / jaswal         | M5819          |

| Supplier           | ItemCode / ItemName                     | Lot #        | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------|---|--------------|-----------------|-------------------------|-----------------------------|----------------|
| Inorganic Ventures | CLPP-CAL-1 / CLP CAL SOLUTION #1, 125mL | T2-MEB714417 | 01/27/2027      | 04/19/2024 / jaswal     | 02/22/2024 / jaswal         | M5875          |

| Supplier         | ItemCode / ItemName   | Lot #  | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|--------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9530-33 / Hydrochloric Acid, Instra-Analyzed (cs/6x2.5L) | 240415 | 11/06/2024      | 06/04/2024 / Al-Terek   | 05/07/2024 / Al-Terek       | M5895          |

| Supplier         | ItemCode / ItemName                                   | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9598-34 / Nitric Acid, Instra-Analyzed (cs/4x2.5L) | 24D1062002 | 11/29/2024      | 05/30/2024 / Al-Terek   | 05/24/2024 / Al-Terek       | M5915          |

## CHEMICAL RECEIPT LOG BOOK

| Supplier         | ItemCode / ItemName                                   | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9598-34 / Nitric Acid, Instra-Analyzed (cs/4x2.5L) | 24D1062002 | 12/08/2024      | 06/21/2024 / Al-Terek   | 06/07/2024 / Al-Terek       | M5935          |

| Supplier         | ItemCode / ItemName                                   | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9598-34 / Nitric Acid, Instra-Analyzed (cs/4x2.5L) | 24D1062002 | 12/20/2024      | 06/21/2024 / Jaswal     | 06/18/2024 / Al-Terek       | M5940          |

| Supplier         | ItemCode / ItemName   | Lot #      | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9530-33 / Hydrochloric Acid, Instra-Analyzed (cs/6x2.5L) | 22G2862015 | 12/27/2024      | 06/27/2024 / Al-Terek   | 06/23/2024 / Al-Terek       | M5947          |

| Supplier         | ItemCode / ItemName | Lot #               | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---------------------|---------------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | DIW / DI Water      | Daily Lab-Certified | 10/24/2024      | 10/24/2019 / apatel     | 10/24/2019 / apatel         | W2606          |





Refine your results. Redefine your industry.

# Certificate of Analysis

300 Technology Drive  
Christiansburg, VA 24073 USA  
inorganicventures.com

P: 800-669-6799/540-585-3030  
F: 540-585-3012  
info@inorganicventures.com

## 1.0 ACCREDITATION / REGISTRATION

**INORGANIC VENTURES** is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



## 2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution  
Catalog Number: CHEM-CLP-4  
Lot Number: S2-MEB711673  
Matrix: 3% (v/v) HNO<sub>3</sub>  
3% (v/v) HF  
Value / Analyte(s): 1 000 µg/mL ea:  
Boron, Molybdenum,  
Silicon, Tin,  
Titanium

## 3.0 CERTIFIED VALUES AND UNCERTAINTIES

| ANALYTE      | CERTIFIED VALUE | ANALYTE        | CERTIFIED VALUE |
|--------------|-----------------|----------------|-----------------|
| Boron, B     | 1 000 ± 6 µg/mL | Molybdenum, Mo | 1 000 ± 6 µg/mL |
| Silicon, Si  | 1 000 ± 7 µg/mL | Tin, Sn        | 1 000 ± 6 µg/mL |
| Titanium, Ti | 1 000 ± 7 µg/mL |                |                 |

**Density:** 1.030 g/mL (measured at 20 ± 4 °C)

### Assay Information:

| ANALYTE | METHOD    | NIST SRM# | SRM LOT# |
|---------|-----------|-----------|----------|
| B       | ICP Assay | 3107      | 110830   |
| Mo      | ICP Assay | 3134      | 130418   |
| Si      | ICP Assay | 3150      | 130912   |
| Sn      | ICP Assay | 3161a     | 140917   |
| Ti      | ICP Assay | 3162a     | 130925   |

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

#### Characterization of CRM/RM by Two or More Methods

Certified Value,  $X_{\text{CRM/RM}}$ , where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum(w_i)(X_i)$$

$X_i$  = mean of Assay Method  $i$  with standard uncertainty  $u_{\text{char } i}$

$w_i$  = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum(1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

$k$  = coverage factor = 2

$u_{\text{char}} = [\sum(w_i)^2(u_{\text{char } i}^2)]^{1/2}$  where  $u_{\text{char } i}$  are the errors from each characterization method

$u_{\text{bb}}$  = bottle to bottle homogeneity standard uncertainty

$u_{\text{Its}}$  = long term stability standard uncertainty (storage)

$u_{\text{ts}}$  = transport stability standard uncertainty

#### Characterization of CRM/RM by One Method

Certified Value,  $X_{\text{CRM/RM}}$ , where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a)(u_{\text{char } a})$$

$X_a$  = mean of Assay Method A with

$u_{\text{char } a}$  = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

$k$  = coverage factor = 2

$u_{\text{char } a}$  = the errors from characterization

$u_{\text{bb}}$  = bottle to bottle homogeneity standard uncertainty

$u_{\text{Its}}$  = long term stability standard uncertainty (storage)

$u_{\text{ts}}$  = transport stability standard uncertainty

## 4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

### 4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

### 4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

### 4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

## 5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

## 6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

## 7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

### 7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit [www.inorganicventures.com/TCT](http://www.inorganicventures.com/TCT)

**HF Note:** This standard should not be prepared or stored in glass.

## 8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

## 9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

## 10.0 QUALITY STANDARD DOCUMENTATION

### 10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

### 10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

### 10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; [inorganicventures.com](http://inorganicventures.com); [info@inorganicventures.com](mailto:info@inorganicventures.com)

## 11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

### 11.1 Certification Issue Date

November 02, 2021

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

### 11.2 Lot Expiration Date

- **November 02, 2026**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

### 11.3 Period of Validity

- Sealed TCT Bag Open Date: \_\_\_\_\_

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

## 12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

### Certificate Approved By:

Michael Booth  
Director, Quality Control



### Certifying Officer:

Paul Gaines  
Chairman / Senior Technical Director





Refine your results. Redefine your industry.

# Certificate of Analysis

300 Technology Drive  
Christiansburg, VA 24073 USA  
inorganicventures.com

P: 800-669-6799/540-585-3030  
F: 540-585-3012  
info@inorganicventures.com

## 1.0 ACCREDITATION / REGISTRATION

**INORGANIC VENTURES** is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



## 2.0 PRODUCT DESCRIPTION

|                     |                                     |                       |
|---------------------|-------------------------------------|-----------------------|
| Product Code:       | Multi Analyte Custom Grade Solution |                       |
| Catalog Number:     | CLPP-CAL-1                          |                       |
| Lot Number:         | T2-MEB714417                        |                       |
| Matrix:             | 5% (v/v) HNO <sub>3</sub>           |                       |
| Value / Analyte(s): | 5 000 µg/mL ea:                     | Potassium,<br>Sodium, |
|                     | Calcium,<br>Magnesium,              |                       |
|                     | 2 000 µg/mL ea:                     | Barium,               |
|                     | Aluminum,                           |                       |
|                     | 1 000 µg/mL ea:                     |                       |
|                     | Iron,                               |                       |
|                     | 500 µg/mL ea:                       | Vanadium,<br>Cobalt,  |
|                     | Nickel,                             |                       |
|                     | Zinc,                               |                       |
|                     | Manganese,                          |                       |
|                     | 250 µg/mL ea:                       | Copper,               |
|                     | Silver,                             |                       |
|                     | 200 µg/mL ea:                       |                       |
|                     | Chromium,                           |                       |
|                     | 50 µg/mL ea:                        |                       |
|                     | Beryllium                           |                       |

## 3.0 CERTIFIED VALUES AND UNCERTAINTIES

|                |                        |                |                        |
|----------------|------------------------|----------------|------------------------|
| <b>ANALYTE</b> | <b>CERTIFIED VALUE</b> | <b>ANALYTE</b> | <b>CERTIFIED VALUE</b> |
| Aluminum, Al   | 2 000 ± 7 µg/mL        | Barium, Ba     | 2 000 ± 9 µg/mL        |
| Beryllium, Be  | 50.00 ± 0.26 µg/mL     | Calcium, Ca    | 5 000 ± 22 µg/mL       |
| Chromium, Cr   | 200.0 ± 1.0 µg/mL      | Cobalt, Co     | 500.0 ± 2.4 µg/mL      |
| Copper, Cu     | 250.0 ± 1.0 µg/mL      | Iron, Fe       | 1 000 ± 4 µg/mL        |
| Magnesium, Mg  | 5 000 ± 20 µg/mL       | Manganese, Mn  | 500.0 ± 2.0 µg/mL      |
| Nickel, Ni     | 500.0 ± 2.2 µg/mL      | Potassium, K   | 5 000 ± 19 µg/mL       |
| Silver, Ag     | 250.0 ± 1.1 µg/mL      | Sodium, Na     | 5 000 ± 18 µg/mL       |
| Vanadium, V    | 499.7 ± 2.2 µg/mL      | Zinc, Zn       | 500.0 ± 2.2 µg/mL      |

**Density:** 1.118 g/mL (measured at 20 ± 4 °C)

**Assay Information:**

| <b>ANALYTE</b> | <b>METHOD</b> | <b>NIST SRM#</b> | <b>SRM LOT#</b> |
|----------------|---------------|------------------|-----------------|
| Ag             | ICP Assay     | 3151             | 160729          |
| Ag             | Volhard       | 999c             | 999c            |
| Al             | ICP Assay     | 3101a            | 140903          |
| Al             | EDTA          | 928              | 928             |
| Ba             | ICP Assay     | 3104a            | 140909          |
| Ba             | Gravimetric   |                  | See Sec. 4.2    |
| Be             | ICP Assay     | 3105a            | 090514          |
| Be             | Calculated    |                  | See Sec. 4.2    |
| Ca             | ICP Assay     | 3109a            | 130213          |
| Ca             | EDTA          | 928              | 928             |
| Co             | ICP Assay     | 3113             | 190630          |
| Co             | EDTA          | 928              | 928             |
| Cr             | ICP Assay     | 3112a            | 170630          |
| Cr             | Calculated    |                  | See Sec. 4.2    |
| Cu             | ICP Assay     | 3114             | 121207          |
| Cu             | EDTA          | 928              | 928             |
| Fe             | ICP Assay     | 3126a            | 140812          |
| Fe             | EDTA          | 928              | 928             |
| K              | ICP Assay     | 3141a            | 140813          |
| K              | Gravimetric   |                  | See Sec. 4.2    |
| Mg             | ICP Assay     | 3131a            | 140110          |
| Mg             | EDTA          | 928              | 928             |
| Mn             | ICP Assay     | 3132             | 050429          |
| Mn             | EDTA          | 928              | 928             |
| Na             | ICP Assay     | 3152a            | 120715          |
| Na             | Gravimetric   |                  | See Sec. 4.2    |
| Ni             | ICP Assay     | 3136             | 120619          |
| Ni             | EDTA          | 928              | 928             |
| V              | IC Assay      | 3165             | 160906          |
| V              | EDTA          | 928              | 928             |
| Zn             | ICP Assay     | 3168a            | 120629          |
| Zn             | EDTA          | 928              | 928             |

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

#### Characterization of CRM/RM by Two or More Methods

Certified Value,  $X_{\text{CRM/RM}}$ , where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum(w_i)(X_i)$$

$X_i$  = mean of Assay Method  $i$  with standard uncertainty  $u_{\text{char } i}$

$w_i$  = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum(1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

$k$  = coverage factor = 2

$u_{\text{char}} = [\sum(w_i)^2 (u_{\text{char } i})^2]^{1/2}$  where  $u_{\text{char } i}$  are the errors from each characterization method

$u_{\text{bb}}$  = bottle to bottle homogeneity standard uncertainty

$u_{\text{Its}}$  = long term stability standard uncertainty (storage)

$u_{\text{ts}}$  = transport stability standard uncertainty

#### Characterization of CRM/RM by One Method

Certified Value,  $X_{\text{CRM/RM}}$ , where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a)(u_{\text{char } a})$$

$X_a$  = mean of Assay Method A with

$u_{\text{char } a}$  = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

$k$  = coverage factor = 2

$u_{\text{char } a}$  = the errors from characterization

$u_{\text{bb}}$  = bottle to bottle homogeneity standard uncertainty

$u_{\text{Its}}$  = long term stability standard uncertainty (storage)

$u_{\text{ts}}$  = transport stability standard uncertainty

## 4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

### 4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

### 4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

### 4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

## 5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

## 6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

## 7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

### 7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit [www.inorganicventures.com/TCT](http://www.inorganicventures.com/TCT)

**Note:** This solution contains Silver (Ag), please refer to our Sample Preparation Guide for more information.

<https://www.inorganicventures.com/sample-preparation-guide/samples-containing-silver>

## 8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

## 9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

## 10.0 QUALITY STANDARD DOCUMENTATION

### 10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

### 10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

### 10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

## 11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

### 11.1 Certification Issue Date

January 27, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

### 11.2 Lot Expiration Date

- **January 27, 2027**

- The date after which this CRM/RM should not be used.
- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

### 11.3 Period of Validity

- Sealed TCT Bag Open Date: \_\_\_\_\_

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

## 12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

### Certificate Approved By:

Thomas Kozikowski  
Manager, Quality Control



### Certifying Officer:

Paul Gaines  
Chairman / Senior Technical Director





Refine your results. Redefine your industry.

# Certificate of Analysis

300 Technology Drive  
Christiansburg, VA 24073 USA  
inorganicventures.com

P: 800-669-6799/540-585-3030  
F: 540-585-3012  
info@inorganicventures.com

## 1.0 ACCREDITATION / REGISTRATION

**INORGANIC VENTURES** is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



## 2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution  
Catalog Number: CLPP-CAL-3  
Lot Number: T2-MEB714159  
Matrix: 7% (v/v) HNO<sub>3</sub>  
Value / Analyte(s):  
1 000 µg/mL ea:  
Arsenic, Lead,  
Selenium, Thallium,  
500 µg/mL ea:  
Cadmium

## 3.0 CERTIFIED VALUES AND UNCERTAINTIES

| ANALYTE      | CERTIFIED VALUE | ANALYTE      | CERTIFIED VALUE   |
|--------------|-----------------|--------------|-------------------|
| Arsenic, As  | 1 000 ± 8 µg/mL | Cadmium, Cd  | 500.0 ± 2.1 µg/mL |
| Lead, Pb     | 1 000 ± 5 µg/mL | Selenium, Se | 1 000 ± 8 µg/mL   |
| Thallium, Tl | 1 000 ± 7 µg/mL |              |                   |

Density: 1.043 g/mL (measured at 20 ± 4 °C)

### Assay Information:

| ANALYTE | METHOD    | NIST SRM# | SRM LOT# |
|---------|-----------|-----------|----------|
| As      | ICP Assay | 3103a     | 100818   |
| Cd      | ICP Assay | 3108      | 130116   |
| Cd      | EDTA      | 928       | 928      |
| Pb      | ICP Assay | 3128      | 101026   |
| Pb      | EDTA      | 928       | 928      |
| Se      | ICP Assay | 3149      | 100901   |
| Tl      | ICP Assay | 3158      | 151215   |

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.



#### Characterization of CRM/RM by Two or More Methods

Certified Value,  $X_{\text{CRM/RM}}$ , where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum(w_i)(X_i)$$

$X_i$  = mean of Assay Method  $i$  with standard uncertainty  $u_{\text{char } i}$

$w_i$  = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum(1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

$k$  = coverage factor = 2

$u_{\text{char}} = [\sum(w_i)^2 (u_{\text{char } i}^2)]^{1/2}$  where  $u_{\text{char } i}$  are the errors from each characterization method

$u_{\text{bb}}$  = bottle to bottle homogeneity standard uncertainty

$u_{\text{Its}}$  = long term stability standard uncertainty (storage)

$u_{\text{ts}}$  = transport stability standard uncertainty

#### Characterization of CRM/RM by One Method

Certified Value,  $X_{\text{CRM/RM}}$ , where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a)(u_{\text{char } a})$$

$X_a$  = mean of Assay Method A with

$u_{\text{char } a}$  = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

$k$  = coverage factor = 2

$u_{\text{char } a}$  = the errors from characterization

$u_{\text{bb}}$  = bottle to bottle homogeneity standard uncertainty

$u_{\text{Its}}$  = long term stability standard uncertainty (storage)

$u_{\text{ts}}$  = transport stability standard uncertainty

## 4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

### 4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

### 4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

### 4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

## 5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

## 6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

## 7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

### 7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit [www.inorganicventures.com/TCT](http://www.inorganicventures.com/TCT)

## 8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

## 9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

## 10.0 QUALITY STANDARD DOCUMENTATION

### 10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

### 10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

### 10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

## 11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

### 11.1 Certification Issue Date

January 13, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

### 11.2 Lot Expiration Date

- **January 13, 2027**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

### 11.3 Period of Validity

- Sealed TCT Bag Open Date: \_\_\_\_\_

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

## 12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

### Certificate Approved By:

Thomas Kozikowski  
Manager, Quality Control



### Certifying Officer:

Paul Gaines  
Chairman / Senior Technical Director





**CERTIFIED WEIGHT REPORT:**

**Part Number:** 57048  
**Lot Number:** 072821  
**Description:** Cadmium (Cd)

**Lot #** 20370011  
**Solvent:** Nitric Acid

**Expiration Date:** 072824  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** **1000**

2.0% 40.0 (mL) Nitric Acid

**NIST Test Number:** 6UTB

5E-05 Balance Uncertainty


**Volume shown below was diluted to (mL):** 2000.02 0.058 Flask Uncertainty

|                          |                   |
|--------------------------|-------------------|
| <i>Giovanni Esposito</i> |                   |
| Formulated By:           | Giovanni Esposito |
|                          | 072821            |
| <i>Pedro L. Rendas</i>   |                   |
| Reviewed By:             | Pedro L. Rendas   |
|                          | 072821            |

**SDS Information**

| Compound | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | (Solvent Safety Info. On Attached pg.) CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|---|----------------|------|----------|
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|---|----------------|------|----------|

1. Cadmium nitrate tetrahydrate (Cd) 58148 010920 0.1000 200.0 0.084 1000 10000.5 **1000.0** **2.2** 10022-68-1 0.2 mg/m3 or-Irat 300 mg/kg 3108

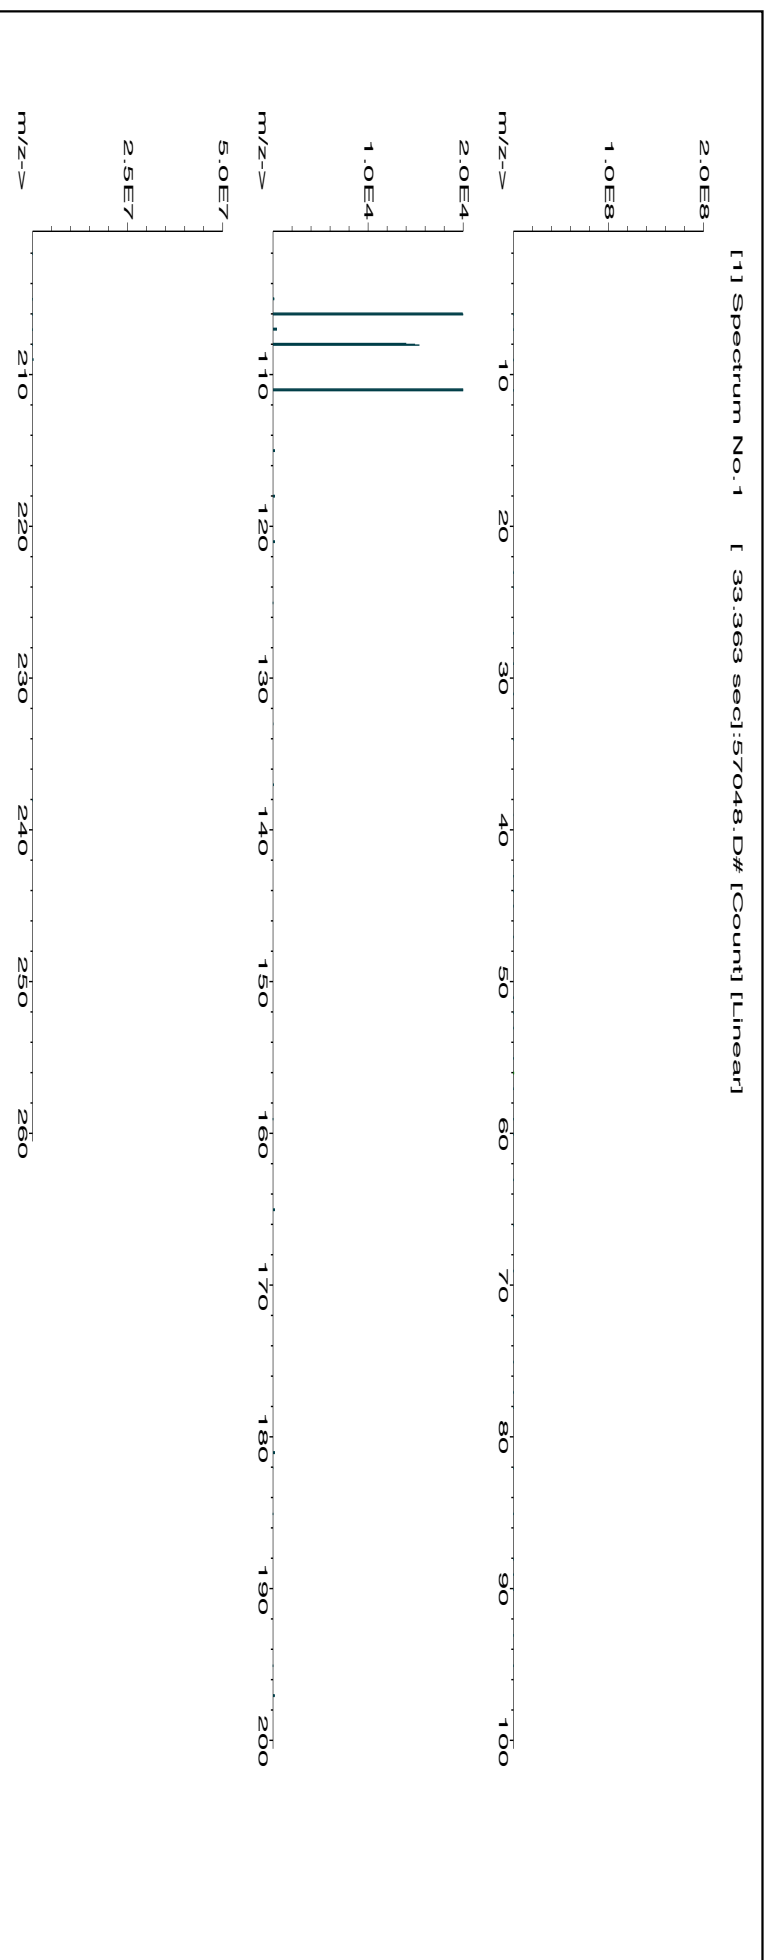



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

| Trace Metals Verification by ICP-MS (µg/mL) |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|---|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al  | <0.02 | Cd | T     | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  |
| Sb  | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 |
| As  | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 |
| Ba  | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  |
| Be  | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 |
| Bi  | <0.02 | Co | <0.02 | Ce | <0.02 | Pb | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 |
| B   | <0.02 | Cu | <0.02 | Au | <0.02 | La | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | Tb | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | Te | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | Tl | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | Th | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | Tm | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | Sn | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | Ti | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | U  | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | V  | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | Yb | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | Y  | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | Zn | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**CERTIFIED WEIGHT REPORT:**

**Part Number:** 57034  
**Lot Number:** 070221  
**Description:** Selenium (Se)


**Lot #** 20370011  
**Solvent:** Nitric Acid

**Expiration Date:** 070224  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** 1000  
**NIST Test Number:** 6UTB  
**Volume shown below was diluted to (mL):** 2000.02  
**Balance Uncertainty:** 5E-05  
**Flask Uncertainty:** 0.058

|                   |                   |
|-------------------|-------------------|
| Giovanni Caporaso |                   |
| Formulated By:    | Giovanni Esposito |
|                   | 070221            |
| Reviewed By:      | Pedro L. Rentas   |
|                   | 070221            |

| Compound |  | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|--|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|
|----------|--|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|

1. Selenium(IV) oxide (Se) 58134 021621 0.1000 200.0 0.084 1000 10000.2 1000.0 2.2 7446-08-4 0.2 mg/m3 or-rat 68 mg/kg 3149

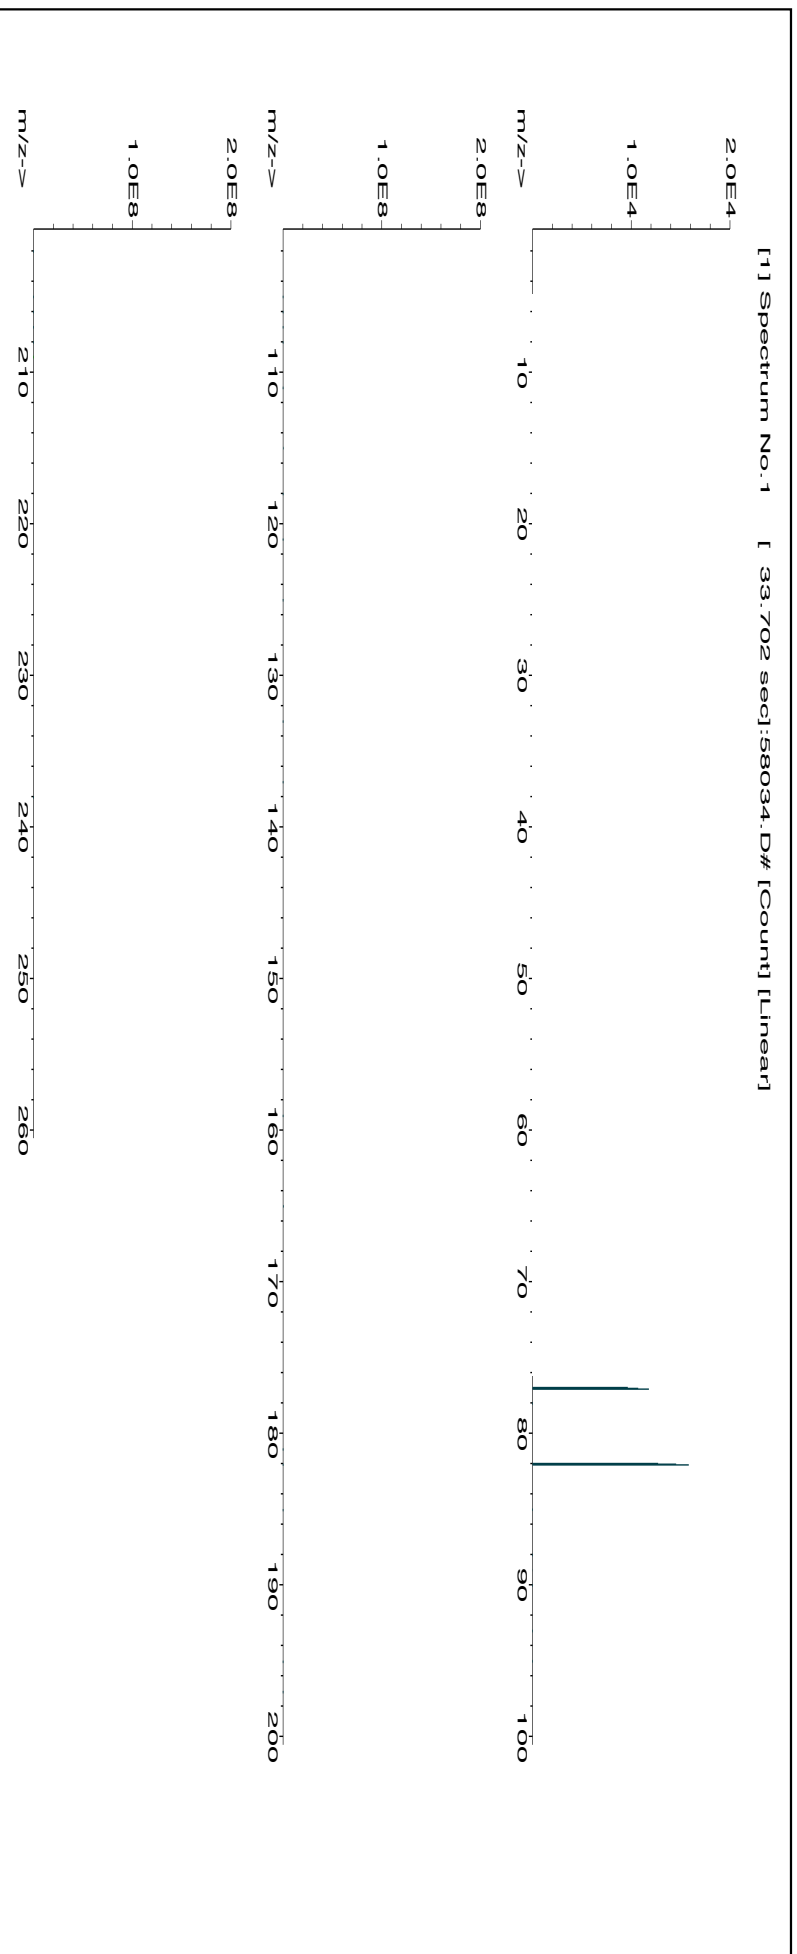



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

| Trace Metals Verification by ICP-MS (µg/mL) |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |    |
|---|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|----|
| Al  | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | T     | Tb | W  |
| Sb  | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | Ti    | Te | U  |
| As  | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | V  |
| Ba  | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | Yb |
| Be  | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | Y  |
| Bi  | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | Zn |
| B   | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Tl | Zr |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

**Certified by:**

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**Certified Reference Material CRM**



**CERTIFIED WEIGHT REPORT:**

**Part Number:** 57047  
**Lot Number:** 072921  
**Description:** Silver (Ag)


**Lot #** 20370011  
**Solvent:** Nitric Acid

**Expiration Date:** 072924  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** **1000**  
**NIST Test Number:** 6UTB  
**Volume shown below was diluted to (mL):** 2000.02  
**Balance Uncertainty:** 5E-05  
**Flask Uncertainty:** 0.058

|                          |                   |
|--------------------------|-------------------|
| <i>Giovanni Esposito</i> |                   |
| Formulated By:           | Giovanni Esposito |
|                          | 072921            |
| <i>Pedro L. Rendas</i>   |                   |
| Reviewed By:             | Pedro L. Rendas   |
|                          | 072921            |

| Compound |  | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|--|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|
|----------|--|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|

1. Silver nitrate (Ag) 58147 010820 0.1000 200.0 0.084 1000 10000.4 1000.0 2.2 7761-88-8 10 µg/m3 N/A 3151

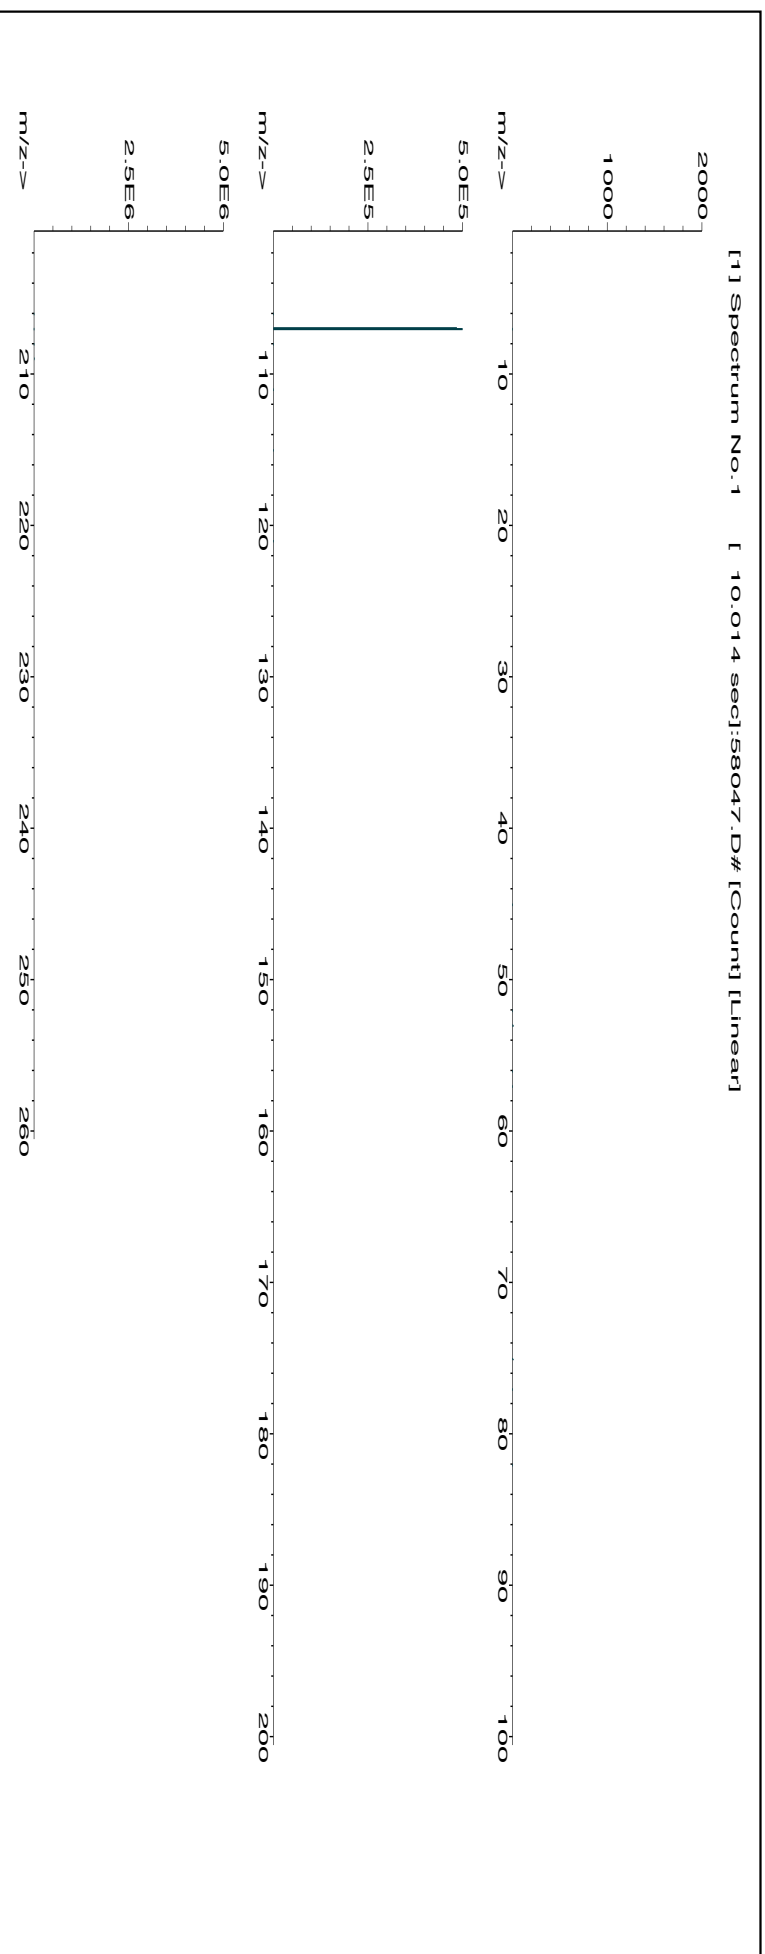



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | T     | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pr | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

**Certified by:**

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).





**CERTIFIED WEIGHT REPORT:**

**Part Number:** 57022  
**Lot Number:** 070721  
**Description:** Titanium (Ti)

**Lot #** 20370011  
**Solvent:** Nitric Acid

**Expiration Date:** 070724

**2.0%** 40.0 (mL) Nitric Acid

**Recommended Storage:** Ambient (20 °C)

**Nominal Concentration (µg/mL):** 1000

**NIST Test Number:** 6UTB

**5E-05** Balance Uncertainty


**Volume shown below was diluted to (mL):** 2000.02 0.058 Flask Uncertainty

|                |                 |
|----------------|-----------------|
|                |                 |
| Formulated By: | Lawrence Barry  |
|                | 070721          |
|                |                 |
| Reviewed By:   | Pedro L. Renias |
|                | 070721          |

**SDS Information**

| Compound | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|-------------|------------|-----------------|-------------------|---------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|
|----------|-------------|------------|-----------------|-------------------|---------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|

1. Ammonium hexafluorotitanate (Ti) 58122 070120 0.1000 200.0 0.084 1000 10000.1 1000.0 2.2 16962-40-6 2.5 (F) mg/m3 NA 3162a

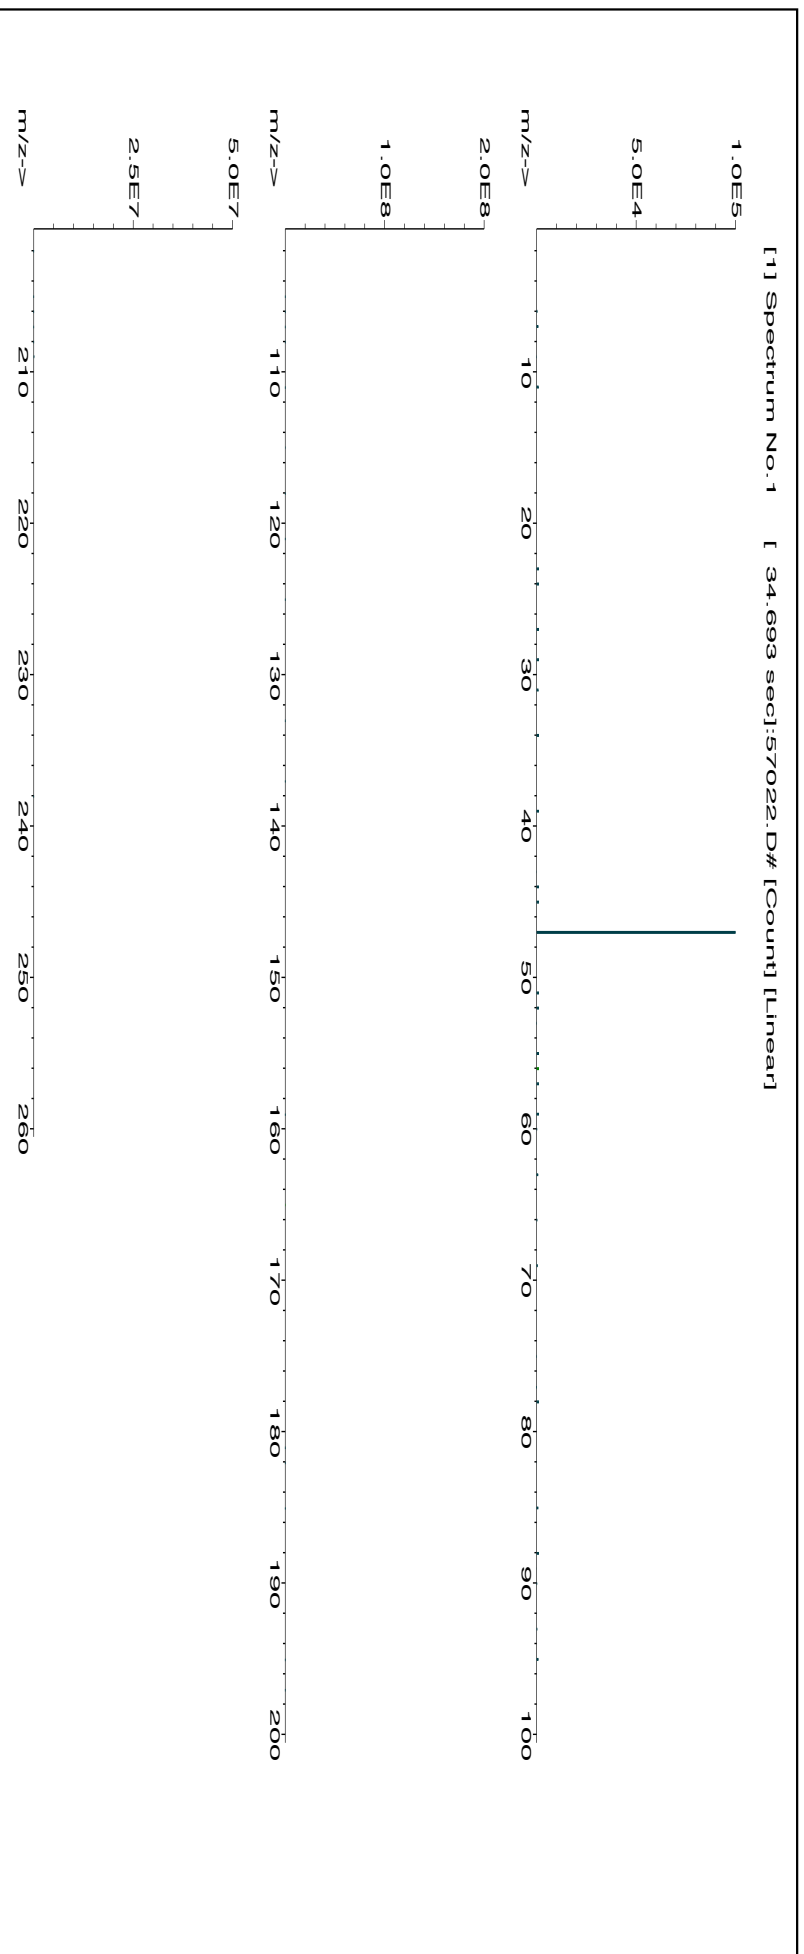



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | T     | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

**Certified by:**

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**CERTIFIED WEIGHT REPORT:**

**Part Number:** 57081  
**Lot Number:** 073021  
**Description:** Thallium (TI)

**Lot #** 20370011  
**Solvent:** Nitric Acid

**Expiration Date:** 073024

2.0%

40.0 (mL)  
Nitric Acid

**Recommended Storage:** Ambient (20 °C)

**Nominal Concentration (µg/mL):** 1000

**NIST Test Number:** 6UTB

5E-05 Balance Uncertainty

**Volume shown below was diluted to (mL):** 2000.02


0.058 Flask Uncertainty

|                          |                   |
|--------------------------|-------------------|
| <i>Giovanni Esposito</i> |                   |
| Formulated By:           | Giovanni Esposito |
|                          | 073021            |
| <i>Pedro L. Rendas</i>   |                   |
| Reviewed By:             | Pedro L. Rendas   |
|                          | 073021            |

**SDS Information**

| Compound | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|

1. Thallium (TI) 58181 060920 0.1000 200.0 0.084 1000 10001.0 1000.0 2.2 7440-28-0 0.1 mg/m3 or-rat 6700 mg/kg 3158

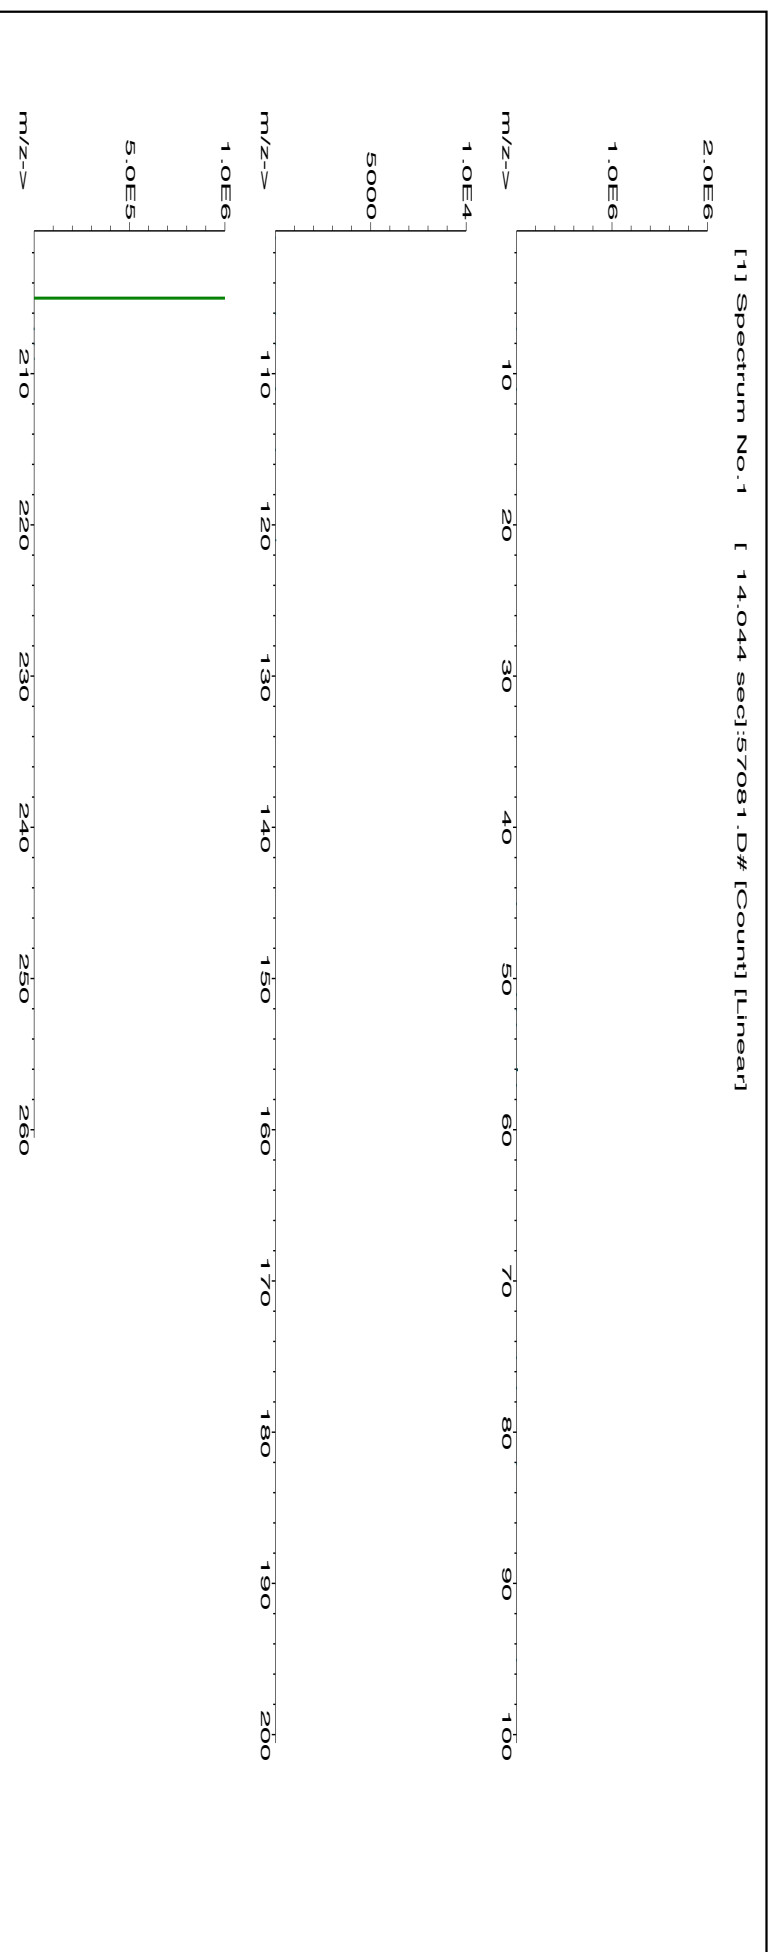





**Certified Reference Material CRM**



**CERTIFIED WEIGHT REPORT:**

**Part Number:** 58149  
**Lot Number:** 100721  
**Description:** Indium (In)

**Solvent:** 20370011 Nitric Acid

**Lot #**

**Expiration Date:** 100724

**Recommended Storage:** Ambient (20 °C)

**Nominal Concentration (µg/mL):** 10000

**NIST Test Number:** 6UTB

**Weight shown below was diluted to (mL):** 500.06 0.058 Flask Uncertainty


**5% 25.0 (mL) Nitric Acid**


|                   |                   |
|-------------------|-------------------|
| Giovanni Caporaso |                   |
| Formulated By:    | Giovanni Esposito |
| Reviewed By:      | Pedro L. Renteria |
|                   | 100721            |

| Compound | RM# | Lot Number | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | SDS Information (Solvent Safety Info. On Attached pg.) | LD50 | NIST SRM |
|----------|-----|------------|-----------------------|------------|-----------------|-----------|-------------------|-------------------|----------------------|----------------------------------|------|----------------|--|------|----------|
|          |     |            |                       |            |                 |           |                   |                   |                      |                                  |      |                |  |      |          |

1. Indium Oxide (In) IN086 W1096A 10000 99.999 0.10 82.6 6.05408 6.05441 10000.6 20.1 1312-43-2 NA NA 3124a

[1] Spectrum No. 1 [ 12.965 sec]:57049.D# [Count] [Linear]

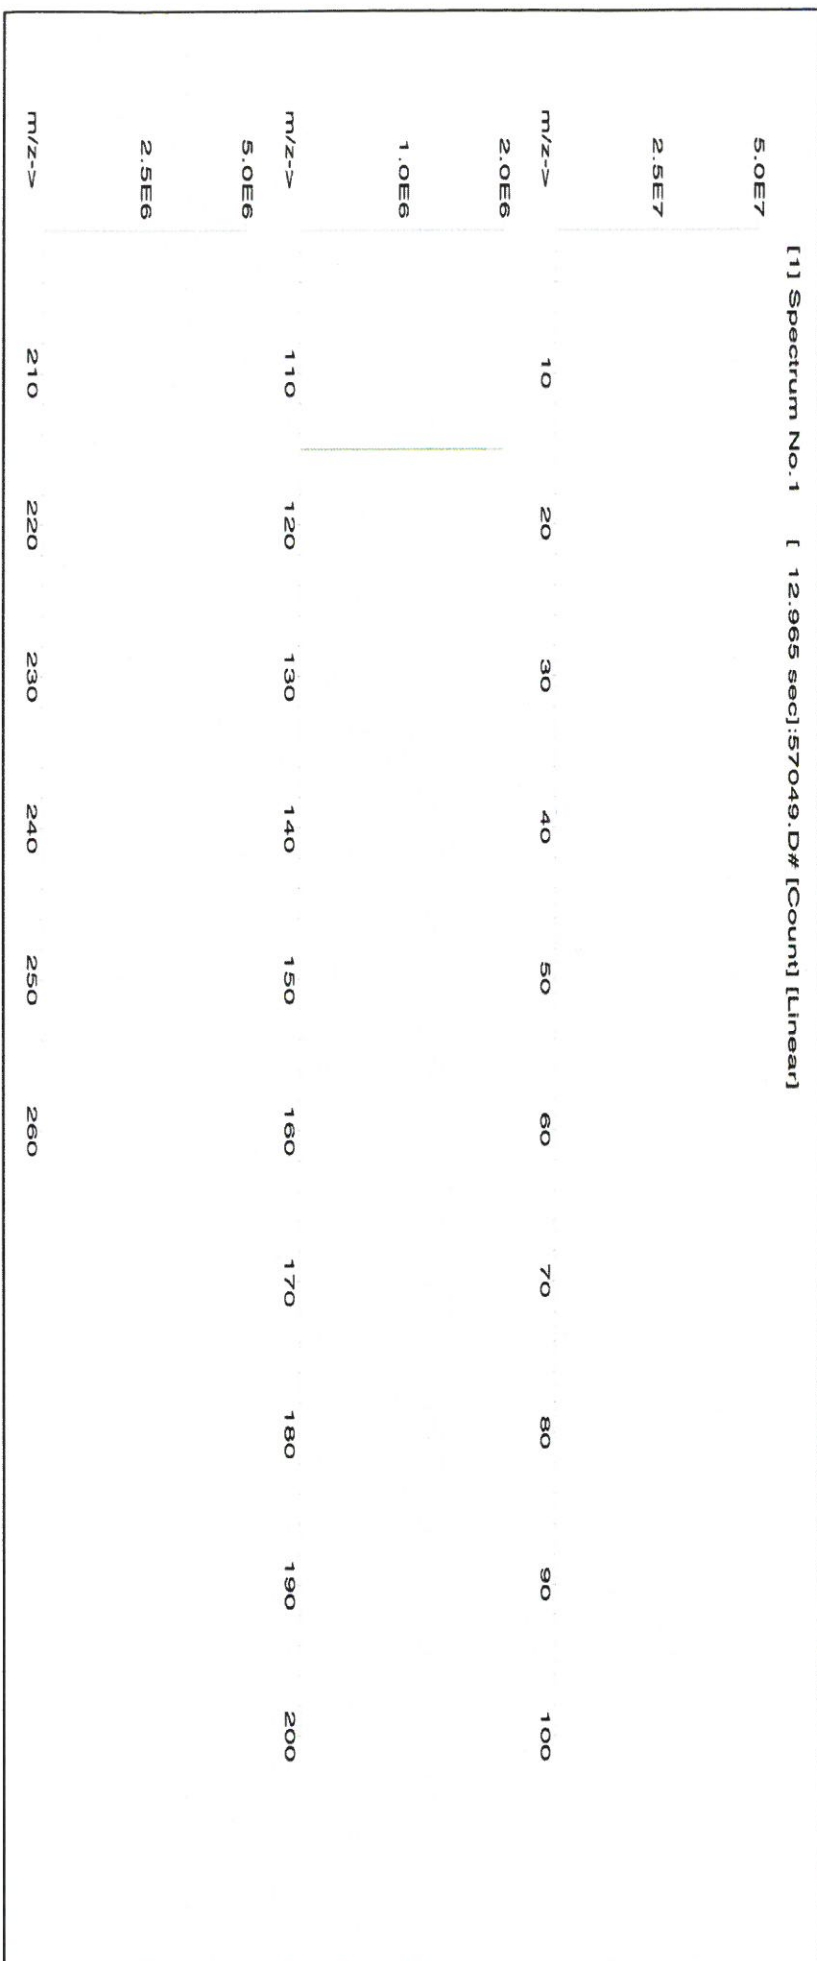



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | T     | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

**Certified by:**

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).





*M4961*  
**Certified Reference Material CRM**  
R: 10/08/21 *(B)*



**CERTIFIED WEIGHT REPORT:**

**Part Number:** 58139  
**Lot Number:** 052521  
**Description:** Yttrium (Y)

**Solvent:** 20370011 Nitric Acid

**Lot #**

**Expiration Date:** 052524  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** 10000  
**NIST Test Number:** 6UTB  
**Weight shown below was diluted to (mL):** 2000.02  
**5E-05 Balance Uncertainty**  
**0.058 Flask Uncertainty**


|                       |                        |
|-----------------------|------------------------|
| <i>Lawrence Barry</i> |                        |
| Formulated By:        | Lawrence Barry         |
| Reviewed By:          | <i>Pedro L. Rentas</i> |
|                       | 052521                 |


**Compound**

1. Yttrium (III) Oxide (Y) IN087 YV012015B1 10000 99.999 0.10 77.9 25.6744 25.6745 10000.0 20.0 1314-36-9 NA NA

**SDS Information**  
Expanded Uncertainty (Solvent Safety Info. On Attached pg.)  
CAS# OSHA PEL (TWA) LD50 SRM

[1] Spectrum No. 1 [ 12.624 sec]:58139.D# [Count] [Linear]

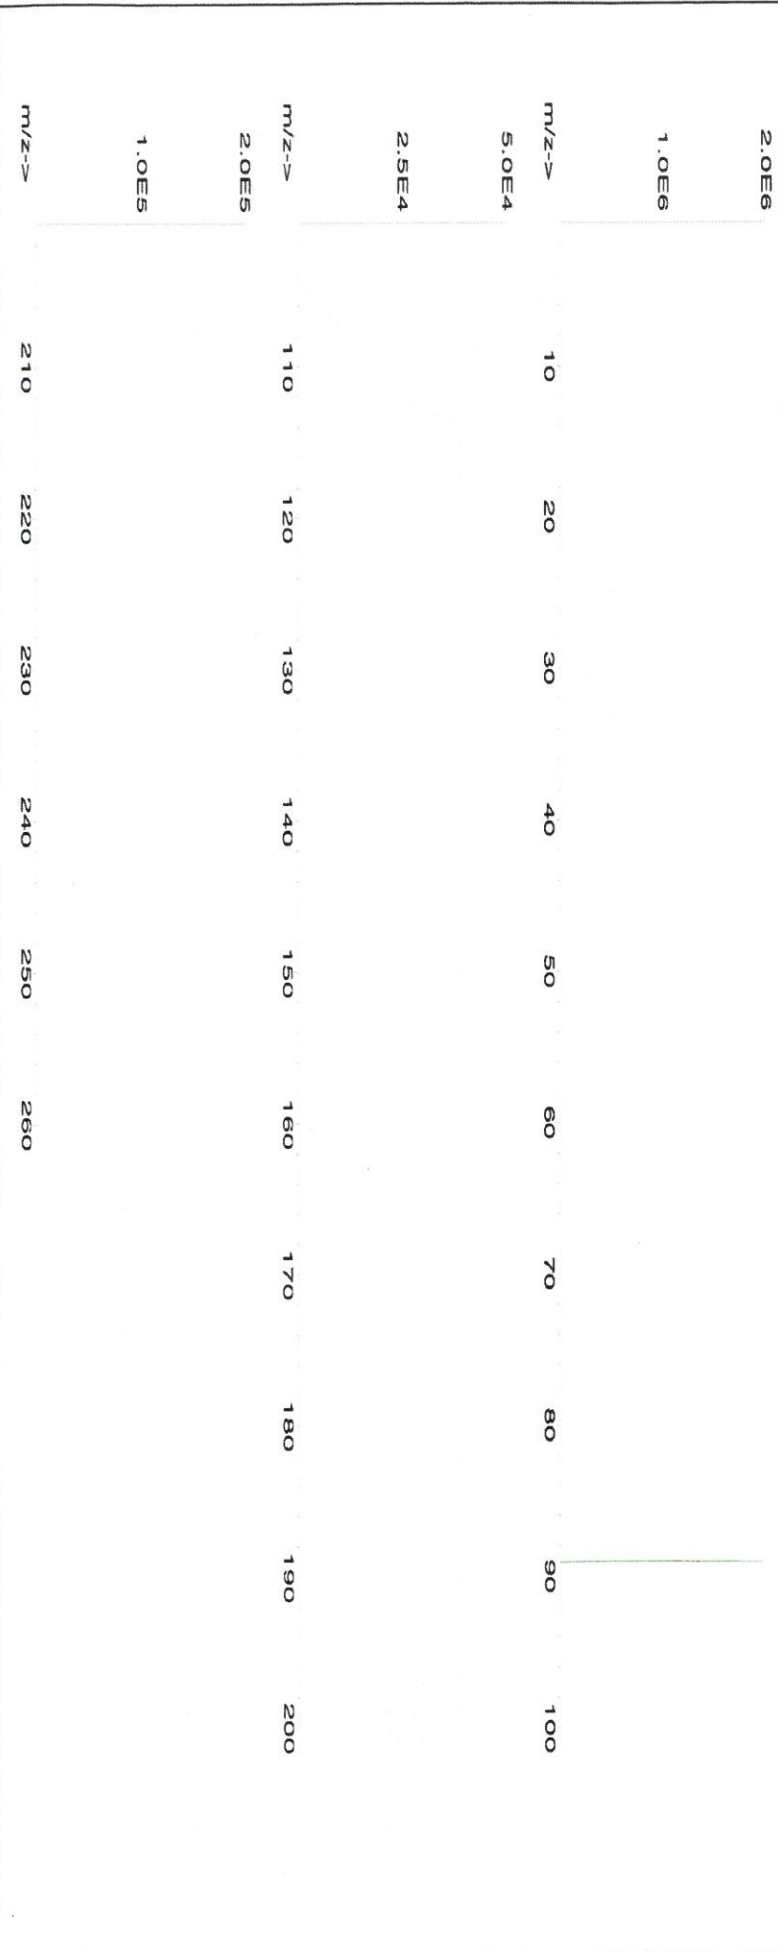



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hi | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Mg | <0.01 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mn | <0.02 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Ti | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Hg | <0.2  | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Mo | <0.02 | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Nd | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 |    |       | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**QATS LABORATORY INORGANIC REFERENCE MATERIAL  
INTERFERENCE CHECK SAMPLE SET FOR ICP-AES (ICSA WITH ICSB)**

**NOTE:** These instructions are for advisory purposes only. If any apparent conflict exists between these instructions and the analytical protocol or your contract, disregard these instructions.

**APPLICATION:** For use with the CLP SFAM01.0 SOW and revisions.

**CAUTION:** Read instructions carefully before opening bottle(s) and proceeding with the analyses.

Contains Heavy Metals  
**HAZARDOUS MATERIAL**

Safety Data Sheets  
Available Upon Request

**(A) SAMPLE DESCRIPTION**

Enclosed is a set of one (1) or more bottles of Aqueous Reference Material, each composed of metals at various concentrations and prepared with nitrate salts and oxy-acids of the respective elements in a 5% nitric acid matrix. **For the reference material source in reporting ICSA and ICSAB mixture use "USEPA". For the reference material lot number for the ICSA use "ICSA-1211" and for the ICSAB mixture use "ICSA-1211+ICSB-0710".**

**CAUTION:** The bottle(s) should be protected from light during storage to ensure the stability of silver which is contained in the ICSB solution. The bottle(s) should be stored at room temperature. **Do not allow the solution(s) to freeze.**

**(B) BREAKAGE OR MISSING ITEMS**

Check the contents of the shipment carefully for any broken, leaking, or missing items. Check that the seal is intact on each bottle. Refer to the enclosed chain of custody record. Report any problems to Mr. Keith Strout, APTIM Federal Services, LLC, at (702) 895-8722. If requested, return the chain-of-custody record with appropriate annotations and signatures to the address provided below.

**QUALITY ASSURANCE TECHNICAL SUPPORT LABORATORY  
APTIM Federal Services, LLC  
2700 Chandler Avenue - Building C  
Las Vegas, NV 89120**

**(C) ANALYSIS OF SAMPLES**

The interference check sample set is to be used to verify inter-element and background correction factors of inductively-coupled plasma (ICP) spectrometers. This reference material set consists of two (2) concentrated solutions. The ICSA solution contains the four (4) interferent elements: Al, Ca, Fe, and Mg. The ICSB solution contains the analytes: Ag, As, Sb, Ba, Be,



Instructions for QATS Reference Material: **ICP-AES ICS**

Cd, Co, Cr, Cu, Mn, Ni, Pb, Tl, Se, V, and Zn. This instruction sheet provides the nominal values for ICP-AES Part A and Part B target analytes when diluted as directed.

Using Class "A" glassware, preparation and analysis must be performed according to the following instructions:

**ICSA-1211, Interferents:** Pipet 10 mL of the ICSA solution into a 100 mL volumetric flask and dilute to volume with 2% v/v HNO<sub>3</sub>. Analyze this ICSA solution by ICP-AES.

**ICSB-0710, Analytes, mixed with ICSA-1211, Interferents:** Pipet 10 mL of the ICSA solution and 10 mL of the ICSB solution into a 100 mL volumetric flask and dilute to volume with 2% v/v HNO<sub>3</sub>. Analyze this ICSAB solution by ICP-AES.

**(D) "CERTIFIED VALUE" CONCENTRATIONS OF QATS ICP-AES ICS SOLUTION(S)**

The "Certified Value" concentrations of the elements, listed in Table 1 below, were derived from statistically pooled analysis results from the following sources, if available: QATS Laboratory, CLP laboratories, Quarterly Blind (QB)/Proficiency Testing (PT) events, CLP pre-award events, and external referee laboratories.


**Table 1. "CERTIFIED VALUES" FOR INTERFERENCE CHECK SAMPLE ICP-AES ICSA-1211, AND ICSA-1211 MIXED WITH ICSB-0710**

| Element | CRQL | Part A (µg/L) | Low Limit (µg/L) | High Limit (µg/L) | Part A +Part B (µg/L) | Low Limit (µg/L) | High Limit (µg/L) |
|---------|------|---------------|------------------|-------------------|-----------------------|------------------|-------------------|
| Al      | 200  | 255000        | 216000           | 294000            | 247000                | 209000           | 285000            |
| Sb      | 60   | (0.0)         | -60.0            | 60.0              | 618                   | 525              | 711               |
| As      | 10   | (0.0)         | -10.0            | 10.0              | 104                   | 88.4             | 120               |
| Ba      | 200  | (6.0)         | -194             | 206               | (537)                 | 337              | 737               |
| Be      | 5.0  | (0.0)         | -5.0             | 5.0               | 495                   | 420              | 570               |
| Cd      | 5.0  | (1.0)         | -4.0             | 6.0               | 972                   | 826              | 1120              |
| Ca      | 5000 | 245000        | 208000           | 282000            | 235000                | 199000           | 271000            |
| Cr      | 10   | (52.0)        | 42.0             | 62.0              | 542                   | 460              | 624               |
| Co      | 50   | (0.0)         | -50.0            | 50.0              | 476                   | 404              | 548               |
| Cu      | 25   | (2.0)         | -23.0            | 27.0              | 511                   | 434              | 588               |
| Fe      | 100  | 101000        | 85600            | 116500            | 99300                 | 84400            | 114500            |
| Pb      | 10   | (0.0)         | -10.0            | 10.0              | (49.0)                | 39.0             | 59.0              |
| Mg      | 5000 | 255000        | 216000           | 294000            | 248000                | 210000           | 286000            |
| Mn      | 15   | (7.0)         | -8.0             | 22.0              | 507                   | 430              | 584               |
| Ni      | 40   | (2.0)         | -38.0            | 42.0              | 954                   | 810              | 1100              |
| Se      | 35   | (0.0)         | -35.0            | 35.0              | (46.0)                | 11.0             | 81.0              |
| Ag      | 10   | (0.0)         | -10.0            | 10.0              | 201                   | 170              | 232               |
| Tl      | 25   | (0.0)         | -25.0            | 25.0              | (108)                 | 83.0             | 133               |
| V       | 50   | (0.0)         | -50.0            | 50.0              | 491                   | 417              | 565               |
| Zn      | 60   | (0.0)         | -60.0            | 60.0              | 952                   | 809              | 1095              |

ICSA  
M5126  
M5127  
M5128  
M5129  
M5130

ICSB  
M5219  
M5220  
M5221  
M5222  
M5223

The acceptance ranges for all analytes in parentheses in the above table were determined using the listed certified value  $\pm 1$  times the associated CLP SOW CRQL. The acceptance ranges for all other analytes were determined using the certified value  $\pm 15$  percent of the listed certified value.



**CERTIFIED WEIGHT REPORT:**

**Part Number:**  
**Lot Number:**  
**Description:**

**57042**  
**051722**  
**Molybdenum (Mo)**

**Lot #**  
**Solvent:**

**MKB08597V** Ammonium hydroxide

**0.5%** **15.0** **Ammonium hydroxide**  
**(mL)**

**Expiration Date:** 051725

**Recommended Storage:** Ambient (20 °C)

**Nominal Concentration (µg/mL):**

**1000**

**NIST Test Number:**

**6UTB**

**Volume shown below was diluted to (mL):**

**3000.41**


**5E-05** **Balance Uncertainty**  
**0.058** **Flask Uncertainty**

|                |                 |
|----------------|-----------------|
|                |                 |
| Formulated By: | Lawrence Barry  |
|                | 051722          |
|                |                 |
| Reviewed By:   | Pedro L. Ruelas |
|                | 051722          |

**SDS Information**

| Compound | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|

1. Ammonium molybdate (Mo) 58142 022222 0.1000 300.0 0.084 1000 10001.0 1000.0 2.1 13106-76-8 5 mg(Mo)/m3 or-trat 333 mg/kg 3134

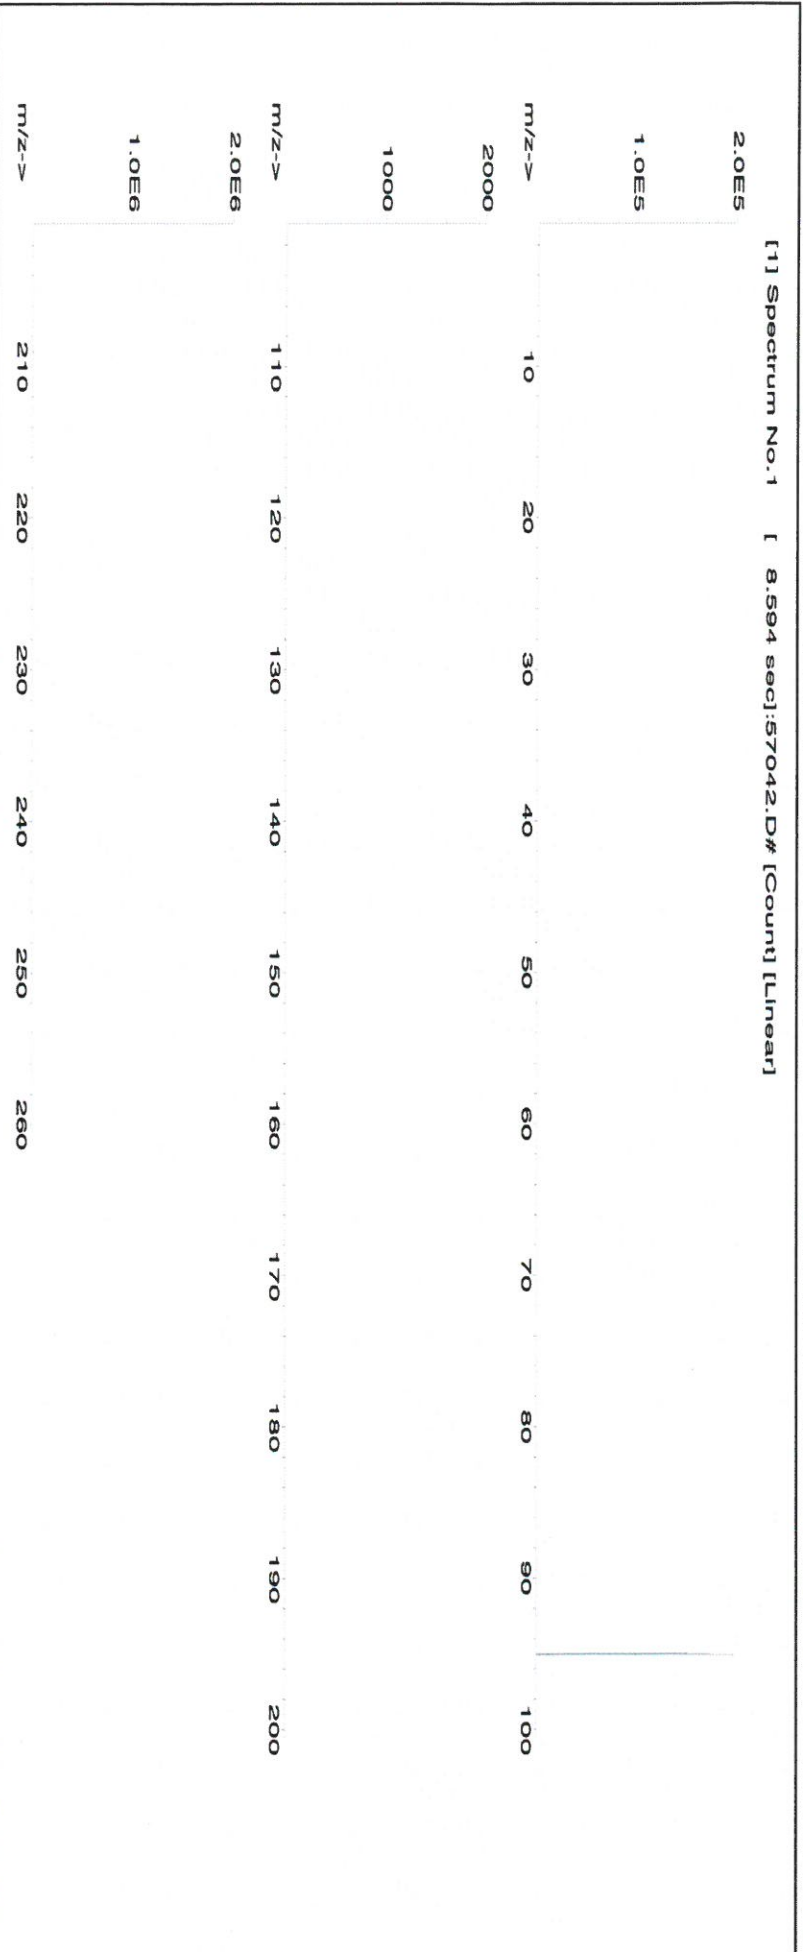



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | T     | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**


Homogeneity: No heterogeneity was observed in the preparation of this standard.

**Certified by:**

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

Printed: 10/4/2021, 3:38:48 PM





**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | T     | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

**Certified by:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**QATS LABORATORY INORGANIC REFERENCE MATERIAL  
INTERFERENCE CHECK SAMPLE SET FOR ICP-AES (ICSA WITH ICSB)**

**NOTE:** These instructions are for advisory purposes only. If any apparent conflict exists between these instructions and the analytical protocol or your contract, disregard these instructions.

**APPLICATION:** For use with the CLP SFAM01.0 SOW and revisions.

**CAUTION:** Read instructions carefully before opening bottle(s) and proceeding with the analyses.

Contains Heavy Metals  
**HAZARDOUS MATERIAL**

Safety Data Sheets  
Available Upon Request

**(A) SAMPLE DESCRIPTION**

Enclosed is a set of one (1) or more bottles of Aqueous Reference Material, each composed of metals at various concentrations and prepared with nitrate salts and oxy-acids of the respective elements in a 5% nitric acid matrix. **For the reference material source in reporting ICSA and ICSAB mixture use "USEPA". For the reference material lot number for the ICSA use "ICSA-1211" and for the ICSAB mixture use "ICSA-1211+ICSB-0710".**

**CAUTION:** The bottle(s) should be protected from light during storage to ensure the stability of silver which is contained in the ICSB solution. The bottle(s) should be stored at room temperature. **Do not allow the solution(s) to freeze.**

**(B) BREAKAGE OR MISSING ITEMS**

Check the contents of the shipment carefully for any broken, leaking, or missing items. Check that the seal is intact on each bottle. Refer to the enclosed chain of custody record. Report any problems to Mr. Keith Strout, APTIM Federal Services, LLC, at (702) 895-8722. If requested, return the chain-of-custody record with appropriate annotations and signatures to the address provided below.

**QUALITY ASSURANCE TECHNICAL SUPPORT LABORATORY  
APTIM Federal Services, LLC  
2700 Chandler Avenue - Building C  
Las Vegas, NV 89120**

**(C) ANALYSIS OF SAMPLES**

The interference check sample set is to be used to verify inter-element and background correction factors of inductively-coupled plasma (ICP) spectrometers. This reference material set consists of two (2) concentrated solutions. The ICSA solution contains the four (4) interferent elements: Al, Ca, Fe, and Mg. The ICSB solution contains the analytes: Ag, As, Sb, Ba, Be,



Instructions for QATS Reference Material: **ICP-AES ICS**

Cd, Co, Cr, Cu, Mn, Ni, Pb, Tl, Se, V, and Zn. This instruction sheet provides the nominal values for ICP-AES Part A and Part B target analytes when diluted as directed.

Using Class "A" glassware, preparation and analysis must be performed according to the following instructions:

**ICSA-1211, Interferents:** Pipet 10 mL of the ICSA solution into a 100 mL volumetric flask and dilute to volume with 2% v/v HNO<sub>3</sub>. Analyze this ICSA solution by ICP-AES.

**ICSB-0710, Analytes, mixed with ICSA-1211, Interferents:** Pipet 10 mL of the ICSA solution and 10 mL of the ICSB solution into a 100 mL volumetric flask and dilute to volume with 2% v/v HNO<sub>3</sub>. Analyze this ICSAB solution by ICP-AES.

**(D) "CERTIFIED VALUE" CONCENTRATIONS OF QATS ICP-AES ICS SOLUTION(S)**

The "Certified Value" concentrations of the elements, listed in Table 1 below, were derived from statistically pooled analysis results from the following sources, if available: QATS Laboratory, CLP laboratories, Quarterly Blind (QB)/Proficiency Testing (PT) events, CLP pre-award events, and external referee laboratories.

**Table 1. "CERTIFIED VALUES" FOR INTERFERENCE CHECK SAMPLE ICP-AES ICSA-1211, AND ICSA-1211 MIXED WITH ICSB-0710**

| Element | CRQL | Part A<br>(µg/L) | Low<br>Limit<br>(µg/L) | High<br>Limit<br>(µg/L) | Part A<br>+Part B<br>(µg/L) | Low<br>Limit<br>(µg/L) | High<br>Limit<br>(µg/L) |
|---------|------|------------------|------------------------|-------------------------|-----------------------------|------------------------|-------------------------|
| Al      | 200  | 255000           | 216000                 | 294000                  | 247000                      | 209000                 | 285000                  |
| Sb      | 60   | (0.0)            | -60.0                  | 60.0                    | 618                         | 525                    | 711                     |
| As      | 10   | (0.0)            | -10.0                  | 10.0                    | 104                         | 88.4                   | 120                     |
| Ba      | 200  | (6.0)            | -194                   | 206                     | (537)                       | 337                    | 737                     |
| Be      | 5.0  | (0.0)            | -5.0                   | 5.0                     | 495                         | 420                    | 570                     |
| Cd      | 5.0  | (1.0)            | -4.0                   | 6.0                     | 972                         | 826                    | 1120                    |
| Ca      | 5000 | 245000           | 208000                 | 282000                  | 235000                      | 199000                 | 271000                  |
| Cr      | 10   | (52.0)           | 42.0                   | 62.0                    | 542                         | 460                    | 624                     |
| Co      | 50   | (0.0)            | -50.0                  | 50.0                    | 476                         | 404                    | 548                     |
| Cu      | 25   | (2.0)            | -23.0                  | 27.0                    | 511                         | 434                    | 588                     |
| Fe      | 100  | 101000           | 85600                  | 116500                  | 99300                       | 84400                  | 114500                  |
| Pb      | 10   | (0.0)            | -10.0                  | 10.0                    | (49.0)                      | 39.0                   | 59.0                    |
| Mg      | 5000 | 255000           | 216000                 | 294000                  | 248000                      | 210000                 | 286000                  |
| Mn      | 15   | (7.0)            | -8.0                   | 22.0                    | 507                         | 430                    | 584                     |
| Ni      | 40   | (2.0)            | -38.0                  | 42.0                    | 954                         | 810                    | 1100                    |
| Se      | 35   | (0.0)            | -35.0                  | 35.0                    | (46.0)                      | 11.0                   | 81.0                    |
| Ag      | 10   | (0.0)            | -10.0                  | 10.0                    | 201                         | 170                    | 232                     |
| Tl      | 25   | (0.0)            | -25.0                  | 25.0                    | (108)                       | 83.0                   | 133                     |
| V       | 50   | (0.0)            | -50.0                  | 50.0                    | 491                         | 417                    | 565                     |
| Zn      | 60   | (0.0)            | -60.0                  | 60.0                    | 952                         | 809                    | 1095                    |

ICSA  
M5126  
M5127  
M5128  
M5129  
M5130

ICSB  
M5219  
M5220  
M5221  
M5222  
M5223

The acceptance ranges for all analytes in parentheses in the above table were determined using the listed certified value  $\pm 1$  times the associated CLP SOW CRQL. The acceptance ranges for all other analytes were determined using the certified value  $\pm 15$  percent of the listed certified value.





**Certified Reference Material CRM**



**CERTIFIED WEIGHT REPORT:**

**Part Number:** 57051  
**Lot Number:** 101521  
**Description:** Antimony (Sb)

**Lot #** 20370011  
**Solvent:** Nitric Acid

**Expiration Date:** 101524  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** **1000**  
**NIST Test Number:** 6UTB  
**Volume shown below was diluted to (mL):** 2000.25


5E-05 Balance Uncertainty  
0.116 Flask Uncertainty

|                          |                   |
|--------------------------|-------------------|
| <i>Giovanni Esposito</i> |                   |
| Formulated By:           | Giovanni Esposito |
|                          | 101521            |
| <i>Pedro L. Rentas</i>   |                   |
| Reviewed By:             | Pedro L. Rentas   |
|                          | 101521            |

**SDS Information**

| Compound | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|

1. Antimony (Sb) 58151 081820 0.1000 200.0 0.084 1000 10001.5 **1000.0** **2.2** 7440-36-0 0.5 mg/m3 or-lrat 7000 mg/kg 3102a

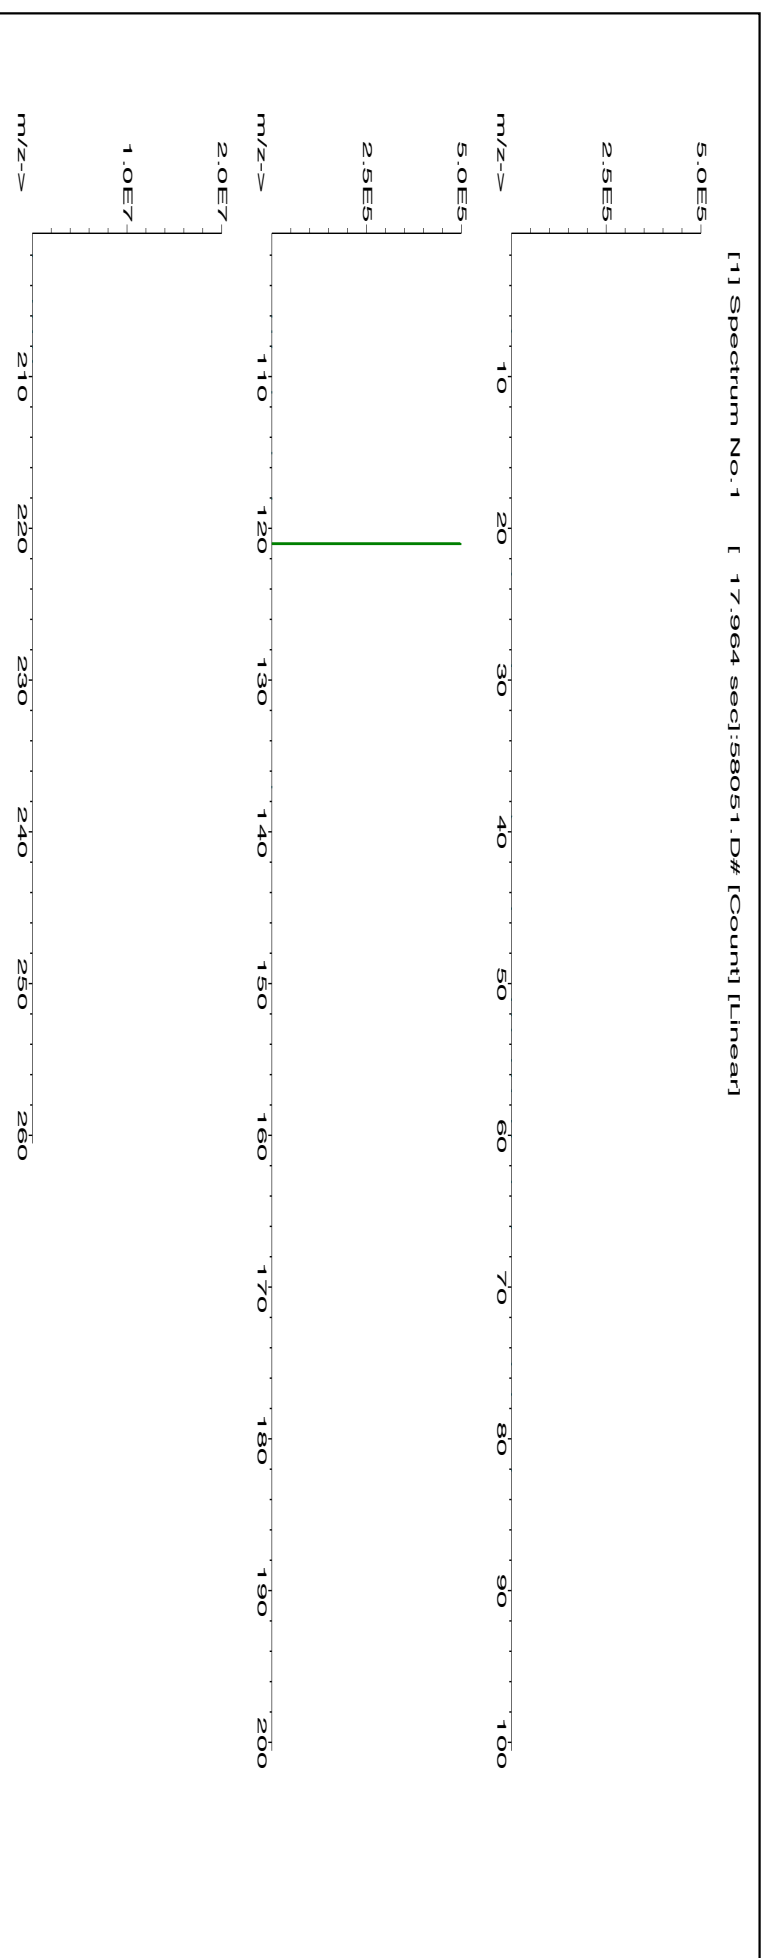



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

| Trace Metals Verification by ICP-MS (µg/mL) |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|---|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al  | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb  | T     | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As  | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba  | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be  | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi  | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B   | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte


**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

**Certified by:**

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

M5227 R: 10/18/2021



**Certified Reference Material CRM**



**CERTIFIED WEIGHT REPORT:**

**Part Number:** 57023  
**Lot Number:** 100121  
**Description:** Vanadium (V)

**Expiration Date:** 100124  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** 1000  
**NIST Test Number:** 6UTB

Volume shown below was diluted to (mL):

**Lot #** 20370011  
**Solvent:** Nitric Acid

2.0% Nitric Acid  
60.0 (mL)

5E-05 Balance Uncertainty  
0.06 Flask Uncertainty


| Compound | Part Number | Lot Number | Dilution Factor | Initial Volume (mL) | Uncertainty (mL) | Nominal Concentration (µg/mL) | Initial Concentration (µg/mL) | Final Concentration (µg/mL) | Expanded Uncertainty |         |       | NIST SRM |
|----------|-------------|------------|-----------------|---------------------|------------------|-------------------------------|-------------------------------|-----------------------------|----------------------|---------|-------|----------|
|          |             |            |                 |                     |                  |                               |                               |                             | (µg/mL)              | (µg/mL) | (TWA) |          |

**SDS Information**

(Solvent Safety Info. On Attached pg.)  
LD50

1. Ammonium Metavanadate (V) 58123 070721 0.1000 300.0 0.084 1000 10000.4 1000.0 2.1 7803-55-6 1.0 mg/m3 or-rat 630 mg/kg 3165

[1] Spectrum No. 1 [ 34.243 sec]:s8023.D# [Count] [Linear]

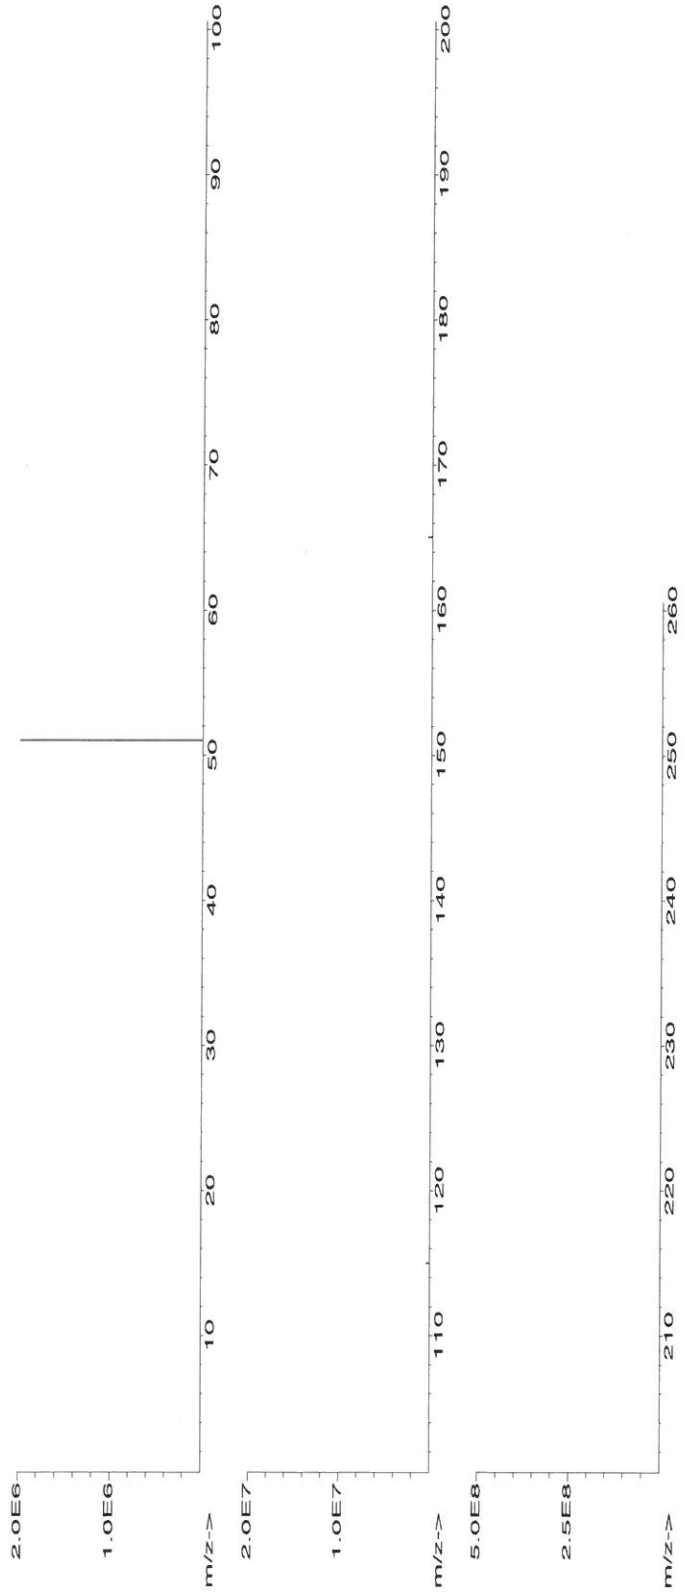



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

**Trace Metals Verification by ICP-MS ( $\mu\text{g/mL}$ )**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.02 | Os | <0.01 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | T     |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.2  | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T)= Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**CERTIFIED WEIGHT REPORT:**

**Part Number:** 57051  
**Lot Number:** 051822  
**Description:** Antimony (Sb)

**Lot #** 20370011  
**Solvent:** Nitric Acid

2.0%

60.0 (mL)

Nitric Acid

**Expiration Date:** 051825

**Recommended Storage:** Ambient (20 °C)

**Nominal Concentration (µg/mL):** 1000

**NIST Test Number:** 6UTB

**Volume shown below was diluted to (mL):** 3000.41

5E-05 Balances Uncertainty  
0.058 Flask Uncertainty

|                       |                   |
|-----------------------|-------------------|
| <i>Therapeutic</i>    |                   |
| <b>Formulated By:</b> | Giovanni Esposito |
| <b>Reviewed By:</b>   | Pedro L. Renteria |
|                       | 051822            |


**SDS Information**

| Compound | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|

**1. Antimony (Sb)**

58151 061021 0.1000 300.0 0.084 1000 10001.0 1000.0 2.1 7440-36-0 0.5 mg/m3 or-at 7000 mg/kg 3102a

[1] Spectrum No. 1 [17.964 sec]:58051.D# [Count] [Linear]

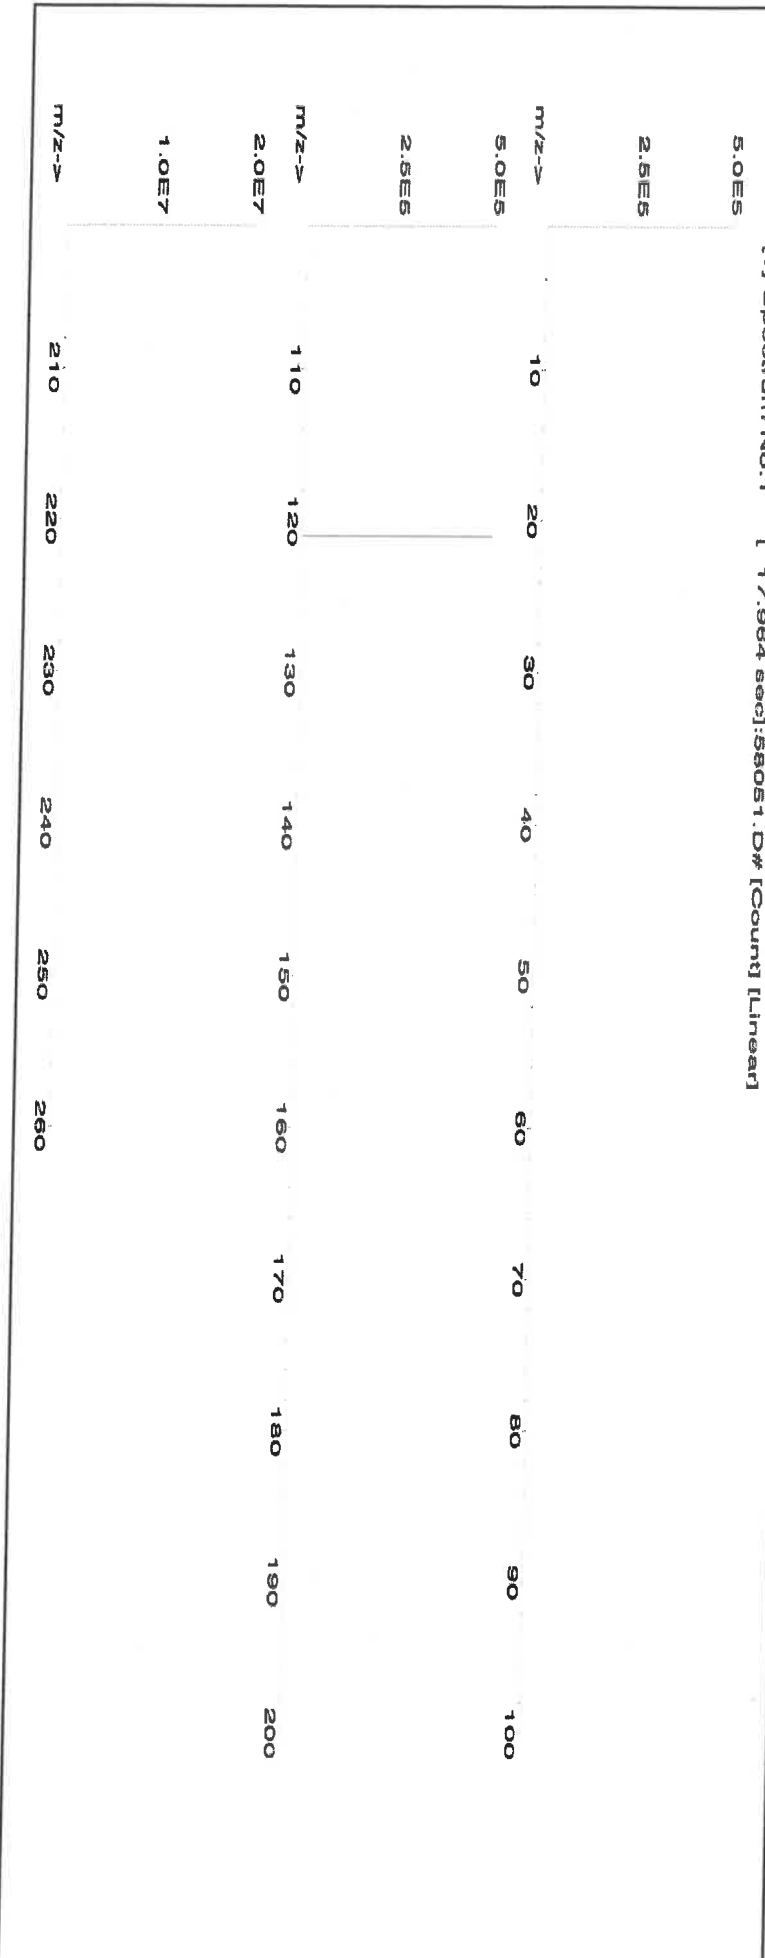



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | T     | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Ti | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ce | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Tl | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

**Certified by:**

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**CERTIFIED WEIGHT REPORT:**

Part Number: **58119**  
Lot Number: **071122**  
Description: **Potassium (K)**

Solvent: 20510011 Nitric Acid

Expiration Date: 071125  
Recommended Storage: Ambient (20 °C)  
Nominal Concentration (µg/mL): **10000**  
NIST Test Number: 6UTB

2% 40.0 (mL) Nitric Acid

Weight shown below was diluted to (mL): 2000.02  
5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

|                |                 |
|----------------|-----------------|
|                |                 |
| Formulated By: | Lawrence Barry  |
|                | 071122          |
|                |                 |
| Reviewed By:   | Pedro L. Rentas |
|                | 071122          |

**Compound**


1. Potassium nitrate (K)

| RM#   | Lot Number | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty Purity (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS#      | OSHA PEL (TWA) | LD50              | NIST SRM |
|-------|------------|-----------------------|------------|------------------------|-----------|-------------------|-------------------|----------------------|----------------------------------|-----------|----------------|-------------------|----------|
| IN034 | KD022021A1 | 10000                 | 99.999     | 0.10                   | 37.6      | 53.1925           | 53.1934           | 10000.2              | 20.0                             | 7757-79-1 | 5 mg/m3        | or-rat 3015 mg/kg | 3141a    |

**SDS Information**

(Solvent Safety Info. On Attached pg.)

[1] Spectrum No. 1 [ 35.763 sec]:58119.D# [Count] [Linear]

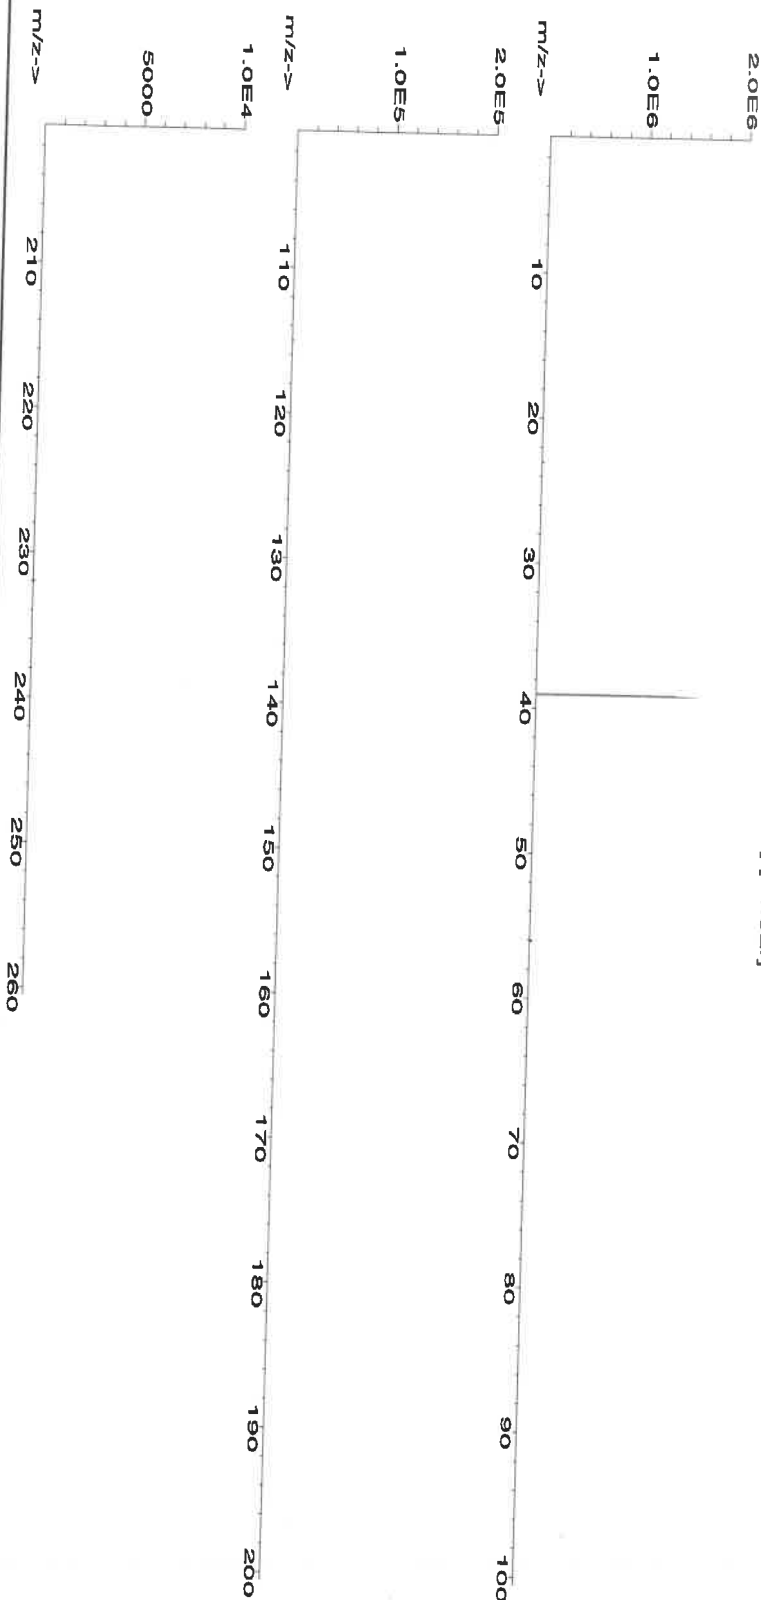



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.02 | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

**Certified by:**

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).





M5289 R: 07/12/22  
Certified Reference Material CRM

34



ANAB ISO 17034 Accredited  
AR-1539 Certificate Number  
https://AbsoluteStandards.com

**CERTIFIED WEIGHT REPORT:**

**Part Number:** 58113  
**Lot Number:** 070622  
**Description:**

Aluminum (Al)

**Lot #**  
**Solvent:** 20370011 Nitric Acid

**Expiration Date:** 070625  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** 10000  
**NIST Test Number:** 6UTB

2% 40.0 Nitric Acid  
(mL)

**Weight shown below was diluted to (mL):** 2000.02 0.058 Balance Uncertainty  
Flask Uncertainty

|                |                   |
|----------------|-------------------|
|                |                   |
| Formulated By: | Lawrence Barry    |
|                | 070622            |
|                |                   |
| Reviewed By:   | Pedro L. Renteria |
|                | 070622            |


**Compound**

| RM# | Lot Number | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty Purity (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|-----|------------|-----------------------|------------|------------------------|-----------|-------------------|-------------------|----------------------|----------------------------------|------|----------------|------|----------|
|-----|------------|-----------------------|------------|------------------------|-----------|-------------------|-------------------|----------------------|----------------------------------|------|----------------|------|----------|

**SDS Information**

1. Aluminum nitrate nonahydrate (Al) IN022 AUD012021A1 10000 99.999 0.10 7.10 281.6956 281.6977 10000.1 20.0 7784-27-2 2 mg/m3 or-tal 3671 mg/kg 3101a

[1] Spectrum No. 1 [15.014 sec]:58113.D# [Count] [Linear]

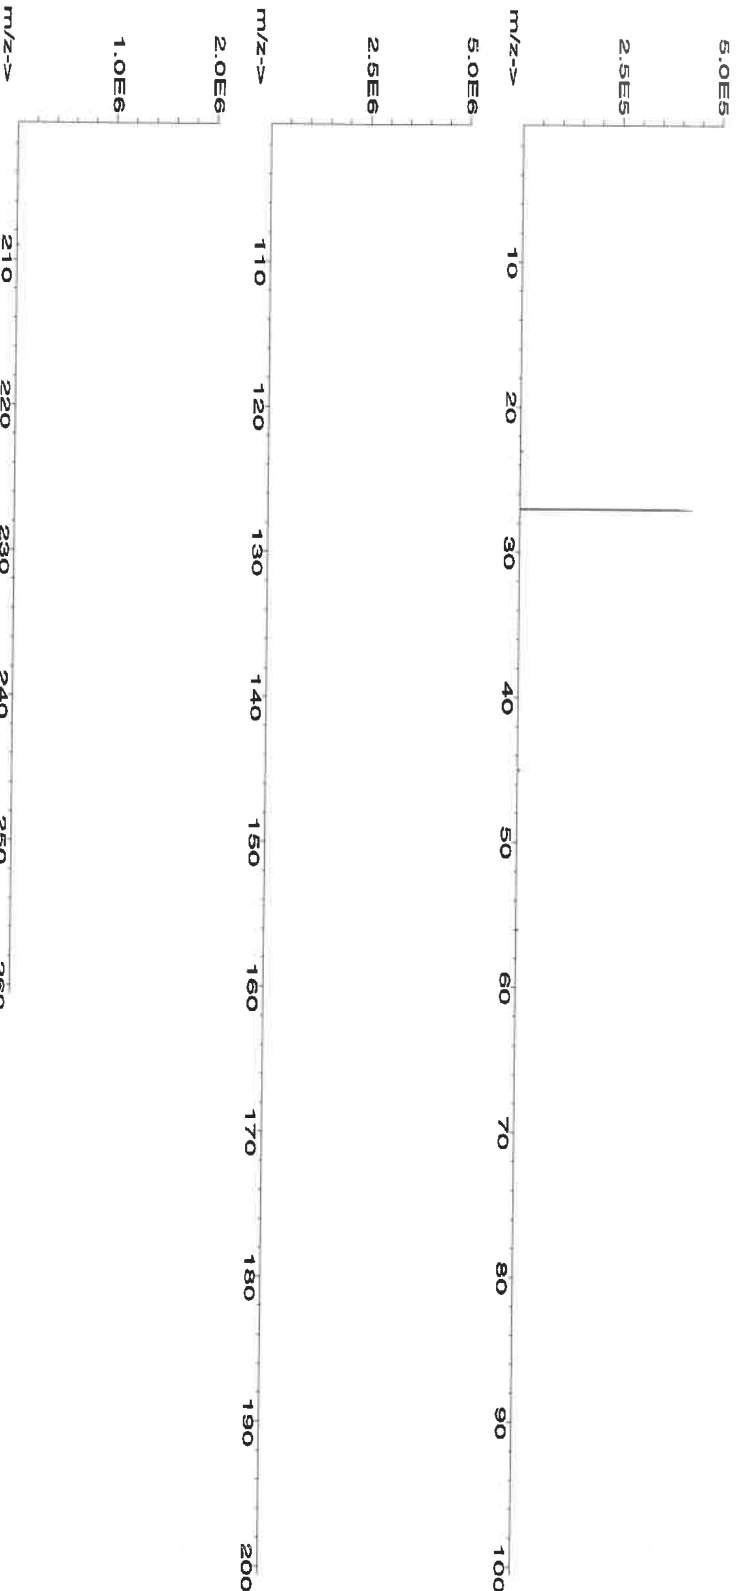



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | T     | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Ru | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Sr | <0.02 | S  | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | Ta | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ti | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



R: 4/20/21

Instructions for QATS Reference Material: *Inorganic ICV Solutions*

QATS LABORATORY INORGANIC REFERENCE MATERIAL  
INITIAL CALIBRATION VERIFICATION SOLUTIONS  
(ICV1, ICV5, AND ICV6)

**NOTE:** These instructions are for advisory purposes only. If any apparent conflict exists between these instructions and the analytical protocol or your contract, disregard these instructions.

**APPLICATION:** For use with the CLP SFAM01.0 SOW and revisions.

**CAUTION:** Read instructions carefully before opening bottle(s) and proceeding with the analyses.

Contains Metals in Dilute Acidic or  
Cyanide in Basic Aqueous Solutions  
**HAZARDOUS MATERIAL**

Safety Data Sheets  
Available Upon Request

M5291  
M15292  
M15293  
M15294  
M15295

**(A) SAMPLE DESCRIPTION**

Enclosed is a set of one (1) or more Aqueous Inorganic Reference Materials containing various analyte concentrations. ICV1 and ICV5 are in a matrix of dilute nitric acid. ICV6 is in a matrix of dilute basic solution. **For the reference material source in reporting ICVs use "USEPA". For the reference material lot number for the ICV1, ICV5, and ICV6 solutions use "ICV1-1014", "ICV5-0415", and "ICV6-0400", respectively.**

**(B) BREAKAGE OR MISSING ITEMS**

Check the contents of the shipment carefully for any broken, leaking, or missing items. Check that the seal is intact on each bottle. Refer to the enclosed chain of custody record. Report any problems to Mr. Keith Strout, APTIM Federal Services, LLC, at (702) 895-8722. If requested, return the chain-of-custody record with appropriate annotations and signatures to the address provided below.

QUALITY ASSURANCE TECHNICAL SUPPORT LABORATORY  
APTIM Federal Services, LLC  
2700 Chandler Avenue - Building C  
Las Vegas, NV 89120

**(C) ANALYSIS OF SAMPLES**

The Initial Calibration Verification Solutions (ICVs) are to be used to evaluate the accuracy of the initial calibrations of ICP, AA, and Cyanide colorimetric instruments, and are to be used with the CLP SOWs and revisions. The values for each element in the ICVs are listed below in µg/L (ppb) for the resulting solution(s) after the dilution of the concentrate(s) according to the following instructions. Use Class 'A' glassware to prepare the solution(s).

**ICV1-1014** For ICP-AES analysis, use a 10-fold dilution by pipetting 10 mL of the ICV1 concentrate into a 100 mL volumetric flask and dilute to volume with 2% (v/v) nitric acid.





**QUALITY ASSURANCE TECHNICAL SUPPORT LABORATORY**  
**"An ISO 9001:2015 Certified Program"**

**Instructions for QATS Reference Material: *Inorganic ICV Solutions***

- ICV1-1014** For ICP-MS analysis, use a 50-fold dilution by pipetting 2 mL of the ICV1 concentrate into a 100 mL volumetric flask and dilute to volume with 1% (v/v) nitric acid.
- ICV5-0415** For the cold vapor analysis of mercury by AA, use a 100-fold dilution by pipetting 1 mL of the ICV5 concentrate into a 100 mL volumetric flask and dilute to volume with 2% (v/v) nitric acid. The ICV5 concentrate is prepared in 0.05% (w/v)  $K_2Cr_2O_7$  and 5% (v/v) nitric acid.
- ICV6-0400** For the analysis of cyanide, use a 100-fold dilution by pipetting 1 mL of the ICV6 concentrate into a 100 mL volumetric flask and dilute to volume with Type II water. Distill this solution along with the samples before analysis. The cyanide concentrate is prepared from  $K_3Fe(CN)_6$ , Type II water, and 0.1 % sodium hydroxide, and will decompose rapidly if exposed to light.

**NOTE:** USE TYPE II WATER AND HIGH-PURITY ACIDS FOR ALL DILUTIONS.

**(D) CERTIFIED CONCENTRATIONS OF QATS ICV1, ICV5, AND ICV6 SOLUTIONS**

| ICV1-1014 |  |  |
|-----------|--|--|
| Element   | Concentration (µg/L)<br>(after 10-fold dilution) | Concentration (µg/L)<br>(after 50-fold dilution) |
| Al        | 2500   | 500  |
| Sb        | 1000   | 200  |
| As        | 1000   | 200  |
| Ba        | 520  | 100  |
| Be        | 510  | 100  |
| Cd        | 510  | 100  |
| Ca        | 10000  | 2000   |
| Cr        | 520  | 100  |
| Co        | 520  | 100  |
| Cu        | 510  | 100  |
| Fe        | 10000  | 2000   |
| Pb        | 1000   | 200  |
| Mg        | 6000   | 1200   |
| Mn        | 520  | 100  |
| Ni        | 530  | 110  |
| K         | 9900   | 2000   |
| Se        | 1000   | 200  |
| Ag        | 250  | 50   |
| Na        | 10000  | 2000   |
| Tl        | 1000   | 210  |
| V         | 500  | 100  |
| Zn        | 1000   | 200  |

| ICV5-0415 |   | ICV6-0400       |   |
|-----------|---|-----------------|---|
| Element   | Concentration (µg/L)<br>(after 100-fold dilution) | Analyte         | Concentration (µg/L)<br>(after 100-fold dilution) |
| Hg        | 4.0   | CN <sup>-</sup> | 99  |



## Certified Reference Material CRM

## CERTIFIED WEIGHT REPORT:

Part Number:  
Lot Number:  
Description:

58126  
020422  
Iron (Fe)

Lot #

Solvent: 20370011 Nitric Acid

Expiration Date:  
Recommended Storage:  
Nominal Concentration (µg/mL):  
NIST Test Number:

020425  
Ambient (20 °C)  
10000  
6UTB  
5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

Weight shown below was diluted to (mL): 3000.41

|                   |                          |
|-------------------|--------------------------|
| Giovanni Esposito |                          |
| Formulated By:    | Giovanni Esposito 020422 |
| Pedro L. Rentas   |                          |
| Reviewed By:      | Pedro L. Rentas 020422   |

## SDS Information

Expanded  
Uncertainty  
+/- (µg/mL)

(Solvent Safety Info. On Attached pg.)

NIST


LD50

CAS# OSHA PEL (TWA)

SRM

| Compound                              | RM#   | Lot Number | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS#      | OSHA PEL (TWA) | LD50 | or-hat 7500mg/kg |
|---------------------------------------|-------|------------|-----------------------|------------|-----------------|-----------|-------------------|-------------------|----------------------|----------------------------------|-----------|----------------|------|------------------|
| 1. Iron(III) nitrate nonahydrate (Fe) | IN346 | 221035107  | 10000                 | 99.999     | 0.10            | 100.0     | 30.0044           | 30.0090           | 10001.5              | 20.0                             | 7782-61-8 | 5 mg/m3        |      | 3126a            |

[1] Spectrum No.1 [ 30.763 sec]:58126.D# [Count] [Linear]

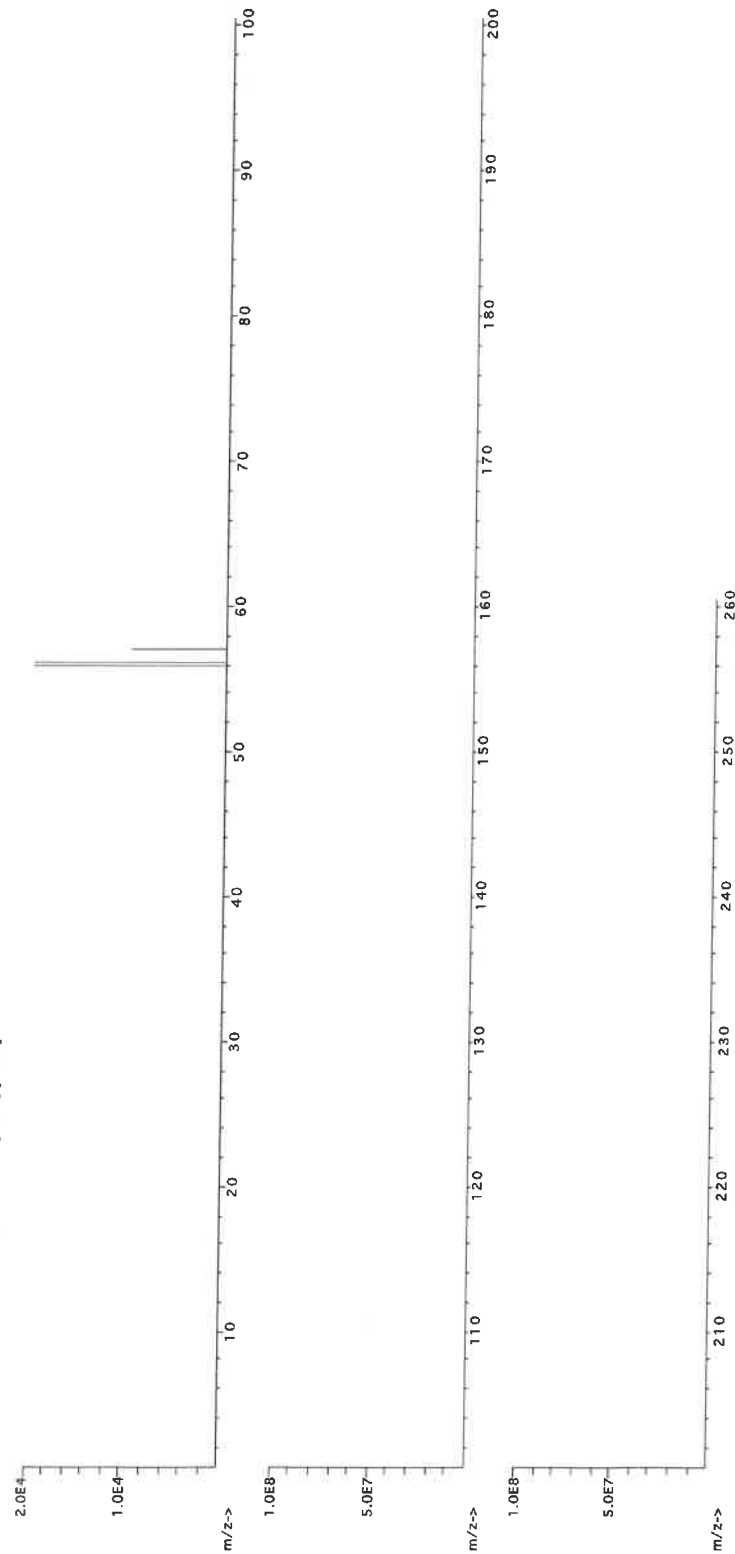



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

**Trace Metals Verification by ICP-MS ( $\mu\text{g/mL}$ )**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.10 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.10 | Mn | <0.10 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.5  | Ga | <0.2  | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.10 | Ge | <0.02 | La | <0.10 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.10 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T)= Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



*R-09/18/22* **(B1)**

**Certified Reference Material CRM**

**CERTIFIED WEIGHT REPORT:**

**Part Number:** 57056  
**Lot Number:** 072122  
**Description:** Barium (Ba)

**Solvent:** 20510011 Nitric Acid

**Lot #**

**Expiration Date:** 072125  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** 1000  
**NIST Test Number:** 6UTB

**2%** 40.0 (mL) Nitric Acid

**Weight shown below was diluted to (mL):** 2000.02 0.058 Flask Uncertainty

|                          |                          |
|--------------------------|--------------------------|
| <i>Giovanni Esposito</i> |                          |
| Formulated By:           | Giovanni Esposito        |
| Reviewed By:             | <i>Pedro L. Renteria</i> |
|                          | 072122                   |

| SDS Information        |                  |                       |            |                        |           |                   |                   |                      |                                  |
|------------------------|------------------|-----------------------|------------|------------------------|-----------|-------------------|-------------------|----------------------|----------------------------------|
| Compound               | Lot Number       | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty Purity (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) |
| 1. Barium nitrate (Ba) | IN023 BA022019A1 | 1000                  | 99.899     | 0.10                   | 52.3      | 3.82417           | 3.82426           | 1000.0               | 2.0                              |
|                        |                  |                       |            |                        |           |                   |                   |                      | 10022-31-8                       |
|                        |                  |                       |            |                        |           |                   |                   |                      | 0.5 mg/m3                        |
|                        |                  |                       |            |                        |           |                   |                   |                      | or 1st 355 mg/kg 31044           |

[1] Spectrum No. 1 [ 12.514 sec]:58156.D# [Count] [Linear]





**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

| Trace Metals Verification by ICP-MS (µg/mL) |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|---|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al  | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.02 | Tb | <0.02 |
| Sb  | <0.02 | Ca | <0.2  | Er | <0.2  | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 |
| As  | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.02 | Os | <0.01 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 |
| Ba  | T     | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 |
| Be  | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.02 | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 |
| Bi  | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 |
| B   | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 |

(T)= Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).





*R-09/18/22* **(B1)**

**Certified Reference Material CRM**

**CERTIFIED WEIGHT REPORT:**

**Part Number:** 57056  
**Lot Number:** 072122  
**Description:** Barium (Ba)

**Solvent:** 20510011 Nitric Acid

**Lot #**


**Expiration Date:** 072125  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** 1000  
**NIST Test Number:** 6UTB  
**Weight shown below was diluted to (mL):** 2000.02  
**5E-05 Balance Uncertainty**  
**0.058 Flask Uncertainty**

**2% 40.0 (mL) Nitric Acid**

|                          |                          |
|--------------------------|--------------------------|
| <i>Giovanni Esposito</i> |                          |
| Formulated By:           | Giovanni Esposito        |
| Reviewed By:             | <i>Pedro L. Renteria</i> |
|                          | 072122                   |

| SDS Information        |                  |                       |            |                        |           |                   |                   |                      |                                  |
|------------------------|------------------|-----------------------|------------|------------------------|-----------|-------------------|-------------------|----------------------|----------------------------------|
| Compound               | Lot Number       | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty Purity (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) |
| 1. Barium nitrate (Ba) | IN023 BA022019A1 | 1000                  | 99.899     | 0.10                   | 52.3      | 3.82417           | 3.82426           | 1000.0               | 2.0                              |
|                        |                  |                       |            |                        |           |                   |                   |                      | 10022-31-8                       |
|                        |                  |                       |            |                        |           |                   |                   |                      | 0.5 mg/m3                        |
|                        |                  |                       |            |                        |           |                   |                   |                      | or 1st 355 mg/kg 31044           |

[1] Spectrum No. 1 [ 12.514 sec]:58156.D# [Count] [Linear]

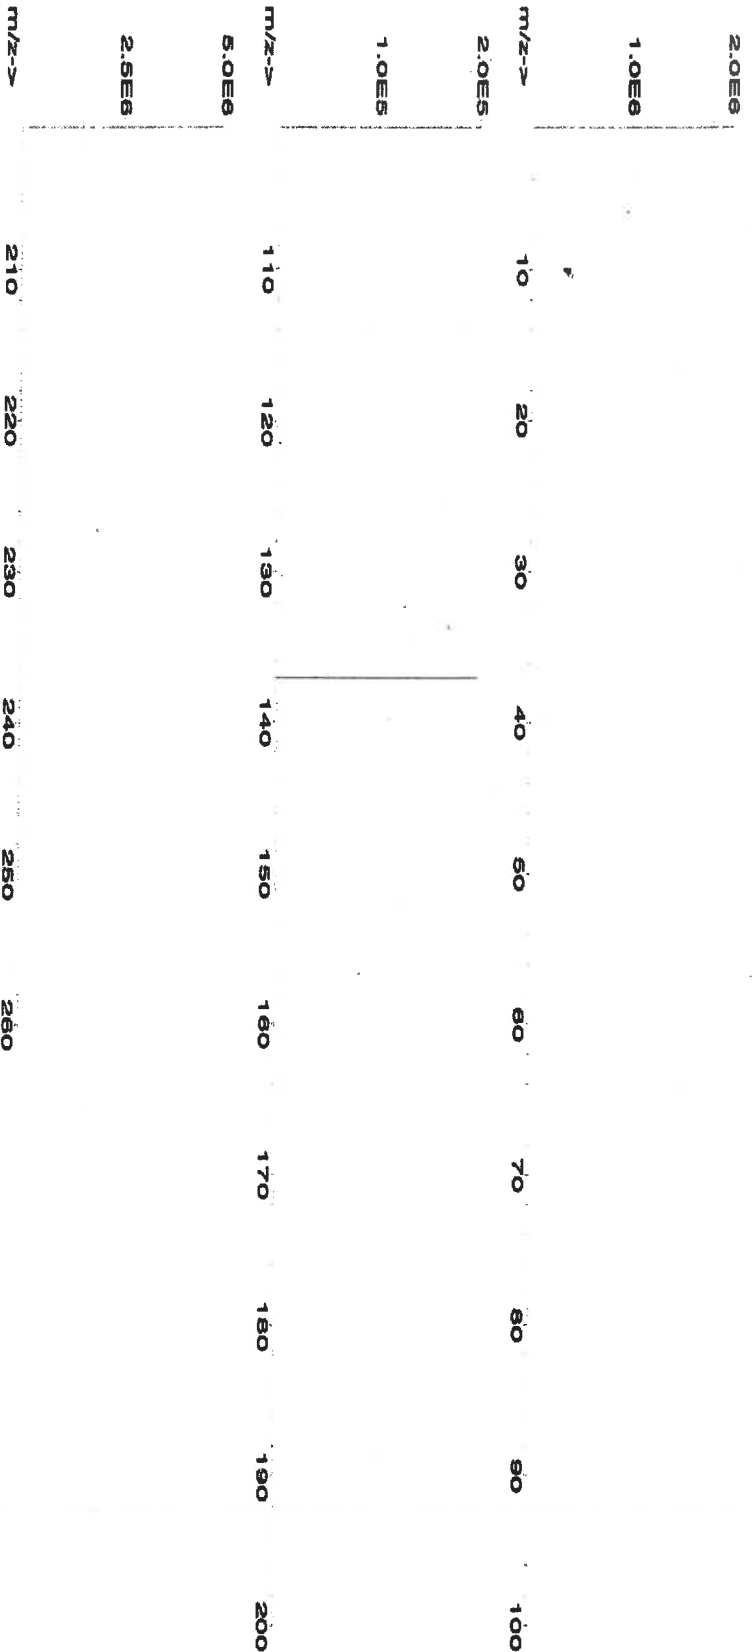



## Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

### Trace Metals Verification by ICP-MS ( $\mu\text{g/mL}$ )

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.02 | Er | <0.2  | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.02 | Os | <0.01 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | T     | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.02 | Hg | <0.2  | P  | <0.2  | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.2  | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

### Physical Characterization:

**Homogeneity:** No heterogeneity was observed in the preparation of this standard.

**Certified by:**

Ben. P. R.

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**Certified Reference Material CRM**

M5429 R1 0126/23 (B)

**CERTIFIED WEIGHT REPORT:**

**Part Number:**  
**Lot Number:**  
**Description:**

57103  
070622  
Lithium (Li)

**Solvent:** 20510011 Nitric Acid

**Expiration Date:**  
**Recommended Storage:**  
**Nominal Concentration (µg/mL):**  
**NIST Test Number:**

070625  
Ambient (20 °C)  
10000  
6UTB

2% 20.0 (mL)

**Weight shown below was diluted to (mL):** 1000.12  
5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

*Lawrence Barry*  
**Formulated By:** Lawrence Barry 070622  
*Pedro L. Rentas*  
**Reviewed By:** Pedro L. Rentas 070622


| Compound | RM# | Lot Number | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty | Assay | Target     |            | Actual        |            | Expanded Uncertainty | (Solvent Safety Info. On Attached pg.) | NIST SRM |
|----------|-----|------------|-----------------------|------------|-------------|-------|------------|------------|---------------|------------|----------------------|--|----------|
|          |     |            |                       |            |             |       | Weight (g) | Weight (g) | Conc. (µg/mL) | Weight (g) |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |
|          |     |            |                       |            |             |       |            |            |               |            |                      |  |          |

|                         |       |            |       |        |      |      |          |          |         |      |           |         |                   |    |
|-------------------------|-------|------------|-------|--------|------|------|----------|----------|---------|------|-----------|---------|-------------------|----|
| 1. Lithium nitrate (Li) | IN019 | L2042019A1 | 10000 | 99.999 | 0.10 | 10.0 | 100.0134 | 100.0173 | 10000.4 | 20.0 | 7790-69-4 | 5 mg/m3 | of-rat 1426 mg/kg | NA |
|-------------------------|-------|------------|-------|--------|------|------|----------|----------|---------|------|-----------|---------|-------------------|----|

**SDS Information**

(Solvent Safety Info. On Attached pg.)  
CAS# OSHA PEL (TWA) LD50

[1] Spectrum No.1 [ 9.619 sec]:58103.D# [Count] [Linear]

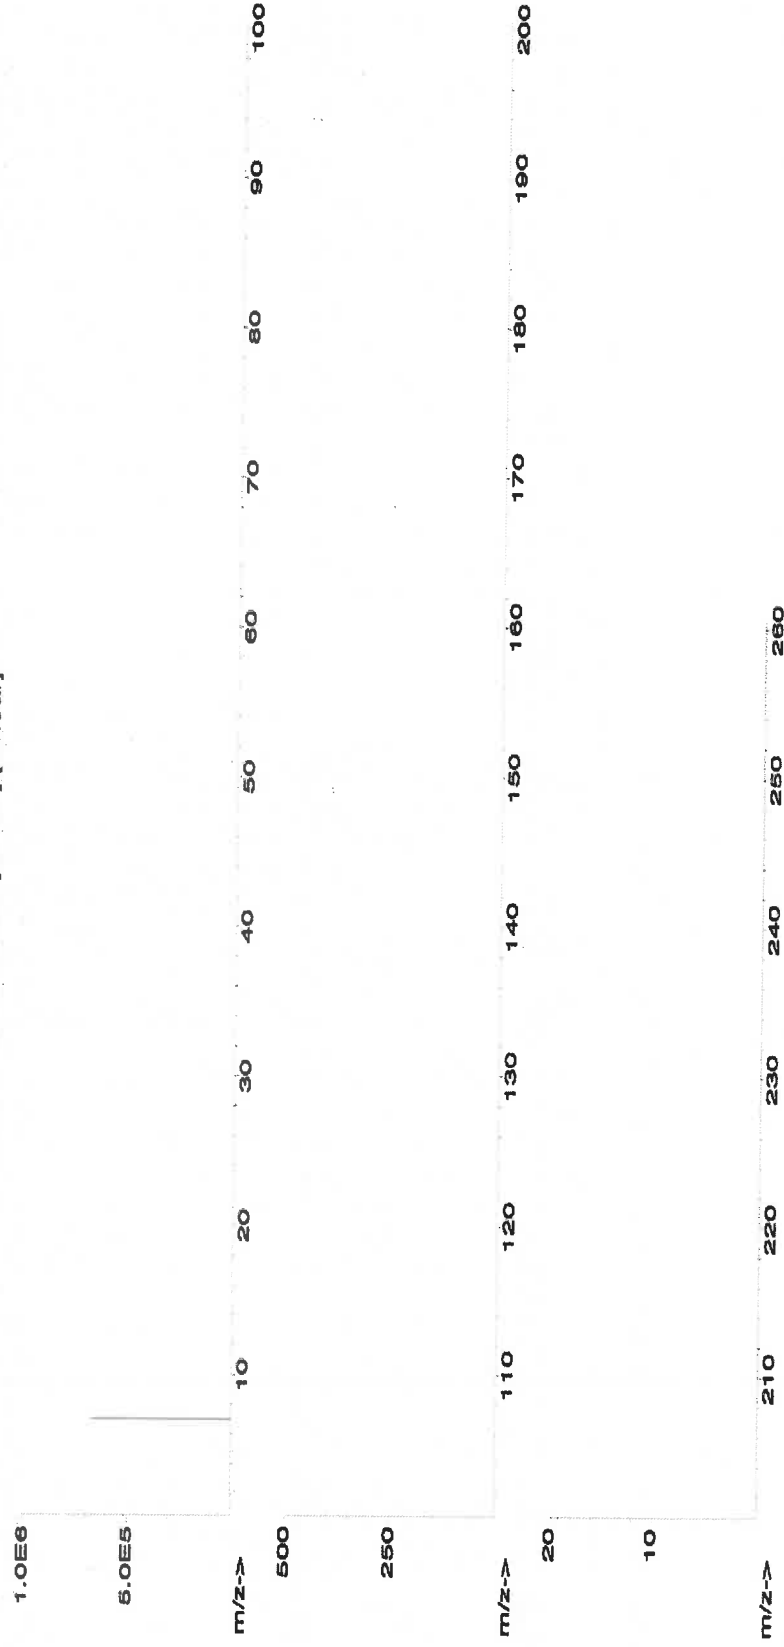



# Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):

## Trace Metals Verification by ICP-MS (µg/mL)

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.2  | Ho | <0.02 | La | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.2  | Na | <0.02 | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

### Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**CERTIFIED WEIGHT REPORT:**

Part Number: **58112**  
Lot Number: **120922**  
Description: **Magnesium (Mg)**

Solvent: 20510011 Nitric Acid

Lot #

2% 60.0 Nitric Acid (ml)

Expiration Date: 120925  
Recommended Storage: Ambient (20 °C)  
Nominal Concentration (µg/mL): 10000  
NIST Test Number: 6UTB

Weight shown below was diluted to (mL): 3000.41 0.058 Balance Uncertainty: 5E-05 Flask Uncertainty:


|                   |                   |
|-------------------|-------------------|
| Giovanni Caporaso |                   |
| Formulated By:    | Giovanni Esposito |
| Reviewed By:      | Pedro L. Renteria |
|                   | 120922            |

**Compound**

| RM# | Lot Number | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | SDS Information (Solvent Safety Info. On Attached pg.) | NIST SRM |
|-----|------------|-----------------------|------------|-----------------|-----------|-------------------|-------------------|----------------------|----------------------------------|------|--|----------|
|-----|------------|-----------------------|------------|-----------------|-----------|-------------------|-------------------|----------------------|----------------------------------|------|--|----------|

1. Magnesium nitrate hexahydrate (Mg) IN030 MAG11221A1 10000 99.999 0.10 8.74 343.2213 343.2669 10001.3 20.0 13446-18-9 NA official 5440 mg/kg 3131a

[1] Spectrum No. 1 [ 19.923 sec]: 58112.D# [Count] [Linear]

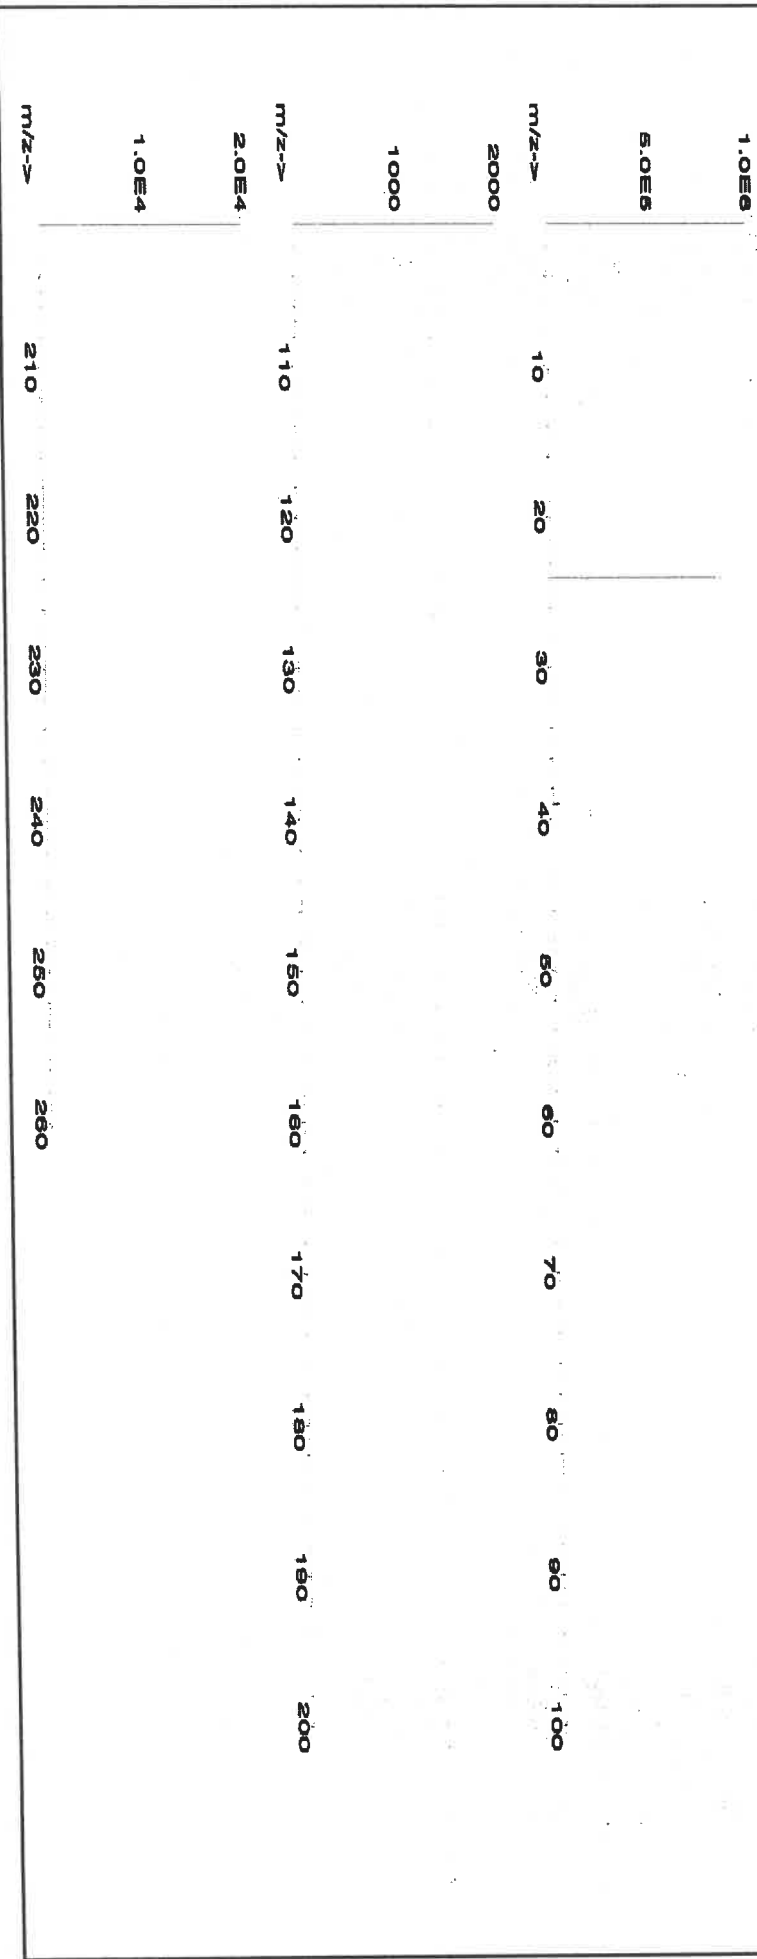



# Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

## Trace Metals Verification by ICP-MS (µg/mL)

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.02 | Os | T     | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.02 | Hg | <0.2  | P  | <0.2  | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

### Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



*M5494* **Certified Reference Material CRM**

*Ri01/19/23*



**CERTIFIED WEIGHT REPORT:**

**Part Number:**  
**Lot Number:**  
**Description:**

**57028**  
**011223**  
**Nickel (Ni)**

**Lot #**  
**20510011**  
**Solvent:**  
**Nitric Acid**

**Expiration Date:**

011226

**Recommended Storage:**  
**Ambient (20 °C)**

**Nominal Concentration (µg/mL):**

1000

**NIST Test Number:**

6UTB

**Volume shown below was diluted to (mL):**


2000.02

|                          |                        |
|--------------------------|------------------------|
| <i>Giovanni Esposito</i> |                        |
| Formulated By:           | Giovanni Esposito      |
| Reviewed By:             | <i>Pedro L. Rentes</i> |
|                          | 011223                 |

| Compound | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | SDS Information                        |      | NIST SRM |
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|--|------|----------|
|          |             |            |                 |                   |                          |                       |                       |                     |                                  | (Solvent Safety Info. On Attached pg.) | LD50 |          |

|  |       |        |        |       |       |      |         |        |     |            |         |                    |      |
|--|-------|--------|--------|-------|-------|------|---------|--------|-----|------------|---------|--------------------|------|
| 1. Nickel(II) nitrate hexahydrate (Ni) | 58128 | 033122 | 0.1000 | 200.0 | 0.084 | 1000 | 10000.9 | 1000.0 | 2.2 | 13478-00-7 | 1 mg/m3 | orl-rat 1620 mg/kg | 3136 |
|--|-------|--------|--------|-------|-------|------|---------|--------|-----|------------|---------|--------------------|------|

[1] Spectrum No.1 [ 9.135 sec]:58028.D# [Count] [Linear]

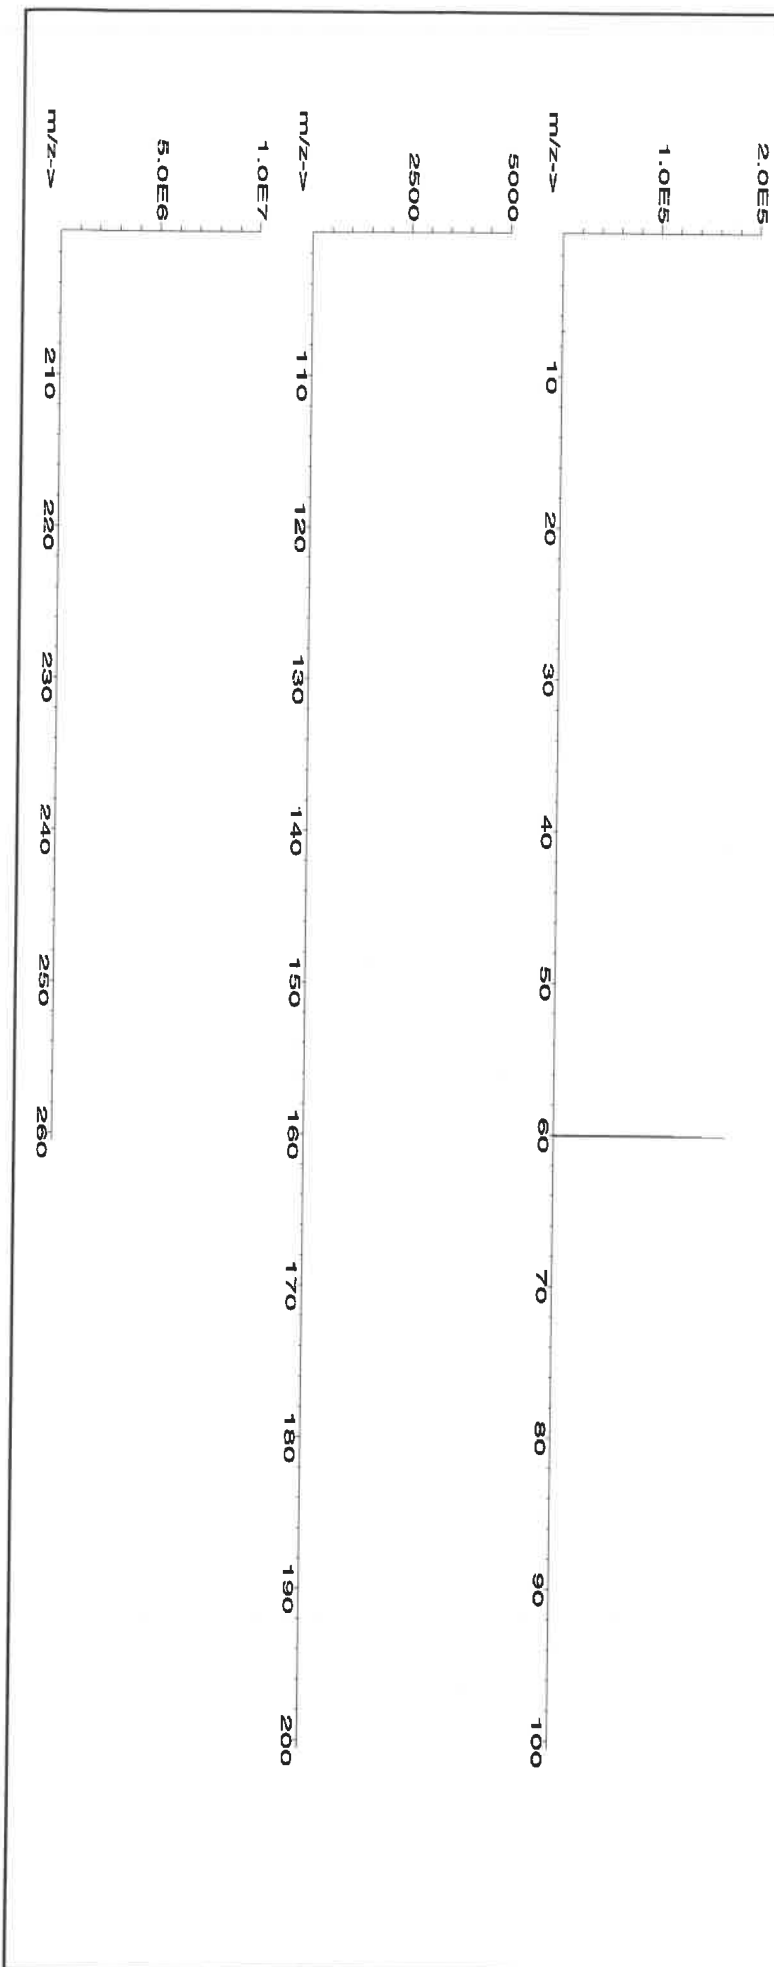



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | T     | Pt | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).





15497-15498 R: 03/17/23 (2)

**CERTIFIED WEIGHT REPORT:**

**Part Number:**  
**Lot Number:**  
**Description:**

**58120**  
**031523**  
**Calcium (Ca)**

**Solvent:** 21110221 Nitric Acid

**Expiration Date:**  
**Recommended Storage:**  
**Nominal Concentration (µg/mL):**  
**NIST Test Number:**

**031526**  
**Ambient (20 °C)**  
**10000**  
**6UTB**  
**5E-05 Balance Uncertainty**  
**0.058 Flask Uncertainty**

**2%**  
**60.0**  
**Nitric Acid**  
**(mL)**

**Weight shown below was diluted to (mL): 3000.41**

|                          |                          |
|--------------------------|--------------------------|
| <i>Giovanni Esposito</i> |                          |
| Formulated By:           | Giovanni Esposito 031523 |
| <i>Pedro L. Rentas</i>   |                          |
| Reviewed By:             | Pedro L. Rentas 031523   |

**SDS Information**

(Solvent Safety Info. On Attached pg.)  
NIST  
SRM

Expanded  
Uncertainty

Actual  
Conc. (µg/mL)

Actual  
Weight (g)

Target  
Weight (g)

Assay  
(%)

Purity  
(%)

Nominal  
Conc. (µg/mL)

Lot  
Number

RM#

Compound

1. Calcium carbonate (Ca)

IN014 CAD072022A1

10000

99.999

0.10

39.9

75.1990

75.2093

10001.4

20.0


471-34-1

5 mg/m3

or: rat >2000mg/kg

3109a

[1] Spectrum No.1 [ 12.514 sec]:58120.D# [Count] [Linear]

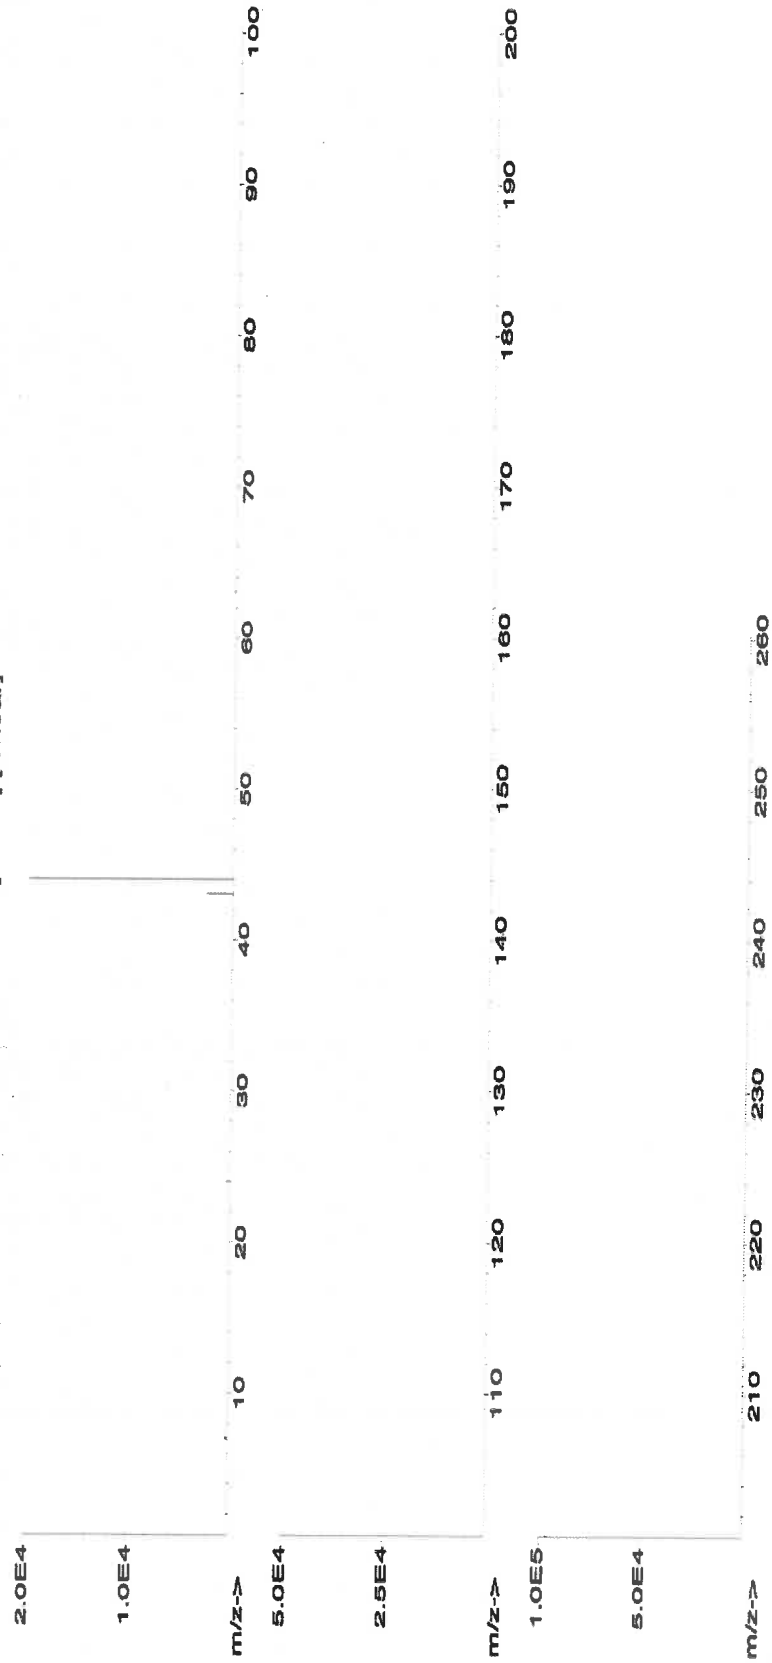



# Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

| Trace Metals Verification by ICP-MS (µg/mL) |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|---|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al  | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  | Tb | <0.02 |
| Sb  | <0.02 | Ca | <0.02 | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Tc | <0.02 |
| As  | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.02 | Os | <0.01 | Rh | <0.02 | Ag | <0.02 | Ti | <0.02 |
| Ba  | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 |
| Be  | <0.01 | Cr | <0.02 | Ga | <0.2  | Fe | <0.02 | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 |
| Bi  | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 |
| B   | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Tl | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       | W  | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       | U  | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       | V  | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       | Yb | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       | Y  | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       | Zn | <0.02 |
|   |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       | Zr | <0.02 |

(T) = Target analyte

## Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



15497-15498 R203/17/23(2)

**CERTIFIED WEIGHT REPORT:**

**Part Number:**  
**Lot Number:**  
**Description:**

**58120**  
**031523**  
**Calcium (Ca)**

**Solvent:** 21110221 Nitric Acid

**Expiration Date:**  
**Recommended Storage:**  
**Nominal Concentration (µg/mL):**  
**NIST Test Number:**

**031526**  
**Ambient (20 °C)**  
**10000**  
**6UTB**

**2%**  
**60.0**  
**(mL)**  
**Nitric Acid**

**Weight shown below was diluted to (mL):** 3000.41  
5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

|                          |                          |
|--------------------------|--------------------------|
| <i>Giovanni Esposito</i> |                          |
| Formulated By:           | Giovanni Esposito 031523 |
| <i>Pedro L. Rentas</i>   |                          |
| Reviewed By:             | Pedro L. Rentas 031523   |

**SDS Information**

(Solvent Safety Info. On Attached pg.)  
NIST  
SRM

Expanded  
Uncertainty

Actual  
Conc. (µg/mL)

Actual  
Weight (g)

Target  
Weight (g)

Assay  
(%)

Purity  
(%)

Nominal  
Conc. (µg/mL)


Lot  
Number

RM#

Compound

|                           |       |             |       |        |      |      |         |         |         |      |          |         |                   |       |
|---------------------------|-------|-------------|-------|--------|------|------|---------|---------|---------|------|----------|---------|-------------------|-------|
| 1. Calcium carbonate (Ca) | IN014 | CAD072022A1 | 10000 | 99.999 | 0.10 | 39.9 | 75.1990 | 75.2093 | 10001.4 | 20.0 | 471-34-1 | 5 mg/m3 | or:rat >2000mg/kg | 3109a |
|---------------------------|-------|-------------|-------|--------|------|------|---------|---------|---------|------|----------|---------|-------------------|-------|

[1] Spectrum No.1 [ 12.514 sec]:58120.D# [Count] [Linear]

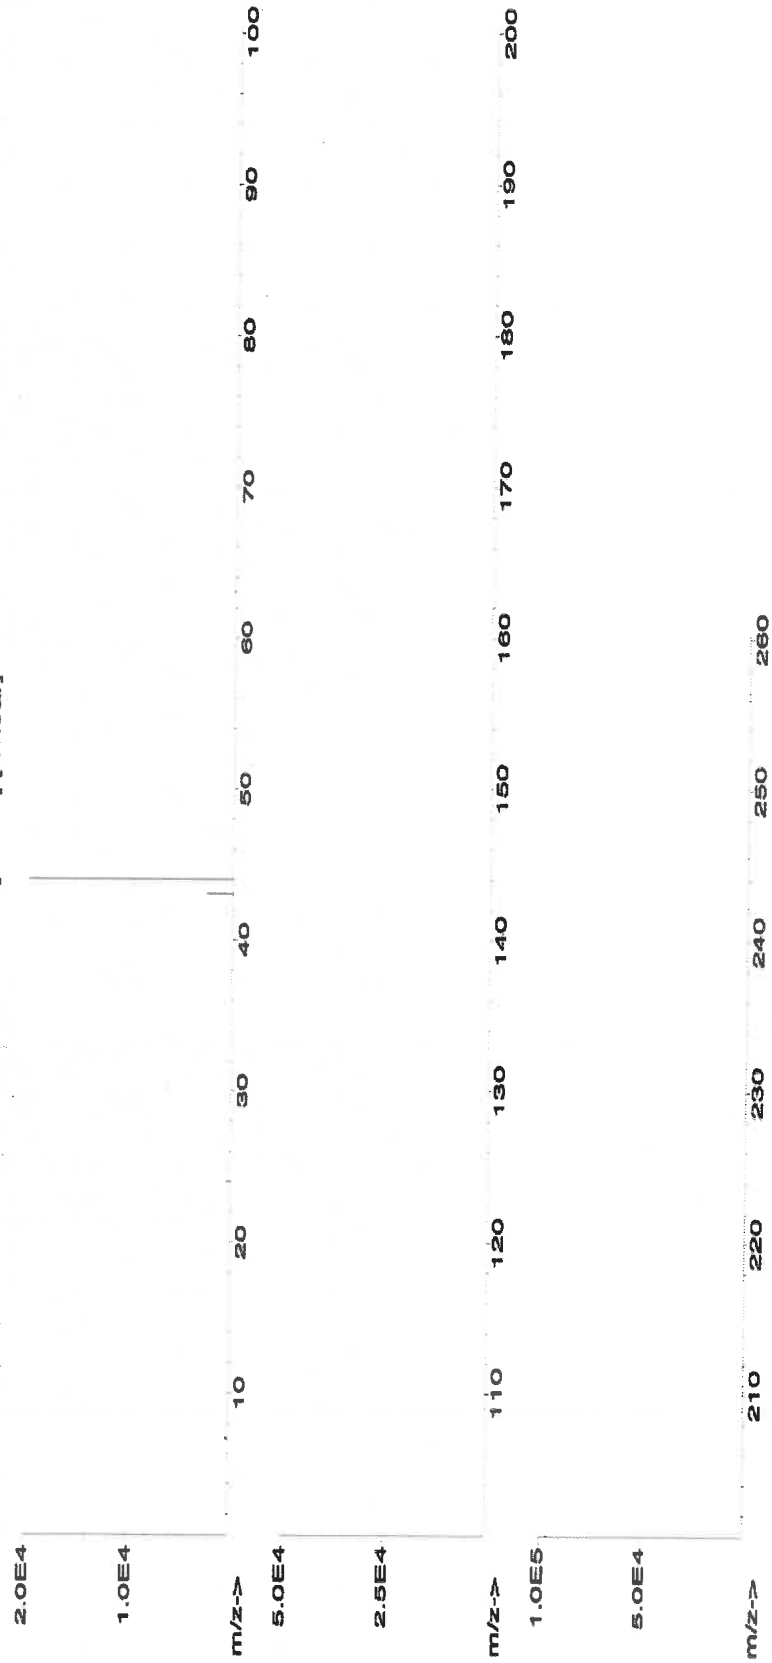



# Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

## Trace Metals Verification by ICP-MS (µg/mL)

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | T     | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Tc | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Ti | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.2  | Fe | <0.02 | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Tl | <0.02 | Zr | <0.02 |

(T) = Target analyte

## Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

**CERTIFIED WEIGHT REPORT:**

**Part Number:**  
**Lot Number:**  
**Description:**

**57182**  
**061522**  
**Lead (Pb)**

**Expiration Date:**  
**Recommended Storage:**  
**Nominal Concentration (µg/mL):**  
**NIST Test Number:**

**061525**  
**Ambient (20 °C)**  
**10000**  
**6UTB**

**Weight shown below was diluted to (mL):**

**2000.02**

**5E-05 Balance Uncertainty**

**0.058 Flask Uncertainty**

**Lot #**

**Solvent:** 20510011 Nitric Acid


**2%** 40.0 Nitric Acid  
(mL)

|                          |                          |
|--------------------------|--------------------------|
| <i>Giovanni Esposito</i> |                          |
| Formulated By:           | Giovanni Esposito 061522 |
| <i>Pedro L. Rentas</i>   |                          |
| Reviewed By:             | Pedro L. Rentas 061522   |

| Compound | RM# | Lot Number | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | SDS Information                        |                |          |
|----------|-----|------------|-----------------------|------------|-----------------|-----------|-------------------|-------------------|----------------------|----------------------------------|--|----------------|----------|
|          |     |            |                       |            |                 |           |                   |                   |                      |                                  | (Solvent Safety Info. On Attached pg.) | OSHA PEL (TWA) | NIST SRM |

|                          |       |             |       |        |      |      |         |         |         |      |            |            |                          |
|--------------------------|-------|-------------|-------|--------|------|------|---------|---------|---------|------|------------|------------|--------------------------|
| 1. Lead(II) nitrate (Pb) | IN029 | PBD12201641 | 10000 | 99.999 | 0.10 | 82.5 | 32.0006 | 32.0041 | 10001.1 | 20.0 | 10098-74-8 | 0.05 mg/m3 | inhalation 88 mg/kg 3128 |
|--------------------------|-------|-------------|-------|--------|------|------|---------|---------|---------|------|------------|------------|--------------------------|

[1] Spectrum No.1 [ 17.284 sec]:58182.D# [Count] [Linear]

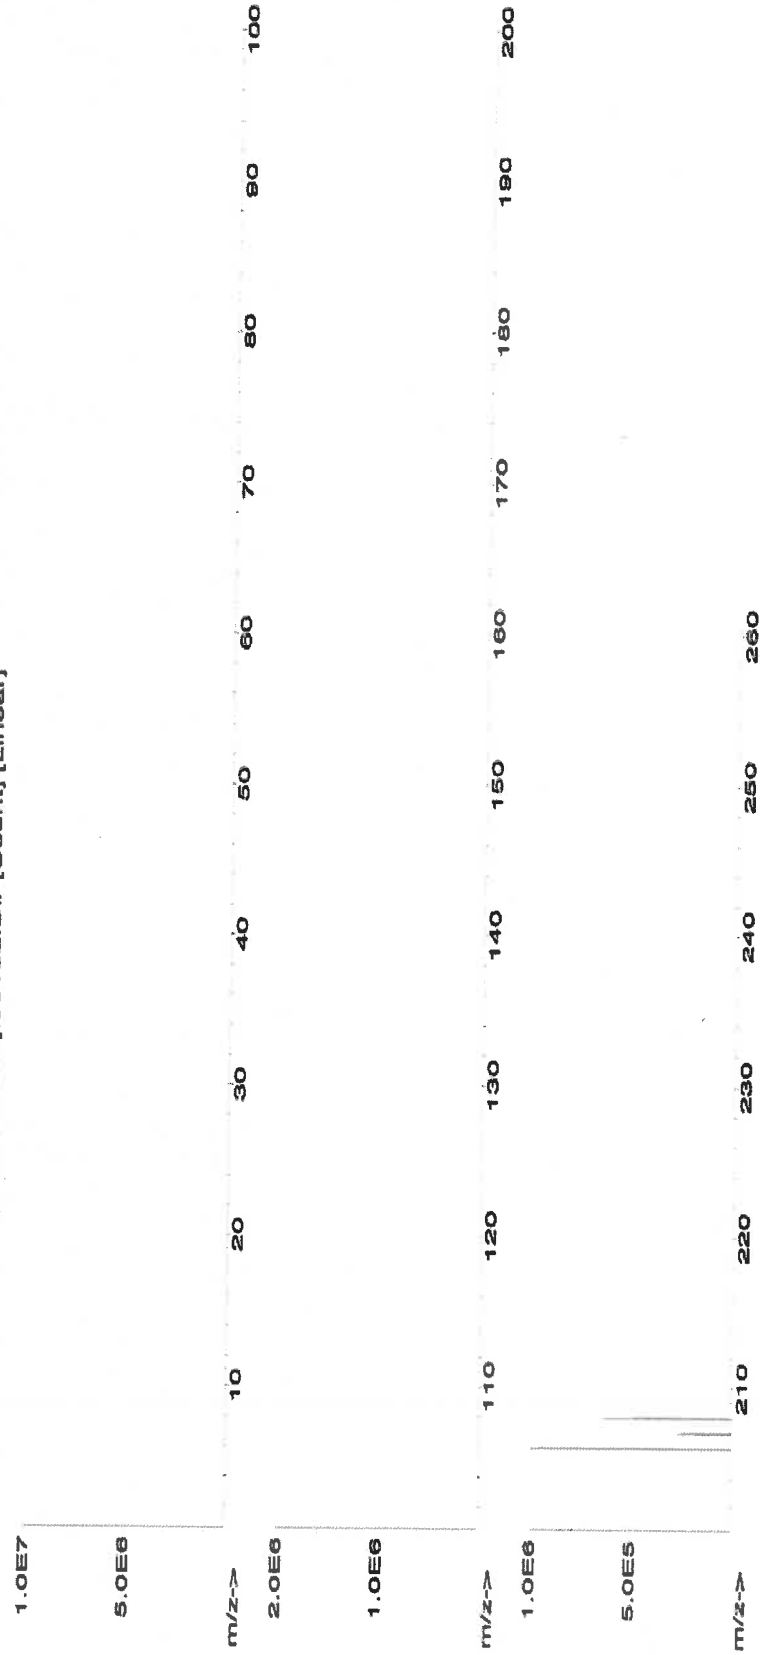



# Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

## Trace Metals Verification by ICP-MS (µg/mL)

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.2  | Fe | <0.02 | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pr | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T)= Target analyte

## Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

*Ben P. Sha*

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

# CORCO CHEMICAL CORPORATION

Manufacturers of ACS Reagents and Semiconductor Grade Chemicals

## CERTIFICATE OF ANALYSIS

Date: 8/3/2022

MS631 MS632 MS633 MS634

Lot No 820803

Hydrogen Peroxide, ACS  
Reagent Grade

| <u>TEST</u>                 | <u>MAXIMUM LIMITS</u>                                | <u>RESULT</u> |
|-----------------------------|--|---------------|
| Appearance                  | Colorless and free from suspended matter or sediment | Pass          |
| Assay                       | 29-32%   | 31.4%         |
| Color (APHA)                | 10   | 5             |
| Residue after Evaporation   | 0.002%   | .0001%        |
| Titrateable Acid            | 0.0006 meq/g   | < .0006 meq/g |
| Chloride (Cl)               | 2 ppm  | < 1 ppm       |
| Nitrate (NO <sub>3</sub> )  | 2 ppm  | < 1 ppm       |
| Phosphate                   | 2 ppm  | < 1 ppm       |
| Sulfate (SO <sub>4</sub> )  | 5 ppm  | < .5 ppm      |
| Ammonium (NH <sub>4</sub> ) | 5 ppm  | < 1 ppm       |
| Heavy Metals (as Pb)        | 1 ppm  | < .1 ppm      |
| Iron (Fe)                   | 0.5 ppm  | < .1 ppm      |
| Sodium Stannate             | 200 – 300 ppb  | Pass          |

\*\*\*Our Hydrogen Peroxide is considered un-stabilized because it is very slightly stabilized with Sodium Stannate, 500 ppb maximum, just for safety purposes.

Date of MFG: 8/2022

Retest date: 8/2024

*Gina M. Rambo*  
Office Manager



**CERTIFIED WEIGHT REPORT:**

Part Number: 58024  
Lot Number: 060523  
Description: Chromium (Cr)

Lot #  
21110221  
Solvent: Nitric Acid


|                |                  |
|----------------|------------------|
|                |                  |
| Formulated By: | Lawrence Barry   |
|                | 060523           |
|                |                  |
| Reviewed By:   | Pedro L. Henrias |
|                | 060523           |

Expiration Date: 060526  
Recommended Storage: Ambient (20 °C)  
Nominal Concentration (µg/mL): 1000  
NIST Test Number: 6UTB  
Volume shown below was diluted to (mL): 2000.02  
5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

| Compound | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|-------------|------------|-----------------|-------------------|------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|
|----------|-------------|------------|-----------------|-------------------|------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|

1. Chromium(III) nitrate nonahydrate (Cr) 58124 071122 0.1000 200.0 0.084 1000 10000.1 1000.0 2.2 7789-02-8 0.5 mg(Cr)/m3 or rat 3250 mg/kg 3112a

[1] Spectrum No.1 [ 31.393 sec]:57024.D# [Count] [Linear]

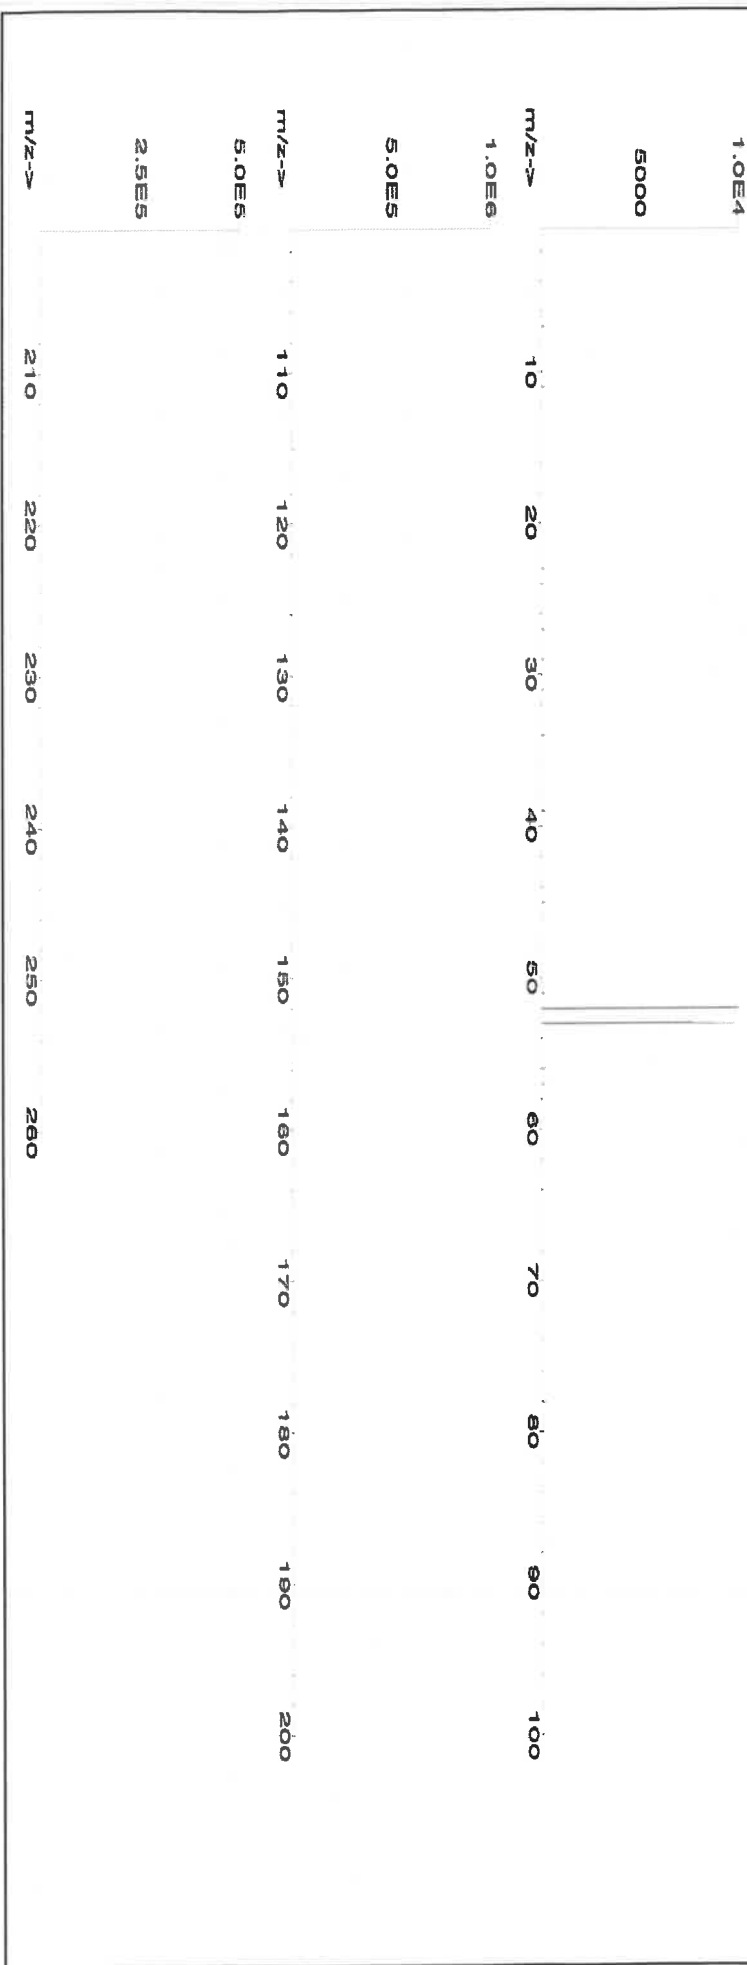





**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | T     | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**CERTIFIED WEIGHT REPORT:**

**Part Number:** 58029  
**Lot Number:** 102523  
**Description:** Copper (Cu)

**Lot #** 24002546  
**Solvent:** Nitric Acid

**Expiration Date:** 102526  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** 1000  
**NIST Test Number:** 6UTB  
**Volume shown below was diluted to (mL):** 2000.02  
**Balance Uncertainty:** 5E-05  
**Flask Uncertainty:** 0.058


|                |                 |
|----------------|-----------------|
|                |                 |
| Formulated By: | Benson Chan     |
|                |                 |
| Reviewed By:   | Pedro L. Rentas |

**SDS Information**

| Compound | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | (Solvent Safety Info. On Attached pg.) CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|---|----------------|------|----------|
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|---|----------------|------|----------|

1. Copper(II) nitrate trihydrate (Cu) 58129 100223 0.1000 200.0 0.084 1000 10000.1 1000.0 2.2 10031-43-3 1 mg/m3 or-rat 794 mg/kg 3114

[1] Spectrum No.1 [ 33.422 sec]:58029.D# [Count] [Linear]

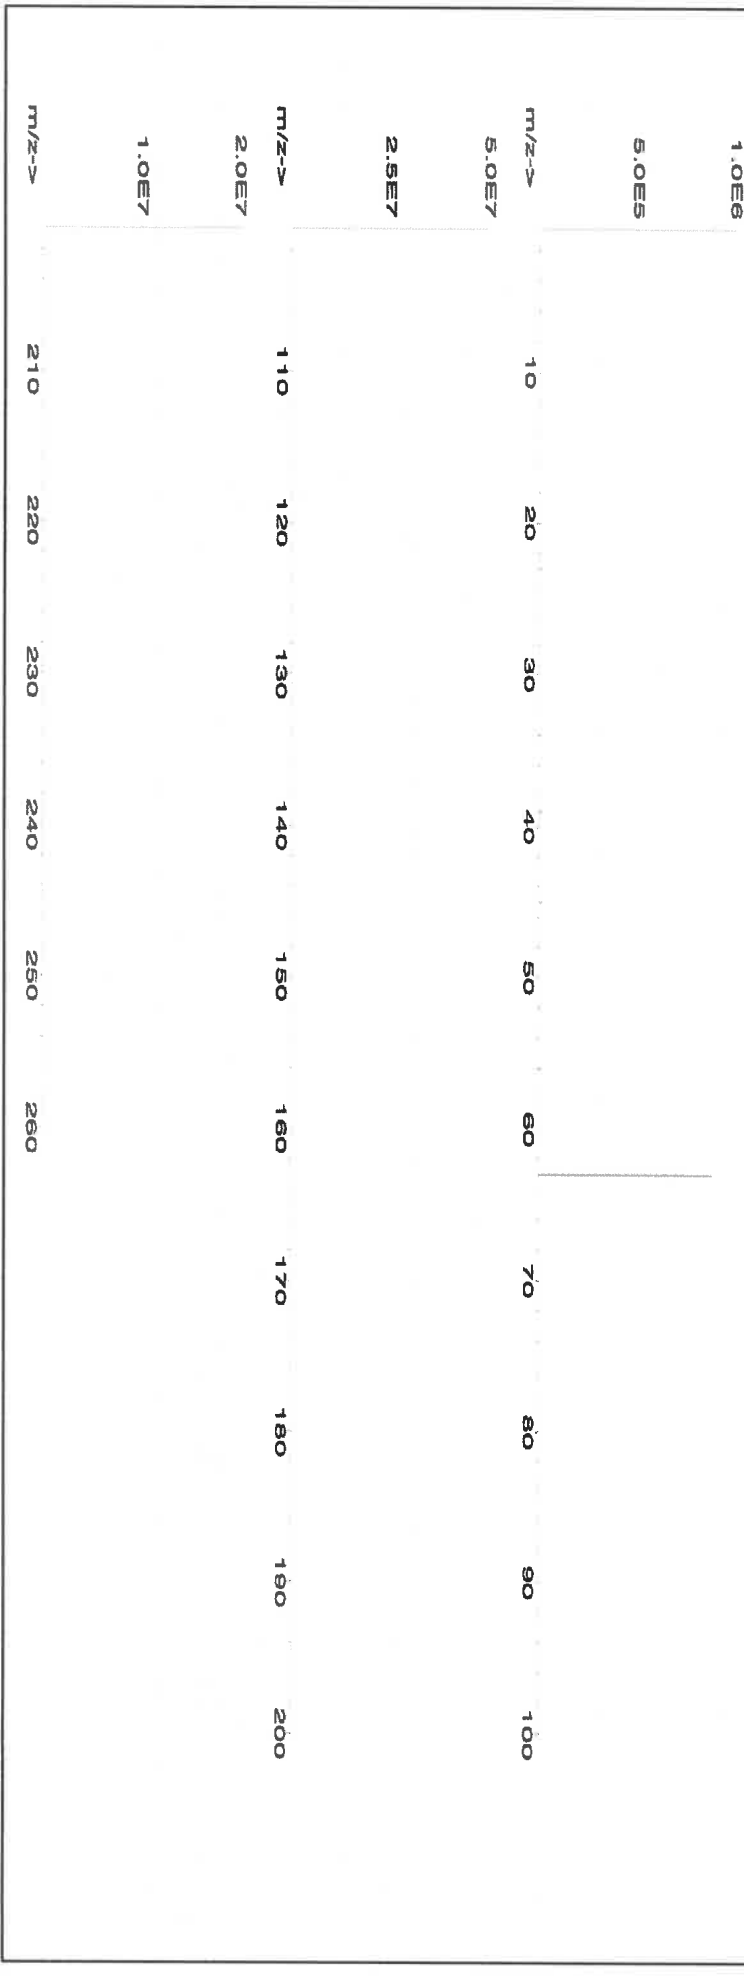



## Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

## Trace Metals Verification by ICP-MS (µg/mL)

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | T     | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

## Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



M5648 R:10123123



**CERTIFIED WEIGHT REPORT:**

Part Number:  
Lot Number:  
Description:

58025  
102623  
Manganese (Mn)

Lot #  
Solvent:

24002546  
Nitric Acid

Expiration Date:

102626

2.0%

60.0  
(mL)

Nitric Acid

Recommended Storage:

Ambient (20 °C)

Nominal Concentration (µg/mL):

1000

NIST Test Number:

6UTB

5E-05

Balance Uncertainty

Volume shown below was diluted to (mL):

3000.41

0.058

Flask Uncertainty


|                |                 |        |
|----------------|-----------------|--------|
| Formulated By: | Benson Chan     | 102623 |
| Reviewed By:   | Pedro L. Ruelas | 102623 |

**Compound**

| Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | SDS Information (Solvent Safety Info. On Attached pg.) | NIST SRM |
|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|--|----------|
|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|--|----------|

1. Manganese(II) nitrate tetrahydrate (Mn) 58125 071123 0.1000 300.0 0.084 1000 10000.1 1000.0 2.1 20694-39-7 5 mg/m3 or-rel>300mg/kg 3132

[1] Spectrum No.1 [34.243 sec]:57025.D# [Count] [Linear]

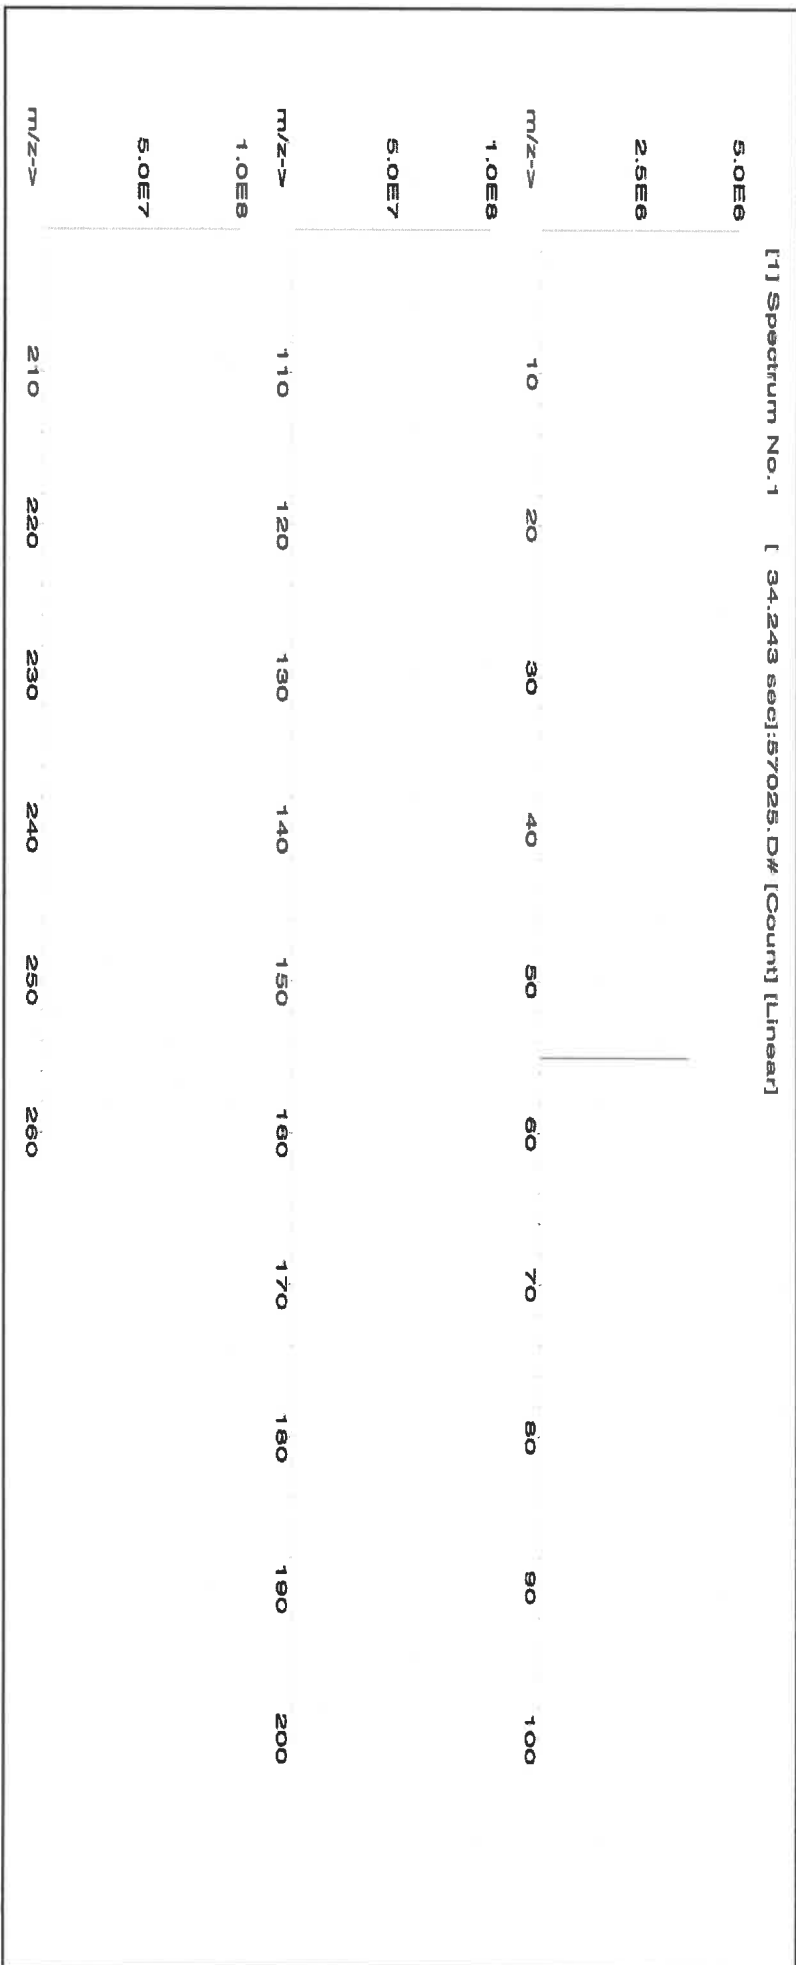



## Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

## Trace Metals Verification by ICP-MS (µg/mL)

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | T     | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

## Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**CERTIFIED WEIGHT REPORT:**

**Part Number:** 57082  
**Lot Number:** 100923  
**Description:** Lead (Pb)

**Solvent:** 24002546 Nitric Acid

**Lot #**

R: 12/20/23 MS747

|                |                 |
|----------------|-----------------|
|                |                 |
| Formulated By: | Lawrence Barry  |
|                | 100923          |
|                |                 |
| Reviewed By:   | Pedro L. Rentas |
|                | 100923          |

**Expiration Date:** 100926  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** 1000  
**NIST Test Number:** 6UTB


**2% 60.0 (mL) Nitric Acid**

**Weight shown below was diluted to (mL):** 3000.41  
**5E-05 Balance Uncertainty**  
**0.06 Flask Uncertainty**

| Compound | RM# | Lot Number | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty Purity (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|-----|------------|-----------------------|------------|------------------------|-----------|-------------------|-------------------|----------------------|----------------------------------|------|----------------|------|----------|
|----------|-----|------------|-----------------------|------------|------------------------|-----------|-------------------|-------------------|----------------------|----------------------------------|------|----------------|------|----------|

1. Lead(II) nitrate (Pb) IN029 PB0122016A1 1000 99.999 0.10 62.5 4.80071 4.80077 1000.0 2.0 10099-74-8 0.05 mg/m3 Intvms-ret 89 mg/kg 3128

[1] Spectrum No. 1 [ 14.144 sec]:58082.D# [Count] [Linear]

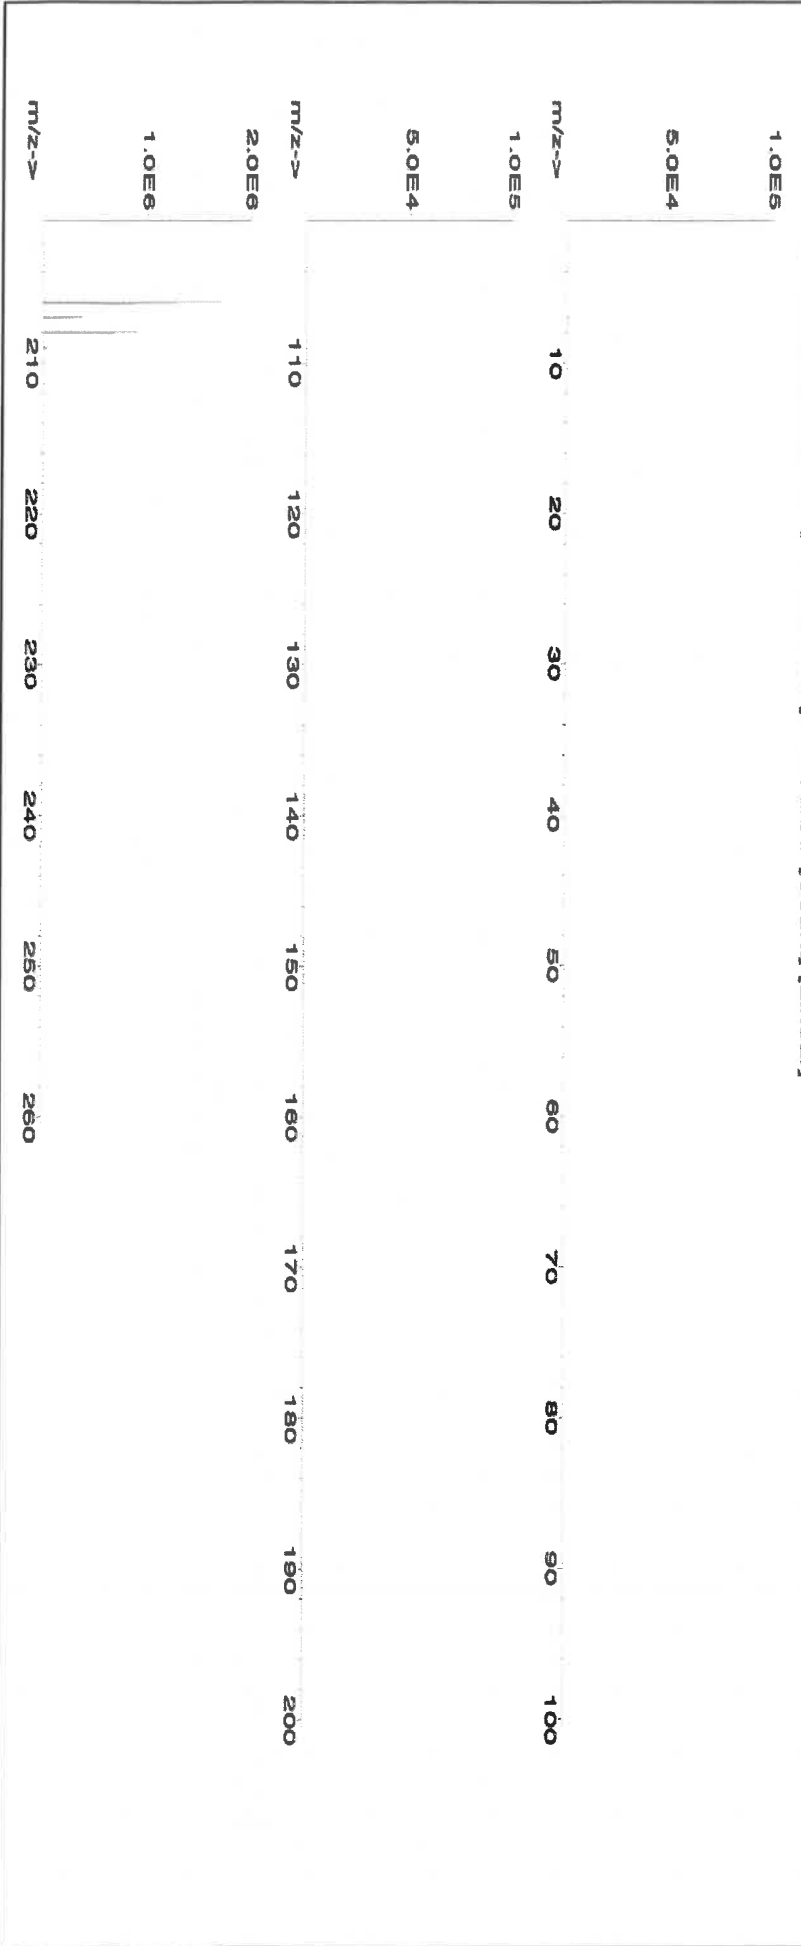



## Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS ( $\mu\text{g/mL}$ )

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Ba | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

## Physical Characterization:

(T) = Target analyte

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



R:12/15/23 M5752 M5753 M5754 M5755



CERTIFIED WEIGHT REPORT:

Part Number: 52166  
Lot Number: 112823  
Description: ILM 05.3 ICP-AES Spike Sample  
Expiration Date: 112826  
Recommended Storage: 18 Components - Water Matrix  
Nominal Concentration (µg/mL): Ambient (20 °C)  
NIST Test Number: Varied  
Volumes shown below were diluted to (mL): 5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

Lot # 24002546  
Solvent: Nitric Acid


5.0% 25.0 (mL) Nitric Acid

|                |                   |
|----------------|-------------------|
| Formulated By: | Giovanni Esposito |
| Reviewed By:   | Pedro L. Renteria |

| Compound | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | SDS Information (Solvent Safety Info. On Attached pg.) | LD50 | NIST SM |
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|--|------|---------|
|----------|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|--|------|---------|

|   |       |        |        |       |       |     |         |       |      |            |              |                         |
|---|-------|--------|--------|-------|-------|-----|---------|-------|------|------------|--------------|-------------------------|
| 1. Aluminum nitrate nonahydrate (Al)        | 58113 | 071123 | 0.0200 | 10.0  | 0.042 | 200 | 10000.1 | 200.0 | 1.7  | 7784-27-2  | 2 mg/m3      | or-rel 3671 mg/kg 3101a |
| 2. Arsenic (As)                             | 57051 | 041823 | 0.0100 | 5.00  | 0.017 | 10  | 1000.0  | 10.0  | 0.07 | 7440-38-0  | 0.5 mg/m3    | or-rel 7000 mg/kg 3102a |
| 3. Barium nitrate (Ba)                      | 58156 | 050222 | 0.0200 | 10.0  | 0.042 | 200 | 10000.1 | 200.0 | 1.7  | 10022-31-8 | 0.5 mg/m3    | or-rel 355 mg/kg 3104a  |
| 4. Beryllium nitrate (Be)                   | 57004 | 102523 | 0.0050 | 2.50  | 0.017 | 5   | 1000.0  | 5.00  | 0.07 | 13697-99-4 | 0.2 µg/m3    | or-rel 3126a            |
| 5. Cadmium nitrate tetrahydrate (Cd)        | 57048 | 071123 | 0.0050 | 2.50  | 0.017 | 5   | 1001.5  | 5.00  | 0.07 | 10022-68-1 | 0.01 mg/m3   | or-rel 60.2 mg/kg 3108  |
| 6. Chromium(III) nitrate nonahydrate (Cr)   | 57024 | 060523 | 0.0200 | 10.0  | 0.042 | 20  | 1000.0  | 20.0  | 0.17 | 7789-02-8  | 0.5 mg/Cr/m3 | or-rel 3250 mg/kg 3112a |
| 7. Cobalt(II) nitrate hexahydrate (Co)      | 58127 | 050923 | 0.0050 | 2.50  | 0.017 | 50  | 10000.0 | 50.0  | 0.7  | 10026-22-9 | 0.02 mg/m3   | or-rel 681 mg/kg 3113   |
| 8. Copper(II) nitrate trihydrate (Cu)       | 57029 | 102523 | 0.0250 | 12.50 | 0.084 | 25  | 1000.0  | 25.0  | 0.3  | 10031-43-3 | 1 mg/m3      | or-rel 794 mg/kg 3114   |
| 9. Iron (Fe)                                | 58126 | 051523 | 0.0100 | 5.00  | 0.017 | 100 | 10001.5 | 100.0 | 0.7  | 7439-89-6  | 5 mg/m3      | or-rel 7500 mg/kg 3126a |
| 10. Lead(II) nitrate (Pb)                   | 57282 | 101223 | 0.0200 | 10.0  | 0.042 | 2   | 100.0   | 2.00  | 0.02 | 10099-74-8 | 0.05 mg/m3   | or-rel 83 mg/kg 3128    |
| 11. Manganese(II) nitrate tetrahydrate (Mn) | 58125 | 071123 | 0.0050 | 2.50  | 0.017 | 50  | 10000.1 | 50.0  | 0.7  | 20894-39-7 | 5 mg/m3      | or-rel >300 mg/kg 3132  |
| 12. Nickel(II) nitrate hexahydrate (Ni)     | 58128 | 062023 | 0.0050 | 2.50  | 0.017 | 50  | 10000.4 | 50.0  | 0.7  | 13478-00-7 | 1 mg/m3      | or-rel 1620 mg/kg 3136  |
| 13. Selenium(IV) oxide (Se)                 | 57034 | 040123 | 0.0050 | 2.50  | 0.017 | 5   | 1000.0  | 5.00  | 0.07 | 7446-08-4  | 0.2 mg/m3    | or-rel 68 mg/kg 3149    |
| 14. Silver nitrate (Ag)                     | 57047 | 071123 | 0.0050 | 2.50  | 0.017 | 5   | 1000.6  | 5.00  | 0.07 | 7761-88-6  | 10 µg/m3     | NA 3151                 |
| 15. Thallium nitrate (Tl)                   | 57081 | 061322 | 0.0050 | 2.50  | 0.017 | 5   | 1000.0  | 5.00  | 0.07 | 10102-45-1 | 5 mg/m3      | or-rel 6700 mg/kg 3158  |
| 16. Ammonium metavanadate (V)               | 58123 | 082823 | 0.0050 | 2.50  | 0.017 | 50  | 10000.0 | 50.0  | 0.7  | 7803-55-6  | 0.05 mg/m3   | or-rel 58.1 mg/kg 3165  |
| 17. Zinc nitrate hexahydrate (Zn)           | 58130 | 063023 | 0.0050 | 2.50  | 0.017 | 50  | 10000.0 | 50.0  | 0.7  | 10196-18-6 | 1 mg/m3      | or-rel 1190 mg/kg 3168  |



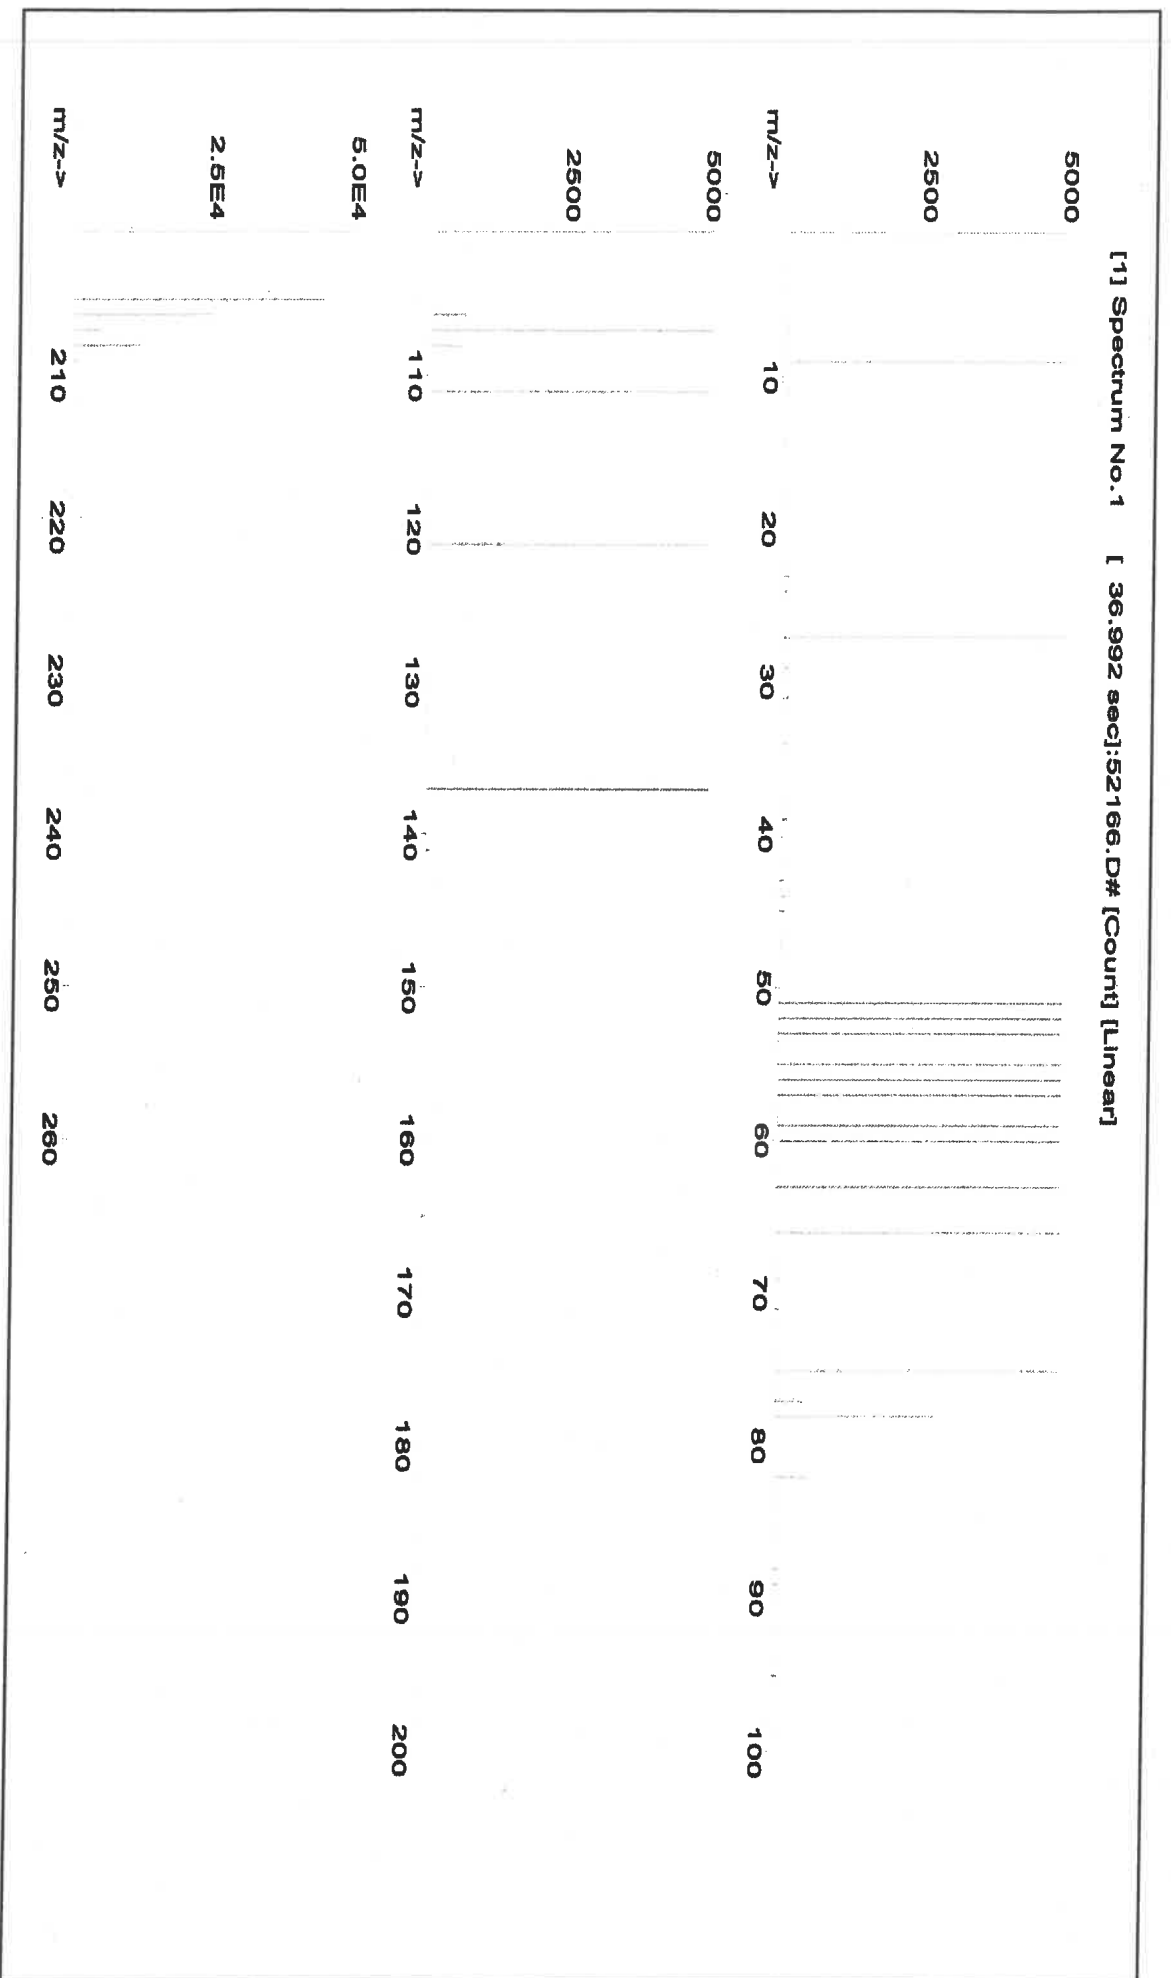



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | T     | Cd | T     | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | T     | Pt | <0.02 | Se | T     | Tb | <0.02 | W  | <0.02 |
| Sb | T     | Ce | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Tc | <0.02 | U  | <0.02 |
| As | T     | Ce | <0.02 | Bu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | T     | Tl | T     | V  | T     |
| Ba | T     | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | T     | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | T     | Cr | T     | Ga | <0.02 | Fe | T     | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | T     | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | T     |
| B  | <0.02 | Cu | T     | Au | <0.02 | Pb | T     | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homoogeneity: No heterogeneity was observed in the preparation of this standard.

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



M5768 M5769  
Certified Reference Material CRM  
R: 1/13/24



**CERTIFIED WEIGHT REPORT:**

Part Number:  
Lot Number:  
Description:

58112  
091823  
Magnesium (Mg)

Solvent: 24002546 Nitric Acid

Lot #

Expiration Date:

091826

2% 40.0 (mL) Nitric Acid

Recommended Storage:

Ambient (20 °C)

Nominal Concentration (µg/mL):

10000

NIST Test Number:

6UTB

5E-05 Balance Uncertainty

R: 1/13/24

Weight shown below was diluted to (mL): 2000.02 0.058 Flask Uncertainty

**Compound**

RW#

Lot

Nominal

Purity (%)

Uncertainty (%)

Assay (%)

Target

Actual

Weight (g)

Actual

Expanded

Uncertainty

CAS#

OSHA PEL (TWA)


LD50

SRM

**SDS Information**

1. Magnesium nitrate hexahydrate (Mg) IN030 M500222A1 10000 99.999 0.10 8.51 234.9118 234.9126 10000.0 20.0 13446-18-9 NA or-rat 5440 mg/kg 3131a

[1] Spectrum No. 1 [ 19.923 sec]: 58112.D# [Count] [Linear]

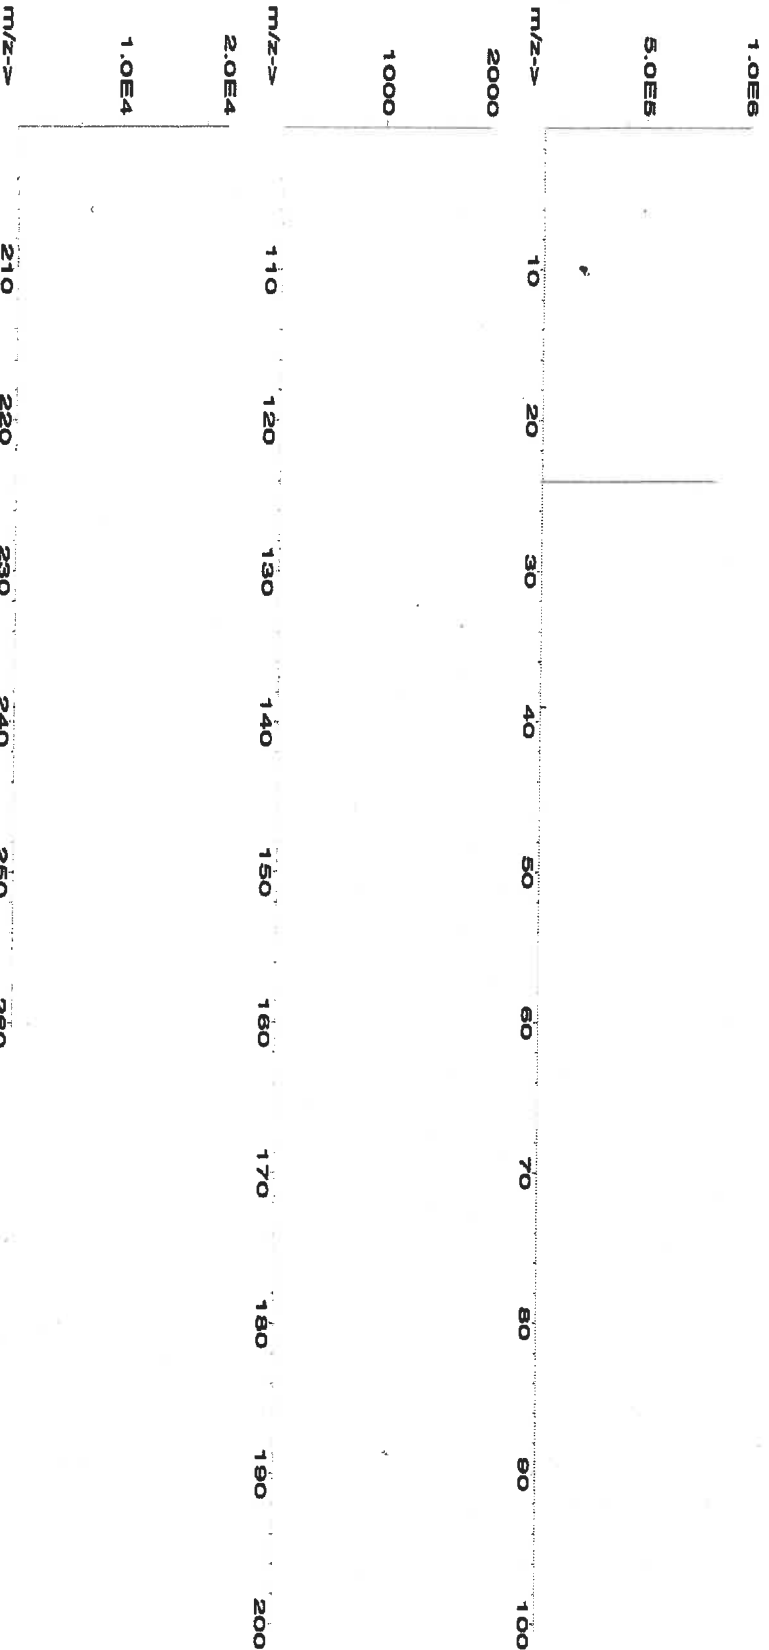



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | T     | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



M5768 M5769  
Certified Reference Material CRM  
R: 1/13/24



ANAB ISO 17034 Accredited  
AR-1539 Certificate Number  
https://AbsoluteStandards.com

**CERTIFIED WEIGHT REPORT:**

Part Number: 58112  
Lot Number: 091823  
Description: Magnesium (Mg)

Solvent: 24002546 Nitric Acid

Lot #

Expiration Date: 091826  
Recommended Storage: Ambient (20 °C)  
Nominal Concentration (µg/mL): 10000  
NIST Test Number: 6UTB  
Weight shown below was diluted to (mL): 2000.02 0.058 Flask Uncertainty

2% 40.0 (mL) Nitric Acid

M5768 M5769  
BP R: 1/13/24


|                                      |  |        |
|--------------------------------------|--|--------|
| Formulated By: <i>Lawrence Barry</i> |  | 091823 |
| Reviewed By: <i>Pedro L. Rentas</i>  |  | 091823 |

**Compound**

| Lot | Nominal | Purity        | Uncertainty | Assay      | Target     | Actual     | Actual        | Expanded    | SDS Information                        | NIST |
|-----|---------|---------------|-------------|------------|------------|------------|---------------|-------------|--|------|
| RW# | Number  | Conc. (µg/mL) | (%)         | Purity (%) | Weight (g) | Weight (g) | Conc. (µg/mL) | +/- (µg/mL) | (Solvent Safety Info. On Attached pg.) | SRM  |

1. Magnesium nitrate hexahydrate (Mg) IN030 M500222A1 10000 99.999 0.10 8.51 234.9118 234.9126 10000.0 20.0 13446-18-9 NA or-rat 5440 mg/kg 3131a

[1] Spectrum No. 1 [ 19.923 sec]: 58112.D# [Count] [Linear]

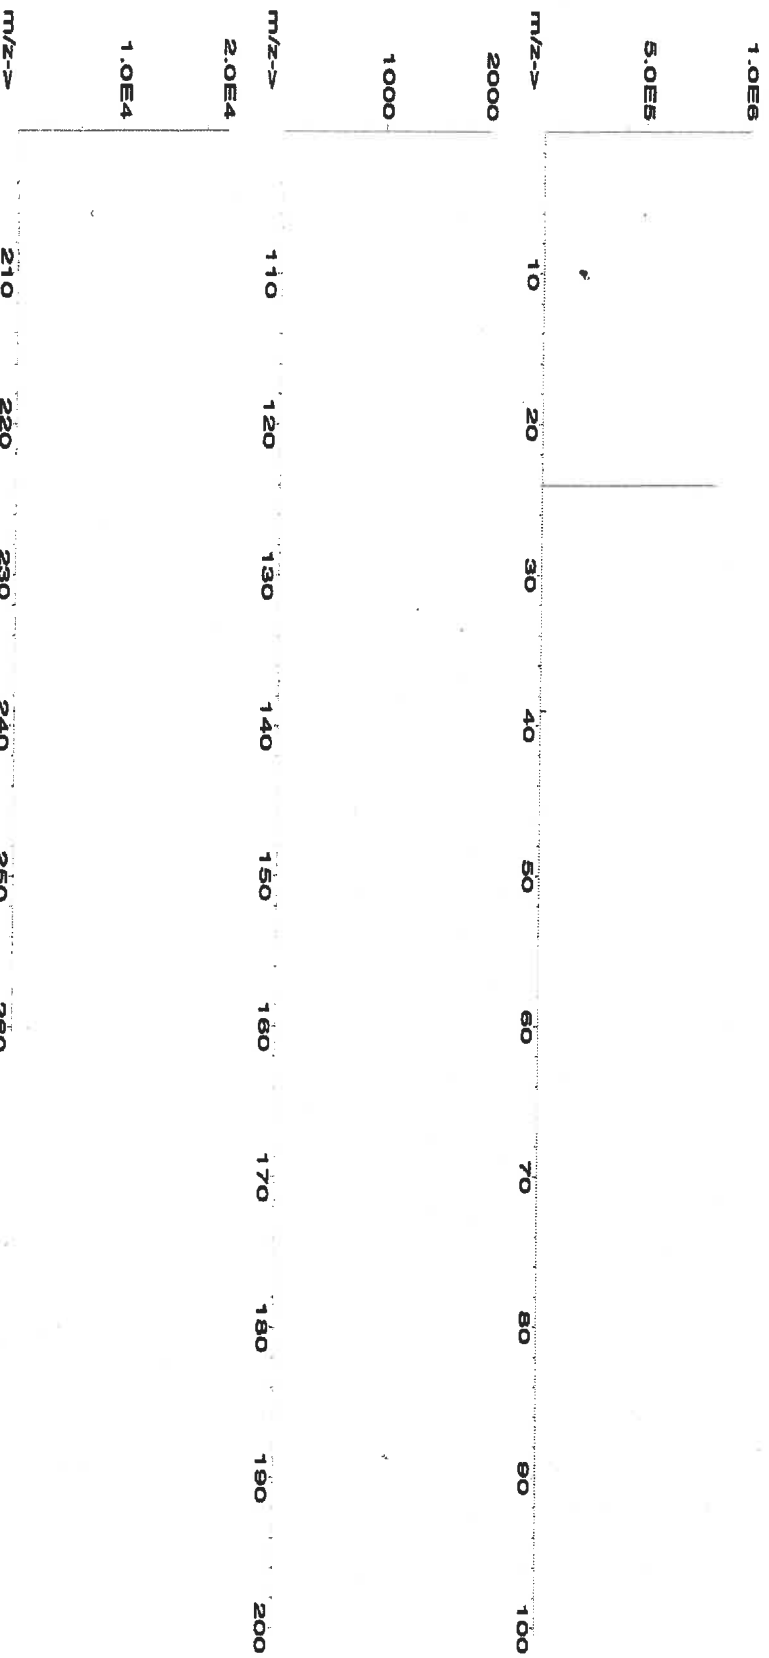



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | T     | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**CERTIFIED WEIGHT REPORT:**

Part Number: **57004**  
Lot Number: **102523**  
Description: **Beryllium (Be)**

Lot # **24002546**  
Solvent: **Nitric Acid**

**Expiration Date:**

102526

**Recommended Storage:**

Ambient (20 °C)

**Nominal Concentration (µg/mL):**

1000

**NIST Test Number:**

6UTB

Volume shown below was diluted to (mL): 2000.02

5E-05 Balance Uncertainty

0.058 Flask Uncertainty

2.0%

40.0 (mL)


Nitric Acid

|                |                 |        |
|----------------|-----------------|--------|
| Formulated By: | Benson Chan     | 102523 |
| Reviewed By:   | Pedro L. Rentas | 102523 |

**SDS Information**

| Compound | Part Number | Lot | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|-------------|-----|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|
|----------|-------------|-----|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|

1. Beryllium nitrate (Be) 58104 091423 0.1000 200.0 0.084 1000 10001.5 1000.0 2.2 13597-99-4 0.2µg/m3 Inj/mg-rat 3.16mg/kg NA

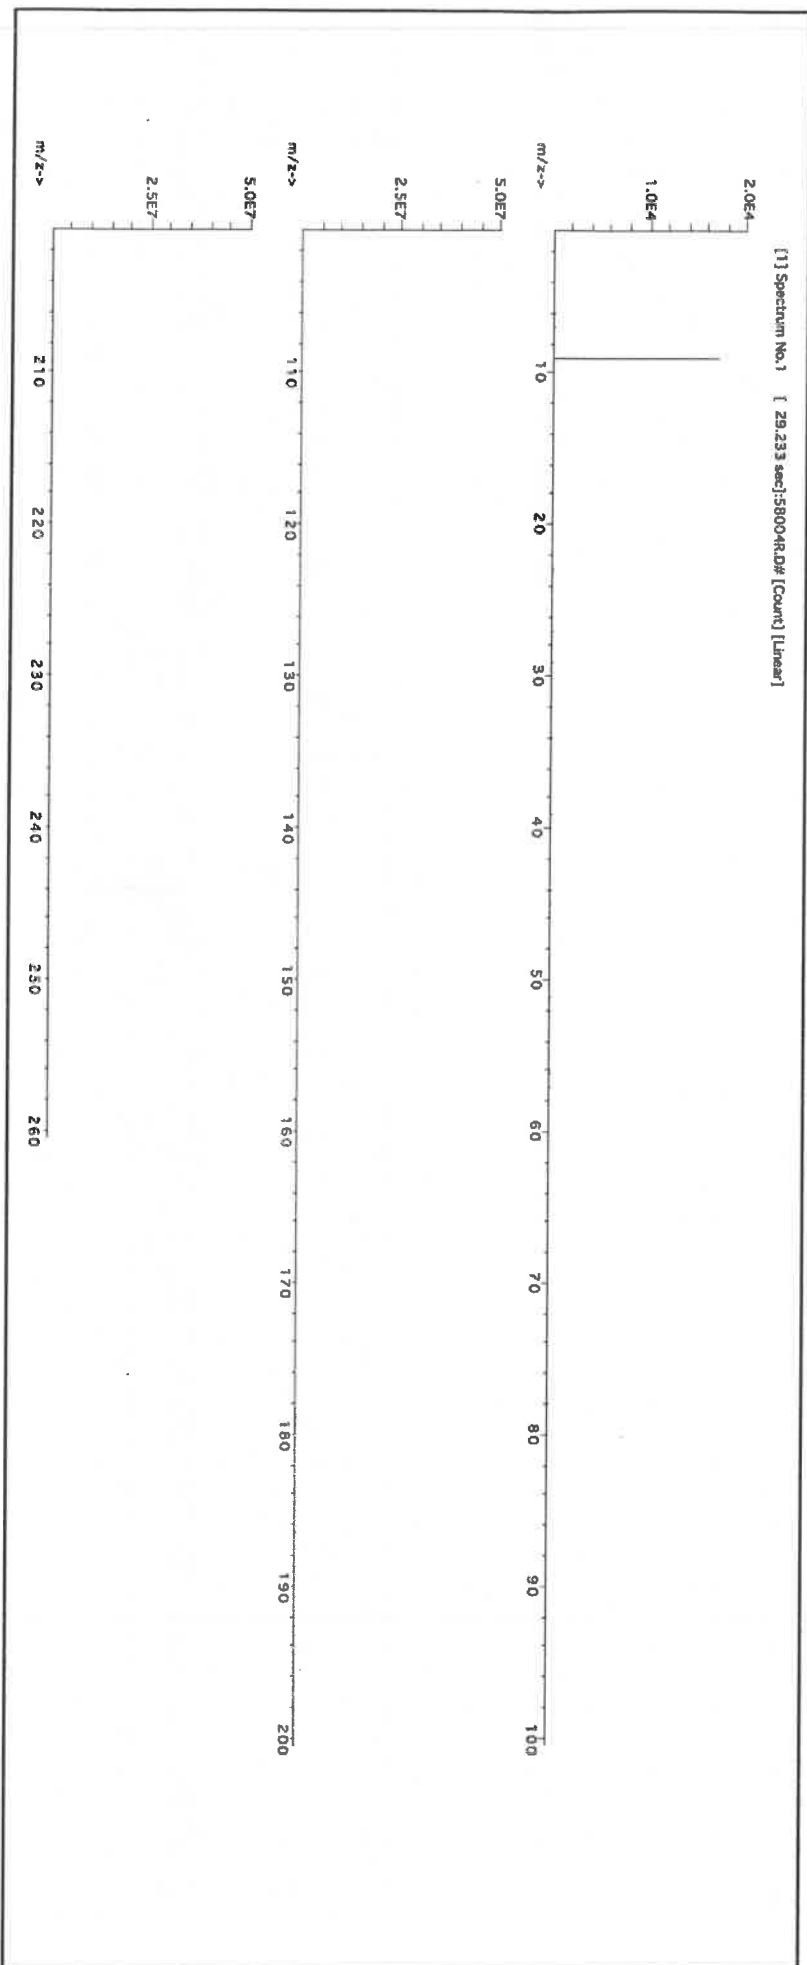



## Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS ( $\mu\text{g/mL}$ )

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Tc | <0.02 | U  | <0.02 |
| As | <0.02 | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Ti | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | T     | Cr | <0.02 | Ga | <0.02 | Fe | <0.02 | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.02 | Sc | <0.02 | Ta | <0.02 | Tl | <0.02 | Zr | <0.02 |

(T) = Target analyte

## Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

\* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
 \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.

\* All standard containers are meticulously cleaned prior to use.

\* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).

\* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.

\* All Standards should be stored with caps tight and under appropriate laboratory conditions.

\* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).





Certified Reference Material CRM

CERTIFIED WEIGHT REPORT:


Part Number: 57050  
Lot Number: 071123  
Description: Tin (Sn)

Solvents: 21110221 Nitric Acid  
22D0562008 Hydrochloric acid

Lot #

R-02509124

M599




Expiration Date: 071126  
Recommended Storage: Ambient (20 °C)  
Nominal Concentration (µg/mL): 1000  
NIST Test Number: 6UTB  
Weight shown below was diluted to (mL): 499.93  
5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

|                |                  |        |
|----------------|------------------|--------|
| Formulated By: | Benson Chan      | 071123 |
| Reviewed By:   | Pedro L. Rientas | 071123 |

| SDS Information |        |                       |            |                 |           |                   |                   |                      |                          |  |  |  |
|-----------------|--------|-----------------------|------------|-----------------|-----------|-------------------|-------------------|----------------------|--------------------------|--|--|--|
| Compound        | Lot    | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty (%) | NIST                                   |  |  |
|                 |        |                       |            |                 |           |                   |                   |                      |                          | (Solvent Safety Info. On Attached pg.) |  |  |
| RM#             | Number |                       |            |                 |           |                   |                   |                      |                          |  |  |  |

1. Ammonium hexafluoroantimonate(V) (Sn) IN010 SMD042023A1 1000 99.999 0.10 44.2 1.13107 1.13286 1001.6 2.0 16919-24-7 7 mg/m3 NA 3161a

[1] Spectrum No. 1 [ 15.034 sec]:56150.D# [Count] [Linear]

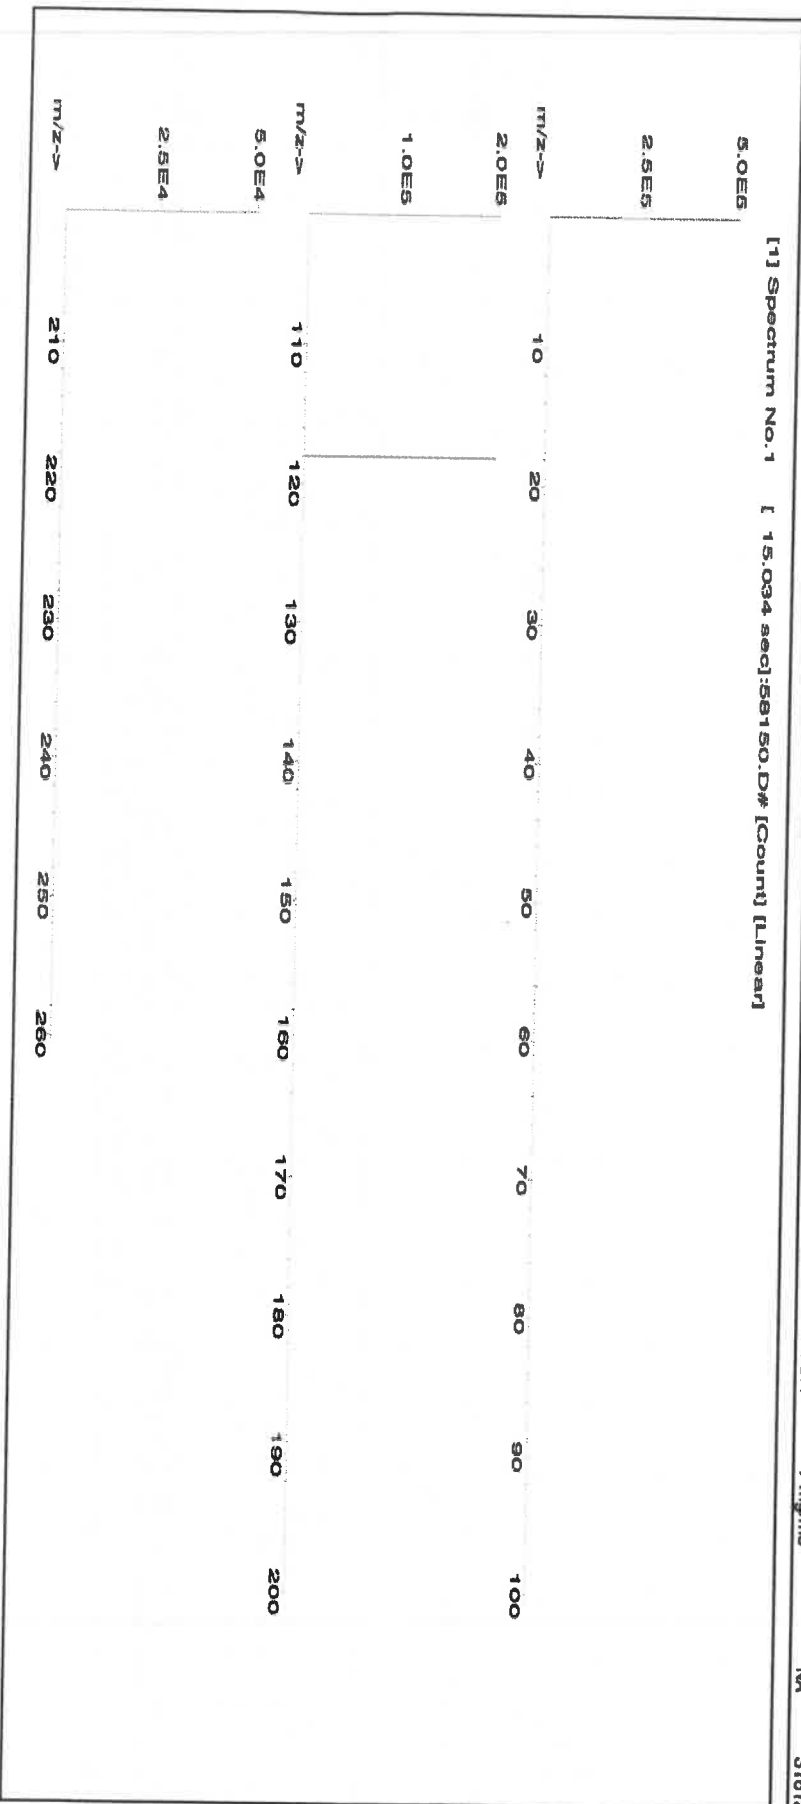



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Ti | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <500  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Ta | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



R: 02/09/24 115800 (54)

CERTIFIED WEIGHT REPORT:

Part Number: 57027  
Lot Number: 091923  
Description: Cobalt (Co)

Expiration Date: 091926  
Recommended Storage: Ambient (20 °C)  
Nominal Concentration (µg/mL): 1000  
NIST Test Number: 6UTB

Volume shown below was diluted to (mL): 2000.02

5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

Lot # 24002546  
Solvent: Nitric Acid

2.0% Nitric Acid  
40.0 (mL)


|                |                 |
|----------------|-----------------|
|                |                 |
| Formulated By: | Lawrence Barry  |
|                |                 |
| Reviewed By:   | Pedro L. Rentas |

SDS Information

Expanded Uncertainty +/- (µg/mL)  
Final Conc. (µg/mL)  
Initial Conc. (µg/mL)  
Nominal Conc. (µg/mL)  
Pipette (mL)  
Initial Vol. (mL)  
Dilution Factor  
Part Number  
Lot Number

(Solvent Safety Info. On Attached pg.)  
CAS#  
OSHA PEL (TWA)  
LD50  
NIST  
SRM

1. Cobalt(II) nitrate hexahydrate (Co) 58127 050923 0.1000 200.0 0.084 1000 10000.0 1000.0 2.2 10026-22-9 0.02 mg/m3 orl-rat 691 mg/kg 3113

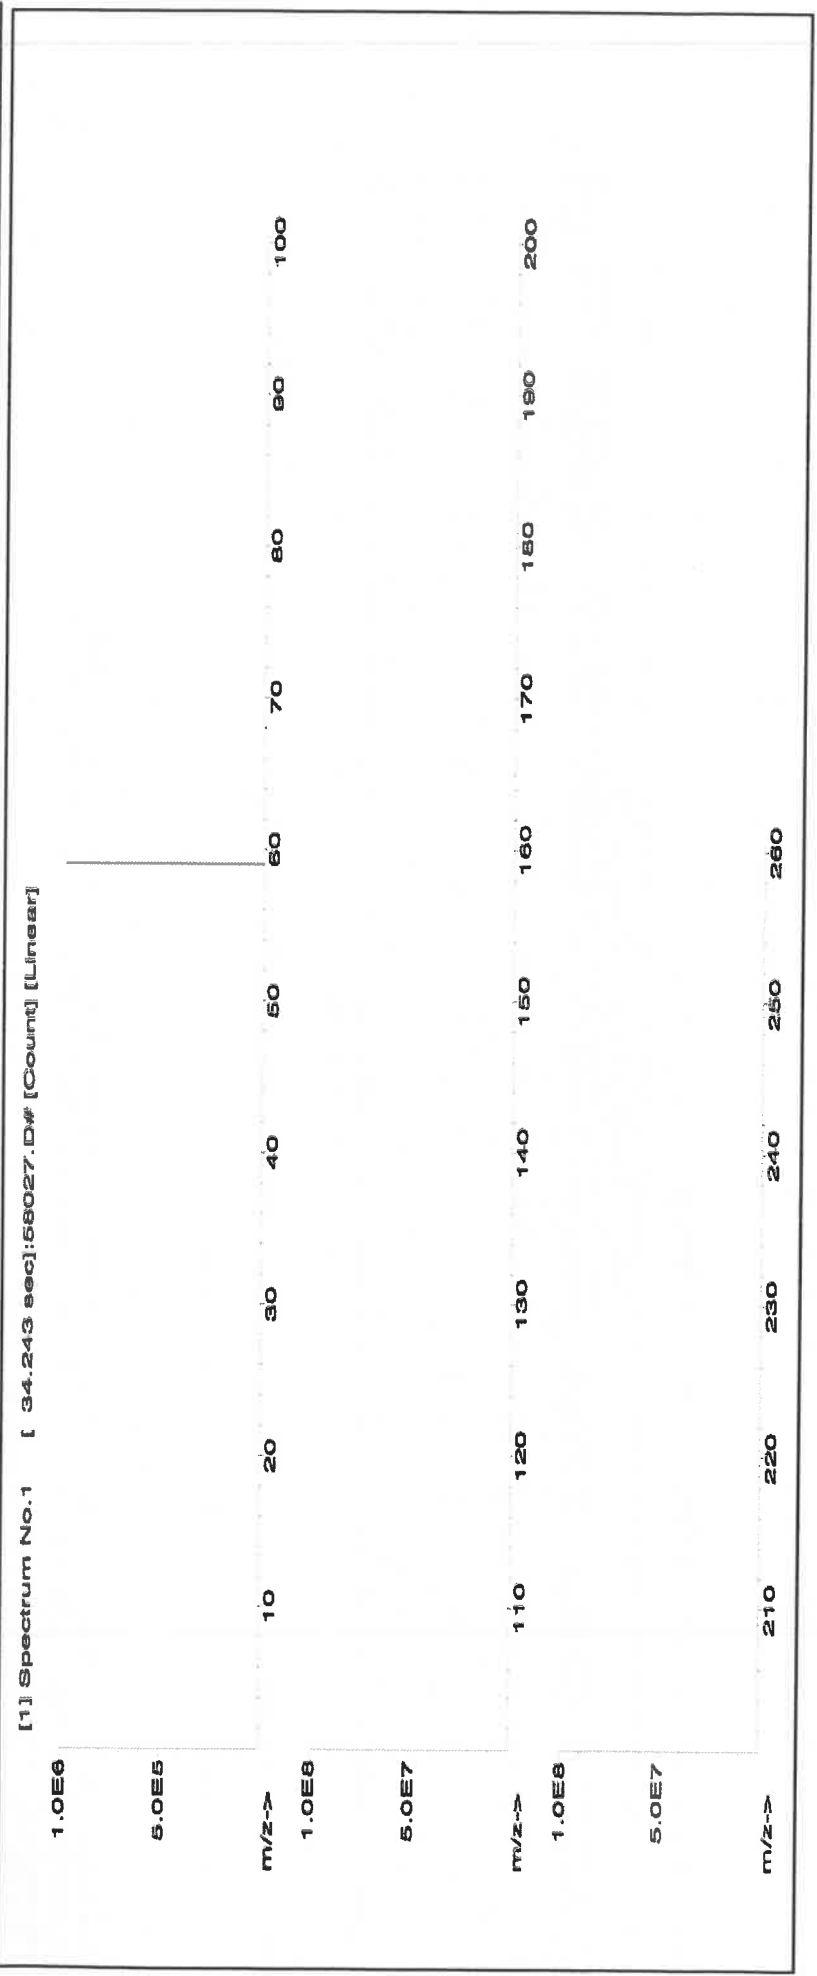



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.02 | Os | <0.01 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.2  | Na | <0.02 | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | T     | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.2  | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T)= Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

**Certified by:**

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**CERTIFIED WEIGHT REPORT:**

**Part Number:**  
**Lot Number:**  
**Description:**

**57033**  
**111323**  
**Arsenic (As)**

**Lot #**  
**Solvent:**

**24002546**  
**Nitric Acid**

**2.0%**

**80.0**

**Nitric Acid**

**Expiration Date:**  
**Recommended Storage:**  
**Nominal Concentration (µg/mL):**

**111326**  
**Ambient (20 °C)**  
**1000**

**NIST Test Number:**  
**Volume shown below was diluted to (mL):**

**6UTB**  
**4000.0**

**5E-05**

**Balance Uncertainty**

**0.06**

**Flask Uncertainty**


|                |                 |
|----------------|-----------------|
|                |                 |
| Formulated By: | Lawrence Barry  |
| Reviewed By:   | Pedro L. Rendas |
|                | 111323          |

**Compound**

| Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Nominal Conc. (µg/mL) | Initial Conc. (µg/mL) | Final Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|
|-------------|------------|-----------------|-------------------|--------------------------|-----------------------|-----------------------|---------------------|----------------------------------|------|----------------|------|----------|

|                 |       |        |        |       |       |      |         |        |     |           |           |                  |       |
|-----------------|-------|--------|--------|-------|-------|------|---------|--------|-----|-----------|-----------|------------------|-------|
| 1. Arsenic (As) | 58133 | 020522 | 0.1000 | 400.0 | 0.084 | 1000 | 10001.0 | 1000.0 | 2.0 | 7440-38-2 | 0.5 mg/m3 | or-rat 500 mg/kg | 3103a |
|-----------------|-------|--------|--------|-------|-------|------|---------|--------|-----|-----------|-----------|------------------|-------|

[1] Spectrum No.1 [34.433 sec]:57033.D# [Count] [Linear]

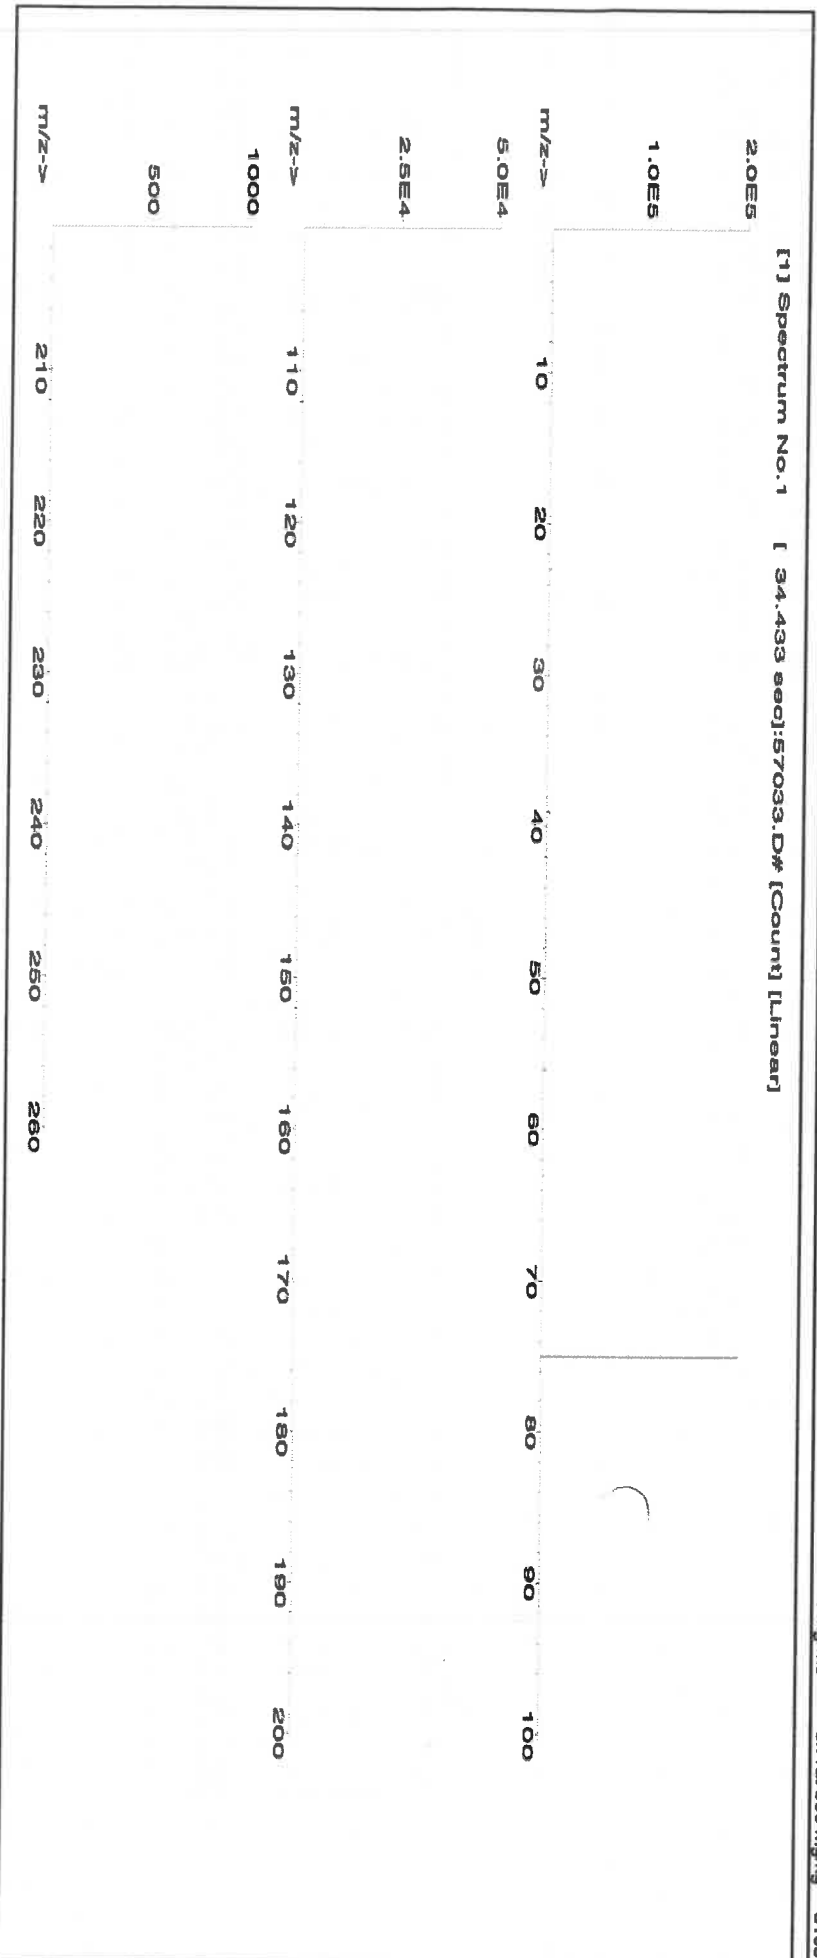



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

**Trace Metals Verification by ICP-MS ( $\mu\text{g/mL}$ )**

|    |       |    |       |                 |       |    |       |    |       |    |       |    |       |    |       |                 |       |    |       |
|----|-------|----|-------|-----------------|-------|----|-------|----|-------|----|-------|----|-------|----|-------|-----------------|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy              | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb              | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er              | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te              | <0.02 | U  | <0.02 |
| As | T     | Ce | <0.02 | Eu              | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl              | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd              | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Tl <sub>h</sub> | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga              | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm              | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge <sup>*</sup> | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn              | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au              | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti              | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**CERTIFIED WEIGHT REPORT:**

**Part Number:** 57115  
**Lot Number:** 041723  
**Description:** Phosphorous (P)

**Solvent:** 21110221 Nitric Acid

**Lot #**

R102109124 M5815

**Expiration Date:** 041726  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** 10000  
**NIST Test Number:** 6UTB

**2% 40.0 (mL) Nitric Acid**


**Weight shown below was diluted to (mL):** 2000.02 0.058 Balance Uncertainty Flask Uncertainty

|                                      |               |
|--------------------------------------|---------------|
|                                      |               |
| <b>Formulated By:</b> Lawrence Barry | <b>041723</b> |
|                                      |               |
| <b>Reviewed By:</b> Pedro L. Rentas  | <b>041723</b> |

| Compound | RM# | Lot Number | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty Purity (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty |                                       | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|-----|------------|-----------------------|------------|------------------------|-----------|-------------------|-------------------|----------------------|----------------------|---------------------------------------|------|----------------|------|----------|
|          |     |            |                       |            |                        |           |                   |                   |                      | +/- (µg/mL)          | (Solute Safety Info. On Attached pg.) |      |                |      |          |

1. Ammonium dihydrogen phosphate (P) IN008 P082019A1 10000 99.999 0.10 27.5 72.7287 72.7289 10000.0 20.0 7722-76-1 5 mg/m3 or-hal >2000mg/kg 3186

[1] Spectrum No.1 [ 12.074 sec]:58115.D# [Count] [Linear]

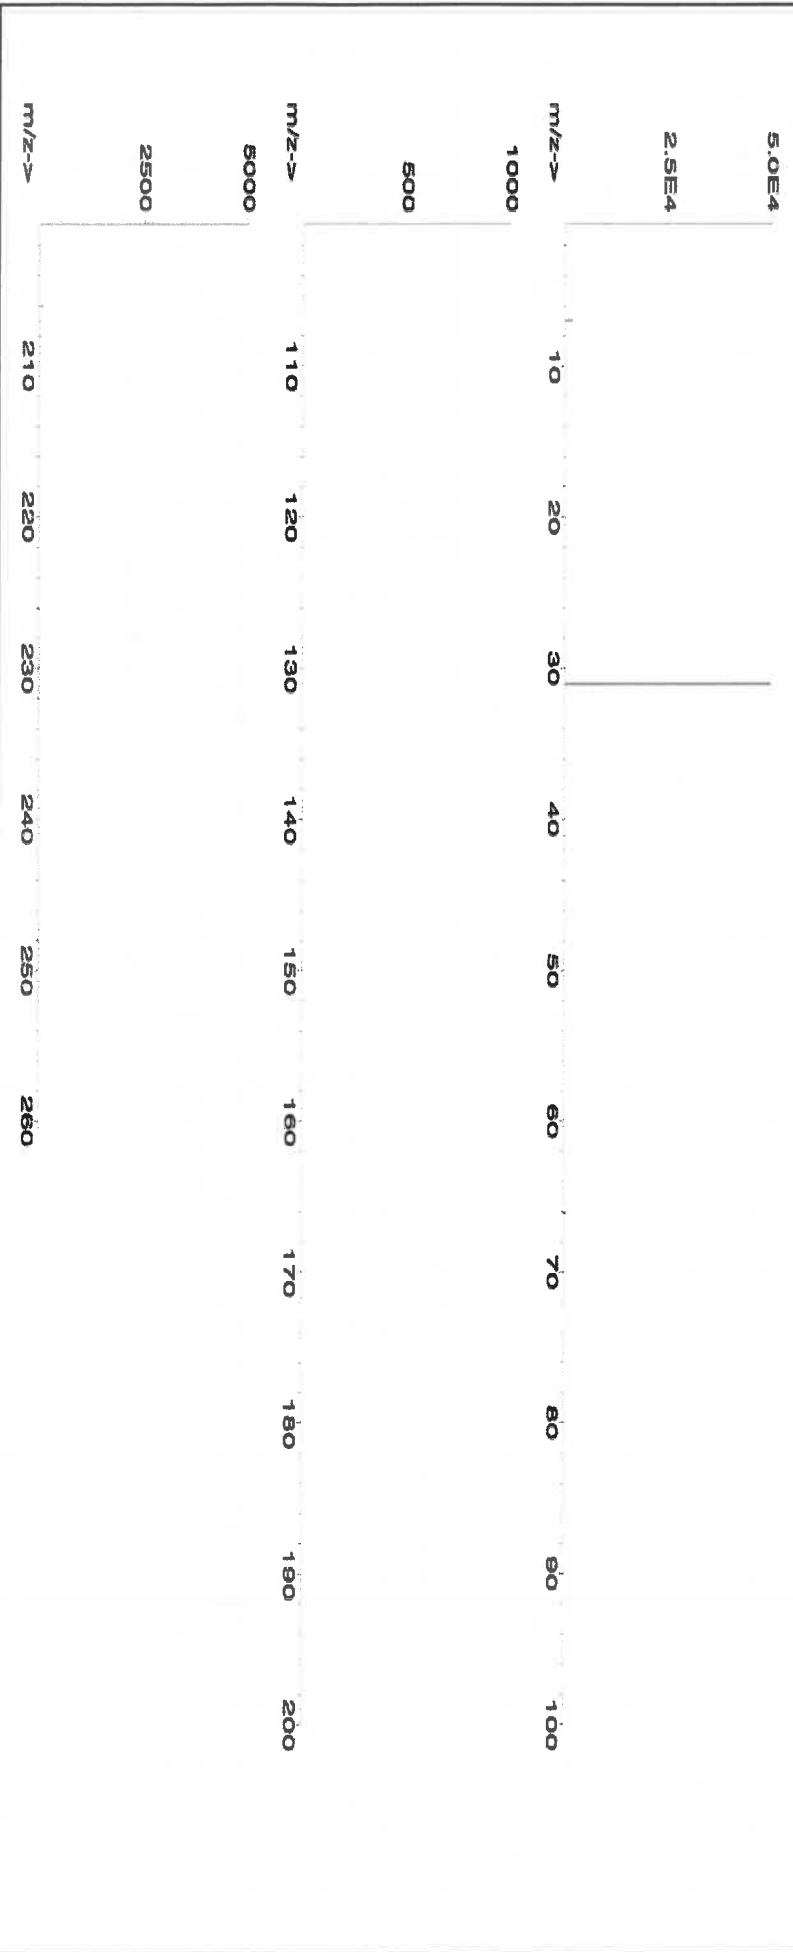



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | T     | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

**Certified by:**

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).





**CERTIFIED WEIGHT REPORT:**

Part Number: **57116**  
Lot Number: **071123**  
Description: **Sulfur (S)**

Lot #  
Solvent: 071123  
ASTM Type 1 Water

|                |                 |
|----------------|-----------------|
|                |                 |
| Formulated By: | Lawrence Barry  |
| 071123         |                 |
|                |                 |
| Reviewed By:   | Pedro L. Rentas |
| 071123         |                 |

Expiration Date: 071126  
Recommended Storage: Ambient (20 °C)  
Nominal Concentration (µg/mL): 10000  
NIST Test Number: 6UTB  
Weight shown below was diluted to (mL): 1999.48  
5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

| SDS Information      |                 |                       |            |                        |           |                   |                   |                      |                                  |
|----------------------|-----------------|-----------------------|------------|------------------------|-----------|-------------------|-------------------|----------------------|----------------------------------|
| Compound             | Lot Number      | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty Purity (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) |
| Ammonium sulfate (S) | IN117 SLBR7225V | 10000                 | 99.9       | 0.10                   | 24.3      | 82.4675           | 82.4692           | 10000.1              | 20.0                             |
|                      |                 |                       |            |                        |           | 7763-20-2         | NA                |                      |                                  |
|                      |                 |                       |            |                        |           |                   | oral 4250mg/kg    | 3181                 |                                  |

[1] Spectrum No. 1 [ 24.004 sec]:58116.D# [Count] [Linear]





**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | T     | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

**Physical Characterization:**

(T)= Target analyte

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**CERTIFIED WEIGHT REPORT:**

Part Number: **57014**  
Lot Number: **122023**  
Description: **Silicon (Si)**

Solvent: **24002546 Nitric Acid**

Lot #

*R: 02/09/24 M5818*

Expiration Date: **122026**

2% 40.0 (mL) Nitric Acid

Recommended Storage: **Ambient (20 °C)**

Nominal Concentration (µg/mL): **1000**

NIST Test Number: **6UTB**

SE-05 Balance Uncertainty

Weight shown below was diluted to (mL): **1999.48 0.058 Flask Uncertainty**


|                      |                        |
|----------------------|------------------------|
| <i>Aleah O Brady</i> |                        |
| Formulated By:       | Aleah O Brady          |
| Reviewed By:         | <i>Pedro L. Rentas</i> |
|                      | Pedro L. Rentas        |
|                      | 122023                 |

**SDS Information**

| Compound | Lot Number | Nominal Conc. (µg/mL) | Purity (%) | Uncertainty (%) | Assay (%) | Target Weight (g) | Actual Weight (g) | Actual Conc. (µg/mL) | Expanded Uncertainty +/- (µg/mL) | CAS# | OSHA PEL (TWA) | LD50 | NIST SRM |
|----------|------------|-----------------------|------------|-----------------|-----------|-------------------|-------------------|----------------------|----------------------------------|------|----------------|------|----------|
|----------|------------|-----------------------|------------|-----------------|-----------|-------------------|-------------------|----------------------|----------------------------------|------|----------------|------|----------|

1. Ammonium hexafluorosilicate (Si) IN009 S1D08022A1 1000 99.999 0.10 14.4 13.8854 13.8855 1000.0 2.0 18919-19-0 2.5 mg/m3 off-mus 70 mg/kg NA

[1] Spectrum No. 1 [ 31.393 sec; 158014.D# [Count] [Linear]

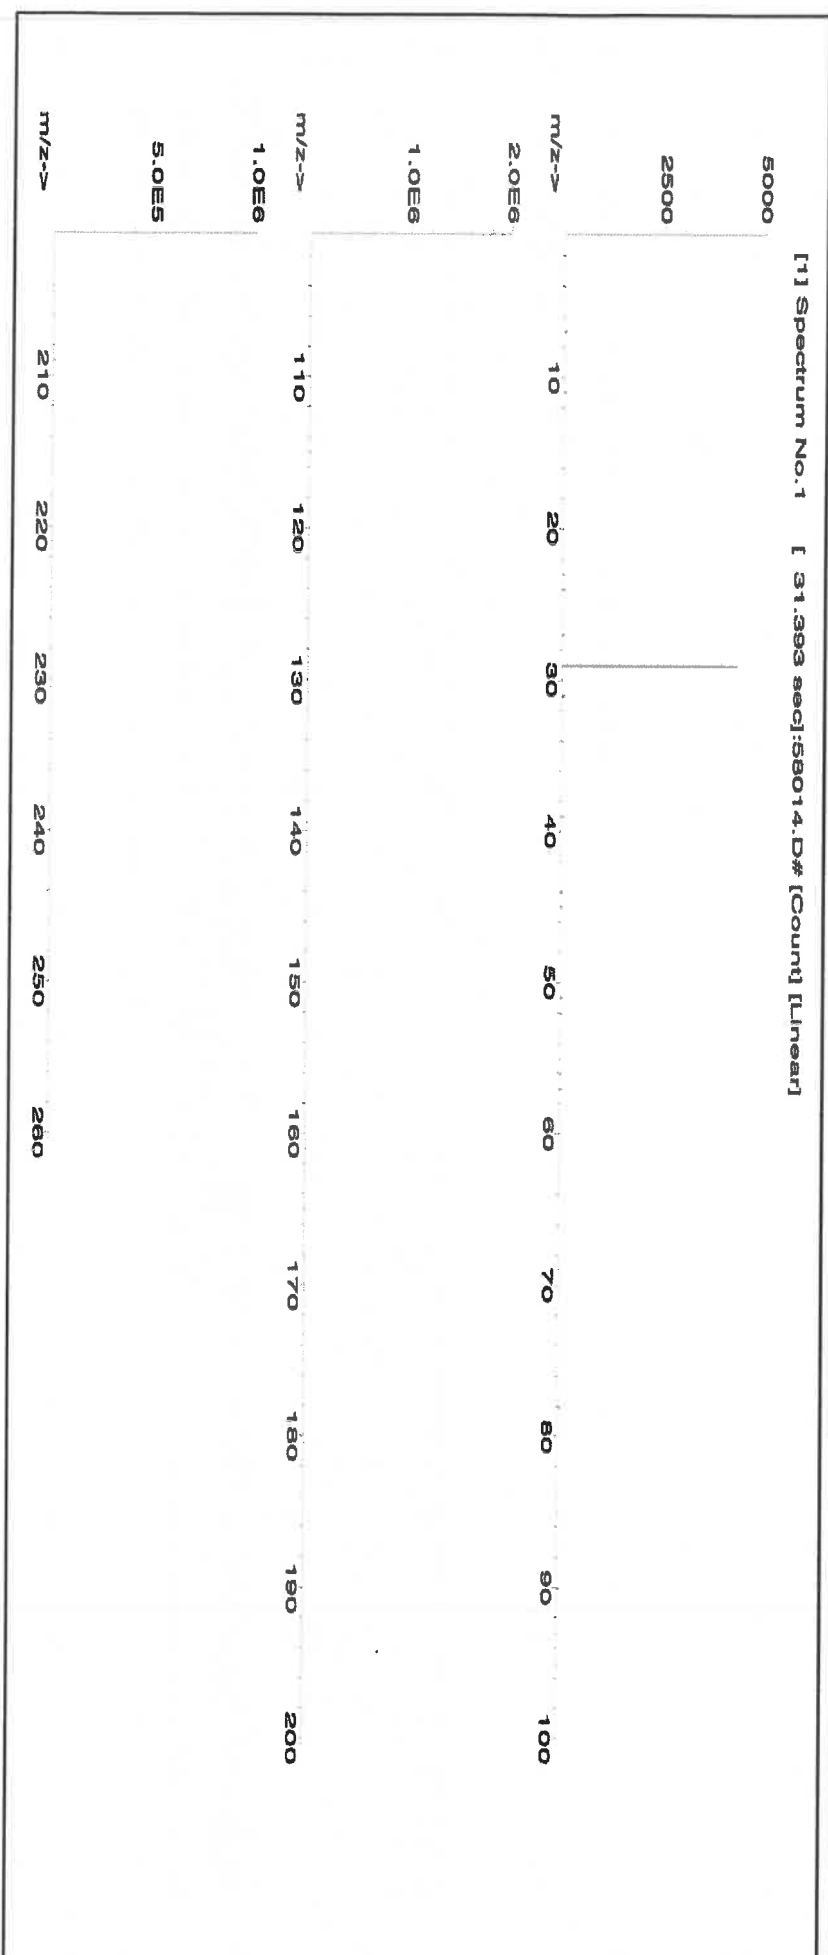



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

**Trace Metals Verification by ICP-MS ( $\mu\text{g/mL}$ )**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pt | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | T     | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Bu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Ru | <0.02 | Ag | <0.02 | Ti | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Tl | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



**CERTIFIED WEIGHT REPORT:**

**Part Number:** 58030  
**Lot Number:** 111623  
**Description:** Zinc (Zn)

**Solvent:** 24002546 Nitric Acid

**2%** 60.0 (mL) Nitric Acid

**Expiration Date:** 111626  
**Recommended Storage:** Ambient (20 °C)  
**Nominal Concentration (µg/mL):** 1000  
**NIST Test Number:** 6UTB

**Weight shown below was diluted to (mL):** 3000.4 0.06 Balance Uncertainty  
Flask Uncertainty


*R: 02/09/24 MS819*

**Lot #**

|                |                  |
|----------------|------------------|
|                |                  |
| Formulated By: | Benson Chan      |
| Reviewed By:   | Pedro L. Reintas |
|                | 111623           |

| SDS Information |     |        |               |        |             |       |            |            |               |             |      |  |  |  |
|-----------------|-----|--------|---------------|--------|-------------|-------|------------|------------|---------------|-------------|------|--|--|--|
| Compound        | Lot |        | Nominal       | Purity | Uncertainty | Assay | Target     | Actual     | Actual        | Expanded    |      | (Solvent Safety Info. On Attached pg.) |  |  |
|                 | RM# | Number | Conc. (µg/mL) | (%)    | Purity (%)  | (%)   | Weight (g) | Weight (g) | Conc. (µg/mL) | +/- (µg/mL) | CAS# |  |  |  |

1. Zinc nitrate hexahydrate (Zn) IN016 ZNE03021A1 1000 99.999 0.10 24.3 12.3475 12.3502 1000.2 2.0 10196-16-6 1 mg/mL 3168 on-rat 1190mg/kg

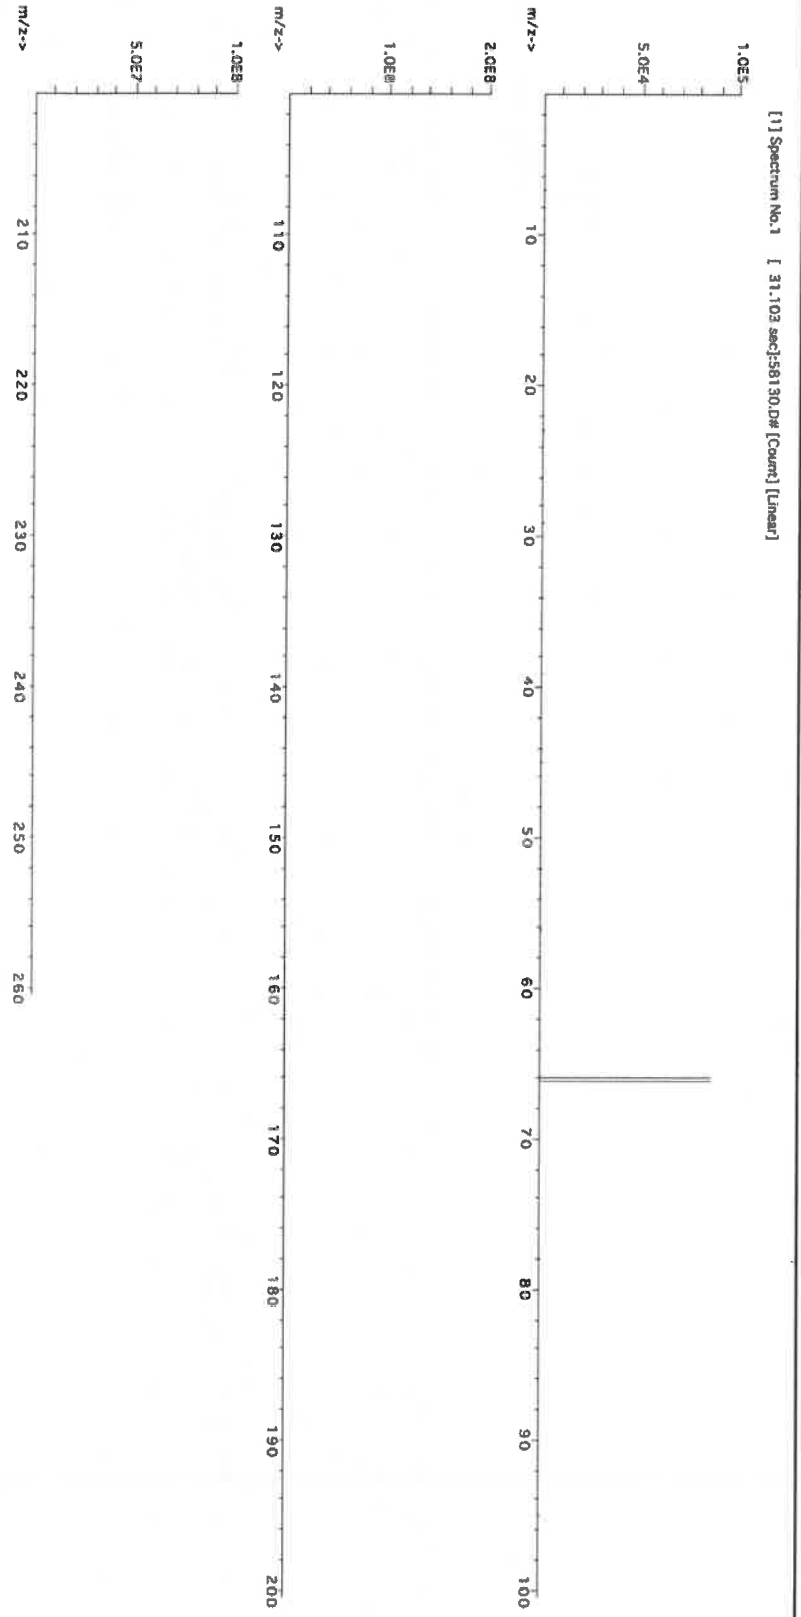



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Bu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | <0.02 | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).









Hydrochloric Acid, 36.5–38.0%  
BAKER INSTRA-ANALYZED® Reagent  
For Trace Metal Analysis



MS947 MS948 MS949  
MS950 MS951 MS952

Material No.: 9530-33  
Batch No.: 22G2862015  
Manufactured Date: 2022-06-15  
Retest Date: 2027-06-14  
Revision No.: 0

## Certificate of Analysis

| Test                                      | Specification | Result      |
|---|---------------|-------------|
| ACS – Assay (as HCl) (by acid–base titrn) | 36.5 – 38.0 % | 37.9 %      |
| ACS – Color (APHA)                        | ≤ 10          | 5           |
| ACS – Residue after Ignition              | ≤ 3 ppm       | < 1 ppm     |
| ACS – Specific Gravity at 60°/60°F        | 1.185 – 1.192 | 1.191       |
| ACS – Bromide (Br)                        | ≤ 0.005 %     | < 0.005 %   |
| ACS – Extractable Organic Substances      | ≤ 5 ppm       | < 1 ppm     |
| ACS – Free Chlorine (as Cl <sub>2</sub> ) | ≤ 0.5 ppm     | < 0.5 ppm   |
| Phosphate (PO <sub>4</sub> )              | ≤ 0.05 ppm    | < 0.03 ppm  |
| Sulfate (SO <sub>4</sub> )                | ≤ 0.5 ppm     | < 0.3 ppm   |
| Sulfite (SO <sub>3</sub> )                | ≤ 0.8 ppm     | 0.3 ppm     |
| Ammonium (NH <sub>4</sub> )               | ≤ 3 ppm       | < 1 ppm     |
| Trace Impurities – Arsenic (As)           | ≤ 0.010 ppm   | < 0.003 ppm |
| Trace Impurities – Aluminum (Al)          | ≤ 10.0 ppb    | 1.3 ppb     |
| Arsenic and Antimony (as As)              | ≤ 5.0 ppb     | < 3.0 ppb   |
| Trace Impurities – Barium (Ba)            | ≤ 1.0 ppb     | 0.2 ppb     |
| Trace Impurities – Beryllium (Be)         | ≤ 1.0 ppb     | < 0.2 ppb   |
| Trace Impurities – Bismuth (Bi)           | ≤ 10.0 ppb    | < 1.0 ppb   |
| Trace Impurities – Boron (B)              | ≤ 20.0 ppb    | < 5.0 ppb   |
| Trace Impurities – Cadmium (Cd)           | ≤ 1.0 ppb     | < 0.3 ppb   |
| Trace Impurities – Calcium (Ca)           | ≤ 50.0 ppb    | 163.0 ppb   |
| Trace Impurities – Chromium (Cr)          | ≤ 1.0 ppb     | 0.7 ppb     |
| Trace Impurities – Cobalt (Co)            | ≤ 1.0 ppb     | < 0.3 ppb   |
| Trace Impurities – Copper (Cu)            | ≤ 1.0 ppb     | < 0.1 ppb   |
| Trace Impurities – Gallium (Ga)           | ≤ 1.0 ppb     | < 0.2 ppb   |
| Trace Impurities – Germanium (Ge)         | ≤ 3.0 ppb     | < 2.0 ppb   |
| Trace Impurities – Gold (Au)              | ≤ 4.0 ppb     | 0.6 ppb     |
| Heavy Metals (as Pb)                      | ≤ 100 ppb     | < 50 ppb    |
| Trace Impurities – Iron (Fe)              | ≤ 15 ppb      | 6 ppb       |

>>> Continued on page 2 >>>

Hydrochloric Acid, 36.5–38.0%  
BAKER INSTRA-ANALYZED® Reagent  
For Trace Metal Analysis

 **avantor™**



Material No.: 9530-33  
Batch No.: 22G2862015

| Test   | Specification | Result     |
|--|---------------|------------|
| Trace Impurities – Lead (Pb)                           | ≤ 1.0 ppb     | < 0.5 ppb  |
| Trace Impurities – Lithium (Li)                        | ≤ 1.0 ppb     | < 0.2 ppb  |
| Trace Impurities – Magnesium (Mg)                      | ≤ 10.0 ppb    | 2.9 ppb    |
| Trace Impurities – Manganese (Mn)                      | ≤ 1.0 ppb     | < 0.4 ppb  |
| Trace Impurities – Mercury (Hg)                        | ≤ 0.5 ppb     | 0.1 ppb    |
| Trace Impurities – Molybdenum (Mo)                     | ≤ 10.0 ppb    | < 3.0 ppb  |
| Trace Impurities – Nickel (Ni)                         | ≤ 4.0 ppb     | < 0.3 ppb  |
| Trace Impurities – Niobium (Nb)                        | ≤ 1.0 ppb     | 0.8 ppb    |
| Trace Impurities – Potassium (K)                       | ≤ 9.0 ppb     | < 2.0 ppb  |
| Trace Impurities – Selenium (Se), For Information Only |               | < 1.0 ppb  |
| Trace Impurities – Silicon (Si)                        | ≤ 100.0 ppb   | < 10.0 ppb |
| Trace Impurities – Silver (Ag)                         | ≤ 1.0 ppb     | 0.5 ppb    |
| Trace Impurities – Sodium (Na)                         | ≤ 100.0 ppb   | 2.3 ppb    |
| Trace Impurities – Strontium (Sr)                      | ≤ 1.0 ppb     | < 0.2 ppb  |
| Trace Impurities – Tantalum (Ta)                       | ≤ 1.0 ppb     | 1.6 ppb    |
| Trace Impurities – Thallium (Tl)                       | ≤ 5.0 ppb     | < 2.0 ppb  |
| Trace Impurities – Tin (Sn)                            | ≤ 5.0 ppb     | 4.0 ppb    |
| Trace Impurities – Titanium (Ti)                       | ≤ 1.0 ppb     | 1.5 ppb    |
| Trace Impurities – Vanadium (V)                        | ≤ 1.0 ppb     | < 0.2 ppb  |
| Trace Impurities – Zinc (Zn)                           | ≤ 5.0 ppb     | 0.8 ppb    |
| Trace Impurities – Zirconium (Zr)                      | ≤ 1.0 ppb     | 0.3 ppb    |

>>> Continued on page 3 >>>

Hydrochloric Acid, 36.5–38.0%

BAKER INSTRA-ANALYZED® Reagent

For Trace Metal Analysis

 **avantor™**




Material No.: 9530-33  
Batch No.: 22G2862015

| Test | Specification | Result |
|------|---------------|--------|
|------|---------------|--------|

For Laboratory, Research, or Manufacturing Use  
Product Information (not specifications):  
Appearance (clear, fuming liquid)  
Meets ACS Specifications  
Storage Condition: Store below 25 °C.

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

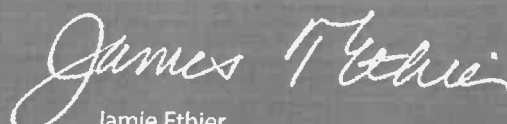  
Jamie Ethier  
Vice President Global Quality



**Certified Reference Material CRM**

**CERTIFIED WEIGHT REPORT:**

R: 03/16/23 MS473 MS474 MS475 MS476

Lot #

Part Number:

**56138**

Solvent: 20510011

Nitric Acid

Lot Number:

**082922**

Description:

**Strontium (Sr)**

Expiration Date:

082925

2%

20.0

Nitric Acid

Recommended Storage:

Ambient (20 °C)

Nominal Concentration (µg/mL):

**10000**

NIST Test Number:

6UTB

Weight shown below was diluted to (mL):

1000.12

0.058

Flask Uncertainty

|                |                   |        |
|----------------|-------------------|--------|
| Formulated By: | Lawrence Barry    | 082922 |
| Reviewed By:   | Pedro L. Renteria | 082922 |

**SDS Information**

**Compound**

RM#

Lot

Number

Nominal

Purity

Uncertainty

Assay

Target

Actual

Actual

Conc. (µg/mL)

Expanded

Uncertainty

CAS#

OSHA PEL (TWA)

LD50

NIST

SRM

or-rat >2000mg/kg

3153a

20.0

10042-76-9

NA

or-rat >2000mg/kg

3153a

or-rat >2000mg/kg

3153a

or-rat >2000mg/kg

3153a

or-rat >2000mg/kg

3153a

or-rat >2000mg/kg

3153a

or-rat >2000mg/kg

3153a

1. Strontium nitrate (Sr)

IN017 SR2022018A1

10000

99.997

0.10

41.2

24.2756

24.2758

10000.1

20.0


10042-76-9

NA

or-rat >2000mg/kg

3153a

[1] Spectrum No. 1 [14.495 sec]: 56138.D# [Count] [Linear]

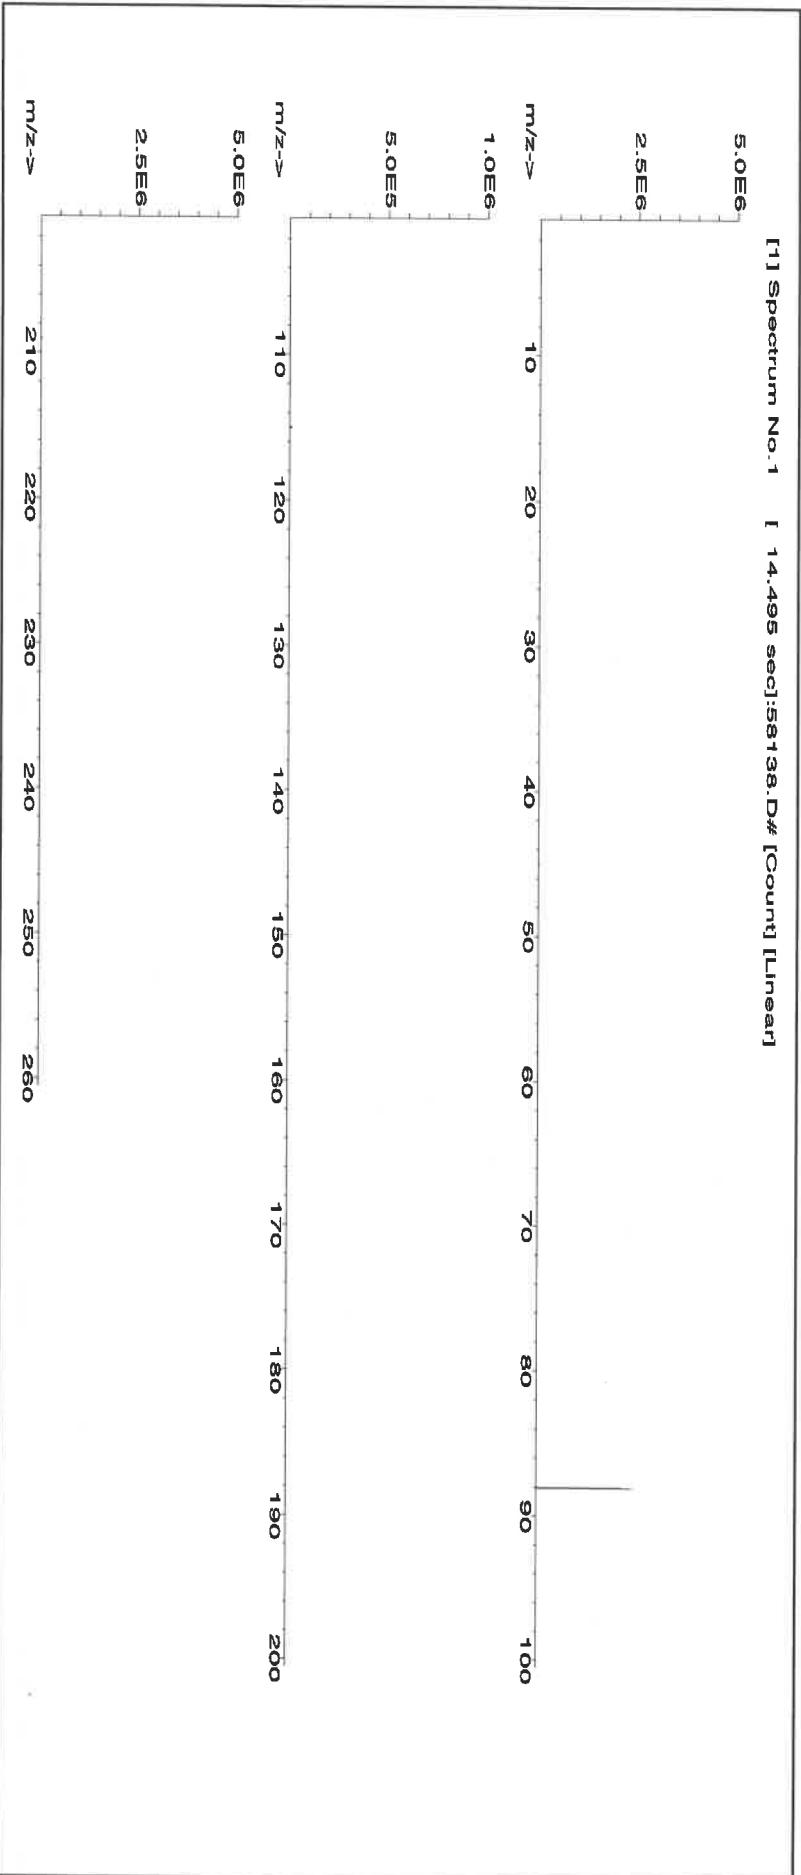



**Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):**

**Trace Metals Verification by ICP-MS (µg/mL)**

|    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |    |       |
|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|----|-------|
| Al | <0.02 | Cd | <0.02 | Dy | <0.02 | Hf | <0.02 | Li | <0.02 | Ni | <0.02 | Pr | <0.02 | Se | <0.2  | Tb | <0.02 | W  | <0.02 |
| Sb | <0.02 | Ca | <0.2  | Er | <0.02 | Ho | <0.02 | Lu | <0.02 | Nb | <0.02 | Re | <0.02 | Si | <0.02 | Te | <0.02 | U  | <0.02 |
| As | <0.2  | Ce | <0.02 | Eu | <0.02 | In | <0.02 | Mg | <0.01 | Os | <0.02 | Rh | <0.02 | Ag | <0.02 | Tl | <0.02 | V  | <0.02 |
| Ba | <0.02 | Cs | <0.02 | Gd | <0.02 | Ir | <0.02 | Mn | <0.02 | Pd | <0.02 | Rb | <0.02 | Na | <0.2  | Th | <0.02 | Yb | <0.02 |
| Be | <0.01 | Cr | <0.02 | Ga | <0.02 | Fe | <0.2  | Hg | <0.2  | P  | <0.02 | Ru | <0.02 | Sr | T     | Tm | <0.02 | Y  | <0.02 |
| Bi | <0.02 | Co | <0.02 | Ge | <0.02 | La | <0.02 | Mo | <0.02 | Pt | <0.02 | Sm | <0.02 | S  | <0.02 | Sn | <0.02 | Zn | <0.02 |
| B  | <0.02 | Cu | <0.02 | Au | <0.02 | Pb | <0.02 | Nd | <0.02 | K  | <0.2  | Sc | <0.02 | Ta | <0.02 | Ti | <0.02 | Zr | <0.02 |

(T) = Target analyte

**Physical Characterization:**

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- \* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- \* Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- \* All standard containers are meticulously cleaned prior to use.
- \* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- \* Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- \* All Standards should be stored with caps tight and under appropriate laboratory conditions.
- \* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).