

### Prep Standard - Chemical Standard Summary

**Order ID :** P3390

**Test :** TPH GC

**Prepbatch ID :** PB162367,

**Sequence ID/Qc Batch ID:** FG073124,

**Standard ID :**

EP2511,EP2518,PP23111,PP23155,PP23156,PP23204,PP23205,PP23206,PP23207,PP23208,PP23518,

**Chemical ID :**

E3551,E3706,E3707,E3725,E3768,E3769,E3771,P11949,P12308,P12309,P13105,P13112,P13206,P13207,P13208,P13209,P13215,P13216,

## Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2017	1:1 ACETONE/METHYLENE CHLORIDE	<a href="#">EP2511</a>	07/12/2024	01/08/2025	Rajesh Parikh	None	None	RUPESHKUMAR SHAH 07/12/2024

**FROM** 8000.00000ml of E3768 + 8000.00000ml of E3769 = Final Quantity: 16000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	<a href="#">EP2518</a>	07/26/2024	01/03/2025	RUPESHKUMAR SHAH	Extraction_SCALE_2	None	Rajesh Parikh 07/26/2024

**FROM** 1.00000gram of E3551 = Final Quantity: 4000.000 gram

(EX-SC-2)

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3609	20 PPM DRO SPIKE SOLUTION (RESTEK)	<a href="#">PP23111</a>	02/21/2024	08/19/2024	Yogesh Patel	None	None	Ankita Jodhani
								02/21/2024

**FROM** 1.00000ml of P13105 + 1.00000ml of P13112 + 48.00000ml of E3706 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
433	100/100 PPM DRO (Restek)	<a href="#">PP23155</a>	03/15/2024	08/21/2024	Yogesh Patel	None	None	Ankita Jodhani
								03/18/2024

**FROM** 1.00000ml of P11949 + 1.00000ml of P12308 + 1.00000ml of P13112 + 7.00000ml of E3707 = Final Quantity: 10.000 ml

[illegible]

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipettelD</u>	<u>Supervised By</u>
435	50 PPM ICC DRO STD (Restek)	<a href="#">PP23204</a>	04/11/2024	08/21/2024	Yogesh Patel	None	None	Ankita Jodhani 04/17/2024
<u>FROM</u>	0.50000ml of E3725 + 0.50000ml of PP23155 = Final Quantity: 1.000 ml							



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
437	20 PPM ICC DRO STD (Restek)	<a href="#">PP23205</a>	04/11/2024	08/21/2024	Yogesh Patel	None	None	Ankita Jodhani 04/17/2024
<u>FROM</u>	0.80000ml of E3725 + 0.20000ml of PP23155 = Final Quantity: 1.000 ml							

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
438	10 PPM ICC DRO STD (Restek)	<a href="#">PP23206</a>	04/11/2024	08/21/2024	Yogesh Patel	None	None	Ankita Jodhani 04/17/2024
<u>FROM</u>	0.90000ml of E3725 + 0.10000ml of PP23155 = Final Quantity: 1.000 ml							

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
439	5 PPM ICC DRO STD (Restek)	<a href="#">PP23207</a>	04/11/2024	08/21/2024	Yogesh Patel	None	None	Ankita Jodhani
04/17/2024								

**FROM** 0.90000ml of E3725 + 0.10000ml of PP23204 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3797	50 PPM DRO ICV STD (CPI)	<a href="#">PP23208</a>	04/11/2024	08/28/2024	Yogesh Patel	None	None	Ankita Jodhani
04/17/2024								

**FROM** 0.50000ml of E3725 + 0.50000ml of PP23156 = Final Quantity: 1.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
147	20 PPM DRO Surrogate Spike Solution	<a href="#">PP23518</a>	07/15/2024	01/08/2025	Yogesh Patel	None	None	Ankita Jodhani 07/16/2024
<p><b><u>FROM</u></b> 1.00000ml of P13206 + 1.00000ml of P13207 + 1.00000ml of P13208 + 1.00000ml of P13209 + 196.00000ml of E3768 = Final Quantity: 200.000 ml</p>								

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	313201	01/03/2025	01/03/2024 / Rajesh	07/20/2023 / Rajesh	E3551

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24A1562007	08/19/2024	02/19/2024 / RUPESH	01/31/2024 / RUPESH	E3706

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24A1562007	08/28/2024	02/28/2024 / Rajesh	02/19/2024 / Rajesh	E3707

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24A1962016	10/04/2024	04/04/2024 / Rajesh	03/20/2024 / Rajesh	E3725

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24E2462004	01/08/2025	07/08/2024 / Rajesh	06/21/2024 / Rajesh	E3768

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	23H1462005	01/12/2025	07/12/2024 /	07/02/2024 / Rajesh	E3769



## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9644-A4 / Methylene Chloride,U-Resi, Cycle-Tainer (215L)	24F1062004	01/19/2025	07/19/2024 / Rajesh	07/16/2024 / Rajesh	E3771

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0186840	09/15/2024	03/15/2024 / yogesh	07/11/2022 / Yogesh	P11949

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	101122	09/15/2024	03/15/2024 / yogesh	02/22/2023 / Yogesh	P12308

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	101122	09/15/2024	03/15/2024 / yogesh	02/22/2023 / Yogesh	P12309

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0204859	08/21/2024	02/21/2024 / yogesh	01/12/2024 / Yogesh	P13105

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	31266 / Florida TRPH Standard	A0204859	08/21/2024	02/21/2024 / yogesh	01/12/2024 / Yogesh	P13112

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	101122	01/15/2025	07/15/2024 / yogesh	01/17/2024 / Ankita	P13206

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	101122	01/15/2025	07/15/2024 / yogesh	01/17/2024 / Ankita	P13207

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	101122	01/15/2025	07/15/2024 / yogesh	01/17/2024 / Ankita	P13208

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	72072 / n-Tetracosane-d50, 1000 ug/ml	101122	01/15/2025	07/15/2024 / yogesh	01/17/2024 / Ankita	P13209

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110400-05-01 / TRPH Standard (C8-C40), 500 mg/L, 1 ml	514983	09/15/2024	03/15/2024 / yogesh	01/31/2024 / Ankita	P13215

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
CPI International	Z-110400-05-01 / TRPH Standard (C8-C40), 500 mg/L, 1 ml	514983	09/15/2024	03/15/2024 / yogesh	01/31/2024 / Ankita	P13216



**PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MEXICO  
CP 64070  
TEL +52 81 13 52 57 57  
www.pqm.com.mx

## CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na <sub>2</sub> SO <sub>4</sub>
SPECIFICATION NUMBER :	6399	RELEASE DATE:	ABR/21/2023
LOT NUMBER :	313201		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na <sub>2</sub> SO <sub>4</sub> )	Min. 99.0%	99.7 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.1
Insoluble matter	Max. 0.01%	0.005 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO <sub>4</sub> )	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.002 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.003 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.1 %
Retained on US Standard No. 60 sieve	Min. 94%	97.3 %
Through US Standard No. 60 sieve	Max. 5%	2.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

### COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

Recd. by R3 on 7/24/23 E 3551

RC-02-01, Ed. 3

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 24A1562007  
Manufactured Date: 2023-12-14  
Expiration Date: 2025-03-14  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	< 1
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.1 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC  
Manufacturer source batch: MG23L14152

REC.  
AS 2/19/24

E 3706

Ken Koehnlein  
Sr. Manager, Quality Assurance

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 24A1562007  
Manufactured Date: 2023-12-14  
Expiration Date: 2025-03-14  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	< 1
Assay (CH <sub>2</sub> Cl <sub>2</sub> ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0$ ppm	0.1 ppm
Titration Acid ( $\mu$ eq/g)	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10$ ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC  
Manufacturer source batch: MG23L14152

E 3707

Ken Koehnlein  
Sr. Manager, Quality Assurance

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 24A1962016  
Manufactured Date: 2023-12-14  
Expiration Date: 2025-03-14  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	2
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.5 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC  
Manufacturer source batch: MG23L14151

E 3725

Ken Koehnlein  
Sr. Manager, Quality Assurance

Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 24E2462004  
Manufactured Date: 2024-04-10  
Expiration Date: 2025-07-10  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	3
Assay ( $\text{CH}_2\text{Cl}_2$ ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0 \text{ ppm}$	0.1 ppm
Titration Acid ( $\mu\text{eq/g}$ )	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10 \text{ ppm}$	5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC  
Manufacturer source batch: MG24D10725

E 3768

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087, U.S.A. Phone 610.386.1700

Page 1 of 1

Acetone

BAKER RESI-ANALYZED® Reagent

For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 23H1462005

Manufactured Date: 2023-07-26

Expiration Date: 2026-07-25

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water)	≥ 99.4 %	99.7 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.3 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	≤ 0.3	0.1
Titration Base (μeq/g)	≤ 0.6	< 0.1
Water (H <sub>2</sub> O)	≤ 0.5 %	0.3 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

Recd. by RP on 7/21/24

E 3769

Ken Koehnlein  
Sr. Manager, Quality Assurance



Methylene Chloride  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis  
(dichloromethane)



Material No.: 9266-A4  
Batch No.: 24F1062004  
Manufactured Date: 2024-04-15  
Expiration Date: 2025-07-15  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	< 1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	$\leq 10$	7
Assay (CH <sub>2</sub> Cl <sub>2</sub> ) (by GC, exclusive of preservative, corrected for water)	$\geq 99.8 \%$	100.0 %
Color (APHA)	$\leq 10$	5
Residue after Evaporation	$\leq 1.0$ ppm	0.1 ppm
Titration Acid ( $\mu$ eq/g)	$\leq 0.3$	< 0.1
Chloride (Cl)	$\leq 10$ ppm	< 5 ppm
Water (by KF, coulometric)	$\leq 0.02 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC  
Manufacturer source batch: MG24D15750

E 3771

Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials, LLC

100 Matsonford Rd, Suite 200, Radnor, PA 19087. U.S.A. Phone 610.386.1700

Page 1 of 1



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle

Belleville, PA 16823-8812

Tel: (800)356-1688

Fax: (814)353-1309

www.restek.com

## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31266

Lot No.: A0186840

Description : Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : July 31, 2029

Storage: 25°C nominal

Handling: Sonicate prior to use.

Ship: Ambient

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	n-Octane (C8) CAS # 111-65-9 Purity 99%	505.0 µg/mL	+/- 2.9995 µg/mL +/- 12.5465 µg/mL +/- 15.0390 µg/mL	Gravimetric Unstressed Unstressed Stressed
2	n-Decane (C10) CAS # 124-18-5 Purity 99%	503.0 µg/mL	+/- 2.9877 µg/mL +/- 12.4968 µg/mL +/- 14.9795 µg/mL	Gravimetric Unstressed Unstressed Stressed
3	n-Dodecane (C12) CAS # 112-40-3 Purity 99%	503.5 µg/mL	+/- 2.9906 µg/mL +/- 12.5092 µg/mL +/- 14.9944 µg/mL	Gravimetric Unstressed Unstressed Stressed
4	n-Tetradecane (C14) CAS # 629-59-4 Purity 99%	505.0 µg/mL	+/- 2.9995 µg/mL +/- 12.5465 µg/mL +/- 15.0390 µg/mL	Gravimetric Unstressed Unstressed Stressed
5	n-Hexadecane (C16) CAS # 544-76-3 Purity 98%	504.7 µg/mL	+/- 2.9978 µg/mL +/- 12.5390 µg/mL +/- 15.0301 µg/mL	Gravimetric Unstressed Unstressed Stressed
6	n-Octadecane (C18) CAS # 593-45-3 Purity 97%	504.4 µg/mL	+/- 2.9960 µg/mL +/- 12.5316 µg/mL +/- 15.0212 µg/mL	Gravimetric Unstressed Unstressed Stressed
7	n-Eicosane (C20) CAS # 112-95-8 Purity 99%	503.5 µg/mL	+/- 2.9906 µg/mL +/- 12.5092 µg/mL +/- 14.9944 µg/mL	Gravimetric Unstressed Unstressed Stressed

P11948 } 7.8  
P11962 } 07/11/16

8	n-Docosane (C22) <b>CAS #</b> 629-97-0 <b>Purity</b> 99%	(Lot MKCL8918)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
9	n-Tetracosane (C24) <b>CAS #</b> 646-31-1 <b>Purity</b> 99%	(Lot MKCN2863)	503.5 µg/mL	+/- 2.9906 +/- 12.5092 +/- 14.9944	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
10	n-Hexacosane (C26) <b>CAS #</b> 630-01-3 <b>Purity</b> 99%	(Lot MKCD4540)	504.0 µg/mL	+/- 2.9936 +/- 12.5216 +/- 15.0093	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
11	n-Octacosane (C28) <b>CAS #</b> 630-02-4 <b>Purity</b> 99%	(Lot BCCG0084)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
12	n-Triacontane (C30) <b>CAS #</b> 638-68-6 <b>Purity</b> 99%	(Lot MKCN9321)	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
13	n-Dotriacontane (C32) <b>CAS #</b> 544-85-4 <b>Purity</b> 99%	(Lot BCBW0661)	505.0 µg/mL	+/- 2.9995 +/- 12.5465 +/- 15.0390	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
14	n-Tetratriacontane (C34) <b>CAS #</b> 14167-59-0 <b>Purity</b> 99%	(Lot OML4N)	504.5 µg/mL	+/- 2.9966 +/- 12.5340 +/- 15.0241	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
15	n-Hexatriacontane (C36) <b>CAS #</b> 630-06-8 <b>Purity</b> 99%	(Lot U25B014)	504.0 µg/mL	+/- 2.9936 +/- 12.5216 +/- 15.0093	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
16	n-Octatriacontane (C38) <b>CAS #</b> 7194-85-6 <b>Purity</b> 97%	(Lot 0000127235)	504.4 µg/mL	+/- 2.9960 +/- 12.5316 +/- 15.0212	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed
17	n-Tetracontane (C40) <b>CAS #</b> 4181-95-7 <b>Purity</b> 98%	(Lot PADGI)	504.7 µg/mL	+/- 2.9978 +/- 12.5390 +/- 15.0301	µg/mL µg/mL µg/mL	Gravimetric Unstressed Stressed

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

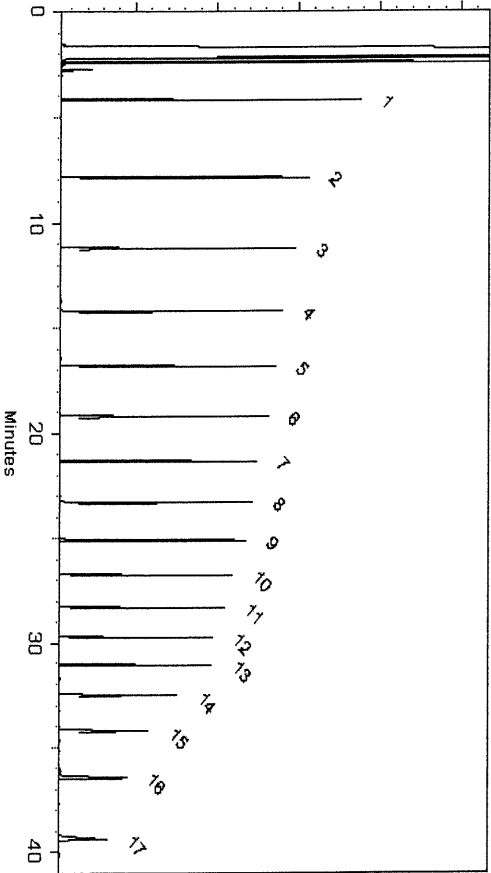

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Brittany Federinko*

Brittany Federinko - Operations Tech I

Date Mixed: 29-Jun-2022

Balance: 1128360905

*Christie Mills*

Christie Mills - Operations Tech II - ARM QC

Date Passed: 01-Jul-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-US](http://www.restek.com/Contact-US) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-US](http://www.restek.com/Contact-US).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED WEIGHT REPORT

Part Number: **72072**  
Lot Number: **101122**  
Description: **n-Tetracosane-d50**

Solvent(s):  
Methylene chloride

Lot#  
105345

<i>Prashant Chauhan</i>		101122
Formulated By:	Prashant Chauhan	DATE
<i>Pedro L. Rentas</i>		101122
Reviewed By:	Pedro L. Rentas	DATE

Expiration Date: 101132  
Recommended Storage: Ambient (20 °C)  
Nominal Concentration (µg/mL): 1000  
NIST Test ID#: 6UTB



5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 200.0

*P12291*  
*↓*  
*P12310* } *Y.P.*  
*02/22/23*

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
											CAS#	OSHA PEL (TWA)	LD50
1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20482	1000.6	4.1	16416-32-3	N/A	N/A

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

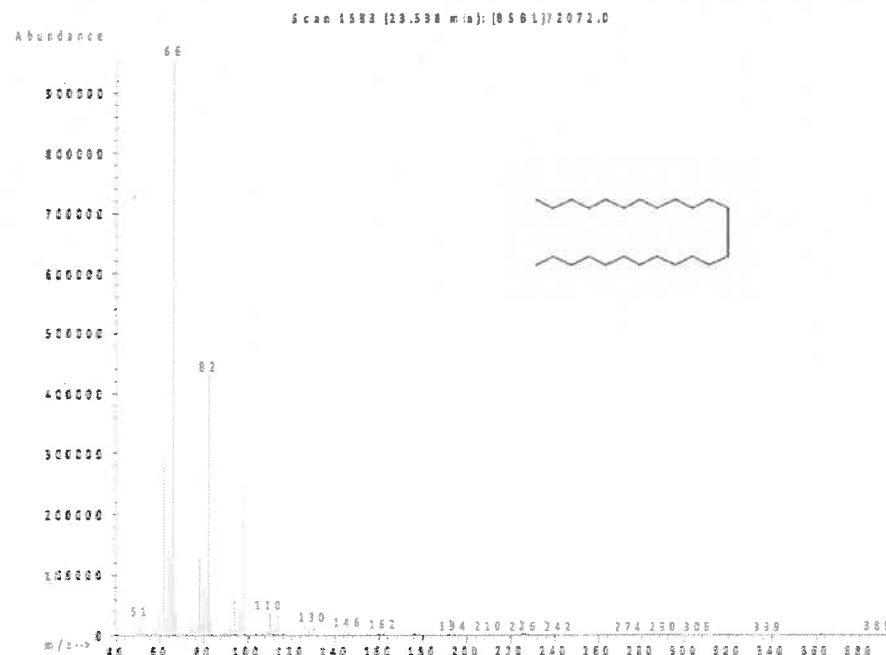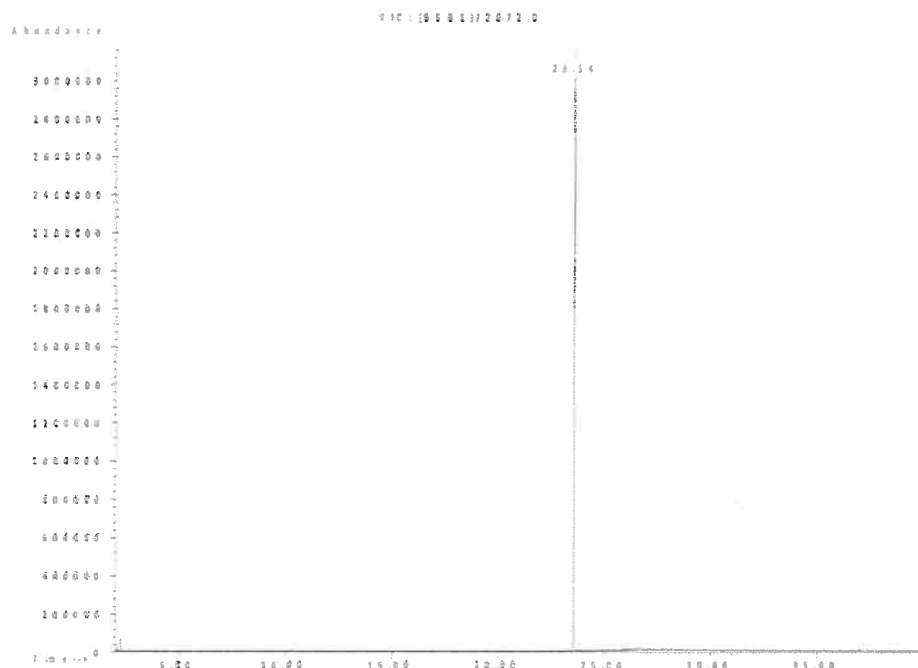

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



## Safety Data Sheet (SDS)

GHS/OSHA Compliant

## Section I Product and Company Identification

## IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHYLENE CHLORIDE

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rosotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2022

## Section II - Hazards Identification

## GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H302	Harmful if swallowed.	H315,H320	Causes skin and eye irritation.
H351	Suspected of causing cancer.	H335	May cause respiratory irritation.
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: WARNING



## Section III - Composition

Components:	CAS#:	OSHA PEL (TWA)	LD50 orl-rat	% (optional)
Dichloromethane	75-09-2	50 ppm	> 2,000 mg/kg	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.  
INTENDED USE: REFERENCE MATERIAL

## Section IV. FIRST AID MEASURES

**General advice**  
Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.

**If inhaled**  
If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.

**In case of skin contact**  
Wash with soap and water. Consult a physician.

**In case of eye contact**  
Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.

**If swallowed**  
Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

## Section V. FIREFIGHTING MEASURES

**Suitable extinguishing media**  
Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.

**Protective equipment for fire**  
Wear self contained breathing apparatus for fire fighting if necessary.

## Section VI. ACCIDENTAL RELEASE MEASURES

**Personal precautions**  
Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.

**Environmental precautions**  
Prevent further leakage or spillage if safe to do so. Do not let product enter drains.

**Clean up**  
Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

## Section VII. HANDLING AND STORAGE

**Precautions for safe handling**  
Avoid contact with skin and eyes. Avoid inhalation of vapour or mist.

**Storage Conditions**  
Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge. Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

## Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methylene chloride 75-09-2 TWA 50 ppm

**Potential for skin absorption, ingestion and inhalation.**

**Personal protective equipment**  
Respiratory protection  
Handle with gloves. Gloves must be inspected prior to use. Eye protection.

**Personal contact with skin, eyes and clothing.**  
Wash hands thoroughly after handling the product.

## Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS

Boiling Point	40°C	Specific Gravity (H2O = 1)	1.325
---------------	------	----------------------------	-------



Vapor Pressure (mm Hg)	353	Melting Point	-97°C
Vapor Density (AIR = 1)	2.93	Evaporation rate (Butyl Acetate = 1)	0.71
Solubility in Water	Slightly soluble		

Appearance and Odor CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.

**Section X. STABILITY AND REACTIVITY**

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	No data available
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Alkali metals, Aluminum, Oxidizing agents, Bases, Amines, Magnesium, Acids, Vinyl compounds
Hazardous decomposition products	- No data available

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - Rat - > 2,000 mg/kg  
LC50 Inhalation - Rat - 52,000 mg/m3  
LD50 Dermal - Rat - > 2,000 mg/kg  
Toxic if absorbed through skin. Causes skin irritation.  
Eye damage/eye irritation  
Toxic if inhaled. Causes respiratory tract irritation.  
Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 1000 lbs.**

LC50 193.00 mg/l - 96 h  
EC50 1,682.00 mg/l - 48 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US) IATA  
UN number: 1593 Class: 6.1 Packing group: III UN number: 1593 Class: 6.1 Packing group: III  
Proper shipping name: Dichloromethane Proper shipping name: Dichloromethane  
Reportable Quantity (RQ): 1000 lbs

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.

# ABSOLUTE STANDARDS, INC.

ISO - 17034



## Certificate of Analysis



### Certified Reference Material (CRM)

**Conformance:** The "Certificate of Analysis" is applicable for CRM's, fulfilling the requirements in the current version of: ISO 17034.

**Health & Safety:** See the attached SDS & Certified Weight Report before use.

**Intended Use:** This Certified Reference Material (CRM) is intended primarily for use in the characterization of unknowns and the establishment of analyzer or instrument response factors by qualified personnel. Typical instrumental organic assays include: GC & LC, and inorganic assays include: ICP & AA. This product is for laboratory use only.

**Characterization Values:** In production, gravimetric/volumetric readings are certified to be within  $\pm 0.5\%$  of the stated value & are valid between 18 °C & 30 °C. The measured characterization of uncertainty can be found on the Certified Weight Report. All product weighings are performed on an analytical balance that is calibrated to NIST Traceable standard weights & certified by the manufacturer. The volumetric glassware used is Class "A" type & conforms to ASTM E-288 unless otherwise stated. The solvents & compounds used are of the highest practical purity & typically meet or exceed ACS Reagent Grade & ACS Standards Grade specifications. The expanded uncertainty field on Certified Wt. Report represents CRM uncertainty as described in ISO 17034.

**Homogeneity:** Uncertainties that are due to the analytical procedure(s) are within  $\pm 0.5\%$  unless specifically stated on the Certified Wt. Report.

**Verification:** Uncertainties that are due to the analytical procedure(s) are within  $\pm 0.5\%$  unless specifically stated on the Certified Wt. Report.

**Stability:** Uncertainties for short-term stability are determined in accordance with ISO 17034. Long-term stability is determined in accordance with ISO 17034. The shelf life is limited by the stated expiration for each product. Expiration dates and additional technical information can be found on the Certified Weight Report and on the product label.

**Uncertainty:** UCRM is the expanded uncertainty which utilizes a  $K = 2$  (coverage factor of 2), in accordance with ISO 17034 as listed above (Characterization, Homogeneity, Verification, and Stability).

**Purity & Identity:** Organic solutions are typically formulated from neat materials whose purity & identity have been characterized by GC-MSD & LC-PDA techniques with comparison to a NIST Traceable library of mass spectra when available. Additional characterization techniques may include but are not limited to: refractive index measurements of liquids, melting point measurements of solids, & GC-FID, ECD, PID, ELCD, LC-PDA measurements for purity. Inorganic solutions & neat are typically formulated from materials whose purity & identity have been characterized by ICPMS with comparison to a NIST SRM® when available. Additional characterization techniques may include but are not limited to: titrimetry, and densitometry.

**Storage:** Sealed ampules and other containers should be stored in the dark and at temperatures indicated on the Certified Weight Report or product label. Certification by Absolute Standards, Inc. is typically valid for 3 years from the date of manufacture. Each product will show its own expiration date as the limit of certification. Certified values are not applicable to opened ampules or for any materials stored in re-sealable containers. Please see the "Certified Weight Report" for specific values and any exceptions.

**Usage:** Ampules & bottles should be brought to room temperature (18 to 30 °C) before opening. Sonication may be required for high concentration solutions or solutions that may precipitate during storage. After opening, care should be exercised to avoid concentration changes owing to evaporation of the solvent or essential components. We recommend that a suitable re-sealable container be available before opening an ampule to decant the standard for short-term storage and use.

**Minimum Sample Size:** 0.5 uL for analytical applications.

**Legal Notice:** Warranty of products are as described when shipped. No warranty as to fitness for any particular application is expressed or implied. Errant shipments and/or quality claims must be made within 10 days of receipt. Liability is limited solely to the replacement of the product or refund of purchase price.

**Certifying Officer:** Stephen J. Arpie, M.S., Director General



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514

Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: Stephen.Arpie@AbsoluteStandards.com

Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019

Page 1 of 2







CERTIFIED WEIGHT REPORT

Part Number: **72072**  
Lot Number: **101122**  
Description: **n-Tetracosane-d50**

Solvent(s):  
Methylene chloride  
Lot#: 105345

<i>Prashant Chauhan</i>		101122
Formulated By:	Prashant Chauhan	DATE
<i>Pedro L. Rentas</i>		101122
Reviewed By:	Pedro L. Rentas	DATE

Expiration Date: 101132  
Recommended Storage: Ambient (20 °C)  
Nominal Concentration (µg/mL): 1000  
NIST Test ID#: 6UTB



Weight(s) shown below were combined and diluted to (mL): 200.0

5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

*P12291*  
*↓*  
*P12310*  
*Y.P.*  
*02/22/23*

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Assay (%)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
											CAS#	OSHA PEL (TWA)	LD50
1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20482	1000.6	4.1	16416-32-3	N/A	N/A

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

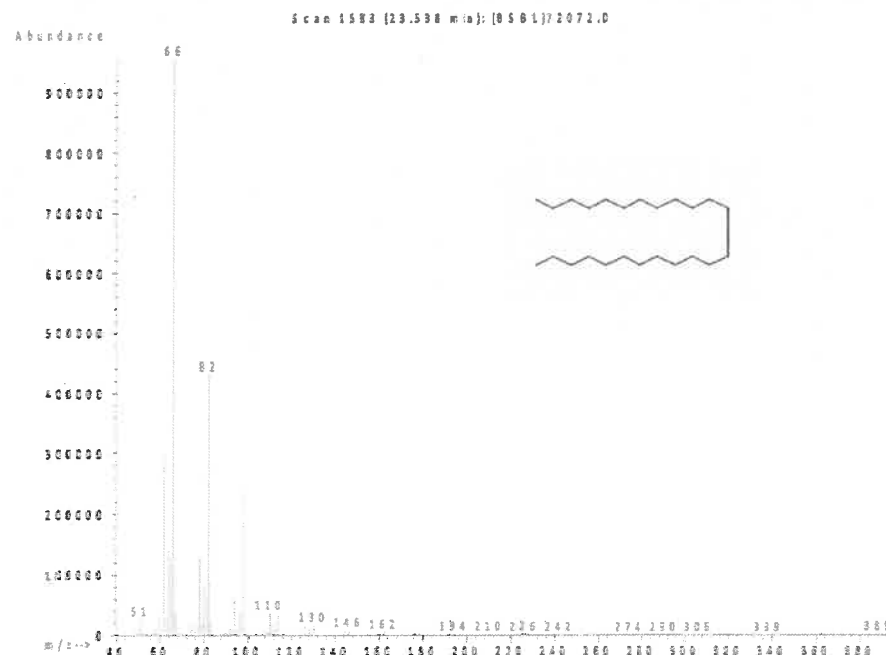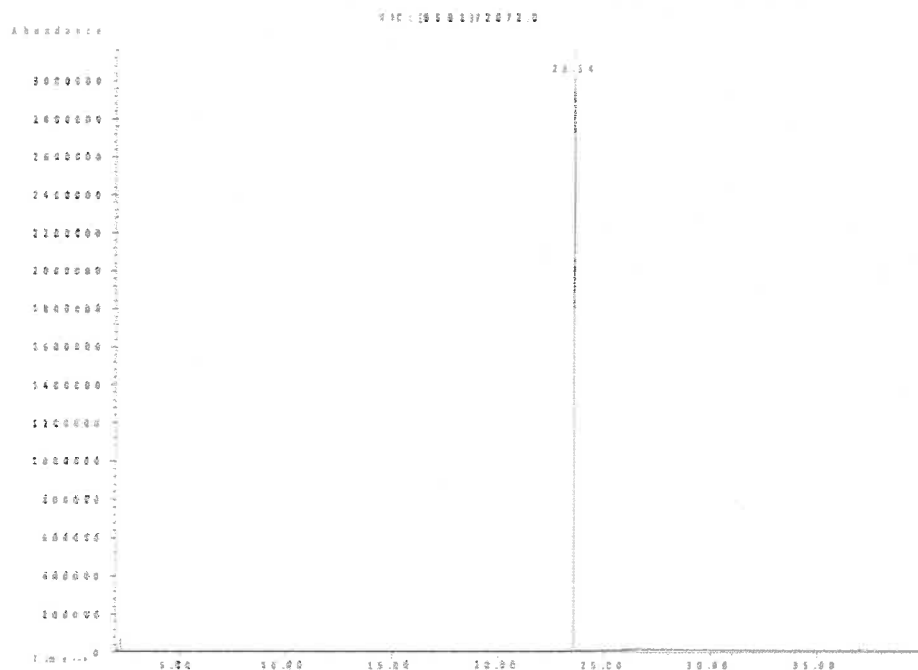

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



## Safety Data Sheet (SDS)

GHS/OSHA Compliant

## Section I Product and Company Identification

## IDENTITY ANALYTICAL STANDARD DISSOLVED IN METHYLENE CHLORIDE

Manufacturer's Name	ABSOLUTE STANDARDS INC	Emergency Telephone USA & CANADA	1-800-535-5053
Address	44 Rosotto Dr. Hamden CT, 06514	Emergency Telephone International Date Prepared/Revised	1-352-323-3500 January 1, 2022

## Section II - Hazards Identification

## GHS Classification in accordance with 29 CFR 1910 (OSHA HCS)

H302	Harmful if swallowed.	H315,H320	Causes skin and eye irritation.
H351	Suspected of causing cancer.	H335	May cause respiratory irritation.
P271	Use in ventilated area	P280	Use gloves, eye protection/face shield
P302,332	If on skin, wash with soap and water	P305,351,338	If in eyes, remove contacts, rinse with water



Signal Word: WARNING

## Section III - Composition

Components:	CAS#:	OSHA PEL (TWA)	LD50 orl-rat	% (optional)
Dichloromethane	75-09-2	50 ppm	> 2,000 mg/kg	> 97

See Certified Weight Report For Other Analytes Present At Trace Quantities.  
INTENDED USE: REFERENCE MATERIAL

## Section IV. FIRST AID MEASURES

**General advice**  
Consult a physician. Show this safety data sheet to the doctor in attendance. Move to safe area.

**If inhaled**  
If inhaled, move person into fresh air. If not breathing, give artificial respiration. Consult a physician.

**In case of skin contact**  
Wash with soap and water. Consult a physician.

**In case of eye contact**  
Rinse thoroughly with plenty of water for at least 15 minutes and consult a physician.

**If swallowed**  
Do NOT induce vomiting. Rinse mouth with water. Consult a physician.

## Section V. FIREFIGHTING MEASURES

**Suitable extinguishing media**  
Use water spray, alcohol-resistant foam, dry chemical or carbon dioxide.

**Protective equipment for fire**  
Wear self contained breathing apparatus for fire fighting if necessary.

## Section VI. ACCIDENTAL RELEASE MEASURES

**Personal precautions**  
Wear respiratory protection. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Remove all sources of ignition. Vapours accumulate to form explosive concentrations.

**Environmental precautions**  
Prevent further leakage or spillage if safe to do so. Do not let product enter drains.

**Clean up**  
Contain spillage, and then collect and place in container for disposal according to local regulations (see section 13).

## Section VII. HANDLING AND STORAGE

**Precautions for safe handling**  
Avoid contact with skin and eyes. Avoid inhalation of vapour or mist.

**Storage Conditions**  
Use ventilation. Keep away from sources of ignition. No smoking. Prevent the build up of electrostatic charge. Keep container tightly closed in a dry and well-ventilated place. Containers which are opened must be carefully resealed and kept upright to prevent leakage.

## Section VIII. EXPOSURE CONTROLS/PERSONAL PROTECTION

Methylene chloride 75-09-2 TWA 50 ppm

Potential for skin absorption, ingestion and inhalation.

Personal protective equipment Respiratory protection Handle with gloves. Gloves must be inspected prior to use. Eye protection.

Avoid contact with skin, eyes and clothing. Wash hands thoroughly after handling the product.

## Section IX - PHYSICAL/CHEMICAL CHARACTERISTICS

Boiling Point	40°C	Specific Gravity (H2O = 1)	1.325
---------------	------	----------------------------	-------

Vapor Pressure (mm Hg)	353	Melting Point	-97°C
Vapor Density (AIR = 1)	2.93	Evaporation rate (Butyl Acetate = 1)	0.71
Solubility in Water	Slightly soluble		

Appearance and Odor CLEAR, COLORLESS LIQUID WITH CHARACTERISTIC PUNGENT ODOR.

**Section X. STABILITY AND REACTIVITY**

Chemical stability	Stable under recommended storage conditions.
Possibility of hazardous reactions	No data available
Conditions to avoid	Heat, flames, sparks, extreme temperature and sunlight.
Materials to avoid	Alkali metals, Aluminum, Oxidizing agents, Bases, Amines, Magnesium, Acids, Vinyl compounds
Hazardous decomposition products	- No data available

**Section XI. TOXICOLOGICAL INFORMATION**

LD50 Oral - Rat - > 2,000 mg/kg  
LC50 Inhalation - Rat - 52,000 mg/m3  
LD50 Dermal - Rat - > 2,000 mg/kg  
Toxic if absorbed through skin. Causes skin irritation.  
Eye damage/eye irritation  
Toxic if inhaled. Causes respiratory tract irritation.  
Toxic if swallowed.

**Section XII. ECOLOGICAL INFORMATION FOR REPORTABLE QUANTITY OF 1000 lbs.**

LC50 193.00 mg/l - 96 h  
EC50 1,682.00 mg/l - 48 h

**Section XIII. DISPOSAL CONSIDERATIONS**

Dispose with normal Laboratory Solvent Waste.

**Section XIV. TRANSPORT INFORMATION**

DOT (US) IATA  
UN number: 1593 Class: 6.1 Packing group: III UN number: 1593 Class: 6.1 Packing group: III  
Proper shipping name: Dichloromethane Proper shipping name: Dichloromethane  
Reportable Quantity (RQ): 1000 lbs

**Section XV. REGULATORY INFORMATION**

OSHA Hazards Flammable liquid, Target Organ Effect, Toxic by inhalation., Toxic by ingestion, Toxic by skin absorption, Irritant  
SARA 302: No chemicals in this material are subject to the reporting requirements of SARA Title III, Section 302.

**Section XVI. Misc. INFORMATION**

The information in this Material Safety Data Sheet meets the requirements of the United States Occupational Safety and Health Act and regulations promulgated thereunder (29 CFR 1910.1200 et. seq.) and Global Harmonized System (GHS). This document is intended only as a guide to the appropriate precautionary handling of the material by trained personnel, or supervised by a person trained in chemical handling. The user is responsible for determining the precautions and dangers of this chemical for his or her particular application. Depending on usage, protective clothing including eye and face guards and respirators must be used to avoid contact with material or breathing chemical vapors/fumes. Exposure to this product may have serious adverse health effects. This chemical may interact with other substances. Since the potential uses are so varied, ABSOLUTE STANDARDS INC. cannot warn of all the potential dangers of use or interaction with other chemicals or substances. ABSOLUTE STANDARDS INC. warrants that the chemical meets the specifications set forth on the label. ABSOLUTE STANDARDS INC. DISCLAIMS ANY OTHER WARRANTIES, EXPRESSED OR IMPLIED WITH REGARD TO THE PRODUCT SUPPLIED HEREUNDER, ITS MERCHANTABILITY OR ITS FITNESS FOR A PARTICULAR APPLICATION. The user should recognize that this product can cause severe injury or death, especially if improperly handled or the known dangers of use are not heeded. READ ALL PRECAUTIONARY INFORMATION. As new documented general safety information becomes available, Absolute Standards Inc. will periodically revise this Material Safety Data Sheet. If you have any questions, please call Technical Service at 1-203-281-2917 for assistance.

# ABSOLUTE STANDARDS, INC.

ISO - 17034



## Certificate of Analysis



### Certified Reference Material (CRM)

**Conformance:** The "Certificate of Analysis" is applicable for CRM's, fulfilling the requirements in the current version of: ISO 17034.

**Health & Safety:** See the attached SDS & Certified Weight Report before use.

**Intended Use:** This Certified Reference Material (CRM) is intended primarily for use in the characterization of unknowns and the establishment of analyzer or instrument response factors by qualified personnel. Typical instrumental organic assays include: GC & LC, and inorganic assays include: ICP & AA. This product is for laboratory use only.

**Characterization Values:** In production, gravimetric/volumetric readings are certified to be within  $\pm 0.5\%$  of the stated value & are valid between 18 °C & 30 °C. The measured characterization of uncertainty can be found on the Certified Weight Report. All product weightings are performed on an analytical balance that is calibrated to NIST Traceable standard weights & certified by the manufacturer. The volumetric glassware used is Class "A" type & conforms to ASTM E-288 unless otherwise stated. The solvents & compounds used are of the highest practical purity & typically meet or exceed ACS Reagent Grade & ACS Standards Grade specifications. The expanded uncertainty field on Certified Wt. Report represents CRM uncertainty as described in ISO 17034.

**Homogeneity:** Uncertainties that are due to the analytical procedure(s) are within  $\pm 0.5\%$  unless specifically stated on the Certified Wt. Report.

**Verification:** Uncertainties that are due to the analytical procedure(s) are within  $\pm 0.5\%$  unless specifically stated on the Certified Wt. Report.

**Stability:** Uncertainties for short-term stability are determined in accordance with ISO 17034. Long-term stability is determined in accordance with ISO 17034. The shelf life is limited by the stated expiration for each product. Expiration dates and additional technical information can be found on the Certified Weight Report and on the product label.

**Uncertainty:** UCRM is the expanded uncertainty which utilizes a  $K = 2$  (coverage factor of 2), in accordance with ISO 17034 as listed above (Characterization, Homogeneity, Verification, and Stability).

**Purity & Identity:** Organic solutions are typically formulated from neat materials whose purity & identity have been characterized by GC-MSD & LC-PDA techniques with comparison to a NIST Traceable library of mass spectra when available. Additional characterization techniques may include but are not limited to: refractive index measurements of liquids, melting point measurements of solids, & GC-FID, ECD, PID, ELCD, LC-PDA measurements for purity. Inorganic solutions & neat are typically formulated from materials whose purity & identity have been characterized by ICPMS with comparison to a NIST SRM® when available. Additional characterization techniques may include but are not limited to: titrimetry, and densitometry.

**Storage:** Sealed ampules and other containers should be stored in the dark and at temperatures indicated on the Certified Weight Report or product label. Certification by Absolute Standards, Inc. is typically valid for 3 years from the date of manufacture. Each product will show its own expiration date as the limit of certification. Certified values are not applicable to opened ampules or for any materials stored in re-sealable containers. Please see the "Certified Weight Report" for specific values and any exceptions.

**Usage:** Ampules & bottles should be brought to room temperature (18 to 30 °C) before opening. Sonication may be required for high concentration solutions or solutions that may precipitate during storage. After opening, care should be exercised to avoid concentration changes owing to evaporation of the solvent or essential components. We recommend that a suitable re-sealable container be available before opening an ampule to decant the standard for short-term storage and use.

**Minimum Sample Size:** 0.5 uL for analytical applications.

**Legal Notice:** Warranty of products are as described when shipped. No warranty as to fitness for any particular application is expressed or implied. Errant shipments and/or quality claims must be made within 10 days of receipt. Liability is limited solely to the replacement of the product or refund of purchase price.

**Certifying Officer:** Stephen J. Arpie, M.S., Director General



Absolute Standards, Inc. • 44 Rossotto Drive • Hamden, CT 06514

Voice: 800-368-1131 • Fax: 800-410-2577 • eMail: Stephen.Arpie@AbsoluteStandards.com

Document Identification: Certificate of Analysis Rev 14, Date Issued: 05/30/2019

Page 1 of 2









110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31266 **Lot No.:** A0204859

**Description :** Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2030 **Storage:** 25°C nominal

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13103 } Y.P.  
↓  
P13112 } 01/12/2024

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Octane (C8)	111-65-9	SHBP9758	99%	504.4 µg/mL	+/- 13.0305
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	503.6 µg/mL	+/- 13.0098
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	503.6 µg/mL	+/- 13.0098
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	504.0 µg/mL	+/- 13.0201
5	n-Hexadecane (C16)	544-76-3	SHBP8192	99%	504.0 µg/mL	+/- 13.0201
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	504.1 µg/mL	+/- 13.0230
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	504.0 µg/mL	+/- 13.0204
8	n-Docosane (C22)	629-97-0	MKQC3882	99%	503.6 µg/mL	+/- 13.0098
9	n-Tetracosane (C24)	646-31-1	MKQC8345	99%	504.0 µg/mL	+/- 13.0201
10	n-Hexacosane (C26)	630-01-3	MKQC4814	99%	504.0 µg/mL	+/- 13.0201
11	n-Octacosane (C28)	630-02-4	BCCG0084	99%	504.0 µg/mL	+/- 13.0201
12	n-Triacontane (C30)	638-68-6	MKQC9436	97%	504.0 µg/mL	+/- 13.0204
13	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	504.0 µg/mL	+/- 13.0201
14	n-Tetratriacontane (C34)	14167-59-0	OML4N	99%	504.4 µg/mL	+/- 13.0305
15	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	504.0 µg/mL	+/- 13.0201
16	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	503.8 µg/mL	+/- 13.0152
17	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	503.6 µg/mL	+/- 13.0098

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

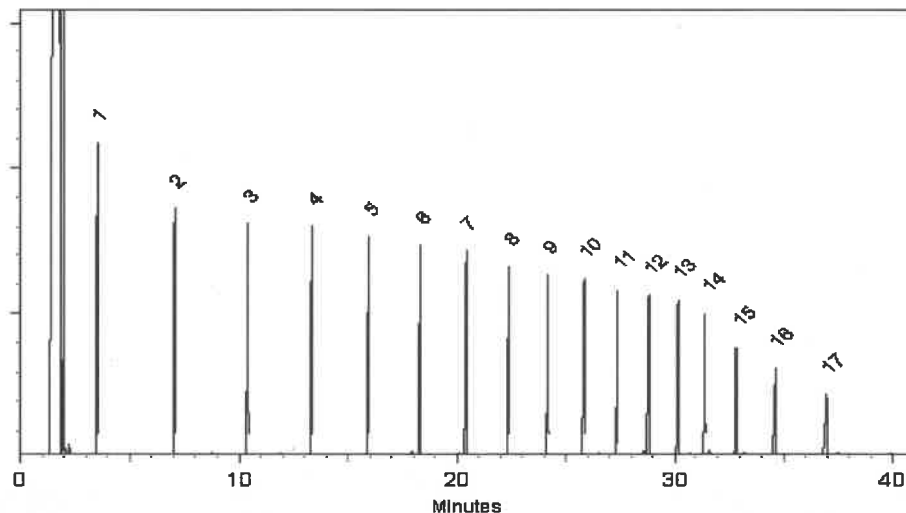

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Dakota Parson - Operations Technician I

**Date Mixed:** 29-Nov-2023

**Balance Serial #** B442140311

  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 01-Dec-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

*chromatographic plus*



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31266 **Lot No.:** A0204859

**Description :** Florida TRPH Standard

Florida TRPH Standard 500µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2030 **Storage:** 25°C nominal

**Handling:** Sonicate prior to use. **Ship:** Ambient

P13103 } Y.P.  
↓  
P13112 } 01/12/2024

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	n-Octane (C8)	111-65-9	SHBP9758	99%	504.4 µg/mL	+/- 13.0305
2	n-Decane (C10)	124-18-5	SHBQ1342	99%	503.6 µg/mL	+/- 13.0098
3	n-Dodecane (C12)	112-40-3	SHBP7054	99%	503.6 µg/mL	+/- 13.0098
4	n-Tetradecane (C14)	629-59-4	STBK5437	99%	504.0 µg/mL	+/- 13.0201
5	n-Hexadecane (C16)	544-76-3	SHBP8192	99%	504.0 µg/mL	+/- 13.0201
6	n-Octadecane (C18)	593-45-3	UE5NG	98%	504.1 µg/mL	+/- 13.0230
7	n-Eicosane (C20)	112-95-8	MKCN8767	97%	504.0 µg/mL	+/- 13.0204
8	n-Docosane (C22)	629-97-0	MKQC3882	99%	503.6 µg/mL	+/- 13.0098
9	n-Tetracosane (C24)	646-31-1	MKQC8345	99%	504.0 µg/mL	+/- 13.0201
10	n-Hexacosane (C26)	630-01-3	MKQC4814	99%	504.0 µg/mL	+/- 13.0201
11	n-Octacosane (C28)	630-02-4	BCCG0084	99%	504.0 µg/mL	+/- 13.0201
12	n-Triacontane (C30)	638-68-6	MKQC9436	97%	504.0 µg/mL	+/- 13.0204
13	n-Dotriacontane (C32)	544-85-4	BCBW0661	99%	504.0 µg/mL	+/- 13.0201
14	n-Tetratriacontane (C34)	14167-59-0	OML4N	99%	504.4 µg/mL	+/- 13.0305
15	n-Hexatriacontane (C36)	630-06-8	Z27H018	99%	504.0 µg/mL	+/- 13.0201
16	n-Octatriacontane (C38)	7194-85-6	0000145137	96%	503.8 µg/mL	+/- 13.0152
17	n-Tetracontane (C40)	4181-95-7	OKEGA	99%	503.6 µg/mL	+/- 13.0098

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**  
30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**  
hydrogen-constant pressure 10 psi.

**Temp. Program:**  
40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)


**Inj. Temp:**  
250°C

**Det. Temp:**  
330°C

**Det. Type:**  
FID

**Split Vent:**  
2 ml/min.

**Inj. Vol**  
1µl

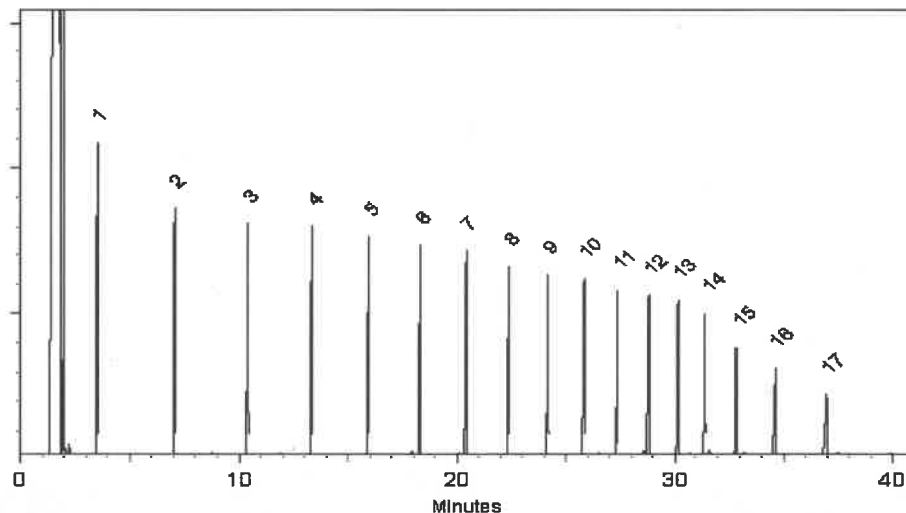

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Dakota Parson - Operations Technician I

**Date Mixed:** 29-Nov-2023

**Balance Serial #** B442140311

  
Jennifer Pollino - Operations Tech III - ARM QC

**Date Passed:** 01-Dec-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ uncertainty} = k \sqrt{u_{gravimetric}^2 + u_{homogeneity}^2 + u_{storage\ stability}^2 + u_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.







Certified Reference Material CRM



CERTIFIED WEIGHT REPORT

Part Number:  
Lot Number:  
Description:

72072  
101122  
n-Tetracosane-d50

Solvent(s):  
Methylene chloride

Lot#  
105345

Expiration Date:  
Recommended Storage:  
Nominal Concentration (µg/mL):  
NIST Test ID#:

101132  
Ambient (20 °C)  
1000  
6UTB

5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 200.0

Formulated By:	Prashant Chauhan	101122	DATE
Reviewed By:	Pedro L. Renteria	101122	DATE


SDS Information

Expanded  
Uncertainty  
(Solvent Safety Info. On Attached pg.)  
CAS# OSHA PEL (TWA) LD50


Compound	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20482	1000.6	4.1	16416-32-3	N/A
----------	------	----------	------	------	-----	------	---------	---------	--------	-----	------------	-----

1. n-Tetracosane-d50  
Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

FIGURE 1: 72072.D

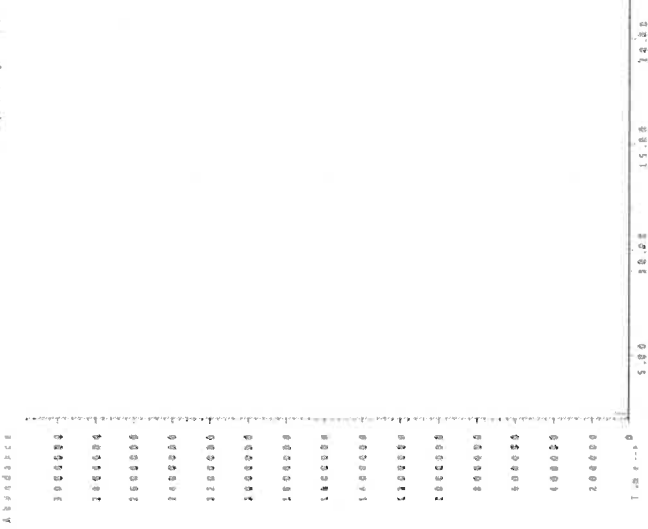

Scan 1589 (3.538 min.): 1053172072.D

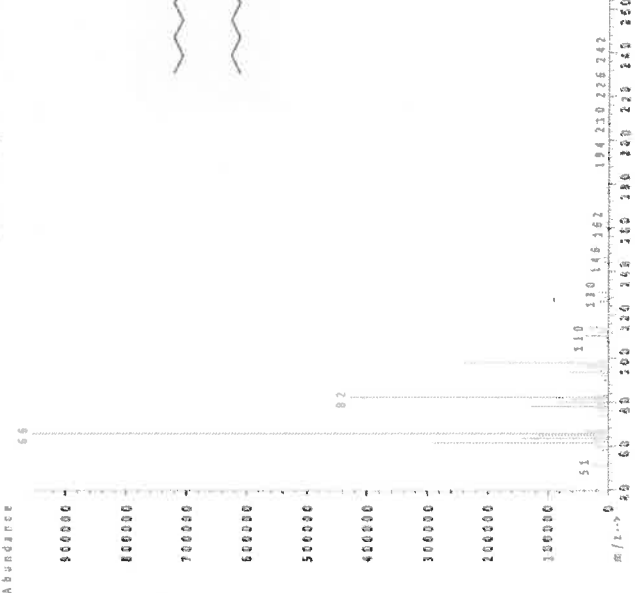

P13205  
↓  
P13214  
A3  
61/17/24

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.  
All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Certified Reference Material CRM



CERTIFIED WEIGHT REPORT

Part Number:  
Lot Number:  
Description:

72072  
101122  
n-Tetracosane-d50

Solvent(s):  
Methylene chloride

Lot#  
105345

Expiration Date:  
Recommended Storage:  
Nominal Concentration (µg/mL):  
NIST Test ID#:

101132  
Ambient (20 °C)  
1000  
6UTB

5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 200.0

Formulated By:	Prashant Chauhan	101122	DATE
Reviewed By:	Pedro L. Renteria	101122	DATE

SDS Information

Expanded Uncertainty (Solvent Safety Info. On Attached pg.)  
Actual Conc (µg/mL) (+/-) (µg/mL) CAS# OSHA PEL (TWA) LD50

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Purity Uncertainty (%)	Assay (%D)	Target Weight(g)	Actual Weight(g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50
1. n-Tetracosane-d50	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20482	1000.6	4.1	16416-32-3	N/A	N/A

Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.


FIGURE 1: 100% TMS



Abundance



Scan 1589 (3.538 min): [M+H]<sup>+</sup> 386.4

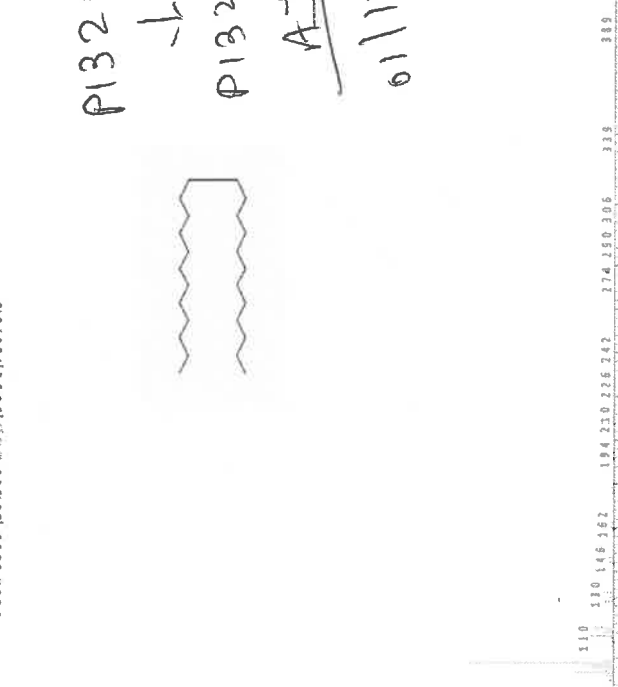

P13205  
P13214  
A3  
61/17/24

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.

Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).

Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.

All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.

Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Certified Reference Material CRM



CERTIFIED WEIGHT REPORT

Part Number:  
Lot Number:  
Description:

72072  
101122  
n-Tetracosane-d50

Solvent(s):  
Methylene chloride

Lot#  
105345

Expiration Date:  
Recommended Storage:  
Nominal Concentration (µg/mL):  
NIST Test ID#:

101132  
Ambient (20 °C)  
1000  
6UTB

5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

Weight(s) shown below were combined and diluted to (mL): 200.0

Formulated By:	Prashant Chauhan	101122	DATE
Reviewed By:	Pedro L. Renteria	101122	DATE


SDS Information

Expanded  
Uncertainty  
(Solute Safety Info. On Attached pg.)  
CAS# OSHA PEL (TWA) LD50

Compound	2072	PR-26606	1000	98.7	0.2	99.0	0.20471	0.20482	1000.6	4.1	16416-32-3	N/A	N/A
----------	------	----------	------	------	-----	------	---------	---------	--------	-----	------------	-----	-----

1. n-Tetracosane-d50  
Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

116 1053172072.0

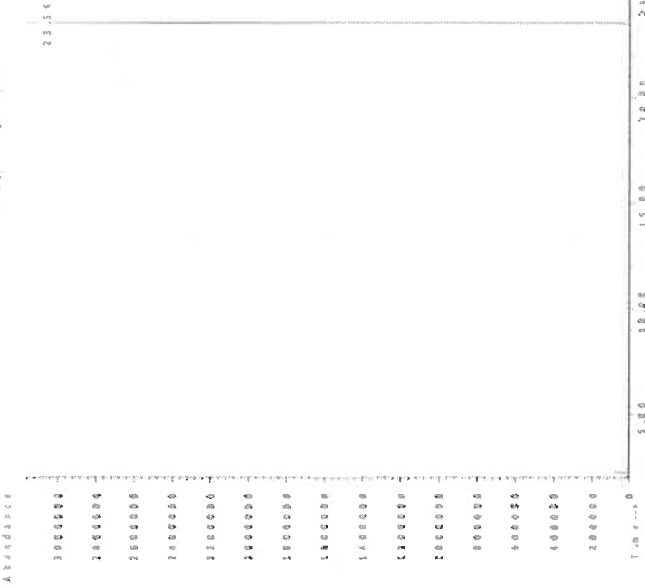

Scan 1589 (3.538 min.): 1053172072.0



P13205  
P13214  
A3  
61/17/24

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.  
Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).  
Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.  
All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.  
Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



# CERTIFIED WEIGHT REPORT

<b>Part Number:</b>	
<b>Lot Number:</b>	
<b>Description:</b>	

**72072**  
**101122**  
**n-Tetracosane-d50**

<b>Solvent(s):</b>	<b>Lot#</b>
Methylene chloride	105345

Formulated By:	Prashant Chauhan	DATE:	10/11/22
----------------	------------------	-------	----------

Expiration Date:	101132
Recommended Storage:	Ambient (20 °C)

Nominal Concentration ( $\mu\text{g/mL}$ ):  
NIST Test ID#:

**Weight(s) shown below were combined and diluted to (mL):**


5E-05 Balance Uncertainty  
0.058 Flask Uncertainty

## SDS Information

Uncertainty (+/-) (ug/mL)	CAS#	OSHA PEL (TWA)	LD50
------------------------------	------	----------------	------

[illegible]

**Method GC8MSD-3.M:** Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Plate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.

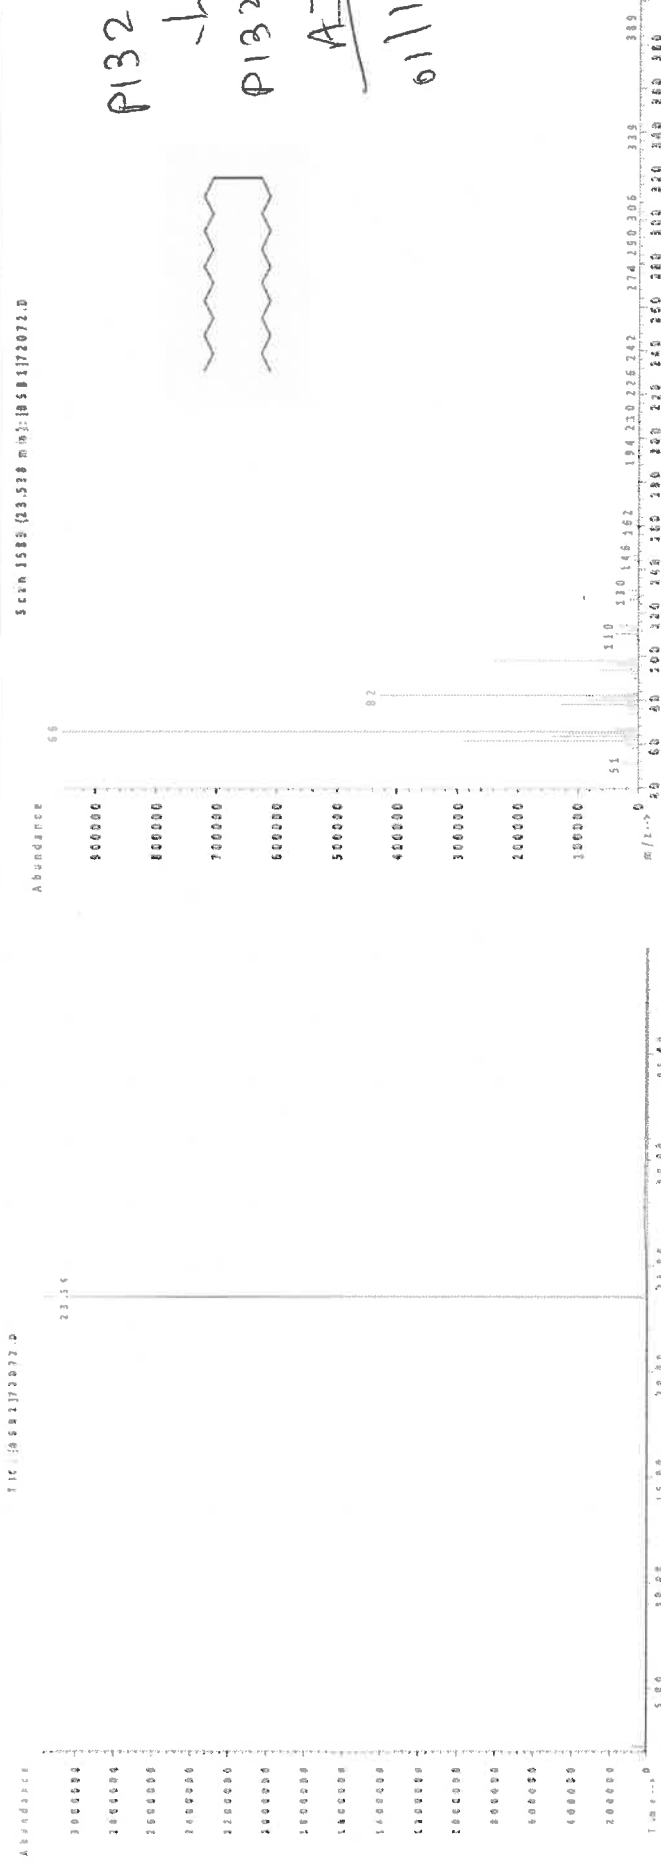

• The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.

- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).

• Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.

- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.

• **Uncertainty Reference:** Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result,"

NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



5580 Skylane Blvd  
Santa Rosa, CA 95403  
(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

Date Received: \_\_\_\_\_

## Certificate of Analysis

Page 1 of 1

Catalog No.: Lot No.: Storage:

Z-110400-05 514983 ≤-10 Degrees C

Solvent:

Hexane

Exp. Date:

11/20/2028

Description:

TRPH Standard (C8-C40), 500 mg/L, 1 ml

-01

### Compound

CAS No.

Purity (%)

Compound Lot No.

Concentration, mg/L

decane (C10)

124-18-5

99.7

415.7.2P

498.5 ± 6.92

docosane (C22)

629-97-0

98.8

420.9.1P

499.4 ± 6.93

dodecane (C12)

112-40-3

99.7

416.9.3P

502 ± 6.97

dotriacontane (C32)

544-85-4

97

425.9.2.2P

499.6 ± 8.53

eicosane (C20)

112-95-8

99.8

419.7.1P

501 ± 6.95

hexacosane (C26)

630-01-3

99.3

422.7.2.1P

501 ± 6.95

hexatriacontane (C36)

630-06-8

98

427.29.1.1P

499.3 ± 8.53

n-hexadecane (C16)

544-76-3

99.45

368.27.1.1P

498.7 ± 6.91

octacosane (C28)

630-02-4

99.1

423.24.1P

500.5 ± 6.95

n-octadecane (C18)

593-45-3

99.5

418.29.1P

499.5 ± 6.92

octane (C8)

111-65-9

99.4

385.7.2.1P

498.5 ± 6.92

octatriacontane (C38)

7194-85-6

95

428.1.2P

500.2 ± 6.94

tetracontane (C40)

4181-95-7

97

429.7.2P

499.6 ± 6.93

n-tetracosane (C24)

646-31-1

99.5

421.7.1P

499.5 ± 6.93

n-tetradecane (C14)

629-59-4

99.3

417.9.1P

500 ± 6.94

tetatriacontane (C34)

14167-59-0

96.1

426.7.2.2P

499.7 ± 8.53

triacontane (C30)

638-68-6

99.5

424.7.1.1P

500 ± 6.94

Let the standard warm to room temperature and sonicate before opening.

P13215

↓

P13224

AJ  
01131124

\*Not a certified value

*Andrea Schaible*

Andrea Schaible  
Chemist

Certified By: \_\_\_\_\_

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.



5580 Skylane Blvd  
Santa Rosa, CA 95403

Manufacturer's Quality System  
Audited & Registered  
by TUV USA to ISO 9001:2015

(707)525-5788  
(800)878-7654 Toll Free  
(707)545-7901 Fax

Date Received: \_\_\_\_\_

## Certificate of Analysis

Page 1 of 1

Catalog No.: Lot No.: Storage:

Z-110400-05 514983 ≤ -10 Degrees C

Solvent:

Hexane

Exp. Date:

11/20/2028

Description:

TRPH Standard (C8-C40), 500 mg/L, 1 ml

-01

### Compound

CAS No.

Purity (%)

Compound Lot No.

Concentration, mg/L

decane (C10)

124-18-5

99.7

415.7.2P

498.5 ± 6.92

docosane (C22)

629-97-0

98.8

420.9.1P

499.4 ± 6.93

dodecane (C12)

112-40-3

99.7

416.9.3P

502 ± 6.97

dotriacontane (C32)

544-85-4

97

425.9.2.2P

499.6 ± 8.53

eicosane (C20)

112-95-8

99.8

419.7.1P

501 ± 6.95

hexacosane (C26)

630-01-3

99.3

422.7.2.1P

501 ± 6.95

hexatriacontane (C36)

630-06-8

98

427.29.1.1P

499.3 ± 8.53

n-hexadecane (C16)

544-76-3

99.45

368.27.1.1P

498.7 ± 6.91

octacosane (C28)

630-02-4

99.1

423.24.1P

500.5 ± 6.95

n-octadecane (C18)

593-45-3

99.5

418.29.1P

499.5 ± 6.92

octane (C8)

111-65-9

99.4

385.7.2.1P

498.5 ± 6.92

octatriacontane (C38)

7194-85-6

95

428.1.2P

500.2 ± 6.94

tetracontane (C40)

4181-95-7

97

429.7.2P

499.6 ± 6.93

n-tetracosane (C24)

646-31-1

99.5

421.7.1P

499.5 ± 6.93

n-tetradecane (C14)

629-59-4

99.3

417.9.1P

500 ± 6.94

tetatriacontane (C34)

14167-59-0

96.1

426.7.2.2P

499.7 ± 8.53

triacontane (C30)

638-68-6

99.5

424.7.1.1P

500 ± 6.94

Let the standard warm to room temperature and sonicate before opening.

P13215

↓

P13224

AJ  
01131124

\*Not a certified value

*Andrea Schaible*

Certified By: \_\_\_\_\_  
Andrea Schaible  
Chemist

All weights are traceable through N. I. S. T. Test No. 822/264157-00.  
Concentration (correct for purity) and uncertainty (95% confidence) values  
listed are determined gravimetrically.