


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080924\
Data File : BF138878.D
Acq On : 09 Aug 2024 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

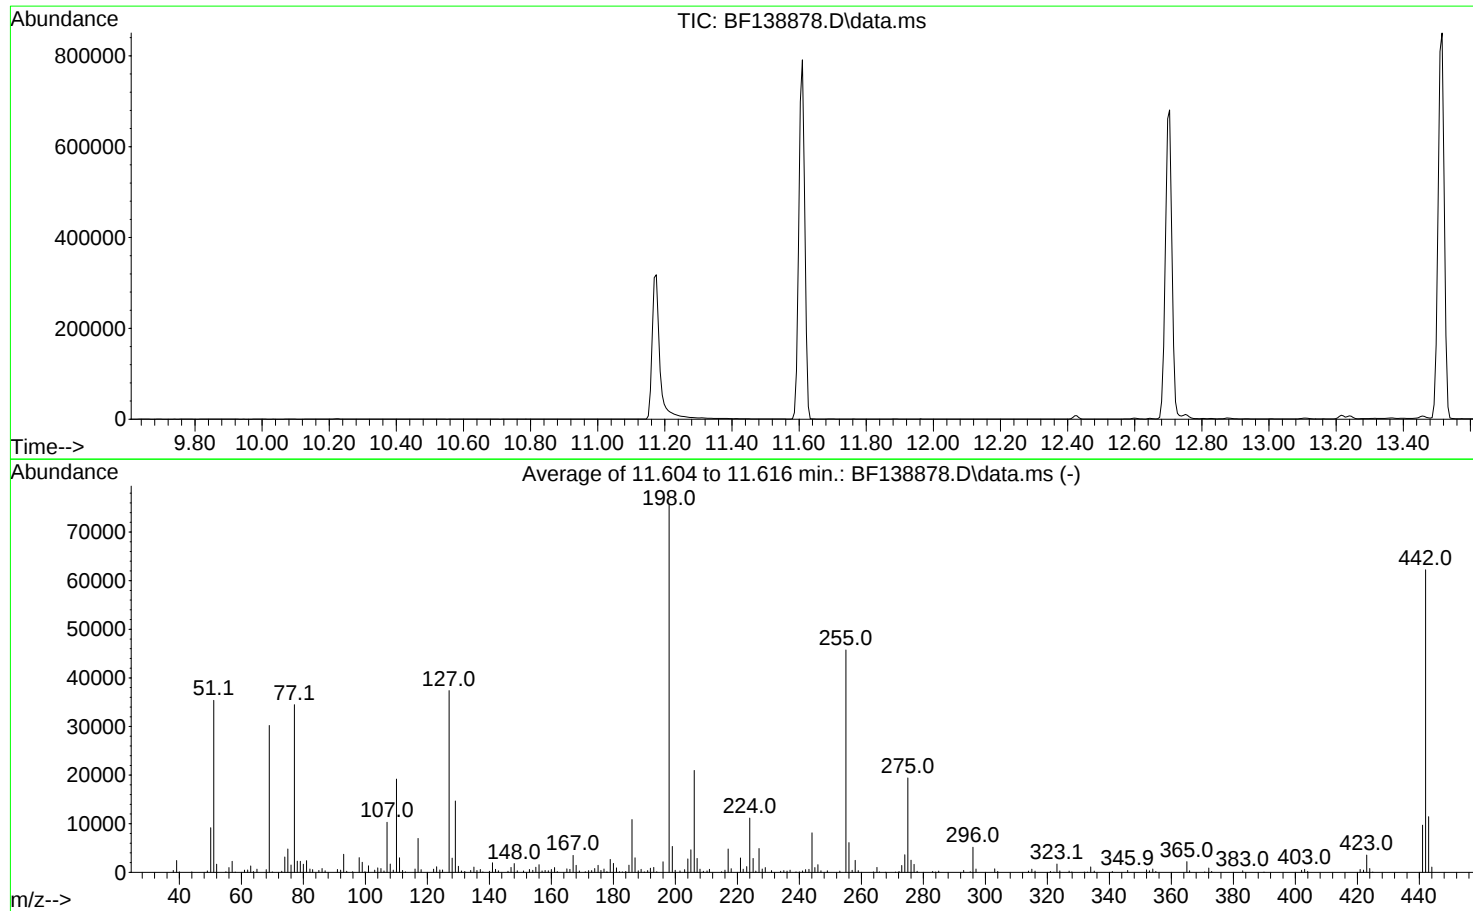

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1610

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	46.8	35389	PASS
68	69	0.00	2	1.9	576	PASS
69	198	0.00	100	39.9	30211	PASS
70	69	0.00	2	0.4	118	PASS
127	198	10	80	49.4	37373	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75667	PASS
199	198	5	9	7.1	5335	PASS
275	198	10	60	25.7	19429	PASS
365	198	1	100	2.9	2201	PASS
441	198	0.01	100	12.8	9714	PASS
442	442	50	100	100.0	62237	PASS
443	442	15	24	18.4	11446	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/9/2024	BNA_F	<u>BF138878.D</u>
Compound Name	Response	Retention Time
DDT	209857	13.515
DDD	5443	13.215
DDE	1045	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6488	216345	3.00

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080924\
Data File : BF138878.D
Acq On : 09 Aug 2024 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 09 10:51:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

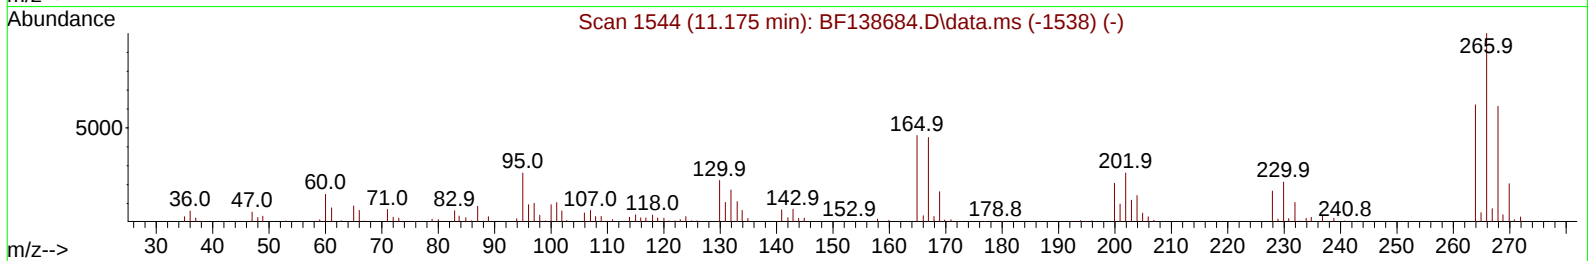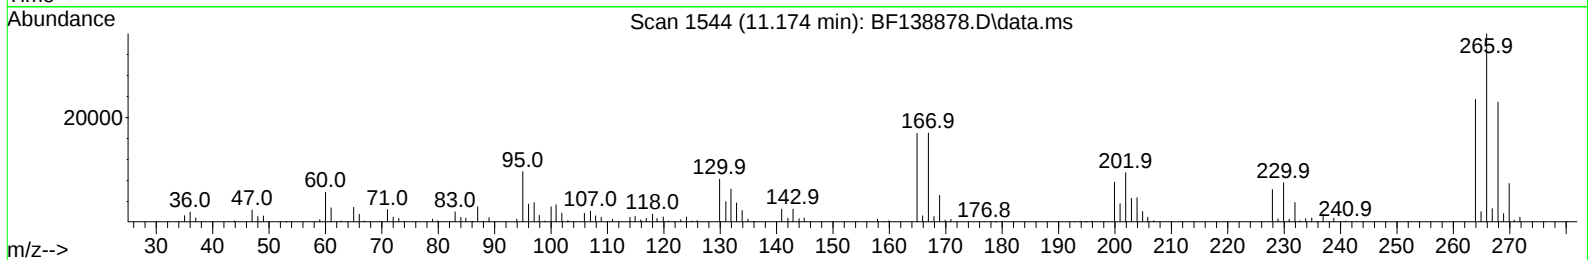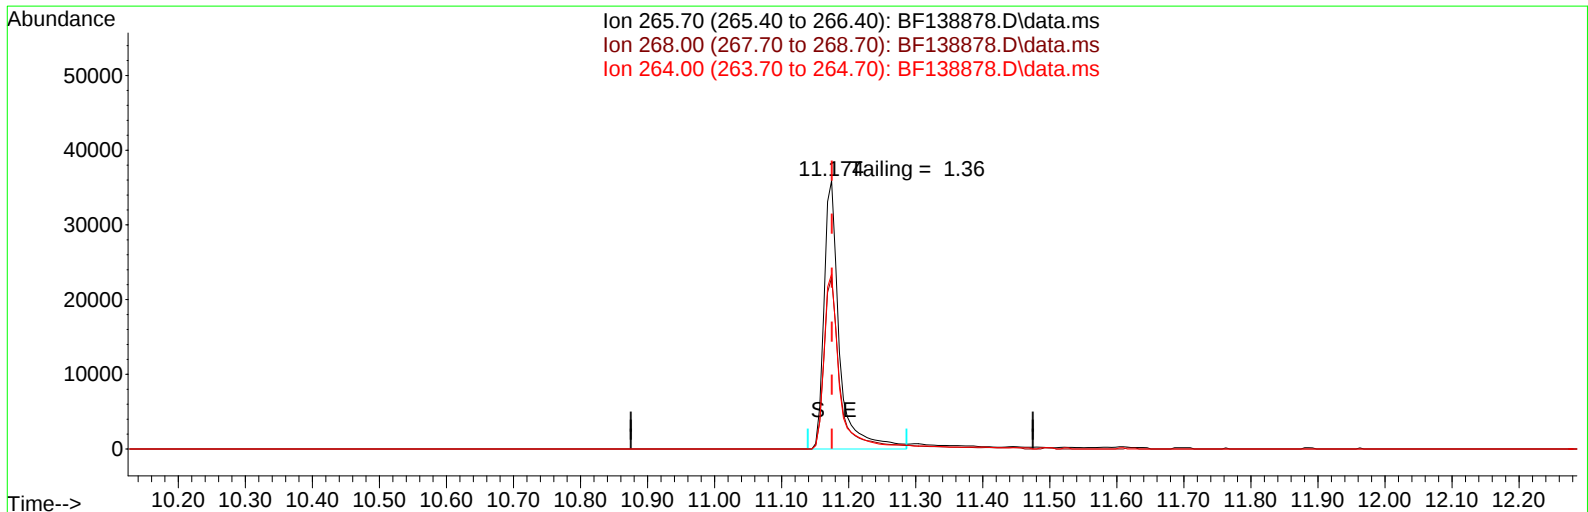

TIC: BF138878.D\data.ms

(70) Pentachlorophenol (C)

11.174min (-0.001) 26324.57 ng




response 57700

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.86
264.00	62.20	65.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080924\
Data File : BF138878.D
Acq On : 09 Aug 2024 09:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 09 10:51:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

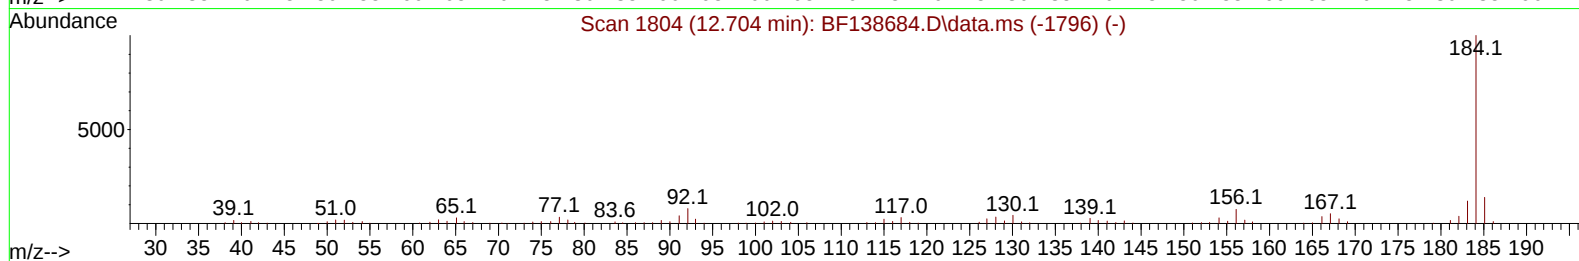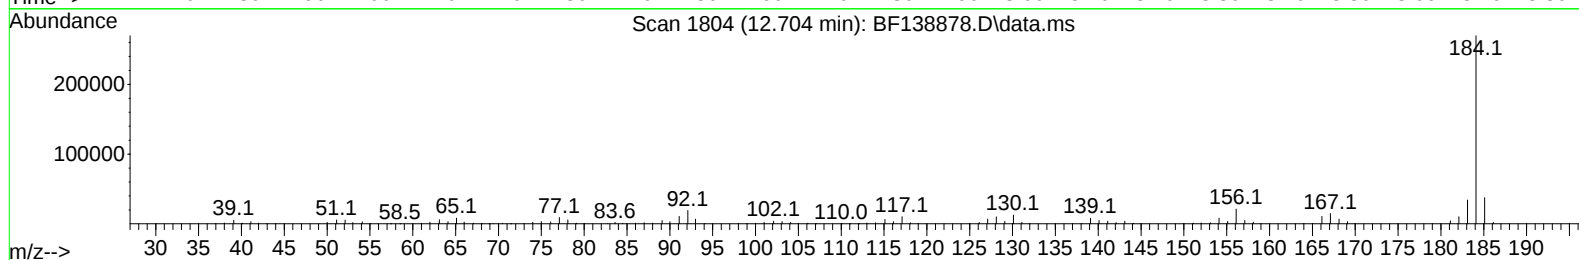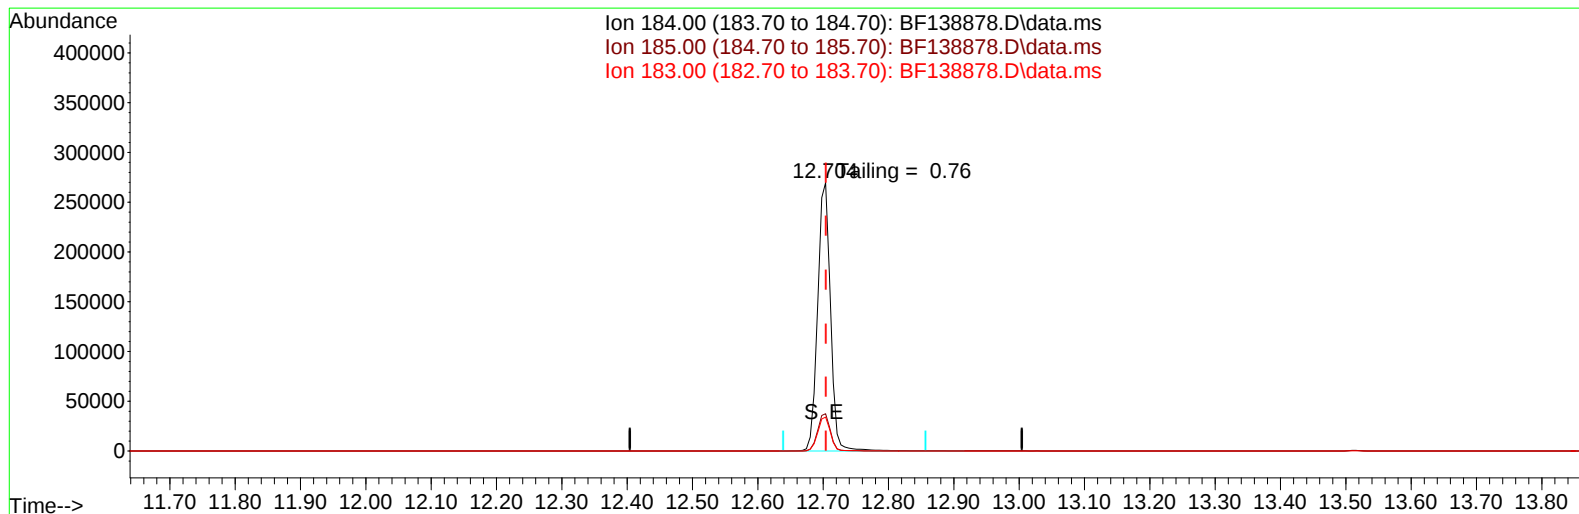

TIC: BF138878.D\data.ms

(77) Benzidine

12.704min (-0.000) 0.00 ng

response 368946

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.92
183.00	12.00	12.68
0.00	0.00	0.00