


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081024\
Data File : BF138900.D
Acq On : 10 Aug 2024 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

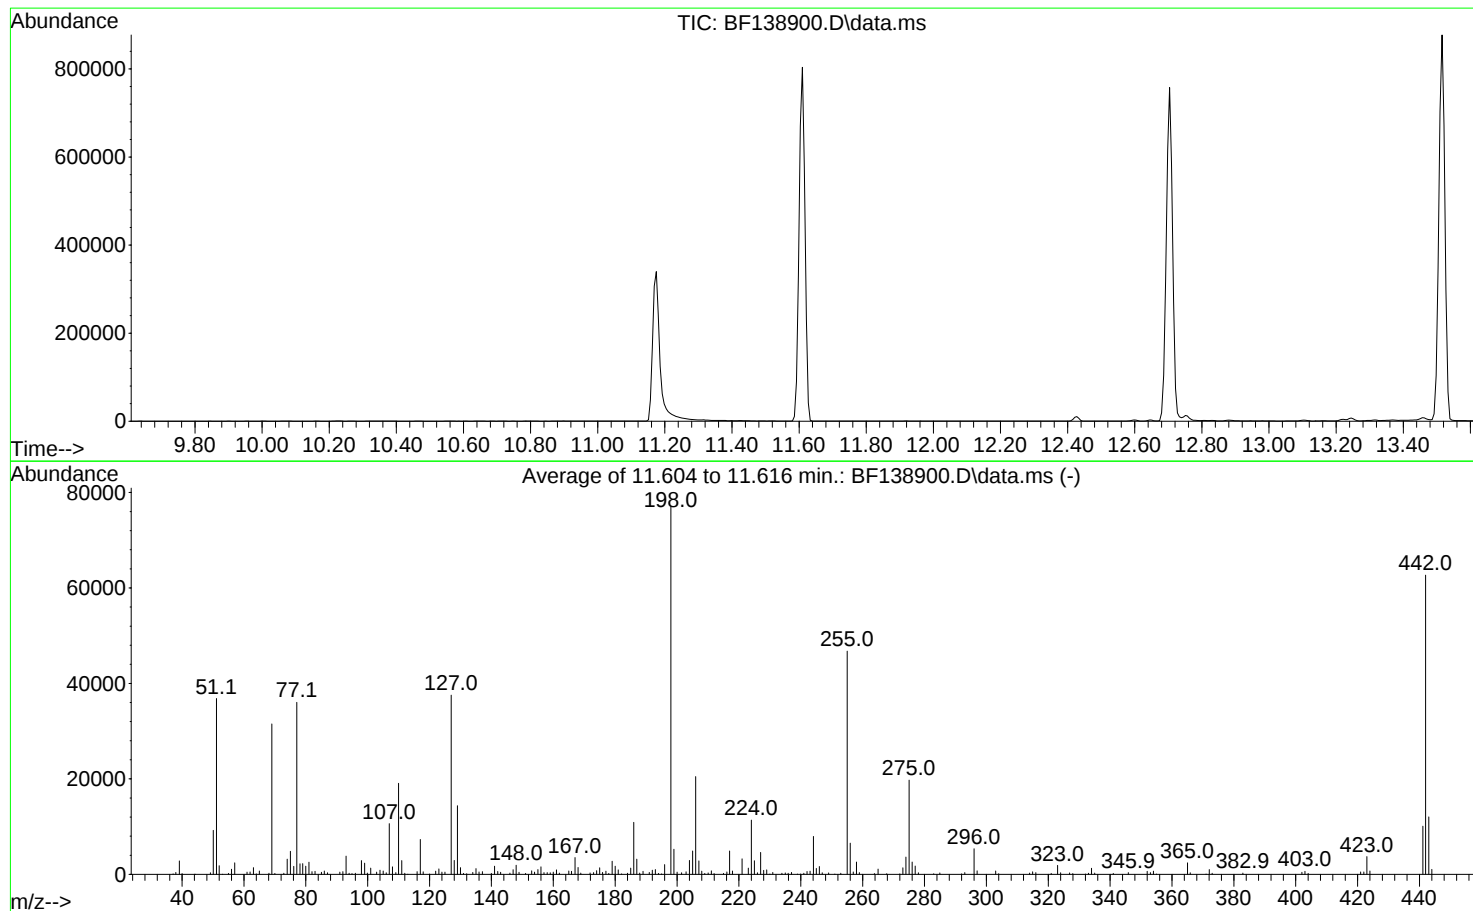

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.8	36840	PASS
68	69	0.00	2	0.8	242	PASS
69	198	0.00	100	40.9	31507	PASS
70	69	0.00	2	0.6	200	PASS
127	198	10	80	48.7	37536	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	77061	PASS
199	198	5	9	6.8	5274	PASS
275	198	10	60	25.6	19728	PASS
365	198	1	100	3.1	2410	PASS
441	198	0.01	100	13.1	10083	PASS
442	442	50	100	100.0	62667	PASS
443	442	15	24	19.2	12045	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/10/2024	BNA_F	<u>BF138900.D</u>
Compound Name	Response	Retention Time
DDT	206441	13.515
DDD	4194	13.245
DDE	1167	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5361	211802	2.53

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081024\
Data File : BF138900.D
Acq On : 10 Aug 2024 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 12 00:49:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

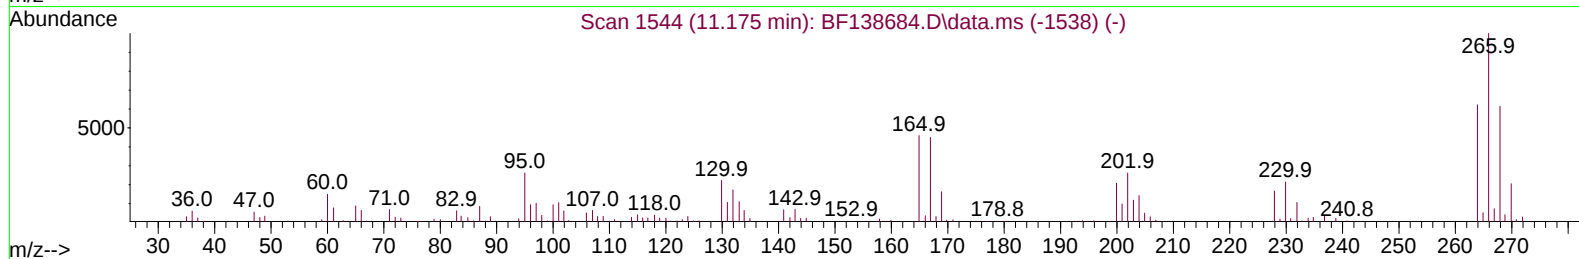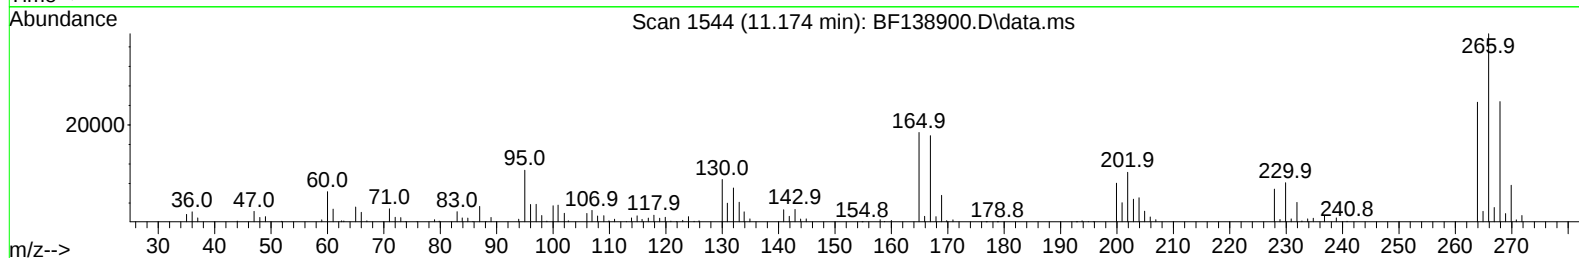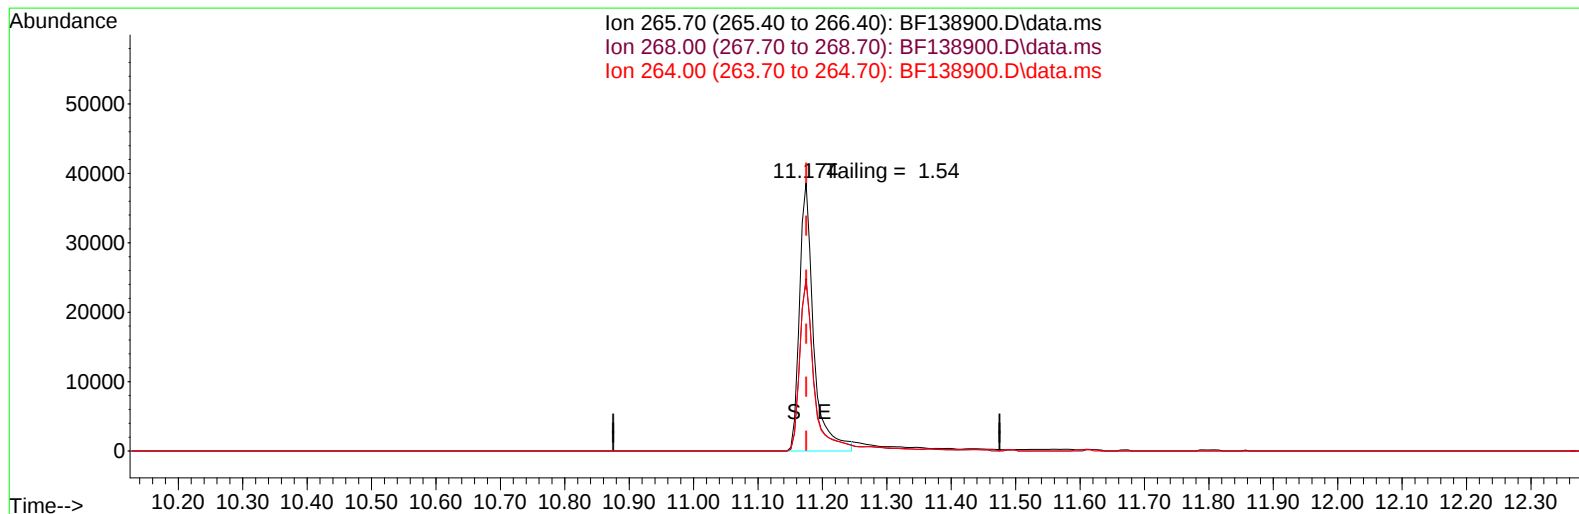

TIC: BF138900.D\data.ms

(70) Pentachlorophenol (C)

11.174min (-0.001) 42180.16 ng




response 64186

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	64.11
264.00	62.20	63.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081024\
Data File : BF138900.D
Acq On : 10 Aug 2024 10:12
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 12 00:49:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

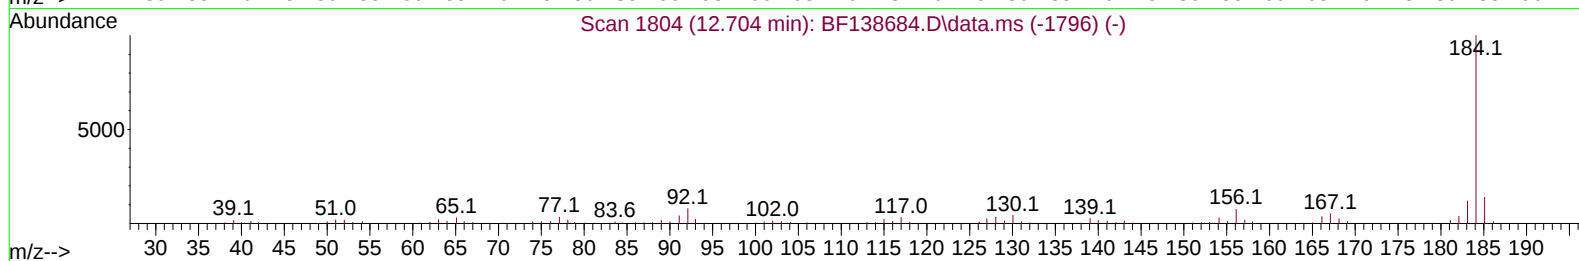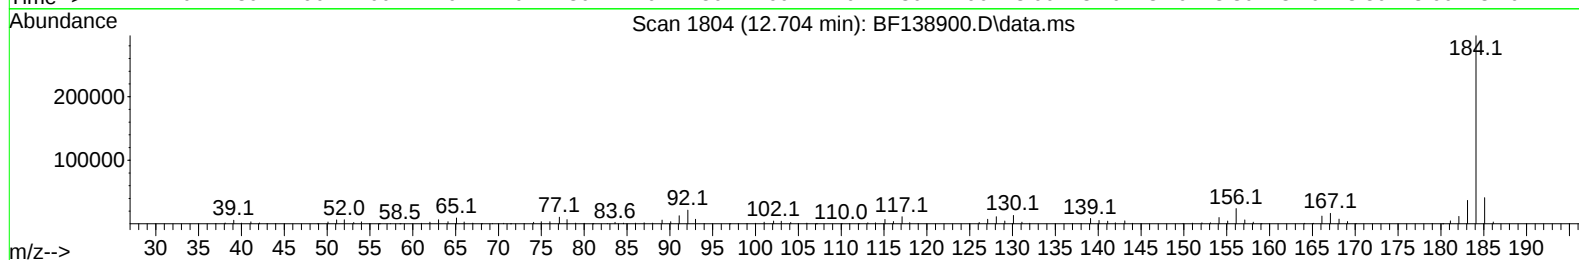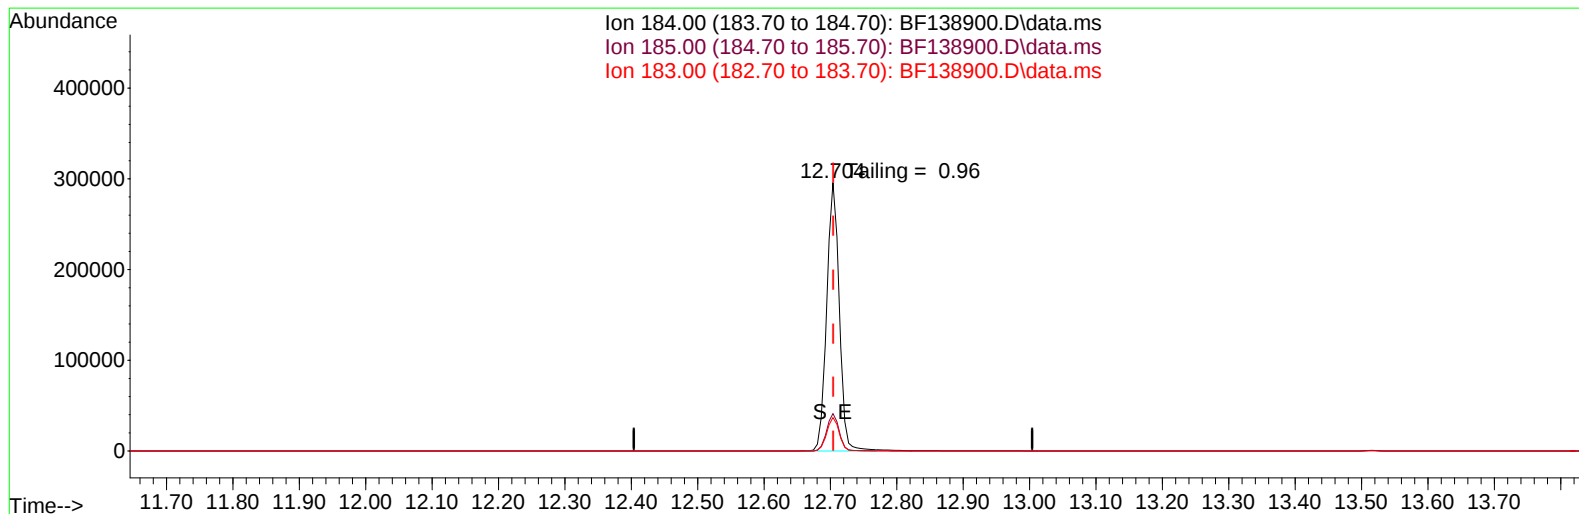

TIC: BF138900.D\data.ms

(77) Benzidine

12.704min (-0.000) 0.00 ng

response 391893

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.95
183.00	12.00	12.47
0.00	0.00	0.00