

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080924\
Data File : BF138883.D
Acq On : 09 Aug 2024 11:52
Operator : RC/JU
Sample : PB162423BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB162423BL

Quant Time: Aug 09 12:30:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.840	152	40879	20.000	ng	0.00
21) Naphthalene-d8	8.122	136	169292	20.000	ng	0.00
39) Acenaphthene-d10	9.875	164	101270	20.000	ng	0.00
64) Phenanthrene-d10	11.357	188	195894	20.000	ng	-0.01
76) Chrysene-d12	13.998	240	116610	20.000	ng	0.00
86) Perylene-d12	15.463	264	79046	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.481	112	425919	160.833	ng	0.01
7) Phenol-d6	6.487	99	571773	160.814	ng	0.00
23) Nitrobenzene-d5	7.404	82	372319	107.525	ng	0.00
42) 2,4,6-Tribromophenol	10.669	330	148717	179.277	ng	0.00
45) 2-Fluorobiphenyl	9.192	172	713549	105.866	ng	-0.01
79) Terphenyl-d14	12.945	244	896366	128.699	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080924\
Data File : BF138883.D
Acq On : 09 Aug 2024 11:52
Operator : RC/JU
Sample : PB162423BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB162423BL


Quant Time: Aug 09 12:30:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

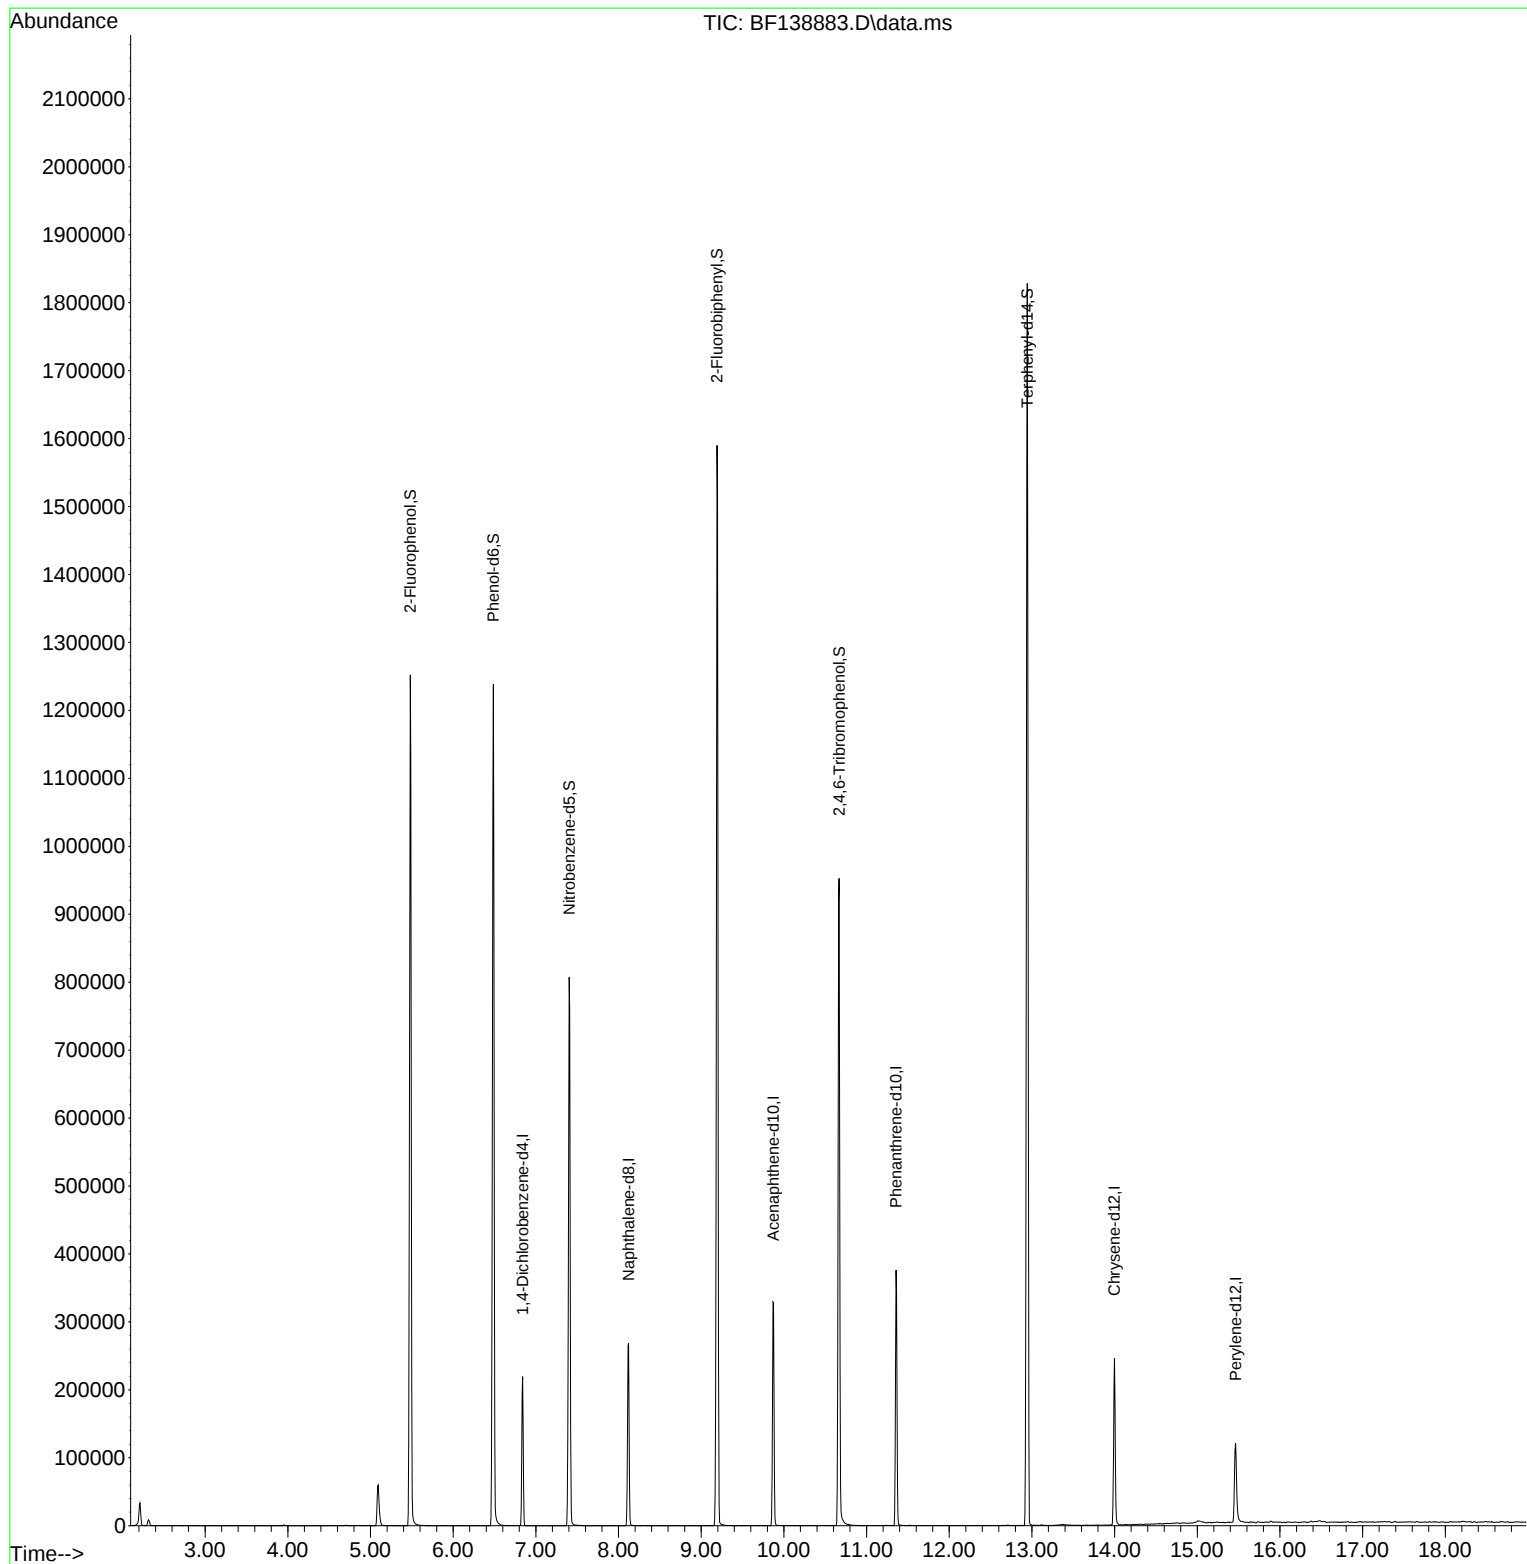





#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.840 min Scan# 80
Delta R.T. -0.005 min
Lab File: BF138883.D
Acq: 09 Aug 2024 11:52

Instrument :
BNA_F
ClientSampleId :
PB162423BL



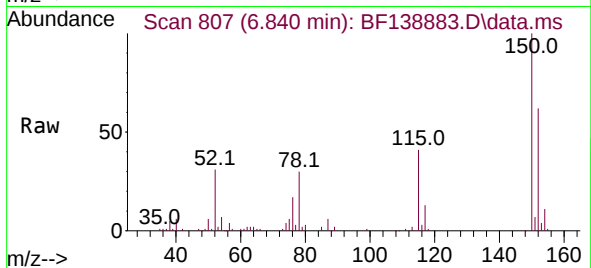


Tgt Ion:152 Resp: 40879
Ion Ratio Lower Upper
152 100
150 160.3 126.0 189.0
115 66.4 51.7 77.5

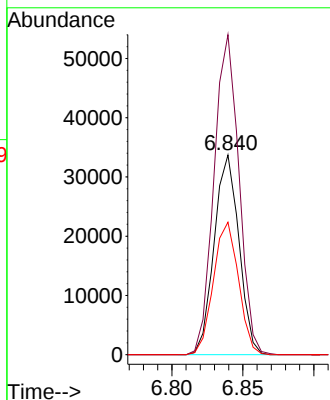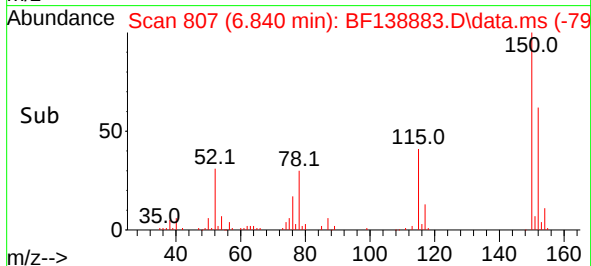

#5
2-Fluorophenol
Concen: 160.833 ng
RT: 5.481 min Scan# 576
Delta R.T. 0.012 min
Lab File: BF138883.D
Acq: 09 Aug 2024 11:52


Tgt Ion:112 Resp: 425919
Ion Ratio Lower Upper
112 100
64 69.5 54.2 81.4
63 38.6 28.7 43.1

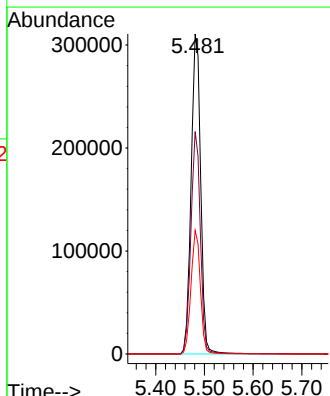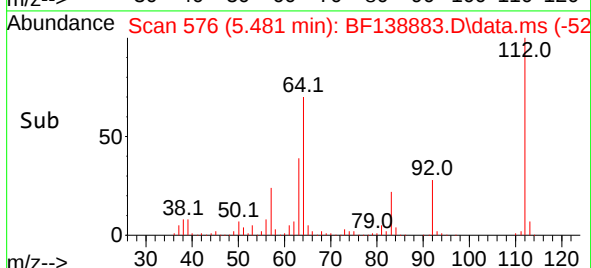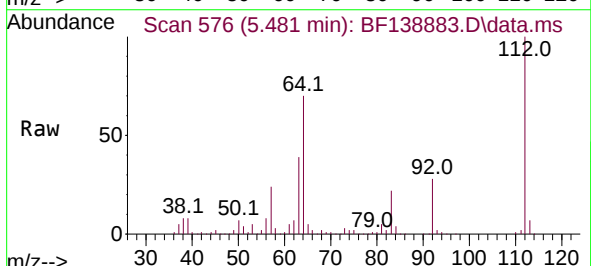





#7
Phenol-d6
Concen: 160.814 ng
RT: 6.487 min Scan# 74
Delta R.T. 0.000 min
Lab File: BF138883.D
Acq: 09 Aug 2024 11:52


Instrument :
BNA_F
ClientSampleId :
PB162423BL

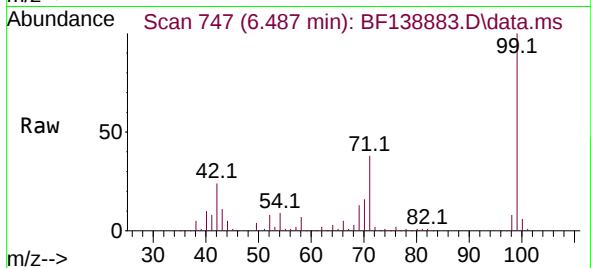



Tgt Ion: 99 Resp: 571773
Ion Ratio Lower Upper
99 100
42 23.7 17.4 26.0
71 38.4 28.1 42.1

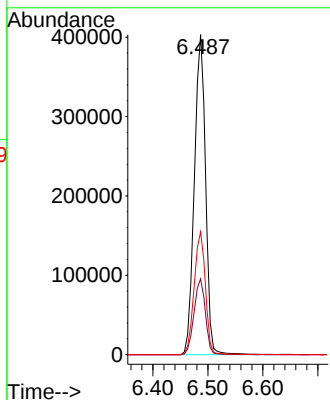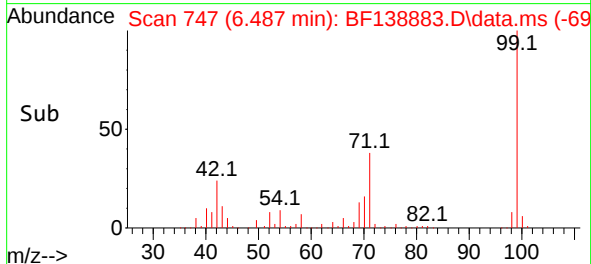


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.122 min Scan# 1025
Delta R.T. -0.006 min
Lab File: BF138883.D
Acq: 09 Aug 2024 11:52

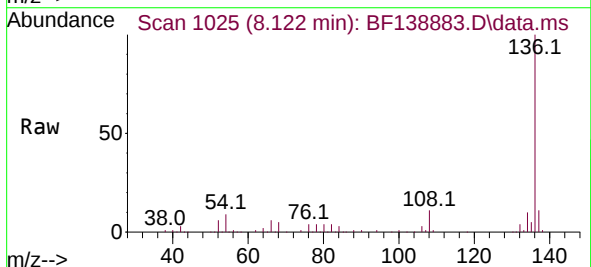

Tgt Ion: 136 Resp: 169292
Ion Ratio Lower Upper
136 100
137 10.9 8.9 13.3
54 9.5 8.6 12.8
68 5.0 4.8 7.2

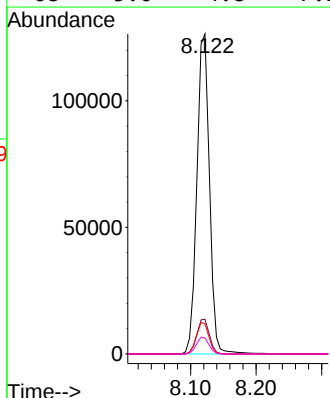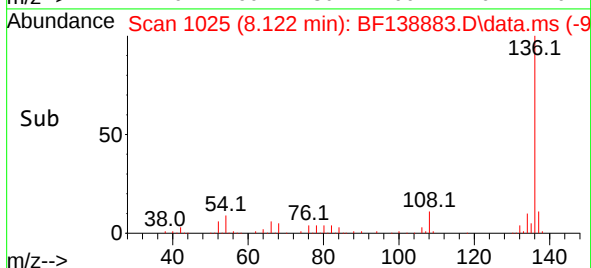

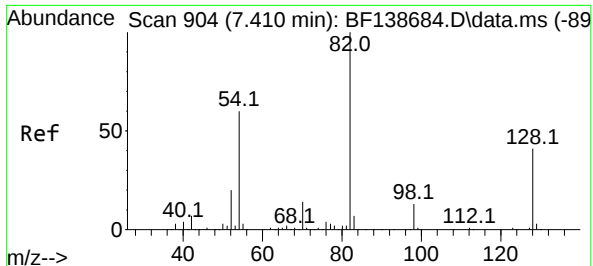

#23

Nitrobenzene-d5

Concen: 107.525 ng

RT: 7.404 min Scan# 904

Delta R.T. -0.006 min

Lab File: BF138883.D

Acq: 09 Aug 2024 11:52

Instrument :

BNA_F

ClientSampleId :

PB162423BL





Tgt Ion: 82 Resp: 372319

Ion Ratio Lower Upper

82 100

128 40.0 32.8 49.2

54 62.4 48.3 72.5

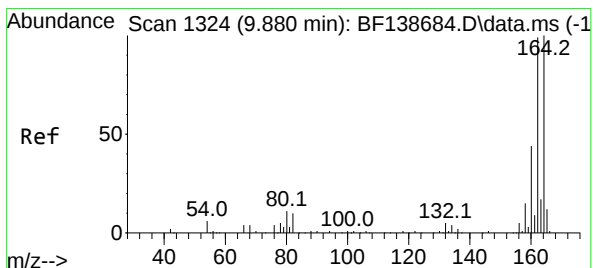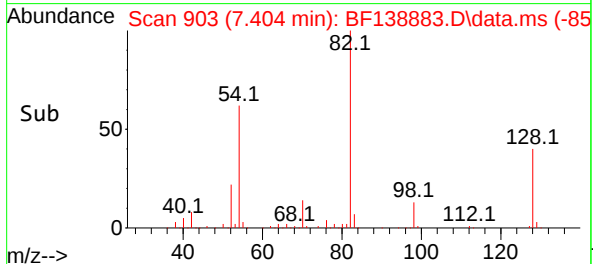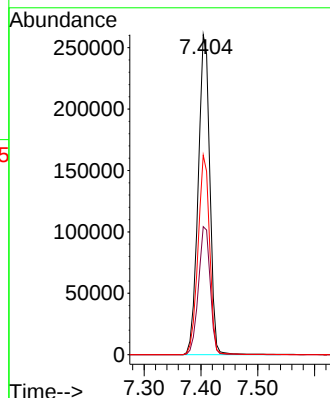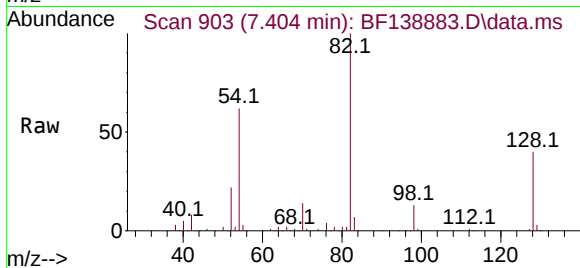

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.875 min Scan# 1323

Delta R.T. -0.005 min

Lab File: BF138883.D

Acq: 09 Aug 2024 11:52




Tgt Ion:164 Resp: 101270

Ion Ratio Lower Upper

164 100

162 100.2 79.4 119.0

160 44.5 35.1 52.7

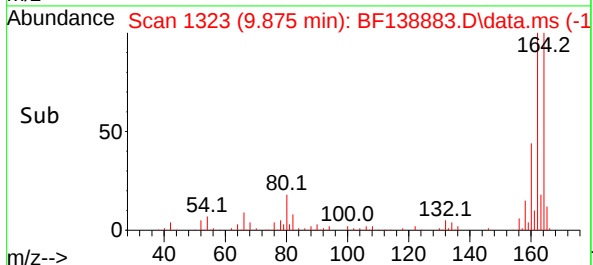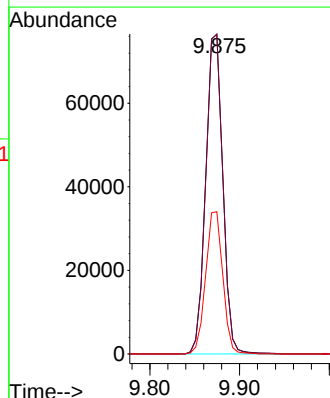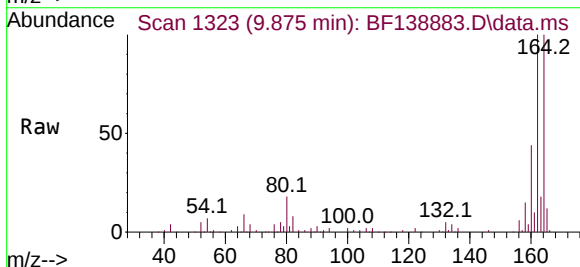



#42

2,4,6-Tribromophenol

Concen: 179.277 ng

RT: 10.669 min Scan# 1458

Delta R.T. 0.000 min

Lab File: BF138883.D


Acq: 09 Aug 2024 11:52

Instrument :

BNA_F

ClientSampleId :

PB162423BL

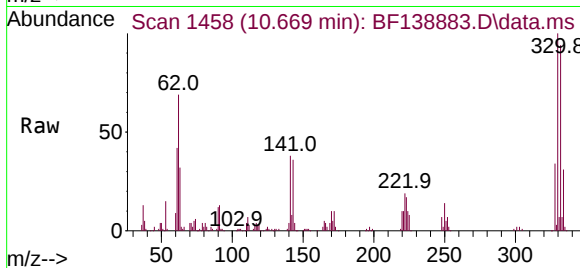




Tgt Ion:330 Resp: 148717

Ion Ratio Lower Upper

330 100

332 94.2 76.4 114.6

141 39.5 31.1 46.7

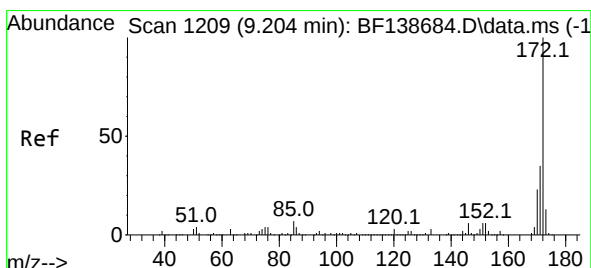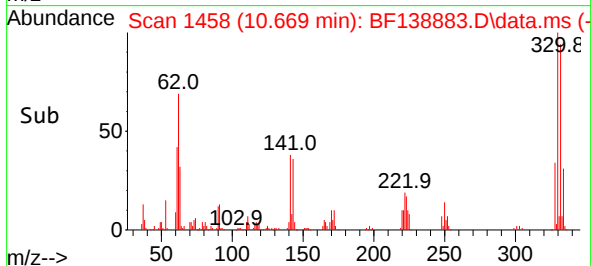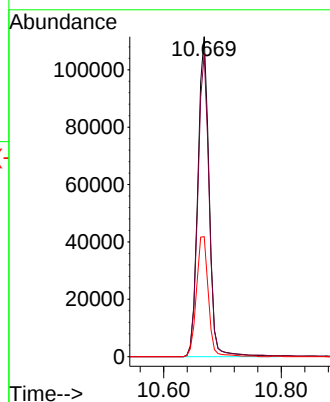

#45

2-Fluorobiphenyl

Concen: 105.866 ng

RT: 9.192 min Scan# 1207

Delta R.T. -0.012 min

Lab File: BF138883.D

Acq: 09 Aug 2024 11:52




Tgt Ion:172 Resp: 713549

Ion Ratio Lower Upper

172 100

171 35.6 28.3 42.5


170 23.1 18.8 28.2

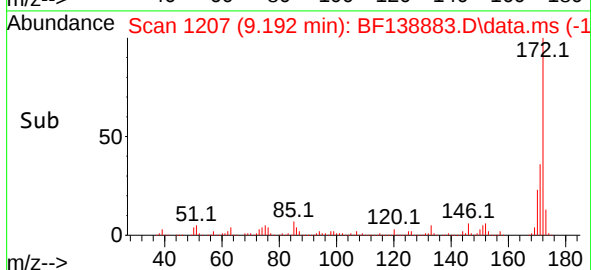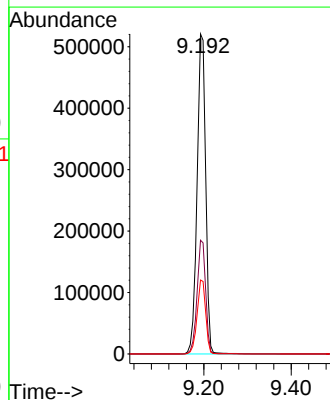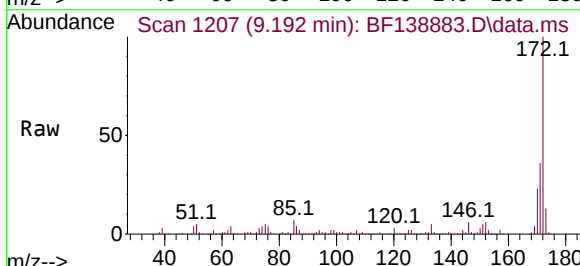





#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.357 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF138883.D
Acq: 09 Aug 2024 11:52

Instrument :
BNA_F
ClientSampleId :
PB162423BL



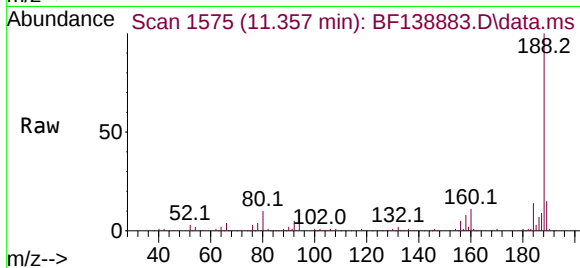



Tgt Ion:188 Resp: 195894
Ion Ratio Lower Upper
188 100
94 9.3 7.6 11.4
80 9.8 8.6 12.8

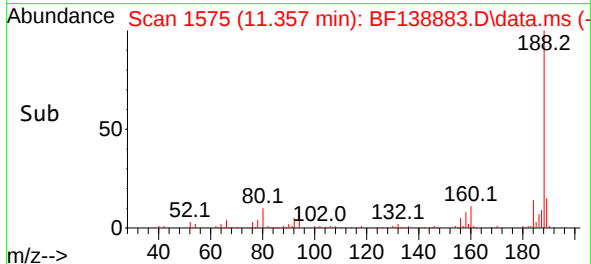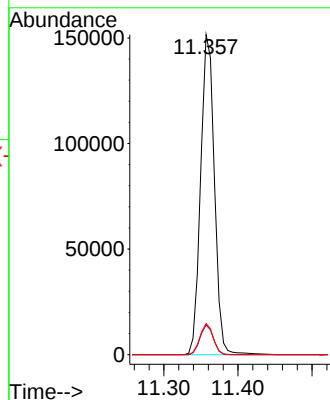

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.998 min Scan# 2024
Delta R.T. -0.006 min
Lab File: BF138883.D
Acq: 09 Aug 2024 11:52


Tgt Ion:240 Resp: 116610
Ion Ratio Lower Upper
240 100
120 10.3 10.2 15.4
236 25.4 19.8 29.8

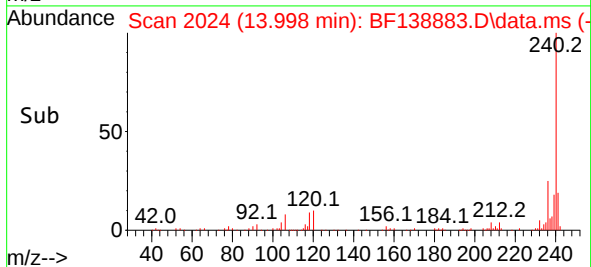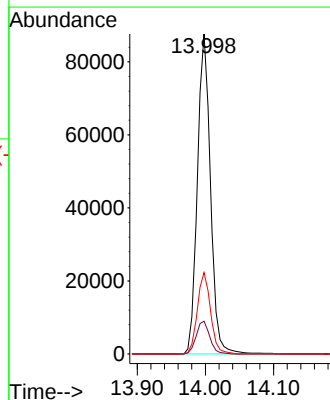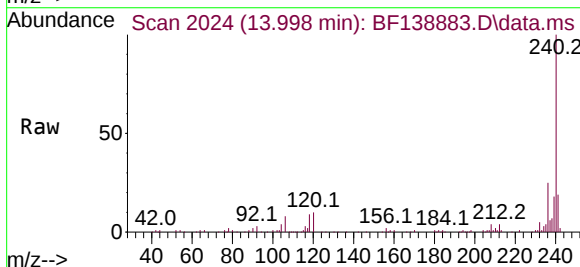



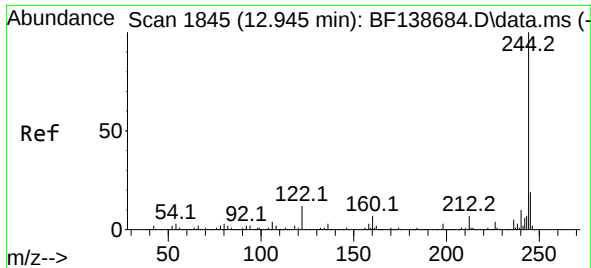


#79
 Terphenyl-d14
 Concen: 128.699 ng
 RT: 12.945 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BF138883.D
 Acq: 09 Aug 2024 11:52


Instrument :
 BNA_F
 ClientSampleId :
 PB162423BL

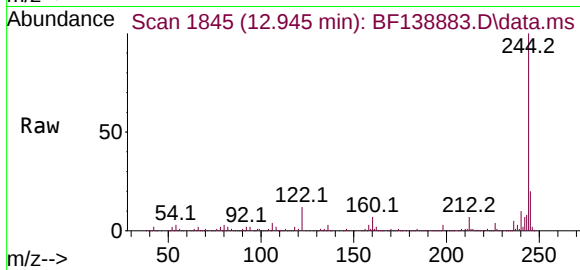

Tgt Ion:244 Resp: 896366
 Ion Ratio Lower Upper
 244 100
 212 7.0 5.4 8.2
 122 11.5 9.6 14.4

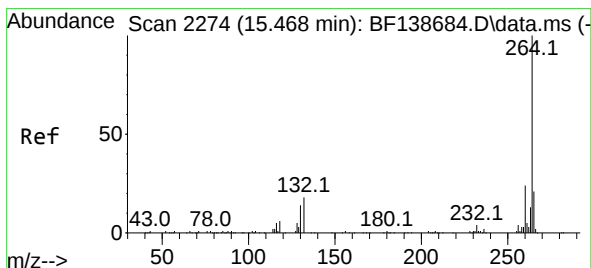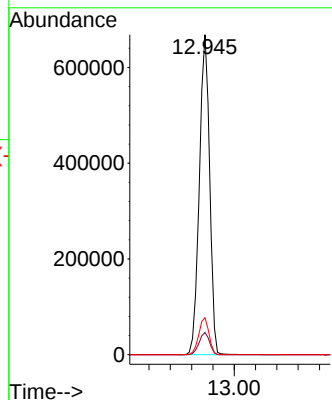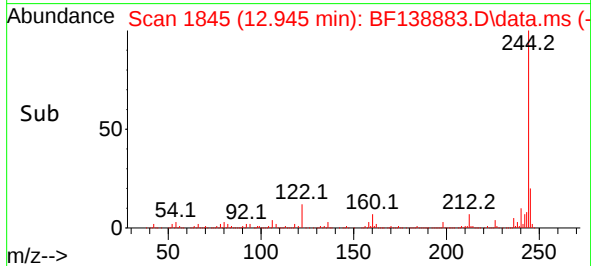

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.463 min Scan# 2273
 Delta R.T. -0.006 min
 Lab File: BF138883.D
 Acq: 09 Aug 2024 11:52

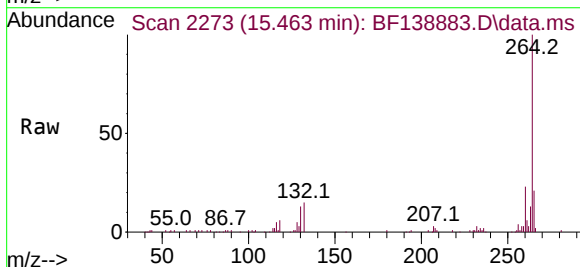

Tgt Ion:264 Resp: 79046
 Ion Ratio Lower Upper
 264 100
 260 23.4 19.0 28.6
 265 20.9 17.0 25.6

